



**Air
Toxics LTD.**
Laboratory Services Since 1989

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

COMPREHENSIVE VALIDATION PACKAGE

Modified TO-15

INVENTORY SHEET

Work Order #: 0704404

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	44
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	45	52
b. Surrogate Recover Summary Form (If Applicable)	53	53
c. Internal Standard Summary Form (If Applicable)	54	54
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	55	166
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	167	180
i. Second Source LCS(Summary + Raw Data)	181	194
i. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	195	196
l. GC/MS Tune (Results + Raw Data)	197	211
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	212	213
b. Chain-of-Custody Records	214	214
c. Sample Log-In Sheet	215	215
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	216	216
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	217	219
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	220	221
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	222	228
i. <u>Data Review Check Sheet</u>	229	229

Comments:

Completed by:

Judy Lee

Judy Lee / Document Control

5/8/07

(Signature)

(Print Name & Title)

(Date)



AN ENVIRONMENTAL ANALYTICAL LABORATORY


WORK ORDER #: 0704404

Work Order Summary

CLIENT:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Dr. Suite 201 Glastonbury, CT 06033	BILL TO:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Dr. Suite 201 Glastonbury, CT 06033
----------------	---	-----------------	---

PHONE:	860-368-5300	P.O. #	NR
FAX:	860-368-5307	PROJECT #	061140-8-1703 Bayshore Southern Cell
DATE RECEIVED:	04/20/2007	CONTACT:	IRM Kelly Buettner
DATE COMPLETED:	05/01/2007		

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>
01A	BS041807AMS2UW	Modified TO-15	6.0 "Hg
02A	BS041807AMS2XXXX	Modified TO-15	6.0 "Hg
03A	BS041807AMS4DW	Modified TO-15	6.0 "Hg
04A	BS041807 TB	Modified TO-15	29.0 "Hg
05A	Lab Blank	Modified TO-15	NA
06A	CCV	Modified TO-15	NA
07A	LCS	Modified TO-15	NA

CERTIFIED BY:  DATE: 05/01/07

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004
NY NELAP - 11291, UT NELAP - 9166389892

Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,
Accreditation number: E87680, Effective date: 07/01/06, Expiration date: 06/30/07

Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards

This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

LABORATORY NARRATIVE
Modified TO-15
GEI Consultants, Inc.
Workorder# 0704404

One 6 Liter Summa Canister and three 6 Liter Summa Canister (100% Certified) samples were received on April 20, 2007. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

Method modifications taken to run these samples are summarized in the below table. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	+/- 30% Difference	<=/= 30% Difference with two allowed out up to <=/=40%.; flag and narrate outliers
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

Receiving Notes

The Chain of Custody (COC) information for sample BS041807AMS2XXXX did not match the entry on the sample tag with regard to sample identification. The discrepancy was noted in the Sample Receipt Confirmation email/fax and the information on the COC was used to process and report the sample.

Sample identification for sample BS041807AMS2UW was not provided on the sample tag. The discrepancy was noted in the Sample Receipt Confirmation email/fax and the information on the Chain of Custody was used to process and report the sample.

Analytical Notes

The trip blank sample BS041807 TB has reportable levels of target compounds present.

All Quality Control Limit failures and affected sample results are noted by flags. Each flag is defined at the bottom of this Case Narrative and on each Sample Result Summary page. Target compound non-detects in the samples that are associated with high bias in QC analyses have not been flagged.

Definition of Data Qualifying Flags

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

B - Compound present in laboratory blank greater than reporting limit (background subtraction not performed).

J - Estimated value.

E - Exceeds instrument calibration range.

S - Saturated peak.

Q - Exceeds quality control limits.

U - Compound analyzed for but not detected above the reporting limit.

UJ- Non-detected compound associated with low bias in the CCV

N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

a-File was requantified

b-File was quantified by a second column and detector

r1-File was requantified for the purpose of reissue

Table 1

Client Sample ID	Lab Sample ID	Date Collected	Date Received	Date Extracted	Sample	Sample Extract		Sample Condition
					Holding Time (Days)	Date Analyzed	Holding Time (Days)	
BS041807AMS2UW	0704404-01A	4/18/2007	4/20/2007	NA	7	4/25/2007	NA	Good
BS041807AMS2XXXX	0704404-02A	4/18/2007	4/20/2007	NA	7	4/25/2007	NA	Good
BS041807AMS4DW	0704404-03A	4/18/2007	4/20/2007	NA	8	4/26/2007	NA	Good
BS041807 TB	0704404-04A	4/18/2007	4/20/2007	NA	8	4/26/2007	NA	Good
Lab Blank	0704404-05A	NA	NA	NA	NA	4/25/2007	NA	Good
CCV	0704404-06A	NA	NA	NA	NA	4/25/2007	NA	Good
LCS	0704404-07A	NA	NA	NA	NA	4/25/2007	NA	Good

Sample Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: BS041807AMS2UW

Lab ID#: 0704404-01A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Acetone	3.4	6.9	8.0	16
2-Butanone (Methyl Ethyl Ketone)	0.84	1.2	2.5	3.6
Tetrahydrofuran	0.84	0.86	2.5	2.5
Ethanol	3.4	3.3 J	6.3	6.3



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807AMS2UW

Lab ID#: 0704404-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042510	Date of Collection:	4/18/07
Dil. Factor:	1.68	Date of Analysis:	4/25/07 07:31 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.84	Not Detected	4.2	Not Detected
Freon 114	0.84	Not Detected	5.9	Not Detected
Vinyl Chloride	0.84	Not Detected	2.1	Not Detected
Bromomethane	0.84	Not Detected	3.3	Not Detected
Chloroethane	0.84	Not Detected	2.2	Not Detected
Freon 11	0.84	Not Detected	4.7	Not Detected
1,1-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Freon 113	0.84	Not Detected	6.4	Not Detected
Methylene Chloride	0.84	Not Detected	2.9	Not Detected
1,1-Dichloroethane	0.84	Not Detected	3.4	Not Detected
cis-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Chloroform	0.84	Not Detected	4.1	Not Detected
1,1,1-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Carbon Tetrachloride	0.84	Not Detected	5.3	Not Detected
Benzene	0.84	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.84	Not Detected	3.4	Not Detected
Trichloroethene	0.84	Not Detected	4.5	Not Detected
1,2-Dichloropropane	0.84	Not Detected	3.9	Not Detected
cis-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
Toluene	0.84	Not Detected	3.2	Not Detected
trans-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
1,1,2-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Tetrachloroethene	0.84	Not Detected	5.7	Not Detected
1,2-Dibromoethane (EDB)	0.84	Not Detected	6.4	Not Detected
Chlorobenzene	0.84	Not Detected	3.9	Not Detected
Ethyl Benzene	0.84	Not Detected	3.6	Not Detected
m,p-Xylene	0.84	Not Detected	3.6	Not Detected
o-Xylene	0.84	Not Detected	3.6	Not Detected
Styrene	0.84	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.84	Not Detected	5.8	Not Detected
1,3,5-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,2,4-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,3-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,4-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
alpha-Chlorotoluene	0.84	Not Detected	4.3	Not Detected
1,2-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,3-Butadiene	0.84	Not Detected	1.8	Not Detected
Hexane	0.84	Not Detected	3.0	Not Detected
Cyclohexane	0.84	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807AMS2UW

Lab ID#: 0704404-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042510	Date of Collection:	4/18/07
Dil. Factor:	1.68	Date of Analysis:	4/25/07 07:31 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.84	Not Detected	3.4	Not Detected
Bromodichloromethane	0.84	Not Detected	5.6	Not Detected
Dibromochloromethane	0.84	Not Detected	7.2	Not Detected
Cumene	0.84	Not Detected	4.1	Not Detected
Propylbenzene	0.84	Not Detected	4.1	Not Detected
Chloromethane	3.4	Not Detected	6.9	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	6.9	8.0	16
Carbon Disulfide	0.84	Not Detected	2.6	Not Detected
2-Propanol	3.4	Not Detected	8.2	Not Detected
trans-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.84	1.2	2.5	3.6
Tetrahydrofuran	0.84	0.86	2.5	2.5
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.84	Not Detected U J	3.4	Not Detected U J
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.84	Not Detected	8.7	Not Detected
4-Ethyltoluene	0.84	Not Detected	4.1	Not Detected
Ethanol	3.4	3.3 J	6.3	6.3
Methyl tert-butyl ether	0.84	Not Detected	3.0	Not Detected
3-Chloropropene	3.4	Not Detected	10	Not Detected
2,2,4-Trimethylpentane	0.84	Not Detected	3.9	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

J = Estimated value.

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	94	70-130
1,2-Dichloroethane-d4	96	70-130
4-Bromofluorobenzene	91	70-130

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042510.d
 Lab Smp Id: 0704404-01A
 Inj Date : 25-APR-2007 19:31
 Operator : jdg Inst ID: msd8.i
 Smp Info : 200mL #33909
 Misc Info : 6.0"Hg-5.0psi
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1
 Dil Factor: 1.68000
 Integrator: HP RTE Compound Sublist: AT04+Na.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395 (1.000)	130	178967	25.0000		80.00-	120.00	100.00	
8.395	8.395 (1.000)	128	146474			48.66-	108.66	81.84	
8.395	8.395 (1.000)	49	521278			263.93-	323.93	291.27	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.275 (1.000)	114	763542	25.0000		80.00-	120.00	100.00	
10.248	10.248 (1.000)	88	146047			0.00-	47.86	19.13	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225 (1.000)	117	552281	25.0000		80.00-	120.00	100.00	
15.225	15.225 (1.000)	82	394917			35.49-	95.49	71.51	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.474 (1.128)	65	369880	23.9098	23.910	80.00-	120.00	100.00	
9.473	9.474 (1.128)	67	184594			27.92-	87.92	49.91	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985 (1.267)	98	709849	23.6403	23.640	80.00-	120.00	100.00	
12.985	12.985 (1.267)	70	90604			0.00-	42.61	12.76	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 102 Toluene-d8 (continued)

12.985	12.985	(1.267)	100	439314			40.27- 100.27	61.89
--------	--------	---------	-----	--------	--	--	---------------	-------

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.773	16.773	(1.102)	174	258382	22.8291	22.829	80.00- 120.00	100.00
16.745	16.745	(1.100)	95	479836			138.42- 198.42	185.71
16.773	16.773	(1.102)	176	252667			67.24- 127.24	97.79

21 Ethanol

CAS #: 64-17-5

4.331	4.331	(0.516)	45	16196	1.99002	3.343	80.00- 120.00	100.00(a)
4.331	4.331	(0.516)	43	1255			0.00- 50.43	7.75
4.331	4.331	(0.516)	46	5902			12.21- 72.21	36.44

30 Acetone

CAS #: 67-64-1

4.994	4.967	(0.595)	58	42405	4.10289	6.893	80.00- 120.00	100.00
4.994	4.967	(0.595)	43	159695			337.35- 397.35	376.59

64 2-Butanone

CAS #: 78-93-3

8.008	8.008	(0.954)	72	6022	0.71855	1.207	80.00- 120.00	100.00
8.008	8.008	(0.954)	43	33868			568.31- 628.31	562.40
8.008	8.008	(0.954)	57	1073			10.61- 70.61	17.82

66 Tetrahydrofuran

CAS #: 109-99-9

8.367	8.368	(0.997)	42	16049	0.51432	0.8640	80.00- 120.00	100.00
8.367	8.368	(0.997)	71	2838			0.00- 55.57	17.68
8.367	8.395	(0.997)	72	3113			0.00- 56.52	19.40

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i
 Lab File ID: 8042510.d
 Lab Smp Id: 0704404-01A
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: jdg
 Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Misc Info: 6.0"Hg-5.0psi

Calibration Date: 25-APR-2007
 Calibration Time: 10:40
 Level: LOW
 Sample Type: AIR

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	178967	-22.99
86 1,4-Difluorobenze	1035529	621317	1449741	763542	-26.27
123 Chlorobenzene-d5	744287	446572	1042002	552281	-25.80

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.25	-0.27
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-25apr
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0704404-01A
Level: LOW Operator: jdg
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04+Na.sub
Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
Misc Info: 6.0"Hg-5.0psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	23.910	95.64	70-130
\$ 102 Toluene-d8	25.000	23.640	94.56	70-130
\$ 138 Bromofluorobenzene	25.000	22.829	91.32	70-130

Data File: /chem/msd8.1/8-25apr.b/8042510.d

Date: 25-APR-2007 19:31

Client ID:


Sample Info: 200mL #33909

Column phase: RTX-624

Instrument: msd8.1

Operator: jdg

Column diameter: 0.53



Date : 25-APR-2007 19:31

Client ID:

Instrument: msd8,i

Sample Info: 200mL #33909








Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

21 Ethanol

Concentration: 3,343 PPBV



Date : 25-APR-2007 19:31

Client ID:

Instrument: msd8.i

Sample Info: 200mL #33909







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

30 Acetone

Concentration: 6.893 PPBV



Date : 25-APR-2007 19:31

Client ID:

Instrument: msd8.i

Sample Info: 200mL #33909








Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

64 2-Butanone

Concentration: 1.207 PPBV



Date : 25-APR-2007 19:31

Client ID:

Instrument: msd8.i

Sample Info: 200mL #33909








Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

66 Tetrahydrofuran

Concentration: 0.8640 PPBV

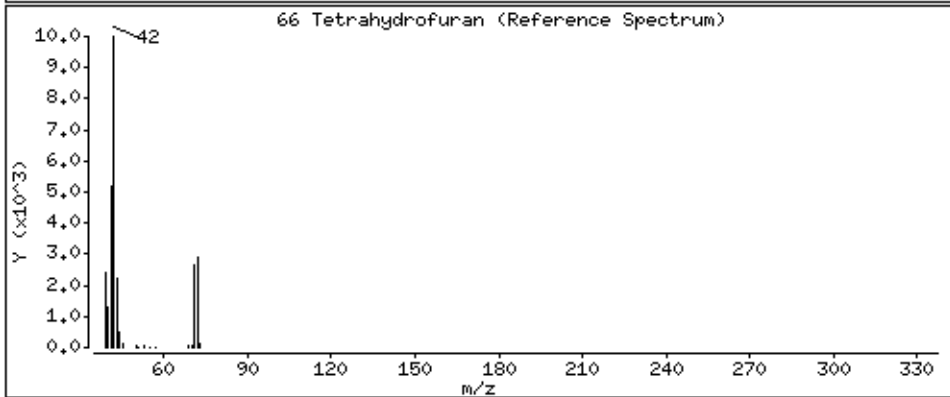



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds
MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: BS041807AMS2XXXX

Lab ID#: 0704404-02A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Acetone	3.4	5.9	8.0	14



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807AMS2XXXX

Lab ID#: 0704404-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042511	Date of Collection:	4/18/07
Dil. Factor:	1.68	Date of Analysis:	4/25/07 08:13 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.84	Not Detected	4.2	Not Detected
Freon 114	0.84	Not Detected	5.9	Not Detected
Vinyl Chloride	0.84	Not Detected	2.1	Not Detected
Bromomethane	0.84	Not Detected	3.3	Not Detected
Chloroethane	0.84	Not Detected	2.2	Not Detected
Freon 11	0.84	Not Detected	4.7	Not Detected
1,1-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Freon 113	0.84	Not Detected	6.4	Not Detected
Methylene Chloride	0.84	Not Detected	2.9	Not Detected
1,1-Dichloroethane	0.84	Not Detected	3.4	Not Detected
cis-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Chloroform	0.84	Not Detected	4.1	Not Detected
1,1,1-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Carbon Tetrachloride	0.84	Not Detected	5.3	Not Detected
Benzene	0.84	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.84	Not Detected	3.4	Not Detected
Trichloroethene	0.84	Not Detected	4.5	Not Detected
1,2-Dichloropropane	0.84	Not Detected	3.9	Not Detected
cis-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
Toluene	0.84	Not Detected	3.2	Not Detected
trans-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
1,1,2-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Tetrachloroethene	0.84	Not Detected	5.7	Not Detected
1,2-Dibromoethane (EDB)	0.84	Not Detected	6.4	Not Detected
Chlorobenzene	0.84	Not Detected	3.9	Not Detected
Ethyl Benzene	0.84	Not Detected	3.6	Not Detected
m,p-Xylene	0.84	Not Detected	3.6	Not Detected
o-Xylene	0.84	Not Detected	3.6	Not Detected
Styrene	0.84	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.84	Not Detected	5.8	Not Detected
1,3,5-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,2,4-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,3-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,4-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
alpha-Chlorotoluene	0.84	Not Detected	4.3	Not Detected
1,2-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,3-Butadiene	0.84	Not Detected	1.8	Not Detected
Hexane	0.84	Not Detected	3.0	Not Detected
Cyclohexane	0.84	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807AMS2XXXX

Lab ID#: 0704404-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042511	Date of Collection:	4/18/07
Dil. Factor:	1.68	Date of Analysis:	4/25/07 08:13 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.84	Not Detected	3.4	Not Detected
Bromodichloromethane	0.84	Not Detected	5.6	Not Detected
Dibromochloromethane	0.84	Not Detected	7.2	Not Detected
Cumene	0.84	Not Detected	4.1	Not Detected
Propylbenzene	0.84	Not Detected	4.1	Not Detected
Chloromethane	3.4	Not Detected	6.9	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	5.9	8.0	14
Carbon Disulfide	0.84	Not Detected	2.6	Not Detected
2-Propanol	3.4	Not Detected	8.2	Not Detected
trans-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.84	Not Detected	2.5	Not Detected
Tetrahydrofuran	0.84	Not Detected	2.5	Not Detected
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.84	Not Detected U J	3.4	Not Detected U J
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.84	Not Detected	8.7	Not Detected
4-Ethyltoluene	0.84	Not Detected	4.1	Not Detected
Ethanol	3.4	Not Detected	6.3	Not Detected
Methyl tert-butyl ether	0.84	Not Detected	3.0	Not Detected
3-Chloropropene	3.4	Not Detected	10	Not Detected
2,2,4-Trimethylpentane	0.84	Not Detected	3.9	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: 6 Liter Summa Canister (100% Certified)

Surrogates	%Recovery	Method Limits
Toluene-d8	96	70-130
1,2-Dichloroethane-d4	94	70-130
4-Bromofluorobenzene	95	70-130

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042511.d
 Lab Smp Id: 0704404-02A
 Inj Date : 25-APR-2007 20:13
 Operator : jdg Inst ID: msd8.i
 Smp Info : 200mL #34002
 Misc Info : 6.0"Hg-5.0psi
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1
 Dil Factor: 1.68000
 Integrator: HP RTE Compound Sublist: AT04+Na.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				(PPBV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====

* 67	Bromochloromethane					CAS #: 74-97-5		
8.395	8.395	(1.000)	130	177594	25.0000	80.00- 120.00	100.00	
8.395	8.395	(1.000)	128	139257		48.66- 108.66	78.41	
8.395	8.395	(1.000)	49	503082		263.93- 323.93	283.28	

* 86	1,4-Difluorobenzene					CAS #: 540-36-3		
10.248	10.275	(1.000)	114	748952	25.0000	80.00- 120.00	100.00	
10.248	10.248	(1.000)	88	135128		0.00- 47.86	18.04	

* 123	Chlorobenzene-d5					CAS #: 3114-55-4		
15.225	15.225	(1.000)	117	551196	25.0000	80.00- 120.00	100.00	
15.225	15.225	(1.000)	82	366197		35.49- 95.49	66.44	

\$ 80	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.474	9.474	(1.128)	65	361409	23.5428	80.00- 120.00	100.00	
9.474	9.474	(1.128)	67	178133		27.92- 87.92	49.29	

\$ 102	Toluene-d8					CAS #: 2037-26-5		
12.985	12.985	(1.267)	98	708915	24.0691	80.00- 120.00	100.00	
12.985	12.985	(1.267)	70	92504		0.00- 42.61	13.05	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 102 Toluene-d8 (continued)

12.985 12.985 (1.267) 100 452573 40.27- 100.27 63.84

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.773 16.773 (1.102) 174 268376 23.7587 23.759 80.00- 120.00 100.00

16.745 16.745 (1.100) 95 477514 138.42- 198.42 177.93

16.773 16.773 (1.102) 176 271760 67.24- 127.24 101.26

30 Acetone

CAS #: 67-64-1

4.994 4.967 (0.595) 58 35914 3.50172 5.883 80.00- 120.00 100.00

4.994 4.967 (0.595) 43 131390 337.35- 397.35 365.85

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msd8.i
Lab File ID: 8042511.d
Lab Smp Id: 0704404-02ACalibration Date: 25-APR-2007
Calibration Time: 10:40

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: jdg

Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m

Misc Info: 6.0"Hg-5.0psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	177594	-23.58
86 1,4-Difluorobenze	1035529	621317	1449741	748952	-27.67
123 Chlorobenzene-d5	744287	446572	1042002	551196	-25.94

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.25	-0.27
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-25apr
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0704404-02A
Level: LOW Operator: jdg
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04+Na.sub
Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
Misc Info: 6.0"Hg-5.0psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	23.543	94.17	70-130
\$ 102 Toluene-d8	25.000	24.069	96.28	70-130
\$ 138 Bromofluorobenzene	25.000	23.759	95.03	70-130

Data File: /chem/msd8.1/8-25apr.b/8042511.d

Date: 25-APR-2007 20:13

Client ID:

Sample Info: 200mL #34002


Column phase: RTX-624

Instrument: msd8.1

Operator: jdg

Column diameter: 0.53

Page 1



Date : 25-APR-2007 20:13

Client ID:

Instrument: msd8.i

Sample Info: 200mL #34002







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

30 Acetone

Concentration: 5.883 PPBV





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds
MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: BS041807AMS4DW

Lab ID#: 0704404-03A

No Detections Were Found.



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807AMS4DW

Lab ID#: 0704404-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042519	Date of Collection:	4/18/07
Dil. Factor:	1.68	Date of Analysis:	4/26/07 01:37 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.84	Not Detected	4.2	Not Detected
Freon 114	0.84	Not Detected	5.9	Not Detected
Vinyl Chloride	0.84	Not Detected	2.1	Not Detected
Bromomethane	0.84	Not Detected	3.3	Not Detected
Chloroethane	0.84	Not Detected	2.2	Not Detected
Freon 11	0.84	Not Detected	4.7	Not Detected
1,1-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Freon 113	0.84	Not Detected	6.4	Not Detected
Methylene Chloride	0.84	Not Detected	2.9	Not Detected
1,1-Dichloroethane	0.84	Not Detected	3.4	Not Detected
cis-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Chloroform	0.84	Not Detected	4.1	Not Detected
1,1,1-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Carbon Tetrachloride	0.84	Not Detected	5.3	Not Detected
Benzene	0.84	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.84	Not Detected	3.4	Not Detected
Trichloroethene	0.84	Not Detected	4.5	Not Detected
1,2-Dichloropropane	0.84	Not Detected	3.9	Not Detected
cis-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
Toluene	0.84	Not Detected	3.2	Not Detected
trans-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
1,1,2-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Tetrachloroethene	0.84	Not Detected	5.7	Not Detected
1,2-Dibromoethane (EDB)	0.84	Not Detected	6.4	Not Detected
Chlorobenzene	0.84	Not Detected	3.9	Not Detected
Ethyl Benzene	0.84	Not Detected	3.6	Not Detected
m,p-Xylene	0.84	Not Detected	3.6	Not Detected
o-Xylene	0.84	Not Detected	3.6	Not Detected
Styrene	0.84	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.84	Not Detected	5.8	Not Detected
1,3,5-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,2,4-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,3-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,4-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
alpha-Chlorotoluene	0.84	Not Detected	4.3	Not Detected
1,2-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,3-Butadiene	0.84	Not Detected	1.8	Not Detected
Hexane	0.84	Not Detected	3.0	Not Detected
Cyclohexane	0.84	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807AMS4DW

Lab ID#: 0704404-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042519	Date of Collection:	4/18/07
Dil. Factor:	1.68	Date of Analysis:	4/26/07 01:37 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.84	Not Detected	3.4	Not Detected
Bromodichloromethane	0.84	Not Detected	5.6	Not Detected
Dibromochloromethane	0.84	Not Detected	7.2	Not Detected
Cumene	0.84	Not Detected	4.1	Not Detected
Propylbenzene	0.84	Not Detected	4.1	Not Detected
Chloromethane	3.4	Not Detected	6.9	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	Not Detected	8.0	Not Detected
Carbon Disulfide	0.84	Not Detected	2.6	Not Detected
2-Propanol	3.4	Not Detected	8.2	Not Detected
trans-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.84	Not Detected	2.5	Not Detected
Tetrahydrofuran	0.84	Not Detected	2.5	Not Detected
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.84	Not Detected U J	3.4	Not Detected U J
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.84	Not Detected	8.7	Not Detected
4-Ethyltoluene	0.84	Not Detected	4.1	Not Detected
Ethanol	3.4	Not Detected	6.3	Not Detected
Methyl tert-butyl ether	0.84	Not Detected	3.0	Not Detected
3-Chloropropene	3.4	Not Detected	10	Not Detected
2,2,4-Trimethylpentane	0.84	Not Detected	3.9	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: 6 Liter Summa Canister (100% Certified)

Surrogates	%Recovery	Method Limits
Toluene-d8	93	70-130
1,2-Dichloroethane-d4	96	70-130
4-Bromofluorobenzene	100	70-130

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042519.d
 Lab Smp Id: 0704404-03A
 Inj Date : 26-APR-2007 01:37
 Operator : kr Inst ID: msd8.i
 Smp Info : 200mL #9573
 Misc Info : 6.0"Hg -> 5psi
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1
 Dil Factor: 1.68000
 Integrator: HP RTE Compound Sublist: AT04+Na.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395 (1.000)	130	179619	25.0000		80.00-	120.00	100.00	
8.395	8.395 (1.000)	128	145236			48.66-	108.66	80.86	
8.395	8.395 (1.000)	49	508056			263.93-	323.93	282.85	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.275 (1.000)	114	740167	25.0000		80.00-	120.00	100.00	
10.248	10.248 (1.000)	88	136402			0.00-	47.86	18.43	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225 (1.000)	117	563218	25.0000		80.00-	120.00	100.00	
15.197	15.225 (1.000)	82	381895			35.49-	95.49	67.81	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.474 (1.128)	65	372042	23.9622	23.962	80.00-	120.00	100.00	
9.473	9.474 (1.128)	67	184641			27.92-	87.92	49.63	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985 (1.267)	98	677855	23.2877	23.288	80.00-	120.00	100.00	
12.985	12.985 (1.267)	70	81790			0.00-	42.61	12.07	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 102 Toluene-d8 (continued)

12.985	12.985	(1.267)	100	468538			40.27- 100.27	69.12
--------	--------	---------	-----	--------	--	--	---------------	-------

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.773	16.773	(1.102)	174	289596	25.0901	25.090	80.00- 120.00	100.00
16.745	16.745	(1.100)	95	487254			138.42- 198.42	168.25
16.773	16.773	(1.102)	176	264074			67.24- 127.24	91.19

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msd8.i
Lab File ID: 8042519.d
Lab Smp Id: 0704404-03ACalibration Date: 25-APR-2007
Calibration Time: 10:40

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m

Misc Info: 6.0"Hg -> 5psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	179619	-22.71
86 1,4-Difluorobenze	1035529	621317	1449741	740167	-28.52
123 Chlorobenzene-d5	744287	446572	1042002	563218	-24.33

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.25	-0.27
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-25apr
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0704404-03A
Level: LOW Operator: kr
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04+Na.sub
Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
Misc Info: 6.0"Hg -> 5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	23.962	95.85	70-130
\$ 102 Toluene-d8	25.000	23.288	93.15	70-130
\$ 138 Bromofluorobenzene	25.000	25.090	100.36	70-130

Data File: /chem/msd8.1/8-25apr.1b/8042519.1.d

Date: 26-Apr-2007 01:37

Client ID:


Sample Info: 200mL #9573

Column phase: RTX-624

Instrument: msd8.1

Operator: kr

Column diameter: 0.53





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: BS041807 TB

Lab ID#: 0704404-04A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Acetone	2.0	2.9	4.8	6.9
2-Butanone (Methyl Ethyl Ketone)	0.50	0.54	1.5	1.6



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807 TB

Lab ID#: 0704404-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042520	Date of Collection:	4/18/07
Dil. Factor:	1.00	Date of Analysis:	4/26/07 02:19 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: BS041807 TB

Lab ID#: 0704404-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042520	Date of Collection:	4/18/07
Dil. Factor:	1.00	Date of Analysis:	4/26/07 02:19 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	2.9	4.8	6.9
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	0.54	1.5	1.6
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected U J	2.0	Not Detected U J
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: 6 Liter Summa Canister (100% Certified)

Surrogates	%Recovery	Method Limits
Toluene-d8	92	70-130
1,2-Dichloroethane-d4	93	70-130
4-Bromofluorobenzene	93	70-130

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042520.d
 Lab Smp Id: 0704404-04A
 Inj Date : 26-APR-2007 02:19
 Operator : kr Inst ID: msd8.i
 Smp Info : 200mL #36033
 Misc Info : 29.0"Hg -> 5psi
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+Na.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	182221	25.0000		80.00- 120.00	100.00	
8.395	8.395	(1.000)	128	134203			48.66- 108.66	73.65	
8.395	8.395	(1.000)	49	491452			263.93- 323.93	269.70	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.247	10.275	(1.000)	114	750864	25.0000		80.00- 120.00	100.00	
10.247	10.248	(1.000)	88	143063			0.00- 47.86	19.05	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.225	(1.000)	117	563512	25.0000		80.00- 120.00	100.00	
15.224	15.225	(1.000)	82	378649			35.49- 95.49	67.19	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.474	(1.128)	65	367348	23.3220	23.322	80.00- 120.00	100.00	
9.473	9.474	(1.128)	67	173664			27.92- 87.92	47.28	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	677752	22.9525	22.952	80.00- 120.00	100.00	
12.985	12.985	(1.267)	70	85113			0.00- 42.61	12.56	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 102 Toluene-d8 (continued)

12.985 12.985 (1.267) 100 468329 40.27- 100.27 69.10

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.773 16.773 (1.102) 174 268262 23.2296 23.230 80.00- 120.00 100.00

16.745 16.745 (1.100) 95 487441 138.42- 198.42 181.70

16.773 16.773 (1.102) 176 280638 67.24- 127.24 104.61

30 Acetone

CAS #: 67-64-1

4.994 4.967 (0.595) 58 30620 2.90973 2.910 80.00- 120.00 100.00

4.994 4.967 (0.595) 43 109910 337.35- 397.35 358.95

64 2-Butanone

CAS #: 78-93-3

8.008 8.008 (0.954) 72 4651 0.54505 0.5450 80.00- 120.00 100.00

7.980 8.008 (0.951) 43 33936 568.31- 628.31 729.65

7.980 8.008 (0.951) 57 2758 10.61- 70.61 59.30

Report Date: 01-May-2007 15:26

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msd8.i
Lab File ID: 8042520.d
Lab Smp Id: 0704404-04ACalibration Date: 25-APR-2007
Calibration Time: 10:40

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m

Misc Info: 29.0"Hg -> 5psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	182221	-21.59
86 1,4-Difluorobenze	1035529	621317	1449741	750864	-27.49
123 Chlorobenzene-d5	744287	446572	1042002	563512	-24.29

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.39	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.25	-0.27
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-25apr
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0704404-04A
Level: LOW Operator: kr
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04+Na.sub
Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
Misc Info: 29.0"Hg -> 5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	23.322	93.29	70-130
\$ 102 Toluene-d8	25.000	22.952	91.81	70-130
\$ 138 Bromofluorobenzene	25.000	23.230	92.92	70-130

Data File: /chem/msd8.1/8-25apr.1b/8042520.d

Date: 26-Apr-2007 02:19

Client ID:


Sample Info: 200mL #36033

Column phase: RTX-624

Instrument: msd8.1

Operator: kr

Column diameter: 0.53



Date : 26-APR-2007 02:19

Client ID:

Instrument: msd8.i

Sample Info: 200mL #36033







Operator: kr

Column phase: RTX-624

Column diameter: 0.53

30 Acetone

Concentration: 2,910 PPBV



Date : 26-APR-2007 02:19

Client ID:

Instrument: msd8.i

Sample Info: 200mL #36033








Operator: kr

Column phase: RTX-624

Column diameter: 0.53

64 2-Butanone

Concentration: 0.5450 PPBV



QC Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0704404-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042505	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 4/25/07 01:21 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0704404-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042505	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 4/25/07 01:21 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected U J	2.0	Not Detected U J
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	93	70-130
1,2-Dichloroethane-d4	98	70-130
4-Bromofluorobenzene	96	70-130

Report Date: 25-Apr-2007 14:17

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042505.d
 Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
 Inj Date : 25-APR-2007 13:21
 Operator : JG Inst ID: msd8.i
 Smp Info : 200mL #13673
 Misc Info : Humid
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	171490	25.0000		80.00- 120.00	100.00	
8.395	8.395	(1.000)	128	137391			48.66- 108.66	80.12	
8.395	8.395	(1.000)	49	485488			263.93- 323.93	283.10	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.275	(1.000)	114	773259	25.0000		80.00- 120.00	100.00	
10.248	10.248	(1.000)	88	131686			0.00- 47.86	17.03	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225	(1.000)	117	574386	25.0000		80.00- 120.00	100.00	
15.225	15.225	(1.000)	82	387203			35.49- 95.49	67.41	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.474	(1.128)	65	361523	24.3885	24.388	80.00- 120.00	100.00	
9.473	9.474	(1.128)	67	179294			27.92- 87.92	49.59	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	705466	23.1991	23.199	80.00- 120.00	100.00	
12.985	12.985	(1.267)	70	89475			0.00- 42.61	12.68	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 102 Toluene-d8 (continued)

12.985 12.985 (1.267) 100 480734 40.27- 100.27 68.14

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.773 16.773 (1.102) 174 282913 24.0345 24.034 80.00- 120.00 100.00

16.745 16.745 (1.100) 95 497747 138.42- 198.42 175.94

16.773 16.773 (1.102) 176 268280 67.24- 127.24 94.83

Report Date: 25-Apr-2007 14:17

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 25-APR-2007

Lab File ID: 8042505.d

Calibration Time: 10:40

Lab Smp Id: Lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m

Misc Info: Humid

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	171490	-26.21
86 1,4-Difluorobenze	1035529	621317	1449741	773259	-25.33
123 Chlorobenzene-d5	744287	446572	1042002	574386	-22.83

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.25	-0.27
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-25apr
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
Level: LOW Operator: JG
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04+ENS.sub
Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
Misc Info: Humid

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	24.388	97.55	70-130
\$ 102 Toluene-d8	25.000	23.199	92.80	70-130
\$ 138 Bromofluorobenzene	25.000	24.034	96.14	70-130

Data File: /chem/msd8.1/8-25apr.1b/8042505.d

Date: 25-APR-2007 13:21

Client ID: Lab Blank


Sample Info: 200mL #13673

Column phase: RTX-624

Instrument: msd8.1

Operator: JG

Column diameter: 0.53



LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0704404

	CLIENT SAMPLE NO.	SURROGATE % RECOVERY						TOTAL OUT
		1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#	
01	BS041807AMS2UW	96		94		91		0
02	BS041807AMS2XXXX	94		96		95		0
03	BS041807AMS4DW	96		93		100		0
04	BS041807 TB	93		92		93		0
05	Lab Blank	98		93		96		0
06	CCV	101		94		106		0
07	LCS	100		98		107		0
08								0
09								0
10								0
11								0
12								0
13								0
14								0
15								0
16								0
17								0
18								0
19								0
20								0
21								0
22								0
23								0
24								0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

* Designates values outside of QC limits

LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD
 Lab File ID: 8042502.d
 Instrument ID: msd8.i

SDG No: 0704404
 Date Analyzed: 04/25/2007
 Time Analyzed: 10:40 AM

		Chlorobenzene-d5		1,4-Difluorobenzene		Bromochloromethane	
		Area	RT	Area	RT	Area	RT
		#	#	#	#	#	#
24-HOUR STD		744287	15.22	1035529	10.28	232391	8.4
UPPER LIMIT		1042002	15.55	1449741	10.61	325347	08.73
LOWER LIMIT		446572	14.89	621317	09.95	139435	08.07
CLIENT SAMPLE NO							
01	BS041807AMS2UW	552281	15.22	763542	10.25	178967	8.4
02	BS041807AMS2XXXX	551196	15.22	748952	10.25	177594	8.4
03	BS041807AMS4DW	563218	15.22	740167	10.25	179619	8.4
04	BS041807 TB	563512	15.22	750864	10.25	182221	8.39
05	Lab Blank	574386	15.22	773259	10.25	171490	8.4
06	CCV	744287	15.22	1035529	10.28	232391	8.4
07	LCS	605228	15.22	790852	10.25	173884	8.4
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

'Area Upper Limit=+40% of internal standard area'
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT
 RT Lower Limit=-0.33 minutes of internal standard RT

* Designates values outside of QC limits

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
27 Freon 113	+++++	2.82232	3.22222	2.14765	2.03365	2.04910			
	1.95455							2.37158	22.064
29 1,1-Dichloroethene	+++++	5.25838	5.05771	3.62935	3.42759	3.47883			
	3.36907							4.03682	21.678
30 Acetone	+++++	+++++	2.05734	1.38732	1.24688	1.27242			
	1.25483							1.44376	24.081
31 Acetaldehyde	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
	+++++							+++++	+++++
32 Freon143a	+++++	+++++	+++++	+++++	+++++	+++++			
	+++++							+++++	+++++
33 Carbon Disulfide	+++++	7.95920	7.71487	5.56651	5.39873	5.39231			
	5.27666							6.21805	20.261
34 2-Propanol	+++++	+++++	6.85744	5.44165	5.29419	5.39097			
	5.29799							5.65645	11.921
35 Acetonitrile	+++++	+++++	+++++	+++++	+++++	+++++			
	+++++							+++++	+++++
36 Cyclopentene	+++++	+++++	+++++	+++++	+++++	+++++			
	+++++							+++++	+++++
37 3-Chloropropene	+++++	+++++	1.33829	0.93944	0.92232	0.92704			
	0.89360							1.00414	18.678

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
38 tert-Butyl-Alcohol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
39 Methylene Chloride	+++++	4.53517	4.27698	3.10830	2.90127	2.94899		3.43297	22.248
40 Acrylonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
41 2-Methyl-1-Butene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
42 MTBE	+++++	8.85745	8.57775	6.27521	5.93540	5.99233		6.91999	20.258
44 1-Pentene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
43 trans-1,2-Dichloroethene	+++++	2.94934	2.54247	1.79033	1.70500	1.72263		2.06297	26.460
45 Hexane	+++++	6.50743	6.29843	4.63124	4.39618	4.38297		5.07809	20.393
46 Ethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
47 Ethanol-high	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
48 Isopropyl ether	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
49 Propanal	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
50 Chloroprene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
51 1-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
52 1,1-Dichloroethane	+++++	5.18323	5.10569	3.98508	3.87923	3.82996		
	3.75100						4.28903	15.560
53 Bromoethane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
54 Vinyl Acetate	+++++	+++++	0.51558	0.49264	0.52336	0.51139		
	0.50793						0.51018	2.229
55 Iodomethane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
56 2,3-Dimethylbutane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
57 Ethyl-tert-butyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
69 Chloroform	6.17803	5.06987	4.49947	3.38493	3.22658	3.26840		
	3.14998						4.11103	28.585
70 2-Butanol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
71 1,1-Dichloropropene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
72 Cyclohexane	+++++	3.97979	3.99673	2.74032	2.57034	2.59050		
	2.50871						3.06440	23.485
74 3-Methyl-1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
73 1,1,1-Trichloroethane	+++++	4.63376	4.65460	3.38033	3.20850	3.24716		
	3.14555						3.71165	19.572
75 Carbon Tetrachloride	+++++	3.35462	3.79930	2.81089	2.69706	2.70088		
	2.62506						2.99797	15.802
76 Isobutanol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
77 tert-amyl-Methyl Ether	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
78 2,2,4-Trimethylpentane	+++++	16.43298	17.99115	13.37425	12.70715	12.77683		
	12.50824						14.29843	16.282

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
79 Benzene	2.03131	1.47626	1.61743	1.22633	1.16525	1.12959		
	1.10050						1.39238	24.519
81 1,2-Dichloroethane	+++++	0.84058	0.78407	0.61043	0.57149	0.55908		
	0.54673						0.65206	19.511
82 Heptane	+++++	0.28296	0.17842	0.14079	0.13652	0.13223		
	0.12701						0.16632	36.075
83 2,3-Dimethylpentane	+++++	+++++	1.93177	+++++	1.34790	+++++		
	1.27765						1.51911	23.639
84 1-Methoxy-2-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
85 2,3,4-Trimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
87 1-Butanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
88 Methyl Methacrylate	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
89 2-Pentanone	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
90 Pentanal	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
91 Ethyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
92 Trichloroethene	+++++	0.48093	0.59807	0.43694	0.40476	0.38896		0.44787	18.426
93 Methyl Cyclohexane	+++++	4.88062	4.87830	3.41153	3.30277	3.30451		3.83302	21.206
94 Dibromomethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
95 1,2-Dichloropropane	+++++	0.67532	0.61108	0.46484	0.45017	0.43591		0.51024	20.748
96 1,4-Dioxane	+++++	+++++	0.34178	0.26004	0.24908	0.24171		0.26600	16.251
97 Octane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
98 Bromodichloromethane	+++++	0.89246	0.94044	0.71928	0.67428	0.65833		0.75448	17.094
99 1-Nitropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
100 cis-1,3-Dichloropropene	+++++	0.76889	0.76757	0.60016	0.57911	0.58023		0.64347	15.119

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
101 4-Methyl-2-pentanone	0.43377	0.67928	0.62422	0.46863	0.46135	0.44565		0.51882	20.265
103 Toluene	1.12371	1.34027	1.57212	1.22204	1.16762	1.13880		1.26076	13.605
104 1-Methoxy-2-propyl acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
105 Epichlorohydrin	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
106 trans-1,3-Dichloropropene	0.76552	1.11760	0.96729	0.81239	0.78942	0.77860		0.87181	16.208
107 1,3-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
108 1,1,2-Trichloroethane	0.42903	0.65309	0.58031	0.47394	0.45806	0.45084		0.50754	17.498
110 alpha-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
109 Tetrachloroethene	0.47984	0.68363	0.56664	0.50273	0.50196	0.49965		0.53907	14.229
111 Butyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
112 2-Hexanone	+++++	+++++	0.88087	0.79222	0.78548	0.79567		
	0.75095						0.80104	5.997
113 trans-1,4-dichloro-2-butene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
114 Dibromochloromethane	+++++	0.83418	0.80967	0.62979	0.62927	0.62191		
	0.60765						0.68875	15.065
115 1,2-Dibromoethane	+++++	0.76691	0.88801	0.67253	0.65651	0.65470		
	0.63435						0.71217	13.750
116 beta-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
117 Decane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
118 Diisobutyl Ketone	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
119 Alphasethylstyrene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
120 Dicyclopentadiene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
121 1,1,1,2-Tetrachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000		
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	% RSD
	200.000							
	Level 7							
122 D-Limonene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
124 Chlorobenzene	+++++	1.40231	1.40389	1.09599	1.09995	1.04079	1.17450	15.381
125 Bis(2-chloroethyl) ether	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
126 Nonane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
127 Ethyl Benzene	+++++	0.82062	0.74191	0.61784	0.60525	0.59030	0.65940	14.931
128 m,p-Xylene	+++++	1.04206	0.97220	0.79323	0.78399	0.76243	0.84792	14.971
129 Undecane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
130 o-Xylene	+++++	0.96930	1.00716	0.76148	0.74636	0.72189	0.81763	16.433
132 2-Heptanone	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
131 Styrene	1.69313	1.14679	1.49850	1.09415	1.11463	1.13886	1.25857	18.889

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
133 Bromoform	200.000	0.61756	0.64606	0.53857	0.55383	0.53227		0.56916	8.818
134 Cyclohexanone	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
135 Cumene	3.45662	2.66945	2.84554	2.18442	2.13966	2.10117		2.49512	20.937
136 1-chloro-2-Bromopropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
137 Bromobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
139 1,2,3-Trichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
140 Dodecane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
141 2-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
142 1,1,2,2-Tetrachloroethane	1.02790	1.37134	1.42089	1.07599	1.06692	1.06370		1.17112	15.006
143 Propylbenzene	2.23406	3.30360	3.36767	2.68855	2.64283	2.69125		2.82133	15.388

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
144 4-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
145 4-Ethyltoluene	+++++	2.88824	2.85962	2.34847	2.37703	2.39701		
	1.84102						2.45190	15.787
146 1,3,5-Trimethylbenzene	+++++	2.72711	3.06967	2.08844	2.05129	2.04889		
	1.93827						2.32061	19.960
147 2,6-Dimethyl-1-propanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
148 tert-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
149 Pentachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
150 sec-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
151 1,2,4-Trimethylbenzene	+++++	2.58151	2.58001	1.89703	1.87135	1.88091		
	1.79705						2.10131	17.749
152 p-Cymene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
153 1,2,3-Trimethylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
154 1,3-Dichlorobenzene	+++++	1.07365	0.96922	0.85086	0.88100	0.84628		
	0.85516						0.91270	10.000
155 1,4-Dichlorobenzene	+++++	1.44035	1.26100	1.03804	1.08377	1.16840		
	0.99164						1.16387	14.264
156 alpha-Chlorotoluene	+++++	1.83854	1.73296	1.52280	1.65167	1.67027		
	1.69415						1.68507	6.144
157 Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
158 1,2-Dichlorobenzene	+++++	1.26589	1.15974	0.89919	0.92239	0.88418		
	0.87873						1.00169	16.735
159 Hexachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
160 Aniline	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
161 1,2-Dibromo-3-Chloropropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
162 Isooctyl Alcohol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
163 1,2,4-Trichlorobenzene	+++++	+++++	0.72875	0.47508	0.58404	0.65031		
	0.68067						0.62377	15.759

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
164 Hexachlorobutadiene	+++++	+++++	1.22486	0.72372	0.69039	0.67531		0.79677	30.150 <-
165 Naphthalene	+++++	+++++	2.69108	1.63439	1.83942	2.02809		1.99311	20.828
166 1,2,3-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
167 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
168 Isooctyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
194 2-Methylpentane	+++++	+++++	2.44385	+++++	1.60008	+++++		1.84349	28.371
195 Thiopene	+++++	+++++	0.98460	+++++	0.65581	+++++		0.75748	26.014
196 Indan	+++++	+++++	2.66528	+++++	1.70640	+++++		2.03589	26.783
197 Indene	+++++	+++++	1.74642	+++++	1.09694	+++++		1.34222	26.277
\$ 80 1,2-Dichloroethane-d4	2.05787	2.08429	2.14741	2.23426	2.05489	2.18260		2.16099	5.197

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 22-MAR-2007 10:41
 End Cal Date : 26-MAR-2007 13:11
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-26mar.b/t14q322b.m
 Cal Date : 27-Mar-2007 06:43 sscott
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	RRF	% RSD
	200.000 Level 7							
\$ 102 Toluene-d8	0.99667	0.96945	0.94994	0.98725	0.97848	0.99102		
	1.00924						0.98315	1.972
\$ 138 Bromofluorobenzene	0.49812	0.46909	0.50906	0.51341	0.54503	0.52622		
	0.52541						0.51234	4.726

Calibration History

Method : /chem/msd8.i/8-26mar.b/t14q322b.m
Start Cal Date: 22-MAR-2007 10:41
End Cal Date : 26-MAR-2007 13:11

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.20000		
22-MAR-2007 10:41	AFCEElow	/chem/msd8.i/8-22mar.b/8032203.d
Cal Level: 2 , Cal Amount: 0.50000		
22-MAR-2007 17:30	ICALlevel2	/chem/msd8.i/8-22mar.b/8032215.d
Cal Level: 3 , Cal Amount: 2.00000		
26-MAR-2007 12:15	sp5b	/chem/msd8.i/8-26mar.b/8032606.d
22-MAR-2007 11:38	AT04mdl+Na+ENSR	/chem/msd8.i/8-22mar.b/8032205.d
Cal Level: 4 , Cal Amount: 25.00000		
22-MAR-2007 12:06	AT04+ENS	/chem/msd8.i/8-22mar.b/8032206.d
Cal Level: 5 , Cal Amount: 50.00000		
26-MAR-2007 12:43	sp5b	/chem/msd8.i/8-26mar.b/8032607.d
22-MAR-2007 12:34	AT04+ENS	/chem/msd8.i/8-22mar.b/8032207.d
Cal Level: 6 , Cal Amount: 100.00000		
22-MAR-2007 13:02	AT04+ENS	/chem/msd8.i/8-22mar.b/8032208.d
Cal Level: 7 , Cal Amount: 200.00000		
26-MAR-2007 13:11	sp5b	/chem/msd8.i/8-26mar.b/8032608.d
22-MAR-2007 13:30	AT04+ENS	/chem/msd8.i/8-22mar.b/8032209.d

Continuing Calibration
Ccal Level Mode: GLOBAL LEVEL 8

```
+-----+-----+-----+-----+-----+-----+-----+-----+-----+
| Ccal Level: 8 , Ccal Amount: 50.000                                     |
+-----+-----+-----+-----+-----+-----+-----+-----+-----+
| 26-MAR-2007 12:43 |sp5bccv                |/chem/msd8.i/8-26mar.b/8032607a.d      |
+-----+-----+-----+-----+-----+-----+-----+-----+-----+
```

@ Air Toxics Ltd.

ION ABUNDANCE CRITERIA

% REL. ABUNDANCE

MSD-8

Logbook #: 1478

m/z	REL. ABUNDANCE
50	15.0 - 40.0% of mass 95
75	30.0 - 60.0% of mass 95
95	Base peak, 100.00% relative abundance
96	5.0 - 9.0% of mass 95
173	Less than 2.0% of mass 174
174	Greater than 50.0% of mass 95
175	5.0 - 9.0% of mass 174
176	Greater than 95.0% but less than 101.0% of mass 174
177	5.0 - 9.0% of mass 176

¹ - value in parenthesis is % mass 174

² - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio: $675517/701792 \times 100 = 96.26$

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{Sample}}}{\text{Area}_{\text{IS}}} \times \text{Conc}_{\text{IS}} \times \text{RRF}$

$(1341361) \times (25) = (1370859) \times (0.98315) = 24.881$

Reported Result 24.881

File ID: 8032207
 Compound: Toluene-d8
 Initials: *[Signature]*

BFB Injection Date: 3/22/07
 BFB Injection Time: 0929
 BFB File ID: 8032201
 Tekmar Purge Flow: 14.8 mL/min
 Vacuum: 6.5e-6
 IS/Std #: 1443-3 Exp. Date: 5/24/07
 BCM: 283735
 1,4-DFB: 1370859
 CB-d5: 1067063
 Verified CCV IS vs ICAL mid-point (-40%D) *[Signature]*

NOAH Cart #: *NA* File #: *NA*

Use	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Loader Init.	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	8032201	BFB Tune check	843-174	50g	2 ml	1.0	T53	3-22-07	9:29	T53	
✓	02	Lab Blank	13673	Humid	200ml		<i>[Signature]</i>		1014	<i>[Signature]</i>	
✓	03	ICM (200ppb) Lvl 1	1487-115	0.2ppbv	0.2ml				1041	<i>[Signature]</i>	ES THQ3224
✓	04			Lvl 2	0.5				1110	<i>[Signature]</i>	
✓	05			Lvl 3	2				1138	<i>[Signature]</i>	
✓	06			Lvl 4	25				1206	<i>[Signature]</i>	
✓	07			Lvl 5	50				1234	<i>[Signature]</i>	
✓	08			Lvl 6	100				1302	<i>[Signature]</i>	
✓	09			Lvl 7	200				1330	<i>[Signature]</i>	

3/22/07 Date

10	X	8032210	Lab blank	13673	Humid	200ml	100	gpc	3/23/07	1359	gpc	-
11	X									1428	gpc	-
12	X									1456	gpc	-
13	X									1606	gpc	-
14	X									1702	gpc	-
15	✓		TCM (200gpc) Lvl 2	1487-115	0.5gpc	0.5ml				1730	gpc	-
16	✓		LS #1408-408	200gpc	50gpc	50ml				1819	gpc	-
17	X		Lab Blank	13673	Humid	second	100	gpc		1949	gpc	-
18	X		Lab Blank							2000	gpc	-
19	X		Lab Blank							2041	gpc	-
20	X		Lab Blank							2224	gpc	-
21												
22												
23												
24												
25												
26												
27												
28												
29												
30												
31												
32												

Comments: WST Flow meter SN: US05E27601 Flow Controller SN: AA9506172

Exp: 8/19/07 Actual: 22.4 ml/min Nominal: 25.5 ml/min

Signature [Signature]

Date 8/23/07

@ Air Toxics Ltd.

MSD-8

ION ABUNDANCE CRITERIA

m/z	REL. ABUNDANCE	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	29.0%
75	30.0 - 60.0% of mass 95	54.1%
95	Base peak; 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.4%
173	Less than 2.0% of mass 174	(0.10) ¹
174	Greater than 50.0% of mass 95	52.0%
175	5.0 - 9.0% of mass 174	(2.95) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(95.40) ¹
177	5.0 - 9.0% of mass 176	(6.53) ²

BFB Injection Date: 3/20/07 Logbook #: 1478
 BFB Injection Time: 09:05
 BFB File ID: 0032601
 Tekmar Purge Flow: 2.3/26/07 SA
 Vacuum:

IS/Std.#:	<u>1143-3</u>	Exp. Date:	<u>9/10/07</u>
BCM	<u>31809</u>		
1.4-DFB	<u>190342</u>		
CB-d5	<u>1370416</u>		

Verified CCV IS vs ICAL mid-point (-40%^D) E7D

Verify 176/174 m/z Ratio: $\frac{(1731969)}{(1020742)} \times \frac{(10.99315)}{(0.9540)}$ = 25

NOAH Cart #: 9/5 File #: F032308 / 1403267

File ID: 0032602

Compound: 161-d4

Initials: E7D

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{sample}}}{\text{Areas}} \times \text{Conc. is RRF} = \frac{(1731969)}{(1020742)} \times (0.99315) = 25$

Use	File #	Sample / Client Name	Can #	Pressure	Amnt Loaded	DF	Loader Init.	Date Analyzed	Time Analyzed	Review Init.	Comments
X	0032601	BFB TUNE CHECK	142-242	5.0ppv	2.0ML	1.10	E7D	3/20/07	1903	E7D	
	02	(UN-1 (200ppb))	147-307	5.0ppv	5.0ml		E7D		0932	E7D	NO Naps
	03	(US-1 (200ppb))	148-408	5.0ppv	5.0ml		E7D		1000	E7D	
	04	Gas Std (10ppm)	149-509	5.0ppv	5.0ml		E7D		1111	E7D	
	05	System blank	150-610	5.0ppv	2.0ml		E7D		1139	E7D	
X	06	ITL Level 3 (100ppb)	151-711	2.0ppv	2.0ml		E7D		1205	AS	SPS6
X	07	ITL Level 3 (100ppb)	152-812	5.0ppv	5.0ml		E7D		1243	AS	SPS6/SPS0A
X	08	ITL Level 3 (100ppb)	153-913	2.0ppv	2.0ml		E7D		1311	AS	
X	09	System blank	154-014	5.0ppv	2.0ml		E7D		1430	AS	

Initial Calibration Narrative for t14q322a.m

A seven-point initial calibration was analyzed on MSD-8 on March 22, 2007. As noted on the accompanying analytical run log(s), the following point (Level 2) was re-analyzed due to:

- a. anomalous unacceptable linearity for THF, trans-1,2-DCE, Bromomethane

The following compounds used 0.2 as the lowest calibration concentration:
Benzene, Chloroform, Styrene and Cumene.

Air Toxics Ltd.
 Modified EPA Methods TO-14A/TO-15
 Internal Standard and Associated Target Compounds and Surrogates

Bromochloromethane
Target Compounds:
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
3-Chloropropene
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
2,2,4-Trimethylpentane
Surrogates:
1,2-Dichloroethane-d4

1,4-Difluorobenzene
Target Compounds:
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
Surrogates:
Toluene-d8

Chlorobenzene-d5
Target Compounds:
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
Surrogates:
Bromofluorobenzene

Report Date: 23-Mar-2007 08:11

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032216.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 22-MAR-2007 18:19
 Operator : ej Inst ID: msd8.i
 Smp Info : 50mL #1408-408
 Misc Info : 200ppbv->50ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:11 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 13:30 Cal File: 8032209.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
		ON-COL		FINAL		TARGET RANGE		RATIO
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====

* 67	Bromochloromethane				CAS #: 74-97-5			
8.368	8.395 (1.000)	130	278522	25.0000		70.00- 130.00	100.00	
8.368	8.395 (1.000)	128	223686			46.35- 106.35	80.31	
8.368	8.395 (1.000)	49	840124			255.78- 315.78	301.64	

* 86	1,4-Difluorobenzene				CAS #: 540-36-3			
10.248	10.248 (1.000)	114	1372474	25.0000		70.00- 130.00	100.00	
10.248	10.248 (1.000)	88	244699			0.00- 48.88	17.83	

* 123	Chlorobenzene-d5				CAS #: 3114-55-4			
15.225	15.224 (1.000)	117	1036564	25.0000		70.00- 130.00	100.00	
15.197	15.224 (1.000)	82	689191			36.68- 96.68	66.49	

\$ 80	1,2-Dichloroethane-d4				CAS #: 17060-07-0			
9.446	9.473 (1.129)	65	612394	25.4366	25.436	70.00- 130.00	100.00	
9.446	9.473 (1.129)	67	348350			27.92- 87.92	56.88	

\$ 102	Toluene-d8				CAS #: 2037-26-5			
12.985	12.985 (1.267)	98	1319513	24.4472	24.447	70.00- 130.00	100.00	
12.985	12.985 (1.267)	70	167973			0.00- 42.61	12.73	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

\$ 102 Toluene-d8 (continued)

12.985 12.985 (1.267) 100 974319 40.27- 100.27 73.84

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.745 16.745 (1.100) 174 512983 24.1486 24.149 70.00- 130.00 100.00

16.745 16.745 (1.100) 95 994391 137.66- 197.66 193.84

16.745 16.745 (1.100) 176 500594 63.61- 123.61 97.58

3 Propylene

CAS #: 115-07-1

2.395 2.395 (0.286) 41 1876430 63.6731 63.673 70.00- 130.00 100.00

2.395 2.395 (0.286) 42 1242992 35.20- 95.20 66.24

2.395 2.395 (0.286) 39 1349895 42.80- 102.80 71.94

4 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.451 2.450 (0.293) 85 3599527 57.7849 57.785 70.00- 130.00 100.00

2.451 2.450 (0.293) 87 1162658 1.89- 61.89 32.30

6 Freon 114

CAS #: 76-14-2

2.589 2.616 (0.309) 135 1892311 53.5618 53.562 70.00- 130.00 100.00

2.589 2.616 (0.309) 137 615847 1.88- 61.88 32.54

8 Chloromethane

CAS #: 74-87-3

2.727 2.727 (0.326) 50 1778031 55.4796 55.480 70.00- 130.00 100.00

2.727 2.727 (0.326) 52 545218 0.00- 59.46 30.66

9 Butane

CAS #: 106-97-8

2.810 2.837 (0.336) 58 444668 53.3149 53.315 70.00- 130.00 100.00

2.810 2.837 (0.336) 43 3526100 772.78- 832.78 792.97

10 Vinyl Chloride

CAS #: 75-01-4

2.893 2.893 (0.346) 62 1691484 56.1894 56.189 70.00- 130.00 100.00

2.893 2.893 (0.346) 64 497353 0.33- 60.33 29.40

11 1,3-Butadiene

CAS #: 106-99-0

2.893 2.920 (0.346) 54 1615957 51.7656 51.766 70.00- 130.00 100.00

2.893 2.920 (0.346) 39 1828365 86.60- 146.60 113.14

13 Bromomethane

CAS #: 74-83-9

3.418 3.446 (0.408) 94 924272 56.1665 56.166 70.00- 130.00 100.00

3.418 3.446 (0.408) 96 853544 64.77- 124.77 92.35

15 Isopentane

CAS #: 78-78-4

3.529 3.556 (0.422) 43 2709546 52.6071 52.607 70.00- 130.00 100.00

3.529 3.556 (0.422) 57 1581385 27.51- 87.51 58.36

3.529 3.556 (0.422) 72 171194 0.00- 35.95 6.32

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

16 Chloroethane CAS #: 75-00-3
 3.557 3.612 (0.425) 64 887054 56.5863 56.586 70.00- 130.00 100.00
 3.557 3.612 (0.425) 49 272964 2.42- 62.42 30.77
 3.557 3.612 (0.425) 66 261670 0.00- 58.92 29.50

18 Trichlorofluoromethane/Fr11 CAS #: 75-69-4
 3.888 3.916 (0.465) 101 2978271 53.3780 53.378 70.00- 130.00 100.00
 3.888 3.916 (0.465) 103 1900616 34.71- 94.71 63.82

21 Ethanol CAS #: 64-17-5
 4.275 4.331 (0.511) 45 661304 52.2111 52.211 70.00- 130.00 100.00
 4.275 4.331 (0.511) 43 132468 0.00- 50.43 20.03
 4.248 4.331 (0.508) 46 280779 12.21- 72.21 42.46

27 Freon 113 CAS #: 76-13-1
 4.718 4.745 (0.564) 151 1414844 53.5490 53.549 70.00- 130.00 100.00
 4.718 4.745 (0.564) 153 905176 32.67- 92.67 63.98
 4.718 4.745 (0.564) 101 2268866 124.83- 184.83 160.36

29 1,1-Dichloroethene CAS #: 75-35-4
 4.773 4.801 (0.570) 61 2448396 54.4406 54.440 70.00- 130.00 100.00
 4.773 4.801 (0.570) 96 1111548 15.10- 75.10 45.40
 4.773 4.801 (0.570) 98 688548 0.00- 58.17 28.12

30 Acetone CAS #: 67-64-1
 4.939 4.939 (0.590) 58 832492 51.7567 51.757 70.00- 130.00 100.00
 4.939 4.939 (0.590) 43 3109773 337.35- 397.35 373.55

33 Carbon Disulfide CAS #: 75-15-0
 5.133 5.160 (0.613) 76 3456368 49.8938 49.894 70.00- 130.00 100.00

34 2-Propanol CAS #: 67-63-0
 5.133 5.160 (0.613) 45 3220225 51.1002 51.100 70.00- 130.00 100.00
 5.133 5.160 (0.613) 43 622351 0.00- 50.64 19.33
 5.133 5.160 (0.613) 59 109991 0.00- 33.21 3.42

37 3-Chloropropene CAS #: 107-05-1
 5.437 5.437 (0.650) 76 582413 52.0618 52.062 70.00- 130.00 100.00
 5.437 5.437 (0.650) 41 2574669 414.53- 474.53 442.07

39 Methylene Chloride CAS #: 75-09-2
 5.686 5.713 (0.679) 49 1928181 50.4149 50.415 70.00- 130.00 100.00
 5.686 5.713 (0.679) 84 959383 18.44- 78.44 49.76
 5.686 5.713 (0.679) 51 576250 0.00- 59.93 29.89

42 MTBE CAS #: 1634-04-4
 6.045 6.045 (0.722) 73 3752786 48.6776 48.678 70.00- 130.00 100.00

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.045	6.045	(0.722)	57	1080934			0.00- 59.33	28.80	
6.045	6.045	(0.722)	41	1183273			1.95- 61.95	31.53	

43 trans-1,2-Dichloroethene					CAS #: 156-60-5				
6.100	6.100	(0.729)	96	1090503	47.4477	47.448	70.00- 130.00	100.00	
6.073	6.100	(0.726)	61	2105343			169.97- 229.97	193.06	
6.100	6.100	(0.729)	98	673150			34.71- 94.71	61.73	

45 Hexane					CAS #: 110-54-3				
6.432	6.432	(0.769)	57	2673909	47.2636	47.264	70.00- 130.00	100.00	
6.432	6.432	(0.769)	43	1951618			44.61- 104.61	72.99	
6.432	6.432	(0.769)	86	377558			0.00- 43.77	14.12	

52 1,1-Dichloroethane					CAS #: 75-34-3				
6.874	6.902	(0.822)	63	2404587	50.3224	50.322	70.00- 130.00	100.00	
6.874	6.902	(0.822)	65	709306			0.00- 59.58	29.50	

54 Vinyl Acetate					CAS #: 108-05-4				
6.957	6.957	(0.831)	86	303994	53.4836	53.484	70.00- 130.00	100.00	
6.957	6.957	(0.831)	43	4738804			1469.62-1529.62	1558.85	
6.957	6.957	(0.831)	42	407364			100.08- 160.08	134.00	

63 cis-1,2-Dichloroethene					CAS #: 156-59-2				
7.925	7.953	(0.947)	61	1766344	48.5859	48.586	70.00- 130.00	100.00	
7.925	7.953	(0.947)	96	996178			27.36- 87.36	56.40	
7.925	7.953	(0.947)	98	603006			5.83- 65.83	34.14	

64 2-Butanone					CAS #: 78-93-3				
7.980	7.980	(0.954)	72	564657	43.2924	43.292	70.00- 130.00	100.00	
7.980	7.980	(0.954)	43	3472194			574.29- 634.29	614.92	
7.980	7.980	(0.954)	57	225366			10.61- 70.61	39.91	

66 Tetrahydrofuran					CAS #: 109-99-9				
8.368	8.367	(1.000)	42	2017236	41.5387	41.539	70.00- 130.00	100.00	
8.368	8.367	(1.000)	71	508113			0.00- 54.93	25.19	
8.368	8.367	(1.000)	72	558622			0.00- 56.52	27.69	

69 Chloroform					CAS #: 67-66-3				
8.506	8.506	(1.017)	83	1925190	42.0342	42.034	70.00- 130.00	100.00	
8.506	8.506	(1.017)	85	1250807			33.71- 93.71	64.97	

72 Cyclohexane					CAS #: 110-82-7				
8.727	8.727	(1.043)	84	1538360	45.0602	45.060	70.00- 130.00	100.00	
8.727	8.727	(1.043)	56	2601694			138.68- 198.68	169.12	
8.727	8.727	(1.043)	41	1546180			73.81- 133.81	100.51	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

73	1,1,1-Trichloroethane					CAS #:	71-55-6			
8.755	8.754	(1.046)	97	1902106	45.9990	45.999	70.00-	130.00	100.00	
8.755	8.754	(1.046)	99	1246434			33.95-	93.95	65.53	

75	Carbon Tetrachloride					CAS #:	56-23-5			
8.976	9.003	(1.073)	119	1575718	47.1772	47.177	70.00-	130.00	100.00	
8.976	9.003	(1.073)	117	1744559			81.67-	141.67	110.72	

78	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.418	9.446	(1.126)	57	7315932	45.9263	45.926	70.00-	130.00	100.00	
9.418	9.446	(1.126)	56	2562625			4.45-	64.45	35.03	
9.418	9.446	(1.126)	41	2159630			0.00-	59.44	29.52	

79	Benzene					CAS #:	71-43-2			
9.418	9.418	(0.919)	78	3340948	43.7066	43.706	70.00-	130.00	100.00	
9.418	9.418	(0.919)	77	774792			0.00-	54.39	23.19	

81	1,2-Dichloroethane					CAS #:	107-06-2			
9.612	9.612	(0.938)	62	1669206	46.6289	46.629	70.00-	130.00	100.00	
9.612	9.612	(0.938)	64	507016			1.44-	61.44	30.37	

82	Heptane					CAS #:	142-82-5			
9.805	9.805	(0.957)	100	377747	41.3701	41.370	70.00-	130.00	100.00	
9.805	9.805	(0.957)	43	3122573			789.66-	849.66	826.63	
9.805	9.805	(0.957)	71	1222459			294.27-	354.27	323.62	

92	Trichloroethene					CAS #:	79-01-6			
10.662	10.662	(1.040)	95	1155008	46.9757	46.976	70.00-	130.00	100.00	
10.662	10.662	(1.040)	130	960049			57.13-	117.13	83.12	
10.662	10.662	(1.040)	97	737325			32.50-	92.50	63.84	

93	Methyl Cyclohexane					CAS #:	108-87-2			
10.884	10.883	(1.301)	83	1922839	45.0279	45.028	70.00-	130.00	100.00	
10.884	10.883	(1.301)	98	908713			15.00-	75.00	47.26	
10.884	10.883	(1.301)	55	2207231			87.18-	147.18	114.79	

95	1,2-Dichloropropane					CAS #:	78-87-5			
11.188	11.188	(1.092)	63	1250358	44.6373	44.637	70.00-	130.00	100.00	
11.188	11.188	(1.092)	62	934234			45.03-	105.03	74.72	
11.188	11.188	(1.092)	41	962531			45.52-	105.52	76.98	

96	1,4-Dioxane					CAS #:	123-91-1			
11.409	11.409	(1.113)	88	645482	44.2024	44.202	70.00-	130.00	100.00	
11.409	11.409	(1.113)	58	619887			70.27-	130.27	96.03	
11.409	11.409	(1.113)	57	198043			0.54-	60.54	30.68	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.713	11.741	(1.143)	83	1880847	45.4089	45.409	70.00- 130.00	100.00	
11.713	11.741	(1.143)	85	1201006			32.38- 92.38	63.85	

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.598	12.625	(1.229)	75	1654311	46.8298	46.830	70.00- 130.00	100.00	
12.598	12.625	(1.229)	77	523109			1.52- 61.52	31.62	
12.598	12.625	(1.229)	39	1241394			48.26- 108.26	75.04	

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.259)	58	1256304	44.1080	44.108	70.00- 130.00	100.00	
12.902	12.902	(1.259)	43	3592445			251.14- 311.14	285.95	
12.902	12.902	(1.259)	85	387104			2.33- 62.33	30.81	

103 Toluene						CAS #: 108-88-3			
13.096	13.095	(1.278)	91	3428164	49.5296	49.530	70.00- 130.00	100.00	
13.096	13.095	(1.278)	92	2053740			29.45- 89.45	59.91	

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	1733104	47.9456	47.946	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	544880			1.42- 61.42	31.44	
13.621	13.621	(0.895)	39	1268743			43.57- 103.57	73.21	

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.870	13.870	(0.911)	97	953253	45.2979	45.298	70.00- 130.00	100.00	
13.870	13.870	(0.911)	99	587815			31.40- 91.40	61.66	
13.870	13.870	(0.911)	83	899793			60.06- 120.06	94.39	

109 Tetrachloroethene						CAS #: 127-18-4			
13.925	13.925	(0.915)	166	1075635	48.1240	48.124	70.00- 130.00	100.00	
13.925	13.925	(0.915)	129	859308			46.36- 106.36	79.89	
13.925	13.925	(0.915)	131	824537			45.00- 105.00	76.66	

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	1547930	46.6060	46.606	70.00- 130.00	100.00	
14.257	14.257	(0.936)	43	3177061			176.52- 236.52	205.25	
14.257	14.257	(0.936)	100	239749			0.00- 45.68	15.49	

114 Dibromochloromethane						CAS #: 124-48-1			
14.423	14.423	(0.947)	129	1351154	47.3140	47.314	70.00- 130.00	100.00	
14.423	14.423	(0.947)	127	1074573			46.96- 106.96	79.53	

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.589	14.588	(0.958)	107	1439089	48.7359	48.736	70.00- 130.00	100.00	
14.589	14.588	(0.958)	109	1320391			62.88- 122.88	91.75	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
124 Chlorobenzene						CAS #: 108-90-7				
15.252	15.252	(1.002)	112	2364677	48.5581	48.558	70.00- 130.00	100.00		
15.252	15.252	(1.002)	114	723136			0.73- 60.73	30.58		
15.252	15.252	(1.002)	77	1645570			40.58- 100.58	69.59		

127 Ethyl Benzene						CAS #: 100-41-4				
15.363	15.363	(1.009)	106	1311932	47.9853	47.985	70.00- 130.00	100.00		
15.363	15.363	(1.009)	91	4511338			309.90- 369.90	343.87		

128 m,p-Xylene						CAS #: 108-38-3				
15.529	15.529	(1.020)	106	1672409	47.5696	47.570	70.00- 130.00	100.00		
15.529	15.529	(1.020)	91	3565698			177.38- 237.38	213.21		

130 o-Xylene						CAS #: 95-47-6				
16.054	16.054	(1.054)	106	1625053	47.9353	47.935	70.00- 130.00	100.00		
16.054	16.054	(1.054)	91	3693663			195.99- 255.99	227.29		

131 Styrene						CAS #: 100-42-5				
16.082	16.082	(1.056)	104	2458659	47.1155	47.115	70.00- 130.00	100.00		
16.082	16.082	(1.056)	78	1484068			28.78- 88.78	60.36		

133 Bromoform						CAS #: 75-25-2				
16.358	16.358	(1.074)	173	1107122	46.9144	46.914	70.00- 130.00	100.00		
16.358	16.358	(1.074)	171	566742			21.17- 81.17	51.19		

135 Cumene						CAS #: 98-82-8				
16.524	16.524	(1.085)	105	4785876	46.2609	46.261	70.00- 130.00	100.00		
16.524	16.524	(1.085)	120	1083750			0.00- 53.14	22.64		
16.496	16.524	(1.084)	51	737073			0.00- 45.39	15.40		

142 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5				
16.966	16.966	(1.114)	83	2314942	47.6739	47.674	70.00- 130.00	100.00		
16.966	16.966	(1.114)	85	1479700			34.35- 94.35	63.92		

143 Propylbenzene						CAS #: 103-65-1				
16.994	16.994	(1.116)	91	6112597	52.2536	52.254	70.00- 130.00	100.00		
16.994	16.994	(1.116)	120	1134482			0.00- 48.79	18.56		
16.994	16.994	(1.116)	105	209533			0.00- 33.35	3.43		

145 4-Ethyltoluene						CAS #: 622-96-8				
17.132	17.132	(1.125)	105	5307532	52.2076	52.208	70.00- 130.00	100.00		
17.132	17.132	(1.125)	120	1325326			0.00- 54.57	24.97		

146 1,3,5-Trimethylbenzene						CAS #: 108-67-8				
17.215	17.215	(1.131)	105	4361594	45.3301	45.330	70.00- 130.00	100.00		
17.215	17.215	(1.131)	120	1879411			12.64- 72.64	43.09		

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	ON-COL		FINAL	TARGET RANGE	RATIO	
				RESPONSE	(PPEV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

151	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
17.602	17.602	(1.156)	105	4025096	46.1987	46.199	70.00- 130.00	100.00	
17.602	17.602	(1.156)	120	1666459			11.41- 71.41	41.40	

154	1,3-Dichlorobenzene					CAS #: 541-73-1			
17.907	17.906	(1.176)	146	1763512	46.6011	46.601	70.00- 130.00	100.00	
17.907	17.906	(1.176)	148	1109821			32.20- 92.20	62.93	
17.879	17.906	(1.174)	111	831855			13.28- 73.28	47.17	

155	1,4-Dichlorobenzene					CAS #: 106-46-7			
17.990	17.989	(1.182)	146	2412413	49.9911	49.991	70.00- 130.00	100.00	
17.990	17.989	(1.182)	148	1546218			34.16- 94.16	64.09	
17.990	17.989	(1.182)	111	1088761			16.41- 76.41	45.13	

156	alpha-Chlorotoluene					CAS #: 100-44-7			
18.128	18.128	(1.191)	91	3406668	48.7592	48.759	70.00- 130.00	100.00	
18.128	18.128	(1.191)	126	594643			0.00- 46.97	17.46	

158	1,2-Dichlorobenzene					CAS #: 95-50-1			
18.321	18.321	(1.203)	146	1870369	45.0339	45.034	70.00- 130.00	100.00	
18.321	18.321	(1.203)	148	1179854			33.83- 93.83	63.08	
18.321	18.321	(1.203)	111	1039079			21.29- 81.29	55.55	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.593	19.593	(1.287)	180	1227104	47.4461	47.446	70.00- 130.00	100.00	
19.593	19.593	(1.287)	182	1149823			62.06- 122.06	93.70	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.676	19.676	(1.292)	225	1408481	42.6344	42.634	70.00- 130.00	100.00	
19.676	19.676	(1.292)	223	915348			35.92- 95.92	64.99	

165	Naphthalene					CAS #: 91-20-3			
19.787	19.787	(1.300)	128	5855301	70.8537	70.854	70.00- 130.00	100.00(R)	
19.787	19.787	(1.300)	127	815433			0.00- 43.72	13.93	

QC Flag Legend

R - Spike/Surrogate failed recovery limits.

Report Date: 23-Mar-2007 08:11

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032216.d

Calibration Time: 12:34

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ej

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv->50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	278522	-1.84
86 1,4-Difluorobenze	1370859	822515	1919203	1372474	0.12
123 Chlorobenzene-d5	1067063	640238	1493888	1036564	-2.86

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.37	-0.33
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT


Client Name: Client SDG: 8-22mar
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: ej
 Data Type: MS DATA SampleType: LCS
 SpikeList File: Spectra+ENS.spk Quant Type: ISTD
 Sublist File: AT04+ENS.sub
 Method File: /chem/msd8.i/8-22mar.b/t14q322a.m
 Misc Info: 200ppbv->50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
131 Styrene	50.000	47.115	94.23	70-130
106 trans-1,3-Dichloro	50.000	47.946	95.89	70-130
4 Dichlorodifluorome	50.000	57.785	115.57	70-130
6 Freon 114	50.000	53.562	107.12	70-130
8 Chloromethane	50.000	55.480	110.96	70-130
10 Vinyl Chloride	50.000	56.189	112.38	70-130
11 1,3-Butadiene	50.000	51.766	103.53	60-140
13 Bromomethane	50.000	56.166	112.33	70-130
16 Chloroethane	50.000	56.586	113.17	70-130
18 Trichlorofluoromet	50.000	53.378	106.76	70-130
21 Ethanol	50.000	52.211	104.42	60-140
27 Freon 113	50.000	53.549	107.10	70-130
29 1,1-Dichloroethene	50.000	54.440	108.88	70-130
30 Acetone	50.000	51.757	103.51	60-140
33 Carbon Disulfide	50.000	49.894	99.79	60-140
34 2-Propanol	50.000	51.100	102.20	60-140
39 Methylene Chloride	50.000	50.415	100.83	70-130
42 MTBE	50.000	48.678	97.36	60-140
43 trans-1,2-Dichloro	50.000	47.448	94.90	60-140
45 Hexane	50.000	47.264	94.53	60-140
52 1,1-Dichloroethane	50.000	50.322	100.64	70-130
63 cis-1,2-Dichloroet	50.000	48.586	97.17	70-130
64 2-Butanone	50.000	43.292	86.58	60-140
66 Tetrahydrofuran	50.000	41.539	83.08	60-140
69 Chloroform	50.000	42.034	84.07	70-130
72 Cyclohexane	50.000	45.060	90.12	60-140
73 1,1,1-Trichloroeth	50.000	45.999	92.00	70-130
75 Carbon Tetrachlori	50.000	47.177	94.35	70-130
79 Benzene	50.000	43.706	87.41	70-130
81 1,2-Dichloroethane	50.000	46.629	93.26	70-130
82 Heptane	50.000	41.370	82.74	60-140
92 Trichloroethene	50.000	46.976	93.95	70-130
95 1,2-Dichloropropan	50.000	44.637	89.27	70-130

Report Date: 23-Mar-2007 08:11

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
96 1,4-Dioxane	50.000	44.202	88.40	60-140
98 Bromodichlorometha	50.000	45.409	90.82	60-140
100 cis-1,3-Dichloropr	50.000	46.830	93.66	70-130
101 4-Methyl-2-pentano	50.000	44.108	88.22	60-140
103 Toluene	50.000	49.530	99.06	70-130
108 1,1,2-Trichloroeth	50.000	45.298	90.60	70-130
109 Tetrachloroethene	50.000	48.124	96.25	70-130
112 2-Hexanone	50.000	46.606	93.21	60-140
114 Dibromochlorometha	50.000	47.314	94.63	60-140
115 1,2-Dibromoethane	50.000	48.736	97.47	70-130
124 Chlorobenzene	50.000	48.558	97.12	70-130
127 Ethyl Benzene	50.000	47.985	95.97	70-130
128 m,p-Xylene	50.000	47.570	95.14	70-130
130 o-Xylene	50.000	47.935	95.87	70-130
133 Bromoform	50.000	46.914	93.83	60-140
142 1,1,2,2-Tetrachlor	50.000	47.674	95.35	70-130
145 4-Ethyltoluene	50.000	52.208	104.42	60-140
146 1,3,5-Trimethylben	50.000	45.330	90.66	70-130
151 1,2,4-Trimethylben	50.000	46.199	92.40	70-130
154 1,3-Dichlorobenzen	50.000	46.601	93.20	70-130
155 1,4-Dichlorobenzen	50.000	49.991	99.98	70-130
156 alpha-Chlorotoluen	50.000	48.759	97.52	70-130
158 1,2-Dichlorobenzen	50.000	45.034	90.07	70-130
163 1,2,4-Trichloroben	50.000	47.446	94.89	70-130
164 Hexachlorobutadien	50.000	42.634	85.27	70-130
135 Cumene	50.000	46.261	92.52	60-140
143 Propylbenzene	50.000	52.254	104.51	60-140
37 3-Chloropropene	50.000	52.062	104.12	60-140
78 2,2,4-Trimethylpen	50.000	45.926	91.85	60-140
9 Butane	50.000	53.315	106.63	70-130
15 Isopentane	50.000	52.607	105.21	70-130
93 Methyl Cyclohexane	50.000	45.028	90.06	70-130
165 Naphthalene	50.000	70.854	141.71*	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	25.436	101.75	70-130
\$ 102 Toluene-d8	25.000	24.447	97.79	70-130
\$ 138 Bromofluorobenzene	25.000	24.149	96.59	70-130

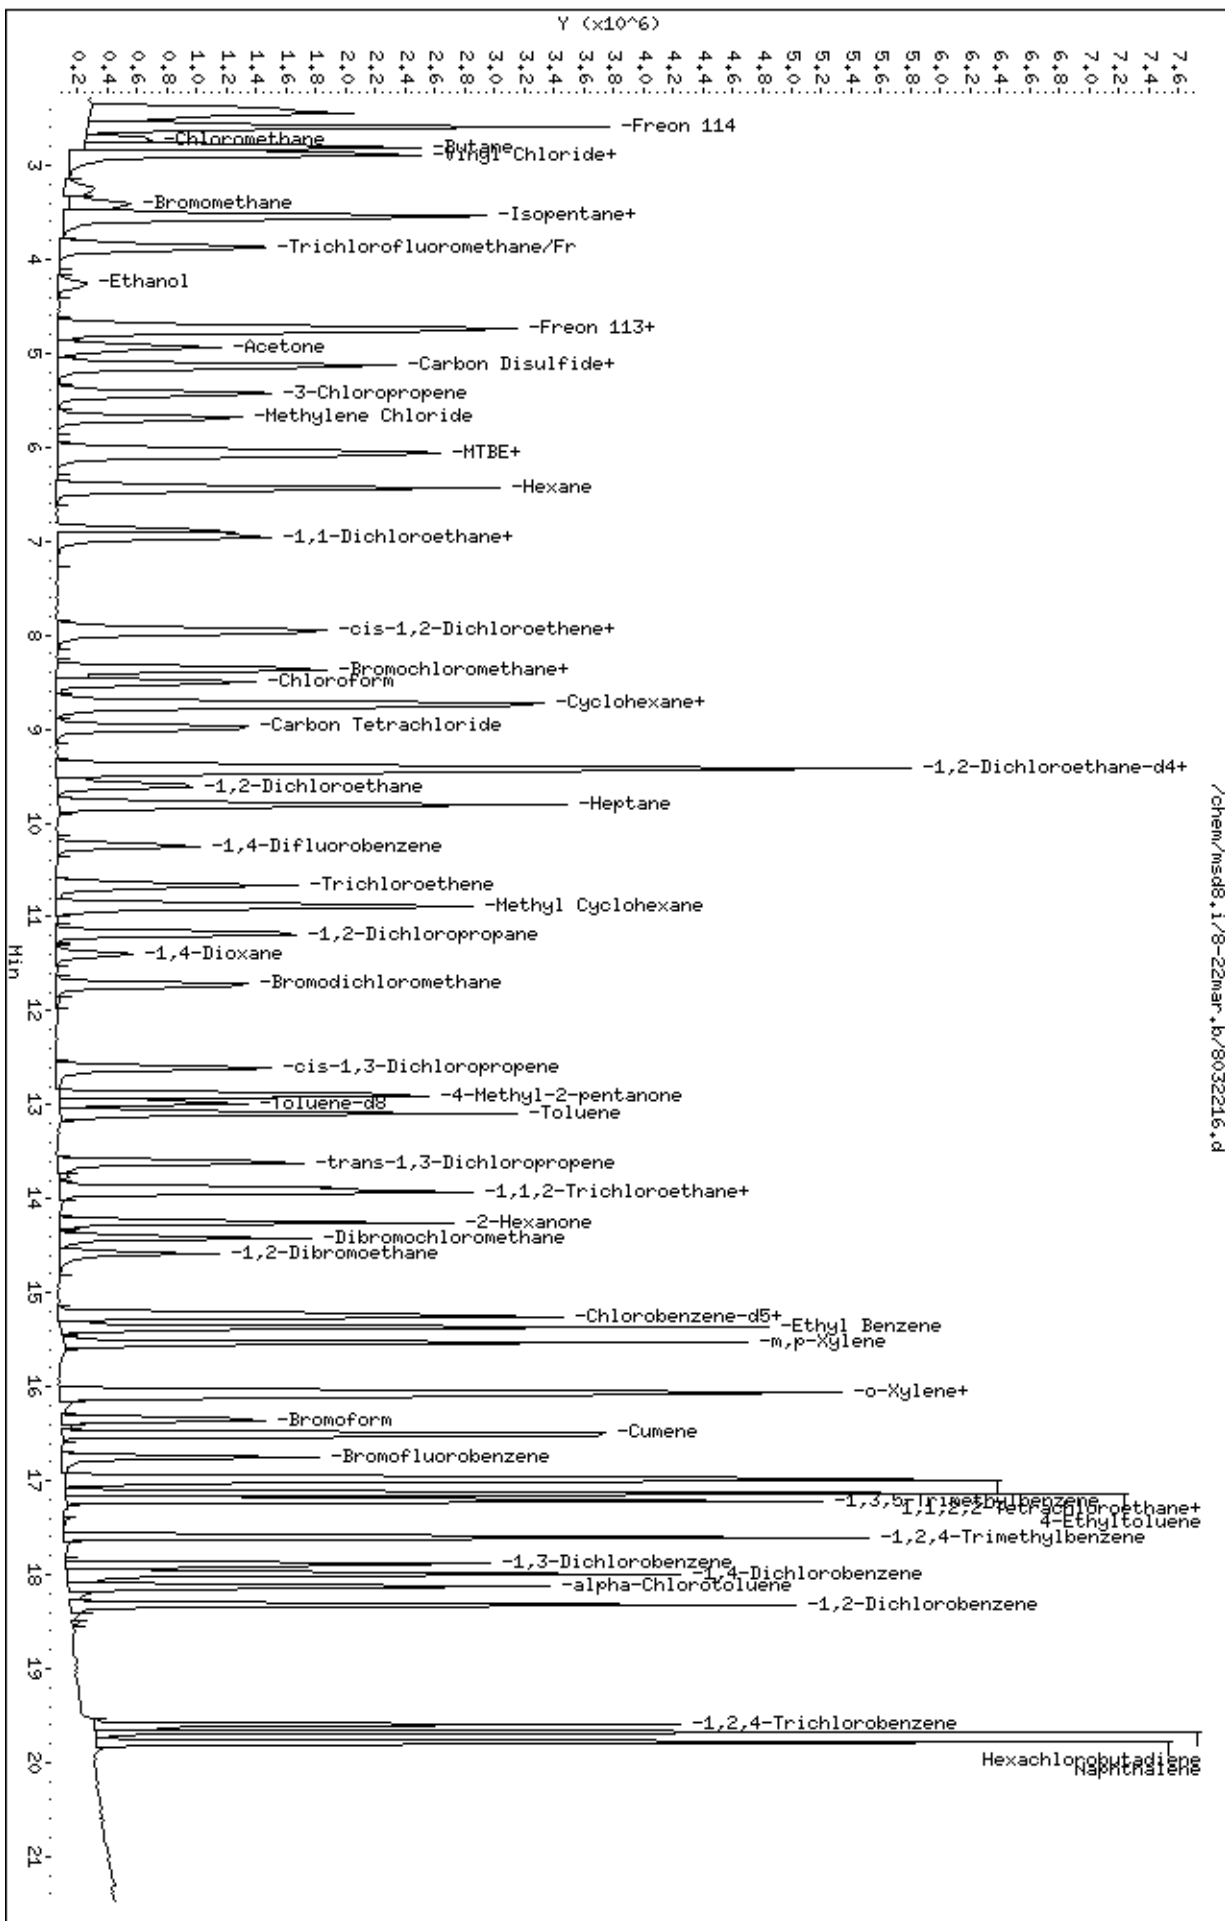

/chem/msd8.1/8-22mar.lb/8032216.d

Report Date: 23-Mar-2007 08:08

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032203.d
 Lab Smp Id: ICAL Client Smp ID: Level 1
 Inj Date : 22-MAR-2007 10:41
 Operator : sjr Inst ID: msd8.i
 Smp Info : 0.2ml 1487-115
 Misc Info : 200ppbv -> 0.2ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:08 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 10:41 Cal File: 8032203.d
 Als bottle: 1 Calibration Sample, Level: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AFCEElow.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

* 67	Bromochloromethane			CAS #: 74-97-5					
8.395	8.395	(1.000)	130	285447	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	222762			46.35- 106.35	78.04	
8.395	8.395	(1.000)	49	841026			255.78- 315.78	294.63	

* 86	1,4-Difluorobenzene			CAS #: 540-36-3					
10.248	10.248	(1.000)	114	1360758	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	259943			0.00- 48.88	19.10	

* 123	Chlorobenzene-d5			CAS #: 3114-55-4					
15.224	15.224	(1.000)	117	1082018	25.0000		70.00- 130.00	100.00	
15.224	15.224	(1.000)	82	726655			0.00- 30.00	67.16	

\$ 80	1,2-Dichloroethane-d4			CAS #: 17060-07-0					
9.473	9.473	(1.128)	65	587414	25.0000	25.018	70.00- 130.00	100.00	
9.473	9.473	(1.128)	67	292096			0.00- 30.00	49.73	

\$ 102	Toluene-d8			CAS #: 2037-26-5					
12.985	12.985	(1.267)	98	1356224	25.0000	25.230	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	172342			0.00- 30.00	12.71	

AMOUNTS											
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO			
==	=====	=====	=====	=====	=====	=====	=====	=====			

\$ 102 Toluene-d8 (continued)											
12.985	12.985	(1.267)	100	890926			0.00- 30.00	65.69			

\$ 138 Bromofluorobenzene											
						CAS #: 460-00-4					
16.773	16.773	(1.102)	174	538970	25.0000	23.876	70.00- 130.00	100.00			
16.745	16.745	(1.100)	95	902384			137.66- 197.66	167.43			
16.773	16.773	(1.102)	176	528806			63.61- 123.61	98.11			

69 Chloroform											
						CAS #: 67-66-3					
8.506	8.506	(1.013)	83	14108	0.20000	0.2628	70.00- 130.00	100.00(a)			
8.533	8.533	(1.016)	85	9243			33.71- 93.71	65.52			

79 Benzene											
						CAS #: 71-43-2					
9.418	9.418	(0.919)	78	22113	0.20000	0.2542	70.00- 130.00	100.00(a)			
9.418	9.418	(0.919)	77	8130			0.00- 30.00	36.77			

131 Styrene											
						CAS #: 100-42-5					
16.109	16.109	(1.058)	104	14656	0.20000	0.2412	70.00- 130.00	100.00(a)			
16.082	16.082	(1.056)	78	11399			28.78- 88.78	77.78			

135 Cumene											
						CAS #: 98-82-8					
16.524	16.524	(1.085)	105	29921	0.20000	0.2471	70.00- 130.00	100.00(a)			
16.524	16.524	(1.085)	120	6949			0.00- 30.00	23.22			
16.496	16.496	(1.084)	51	6483			0.00- 30.00	21.67			

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 23-Mar-2007 08:08

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032203.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv -> 0.2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	285447	0.60
86 1,4-Difluorobenze	1370859	822515	1919203	1360758	-0.74
123 Chlorobenzene-d5	1067063	640238	1493888	1082018	1.40

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22mar.lb/8032203.d

Date : 22-MAR-2007 10:41

Client ID: Level 1


Sample Info: 0.2ml 1487-115

Column phase: RTX-624

Instrument: msd8.1

Operator: sjr

Column diameter: 0.53



Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032215.d
 Lab Smp Id: ICAL Client Smp ID: Level 2
 Inj Date : 22-MAR-2007 17:30
 Operator : sjr Inst ID: msd8.i
 Smp Info : 0.5ml 1487-115
 Misc Info : 200ppbv -> 0.5ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:09 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 17:30 Cal File: 8032215.d
 Als bottle: 1 Calibration Sample, Level: 2
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: ICALlevel2.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	270806	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	205077			46.35- 106.35	75.73	
8.367	8.367	(1.000)	49	794498			255.78- 315.78	293.38	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1311826	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	240488			0.00- 48.88	18.33	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225	(1.000)	117	1039819	25.0000		70.00- 130.00	100.00	
15.197	15.197	(1.000)	82	701224			0.00- 30.00	67.44	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.473	(1.128)	65	564438	25.0000	25.225	70.00- 130.00	100.00	
9.473	9.473	(1.128)	67	303193			0.00- 30.00	53.72	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	1271754	25.0000	24.692	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	162520			0.00- 30.00	12.78	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 102 Toluene-d8 (continued)										
12.985	12.985	(1.267)	100	881454			0.00- 30.00	69.31		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.773	16.773	(1.102)	174	487769	25.0000	23.265	70.00- 130.00	100.00		
16.745	16.745	(1.100)	95	897698			137.66- 197.66	184.04		
16.773	16.773	(1.102)	176	495471			63.61- 123.61	101.58		

4 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.450	2.450	(0.292)	85	42030	0.50000	0.6249	70.00- 130.00	100.00		
2.478	2.478	(0.295)	87	13507			0.00- 30.00	32.14		

6 Freon 114										
						CAS #: 76-14-2				
2.616	2.616	(0.312)	135	22788	0.50000	0.6009	70.00- 130.00	100.00		
2.644	2.644	(0.315)	137	8952			1.88- 61.88	39.28		

10 Vinyl Chloride										
						CAS #: 75-01-4				
2.921	2.921	(0.348)	62	16055	0.50000	0.5515	70.00- 130.00	100.00		
2.893	2.893	(0.345)	64	2845			0.00- 30.00	17.72		

11 1,3-Butadiene										
						CAS #: 106-99-0				
2.893	2.893	(0.345)	54	18194	0.50000	0.5819	70.00- 130.00	100.00		
2.893	2.893	(0.345)	39	71814			0.00- 30.00	394.71		

13 Bromomethane										
						CAS #: 74-83-9				
3.446	3.446	(0.410)	94	11062	0.50000	0.6255	70.00- 130.00	100.00		
3.418	3.418	(0.407)	96	21718			64.77- 124.77	196.33		

16 Chloroethane										
						CAS #: 75-00-3				
3.584	3.584	(0.427)	64	9404	0.50000	0.5914	70.00- 130.00	100.00		
3.612	3.612	(0.430)	49	4248			0.00- 30.00	45.17		
3.695	3.695	(0.440)	66	2350			0.00- 30.00	24.99		

18 Trichlorofluoromethane/Fr11										
						CAS #: 75-69-4				
3.916	3.916	(0.466)	101	29095	0.50000	0.5434	70.00- 130.00	100.00		
3.916	3.916	(0.466)	103	24541			34.71- 94.71	84.35		

27 Freon 113										
						CAS #: 76-13-1				
4.745	4.745	(0.565)	151	15286	0.50000	0.5812	70.00- 130.00	100.00		
4.745	4.745	(0.565)	153	10476			32.67- 92.67	68.53		
4.745	4.745	(0.565)	101	25478			124.83- 184.83	166.68		

29 1,1-Dichloroethene										
						CAS #: 75-35-4				
4.773	4.773	(0.569)	61	28480	0.50000	0.6054	70.00- 130.00	100.00		
4.801	4.801	(0.572)	96	16319			15.10- 75.10	57.30		
4.773	4.773	(0.569)	98	11574			0.00- 58.17	40.64		

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

33	Carbon Disulfide					CAS #:	75-15-0			
5.160	5.160	(0.615)	76	43108	0.50000	0.5958	70.00-	130.00	100.00	

39	Methylene Chloride					CAS #:	75-09-2			
5.713	5.713	(0.681)	49	24563	0.50000	0.6098	70.00-	130.00	100.00	
5.713	5.713	(0.681)	84	13379			18.44-	78.44	54.47	
5.713	5.713	(0.681)	51	6981			0.00-	30.00	28.42	

42	MTBE					CAS #:	1634-04-4			
6.045	6.045	(0.720)	73	47973	0.50000	0.5988	70.00-	130.00	100.00	
6.045	6.045	(0.720)	57	13535			0.00-	59.33	28.21	
6.045	6.045	(0.720)	41	17986			0.00-	30.00	37.49	

43	trans-1,2-Dichloroethene					CAS #:	156-60-5			
6.100	6.100	(0.727)	96	15974	0.50000	0.6337	70.00-	130.00	100.00	
6.100	6.100	(0.727)	61	28116			169.97-	229.97	176.01	
6.100	6.100	(0.727)	98	12293			0.00-	30.00	76.96	

45	Hexane					CAS #:	110-54-3			
6.460	6.460	(0.769)	57	35245	0.50000	0.5968	70.00-	130.00	100.00	
6.432	6.432	(0.766)	43	24536			0.00-	30.00	69.62	
6.460	6.460	(0.769)	86	5992			0.00-	30.00	17.00	

52	1,1-Dichloroethane					CAS #:	75-34-3			
6.902	6.902	(0.822)	63	28073	0.50000	0.5719	70.00-	130.00	100.00	
6.902	6.902	(0.822)	65	12707			0.00-	59.58	45.26	

64	2-Butanone					CAS #:	78-93-3			
7.980	7.980	(0.951)	72	9064	0.50000	0.6310	70.00-	130.00	100.00	
7.980	7.980	(0.951)	43	37052			574.29-	634.29	408.78	
7.980	7.980	(0.951)	57	3317			0.00-	30.00	36.60	

63	cis-1,2-Dichloroethene					CAS #:	156-59-2			
7.953	7.953	(0.947)	61	19760	0.50000	0.5612	70.00-	130.00	100.00	
7.953	7.953	(0.947)	96	10181			27.36-	87.36	51.52	
7.953	7.953	(0.947)	98	11221			5.83-	65.83	56.79	

66	Tetrahydrofuran					CAS #:	109-99-9			
8.367	8.367	(0.997)	42	36347	0.50000	0.6537	70.00-	130.00	100.00	
8.395	8.395	(1.000)	71	10429			0.00-	54.93	28.69	
8.367	8.367	(0.997)	72	9696			0.00-	30.00	26.68	

69	Chloroform					CAS #:	67-66-3			
8.506	8.506	(1.013)	83	27459	0.50000	0.5254	70.00-	130.00	100.00	
8.533	8.533	(1.016)	85	14750			33.71-	93.71	53.72	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	

73	1,1,1-Trichloroethane					CAS #: 71-55-6				
8.755	8.755	(1.043)	97	25097	0.50000	0.5909	70.00- 130.00	100.00		
8.755	8.755	(1.043)	99	15727			33.95- 93.95	62.66		

72	Cyclohexane					CAS #: 110-82-7				
8.727	8.727	(1.040)	84	21555	0.50000	0.6076	70.00- 130.00	100.00		
8.727	8.727	(1.040)	56	31282			138.68- 198.68	145.13		
8.727	8.727	(1.040)	41	25266			73.81- 133.81	117.22		

75	Carbon Tetrachloride					CAS #: 56-23-5				
9.003	9.003	(1.072)	119	18169	0.50000	0.5543	70.00- 130.00	100.00		
9.003	9.003	(1.072)	117	20156			81.67- 141.67	110.94		

79	Benzene					CAS #: 71-43-2				
9.418	9.418	(0.919)	78	38732	0.50000	0.4739	70.00- 130.00	100.00(a)		
9.418	9.418	(0.919)	77	13594			0.00- 30.00	35.10		

81	1,2-Dichloroethane					CAS #: 107-06-2				
9.612	9.612	(0.938)	62	22054	0.50000	0.5953	70.00- 130.00	100.00		
9.612	9.612	(0.938)	64	7025			0.00- 30.00	31.85		

82	Heptane					CAS #: 142-82-5				
9.805	9.805	(0.957)	100	7424	0.50000	0.6746	70.00- 130.00	100.00		
9.805	9.805	(0.957)	43	52953			0.00- 30.00	713.27		
9.833	9.833	(0.960)	71	18647			0.00- 30.00	251.17		

92	Trichloroethene					CAS #: 79-01-6				
10.662	10.662	(1.040)	95	12618	0.50000	0.5430	70.00- 130.00	100.00		
10.690	10.690	(1.043)	130	13346			57.13- 117.13	105.77		
10.662	10.662	(1.040)	97	8061			32.50- 92.50	63.88		

95	1,2-Dichloropropane					CAS #: 78-87-5				
11.188	11.188	(1.092)	63	17718	0.50000	0.6000	70.00- 130.00	100.00		
11.188	11.188	(1.092)	62	12940			45.03- 105.03	73.03		
11.188	11.188	(1.092)	41	12462			45.52- 105.52	70.34		

98	Bromodichloromethane					CAS #: 75-27-4				
11.741	11.741	(1.146)	83	23415	0.50000	0.5696	70.00- 130.00	100.00		
11.741	11.741	(1.146)	85	15224			32.38- 92.38	65.02		

100	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.625	12.625	(1.232)	75	20173	0.50000	0.5704	70.00- 130.00	100.00		
12.625	12.625	(1.232)	77	7291			1.52- 61.52	36.14		
12.625	12.625	(1.232)	39	11695			48.26- 108.26	57.97		

101	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.902	12.902	(1.259)	58	17822	0.50000	0.5955	70.00- 130.00	100.00		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
101 4-Methyl-2-pentanone (continued)									
12.902	12.902	(1.259)	43	51793			0.00- 30.00	290.61	
12.902	12.902	(1.259)	85	9743			0.00- 30.00	54.67	

103 Toluene CAS #: 108-88-3									
13.096	13.096	(1.278)	91	35164	0.50000	0.5344	70.00- 130.00	100.00	
13.096	13.096	(1.278)	92	25326			29.45- 89.45	72.02	

106 trans-1,3-Dichloropropene CAS #: 10061-02-6									
13.621	13.621	(0.895)	75	23242	0.50000	0.5860	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	8854			1.42- 61.42	38.09	
13.621	13.621	(0.895)	39	14308			43.57- 103.57	61.56	

108 1,1,2-Trichloroethane CAS #: 79-00-5									
13.897	13.897	(0.913)	97	13582	0.50000	0.5878	70.00- 130.00	100.00	
13.870	13.870	(0.911)	99	8275			31.40- 91.40	60.93	
13.870	13.870	(0.911)	83	13152			60.06- 120.06	96.83	

109 Tetrachloroethene CAS #: 127-18-4									
13.925	13.925	(0.915)	166	14217	0.50000	0.5766	70.00- 130.00	100.00	
13.925	13.925	(0.915)	129	11924			46.36- 106.36	83.87	
13.925	13.925	(0.915)	131	8940			45.00- 105.00	62.88	

112 2-Hexanone CAS #: 591-78-6									
14.257	14.257	(0.936)	58	20545	0.50000	0.6288	70.00- 130.00	100.00	
14.257	14.257	(0.936)	43	38619			176.52- 236.52	187.97	
14.257	14.257	(0.936)	100	6148			0.00- 30.00	29.92	

114 Dibromochloromethane CAS #: 124-48-1									
14.423	14.423	(0.947)	129	17348	0.50000	0.5700	70.00- 130.00	100.00	
14.423	14.423	(0.947)	127	15277			0.00- 30.00	88.06	

115 1,2-Dibromoethane CAS #: 106-93-4									
14.589	14.589	(0.958)	107	15949	0.50000	0.5388	70.00- 130.00	100.00	
14.589	14.589	(0.958)	109	17920			62.88- 122.88	112.36	

124 Chlorobenzene CAS #: 108-90-7									
15.252	15.252	(1.002)	112	29163	0.50000	0.5604	70.00- 130.00	100.00	
15.252	15.252	(1.002)	114	13422			0.73- 60.73	46.02	
15.252	15.252	(1.002)	77	29566			40.58- 100.58	101.38	

127 Ethyl Benzene CAS #: 100-41-4									
15.363	15.363	(1.009)	106	17066	0.50000	0.5755	70.00- 130.00	100.00	
15.363	15.363	(1.009)	91	51748			0.00- 30.00	303.22	

128 m,p-Xylene CAS #: 108-38-3									
15.529	15.529	(1.020)	106	21671	0.50000	0.5707	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
128 m,p-Xylene (continued)									
15.529	15.529	(1.020)	91	45416			0.00- 30.00	209.57	

130 o-Xylene CAS #: 95-47-6									
16.054	16.054	(1.054)	106	20158	0.50000	0.5650	70.00- 130.00	100.00	
16.054	16.054	(1.054)	91	42807			195.99- 255.99	212.36	

131 Styrene CAS #: 100-42-5									
16.109	16.109	(1.058)	104	23849	0.50000	0.4350	70.00- 130.00	100.00(a)	
16.082	16.082	(1.056)	78	14289			28.78- 88.78	59.91	

133 Bromoform CAS #: 75-25-2									
16.358	16.358	(1.074)	173	12843	0.50000	0.5272	70.00- 130.00	100.00	
16.358	16.358	(1.074)	171	8122			21.17- 81.17	63.24	

142 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.966	16.966	(1.114)	83	28519	0.50000	0.5624	70.00- 130.00	100.00	
16.966	16.966	(1.114)	85	16875			34.35- 94.35	59.17	

145 4-Ethyltoluene CAS #: 622-96-8									
17.132	17.132	(1.125)	105	60065	0.50000	0.5485	70.00- 130.00	100.00	
17.132	17.132	(1.125)	120	14682			0.00- 54.57	24.44	

146 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.215	17.215	(1.131)	105	56714	0.50000	0.5707	70.00- 130.00	100.00	
17.215	17.215	(1.131)	120	22159			0.00- 30.00	39.07	

151 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.602	17.602	(1.156)	105	53686	0.50000	0.5797	70.00- 130.00	100.00	
17.602	17.602	(1.156)	120	22150			11.41- 71.41	41.26	

154 1,3-Dichlorobenzene CAS #: 541-73-1									
17.907	17.907	(1.176)	146	22328	0.50000	0.5493	70.00- 130.00	100.00	
17.907	17.907	(1.176)	148	16082			0.00- 30.00	72.03	
17.879	17.879	(1.174)	111	10660			0.00- 30.00	47.74	

155 1,4-Dichlorobenzene CAS #: 106-46-7									
17.989	17.989	(1.182)	146	29954	0.50000	0.5706	70.00- 130.00	100.00	
17.989	17.989	(1.182)	148	13724			0.00- 30.00	45.82	
17.989	17.989	(1.182)	111	11705			0.00- 30.00	39.08	

156 alpha-Chlorotoluene CAS #: 100-44-7									
18.128	18.128	(1.191)	91	38235	0.50000	0.5268	70.00- 130.00	100.00	
18.128	18.128	(1.191)	126	7448			0.00- 30.00	19.48	

158 1,2-Dichlorobenzene CAS #: 95-50-1									
18.321	18.321	(1.203)	146	26326	0.50000	0.5785	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
158 1,2-Dichlorobenzene (continued)									
18.321	18.321	(1.203)	148	16880			33.83- 93.83	64.12	
18.321	18.321	(1.203)	111	14335			21.29- 81.29	54.45	

135 Cumene CAS #: 98-82-8									
16.524	16.524	(1.085)	105	55515	0.50000	0.4844	70.00- 130.00	100.00(a)	
16.524	16.524	(1.085)	120	14849			0.00- 30.00	26.75	
16.496	16.496	(1.084)	51	10327			0.00- 30.00	18.60	

143 Propylbenzene CAS #: 103-65-1									
16.994	16.994	(1.116)	91	68703	0.50000	0.5556	70.00- 130.00	100.00	
16.994	16.994	(1.116)	120	14050			0.00- 30.00	20.45	
16.994	16.994	(1.116)	105	6002			0.00- 30.00	8.74	

78 2,2,4-Trimethylpentane CAS #: 540-84-1									
9.418	9.418	(1.122)	57	89003	0.50000	0.5639	70.00- 130.00	100.00	
9.418	9.418	(1.122)	56	33063			0.00- 30.00	37.15	
9.418	9.418	(1.122)	41	31452			0.00- 30.00	35.34	

93 Methyl Cyclohexane CAS #: 108-87-2									
10.911	10.911	(1.300)	83	26434	0.50000	0.5964	70.00- 130.00	100.00	
10.884	10.884	(1.296)	98	14042			0.00- 30.00	53.12	
10.884	10.884	(1.296)	55	27351			0.00- 30.00	103.47	

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032215.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv -> 0.5ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	270806	-4.56
86 1,4-Difluorobenze	1370859	822515	1919203	1311826	-4.31
123 Chlorobenzene-d5	1067063	640238	1493888	1039819	-2.55

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22mar.lb/8032215.d

Date: 22-MAR-2007 17:30

Client ID: Level 2


Sample Info: 0.5ml 1487-115

Column phase: RTX-624

Instrument: msd8.1

Operator: sjr

Column diameter: 0.53



Report Date: 26-Mar-2007 13:58

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-26mar.b/8032606.d
 Lab Smp Id: ICAL Client Smp ID: LEVEL 3
 Inj Date : 26-MAR-2007 12:15
 Operator : ea Inst ID: msd8.i
 Smp Info : 2.0ml #1487-42
 Misc Info : 200ppbv-2.0ppbv
 Comment :
 Method : /chem/msd8.i/8-26mar.b/t14q322b.m
 Meth Date : 26-Mar-2007 13:58 ealcan Quant Type: ISTD
 Cal Date : 26-MAR-2007 12:15 Cal File: 8032606.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	293727	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	225479			46.88- 106.88	76.76	
8.367	8.367	(1.000)	49	828524			254.92- 314.92	282.07	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1372405	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	259807			0.00- 48.81	18.93	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1065309	25.0000		70.00- 130.00	100.00	
15.224	15.224	(1.000)	82	720886			0.00- 30.00	67.67	

194 2-Methylpentane CAS #: 107-83-5									
5.547	5.547	(0.661)	71	57426	2.00000	2.417	70.00- 130.00	100.00	
5.547	5.547	(0.661)	43	218120			0.00- 30.00	379.83	
5.547	5.547	(0.661)	42	109426			0.00- 30.00	190.55	

195 Thiopene CAS #: 110-02-1									
9.833	9.833	(0.960)	84	108102	2.00000	2.401	70.00- 130.00	100.00(T)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
195 Thiopene (continued)									
9.833	9.833	(0.960)	58	79477			0.00- 30.00	73.52	
0.000	1.000	(0.000)	0	0			0.00- 30.00	0.00	

196 Indan									
						CAS #: 496-11-7			
18.183	18.183	(1.194)	117	227148	2.00000	2.439	70.00- 130.00	100.00	
18.183	18.183	(1.194)	118	124147			0.00- 30.00	54.65	
18.183	18.183	(1.194)	91	53358			0.00- 30.00	23.49	

197 Indene									
						CAS #: 95-13-6			
18.404	18.404	(1.209)	115	148838	2.00000	2.457	70.00- 130.00	100.00(T)	
0.000	1.000	(0.000)	16	0			0.00- 30.00	0.00	

83 2,3-Dimethylpentane									
						CAS #: 565-59-3			
8.782	8.782	(1.046)	71	45393	2.00000	2.356	70.00- 130.00	100.00	
8.810	8.810	(1.049)	56	153558			314.83- 374.83	338.29	
8.782	8.782	(1.046)	43	145616			0.00- 30.00	320.79	

QC Flag Legend

T - Target compound detected outside RT window.

Report Date: 26-Mar-2007 13:58

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 26-MAR-2007

Lab File ID: 8032606.d

Calibration Time: 12:43

Lab Smp Id: ICAL

Client Smp ID: LEVEL 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ea

Method File: /chem/msd8.i/8-26mar.b/t14q322b.m

Misc Info: 200ppbv-2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	291821	175093	408549	293727	0.65
86 1,4-Difluorobenze	1354208	812525	1895891	1372405	1.34
123 Chlorobenzene-d5	1071895	643137	1500653	1065309	-0.61

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.39	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-26mar.lb/8032606.d

Date: 26-MAR-2007 12:15

Client ID: LEVEL 3


Sample Info: 2.0ml #1487-42

Column phase: RTX-624

Instrument: msd8.1

Operator: ea

Column diameter: 0.53



Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032205.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 22-MAR-2007 11:38
 Operator : sjr Inst ID: msd8.i
 Smp Info : 2.0ml 1487-115
 Misc Info : 200ppbv -> 2ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:09 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 11:38 Cal File: 8032205.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+Na+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	275416	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	214844			46.35- 106.35	78.01	
8.395	8.395	(1.000)	49	843588			255.78- 315.78	306.30	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1361295	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	247284			0.00- 48.88	18.17	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1067969	25.0000		70.00- 130.00	100.00	
15.224	15.224	(1.000)	82	699917			0.00- 30.00	65.54	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.473	(1.128)	65	591430	25.0000	25.734	70.00- 130.00	100.00	
9.473	9.473	(1.128)	67	299310			0.00- 30.00	50.61	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	1293142	25.0000	24.391	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	177809			0.00- 30.00	13.75	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 102 Toluene-d8 (continued)									
12.985	12.985	(1.267)	100	845124			0.00- 30.00	65.35	

\$ 138 Bromofluorobenzene CAS #: 460-00-4									
16.773	16.773	(1.102)	174	543659	25.0000	25.185	70.00- 130.00	100.00	
16.745	16.745	(1.100)	95	861291			137.66- 197.66	158.42	
16.773	16.773	(1.102)	176	504513			63.61- 123.61	92.80	

3 Propylene CAS #: 115-07-1									
2.395	2.395	(0.285)	41	80391	2.00000	2.431	70.00- 130.00	100.00	
2.395	2.395	(0.285)	42	56887			0.00- 30.00	70.76	
2.395	2.395	(0.285)	39	58801			0.00- 30.00	73.14	

4 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.450	2.450	(0.292)	85	150641	2.00000	2.130	70.00- 130.00	100.00	
2.450	2.450	(0.292)	87	52547			0.00- 30.00	34.88	

6 Freon 114 CAS #: 76-14-2									
2.616	2.616	(0.312)	135	80893	2.00000	2.064	70.00- 130.00	100.00(H)	
2.616	2.616	(0.312)	137	25279			1.88- 61.88	31.25	

8 Chloromethane CAS #: 74-87-3									
2.755	2.755	(0.328)	50	94717	2.00000	2.511	70.00- 130.00	100.00	
2.755	2.755	(0.328)	52	32017			0.00- 30.00	33.80	

10 Vinyl Chloride CAS #: 75-01-4									
2.920	2.920	(0.348)	62	77330	2.00000	2.370	70.00- 130.00	100.00	
2.893	2.893	(0.345)	64	28295			0.00- 30.00	36.59	

11 1,3-Butadiene CAS #: 106-99-0									
2.893	2.893	(0.345)	54	81680	2.00000	2.346	70.00- 130.00	100.00	
2.893	2.893	(0.345)	39	193417			0.00- 30.00	236.80	

13 Bromomethane CAS #: 74-83-9									
3.446	3.446	(0.410)	94	37760	2.00000	2.065	70.00- 130.00	100.00	
3.446	3.446	(0.410)	96	36806			64.77- 124.77	97.47	

16 Chloroethane CAS #: 75-00-3									
3.612	3.612	(0.430)	64	38142	2.00000	2.226	70.00- 130.00	100.00	
3.612	3.612	(0.430)	49	14286			0.00- 30.00	37.45	
3.612	3.612	(0.430)	66	9687			0.00- 30.00	25.40	

18 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
3.916	3.916	(0.466)	101	139609	2.00000	2.343	70.00- 130.00	100.00	
3.916	3.916	(0.466)	103	94957			34.71- 94.71	68.02	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
21 Ethanol						CAS #: 64-17-5			
4.275	4.275	(0.509)	45	32514	2.00000	2.322	70.00- 130.00	100.00	
4.248	4.248	(0.506)	43	13134			0.00- 30.00	40.39	
4.248	4.248	(0.506)	46	17713			0.00- 30.00	54.48	

27 Freon 113						CAS #: 76-13-1			
4.745	4.745	(0.565)	151	70996	2.00000	2.393	70.00- 130.00	100.00	
4.745	4.745	(0.565)	153	39185			32.67- 92.67	55.19	
4.745	4.745	(0.565)	101	96260			124.83- 184.83	135.59	

29 1,1-Dichloroethene						CAS #: 75-35-4			
4.801	4.801	(0.572)	61	111438	2.00000	2.208	70.00- 130.00	100.00	
4.801	4.801	(0.572)	96	54692			15.10- 75.10	49.08	
4.801	4.801	(0.572)	98	30302			0.00- 58.17	27.19	

30 Acetone						CAS #: 67-64-1			
4.939	4.939	(0.588)	58	45330	2.00000	2.490	70.00- 130.00	100.00	
4.939	4.939	(0.588)	43	136965			0.00- 30.00	302.15	

34 2-Propanol						CAS #: 67-63-0			
5.160	5.160	(0.615)	45	151092	2.00000	2.257	70.00- 130.00	100.00	
5.160	5.160	(0.615)	43	47357			0.00- 30.00	31.34	
5.160	5.160	(0.615)	59	7137			0.00- 30.00	4.72	

33 Carbon Disulfide						CAS #: 75-15-0			
5.160	5.160	(0.615)	76	169984	2.00000	2.197	70.00- 130.00	100.00	

39 Methylene Chloride						CAS #: 75-09-2			
5.713	5.713	(0.681)	49	94236	2.00000	2.191	70.00- 130.00	100.00	
5.713	5.713	(0.681)	84	43931			18.44- 78.44	46.62	
5.713	5.713	(0.681)	51	30460			0.00- 30.00	32.32	

42 MTBE						CAS #: 1634-04-4			
6.045	6.045	(0.720)	73	188996	2.00000	2.202	70.00- 130.00	100.00	
6.045	6.045	(0.720)	57	57183			0.00- 59.33	30.26	
6.045	6.045	(0.720)	41	64052			0.00- 30.00	33.89	

43 trans-1,2-Dichloroethene						CAS #: 156-60-5			
6.100	6.100	(0.727)	96	56019	2.00000	2.120	70.00- 130.00	100.00	
6.100	6.100	(0.727)	61	104489			169.97- 229.97	186.52	
6.100	6.100	(0.727)	98	37274			0.00- 30.00	66.54	

45 Hexane						CAS #: 110-54-3			
6.460	6.460	(0.769)	57	138775	2.00000	2.197	70.00- 130.00	100.00	
6.432	6.432	(0.766)	43	105650			0.00- 30.00	76.13	
6.460	6.460	(0.769)	86	17560			0.00- 30.00	12.65	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
54 Vinyl Acetate						CAS #:	108-05-4			
6.957	6.957	(0.829)	86	11360	2.00000	1.985	70.00-	130.00	100.00(a)	
6.985	6.985	(0.832)	43	222873			0.00-	30.00	1961.91	
6.985	6.985	(0.832)	42	30814			0.00-	30.00	271.25	

52 1,1-Dichloroethane						CAS #:	75-34-3			
6.902	6.902	(0.822)	63	112495	2.00000	2.162	70.00-	130.00	100.00	
6.902	6.902	(0.822)	65	38326			0.00-	59.58	34.07	

64 2-Butanone						CAS #:	78-93-3			
8.008	8.008	(0.954)	72	31076	2.00000	2.083	70.00-	130.00	100.00	
7.980	7.980	(0.951)	43	189499			574.29-	634.29	609.79	
8.008	8.008	(0.954)	57	13265			0.00-	30.00	42.69	

63 cis-1,2-Dichloroethene						CAS #:	156-59-2			
7.953	7.953	(0.947)	61	93793	2.00000	2.374	70.00-	130.00	100.00	
7.953	7.953	(0.947)	96	53841			27.36-	87.36	57.40	
7.953	7.953	(0.947)	98	35782			5.83-	65.83	38.15	

66 Tetrahydrofuran						CAS #:	109-99-9			
8.367	8.367	(0.997)	42	112088	2.00000	1.988	70.00-	130.00	100.00	
8.367	8.367	(0.997)	71	31794			0.00-	54.93	28.37	
8.367	8.367	(0.997)	72	36828			0.00-	30.00	32.86	

69 Chloroform						CAS #:	67-66-3			
8.506	8.506	(1.013)	83	99138	2.00000	1.897	70.00-	130.00	100.00	
8.506	8.506	(1.013)	85	60557			33.71-	93.71	61.08	

73 1,1,1-Trichloroethane						CAS #:	71-55-6			
8.754	8.754	(1.043)	97	102556	2.00000	2.235	70.00-	130.00	100.00	
8.754	8.754	(1.043)	99	65946			33.95-	93.95	64.30	

72 Cyclohexane						CAS #:	110-82-7			
8.727	8.727	(1.040)	84	88061	2.00000	2.274	70.00-	130.00	100.00	
8.727	8.727	(1.040)	56	144374			138.68-	198.68	163.95	
8.727	8.727	(1.040)	41	83275			73.81-	133.81	94.57	

75 Carbon Tetrachloride						CAS #:	56-23-5			
9.003	9.003	(1.072)	119	83711	2.00000	2.314	70.00-	130.00	100.00	
9.003	9.003	(1.072)	117	90621			81.67-	141.67	108.25	

79 Benzene						CAS #:	71-43-2			
9.418	9.418	(0.919)	78	176144	2.00000	2.057	70.00-	130.00	100.00	
9.418	9.418	(0.919)	77	42211			0.00-	30.00	23.96	

81 1,2-Dichloroethane						CAS #:	107-06-2			
9.612	9.612	(0.938)	62	85388	2.00000	2.142	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
81 1,2-Dichloroethane (continued)									
9.612	9.612	(0.938)	64	28911			0.00- 30.00	33.86	

82 Heptane CAS #: 142-82-5									
9.805	9.805	(0.957)	100	19431	2.00000	1.790	70.00- 130.00	100.00	
9.805	9.805	(0.957)	43	173362			0.00- 30.00	892.19	
9.805	9.805	(0.957)	71	61608			0.00- 30.00	317.06	

92 Trichloroethene CAS #: 79-01-6									
10.662	10.662	(1.040)	95	65132	2.00000	2.418	70.00- 130.00	100.00	
10.690	10.690	(1.043)	130	44283			57.13- 117.13	67.99	
10.662	10.662	(1.040)	97	42276			32.50- 92.50	64.91	

95 1,2-Dichloropropane CAS #: 78-87-5									
11.188	11.188	(1.092)	63	66549	2.00000	2.111	70.00- 130.00	100.00	
11.188	11.188	(1.092)	62	52517			45.03- 105.03	78.91	
11.188	11.188	(1.092)	41	54992			45.52- 105.52	82.63	

96 1,4-Dioxane CAS #: 123-91-1									
11.409	11.409	(1.113)	88	37221	2.00000	2.314	70.00- 130.00	100.00	
11.409	11.409	(1.113)	58	35515			70.27- 130.27	95.42	
11.409	11.409	(1.113)	57	15135			0.00- 30.00	40.66	

98 Bromodichloromethane CAS #: 75-27-4									
11.741	11.741	(1.146)	83	102417	2.00000	2.250	70.00- 130.00	100.00	
11.741	11.741	(1.146)	85	67122			32.38- 92.38	65.54	

100 cis-1,3-Dichloropropene CAS #: 10061-01-5									
12.625	12.625	(1.232)	75	83591	2.00000	2.177	70.00- 130.00	100.00	
12.625	12.625	(1.232)	77	23874			1.52- 61.52	28.56	
12.625	12.625	(1.232)	39	64418			48.26- 108.26	77.06	

101 4-Methyl-2-pentanone CAS #: 108-10-1									
12.902	12.902	(1.259)	58	67980	2.00000	2.122	70.00- 130.00	100.00	
12.902	12.902	(1.259)	43	203570			0.00- 30.00	299.46	
12.902	12.902	(1.259)	85	22270			0.00- 30.00	32.76	

103 Toluene CAS #: 108-88-3									
13.095	13.095	(1.278)	91	171210	2.00000	2.312	70.00- 130.00	100.00	
13.095	13.095	(1.278)	92	93386			29.45- 89.45	54.54	

106 trans-1,3-Dichloropropene CAS #: 10061-02-6									
13.621	13.621	(0.895)	75	82643	2.00000	2.019	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	31993			1.42- 61.42	38.71	
13.621	13.621	(0.895)	39	78281			43.57- 103.57	94.72	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

108	1,1,2-Trichloroethane					CAS #:	79-00-5			
13.897	13.897	(0.913)	97	49580	2.00000	2.058	70.00-	130.00	100.00	
13.897	13.897	(0.913)	99	31406			31.40-	91.40	63.34	
13.897	13.897	(0.913)	83	46646			60.06-	120.06	94.08	

109	Tetrachloroethene					CAS #:	127-18-4			
13.925	13.925	(0.915)	166	48412	2.00000	1.940	70.00-	130.00	100.00	
13.925	13.925	(0.915)	129	47041			46.36-	106.36	97.17	
13.925	13.925	(0.915)	131	40366			45.00-	105.00	83.38	

112	2-Hexanone					CAS #:	591-78-6			
14.257	14.257	(0.936)	58	75259	2.00000	2.114	70.00-	130.00	100.00	
14.257	14.257	(0.936)	43	175210			176.52-	236.52	232.81	
14.257	14.257	(0.936)	100	13078			0.00-	30.00	17.38	

114	Dibromochloromethane					CAS #:	124-48-1			
14.423	14.423	(0.947)	129	69176	2.00000	2.137	70.00-	130.00	100.00	
14.423	14.423	(0.947)	127	50548			0.00-	30.00	73.07	

115	1,2-Dibromoethane					CAS #:	106-93-4			
14.589	14.589	(0.958)	107	75869	2.00000	2.305	70.00-	130.00	100.00	
14.589	14.589	(0.958)	109	73073			62.88-	122.88	96.31	

124	Chlorobenzene					CAS #:	108-90-7			
15.252	15.252	(1.002)	112	119945	2.00000	2.156	70.00-	130.00	100.00	
15.252	15.252	(1.002)	114	44278			0.73-	60.73	36.92	
15.252	15.252	(1.002)	77	94503			40.58-	100.58	78.79	

127	Ethyl Benzene					CAS #:	100-41-4			
15.363	15.363	(1.009)	106	63387	2.00000	2.053	70.00-	130.00	100.00	
15.363	15.363	(1.009)	91	227641			0.00-	30.00	359.13	

128	m,p-Xylene					CAS #:	108-38-3			
15.529	15.529	(1.020)	106	83062	2.00000	2.084	70.00-	130.00	100.00	
15.529	15.529	(1.020)	91	188273			0.00-	30.00	226.67	

130	o-Xylene					CAS #:	95-47-6			
16.054	16.054	(1.054)	106	86049	2.00000	2.219	70.00-	130.00	100.00	
16.054	16.054	(1.054)	91	194934			195.99-	255.99	226.54	

131	Styrene					CAS #:	100-42-5			
16.082	16.082	(1.056)	104	128028	2.00000	2.198	70.00-	130.00	100.00	
16.082	16.082	(1.056)	78	77317			28.78-	88.78	60.39	

133	Bromoform					CAS #:	75-25-2			
16.358	16.358	(1.074)	173	55198	2.00000	2.133	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
133 Bromoform (continued)									
16.358	16.358	(1.074)	171	30668			21.17- 81.17	55.56	

142 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.966	16.966	(1.114)	83	121397	2.00000	2.209	70.00- 130.00	100.00	
16.966	16.966	(1.114)	85	81065			34.35- 94.35	66.78	

145 4-Ethyltoluene CAS #: 622-96-8									
17.132	17.132	(1.125)	105	244319	2.00000	2.112	70.00- 130.00	100.00	
17.132	17.132	(1.125)	120	57573			0.00- 54.57	23.56	

146 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.215	17.215	(1.131)	105	262265	2.00000	2.347	70.00- 130.00	100.00	
17.215	17.215	(1.131)	120	111702			0.00- 30.00	42.59	

151 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.602	17.602	(1.156)	105	220430	2.00000	2.201	70.00- 130.00	100.00	
17.602	17.602	(1.156)	120	92573			11.41- 71.41	42.00	

154 1,3-Dichlorobenzene CAS #: 541-73-1									
17.906	17.906	(1.176)	146	82808	2.00000	1.989	70.00- 130.00	100.00	
17.906	17.906	(1.176)	148	57275			0.00- 30.00	69.17	
17.906	17.906	(1.176)	111	36240			0.00- 30.00	43.76	

155 1,4-Dichlorobenzene CAS #: 106-46-7									
17.989	17.989	(1.182)	146	107737	2.00000	1.999	70.00- 130.00	100.00	
17.989	17.989	(1.182)	148	72586			0.00- 30.00	67.37	
17.989	17.989	(1.182)	111	44084			0.00- 30.00	40.92	

156 alpha-Chlorotoluene CAS #: 100-44-7									
18.128	18.128	(1.191)	91	148060	2.00000	1.991	70.00- 130.00	100.00	
18.128	18.128	(1.191)	126	30145			0.00- 30.00	20.36	

158 1,2-Dichlorobenzene CAS #: 95-50-1									
18.321	18.321	(1.203)	146	99085	2.00000	2.078	70.00- 130.00	100.00	
18.321	18.321	(1.203)	148	58889			33.83- 93.83	59.43	
18.321	18.321	(1.203)	111	46285			21.29- 81.29	46.71	

163 1,2,4-Trichlorobenzene CAS #: 120-82-1									
19.593	19.593	(1.287)	180	62263	2.00000	2.220	70.00- 130.00	100.00	
19.593	19.593	(1.287)	182	58921			62.06- 122.06	94.63	

164 Hexachlorobutadiene CAS #: 87-68-3									
19.676	19.676	(1.292)	225	104649	2.00000	2.558	70.00- 130.00	100.00	
19.676	19.676	(1.292)	223	57449			35.92- 95.92	54.90	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

135 Cumene						CAS #: 98-82-8			
16.524	16.524	(1.085)	105	243116	2.00000	2.049	70.00- 130.00	100.00	
16.524	16.524	(1.085)	120	52203			0.00- 30.00	21.47	
16.496	16.496	(1.084)	51	38911			0.00- 30.00	16.01	

143 Propylbenzene						CAS #: 103-65-1			
16.994	16.994	(1.116)	91	287725	2.00000	2.169	70.00- 130.00	100.00	
16.994	16.994	(1.116)	120	52173			0.00- 30.00	18.13	
16.994	16.994	(1.116)	105	13051			0.00- 30.00	4.54	

37 3-Chloropropene						CAS #: 107-05-1			
5.437	5.437	(0.648)	76	29487	2.00000	2.368	70.00- 130.00	100.00	
5.437	5.437	(0.648)	41	139623			0.00- 30.00	473.51	

78 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.446	9.446	(1.125)	57	396404	2.00000	2.290	70.00- 130.00	100.00	
9.418	9.418	(1.122)	56	133818			0.00- 30.00	33.76	
9.418	9.418	(1.122)	41	121704			0.00- 30.00	30.70	

165 Naphthalene						CAS #: 91-20-3			
19.787	19.787	(1.300)	128	229919	2.00000	2.376	70.00- 130.00	100.00	
19.787	19.787	(1.300)	127	33934			0.00- 30.00	14.76	

9 Butane						CAS #: 106-97-8			
2.837	2.837	(0.338)	58	25473	2.00000	2.569	70.00- 130.00	100.00	
2.837	2.837	(0.338)	43	171107			0.00- 30.00	671.72	

15 Isopentane						CAS #: 78-78-4			
3.556	3.556	(0.424)	43	146320	2.00000	2.466	70.00- 130.00	100.00	
3.556	3.556	(0.424)	57	75097			0.00- 30.00	51.32	
3.556	3.556	(0.424)	72	9820			0.00- 30.00	6.71	

93 Methyl Cyclohexane						CAS #: 108-87-2			
10.883	10.883	(1.296)	83	107485	2.00000	2.241	70.00- 130.00	100.00	
10.911	10.911	(1.300)	98	43831			0.00- 30.00	40.78	
10.883	10.883	(1.296)	55	121330			0.00- 30.00	112.88	

QC Flag Legend

- a - Target compound detected but, quantitated amount Below Limit Of Quantitation(BLOQ).
- H - Operator selected an alternate compound hit.

Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032205.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv -> 2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	275416	-2.93
86 1,4-Difluorobenze	1370859	822515	1919203	1361295	-0.70
123 Chlorobenzene-d5	1067063	640238	1493888	1067969	0.08

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22mar.lb/8032205.d
Date: 22-MAR-2007 11:38
Client ID: Level 3
Sample Info: 2.0ml 1487-115

Column phase: RTX-624

Instrument: msd8.1
Operator: sjr
Column diameter: 0.53



Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032206.d
 Lab Smp Id: ICAL Client Smp ID: Level 4
 Inj Date : 22-MAR-2007 12:06
 Operator : sjr Inst ID: msd8.i
 Smp Info : 25ml 1487-115
 Misc Info : 200ppbv->25ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:09 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 12:06 Cal File: 8032206.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	284047	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	223837			46.35- 106.35	78.80	
8.368	8.368	(1.000)	49	821968			255.78- 315.78	289.38	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1370589	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	261113			0.00- 48.88	19.05	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225	(1.000)	117	1101300	25.0000		70.00- 130.00	100.00	
15.197	15.197	(1.000)	82	733265			0.00- 30.00	66.58	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.474	9.474	(1.128)	65	634634	25.0000	26.400	70.00- 130.00	100.00	
9.474	9.474	(1.128)	67	318417			0.00- 30.00	50.17	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	1353120	25.0000	25.279	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	171655			0.00- 30.00	12.69	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 102 Toluene-d8 (continued)										
12.985	12.985	(1.267)	100	916907			0.00- 30.00	67.76		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.745	16.745	(1.100)	174	565422	25.0000	25.319	70.00- 130.00	100.00		
16.745	16.745	(1.100)	95	952630			137.66- 197.66	168.48		
16.745	16.745	(1.100)	176	564473			63.61- 123.61	99.83		

3 Propylene										
						CAS #: 115-07-1				
2.395	2.395	(0.285)	41	699671	25.0000	21.819	70.00- 130.00	100.00		
2.395	2.395	(0.285)	42	459264			0.00- 30.00	65.64		
2.395	2.395	(0.285)	39	505920			0.00- 30.00	72.31		

4 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.451	2.451	(0.292)	85	1439765	25.0000	20.838	70.00- 130.00	100.00		
2.451	2.451	(0.292)	87	454966			0.00- 30.00	31.60		

6 Freon 114										
						CAS #: 76-14-2				
2.589	2.589	(0.308)	135	827106	25.0000	21.434	70.00- 130.00	100.00		
2.589	2.589	(0.308)	137	245941			1.88- 61.88	29.74		

8 Chloromethane										
						CAS #: 74-87-3				
2.727	2.727	(0.325)	50	760770	25.0000	21.088	70.00- 130.00	100.00		
2.727	2.727	(0.325)	52	240634			0.00- 30.00	31.63		

9 Butane										
						CAS #: 106-97-8				
2.810	2.810	(0.335)	58	193671	25.0000	20.606	70.00- 130.00	100.00		
2.810	2.810	(0.335)	43	1529744			0.00- 30.00	789.87		

10 Vinyl Chloride										
						CAS #: 75-01-4				
2.893	2.893	(0.345)	62	722193	25.0000	22.250	70.00- 130.00	100.00		
2.921	2.921	(0.348)	64	215629			0.00- 30.00	29.86		

11 1,3-Butadiene										
						CAS #: 106-99-0				
2.865	2.865	(0.341)	54	720558	25.0000	21.110	70.00- 130.00	100.00		
2.865	2.865	(0.341)	39	880604			0.00- 30.00	122.21		

13 Bromomethane										
						CAS #: 74-83-9				
3.418	3.418	(0.407)	94	363545	25.0000	20.450	70.00- 130.00	100.00		
3.418	3.418	(0.407)	96	329744			64.77- 124.77	90.70		

15 Isopentane										
						CAS #: 78-78-4				
3.557	3.557	(0.424)	43	1199529	25.0000	21.120	70.00- 130.00	100.00		
3.557	3.557	(0.424)	57	727109			0.00- 30.00	60.62		
3.557	3.557	(0.424)	72	67241			0.00- 30.00	5.61		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

16 Chloroethane						CAS #: 75-00-3			
3.557	3.557	(0.424)	64	369678	25.0000	21.806	70.00- 130.00	100.00	
3.557	3.557	(0.424)	49	113454			0.00- 30.00	30.69	
3.557	3.557	(0.424)	66	115437			0.00- 30.00	31.23	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.888	3.888	(0.463)	101	1352144	25.0000	22.686	70.00- 130.00	100.00	
3.888	3.888	(0.463)	103	878754			34.71- 94.71	64.99	

21 Ethanol						CAS #: 64-17-5			
4.248	4.248	(0.506)	45	314916	25.0000	22.776	70.00- 130.00	100.00	
4.248	4.248	(0.506)	43	69502			0.00- 30.00	22.07	
4.248	4.248	(0.506)	46	143603			0.00- 30.00	45.60	

27 Freon 113						CAS #: 76-13-1			
4.745	4.745	(0.565)	151	610034	25.0000	21.002	70.00- 130.00	100.00	
4.745	4.745	(0.565)	153	389700			32.67- 92.67	63.88	
4.745	4.745	(0.565)	101	945928			124.83- 184.83	155.06	

29 1,1-Dichloroethene						CAS #: 75-35-4			
4.773	4.773	(0.569)	61	1030905	25.0000	20.891	70.00- 130.00	100.00	
4.773	4.773	(0.569)	96	462006			15.10- 75.10	44.82	
4.773	4.773	(0.569)	98	282914			0.00- 58.17	27.44	

30 Acetone						CAS #: 67-64-1			
4.939	4.939	(0.588)	58	394063	25.0000	22.178	70.00- 130.00	100.00	
4.939	4.939	(0.588)	43	1348833			0.00- 30.00	342.29	

33 Carbon Disulfide						CAS #: 75-15-0			
5.133	5.133	(0.611)	76	1581151	25.0000	20.896	70.00- 130.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
5.133	5.133	(0.611)	45	1545684	25.0000	23.198	70.00- 130.00	100.00	
5.133	5.133	(0.611)	43	332266			0.00- 30.00	21.50	
5.133	5.133	(0.611)	59	50332			0.00- 30.00	3.26	

37 3-Chloropropene						CAS #: 107-05-1			
5.437	5.437	(0.648)	76	266845	25.0000	22.018	70.00- 130.00	100.00	
5.437	5.437	(0.648)	41	1223525			0.00- 30.00	458.52	

39 Methylene Chloride						CAS #: 75-09-2			
5.686	5.686	(0.677)	49	882904	25.0000	20.971	70.00- 130.00	100.00	
5.713	5.713	(0.681)	84	418715			18.44- 78.44	47.42	
5.686	5.686	(0.677)	51	255897			0.00- 30.00	28.98	

42 MTBE						CAS #: 1634-04-4			
6.045	6.045	(0.720)	73	1782455	25.0000	21.167	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.045	6.045	(0.720)	57	538572			0.00- 59.33	30.22	
6.045	6.045	(0.720)	41	553460			0.00- 30.00	31.05	

43 trans-1,2-Dichloroethene CAS #: 156-60-5									
6.100	6.100	(0.727)	96	508539	25.0000	19.921	70.00- 130.00	100.00	
6.100	6.100	(0.727)	61	1024177			169.97- 229.97	201.40	
6.100	6.100	(0.727)	98	320921			0.00- 30.00	63.11	

45 Hexane CAS #: 110-54-3									
6.432	6.432	(0.766)	57	1315489	25.0000	21.212	70.00- 130.00	100.00	
6.432	6.432	(0.766)	43	960958			0.00- 30.00	73.05	
6.460	6.460	(0.769)	86	174067			0.00- 30.00	13.23	

52 1,1-Dichloroethane CAS #: 75-34-3									
6.902	6.902	(0.822)	63	1131951	25.0000	21.952	70.00- 130.00	100.00	
6.902	6.902	(0.822)	65	333923			0.00- 59.58	29.50	

54 Vinyl Acetate CAS #: 108-05-4									
6.957	6.957	(0.829)	86	139932	25.0000	24.124	70.00- 130.00	100.00	
6.957	6.957	(0.829)	43	2265817			0.00- 30.00	1619.23	
6.957	6.957	(0.829)	42	212529			0.00- 30.00	151.88	

63 cis-1,2-Dichloroethene CAS #: 156-59-2									
7.953	7.953	(0.947)	61	864179	25.0000	22.046	70.00- 130.00	100.00	
7.953	7.953	(0.947)	96	478959			27.36- 87.36	55.42	
7.953	7.953	(0.947)	98	310381			5.83- 65.83	35.92	

64 2-Butanone CAS #: 78-93-3									
7.980	7.980	(0.951)	72	288208	25.0000	19.985	70.00- 130.00	100.00	
7.980	7.980	(0.951)	43	1731315			574.29- 634.29	600.72	
7.980	7.980	(0.951)	57	111897			0.00- 30.00	38.83	

66 Tetrahydrofuran CAS #: 109-99-9									
8.368	8.368	(0.997)	42	1059865	25.0000	19.552	70.00- 130.00	100.00	
8.368	8.368	(0.997)	71	251229			0.00- 54.93	23.70	
8.368	8.368	(0.997)	72	268980			0.00- 30.00	25.38	

69 Chloroform CAS #: 67-66-3									
8.506	8.506	(1.013)	83	961478	25.0000	18.924	70.00- 130.00	100.00	
8.506	8.506	(1.013)	85	617819			33.71- 93.71	64.26	

72 Cyclohexane CAS #: 110-82-7									
8.727	8.727	(1.040)	84	778381	25.0000	20.624	70.00- 130.00	100.00	
8.727	8.727	(1.040)	56	1305092			138.68- 198.68	167.67	
8.727	8.727	(1.040)	41	792458			73.81- 133.81	101.81	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

73	1,1,1-Trichloroethane					CAS #:	71-55-6			
8.755	8.755	(1.043)	97	960173	25.0000	21.290	70.00-	130.00	100.00	
8.755	8.755	(1.043)	99	617103			33.95-	93.95	64.27	

75	Carbon Tetrachloride					CAS #:	56-23-5			
9.003	9.003	(1.072)	119	798425	25.0000	22.200	70.00-	130.00	100.00	
9.003	9.003	(1.072)	117	880568			81.67-	141.67	110.29	

78	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.418	9.418	(1.122)	57	3798916	25.0000	22.104	70.00-	130.00	100.00	
9.418	9.418	(1.122)	56	1325359			0.00-	30.00	34.89	
9.418	9.418	(1.122)	41	1128592			0.00-	30.00	29.71	

79	Benzene					CAS #:	71-43-2			
9.418	9.418	(0.919)	78	1680797	25.0000	20.394	70.00-	130.00	100.00	
9.418	9.418	(0.919)	77	402439			0.00-	30.00	23.94	

81	1,2-Dichloroethane					CAS #:	107-06-2			
9.612	9.612	(0.938)	62	836643	25.0000	21.750	70.00-	130.00	100.00	
9.612	9.612	(0.938)	64	261907			0.00-	30.00	31.30	

82	Heptane					CAS #:	142-82-5			
9.805	9.805	(0.957)	100	192971	25.0000	19.060	70.00-	130.00	100.00	
9.805	9.805	(0.957)	43	1616070			0.00-	30.00	837.47	
9.805	9.805	(0.957)	71	627603			0.00-	30.00	325.23	

92	Trichloroethene					CAS #:	79-01-6			
10.662	10.662	(1.040)	95	598872	25.0000	22.749	70.00-	130.00	100.00	
10.662	10.662	(1.040)	130	522988			57.13-	117.13	87.33	
10.662	10.662	(1.040)	97	363933			32.50-	92.50	60.77	

93	Methyl Cyclohexane					CAS #:	108-87-2			
10.884	10.884	(1.296)	83	969035	25.0000	20.710	70.00-	130.00	100.00	
10.911	10.911	(1.300)	98	462139			0.00-	30.00	47.69	
10.884	10.884	(1.296)	55	1129900			0.00-	30.00	116.60	

95	1,2-Dichloropropane					CAS #:	78-87-5			
11.188	11.188	(1.092)	63	637102	25.0000	21.115	70.00-	130.00	100.00	
11.188	11.188	(1.092)	62	495731			45.03-	105.03	77.81	
11.188	11.188	(1.092)	41	503325			45.52-	105.52	79.00	

96	1,4-Dioxane					CAS #:	123-91-1			
11.409	11.409	(1.113)	88	356412	25.0000	22.920	70.00-	130.00	100.00	
11.409	11.409	(1.113)	58	364281			70.27-	130.27	102.21	
11.409	11.409	(1.113)	57	104086			0.00-	30.00	29.20	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.741	11.741	(1.146)	83	985831	25.0000	22.293	70.00- 130.00	100.00	
11.741	11.741	(1.146)	85	589435			32.38- 92.38	59.79	

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.626	12.626	(1.232)	75	822568	25.0000	22.099	70.00- 130.00	100.00	
12.626	12.626	(1.232)	77	258696			1.52- 61.52	31.45	
12.626	12.626	(1.232)	39	632684			48.26- 108.26	76.92	

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.259)	58	642296	25.0000	20.982	70.00- 130.00	100.00	
12.902	12.902	(1.259)	43	1883753			0.00- 30.00	293.28	
12.902	12.902	(1.259)	85	212522			0.00- 30.00	33.09	

103 Toluene						CAS #: 108-88-3			
13.096	13.096	(1.278)	91	1674918	25.0000	23.048	70.00- 130.00	100.00	
13.096	13.096	(1.278)	92	988440			29.45- 89.45	59.01	

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	894690	25.0000	22.036	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	266256			1.42- 61.42	29.76	
13.621	13.621	(0.895)	39	639695			43.57- 103.57	71.50	

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.897	13.897	(0.913)	97	521949	25.0000	21.887	70.00- 130.00	100.00	
13.897	13.897	(0.913)	99	318557			31.40- 91.40	61.03	
13.870	13.870	(0.911)	83	451486			60.06- 120.06	86.50	

109 Tetrachloroethene						CAS #: 127-18-4			
13.925	13.925	(0.915)	166	553653	25.0000	22.294	70.00- 130.00	100.00	
13.925	13.925	(0.915)	129	429899			46.36- 106.36	77.65	
13.925	13.925	(0.915)	131	425518			45.00- 105.00	76.86	

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	872471	25.0000	24.167	70.00- 130.00	100.00	
14.257	14.257	(0.936)	43	1780965			176.52- 236.52	204.13	
14.257	14.257	(0.936)	100	123096			0.00- 30.00	14.11	

114 Dibromochloromethane						CAS #: 124-48-1			
14.423	14.423	(0.947)	129	693588	25.0000	21.695	70.00- 130.00	100.00	
14.423	14.423	(0.947)	127	548637			0.00- 30.00	79.10	

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.589	14.589	(0.958)	107	740660	25.0000	22.538	70.00- 130.00	100.00	
14.589	14.589	(0.958)	109	692469			62.88- 122.88	93.49	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
124 Chlorobenzene						CAS #:	108-90-7			
15.252	15.252	(1.002)	112	1207014	25.0000	21.910	70.00- 130.00	100.00		
15.252	15.252	(1.002)	114	382995			0.73- 60.73	31.73		
15.252	15.252	(1.002)	77	865791			40.58- 100.58	71.73		

127 Ethyl Benzene						CAS #:	100-41-4			
15.363	15.363	(1.009)	106	680428	25.0000	22.180	70.00- 130.00	100.00		
15.363	15.363	(1.009)	91	2265782			0.00- 30.00	332.99		

128 m,p-Xylene						CAS #:	108-38-3			
15.529	15.529	(1.020)	106	873579	25.0000	22.086	70.00- 130.00	100.00		
15.529	15.529	(1.020)	91	1802209			0.00- 30.00	206.30		

130 o-Xylene						CAS #:	95-47-6			
16.054	16.054	(1.054)	106	838616	25.0000	21.854	70.00- 130.00	100.00		
16.054	16.054	(1.054)	91	1922174			195.99- 255.99	229.21		

131 Styrene						CAS #:	100-42-5			
16.082	16.082	(1.056)	104	1204987	25.0000	20.890	70.00- 130.00	100.00		
16.082	16.082	(1.056)	78	711465			28.78- 88.78	59.04		

133 Bromoform						CAS #:	75-25-2			
16.358	16.358	(1.074)	173	593128	25.0000	22.859	70.00- 130.00	100.00		
16.358	16.358	(1.074)	171	316737			21.17- 81.17	53.40		

135 Cumene						CAS #:	98-82-8			
16.524	16.524	(1.085)	105	2405704	25.0000	20.537	70.00- 130.00	100.00		
16.524	16.524	(1.085)	120	559413			0.00- 30.00	23.25		
16.496	16.496	(1.084)	51	372808			0.00- 30.00	15.50		

142 1,1,2,2-Tetrachloroethane						CAS #:	79-34-5			
16.966	16.966	(1.114)	83	1184990	25.0000	21.803	70.00- 130.00	100.00		
16.966	16.966	(1.114)	85	748184			34.35- 94.35	63.14		

143 Propylbenzene						CAS #:	103-65-1			
16.994	16.994	(1.116)	91	2960905	25.0000	22.400	70.00- 130.00	100.00		
16.994	16.994	(1.116)	120	542929			0.00- 30.00	18.34		
16.994	16.994	(1.116)	105	98090			0.00- 30.00	3.31		

145 4-Ethyltoluene						CAS #:	622-96-8			
17.132	17.132	(1.125)	105	2586366	25.0000	22.423	70.00- 130.00	100.00		
17.132	17.132	(1.125)	120	631838			0.00- 54.57	24.43		

146 1,3,5-Trimethylbenzene						CAS #:	108-67-8			
17.215	17.215	(1.131)	105	2299995	25.0000	21.018	70.00- 130.00	100.00		
17.215	17.215	(1.131)	120	981553			0.00- 30.00	42.68		

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

151	17.602	17.602	(1.156)	105	2089195	25.0000	21.244	70.00-	130.00	100.00
	17.602	17.602	(1.156)	120	847393			11.41-	71.41	40.56
	CAS #: 95-63-6									

154	17.907	17.907	(1.176)	146	937051	25.0000	22.541	70.00-	130.00	100.00
	17.907	17.907	(1.176)	148	591360			0.00-	30.00	63.11
	17.907	17.907	(1.176)	111	405175			0.00-	30.00	43.24
	CAS #: 541-73-1									

155	17.990	17.990	(1.182)	146	1143190	25.0000	21.522	70.00-	130.00	100.00
	17.990	17.990	(1.182)	148	726109			0.00-	30.00	63.52
	17.990	17.990	(1.182)	111	570439			0.00-	30.00	49.90
	CAS #: 106-46-7									

156	18.128	18.128	(1.191)	91	1677056	25.0000	22.573	70.00-	130.00	100.00
	18.128	18.128	(1.191)	126	286781			0.00-	30.00	17.10
	CAS #: 100-44-7									

158	18.321	18.321	(1.203)	146	990283	25.0000	21.171	70.00-	130.00	100.00
	18.321	18.321	(1.203)	148	626661			33.83-	93.83	63.28
	18.321	18.321	(1.203)	111	534286			21.29-	81.29	53.95
	CAS #: 95-50-1									

163	19.593	19.593	(1.287)	180	523210	25.0000	19.929	70.00-	130.00	100.00
	19.593	19.593	(1.287)	182	494582			62.06-	122.06	94.53
	CAS #: 120-82-1									

164	19.676	19.676	(1.292)	225	797028	25.0000	20.568	70.00-	130.00	100.00
	19.676	19.676	(1.292)	223	512717			35.92-	95.92	64.33
	CAS #: 87-68-3									

165	19.787	19.787	(1.300)	128	1799958	25.0000	19.884	70.00-	130.00	100.00
	19.787	19.787	(1.300)	127	250333			0.00-	30.00	13.91
	CAS #: 91-20-3									

Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032206.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv->25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	284047	0.11
86 1,4-Difluorobenze	1370859	822515	1919203	1370589	-0.02
123 Chlorobenzene-d5	1067063	640238	1493888	1101300	3.21


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 26-Mar-2007 13:58

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-26mar.b/8032607.d
 Lab Smp Id: ICAL Client Smp ID: LEVEL 5
 Inj Date : 26-MAR-2007 12:43
 Operator : ea Inst ID: msd8.i
 Smp Info : 50ml #1487-42
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /chem/msd8.i/8-26mar.b/t14q322b.m
 Meth Date : 26-Mar-2007 13:58 ealcan Quant Type: ISTD
 Cal Date : 26-MAR-2007 12:43 Cal File: 8032607.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	291821	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	224346			46.88- 106.88	76.88	
8.367	8.367	(1.000)	49	831446			254.92- 314.92	284.92	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1354208	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	254759			0.00- 48.81	18.81	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1071895	25.0000		70.00- 130.00	100.00	
15.224	15.224	(1.000)	82	702024			35.49- 95.49	65.49	

194 2-Methylpentane CAS #: 107-83-5									
5.547	5.547	(0.661)	71	933874	50.0000	39.567	70.00- 130.00	100.00	
5.547	5.547	(0.661)	43	3483599			343.03- 403.03	373.03	
5.547	5.547	(0.661)	42	1817422			164.61- 224.61	194.61	

195 Thiopene CAS #: 110-02-1									
9.833	9.833	(0.960)	84	1776200	50.0000	39.978	70.00- 130.00	100.00(T)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
195 Thiopene (continued)									
9.833	9.833	(0.960)	58	1416688			49.76- 109.76	79.76	
0.000	1.000	(0.000)	0	0			0.00- 30.00	0.00	

196 Indan									
						CAS #: 496-11-7			
18.183	18.183	(1.194)	117	3658164	50.0000	39.033	70.00- 130.00	100.00	
18.183	18.183	(1.194)	118	2078338			26.81- 86.81	56.81	
18.183	18.183	(1.194)	91	672898			0.00- 48.39	18.39	

197 Indene									
						CAS #: 95-13-6			
18.404	18.404	(1.209)	115	2351599	50.0000	38.579	70.00- 130.00	100.00(T)	
0.000	1.000	(0.000)	16	0			0.00- 30.00	0.00	

83 2,3-Dimethylpentane									
						CAS #: 565-59-3			
8.810	8.810	(1.049)	71	786693	50.0000	41.099	70.00- 130.00	100.00	
8.782	8.782	(1.046)	56	2712744			314.83- 374.83	344.83	
8.782	8.782	(1.046)	43	2371887			271.50- 331.50	301.50	

QC Flag Legend

T - Target compound detected outside RT window.

Report Date: 26-Mar-2007 13:58

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 26-MAR-2007

Lab File ID: 8032607.d

Calibration Time: 12:43

Lab Smp Id: ICAL

Client Smp ID: LEVEL 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ea

Method File: /chem/msd8.i/8-26mar.b/t14q322b.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	291821	175093	408549	291821	0.00
86 1,4-Difluorobenze	1354208	812525	1895891	1354208	0.00
123 Chlorobenzene-d5	1071895	643137	1500653	1071895	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-26mar.b/8032607.d

Date: 26-MAR-2007 12:43

Client ID: LEVEL 5

Sample Info: 50ml #1487-42


Column phase: RTX-624

Instrument: msd8.1

Operator: ea

Column diameter: 0.53

/chem/msd8.1/8-26mar.b/8032607.d



Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032207.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 22-MAR-2007 12:34
 Operator : sjr Inst ID: msd8.i
 Smp Info : 50ml 1487-115
 Misc Info : 200ppbv->50ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:09 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 12:34 Cal File: 8032207.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	283735	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	216638			46.35- 106.35	76.35	
8.367	8.367	(1.000)	49	810859			255.78- 315.78	285.78	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.247	10.247	(1.000)	114	1370859	25.0000		70.00- 130.00	100.00	
10.247	10.247	(1.000)	88	258843			0.00- 48.88	18.88	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1067063	25.0000		70.00- 130.00	100.00	
15.197	15.197	(1.000)	82	711546			36.68- 96.68	66.68	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.473	(1.128)	65	583045	25.0000	24.281	70.00- 130.00	100.00	
9.473	9.473	(1.128)	67	337682			27.92- 87.92	57.92	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	1341361	25.0000	25.054	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	169183			0.00- 42.61	12.61	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 102 Toluene-d8 (continued)									
12.985	12.985	(1.267)	100	942630			40.27- 100.27	70.27	

\$ 138 Bromofluorobenzene									
								CAS #: 460-00-4	
16.745	16.745	(1.100)	174	581586	25.0000	26.878	70.00- 130.00	100.00	
16.745	16.745	(1.100)	95	975068			137.66- 197.66	167.66	
16.773	16.773	(1.102)	176	544422			63.61- 123.61	93.61	

3 Propylene									
								CAS #: 115-07-1	
2.395	2.395	(0.285)	41	1336408	50.0000	41.722	70.00- 130.00	100.00	
2.395	2.395	(0.285)	42	871400			35.20- 95.20	65.20	
2.395	2.395	(0.285)	39	972963			42.80- 102.80	72.80	

4 Dichlorodifluoromethane/Fr12									
								CAS #: 75-71-8	
2.450	2.450	(0.292)	85	2643697	50.0000	38.305	70.00- 130.00	100.00	
2.450	2.450	(0.292)	87	843092			1.89- 61.89	31.89	

6 Freon 114									
								CAS #: 76-14-2	
2.588	2.588	(0.308)	135	1585935	50.0000	41.143	70.00- 130.00	100.00	
2.588	2.588	(0.308)	137	505651			1.88- 61.88	31.88	

8 Chloromethane									
								CAS #: 74-87-3	
2.727	2.727	(0.325)	50	1446083	50.0000	40.129	70.00- 130.00	100.00	
2.727	2.727	(0.325)	52	426042			0.00- 59.46	29.46	

9 Butane									
								CAS #: 106-97-8	
2.810	2.810	(0.335)	58	365258	50.0000	38.906	70.00- 130.00	100.00	
2.810	2.810	(0.335)	43	2932236			772.78- 832.78	802.78	

10 Vinyl Chloride									
								CAS #: 75-01-4	
2.920	2.920	(0.348)	62	1367972	50.0000	42.192	70.00- 130.00	100.00	
2.893	2.893	(0.345)	64	414838			0.33- 60.33	30.33	

11 1,3-Butadiene									
								CAS #: 106-99-0	
2.893	2.893	(0.345)	54	1369603	50.0000	40.170	70.00- 130.00	100.00	
2.893	2.893	(0.345)	39	1597009			86.60- 146.60	116.60	

13 Bromomethane									
								CAS #: 74-83-9	
3.446	3.446	(0.410)	94	693802	50.0000	39.070	70.00- 130.00	100.00	
3.446	3.446	(0.410)	96	657527			64.77- 124.77	94.77	

15 Isopentane									
								CAS #: 78-78-4	
3.556	3.556	(0.424)	43	2345298	50.0000	41.338	70.00- 130.00	100.00	
3.556	3.556	(0.424)	57	1348763			27.51- 87.51	57.51	
3.556	3.556	(0.424)	72	139482			0.00- 35.95	5.95	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

16 Chloroethane						CAS #: 75-00-3			
3.584	3.584	(0.427)	64	680681	50.0000	40.195	70.00- 130.00	100.00	
3.556	3.556	(0.424)	49	220676			2.42- 62.42	32.42	
3.556	3.556	(0.424)	66	196848			0.00- 58.92	28.92	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.888	3.888	(0.463)	101	2561964	50.0000	43.032	70.00- 130.00	100.00	
3.888	3.888	(0.463)	103	1657808			34.71- 94.71	64.71	

21 Ethanol						CAS #: 64-17-5			
4.247	4.247	(0.506)	45	605204	50.0000	43.818	70.00- 130.00	100.00	
4.247	4.247	(0.506)	43	123622			0.00- 50.43	20.43	
4.247	4.247	(0.506)	46	255462			12.21- 72.21	42.21	

27 Freon 113						CAS #: 76-13-1			
4.745	4.745	(0.565)	151	1154034	50.0000	39.775	70.00- 130.00	100.00	
4.745	4.745	(0.565)	153	723187			32.67- 92.67	62.67	
4.745	4.745	(0.565)	101	1786742			124.83- 184.83	154.83	

29 1,1-Dichloroethene						CAS #: 75-35-4			
4.773	4.773	(0.569)	61	1945054	50.0000	39.459	70.00- 130.00	100.00	
4.773	4.773	(0.569)	96	877311			15.10- 75.10	45.10	
4.773	4.773	(0.569)	98	547880			0.00- 58.17	28.17	

30 Acetone						CAS #: 67-64-1			
4.939	4.939	(0.588)	58	707567	50.0000	39.866	70.00- 130.00	100.00	
4.939	4.939	(0.588)	43	2599224			337.35- 397.35	367.35	

33 Carbon Disulfide						CAS #: 75-15-0			
5.132	5.132	(0.611)	76	3063615	50.0000	40.532	70.00- 130.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
5.160	5.160	(0.615)	45	3004294	50.0000	45.138	70.00- 130.00	100.00	
5.132	5.132	(0.611)	43	620101			0.00- 50.64	20.64	
5.160	5.160	(0.615)	59	96296			0.00- 33.21	3.21	

37 3-Chloropropene						CAS #: 107-05-1			
5.436	5.436	(0.648)	76	523387	50.0000	43.233	70.00- 130.00	100.00	
5.436	5.436	(0.648)	41	2326588			414.53- 474.53	444.53	

39 Methylene Chloride						CAS #: 75-09-2			
5.685	5.685	(0.677)	49	1646381	50.0000	39.149	70.00- 130.00	100.00	
5.713	5.713	(0.681)	84	797447			18.44- 78.44	48.44	
5.685	5.685	(0.677)	51	492691			0.00- 59.93	29.93	

42 MTBE						CAS #: 1634-04-4			
6.045	6.045	(0.720)	73	3368161	50.0000	40.042	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.045	6.045	(0.720)	57	987717			0.00- 59.33	29.33	
6.045	6.045	(0.720)	41	1076052			1.95- 61.95	31.95	

43 trans-1,2-Dichloroethene CAS #: 156-60-5									
6.100	6.100	(0.727)	96	967537	50.0000	37.943	70.00- 130.00	100.00	
6.100	6.100	(0.727)	61	1934805			169.97- 229.97	199.97	
6.100	6.100	(0.727)	98	626055			34.71- 94.71	64.71	

45 Hexane CAS #: 110-54-3									
6.432	6.432	(0.766)	57	2494698	50.0000	40.270	70.00- 130.00	100.00	
6.432	6.432	(0.766)	43	1861340			44.61- 104.61	74.61	
6.459	6.459	(0.769)	86	343624			0.00- 43.77	13.77	

52 1,1-Dichloroethane CAS #: 75-34-3									
6.902	6.902	(0.822)	63	2201347	50.0000	42.739	70.00- 130.00	100.00	
6.902	6.902	(0.822)	65	651146			0.00- 59.58	29.58	

54 Vinyl Acetate CAS #: 108-05-4									
6.957	6.957	(0.829)	86	296991	50.0000	51.257	70.00- 130.00	100.00	
6.957	6.957	(0.829)	43	4453738			1469.62-1529.62	1499.62	
6.957	6.957	(0.829)	42	386333			100.08- 160.08	130.08	

63 cis-1,2-Dichloroethene CAS #: 156-59-2									
7.952	7.952	(0.947)	61	1618525	50.0000	41.336	70.00- 130.00	100.00	
7.952	7.952	(0.947)	96	928352			27.36- 87.36	57.36	
7.952	7.952	(0.947)	98	579920			5.83- 65.83	35.83	

64 2-Butanone CAS #: 78-93-3									
7.980	7.980	(0.951)	72	555279	50.0000	38.546	70.00- 130.00	100.00	
7.980	7.980	(0.951)	43	3355513			574.29- 634.29	604.29	
7.980	7.980	(0.951)	57	225503			10.61- 70.61	40.61	

66 Tetrahydrofuran CAS #: 109-99-9									
8.367	8.367	(0.997)	42	2017304	50.0000	37.255	70.00- 130.00	100.00	
8.367	8.367	(0.997)	71	502892			0.00- 54.93	24.93	
8.367	8.367	(0.997)	72	534966			0.00- 56.52	26.52	

69 Chloroform CAS #: 67-66-3									
8.505	8.505	(1.013)	83	1830986	50.0000	36.077	70.00- 130.00	100.00	
8.505	8.505	(1.013)	85	1166454			33.71- 93.71	63.71	

72 Cyclohexane CAS #: 110-82-7									
8.727	8.727	(1.040)	84	1458593	50.0000	38.689	70.00- 130.00	100.00	
8.727	8.727	(1.040)	56	2460409			138.68- 198.68	168.68	
8.727	8.727	(1.040)	41	1514191			73.81- 133.81	103.81	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

73	1,1,1-Trichloroethane					CAS #: 71-55-6				
8.754	8.754	(1.043)	97	1820730	50.0000	40.416	70.00- 130.00	100.00		
8.754	8.754	(1.043)	99	1164340			33.95- 93.95	63.95		

75	Carbon Tetrachloride					CAS #: 56-23-5				
9.003	9.003	(1.072)	119	1530499	50.0000	42.601	70.00- 130.00	100.00		
9.003	9.003	(1.072)	117	1709055			81.67- 141.67	111.67		

78	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.418	9.418	(1.122)	57	7210928	50.0000	42.003	70.00- 130.00	100.00		
9.446	9.446	(1.125)	56	2483917			4.45- 64.45	34.45		
9.418	9.418	(1.122)	41	2123088			0.00- 59.44	29.44		

79	Benzene					CAS #: 71-43-2				
9.418	9.418	(0.919)	78	3194794	50.0000	38.756	70.00- 130.00	100.00		
9.418	9.418	(0.919)	77	779333			0.00- 54.39	24.39		

81	1,2-Dichloroethane					CAS #: 107-06-2				
9.611	9.611	(0.938)	62	1566874	50.0000	40.725	70.00- 130.00	100.00		
9.611	9.611	(0.938)	64	492564			1.44- 61.44	31.44		

82	Heptane					CAS #: 142-82-5				
9.805	9.805	(0.957)	100	374296	50.0000	36.962	70.00- 130.00	100.00		
9.805	9.805	(0.957)	43	3067958			789.66- 849.66	819.66		
9.805	9.805	(0.957)	71	1213714			294.27- 354.27	324.27		

92	Trichloroethene					CAS #: 79-01-6				
10.662	10.662	(1.040)	95	1109731	50.0000	42.147	70.00- 130.00	100.00		
10.662	10.662	(1.040)	130	966953			57.13- 117.13	87.13		
10.662	10.662	(1.040)	97	693589			32.50- 92.50	62.50		

93	Methyl Cyclohexane					CAS #: 108-87-2				
10.883	10.883	(1.296)	83	1874222	50.0000	40.099	70.00- 130.00	100.00		
10.911	10.911	(1.300)	98	843453			15.00- 75.00	45.00		
10.883	10.883	(1.296)	55	2196126			87.18- 147.18	117.18		

95	1,2-Dichloropropane					CAS #: 78-87-5				
11.187	11.187	(1.092)	63	1234251	50.0000	40.899	70.00- 130.00	100.00		
11.187	11.187	(1.092)	62	926110			45.03- 105.03	75.03		
11.187	11.187	(1.092)	41	932094			45.52- 105.52	75.52		

96	1,4-Dioxane					CAS #: 123-91-1				
11.409	11.409	(1.113)	88	682915	50.0000	43.909	70.00- 130.00	100.00		
11.409	11.409	(1.113)	58	684769			70.27- 130.27	100.27		
11.409	11.409	(1.113)	57	208541			0.54- 60.54	30.54		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.740	11.740	(1.146)	83	1848691	50.0000	41.797	70.00- 130.00	100.00	
11.740	11.740	(1.146)	85	1153190			32.38- 92.38	62.38	

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.625	12.625	(1.232)	75	1587750	50.0000	42.648	70.00- 130.00	100.00	
12.625	12.625	(1.232)	77	500399			1.52- 61.52	31.52	
12.625	12.625	(1.232)	39	1242642			48.26- 108.26	78.26	

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.259)	58	1264881	50.0000	41.312	70.00- 130.00	100.00	
12.902	12.902	(1.259)	43	3556128			251.14- 311.14	281.14	
12.902	12.902	(1.259)	85	408924			2.33- 62.33	32.33	

103 Toluene						CAS #: 108-88-3			
13.095	13.095	(1.278)	91	3201294	50.0000	44.044	70.00- 130.00	100.00	
13.095	13.095	(1.278)	92	1903249			29.45- 89.45	59.45	

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	1684729	50.0000	42.825	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	529324			1.42- 61.42	31.42	
13.621	13.621	(0.895)	39	1239393			43.57- 103.57	73.57	

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.897	13.897	(0.913)	97	977558	50.0000	42.307	70.00- 130.00	100.00	
13.897	13.897	(0.913)	99	600253			31.40- 91.40	61.40	
13.869	13.869	(0.911)	83	880417			60.06- 120.06	90.06	

109 Tetrachloroethene						CAS #: 127-18-4			
13.925	13.925	(0.915)	166	1071236	50.0000	44.520	70.00- 130.00	100.00	
13.925	13.925	(0.915)	129	817997			46.36- 106.36	76.36	
13.925	13.925	(0.915)	131	803418			45.00- 105.00	75.00	

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	1676318	50.0000	47.923	70.00- 130.00	100.00	
14.257	14.257	(0.936)	43	3461935			176.52- 236.52	206.52	
14.257	14.257	(0.936)	100	262861			0.00- 45.68	15.68	

114 Dibromochloromethane						CAS #: 124-48-1			
14.422	14.422	(0.947)	129	1342940	50.0000	43.354	70.00- 130.00	100.00	
14.422	14.422	(0.947)	127	1033514			46.96- 106.96	76.96	

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.588	14.588	(0.958)	107	1401072	50.0000	44.002	70.00- 130.00	100.00	
14.588	14.588	(0.958)	109	1301357			62.88- 122.88	92.88	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
124 Chlorobenzene						CAS #: 108-90-7			
15.252	15.252	(1.002)	112	2347440	50.0000	43.979	70.00- 130.00	100.00	
15.252	15.252	(1.002)	114	721344			0.73- 60.73	30.73	
15.252	15.252	(1.002)	77	1656838			40.58- 100.58	70.58	

127 Ethyl Benzene						CAS #: 100-41-4			
15.363	15.363	(1.009)	106	1291684	50.0000	43.455	70.00- 130.00	100.00	
15.363	15.363	(1.009)	91	4390490			309.90- 369.90	339.90	

128 m,p-Xylene						CAS #: 108-38-3			
15.528	15.528	(1.020)	106	1673125	50.0000	43.658	70.00- 130.00	100.00	
15.528	15.528	(1.020)	91	3469703			177.38- 237.38	207.38	

130 o-Xylene						CAS #: 95-47-6			
16.054	16.054	(1.054)	106	1592825	50.0000	42.841	70.00- 130.00	100.00	
16.054	16.054	(1.054)	91	3599628			195.99- 255.99	225.99	

131 Styrene						CAS #: 100-42-5			
16.081	16.081	(1.056)	104	2378760	50.0000	42.561	70.00- 130.00	100.00	
16.081	16.081	(1.056)	78	1398236			28.78- 88.78	58.78	

133 Bromoform						CAS #: 75-25-2			
16.358	16.358	(1.074)	173	1181942	50.0000	47.014	70.00- 130.00	100.00	
16.358	16.358	(1.074)	171	604836			21.17- 81.17	51.17	

135 Cumene						CAS #: 98-82-8			
16.524	16.524	(1.085)	105	4566296	50.0000	40.232	70.00- 130.00	100.00	
16.524	16.524	(1.085)	120	1056482			0.00- 53.14	23.14	
16.496	16.496	(1.084)	51	702949			0.00- 45.39	15.39	

142 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5			
16.966	16.966	(1.114)	83	2276949	50.0000	43.238	70.00- 130.00	100.00	
16.966	16.966	(1.114)	85	1465188			34.35- 94.35	64.35	

143 Propylbenzene						CAS #: 103-65-1			
16.994	16.994	(1.116)	91	5640137	50.0000	44.037	70.00- 130.00	100.00	
16.994	16.994	(1.116)	120	1059941			0.00- 48.79	18.79	
16.994	16.994	(1.116)	105	188920			0.00- 33.35	3.35	

145 4-Ethyltoluene						CAS #: 622-96-8			
17.132	17.132	(1.125)	105	5072880	50.0000	45.392	70.00- 130.00	100.00	
17.132	17.132	(1.125)	120	1246244			0.00- 54.57	24.57	

146 1,3,5-Trimethylbenzene						CAS #: 108-67-8			
17.215	17.215	(1.131)	105	4377709	50.0000	41.288	70.00- 130.00	100.00	
17.215	17.215	(1.131)	120	1866622			12.64- 72.64	42.64	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

151	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
17.602	17.602	(1.156)	105	3993702	50.0000	41.912	70.00- 130.00	100.00	
17.602	17.602	(1.156)	120	1653770			11.41- 71.41	41.41	

154	1,3-Dichlorobenzene					CAS #: 541-73-1			
17.906	17.906	(1.176)	146	1880169	50.0000	46.679	70.00- 130.00	100.00	
17.906	17.906	(1.176)	148	1169490			32.20- 92.20	62.20	
17.879	17.879	(1.174)	111	813794			13.28- 73.28	43.28	

155	1,4-Dichlorobenzene					CAS #: 106-46-7			
17.989	17.989	(1.182)	146	2312899	50.0000	44.940	70.00- 130.00	100.00	
17.989	17.989	(1.182)	148	1483842			34.16- 94.16	64.16	
17.989	17.989	(1.182)	111	1073528			16.41- 76.41	46.41	

156	alpha-Chlorotoluene					CAS #: 100-44-7			
18.127	18.127	(1.191)	91	3524875	50.0000	48.968	70.00- 130.00	100.00	
18.127	18.127	(1.191)	126	598031			0.00- 46.97	16.97	

158	1,2-Dichlorobenzene					CAS #: 95-50-1			
18.321	18.321	(1.203)	146	1968486	50.0000	43.435	70.00- 130.00	100.00	
18.321	18.321	(1.203)	148	1256428			33.83- 93.83	63.83	
18.321	18.321	(1.203)	111	1009554			21.29- 81.29	51.29	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.593	19.593	(1.287)	180	1246406	50.0000	49.000	70.00- 130.00	100.00	
19.593	19.593	(1.287)	182	1147386			62.06- 122.06	92.06	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.676	19.676	(1.292)	225	1473379	50.0000	39.242	70.00- 130.00	100.00	
19.676	19.676	(1.292)	223	971308			35.92- 95.92	65.92	

165	Naphthalene					CAS #: 91-20-3			
19.786	19.786	(1.300)	128	3925545	50.0000	44.755	70.00- 130.00	100.00	
19.786	19.786	(1.300)	127	538768			0.00- 43.72	13.72	

Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032207.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv->50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	283735	0.00
86 1,4-Difluorobenze	1370859	822515	1919203	1370859	0.00
123 Chlorobenzene-d5	1067063	640238	1493888	1067063	0.00


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.39	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032208.d
 Lab Smp Id: ICAL Client Smp ID: Level 6
 Inj Date : 22-MAR-2007 13:02
 Operator : sjr Inst ID: msd8.i
 Smp Info : 100ml 1487-115
 Misc Info : 200ppbv->100ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:09 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 13:02 Cal File: 8032208.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	274410	25.0000		70.00- 130.00	100.00	
8.367	8.367	(1.000)	128	219163			46.35- 106.35	79.87	
8.367	8.367	(1.000)	49	829492			255.78- 315.78	302.28	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1375928	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	254568			0.00- 48.88	18.50	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1061257	25.0000		70.00- 130.00	100.00	
15.197	15.197	(1.000)	82	723053			36.68- 96.68	68.13	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.473	(1.128)	65	598928	25.0000	25.655	70.00- 130.00	100.00	
9.473	9.473	(1.128)	67	388652			27.92- 87.92	64.89	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	1363568	25.0000	25.312	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	193391			0.00- 42.61	14.18	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 102 Toluene-d8 (continued)										
12.985	12.985	(1.267)	100	1047544			40.27- 100.27	76.82		

\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.745	16.745	(1.100)	174	558459	25.0000	25.787	70.00- 130.00	100.00		
16.745	16.745	(1.100)	95	992994			137.66- 197.66	177.81		
16.745	16.745	(1.100)	176	541545			63.61- 123.61	96.97		

3 Propylene						CAS #:	115-07-1			
2.395	2.395	(0.285)	41	2618213	100.000	87.920	70.00- 130.00	100.00		
2.395	2.395	(0.285)	42	1727704			35.20- 95.20	65.99		
2.395	2.395	(0.285)	39	1908330			42.80- 102.80	72.89		

4 Dichlorodifluoromethane/Fr12						CAS #:	75-71-8			
2.450	2.450	(0.292)	85	5165186	100.000	81.048	70.00- 130.00	100.00		
2.450	2.450	(0.292)	87	1658624			1.89- 61.89	32.11		

6 Freon 114						CAS #:	76-14-2			
2.616	2.616	(0.312)	135	3080858	100.000	85.614	70.00- 130.00	100.00		
2.616	2.616	(0.312)	137	966687			1.88- 61.88	31.38		

8 Chloromethane						CAS #:	74-87-3			
2.727	2.727	(0.325)	50	2730912	100.000	82.840	70.00- 130.00	100.00		
2.727	2.727	(0.325)	52	817475			0.00- 59.46	29.93		

9 Butane						CAS #:	106-97-8			
2.810	2.810	(0.335)	58	698080	100.000	81.599	70.00- 130.00	100.00		
2.810	2.810	(0.335)	43	5628034			772.78- 832.78	806.22		

10 Vinyl Chloride						CAS #:	75-01-4			
2.920	2.920	(0.348)	62	2663225	100.000	87.571	70.00- 130.00	100.00		
2.920	2.920	(0.348)	64	808264			0.33- 60.33	30.35		

11 1,3-Butadiene						CAS #:	106-99-0			
2.893	2.893	(0.345)	54	2662607	100.000	83.980	70.00- 130.00	100.00		
2.893	2.893	(0.345)	39	3839969			86.60- 146.60	144.22		

13 Bromomethane						CAS #:	74-83-9			
3.446	3.446	(0.410)	94	1439798	100.000	86.635	70.00- 130.00	100.00		
3.446	3.446	(0.410)	96	1295850			64.77- 124.77	90.00		

15 Isopentane						CAS #:	78-78-4			
3.556	3.556	(0.424)	43	4528672	100.000	86.303	70.00- 130.00	100.00		
3.556	3.556	(0.424)	57	2630973			27.51- 87.51	58.10		
3.556	3.556	(0.424)	72	266218			0.00- 35.95	5.88		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

16 Chloroethane						CAS #: 75-00-3			
3.584	3.584	(0.427)	64	1367985	100.000	86.372	70.00- 130.00	100.00	
3.584	3.584	(0.427)	49	426326			2.42- 62.42	31.16	
3.584	3.584	(0.427)	66	409887			0.00- 58.92	29.96	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.888	3.888	(0.463)	101	5036405	100.000	89.717	70.00- 130.00	100.00	
3.888	3.888	(0.463)	103	3222575			34.71- 94.71	63.99	

21 Ethanol						CAS #: 64-17-5			
4.275	4.275	(0.509)	45	1124988	100.000	87.679	70.00- 130.00	100.00	
4.275	4.275	(0.509)	43	236899			0.00- 50.43	21.06	
4.275	4.275	(0.509)	46	475472			12.21- 72.21	42.26	

27 Freon 113						CAS #: 76-13-1			
4.745	4.745	(0.565)	151	2249177	100.000	83.467	70.00- 130.00	100.00	
4.745	4.745	(0.565)	153	1390357			32.67- 92.67	61.82	
4.745	4.745	(0.565)	101	3469458			124.83- 184.83	154.25	

29 1,1-Dichloroethene						CAS #: 75-35-4			
4.773	4.773	(0.569)	61	3818502	100.000	83.418	70.00- 130.00	100.00	
4.773	4.773	(0.569)	96	1663923			15.10- 75.10	43.58	
4.773	4.773	(0.569)	98	1077180			0.00- 58.17	28.21	

30 Acetone						CAS #: 67-64-1			
4.939	4.939	(0.588)	58	1396656	100.000	85.340	70.00- 130.00	100.00	
4.939	4.939	(0.588)	43	5093705			337.35- 397.35	364.71	

33 Carbon Disulfide						CAS #: 75-15-0			
5.132	5.132	(0.611)	76	5918817	100.000	84.172	70.00- 130.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
5.160	5.160	(0.615)	45	5917346	100.000	93.820	70.00- 130.00	100.00	
5.160	5.160	(0.615)	43	1171046			0.00- 50.64	19.79	
5.160	5.160	(0.615)	59	195660			0.00- 33.21	3.31	

37 3-Chloropropene						CAS #: 107-05-1			
5.437	5.437	(0.648)	76	1017552	100.000	89.849	70.00- 130.00	100.00	
5.437	5.437	(0.648)	41	4591103			414.53- 474.53	451.19	

39 Methylene Chloride						CAS #: 75-09-2			
5.713	5.713	(0.681)	49	3236926	100.000	82.973	70.00- 130.00	100.00	
5.713	5.713	(0.681)	84	1550495			18.44- 78.44	47.90	
5.713	5.713	(0.681)	51	949361			0.00- 59.93	29.33	

42 MTBE						CAS #: 1634-04-4			
6.045	6.045	(0.720)	73	6577424	100.000	84.072	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.045	6.045	(0.720)	57	1977342			0.00- 59.33	30.06	
6.045	6.045	(0.720)	41	2097752			1.95- 61.95	31.89	

43 trans-1,2-Dichloroethene					CAS #: 156-60-5				
6.100	6.100	(0.727)	96	1890823	100.000	80.423	70.00- 130.00	100.00	
6.100	6.100	(0.727)	61	3716781			169.97- 229.97	196.57	
6.100	6.100	(0.727)	98	1203185			34.71- 94.71	63.63	

45 Hexane					CAS #: 110-54-3				
6.460	6.460	(0.769)	57	4810920	100.000	83.593	70.00- 130.00	100.00	
6.432	6.432	(0.766)	43	3611629			44.61- 104.61	75.07	
6.460	6.460	(0.769)	86	673414			0.00- 43.77	14.00	

52 1,1-Dichloroethane					CAS #: 75-34-3				
6.902	6.902	(0.822)	63	4203914	100.000	87.111	70.00- 130.00	100.00	
6.902	6.902	(0.822)	65	1256075			0.00- 59.58	29.88	

54 Vinyl Acetate					CAS #: 108-05-4				
6.957	6.957	(0.829)	86	561325	100.000	100.13	70.00- 130.00	100.00	
6.957	6.957	(0.829)	43	8762705			1469.62-1529.62	1561.08	
6.957	6.957	(0.829)	42	753113			100.08- 160.08	134.17	

63 cis-1,2-Dichloroethene					CAS #: 156-59-2				
7.953	7.953	(0.947)	61	3211133	100.000	87.457	70.00- 130.00	100.00	
7.953	7.953	(0.947)	96	1802223			27.36- 87.36	56.12	
7.953	7.953	(0.947)	98	1120011			5.83- 65.83	34.88	

64 2-Butanone					CAS #: 78-93-3				
7.980	7.980	(0.951)	72	1085412	100.000	81.509	70.00- 130.00	100.00	
7.980	7.980	(0.951)	43	6532458			574.29- 634.29	601.84	
7.980	7.980	(0.951)	57	434813			10.61- 70.61	40.06	

66 Tetrahydrofuran					CAS #: 109-99-9				
8.367	8.367	(0.997)	42	3913572	100.000	78.708	70.00- 130.00	100.00	
8.367	8.367	(0.997)	71	979340			0.00- 54.93	25.02	
8.367	8.367	(0.997)	72	1068465			0.00- 56.52	27.30	

69 Chloroform					CAS #: 67-66-3				
8.506	8.506	(1.013)	83	3587527	100.000	76.522	70.00- 130.00	100.00	
8.506	8.506	(1.013)	85	2300838			33.71- 93.71	64.13	

72 Cyclohexane					CAS #: 110-82-7				
8.727	8.727	(1.040)	84	2843440	100.000	81.577	70.00- 130.00	100.00	
8.727	8.727	(1.040)	56	4887392			138.68- 198.68	171.88	
8.727	8.727	(1.040)	41	2925031			73.81- 133.81	102.87	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

73	1,1,1-Trichloroethane					CAS #: 71-55-6				
8.754	8.754	(1.043)	97	3564210	100.000	84.896	70.00- 130.00	100.00		
8.754	8.754	(1.043)	99	2252502			33.95- 93.95	63.20		

75	Carbon Tetrachloride					CAS #: 56-23-5				
9.003	9.003	(1.072)	119	2964590	100.000	87.903	70.00- 130.00	100.00		
9.003	9.003	(1.072)	117	3302720			81.67- 141.67	111.41		

78	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.446	9.446	(1.125)	57	14024361	100.000	87.175	70.00- 130.00	100.00		
9.446	9.446	(1.125)	56	4907939			4.45- 64.45	35.00		
9.446	9.446	(1.125)	41	4092884			0.00- 59.44	29.18		

79	Benzene					CAS #: 71-43-2				
9.418	9.418	(0.919)	78	6216949	100.000	78.388	70.00- 130.00	100.00		
9.418	9.418	(0.919)	77	1485753			0.00- 54.39	23.90		

81	1,2-Dichloroethane					CAS #: 107-06-2				
9.612	9.612	(0.938)	62	3077011	100.000	83.056	70.00- 130.00	100.00		
9.612	9.612	(0.938)	64	957111			1.44- 61.44	31.11		

82	Heptane					CAS #: 142-82-5				
9.805	9.805	(0.957)	100	727731	100.000	75.911	70.00- 130.00	100.00		
9.805	9.805	(0.957)	43	6016039			789.66- 849.66	826.68		
9.805	9.805	(0.957)	71	2332656			294.27- 354.27	320.54		

92	Trichloroethene					CAS #: 79-01-6				
10.662	10.662	(1.040)	95	2140717	100.000	84.202	70.00- 130.00	100.00		
10.662	10.662	(1.040)	130	1842017			57.13- 117.13	86.05		
10.662	10.662	(1.040)	97	1345032			32.50- 92.50	62.83		

93	Methyl Cyclohexane					CAS #: 108-87-2				
10.911	10.911	(1.300)	83	3627158	100.000	83.541	70.00- 130.00	100.00		
10.911	10.911	(1.300)	98	1658014			15.00- 75.00	45.71		
10.883	10.883	(1.296)	55	4177340			87.18- 147.18	115.17		

95	1,2-Dichloropropane					CAS #: 78-87-5				
11.188	11.188	(1.092)	63	2399132	100.000	82.643	70.00- 130.00	100.00		
11.188	11.188	(1.092)	62	1815553			45.03- 105.03	75.68		
11.188	11.188	(1.092)	41	1814245			45.52- 105.52	75.62		

96	1,4-Dioxane					CAS #: 123-91-1				
11.409	11.409	(1.113)	88	1330284	100.000	88.488	70.00- 130.00	100.00		
11.409	11.409	(1.113)	58	1317282			70.27- 130.27	99.02		
11.409	11.409	(1.113)	57	412040			0.54- 60.54	30.97		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.741	11.741	(1.146)	83	3623259	100.000	84.732	70.00- 130.00	100.00	
11.741	11.741	(1.146)	85	2296301			32.38- 92.38	63.38	

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.625	12.625	(1.232)	75	3193433	100.000	88.022	70.00- 130.00	100.00	
12.625	12.625	(1.232)	77	980903			1.52- 61.52	30.72	
12.598	12.598	(1.229)	39	2427968			48.26- 108.26	76.03	

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.259)	58	2452733	100.000	83.171	70.00- 130.00	100.00	
12.902	12.902	(1.259)	43	7163978			251.14- 311.14	292.08	
12.902	12.902	(1.259)	85	787723			2.33- 62.33	32.12	

103 Toluene						CAS #: 108-88-3			
13.095	13.095	(1.278)	91	6267602	100.000	88.404	70.00- 130.00	100.00	
13.095	13.095	(1.278)	92	3773465			29.45- 89.45	60.21	

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	3305187	100.000	87.183	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	1023953			1.42- 61.42	30.98	
13.621	13.621	(0.895)	39	2407291			43.57- 103.57	72.83	

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.897	13.897	(0.913)	97	1913808	100.000	86.161	70.00- 130.00	100.00	
13.897	13.897	(0.913)	99	1142609			31.40- 91.40	59.70	
13.870	13.870	(0.911)	83	1742327			60.06- 120.06	91.04	

109 Tetrachloroethene						CAS #: 127-18-4			
13.925	13.925	(0.915)	166	2121016	100.000	90.693	70.00- 130.00	100.00	
13.925	13.925	(0.915)	129	1630806			46.36- 106.36	76.89	
13.925	13.925	(0.915)	131	1573448			45.00- 105.00	74.18	

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	3377651	100.000	97.801	70.00- 130.00	100.00	
14.257	14.257	(0.936)	43	6644301			176.52- 236.52	196.71	
14.257	14.257	(0.936)	100	491901			0.00- 45.68	14.56	

114 Dibromochloromethane						CAS #: 124-48-1			
14.423	14.423	(0.947)	129	2640038	100.000	88.219	70.00- 130.00	100.00	
14.423	14.423	(0.947)	127	2071838			46.96- 106.96	78.48	

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.589	14.589	(0.958)	107	2779224	100.000	89.964	70.00- 130.00	100.00	
14.589	14.589	(0.958)	109	2584978			62.88- 122.88	93.01	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
124 Chlorobenzene						CAS #: 108-90-7			
15.252	15.252	(1.002)	112	4418200	100.000	86.116	70.00- 130.00	100.00	
15.252	15.252	(1.002)	114	1396554			0.73- 60.73	31.61	
15.252	15.252	(1.002)	77	3350897			40.58- 100.58	75.84	

127 Ethyl Benzene						CAS #: 100-41-4			
15.363	15.363	(1.009)	106	2505821	100.000	87.427	70.00- 130.00	100.00	
15.363	15.363	(1.009)	91	8779160			309.90- 369.90	350.35	

128 m,p-Xylene						CAS #: 108-38-3			
15.529	15.529	(1.020)	106	3236516	100.000	87.557	70.00- 130.00	100.00	
15.529	15.529	(1.020)	91	6982531			177.38- 237.38	215.74	

130 o-Xylene						CAS #: 95-47-6			
16.054	16.054	(1.054)	106	3064463	100.000	85.813	70.00- 130.00	100.00	
16.054	16.054	(1.054)	91	7129975			195.99- 255.99	232.67	

131 Styrene						CAS #: 100-42-5			
16.082	16.082	(1.056)	104	4834510	100.000	88.904	70.00- 130.00	100.00	
16.082	16.082	(1.056)	78	2868142			28.78- 88.78	59.33	

133 Bromoform						CAS #: 75-25-2			
16.358	16.358	(1.074)	173	2259499	100.000	92.143	70.00- 130.00	100.00	
16.358	16.358	(1.074)	171	1149935			21.17- 81.17	50.89	

135 Cumene						CAS #: 98-82-8			
16.524	16.524	(1.085)	105	8919536	100.000	81.880	70.00- 130.00	100.00	
16.524	16.524	(1.085)	120	2075981			0.00- 53.14	23.27	
16.496	16.496	(1.084)	51	1377696			0.00- 45.39	15.45	

142 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5			
16.966	16.966	(1.114)	83	4515433	100.000	88.659	70.00- 130.00	100.00	
16.966	16.966	(1.114)	85	2869533			34.35- 94.35	63.55	

143 Propylbenzene						CAS #: 103-65-1			
16.994	16.994	(1.116)	91	11424449	100.000	91.577	70.00- 130.00	100.00	
16.994	16.994	(1.116)	120	1995294			0.00- 48.79	17.47	
16.994	16.994	(1.116)	105	392922			0.00- 33.35	3.44	

145 4-Ethyltoluene						CAS #: 622-96-8			
17.132	17.132	(1.125)	105	10175388	100.000	93.121	70.00- 130.00	100.00	
17.132	17.132	(1.125)	120	2508882			0.00- 54.57	24.66	

146 1,3,5-Trimethylbenzene						CAS #: 108-67-8			
17.215	17.215	(1.131)	105	8697612	100.000	85.474	70.00- 130.00	100.00	
17.215	17.215	(1.131)	120	3667776			12.64- 72.64	42.17	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

151	17.602	17.602	105	7984521	100.000	86.992	70.00- 130.00	100.00	
	17.602	(1.156)	120	3290133			11.41- 71.41	41.21	
	CAS #: 95-63-6								

154	17.906	17.906	146	3592491	100.000	91.569	70.00- 130.00	100.00	
	17.906	(1.176)	148	2270275			32.20- 92.20	63.20	
	17.879	(1.174)	111	1698157			13.28- 73.28	47.27	
	CAS #: 541-73-1								

155	17.989	17.989	146	4959897	100.000	97.504	70.00- 130.00	100.00	
	17.989	(1.182)	148	3107048			34.16- 94.16	62.64	
	17.989	(1.182)	111	2095150			16.41- 76.41	42.24	
	CAS #: 106-46-7								

156	18.128	18.128	91	7090361	100.000	99.229	70.00- 130.00	100.00	
	18.128	(1.191)	126	1205592			0.00- 46.97	17.00	
	CAS #: 100-44-7								

158	18.321	18.321	146	3753348	100.000	86.154	70.00- 130.00	100.00	
	18.321	(1.203)	148	2318870			33.83- 93.83	61.78	
	18.321	(1.203)	111	1975932			21.29- 81.29	52.64	
	CAS #: 95-50-1								

163	19.593	19.593	180	2760569	100.000	106.69	70.00- 130.00	100.00	
	19.593	(1.287)	182	2604598			62.06- 122.06	94.35	
	CAS #: 120-82-1								

164	19.676	19.676	225	2866710	100.000	81.503	70.00- 130.00	100.00	
	19.676	(1.292)	223	1823041			35.92- 95.92	63.59	
	CAS #: 87-68-3								

165	19.787	19.787	128	8609290	100.000	99.016	70.00- 130.00	100.00	
	19.787	(1.300)	127	1214285			0.00- 43.72	14.10	
	CAS #: 91-20-3								

Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032208.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv->100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	274410	-3.29
86 1,4-Difluorobenze	1370859	822515	1919203	1375928	0.37
123 Chlorobenzene-d5	1067063	640238	1493888	1061257	-0.54

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22mar.b/8032208.d
Date: 22-MAR-2007 13:02
Client ID: Level 6
Sample Info: 100ml 1487-115

Column phase: RTX-624

Instrument: msd8.1
Operator: sjr
Column diameter: 0.53

/chem/msd8.1/8-22mar.b/8032208.d



Report Date: 26-Mar-2007 13:58

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-26mar.b/8032608.d
 Lab Smp Id: ICAL Client Smp ID: LEVEL 7
 Inj Date : 26-MAR-2007 13:11
 Operator : ea Inst ID: msd8.i
 Smp Info : 200ml #1487-42
 Misc Info : 200ppbv-200ppbv
 Comment :
 Method : /chem/msd8.i/8-26mar.b/t14q322b.m
 Meth Date : 26-Mar-2007 13:58 ealcan Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	281494	25.0000			70.00- 130.00	100.00
8.395	8.395	(1.000)	128	230544				46.88- 106.88	81.90
8.367	8.367	(1.000)	49	801676				254.92- 314.92	284.79

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1332533	25.0000			70.00- 130.00	100.00
10.248	10.248	(1.000)	88	260063				0.00- 48.81	19.52

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1030363	25.0000			70.00- 130.00	100.00
15.197	15.197	(1.000)	82	675300				35.49- 95.49	65.54

194 2-Methylpentane CAS #: 107-83-5									
5.519	5.519	(0.657)	71	3347631	200.000	161.28		70.00- 130.00	100.00
5.519	5.519	(0.657)	43	13000628				343.03- 403.03	388.35
5.519	5.519	(0.657)	42	6719106				164.61- 224.61	200.71

195 Thiopene CAS #: 110-02-1									
9.833	9.833	(0.960)	84	6737660	200.000	166.88		70.00- 130.00	100.00(T)

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
195 Thiopene (continued)									
9.833	9.833	(0.960)	58	5424886			49.76- 109.76	80.52	
0.000	1.000	(0.000)	0	0			0.00- 30.00	0.00	

196 Indan									
						CAS #: 496-11-7			
18.183	18.183	(1.194)	117	14309681	200.000	170.54	70.00- 130.00	100.00	
18.183	18.183	(1.194)	118	8094903			26.81- 86.81	56.57	
18.183	18.183	(1.194)	91	2643183			0.00- 48.39	18.47	

197 Indene									
						CAS #: 95-13-6			
18.404	18.404	(1.209)	115	9753957	200.000	176.32	70.00- 130.00	100.00(T)	
0.000	1.000	(0.000)	16	0			0.00- 30.00	0.00	

83 2,3-Dimethylpentane									
						CAS #: 565-59-3			
8.782	8.782	(1.046)	71	2877196	200.000	168.21	70.00- 130.00	100.00	
8.782	8.782	(1.046)	56	10172829			314.83- 374.83	353.57	
8.782	8.782	(1.046)	43	8826150			271.50- 331.50	306.76	

QC Flag Legend

T - Target compound detected outside RT window.

Report Date: 26-Mar-2007 13:58

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 26-MAR-2007

Lab File ID: 8032608.d

Calibration Time: 12:43

Lab Smp Id: ICAL

Client Smp ID: LEVEL 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ea

Method File: /chem/msd8.i/8-26mar.b/t14q322b.m

Misc Info: 200ppbv-200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	291821	175093	408549	281494	-3.54
86 1,4-Difluorobenze	1354208	812525	1895891	1332533	-1.60
123 Chlorobenzene-d5	1071895	643137	1500653	1030363	-3.87

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.39	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-26mar.1b/8032608.d

Date: 26-MAR-2007 13:11

Client ID: LEVEL 7

Sample Info: 200ml #1487-42


Column phase: RTX-624

Instrument: msd8.1

Operator: ea

Column diameter: 0.53

/chem/msd8.1/8-26mar.1b/8032608.d



Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22mar.b/8032209.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 22-MAR-2007 13:30
 Operator : sjr Inst ID: msd8.i
 Smp Info : 200ml 1487-115
 Misc Info : 200ppbv->200ppbv
 Comment :
 Method : /chem/msd8.i/8-22mar.b/t14q322a.m
 Meth Date : 23-Mar-2007 08:09 sscott Quant Type: ISTD
 Cal Date : 22-MAR-2007 13:30 Cal File: 8032209.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	279518	25.0000		70.00- 130.00	100.00	
8.395	8.395	(1.000)	128	222977			46.35- 106.35	79.77	
8.367	8.367	(1.000)	49	860256			255.78- 315.78	307.76	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.248	(1.000)	114	1399810	25.0000		70.00- 130.00	100.00	
10.248	10.248	(1.000)	88	256707			0.00- 48.88	18.34	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.224	15.224	(1.000)	117	1085707	25.0000		70.00- 130.00	100.00	
15.197	15.197	(1.000)	82	735939			36.68- 96.68	67.78	

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.473	(1.128)	65	661231	25.0000	27.367	70.00- 130.00	100.00	
9.446	9.446	(1.125)	67	465615			27.92- 87.92	70.42	

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.267)	98	1412741	25.0000	25.663	70.00- 130.00	100.00	
12.985	12.985	(1.267)	70	173136			0.00- 42.61	12.26	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 102 Toluene-d8 (continued)										
12.985	12.985	(1.267)	100	954832			40.27- 100.27	67.59		

\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.745	16.745	(1.100)	174	570442	25.0000	25.638	70.00- 130.00	100.00		
16.745	16.745	(1.100)	95	1011334			137.66- 197.66	177.29		
16.745	16.745	(1.100)	176	558711			63.61- 123.61	97.94		

3 Propylene										
						CAS #:	115-07-1			
2.395	2.395	(0.285)	41	5308101	200.000	179.48	70.00- 130.00	100.00		
2.395	2.395	(0.285)	42	3479256			35.20- 95.20	65.55		
2.395	2.395	(0.285)	39	3813826			42.80- 102.80	71.85		

4 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.450	2.450	(0.292)	85	10101380	200.000	161.58	70.00- 130.00	100.00		
2.450	2.450	(0.292)	87	3235750			1.89- 61.89	32.03		

6 Freon 114										
						CAS #:	76-14-2			
2.616	2.616	(0.312)	135	5891518	200.000	166.16	70.00- 130.00	100.00		
2.616	2.616	(0.312)	137	1868154			1.88- 61.88	31.71		

8 Chloromethane										
						CAS #:	74-87-3			
2.727	2.727	(0.325)	50	5299226	200.000	164.76	70.00- 130.00	100.00		
2.727	2.727	(0.325)	52	1522402			0.00- 59.46	28.73		

9 Butane										
						CAS #:	106-97-8			
2.837	2.837	(0.338)	58	1398871	200.000	167.12	70.00- 130.00	100.00		
2.837	2.837	(0.338)	43	11305102			772.78- 832.78	808.16		

10 Vinyl Chloride										
						CAS #:	75-01-4			
2.893	2.893	(0.345)	62	5274740	200.000	174.60	70.00- 130.00	100.00		
2.893	2.893	(0.345)	64	1597095			0.33- 60.33	30.28		

11 1,3-Butadiene										
						CAS #:	106-99-0			
2.920	2.920	(0.348)	54	5298869	200.000	169.14	70.00- 130.00	100.00		
2.893	2.893	(0.345)	39	7534296			86.60- 146.60	142.19		

13 Bromomethane										
						CAS #:	74-83-9			
3.446	3.446	(0.410)	94	2889199	200.000	174.95	70.00- 130.00	100.00		
3.446	3.446	(0.410)	96	2663390			64.77- 124.77	92.18		

15 Isopentane										
						CAS #:	78-78-4			
3.556	3.556	(0.424)	43	8928696	200.000	172.74	70.00- 130.00	100.00		
3.556	3.556	(0.424)	57	5194820			27.51- 87.51	58.18		
3.584	3.584	(0.427)	72	519565			0.00- 35.95	5.82		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

16 Chloroethane						CAS #: 75-00-3			
3.612	3.612	(0.430)	64	2745566	200.000	174.52	70.00- 130.00	100.00	
3.584	3.584	(0.427)	49	861002			2.42- 62.42	31.36	
3.612	3.612	(0.430)	66	805195			0.00- 58.92	29.33	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.916	3.916	(0.466)	101	10012696	200.000	178.81	70.00- 130.00	100.00	
3.916	3.916	(0.466)	103	6341136			34.71- 94.71	63.33	

21 Ethanol						CAS #: 64-17-5			
4.331	4.331	(0.516)	45	2255570	200.000	177.45	70.00- 130.00	100.00	
4.331	4.331	(0.516)	43	448642			0.00- 50.43	19.89	
4.331	4.331	(0.516)	46	957418			12.21- 72.21	42.45	

27 Freon 113						CAS #: 76-13-1			
4.745	4.745	(0.565)	151	4370646	200.000	164.83	70.00- 130.00	100.00	
4.745	4.745	(0.565)	153	2713210			32.67- 92.67	62.08	
4.745	4.745	(0.565)	101	6769526			124.83- 184.83	154.89	

29 1,1-Dichloroethene						CAS #: 75-35-4			
4.801	4.801	(0.572)	61	7533717	200.000	166.92	70.00- 130.00	100.00	
4.801	4.801	(0.572)	96	3316120			15.10- 75.10	44.02	
4.801	4.801	(0.572)	98	2080886			0.00- 58.17	27.62	

30 Acetone						CAS #: 67-64-1			
4.939	4.939	(0.588)	58	2805977	200.000	173.83	70.00- 130.00	100.00	
4.939	4.939	(0.588)	43	10159313			337.35- 397.35	362.06	

33 Carbon Disulfide						CAS #: 75-15-0			
5.160	5.160	(0.615)	76	11799377	200.000	169.72	70.00- 130.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
5.160	5.160	(0.615)	45	11847068	200.000	187.32	70.00- 130.00	100.00	
5.160	5.160	(0.615)	43	2329975			0.00- 50.64	19.67	
5.160	5.160	(0.615)	59	395213			0.00- 33.21	3.34	

37 3-Chloropropene						CAS #: 107-05-1			
5.437	5.437	(0.648)	76	1998211	200.000	177.98	70.00- 130.00	100.00	
5.437	5.437	(0.648)	41	8970627			414.53- 474.53	448.93	

39 Methylene Chloride						CAS #: 75-09-2			
5.713	5.713	(0.681)	49	6321788	200.000	164.70	70.00- 130.00	100.00	
5.713	5.713	(0.681)	84	3055111			18.44- 78.44	48.33	
5.713	5.713	(0.681)	51	1846237			0.00- 59.93	29.20	

42 MTBE						CAS #: 1634-04-4			
6.045	6.045	(0.720)	73	13152510	200.000	169.99	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.045	6.045	(0.720)	57	3882461			0.00- 59.33	29.52	
6.045	6.045	(0.720)	41	4049097			1.95- 61.95	30.79	

43 trans-1,2-Dichloroethene					CAS #: 156-60-5				
6.100	6.100	(0.727)	96	3729950	200.000	161.71	70.00- 130.00	100.00	
6.100	6.100	(0.727)	61	7405681			169.97- 229.97	198.55	
6.100	6.100	(0.727)	98	2367667			34.71- 94.71	63.48	

45 Hexane					CAS #: 110-54-3				
6.432	6.432	(0.766)	57	9508794	200.000	167.48	70.00- 130.00	100.00	
6.432	6.432	(0.766)	43	7106283			44.61- 104.61	74.73	
6.460	6.460	(0.769)	86	1305143			0.00- 43.77	13.73	

52 1,1-Dichloroethane					CAS #: 75-34-3				
6.902	6.902	(0.822)	63	8387780	200.000	174.91	70.00- 130.00	100.00	
6.902	6.902	(0.822)	65	2490463			0.00- 59.58	29.69	

54 Vinyl Acetate					CAS #: 108-05-4				
6.957	6.957	(0.829)	86	1135815	200.000	199.12	70.00- 130.00	100.00	
6.957	6.957	(0.829)	43	17639765			1469.62-1529.62	1553.05	
6.957	6.957	(0.829)	42	1475594			100.08- 160.08	129.91	

63 cis-1,2-Dichloroethene					CAS #: 156-59-2				
7.953	7.953	(0.947)	61	6381943	200.000	174.92	70.00- 130.00	100.00	
7.953	7.953	(0.947)	96	3500554			27.36- 87.36	54.85	
7.953	7.953	(0.947)	98	2250958			5.83- 65.83	35.27	

64 2-Butanone					CAS #: 78-93-3				
7.980	7.980	(0.951)	72	2143034	200.000	163.72	70.00- 130.00	100.00	
7.980	7.980	(0.951)	43	13228944			574.29- 634.29	617.30	
7.980	7.980	(0.951)	57	881095			10.61- 70.61	41.11	

66 Tetrahydrofuran					CAS #: 109-99-9				
8.367	8.367	(0.997)	42	7835677	200.000	160.78	70.00- 130.00	100.00	
8.367	8.367	(0.997)	71	1964568			0.00- 54.93	25.07	
8.367	8.367	(0.997)	72	2111107			0.00- 56.52	26.94	

69 Chloroform					CAS #: 67-66-3				
8.506	8.506	(1.013)	83	7043808	200.000	153.24	70.00- 130.00	100.00	
8.506	8.506	(1.013)	85	4530865			33.71- 93.71	64.32	

72 Cyclohexane					CAS #: 110-82-7				
8.727	8.727	(1.040)	84	5609830	200.000	163.73	70.00- 130.00	100.00	
8.727	8.727	(1.040)	56	9584320			138.68- 198.68	170.85	
8.727	8.727	(1.040)	41	5766105			73.81- 133.81	102.79	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

73	1,1,1-Trichloroethane					CAS #: 71-55-6				
8.754	8.754	(1.043)	97	7033900	200.000	169.50	70.00- 130.00	100.00		
8.754	8.754	(1.043)	99	4470247			33.95- 93.95	63.55		

75	Carbon Tetrachloride					CAS #: 56-23-5				
9.003	9.003	(1.072)	119	5870008	200.000	175.12	70.00- 130.00	100.00		
9.003	9.003	(1.072)	117	6520132			81.67- 141.67	111.08		

78	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.446	9.446	(1.125)	57	27970218	200.000	174.96	70.00- 130.00	100.00		
9.446	9.446	(1.125)	56	9810126			4.45- 64.45	35.07		
9.446	9.446	(1.125)	41	8184579			0.00- 59.44	29.26		

79	Benzene					CAS #: 71-43-2				
9.418	9.418	(0.919)	78	12323899	200.000	158.07	70.00- 130.00	100.00		
9.418	9.418	(0.919)	77	2904375			0.00- 54.39	23.57		

81	1,2-Dichloroethane					CAS #: 107-06-2				
9.612	9.612	(0.938)	62	6122562	200.000	167.69	70.00- 130.00	100.00		
9.612	9.612	(0.938)	64	1881649			1.44- 61.44	30.73		

82	Heptane					CAS #: 142-82-5				
9.805	9.805	(0.957)	100	1422278	200.000	152.72	70.00- 130.00	100.00		
9.805	9.805	(0.957)	43	11924797			789.66- 849.66	838.43		
9.805	9.805	(0.957)	71	4647758			294.27- 354.27	326.78		

92	Trichloroethene					CAS #: 79-01-6				
10.662	10.662	(1.040)	95	4227724	200.000	168.59	70.00- 130.00	100.00		
10.662	10.662	(1.040)	130	3693207			57.13- 117.13	87.36		
10.662	10.662	(1.040)	97	2711041			32.50- 92.50	64.13		

93	Methyl Cyclohexane					CAS #: 108-87-2				
10.883	10.883	(1.296)	83	7201337	200.000	168.04	70.00- 130.00	100.00		
10.911	10.911	(1.300)	98	3309603			15.00- 75.00	45.96		
10.883	10.883	(1.296)	55	8341830			87.18- 147.18	115.84		

95	1,2-Dichloropropane					CAS #: 78-87-5				
11.188	11.188	(1.092)	63	4749296	200.000	166.24	70.00- 130.00	100.00		
11.188	11.188	(1.092)	62	3604653			45.03- 105.03	75.90		
11.188	11.188	(1.092)	41	3676935			45.52- 105.52	77.42		

96	1,4-Dioxane					CAS #: 123-91-1				
11.409	11.409	(1.113)	88	2658131	200.000	178.47	70.00- 130.00	100.00		
11.409	11.409	(1.113)	58	2649215			70.27- 130.27	99.66		
11.409	11.409	(1.113)	57	807873			0.54- 60.54	30.39		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.741	11.741	(1.146)	83	7190559	200.000	170.21	70.00- 130.00	100.00	
11.741	11.741	(1.146)	85	4538542			32.38- 92.38	63.12	

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.625	12.625	(1.232)	75	6325832	200.000	175.57	70.00- 130.00	100.00	
12.625	12.625	(1.232)	77	1954764			1.52- 61.52	30.90	
12.598	12.598	(1.229)	39	4867305			48.26- 108.26	76.94	

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.259)	58	4857563	200.000	167.22	70.00- 130.00	100.00	
12.902	12.902	(1.259)	43	14289544			251.14- 311.14	294.17	
12.902	12.902	(1.259)	85	1557025			2.33- 62.33	32.05	

103 Toluene						CAS #: 108-88-3			
13.095	13.095	(1.278)	91	12583853	200.000	178.26	70.00- 130.00	100.00	
13.095	13.095	(1.278)	92	7516713			29.45- 89.45	59.73	

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	6649054	200.000	175.62	70.00- 130.00	100.00	
13.621	13.621	(0.895)	77	2070772			1.42- 61.42	31.14	
13.621	13.621	(0.895)	39	4783510			43.57- 103.57	71.94	

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.870	13.870	(0.911)	97	3726387	200.000	169.06	70.00- 130.00	100.00	
13.870	13.870	(0.911)	99	2290121			31.40- 91.40	61.46	
13.870	13.870	(0.911)	83	3451808			60.06- 120.06	92.63	

109 Tetrachloroethene						CAS #: 127-18-4			
13.925	13.925	(0.915)	166	4167743	200.000	178.02	70.00- 130.00	100.00	
13.925	13.925	(0.915)	129	3212119			46.36- 106.36	77.07	
13.925	13.925	(0.915)	131	3048828			45.00- 105.00	73.15	

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	6522486	200.000	187.49	70.00- 130.00	100.00	
14.257	14.257	(0.936)	43	13577863			176.52- 236.52	208.17	
14.257	14.257	(0.936)	100	1038835			0.00- 45.68	15.93	

114 Dibromochloromethane						CAS #: 124-48-1			
14.423	14.423	(0.947)	129	5277849	200.000	176.45	70.00- 130.00	100.00	
14.423	14.423	(0.947)	127	4101573			46.96- 106.96	77.71	

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.588	14.588	(0.958)	107	5509731	200.000	178.14	70.00- 130.00	100.00	
14.588	14.588	(0.958)	109	5152228			62.88- 122.88	93.51	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
124 Chlorobenzene						CAS #: 108-90-7			
15.252	15.252	(1.002)	112	8721021	200.000	170.98	70.00- 130.00	100.00	
15.252	15.252	(1.002)	114	2743027			0.73- 60.73	31.45	
15.252	15.252	(1.002)	77	6567675			40.58- 100.58	75.31	

127 Ethyl Benzene						CAS #: 100-41-4			
15.363	15.363	(1.009)	106	5041657	200.000	176.06	70.00- 130.00	100.00	
15.363	15.363	(1.009)	91	17579589			309.90- 369.90	348.69	

128 m,p-Xylene						CAS #: 108-38-3			
15.529	15.529	(1.020)	106	6372305	200.000	173.05	70.00- 130.00	100.00	
15.529	15.529	(1.020)	91	13893912			177.38- 237.38	218.04	

130 o-Xylene						CAS #: 95-47-6			
16.054	16.054	(1.054)	106	6076266	200.000	171.12	70.00- 130.00	100.00	
16.054	16.054	(1.054)	91	14006948			195.99- 255.99	230.52	

131 Styrene						CAS #: 100-42-5			
16.082	16.082	(1.056)	104	9762261	200.000	178.61	70.00- 130.00	100.00	
16.082	16.082	(1.056)	78	5787443			28.78- 88.78	59.28	

133 Bromoform						CAS #: 75-25-2			
16.358	16.358	(1.074)	173	4574387	200.000	185.07	70.00- 130.00	100.00	
16.358	16.358	(1.074)	171	2341683			21.17- 81.17	51.19	

135 Cumene						CAS #: 98-82-8			
16.524	16.524	(1.085)	105	17970251	200.000	165.84	70.00- 130.00	100.00	
16.524	16.524	(1.085)	120	3974756			0.00- 53.14	22.12	
16.496	16.496	(1.084)	51	2706656			0.00- 45.39	15.06	

142 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5			
16.966	16.966	(1.114)	83	8927989	200.000	175.54	70.00- 130.00	100.00	
16.966	16.966	(1.114)	85	5676275			34.35- 94.35	63.58	

143 Propylbenzene						CAS #: 103-65-1			
16.994	16.994	(1.116)	91	19404297	200.000	158.37	70.00- 130.00	100.00	
16.994	16.994	(1.116)	120	3967403			0.00- 48.79	20.45	
16.994	16.994	(1.116)	105	753290			0.00- 33.35	3.88	

145 4-Ethyltoluene						CAS #: 622-96-8			
17.132	17.132	(1.125)	105	15990495	200.000	150.17	70.00- 130.00	100.00	
17.132	17.132	(1.125)	120	4984716			0.00- 54.57	31.17	

146 1,3,5-Trimethylbenzene						CAS #: 108-67-8			
17.215	17.215	(1.131)	105	16835111	200.000	167.05	70.00- 130.00	100.00	
17.215	17.215	(1.131)	120	7155884			12.64- 72.64	42.51	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

151	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
17.602	17.602	(1.156)	105	15608537	200.000	171.04	70.00- 130.00	100.00	
17.602	17.602	(1.156)	120	6302882			11.41- 71.41	40.38	

154	1,3-Dichlorobenzene					CAS #: 541-73-1			
17.906	17.906	(1.176)	146	7427639	200.000	187.39	70.00- 130.00	100.00	
17.906	17.906	(1.176)	148	4681195			32.20- 92.20	63.02	
17.879	17.879	(1.174)	111	3455393			13.28- 73.28	46.52	

155	1,4-Dichlorobenzene					CAS #: 106-46-7			
17.989	17.989	(1.182)	146	8613025	200.000	170.40	70.00- 130.00	100.00	
17.989	17.989	(1.182)	148	5485543			34.16- 94.16	63.69	
17.989	17.989	(1.182)	111	3763221			16.41- 76.41	43.69	

156	alpha-Chlorotoluene					CAS #: 100-44-7			
18.128	18.128	(1.191)	91	14714814	200.000	201.08	70.00- 130.00	100.00(A)	
18.128	18.128	(1.191)	126	2503464			0.00- 46.97	17.01	

158	1,2-Dichlorobenzene					CAS #: 95-50-1			
18.321	18.321	(1.203)	146	7632385	200.000	175.45	70.00- 130.00	100.00	
18.321	18.321	(1.203)	148	4754513			33.83- 93.83	62.29	
18.321	18.321	(1.203)	111	3985203			21.29- 81.29	52.21	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.593	19.593	(1.287)	180	5912056	200.000	218.24	70.00- 130.00	100.00(A)	
19.593	19.593	(1.287)	182	5405242			62.06- 122.06	91.43	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.676	19.676	(1.292)	225	5815816	200.000	168.08	70.00- 130.00	100.00	
19.676	19.676	(1.292)	223	3716506			35.92- 95.92	63.90	

165	Naphthalene					CAS #: 91-20-3			
19.787	19.787	(1.300)	128	15395818	200.000	177.87	70.00- 130.00	100.00(A)	
19.787	19.787	(1.300)	127	2483525			0.00- 43.72	16.13	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 23-Mar-2007 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-MAR-2007

Lab File ID: 8032209.d

Calibration Time: 12:34

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd8.i/8-22mar.b/t14q322a.m

Misc Info: 200ppbv->200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	283735	170241	397229	279518	-1.49
86 1,4-Difluorobenze	1370859	822515	1919203	1399810	2.11
123 Chlorobenzene-d5	1067063	640238	1493888	1085707	1.75

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.39	8.06	8.72	8.40	0.00
86 1,4-Difluorobenze	10.25	9.92	10.58	10.25	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22mar.lb/8032209.d
Date: 22-MAR-2007 13:30
Client ID: Level 7
Sample Info: 200ml 1487-115

Column phase: RTX-624

Instrument: msd8.1
Operator: sjr
Column diameter: 0.53





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0704404-06A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042502	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 4/25/07 10:40 AM

Compound	%Recovery
Freon 12	85
Freon 114	99
Vinyl Chloride	102
Bromomethane	93
Chloroethane	92
Freon 11	95
1,1-Dichloroethene	91
Freon 113	96
Methylene Chloride	92
1,1-Dichloroethane	90
cis-1,2-Dichloroethene	87
Chloroform	75
1,1,1-Trichloroethane	86
Carbon Tetrachloride	88
Benzene	82
1,2-Dichloroethane	94
Trichloroethene	87
1,2-Dichloropropane	77
cis-1,3-Dichloropropene	78
Toluene	81
trans-1,3-Dichloropropene	89
1,1,2-Trichloroethane	91
Tetrachloroethene	101
1,2-Dibromoethane (EDB)	94
Chlorobenzene	90
Ethyl Benzene	87
m,p-Xylene	86
o-Xylene	87
Styrene	85
1,1,2,2-Tetrachloroethane	82
1,3,5-Trimethylbenzene	92
1,2,4-Trimethylbenzene	90
1,3-Dichlorobenzene	100
1,4-Dichlorobenzene	100
alpha-Chlorotoluene	87
1,2-Dichlorobenzene	99
1,3-Butadiene	97
Hexane	87
Cyclohexane	80



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0704404-06A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042502	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 4/25/07 10:40 AM

Compound	%Recovery
Heptane	79
Bromodichloromethane	83
Dibromochloromethane	96
Cumene	86
Propylbenzene	89
Chloromethane	106
1,2,4-Trichlorobenzene	96
Hexachlorobutadiene	110
Acetone	91
Carbon Disulfide	92
2-Propanol	92
trans-1,2-Dichloroethene	88
2-Butanone (Methyl Ethyl Ketone)	77
Tetrahydrofuran	71
1,4-Dioxane	79
4-Methyl-2-pentanone	68 Q
2-Hexanone	81
Bromoform	98
4-Ethyltoluene	92
Ethanol	94
Methyl tert-butyl ether	85
3-Chloropropene	94
2,2,4-Trimethylpentane	78
Naphthalene	97

Q = Exceeds Quality Control limits.

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	94	70-130
1,2-Dichloroethane-d4	101	70-130
4-Bromofluorobenzene	106	70-130

Report Date: 25-Apr-2007 11:02

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd8.i Injection Date: 25-APR-2007 10:40
 Lab File ID: 8042502.d Init. Cal. Date(s): 22-MAR-2007 26-MAR-2007
 Analysis Type: AIR Init. Cal. Times: 10:41 13:11
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /var/chem/msd8.i/8-25apr.b/t14q322b.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 80 1,2-Dichloroethane-d4	2.16099	2.17485	0.010	-0.64144	30.00000	Averaged
\$ 102 Toluene-d8	0.98315	0.92850	0.010	5.55870	30.00000	Averaged
\$ 138 Bromofluorobenzene	0.51234	0.54180	0.010	-5.75009	30.00000	Averaged
3 Propylene	2.64519	2.75180	0.010	-4.03046	30.00000	Averaged
4 Dichlorodifluoromethane/Fr1	5.59128	4.73100	0.010	15.38606	30.00000	Averaged
6 Freon 114	3.17116	3.13650	0.010	1.09267	30.00000	Averaged
8 Chloromethane	2.87665	3.05228	0.010	-6.10546	30.00000	Averaged
9 Butane	0.74863	0.69920	0.010	6.60338	30.00000	Averaged
10 Vinyl Chloride	2.70205	2.77101	0.010	-2.55192	30.00000	Averaged
11 1,3-Butadiene	2.80201	2.72963	0.010	2.58291	30.00000	Averaged
13 Bromomethane	1.47708	1.37926	0.010	6.62233	30.00000	Averaged
15 Isopentane	4.62310	4.63698	0.010	-0.30040	30.00000	Averaged
16 Chloroethane	1.40708	1.30051	0.010	7.57384	30.00000	Averaged
18 Trichlorofluoromethane/Fr11	5.00821	4.76087	0.010	4.93867	30.00000	Averaged
21 Ethanol	1.13689	1.07461	0.010	5.47780	30.00000	Averaged
27 Freon 113	2.37158	2.27023	0.010	4.27371	30.00000	Averaged
29 1,1-Dichloroethene	4.03682	3.69075	0.010	8.57285	30.00000	Averaged
30 Acetone	1.44376	1.31877	0.010	8.65699	30.00000	Averaged
33 Carbon Disulfide	6.21805	5.75526	0.010	7.44271	30.00000	Averaged
34 2-Propanol	5.65645	5.19199	0.010	8.21108	30.00000	Averaged
37 3-Chloropropene	1.00414	0.93937	0.010	6.44960	30.00000	Averaged
39 Methylene Chloride	3.43297	3.15035	0.010	8.23249	30.00000	Averaged
42 MTBE	6.91999	5.87819	0.010	15.05484	30.00000	Averaged
43 trans-1,2-Dichloroethene	2.06297	1.81527	0.010	12.00673	30.00000	Averaged
45 Hexane	5.07809	4.42567	0.010	12.84772	30.00000	Averaged
52 1,1-Dichloroethane	4.28903	3.85689	0.010	10.07561	30.00000	Averaged
54 Vinyl Acetate	0.51018	0.47959	0.010	5.99696	30.00000	Averaged
63 cis-1,2-Dichloroethene	3.26321	2.82647	0.010	13.38377	30.00000	Averaged
64 2-Butanone	1.17072	0.90035	0.010	23.09407	30.00000	Averaged
66 Tetrahydrofuran	4.35898	3.11330	0.010	28.57727	30.00000	Averaged
69 Chloroform	4.11103	3.09604	0.010	24.68945	30.00000	Averaged
72 Cyclohexane	3.06440	2.44915	0.010	20.07722	30.00000	Averaged
73 1,1,1-Trichloroethane	3.71165	3.17438	0.010	14.47520	30.00000	Averaged
75 Carbon Tetrachloride	2.99797	2.64500	0.010	11.77361	30.00000	Averaged
78 2,2,4-Trimethylpentane	14.29843	11.21650	0.010	21.55433	30.00000	Averaged
79 Benzene	1.39238	1.13806	0.010	18.26531	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd8.i Injection Date: 25-APR-2007 10:40
 Lab File ID: 8042502.d Init. Cal. Date(s): 22-MAR-2007 26-MAR-2007
 Analysis Type: AIR Init. Cal. Times: 10:41 13:11
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /var/chem/msd8.i/8-25apr.b/t14q322b.m

COMPOUND	RRF / AMOUNT	RF50	MIN RRF	%D / %DRIFT	MAX RRF	%D / %DRIFT	CURVE TYPE
81 1,2-Dichloroethane	0.65206	0.61118	0.010	6.26958	30.00000	Averaged	
82 Heptane	0.16632	0.13086	0.010	21.31982	30.00000	Averaged	
92 Trichloroethene	0.44787	0.39160	0.010	12.56289	30.00000	Averaged	
93 Methyl Cyclohexane	3.83302	2.77931	0.010	27.49050	30.00000	Averaged	
95 1,2-Dichloropropane	0.51024	0.39343	0.010	22.89349	30.00000	Averaged	
96 1,4-Dioxane	0.26600	0.20934	0.010	21.29909	30.00000	Averaged	
98 Bromodichloromethane	0.75448	0.62938	0.010	16.58126	30.00000	Averaged	
100 cis-1,3-Dichloropropene	0.64347	0.49984	0.010	22.32204	30.00000	Averaged	
101 4-Methyl-2-pentanone	0.51882	0.35343	0.010	31.87754	30.00000	Averaged	<-
103 Toluene	1.26076	1.02324	0.010	18.83943	30.00000	Averaged	
106 trans-1,3-Dichloropropene	0.87181	0.77526	0.010	11.07385	30.00000	Averaged	
108 1,1,2-Trichloroethane	0.50754	0.46125	0.010	9.12021	30.00000	Averaged	
109 Tetrachloroethene	0.53907	0.54416	0.010	-0.94291	30.00000	Averaged	
112 2-Hexanone	0.80104	0.64832	0.010	19.06552	30.00000	Averaged	
114 Dibromochloromethane	0.68875	0.66267	0.010	3.78641	30.00000	Averaged	
115 1,2-Dibromoethane	0.71217	0.66903	0.010	6.05688	30.00000	Averaged	
124 Chlorobenzene	1.17450	1.05399	0.010	10.26070	30.00000	Averaged	
127 Ethyl Benzene	0.65940	0.57388	0.010	12.96902	30.00000	Averaged	
128 m,p-Xylene	0.84792	0.73119	0.010	13.76712	30.00000	Averaged	
130 o-Xylene	0.81763	0.71325	0.010	12.76639	30.00000	Averaged	
131 Styrene	1.25857	1.07364	0.010	14.69391	30.00000	Averaged	
133 Bromoform	0.56916	0.55662	0.010	2.20373	30.00000	Averaged	
135 Cumene	2.49512	2.14663	0.010	13.96688	30.00000	Averaged	
142 1,1,2,2-Tetrachloroethane	1.17112	0.96327	0.010	17.74785	30.00000	Averaged	
143 Propylbenzene	2.82133	2.51216	0.010	10.95841	30.00000	Averaged	
145 4-Ethyltoluene	2.45190	2.26539	0.010	7.60664	30.00000	Averaged	
146 1,3,5-Trimethylbenzene	2.32061	2.13486	0.010	8.00448	30.00000	Averaged	
151 1,2,4-Trimethylbenzene	2.10131	1.90081	0.010	9.54180	30.00000	Averaged	
154 1,3-Dichlorobenzene	0.91270	0.91342	0.010	-0.07931	30.00000	Averaged	
155 1,4-Dichlorobenzene	1.16387	1.16547	0.010	-0.13821	30.00000	Averaged	
156 alpha-Chlorotoluene	1.68507	1.46120	0.010	13.28508	30.00000	Averaged	
158 1,2-Dichlorobenzene	1.00169	0.98874	0.010	1.29211	30.00000	Averaged	
163 1,2,4-Trichlorobenzene	0.62377	0.59662	0.010	4.35289	30.00000	Averaged	
164 Hexachlorobutadiene	0.79677	0.88000	0.010	-10.44603	30.00000	Averaged	
165 Naphthalene	1.99311	1.93568	0.010	2.88101	30.00000	Averaged	

Report Date: 25-Apr-2007 11:02

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042502.d
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1
 Inj Date : 25-APR-2007 10:40
 Operator : JG Inst ID: msd8.i
 Smp Info : 100mL #1408-387A
 Misc Info : 100ppbv-50ppbv
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable

Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395	(1.000)	130	232391	25.0000			80.00- 120.00	100.00
8.395	8.395	(1.000)	128	182796				48.66- 108.66	78.66
8.395	8.395	(1.000)	49	683076				263.93- 323.93	293.93

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.275	10.275	(1.000)	114	1035529	25.0000			80.00- 120.00	100.00
10.248	10.248	(1.000)	88	184923				0.00- 47.86	17.86

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225	(1.000)	117	744287	25.0000			80.00- 120.00	100.00
15.225	15.225	(1.000)	82	503050				35.49- 95.49	67.59

\$ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.474	9.474	(1.128)	65	505416	25.0000	25.160		80.00- 120.00	100.00
9.474	9.474	(1.128)	67	267191				27.92- 87.92	52.87

\$ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985	(1.264)	98	961488	25.0000	23.610		80.00- 120.00	100.00
12.985	12.985	(1.264)	70	125022				0.00- 42.61	13.00

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 102 Toluene-d8 (continued)										
12.985	12.985	(1.264)	100	700722			40.27- 100.27	72.88		

\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.773	16.773	(1.102)	174	403251	25.0000	26.438	80.00- 120.00	100.00		
16.745	16.745	(1.100)	95	679173			138.42- 198.42	168.42		
16.773	16.773	(1.102)	176	392109			67.24- 127.24	97.24		

3 Propylene										
						CAS #:	115-07-1			
2.451	2.451	(0.292)	41	1278989	50.0000	52.015	80.00- 120.00	100.00		
2.451	2.451	(0.292)	42	852113			35.20- 95.20	66.62		
2.451	2.451	(0.292)	39	911209			42.80- 102.80	71.24		

4 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.506	2.506	(0.298)	85	2198885	50.0000	42.307	80.00- 120.00	100.00		
2.506	2.506	(0.298)	87	700036			1.89- 61.89	31.84		

6 Freon 114										
						CAS #:	76-14-2			
2.644	2.644	(0.315)	135	1457791	50.0000	49.454	80.00- 120.00	100.00		
2.644	2.644	(0.315)	137	457363			1.37- 61.37	31.37		

8 Chloromethane										
						CAS #:	74-87-3			
2.782	2.782	(0.331)	50	1418644	50.0000	53.053	80.00- 120.00	100.00		
2.782	2.782	(0.331)	52	382608			0.00- 59.46	26.97		

9 Butane										
						CAS #:	106-97-8			
2.838	2.838	(0.338)	58	324974	50.0000	46.698	80.00- 120.00	100.00		
2.838	2.838	(0.338)	43	2728388			772.78- 832.78	839.57		

10 Vinyl Chloride										
						CAS #:	75-01-4			
2.948	2.948	(0.351)	62	1287915	50.0000	51.276	80.00- 120.00	100.00		
2.948	2.948	(0.351)	64	397216			0.33- 60.33	30.84		

11 1,3-Butadiene										
						CAS #:	106-99-0			
2.921	2.921	(0.348)	54	1268684	50.0000	48.708	80.00- 120.00	100.00		
2.921	2.921	(0.348)	39	1854780			86.60- 146.60	146.20		

13 Bromomethane										
						CAS #:	74-83-9			
3.474	3.474	(0.414)	94	641055	50.0000	46.689	80.00- 120.00	100.00		
3.474	3.474	(0.414)	96	592120			62.37- 122.37	92.37		

15 Isopentane										
						CAS #:	78-78-4			
3.584	3.584	(0.427)	43	2155187	50.0000	50.150	80.00- 120.00	100.00		
3.584	3.584	(0.427)	57	1230724			27.51- 87.51	57.11		
3.584	3.584	(0.427)	72	127996			0.00- 35.95	5.94		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

16 Chloroethane						CAS #: 75-00-3			
3.640	3.640	(0.434)	64	604454	50.0000	46.213	80.00- 120.00	100.00	
3.612	3.612	(0.430)	49	197608			2.42- 62.42	32.69	
3.640	3.640	(0.434)	66	186934			0.00- 58.92	30.93	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.916	3.916	(0.466)	101	2212767	50.0000	47.531	80.00- 120.00	100.00	
3.944	3.944	(0.470)	103	1431731			34.70- 94.70	64.70	

21 Ethanol						CAS #: 64-17-5			
4.331	4.331	(0.516)	45	499461	50.0000	47.261	80.00- 120.00	100.00	
4.331	4.331	(0.516)	43	114062			0.00- 50.43	22.84	
4.331	4.331	(0.516)	46	215432			12.21- 72.21	43.13	

27 Freon 113						CAS #: 76-13-1			
4.773	4.773	(0.569)	151	1055160	50.0000	47.863	80.00- 120.00	100.00	
4.773	4.773	(0.569)	153	669070			33.41- 93.41	63.41	
4.773	4.773	(0.569)	101	1611773			122.75- 182.75	152.75	

29 1,1-Dichloroethene						CAS #: 75-35-4			
4.801	4.801	(0.572)	61	1715394	50.0000	45.714	80.00- 120.00	100.00	
4.828	4.828	(0.575)	96	761110			14.37- 74.37	44.37	
4.828	4.828	(0.575)	98	498021			0.00- 59.03	29.03	

30 Acetone						CAS #: 67-64-1			
4.967	4.967	(0.592)	58	612941	50.0000	45.672	80.00- 120.00	100.00	
4.967	4.967	(0.592)	43	2190186			337.35- 397.35	357.32	

33 Carbon Disulfide						CAS #: 75-15-0			
5.188	5.188	(0.618)	76	2674940	50.0000	46.279	80.00- 120.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
5.188	5.188	(0.618)	45	2413145	50.0000	45.894	80.00- 120.00	100.00	
5.188	5.188	(0.618)	43	530899			0.00- 50.64	22.00	
5.188	5.188	(0.618)	59	81156			0.00- 33.21	3.36	

37 3-Chloropropene						CAS #: 107-05-1			
5.464	5.464	(0.651)	76	436604	50.0000	46.775	80.00- 120.00	100.00	
5.464	5.464	(0.651)	41	1965234			414.53- 474.53	450.12	

39 Methylene Chloride						CAS #: 75-09-2			
5.741	5.741	(0.684)	49	1464225	50.0000	45.884	80.00- 120.00	100.00	
5.741	5.741	(0.684)	84	710384			18.52- 78.52	48.52	
5.741	5.741	(0.684)	51	416419			0.00- 59.93	28.44	

42 MTBE						CAS #: 1634-04-4			
6.073	6.073	(0.723)	73	2732079	50.0000	42.472	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.073	6.073	(0.723)	57	784713			0.00- 58.72	28.72	
6.073	6.073	(0.723)	41	903876			1.95- 61.95	33.08	

43 trans-1,2-Dichloroethene					CAS #: 156-60-5				
6.128	6.128	(0.730)	96	843706	50.0000	43.997	80.00- 120.00	100.00	
6.128	6.128	(0.730)	61	1660914			166.86- 226.86	196.86	
6.128	6.128	(0.730)	98	537479			34.71- 94.71	63.70	

45 Hexane					CAS #: 110-54-3				
6.460	6.460	(0.769)	57	2056973	50.0000	43.576	80.00- 120.00	100.00	
6.460	6.460	(0.769)	43	1539476			44.61- 104.61	74.84	
6.460	6.460	(0.769)	86	282666			0.00- 43.77	13.74	

52 1,1-Dichloroethane					CAS #: 75-34-3				
6.930	6.930	(0.825)	63	1792611	50.0000	44.962	80.00- 120.00	100.00	
6.930	6.930	(0.825)	65	537514			0.00- 59.98	29.98	

54 Vinyl Acetate					CAS #: 108-05-4				
6.985	6.985	(0.832)	86	222903	50.0000	47.002	80.00- 120.00	100.00	
6.985	6.985	(0.832)	43	3469388			1469.62-1529.62	1556.46	
6.985	6.985	(0.832)	42	306112			100.08- 160.08	137.33	

63 cis-1,2-Dichloroethene					CAS #: 156-59-2				
7.953	7.953	(0.947)	61	1313694	50.0000	43.308	80.00- 120.00	100.00	
7.953	7.953	(0.947)	96	734549			25.91- 85.91	55.91	
7.953	7.953	(0.947)	98	469912			5.77- 65.77	35.77	

64 2-Butanone					CAS #: 78-93-3				
8.008	8.008	(0.954)	72	418468	50.0000	38.453	80.00- 120.00	100.00	
8.008	8.008	(0.954)	43	2503741			568.31- 628.31	598.31	
8.008	8.008	(0.954)	57	172902			10.61- 70.61	41.32	

66 Tetrahydrofuran					CAS #: 109-99-9				
8.368	8.368	(0.997)	42	1447006	50.0000	35.711	80.00- 120.00	100.00	
8.368	8.368	(0.997)	71	370015			0.00- 55.57	25.57	
8.395	8.395	(1.000)	72	391472			0.00- 56.52	27.05	

69 Chloroform					CAS #: 67-66-3				
8.533	8.533	(1.016)	83	1438985	50.0000	37.655	80.00- 120.00	100.00	
8.533	8.533	(1.016)	85	922689			34.12- 94.12	64.12	

72 Cyclohexane					CAS #: 110-82-7				
8.755	8.755	(1.043)	84	1138322	50.0000	39.961	80.00- 120.00	100.00	
8.755	8.755	(1.043)	56	1855470			133.00- 193.00	163.00	
8.755	8.755	(1.043)	41	1128655			69.15- 129.15	99.15	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

73	1,1,1-Trichloroethane				CAS #:		71-55-6		
8.782	8.782	(1.046)	97	1475395	50.0000	42.762	80.00-	120.00	100.00
8.782	8.782	(1.046)	99	939040			33.65-	93.65	63.65

75	Carbon Tetrachloride				CAS #:		56-23-5		
9.004	9.004	(1.072)	119	1229347	50.0000	44.113	80.00-	120.00	100.00
9.004	9.004	(1.072)	117	1391245			83.17-	143.17	113.17

78	2,2,4-Trimethylpentane				CAS #:		540-84-1		
9.446	9.446	(1.125)	57	5213228	50.0000	39.223	80.00-	120.00	100.00
9.446	9.446	(1.125)	56	1858415			4.45-	64.45	35.65
9.446	9.446	(1.125)	41	1586549			0.00-	59.44	30.43

79	Benzene				CAS #:		71-43-2		
9.446	9.446	(0.919)	78	2356988	50.0000	40.867	80.00-	120.00	100.00
9.446	9.446	(0.919)	77	588467			0.00-	54.39	24.97

81	1,2-Dichloroethane				CAS #:		107-06-2		
9.612	9.612	(0.935)	62	1265794	50.0000	46.865	80.00-	120.00	100.00
9.612	9.612	(0.935)	64	402391			1.44-	61.44	31.79

82	Heptane				CAS #:		142-82-5		
9.833	9.833	(0.957)	100	271024	50.0000	39.340	80.00-	120.00	100.00
9.833	9.833	(0.957)	43	2248293			789.66-	849.66	829.55
9.833	9.833	(0.957)	71	859374			294.27-	354.27	317.08

92	Trichloroethene				CAS #:		79-01-6		
10.690	10.690	(1.040)	95	811027	50.0000	43.718	80.00-	120.00	100.00
10.690	10.690	(1.040)	130	714169			58.06-	118.06	88.06
10.690	10.690	(1.040)	97	500644			31.73-	91.73	61.73

93	Methyl Cyclohexane				CAS #:		108-87-2		
10.911	10.911	(1.300)	83	1291772	50.0000	36.255	80.00-	120.00	100.00
10.911	10.911	(1.300)	98	599859			15.00-	75.00	46.44
10.911	10.911	(1.300)	55	1485410			87.18-	147.18	114.99

95	1,2-Dichloropropane				CAS #:		78-87-5		
11.188	11.188	(1.089)	63	814809	50.0000	38.553	80.00-	120.00	100.00
11.188	11.188	(1.089)	62	604202			44.15-	104.15	74.15
11.188	11.188	(1.089)	41	703303			56.32-	116.32	86.32

96	1,4-Dioxane				CAS #:		123-91-1		
11.409	11.409	(1.110)	88	433557	50.0000	39.350	80.00-	120.00	100.00
11.409	11.409	(1.110)	58	407167			63.91-	123.91	93.91
11.409	11.409	(1.110)	57	129910			0.54-	60.54	29.96

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.741	11.741	(1.143)	83	1303479	50.0000	41.709	80.00- 120.00	100.00	
11.741	11.741	(1.143)	85	837932			34.28- 94.28	64.28	

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.626	12.626	(1.229)	75	1035191	50.0000	38.839	80.00- 120.00	100.00	
12.626	12.626	(1.229)	77	342361			3.07- 63.07	33.07	
12.626	12.626	(1.229)	39	882806			55.28- 115.28	85.28	

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.256)	58	731975	50.0000	34.061	80.00- 120.00	100.00	
12.902	12.902	(1.256)	43	2180669			251.14- 311.14	297.92	
12.902	12.902	(1.256)	85	257106			2.33- 62.33	35.12	

103 Toluene						CAS #: 108-88-3			
13.096	13.096	(1.274)	91	2119191	50.0000	40.580	80.00- 120.00	100.00	
13.096	13.096	(1.274)	92	1334225			32.96- 92.96	62.96	

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	1154036	50.0000	44.463	80.00- 120.00	100.00	
13.621	13.621	(0.895)	77	371903			2.23- 62.23	32.23	
13.621	13.621	(0.895)	39	900302			48.01- 108.01	78.01	

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.897	13.897	(0.913)	97	686612	50.0000	45.440	80.00- 120.00	100.00	
13.897	13.897	(0.913)	99	412019			30.01- 90.01	60.01	
13.897	13.897	(0.913)	83	571553			53.24- 113.24	83.24	

109 Tetrachloroethene						CAS #: 127-18-4			
13.953	13.953	(0.916)	166	810016	50.0000	50.471	80.00- 120.00	100.00	
13.925	13.925	(0.915)	129	596438			43.63- 103.63	73.63	
13.925	13.925	(0.915)	131	581982			41.85- 101.85	71.85	

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	965066	50.0000	40.467	80.00- 120.00	100.00	
14.257	14.257	(0.936)	43	2070354			184.53- 244.53	214.53	
14.257	14.257	(0.936)	100	163914			0.00- 45.68	16.98	

114 Dibromochloromethane						CAS #: 124-48-1			
14.423	14.423	(0.947)	129	986429	50.0000	48.107	80.00- 120.00	100.00	
14.423	14.423	(0.947)	127	756764			46.96- 106.96	76.72	

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.589	14.589	(0.958)	107	995905	50.0000	46.972	80.00- 120.00	100.00	
14.589	14.589	(0.958)	109	929738			63.36- 123.36	93.36	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
124 Chlorobenzene						CAS #:	108-90-7			
15.252	15.252	(1.002)	112	1568942	50.0000	44.870	80.00-	120.00	100.00	
15.252	15.252	(1.002)	114	486883			1.03-	61.03	31.03	
15.252	15.252	(1.002)	77	1093276			39.68-	99.68	69.68	

127 Ethyl Benzene						CAS #:	100-41-4			
15.363	15.363	(1.009)	106	854262	50.0000	43.515	80.00-	120.00	100.00	
15.363	15.363	(1.009)	91	2909796			309.90-	369.90	340.62	

128 m,p-Xylene						CAS #:	108-38-3			
15.529	15.529	(1.020)	106	1088430	50.0000	43.116	80.00-	120.00	100.00	
15.529	15.529	(1.020)	91	2354119			177.38-	237.38	216.29	

130 o-Xylene						CAS #:	95-47-6			
16.054	16.054	(1.054)	106	1061720	50.0000	43.617	80.00-	120.00	100.00	
16.054	16.054	(1.054)	91	2445497			200.33-	260.33	230.33	

131 Styrene						CAS #:	100-42-5			
16.109	16.109	(1.058)	104	1598192	50.0000	42.653	80.00-	120.00	100.00	
16.082	16.082	(1.056)	78	981613			31.42-	91.42	61.42	

133 Bromoform						CAS #:	75-25-2			
16.358	16.358	(1.074)	173	828564	50.0000	48.898	80.00-	120.00	100.00	
16.358	16.358	(1.074)	171	422160			20.95-	80.95	50.95	

135 Cumene						CAS #:	98-82-8			
16.524	16.524	(1.085)	105	3195414	50.0000	43.016	80.00-	120.00	100.00	
16.524	16.524	(1.085)	120	712426			0.00-	53.14	22.30	
16.496	16.496	(1.084)	51	493360			0.00-	45.39	15.44	

142 1,1,2,2-Tetrachloroethane						CAS #:	79-34-5			
16.967	16.967	(1.114)	83	1433906	50.0000	41.126	80.00-	120.00	100.00	
16.967	16.967	(1.114)	85	911056			33.54-	93.54	63.54	

143 Propylbenzene						CAS #:	103-65-1			
16.994	16.994	(1.116)	91	3739530	50.0000	44.521	80.00-	120.00	100.00	
16.994	16.994	(1.116)	120	697951			0.00-	48.79	18.66	
16.994	16.994	(1.116)	105	127699			0.00-	33.35	3.41	

145 4-Ethyltoluene						CAS #:	622-96-8			
17.132	17.132	(1.125)	105	3372204	50.0000	46.197	80.00-	120.00	100.00	
17.132	17.132	(1.125)	120	812385			0.00-	54.09	24.09	

146 1,3,5-Trimethylbenzene						CAS #:	108-67-8			
17.215	17.215	(1.131)	105	3177894	50.0000	45.998	80.00-	120.00	100.00	
17.215	17.215	(1.131)	120	1324516			12.64-	72.64	41.68	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

151	17.602	17.602	105	2829492	50.0000	45.229	80.00- 120.00	100.00	
	17.602	17.602	120	1106514			9.11- 69.11	39.11	
	CAS #: 95-63-6								

154	17.907	17.907	146	1359693	50.0000	50.040	80.00- 120.00	100.00	
	17.907	17.907	148	860224			32.20- 92.20	63.27	
	17.907	17.907	111	594505			13.28- 73.28	43.72	
	CAS #: 541-73-1								

155	17.990	17.990	146	1734895	50.0000	50.069	80.00- 120.00	100.00	
	17.990	17.990	148	1119861			34.16- 94.16	64.55	
	17.990	17.990	111	819078			16.41- 76.41	47.21	
	CAS #: 106-46-7								

156	18.128	18.128	91	2175110	50.0000	43.357	80.00- 120.00	100.00	
	18.128	18.128	126	369176			0.00- 46.97	16.97	
	CAS #: 100-44-7								

158	18.321	18.321	146	1471818	50.0000	49.354	80.00- 120.00	100.00	
	18.321	18.321	148	908201			31.71- 91.71	61.71	
	18.321	18.321	111	737553			20.11- 80.11	50.11	
	CAS #: 95-50-1								

163	19.593	19.593	180	888110	50.0000	47.824	80.00- 120.00	100.00	
	19.593	19.593	182	819411			62.26- 122.26	92.26	
	CAS #: 120-82-1								

164	19.676	19.676	225	1309951	50.0000	55.223	80.00- 120.00	100.00	
	19.676	19.676	223	860906			35.72- 95.72	65.72	
	CAS #: 87-68-3								

165	19.787	19.787	128	1440705	25.0000	24.280	80.00- 120.00	100.00	
	19.787	19.787	127	215044			0.00- 43.72	14.93	
	CAS #: 91-20-3								

Report Date: 25-Apr-2007 11:02

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 25-APR-2007

Lab File ID: 8042502.d

Calibration Time: 10:40

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m

Misc Info: 100ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	232391	0.00
86 1,4-Difluorobenze	1035529	621317	1449741	1035529	0.00
123 Chlorobenzene-d5	744287	446572	1042002	744287	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.28	0.00
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-25apr.1b/8042502.d
Date: 25-APR-2007 10:40
Client ID: CCV-1
Sample Info: 100mL #1408-387A

Column phase: RTX-624

Instrument: msd8.1
Operator: JG
Column diameter: 0.53





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0704404-07A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042503	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 4/25/07 11:08 AM

Compound	%Recovery
Freon 12	88
Freon 114	95
Vinyl Chloride	97
Bromomethane	89
Chloroethane	80
Freon 11	98
1,1-Dichloroethene	106
Freon 113	109
Methylene Chloride	104
1,1-Dichloroethane	98
cis-1,2-Dichloroethene	94
Chloroform	84
1,1,1-Trichloroethane	96
Carbon Tetrachloride	101
Benzene	86
1,2-Dichloroethane	103
Trichloroethene	93
1,2-Dichloropropane	85
cis-1,3-Dichloropropene	88
Toluene	95
trans-1,3-Dichloropropene	92
1,1,2-Trichloroethane	92
Tetrachloroethene	102
1,2-Dibromoethane (EDB)	95
Chlorobenzene	92
Ethyl Benzene	91
m,p-Xylene	92
o-Xylene	91
Styrene	85
1,1,2,2-Tetrachloroethane	91
1,3,5-Trimethylbenzene	92
1,2,4-Trimethylbenzene	93
1,3-Dichlorobenzene	111
1,4-Dichlorobenzene	103
alpha-Chlorotoluene	112
1,2-Dichlorobenzene	106
1,3-Butadiene	91
Hexane	90
Cyclohexane	85



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0704404-07A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8042503	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 4/25/07 11:08 AM

Compound	%Recovery
Heptane	85
Bromodichloromethane	94
Dibromochloromethane	101
Cumene	91
Propylbenzene	100
Chloromethane	100
1,2,4-Trichlorobenzene	123
Hexachlorobutadiene	106
Acetone	96
Carbon Disulfide	96
2-Propanol	98
trans-1,2-Dichloroethene	93
2-Butanone (Methyl Ethyl Ketone)	84
Tetrahydrofuran	80
1,4-Dioxane	93
4-Methyl-2-pentanone	78
2-Hexanone	87
Bromoform	106
4-Ethyltoluene	105
Ethanol	116
Methyl tert-butyl ether	91
3-Chloropropene	101
2,2,4-Trimethylpentane	84
Naphthalene	95

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	98	70-130
1,2-Dichloroethane-d4	100	70-130
4-Bromofluorobenzene	107	70-130

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-25apr
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: JG
 Data Type: MS DATA SampleType: LCS
 SpikeList File: Spectra+ENS.spk Quant Type: ISTD
 Sublist File: AT04+ENS.sub
 Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Misc Info: 200ppbv-50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
131 Styrene	50.000	42.309	84.62	70-130
106 trans-1,3-Dichloro	50.000	46.291	92.58	70-130
3 Propylene	50.000	49.577	99.15	60-140
4 Dichlorodifluorome	50.000	43.883	87.77	70-130
6 Freon 114	50.000	47.569	95.14	70-130
8 Chloromethane	50.000	49.858	99.72	70-130
10 Vinyl Chloride	50.000	48.473	96.95	70-130
11 1,3-Butadiene	50.000	45.538	91.08	60-140
13 Bromomethane	50.000	44.459	88.92	70-130
16 Chloroethane	50.000	40.139	80.28	70-130
18 Trichlorofluoromet	50.000	48.844	97.69	70-130
21 Ethanol	50.000	58.116	116.23	60-140
27 Freon 113	50.000	54.404	108.81	70-130
29 1,1-Dichloroethene	50.000	52.853	105.71	70-130
30 Acetone	50.000	47.876	95.75	60-140
33 Carbon Disulfide	50.000	48.123	96.25	60-140
34 2-Propanol	50.000	48.778	97.56	60-140
39 Methylene Chloride	50.000	52.274	104.55	70-130
42 MTBE	50.000	45.504	91.01	60-140
43 trans-1,2-Dichloro	50.000	46.498	93.00	60-140
45 Hexane	50.000	45.101	90.20	60-140
52 1,1-Dichloroethane	50.000	48.903	97.81	70-130
63 cis-1,2-Dichloroet	50.000	47.021	94.04	70-130
64 2-Butanone	50.000	42.114	84.23	60-140
66 Tetrahydrofuran	50.000	40.124	80.25	60-140
69 Chloroform	50.000	41.895	83.79	70-130
72 Cyclohexane	50.000	42.698	85.40	60-140
73 1,1,1-Trichloroeth	50.000	48.264	96.53	70-130
75 Carbon Tetrachlori	50.000	50.303	100.61	70-130
79 Benzene	50.000	43.248	86.50	70-130
81 1,2-Dichloroethane	50.000	51.513	103.03	70-130
82 Heptane	50.000	42.507	85.01	60-140
92 Trichloroethene	50.000	46.444	92.89	70-130

Report Date: 25-Apr-2007 11:29

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
95 1,2-Dichloropropan	50.000	42.737	85.47	70-130
96 1,4-Dioxane	50.000	46.444	92.89	60-140
98 Bromodichlorometha	50.000	46.859	93.72	60-140
100 cis-1,3-Dichloropr	50.000	44.201	88.40	70-130
101 4-Methyl-2-pentano	50.000	38.950	77.90	60-140
103 Toluene	50.000	47.517	95.03	70-130
108 1,1,2-Trichloroeth	50.000	45.938	91.88	70-130
109 Tetrachloroethene	50.000	50.827	101.65	70-130
112 2-Hexanone	50.000	43.403	86.81	60-140
114 Dibromochlorometha	50.000	50.481	100.96	60-140
115 1,2-Dibromoethane	50.000	47.422	94.84	70-130
124 Chlorobenzene	50.000	46.079	92.16	70-130
127 Ethyl Benzene	50.000	45.730	91.46	70-130
128 m,p-Xylene	50.000	46.102	92.20	70-130
130 o-Xylene	50.000	45.432	90.86	70-130
133 Bromoform	50.000	53.118	106.24	60-140
142 1,1,2,2-Tetrachlor	50.000	45.331	90.66	70-130
145 4-Ethyltoluene	50.000	52.404	104.81	60-140
146 1,3,5-Trimethylben	50.000	45.857	91.71	70-130
151 1,2,4-Trimethylben	50.000	46.742	93.48	70-130
154 1,3-Dichlorobenzen	50.000	55.708	111.42	70-130
155 1,4-Dichlorobenzen	50.000	51.700	103.40	70-130
156 alpha-Chlorotoluen	50.000	56.273	112.55	70-130
158 1,2-Dichlorobenzen	50.000	52.928	105.86	70-130
163 1,2,4-Trichloroben	50.000	61.509	123.02	70-130
164 Hexachlorobutadien	50.000	52.790	105.58	70-130
135 Cumene	50.000	45.592	91.18	60-140
143 Propylbenzene	50.000	50.094	100.19	60-140
37 3-Chloropropene	50.000	50.436	100.87	60-140
78 2,2,4-Trimethylpen	50.000	42.034	84.07	60-140
9 Butane	50.000	47.569	95.14	70-130
15 Isopentane	50.000	48.838	97.68	70-130
93 Methyl Cyclohexane	50.000	40.757	81.51	70-130
165 Naphthalene	50.000	47.618	95.24	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 80 1,2-Dichloroethane	25.000	24.964	99.86	70-130
\$ 102 Toluene-d8	25.000	24.437	97.75	70-130
\$ 138 Bromofluorobenzene	25.000	26.772	107.09	70-130

Report Date: 25-Apr-2007 11:29

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-25apr.b/8042503.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 25-APR-2007 11:08
 Operator : JG Inst ID: msd8.i
 Smp Info : 50mL #1487-194
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/t14q322b.m
 Meth Date : 25-Apr-2007 11:02 jgray Quant Type: ISTD
 Cal Date : 26-MAR-2007 13:11 Cal File: 8032608.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENS.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 67 Bromochloromethane CAS #: 74-97-5									
8.395	8.395 (1.000)	130	173884	25.0000		80.00-	120.00	100.00	
8.395	8.395 (1.000)	128	138781			48.66-	108.66	79.81	
8.367	8.395 (1.000)	49	504123			263.93-	323.93	289.92	

* 86 1,4-Difluorobenzene CAS #: 540-36-3									
10.248	10.275 (1.000)	114	790852	25.0000		80.00-	120.00	100.00	
10.248	10.248 (1.000)	88	145336			0.00-	47.86	18.38	

* 123 Chlorobenzene-d5 CAS #: 3114-55-4									
15.225	15.225 (1.000)	117	605228	25.0000		80.00-	120.00	100.00	
15.197	15.225 (1.000)	82	399475			35.49-	95.49	66.00	

§ 80 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.473	9.474 (1.128)	65	375217	24.9638	24.964	80.00-	120.00	100.00	
9.473	9.474 (1.128)	67	220628			27.92-	87.92	58.80	

§ 102 Toluene-d8 CAS #: 2037-26-5									
12.985	12.985 (1.267)	98	760017	24.4370	24.437	80.00-	120.00	100.00	
12.985	12.985 (1.267)	70	101149			0.00-	42.61	13.31	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 102 Toluene-d8 (continued)

12.985	12.985	(1.267)	100	530639			40.27- 100.27	69.82
--------	--------	---------	-----	--------	--	--	---------------	-------

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.745	16.773	(1.100)	174	332062	26.7723	26.772	80.00- 120.00	100.00
16.745	16.745	(1.100)	95	562263			138.42- 198.42	169.32
16.745	16.773	(1.100)	176	301367			67.24- 127.24	90.76

3 Propylene

CAS #: 115-07-1

2.395	2.451	(0.285)	41	912130	49.5770	49.577	80.00- 120.00	100.00
2.395	2.451	(0.285)	42	586776			35.20- 95.20	64.33
2.395	2.451	(0.285)	39	641478			42.80- 102.80	70.33

4 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.450	2.506	(0.292)	85	1706583	43.8830	43.883	80.00- 120.00	100.00
2.450	2.506	(0.292)	87	553030			1.89- 61.89	32.41

6 Freon 114

CAS #: 76-14-2

2.589	2.644	(0.308)	135	1049217	47.5695	47.569	80.00- 120.00	100.00
2.589	2.644	(0.308)	137	327247			1.37- 61.37	31.19

8 Chloromethane

CAS #: 74-87-3

2.727	2.782	(0.325)	50	997568	49.8582	49.858	80.00- 120.00	100.00
2.727	2.782	(0.325)	52	302295			0.00- 59.46	30.30

9 Butane

CAS #: 106-97-8

2.810	2.838	(0.335)	58	247692	47.5690	47.569	80.00- 120.00	100.00
2.810	2.838	(0.335)	43	2024753			772.78- 832.78	817.45

10 Vinyl Chloride

CAS #: 75-01-4

2.893	2.948	(0.345)	62	910990	48.4730	48.473	80.00- 120.00	100.00
2.893	2.948	(0.345)	64	284000			0.33- 60.33	31.17

11 1,3-Butadiene

CAS #: 106-99-0

2.893	2.921	(0.345)	54	887489	45.5380	45.538	80.00- 120.00	100.00
2.893	2.921	(0.345)	39	1035841			86.60- 146.60	116.72

13 Bromomethane

CAS #: 74-83-9

3.418	3.474	(0.407)	94	456759	44.4595	44.459	80.00- 120.00	100.00
3.418	3.474	(0.407)	96	440308			62.37- 122.37	96.40

15 Isopentane

CAS #: 78-78-4

3.556	3.584	(0.424)	43	1570397	48.8379	48.838	80.00- 120.00	100.00
3.556	3.584	(0.424)	57	897297			27.51- 87.51	57.14
3.556	3.584	(0.424)	72	88841			0.00- 35.95	5.66

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

16 Chloroethane CAS #: 75-00-3
 3.584 3.640 (0.427) 64 392829 40.1388 40.139 80.00- 120.00 100.00
 3.584 3.612 (0.427) 49 130060 2.42- 62.42 33.11
 3.584 3.640 (0.427) 66 120971 0.00- 58.92 30.79

18 Trichlorofluoromethane/Fr11 CAS #: 75-69-4
 3.888 3.916 (0.463) 101 1701415 48.8437 48.844 80.00- 120.00 100.00
 3.888 3.944 (0.463) 103 1118851 34.70- 94.70 65.76

21 Ethanol CAS #: 64-17-5
 4.275 4.331 (0.509) 45 459555 58.1165 58.116 80.00- 120.00 100.00
 4.248 4.331 (0.506) 43 94471 0.00- 50.43 20.56
 4.275 4.331 (0.509) 46 207424 12.21- 72.21 45.14

27 Freon 113 CAS #: 76-13-1
 4.745 4.773 (0.565) 151 897412 54.4045 54.404 80.00- 120.00 100.00
 4.745 4.773 (0.565) 153 565604 33.41- 93.41 63.03
 4.745 4.773 (0.565) 101 1381178 122.75- 182.75 153.91

29 1,1-Dichloroethene CAS #: 75-35-4
 4.773 4.801 (0.569) 61 1483988 52.8532 52.853 80.00- 120.00 100.00
 4.773 4.828 (0.569) 96 662589 14.37- 74.37 44.65
 4.773 4.828 (0.569) 98 418295 0.00- 59.03 28.19

30 Acetone CAS #: 67-64-1
 4.939 4.967 (0.588) 58 480764 47.8760 47.876 80.00- 120.00 100.00
 4.939 4.967 (0.588) 43 1763394 337.35- 397.35 366.79

33 Carbon Disulfide CAS #: 75-15-0
 5.132 5.188 (0.611) 76 2081253 48.1228 48.123 80.00- 120.00 100.00

34 2-Propanol CAS #: 67-63-0
 5.160 5.188 (0.615) 45 1919069 48.7783 48.778 80.00- 120.00 100.00
 5.160 5.188 (0.615) 43 436792 0.00- 50.64 22.76
 5.160 5.188 (0.615) 59 63332 0.00- 33.21 3.30

37 3-Chloropropene CAS #: 107-05-1
 5.437 5.464 (0.648) 76 352255 50.4365 50.436 80.00- 120.00 100.00
 5.437 5.464 (0.648) 41 1560656 414.53- 474.53 443.05

39 Methylene Chloride CAS #: 75-09-2
 5.713 5.741 (0.681) 49 1248170 52.2739 52.274 80.00- 120.00 100.00
 5.713 5.741 (0.681) 84 599116 18.52- 78.52 48.00
 5.713 5.741 (0.681) 51 363466 0.00- 59.93 29.12

42 MTBE CAS #: 1634-04-4
 6.045 6.073 (0.720) 73 2190142 45.5038 45.504 80.00- 120.00 100.00

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
42 MTBE (continued)									
6.045	6.073	(0.720)	57	630076			0.00- 58.72	28.77	
6.045	6.073	(0.720)	41	724948			1.95- 61.95	33.10	

43 trans-1,2-Dichloroethene					CAS #: 156-60-5				
6.100	6.128	(0.727)	96	667178	46.4975	46.498	80.00- 120.00	100.00	
6.100	6.128	(0.727)	61	1309035			166.86- 226.86	196.20	
6.100	6.128	(0.727)	98	421487			34.71- 94.71	63.17	

45 Hexane					CAS #: 110-54-3				
6.460	6.460	(0.769)	57	1592960	45.1008	45.101	80.00- 120.00	100.00	
6.460	6.460	(0.769)	43	1176023			44.61- 104.61	73.83	
6.460	6.460	(0.769)	86	222861			0.00- 43.77	13.99	

52 1,1-Dichloroethane					CAS #: 75-34-3				
6.902	6.930	(0.822)	63	1458863	48.9030	48.903	80.00- 120.00	100.00	
6.902	6.930	(0.822)	65	438420			0.00- 59.98	30.05	

54 Vinyl Acetate					CAS #: 108-05-4				
6.957	6.985	(0.829)	86	172482	48.6071	48.607	80.00- 120.00	100.00	
6.957	6.985	(0.829)	43	2720645			1469.62-1529.62	1577.35	
6.957	6.985	(0.829)	42	233280			100.08- 160.08	135.25	

63 cis-1,2-Dichloroethene					CAS #: 156-59-2				
7.953	7.953	(0.947)	61	1067231	47.0211	47.021	80.00- 120.00	100.00	
7.953	7.953	(0.947)	96	618684			25.91- 85.91	57.97	
7.953	7.953	(0.947)	98	384031			5.77- 65.77	35.98	

64 2-Butanone					CAS #: 78-93-3				
7.980	8.008	(0.951)	72	342925	42.1140	42.114	80.00- 120.00	100.00	
7.980	8.008	(0.951)	43	2015072			568.31- 628.31	587.61	
7.980	8.008	(0.951)	57	133574			10.61- 70.61	38.95	

66 Tetrahydrofuran					CAS #: 109-99-9				
8.367	8.368	(0.997)	42	1216478	40.1236	40.124	80.00- 120.00	100.00	
8.367	8.368	(0.997)	71	295333			0.00- 55.57	24.28	
8.367	8.395	(0.997)	72	333920			0.00- 56.52	27.45	

69 Chloroform					CAS #: 67-66-3				
8.506	8.533	(1.013)	83	1197931	41.8949	41.895	80.00- 120.00	100.00	
8.506	8.533	(1.013)	85	773539			34.12- 94.12	64.57	

72 Cyclohexane					CAS #: 110-82-7				
8.755	8.755	(1.043)	84	910056	42.6976	42.698	80.00- 120.00	100.00	
8.727	8.755	(1.040)	56	1477210			133.00- 193.00	162.32	
8.727	8.755	(1.040)	41	908407			69.15- 129.15	99.82	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

73	1,1,1-Trichloroethane					CAS #:	71-55-6			
8.755	8.782	(1.043)	97	1245968	48.2637	48.264	80.00-	120.00	100.00	
8.755	8.782	(1.043)	99	785161			33.65-	93.65	63.02	

75	Carbon Tetrachloride					CAS #:	56-23-5			
9.003	9.004	(1.072)	119	1048912	50.3029	50.303	80.00-	120.00	100.00	
9.003	9.004	(1.072)	117	1147915			83.17-	143.17	109.44	

78	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.418	9.446	(1.122)	57	4180319	42.0341	42.034	80.00-	120.00	100.00	
9.418	9.446	(1.122)	56	1466451			4.45-	64.45	35.08	
9.418	9.446	(1.122)	41	1287466			0.00-	59.44	30.80	

79	Benzene					CAS #:	71-43-2			
9.418	9.446	(0.919)	78	1904928	43.2479	43.248	80.00-	120.00	100.00	
9.418	9.446	(0.919)	77	475777			0.00-	54.39	24.98	

81	1,2-Dichloroethane					CAS #:	107-06-2			
9.612	9.612	(0.938)	62	1062574	51.5126	51.513	80.00-	120.00	100.00	
9.612	9.612	(0.938)	64	327123			1.44-	61.44	30.79	

82	Heptane					CAS #:	142-82-5			
9.805	9.833	(0.957)	100	223648	42.5069	42.507	80.00-	120.00	100.00	
9.805	9.833	(0.957)	43	1792015			789.66-	849.66	801.27	
9.805	9.833	(0.957)	71	719332			294.27-	354.27	321.64	

92	Trichloroethene					CAS #:	79-01-6			
10.662	10.690	(1.040)	95	658004	46.4436	46.444	80.00-	120.00	100.00	
10.662	10.690	(1.040)	130	590153			58.06-	118.06	89.69	
10.662	10.690	(1.040)	97	429878			31.73-	91.73	65.33	

93	Methyl Cyclohexane					CAS #:	108-87-2			
10.911	10.911	(1.300)	83	1086587	40.7571	40.757	80.00-	120.00	100.00	
10.911	10.911	(1.300)	98	500491			15.00-	75.00	46.06	
10.884	10.911	(1.296)	55	1261280			87.18-	147.18	116.08	

95	1,2-Dichloropropane					CAS #:	78-87-5			
11.188	11.188	(1.092)	63	689812	42.7369	42.737	80.00-	120.00	100.00	
11.188	11.188	(1.092)	62	520514			44.15-	104.15	75.46	
11.188	11.188	(1.092)	41	598462			56.32-	116.32	86.76	

96	1,4-Dioxane					CAS #:	123-91-1			
11.409	11.409	(1.113)	88	390807	46.4444	46.444	80.00-	120.00	100.00	
11.409	11.409	(1.113)	58	359452			63.91-	123.91	91.98	
11.409	11.409	(1.113)	57	124342			0.54-	60.54	31.82	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

98 Bromodichloromethane						CAS #: 75-27-4			
11.741	11.741	(1.146)	83	1118397	46.8590	46.859	80.00-	120.00	100.00
11.741	11.741	(1.146)	85	714554			34.28-	94.28	63.89

100 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.625	12.626	(1.232)	75	899740	44.2009	44.201	80.00-	120.00	100.00
12.625	12.626	(1.232)	77	271416			3.07-	63.07	30.17
12.625	12.626	(1.232)	39	756409			55.28-	115.28	84.07

101 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.902	12.902	(1.259)	58	639267	38.9505	38.950	80.00-	120.00	100.00
12.902	12.902	(1.259)	43	1909148			251.14-	311.14	298.65
12.902	12.902	(1.259)	85	215072			2.33-	62.33	33.64

103 Toluene						CAS #: 108-88-3			
13.096	13.096	(1.278)	91	1895120	47.5170	47.517	80.00-	120.00	100.00
13.096	13.096	(1.278)	92	1132891			32.96-	92.96	59.78

106 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.621	13.621	(0.895)	75	977005	46.2912	46.291	80.00-	120.00	100.00
13.621	13.621	(0.895)	77	302399			2.23-	62.23	30.95
13.621	13.621	(0.895)	39	751598			48.01-	108.01	76.93

108 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.870	13.897	(0.911)	97	564453	45.9383	45.938	80.00-	120.00	100.00
13.897	13.897	(0.913)	99	358841			30.01-	90.01	63.57
13.870	13.897	(0.911)	83	490762			53.24-	113.24	86.94

109 Tetrachloroethene						CAS #: 127-18-4			
13.925	13.953	(0.915)	166	663317	50.8270	50.827	80.00-	120.00	100.00
13.925	13.925	(0.915)	129	514158			43.63-	103.63	77.51
13.925	13.925	(0.915)	131	493593			41.85-	101.85	74.41

112 2-Hexanone						CAS #: 591-78-6			
14.257	14.257	(0.936)	58	841682	43.4026	43.403	80.00-	120.00	100.00
14.257	14.257	(0.936)	43	1827244			184.53-	244.53	217.09
14.257	14.257	(0.936)	100	134674			0.00-	45.68	16.00

114 Dibromochloromethane						CAS #: 124-48-1			
14.423	14.423	(0.947)	129	841716	50.4810	50.481	80.00-	120.00	100.00
14.423	14.423	(0.947)	127	651928			46.96-	106.96	77.45

115 1,2-Dibromoethane						CAS #: 106-93-4			
14.589	14.589	(0.958)	107	817601	47.4220	47.422	80.00-	120.00	100.00
14.589	14.589	(0.958)	109	763378			63.36-	123.36	93.37

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
124 Chlorobenzene						CAS #: 108-90-7				
15.252	15.252	(1.002)	112	1310206	46.0794	46.079	80.00- 120.00	100.00		
15.252	15.252	(1.002)	114	412585			1.03- 61.03	31.49		
15.252	15.252	(1.002)	77	979966			39.68- 99.68	74.79		

127 Ethyl Benzene						CAS #: 100-41-4				
15.363	15.363	(1.009)	106	729999	45.7295	45.730	80.00- 120.00	100.00		
15.363	15.363	(1.009)	91	2519352			309.90- 369.90	345.12		

128 m,p-Xylene						CAS #: 108-38-3				
15.529	15.529	(1.020)	106	946353	46.1017	46.102	80.00- 120.00	100.00		
15.529	15.529	(1.020)	91	1995161			177.38- 237.38	210.83		

130 o-Xylene						CAS #: 95-47-6				
16.054	16.054	(1.054)	106	899275	45.4316	45.432	80.00- 120.00	100.00		
16.054	16.054	(1.054)	91	2061050			200.33- 260.33	229.19		

131 Styrene						CAS #: 100-42-5				
16.082	16.109	(1.056)	104	1289114	42.3091	42.309	80.00- 120.00	100.00		
16.082	16.082	(1.056)	78	803959			31.42- 91.42	62.37		

133 Bromoform						CAS #: 75-25-2				
16.358	16.358	(1.074)	173	731909	53.1184	53.118	80.00- 120.00	100.00		
16.358	16.358	(1.074)	171	372703			20.95- 80.95	50.92		

135 Cumene						CAS #: 98-82-8				
16.524	16.524	(1.085)	105	2753991	45.5924	45.592	80.00- 120.00	100.00		
16.524	16.524	(1.085)	120	633510			0.00- 53.14	23.00		
16.496	16.496	(1.084)	51	421145			0.00- 45.39	15.29		

142 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5				
16.966	16.967	(1.114)	83	1285228	45.3313	45.331	80.00- 120.00	100.00		
16.966	16.967	(1.114)	85	822505			33.54- 93.54	64.00		

143 Propylbenzene						CAS #: 103-65-1				
16.994	16.994	(1.116)	91	3421509	50.0939	50.094	80.00- 120.00	100.00		
16.994	16.994	(1.116)	120	628955			0.00- 48.79	18.38		
16.994	16.994	(1.116)	105	120519			0.00- 33.35	3.52		

145 4-Ethyltoluene						CAS #: 622-96-8				
17.132	17.132	(1.125)	105	3110585	52.4035	52.404	80.00- 120.00	100.00		
17.132	17.132	(1.125)	120	746837			0.00- 54.09	24.01		

146 1,3,5-Trimethylbenzene						CAS #: 108-67-8				
17.215	17.215	(1.131)	105	2576248	45.8571	45.857	80.00- 120.00	100.00		
17.215	17.215	(1.131)	120	1073737			12.64- 72.64	41.68		

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

151	1,2,4-Trimethylbenzene						CAS #: 95-63-6		
17.602	17.602	(1.156)	105	2377788	46.7417	46.742	80.00-	120.00	100.00
17.602	17.602	(1.156)	120	941492			9.11-	69.11	39.60

154	1,3-Dichlorobenzene						CAS #: 541-73-1		
17.907	17.907	(1.176)	146	1230896	55.7078	55.708	80.00-	120.00	100.00
17.907	17.907	(1.176)	148	783232			32.20-	92.20	63.63
17.879	17.907	(1.174)	111	539365			13.28-	73.28	43.82

155	1,4-Dichlorobenzene						CAS #: 106-46-7		
17.989	17.990	(1.182)	146	1456721	51.7005	51.700	80.00-	120.00	100.00
17.989	17.990	(1.182)	148	926830			34.16-	94.16	63.62
17.989	17.990	(1.182)	111	682684			16.41-	76.41	46.86

156	alpha-Chlorotoluene						CAS #: 100-44-7		
18.128	18.128	(1.191)	91	2295597	56.2730	56.273	80.00-	120.00	100.00
18.128	18.128	(1.191)	126	378569			0.00-	46.97	16.49

158	1,2-Dichlorobenzene						CAS #: 95-50-1		
18.321	18.321	(1.203)	146	1283508	52.9283	52.928	80.00-	120.00	100.00
18.321	18.321	(1.203)	148	816740			31.71-	91.71	63.63
18.321	18.321	(1.203)	111	663860			20.11-	80.11	51.72

163	1,2,4-Trichlorobenzene						CAS #: 120-82-1		
19.593	19.593	(1.287)	180	928847	61.5093	61.509	80.00-	120.00	100.00
19.593	19.593	(1.287)	182	879313			62.26-	122.26	94.67

164	Hexachlorobutadiene						CAS #: 87-68-3		
19.676	19.676	(1.292)	225	1018280	52.7902	52.790	80.00-	120.00	100.00
19.676	19.676	(1.292)	223	653913			35.72-	95.72	64.22

165	Naphthalene						CAS #: 91-20-3		
19.787	19.787	(1.300)	128	2297622	47.6178	47.618	80.00-	120.00	100.00
19.787	19.787	(1.300)	127	328623			0.00-	43.72	14.30

Report Date: 25-Apr-2007 11:29

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 25-APR-2007

Lab File ID: 8042503.d

Calibration Time: 10:40

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /var/chem/msd8.i/8-25apr.b/t14q322b.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	232391	139435	325347	173884	-25.18
86 1,4-Difluorobenze	1035529	621317	1449741	790852	-23.63
123 Chlorobenzene-d5	744287	446572	1042002	605228	-18.68

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
67 Bromochloromethan	8.40	8.07	8.73	8.40	0.00
86 1,4-Difluorobenze	10.28	9.95	10.61	10.25	-0.27
123 Chlorobenzene-d5	15.22	14.89	15.55	15.22	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-25apr.1b/8042503.d
Date: 25-APR-2007 11:08
Client ID: LCS-1
Sample Info: 50mL #1487-194

Column phase: RTX-624

Instrument: msd8.1
Operator: JG
Column diameter: 0.53

/chem/msd8.1/8-25apr.1b/8042503.d

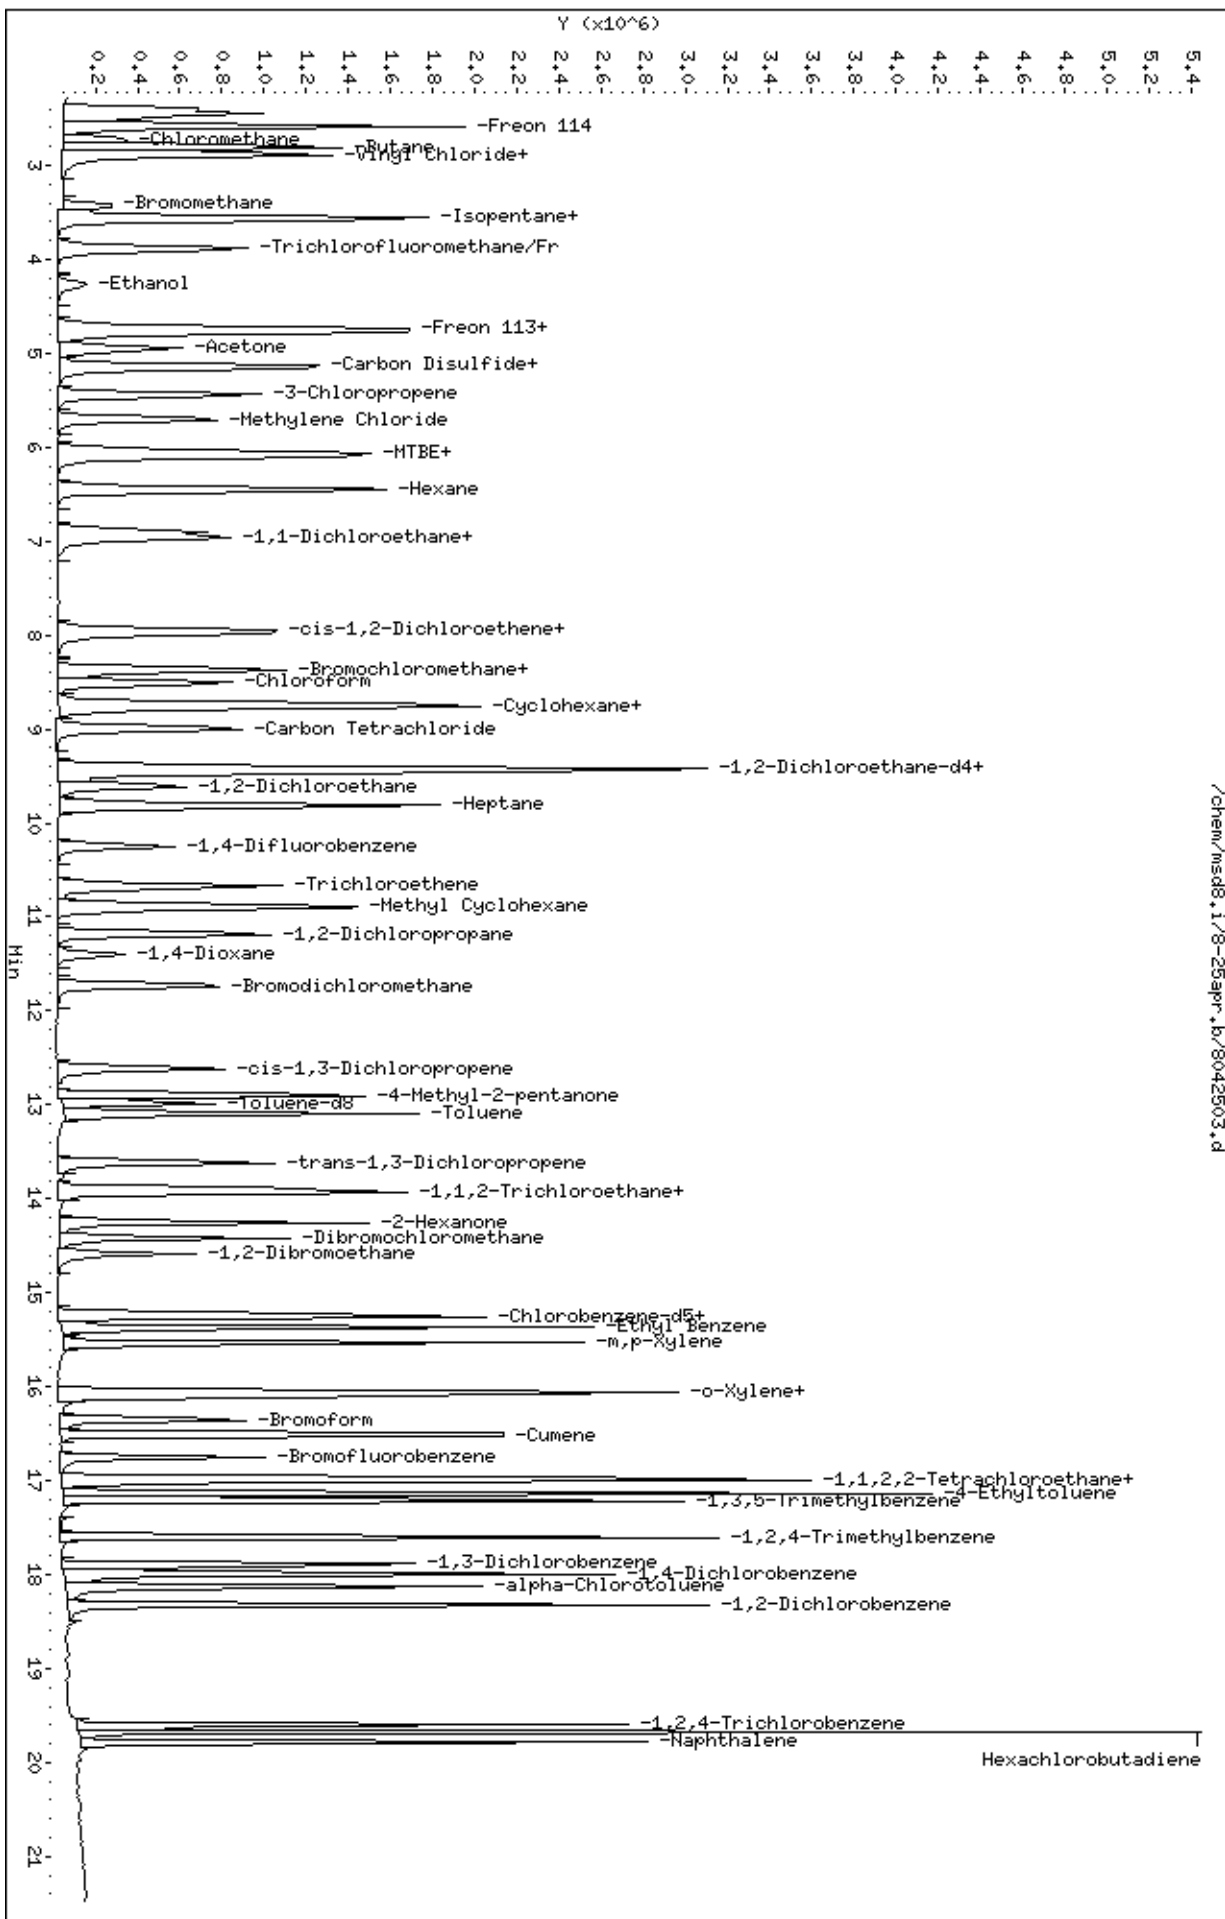

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	32.21
75	30.0 - 60.0% of mass 95	58.81
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.24
173	Less than 2.0% of mass 174	(0.00) ¹
174	Greater than 50.0% of mass 95	55.12
175	5.0 - 9.0% of mass 174	(8.03) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(96.69) ¹
177	5.0 - 9.0% of mass 176	(0.44) ²

BFB Injection Date: 4/25/07 Logbook #: 1478
 BFB Injection Time: 1012
 BFB File ID: 8042501
 Tekmar Purge Flow: AS 4/25/07
 Vacuum: AS 4/25/07
 IS/S Std #: 1443-3 Exp. Date: 5/26/07
 BCM 2323A1
 1,4-DFB 103552A
 CB-d5 244287
 Verified CCVIS vs ICAL mid-point (-40%D) AS
Initials

1 - value in parenthesis is % mass 174
 2 - value in parenthesis is % mass 176
 Verify 176/174 m/z Ratio: 605056/625728 = 96.90%

NOAH Cart #: 5/15 File #: 8042508/8042507

File ID: 8042502
 Compound: FDL-AL8
 Initials: AS

Calculation Check:

$$\text{ppbv of compound} = \frac{\text{Area}_{\text{sample}}}{\text{Areas}} \times \frac{\text{Conc. in RRF}}{\text{Conc. in sample}} = \frac{(961488)}{(1035529)} \times \frac{(25)}{(0.98315)} = 23.610$$

Reported Result 23.610

Use	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Loader Init.	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	8042501	BFB Tune Check	843-2A12	5.0g	2µL	1.00	AS	4/25/07	1012	AS	
✓	02	CCV # 1408-387A	100 ppbv - 50 ppbv	50 ppbv	100 µL				1040	AS	
✓	03	LES # 1487-1A1	200 ppbv - 50 ppbv	50 ppbv	50 µL				1108	AS	
✓	04	Synkin Blank	13693	Humid	200 µL				1252	AS	
✓	05	Lab Blank							1321	AS	
✓	06	Noah Cart Cont	12911	Humid	800 µL	1.00	AS		1457	AS	Noah #8 legs 5 only
✓	07	part #15, leg 2	13673		1	1.00	AS		1666	AS	
✓	08	070441A-01A	4192	90% H ₂ O	8 µL	4.00			1741	AS	100X problem
✓	09	070439A-01A	33378	14.0% H ₂ O	200 µL	2.51			1813	AS	100X problem

Signature: AS Date: 4/25/07
 Revision 05/2005 Page 241

10	✓	8042510	0704404-01A	33805	6.0 ¹ / ₄ - 5psi	200ml	1.68	ES	4/15/07	1931	44	
11	✓	11	↓ -02A	34002	6.0 ¹ / ₄ - 5psi	↓	1.68	↓		2019	44	
12	✓	12	0704415-01A	14016	0.2psi - 5psi	↓	1.32	↓		2050a	44	
13	✓	13	↓ 02A	14882	1.0 ¹ / ₄ - 5psi	0.8ml	348	↓		2133	KR	RE 0.6ml
14	✓	14	0704397-01A	33710	3.0 ¹ / ₄ - 5psi	5.4ml	55.2	↓		2204	KR	"E" 2-propanol
15	✓	15	02A	341250	2.0 ¹ / ₄ - 5psi	2.1ml	191	↓		2232	KR	"B" 2-propanol
16	✓	16	↓ 02A	↓	1.0 ¹ / ₄ - 5psi	2.1ml	↓	↓		2352	KR	"B" 2-propanol
17	✓	17	0704415-02A	14852	1.0 ¹ / ₄ - 5psi	0.6ml	463	↓		0004	KR	
18	✓	18	070441A-01A	4192	6.0 ¹ / ₄ - 5psi	16ml	2320	↓		0045	KR	
19	✓	19	0704404-03A	9573	6.0 ¹ / ₄ - 5psi	200ml	168	↓		0137	KR	
20	✓	20	↓ -04A	36033	2.0 ¹ / ₄ - 5psi	↓	100	↓		0219	KR	
21	✓	21	0704442-01A	1399	0.5 ¹ / ₄ - 5psi	↓	136	↓		0301	KR	FB @ Acetone 2-2.5
22	✓	22	↓ -01A	1399	↓	↓	↓	↓		0344	KR	
23	✓	23	↓ -02A	1472	1.0 ¹ / ₄ - 15psi	65ml	643	↓		0421	KR	RE 200ml
24	✓	24	↓ -03A	2065	1.0 ¹ / ₄ - 15psi	200ml	209	↓		0503	KR	
25	✓	25	0704341-01A	12205	2.0 ¹ / ₄ - 5psi	50ml	700	↓		0540	KR	100% RE 4ml
26	✓	26	↓ -02A	12459	↓	↓	↓	↓				
27	✓	27	↓ -02AA	↓	↓	↓	↓	↓				
28	✓	28	System Blank	12941	Humid	200ml	1.00	KR		0635	KR	
29												
30												
31												
32												

Comments:

[Handwritten notes and scribbles in the comments section]

Signature *[Handwritten Signature]*

Date *2/16/07*

Report Date: 22-Mar-2007 09:23

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-22mar.b/8032201.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 22-MAR-2007 09:29
 Operator : srs Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2786
 Comment :
 Method : /var/chem/msd8.i/8-22mar.b/bfb30.m
 Meth Date : 22-Mar-2007 09:23 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb						CAS #: 460-00-4	
3.803	3.748	0.055	95	1175749			100.00- 100.00	100.00
3.803	3.748	0.055	50	367505			15.00- 40.00	31.26
3.803	3.748	0.055	75	659620			30.00- 60.00	56.10
3.803	3.748	0.055	96	74114			5.00- 9.00	6.30
3.803	3.748	0.055	173	176			0.00- 2.00	0.03
3.803	3.748	0.055	174	701792			50.00- 100.00	59.69
3.803	3.748	0.055	175	44998			5.00- 9.00	6.41
3.803	3.748	0.055	176	675517			95.00- 101.00	96.26
3.803	3.748	0.055	177	43845			5.00- 9.00	6.49

Date : 22-MAR-2007 09:29

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: srs

Column phase:

Column diameter: 0.53



Date : 22-MAR-2007 09:29

Client ID: BFB

Instrument: msd8,i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: srs

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	31.26
75	30.00 - 60.00% of mass 95	56.10
96	5.00 - 9.00% of mass 95	6.30
173	Less than 2.00% of mass 174	0.01 (0.03)
174	50.00 - 100.00% of mass 95	59.69
175	5.00 - 9.00% of mass 174	3.83 (6.41)
176	95.00 - 101.00% of mass 174	57.45 (96.26)
177	5.00 - 9.00% of mass 176	3.73 (6.49)

Date : 22-MAR-2007 09:29

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: srs

Column phase:

Column diameter: 0.53

Data File: 8032201.d

Spectrum: Avg. Scans 26-28 (3.80), Background Scan 24

Location of Maximum: 95.00

Number of points: 216

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	17368	95.00	1175552	156.00	547	230.00	147
37.00	95296	96.00	74112	157.00	1221	231.00	120
38.00	79344	97.00	1966	159.00	1076	238.00	137
39.00	30888	102.00	374	160.00	412	242.00	192
40.00	1004	103.00	713	161.00	978	243.00	158
42.00	747	104.00	3265	162.00	76	245.00	103
44.00	8653	105.00	1211	163.00	156	247.00	145
45.00	14978	106.00	3258	164.00	185	248.00	153
46.00	1377	107.00	1067	165.00	212	249.00	152
47.00	24584	108.00	211	166.00	512	250.00	70
48.00	10631	109.00	364	167.00	233	253.00	677
49.00	81272	110.00	373	168.00	477	255.00	60
50.00	367488	111.00	793	169.00	450	257.00	111
51.00	109000	112.00	548	170.00	961	258.00	314
52.00	4533	113.00	829	171.00	617	259.00	138
53.00	295	115.00	620	172.00	200	260.00	411
54.00	656	116.00	2850	173.00	176	261.00	201
55.00	4277	117.00	4491	174.00	701760	262.00	199
56.00	23336	118.00	3301	175.00	44992	263.00	144
57.00	39272	119.00	3137	176.00	675456	267.00	241
58.00	1897	120.00	285	177.00	43840	273.00	69
59.00	523	121.00	749	178.00	1250	284.00	162
60.00	14828	122.00	199	179.00	221	289.00	71
61.00	68712	123.00	280	180.00	99	290.00	167
62.00	64208	124.00	489	181.00	96	293.00	90
63.00	46984	125.00	96	182.00	48	296.00	181
64.00	4051	126.00	136	184.00	158	297.00	152
65.00	326	127.00	288	185.00	75	298.00	89
66.00	502	128.00	2354	187.00	233	300.00	159
67.00	1549	129.00	1080	191.00	383	303.00	180
68.00	136640	130.00	2707	192.00	28	304.00	82
69.00	131392	131.00	1090	194.00	245	306.00	188
70.00	8582	132.00	77	195.00	83	307.00	71
71.00	1100	133.00	759	197.00	112	309.00	220
72.00	7269	134.00	381	201.00	76	310.00	73

Date : 22-MAR-2007 09:29

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: srs

Column phase:

Column diameter: 0.53

Data File: 8032201.d

Spectrum: Avg. Scans 26-28 (3.80), Background Scan 24

Location of Maximum: 95.00

Number of points: 216

m/z	Y	m/z	Y	m/z	Y	m/z	Y
73.00	57272	135.00	1208	202.00	314	311.00	185
74.00	219264	136.00	521	203.00	77	312.00	76
75.00	659584	137.00	1129	205.00	105	313.00	40
76.00	55072	138.00	58	207.00	644	314.00	151
77.00	6210	139.00	602	208.00	178	316.00	68
78.00	4088	141.00	8415	210.00	259	317.00	69
79.00	25056	142.00	737	211.00	74	319.00	72
80.00	8805	143.00	9048	212.00	88	322.00	40
81.00	25072	144.00	821	214.00	182	326.00	78
82.00	5117	145.00	1133	215.00	73	331.00	79
83.00	380	146.00	882	216.00	224	336.00	74
84.00	413	147.00	301	217.00	176	337.00	101
86.00	1542	148.00	1337	219.00	301	341.00	103
87.00	50160	149.00	391	220.00	204	343.00	481
88.00	47656	150.00	1148	221.00	118	344.00	292
89.00	267	151.00	708	223.00	202	346.00	47
91.00	3315	152.00	499	225.00	170		
92.00	30656	153.00	823	226.00	164		
93.00	48528	154.00	585	228.00	128		
94.00	142784	155.00	1853	229.00	71		

Report Date: 26-Mar-2007 08:57

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-26mar.b/8032601.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 26-MAR-2007 09:03
 Operator : ea Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2912
 Comment :
 Method : /var/chem/msd8.i/8-26mar.b/bfb30.m
 Meth Date : 26-Mar-2007 08:57 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb								
3.803	3.748	0.055	95	2384521			100.00- 100.00	100.00
3.803	3.748	0.055	50	692921			15.00- 40.00	29.06
3.803	3.748	0.055	75	1291079			30.00- 60.00	54.14
3.803	3.748	0.055	96	153259			5.00- 9.00	6.43
3.803	3.748	0.055	173	0			0.00- 2.00	0.00
3.803	3.748	0.055	174	1255899			50.00- 100.00	52.67
3.803	3.748	0.055	175	99889			5.00- 9.00	7.95
3.803	3.748	0.055	176	1198128			95.00- 101.00	95.40
3.803	3.748	0.055	177	78262			5.00- 9.00	6.53

Date : 26-MAR-2007 09:03

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: ea

Column phase:

Column diameter: 0.53



Date : 26-MAR-2007 09:03

Client ID: BFB

Instrument: msd8,i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: ea

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	29.06
75	30.00 - 60.00% of mass 95	54.14
96	5.00 - 9.00% of mass 95	6.43
173	Less than 2.00% of mass 174	0.00 (0.00)
174	50.00 - 100.00% of mass 95	52.67
175	5.00 - 9.00% of mass 174	4.19 (7.95)
176	95.00 - 101.00% of mass 174	50.25 (95.40)
177	5.00 - 9.00% of mass 176	3.28 (6.53)

Date : 26-MAR-2007 09:03

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: ea

Column phase:

Column diameter: 0.53

Data File: 8032601.d

Spectrum: Avg. Scans 26-28 (3.80), Background Scan 24

Location of Maximum: 95.00

Number of points: 203

m/z	Y	m/z	Y	m/z	Y	m/z	Y
35.00	195	91.00	6069	149.00	856	232.00	975
36.00	29232	92.00	62096	150.00	1457	236.00	199
37.00	163072	93.00	96864	151.00	920	244.00	235
38.00	139136	94.00	261312	152.00	276	246.00	291
39.00	54504	95.00	2384384	153.00	1211	250.00	294
40.00	476	96.00	153216	154.00	515	252.00	248
44.00	9853	97.00	3416	155.00	3267	254.00	26
45.00	26728	98.00	440	157.00	2464	256.00	5
47.00	47912	100.00	128	158.00	425	257.00	317
48.00	20328	101.00	987	159.00	1563	259.00	100
49.00	140992	104.00	6092	160.00	134	263.00	388
50.00	692864	105.00	1471	161.00	1495	267.00	53
51.00	200768	106.00	5907	162.00	248	268.00	17
52.00	7992	107.00	1526	163.00	126	269.00	224
54.00	568	108.00	19	166.00	463	270.00	186
55.00	6269	110.00	730	168.00	783	271.00	64
56.00	42136	111.00	1093	169.00	1180	273.00	57
57.00	74808	112.00	933	170.00	701	274.00	358
58.00	2453	113.00	853	171.00	1361	276.00	71
59.00	1045	114.00	317	174.00	1255424	277.00	179
60.00	25104	115.00	1261	175.00	99888	279.00	160
61.00	129520	116.00	5132	176.00	1198080	285.00	234
62.00	129464	117.00	8915	177.00	78256	286.00	70
63.00	90936	118.00	4419	178.00	2052	287.00	97
64.00	7300	119.00	7927	179.00	52	288.00	166
65.00	952	121.00	53	181.00	208	290.00	14
66.00	177	124.00	1048	182.00	25	292.00	113
67.00	7131	125.00	179	183.00	103	293.00	88
68.00	255232	126.00	635	184.00	24	297.00	55
69.00	261568	127.00	482	186.00	45	301.00	237
70.00	16728	128.00	5195	188.00	320	305.00	165
71.00	946	129.00	2340	189.00	192	307.00	191
72.00	12813	130.00	4681	191.00	669	309.00	173
73.00	105472	131.00	1755	192.00	550	311.00	511
74.00	409664	132.00	97	193.00	171	312.00	167

Date : 26-MAR-2007 09:03

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: ea

Column phase:

Column diameter: 0.53

Data File: 8032601.d

Spectrum: Avg. Scans 26-28 (3.80), Background Scan 24

Location of Maximum: 95.00

Number of points: 203

m/z	Y	m/z	Y	m/z	Y	m/z	Y
75.00	1290752	133.00	1720	197.00	21	313.00	174
76.00	108680	134.00	1145	198.00	104	315.00	130
77.00	12010	135.00	1028	199.00	132	323.00	77
78.00	7804	136.00	442	201.00	86	324.00	295
79.00	44592	137.00	1916	203.00	239	327.00	37
80.00	13959	138.00	222	204.00	112	328.00	138
81.00	46472	139.00	458	206.00	279	329.00	193
82.00	8716	140.00	409	207.00	1386	332.00	130
83.00	1106	141.00	14444	211.00	262	334.00	233
84.00	86	142.00	2541	215.00	164	335.00	129
85.00	637	143.00	15084	218.00	320	340.00	104
86.00	843	144.00	623	223.00	362	341.00	351
87.00	96208	145.00	495	224.00	160	344.00	386
88.00	88216	146.00	1934	226.00	114	346.00	405
89.00	256	147.00	1293	228.00	159	349.00	73
90.00	728	148.00	3617	231.00	208		

Report Date: 25-Apr-2007 10:05

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-25apr.b/8042501.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 25-APR-2007 10:12
 Operator : JG Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2912
 Comment :
 Method : /var/chem/msd8.i/8-25apr.b/bfb30.m
 Meth Date : 25-Apr-2007 10:05 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb					CAS #: 460-00-4	
3.803	3.748	0.055	95	1135213		100.00- 100.00	100.00
3.803	3.748	0.055	50	371272		15.00- 40.00	32.71
3.803	3.748	0.055	75	667597		30.00- 60.00	58.81
3.803	3.748	0.055	96	76481		5.00- 9.00	6.74
3.803	3.748	0.055	173	0		0.00- 2.00	0.00
3.803	3.748	0.055	174	625782		50.00- 100.00	55.12
3.803	3.748	0.055	175	50231		5.00- 9.00	8.03
3.803	3.748	0.055	176	605095		95.00- 101.00	96.69
3.803	3.748	0.055	177	38964		5.00- 9.00	6.44

Date : 25-APR-2007 10:12

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53



Date : 25-APR-2007 10:12

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	32.71
75	30.00 - 60.00% of mass 95	58.81
96	5.00 - 9.00% of mass 95	6.74
173	Less than 2.00% of mass 174	0.00 (0.00)
174	50.00 - 100.00% of mass 95	55.12
175	5.00 - 9.00% of mass 174	4.42 (8.03)
176	95.00 - 101.00% of mass 174	53.30 (96.69)
177	5.00 - 9.00% of mass 176	3.43 (6.44)

Date : 25-APR-2007 10:12

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8042501.d

Spectrum: Avg. Scans 26-28 (3.80), Background Scan 24

Location of Maximum: 95.00

Number of points: 189

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	17048	88.00	36888	144.00	645	212.00	153
37.00	93072	89.00	26	145.00	858	213.00	86
38.00	78552	90.00	97	146.00	773	214.00	93
39.00	31800	91.00	4307	147.00	1046	216.00	240
40.00	824	92.00	31344	148.00	2297	219.00	179
42.00	124	93.00	49464	149.00	732	220.00	85
43.00	351	94.00	132224	150.00	909	223.00	177
44.00	9338	95.00	1135104	151.00	176	231.00	92
45.00	14259	96.00	76480	152.00	508	232.00	353
46.00	25	97.00	2044	153.00	772	233.00	267
47.00	21096	100.00	69	154.00	728	234.00	74
48.00	11167	101.00	111	155.00	2118	236.00	79
49.00	79208	103.00	355	156.00	844	241.00	165
50.00	371264	104.00	3463	157.00	1433	246.00	67
51.00	108680	105.00	1267	158.00	528	247.00	164
52.00	4765	106.00	3208	159.00	942	250.00	251
55.00	3602	107.00	525	160.00	145	251.00	165
56.00	24040	108.00	304	161.00	942	253.00	286
57.00	41120	109.00	17	163.00	222	254.00	206
58.00	1991	110.00	363	164.00	429	255.00	111
59.00	292	111.00	802	165.00	4	260.00	591
60.00	13827	112.00	419	166.00	124	261.00	43
61.00	71584	113.00	800	167.00	46	266.00	82
62.00	68792	114.00	94	168.00	262	270.00	46
63.00	50640	115.00	913	169.00	368	272.00	174
64.00	4285	116.00	2640	170.00	723	273.00	88
65.00	653	117.00	5026	171.00	1290	274.00	84
66.00	87	118.00	3020	172.00	102	285.00	80
67.00	3040	119.00	3353	174.00	625728	286.00	90
68.00	132480	120.00	391	175.00	50224	290.00	70
69.00	132544	122.00	229	176.00	605056	293.00	124
70.00	9355	123.00	489	177.00	38960	295.00	94
71.00	235	124.00	435	178.00	1237	296.00	80
72.00	6476	125.00	312	181.00	96	297.00	194
73.00	56456	126.00	405	182.00	86	301.00	72

Date : 25-APR-2007 10:12

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8042501.d

Spectrum: Avg. Scans 26-28 (3.80), Background Scan 24

Location of Maximum: 95.00

Number of points: 189

m/z	Y	m/z	Y	m/z	Y	m/z	Y
74.00	213504	128.00	3195	187.00	98	312.00	68
75.00	667584	129.00	1127	189.00	70	322.00	146
76.00	54824	130.00	2778	190.00	301	324.00	81
77.00	5860	131.00	1043	194.00	151	327.00	72
78.00	1967	132.00	144	195.00	5	336.00	154
79.00	27200	135.00	1419	196.00	172	341.00	123
80.00	7345	137.00	1572	197.00	67	342.00	105
81.00	27744	138.00	76	201.00	149	343.00	378
82.00	5351	139.00	620	203.00	71	347.00	85
83.00	699	140.00	379	204.00	126	349.00	70
85.00	392	141.00	8531	207.00	785		
86.00	1037	142.00	1245	208.00	190		
87.00	39208	143.00	9074	211.00	177		

Shipping/ Receiving Documents



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: _____ GEI Consultants, Inc.
ATTENTION: _____ Ms. Sarah Aldridge
FAX #: _____ 860-368-5307
FROM: _____ Sample Receiving
Workorder #: _____ 0704404
of pages (Including Cover): _____ 1

5/8/2007

Thank you for selecting Air Toxics Ltd. We have received your samples and have found discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Kelly Buettner at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

The following discrepancies have been observed:

We have found a discrepancy between the Chain of Custody (COC) and the sample tag. The sample labeled BS041807AMS2XXXX on the COC is labeled as BS041807AMSXXXX on the sample tag. ATL will report the sample identification on the COC unless otherwise notified.

Sample identification for sample BS041807AMS2UW was not provided on the sample tag. The information on the Chain of Custody will be used to process and report the sample.

Your prompt response is appreciated.



AN ENVIRONMENTAL ANALYTICAL LABORATORY

SAMPLE RECEIPT SUMMARY

WORKORDER 0704404

Client	Phone	Date Promised: 05/04/07
Ms. Sarah Aldridge	860-368-5300	Date Completed: 5/1/07
GEI Consultants, Inc.		Date Received: 4/20/07
455 Winding Brook Dr. Suite 201	Fax	PO#: NR
Glastonbury, CT 06033	860-368-5307	Project#: 061140-8-1703 Bayshore Southern Cell IRM
Sales Rep: ANS		Total \$: \$ 1,308.00
		Logged By: BL

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A	BS041807AMS2UW	Modified TO-15	4/18/2007	6.0 "Hg	\$225.00
02A	BS041807AMS2XXXX	Modified TO-15	4/18/2007	6.0 "Hg	\$225.00
03A	BS041807AMS4DW	Modified TO-15	4/18/2007	6.0 "Hg	\$225.00
04A	BS041807 TB	Modified TO-15	4/18/2007	29.0 "Hg	\$225.00
05A	Lab Blank	Modified TO-15	NA	NA	\$0.00
06A	CCV	Modified TO-15	NA	NA	\$0.00
07A	LCS	Modified TO-15	NA	NA	\$0.00

Misc. Charges 6 Liter Summa Canister (1) @ \$50.00 each.	\$50.00
6 Liter Summa Canister (100% Certified) (3) @ \$65.00 each.	\$195.00
Fuel Surcharge (4) @ \$2.00 each.	\$8.00
Blue Body Flow Controller (100% Certified) (3) @ \$40.00 each.	\$120.00
Blue Body Flow Controller (1) @ \$35.00 each.	\$35.00

Note: Samples received after 3 P.M. PST are considered to be received on the following work day.
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

BILL TO: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Dr. Suite 201
Glastonbury, CT 06033

Analysis Code: TO-14A

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

Sample Discrepancy Report

If Section III or IV is filled out CSR must be notified within 24 hrs of initiation

Initiated By: BZ

Date: 4-20-07

Given To: _____

File to folder

Sections I – II/III/IV must be filled out by person initiating this Sample Discrepancy Report

I. **Workorder(s) affected:** 6704404
Sample(s) affected: O1A & O2A

II. Sample Receipt Discrepancies (Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative)

- | | |
|---|---|
| <input type="checkbox"/> COC improperly relinquished / received. | <input type="checkbox"/> Flow controller used - canister samples received at ambient or under pressure. |
| <input type="checkbox"/> COC was not filled out in ink. | <input type="checkbox"/> No brass cap on canister (<i>do not narrate</i>). |
| <input checked="" type="checkbox"/> Sample tags / labels do not match the COC. | <input type="checkbox"/> VOA vial for RSK-175 analysis received with headspace bubble <5mm (<i>do not narrate</i>). |
| <input type="checkbox"/> Samples received at wrong temperature ($\neq 4\pm 2$ °C); ice / blue ice (circle one) was present. A temp. blank was / was <i>not</i> present (circle one). | <input type="checkbox"/> Other (describe below). |
| <input type="checkbox"/> Sample container (Tube/VOA vial) was received broken, <i>however</i> sample was intact. | |

Describe the Discrepancy: Sample O1A had no ID on the sample tag (used can # to ID). Sample O2A was labeled "BS041807AMS2XXXX" on the COC, and "BS041807AMSXXXX" on the sample tag.

Initials: _____ Date: _____

III. Sample Receipt Discrepancies requiring CSR notification (document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative)

- | | |
|---|--|
| <input type="checkbox"/> COC was not received with samples. | <input type="checkbox"/> Canister leaked to ambient during pressurization. |
| <input type="checkbox"/> Analysis method(s) is not specified / incorrectly specified (circle one) on the COC. | <input type="checkbox"/> Tedlar bag / canister received emitting a strong odor; sample can / cannot (circle one) be analyzed. |
| <input type="checkbox"/> Number of samples on the COC does not match the number of samples that were received. | <input type="checkbox"/> Canister sample received with a vacuum difference >7.0"Hg between the receipt vac. and the final vac. reported on the COC, indicating loss of vacuum. |
| <input type="checkbox"/> Samples were received expired. | <input type="checkbox"/> Canister sample received at >15"Hg (<i>not</i> identified as a Trip/Field Blank). |
| <input type="checkbox"/> Sampling date / time is not documented for <i>some</i> / <i>any</i> samples (circle one). | <input type="checkbox"/> Trip Blank received at low vacuum (< 25"Hg). |
| <input type="checkbox"/> Sample received with discernable volume of H ₂ O in the Tedlar Bag. | <input type="checkbox"/> Tedlar Bag for Sulfur analysis has metal fitting. |
| <input type="checkbox"/> Sample container (Tube/VOA vial/DNPH Bottle, etc.) was received broken / leaking (circle one). | <input type="checkbox"/> Incorrect sampling media / container for analysis requested. |
| <input type="checkbox"/> VOA vial for RSK-175 analysis received with headspace bubble >5mm. | <input type="checkbox"/> Custody Seal on the outside of the container was broken / improperly placed (circle one). |
| <input type="checkbox"/> Samples for RSK-175 CO ₂ analysis received preserved with HCl. | <input type="checkbox"/> Other (describe below). |
| <input type="checkbox"/> Tedlar Bag received leaking / flat (circle one). Sample can / cannot (circle one) be analyzed. | |

Describe the Discrepancy: _____

Initials: _____ Date: _____

Other Records

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	



www.airtoxics.com
1-800-985-5955

Media Certification Report

Canister Number: 6L#34002 10.2ml w/ T
Can#: 51073-34002
Date : 03/27/07 19:03
Data File: u032713.d

Name	CAS	Type	Conc.	Units
Ethyl Benzene	100-41-4	Not Found	0.00	ppbv
Styrene	100-42-5	Not Found	0.00	ppbv
alpha-Chlorotoluene	100-44-7	Not Found	0.00	ppbv
cis-1,3-Dichloropropene	10061-01-5	Not Found	0.00	ppbv
trans-1,3-Dichloropropene	10061-02-6	Not Found	0.00	ppbv
Propylbenzene	103-65-1	Not Found	0.00	ppbv
1,4-Dichlorobenzene	106-46-7	Not Found	0.00	ppbv
1,2-Dibromoethane (EDB)	106-93-4	Not Found	0.00	ppbv
1,3-Butadiene	106-99-0	Not Found	0.00	ppbv
3-Chloropropene	107-05-1	Not Found	0.00	ppbv
1,2-Dichloroethane	107-06-2	Not Found	0.00	ppbv
4-Methyl-2-pentanone	108-10-1	Not Found	0.00	ppbv
m,p-Xylene	108-38-3	Not Found	0.00	ppbv
1,3,5-Trimethylbenzene	108-67-8	Not Found	0.00	ppbv
Toluene	108-88-3	Not Found	0.00	ppbv
Chlorobenzene	108-90-7	Not Found	0.00	ppbv
Tetrahydrofuran	109-99-9	Not Found	0.00	ppbv
Hexane	110-54-3	Not Found	0.00	ppbv
Cyclohexane	110-82-7	Not Found	0.00	ppbv
1,2,4-Trichlorobenzene	120-82-1	Not Found	0.00	ppbv
1,4-Dioxane	123-91-1	Not Found	0.00	ppbv
Dibromochloromethane	124-48-1	Not Found	0.00	ppbv
Tetrachloroethene	127-18-4	Not Found	0.00	ppbv
Heptane	142-82-5	Not Found	0.00	ppbv
cis-1,2-Dichloroethene	156-59-2	Not Found	0.00	ppbv
trans-1,2-Dichloroethene	156-60-5	Not Found	0.00	ppbv
Methyl tert-butyl ether	1634-04-4	Not Found	0.00	ppbv
2,2,4-Trimethylpentane	540-84-1	Not Found	0.00	ppbv
1,3-Dichlorobenzene	541-73-1	Not Found	0.00	ppbv
Carbon Tetrachloride	56-23-5	Not Found	0.00	ppbv
2-Hexanone	591-78-6	Not Found	0.00	ppbv
4-Ethyltoluene	622-96-8	Not Found	0.00	ppbv
Ethanol	64-17-5	Not Found	0.00	ppbv
2-Propanol	67-63-0	Not Found	0.00	ppbv
Acetone	67-64-1	Not Found	0.00	ppbv
Chloroform	67-66-3	Not Found	0.00	ppbv
Benzene	71-43-2	Not Found	0.00	ppbv
1,1,1-Trichloroethane	71-55-6	Not Found	0.00	ppbv
Bromomethane	74-83-9	Not Found	0.00	ppbv
Chloromethane	74-87-3	Not Found	0.00	ppbv
Chloroethane	75-00-3	Not Found	0.00	ppbv
Vinyl Chloride	75-01-4	Not Found	0.00	ppbv
Methylene Chloride	75-09-2	Not Found	0.00	ppbv

Name	CAS	Type	Conc.	Units
Carbon Disulfide	75-15-0	Not Found	0.00	ppbv
Bromoform	75-25-2	Not Found	0.00	ppbv
Bromodichloromethane	75-27-4	Not Found	0.00	ppbv
1,1-Dichloroethane	75-34-3	Not Found	0.00	ppbv
1,1-Dichloroethene	75-35-4	Not Found	0.00	ppbv
Freon 11	75-69-4	Not Found	0.00	ppbv
Freon 12	75-71-8	Not Found	0.00	ppbv
Freon 113	76-13-1	Not Found	0.00	ppbv
Freon 114	76-14-2	Not Found	0.00	ppbv
1,2-Dichloropropane	78-87-5	Not Found	0.00	ppbv
2-Butanone (Methyl Ethyl	78-93-3	Not Found	0.00	ppbv
1,1,2-Trichloroethane	79-00-5	Not Found	0.00	ppbv
Trichloroethene	79-01-6	Not Found	0.00	ppbv
1,1,2,2-Tetrachloroethane	79-34-5	Not Found	0.00	ppbv
Hexachlorobutadiene	87-68-3	Not Found	0.00	ppbv
Naphthalene	91-20-3	Not Found	0.00	ppbv
o-Xylene	95-47-6	Not Found	0.00	ppbv
1,2-Dichlorobenzene	95-50-1	Not Found	0.00	ppbv
1,2,4-Trimethylbenzene	95-63-6	Not Found	0.00	ppbv
Cumene	98-82-8	Not Found	0.00	ppbv
1,2-Dichloroethane-d4	17060-07-0		94.00	% Recovery
Toluene-d8	2037-26-5		97.00	% Recovery
4-Bromofluorobenzene	460-00-4		102.00	% Recovery



www.airtoxics.com
1-800-985-5955

Media Certification Report

Canister Number: 6L#9573 w/10.2ml

Can#: 51073-9573

Date : 03/27/07 16:33

Data File: u032710.d

Name	CAS	Type	Conc.	Units
Ethyl Benzene	100-41-4	Not Found	0.00	ppbv
Styrene	100-42-5	Not Found	0.00	ppbv
alpha-Chlorotoluene	100-44-7	Not Found	0.00	ppbv
cis-1,3-Dichloropropene	10061-01-5	Not Found	0.00	ppbv
trans-1,3-Dichloropropene	10061-02-6	Not Found	0.00	ppbv
Propylbenzene	103-65-1	Not Found	0.00	ppbv
1,4-Dichlorobenzene	106-46-7	Not Found	0.00	ppbv
1,2-Dibromoethane (EDB)	106-93-4	Not Found	0.00	ppbv
1,3-Butadiene	106-99-0	Not Found	0.00	ppbv
3-Chloropropene	107-05-1	Not Found	0.00	ppbv
1,2-Dichloroethane	107-06-2	Not Found	0.00	ppbv
4-Methyl-2-pentanone	108-10-1	Not Found	0.00	ppbv
m,p-Xylene	108-38-3	Not Found	0.00	ppbv
1,3,5-Trimethylbenzene	108-67-8	Not Found	0.00	ppbv
Toluene	108-88-3	Not Found	0.00	ppbv
Chlorobenzene	108-90-7	Not Found	0.00	ppbv
Tetrahydrofuran	109-99-9	Not Found	0.00	ppbv
Hexane	110-54-3	Not Found	0.00	ppbv
Cyclohexane	110-82-7	Not Found	0.00	ppbv
1,2,4-Trichlorobenzene	120-82-1	Not Found	0.00	ppbv
1,4-Dioxane	123-91-1	Not Found	0.00	ppbv
Dibromochloromethane	124-48-1	Not Found	0.00	ppbv
Tetrachloroethene	127-18-4	Not Found	0.00	ppbv
Heptane	142-82-5	Not Found	0.00	ppbv
cis-1,2-Dichloroethene	156-59-2	Not Found	0.00	ppbv
trans-1,2-Dichloroethene	156-60-5	Not Found	0.00	ppbv
Methyl tert-butyl ether	1634-04-4	Not Found	0.00	ppbv
2,2,4-Trimethylpentane	540-84-1	Not Found	0.00	ppbv
1,3-Dichlorobenzene	541-73-1	Not Found	0.00	ppbv
Carbon Tetrachloride	56-23-5	Not Found	0.00	ppbv
2-Hexanone	591-78-6	Not Found	0.00	ppbv
4-Ethyltoluene	622-96-8	Not Found	0.00	ppbv
Ethanol	64-17-5	Not Found	0.00	ppbv
2-Propanol	67-63-0	Not Found	0.00	ppbv
Acetone	67-64-1	Not Found	0.00	ppbv
Chloroform	67-66-3	Not Found	0.00	ppbv
Benzene	71-43-2	Not Found	0.00	ppbv
1,1,1-Trichloroethane	71-55-6	Not Found	0.00	ppbv
Bromomethane	74-83-9	Not Found	0.00	ppbv
Chloromethane	74-87-3	Not Found	0.00	ppbv
Chloroethane	75-00-3	Not Found	0.00	ppbv
Vinyl Chloride	75-01-4	Not Found	0.00	ppbv
Methylene Chloride	75-09-2	Not Found	0.00	ppbv

Name	CAS	Type	Conc.	Units
Carbon Disulfide	75-15-0	Not Found	0.00	ppbv
Bromoform	75-25-2	Not Found	0.00	ppbv
Bromodichloromethane	75-27-4	Not Found	0.00	ppbv
1,1-Dichloroethane	75-34-3	Not Found	0.00	ppbv
1,1-Dichloroethene	75-35-4	Not Found	0.00	ppbv
Freon 11	75-69-4	Not Found	0.00	ppbv
Freon 12	75-71-8	Not Found	0.00	ppbv
Freon 113	76-13-1	Not Found	0.00	ppbv
Freon 114	76-14-2	Not Found	0.00	ppbv
1,2-Dichloropropane	78-87-5	Not Found	0.00	ppbv
2-Butanone (Methyl Ethyl	78-93-3	Not Found	0.00	ppbv
1,1,2-Trichloroethane	79-00-5	Not Found	0.00	ppbv
Trichloroethene	79-01-6	Not Found	0.00	ppbv
1,1,2,2-Tetrachloroethane	79-34-5	Not Found	0.00	ppbv
Hexachlorobutadiene	87-68-3	Not Found	0.00	ppbv
Naphthalene	91-20-3	Not Found	0.00	ppbv
o-Xylene	95-47-6	Not Found	0.00	ppbv
1,2-Dichlorobenzene	95-50-1	Not Found	0.00	ppbv
1,2,4-Trimethylbenzene	95-63-6	Not Found	0.00	ppbv
Cumene	98-82-8	Not Found	0.00	ppbv
1,2-Dichloroethane-d4	17060-07-0		95.00	% Recovery
Toluene-d8	2037-26-5		102.00	% Recovery
4-Bromofluorobenzene	460-00-4		104.00	% Recovery



www.airtoxics.com
1-800-985-5955

Media Certification Report

Canister Number: F032336; 6L#36033 w/11.5ml FC:1

Date: 3/24/2007 02:28:51

Peak #	Quantification	CAS	Type	Conc.	Units
	1,1,1,2-Tetrafluoroethane		Not Found	0.000	ppbv
	Propylene		Not Found	0.000	ppbv
	Freon 12		Not Found	0.000	ppbv
	Freon 114		Not Found	0.000	ppbv
	Chloromethane		Not Found	0.000	ppbv
	Butane		Not Found	0.000	ppbv
	Vinyl Chloride		Not Found	0.000	ppbv
	1,3-Butadiene		Not Found	0.000	ppbv
	Bromomethane		Not Found	0.000	ppbv
	Chloroethane		Not Found	0.000	ppbv
	Isopentane		Not Found	0.000	ppbv
	Vinyl bromide		Not Found	0.000	ppbv
	Freon 11		Not Found	0.000	ppbv
	Freon 113		Not Found	0.000	ppbv
	1,1-Dichloroethene		Not Found	0.000	ppbv
	3-Chloropropene		Not Found	0.000	ppbv
	Methyl Acetate		Not Found	0.000	ppbv
	trans-1,2-Dichloroethene		Not Found	0.000	ppbv
	Methyl tert-butyl ether		Not Found	0.000	ppbv
	Acrylonitrile		Not Found	0.000	ppbv
	Hexane		Not Found	0.000	ppbv
	Isopropyl ether		Not Found	0.000	ppbv
	1,1-Dichloroethane		Not Found	0.000	ppbv
	Vinyl Acetate		Not Found	0.000	ppbv
	Chloroprene		Not Found	0.000	ppbv
	Ethyl-tert-butyl ether		Not Found	0.000	ppbv
	2,2-Dichloropropane		Not Found	0.000	ppbv
	cis-1,2-Dichloroethene		Not Found	0.000	ppbv
	Chloroform		Not Found	0.000	ppbv
	Cyclohexane		Not Found	0.000	ppbv
	2,3-Dimethylpentane		Not Found	0.000	ppbv
	1,1,1-Trichloroethane		Not Found	0.000	ppbv
	Carbon Tetrachloride		Not Found	0.000	ppbv
	1,1-Dichloropropene		Not Found	0.000	ppbv
	2,2,4-Trimethylpentane		Not Found	0.000	ppbv
	tert-Amyl Methyl ether		Not Found	0.000	ppbv
	1,2-Dichloroethane		Not Found	0.000	ppbv
	Thiophene		Not Found	0.000	ppbv
	Trichloroethene		Not Found	0.000	ppbv
	Methylcyclohexane		Not Found	0.000	ppbv
	1,2-Dichloropropane		Not Found	0.000	ppbv
	Bromodichloromethane		Not Found	0.000	ppbv
	cis-1,3-Dichloropropene		Not Found	0.000	ppbv
	4-Methyl-2-pentanone		Not Found	0.000	ppbv
	trans-1,3-Dichloropropene		Not Found	0.000	ppbv
	1,1,2-Trichloroethane		Not Found	0.000	ppbv
	Tetrachloroethene		Not Found	0.000	ppbv
	2-Hexanone		Not Found	0.000	ppbv



www.airtoxics.com
1-800-985-5955

Media Certification Report

Canister Number: F032336; 6L#36033 w/11.5ml FC:1

Date: 3/24/2007 02:28:51

Peak #	Quantification	CAS	Type	Conc.	Units
	Dibromochloromethane		Not Found	0.000	ppbv
	1,2-Dibromoethane (EDB)		Not Found	0.000	ppbv
	Chlorobenzene		Not Found	0.000	ppbv
	Ethyl Benzene		Not Found	0.000	ppbv
	1,1,1,2-Tetrachloroethane		Not Found	0.000	ppbv
	m,p-Xylene		Not Found	0.000	ppbv
	o-Xylene		Not Found	0.000	ppbv
	Styrene		Not Found	0.000	ppbv
	Bromoform		Not Found	0.000	ppbv
	Cumene		Not Found	0.000	ppbv
	1,1,2,2-Tetrachloroethane		Not Found	0.000	ppbv
	Propylbenzene		Not Found	0.000	ppbv
	1,2,3-Trichloropropane		Not Found	0.000	ppbv
	4-Ethyltoluene		Not Found	0.000	ppbv
	tert-Butylbenzene		Not Found	0.000	ppbv
	1,2,4-Trimethylbenzene		Not Found	0.000	ppbv
	Pentachloroethane		Not Found	0.000	ppbv
	p-Cymene		Not Found	0.000	ppbv
	1,3-Dichlorobenzene		Not Found	0.000	ppbv
	1,4-Dichlorobenzene		Not Found	0.000	ppbv
	alpha-Chlorotoluene		Not Found	0.000	ppbv
	Indan		Not Found	0.000	ppbv
	Butylbenzene		Not Found	0.000	ppbv
	1,2-Dichlorobenzene		Not Found	0.000	ppbv
	Indene		Not Found	0.000	ppbv
	Hexachloroethane		Not Found	0.000	ppbv
	1,2-Dibromo-3-chloropropane		Not Found	0.000	ppbv
	1,2,4-Trichlorobenzene		Not Found	0.000	ppbv
	Hexachlorobutadiene		Not Found	0.000	ppbv
	Naphthalene		Not Found	0.000	ppbv
	1,2,3-Trichlorobenzene		Not Found	0.000	ppbv
2	1,1-Difluoroethane	0-00-0	Quantified	0.03009	ppbv
5	Ethanol	55255-50-0	Quantified	0.1349	ppbv
6	Acrolein	0-00-0	Quantified	0.000	ppbv
8	Carbon Disulfide	3294-96-0	Quantified	0.04207	ppbv
10	Acetone	67-64-1	Quantified	1.097	ppbv
11	2-Propanol	56053-19-1	Quantified	0.03068	ppbv
12	2-Methylpentane	55255-50-0	Quantified	0.01316	ppbv
14	Methylene Chloride	21133-52-8	Quantified	0.01777	ppbv
15	tert-Butyl alcohol	341500-94-5	Quantified	0.02449	ppbv
24	2-Butanone (Methyl Ethyl Ketone)	0-00-0	Quantified	0.1286	ppbv
24	Ethyl Acetate	0-00-0	Quantified	0.1270	ppbv
26	Bromochloromethane-IS	74-97-5	Quantified	0.000	ppbv
28	Tetrahydrofuran	109-99-9	Quantified	0.05680	ppbv
30	Benzene	71-43-2	Quantified	0.04021	ppbv
31	1,2-Dichloroethane-d4	121505-32-6	Quantified	5.051	ppbv
32	Heptane	341500-94-5	Quantified	0.01307	ppbv
33	1,4-Difluorobenzene-IS	540-36-3	Quantified	0.000	ppbv



www.airtoxics.com
1-800-985-5955

Media Certification Report

Canister Number: F032336; 6L#36033 w/11.5ml FC:1

Date: 3/24/2007 02:28:51

Peak #	Quantification	CAS	Type	Conc.	Units
39	1,4-Dioxane	55162-78-2	Quantified	0.01408	ppbv
40	Dibromomethane	149180-87-0	Quantified	0.000	ppbv
41	Toluene-D8	2037-26-5	Quantified	4.660	ppbv
42	Toluene	103438-94-4	Quantified	0.007217	ppbv
50	Chlorobenzene-d5-IS	3114-55-4	Quantified	0.000	ppbv
53	Bromofluorobenzene	460-00-4	Quantified	5.139	ppbv
54	1,3,5-Trimethylbenzene	0-00-0	Quantified	0.01568	ppbv
55	sec-Butylbenzene	0-00-0	Quantified	0.004587	ppbv

DATA REVIEW CHECKLIST Work Order #:

0704404

- Analysis/Reporting vs. Project Profile/SOP requirements checked (i.e. 100% Dups, J-Flag to MDL, etc)
- The final report has the correct reporting list, special units, and header info.
- Lab Narrative is correct (proper method & description/Receiving & Analytical notes correct)
- Corrective Action issued - # _____
- Unusual circumstances have been documented in the notes section below

LUMEN validation report present and initialed

CIRCLE (YES / NO)

- Lab Blank, CCV, LCS and DUP met QC criteria
- Hold time is met for all samples
- Appropriate data qualifier flags are applied
- Manual integrations for samples and QC are properly documented
- Samples analyzed within the project or method specific clock
- Retention times have been verified
- Appropriate ICAL(s) included
- At least one result per sample is verified against the target quant sheets/raw data

- Dilution factor correctly calculated (sample load volume, syringe and bag dilutions, can pressurization(s))
- Correct amount of sample analyzed (i.e. sample not over-diluted)
- Spectra verified - documentation of spectral defense included (Section 5A of eCVP pkg)
- TICs resemble reference spectra
- TICs between duplicate samples are consistent
- Checked samples for trends (i.e. Influent>Effluent, Landfill or Ambient etc)
- Special units for all samples in the final report are correctly calculated
- Manually entered results checked (i.e. special CCV compounds)
- TPH/NMOC (verify calculations and correct reference compound used)
- Chain of Custody scanned correctly
- Verify sample id's vs. chain of custody
- Samples pressurized w/ appropriate gas (N₂ or He) Tedlar Bag only
- Final pressure consistent with canister size (6L vs. 1L)
- Verify receipt pressures against logbook and Target
- Verify canister ID #'s
- Extra printed copies are provided per client profile
- Final invoice amount correct (adjusted for TAT, Penalties, Re-issue Charges etc.)
- Client LUMEN report reviewed for accuracy and completeness

Notes: (to include: noting samples with QA/QC problems, Blanks with positive hits, narratives, etc.)

A/R: TB has hits for Acetone 2 Butanone 1 out in CCV
Confirmation on MSD-7 7042626

M/Q:

A (Analytical Review/Date)

R/T (Reporting Review/Date)

M (Management Review/Date)

Q (QA Review/Date)

JR 4/26/07

R: [Signature] 5/11/07

[Signature] 5/11/07

T: _____

Not Applicable