



***Air
Toxics LTD.***
Laboratory Services Since 1989

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

COMPREHENSIVE VALIDATION PACKAGE

Modified TO-15

INVENTORY SHEET

Work Order #: 0706057

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	28
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	29	36
b. Surrogate Recover Summary Form (If Applicable)	37	37
c. Internal Standard Summary Form (If Applicable)	38	38
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	39	138
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	139	153
i. Second Source LCS(Summary + Raw Data)	154	167
j. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	168	168
l. GC/MS Tune (Results + Raw Data)	169	178
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	179	180
b. Chain-of-Custody Records	181	181
c. Sample Log-In Sheet	182	182
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	183	183
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	184	186
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	187	188
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	--	--
i. <u>Data Review Check Sheet</u>	189	189

Comments:

Completed by:

Judy Lee

Judy Lee / Document Control

6/20/07

(Signature)

(Print Name & Title)

(Date)




AN ENVIRONMENTAL ANALYTICAL LABORATORY

WORK ORDER #: 0706057

Work Order Summary

CLIENT:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Dr. Suite 201 Glastonbury, CT 06033	BILL TO:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Dr. Suite 201 Glastonbury, CT 06033
PHONE:	860-368-5300	P.O. #	NR
FAX:	860-368-5307	PROJECT #	061140-8-1703 Bay Barrier Wall Instalation
DATE RECEIVED:	06/04/2007	CONTACT:	Bryanna Langley
DATE COMPLETED:	06/14/2007		

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>
01A	AMS6-UW	Modified TO-15	6.0 "Hg
02A	AMS2-DW	Modified TO-15	6.0 "Hg
03A	Lab Blank	Modified TO-15	NA
04A	CCV	Modified TO-15	NA
05A	LCS	Modified TO-15	NA

CERTIFIED BY:  DATE: 06/15/07

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004
NY NELAP - 11291, UT NELAP - 9166389892

Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,
Accreditation number: E87680, Effective date: 07/01/06, Expiration date: 06/30/07

Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards

This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

**LABORATORY NARRATIVE
Modified TO-15
GEI Consultants, Inc.
Workorder# 0706057**

Two 6 Liter Summa Canister samples were received on June 04, 2007. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

Method modifications taken to run these samples are summarized in the below table. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	+/- 30% Difference	<= 30% Difference with two allowed out up to <=40%.; flag and narrate outliers
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

Receiving Notes

The Chain of Custody (COC) information for samples AMS6-UW and AMS2-DW did not match the entries on the sample tags with regard to sample identification. Therefore the information on the COC was used to process and report the samples.

Analytical Notes

All Quality Control Limit failures and affected sample results are noted by flags. Each flag is defined at the bottom of this Case Narrative and on each Sample Result Summary page. Target compound non-detects in the samples that are associated with high bias in QC analyses have not been flagged.

Definition of Data Qualifying Flags

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

- B - Compound present in laboratory blank greater than reporting limit (background subtraction no performed).
- J - Estimated value.
- E - Exceeds instrument calibration range.
- S - Saturated peak.
- Q - Exceeds quality control limits.
- U - Compound analyzed for but not detected above the reporting limit.
- UJ- Non-detected compound associated with low bias in the CCV
- N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

a-File was requantified

b-File was quantified by a second column and detector

r1-File was requantified for the purpose of reissue

Table 1

Client Sample ID	Lab Sample ID	Date Collected	Date Received	Date Extracted	Sample	Sample Extract		Sample Condition
					Holding Time (Days)	Date Analyzed	Holding Time (Days)	
AMS6-UW	0706057-01A	5/30/2007	6/ 4/2007	NA	8	6/ 7/2007	NA	Good
AMS2-DW	0706057-02A	5/30/2007	6/ 4/2007	NA	8	6/ 7/2007	NA	Good
Lab Blank	0706057-03A	NA	NA	NA	NA	6/ 7/2007	NA	Good
CCV	0706057-04A	NA	NA	NA	NA	6/ 7/2007	NA	Good
LCS	0706057-05A	NA	NA	NA	NA	6/ 7/2007	NA	Good

Sample Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: AMS6-UW

Lab ID#: 0706057-01A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.84	0.87	4.2	4.3
Toluene	0.84	1.4	3.2	5.4
Acetone	3.4	3.8	8.0	9.0



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS6-UW

Lab ID#: 0706057-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060713	Date of Collection:	5/30/07
Dil. Factor:	1.68	Date of Analysis:	6/7/07 05:42 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.84	0.87	4.2	4.3
Freon 114	0.84	Not Detected	5.9	Not Detected
Vinyl Chloride	0.84	Not Detected	2.1	Not Detected
Bromomethane	0.84	Not Detected	3.3	Not Detected
Chloroethane	0.84	Not Detected	2.2	Not Detected
Freon 11	0.84	Not Detected	4.7	Not Detected
1,1-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Freon 113	0.84	Not Detected	6.4	Not Detected
Methylene Chloride	0.84	Not Detected	2.9	Not Detected
1,1-Dichloroethane	0.84	Not Detected	3.4	Not Detected
cis-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Chloroform	0.84	Not Detected	4.1	Not Detected
1,1,1-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Carbon Tetrachloride	0.84	Not Detected	5.3	Not Detected
Benzene	0.84	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.84	Not Detected	3.4	Not Detected
Trichloroethene	0.84	Not Detected	4.5	Not Detected
1,2-Dichloropropane	0.84	Not Detected	3.9	Not Detected
cis-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
Toluene	0.84	1.4	3.2	5.4
trans-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
1,1,2-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Tetrachloroethene	0.84	Not Detected	5.7	Not Detected
1,2-Dibromoethane (EDB)	0.84	Not Detected	6.4	Not Detected
Chlorobenzene	0.84	Not Detected	3.9	Not Detected
Ethyl Benzene	0.84	Not Detected	3.6	Not Detected
m,p-Xylene	0.84	Not Detected	3.6	Not Detected
o-Xylene	0.84	Not Detected	3.6	Not Detected
Styrene	0.84	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.84	Not Detected	5.8	Not Detected
1,3,5-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,2,4-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,3-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,4-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
alpha-Chlorotoluene	0.84	Not Detected	4.3	Not Detected
1,2-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,3-Butadiene	0.84	Not Detected	1.8	Not Detected
Hexane	0.84	Not Detected	3.0	Not Detected
Cyclohexane	0.84	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS6-UW

Lab ID#: 0706057-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060713	Date of Collection:	5/30/07
Dil. Factor:	1.68	Date of Analysis:	6/7/07 05:42 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.84	Not Detected	3.4	Not Detected
Bromodichloromethane	0.84	Not Detected	5.6	Not Detected
Dibromochloromethane	0.84	Not Detected	7.2	Not Detected
Cumene	0.84	Not Detected	4.1	Not Detected
Propylbenzene	0.84	Not Detected	4.1	Not Detected
Chloromethane	3.4	Not Detected	6.9	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	3.8	8.0	9.0
Carbon Disulfide	0.84	Not Detected	2.6	Not Detected
2-Propanol	3.4	Not Detected	8.2	Not Detected
trans-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.84	Not Detected	2.5	Not Detected
Tetrahydrofuran	0.84	Not Detected	2.5	Not Detected
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.84	Not Detected	3.4	Not Detected
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.84	Not Detected	8.7	Not Detected
4-Ethyltoluene	0.84	Not Detected	4.1	Not Detected
Ethanol	3.4	Not Detected	6.3	Not Detected
Methyl tert-butyl ether	0.84	Not Detected U J	3.0	Not Detected U J
3-Chloropropene	3.4	Not Detected	10	Not Detected
2,2,4-Trimethylpentane	0.84	Not Detected	3.9	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	99	70-130
1,2-Dichloroethane-d4	103	70-130
4-Bromofluorobenzene	98	70-130

Report Date: 14-Jun-2007 15:58

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-07jun.b/5060713.d
 Lab Smp Id: 0706057-01A
 Inj Date : 07-JUN-2007 17:42
 Operator : jdg Inst ID: msd5.i
 Smp Info : 200ml #11006
 Misc Info : 6.0"Hg-5psi
 Comment :
 Method : /chem/msd5.i/5-07jun.b/t14q529a.m
 Meth Date : 07-Jun-2007 21:01 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1
 Dil Factor: 1.68000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 57 Bromochloromethane CAS #: 74-97-5									
8.187	8.214	(1.000)	130	229001	25.0000		80.00- 120.00	100.00	
8.187	8.214	(1.000)	128	175455			48.55- 108.55	76.62	
8.187	8.187	(1.000)	49	599128			229.31- 289.31	261.63	

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	883551	25.0000		80.00- 120.00	100.00	
10.067	10.067	(1.000)	88	170629			0.00- 49.97	19.31	

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	693581	25.0000		80.00- 120.00	100.00	
15.099	15.099	(1.000)	82	456045			33.54- 93.54	65.75	

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.132)	65	473118	25.7725	25.772	80.00- 120.00	100.00	
9.265	9.265	(1.132)	67	216130			25.98- 85.98	45.68	

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	797658	24.8026	24.803	80.00- 120.00	100.00	
12.832	12.832	(1.275)	70	94566			0.00- 41.05	11.86	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 97 Toluene-d8 (continued)

12.832	12.832	(1.275)	100	480524			36.04- 96.04	60.24
--------	--------	---------	-----	--------	--	--	--------------	-------

\$ 122 Bromofluorobenzene

CAS #: 460-00-4

16.675	16.675	(1.104)	174	426754	24.4892	24.489	80.00- 120.00	100.00
16.675	16.675	(1.104)	95	754480			136.90- 196.90	176.79
16.675	16.675	(1.104)	176	432692			64.74- 124.74	101.39

2 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.408	2.436	(0.294)	85	21078	0.51880	0.8716	80.00- 120.00	100.00
2.380	2.436	(0.291)	87	7878			1.62- 61.62	37.38

22 Acetone

CAS #: 67-64-1

4.841	4.841	(0.591)	58	33108	2.26991	3.813	80.00- 120.00	100.00
4.869	4.841	(0.595)	43	116921			327.94- 387.94	353.14

99 Toluene

CAS #: 108-88-3

12.942	12.942	(1.286)	91	32378	0.84984	1.428	80.00- 120.00	100.00
12.942	12.942	(1.286)	92	15315			29.80- 89.80	47.30

Report Date: 14-Jun-2007 15:58

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i
 Lab File ID: 5060713.d
 Lab Smp Id: 0706057-01A
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: jdg
 Method File: /chem/msd5.i/5-07jun.b/t14q529a.m
 Misc Info: 6.0"Hg-5psi

Calibration Date: 07-JUN-2007
 Calibration Time: 13:20
 Level: LOW
 Sample Type: AIR

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	292964	175778	410150	229001	-21.83
79 1,4-Difluorobenze	1106143	663686	1548600	883551	-20.12
108 Chlorobenzene-d5	855448	513269	1197627	693581	-18.92

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.21	7.88	8.54	8.19	-0.34
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-07jun
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0706057-01A
Level: LOW Operator: jdg
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 1502+Na.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /chem/msd5.i/5-07jun.b/t14q529a.m
Misc Info: 6.0"Hg-5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 71 1,2-Dichloroethane	25.000	25.772	103.09	70-130
\$ 97 Toluene-d8	25.000	24.803	99.21	70-130
\$ 122 Bromofluorobenzene	25.000	24.489	97.96	70-130

Data File: /chem/msd5.1/5-07jun.b/5060713.d

Date: 07-JUN-2007 17:42

Client ID:

Sample Info: 200ml #11006


Column phase: RTX-624

Instrument: msd5.1

Operator: jdg

Column diameter: 0.53

/chem/msd5.1/5-07jun.b/5060713.d

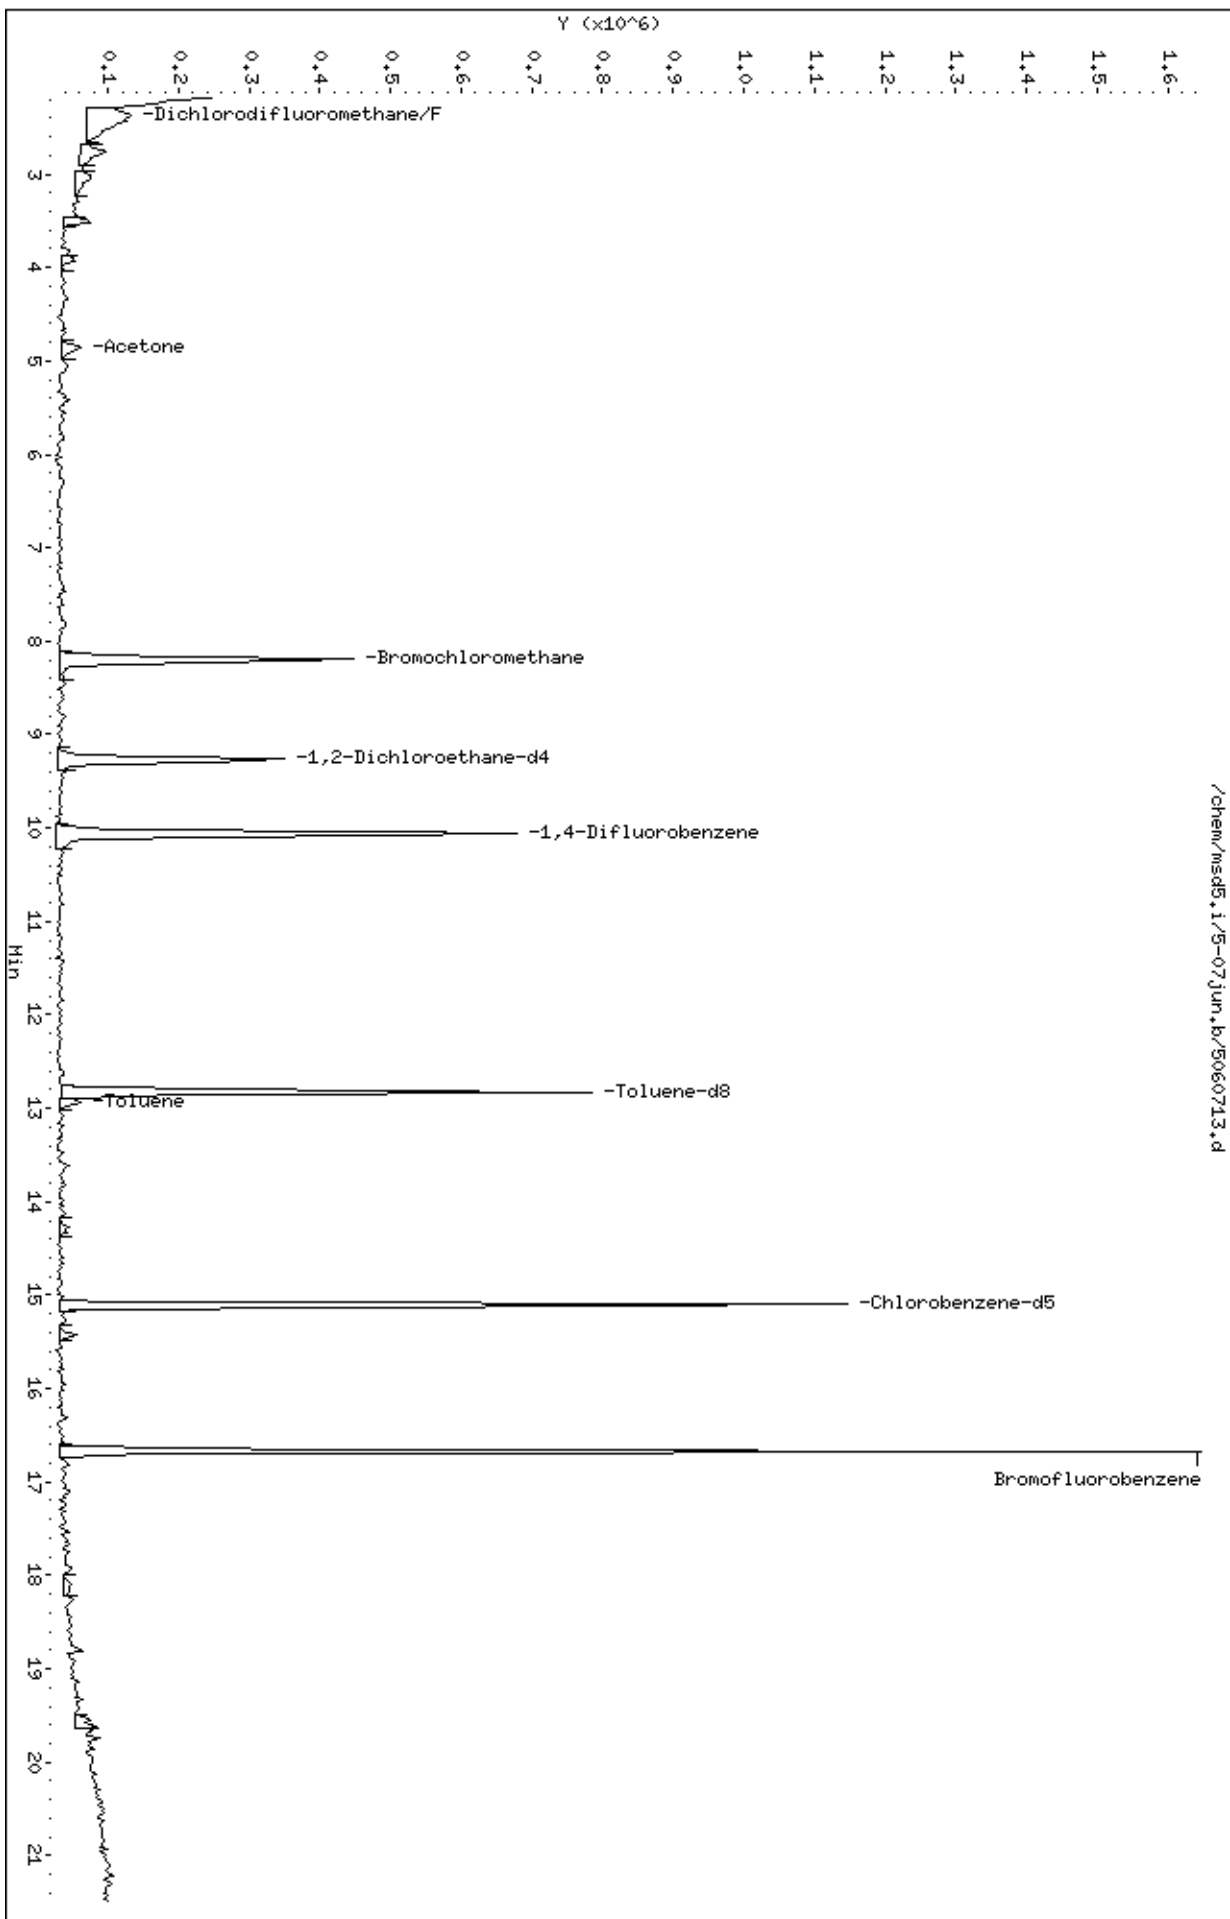

Date : 07-JUN-2007 17:42

Client ID:

Instrument: msd5.i

Sample Info: 200ml #11006







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

2 Dichlorodifluoromethane/Fr12

Concentration: 0.8716 PPBV

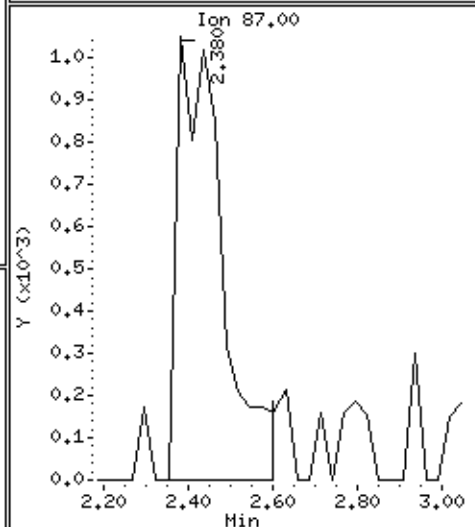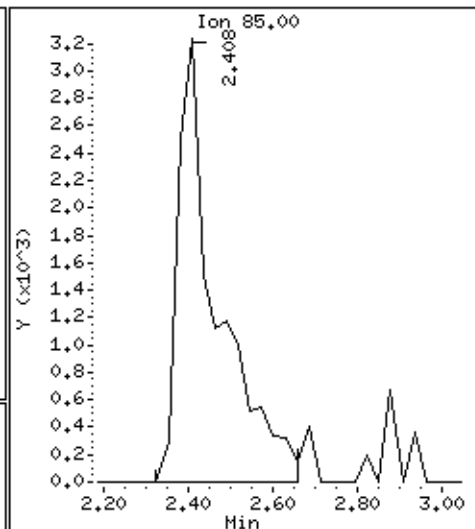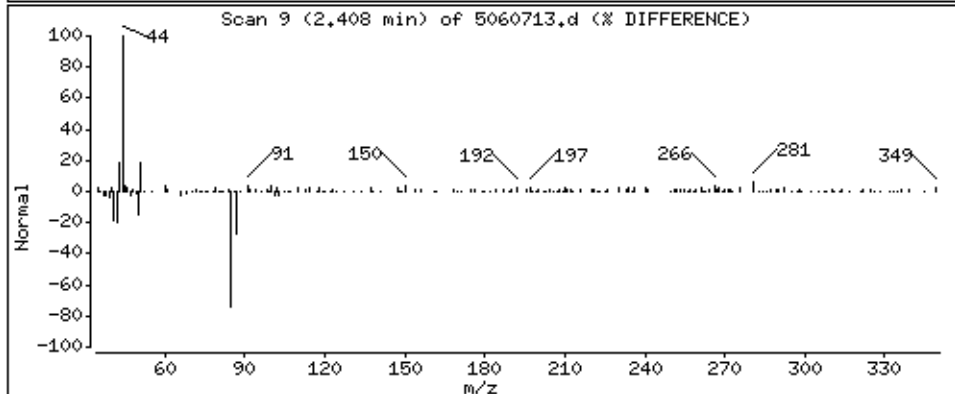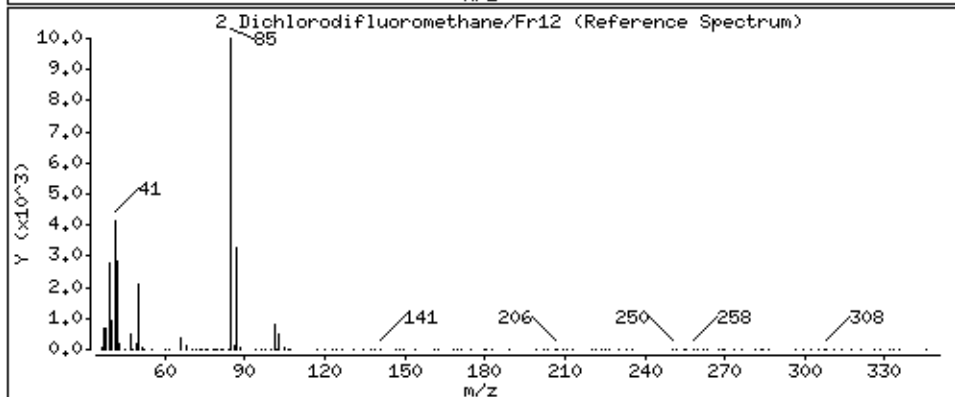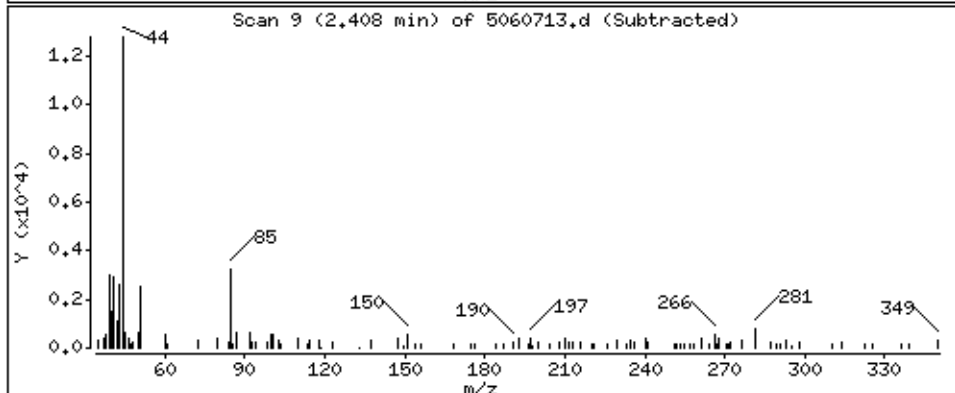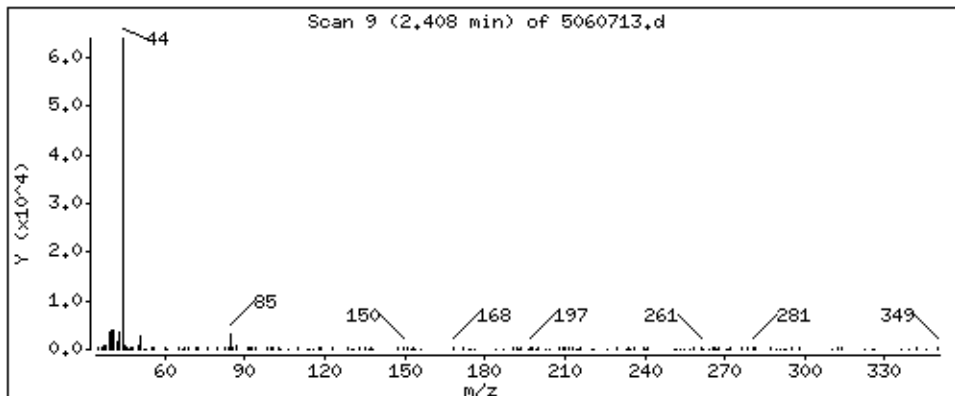

Date : 07-JUN-2007 17:42

Client ID:

Instrument: msd5.i

Sample Info: 200ml #11006







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

22 Acetone

Concentration: 3.813 PPBV

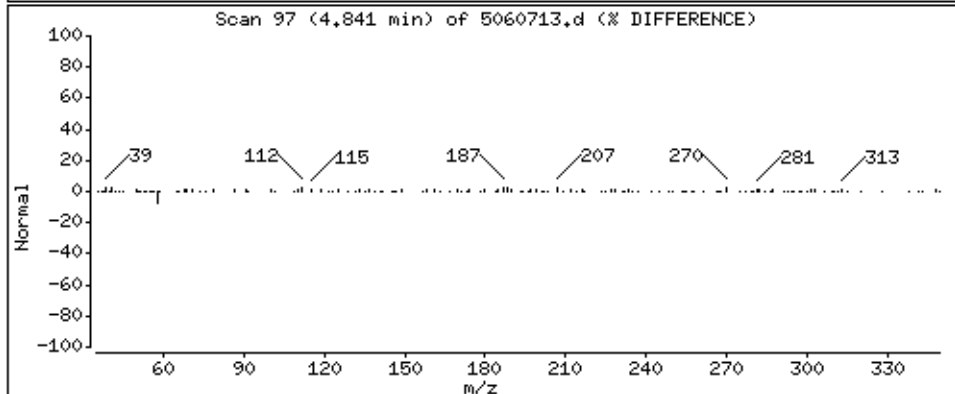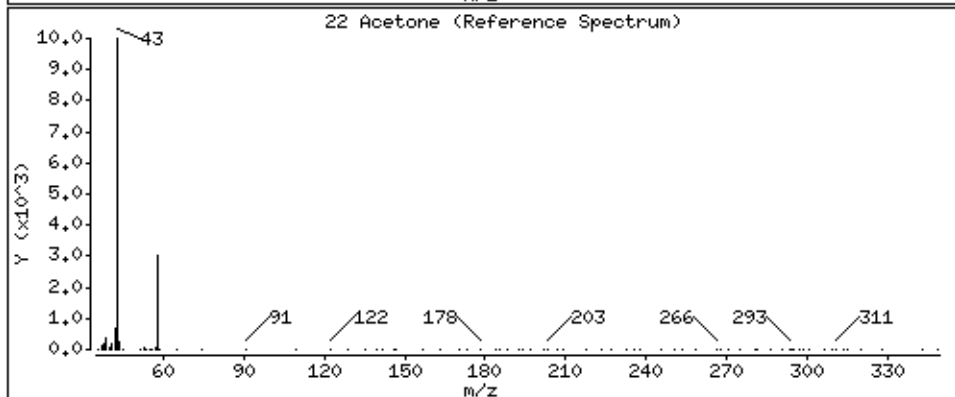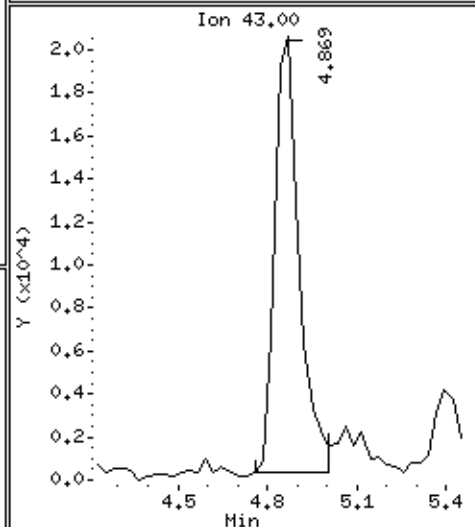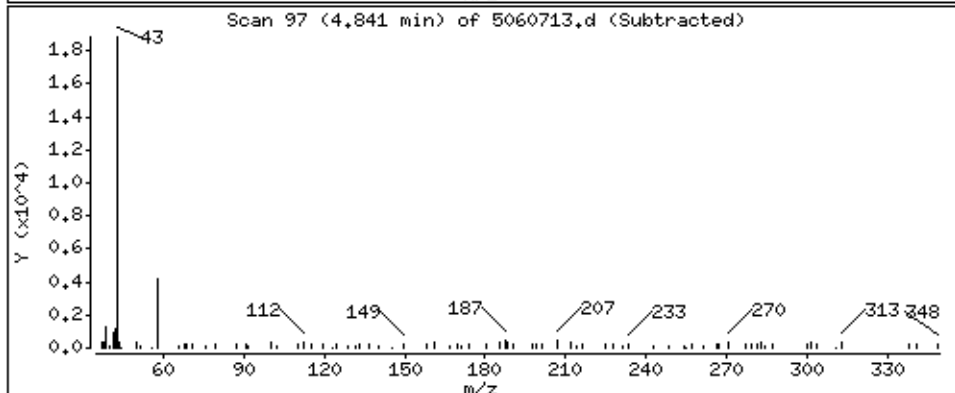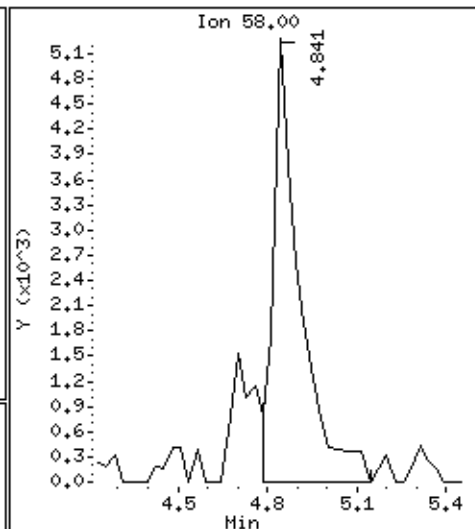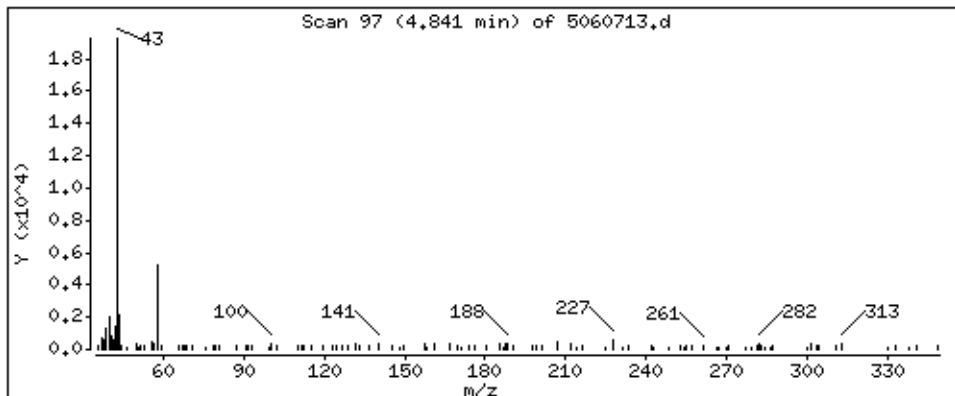

Date : 07-JUN-2007 17:42

Client ID:

Instrument: msd5,i

Sample Info: 200ml #11006







Operator: jdg

Column phase: RTx-624

Column diameter: 0.53

99 Toluene

Concentration: 1,428 PPBV

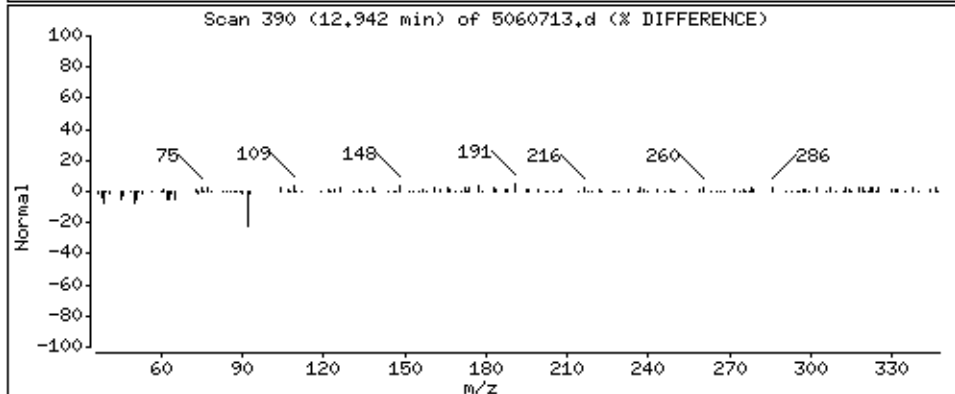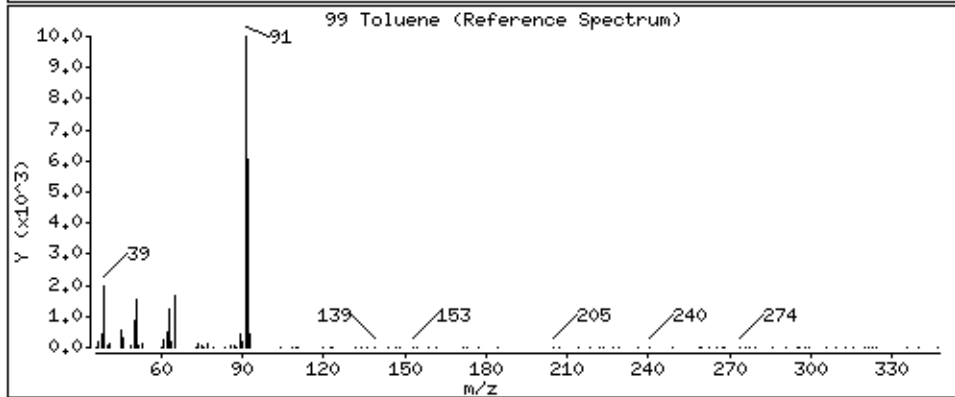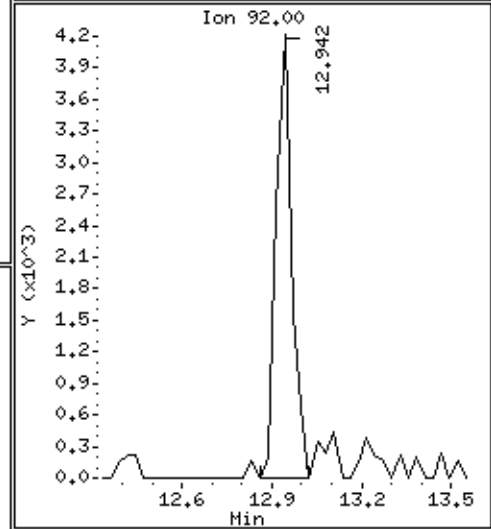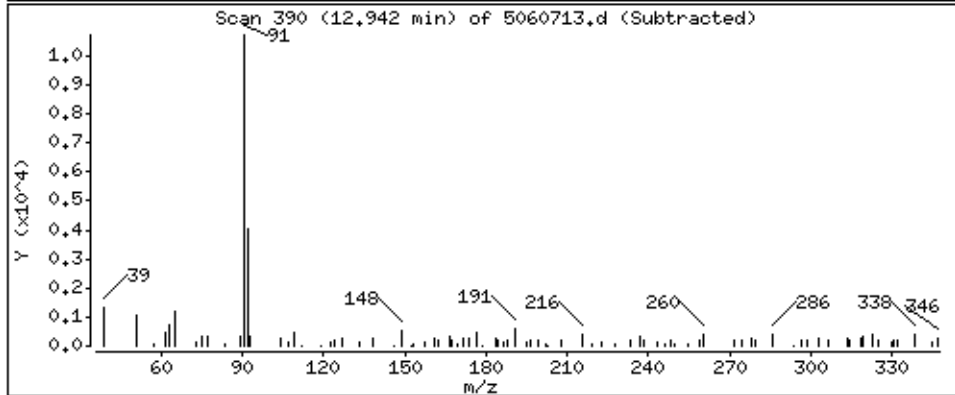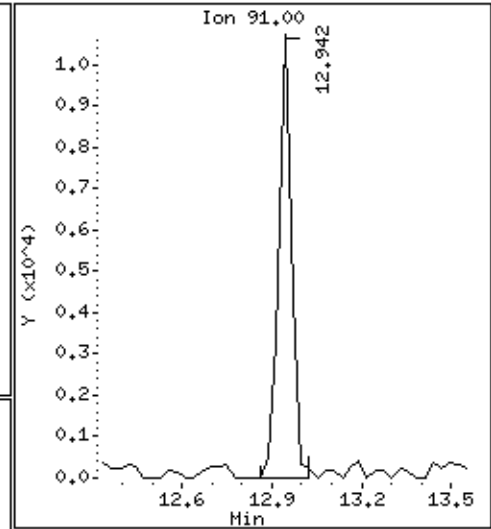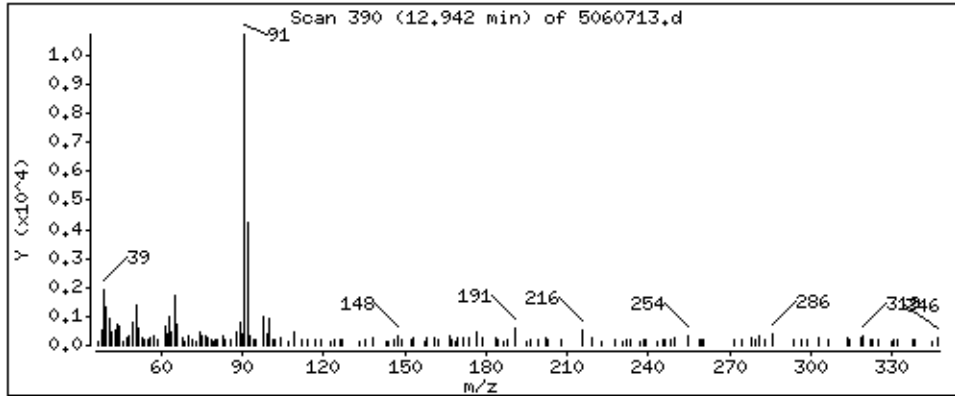



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: AMS2-DW

Lab ID#: 0706057-02A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Toluene	0.84	1.7	3.2	6.3
m,p-Xylene	0.84	0.86	3.6	3.7
Acetone	3.4	6.8	8.0	16
2-Butanone (Methyl Ethyl Ketone)	0.84	1.1	2.5	3.3



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS2-DW

Lab ID#: 0706057-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060714	Date of Collection:	5/30/07
Dil. Factor:	1.68	Date of Analysis:	6/7/07 06:14 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.84	Not Detected	4.2	Not Detected
Freon 114	0.84	Not Detected	5.9	Not Detected
Vinyl Chloride	0.84	Not Detected	2.1	Not Detected
Bromomethane	0.84	Not Detected	3.3	Not Detected
Chloroethane	0.84	Not Detected	2.2	Not Detected
Freon 11	0.84	Not Detected	4.7	Not Detected
1,1-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Freon 113	0.84	Not Detected	6.4	Not Detected
Methylene Chloride	0.84	Not Detected	2.9	Not Detected
1,1-Dichloroethane	0.84	Not Detected	3.4	Not Detected
cis-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
Chloroform	0.84	Not Detected	4.1	Not Detected
1,1,1-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Carbon Tetrachloride	0.84	Not Detected	5.3	Not Detected
Benzene	0.84	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.84	Not Detected	3.4	Not Detected
Trichloroethene	0.84	Not Detected	4.5	Not Detected
1,2-Dichloropropane	0.84	Not Detected	3.9	Not Detected
cis-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
Toluene	0.84	1.7	3.2	6.3
trans-1,3-Dichloropropene	0.84	Not Detected	3.8	Not Detected
1,1,2-Trichloroethane	0.84	Not Detected	4.6	Not Detected
Tetrachloroethene	0.84	Not Detected	5.7	Not Detected
1,2-Dibromoethane (EDB)	0.84	Not Detected	6.4	Not Detected
Chlorobenzene	0.84	Not Detected	3.9	Not Detected
Ethyl Benzene	0.84	Not Detected	3.6	Not Detected
m,p-Xylene	0.84	0.86	3.6	3.7
o-Xylene	0.84	Not Detected	3.6	Not Detected
Styrene	0.84	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.84	Not Detected	5.8	Not Detected
1,3,5-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,2,4-Trimethylbenzene	0.84	Not Detected	4.1	Not Detected
1,3-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,4-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
alpha-Chlorotoluene	0.84	Not Detected	4.3	Not Detected
1,2-Dichlorobenzene	0.84	Not Detected	5.0	Not Detected
1,3-Butadiene	0.84	Not Detected	1.8	Not Detected
Hexane	0.84	Not Detected	3.0	Not Detected
Cyclohexane	0.84	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS2-DW

Lab ID#: 0706057-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060714	Date of Collection:	5/30/07
Dil. Factor:	1.68	Date of Analysis:	6/7/07 06:14 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.84	Not Detected	3.4	Not Detected
Bromodichloromethane	0.84	Not Detected	5.6	Not Detected
Dibromochloromethane	0.84	Not Detected	7.2	Not Detected
Cumene	0.84	Not Detected	4.1	Not Detected
Propylbenzene	0.84	Not Detected	4.1	Not Detected
Chloromethane	3.4	Not Detected	6.9	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	6.8	8.0	16
Carbon Disulfide	0.84	Not Detected	2.6	Not Detected
2-Propanol	3.4	Not Detected	8.2	Not Detected
trans-1,2-Dichloroethene	0.84	Not Detected	3.3	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.84	1.1	2.5	3.3
Tetrahydrofuran	0.84	Not Detected	2.5	Not Detected
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.84	Not Detected	3.4	Not Detected
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.84	Not Detected	8.7	Not Detected
4-Ethyltoluene	0.84	Not Detected	4.1	Not Detected
Ethanol	3.4	Not Detected	6.3	Not Detected
Methyl tert-butyl ether	0.84	Not Detected U J	3.0	Not Detected U J
3-Chloropropene	3.4	Not Detected	10	Not Detected
2,2,4-Trimethylpentane	0.84	Not Detected	3.9	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	100	70-130
1,2-Dichloroethane-d4	101	70-130
4-Bromofluorobenzene	102	70-130

Report Date: 14-Jun-2007 15:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-07jun.b/5060714.d
 Lab Smp Id: 0706057-02A
 Inj Date : 07-JUN-2007 18:14
 Operator : jdg Inst ID: msd5.i
 Smp Info : 200ml #TO-1560
 Misc Info : 6.0"Hg-5psi
 Comment :
 Method : /chem/msd5.i/5-07jun.b/t14q529a.m
 Meth Date : 07-Jun-2007 21:01 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1
 Dil Factor: 1.68000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 57 Bromochloromethane CAS #: 74-97-5									
8.187	8.214 (1.000)	130	216194	25.0000		80.00-	120.00	100.00	
8.214	8.214 (1.000)	128	167335			48.55-	108.55	77.40	
8.187	8.187 (1.000)	49	569175			229.31-	289.31	263.27	

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067 (1.000)	114	838821	25.0000		80.00-	120.00	100.00	
10.067	10.067 (1.000)	88	159969			0.00-	49.97	19.07	

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099 (1.000)	117	657289	25.0000		80.00-	120.00	100.00	
15.099	15.099 (1.000)	82	458818			33.54-	93.54	69.80	

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265 (1.132)	65	437033	25.2171	25.217	80.00-	120.00	100.00	
9.265	9.265 (1.132)	67	189232			25.98-	85.98	43.30	

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832 (1.275)	98	760026	24.8927	24.893	80.00-	120.00	100.00	
12.832	12.832 (1.275)	70	94378			0.00-	41.05	12.42	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT (REL RT)	MASS	RESPONSE (PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====

\$ 97 Toluene-d8 (continued)

12.832	12.832 (1.275)	100	484149		36.04- 96.04	63.70
--------	----------------	-----	--------	--	--------------	-------

\$ 122 Bromofluorobenzene

CAS #: 460-00-4

16.675	16.675 (1.104)	174	420554	25.4659	25.466 80.00- 120.00	100.00
16.675	16.675 (1.104)	95	684652		136.90- 196.90	162.80
16.675	16.675 (1.104)	176	417240		64.74- 124.74	99.21

22 Acetone

CAS #: 67-64-1

4.841	4.841 (0.591)	58	55526	4.03242	6.774 80.00- 120.00	100.00
4.841	4.841 (0.591)	43	226965		327.94- 387.94	408.75

53 2-Butanone

CAS #: 78-93-3

7.827	7.800 (0.956)	72	4701	0.66096	1.110 80.00- 120.00	100.00
7.800	7.800 (0.953)	43	44625		710.69- 770.69	949.15
7.827	7.800 (0.956)	57	3913		23.20- 83.20	83.24

99 Toluene

CAS #: 108-88-3

12.942	12.942 (1.286)	91	35855	0.99129	1.665 80.00- 120.00	100.00
12.942	12.942 (1.286)	92	16711		29.80- 89.80	46.61

113 m,p-Xylene

CAS #: 108-38-3

15.431	15.431 (1.022)	106	9867	0.51233	0.8607 80.00- 120.00	100.00
15.431	15.431 (1.022)	91	16372		202.98- 262.98	165.92

Report Date: 14-Jun-2007 15:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i
 Lab File ID: 5060714.d
 Lab Smp Id: 0706057-02A
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: jdg
 Method File: /chem/msd5.i/5-07jun.b/t14q529a.m
 Misc Info: 6.0"Hg-5psi

Calibration Date: 07-JUN-2007
 Calibration Time: 13:20
 Level: LOW
 Sample Type: AIR

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	292964	175778	410150	216194	-26.20
79 1,4-Difluorobenze	1106143	663686	1548600	838821	-24.17
108 Chlorobenzene-d5	855448	513269	1197627	657289	-23.16

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.21	7.88	8.54	8.19	-0.34
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-07jun
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0706057-02A
Level: LOW Operator: jdg
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 1502+Na.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /chem/msd5.i/5-07jun.b/t14q529a.m
Misc Info: 6.0"Hg-5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 71 1,2-Dichloroethane	25.000	25.217	100.87	70-130
\$ 97 Toluene-d8	25.000	24.893	99.57	70-130
\$ 122 Bromofluorobenzene	25.000	25.466	101.86	70-130

Data File: /chem/msd5.1/5-07jun.b/5060714.d

Date: 07-JUN-2007 18:14

Client ID:

Sample Info: 200ml #T0-1560


Column phase: RTX-624

Instrument: msd5.1

Operator: jdg

Column diameter: 0.53

/chem/msd5.1/5-07jun.b/5060714.d

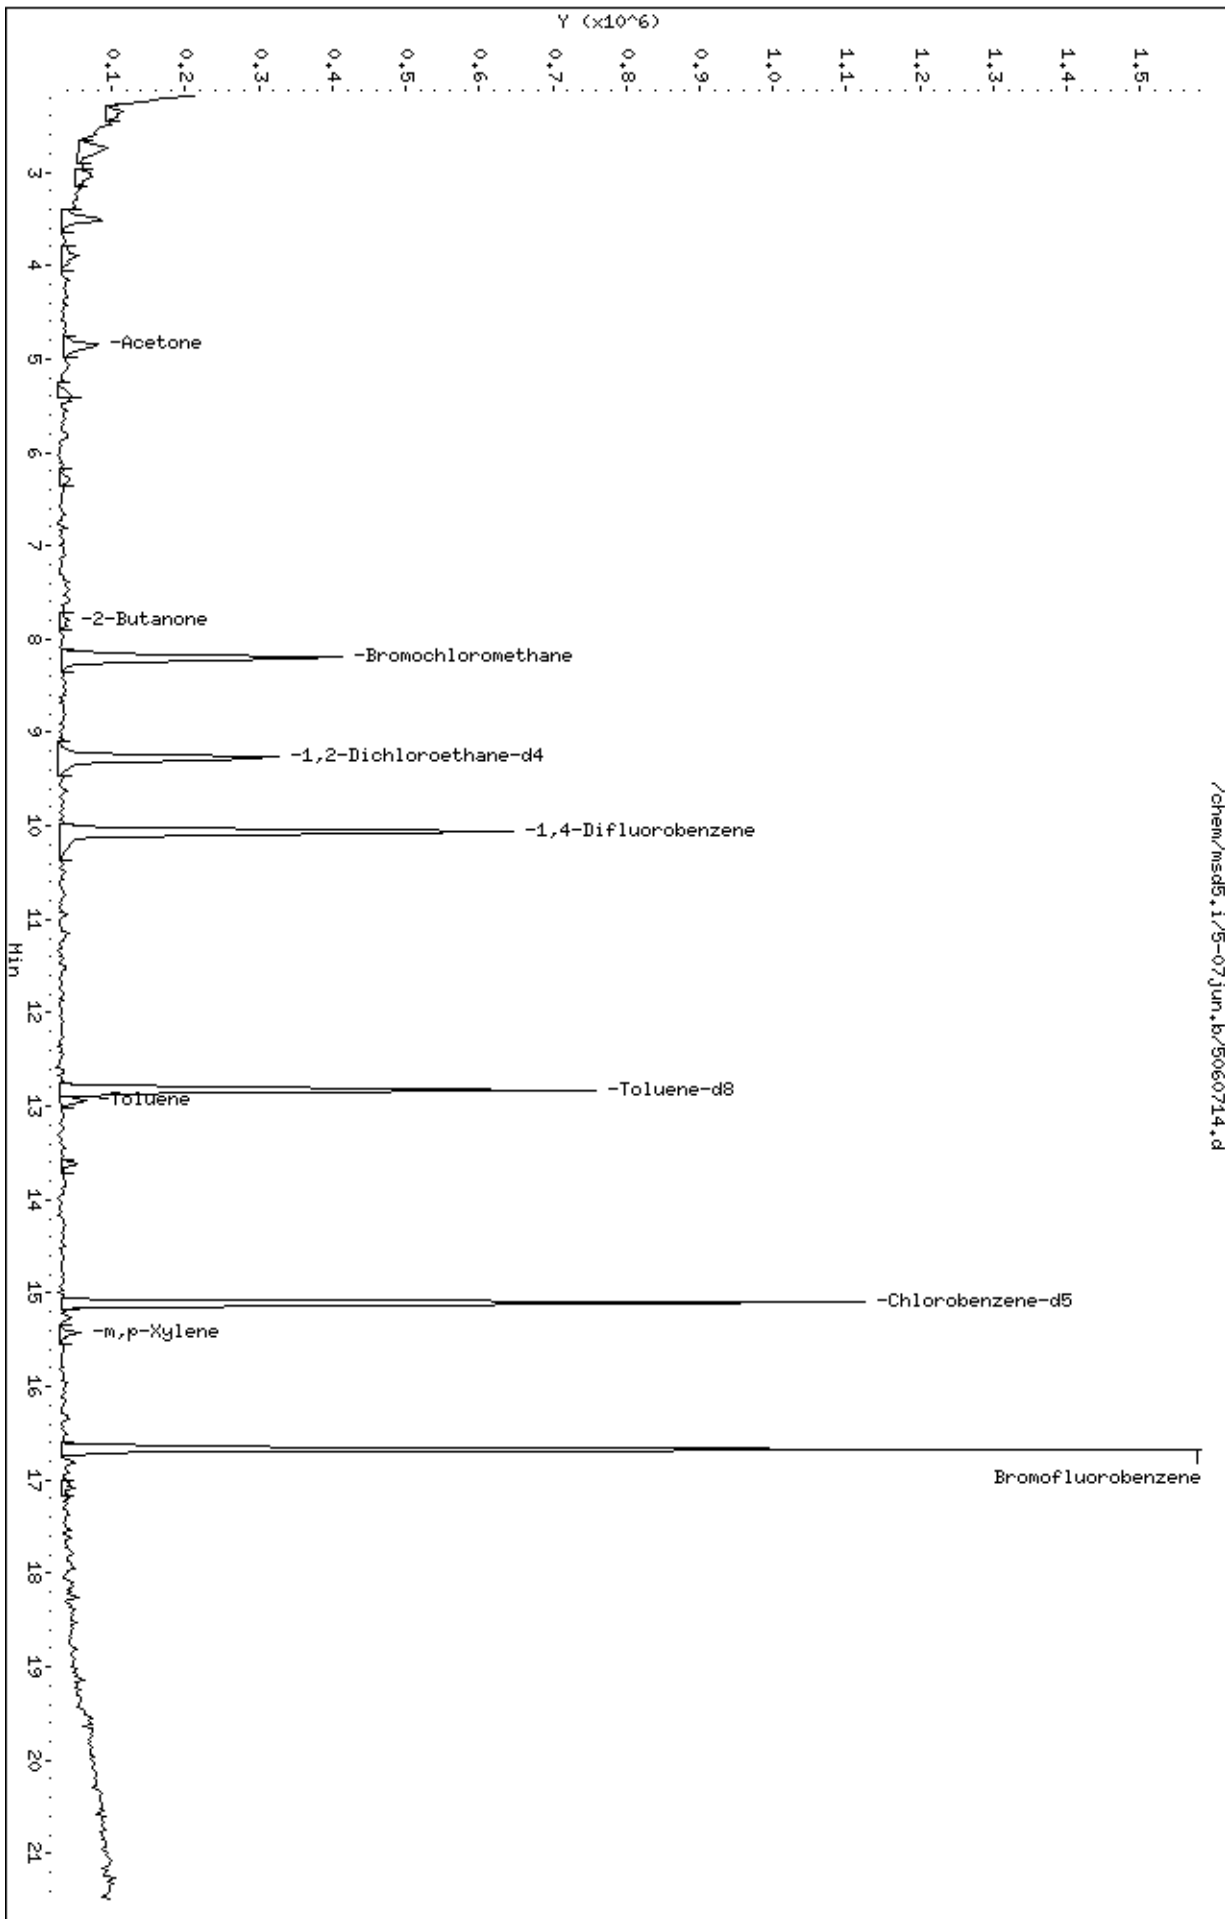

Date : 07-JUN-2007 18:14

Client ID:

Instrument: msd5.i

Sample Info: 200ml #TO-1560







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

22 Acetone

Concentration: 6.774 PPBV

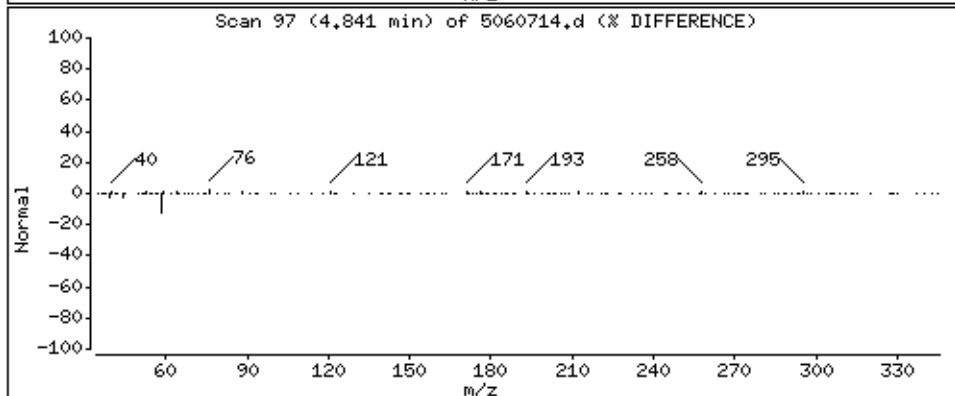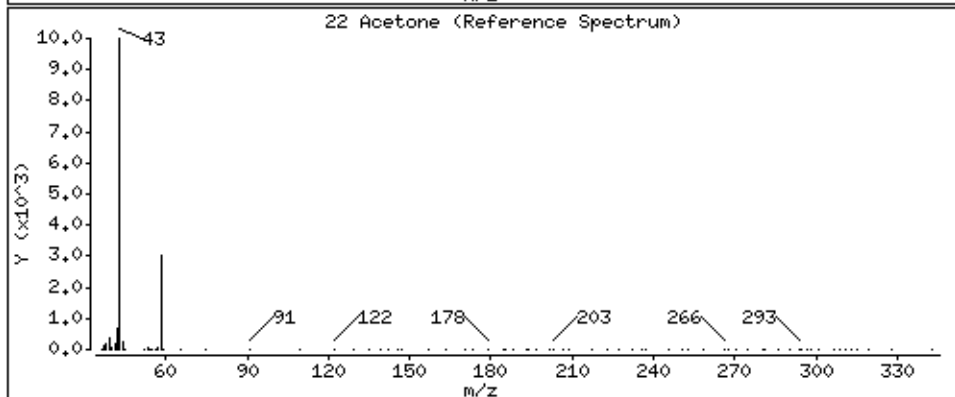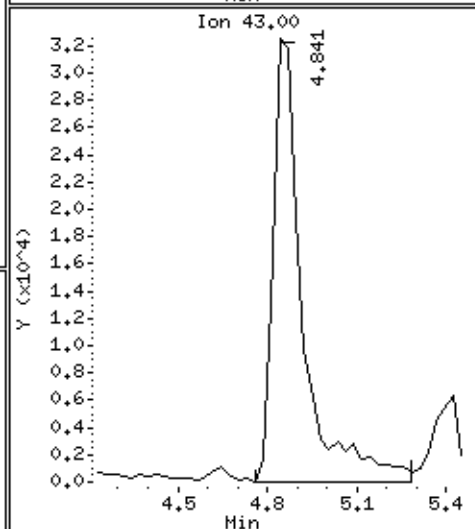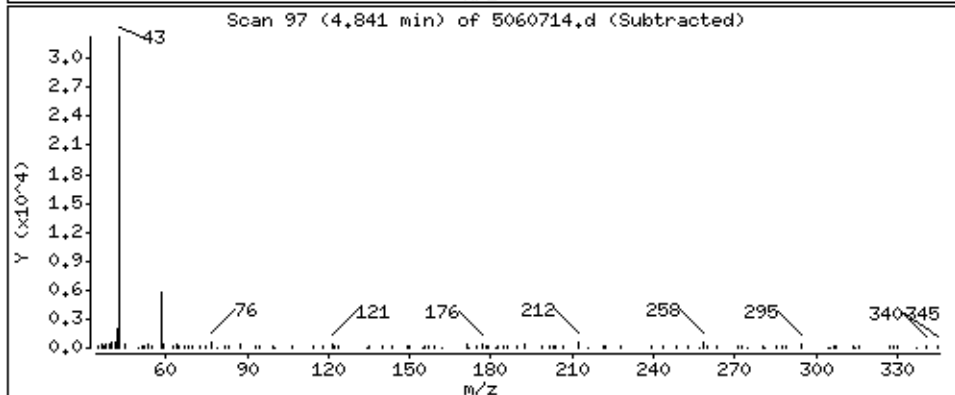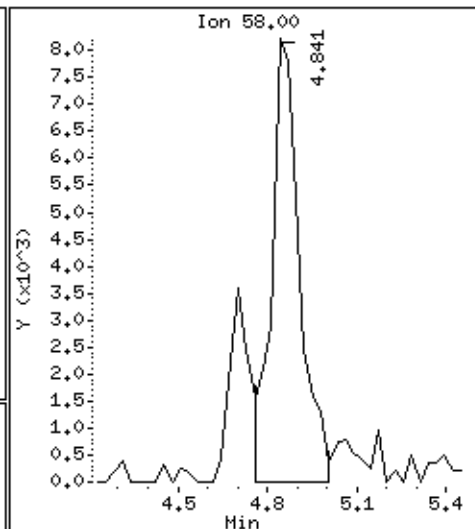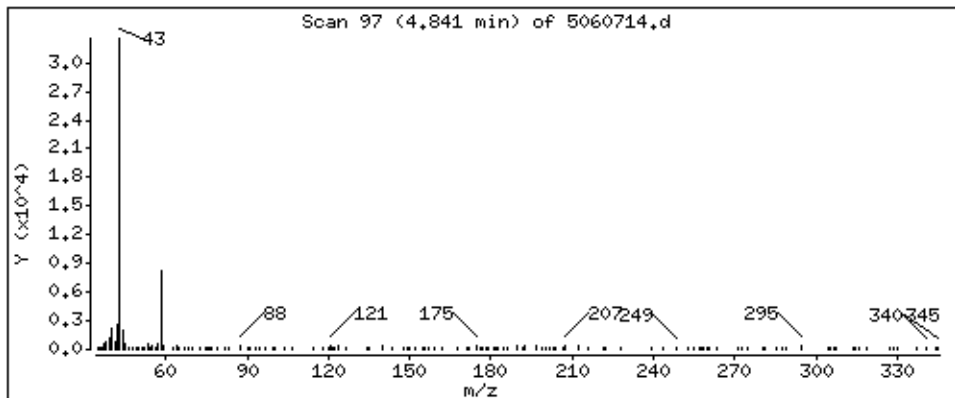

Date : 07-JUN-2007 18:14

Client ID:

Instrument: msd5.i

Sample Info: 200ml #T0-1560








Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

53 2-Butanone

Concentration: 1,110 PPBV

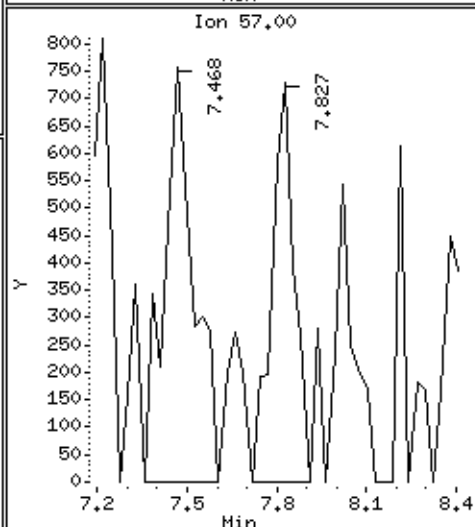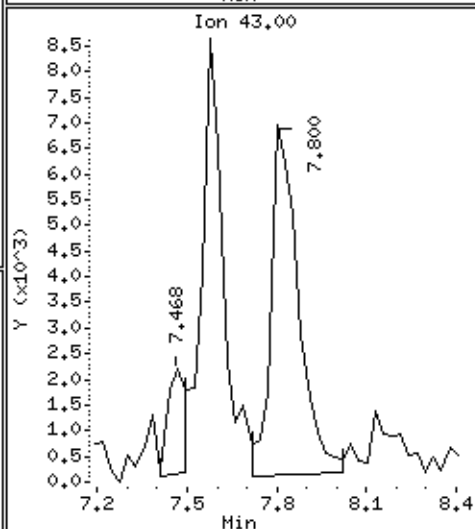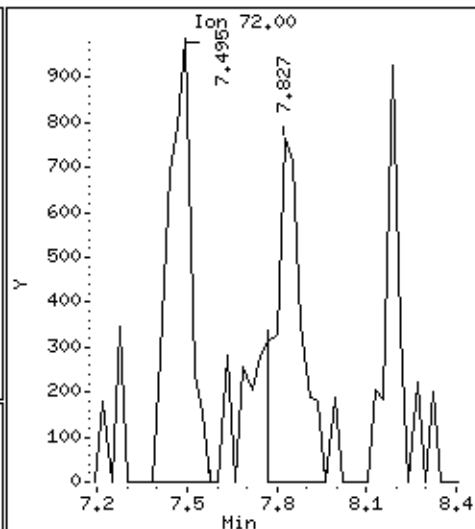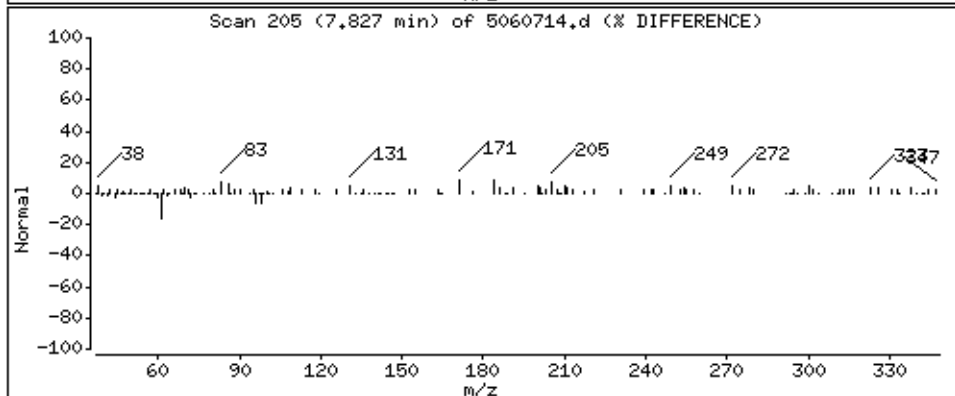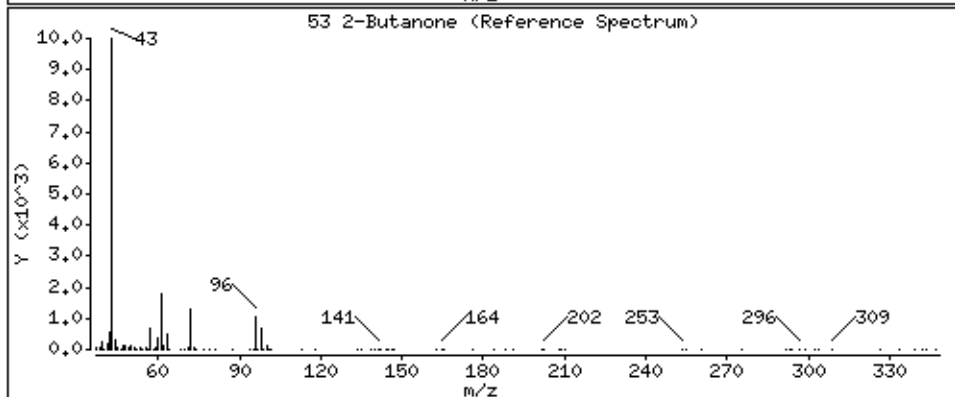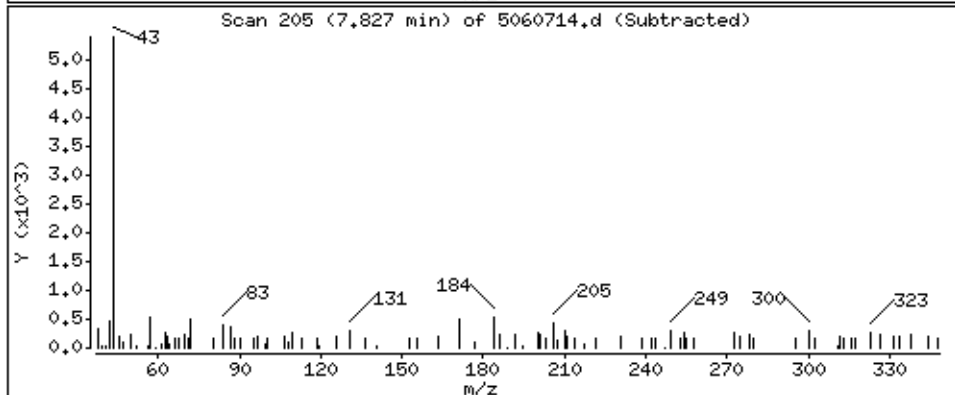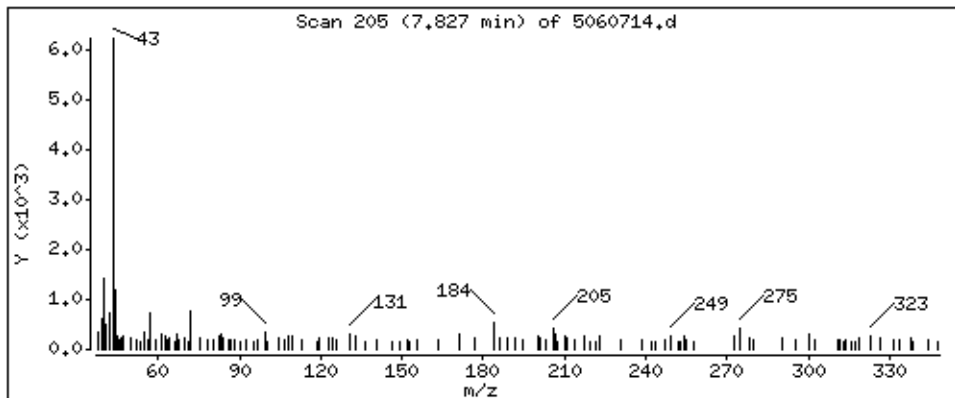

Date : 07-JUN-2007 18:14

Client ID:

Instrument: msd5.i

Sample Info: 200ml #T0-1560







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

99 Toluene

Concentration: 1,665 PPBV

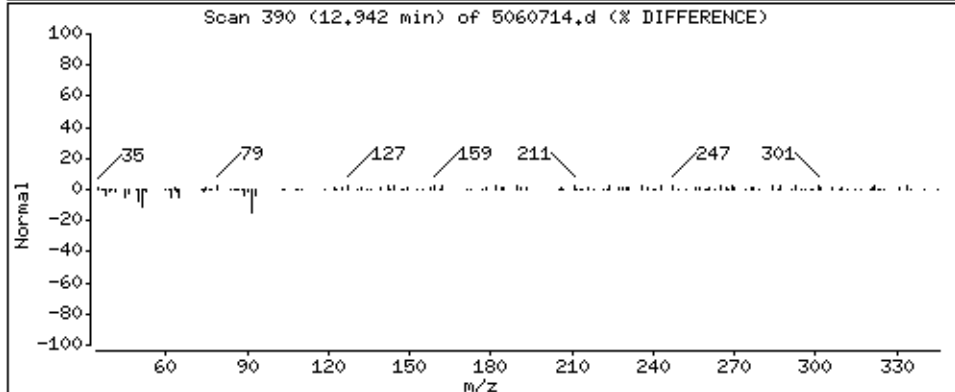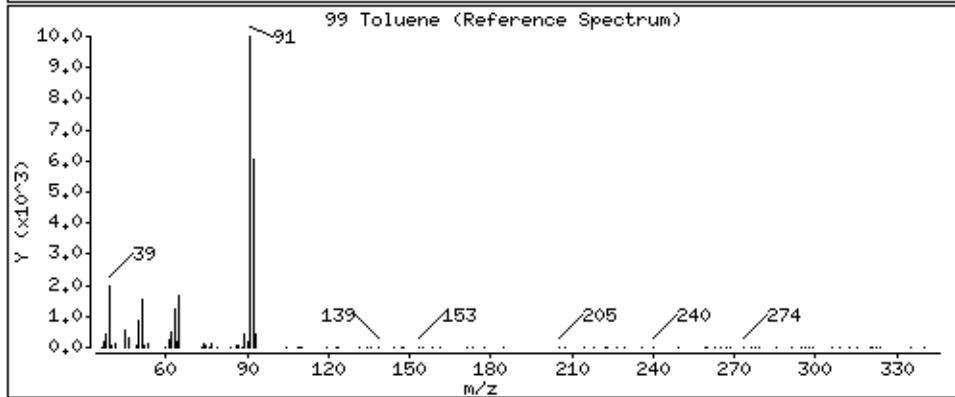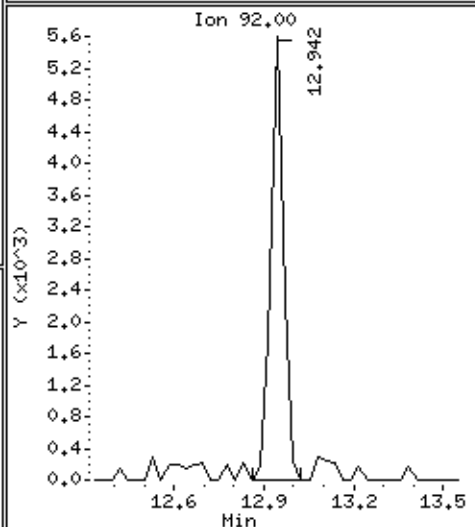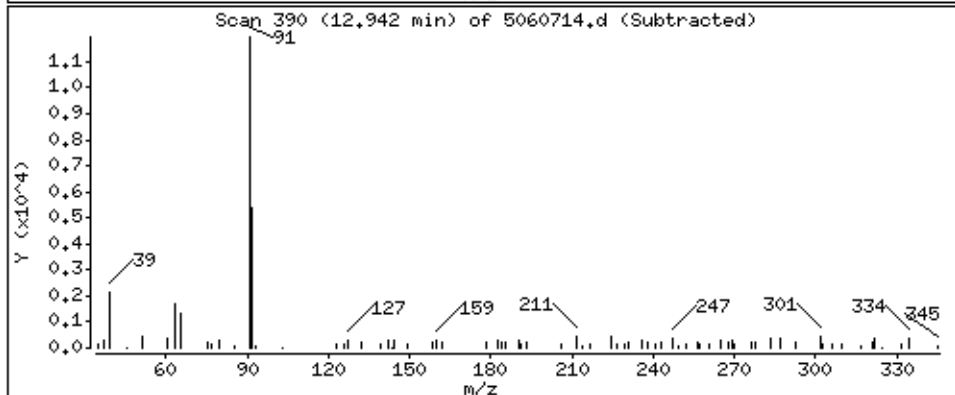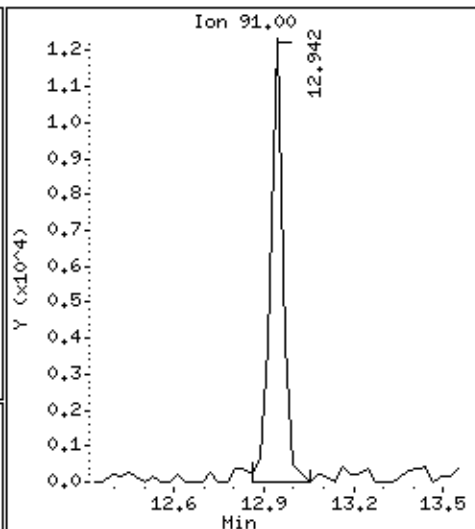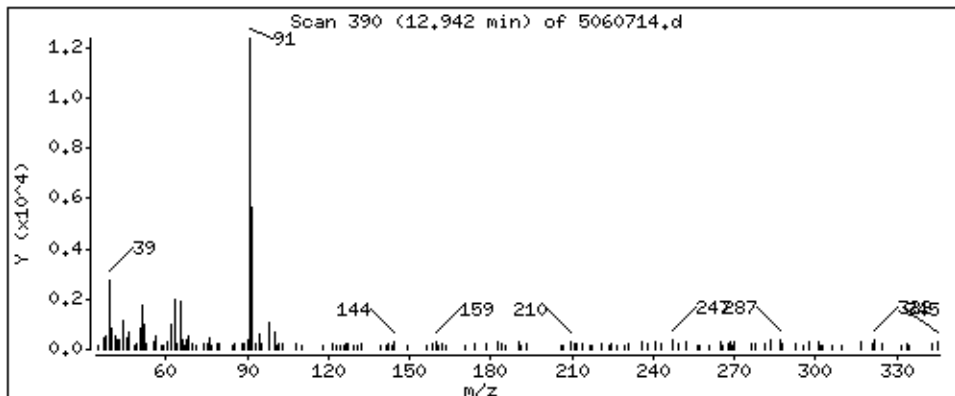

Date : 07-JUN-2007 18:14

Client ID:

Instrument: msd5.i

Sample Info: 200ml #T0-1560







Operator: jdg

Column phase: RTX-624

Column diameter: 0.53

113 m,p-Xylene

Concentration: 0.8607 PPBV

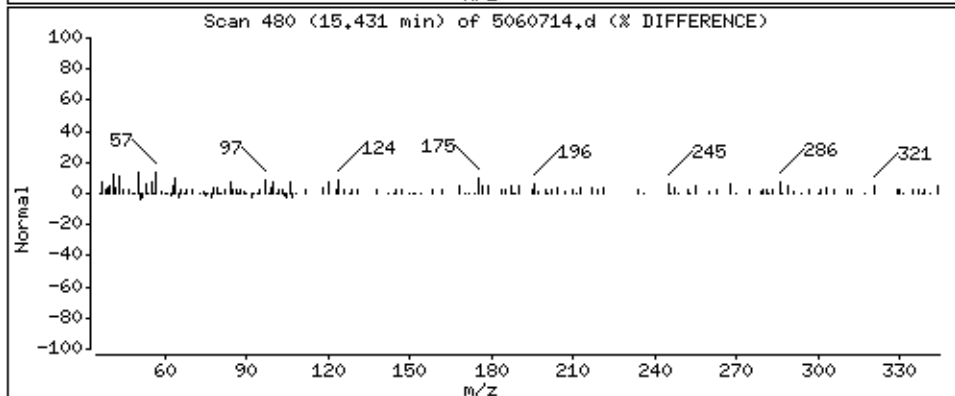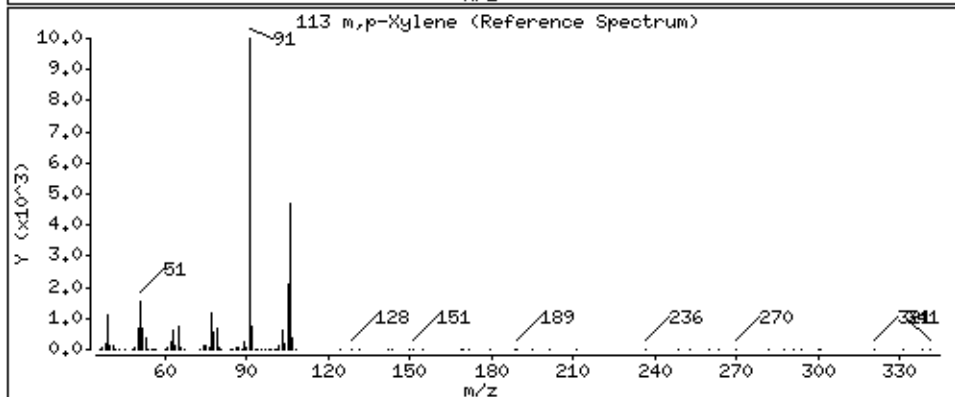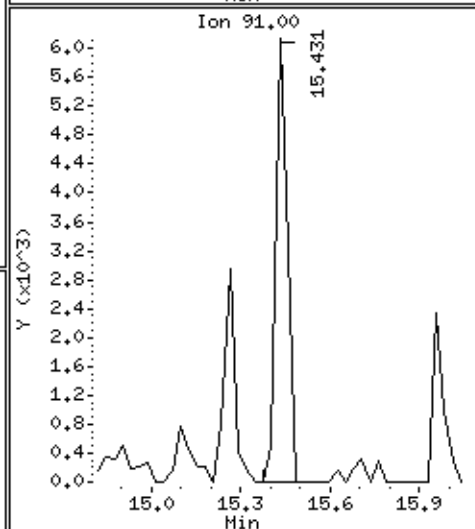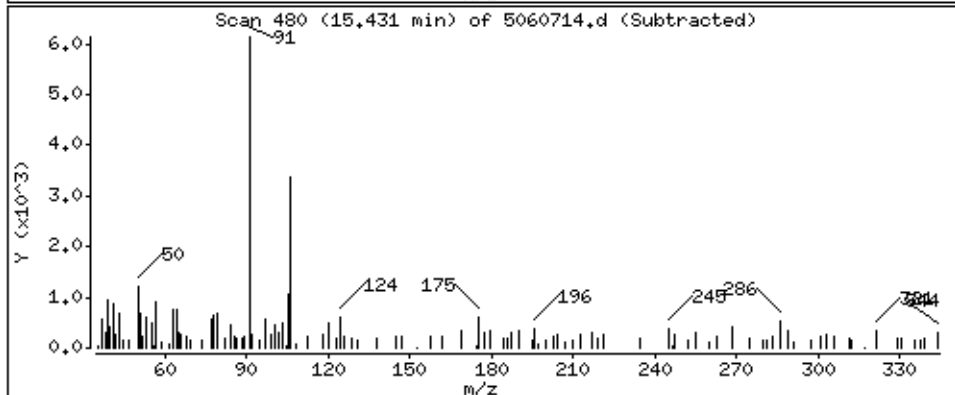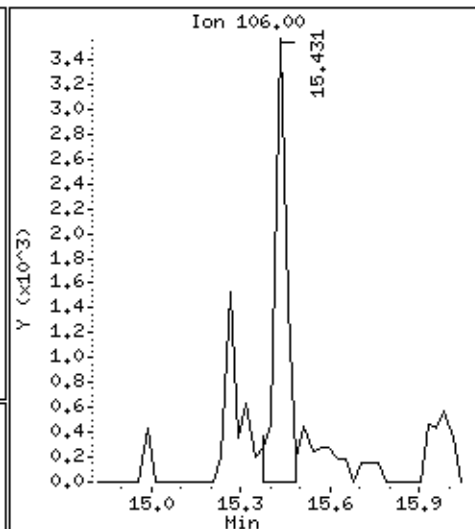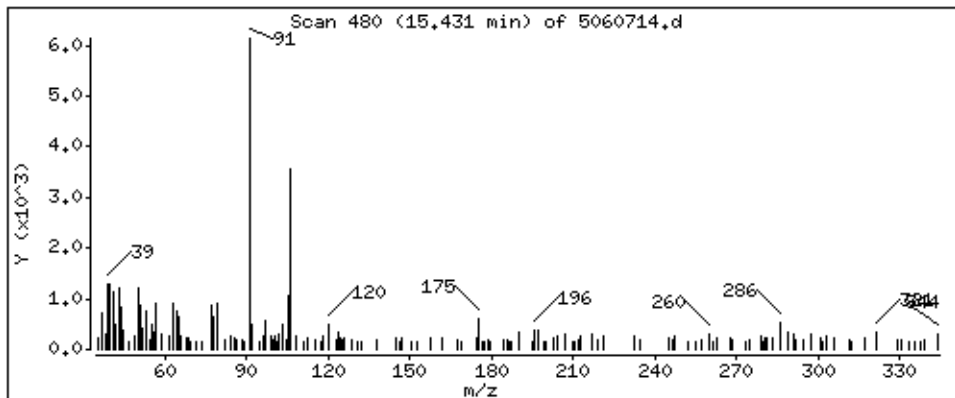

QC Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0706057-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060712	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/7/07 04:10 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0706057-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060712	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/7/07 04:10 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected	2.0	Not Detected
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected U J	1.8	Not Detected U J
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

UJ = Non-detected compound associated with low bias in the CCV

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	102	70-130
1,2-Dichloroethane-d4	102	70-130
4-Bromofluorobenzene	105	70-130

Report Date: 07-Jun-2007 16:46

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-07jun.b/5060712.d
 Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
 Inj Date : 07-JUN-2007 16:10
 Operator : JG Inst ID: msd5.i
 Smp Info : 200mL #13673
 Misc Info : Humid
 Comment :
 Method : /var/chem/msd5.i/5-07jun.b/t14q529a.m
 Meth Date : 07-Jun-2007 14:03 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS										
ON-COL FINAL										
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

* 57	Bromochloromethane					CAS #: 74-97-5				
8.187	8.214	(1.000)	130	224014	25.0000		80.00- 120.00	100.00		
8.214	8.214	(1.000)	128	172796			48.55- 108.55	77.14		
8.187	8.187	(1.000)	49	592428			229.31- 289.31	264.46		

* 79	1,4-Difluorobenzene					CAS #: 540-36-3				
10.067	10.067	(1.000)	114	887348	25.0000		80.00- 120.00	100.00		
10.067	10.067	(1.000)	88	164068			0.00- 49.97	18.49		

* 108	Chlorobenzene-d5					CAS #: 3114-55-4				
15.099	15.099	(1.000)	117	681503	25.0000		80.00- 120.00	100.00		
15.099	15.099	(1.000)	82	461613			33.54- 93.54	67.73		

\$ 71	1,2-Dichloroethane-d4					CAS #: 17060-07-0				
9.265	9.265	(1.132)	65	458175	25.5141	25.514	80.00- 120.00	100.00		
9.265	9.265	(1.132)	67	207136			25.98- 85.98	45.21		

\$ 97	Toluene-d8					CAS #: 2037-26-5				
12.832	12.832	(1.275)	98	821306	25.4287	25.429	80.00- 120.00	100.00		
12.832	12.832	(1.275)	70	98118			0.00- 41.05	11.95		

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 97 Toluene-d8 (continued)

12.832 12.832 (1.275) 100 493037 36.04- 96.04 60.03

\$ 122 Bromofluorobenzene

CAS #: 460-00-4

16.675 16.675 (1.104) 174 448568 26.1971 26.197 80.00- 120.00 100.00

16.675 16.675 (1.104) 95 719041 136.90- 196.90 160.30

16.675 16.675 (1.104) 176 420992 64.74- 124.74 93.85

Report Date: 07-Jun-2007 16:46

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 07-JUN-2007

Lab File ID: 5060712.d

Calibration Time: 13:20

Lab Smp Id: Lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /var/chem/msd5.i/5-07jun.b/t14q529a.m

Misc Info: Humid

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	292964	175778	410150	224014	-23.54
79 1,4-Difluorobenze	1106143	663686	1548600	887348	-19.78
108 Chlorobenzene-d5	855448	513269	1197627	681503	-20.33

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.21	7.88	8.54	8.19	-0.34
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-07jun
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
Level: LOW Operator: JG
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 1502+Na.spk Quant Type: ISTD
Sublist File: AT04+ENSR.sub
Method File: /var/chem/msd5.i/5-07jun.b/t14q529a.m
Misc Info: Humid

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 71 1,2-Dichloroethane	25.000	25.514	102.06	70-130
\$ 97 Toluene-d8	25.000	25.429	101.71	70-130
\$ 122 Bromofluorobenzene	25.000	26.197	104.79	70-130

Data File: /chem/msd5.1/5-07jun.b/5060712.d

Date: 07-JUN-2007 16:10

Client ID: Lab Blank

Sample Info: 200mL #13673


Column phase: RTX-624

Instrument: msd5.1

Operator: JG

Column diameter: 0.53

/chem/msd5.1/5-07jun.b/5060712.d

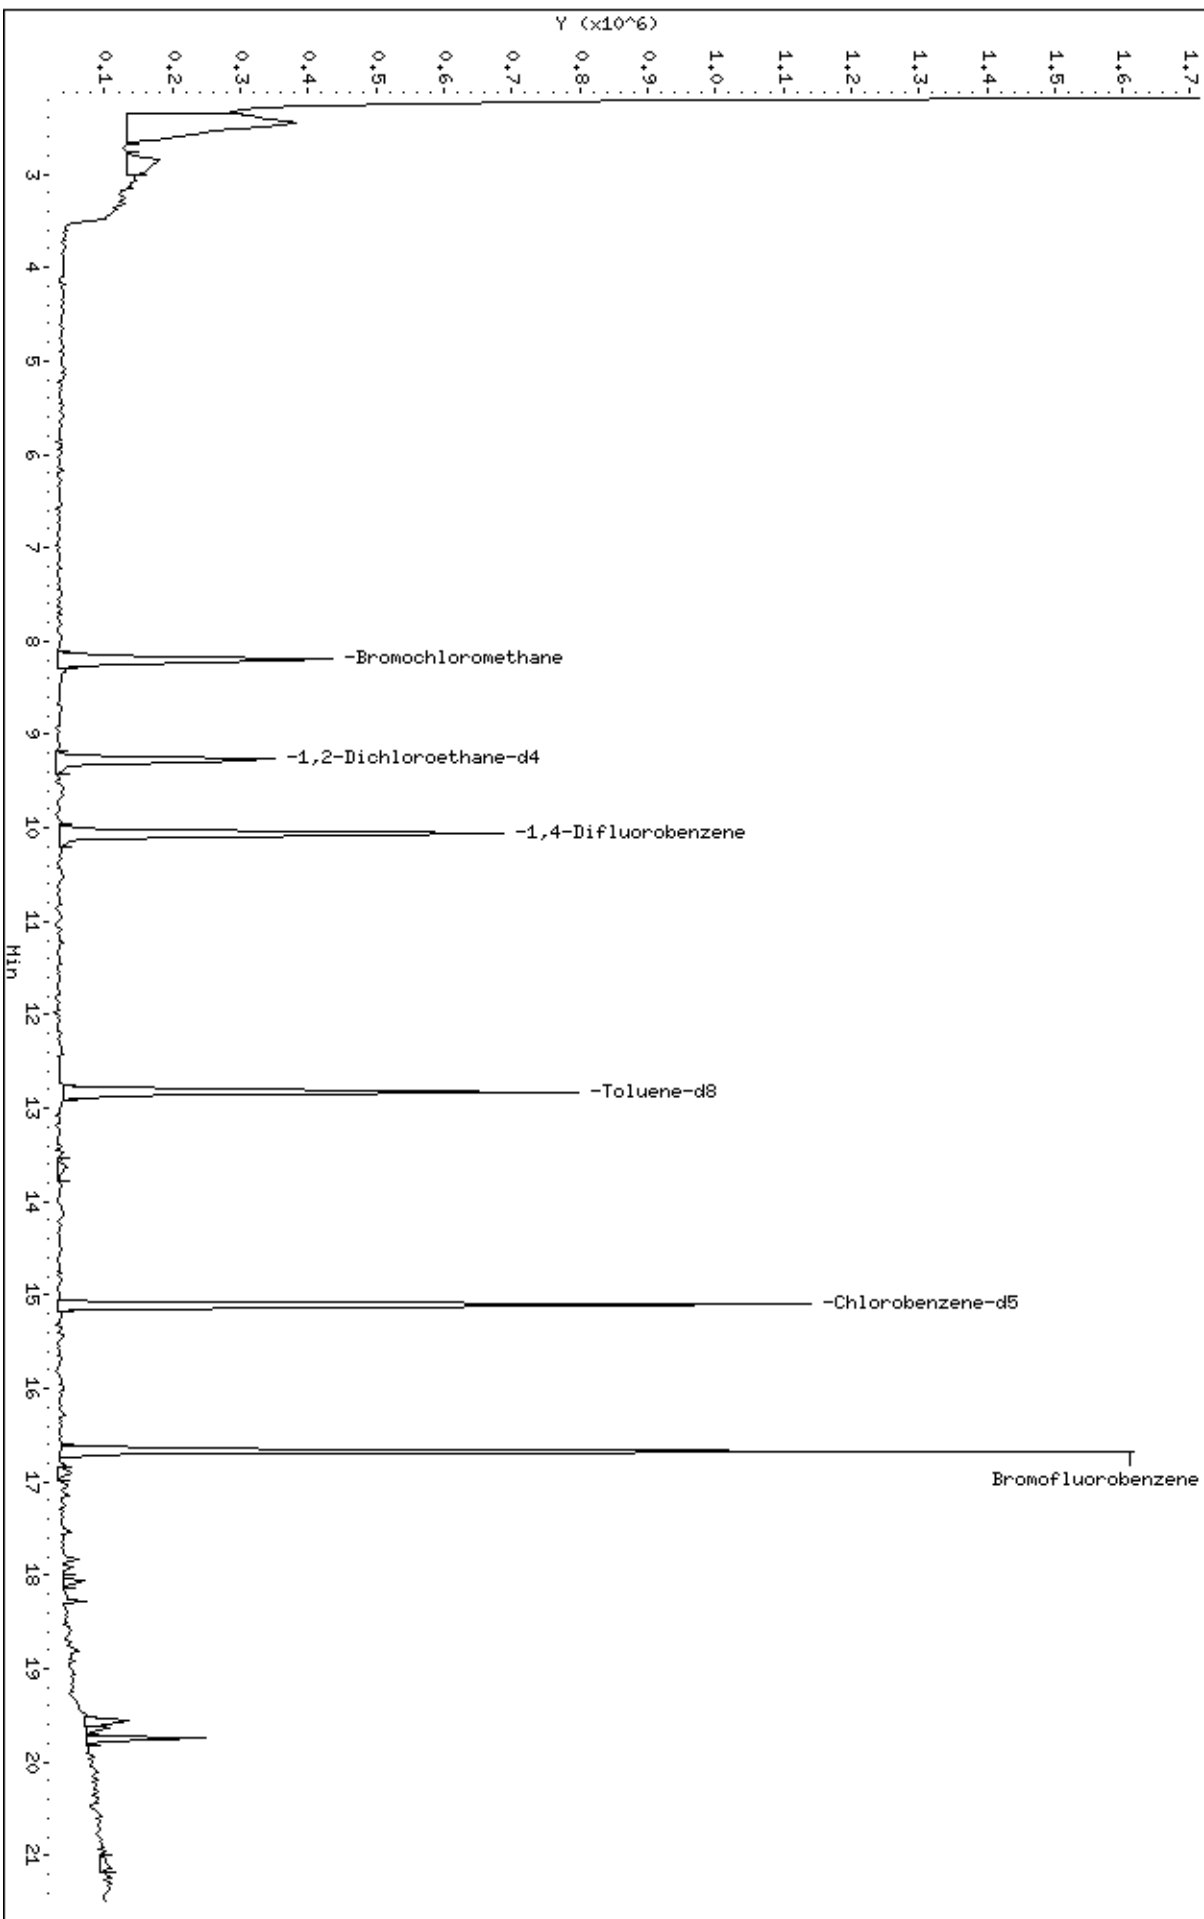

LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0706057

	CLIENT SAMPLE NO.	SURROGATE % RECOVERY						TOTAL OUT
		1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#	
01	AMS6-UW	103		99		98		0
02	AMS2-DW	101		100		102		0
03	Lab Blank	102		102		105		0
04	CCV	104		104		106		0
05	LCS	104		100		105		0
06								0
07								0
08								0
09								0
10								0
11								0
12								0
13								0
14								0
15								0
16								0
17								0
18								0
19								0
20								0
21								0
22								0
23								0
24								0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

* Designates values outside of QC limits

LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan

INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD
 Lab File ID: 5060709.d
 Instrument ID: msd5.i

SDG No: 0706057
 Date Analyzed: 06/07/2007
 Time Analyzed: 01:20 PM

	Chlorobenzene-d5			1,4-Difluorobenzene			Bromochloromethane			
	Area	#	RT	Area	#	RT	Area	#	RT	
24-HOUR STD	855448		15.1	1106143		10.07	292964		8.21	
UPPER LIMIT	1197627		15.43	1548600		10.40	410150		08.54	
LOWER LIMIT	513269		14.77	663686		09.74	175778		07.88	
CLIENT SAMPLE NO										
01	AMS6-UW	693581		15.1	883551		10.07	229001		8.19
02	AMS2-DW	657289		15.1	838821		10.07	216194		8.19
03	Lab Blank	681503		15.1	887348		10.07	224014		8.19
04	CCV	855448		15.1	1106143		10.07	292964		8.21
05	LCS	712923		15.1	921544		10.07	238932		8.19
06										
07										
08										
09										
10										
11										
12										
13										
14										
15										
16										
17										
18										
19										
20										
21										
22										

'Area Upper Limit=+40% of internal standard area'
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT
 RT Lower Limit=-0.33 minutes of internal standard RT

* Designates values outside of QC limits

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
2 Dichlorodifluoromethane/Fr12	200.000 4.46096	3.72970	5.87500	4.30608	4.15708	4.08363		4.43541	16.839
3 Freon 114	3.92809	3.68098	5.27186	4.28692	4.14578	4.13891		4.24209	12.893
4 Chloromethane	3.46383	+++++	4.80871	3.84264	4.02746	3.88042		4.00461	12.368
21 Butane	0.85310	+++++	1.11940	0.90873	0.86908	0.86095		0.92225	12.173
6 1,3-Butadiene	3.16479	2.48402	3.95675	3.27523	3.25400	3.25905		3.23231	14.460
5 Vinyl Chloride	3.20385	2.51337	3.71794	3.46633	3.33712	3.29960		3.25637	12.439
27 Methanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
7 Bromomethane	1.87318	1.67053	2.35356	1.89691	1.89882	1.91404		1.93451	11.608
35 Dichlorofluoromethane/Fr21	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
30 Isopentane	5.20818	+++++	6.87370	5.58592	5.24023	5.35874		5.65336	12.349

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
8 Chloroethane	+++++	1.67194	2.04815	1.72271	1.69648	1.64213			
	1.57937							1.72680	9.555
37 Pentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
9 Trichlorofluoromethane/Fr11	+++++	3.40227	5.66703	4.54945	4.36369	4.45020			
	4.39434							4.47116	16.118
11 Dimethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
41 Freon123a	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
14 Freon 13	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
42 Freon123	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
13 Ethanol	+++++	+++++	1.61498	1.31750	1.35578	1.27302			
	1.29726							1.37171	10.157
45 Acrolein	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
17 Isobutylene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
23 Acetaldehyde	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
19 Freon 113	+++++	2.48402	3.11662	2.67387	2.74041	2.76627		2.73760	7.689
24 Freon143a	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
20 1,1-Dichloroethene	+++++	3.58543	5.28257	4.26379	4.08669	4.21816		4.26876	12.997
22 Acetone	+++++	+++++	1.87352	1.52120	1.51107	1.51609		1.59231	9.896
49 Methyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
50 Acetonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
25 Carbon Disulfide	+++++	4.89091	7.20307	5.91247	5.78364	5.74795		5.87706	12.689
28 3-Chloropropene	+++++	+++++	1.12260	0.95389	0.95729	0.97711		0.99294	7.365
26 2-Propanol	+++++	+++++	9.06868	6.34052	6.28378	6.51673		6.93947	17.210

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
51 tert-Butyl-Alcohol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
54 Acrylonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
33 2-Methyl-1-Butene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
34 Vinyl Bromide	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
36 1-Pentene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
29 Methylene Chloride	+++++	3.91738	4.45296	4.05803	3.93492	3.87793		4.00350	5.942
39 Ethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
40 Ethanol-high	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
31 MTBE	+++++	2.70449	2.51114	3.88652	3.47320	3.32988		3.12343	16.824
32 trans-1,2-Dichloroethene	+++++	1.86664	2.57121	2.15060	2.08051	2.09402		2.12856	11.176

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
44 Propanal	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
60 Isopropyl ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
38 Hexane	+++++	4.78036	6.59127	5.26321	5.19213	5.19510		5.35177	11.788
63 Vinyl Acetate	+++++	+++++	0.48526	0.48004	0.49455	0.51192		0.49588	2.782
46 Bromoethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
59 Chloroprene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
47 Iodomethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
48 2,3-Dimethylbutane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
43 1,1-Dichloroethane	+++++	3.28689	5.28060	4.36747	4.20880	4.22479		4.25730	14.897
67 Ethyl-tert-butyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
55 1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
110 1,3-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
74 2,2-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
73 Ethyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
77 Methyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
66 2,4-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
64 1-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
70 Butanal	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
52 cis-1,2-Dichloroethene	+++++	2.97211	3.96711	3.21722	3.26373	3.25730	3.16169	3.30653	10.313
53 2-Butanone	+++++	0.71855	0.95624	0.80862	0.80671	0.83146	0.81311	0.82245	9.308

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
76 2-Butanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
78 3-Methyl-1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
56 Tetrahydrofuran	+++++	4.02761	5.76261	4.00834	3.95228	3.95033		4.26523	17.236
58 Chloroform	2.63247	2.89638	3.60773	3.05828	3.09415	3.04360		3.04977	9.580
187 1,1-Dichloropropene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
61 Cyclohexane	+++++	1.71706	2.83715	2.36745	2.22235	2.22883		2.25587	15.998
62 1,1,1-Trichloroethane	+++++	2.90528	3.94631	3.25147	3.26835	3.29077		3.32174	10.210
81 Isobutanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
65 Carbon Tetrachloride	+++++	2.44311	3.38869	2.84513	2.86611	2.88706		2.89398	10.399
83 tert-amyl-Methyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
75 Heptane	+++++	0.19465	0.19356	0.13746	0.12638	0.13170			
	0.13154							0.15255	21.225
86 1-Butanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
80 Trichloroethene	+++++	0.38172	0.64616	0.47752	0.44124	0.44152			
	0.43515							0.47055	19.415
96 Methyl Cyclohexane	+++++	0.59621	0.87511	0.65319	0.64182	0.61614			
	0.61002							0.66541	15.757
98 Dibromomethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
92 Methyl Methacrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
107 1-Nitropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
82 1,2-Dichloropropane	+++++	0.42725	0.59919	0.49504	0.47458	0.46780			
	0.46990							0.48896	11.930
84 1,4-Dioxane	+++++	+++++	0.31521	0.23910	0.24614	0.23018			
	0.22749							0.25162	14.428
85 Bromodichloromethane	+++++	0.54599	0.82970	0.69971	0.69902	0.69951			
	0.69687							0.69513	12.933

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
120 1-Methoxy-2-propyl acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
121 Epichlorohydrin	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
90 cis-1,3-Dichloropropene	+++++	0.39754	0.59007	0.53286	0.48983	0.50627		0.50154	12.570
136 Decane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
127 alpha-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
91 4-Methyl-2-pentanone	+++++	0.30898	0.64288	0.49905	0.48636	0.47601		0.48102	22.049
99 Toluene	+++++	0.93138	1.32845	1.10392	1.05615	1.03627		1.07800	12.548
132 trans-1,4-dichloro-2-butene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
135 beta-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
186 Dicyclopentadiene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
140 Alphamethylstyrene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
100 trans-1,3-Dichloropropene	+++++	0.50845	0.84881	0.70278	0.71353	0.72089		0.70246	15.574
101 1,1,2-Trichloroethane	+++++	0.37764	0.62765	0.48112	0.45255	0.46075		0.47424	17.485
145 D-Limonene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
102 Tetrachloroethene	+++++	0.61301	0.73852	0.56801	0.55407	0.55058		0.59311	12.828
148 Bis(2-chloroethyl) ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
112 Butyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
103 2-Hexanone	+++++	+++++	1.06323	0.81955	0.84521	0.85038		0.88672	11.235
105 Dibromochloromethane	+++++	0.68385	0.87093	0.76438	0.75839	0.77552		0.77203	7.742
151 Undecane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
106 1,2-Dibromoethane	+++++	0.64923	0.82491	0.73006	0.72693	0.71970		0.72482	7.927
117 1,1,1,2-Tetrachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
152 1-chloro-2-Bromopropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
109 Chlorobenzene	+++++	1.15882	1.45125	1.10431	1.04671	1.06721		1.14489	13.652
116 Nonane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
111 Ethyl Benzene	+++++	0.38972	0.69470	0.59090	0.58323	0.57050		0.56264	17.572
157 Dodecane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
113 m,p-Xylene	+++++	0.62324	0.92967	0.72713	0.71720	0.71124		0.73252	14.138
125 2-Heptanone	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
114 o-Xylene	+++++	0.49847	1.00166	0.68801	0.66790	0.66206		0.69275	23.956

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
115 Styrene	0.75182	0.79894	1.28435	1.06831	1.06959	1.06229		
	1.05248						1.01254	17.937
118 Bromoform	+++++	0.48430	0.79842	0.65484	0.66649	0.68314		
	0.68260						0.66163	15.284
129 Cyclohexanone	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
119 Cumene	1.61745	1.82447	2.95026	2.17017	2.11436	2.08005		
	2.05891						2.11652	19.642
130 Bromobenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
133 1,2,3-Trichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
134 2-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
123 1,1,2,2-Tetrachloroethane	+++++	0.97509	1.47796	1.04416	1.01239	1.01413		
	0.96842						1.08202	18.110
124 Propylbenzene	+++++	2.26537	3.81444	2.83305	2.75807	2.76105		
	2.07992						2.75198	21.947
137 4-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
149 1,2,3-Trimethylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
138 1,3-Dichlorobenzene	+++++	1.30968	1.97642	1.32930	1.29022	1.29864		1.40355	20.181
141 1,4-Dichlorobenzene	+++++	0.90964	1.46709	1.05261	1.08296	1.07267		1.10990	16.824
143 alpha-Chlorotoluene	+++++	1.06838	2.07154	1.86993	1.97204	2.10109		1.85176	21.190
150 Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
146 1,2-Dichlorobenzene	+++++	1.47556	2.12615	1.34329	1.29080	1.29237		1.45593	23.354
190 Hexachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
153 1,2-Dibromo-3-Chloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
160 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
154 1,2,4-Trichlorobenzene	+++++	+++++	1.53874	0.86580	0.89893	0.93748		1.02387	28.236

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 29-MAY-2007 15:42
 End Cal Date : 29-MAY-2007 20:44
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-29may.b/t14q529a.m
 Cal Date : 30-May-2007 15:48 jgray
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
155 Hexachlorobutadiene	0.67947	+++++	1.39614	0.70711	0.74504	0.71452		0.84846	36.190 <-
156 Naphthalene	2.16556	+++++	4.72728	2.58758	2.81032	2.90596		3.03934	32.434 <-
188 1,2,3-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
161 Isooctyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
\$ 71 1,2-Dichloroethane-d4	2.27213	1.89977	1.95214	1.91095	1.94055	2.04894		2.00408	7.062
\$ 97 Toluene-d8	0.91334	0.88388	0.90642	0.93226	0.91722	0.90670		0.90997	1.748
\$ 122 Bromofluorobenzene	0.64369	0.60688	0.62071	0.64948	0.62853	0.61947		0.62813	2.547

Calibration History

Method : /chem/msd5.i/5-29may.b/t14q529a.m
Start Cal Date: 29-MAY-2007 15:42
End Cal Date : 29-MAY-2007 20:44

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.30000		
29-MAY-2007 15:42	AFCEElow	/chem/msd5.i/5-29may.b/5052911.d
Cal Level: 2 , Cal Amount: 0.50000		
29-MAY-2007 16:10	AT04Low+ENSR	/chem/msd5.i/5-29may.b/5052912.d
Cal Level: 3 , Cal Amount: 2.00000		
29-MAY-2007 20:44	AT04MDL+ENSR	/chem/msd5.i/5-29may.b/5052920.d
Cal Level: 4 , Cal Amount: 25.00000		
29-MAY-2007 17:06	AT04MDL+ENSR	/chem/msd5.i/5-29may.b/5052914.d
Cal Level: 5 , Cal Amount: 50.00000		
29-MAY-2007 17:34	AT04MDL+ENSR	/chem/msd5.i/5-29may.b/5052915.d
Cal Level: 6 , Cal Amount: 100.00000		
29-MAY-2007 18:02	AT04MDL+ENSR	/chem/msd5.i/5-29may.b/5052916.d
Cal Level: 7 , Cal Amount: 200.00000		
29-MAY-2007 18:31	AT04MDL+ENSR	/chem/msd5.i/5-29may.b/5052917.d

Continuing Calibration
Ccal Level Mode: GLOBAL LEVEL 8

| Ccal Level: 8 , Ccal Amount: 50.000 |

+=====+

| 29-MAY-2007 17:34 | AT04MDL+ENSR | /chem/msd5.i/5-29may.b/5052915a.d |

+-----+

ION ABUNDANCE CRITERIA

m/z	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95
75	30.0 - 60.0% of mass 95
95	Base peak, 100.00% relative abundance
96	5.0 - 9.0% of mass 95
173	Less than 2.0% of mass 174
174	Greater than 50.0% of mass 95
175	5.0 - 9.0% of mass 174
176	Greater than 95.0% but less than 101.0% of mass 174
177	5.0 - 9.0% of mass 176

1 - value in parenthesis is % mass 174
 Verify 176/174 m/z Ratio: $\frac{878 \text{ (272)}}{5124107} / \frac{907 \text{ (276)}}{5124107} = 96.75\%$

Calculation Check: $\frac{5124107 \text{ (272)}}{5124107} = 100\%$

ppbv of compound

Area Sample

Conc:is

RRF

Reported Result

BFB Injection Date: 5/29/07
 BFB Injection Time: 1443
 BFB File ID: SDS29009
 Tekmar Purge Flow: 12.2 mL/min
 Vacuum: 6.33 x 10⁻⁶ Torr
 IS/Std #: 1483-7259 Exp. Date: 8/10/07
 BCM 313773
 1,4-DFB 1272249
 CB-d5 1008159
 Verified CCV IS vs ICAL mid-point (-40%AD) 45

NOAH Cart #: NA

File #: NA

File #: NA

File ID: _____
 Compound: _____
 Initials: _____

Sample #	File #	Sample / Client Name	Can #	Pressure	Amnt Loaded	DF	Encoder Int.	Date Analyzed	Time Analyzed	Review Int.	Comments	
1	✓	SDS29009	BFB Time Check	443-2080	50mg	2mL	1.00	02	5/29/07	1443	RL	
2	X	10	System Blank	1241	Humid	200 mL	1.00	02	5/29/07	1515	02	
3	✓	11	ICAR Level 1	1483-288	0.3 ppbv	0.3 mL				1542	02	4145200
4	✓	12			0.5 ppbv	0.5 mL				1610	02	
5	X	13			2.0 ppbv	2.0 mL				1638	45	Send Level
6	✓	14			25 ppbv	25 mL				1780	45	
7	✓	15			50 ppbv	50 mL				1724	45	
8	✓	16			100 ppbv	100 mL				1802	45	
9	✓	17			200 ppbv	200 mL				1831	45	

Signature: *Amiee Green*

Date: 5/29/07

10	X	CDS 2918	System Blank	7441	Humid	250umL	1.00	54	5/29/07	1855	45
11	✓	5052919	System Blank	34583	Humid	200umL	1.00	54		1858	63
12	✓	20	REAL: Level 3	1487288	200umL	200umL	1.00	45		2094	45
13	✓	21	REAL: LCS	1487292	50umL	50umL	1.00	54		2153	44
14											
15											
16											
17											
18											
19											
20											
21											
22											
23											
24											
25											
26											
27											
28											
29											
30											
31											
32											

Comments: Flow Controller: AA9203108 Flow Meter: 200-3344, Exp. 7/28/07

Actual: 25.0 mL/min Nominal: 22.4 mL/min At 5/29/07

Signature 







Date 5/29/07

Initial Calibration Narrative

A seven-point initial calibration was analyzed on MSD-5 on May 29, 2007.

Sample: ICAL Type: CALIB_2 Inj.Date: 29-MAY-2007 16:10

- ** 57 Bromochlorometl
- ** 79 1,4-Difluorobe
- ** 108 Chlorobenzene-
- ** 71 1,2-Dichloroetl
- ** 97 Toluene-d8
- ** 122 Bromofluoroben:
- + 2 Dichlorodifluo
- + 3 Freon 114
- + 5 Vinyl Chloride
- + 6 1,3-Butadiene
- + 7 Bromomethane
- + 8 Chloroethane**
- + 9 Trichlorofluor
- + 19 Freon 113
- + 20 1,1-Dichloroetl
- + 25 Carbon Disulfu
- + 29 Methylene Chlo
- + 31 MTBE
- + 32 trans-1,2-Dich.
- + 38 Hexane
- + 43 1,1-Dichloroetl
- + 53 2-Butanone
- + 52 cis-1,2-Dichlo
- + 56 Tetrahydrofura
- + 58 Chloroform

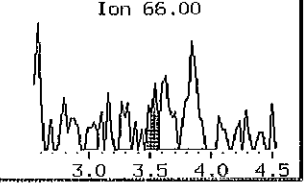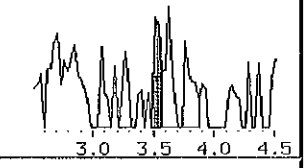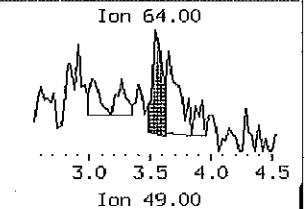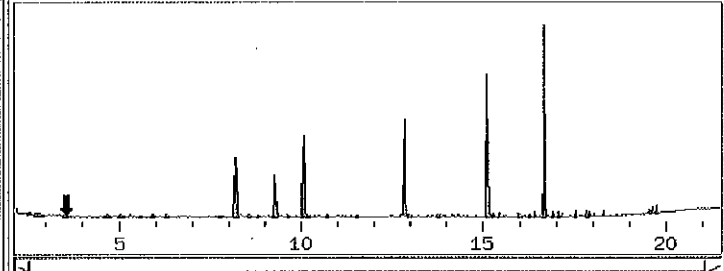

5052912.d

Hit#	RT(mIn)	Response	Amount	Conc	Ratio	Flags	Report:
3	3.542	9287	0.4291	0.4291	100	a	
	3.514	2538			27		
	3.542	2673			29		
4	3.652	9316	0.4304	0.4304	100	Ta	
	3.625	3019			32		

For Integration	GL 5/30/07
Split Peak	✓
Peak Tailing	
Background Subtraction	
Sum In	
Selected Peak	

Mr 5/30/07

File Security Edit Display Process Spectra Help

Sample: ICAL Type: CALIB_2 Inj.Date: 29-MAY-2007 16:10

- ** 57 Bromochlorometl
- ** 79 1,4-Difluorober
- ** 108 Chlorobenzene-
- ** 71 1,2-Dichloroetl
- ** 97 Toluene-d8
- ** 122 Bromofluoroben:
- + 2 Dichlorodifluo
- + 3 Freon 114
- + 5 Vinyl Chloride
- + 6 1,3-Butadiens
- + 7 Bromomethane
- + 8 Chloroethane**
- + 9 Trichlorofluor
- + 19 Freon 113
- + 20 1,1-Dichloroetl
- + 25 Carbon Disulfid
- + 29 Methylene Chlor
- + 31 MTBE
- + 32 trans-1,2-Dich.
- + 38 Hexane
- + 43 1,1-Dichloroetl
- + 53 2-Butanone
- + 52 cis-1,2-Dichlo
- + 56 Tetrahydrofural
- + 58 Chloroform

HP MS 5052912.d, Scan 50: 3.542 min. (SUB)

43 105 182 243 290 349

Reference Spectrum for Chloroethane

43 98 201 265 295 348

Hit#	RT (min)	Response	Amount	Conc	Ratio	Flags	Report:
1	3.542	10708	0.4964	0.4964	100	AM	
	3.514	2538			24		
	3.542	2672			25		

- Mark Chloroethane Undetected.

Air Toxics Ltd.
 Modified EPA Methods TO-14A/TO-15
 Internal Standard and Associated Target Compounds and Surrogates

Bromochloromethane
Target Compounds:
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
3-Chloropropene
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
2,2,4-Trimethylpentane
Surrogates:
1,2-Dichloroethane-d4

1,4-Difluorobenzene
Target Compounds:
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
Surrogates:
Toluene-d8

Chlorobenzene-d5
Target Compounds:
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
Surrogates:
Bromofluorobenzene

Report Date: 30-May-2007 15:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052921.d
 Lab Smp Id: ICAL Client Smp ID: LCS
 Inj Date : 29-MAY-2007 21:53
 Operator : JG Inst ID: msd5.i
 Smp Info : 50mL #1487-272
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE (PPBV)		TARGET RANGE	RATIO	
				ON-COL	FINAL			
==	=====	=====	=====	=====	=====	=====	=====	=====

* 57	Bromochloromethane					CAS #: 74-97-5		
8.187	8.187	(1.000)	130	328581	25.0000	80.00- 120.00	100.00	
8.187	8.187	(1.000)	128	246155		50.27- 110.27	74.91	
8.187	8.187	(1.000)	49	1012849		281.04- 341.04	308.25	

* 79	1,4-Difluorobenzene					CAS #: 540-36-3		
10.067	10.067	(1.000)	114	1294035	25.0000	80.00- 120.00	100.00	
10.067	10.067	(1.000)	88	234097		0.00- 48.57	18.09	

* 108	Chlorobenzene-d5					CAS #: 3114-55-4		
15.099	15.099	(1.000)	117	1016588	25.0000	80.00- 120.00	100.00	
15.099	15.099	(1.000)	82	638981		33.54- 93.54	62.86	

\$ 71	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.265	9.265	(1.132)	65	633360	24.0454	24.045 80.00- 120.00	100.00	
9.265	9.265	(1.132)	67	311083		25.98- 85.98	49.12	

\$ 97	Toluene-d8					CAS #: 2037-26-5		
12.832	12.832	(1.275)	98	1187396	25.2094	25.209 80.00- 120.00	100.00	
12.832	12.832	(1.275)	70	136597		0.00- 41.05	11.50	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 97 Toluene-d8 (continued)

12.832	12.832	(1.275)	100	757476			36.04- 96.04	63.79
--------	--------	---------	-----	--------	--	--	--------------	-------

\$ 122 Bromofluorobenzene

CAS #: 460-00-4

16.675	16.675	(1.104)	174	632002	24.7438	24.744	80.00- 120.00	100.00
16.675	16.675	(1.104)	95	1045367			131.53- 191.53	165.41
16.675	16.675	(1.104)	176	615640			65.40- 125.40	97.41

1 Propylene

CAS #: 115-07-1

2.353	2.353	(0.287)	41	2233228	50.9588	50.959	80.00- 120.00	100.00
2.353	2.353	(0.287)	42	1504094			36.96- 96.96	67.35
2.353	2.353	(0.287)	39	1558713			37.69- 97.69	69.80

2 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.408	2.408	(0.294)	85	2842771	48.7647	48.765	80.00- 120.00	100.00
2.408	2.408	(0.294)	87	929381			1.62- 61.62	32.69

3 Freon 114

CAS #: 76-14-2

2.518	2.546	(0.308)	135	2788676	50.0168	50.017	80.00- 120.00	100.00
2.518	2.546	(0.308)	137	898608			0.80- 60.80	32.22

4 Chloromethane

CAS #: 74-87-3

2.657	2.657	(0.325)	50	2485583	47.2243	47.224	80.00- 120.00	100.00
2.657	2.684	(0.325)	52	777295			0.00- 59.51	31.27

5 Vinyl Chloride

CAS #: 75-01-4

2.850	2.850	(0.348)	62	2295483	53.6338	53.634	80.00- 120.00	100.00
2.850	2.850	(0.348)	64	679679			0.00- 59.15	29.61

6 1,3-Butadiene

CAS #: 106-99-0

2.823	2.823	(0.345)	54	2197289	51.7216	51.722	80.00- 120.00	100.00
2.823	2.823	(0.345)	39	2510833			92.11- 152.11	114.27

7 Bromomethane

CAS #: 74-83-9

3.376	3.376	(0.412)	94	1325019	52.1134	52.113	80.00- 120.00	100.00
3.376	3.376	(0.412)	96	1242843			64.95- 124.95	93.80

8 Chloroethane

CAS #: 75-00-3

3.486	3.514	(0.426)	64	1169705	51.5386	51.539	80.00- 120.00	100.00
3.486	3.486	(0.426)	49	366779			1.83- 61.83	31.36
3.486	3.514	(0.426)	66	327916			0.00- 57.39	28.03

9 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.818	3.818	(0.466)	101	2981684	50.7386	50.739	80.00- 120.00	100.00
3.818	3.818	(0.466)	103	1908394			35.72- 95.72	64.00

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

13 Ethanol CAS #: 64-17-5
 4.177 4.177 (0.510) 45 1001511 55.5509 55.551 80.00- 120.00 100.00
 4.177 4.177 (0.510) 43 184480 0.00- 49.45 18.42
 4.177 4.177 (0.510) 46 406974 11.95- 71.95 40.64

19 Freon 113 CAS #: 76-13-1
 4.647 4.647 (0.568) 151 2050329 56.9837 56.984 80.00- 120.00 100.00
 4.647 4.647 (0.568) 153 1266678 32.16- 92.16 61.78
 4.647 4.647 (0.568) 101 2667615 100.00- 160.00 130.11

20 1,1-Dichloroethene CAS #: 75-35-4
 4.675 4.675 (0.571) 61 3085705 54.9984 54.998 80.00- 120.00 100.00
 4.675 4.675 (0.571) 96 1447359 19.13- 79.13 46.91
 4.675 4.675 (0.571) 98 952584 0.28- 60.28 30.87

22 Acetone CAS #: 67-64-1
 4.841 4.841 (0.591) 58 1024500 48.9533 48.953 80.00- 120.00 100.00
 4.813 4.841 (0.588) 43 3671091 327.94- 387.94 358.33

26 2-Propanol CAS #: 67-63-0
 5.035 5.035 (0.615) 45 4365491 47.8635 47.863 80.00- 120.00 100.00
 5.035 5.035 (0.615) 43 854212 0.00- 49.24 19.57
 5.035 5.035 (0.615) 59 143011 0.00- 33.25 3.28

25 Carbon Disulfide CAS #: 75-15-0
 5.007 5.007 (0.612) 76 3890875 50.3715 50.371 80.00- 120.00 100.00

28 3-Chloropropene CAS #: 107-05-1
 5.311 5.311 (0.649) 76 630854 48.3397 48.340 80.00- 120.00 100.00
 5.311 5.311 (0.649) 41 3347565 480.64- 540.64 530.64

29 Methylene Chloride CAS #: 75-09-2
 5.560 5.560 (0.679) 49 2785514 52.9374 52.937 80.00- 120.00 100.00
 5.560 5.560 (0.679) 84 1134060 9.87- 69.87 40.71
 5.560 5.560 (0.679) 51 806371 0.00- 59.58 28.95

31 MTBE CAS #: 1634-04-4
 5.892 5.892 (0.720) 73 1907407 46.4632 46.463 80.00- 120.00 100.00
 5.892 5.892 (0.720) 57 736012 5.77- 65.77 38.59
 5.892 5.892 (0.720) 41 792960 10.34- 70.34 41.57

32 trans-1,2-Dichloroethene CAS #: 156-60-5
 5.947 5.947 (0.726) 96 1344405 48.0554 48.055 80.00- 120.00 100.00
 5.947 5.947 (0.726) 61 2652163 164.17- 224.17 197.27
 5.947 5.947 (0.726) 98 853292 32.40- 92.40 63.47

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

38 Hexane CAS #: 110-54-3
 6.279 6.279 (0.767) 57 3373087 47.9543 47.954 80.00- 120.00 100.00
 6.279 6.279 (0.767) 43 2580083 46.14- 106.14 76.49
 6.279 6.279 (0.767) 86 390543 0.00- 41.50 11.58

43 1,1-Dichloroethane CAS #: 75-34-3
 6.721 6.721 (0.821) 63 2854811 51.0200 51.020 80.00- 120.00 100.00
 6.721 6.721 (0.821) 65 841440 0.00- 59.00 29.47

53 2-Butanone CAS #: 78-93-3
 7.799 7.800 (0.953) 72 533620 49.3653 49.365 80.00- 120.00 100.00
 7.799 7.800 (0.953) 43 4341216 796.36- 856.36 813.54
 7.799 7.800 (0.953) 57 283771 23.20- 83.20 53.18

52 cis-1,2-Dichloroethene CAS #: 156-59-2
 7.772 7.744 (0.949) 61 2136568 49.1634 49.163 80.00- 120.00 100.00
 7.772 7.772 (0.949) 96 1129748 25.31- 85.31 52.88
 7.772 7.772 (0.949) 98 715273 2.88- 62.88 33.48

56 Tetrahydrofuran CAS #: 109-99-9
 8.187 8.187 (1.000) 42 2540884 45.3252 45.325 80.00- 120.00 100.00
 8.187 8.187 (1.000) 71 478922 0.00- 48.47 18.85
 8.187 8.187 (1.000) 72 513127 0.00- 49.73 20.19

58 Chloroform CAS #: 67-66-3
 8.325 8.325 (1.017) 83 2011562 50.1838 50.184 80.00- 120.00 100.00
 8.325 8.325 (1.017) 85 1282416 33.68- 93.68 63.75

62 1,1,1-Trichloroethane CAS #: 71-55-6
 8.574 8.574 (1.047) 97 2131561 48.8237 48.824 80.00- 120.00 100.00
 8.574 8.574 (1.047) 99 1367254 32.24- 92.24 64.14

61 Cyclohexane CAS #: 110-82-7
 8.546 8.546 (1.044) 84 1446241 48.7781 48.778 80.00- 120.00 100.00
 8.546 8.546 (1.044) 56 3030397 177.94- 237.94 209.54
 8.546 8.546 (1.044) 41 1867779 93.55- 153.55 129.15

63 Vinyl Acetate CAS #: 108-05-4
 6.776 6.776 (0.828) 86 335258 51.4397 51.440 80.00- 120.00 100.00
 6.776 6.776 (0.828) 43 5941317 1767.50-1827.50 1772.16
 6.776 6.776 (0.828) 42 440302 104.58- 164.58 131.33

65 Carbon Tetrachloride CAS #: 56-23-5
 8.822 8.795 (1.078) 119 1872056 49.2177 49.218 80.00- 120.00 100.00
 8.822 8.795 (1.078) 117 1925632 71.97- 131.97 102.86

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

68	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.237	9.237	(1.128)	57	8141017	48.7028	48.703	80.00-	120.00	100.00	
9.237	9.237	(1.128)	56	2670713			2.91-	62.91	32.81	
9.237	9.237	(1.128)	41	2455108			0.00-	59.75	30.16	

69	Benzene					CAS #:	71-43-2			
9.237	9.237	(0.918)	78	2795203	48.1077	48.108	80.00-	120.00	100.00	
9.237	9.237	(0.918)	77	668273			0.00-	53.04	23.91	

72	1,2-Dichloroethane					CAS #:	107-06-2			
9.403	9.403	(0.934)	62	2027123	51.2890	51.289	80.00-	120.00	100.00	
9.403	9.403	(0.934)	64	600657			0.57-	60.57	29.63	

75	Heptane					CAS #:	142-82-5			
9.624	9.624	(0.956)	100	346412	43.8709	43.871	80.00-	120.00	100.00	
9.624	9.624	(0.956)	43	3847579			1063.83-	1123.83	1110.69	
9.624	9.624	(0.956)	71	1048504			257.42-	317.42	302.68	

80	Trichloroethene					CAS #:	79-01-6			
10.481	10.481	(1.041)	95	1190865	48.8932	48.893	80.00-	120.00	100.00	
10.481	10.481	(1.041)	130	1096871			65.35-	125.35	92.11	
10.481	10.481	(1.041)	97	763310			35.05-	95.05	64.10	

82	1,2-Dichloropropane					CAS #:	78-87-5			
10.979	10.979	(1.091)	63	1228584	48.5426	48.543	80.00-	120.00	100.00	
10.979	10.979	(1.091)	62	900625			43.36-	103.36	73.31	
10.979	10.979	(1.091)	41	1134771			62.33-	122.33	92.36	

84	1,4-Dioxane					CAS #:	123-91-1			
11.200	11.200	(1.113)	88	595375	45.7124	45.712	80.00-	120.00	100.00	
11.200	11.200	(1.113)	58	731250			87.73-	147.73	122.82	
11.200	11.200	(1.113)	57	239506			11.42-	71.42	40.23	

85	Bromodichloromethane					CAS #:	75-27-4			
11.532	11.532	(1.146)	83	1845676	51.2958	51.296	80.00-	120.00	100.00	
11.532	11.532	(1.146)	85	1170404			33.28-	93.28	63.41	

90	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.445	12.445	(1.236)	75	1293446	49.8242	49.824	80.00-	120.00	100.00	
12.445	12.445	(1.236)	77	403556			2.34-	62.34	31.20	
12.445	12.445	(1.236)	39	1392068			80.54-	140.54	107.62	

91	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.721	12.721	(1.264)	58	1261156	50.6519	50.652	80.00-	120.00	100.00	
12.721	12.721	(1.264)	43	4191997			296.95-	356.95	332.39	
12.721	12.721	(1.264)	85	335448			0.00-	57.61	26.60	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
99 Toluene						CAS #:	108-88-3		
12.942	12.942	(1.286)	91	2840038	50.8977	50.898	80.00-	120.00	100.00
12.942	12.942	(1.286)	92	1722805			28.86-	88.86	60.66

100 trans-1,3-Dichloropropene						CAS #:	10061-02-6		
13.468	13.468	(0.892)	75	1449562	50.7470	50.747	80.00-	120.00	100.00
13.468	13.468	(0.892)	77	452827			1.06-	61.06	31.24
13.468	13.468	(0.892)	39	1379718			66.05-	126.05	95.18

101 1,1,2-Trichloroethane						CAS #:	79-00-5		
13.744	13.744	(0.910)	97	944433	48.9743	48.974	80.00-	120.00	100.00
13.744	13.744	(0.910)	99	590028			31.72-	91.72	62.47
13.744	13.744	(0.910)	83	758791			52.19-	112.19	80.34

102 Tetrachloroethene						CAS #:	127-18-4		
13.799	13.799	(0.914)	166	1169576	48.4943	48.494	80.00-	120.00	100.00
13.799	13.799	(0.914)	129	924700			54.09-	114.09	79.06
13.799	13.799	(0.914)	131	909075			52.34-	112.34	77.73

103 2-Hexanone						CAS #:	591-78-6		
14.131	14.131	(0.936)	58	1701830	47.1980	47.198	80.00-	120.00	100.00
14.131	14.131	(0.936)	43	4059070			204.79-	264.79	238.51
14.131	14.131	(0.936)	100	205885			0.00-	42.78	12.10

105 Dibromochloromethane						CAS #:	124-48-1		
14.297	14.297	(0.947)	129	1561225	49.7308	49.731	80.00-	120.00	100.00
14.297	14.297	(0.947)	127	1212556			48.77-	108.77	77.67

106 1,2-Dibromoethane						CAS #:	106-93-4		
14.463	14.463	(0.958)	107	1400509	47.5171	47.517	80.00-	120.00	100.00
14.463	14.463	(0.958)	109	1321879			62.51-	122.51	94.39

109 Chlorobenzene						CAS #:	108-90-7		
15.154	15.154	(1.004)	112	2159699	46.3899	46.390	80.00-	120.00	100.00
15.154	15.154	(1.004)	114	675757			2.97-	62.97	31.29
15.154	15.154	(1.004)	77	1399699			34.70-	94.70	64.81

111 Ethyl Benzene						CAS #:	100-41-4		
15.265	15.265	(1.011)	106	1144210	50.0113	50.011	80.00-	120.00	100.00
15.265	15.265	(1.011)	91	4013568			322.22-	382.22	350.77

113 m,p-Xylene						CAS #:	108-38-3		
15.431	15.431	(1.022)	106	1399608	46.9872	46.987	80.00-	120.00	100.00
15.431	15.431	(1.022)	91	3256875			202.98-	262.98	232.70

114 o-Xylene						CAS #:	95-47-6		
15.956	15.956	(1.057)	106	1347025	47.8185	47.818	80.00-	120.00	100.00

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	3254697			210.36- 270.36	241.62	

115 Styrene CAS #: 100-42-5									
16.011	16.011	(1.060)	104	2142520	52.0365	52.036	80.00- 120.00	100.00	
16.011	16.011	(1.060)	78	1282063			31.61- 91.61	59.84	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	1397096	51.9281	51.928	80.00- 120.00	100.00	
16.260	16.260	(1.077)	171	713676			21.89- 81.89	51.08	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	2016866	45.8390	45.839	80.00- 120.00	100.00	
16.896	16.896	(1.119)	85	1315247			35.56- 95.56	65.21	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	4879392	50.4481	50.448	80.00- 120.00	100.00	
17.062	17.062	(1.130)	120	1412960			0.00- 58.00	28.96	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	4001483	49.3427	49.343	80.00- 120.00	100.00	
17.145	17.145	(1.135)	120	1829481			16.58- 76.58	45.72	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	4285275	49.2156	49.216	80.00- 120.00	100.00	
17.532	17.532	(1.161)	120	1799437			13.06- 73.06	41.99	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	2541505	44.5306	44.531	80.00- 120.00	100.00	
17.836	17.836	(1.181)	148	1663398			33.12- 93.12	65.45	
17.836	17.836	(1.181)	111	1198332			15.78- 75.78	47.15	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	2106072	46.6644	46.664	80.00- 120.00	100.00	
17.919	17.919	(1.187)	148	1337569			34.33- 94.33	63.51	
17.919	17.919	(1.187)	111	982215			18.49- 78.49	46.64	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.057	18.057	(1.196)	91	3955552	52.5311	52.531	80.00- 120.00	100.00	
18.057	18.057	(1.196)	126	660353			0.00- 47.06	16.69	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	2607052	44.0355	44.035	80.00- 120.00	100.00	
18.279	18.279	(1.211)	148	1600083			33.74- 93.74	61.38	
18.279	18.279	(1.211)	111	1182260			15.34- 75.34	45.35	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #:	120-82-1		
19.578	19.578	(1.297)	180	1707198	41.0049	41.005	80.00-	120.00	100.00
19.578	19.578	(1.297)	182	1691728			65.13-	125.13	99.09

155	Hexachlorobutadiene					CAS #:	87-68-3		
19.661	19.661	(1.302)	225	1416907	41.0683	41.068	80.00-	120.00	100.00
19.661	19.661	(1.302)	223	909647			29.70-	89.70	64.20

124	Propylbenzene					CAS #:	103-65-1		
16.924	16.924	(1.121)	91	5651398	50.5016	50.502	80.00-	120.00	100.00
16.924	16.924	(1.121)	120	1193922			0.00-	50.53	21.13
16.924	16.924	(1.121)	105	199897			0.00-	33.52	3.54

119	Cumene					CAS #:	98-82-8		
16.426	16.426	(1.088)	105	4346404	50.5012	50.501	80.00-	120.00	100.00
16.426	16.426	(1.088)	120	1127154			0.00-	55.50	25.93
16.426	16.426	(1.088)	51	974611			0.00-	50.84	22.42

156	Naphthalene					CAS #:	91-20-3		
19.744	19.744	(1.308)	128	4747848	38.4160	38.416	80.00-	120.00	100.00
19.744	19.744	(1.308)	127	612458			0.00-	42.90	12.90

30	Isopentane					CAS #:	78-78-4		
3.514	3.514	(0.429)	43	3633174	48.8965	48.896	80.00-	120.00	100.00
3.514	3.514	(0.429)	57	2156441			30.33-	90.33	59.35
3.514	3.514	(0.429)	72	171680			0.00-	34.69	4.73

21	Butane					CAS #:	106-97-8		
2.740	2.767	(0.335)	58	601819	49.6493	49.649	80.00-	120.00	100.00
2.740	2.740	(0.335)	43	4717176			773.30-	833.30	783.82

96	Methyl Cyclohexane					CAS #:	108-87-2		
10.703	10.703	(1.063)	83	1670135	48.4902	48.490	80.00-	120.00	100.00
10.703	10.703	(1.063)	98	855898			20.58-	80.58	51.25
10.703	10.703	(1.063)	55	2526188			125.23-	185.23	151.26

Report Date: 30-May-2007 15:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052921.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: LCS

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	328581	4.72
79 1,4-Difluorobenze	1277249	766349	1788149	1294035	1.31
108 Chlorobenzene-d5	1008759	605255	1412263	1016588	0.78

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.


RECOVERY REPORT

Client Name: Client SDG: 5-29may
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: ICAL Client Smp ID: LCS
 Level: LOW Operator: JG
 Data Type: MS DATA SampleType: LCS
 SpikeList File: 2926Spectra.spk Quant Type: ISTD
 Sublist File: AT04+ENSR.sub
 Method File: /chem/msd5.i/5-29may.b/t14q529a.m
 Misc Info: 200ppbv -> 50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
2 Dichlorodifluorome	50.000	48.765	97.53	70-130
3 Freon 114	50.000	50.017	100.03	70-130
4 Chloromethane	50.000	47.224	94.45	70-130
5 Vinyl Chloride	50.000	53.634	107.27	70-130
6 1,3-Butadiene	50.000	51.722	103.44	60-140
7 Bromomethane	50.000	52.113	104.23	70-130
8 Chloroethane	50.000	51.539	103.08	70-130
9 Trichlorofluoromet	50.000	50.739	101.48	70-130
13 Ethanol	50.000	55.551	111.10	60-140
19 Freon 113	50.000	56.984	113.97	70-130
20 1,1-Dichloroethene	50.000	54.998	110.00	70-130
25 Carbon Disulfide	50.000	50.371	100.74	60-140
22 Acetone	50.000	48.953	97.91	60-140
26 2-Propanol	50.000	47.863	95.73	60-140
28 3-Chloropropene	50.000	48.340	96.68	60-140
29 Methylene Chloride	50.000	52.937	105.87	70-130
31 MTBE	50.000	46.463	92.93	60-140
32 trans-1,2-Dichloro	50.000	48.055	96.11	60-140
38 Hexane	50.000	47.954	95.91	60-140
43 1,1-Dichloroethane	50.000	51.020	102.04	70-130
52 cis-1,2-Dichloroet	50.000	49.163	98.33	70-130
53 2-Butanone	50.000	49.365	98.73	60-140
56 Tetrahydrofuran	50.000	45.325	90.65	60-140
58 Chloroform	50.000	50.184	100.37	70-130
61 Cyclohexane	50.000	48.778	97.56	60-140
62 1,1,1-Trichloroeth	50.000	48.824	97.65	70-130
63 Vinyl Acetate	50.000	51.440	102.88	60-140
65 Carbon Tetrachlori	50.000	49.218	98.44	70-130
68 2,2,4-Trimethylpen	50.000	48.703	97.41	60-140
69 Benzene	50.000	48.108	96.22	70-130
72 1,2-Dichloroethane	50.000	51.289	102.58	70-130
75 Heptane	50.000	43.871	87.74	60-140
80 Trichloroethene	50.000	48.893	97.79	70-130

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
82 1,2-Dichloropropan	50.000	48.543	97.09	70-130
84 1,4-Dioxane	50.000	45.712	91.42	60-140
85 Bromodichlorometha	50.000	51.296	102.59	60-140
90 cis-1,3-Dichloropr	50.000	49.824	99.65	70-130
91 4-Methyl-2-pentano	50.000	50.652	101.30	60-140
99 Toluene	50.000	50.898	101.80	70-130
100 trans-1,3-Dichloro	50.000	50.747	101.49	70-130
101 1,1,2-Trichloroeth	50.000	48.974	97.95	70-130
102 Tetrachloroethene	50.000	48.494	96.99	70-130
103 2-Hexanone	50.000	47.198	94.40	60-140
105 Dibromochlorometha	50.000	49.731	99.46	60-140
106 1,2-Dibromoethane	50.000	47.517	95.03	70-130
109 Chlorobenzene	50.000	46.390	92.78	70-130
111 Ethyl Benzene	50.000	50.011	100.02	70-130
113 m,p-Xylene	50.000	46.987	93.97	70-130
114 o-Xylene	50.000	47.818	95.64	70-130
115 Styrene	50.000	52.036	104.07	70-130
118 Bromoform	50.000	51.928	103.86	60-140
119 Cumene	50.000	50.501	101.00	60-140
123 1,1,2,2-Tetrachlor	50.000	45.839	91.68	70-130
124 Propylbenzene	50.000	50.502	101.00	60-140
126 4-Ethyltoluene	50.000	50.448	100.90	60-140
128 1,3,5-Trimethylben	50.000	49.343	98.69	70-130
131 1,2,4-Trimethylben	50.000	49.216	98.43	70-130
138 1,3-Dichlorobenzen	50.000	44.531	89.06	70-130
141 1,4-Dichlorobenzen	50.000	46.664	93.33	70-130
143 alpha-Chlorotoluen	50.000	52.531	105.06	70-130
146 1,2-Dichlorobenzen	50.000	44.035	88.07	70-130
154 1,2,4-Trichloroben	50.000	41.005	82.01	70-130
155 Hexachlorobutadien	50.000	41.068	82.14	70-130
1 Propylene	50.000	50.959	101.92	70-130
156 Naphthalene	50.000	38.416	76.83	60-140
21 Butane	50.000	49.649	99.30	70-130
30 Isopentane	50.000	48.896	97.79	70-130
96 Methyl Cyclohexane	50.000	48.490	96.98	70-130

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 71 1,2-Dichloroethane	25.000	24.045	96.18	70-130
\$ 97 Toluene-d8	25.000	25.209	100.84	70-130
\$ 122 Bromofluorobenzene	25.000	24.744	98.98	70-130

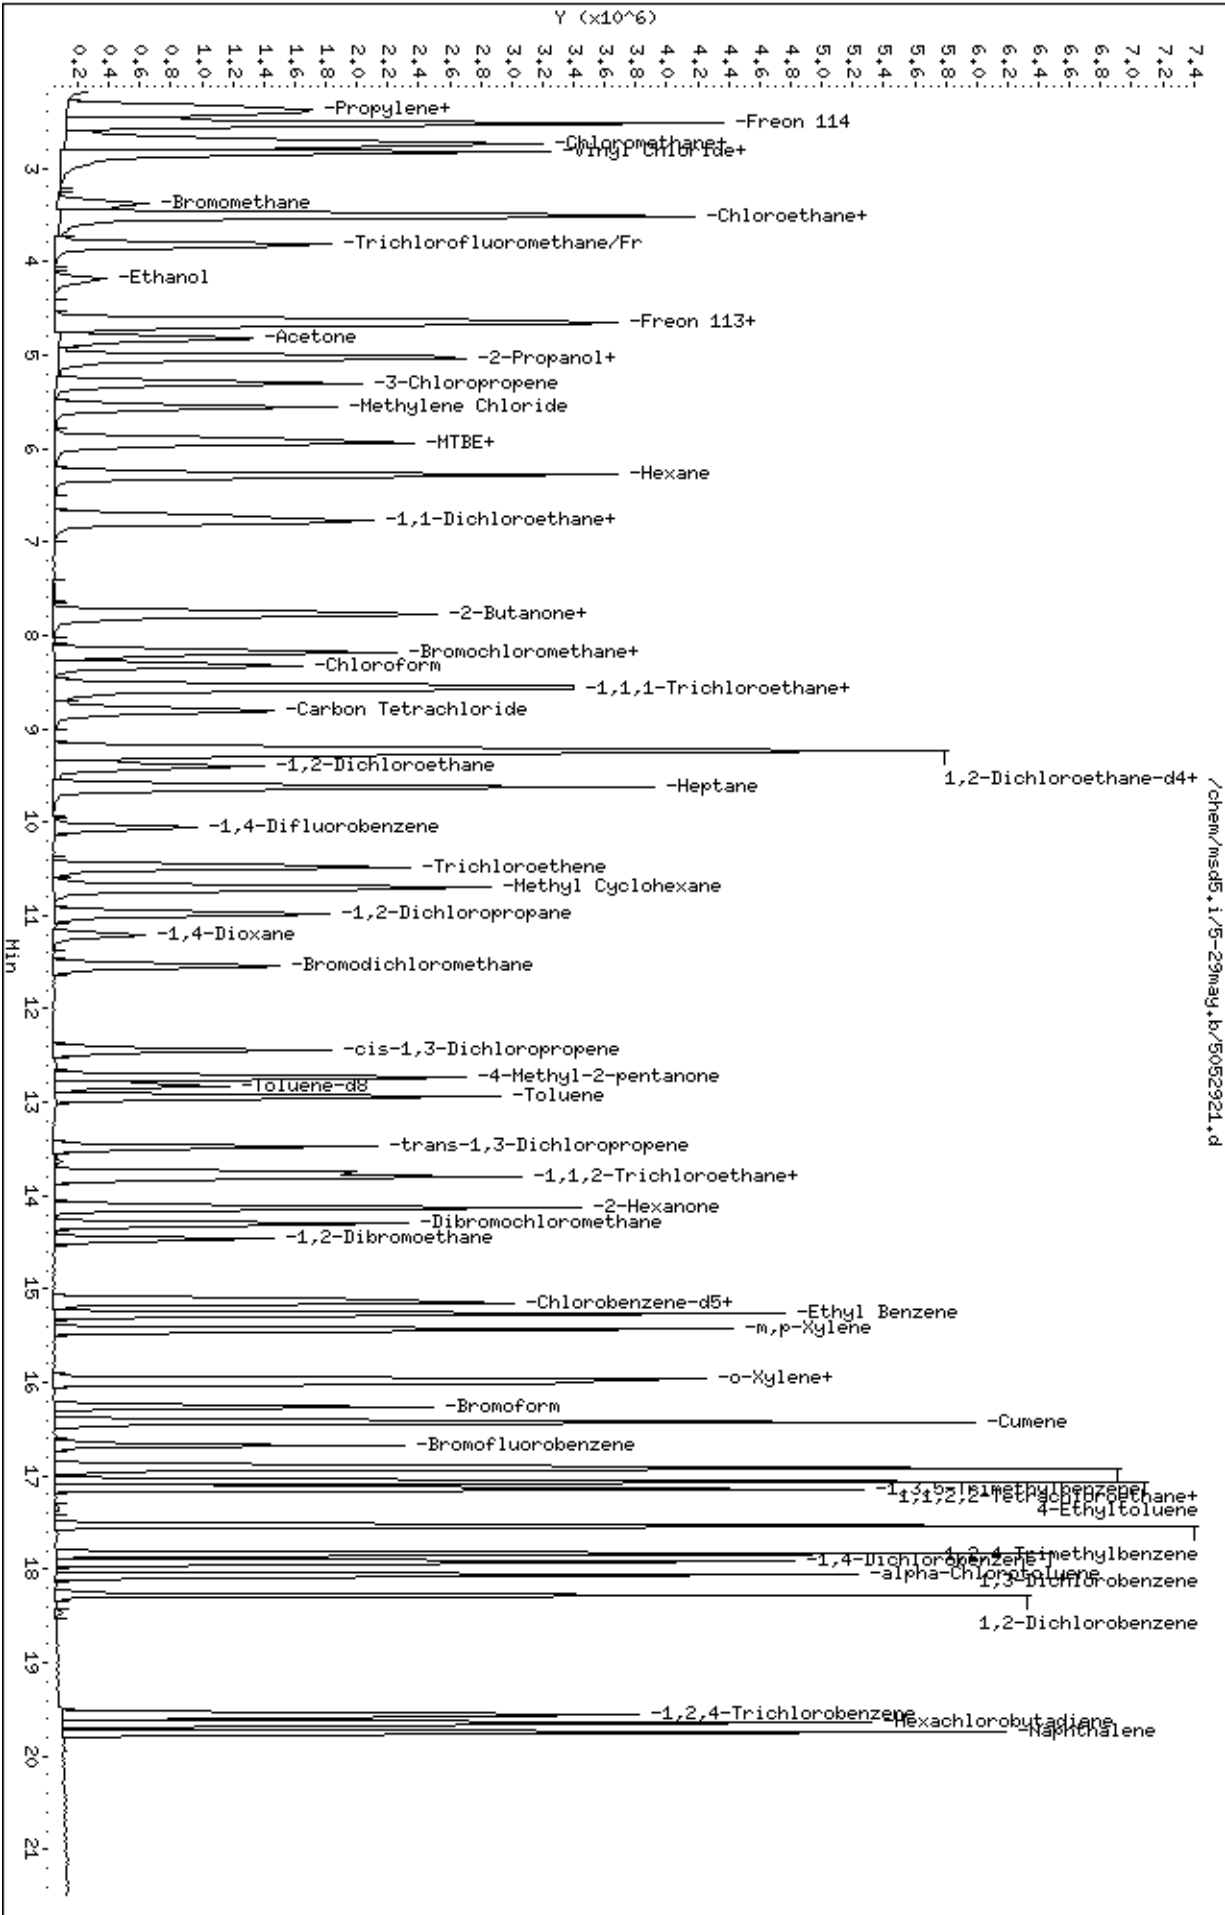

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052911.d
 Lab Smp Id: ICAL Client Smp ID: Level 1
 Inj Date : 29-MAY-2007 15:42
 Operator : JG Inst ID: msd5.i
 Smp Info : 0.3mL #1487-288
 Misc Info : 200ppbv-0.3ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 15:42 Cal File: 5052911.d
 Als bottle: 1 Calibration Sample, Level: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AFCEElow.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

* 57	Bromochloromethane					CAS #:	74-97-5	
8.187	8.187	(1.000)	130	321276	25.0000		70.00- 130.00	100.00
8.187	8.187	(1.000)	128	254210			50.27- 110.27	79.13
8.187	8.187	(1.000)	49	965206			281.04- 341.04	300.43

* 79	1,4-Difluorobenzene					CAS #:	540-36-3	
10.067	10.067	(1.000)	114	1271328	25.0000		70.00- 130.00	100.00
10.067	10.067	(1.000)	88	230292			0.00- 48.57	18.11

* 108	Chlorobenzene-d5					CAS #:	3114-55-4	
15.099	15.099	(1.000)	117	1006780	25.0000		70.00- 130.00	100.00
15.099	15.099	(1.000)	82	644412			0.00- 30.00	64.01

\$ 71	1,2-Dichloroethane-d4					CAS #:	17060-07-0	
9.265	9.265	(1.132)	65	625671	25.0000	24.294	70.00- 130.00	100.00
9.265	9.265	(1.132)	67	271934			0.00- 30.00	43.46

\$ 97	Toluene-d8					CAS #:	2037-26-5	
12.832	12.832	(1.275)	98	1162897	25.0000	25.130	70.00- 130.00	100.00
12.832	12.832	(1.275)	70	128701			0.00- 30.00	11.07

AMOUNTS

CAL-AMT ON-COL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

\$ 97 Toluene-d8 (continued)

12.832 12.832 (1.275) 100 733968 0.00- 30.00 63.12

\$ 122 Bromofluorobenzene

CAS #: 460-00-4

16.675 16.675 (1.104) 174 628671 25.0000 24.853 70.00- 130.00 100.00

16.675 16.675 (1.104) 95 995730 131.53- 191.53 158.39

16.675 16.675 (1.104) 176 574568 65.40- 125.40 91.39

58 Chloroform

CAS #: 67-66-3

8.325 8.325 (1.017) 83 10149 0.30000 0.2590 70.00- 130.00 100.00

8.325 8.325 (1.017) 85 7818 33.68- 93.68 77.03

69 Benzene

CAS #: 71-43-2

9.237 9.237 (0.918) 78 17129 0.30000 0.3001 70.00- 130.00 100.00

9.237 9.237 (0.918) 77 4953 0.00- 30.00 28.92

115 Styrene

CAS #: 100-42-5

16.012 16.012 (1.060) 104 9083 0.30000 0.2228 70.00- 130.00 100.00

16.012 16.012 (1.060) 78 7332 31.61- 91.61 80.72

119 Cumene

CAS #: 98-82-8

16.426 16.426 (1.088) 105 19541 0.30000 0.2293 70.00- 130.00 100.00

16.426 16.426 (1.088) 120 5426 0.00- 30.00 27.77

16.426 16.426 (1.088) 51 7370 0.00- 30.00 37.72

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052911.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-0.3ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	321276	2.39
79 1,4-Difluorobenze	1277249	766349	1788149	1271328	-0.46
108 Chlorobenzene-d5	1008759	605255	1412263	1006780	-0.20

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-29maj.b/5052911.d

Date: 29-MAY-2007 15:42

Client ID: Level 1

Sample Info: 0.3mL #1487-288


Column phase: RTX-624

Instrument: msd5.1

Operator: JG

Column diameter: 0.53

/chem/msd5.1/5-29maj.b/5052911.d

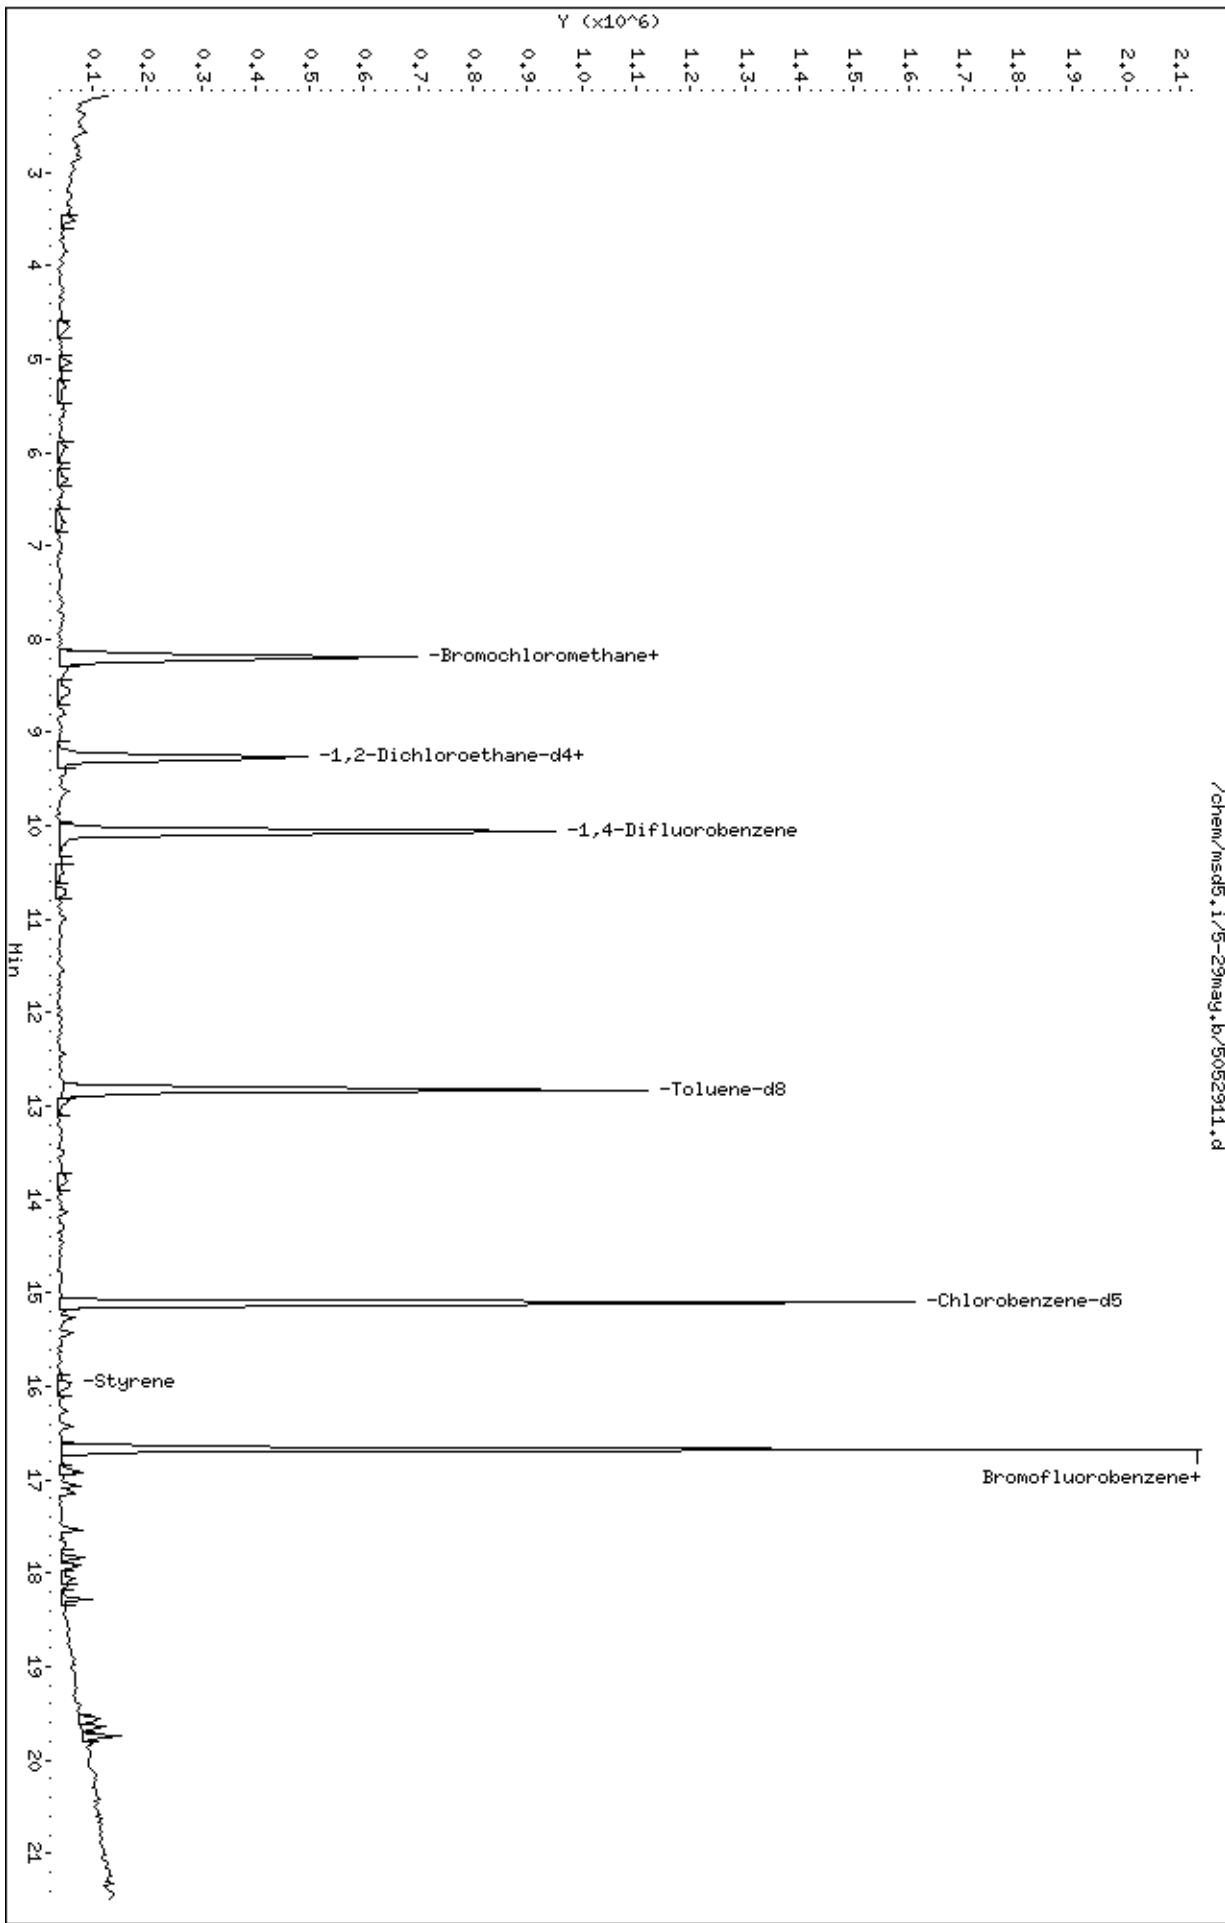

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052912.d
 Lab Smp Id: ICAL Client Smp ID: Level 2
 Inj Date : 29-MAY-2007 16:10
 Operator : JG Inst ID: msd5.i
 Smp Info : 0.5mL #1487-288
 Misc Info : 200ppbv-0.5ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 16:10 Cal File: 5052912.d
 Als bottle: 1 Calibration Sample, Level: 2
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04Low+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 57 Bromochloromethane CAS #: 74-97-5									
8.187	8.187	(1.000)	130	320227	25.0000			70.00- 130.00	100.00
8.187	8.187	(1.000)	128	242343				50.27- 110.27	75.68
8.187	8.187	(1.000)	49	989401				281.04- 341.04	308.97

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	1280514	25.0000			70.00- 130.00	100.00
10.067	10.067	(1.000)	88	225538				0.00- 48.57	17.61

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	1002266	25.0000			70.00- 130.00	100.00
15.099	15.099	(1.000)	82	636566				0.00- 30.00	63.51

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.132)	65	608358	25.0000	23.699		70.00- 130.00	100.00
9.265	9.265	(1.132)	67	275344				0.00- 30.00	45.26

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	1131826	25.0000	24.283		70.00- 130.00	100.00
12.832	12.832	(1.275)	70	133637				0.00- 30.00	11.81

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 97 Toluene-d8 (continued)									
12.832	12.832	(1.275)	100	718153			0.00- 30.00	63.45	

\$ 122 Bromofluorobenzene CAS #: 460-00-4									
16.675	16.675	(1.104)	174	608252	25.0000	24.154	70.00- 130.00	100.00	
16.675	16.675	(1.104)	95	993460			131.53- 191.53	163.33	
16.675	16.675	(1.104)	176	565354			65.40- 125.40	92.95	

2 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.408	2.408	(0.294)	85	23887	0.50000	0.4204	70.00- 130.00	100.00(a)	
2.436	2.436	(0.298)	87	10725			0.00- 30.00	44.90	

3 Freon 114 CAS #: 76-14-2									
2.574	2.574	(0.314)	135	23575	0.50000	0.4339	70.00- 130.00	100.00(a)	
2.574	2.574	(0.314)	137	6815			0.80- 60.80	28.91	

5 Vinyl Chloride CAS #: 75-01-4									
2.850	2.850	(0.348)	62	16097	0.50000	0.3859	70.00- 130.00	100.00(a)	
2.823	2.823	(0.345)	64	2335			0.00- 30.00	14.51	

6 1,3-Butadiene CAS #: 106-99-0									
2.850	2.850	(0.348)	54	15909	0.50000	0.3842	70.00- 130.00	100.00(a)	
2.823	2.823	(0.345)	39	19757			0.00- 30.00	124.19	

7 Bromomethane CAS #: 74-83-9									
3.376	3.376	(0.412)	94	10699	0.50000	0.4318	70.00- 130.00	100.00(a)	
3.376	3.376	(0.412)	96	11343			64.95- 124.95	106.02	

8 Chloroethane CAS #: 75-00-3									
3.542	3.542	(0.433)	64	10708	0.50000	0.4841	70.00- 130.00	100.00(aM)	
3.514	3.514	(0.429)	49	2538			0.00- 30.00	23.70	
3.542	3.542	(0.433)	66	2672			0.00- 30.00	24.95	

9 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
3.846	3.846	(0.470)	101	21790	0.50000	0.3805	70.00- 130.00	100.00(a)	
3.846	3.846	(0.470)	103	14799			35.72- 95.72	67.92	

19 Freon 113 CAS #: 76-13-1									
4.648	4.648	(0.568)	151	15909	0.50000	0.4537	70.00- 130.00	100.00(a)	
4.675	4.675	(0.571)	153	9623			32.16- 92.16	60.49	
4.648	4.648	(0.568)	101	17694			100.00- 160.00	111.22	

20 1,1-Dichloroethene CAS #: 75-35-4									
4.675	4.675	(0.571)	61	22963	0.50000	0.4200	70.00- 130.00	100.00(a)	
4.703	4.703	(0.574)	96	13121			19.13- 79.13	57.14	
4.675	4.675	(0.571)	98	8419			0.28- 60.28	36.66	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

25	Carbon Disulfide					CAS #: 75-15-0			
5.035	5.035	(0.615)	76	31324	0.50000	0.4161	70.00- 130.00	100.00(a)	

29	Methylene Chloride					CAS #: 75-09-2			
5.560	5.560	(0.679)	49	25089	0.50000	0.4892	70.00- 130.00	100.00(a)	
5.560	5.560	(0.679)	84	12478			9.87- 69.87	49.73	
5.588	5.588	(0.683)	51	11156			0.00- 30.00	44.47	

31	MTBE					CAS #: 1634-04-4			
5.892	5.892	(0.720)	73	17321	0.50000	0.4329	70.00- 130.00	100.00(a)	
5.892	5.892	(0.720)	57	10505			5.77- 65.77	60.65	
5.892	5.892	(0.720)	41	11670			0.00- 30.00	67.37	

32	trans-1,2-Dichloroethene					CAS #: 156-60-5			
5.947	5.947	(0.726)	96	11955	0.50000	0.4385	70.00- 130.00	100.00(a)	
5.947	5.947	(0.726)	61	22533			164.17- 224.17	188.48	
5.947	5.947	(0.726)	98	8954			0.00- 30.00	74.90	

38	Hexane					CAS #: 110-54-3			
6.279	6.279	(0.767)	57	30616	0.50000	0.4466	70.00- 130.00	100.00(a)	
6.307	6.307	(0.770)	43	19399			0.00- 30.00	63.36	
6.279	6.279	(0.767)	86	2664			0.00- 30.00	8.70	

43	1,1-Dichloroethane					CAS #: 75-34-3			
6.749	6.749	(0.824)	63	21051	0.50000	0.3860	70.00- 130.00	100.00(a)	
6.721	6.721	(0.821)	65	8949			0.00- 59.00	42.51	

53	2-Butanone					CAS #: 78-93-3			
7.827	7.827	(0.956)	72	4602	0.50000	0.4368	70.00- 130.00	100.00(a)	
7.827	7.827	(0.956)	43	30590			796.36- 856.36	664.71	
7.800	7.800	(0.953)	57	3193			0.00- 30.00	69.38	

52	cis-1,2-Dichloroethene					CAS #: 156-59-2			
7.772	7.772	(0.949)	61	19035	0.50000	0.4494	70.00- 130.00	100.00(a)	
7.772	7.772	(0.949)	96	8942			25.31- 85.31	46.98	
7.744	7.744	(0.946)	98	6446			2.88- 62.88	33.86	

56	Tetrahydrofuran					CAS #: 109-99-9			
8.187	8.187	(1.000)	42	25795	0.50000	0.4721	70.00- 130.00	100.00(a)	
8.187	8.187	(1.000)	71	5366			0.00- 48.47	20.80	
8.187	8.187	(1.000)	72	6815			0.00- 30.00	26.42	

58	Chloroform					CAS #: 67-66-3			
8.325	8.325	(1.017)	83	18550	0.50000	0.4748	70.00- 130.00	100.00(a)	
8.325	8.325	(1.017)	85	13138			33.68- 93.68	70.82	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

62	1,1,1-Trichloroethane					CAS #:	71-55-6			
8.574	8.574	(1.047)	97	18607	0.50000	0.4373	70.00-	130.00	100.00(a)	
8.574	8.574	(1.047)	99	9899			32.24-	92.24	53.20	

61	Cyclohexane					CAS #:	110-82-7			
8.546	8.546	(1.044)	84	10997	0.50000	0.3806	70.00-	130.00	100.00(a)	
8.546	8.546	(1.044)	56	25188			177.94-	237.94	229.04	
8.546	8.546	(1.044)	41	17561			93.55-	153.55	159.69	

65	Carbon Tetrachloride					CAS #:	56-23-5			
8.823	8.823	(1.078)	119	15647	0.50000	0.4221	70.00-	130.00	100.00(a)	
8.795	8.795	(1.074)	117	13079			71.97-	131.97	83.59	

68	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.237	9.237	(1.128)	57	65681	0.50000	0.4032	70.00-	130.00	100.00(a)	
9.237	9.237	(1.128)	56	24350			0.00-	30.00	37.07	
9.237	9.237	(1.128)	41	18060			0.00-	30.00	27.50	

69	Benzene					CAS #:	71-43-2			
9.237	9.237	(0.918)	78	26710	0.50000	0.4646	70.00-	130.00	100.00(a)	
9.237	9.237	(0.918)	77	6178			0.00-	30.00	23.13	

72	1,2-Dichloroethane					CAS #:	107-06-2			
9.403	9.403	(0.934)	62	16969	0.50000	0.4339	70.00-	130.00	100.00(a)	
9.431	9.431	(0.937)	64	7803			0.00-	30.00	45.98	

75	Heptane					CAS #:	142-82-5			
9.625	9.625	(0.956)	100	4985	0.50000	0.6380	70.00-	130.00	100.00	
9.625	9.625	(0.956)	43	26220			0.00-	30.00	525.98	
9.625	9.625	(0.956)	71	8530			0.00-	30.00	171.11	

80	Trichloroethene					CAS #:	79-01-6			
10.482	10.482	(1.041)	95	9776	0.50000	0.4056	70.00-	130.00	100.00(a)	
10.482	10.482	(1.041)	130	10501			65.35-	125.35	107.42	
10.509	10.509	(1.044)	97	7241			35.05-	95.05	74.07	

82	1,2-Dichloropropane					CAS #:	78-87-5			
10.979	10.979	(1.091)	63	10942	0.50000	0.4369	70.00-	130.00	100.00(a)	
10.979	10.979	(1.091)	62	10300			43.36-	103.36	94.13	
10.979	10.979	(1.091)	41	12824			62.33-	122.33	117.20	

85	Bromodichloromethane					CAS #:	75-27-4			
11.532	11.532	(1.146)	83	13983	0.50000	0.3927	70.00-	130.00	100.00(a)	
11.532	11.532	(1.146)	85	9417			33.28-	93.28	67.35	

90	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.445	12.445	(1.236)	75	10181	0.50000	0.3963	70.00-	130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
90 cis-1,3-Dichloropropene (continued)									
12.445	12.445	(1.236)	77	4724			2.34- 62.34	46.40	
12.445	12.445	(1.236)	39	13321			80.54- 140.54	130.84	

91 4-Methyl-2-pentanone CAS #: 108-10-1									
12.749	12.749	(1.266)	58	7913	0.50000	0.3212	70.00- 130.00	100.00(a)	
12.721	12.721	(1.264)	43	40882			0.00- 30.00	516.64	
12.721	12.721	(1.264)	85	3216			0.00- 30.00	40.64	

99 Toluene CAS #: 108-88-3									
12.943	12.943	(1.286)	91	23853	0.50000	0.4320	70.00- 130.00	100.00(a)	
12.943	12.943	(1.286)	92	16171			28.86- 88.86	67.79	

100 trans-1,3-Dichloropropene CAS #: 10061-02-6									
13.468	13.468	(0.892)	75	10192	0.50000	0.3619	70.00- 130.00	100.00(a)	
13.468	13.468	(0.892)	77	3040			1.06- 61.06	29.83	
13.468	13.468	(0.892)	39	12412			66.05- 126.05	121.78	

101 1,1,2-Trichloroethane CAS #: 79-00-5									
13.772	13.772	(0.912)	97	7570	0.50000	0.3982	70.00- 130.00	100.00(a)	
13.772	13.772	(0.912)	99	5988			31.72- 91.72	79.10	
13.744	13.744	(0.910)	83	6694			52.19- 112.19	88.43	

102 Tetrachloroethene CAS #: 127-18-4									
13.800	13.800	(0.914)	166	12288	0.50000	0.5168	70.00- 130.00	100.00	
13.800	13.800	(0.914)	129	12759			54.09- 114.09	103.83	
13.800	13.800	(0.914)	131	10780			52.34- 112.34	87.73	

105 Dibromochloromethane CAS #: 124-48-1									
14.297	14.297	(0.947)	129	13708	0.50000	0.4429	70.00- 130.00	100.00(a)	
14.297	14.297	(0.947)	127	8932			0.00- 30.00	65.16	

106 1,2-Dibromoethane CAS #: 106-93-4									
14.463	14.463	(0.958)	107	13014	0.50000	0.4478	70.00- 130.00	100.00(a)	
14.463	14.463	(0.958)	109	10566			62.51- 122.51	81.19	

109 Chlorobenzene CAS #: 108-90-7									
15.154	15.154	(1.004)	112	23229	0.50000	0.5061	70.00- 130.00	100.00	
15.154	15.154	(1.004)	114	7938			2.97- 62.97	34.17	
15.099	15.099	(1.000)	77	21831			34.70- 94.70	93.98	

111 Ethyl Benzene CAS #: 100-41-4									
15.265	15.265	(1.011)	106	7812	0.50000	0.3463	70.00- 130.00	100.00(a)	
15.265	15.265	(1.011)	91	34822			0.00- 30.00	445.75	

113 m,p-Xylene CAS #: 108-38-3									
15.431	15.431	(1.022)	106	12493	0.50000	0.4254	70.00- 130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
113 m,p-Xylene (continued)									
15.431	15.431	(1.022)	91	28543			0.00- 30.00	228.47	

114 o-Xylene CAS #: 95-47-6									
15.956	15.956	(1.057)	106	9992	0.50000	0.3598	70.00- 130.00	100.00(a)	
15.956	15.956	(1.057)	91	27995			210.36- 270.36	280.17	

115 Styrene CAS #: 100-42-5									
16.012	16.012	(1.060)	104	16015	0.50000	0.3945	70.00- 130.00	100.00(a)	
16.012	16.012	(1.060)	78	11749			31.61- 91.61	73.36	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	9708	0.50000	0.3660	70.00- 130.00	100.00(a)	
16.260	16.260	(1.077)	171	6307			21.89- 81.89	64.97	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	19546	0.50000	0.4506	70.00- 130.00	100.00(a)	
16.896	16.896	(1.119)	85	10994			35.56- 95.56	56.25	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	38045	0.50000	0.3990	70.00- 130.00	100.00(a)	
17.062	17.062	(1.130)	120	10793			0.00- 58.00	28.37	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	31915	0.50000	0.3992	70.00- 130.00	100.00(a)	
17.145	17.145	(1.135)	120	16327			0.00- 30.00	51.16	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	33871	0.50000	0.3946	70.00- 130.00	100.00(a)	
17.532	17.532	(1.161)	120	15171			13.06- 73.06	44.79	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	26253	0.50000	0.4666	70.00- 130.00	100.00(a)	
17.836	17.836	(1.181)	148	12691			0.00- 30.00	48.34	
17.836	17.836	(1.181)	111	11047			0.00- 30.00	42.08	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	18234	0.50000	0.4098	70.00- 130.00	100.00(a)	
17.919	17.919	(1.187)	148	13738			0.00- 30.00	75.34	
17.919	17.919	(1.187)	111	11777			0.00- 30.00	64.59	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.058	18.058	(1.196)	91	21416	0.50000	0.2885	70.00- 130.00	100.00(a)	
18.058	18.058	(1.196)	126	5259			0.00- 30.00	24.56	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	29578	0.50000	0.5067	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	ON-COL	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
146 1,2-Dichlorobenzene (continued)									
18.279	18.279	(1.211)	148	14247				33.74- 93.74	48.17
18.279	18.279	(1.211)	111	11347				15.34- 75.34	38.36

124 Propylbenzene CAS #: 103-65-1									
16.924	16.924	(1.121)	91	45410	0.50000	0.4116		70.00- 130.00	100.00(a)
16.924	16.924	(1.121)	120	9673				0.00- 30.00	21.30
16.924	16.924	(1.121)	105	3079				0.00- 30.00	6.78

119 Cumene CAS #: 98-82-8									
16.426	16.426	(1.088)	105	36572	0.50000	0.4310		70.00- 130.00	100.00(a)
16.426	16.426	(1.088)	120	7574				0.00- 30.00	20.71
16.426	16.426	(1.088)	51	10237				0.00- 30.00	27.99

96 Methyl Cyclohexane CAS #: 108-87-2									
10.703	10.703	(1.063)	83	15269	0.50000	0.4480		70.00- 130.00	100.00(a)
10.703	10.703	(1.063)	98	8344				0.00- 30.00	54.65
10.703	10.703	(1.063)	55	20506				0.00- 30.00	134.30

QC Flag Legend

- a - Target compound detected but, quantitated amount Below Limit Of Quantitation(BLOQ).
- M - Compound response manually integrated.

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052912.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-0.5ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	320227	2.06
79 1,4-Difluorobenze	1277249	766349	1788149	1280514	0.26
108 Chlorobenzene-d5	1008759	605255	1412263	1002266	-0.64

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-29maj.b/5052912.d

Date: 29-May-2007 16:10

Client ID: Level 2

Sample Info: 0.5mL #1487-288


Column phase: RTX-624

Instrument: msd5.1

Operator: JG

Column diameter: 0.53

/chem/msd5.1/5-29maj.b/5052912.d

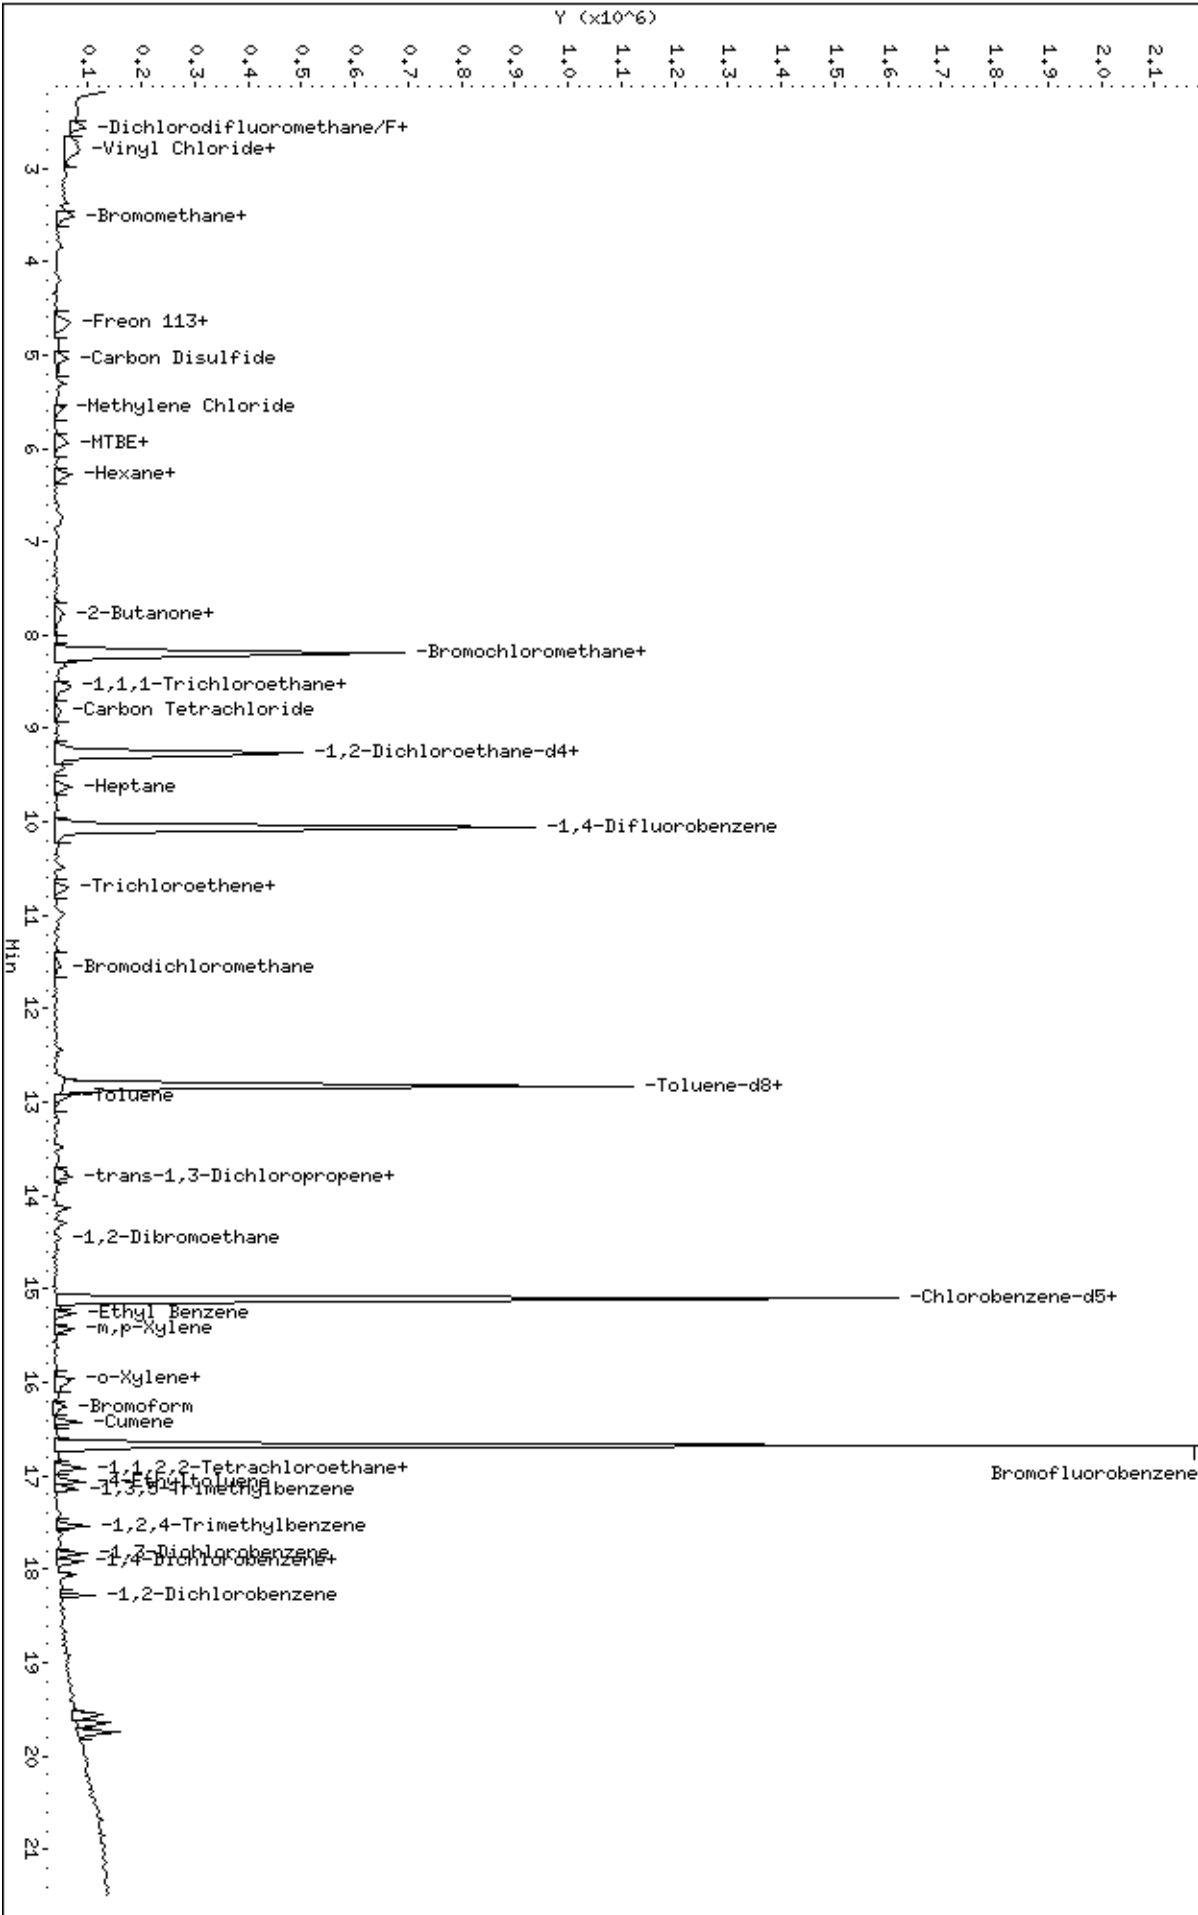

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052920.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 29-MAY-2007 20:44
 Operator : JG Inst ID: msd5.i
 Smp Info : 2.0mL #1487-288
 Misc Info : 200ppbv-2.0ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 57 Bromochloromethane CAS #: 74-97-5									
8.187	8.187	(1.000)	130	316096	25.0000			70.00- 130.00	100.00
8.187	8.187	(1.000)	128	247135				50.32- 110.32	78.18
8.187	8.187	(1.000)	49	960997				291.93- 351.93	304.02

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	1251763	25.0000			70.00- 130.00	100.00
10.067	10.067	(1.000)	88	223571				0.00- 47.76	17.86

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	961284	25.0000			70.00- 130.00	100.00
15.099	15.099	(1.000)	82	600538				33.54- 93.54	62.47

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.132)	65	617065	25.0000	24.352		70.00- 130.00	100.00
9.265	9.265	(1.132)	67	276389				25.98- 85.98	44.79

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	1134629	25.0000	24.903		70.00- 130.00	100.00
12.832	12.832	(1.275)	70	126127				0.00- 41.05	11.12

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 97 Toluene-d8 (continued)									
12.832	12.832	(1.275)	100	735073			36.04- 96.04	64.79	

\$ 122 Bromofluorobenzene CAS #: 460-00-4									
16.675	16.675	(1.104)	174	596682	25.0000	24.705	70.00- 130.00	100.00	
16.675	16.675	(1.104)	95	983772			139.49- 199.49	164.87	
16.675	16.675	(1.104)	176	580470			69.76- 129.76	97.28	

1 Propylene CAS #: 115-07-1									
2.353	2.353	(0.287)	41	103421	2.00000	2.453	70.00- 130.00	100.00	
2.353	2.353	(0.287)	42	71432			36.96- 96.96	69.07	
2.353	2.353	(0.287)	39	67277			37.69- 97.69	65.05	

2 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.408	2.408	(0.294)	85	148565	2.00000	2.649	70.00- 130.00	100.00	
2.408	2.408	(0.294)	87	48870			1.62- 61.62	32.89	

3 Freon 114 CAS #: 76-14-2									
2.574	2.574	(0.314)	135	133313	2.00000	2.485	70.00- 130.00	100.00	
2.574	2.574	(0.314)	137	39543			1.52- 61.52	29.66	

4 Chloromethane CAS #: 74-87-3									
2.712	2.712	(0.331)	50	121601	2.00000	2.402	70.00- 130.00	100.00	
2.712	2.712	(0.331)	52	38677			0.00- 59.51	31.81	

5 Vinyl Chloride CAS #: 75-01-4									
2.850	2.850	(0.348)	62	94018	2.00000	2.283	70.00- 130.00	100.00	
2.850	2.850	(0.348)	64	38541			0.00- 59.15	40.99	

6 1,3-Butadiene CAS #: 106-99-0									
2.850	2.850	(0.348)	54	100057	2.00000	2.448	70.00- 130.00	100.00	
2.850	2.850	(0.348)	39	153795			92.11- 152.11	153.71	

7 Bromomethane CAS #: 74-83-9									
3.376	3.376	(0.412)	94	59516	2.00000	2.433	70.00- 130.00	100.00	
3.376	3.376	(0.412)	96	54357			64.13- 124.13	91.33	

8 Chloroethane CAS #: 75-00-3									
3.569	3.569	(0.436)	64	51793	2.00000	2.372	70.00- 130.00	100.00	
3.569	3.569	(0.436)	49	16946			1.83- 61.83	32.72	
3.541	3.541	(0.433)	66	14824			0.00- 57.39	28.62	

9 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
3.846	3.846	(0.470)	101	143306	2.00000	2.535	70.00- 130.00	100.00	
3.846	3.846	(0.470)	103	89746			34.13- 94.13	62.63	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
13 Ethanol						CAS #: 64-17-5			
4.205	4.205	(0.514)	45	40839	2.00000	2.355	70.00- 130.00	100.00	
4.205	4.205	(0.514)	43	12359			0.00- 49.45	30.26	
4.177	4.177	(0.510)	46	16246			11.95- 71.95	39.78	

19 Freon 113						CAS #: 76-13-1			
4.647	4.647	(0.568)	151	78812	2.00000	2.277	70.00- 130.00	100.00	
4.647	4.647	(0.568)	153	55161			33.02- 93.02	69.99	
4.647	4.647	(0.568)	101	110743			99.23- 159.23	140.52	

20 1,1-Dichloroethene						CAS #: 75-35-4			
4.675	4.675	(0.571)	61	133584	2.00000	2.475	70.00- 130.00	100.00	
4.675	4.675	(0.571)	96	65366			16.83- 76.83	48.93	
4.675	4.675	(0.571)	98	38535			0.21- 60.21	28.85	

22 Acetone						CAS #: 67-64-1			
4.841	4.841	(0.591)	58	47377	2.00000	2.353	70.00- 130.00	100.00	
4.841	4.841	(0.591)	43	157055			327.94- 387.94	331.50	

26 2-Propanol						CAS #: 67-63-0			
5.035	5.035	(0.615)	45	229326	2.00000	2.614	70.00- 130.00	100.00	
5.035	5.035	(0.615)	43	56842			0.00- 49.24	24.79	
5.062	5.062	(0.618)	59	7792			0.00- 33.25	3.40	

25 Carbon Disulfide						CAS #: 75-15-0			
5.035	5.035	(0.615)	76	182149	2.00000	2.451	70.00- 130.00	100.00	

28 3-Chloropropene						CAS #: 107-05-1			
5.311	5.311	(0.649)	76	28388	2.00000	2.261	70.00- 130.00	100.00	
5.311	5.311	(0.649)	41	145705			480.64- 540.64	513.26	

29 Methylene Chloride						CAS #: 75-09-2			
5.560	5.560	(0.679)	49	112605	2.00000	2.224	70.00- 130.00	100.00	
5.588	5.588	(0.683)	84	51772			11.41- 71.41	45.98	
5.588	5.588	(0.683)	51	41098			0.00- 59.58	36.50	

31 MTBE						CAS #: 1634-04-4			
5.892	5.892	(0.720)	73	63501	2.00000	1.608	70.00- 130.00	100.00	
5.892	5.892	(0.720)	57	25359			8.02- 68.02	39.93	
5.919	5.919	(0.723)	41	24865			10.34- 70.34	39.16	

32 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.947	5.947	(0.726)	96	65020	2.00000	2.416	70.00- 130.00	100.00	
5.947	5.947	(0.726)	61	125850			163.30- 223.30	193.56	
5.947	5.947	(0.726)	98	40670			32.40- 92.40	62.55	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
38 Hexane						CAS #:	110-54-3			
6.279	6.279	(0.767)	57	166678	2.00000	2.463	70.00-	130.00	100.00	
6.279	6.279	(0.767)	43	114670			46.14-	106.14	68.80	
6.306	6.306	(0.770)	86	20312			0.00-	41.50	12.19	

43 1,1-Dichloroethane						CAS #:	75-34-3			
6.721	6.721	(0.821)	63	133534	2.00000	2.481	70.00-	130.00	100.00	
6.749	6.749	(0.824)	65	36083			0.00-	58.49	27.02	

53 2-Butanone						CAS #:	78-93-3			
7.800	7.800	(0.953)	72	24181	2.00000	2.325	70.00-	130.00	100.00	
7.800	7.800	(0.953)	43	203952			783.34-	843.34	843.44	
7.800	7.800	(0.953)	57	13069			23.20-	83.20	54.05	

52 cis-1,2-Dichloroethene						CAS #:	156-59-2			
7.772	7.772	(0.949)	61	100319	2.00000	2.400	70.00-	130.00	100.00	
7.772	7.772	(0.949)	96	56182			23.43-	83.43	56.00	
7.772	7.772	(0.949)	98	33485			4.05-	64.05	33.38	

56 Tetrahydrofuran						CAS #:	109-99-9			
8.187	8.187	(1.000)	42	145723	2.00000	2.702	70.00-	130.00	100.00	
8.187	8.187	(1.000)	71	25088			0.00-	48.28	17.22	
8.187	8.187	(1.000)	72	23711			0.00-	49.73	16.27	

58 Chloroform						CAS #:	67-66-3			
8.325	8.325	(1.017)	83	91231	2.00000	2.366	70.00-	130.00	100.00	
8.325	8.325	(1.017)	85	58564			35.36-	95.36	64.19	

62 1,1,1-Trichloroethane						CAS #:	71-55-6			
8.574	8.574	(1.047)	97	99793	2.00000	2.376	70.00-	130.00	100.00	
8.574	8.574	(1.047)	99	61069			34.25-	94.25	61.20	

61 Cyclohexane						CAS #:	110-82-7			
8.546	8.546	(1.044)	84	71745	2.00000	2.515	70.00-	130.00	100.00	
8.546	8.546	(1.044)	56	139115			178.96-	238.96	193.90	
8.546	8.546	(1.044)	41	86037			98.39-	158.39	119.92	

63 Vinyl Acetate						CAS #:	108-05-4			
6.804	6.804	(0.831)	86	12271	2.00000	1.957	70.00-	130.00	100.00(a)	
6.804	6.804	(0.831)	43	232470			1767.50-	1827.50	1894.47	
6.804	6.804	(0.831)	42	23469			104.58-	164.58	191.26	

65 Carbon Tetrachloride						CAS #:	56-23-5			
8.795	8.795	(1.074)	119	85692	2.00000	2.342	70.00-	130.00	100.00	
8.795	8.795	(1.074)	117	82137			75.27-	135.27	95.85	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

68	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.237	9.237	(1.128)	57	400802	2.00000	2.492	70.00-	130.00	100.00	
9.237	9.237	(1.128)	56	134866			2.91-	62.91	33.65	
9.237	9.237	(1.128)	41	117674			0.00-	59.75	29.36	

69	Benzene					CAS #:	71-43-2			
9.237	9.237	(0.918)	78	139372	2.00000	2.480	70.00-	130.00	100.00	
9.237	9.237	(0.918)	77	32010			0.00-	53.04	22.97	

72	1,2-Dichloroethane					CAS #:	107-06-2			
9.403	9.403	(0.934)	62	89858	2.00000	2.350	70.00-	130.00	100.00	
9.403	9.403	(0.934)	64	25857			0.57-	60.57	28.78	

75	Heptane					CAS #:	142-82-5			
9.624	9.624	(0.956)	100	19383	2.00000	2.538	70.00-	130.00	100.00	
9.624	9.624	(0.956)	43	174769			1063.83-	1123.83	901.66	
9.624	9.624	(0.956)	71	48620			257.42-	317.42	250.84	

80	Trichloroethene					CAS #:	79-01-6			
10.482	10.482	(1.041)	95	64707	2.00000	2.746	70.00-	130.00	100.00	
10.482	10.482	(1.041)	130	52528			62.27-	122.27	81.18	
10.482	10.482	(1.041)	97	37969			34.70-	94.70	58.68	

82	1,2-Dichloropropane					CAS #:	78-87-5			
10.979	10.979	(1.091)	63	60004	2.00000	2.451	70.00-	130.00	100.00	
10.979	10.979	(1.091)	62	45498			45.60-	105.60	75.82	
10.979	10.979	(1.091)	41	59347			64.20-	124.20	98.91	

84	1,4-Dioxane					CAS #:	123-91-1			
11.228	11.228	(1.115)	88	31565	2.00000	2.505	70.00-	130.00	100.00	
11.228	11.228	(1.115)	58	38115			92.25-	152.25	120.75	
11.228	11.228	(1.115)	57	13457			11.42-	71.42	42.63	

85	Bromodichloromethane					CAS #:	75-27-4			
11.560	11.560	(1.148)	83	83087	2.00000	2.387	70.00-	130.00	100.00	
11.560	11.560	(1.148)	85	50655			33.44-	93.44	60.97	

90	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.445	12.445	(1.236)	75	59090	2.00000	2.353	70.00-	130.00	100.00	
12.445	12.445	(1.236)	77	19453			1.12-	61.12	32.92	
12.445	12.445	(1.236)	39	65513			75.09-	135.09	110.87	

91	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.749	12.749	(1.266)	58	64379	2.00000	2.673	70.00-	130.00	100.00	
12.749	12.749	(1.266)	43	224759			296.95-	356.95	349.12	
12.749	12.749	(1.266)	85	18016			0.00-	57.61	27.98	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
99 Toluene						CAS #:	108-88-3			
12.942	12.942	(1.286)	91	133032	2.00000	2.465	70.00-	130.00	100.00	
12.942	12.942	(1.286)	92	83331			29.10-	89.10	62.64	

100 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.495	13.495	(0.894)	75	65276	2.00000	2.417	70.00-	130.00	100.00	
13.468	13.468	(0.892)	77	17228			2.77-	62.77	26.39	
13.468	13.468	(0.892)	39	53935			66.19-	126.19	82.63	

101 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.744	13.744	(0.910)	97	48268	2.00000	2.647	70.00-	130.00	100.00	
13.744	13.744	(0.910)	99	28065			30.49-	90.49	58.14	
13.744	13.744	(0.910)	83	37994			51.49-	111.49	78.71	

102 Tetrachloroethene						CAS #:	127-18-4			
13.799	13.799	(0.914)	166	56794	2.00000	2.490	70.00-	130.00	100.00	
13.799	13.799	(0.914)	129	52595			53.95-	113.95	92.61	
13.799	13.799	(0.914)	131	45371			50.65-	110.65	79.89	

103 2-Hexanone						CAS #:	591-78-6			
14.131	14.131	(0.936)	58	81765	2.00000	2.398	70.00-	130.00	100.00	
14.131	14.131	(0.936)	43	191037			208.96-	268.96	233.64	
14.131	14.131	(0.936)	100	9310			0.00-	42.78	11.39	

105 Dibromochloromethane						CAS #:	124-48-1			
14.297	14.297	(0.947)	129	66977	2.00000	2.256	70.00-	130.00	100.00	
14.297	14.297	(0.947)	127	48056			48.77-	108.77	71.75	

106 1,2-Dibromoethane						CAS #:	106-93-4			
14.463	14.463	(0.958)	107	63438	2.00000	2.276	70.00-	130.00	100.00	
14.463	14.463	(0.958)	109	58926			63.89-	123.89	92.89	

109 Chlorobenzene						CAS #:	108-90-7			
15.154	15.154	(1.004)	112	111605	2.00000	2.535	70.00-	130.00	100.00	
15.154	15.154	(1.004)	114	35441			2.73-	62.73	31.76	
15.154	15.154	(1.004)	77	75096			34.32-	94.32	67.29	

111 Ethyl Benzene						CAS #:	100-41-4			
15.265	15.265	(1.011)	106	53424	2.00000	2.469	70.00-	130.00	100.00	
15.265	15.265	(1.011)	91	203990			322.22-	382.22	381.83	

113 m,p-Xylene						CAS #:	108-38-3			
15.431	15.431	(1.022)	106	71494	2.00000	2.538	70.00-	130.00	100.00	
15.431	15.431	(1.022)	91	168950			202.98-	262.98	236.31	

114 o-Xylene						CAS #:	95-47-6			
15.956	15.956	(1.057)	106	77030	2.00000	2.892	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	167364			213.72- 273.72	217.27	

115 Styrene									
16.011	16.011	(1.060)	104	98770	2.00000	2.537	70.00- 130.00	100.00	
16.011	16.011	(1.060)	78	56379			31.90- 91.90	57.08	

118 Bromoform									
16.260	16.260	(1.077)	173	61401	2.00000	2.413	70.00- 130.00	100.00	
16.260	16.260	(1.077)	171	29883			22.82- 82.82	48.67	

123 1,1,2,2-Tetrachloroethane									
16.896	16.896	(1.119)	83	113659	2.00000	2.732	70.00- 130.00	100.00	
16.896	16.896	(1.119)	85	76386			35.41- 95.41	67.21	

126 4-Ethyltoluene									
17.062	17.062	(1.130)	105	243984	2.00000	2.668	70.00- 130.00	100.00	
17.062	17.062	(1.130)	120	71225			0.00- 58.34	29.19	

128 1,3,5-Trimethylbenzene									
17.145	17.145	(1.135)	105	200401	2.00000	2.613	70.00- 130.00	100.00	
17.145	17.145	(1.135)	120	95719			16.58- 76.58	47.76	

131 1,2,4-Trimethylbenzene									
17.532	17.532	(1.161)	105	222185	2.00000	2.698	70.00- 130.00	100.00	
17.532	17.532	(1.161)	120	100228			12.83- 72.83	45.11	

138 1,3-Dichlorobenzene									
17.836	17.836	(1.181)	146	151992	2.00000	2.816	70.00- 130.00	100.00	
17.836	17.836	(1.181)	148	88732			33.12- 93.12	58.38	
17.836	17.836	(1.181)	111	61470			15.78- 75.78	40.44	

141 1,4-Dichlorobenzene									
17.919	17.919	(1.187)	146	112823	2.00000	2.644	70.00- 130.00	100.00	
17.919	17.919	(1.187)	148	70761			34.33- 94.33	62.72	
17.919	17.919	(1.187)	111	48344			18.49- 78.49	42.85	

143 alpha-Chlorotoluene									
18.057	18.057	(1.196)	91	159307	2.00000	2.237	70.00- 130.00	100.00	
18.057	18.057	(1.196)	126	27823			0.00- 47.06	17.47	

146 1,2-Dichlorobenzene									
18.279	18.279	(1.211)	146	163507	2.00000	2.921	70.00- 130.00	100.00	
18.279	18.279	(1.211)	148	94461			33.02- 93.02	57.77	
18.279	18.279	(1.211)	111	70285			16.95- 76.95	42.99	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.578	19.578	(1.297)	180	118333	2.00000	3.006	70.00- 130.00	100.00	
19.578	19.578	(1.297)	182	112241			62.53- 122.53	94.85	

155	Hexachlorobutadiene					CAS #: 87-68-3			
19.661	19.661	(1.302)	225	107367	2.00000	3.291	70.00- 130.00	100.00	
19.661	19.661	(1.302)	223	65631			31.16- 91.16	61.13	

124	Propylbenzene					CAS #: 103-65-1			
16.924	16.924	(1.121)	91	293341	2.00000	2.772	70.00- 130.00	100.00	
16.924	16.924	(1.121)	120	57107			0.00- 50.53	19.47	
16.924	16.924	(1.121)	105	9907			0.00- 33.52	3.38	

119	Cumene					CAS #: 98-82-8			
16.426	16.426	(1.088)	105	226883	2.00000	2.788	70.00- 130.00	100.00	
16.426	16.426	(1.088)	120	56435			0.00- 55.50	24.87	
16.426	16.426	(1.088)	51	42871			0.00- 50.84	18.90	

156	Naphthalene					CAS #: 91-20-3			
19.744	19.744	(1.308)	128	363541	2.00000	3.111	70.00- 130.00	100.00	
19.744	19.744	(1.308)	127	44478			0.00- 42.90	12.23	

30	Isopentane					CAS #: 78-78-4			
3.514	3.514	(0.429)	43	173820	2.00000	2.432	70.00- 130.00	100.00	
3.514	3.514	(0.429)	57	107697			30.33- 90.33	61.96	
3.514	3.514	(0.429)	72	9046			0.00- 34.69	5.20	

21	Butane					CAS #: 106-97-8			
2.767	2.767	(0.338)	58	28307	2.00000	2.428	70.00- 130.00	100.00	
2.767	2.767	(0.338)	43	228460			773.30- 833.30	807.08	

96	Methyl Cyclohexane					CAS #: 108-87-2			
10.703	10.703	(1.063)	83	87634	2.00000	2.630	70.00- 130.00	100.00	
10.703	10.703	(1.063)	98	45970			20.58- 80.58	52.46	
10.703	10.703	(1.063)	55	116521			125.23- 185.23	132.96	

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052920.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	316096	0.74
79 1,4-Difluorobenze	1277249	766349	1788149	1251763	-2.00
108 Chlorobenzene-d5	1008759	605255	1412263	961284	-4.71

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-29maj.b/5052920.d
 Date: 29-May-2007 20:44
 Client ID: Level 3
 Sample Info: 2.0mL #1487-288
 Column phase: RTX-624

Instrument: msd5.1
 Operator: JG
 Column diameter: 0.53

/chem/msd5.1/5-29maj.b/5052920.d

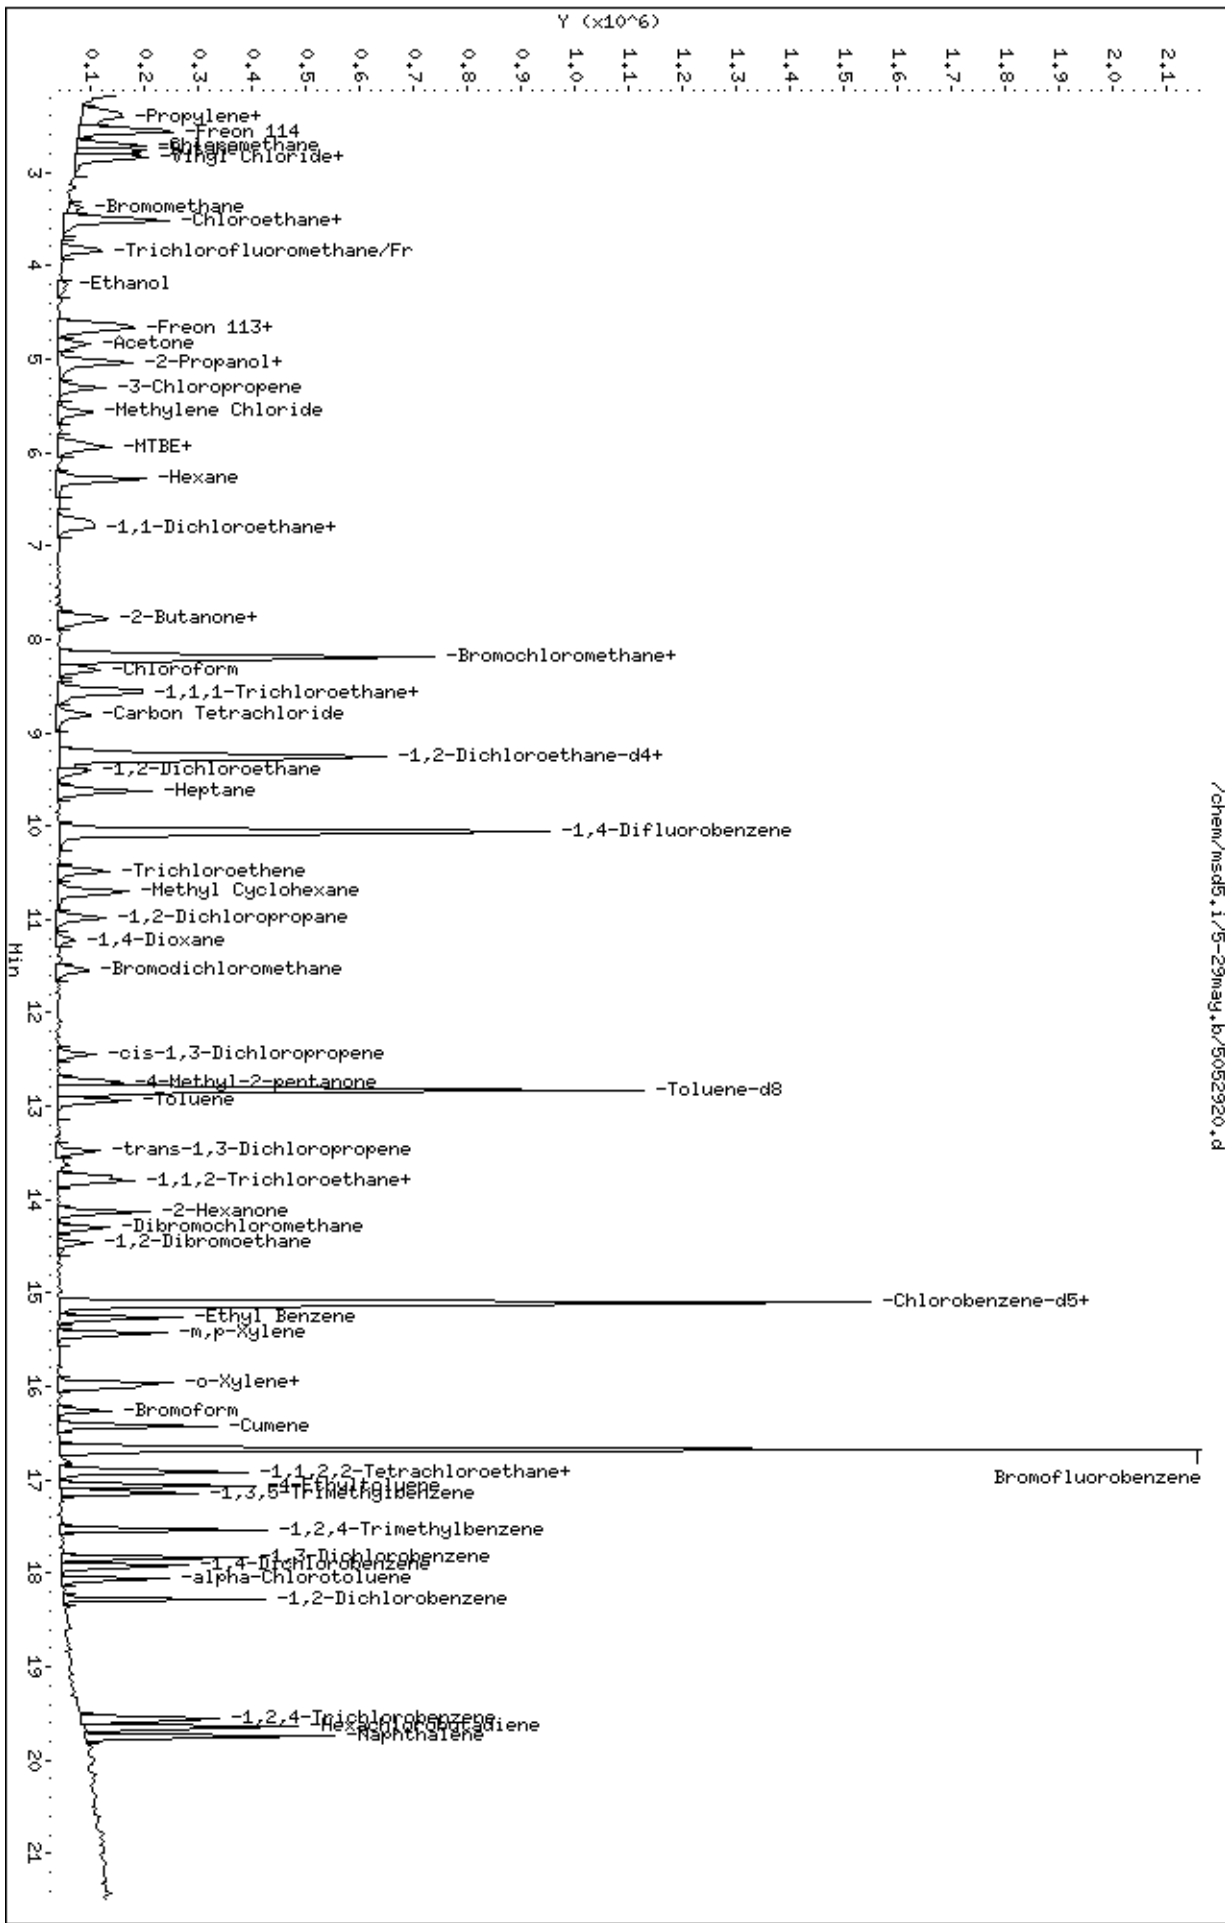

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052914.d
 Lab Smp Id: ICAL Client Smp ID: Level 4
 Inj Date : 29-MAY-2007 17:06
 Operator : JG Inst ID: msd5.i
 Smp Info : 25mL #1487-288
 Misc Info : 200ppbv-25ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 17:06 Cal File: 5052914.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 57 Bromochloromethane CAS #: 74-97-5									
8.187	8.187	(1.000)	130	313031	25.0000			70.00- 130.00	100.00
8.187	8.187	(1.000)	128	248012				50.27- 110.27	79.23
8.187	8.187	(1.000)	49	934584				281.04- 341.04	298.56

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	1249721	25.0000			70.00- 130.00	100.00
10.067	10.067	(1.000)	88	214958				0.00- 48.57	17.20

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	1007739	25.0000			70.00- 130.00	100.00
15.099	15.099	(1.000)	82	649705				0.00- 30.00	64.47

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.132)	65	598187	25.0000	23.838		70.00- 130.00	100.00
9.265	9.265	(1.132)	67	297515				0.00- 30.00	49.74

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	1165064	25.0000	25.612		70.00- 130.00	100.00
12.832	12.832	(1.275)	70	128433				0.00- 30.00	11.02

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 97 Toluene-d8 (continued)										
12.832	12.832	(1.275)	100	745926			0.00- 30.00	64.02		

\$ 122 Bromofluorobenzene										
						CAS #: 460-00-4				
16.675	16.675	(1.104)	174	654502	25.0000	25.850	70.00- 130.00	100.00		
16.675	16.675	(1.104)	95	1018554			131.53- 191.53	155.62		
16.675	16.675	(1.104)	176	602109			65.40- 125.40	91.99		

1 Propylene										
						CAS #: 115-07-1				
2.353	2.353	(0.287)	41	1011009	25.0000	24.216	70.00- 130.00	100.00		
2.353	2.353	(0.287)	42	666998			0.00- 30.00	65.97		
2.353	2.353	(0.287)	39	709842			0.00- 30.00	70.21		

2 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.408	2.408	(0.294)	85	1347935	25.0000	24.271	70.00- 130.00	100.00		
2.408	2.408	(0.294)	87	442032			0.00- 30.00	32.79		

3 Freon 114										
						CAS #: 76-14-2				
2.518	2.518	(0.308)	135	1341940	25.0000	25.264	70.00- 130.00	100.00		
2.518	2.518	(0.308)	137	410164			0.80- 60.80	30.57		

4 Chloromethane										
						CAS #: 74-87-3				
2.657	2.657	(0.325)	50	1202867	25.0000	23.989	70.00- 130.00	100.00		
2.657	2.657	(0.325)	52	347608			0.00- 30.00	28.90		

5 Vinyl Chloride										
						CAS #: 75-01-4				
2.850	2.850	(0.348)	62	1085068	25.0000	26.612	70.00- 130.00	100.00		
2.850	2.850	(0.348)	64	330164			0.00- 30.00	30.43		

6 1,3-Butadiene										
						CAS #: 106-99-0				
2.823	2.823	(0.345)	54	1025249	25.0000	25.332	70.00- 130.00	100.00		
2.823	2.823	(0.345)	39	1171748			0.00- 30.00	114.29		

7 Bromomethane										
						CAS #: 74-83-9				
3.376	3.376	(0.412)	94	593792	25.0000	24.514	70.00- 130.00	100.00		
3.376	3.376	(0.412)	96	597150			64.95- 124.95	100.57		

8 Chloroethane										
						CAS #: 75-00-3				
3.486	3.486	(0.426)	64	539261	25.0000	24.941	70.00- 130.00	100.00		
3.486	3.486	(0.426)	49	178886			0.00- 30.00	33.17		
3.486	3.486	(0.426)	66	162376			0.00- 30.00	30.11		

9 Trichlorofluoromethane/Fr11										
						CAS #: 75-69-4				
3.818	3.818	(0.466)	101	1424119	25.0000	25.438	70.00- 130.00	100.00		
3.818	3.818	(0.466)	103	932785			35.72- 95.72	65.50		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

13 Ethanol						CAS #: 64-17-5			
4.177	4.177	(0.510)	45	412419	25.0000	24.012	70.00- 130.00	100.00	
4.177	4.177	(0.510)	43	83275			0.00- 30.00	20.19	
4.177	4.177	(0.510)	46	165474			0.00- 30.00	40.12	

19 Freon 113						CAS #: 76-13-1			
4.647	4.647	(0.568)	151	837003	25.0000	24.418	70.00- 130.00	100.00	
4.647	4.647	(0.568)	153	552164			32.16- 92.16	65.97	
4.647	4.647	(0.568)	101	1138630			100.00- 160.00	136.04	

20 1,1-Dichloroethene						CAS #: 75-35-4			
4.675	4.675	(0.571)	61	1334698	25.0000	24.971	70.00- 130.00	100.00	
4.675	4.675	(0.571)	96	617724			19.13- 79.13	46.28	
4.675	4.675	(0.571)	98	404045			0.28- 60.28	30.27	

22 Acetone						CAS #: 67-64-1			
4.841	4.841	(0.591)	58	476184	25.0000	23.884	70.00- 130.00	100.00	
4.841	4.841	(0.591)	43	1621035			0.00- 30.00	340.42	

26 2-Propanol						CAS #: 67-63-0			
5.035	5.035	(0.615)	45	1984779	25.0000	22.842	70.00- 130.00	100.00	
5.035	5.035	(0.615)	43	414160			0.00- 30.00	20.87	
5.035	5.035	(0.615)	59	68357			0.00- 30.00	3.44	

25 Carbon Disulfide						CAS #: 75-15-0			
5.007	5.007	(0.612)	76	1850785	25.0000	25.151	70.00- 130.00	100.00	

28 3-Chloropropene						CAS #: 107-05-1			
5.311	5.311	(0.649)	76	298597	25.0000	24.017	70.00- 130.00	100.00	
5.311	5.311	(0.649)	41	1564994			0.00- 30.00	524.12	

29 Methylene Chloride						CAS #: 75-09-2			
5.560	5.560	(0.679)	49	1270288	25.0000	25.340	70.00- 130.00	100.00	
5.560	5.560	(0.679)	84	525898			9.87- 69.87	41.40	
5.560	5.560	(0.679)	51	367300			0.00- 30.00	28.91	

31 MTBE						CAS #: 1634-04-4			
5.892	5.892	(0.720)	73	1216602	25.0000	31.108	70.00- 130.00	100.00	
5.892	5.892	(0.720)	57	453109			5.77- 65.77	37.24	
5.892	5.892	(0.720)	41	500006			0.00- 30.00	41.10	

32 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.947	5.947	(0.726)	96	673204	25.0000	25.259	70.00- 130.00	100.00	
5.947	5.947	(0.726)	61	1295581			164.17- 224.17	192.45	
5.947	5.947	(0.726)	98	426270			0.00- 30.00	63.32	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Hexane						CAS #: 110-54-3			
6.279	6.279	(0.767)	57	1647548	25.0000	24.586	70.00- 130.00	100.00	
6.279	6.279	(0.767)	43	1257284			0.00- 30.00	76.31	
6.279	6.279	(0.767)	86	208383			0.00- 30.00	12.65	

43 1,1-Dichloroethane						CAS #: 75-34-3			
6.721	6.721	(0.821)	63	1367153	25.0000	25.647	70.00- 130.00	100.00	
6.721	6.721	(0.821)	65	388099			0.00- 59.00	28.39	

53 2-Butanone						CAS #: 78-93-3			
7.800	7.800	(0.953)	72	253122	25.0000	24.580	70.00- 130.00	100.00	
7.800	7.800	(0.953)	43	2091217			796.36- 856.36	826.17	
7.800	7.800	(0.953)	57	137774			0.00- 30.00	54.43	

52 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.744	7.744	(0.946)	61	1007089	25.0000	24.325	70.00- 130.00	100.00	
7.772	7.772	(0.949)	96	571660			25.31- 85.31	56.76	
7.772	7.772	(0.949)	98	362354			2.88- 62.88	35.98	

56 Tetrahydrofuran						CAS #: 109-99-9			
8.187	8.187	(1.000)	42	1254736	25.0000	23.494	70.00- 130.00	100.00	
8.187	8.187	(1.000)	71	224600			0.00- 48.47	17.90	
8.187	8.187	(1.000)	72	233351			0.00- 30.00	18.60	

58 Chloroform						CAS #: 67-66-3			
8.325	8.325	(1.017)	83	957335	25.0000	25.070	70.00- 130.00	100.00	
8.325	8.325	(1.017)	85	645239			33.68- 93.68	67.40	

62 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.574	8.574	(1.047)	97	1017811	25.0000	24.471	70.00- 130.00	100.00	
8.574	8.574	(1.047)	99	666965			32.24- 92.24	65.53	

61 Cyclohexane						CAS #: 110-82-7			
8.546	8.546	(1.044)	84	741086	25.0000	26.237	70.00- 130.00	100.00	
8.546	8.546	(1.044)	56	1447053			177.94- 237.94	195.26	
8.546	8.546	(1.044)	41	876222			93.55- 153.55	118.23	

63 Vinyl Acetate						CAS #: 108-05-4			
6.776	6.776	(0.828)	86	150268	25.0000	24.201	70.00- 130.00	100.00	
6.776	6.776	(0.828)	43	2750215			0.00- 30.00	1830.21	
6.776	6.776	(0.828)	42	197923			0.00- 30.00	131.71	

65 Carbon Tetrachloride						CAS #: 56-23-5			
8.795	8.795	(1.074)	119	890614	25.0000	24.578	70.00- 130.00	100.00	
8.795	8.795	(1.074)	117	940860			71.97- 131.97	105.64	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

68	2,2,4-Trimethylpentane				CAS #: 540-84-1				
9.237	9.237	(1.128)	57	4119169	25.0000	25.867	70.00-	130.00	100.00
9.237	9.237	(1.128)	56	1386524			0.00-	30.00	33.66
9.237	9.237	(1.128)	41	1238030			0.00-	30.00	30.06

69	Benzene				CAS #: 71-43-2				
9.237	9.237	(0.918)	78	1432495	25.0000	25.529	70.00-	130.00	100.00
9.237	9.237	(0.918)	77	337983			0.00-	30.00	23.59

72	1,2-Dichloroethane				CAS #: 107-06-2				
9.403	9.403	(0.934)	62	991451	25.0000	25.974	70.00-	130.00	100.00
9.403	9.403	(0.934)	64	269322			0.00-	30.00	27.16

75	Heptane				CAS #: 142-82-5				
9.624	9.624	(0.956)	100	171791	25.0000	22.528	70.00-	130.00	100.00
9.624	9.624	(0.956)	43	1911392			0.00-	30.00	1112.63
9.624	9.624	(0.956)	71	494847			0.00-	30.00	288.05

80	Trichloroethene				CAS #: 79-01-6				
10.482	10.482	(1.041)	95	596772	25.0000	25.370	70.00-	130.00	100.00
10.482	10.482	(1.041)	130	559516			65.35-	125.35	93.76
10.482	10.482	(1.041)	97	372828			35.05-	95.05	62.47

82	1,2-Dichloropropane				CAS #: 78-87-5				
10.979	10.979	(1.091)	63	618665	25.0000	25.311	70.00-	130.00	100.00
10.979	10.979	(1.091)	62	472710			43.36-	103.36	76.41
10.979	10.979	(1.091)	41	566826			62.33-	122.33	91.62

84	1,4-Dioxane				CAS #: 123-91-1				
11.200	11.200	(1.113)	88	298809	25.0000	23.756	70.00-	130.00	100.00
11.200	11.200	(1.113)	58	352148			87.73-	147.73	117.85
11.200	11.200	(1.113)	57	119060			0.00-	30.00	39.84

85	Bromodichloromethane				CAS #: 75-27-4				
11.532	11.532	(1.146)	83	874442	25.0000	25.164	70.00-	130.00	100.00
11.532	11.532	(1.146)	85	581003			33.28-	93.28	66.44

90	cis-1,3-Dichloropropene				CAS #: 10061-01-5				
12.445	12.445	(1.236)	75	665925	25.0000	26.561	70.00-	130.00	100.00
12.445	12.445	(1.236)	77	195976			2.34-	62.34	29.43
12.445	12.445	(1.236)	39	720943			80.54-	140.54	108.26

91	4-Methyl-2-pentanone				CAS #: 108-10-1				
12.721	12.721	(1.264)	58	623679	25.0000	25.937	70.00-	130.00	100.00
12.721	12.721	(1.264)	43	2035637			0.00-	30.00	326.39
12.749	12.749	(1.266)	85	166620			0.00-	30.00	26.72

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
99 Toluene						CAS #: 108-88-3			
12.942	12.942	(1.286)	91	1379591	25.0000	25.601	70.00- 130.00	100.00	
12.942	12.942	(1.286)	92	821910			28.86- 88.86	59.58	

100 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.468	13.468	(0.892)	75	708220	25.0000	25.011	70.00- 130.00	100.00	
13.468	13.468	(0.892)	77	229673			1.06- 61.06	32.43	
13.468	13.468	(0.892)	39	704714			66.05- 126.05	99.50	

101 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.744	13.744	(0.910)	97	484845	25.0000	25.363	70.00- 130.00	100.00	
13.744	13.744	(0.910)	99	285477			31.72- 91.72	58.88	
13.744	13.744	(0.910)	83	388759			52.19- 112.19	80.18	

102 Tetrachloroethene						CAS #: 127-18-4			
13.799	13.799	(0.914)	166	572403	25.0000	23.942	70.00- 130.00	100.00	
13.799	13.799	(0.914)	129	495873			54.09- 114.09	86.63	
13.799	13.799	(0.914)	131	466259			52.34- 112.34	81.46	

103 2-Hexanone						CAS #: 591-78-6			
14.131	14.131	(0.936)	58	825888	25.0000	23.106	70.00- 130.00	100.00	
14.131	14.131	(0.936)	43	1969807			204.79- 264.79	238.51	
14.131	14.131	(0.936)	100	117306			0.00- 30.00	14.20	

105 Dibromochloromethane						CAS #: 124-48-1			
14.297	14.297	(0.947)	129	770291	25.0000	24.752	70.00- 130.00	100.00	
14.297	14.297	(0.947)	127	599597			0.00- 30.00	77.84	

106 1,2-Dibromoethane						CAS #: 106-93-4			
14.463	14.463	(0.958)	107	735711	25.0000	25.181	70.00- 130.00	100.00	
14.463	14.463	(0.958)	109	710546			62.51- 122.51	96.58	

109 Chlorobenzene						CAS #: 108-90-7			
15.154	15.154	(1.004)	112	1112852	25.0000	24.114	70.00- 130.00	100.00	
15.154	15.154	(1.004)	114	355744			2.97- 62.97	31.97	
15.154	15.154	(1.004)	77	712512			34.70- 94.70	64.03	

111 Ethyl Benzene						CAS #: 100-41-4			
15.265	15.265	(1.011)	106	595476	25.0000	26.256	70.00- 130.00	100.00	
15.265	15.265	(1.011)	91	2068831			0.00- 30.00	347.42	

113 m,p-Xylene						CAS #: 108-38-3			
15.431	15.431	(1.022)	106	732758	25.0000	24.816	70.00- 130.00	100.00	
15.431	15.431	(1.022)	91	1678977			0.00- 30.00	229.13	

114 o-Xylene						CAS #: 95-47-6			
15.956	15.956	(1.057)	106	693334	25.0000	24.829	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	1659603			210.36- 270.36	239.37	

115 Styrene CAS #: 100-42-5									
16.011	16.011	(1.060)	104	1076573	25.0000	26.377	70.00- 130.00	100.00	
16.011	16.011	(1.060)	78	637356			31.61- 91.61	59.20	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	659910	25.0000	24.743	70.00- 130.00	100.00	
16.260	16.260	(1.077)	171	324278			21.89- 81.89	49.14	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	1052242	25.0000	24.125	70.00- 130.00	100.00	
16.896	16.896	(1.119)	85	686767			35.56- 95.56	65.27	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	2461960	25.0000	25.678	70.00- 130.00	100.00	
17.062	17.062	(1.130)	120	708074			0.00- 58.00	28.76	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	1968559	25.0000	24.488	70.00- 130.00	100.00	
17.145	17.145	(1.135)	120	919042			0.00- 30.00	46.69	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	2186124	25.0000	25.328	70.00- 130.00	100.00	
17.532	17.532	(1.161)	120	967732			13.06- 73.06	44.27	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	1339584	25.0000	23.677	70.00- 130.00	100.00	
17.836	17.836	(1.181)	148	847624			0.00- 30.00	63.28	
17.836	17.836	(1.181)	111	619126			0.00- 30.00	46.22	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	1060761	25.0000	23.710	70.00- 130.00	100.00	
17.919	17.919	(1.187)	148	665597			0.00- 30.00	62.75	
17.919	17.919	(1.187)	111	504987			0.00- 30.00	47.61	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.057	18.057	(1.196)	91	1884401	25.0000	25.245	70.00- 130.00	100.00	
18.057	18.057	(1.196)	126	306550			0.00- 30.00	16.27	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	1353685	25.0000	23.066	70.00- 130.00	100.00	
18.279	18.279	(1.211)	148	841721			33.74- 93.74	62.18	
18.279	18.279	(1.211)	111	607170			15.34- 75.34	44.85	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.578	19.578	(1.297)	180	872502	25.0000	21.140	70.00- 130.00	100.00	
19.578	19.578	(1.297)	182	847621			65.13- 125.13	97.15	

155	Hexachlorobutadiene					CAS #: 87-68-3			
19.661	19.661	(1.302)	225	712580	25.0000	20.835	70.00- 130.00	100.00	
19.661	19.661	(1.302)	223	438929			29.70- 89.70	61.60	

124	Propylbenzene					CAS #: 103-65-1			
16.924	16.924	(1.121)	91	2854973	25.0000	25.736	70.00- 130.00	100.00	
16.924	16.924	(1.121)	120	584264			0.00- 30.00	20.46	
16.924	16.924	(1.121)	105	97333			0.00- 30.00	3.41	

119	Cumene					CAS #: 98-82-8			
16.426	16.426	(1.088)	105	2186960	25.0000	25.634	70.00- 130.00	100.00	
16.426	16.426	(1.088)	120	563198			0.00- 30.00	25.75	
16.426	16.426	(1.088)	51	462359			0.00- 30.00	21.14	

156	Naphthalene					CAS #: 91-20-3			
19.744	19.744	(1.308)	128	2607606	25.0000	21.284	70.00- 130.00	100.00	
19.744	19.744	(1.308)	127	340365			0.00- 30.00	13.05	

30	Isopentane					CAS #: 78-78-4			
3.514	3.514	(0.429)	43	1748567	25.0000	24.702	70.00- 130.00	100.00	
3.514	3.514	(0.429)	57	1019300			0.00- 30.00	58.29	
3.514	3.514	(0.429)	72	77066			0.00- 30.00	4.41	

21	Butane					CAS #: 106-97-8			
2.740	2.740	(0.335)	58	284462	25.0000	24.634	70.00- 130.00	100.00	
2.740	2.740	(0.335)	43	2202115			0.00- 30.00	774.13	

96	Methyl Cyclohexane					CAS #: 108-87-2			
10.703	10.703	(1.063)	83	816309	25.0000	24.541	70.00- 130.00	100.00	
10.703	10.703	(1.063)	98	438875			0.00- 30.00	53.76	
10.703	10.703	(1.063)	55	1257458			0.00- 30.00	154.04	

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052914.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	313031	-0.24
79 1,4-Difluorobenze	1277249	766349	1788149	1249721	-2.16
108 Chlorobenzene-d5	1008759	605255	1412263	1007739	-0.10


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

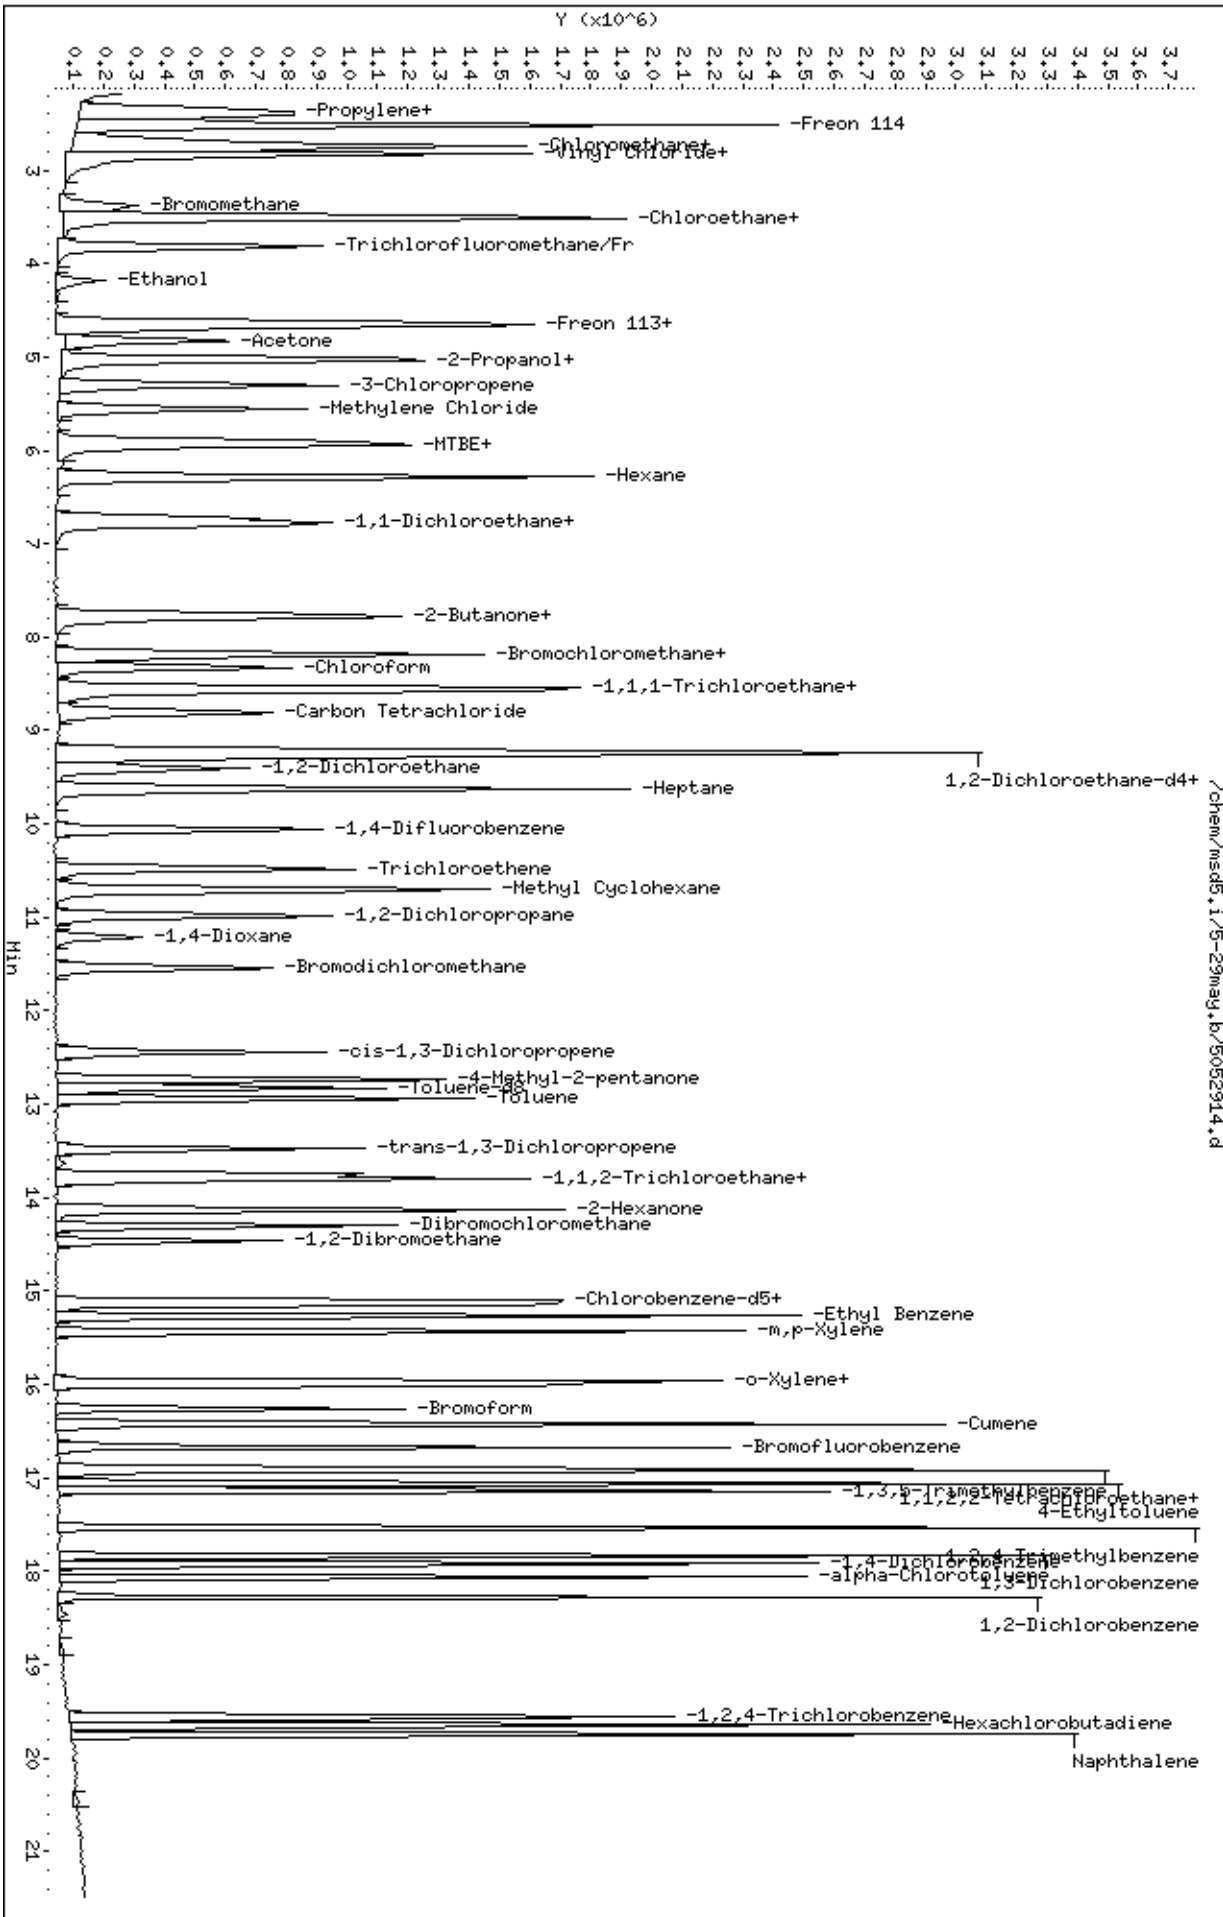

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052915.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 29-MAY-2007 17:34
 Operator : JG Inst ID: msd5.i
 Smp Info : 50mL #1487-288
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 17:34 Cal File: 5052915.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 57 Bromochloromethane CAS #: 74-97-5									
8.187	8.187	(1.000)	130	313773	25.0000			70.00- 130.00	100.00
8.187	8.187	(1.000)	128	251870				50.27- 110.27	80.27
8.187	8.187	(1.000)	49	975944				281.04- 341.04	311.04

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	1277249	25.0000			70.00- 130.00	100.00
10.067	10.067	(1.000)	88	237130				0.00- 48.57	18.57

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	1008759	25.0000			70.00- 130.00	100.00
15.099	15.099	(1.000)	82	646754				0.00- 30.00	64.11

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.132)	65	608892	25.0000	24.207		70.00- 130.00	100.00
9.265	9.265	(1.132)	67	325067				0.00- 30.00	53.39

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	1171514	25.0000	25.199		70.00- 130.00	100.00
12.832	12.832	(1.275)	70	130769				0.00- 30.00	11.16

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 97 Toluene-d8 (continued)										
12.832	12.832	(1.275)	100	752358			0.00- 30.00	64.22		

\$ 122 Bromofluorobenzene										
						CAS #:	460-00-4			
16.675	16.675	(1.104)	174	634034	25.0000	25.016	70.00- 130.00	100.00		
16.675	16.675	(1.104)	95	1024178			131.53- 191.53	161.53		
16.675	16.675	(1.104)	176	604889			65.40- 125.40	95.40		

1 Propylene										
						CAS #:	115-07-1			
2.353	2.353	(0.287)	41	1977541	50.0000	47.254	70.00- 130.00	100.00		
2.353	2.353	(0.287)	42	1330489			0.00- 30.00	67.28		
2.353	2.353	(0.287)	39	1342456			0.00- 30.00	67.89		

2 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.408	2.408	(0.294)	85	2608760	50.0000	46.862	70.00- 130.00	100.00		
2.408	2.408	(0.294)	87	852896			0.00- 30.00	32.69		

3 Freon 114										
						CAS #:	76-14-2			
2.546	2.546	(0.311)	135	2601667	50.0000	48.865	70.00- 130.00	100.00		
2.546	2.546	(0.311)	137	801189			0.80- 60.80	30.80		

4 Chloromethane										
						CAS #:	74-87-3			
2.657	2.657	(0.325)	50	2527415	50.0000	50.285	70.00- 130.00	100.00		
2.684	2.684	(0.328)	52	743142			0.00- 30.00	29.40		

5 Vinyl Chloride										
						CAS #:	75-01-4			
2.850	2.850	(0.348)	62	2094194	50.0000	51.240	70.00- 130.00	100.00		
2.850	2.850	(0.348)	64	615056			0.00- 30.00	29.37		

6 1,3-Butadiene										
						CAS #:	106-99-0			
2.823	2.823	(0.345)	54	2042037	50.0000	50.336	70.00- 130.00	100.00		
2.823	2.823	(0.345)	39	2379579			0.00- 30.00	116.53		

7 Bromomethane										
						CAS #:	74-83-9			
3.376	3.376	(0.412)	94	1191599	50.0000	49.078	70.00- 130.00	100.00		
3.376	3.376	(0.412)	96	1131476			64.95- 124.95	94.95		

8 Chloroethane										
						CAS #:	75-00-3			
3.514	3.514	(0.429)	64	1064620	50.0000	49.122	70.00- 130.00	100.00		
3.486	3.486	(0.426)	49	351878			0.00- 30.00	33.05		
3.514	3.514	(0.429)	66	294927			0.00- 30.00	27.70		

9 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.818	3.818	(0.466)	101	2738419	50.0000	48.798	70.00- 130.00	100.00		
3.818	3.818	(0.466)	103	1799740			35.72- 95.72	65.72		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

13 Ethanol						CAS #: 64-17-5			
4.177	4.177	(0.510)	45	850814	50.0000	49.419	70.00- 130.00	100.00	
4.177	4.177	(0.510)	43	155554			0.00- 30.00	18.28	
4.177	4.177	(0.510)	46	329644			0.00- 30.00	38.74	

19 Freon 113						CAS #: 76-13-1			
4.647	4.647	(0.568)	151	1719734	50.0000	50.051	70.00- 130.00	100.00	
4.647	4.647	(0.568)	153	1068957			32.16- 92.16	62.16	
4.647	4.647	(0.568)	101	2235644			100.00- 160.00	130.00	

20 1,1-Dichloroethene						CAS #: 75-35-4			
4.675	4.675	(0.571)	61	2564587	50.0000	47.867	70.00- 130.00	100.00	
4.675	4.675	(0.571)	96	1260077			19.13- 79.13	49.13	
4.675	4.675	(0.571)	98	776684			0.28- 60.28	30.28	

22 Acetone						CAS #: 67-64-1			
4.841	4.841	(0.591)	58	948264	50.0000	47.449	70.00- 130.00	100.00	
4.841	4.841	(0.591)	43	3279219			0.00- 30.00	345.81	

26 2-Propanol						CAS #: 67-63-0			
5.035	5.035	(0.615)	45	3943361	50.0000	45.276	70.00- 130.00	100.00	
5.035	5.035	(0.615)	43	826999			0.00- 30.00	20.97	
5.035	5.035	(0.615)	59	130846			0.00- 30.00	3.32	

25 Carbon Disulfide						CAS #: 75-15-0			
5.007	5.007	(0.612)	76	3629502	50.0000	49.205	70.00- 130.00	100.00	

28 3-Chloropropene						CAS #: 107-05-1			
5.311	5.311	(0.649)	76	600746	50.0000	48.205	70.00- 130.00	100.00	
5.311	5.311	(0.649)	41	3100941			0.00- 30.00	516.18	

29 Methylene Chloride						CAS #: 75-09-2			
5.560	5.560	(0.679)	49	2469346	50.0000	49.144	70.00- 130.00	100.00	
5.560	5.560	(0.679)	84	984532			9.87- 69.87	39.87	
5.560	5.560	(0.679)	51	728946			0.00- 30.00	29.52	

31 MTBE						CAS #: 1634-04-4			
5.892	5.892	(0.720)	73	2179595	50.0000	55.599	70.00- 130.00	100.00	
5.892	5.892	(0.720)	57	779620			5.77- 65.77	35.77	
5.892	5.892	(0.720)	41	903114			0.00- 30.00	41.43	

32 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.947	5.947	(0.726)	96	1305614	50.0000	48.871	70.00- 130.00	100.00	
5.947	5.947	(0.726)	61	2535129			164.17- 224.17	194.17	
5.947	5.947	(0.726)	98	833020			0.00- 30.00	63.80	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
38 Hexane						CAS #: 110-54-3			
6.279	6.279	(0.767)	57	3258302	50.0000	48.508	70.00- 130.00	100.00	
6.279	6.279	(0.767)	43	2453877			0.00- 30.00	75.31	
6.279	6.279	(0.767)	86	372964			0.00- 30.00	11.45	

43 1,1-Dichloroethane						CAS #: 75-34-3			
6.721	6.721	(0.821)	63	2641217	50.0000	49.430	70.00- 130.00	100.00	
6.721	6.721	(0.821)	65	765910			0.00- 59.00	29.00	

53 2-Butanone						CAS #: 78-93-3			
7.800	7.800	(0.953)	72	506249	50.0000	49.043	70.00- 130.00	100.00	
7.800	7.800	(0.953)	43	4183434			796.36- 856.36	826.36	
7.800	7.800	(0.953)	57	285976			0.00- 30.00	56.49	

52 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.744	7.744	(0.946)	61	2048143	50.0000	49.353	70.00- 130.00	100.00	
7.772	7.772	(0.949)	96	1132802			25.31- 85.31	55.31	
7.772	7.772	(0.949)	98	673477			2.88- 62.88	32.88	

56 Tetrahydrofuran						CAS #: 109-99-9			
8.187	8.187	(1.000)	42	2480236	50.0000	46.331	70.00- 130.00	100.00	
8.187	8.187	(1.000)	71	458003			0.00- 48.47	18.47	
8.187	8.187	(1.000)	72	511272			0.00- 30.00	20.61	

58 Chloroform						CAS #: 67-66-3			
8.325	8.325	(1.017)	83	1941721	50.0000	50.728	70.00- 130.00	100.00	
8.325	8.325	(1.017)	85	1236401			33.68- 93.68	63.68	

62 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.574	8.574	(1.047)	97	2051039	50.0000	49.196	70.00- 130.00	100.00	
8.574	8.574	(1.047)	99	1276636			32.24- 92.24	62.24	

61 Cyclohexane						CAS #: 110-82-7			
8.546	8.546	(1.044)	84	1394628	50.0000	49.257	70.00- 130.00	100.00	
8.546	8.546	(1.044)	56	2899995			177.94- 237.94	207.94	
8.546	8.546	(1.044)	41	1723103			93.55- 153.55	123.55	

63 Vinyl Acetate						CAS #: 108-05-4			
6.776	6.776	(0.828)	86	310352	50.0000	49.866	70.00- 130.00	100.00	
6.776	6.776	(0.828)	43	5590923			0.00- 30.00	1801.48	
6.776	6.776	(0.828)	42	423247			0.00- 30.00	136.38	

65 Carbon Tetrachloride						CAS #: 56-23-5			
8.795	8.795	(1.074)	119	1798619	50.0000	49.519	70.00- 130.00	100.00	
8.795	8.795	(1.074)	117	1834112			71.97- 131.97	101.97	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

68	2,2,4-Trimethylpentane						CAS #: 540-84-1		
9.237	9.237	(1.128)	57	7899842	50.0000	49.490	70.00- 130.00	100.00	
9.237	9.237	(1.128)	56	2631057			0.00- 30.00	33.31	
9.237	9.237	(1.128)	41	2363844			0.00- 30.00	29.92	

69	Benzene						CAS #: 71-43-2		
9.237	9.237	(0.918)	78	2792699	50.0000	48.696	70.00- 130.00	100.00	
9.237	9.237	(0.918)	77	635503			0.00- 30.00	22.76	

72	1,2-Dichloroethane						CAS #: 107-06-2		
9.403	9.403	(0.934)	62	1890991	50.0000	48.473	70.00- 130.00	100.00	
9.403	9.403	(0.934)	64	564826			0.00- 30.00	29.87	

75	Heptane						CAS #: 142-82-5		
9.624	9.624	(0.956)	100	322848	50.0000	41.424	70.00- 130.00	100.00	
9.624	9.624	(0.956)	43	3735777			0.00- 30.00	1157.13	
9.624	9.624	(0.956)	71	966967			0.00- 30.00	299.51	

80	Trichloroethene						CAS #: 79-01-6		
10.481	10.481	(1.041)	95	1127151	50.0000	46.886	70.00- 130.00	100.00	
10.481	10.481	(1.041)	130	1074741			65.35- 125.35	95.35	
10.481	10.481	(1.041)	97	733182			35.05- 95.05	65.05	

82	1,2-Dichloropropane						CAS #: 78-87-5		
10.979	10.979	(1.091)	63	1212312	50.0000	48.529	70.00- 130.00	100.00	
10.979	10.979	(1.091)	62	889293			43.36- 103.36	73.36	
10.979	10.979	(1.091)	41	1119289			62.33- 122.33	92.33	

84	1,4-Dioxane						CAS #: 123-91-1		
11.200	11.200	(1.113)	88	628761	50.0000	48.910	70.00- 130.00	100.00	
11.200	11.200	(1.113)	58	740218			87.73- 147.73	117.73	
11.200	11.200	(1.113)	57	250012			0.00- 30.00	39.76	

85	Bromodichloromethane						CAS #: 75-27-4		
11.532	11.532	(1.146)	83	1785638	50.0000	50.279	70.00- 130.00	100.00	
11.532	11.532	(1.146)	85	1129938			33.28- 93.28	63.28	

90	cis-1,3-Dichloropropene						CAS #: 10061-01-5		
12.445	12.445	(1.236)	75	1251269	50.0000	48.833	70.00- 130.00	100.00	
12.445	12.445	(1.236)	77	404698			2.34- 62.34	32.34	
12.445	12.445	(1.236)	39	1383202			80.54- 140.54	110.54	

91	4-Methyl-2-pentanone						CAS #: 108-10-1		
12.721	12.721	(1.264)	58	1242393	50.0000	50.554	70.00- 130.00	100.00	
12.721	12.721	(1.264)	43	4006168			0.00- 30.00	322.46	
12.721	12.721	(1.264)	85	334037			0.00- 30.00	26.89	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
99 Toluene						CAS #: 108-88-3			
12.942	12.942	(1.286)	91	2697941	50.0000	48.986	70.00- 130.00	100.00	
12.942	12.942	(1.286)	92	1587962			28.86- 88.86	58.86	

100 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.468	13.468	(0.892)	75	1439559	50.0000	50.788	70.00- 130.00	100.00	
13.468	13.468	(0.892)	77	447190			1.06- 61.06	31.06	
13.468	13.468	(0.892)	39	1382710			66.05- 126.05	96.05	

101 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.744	13.744	(0.910)	97	913026	50.0000	47.713	70.00- 130.00	100.00	
13.744	13.744	(0.910)	99	563497			31.72- 91.72	61.72	
13.744	13.744	(0.910)	83	750381			52.19- 112.19	82.19	

102 Tetrachloroethene						CAS #: 127-18-4			
13.799	13.799	(0.914)	166	1117843	50.0000	46.709	70.00- 130.00	100.00	
13.799	13.799	(0.914)	129	940032			54.09- 114.09	84.09	
13.799	13.799	(0.914)	131	920420			52.34- 112.34	82.34	

103 2-Hexanone						CAS #: 591-78-6			
14.131	14.131	(0.936)	58	1705223	50.0000	47.659	70.00- 130.00	100.00	
14.131	14.131	(0.936)	43	4003631			204.79- 264.79	234.79	
14.131	14.131	(0.936)	100	215039			0.00- 30.00	12.61	

105 Dibromochloromethane						CAS #: 124-48-1			
14.297	14.297	(0.947)	129	1530062	50.0000	49.116	70.00- 130.00	100.00	
14.297	14.297	(0.947)	127	1187608			0.00- 30.00	77.62	

106 1,2-Dibromoethane						CAS #: 106-93-4			
14.463	14.463	(0.958)	107	1466592	50.0000	50.145	70.00- 130.00	100.00	
14.463	14.463	(0.958)	109	1356701			62.51- 122.51	92.51	

109 Chlorobenzene						CAS #: 108-90-7			
15.154	15.154	(1.004)	112	2111756	50.0000	45.712	70.00- 130.00	100.00	
15.154	15.154	(1.004)	114	696282			2.97- 62.97	32.97	
15.154	15.154	(1.004)	77	1366218			34.70- 94.70	64.70	

111 Ethyl Benzene						CAS #: 100-41-4			
15.265	15.265	(1.011)	106	1176670	50.0000	51.829	70.00- 130.00	100.00	
15.265	15.265	(1.011)	91	4011717			0.00- 30.00	340.94	

113 m,p-Xylene						CAS #: 108-38-3			
15.431	15.431	(1.022)	106	1446967	50.0000	48.954	70.00- 130.00	100.00	
15.431	15.431	(1.022)	91	3292215			0.00- 30.00	227.53	

114 o-Xylene						CAS #: 95-47-6			
15.956	15.956	(1.057)	106	1347497	50.0000	48.206	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	3238877			210.36- 270.36	240.36	

115 Styrene CAS #: 100-42-5									
16.011	16.011	(1.060)	104	2157926	50.0000	52.817	70.00- 130.00	100.00	
16.011	16.011	(1.060)	78	1329527			31.61- 91.61	61.61	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	1344664	50.0000	50.367	70.00- 130.00	100.00	
16.260	16.260	(1.077)	171	697697			21.89- 81.89	51.89	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	2042509	50.0000	46.782	70.00- 130.00	100.00	
16.896	16.896	(1.119)	85	1339122			35.56- 95.56	65.56	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	4892980	50.0000	50.981	70.00- 130.00	100.00	
17.062	17.062	(1.130)	120	1370048			0.00- 58.00	28.00	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	3867275	50.0000	48.058	70.00- 130.00	100.00	
17.145	17.145	(1.135)	120	1829395			0.00- 30.00	47.30	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	4293478	50.0000	49.692	70.00- 130.00	100.00	
17.532	17.532	(1.161)	120	1848724			13.06- 73.06	43.06	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	2603043	50.0000	45.963	70.00- 130.00	100.00	
17.836	17.836	(1.181)	148	1652604			0.00- 30.00	63.49	
17.836	17.836	(1.181)	111	1199103			0.00- 30.00	46.07	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	2184894	50.0000	48.787	70.00- 130.00	100.00	
17.919	17.919	(1.187)	148	1424849			0.00- 30.00	65.21	
17.919	17.919	(1.187)	111	1044325			0.00- 30.00	47.80	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.057	18.057	(1.196)	91	3978618	50.0000	53.248	70.00- 130.00	100.00	
18.057	18.057	(1.196)	126	670352			0.00- 30.00	16.85	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	2604216	50.0000	44.329	70.00- 130.00	100.00	
18.279	18.279	(1.211)	148	1659847			33.74- 93.74	63.74	
18.279	18.279	(1.211)	111	1180710			15.34- 75.34	45.34	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.578	19.578	(1.297)	180	1813598	50.0000	43.898	70.00- 130.00	100.00	
19.578	19.578	(1.297)	182	1725272			65.13- 125.13	95.13	

155	Hexachlorobutadiene					CAS #: 87-68-3			
19.661	19.661	(1.302)	225	1503130	50.0000	43.906	70.00- 130.00	100.00	
19.661	19.661	(1.302)	223	897376			29.70- 89.70	59.70	

124	Propylbenzene					CAS #: 103-65-1			
16.924	16.924	(1.121)	91	5564453	50.0000	50.110	70.00- 130.00	100.00	
16.924	16.924	(1.121)	120	1167670			0.00- 30.00	20.98	
16.924	16.924	(1.121)	105	195614			0.00- 30.00	3.52	

119	Cumene					CAS #: 98-82-8			
16.426	16.426	(1.088)	105	4265763	50.0000	49.949	70.00- 130.00	100.00	
16.426	16.426	(1.088)	120	1113653			0.00- 30.00	26.11	
16.426	16.426	(1.088)	51	874603			0.00- 30.00	20.50	

156	Naphthalene					CAS #: 91-20-3			
19.744	19.744	(1.308)	128	5669868	50.0000	46.232	70.00- 130.00	100.00	
19.744	19.744	(1.308)	127	729925			0.00- 30.00	12.87	

30	Isopentane					CAS #: 78-78-4			
3.514	3.514	(0.429)	43	3288486	50.0000	46.346	70.00- 130.00	100.00	
3.514	3.514	(0.429)	57	1973329			0.00- 30.00	60.01	
3.514	3.514	(0.429)	72	153849			0.00- 30.00	4.68	

21	Butane					CAS #: 106-97-8			
2.767	2.767	(0.338)	58	545387	50.0000	47.117	70.00- 130.00	100.00	
2.740	2.740	(0.335)	43	4300789			0.00- 30.00	788.58	

96	Methyl Cyclohexane					CAS #: 108-87-2			
10.703	10.703	(1.063)	83	1639531	50.0000	48.227	70.00- 130.00	100.00	
10.703	10.703	(1.063)	98	831057			0.00- 30.00	50.69	
10.703	10.703	(1.063)	55	2454744			0.00- 30.00	149.72	

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052915.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	313773	0.00
79 1,4-Difluorobenze	1277249	766349	1788149	1277249	0.00
108 Chlorobenzene-d5	1008759	605255	1412263	1008759	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msds.1/5-29maj.b/5052915.d
 Date: 29-May-2007 17:34
 Client ID: Level 5
 Sample Info: 50mL #1487-288

Column phase: RTX-624

Instrument: msds.i
 Operator: JG
 Column diameter: 0.53

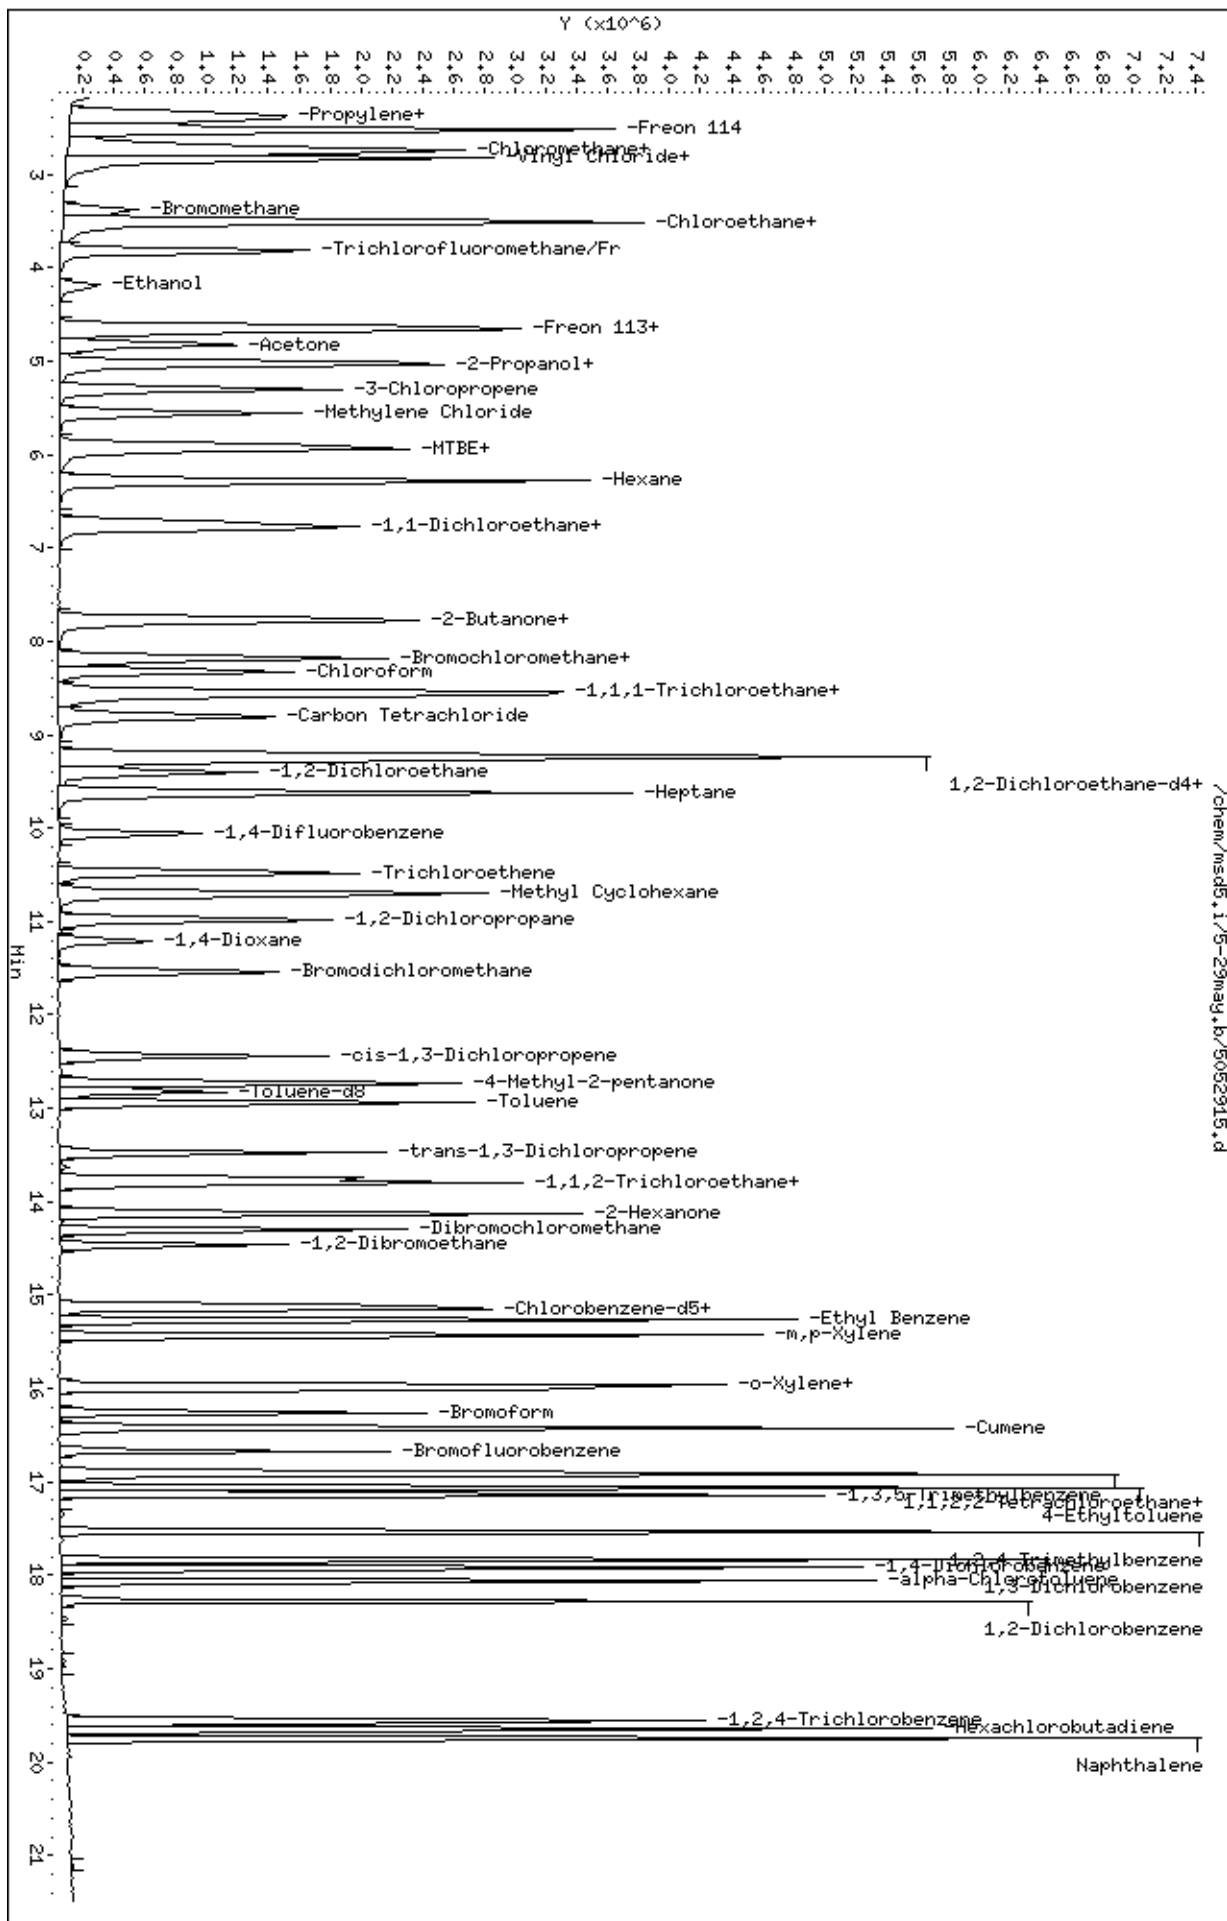

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052916.d
 Lab Smp Id: ICAL Client Smp ID: Level 6
 Inj Date : 29-MAY-2007 18:02
 Operator : JG Inst ID: msd5.i
 Smp Info : 100mL #1487-288
 Misc Info : 200ppbv-100ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 18:02 Cal File: 5052916.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

* 57	Bromochloromethane					CAS #:	74-97-5	
8.187	8.187	(1.000)	130	308132	25.0000		70.00- 130.00	100.00
8.187	8.187	(1.000)	128	247507			50.32- 110.32	80.32
8.187	8.187	(1.000)	49	991965			291.93- 351.93	321.93

* 79	1,4-Difluorobenzene					CAS #:	540-36-3	
10.067	10.067	(1.000)	114	1290059	25.0000		70.00- 130.00	100.00
10.067	10.067	(1.000)	88	229089			0.00- 47.76	17.76

* 108	Chlorobenzene-d5					CAS #:	3114-55-4	
15.099	15.099	(1.000)	117	997837	25.0000		70.00- 130.00	100.00
15.099	15.099	(1.000)	82	634003			33.54- 93.54	63.54

\$ 71	1,2-Dichloroethane-d4					CAS #:	17060-07-0	
9.265	9.265	(1.132)	65	631345	25.0000	25.560	70.00- 130.00	100.00
9.265	9.265	(1.132)	67	353451			25.98- 85.98	55.98

\$ 97	Toluene-d8					CAS #:	2037-26-5	
12.832	12.832	(1.275)	98	1169696	25.0000	24.910	70.00- 130.00	100.00
12.832	12.832	(1.275)	70	129202			0.00- 41.05	11.05

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 97 Toluene-d8 (continued)									
12.832	12.832	(1.275)	100	772486			36.04- 96.04	66.04	

\$ 122 Bromofluorobenzene									
						CAS #: 460-00-4			
16.675	16.675	(1.104)	174	618126	25.0000	24.655	70.00- 130.00	100.00	
16.675	16.675	(1.104)	95	1047686			139.49- 199.49	169.49	
16.675	16.675	(1.104)	176	616660			69.76- 129.76	99.76	

1 Propylene									
						CAS #: 115-07-1			
2.353	2.353	(0.287)	41	3879844	100.000	94.407	70.00- 130.00	100.00	
2.353	2.353	(0.287)	42	2597832			36.96- 96.96	66.96	
2.353	2.353	(0.287)	39	2626382			37.69- 97.69	67.69	

2 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
2.408	2.408	(0.294)	85	5033193	100.000	92.069	70.00- 130.00	100.00	
2.408	2.408	(0.294)	87	1591457			1.62- 61.62	31.62	

3 Freon 114									
						CAS #: 76-14-2			
2.546	2.546	(0.311)	135	5101322	100.000	97.568	70.00- 130.00	100.00	
2.546	2.546	(0.311)	137	1608156			1.52- 61.52	31.52	

4 Chloromethane									
						CAS #: 74-87-3			
2.685	2.685	(0.328)	50	4782731	100.000	96.899	70.00- 130.00	100.00	
2.685	2.685	(0.328)	52	1411565			0.00- 59.51	29.51	

5 Vinyl Chloride									
						CAS #: 75-01-4			
2.850	2.850	(0.348)	62	4066850	100.000	101.33	70.00- 130.00	100.00	
2.850	2.850	(0.348)	64	1185286			0.00- 59.15	29.15	

6 1,3-Butadiene									
						CAS #: 106-99-0			
2.850	2.850	(0.348)	54	4016871	100.000	100.83	70.00- 130.00	100.00	
2.850	2.850	(0.348)	39	4905143			92.11- 152.11	122.11	

7 Bromomethane									
						CAS #: 74-83-9			
3.376	3.376	(0.412)	94	2359109	100.000	98.942	70.00- 130.00	100.00	
3.376	3.376	(0.412)	96	2220516			64.13- 124.13	94.13	

8 Chloroethane									
						CAS #: 75-00-3			
3.514	3.514	(0.429)	64	2023968	100.000	95.097	70.00- 130.00	100.00	
3.514	3.514	(0.429)	49	644239			1.83- 61.83	31.83	
3.514	3.514	(0.429)	66	554266			0.00- 57.39	27.39	

9 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
3.846	3.846	(0.470)	101	5484992	100.000	99.531	70.00- 130.00	100.00	
3.846	3.846	(0.470)	103	3517416			34.13- 94.13	64.13	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

13 Ethanol						CAS #: 64-17-5			
4.233	4.233	(0.517)	45	1569037	100.000	92.806	70.00- 130.00	100.00	
4.233	4.233	(0.517)	43	305119			0.00- 49.45	19.45	
4.233	4.233	(0.517)	46	658234			11.95- 71.95	41.95	

19 Freon 113						CAS #: 76-13-1			
4.648	4.648	(0.568)	151	3409505	100.000	101.05	70.00- 130.00	100.00	
4.648	4.648	(0.568)	153	2148525			33.02- 93.02	63.02	
4.648	4.648	(0.568)	101	4406174			99.23- 159.23	129.23	

20 1,1-Dichloroethene						CAS #: 75-35-4			
4.675	4.675	(0.571)	61	5199006	100.000	98.815	70.00- 130.00	100.00	
4.675	4.675	(0.571)	96	2434705			16.83- 76.83	46.83	
4.675	4.675	(0.571)	98	1570825			0.21- 60.21	30.21	

22 Acetone						CAS #: 67-64-1			
4.841	4.841	(0.591)	58	1868628	100.000	95.214	70.00- 130.00	100.00	
4.841	4.841	(0.591)	43	6688576			327.94- 387.94	357.94	

26 2-Propanol						CAS #: 67-63-0			
5.035	5.035	(0.615)	45	8032048	100.000	93.908	70.00- 130.00	100.00	
5.035	5.035	(0.615)	43	1545550			0.00- 49.24	19.24	
5.035	5.035	(0.615)	59	260764			0.00- 33.25	3.25	

25 Carbon Disulfide						CAS #: 75-15-0			
5.035	5.035	(0.615)	76	7084508	100.000	97.803	70.00- 130.00	100.00	

28 3-Chloropropene						CAS #: 107-05-1			
5.311	5.311	(0.649)	76	1204311	100.000	98.405	70.00- 130.00	100.00	
5.311	5.311	(0.649)	41	6149635			480.64- 540.64	510.64	

29 Methylene Chloride						CAS #: 75-09-2			
5.560	5.560	(0.679)	49	4779654	100.000	96.863	70.00- 130.00	100.00	
5.560	5.560	(0.679)	84	1979250			11.41- 71.41	41.41	
5.560	5.560	(0.679)	51	1413858			0.00- 59.58	29.58	

31 MTBE						CAS #: 1634-04-4			
5.892	5.892	(0.720)	73	4104171	100.000	106.61	70.00- 130.00	100.00	
5.892	5.892	(0.720)	57	1560239			8.02- 68.02	38.02	
5.892	5.892	(0.720)	41	1655494			10.34- 70.34	40.34	

32 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.947	5.947	(0.726)	96	2580935	100.000	98.377	70.00- 130.00	100.00	
5.947	5.947	(0.726)	61	4989046			163.30- 223.30	193.30	
5.947	5.947	(0.726)	98	1610606			32.40- 92.40	62.40	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Hexane						CAS #: 110-54-3			
6.279	6.279	(0.767)	57	6403104	100.000	97.072	70.00- 130.00	100.00	
6.279	6.279	(0.767)	43	4875282			46.14- 106.14	76.14	
6.279	6.279	(0.767)	86	736385			0.00- 41.50	11.50	

43 1,1-Dichloroethane						CAS #: 75-34-3			
6.721	6.721	(0.821)	63	5207169	100.000	99.236	70.00- 130.00	100.00	
6.721	6.721	(0.821)	65	1483351			0.00- 58.49	28.49	

53 2-Butanone						CAS #: 78-93-3			
7.800	7.800	(0.953)	72	1024798	100.000	101.10	70.00- 130.00	100.00	
7.800	7.800	(0.953)	43	8335090			783.34- 843.34	813.34	
7.800	7.800	(0.953)	57	545182			23.20- 83.20	53.20	

52 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.772	7.772	(0.949)	61	4014716	100.000	98.511	70.00- 130.00	100.00	
7.772	7.772	(0.949)	96	2145130			23.43- 83.43	53.43	
7.772	7.772	(0.949)	98	1366850			4.05- 64.05	34.05	

56 Tetrahydrofuran						CAS #: 109-99-9			
8.187	8.187	(1.000)	42	4868887	100.000	92.617	70.00- 130.00	100.00	
8.187	8.187	(1.000)	71	889880			0.00- 48.28	18.28	
8.187	8.187	(1.000)	72	960479			0.00- 49.73	19.73	

58 Chloroform						CAS #: 67-66-3			
8.325	8.325	(1.017)	83	3751320	100.000	99.798	70.00- 130.00	100.00	
8.325	8.325	(1.017)	85	2451973			35.36- 95.36	65.36	

62 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.574	8.574	(1.047)	97	4055971	100.000	99.068	70.00- 130.00	100.00	
8.574	8.574	(1.047)	99	2605972			34.25- 94.25	64.25	

61 Cyclohexane						CAS #: 110-82-7			
8.546	8.546	(1.044)	84	2747098	100.000	98.802	70.00- 130.00	100.00	
8.546	8.546	(1.044)	56	5740280			178.96- 238.96	208.96	
8.546	8.546	(1.044)	41	3527065			98.39- 158.39	128.39	

63 Vinyl Acetate						CAS #: 108-05-4			
6.777	6.777	(0.828)	86	630955	100.000	103.23	70.00- 130.00	100.00	
6.777	6.777	(0.828)	43	11341423			1767.50-1827.50	1797.50	
6.777	6.777	(0.828)	42	849118			104.58- 164.58	134.58	

65 Carbon Tetrachloride						CAS #: 56-23-5			
8.823	8.823	(1.078)	119	3558381	100.000	99.761	70.00- 130.00	100.00	
8.823	8.823	(1.078)	117	3745957			75.27- 135.27	105.27	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

68	2,2,4-Trimethylpentane						CAS #: 540-84-1		
9.237	9.237	(1.128)	57	15310497	100.000	97.672	70.00- 130.00	100.00	
9.237	9.237	(1.128)	56	5039229			2.91- 62.91	32.91	
9.237	9.237	(1.128)	41	4555569			0.00- 59.75	29.75	

69	Benzene						CAS #: 71-43-2		
9.237	9.237	(0.918)	78	5399733	100.000	93.220	70.00- 130.00	100.00	
9.237	9.237	(0.918)	77	1243997			0.00- 53.04	23.04	

72	1,2-Dichloroethane						CAS #: 107-06-2		
9.403	9.403	(0.934)	62	3831760	100.000	97.248	70.00- 130.00	100.00	
9.403	9.403	(0.934)	64	1171222			0.57- 60.57	30.57	

75	Heptane						CAS #: 142-82-5		
9.625	9.625	(0.956)	100	679599	100.000	86.332	70.00- 130.00	100.00	
9.625	9.625	(0.956)	43	7433656			1063.83-1123.83	1093.83	
9.625	9.625	(0.956)	71	1953286			257.42- 317.42	287.42	

80	Trichloroethene						CAS #: 79-01-6		
10.482	10.482	(1.041)	95	2278344	100.000	93.830	70.00- 130.00	100.00	
10.482	10.482	(1.041)	130	2102331			62.27- 122.27	92.27	
10.482	10.482	(1.041)	97	1474171			34.70- 94.70	64.70	

82	1,2-Dichloropropane						CAS #: 78-87-5		
10.979	10.979	(1.091)	63	2413976	100.000	95.673	70.00- 130.00	100.00	
10.979	10.979	(1.091)	62	1824908			45.60- 105.60	75.60	
10.979	10.979	(1.091)	41	2274016			64.20- 124.20	94.20	

84	1,4-Dioxane						CAS #: 123-91-1		
11.201	11.201	(1.113)	88	1187787	100.000	91.478	70.00- 130.00	100.00	
11.201	11.201	(1.113)	58	1452095			92.25- 152.25	122.25	
11.201	11.201	(1.113)	57	491962			11.42- 71.42	41.42	

85	Bromodichloromethane						CAS #: 75-27-4		
11.532	11.532	(1.146)	83	3609641	100.000	100.63	70.00- 130.00	100.00	
11.532	11.532	(1.146)	85	2290045			33.44- 93.44	63.44	

90	cis-1,3-Dichloropropene						CAS #: 10061-01-5		
12.445	12.445	(1.236)	75	2612482	100.000	100.94	70.00- 130.00	100.00	
12.445	12.445	(1.236)	77	813057			1.12- 61.12	31.12	
12.445	12.445	(1.236)	39	2745467			75.09- 135.09	105.09	

91	4-Methyl-2-pentanone						CAS #: 108-10-1		
12.721	12.721	(1.264)	58	2456307	100.000	98.957	70.00- 130.00	100.00	
12.721	12.721	(1.264)	43	8030829			296.95- 356.95	326.95	
12.721	12.721	(1.264)	85	678307			0.00- 57.61	27.61	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
99 Toluene						CAS #: 108-88-3			
12.942	12.942	(1.286)	91	5347388	100.000	96.128	70.00- 130.00	100.00	
12.942	12.942	(1.286)	92	3160182			29.10- 89.10	59.10	

100 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.468	13.468	(0.892)	75	2877329	100.000	102.62	70.00- 130.00	100.00	
13.468	13.468	(0.892)	77	942837			2.77- 62.77	32.77	
13.468	13.468	(0.892)	39	2767706			66.19- 126.19	96.19	

101 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.744	13.744	(0.910)	97	1839021	100.000	97.156	70.00- 130.00	100.00	
13.744	13.744	(0.910)	99	1112402			30.49- 90.49	60.49	
13.744	13.744	(0.910)	83	1498571			51.49- 111.49	81.49	

102 Tetrachloroethene						CAS #: 127-18-4			
13.800	13.800	(0.914)	166	2197559	100.000	92.830	70.00- 130.00	100.00	
13.800	13.800	(0.914)	129	1844801			53.95- 113.95	83.95	
13.800	13.800	(0.914)	131	1772251			50.65- 110.65	80.65	

103 2-Hexanone						CAS #: 591-78-6			
14.131	14.131	(0.936)	58	3394161	100.000	95.901	70.00- 130.00	100.00	
14.131	14.131	(0.936)	43	8110792			208.96- 268.96	238.96	
14.131	14.131	(0.936)	100	433695			0.00- 42.78	12.78	

105 Dibromochloromethane						CAS #: 124-48-1			
14.297	14.297	(0.947)	129	3095365	100.000	100.45	70.00- 130.00	100.00	
14.297	14.297	(0.947)	127	2438261			48.77- 108.77	78.77	

106 1,2-Dibromoethane						CAS #: 106-93-4			
14.463	14.463	(0.958)	107	2872558	100.000	99.293	70.00- 130.00	100.00	
14.463	14.463	(0.958)	109	2696963			63.89- 123.89	93.89	

109 Chlorobenzene						CAS #: 108-90-7			
15.154	15.154	(1.004)	112	4259591	100.000	93.214	70.00- 130.00	100.00	
15.154	15.154	(1.004)	114	1394183			2.73- 62.73	32.73	
15.154	15.154	(1.004)	77	2739957			34.32- 94.32	64.32	

111 Ethyl Benzene						CAS #: 100-41-4			
15.265	15.265	(1.011)	106	2277050	100.000	101.40	70.00- 130.00	100.00	
15.265	15.265	(1.011)	91	8020329			322.22- 382.22	352.22	

113 m,p-Xylene						CAS #: 108-38-3			
15.431	15.431	(1.022)	106	2838789	100.000	97.094	70.00- 130.00	100.00	
15.431	15.431	(1.022)	91	6613844			202.98- 262.98	232.98	

114 o-Xylene						CAS #: 95-47-6			
15.956	15.956	(1.057)	106	2642508	100.000	95.570	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	6440442			213.72- 273.72	243.72	

115 Styrene CAS #: 100-42-5									
16.012	16.012	(1.060)	104	4239974	100.000	104.91	70.00- 130.00	100.00	
16.012	16.012	(1.060)	78	2624755			31.90- 91.90	61.90	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	2726657	100.000	103.25	70.00- 130.00	100.00	
16.260	16.260	(1.077)	171	1440322			22.82- 82.82	52.82	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	4047765	100.000	93.726	70.00- 130.00	100.00	
16.896	16.896	(1.119)	85	2647483			35.41- 95.41	65.41	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	9535697	100.000	100.44	70.00- 130.00	100.00	
17.062	17.062	(1.130)	120	2702404			0.00- 58.34	28.34	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	7805911	100.000	98.064	70.00- 130.00	100.00	
17.145	17.145	(1.135)	120	3635863			16.58- 76.58	46.58	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	8458160	100.000	98.966	70.00- 130.00	100.00	
17.532	17.532	(1.161)	120	3622293			12.83- 72.83	42.83	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	5183315	100.000	92.525	70.00- 130.00	100.00	
17.836	17.836	(1.181)	148	3271653			33.12- 93.12	63.12	
17.836	17.836	(1.181)	111	2372815			15.78- 75.78	45.78	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	4281403	100.000	96.646	70.00- 130.00	100.00	
17.919	17.919	(1.187)	148	2754246			34.33- 94.33	64.33	
17.919	17.919	(1.187)	111	2075867			18.49- 78.49	48.49	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.058	18.058	(1.196)	91	8386201	100.000	113.46	70.00- 130.00	100.00	
18.058	18.058	(1.196)	126	1430784			0.00- 47.06	17.06	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	5158293	100.000	88.766	70.00- 130.00	100.00	
18.279	18.279	(1.211)	148	3250770			33.02- 93.02	63.02	
18.279	18.279	(1.211)	111	2421915			16.95- 76.95	46.95	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.578	19.578	(1.297)	180	3741818	100.000	91.563	70.00- 130.00	100.00	
19.578	19.578	(1.297)	182	3462449			62.53- 122.53	92.53	

155	Hexachlorobutadiene					CAS #: 87-68-3			
19.661	19.661	(1.302)	225	2851907	100.000	84.214	70.00- 130.00	100.00	
19.661	19.661	(1.302)	223	1744085			31.16- 91.16	61.16	

124	Propylbenzene					CAS #: 103-65-1			
16.924	16.924	(1.121)	91	11020317	100.000	100.33	70.00- 130.00	100.00	
16.924	16.924	(1.121)	120	2262141			0.00- 50.53	20.53	
16.924	16.924	(1.121)	105	387472			0.00- 33.52	3.52	

119	Cumene					CAS #: 98-82-8			
16.426	16.426	(1.088)	105	8302219	100.000	98.277	70.00- 130.00	100.00	
16.426	16.426	(1.088)	120	2117285			0.00- 55.50	25.50	
16.426	16.426	(1.088)	51	1730031			0.00- 50.84	20.84	

156	Naphthalene					CAS #: 91-20-3			
19.744	19.744	(1.308)	128	11598716	100.000	95.612	70.00- 130.00	100.00	
19.744	19.744	(1.308)	127	1496376			0.00- 42.90	12.90	

30	Isopentane					CAS #: 78-78-4			
3.514	3.514	(0.429)	43	6604801	100.000	94.789	70.00- 130.00	100.00	
3.514	3.514	(0.429)	57	3984828			30.33- 90.33	60.33	
3.514	3.514	(0.429)	72	310048			0.00- 34.69	4.69	

21	Butane					CAS #: 106-97-8			
2.767	2.767	(0.338)	58	1061151	100.000	93.353	70.00- 130.00	100.00	
2.767	2.767	(0.338)	43	8524222			773.30- 833.30	803.30	

96	Methyl Cyclohexane					CAS #: 108-87-2			
10.703	10.703	(1.063)	83	3179405	100.000	92.594	70.00- 130.00	100.00	
10.703	10.703	(1.063)	98	1608008			20.58- 80.58	50.58	
10.703	10.703	(1.063)	55	4935422			125.23- 185.23	155.23	

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052916.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	308132	-1.80
79 1,4-Difluorobenze	1277249	766349	1788149	1290059	1.00
108 Chlorobenzene-d5	1008759	605255	1412263	997837	-1.08

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.19	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-29maj.b/5052916.d
 Date: 29-May-2007 18:02
 Client ID: Level 6
 Sample Info: 100mL #1487-288

Column phase: RTX-624

Instrument: msd5.1
 Operator: JG
 Column diameter: 0.53

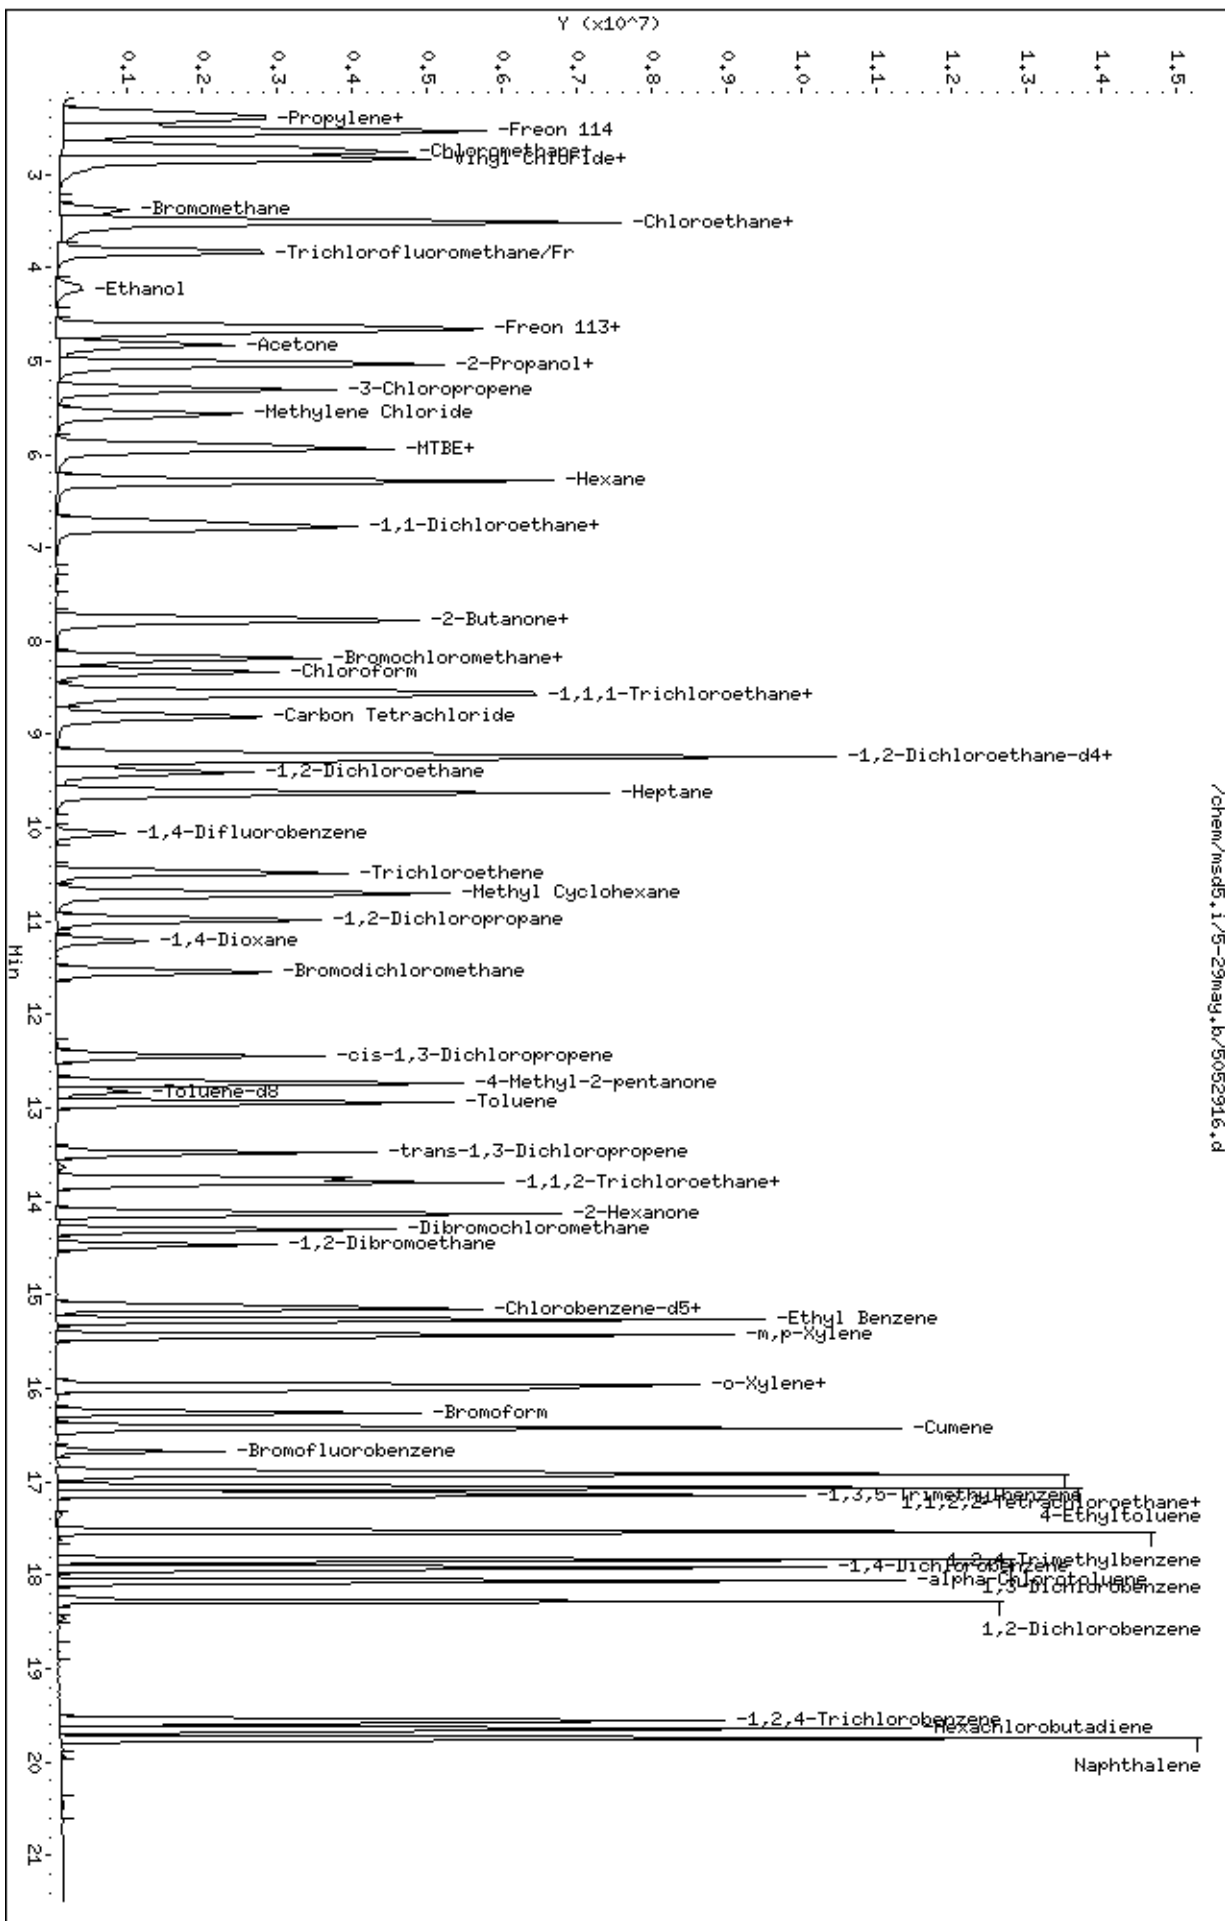

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-29may.b/5052917.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 29-MAY-2007 18:31
 Operator : JG Inst ID: msd5.i
 Smp Info : 200mL #1487-288
 Misc Info : 200ppbv-200ppbv
 Comment :
 Method : /chem/msd5.i/5-29may.b/t14q529a.m
 Meth Date : 30-May-2007 15:39 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 18:31 Cal File: 5052917.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 57 Bromochloromethane CAS #: 74-97-5									
8.214	8.214	(1.000)	130	311601	25.0000		70.00- 130.00	100.00	
8.214	8.214	(1.000)	128	254347			50.32- 110.32	81.63	
8.187	8.187	(1.000)	49	1022869			291.93- 351.93	328.26	

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	1306041	25.0000		70.00- 130.00	100.00	
10.067	10.067	(1.000)	88	235493			0.00- 47.76	18.03	

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	1015050	25.0000		70.00- 130.00	100.00	
15.099	15.099	(1.000)	82	657859			33.54- 93.54	64.81	

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.128)	65	707999	25.0000	28.344	70.00- 130.00	100.00	
9.265	9.265	(1.128)	67	454516			25.98- 85.98	64.20	

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	1192853	25.0000	25.092	70.00- 130.00	100.00	
12.832	12.832	(1.275)	70	122977			0.00- 41.05	10.31	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 97 Toluene-d8 (continued)									
12.832	12.832	(1.275)	100	847642			36.04- 96.04	71.06	

\$ 122 Bromofluorobenzene CAS #: 460-00-4									
16.675	16.675	(1.104)	174	653382	25.0000	25.620	70.00- 130.00	100.00	
16.675	16.675	(1.104)	95	1082477			139.49- 199.49	165.67	
16.675	16.675	(1.104)	176	631949			69.76- 129.76	96.72	

1 Propylene CAS #: 115-07-1									
2.353	2.353	(0.286)	41	7610915	200.000	183.13	70.00- 130.00	100.00	
2.353	2.353	(0.286)	42	5059607			36.96- 96.96	66.48	
2.353	2.353	(0.286)	39	5181095			37.69- 97.69	68.07	

2 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.408	2.408	(0.293)	85	11120306	200.000	201.15	70.00- 130.00	100.00(A)	
2.408	2.408	(0.293)	87	3600922			1.62- 61.62	32.38	

3 Freon 114 CAS #: 76-14-2									
2.574	2.574	(0.313)	135	9791972	200.000	185.20	70.00- 130.00	100.00	
2.574	2.574	(0.313)	137	3092102			1.52- 61.52	31.58	

4 Chloromethane CAS #: 74-87-3									
2.712	2.712	(0.330)	50	8634661	200.000	172.99	70.00- 130.00	100.00	
2.712	2.712	(0.330)	52	2502871			0.00- 59.51	28.99	

5 Vinyl Chloride CAS #: 75-01-4									
2.850	2.850	(0.347)	62	7986588	200.000	196.77	70.00- 130.00	100.00	
2.850	2.850	(0.347)	64	2363393			0.00- 59.15	29.59	

6 1,3-Butadiene CAS #: 106-99-0									
2.850	2.850	(0.347)	54	7889222	200.000	195.82	70.00- 130.00	100.00	
2.850	2.850	(0.347)	39	9912886			92.11- 152.11	125.65	

7 Bromomethane CAS #: 74-83-9									
3.376	3.376	(0.411)	94	4669479	200.000	193.66	70.00- 130.00	100.00	
3.376	3.376	(0.411)	96	4386551			64.13- 124.13	93.94	

8 Chloroethane CAS #: 75-00-3									
3.542	3.542	(0.431)	64	3937068	200.000	182.92	70.00- 130.00	100.00	
3.542	3.542	(0.431)	49	1326662			1.83- 61.83	33.70	
3.542	3.542	(0.431)	66	1093780			0.00- 57.39	27.78	

9 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
3.846	3.846	(0.468)	101	10954255	200.000	196.56	70.00- 130.00	100.00	
3.846	3.846	(0.468)	103	7062299			34.13- 94.13	64.47	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
13 Ethanol						CAS #: 64-17-5			
4.260	4.260	(0.519)	45	3233825	200.000	189.14	70.00- 130.00	100.00	
4.260	4.260	(0.519)	43	606805			0.00- 49.45	18.76	
4.260	4.260	(0.519)	46	1345732			11.95- 71.95	41.61	

19 Freon 113						CAS #: 76-13-1			
4.648	4.648	(0.566)	151	6592063	200.000	193.19	70.00- 130.00	100.00	
4.648	4.648	(0.566)	153	4201876			33.02- 93.02	63.74	
4.648	4.648	(0.566)	101	8659295			99.23- 159.23	131.36	

20 1,1-Dichloroethene						CAS #: 75-35-4			
4.703	4.703	(0.573)	61	10409747	200.000	195.65	70.00- 130.00	100.00	
4.703	4.703	(0.573)	96	4849812			16.83- 76.83	46.59	
4.703	4.703	(0.573)	98	3028738			0.21- 60.21	29.10	

22 Acetone						CAS #: 67-64-1			
4.841	4.841	(0.589)	58	3838077	200.000	193.39	70.00- 130.00	100.00	
4.841	4.841	(0.589)	43	13290914			327.94- 387.94	346.29	

26 2-Propanol						CAS #: 67-63-0			
5.035	5.035	(0.613)	45	16172441	200.000	186.98	70.00- 130.00	100.00	
5.035	5.035	(0.613)	43	3066653			0.00- 49.24	18.96	
5.035	5.035	(0.613)	59	522092			0.00- 33.25	3.23	

25 Carbon Disulfide						CAS #: 75-15-0			
5.035	5.035	(0.613)	76	14269656	200.000	194.80	70.00- 130.00	100.00	

28 3-Chloropropene						CAS #: 107-05-1			
5.311	5.311	(0.647)	76	2377652	200.000	192.12	70.00- 130.00	100.00	
5.311	5.311	(0.647)	41	12128414			480.64- 540.64	510.10	

29 Methylene Chloride						CAS #: 75-09-2			
5.588	5.588	(0.680)	49	9422323	200.000	188.82	70.00- 130.00	100.00	
5.588	5.588	(0.680)	84	3913369			11.41- 71.41	41.53	
5.588	5.588	(0.680)	51	2783900			0.00- 59.58	29.55	

31 MTBE						CAS #: 1634-04-4			
5.892	5.892	(0.717)	73	7067928	200.000	181.55	70.00- 130.00	100.00	
5.892	5.892	(0.717)	57	2729388			8.02- 68.02	38.62	
5.892	5.892	(0.717)	41	2774227			10.34- 70.34	39.25	

32 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.947	5.947	(0.724)	96	5006508	200.000	188.71	70.00- 130.00	100.00	
5.947	5.947	(0.724)	61	9884360			163.30- 223.30	197.43	
5.947	5.947	(0.724)	98	3206398			32.40- 92.40	64.04	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Hexane						CAS #: 110-54-3			
6.279	6.279	(0.764)	57	12684813	200.000	190.16	70.00- 130.00	100.00	
6.279	6.279	(0.764)	43	9609118			46.14- 106.14	75.75	
6.307	6.307	(0.768)	86	1442359			0.00- 41.50	11.37	

43 1,1-Dichloroethane						CAS #: 75-34-3			
6.721	6.721	(0.818)	63	10408193	200.000	196.15	70.00- 130.00	100.00	
6.721	6.721	(0.818)	65	3024070			0.00- 58.49	29.05	

53 2-Butanone						CAS #: 78-93-3			
7.800	7.800	(0.950)	72	2026920	200.000	197.73	70.00- 130.00	100.00	
7.800	7.800	(0.950)	43	16911919			783.34- 843.34	834.37	
7.800	7.800	(0.950)	57	1096576			23.20- 83.20	54.10	

52 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.772	7.772	(0.946)	61	7881475	200.000	191.24	70.00- 130.00	100.00	
7.772	7.772	(0.946)	96	4217655			23.43- 83.43	53.51	
7.772	7.772	(0.946)	98	2704729			4.05- 64.05	34.32	

56 Tetrahydrofuran						CAS #: 109-99-9			
8.187	8.187	(0.997)	42	9697540	200.000	182.41	70.00- 130.00	100.00	
8.187	8.187	(0.997)	71	1752371			0.00- 48.28	18.07	
8.187	8.187	(0.997)	72	1915705			0.00- 49.73	19.75	

58 Chloroform						CAS #: 67-66-3			
8.325	8.325	(1.013)	83	7517837	200.000	197.77	70.00- 130.00	100.00	
8.325	8.325	(1.013)	85	4864330			35.36- 95.36	64.70	

62 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.574	8.574	(1.044)	97	8147060	200.000	196.78	70.00- 130.00	100.00	
8.574	8.574	(1.044)	99	5190937			34.25- 94.25	63.72	

61 Cyclohexane						CAS #: 110-82-7			
8.546	8.546	(1.040)	84	5390315	200.000	191.71	70.00- 130.00	100.00	
8.546	8.546	(1.040)	56	11510598			178.96- 238.96	213.54	
8.546	8.546	(1.040)	41	7019487			98.39- 158.39	130.22	

63 Vinyl Acetate						CAS #: 108-05-4			
6.804	6.804	(0.828)	86	1265458	200.000	204.74	70.00- 130.00	100.00(A)	
6.777	6.777	(0.825)	43	23335670			1767.50-1827.50	1844.05	
6.777	6.777	(0.825)	42	1723684			104.58- 164.58	136.21	

65 Carbon Tetrachloride						CAS #: 56-23-5			
8.823	8.823	(1.074)	119	7313294	200.000	202.75	70.00- 130.00	100.00(A)	
8.823	8.823	(1.074)	117	7567558			75.27- 135.27	103.48	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

68	2,2,4-Trimethylpentane				CAS #: 540-84-1				
9.237	9.237	(1.125)	57	29998509	200.000	189.24	70.00- 130.00	100.00	
9.237	9.237	(1.125)	56	9991359			2.91- 62.91	33.31	
9.237	9.237	(1.125)	41	8983000			0.00- 59.75	29.94	

69	Benzene				CAS #: 71-43-2				
9.237	9.237	(0.918)	78	10596976	200.000	180.71	70.00- 130.00	100.00	
9.237	9.237	(0.918)	77	2475897			0.00- 53.04	23.36	

72	1,2-Dichloroethane				CAS #: 107-06-2				
9.403	9.403	(0.934)	62	7787936	200.000	195.23	70.00- 130.00	100.00	
9.403	9.403	(0.934)	64	2300497			0.57- 60.57	29.54	

75	Heptane				CAS #: 142-82-5				
9.624	9.624	(0.956)	100	1374422	200.000	172.46	70.00- 130.00	100.00	
9.624	9.624	(0.956)	43	15000867			1063.83-1123.83	1091.43	
9.624	9.624	(0.956)	71	3890710			257.42- 317.42	283.08	

80	Trichloroethene				CAS #: 79-01-6				
10.482	10.482	(1.041)	95	4546558	200.000	184.95	70.00- 130.00	100.00	
10.482	10.482	(1.041)	130	4231407			62.27- 122.27	93.07	
10.482	10.482	(1.041)	97	2923838			34.70- 94.70	64.31	

82	1,2-Dichloropropane				CAS #: 78-87-5				
10.979	10.979	(1.091)	63	4909719	200.000	192.20	70.00- 130.00	100.00	
10.979	10.979	(1.091)	62	3592121			45.60- 105.60	73.16	
10.979	10.979	(1.091)	41	4487523			64.20- 124.20	91.40	

84	1,4-Dioxane				CAS #: 123-91-1				
11.200	11.200	(1.113)	88	2376895	200.000	180.82	70.00- 130.00	100.00	
11.200	11.200	(1.113)	58	2881491			92.25- 152.25	121.23	
11.200	11.200	(1.113)	57	942507			11.42- 71.42	39.65	

85	Bromodichloromethane				CAS #: 75-27-4				
11.532	11.532	(1.146)	83	7281120	200.000	200.50	70.00- 130.00	100.00(A)	
11.532	11.532	(1.146)	85	4622385			33.44- 93.44	63.48	

90	cis-1,3-Dichloropropene				CAS #: 10061-01-5				
12.445	12.445	(1.236)	75	5147361	200.000	196.46	70.00- 130.00	100.00	
12.445	12.445	(1.236)	77	1635309			1.12- 61.12	31.77	
12.445	12.445	(1.236)	39	5600062			75.09- 135.09	108.79	

91	4-Methyl-2-pentanone				CAS #: 108-10-1				
12.721	12.721	(1.264)	58	4940698	200.000	196.61	70.00- 130.00	100.00	
12.721	12.721	(1.264)	43	16261496			296.95- 356.95	329.13	
12.721	12.721	(1.264)	85	1350014			0.00- 57.61	27.32	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
99 Toluene						CAS #: 108-88-3			
12.942	12.942	(1.286)	91	10572151	200.000	187.73	70.00- 130.00	100.00	
12.942	12.942	(1.286)	92	6337907			29.10- 89.10	59.95	

100 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.468	13.468	(0.892)	75	5849078	200.000	205.08	70.00- 130.00	100.00(A)	
13.468	13.468	(0.892)	77	1863853			2.77- 62.77	31.87	
13.468	13.468	(0.892)	39	5629501			66.19- 126.19	96.25	

101 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.744	13.744	(0.910)	97	3619415	200.000	187.97	70.00- 130.00	100.00	
13.744	13.744	(0.910)	99	2250575			30.49- 90.49	62.18	
13.744	13.744	(0.910)	83	2943200			51.49- 111.49	81.32	

102 Tetrachloroethene						CAS #: 127-18-4			
13.800	13.800	(0.914)	166	4340016	200.000	180.22	70.00- 130.00	100.00	
13.800	13.800	(0.914)	129	3646060			53.95- 113.95	84.01	
13.800	13.800	(0.914)	131	3440037			50.65- 110.65	79.26	

103 2-Hexanone						CAS #: 591-78-6			
14.131	14.131	(0.936)	58	6944992	200.000	192.90	70.00- 130.00	100.00	
14.131	14.131	(0.936)	43	16514542			208.96- 268.96	237.79	
14.131	14.131	(0.936)	100	839072			0.00- 42.78	12.08	

105 Dibromochloromethane						CAS #: 124-48-1			
14.297	14.297	(0.947)	129	6326805	200.000	201.84	70.00- 130.00	100.00(A)	
14.297	14.297	(0.947)	127	4939086			48.77- 108.77	78.07	

106 1,2-Dibromoethane						CAS #: 106-93-4			
14.463	14.463	(0.958)	107	5668890	200.000	192.63	70.00- 130.00	100.00	
14.463	14.463	(0.958)	109	5302620			63.89- 123.89	93.54	

109 Chlorobenzene						CAS #: 108-90-7			
15.154	15.154	(1.004)	112	8453821	200.000	181.86	70.00- 130.00	100.00	
15.154	15.154	(1.004)	114	2681212			2.73- 62.73	31.72	
15.154	15.154	(1.004)	77	5475393			34.32- 94.32	64.77	

111 Ethyl Benzene						CAS #: 100-41-4			
15.265	15.265	(1.011)	106	4440393	200.000	194.38	70.00- 130.00	100.00	
15.265	15.265	(1.011)	91	15885893			322.22- 382.22	357.76	

113 m,p-Xylene						CAS #: 108-38-3			
15.431	15.431	(1.022)	106	5576004	200.000	187.48	70.00- 130.00	100.00	
15.431	15.431	(1.022)	91	13064272			202.98- 262.98	234.29	

114 o-Xylene						CAS #: 95-47-6			
15.956	15.956	(1.057)	106	5184008	200.000	184.31	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	12782837			213.72- 273.72	246.58	

115 Styrene CAS #: 100-42-5									
16.012	16.012	(1.060)	104	8546552	200.000	207.89	70.00- 130.00	100.00(A)	
16.012	16.012	(1.060)	78	5250640			31.90- 91.90	61.44	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	5543024	200.000	206.34	70.00- 130.00	100.00(A)	
16.260	16.260	(1.077)	171	2832334			22.82- 82.82	51.10	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	7863927	200.000	179.00	70.00- 130.00	100.00	
16.896	16.896	(1.119)	85	5093859			35.41- 95.41	64.78	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	15781622	200.000	163.41	70.00- 130.00	100.00	
17.062	17.062	(1.130)	120	5346801			0.00- 58.34	33.88	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	15768476	200.000	194.74	70.00- 130.00	100.00	
17.145	17.145	(1.135)	120	7195408			16.58- 76.58	45.63	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	15040233	200.000	173.00	70.00- 130.00	100.00	
17.532	17.532	(1.161)	120	6888328			12.83- 72.83	45.80	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	9882802	200.000	173.42	70.00- 130.00	100.00	
17.836	17.836	(1.181)	148	6212153			33.12- 93.12	62.86	
17.836	17.836	(1.181)	111	4630904			15.78- 75.78	46.86	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	8724568	200.000	193.60	70.00- 130.00	100.00	
17.919	17.919	(1.187)	148	5439656			34.33- 94.33	62.35	
17.919	17.919	(1.187)	111	4133275			18.49- 78.49	47.38	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.058	18.058	(1.196)	91	16464946	200.000	218.99	70.00- 130.00	100.00(A)	
18.058	18.058	(1.196)	126	2840876			0.00- 47.06	17.25	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	9804876	200.000	165.86	70.00- 130.00	100.00	
18.279	18.279	(1.211)	148	6227360			33.02- 93.02	63.51	
18.279	18.279	(1.211)	111	4801844			16.95- 76.95	48.97	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.578	19.578	(1.297)	180	7132880	200.000	171.58	70.00- 130.00	100.00	
19.578	19.578	(1.297)	182	6850489			62.53- 122.53	96.04	

155	Hexachlorobutadiene					CAS #: 87-68-3			
19.661	19.661	(1.302)	225	5517576	200.000	160.17	70.00- 130.00	100.00	
19.661	19.661	(1.302)	223	3460043			31.16- 91.16	62.71	

124	Propylbenzene					CAS #: 103-65-1			
16.924	16.924	(1.121)	91	16889779	200.000	151.16	70.00- 130.00	100.00	
16.924	16.924	(1.121)	120	4448192			0.00- 50.53	26.34	
16.924	16.924	(1.121)	105	763455			0.00- 33.52	4.52	

119	Cumene					CAS #: 98-82-8			
16.426	16.426	(1.088)	105	16719164	200.000	194.56	70.00- 130.00	100.00	
16.426	16.426	(1.088)	120	4205110			0.00- 55.50	25.15	
16.426	16.426	(1.088)	51	3534766			0.00- 50.84	21.14	

156	Naphthalene					CAS #: 91-20-3			
19.744	19.744	(1.308)	128	17585232	200.000	142.50	70.00- 130.00	100.00	
19.744	19.744	(1.308)	127	2898078			0.00- 42.90	16.48	

30	Isopentane					CAS #: 78-78-4			
3.514	3.514	(0.428)	43	12983005	200.000	184.25	70.00- 130.00	100.00	
3.514	3.514	(0.428)	57	7730301			30.33- 90.33	59.54	
3.514	3.514	(0.428)	72	621098			0.00- 34.69	4.78	

21	Butane					CAS #: 106-97-8			
2.823	2.823	(0.344)	58	2126624	200.000	185.00	70.00- 130.00	100.00	
2.823	2.823	(0.344)	43	16915677			773.30- 833.30	795.42	

96	Methyl Cyclohexane					CAS #: 108-87-2			
10.703	10.703	(1.063)	83	6373668	200.000	183.35	70.00- 130.00	100.00	
10.703	10.703	(1.063)	98	3219742			20.58- 80.58	50.52	
10.703	10.703	(1.063)	55	9727631			125.23- 185.23	152.62	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 30-May-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 29-MAY-2007

Lab File ID: 5052917.d

Calibration Time: 17:34

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-29may.b/t14q529a.m

Misc Info: 200ppbv-200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	313773	188264	439282	311601	-0.69
79 1,4-Difluorobenze	1277249	766349	1788149	1306041	2.25
108 Chlorobenzene-d5	1008759	605255	1412263	1015050	0.62

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.19	7.86	8.52	8.21	0.34
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-29maj.b/5052917.d
Date: 29-May-2007 18:31
Client ID: Level 7
Sample Info: 200mL #1487-288

Column phase: RTX-624

Instrument: msd5.1
Operator: JG
Column diameter: 0.53

/chem/msd5.1/5-29maj.b/5052917.d

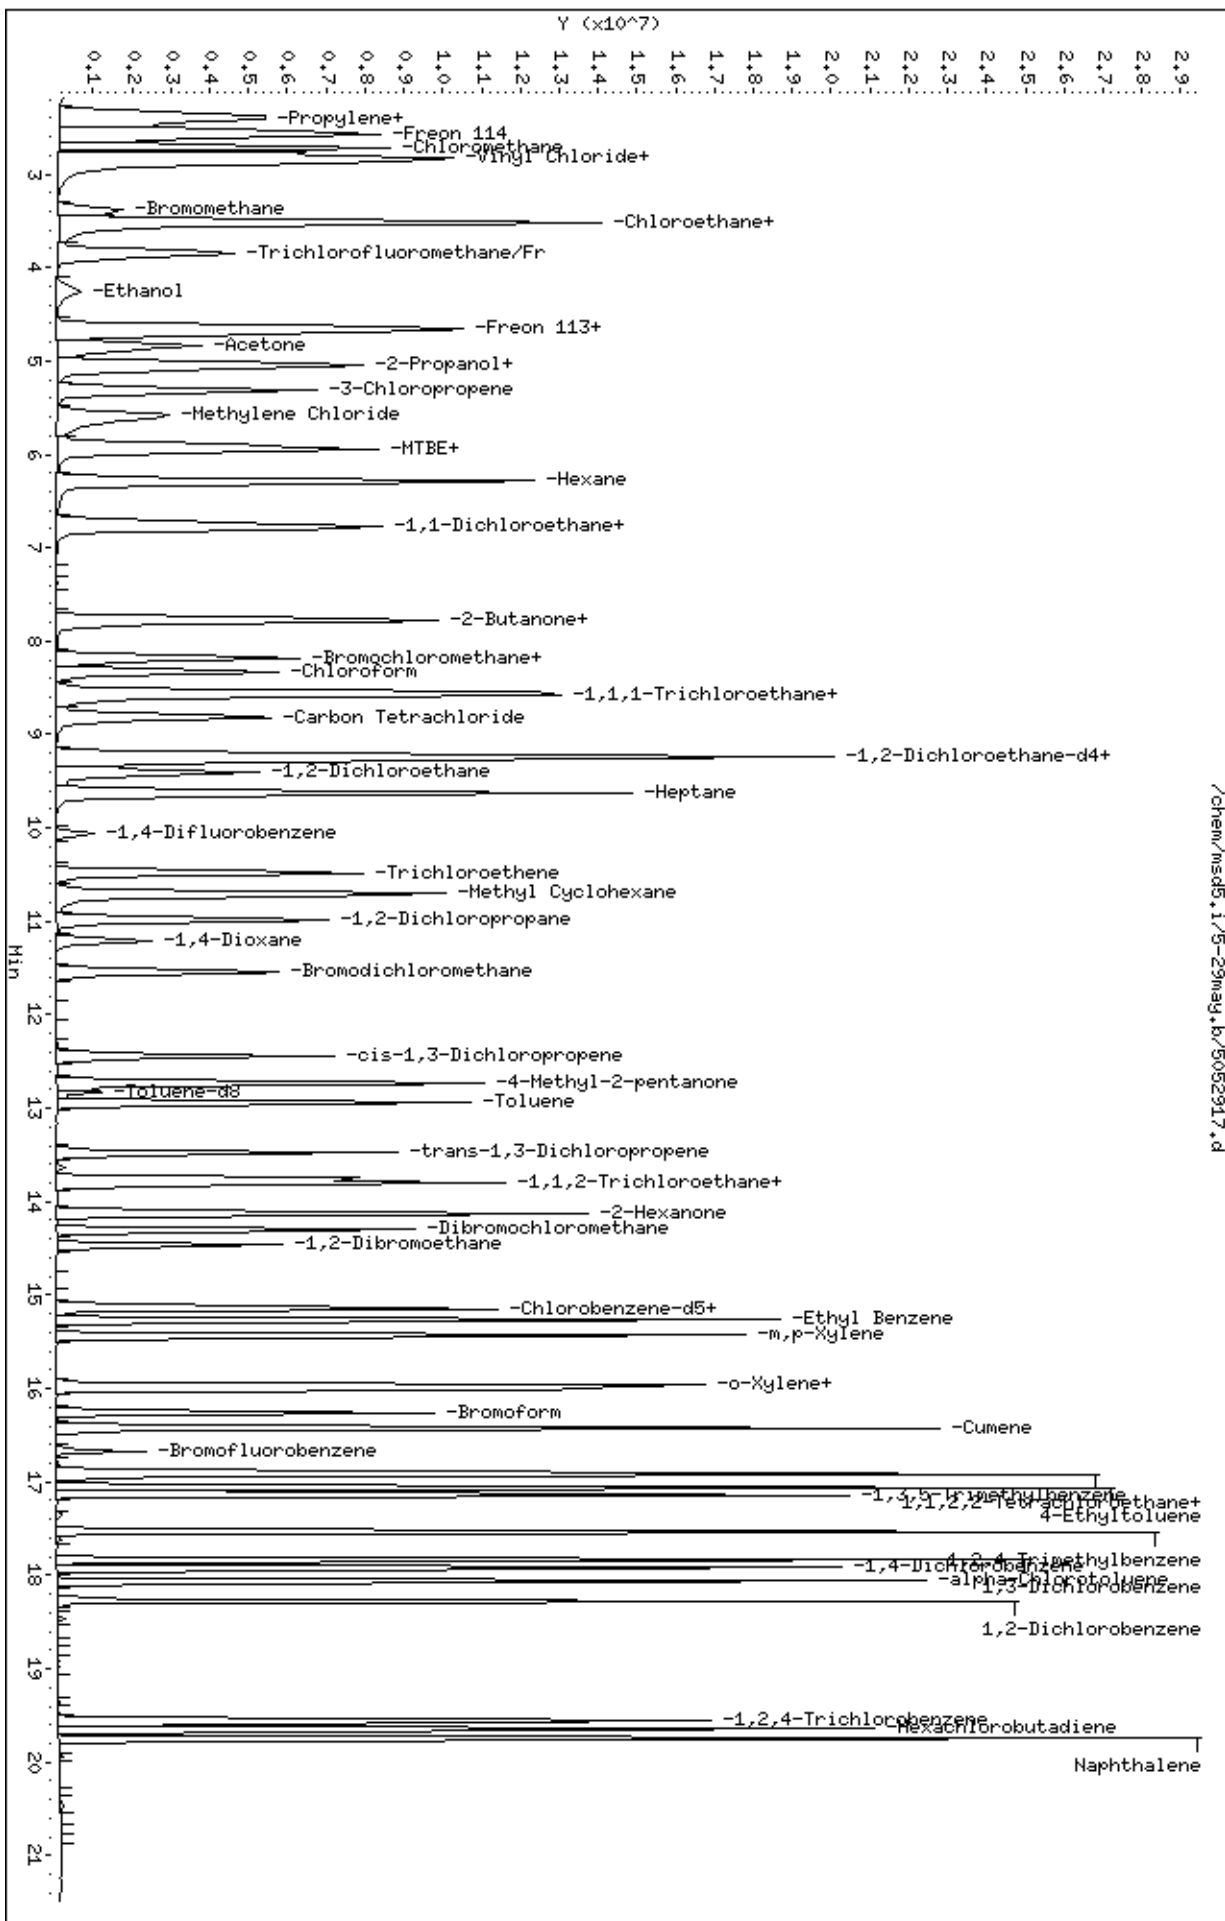



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0706057-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060709	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/7/07 01:20 PM

Compound	%Recovery
Freon 12	99
Freon 114	110
Vinyl Chloride	101
Bromomethane	108
Chloroethane	91
Freon 11	116
1,1-Dichloroethene	95
Freon 113	110
Methylene Chloride	89
1,1-Dichloroethane	94
cis-1,2-Dichloroethene	87
Chloroform	107
1,1,1-Trichloroethane	110
Carbon Tetrachloride	113
Benzene	101
1,2-Dichloroethane	113
Trichloroethene	104
1,2-Dichloropropane	91
cis-1,3-Dichloropropene	110
Toluene	104
trans-1,3-Dichloropropene	117
1,1,2-Trichloroethane	103
Tetrachloroethene	104
1,2-Dibromoethane (EDB)	106
Chlorobenzene	100
Ethyl Benzene	108
m,p-Xylene	104
o-Xylene	102
Styrene	113
1,1,2,2-Tetrachloroethane	98
1,3,5-Trimethylbenzene	111
1,2,4-Trimethylbenzene	109
1,3-Dichlorobenzene	102
1,4-Dichlorobenzene	103
alpha-Chlorotoluene	118
1,2-Dichlorobenzene	96
1,3-Butadiene	98
Hexane	82
Cyclohexane	93



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0706057-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060709	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/7/07 01:20 PM

Compound	%Recovery
Heptane	93
Bromodichloromethane	118
Dibromochloromethane	116
Cumene	110
Propylbenzene	110
Chloromethane	93
1,2,4-Trichlorobenzene	100
Hexachlorobutadiene	110
Acetone	89
Carbon Disulfide	99
2-Propanol	83
trans-1,2-Dichloroethene	100
2-Butanone (Methyl Ethyl Ketone)	95
Tetrahydrofuran	80
1,4-Dioxane	98
4-Methyl-2-pentanone	92
2-Hexanone	85
Bromoform	120
4-Ethyltoluene	110
Ethanol	82
Methyl tert-butyl ether	61 Q
3-Chloropropene	94
2,2,4-Trimethylpentane	74
Naphthalene	94

Q = Exceeds Quality Control limits.

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	104	70-130
1,2-Dichloroethane-d4	104	70-130
4-Bromofluorobenzene	106	70-130

Report Date: 07-Jun-2007 21:01

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i Injection Date: 07-JUN-2007 13:20
 Lab File ID: 5060709.d Init. Cal. Date(s): 29-MAY-2007 29-MAY-2007
 Analysis Type: AIR Init. Cal. Times: 15:42 20:44
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /chem/msd5.i/5-07jun.b/t14q529a.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 71 1,2-Dichloroethane-d4	2.00408	2.08616	0.010	-4.09557	30.00000	Averaged
\$ 97 Toluene-d8	0.90997	0.94917	0.010	-4.30827	30.00000	Averaged
\$ 122 Bromofluorobenzene	0.62813	0.66674	0.010	-6.14800	30.00000	Averaged
1 Propylene	3.33435	3.01416	0.010	9.60277	30.00000	Averaged
2 Dichlorodifluoromethane/Fr1	4.43541	4.38746	0.010	1.08091	30.00000	Averaged
3 Freon 114	4.24209	4.68528	0.010	-10.44754	30.00000	Averaged
4 Chloromethane	4.00461	3.72460	0.010	6.99226	30.00000	Averaged
5 Vinyl Chloride	3.25637	3.28608	0.010	-0.91252	30.00000	Averaged
6 1,3-Butadiene	3.23231	3.16049	0.010	2.22180	30.00000	Averaged
7 Bromomethane	1.93451	2.10033	0.010	-8.57197	30.00000	Averaged
8 Chloroethane	1.72680	1.57487	0.010	8.79791	30.00000	Averaged
9 Trichlorofluoromethane/Fr11	4.47116	5.19677	0.010	-16.22851	30.00000	Averaged
13 Ethanol	1.37171	1.11914	0.010	18.41264	30.00000	Averaged
19 Freon 113	2.73760	3.00406	0.010	-9.73306	30.00000	Averaged
20 1,1-Dichloroethene	4.26876	4.04623	0.010	5.21303	30.00000	Averaged
22 Acetone	1.59231	1.41197	0.010	11.32540	30.00000	Averaged
26 2-Propanol	6.93947	5.77249	0.010	16.81657	30.00000	Averaged
25 Carbon Disulfide	5.87706	5.79520	0.010	1.39295	30.00000	Averaged
28 3-Chloropropene	0.99294	0.93642	0.010	5.69224	30.00000	Averaged
29 Methylene Chloride	4.00350	3.57989	0.010	10.58113	30.00000	Averaged
31 MTBE	3.12343	1.90512	0.010	39.00559	30.00000	Averaged <-
32 trans-1,2-Dichloroethene	2.12856	2.12735	0.010	0.05685	30.00000	Averaged
38 Hexane	5.35177	4.39648	0.010	17.84999	30.00000	Averaged
43 1,1-Dichloroethane	4.25730	4.00407	0.010	5.94815	30.00000	Averaged
53 2-Butanone	0.82245	0.78267	0.010	4.83612	30.00000	Averaged
52 cis-1,2-Dichloroethene	3.30653	2.87137	0.010	13.16059	30.00000	Averaged
56 Tetrahydrofuran	4.26523	3.42925	0.010	19.59977	30.00000	Averaged
58 Chloroform	3.04977	3.25975	0.010	-6.88506	30.00000	Averaged
62 1,1,1-Trichloroethane	3.32174	3.67135	0.010	-10.52503	30.00000	Averaged
61 Cyclohexane	2.25587	2.10574	0.010	6.65478	30.00000	Averaged
63 Vinyl Acetate	0.49588	0.47643	0.010	3.92189	30.00000	Averaged
65 Carbon Tetrachloride	2.89398	3.27781	0.010	-13.26315	30.00000	Averaged
68 2,2,4-Trimethylpentane	12.71810	9.41307	0.010	25.98681	30.00000	Averaged
69 Benzene	1.12252	1.13461	0.010	-1.07765	30.00000	Averaged
72 1,2-Dichloroethane	0.76357	0.86081	0.010	-12.73518	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i Injection Date: 07-JUN-2007 13:20
 Lab File ID: 5060709.d Init. Cal. Date(s): 29-MAY-2007 29-MAY-2007
 Analysis Type: AIR Init. Cal. Times: 15:42 20:44
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /chem/msd5.i/5-07jun.b/tl4q529a.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE
			RRF %D / %DRIFT	%D / %DRIFT	
75 Heptane	0.15255	0.14151	0.010 7.23654	30.00000	Averaged
80 Trichloroethene	0.47055	0.49049	0.010 -4.23635	30.00000	Averaged
82 1,2-Dichloropropane	0.48896	0.44527	0.010 8.93609	30.00000	Averaged
84 1,4-Dioxane	0.25162	0.24758	0.010 1.60573	30.00000	Averaged
85 Bromodichloromethane	0.69513	0.82429	0.010 -18.57996	30.00000	Averaged
90 cis-1,3-Dichloropropene	0.50154	0.54955	0.010 -9.57361	30.00000	Averaged
91 4-Methyl-2-pentanone	0.48102	0.44288	0.010 7.92986	30.00000	Averaged
99 Toluene	1.07800	1.11703	0.010 -3.62034	30.00000	Averaged
100 trans-1,3-Dichloropropene	0.70246	0.82022	0.010 -16.76343	30.00000	Averaged
101 1,1,2-Trichloroethane	0.47424	0.48975	0.010 -3.27073	30.00000	Averaged
102 Tetrachloroethene	0.59311	0.61982	0.010 -4.50333	30.00000	Averaged
103 2-Hexanone	0.88672	0.75622	0.010 14.71685	30.00000	Averaged
105 Dibromochloromethane	0.77203	0.89443	0.010 -15.85418	30.00000	Averaged
106 1,2-Dibromoethane	0.72482	0.77042	0.010 -6.29040	30.00000	Averaged
109 Chlorobenzene	1.14489	1.14408	0.010 0.07060	30.00000	Averaged
111 Ethyl Benzene	0.56264	0.60763	0.010 -7.99620	30.00000	Averaged
113 m,p-Xylene	0.73252	0.76021	0.010 -3.77929	30.00000	Averaged
114 o-Xylene	0.69275	0.70806	0.010 -2.21047	30.00000	Averaged
115 Styrene	1.01254	1.14652	0.010 -13.23177	30.00000	Averaged
118 Bromoform	0.66163	0.79677	0.010 -20.42462	30.00000	Averaged
123 1,1,2,2-Tetrachloroethane	1.08202	1.05769	0.010 2.24886	30.00000	Averaged
126 4-Ethyltoluene	2.37857	2.62458	0.010 -10.34251	30.00000	Averaged
128 1,3,5-Trimethylbenzene	1.99431	2.21164	0.010 -10.89735	30.00000	Averaged
131 1,2,4-Trimethylbenzene	2.14127	2.34442	0.010 -9.48759	30.00000	Averaged
138 1,3-Dichlorobenzene	1.40355	1.42982	0.010 -1.87183	30.00000	Averaged
141 1,4-Dichlorobenzene	1.10990	1.14105	0.010 -2.80691	30.00000	Averaged
143 alpha-Chlorotoluene	1.85176	2.18460	0.010 -17.97398	30.00000	Averaged
146 1,2-Dichlorobenzene	1.45593	1.39841	0.010 3.95108	30.00000	Averaged
154 1,2,4-Trichlorobenzene	1.02387	1.02641	0.010 -0.24849	30.00000	Averaged
155 Hexachlorobutadiene	0.84846	0.92995	0.010 -9.60546	30.00000	Averaged
124 Propylbenzene	2.75198	3.04088	0.010 -10.49763	30.00000	Averaged
119 Cumene	2.11652	2.32259	0.010 -9.73588	30.00000	Averaged
156 Naphthalene	3.03934	2.85739	0.010 5.98654	30.00000	Averaged
30 Isopentane	5.65336	5.25952	0.010 6.96649	30.00000	Averaged
21 Butane	0.92225	0.84993	0.010 7.84262	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i Injection Date: 07-JUN-2007 13:20
Lab File ID: 5060709.d Init. Cal. Date(s): 29-MAY-2007 29-MAY-2007
Analysis Type: AIR Init. Cal. Times: 15:42 20:44
Lab Sample ID: CCV-1 Quant Type: ISTD
Method: /chem/msd5.i/5-07jun.b/t14q529a.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE
96 Methyl Cyclohexane	0.66541	0.62104	0.010	6.66907	30.00000 Averaged

Report Date: 07-Jun-2007 21:01

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-07jun.b/5060709.d
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1
 Inj Date : 07-JUN-2007 13:20
 Operator : JG Inst ID: msd5.i
 Smp Info : 50mL #1487-286
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /chem/msd5.i/5-07jun.b/t14q529a.m
 Meth Date : 07-Jun-2007 21:01 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 57 Bromochloromethane CAS #: 74-97-5									
8.214	8.214	(1.000)	130	292964	25.0000		80.00- 120.00	100.00	
8.214	8.214	(1.000)	128	230121			48.55- 108.55	78.55	
8.187	8.187	(1.000)	49	759680			229.31- 289.31	259.31	

* 79 1,4-Difluorobenzene CAS #: 540-36-3									
10.067	10.067	(1.000)	114	1106143	25.0000		80.00- 120.00	100.00	
10.067	10.067	(1.000)	88	220897			0.00- 49.97	19.97	

* 108 Chlorobenzene-d5 CAS #: 3114-55-4									
15.099	15.099	(1.000)	117	855448	25.0000		80.00- 120.00	100.00	
15.099	15.099	(1.000)	82	590229			33.54- 93.54	69.00	

\$ 71 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.265	9.265	(1.128)	65	611170	25.0000	26.024	80.00- 120.00	100.00	
9.265	9.265	(1.128)	67	300036			25.98- 85.98	49.09	

\$ 97 Toluene-d8 CAS #: 2037-26-5									
12.832	12.832	(1.275)	98	1049922	25.0000	26.077	80.00- 120.00	100.00	
12.832	12.832	(1.275)	70	121821			0.00- 41.05	11.60	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 97 Toluene-d8 (continued)									
12.832	12.832	(1.275)	100	682145			36.04- 96.04	64.97	

\$ 122 Bromofluorobenzene CAS #: 460-00-4									
16.675	16.675	(1.104)	174	570364	25.0000	26.537	80.00- 120.00	100.00	
16.675	16.675	(1.104)	95	951939			136.90- 196.90	166.90	
16.675	16.675	(1.104)	176	540379			64.74- 124.74	94.74	

1 Propylene CAS #: 115-07-1									
2.380	2.380	(0.290)	41	1766083	50.0000	45.199	80.00- 120.00	100.00	
2.380	2.380	(0.290)	42	1198841			36.96- 96.96	67.88	
2.380	2.380	(0.290)	39	1222843			37.69- 97.69	69.24	

2 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.436	2.436	(0.296)	85	2570738	50.0000	49.460	80.00- 120.00	100.00	
2.436	2.436	(0.296)	87	827723			1.62- 61.62	32.20	

3 Freon 114 CAS #: 76-14-2									
2.546	2.546	(0.310)	135	2745239	50.0000	55.224	80.00- 120.00	100.00	
2.546	2.546	(0.310)	137	856152			1.19- 61.19	31.19	

4 Chloromethane CAS #: 74-87-3									
2.712	2.712	(0.330)	50	2182347	50.0000	46.504	80.00- 120.00	100.00	
2.712	2.712	(0.330)	52	637311			0.00- 59.51	29.20	

5 Vinyl Chloride CAS #: 75-01-4									
2.878	2.878	(0.350)	62	1925408	50.0000	50.456	80.00- 120.00	100.00	
2.878	2.878	(0.350)	64	563764			0.00- 59.15	29.28	

6 1,3-Butadiene CAS #: 106-99-0									
2.850	2.850	(0.347)	54	1851821	50.0000	48.889	80.00- 120.00	100.00	
2.850	2.850	(0.347)	39	2230423			92.11- 152.11	120.44	

7 Bromomethane CAS #: 74-83-9									
3.403	3.403	(0.414)	94	1230644	50.0000	54.286	80.00- 120.00	100.00	
3.403	3.403	(0.414)	96	1116286			60.71- 120.71	90.71	

8 Chloroethane CAS #: 75-00-3									
3.542	3.542	(0.431)	64	922763	50.0000	45.601	80.00- 120.00	100.00	
3.542	3.542	(0.431)	49	324664			1.83- 61.83	35.18	
3.542	3.542	(0.431)	66	296459			0.00- 57.39	32.13	

9 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
3.846	3.846	(0.468)	101	3044932	50.0000	58.114	80.00- 120.00	100.00	
3.846	3.846	(0.468)	103	1967994			34.63- 94.63	64.63	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

13 Ethanol						CAS #: 64-17-5			
4.205	4.205	(0.512)	45	655736	50.0000	40.794	80.00-	120.00	100.00
4.205	4.205	(0.512)	43	139019			0.00-	49.45	21.20
4.205	4.205	(0.512)	46	285910			11.95-	71.95	43.60

19 Freon 113						CAS #: 76-13-1			
4.675	4.675	(0.569)	151	1760160	50.0000	54.866	80.00-	120.00	100.00
4.675	4.675	(0.569)	153	1070168			30.80-	90.80	60.80
4.648	4.648	(0.566)	101	2240439			97.29-	157.29	127.29

20 1,1-Dichloroethene						CAS #: 75-35-4			
4.703	4.703	(0.573)	61	2370798	50.0000	47.393	80.00-	120.00	100.00
4.703	4.703	(0.573)	96	1212158			21.13-	81.13	51.13
4.703	4.703	(0.573)	98	767724			2.38-	62.38	32.38

22 Acetone						CAS #: 67-64-1			
4.841	4.841	(0.589)	58	827315	50.0000	44.337	80.00-	120.00	100.00
4.841	4.841	(0.589)	43	3023948			327.94-	387.94	365.51

26 2-Propanol						CAS #: 67-63-0			
5.062	5.062	(0.616)	45	3382263	50.0000	41.592	80.00-	120.00	100.00
5.035	5.035	(0.613)	43	699691			0.00-	49.24	20.69
5.062	5.062	(0.616)	59	110740			0.00-	33.25	3.27

25 Carbon Disulfide						CAS #: 75-15-0			
5.035	5.035	(0.613)	76	3395568	50.0000	49.304	80.00-	120.00	100.00

28 3-Chloropropene						CAS #: 107-05-1			
5.311	5.311	(0.647)	76	548674	50.0000	47.154	80.00-	120.00	100.00
5.311	5.311	(0.647)	41	2732476			480.64-	540.64	498.01

29 Methylene Chloride						CAS #: 75-09-2			
5.588	5.588	(0.680)	49	2097556	50.0000	44.709	80.00-	120.00	100.00
5.588	5.588	(0.680)	84	942482			14.93-	74.93	44.93
5.588	5.588	(0.680)	51	618007			0.00-	59.58	29.46

31 MTBE						CAS #: 1634-04-4			
5.920	5.920	(0.721)	73	1116261	50.0000	30.497	80.00-	120.00	100.00
5.920	5.920	(0.721)	57	354492			1.76-	61.76	31.76
5.892	5.892	(0.717)	41	425837			10.34-	70.34	38.15

32 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.975	5.975	(0.727)	96	1246474	50.0000	49.972	80.00-	120.00	100.00
5.947	5.947	(0.724)	61	2157780			143.11-	203.11	173.11
5.975	5.975	(0.727)	98	766595			32.40-	92.40	61.50

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Hexane						CAS #: 110-54-3			
6.307	6.307	(0.768)	57	2576022	50.0000	41.075	80.00- 120.00	100.00	
6.307	6.307	(0.768)	43	1955906			46.14- 106.14	75.93	
6.307	6.307	(0.768)	86	341552			0.00- 41.50	13.26	

43 1,1-Dichloroethane						CAS #: 75-34-3			
6.749	6.749	(0.822)	63	2346099	50.0000	47.026	80.00- 120.00	100.00	
6.749	6.749	(0.822)	65	670953			0.00- 58.60	28.60	

53 2-Butanone						CAS #: 78-93-3			
7.800	7.800	(0.950)	72	458590	50.0000	47.582	80.00- 120.00	100.00	
7.800	7.800	(0.950)	43	3396749			710.69- 770.69	740.69	
7.800	7.800	(0.950)	57	232743			23.20- 83.20	50.75	

52 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.772	7.772	(0.946)	61	1682415	50.0000	43.420	80.00- 120.00	100.00	
7.772	7.772	(0.946)	96	1006022			29.80- 89.80	59.80	
7.772	7.772	(0.946)	98	615900			6.61- 66.61	36.61	

56 Tetrahydrofuran						CAS #: 109-99-9			
8.187	8.187	(0.997)	42	2009296	50.0000	40.200	80.00- 120.00	100.00	
8.187	8.187	(0.997)	71	399002			0.00- 49.86	19.86	
8.187	8.187	(0.997)	72	425179			0.00- 49.73	21.16	

58 Chloroform						CAS #: 67-66-3			
8.325	8.325	(1.013)	83	1909980	50.0000	53.442	80.00- 120.00	100.00	
8.325	8.325	(1.013)	85	1244724			35.17- 95.17	65.17	

62 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.574	8.574	(1.044)	97	2151146	50.0000	55.262	80.00- 120.00	100.00	
8.574	8.574	(1.044)	99	1352100			32.85- 92.85	62.85	

61 Cyclohexane						CAS #: 110-82-7			
8.574	8.574	(1.044)	84	1233814	50.0000	46.673	80.00- 120.00	100.00	
8.574	8.574	(1.044)	56	2178513			146.57- 206.57	176.57	
8.546	8.546	(1.040)	41	1479448			89.91- 149.91	119.91	

63 Vinyl Acetate						CAS #: 108-05-4			
6.804	6.804	(0.828)	86	279156	50.0000	48.039	80.00- 120.00	100.00	
6.804	6.804	(0.828)	43	4577512			1767.50-1827.50	1639.77	
6.804	6.804	(0.828)	42	390240			104.58- 164.58	139.79	

65 Carbon Tetrachloride						CAS #: 56-23-5			
8.823	8.823	(1.074)	119	1920560	50.0000	56.632	80.00- 120.00	100.00	
8.823	8.823	(1.074)	117	2029605			75.68- 135.68	105.68	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

68	2,2,4-Trimethylpentane						CAS #: 540-84-1		
9.237	9.237	(1.125)	57	5515380	50.0000	37.006	80.00- 120.00	100.00	
9.237	9.237	(1.125)	56	1822316			2.91- 62.91	33.04	
9.237	9.237	(1.125)	41	1991743			0.00- 59.75	36.11	

69	Benzene						CAS #: 71-43-2		
9.237	9.237	(0.918)	78	2510088	50.0000	50.539	80.00- 120.00	100.00	
9.237	9.237	(0.918)	77	575887			0.00- 53.04	22.94	

72	1,2-Dichloroethane						CAS #: 107-06-2		
9.431	9.431	(0.937)	62	1904366	50.0000	56.368	80.00- 120.00	100.00	
9.431	9.431	(0.937)	64	554312			0.57- 60.57	29.11	

75	Heptane						CAS #: 142-82-5		
9.625	9.625	(0.956)	100	313061	50.0000	46.382	80.00- 120.00	100.00	
9.625	9.625	(0.956)	43	2897012			1063.83-1123.83	925.38	
9.625	9.625	(0.956)	71	895769			257.42- 317.42	286.13	

80	Trichloroethene						CAS #: 79-01-6		
10.482	10.482	(1.041)	95	1085096	50.0000	52.118	80.00- 120.00	100.00	
10.482	10.482	(1.041)	130	991665			61.39- 121.39	91.39	
10.482	10.482	(1.041)	97	710800			35.51- 95.51	65.51	

82	1,2-Dichloropropane						CAS #: 78-87-5		
11.007	11.007	(1.093)	63	985061	50.0000	45.532	80.00- 120.00	100.00	
11.007	11.007	(1.093)	62	723260			43.42- 103.42	73.42	
10.979	10.979	(1.091)	41	1101672			81.84- 141.84	111.84	

84	1,4-Dioxane						CAS #: 123-91-1		
11.228	11.228	(1.115)	88	547724	50.0000	49.197	80.00- 120.00	100.00	
11.228	11.228	(1.115)	58	557091			71.71- 131.71	101.71	
11.201	11.201	(1.113)	57	189468			11.42- 71.42	34.59	

85	Bromodichloromethane						CAS #: 75-27-4		
11.560	11.560	(1.148)	83	1823562	50.0000	59.290	80.00- 120.00	100.00	
11.560	11.560	(1.148)	85	1174669			34.42- 94.42	64.42	

90	cis-1,3-Dichloropropene						CAS #: 10061-01-5		
12.445	12.445	(1.236)	75	1215763	50.0000	54.787	80.00- 120.00	100.00	
12.445	12.445	(1.236)	77	363790			0.00- 59.92	29.92	
12.445	12.445	(1.236)	39	1352722			81.27- 141.27	111.27	

91	4-Methyl-2-pentanone						CAS #: 108-10-1		
12.749	12.749	(1.266)	58	979777	50.0000	46.035	80.00- 120.00	100.00	
12.721	12.721	(1.264)	43	3179821			296.95- 356.95	324.55	
12.749	12.749	(1.266)	85	304685			0.00- 57.61	31.10	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
99 Toluene						CAS #: 108-88-3			
12.942	12.942	(1.286)	91	2471192	50.0000	51.810	80.00- 120.00	100.00	
12.942	12.942	(1.286)	92	1477831			29.80- 89.80	59.80	

100 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.468	13.468	(0.892)	75	1403304	50.0000	58.382	80.00- 120.00	100.00	
13.468	13.468	(0.892)	77	428997			0.57- 60.57	30.57	
13.468	13.468	(0.892)	39	1301497			62.75- 122.75	92.75	

101 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.744	13.744	(0.910)	97	837912	50.0000	51.635	80.00- 120.00	100.00	
13.744	13.744	(0.910)	99	515979			31.58- 91.58	61.58	
13.744	13.744	(0.910)	83	685695			51.83- 111.83	81.83	

102 Tetrachloroethene						CAS #: 127-18-4			
13.800	13.800	(0.914)	166	1060442	50.0000	52.252	80.00- 120.00	100.00	
13.800	13.800	(0.914)	129	894398			54.34- 114.34	84.34	
13.800	13.800	(0.914)	131	869672			52.01- 112.01	82.01	

103 2-Hexanone						CAS #: 591-78-6			
14.131	14.131	(0.936)	58	1293822	50.0000	42.642	80.00- 120.00	100.00	
14.131	14.131	(0.936)	43	3134391			212.26- 272.26	242.26	
14.131	14.131	(0.936)	100	186956			0.00- 42.78	14.45	

105 Dibromochloromethane						CAS #: 124-48-1			
14.297	14.297	(0.947)	129	1530278	50.0000	57.927	80.00- 120.00	100.00	
14.297	14.297	(0.947)	127	1193663			48.77- 108.77	78.00	

106 1,2-Dibromoethane						CAS #: 106-93-4			
14.463	14.463	(0.958)	107	1318102	50.0000	53.145	80.00- 120.00	100.00	
14.463	14.463	(0.958)	109	1226571			63.06- 123.06	93.06	

109 Chlorobenzene						CAS #: 108-90-7			
15.154	15.154	(1.004)	112	1957409	50.0000	49.965	80.00- 120.00	100.00	
15.154	15.154	(1.004)	114	622944			1.82- 61.82	31.82	
15.154	15.154	(1.004)	77	1302256			36.53- 96.53	66.53	

111 Ethyl Benzene						CAS #: 100-41-4			
15.265	15.265	(1.011)	106	1039597	50.0000	53.998	80.00- 120.00	100.00	
15.265	15.265	(1.011)	91	3709270			322.22- 382.22	356.80	

113 m,p-Xylene						CAS #: 108-38-3			
15.431	15.431	(1.022)	106	1300636	50.0000	51.890	80.00- 120.00	100.00	
15.431	15.431	(1.022)	91	3070203			202.98- 262.98	236.05	

114 o-Xylene						CAS #: 95-47-6			
15.956	15.956	(1.057)	106	1211418	50.0000	51.105	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	3054018			222.10- 282.10	252.10	

115 Styrene CAS #: 100-42-5									
16.012	16.012	(1.060)	104	1961571	50.0000	56.616	80.00- 120.00	100.00	
16.012	16.012	(1.060)	78	1277710			35.14- 95.14	65.14	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	1363193	50.0000	60.212	80.00- 120.00	100.00	
16.260	16.260	(1.077)	171	700977			21.42- 81.42	51.42	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	1809600	50.0000	48.876	80.00- 120.00	100.00	
16.896	16.896	(1.119)	85	1178773			35.14- 95.14	65.14	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	4490375	50.0000	55.171	80.00- 120.00	100.00	
17.062	17.062	(1.130)	120	1260944			0.00- 58.08	28.08	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	3783886	50.0000	55.449	80.00- 120.00	100.00	
17.145	17.145	(1.135)	120	1710510			16.58- 76.58	45.21	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	4011062	50.0000	54.744	80.00- 120.00	100.00	
17.532	17.532	(1.161)	120	1702270			12.44- 72.44	42.44	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	2446274	50.0000	50.936	80.00- 120.00	100.00	
17.836	17.836	(1.181)	148	1501281			33.12- 93.12	61.37	
17.836	17.836	(1.181)	111	1149467			15.78- 75.78	46.99	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	1952217	50.0000	51.403	80.00- 120.00	100.00	
17.919	17.919	(1.187)	148	1226703			34.33- 94.33	62.84	
17.919	17.919	(1.187)	111	959459			18.49- 78.49	49.15	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.058	18.058	(1.196)	91	3737622	50.0000	58.987	80.00- 120.00	100.00	
18.058	18.058	(1.196)	126	601515			0.00- 47.06	16.09	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	2392533	50.0000	48.024	80.00- 120.00	100.00	
18.279	18.279	(1.211)	148	1484327			32.04- 92.04	62.04	
18.279	18.279	(1.211)	111	1160535			18.51- 78.51	48.51	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

154	1,2,4-Trichlorobenzene					CAS #:	120-82-1		
19.578	19.578	(1.297)	180	1756083	50.0000	50.124	80.00-	120.00	100.00
19.578	19.578	(1.297)	182	1666775			64.91-	124.91	94.91

155	Hexachlorobutadiene					CAS #:	87-68-3		
19.661	19.661	(1.302)	225	1591055	50.0000	54.803	80.00-	120.00	100.00
19.661	19.661	(1.302)	223	987076			32.04-	92.04	62.04

124	Propylbenzene					CAS #:	103-65-1		
16.924	16.924	(1.121)	91	5202622	50.0000	55.249	80.00-	120.00	100.00
16.924	16.924	(1.121)	120	1050594			0.00-	50.53	20.19
16.924	16.924	(1.121)	105	191103			0.00-	33.52	3.67

119	Cumene					CAS #:	98-82-8		
16.426	16.426	(1.088)	105	3973703	50.0000	54.868	80.00-	120.00	100.00
16.426	16.426	(1.088)	120	995204			0.00-	55.50	25.04
16.426	16.426	(1.088)	51	799964			0.00-	50.84	20.13

156	Naphthalene					CAS #:	91-20-3		
19.744	19.744	(1.308)	128	4888698	50.0000	47.007	80.00-	120.00	100.00
19.744	19.744	(1.308)	127	617056			0.00-	42.90	12.62

30	Isopentane					CAS #:	78-78-4		
3.542	3.542	(0.431)	43	3081698	50.0000	46.517	80.00-	120.00	100.00
3.542	3.542	(0.431)	57	1792271			30.33-	90.33	58.16
3.542	3.542	(0.431)	72	163071			0.00-	34.69	5.29

21	Butane					CAS #:	106-97-8		
2.767	2.767	(0.337)	58	497995	50.0000	46.079	80.00-	120.00	100.00
2.767	2.767	(0.337)	43	4006630			773.30-	833.30	804.55

96	Methyl Cyclohexane					CAS #:	108-87-2		
10.703	10.703	(1.063)	83	1373910	50.0000	46.665	80.00-	120.00	100.00
10.703	10.703	(1.063)	98	729732			20.58-	80.58	53.11
10.703	10.703	(1.063)	55	1904118			125.23-	185.23	138.59

Report Date: 07-Jun-2007 21:01

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 07-JUN-2007

Lab File ID: 5060709.d

Calibration Time: 13:20

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd5.i/5-07jun.b/t14q529a.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	292964	175778	410150	292964	0.00
79 1,4-Difluorobenze	1106143	663686	1548600	1106143	0.00
108 Chlorobenzene-d5	855448	513269	1197627	855448	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.21	7.88	8.54	8.21	0.00
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-07jun.b/5060709.d
 Date: 07-JUN-2007 13:20
 Client ID: CCV-1
 Sample Info: 50mL #1487-286

Column phase: RTX-624

Instrument: msd5.1
 Operator: JG
 Column diameter: 0.53

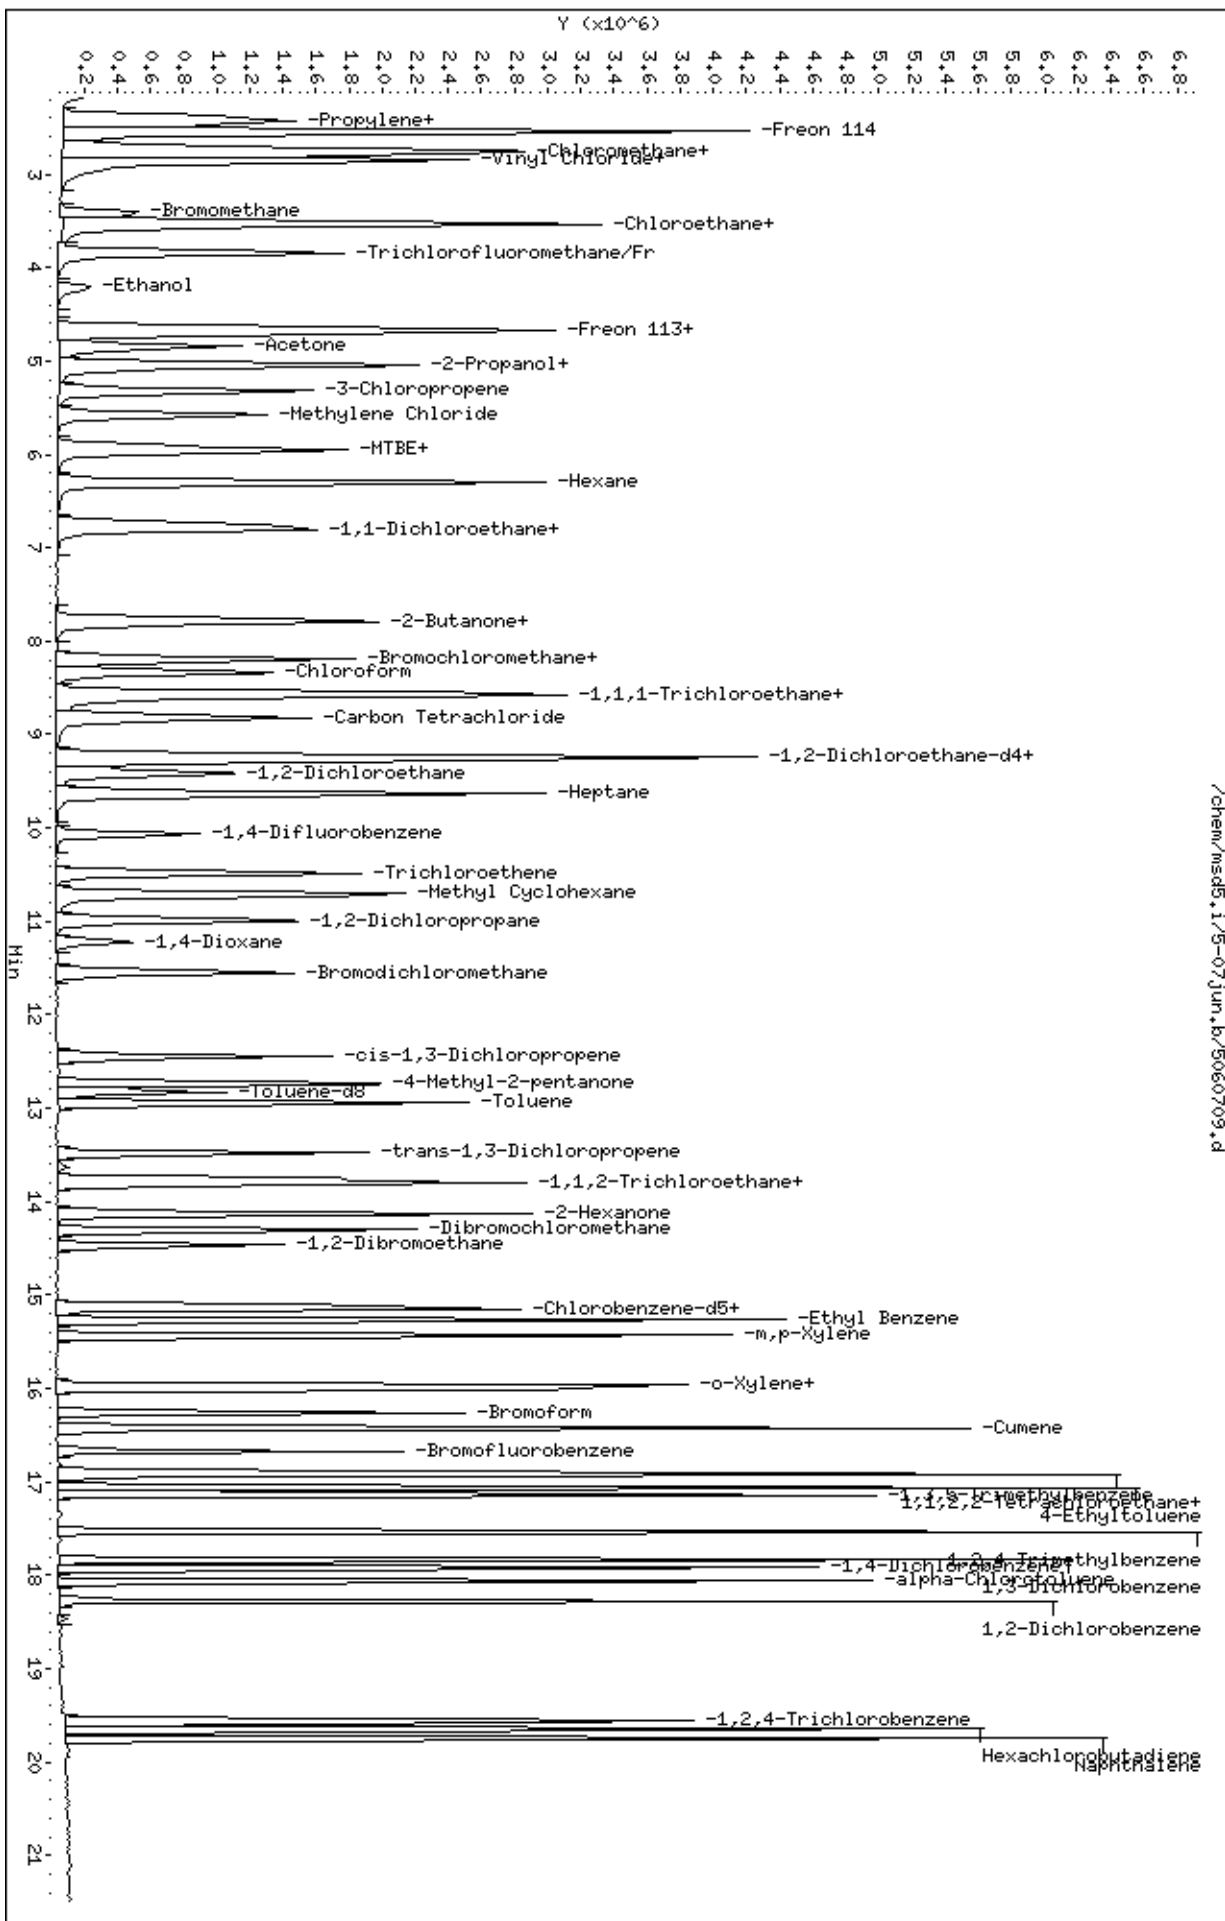



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0706057-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060711	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/7/07 02:35 PM

Compound	%Recovery
Freon 12	119
Freon 114	114
Vinyl Chloride	108
Bromomethane	115
Chloroethane	99
Freon 11	125
1,1-Dichloroethene	110
Freon 113	128
Methylene Chloride	104
1,1-Dichloroethane	103
cis-1,2-Dichloroethene	97
Chloroform	119
1,1,1-Trichloroethane	121
Carbon Tetrachloride	128
Benzene	105
1,2-Dichloroethane	123
Trichloroethene	112
1,2-Dichloropropane	96
cis-1,3-Dichloropropene	114
Toluene	117
trans-1,3-Dichloropropene	127
1,1,2-Trichloroethane	112
Tetrachloroethene	113
1,2-Dibromoethane (EDB)	110
Chlorobenzene	108
Ethyl Benzene	115
m,p-Xylene	110
o-Xylene	108
Styrene	116
1,1,2,2-Tetrachloroethane	103
1,3,5-Trimethylbenzene	115
1,2,4-Trimethylbenzene	119
1,3-Dichlorobenzene	107
1,4-Dichlorobenzene	110
alpha-Chlorotoluene	136 Q
1,2-Dichlorobenzene	103
1,3-Butadiene	102
Hexane	86
Cyclohexane	102



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0706057-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5060711	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/7/07 02:35 PM

Compound	%Recovery
Heptane	98
Bromodichloromethane	127
Dibromochloromethane	128
Cumene	122
Propylbenzene	123
Chloromethane	102
1,2,4-Trichlorobenzene	98
Hexachlorobutadiene	109
Acetone	96
Carbon Disulfide	103
2-Propanol	94
trans-1,2-Dichloroethene	101
2-Butanone (Methyl Ethyl Ketone)	104
Tetrahydrofuran	84
1,4-Dioxane	102
4-Methyl-2-pentanone	97
2-Hexanone	91
Bromoform	130
4-Ethyltoluene	121
Ethanol	108
Methyl tert-butyl ether	71
3-Chloropropene	101
2,2,4-Trimethylpentane	84
Naphthalene	94

Q = Exceeds Quality Control limits.

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	100	70-130
1,2-Dichloroethane-d4	104	70-130
4-Bromofluorobenzene	105	70-130

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-07jun
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: JG
 Data Type: MS DATA SampleType: LCS
 SpikeList File: 2926Spectra.spk Quant Type: ISTD
 Sublist File: AT04+ENSR.sub
 Method File: /var/chem/msd5.i/5-07jun.b/t14q529a.m
 Misc Info: 200ppbv-50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
2 Dichlorodifluorome	50.000	59.380	118.76	70-130
3 Freon 114	50.000	56.972	113.94	70-130
4 Chloromethane	50.000	51.195	102.39	70-130
5 Vinyl Chloride	50.000	53.814	107.63	70-130
6 1,3-Butadiene	50.000	51.029	102.06	60-140
7 Bromomethane	50.000	57.612	115.22	70-130
8 Chloroethane	50.000	49.400	98.80	70-130
9 Trichlorofluoromet	50.000	62.686	125.37	70-130
13 Ethanol	50.000	54.089	108.18	60-140
19 Freon 113	50.000	63.981	127.96	70-130
20 1,1-Dichloroethene	50.000	54.756	109.51	70-130
25 Carbon Disulfide	50.000	51.370	102.74	60-140
22 Acetone	50.000	47.989	95.98	60-140
26 2-Propanol	50.000	47.097	94.19	60-140
28 3-Chloropropene	50.000	50.708	101.42	60-140
29 Methylene Chloride	50.000	52.149	104.30	70-130
31 MTBE	50.000	35.413	70.83	60-140
32 trans-1,2-Dichloro	50.000	50.496	100.99	60-140
38 Hexane	50.000	42.985	85.97	60-140
43 1,1-Dichloroethane	50.000	51.423	102.85	70-130
52 cis-1,2-Dichloroet	50.000	48.746	97.49	70-130
53 2-Butanone	50.000	51.803	103.61	60-140
56 Tetrahydrofuran	50.000	42.293	84.59	60-140
58 Chloroform	50.000	59.472	118.94	70-130
61 Cyclohexane	50.000	51.083	102.17	60-140
62 1,1,1-Trichloroeth	50.000	60.593	121.19	70-130
63 Vinyl Acetate	50.000	53.698	107.40	60-140
65 Carbon Tetrachlori	50.000	63.987	127.97	70-130
68 2,2,4-Trimethylpen	50.000	42.198	84.40	60-140
69 Benzene	50.000	52.382	104.76	70-130
72 1,2-Dichloroethane	50.000	61.528	123.06	70-130
75 Heptane	50.000	48.889	97.78	60-140
80 Trichloroethene	50.000	56.235	112.47	70-130

Report Date: 07-Jun-2007 15:25

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
82 1,2-Dichloropropan	50.000	47.901	95.80	70-130
84 1,4-Dioxane	50.000	51.087	102.17	60-140
85 Bromodichlorometha	50.000	63.635	127.27	60-140
90 cis-1,3-Dichloropr	50.000	57.224	114.45	70-130
91 4-Methyl-2-pentano	50.000	48.556	97.11	60-140
99 Toluene	50.000	58.342	116.68	70-130
100 trans-1,3-Dichloro	50.000	63.360	126.72	70-130
101 1,1,2-Trichloroeth	50.000	55.954	111.91	70-130
102 Tetrachloroethene	50.000	56.592	113.18	70-130
103 2-Hexanone	50.000	45.437	90.87	60-140
105 Dibromochlorometha	50.000	64.088	128.18	60-140
106 1,2-Dibromoethane	50.000	55.099	110.20	70-130
109 Chlorobenzene	50.000	53.994	107.99	70-130
111 Ethyl Benzene	50.000	57.677	115.35	70-130
113 m,p-Xylene	50.000	55.210	110.42	70-130
114 o-Xylene	50.000	53.919	107.84	70-130
115 Styrene	50.000	58.082	116.16	70-130
118 Bromoform	50.000	64.915	129.83	60-140
119 Cumene	50.000	60.758	121.52	60-140
123 1,1,2,2-Tetrachlor	50.000	51.488	102.98	70-130
124 Propylbenzene	50.000	61.344	122.69	60-140
126 4-Ethyltoluene	50.000	60.378	120.76	60-140
128 1,3,5-Trimethylben	50.000	57.582	115.16	70-130
131 1,2,4-Trimethylben	50.000	59.738	119.48	70-130
138 1,3-Dichlorobenzen	50.000	53.490	106.98	70-130
141 1,4-Dichlorobenzen	50.000	55.148	110.30	70-130
143 alpha-Chlorotoluen	50.000	67.854	135.71*	70-130
146 1,2-Dichlorobenzen	50.000	51.548	103.10	70-130
154 1,2,4-Trichloroben	50.000	49.235	98.47	70-130
155 Hexachlorobutadien	50.000	54.686	109.37	70-130
1 Propylene	50.000	52.999	106.00	70-130
156 Naphthalene	50.000	46.758	93.52	60-140
21 Butane	50.000	50.498	101.00	70-130
30 Isopentane	50.000	48.670	97.34	70-130
96 Methyl Cyclohexane	50.000	51.560	103.12	70-130

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 71 1,2-Dichloroethane	25.000	26.002	104.01	70-130
\$ 97 Toluene-d8	25.000	25.111	100.45	70-130
\$ 122 Bromofluorobenzene	25.000	26.362	105.45	70-130

Report Date: 07-Jun-2007 15:25

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-07jun.b/5060711.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 07-JUN-2007 14:35
 Operator : JG Inst ID: msd5.i
 Smp Info : 50mL #1487-275
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /var/chem/msd5.i/5-07jun.b/t14q529a.m
 Meth Date : 07-Jun-2007 14:03 jgray Quant Type: ISTD
 Cal Date : 29-MAY-2007 20:44 Cal File: 5052920.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				(PPBV)	(PPBV)			
==	=====	=====	====	=====	=====	=====	=====	=====

* 57	Bromochloromethane					CAS #: 74-97-5		
8.187	8.214	(1.000)	130	238932	25.0000	80.00- 120.00	100.00	
8.187	8.214	(1.000)	128	188349		48.55- 108.55	78.83	
8.187	8.187	(1.000)	49	618778		229.31- 289.31	258.98	

* 79	1,4-Difluorobenzene					CAS #: 540-36-3		
10.067	10.067	(1.000)	114	921544	25.0000	80.00- 120.00	100.00	
10.067	10.067	(1.000)	88	165911		0.00- 49.97	18.00	

* 108	Chlorobenzene-d5					CAS #: 3114-55-4		
15.099	15.099	(1.000)	117	712923	25.0000	80.00- 120.00	100.00	
15.099	15.099	(1.000)	82	484207		33.54- 93.54	67.92	

\$ 71	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.265	9.265	(1.132)	65	498030	26.0019	26.002 80.00- 120.00	100.00	
9.265	9.265	(1.132)	67	250885		25.98- 85.98	50.38	

\$ 97	Toluene-d8					CAS #: 2037-26-5		
12.832	12.832	(1.275)	98	842315	25.1114	25.111 80.00- 120.00	100.00	
12.832	12.832	(1.275)	70	102560		0.00- 41.05	12.18	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 97 Toluene-d8 (continued)

12.832	12.832	(1.275)	100	548931			36.04- 96.04	65.17
--------	--------	---------	-----	--------	--	--	--------------	-------

\$ 122 Bromofluorobenzene

CAS #: 460-00-4

16.675	16.675	(1.104)	174	472201	26.3620	26.362	80.00- 120.00	100.00
16.675	16.675	(1.104)	95	779895			136.90- 196.90	165.16
16.675	16.675	(1.104)	176	429397			64.74- 124.74	90.94

1 Propylene

CAS #: 115-07-1

2.325	2.380	(0.284)	41	1688953	52.9995	52.999	80.00- 120.00	100.00
2.325	2.380	(0.284)	42	1106948			36.96- 96.96	65.54
2.325	2.380	(0.284)	39	1173512			37.69- 97.69	69.48

2 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.408	2.436	(0.294)	85	2517164	59.3805	59.380	80.00- 120.00	100.00
2.408	2.436	(0.294)	87	822784			1.62- 61.62	32.69

3 Freon 114

CAS #: 76-14-2

2.519	2.546	(0.308)	135	2309805	56.9720	56.972	80.00- 120.00	100.00
2.519	2.546	(0.308)	137	729460			1.19- 61.19	31.58

4 Chloromethane

CAS #: 74-87-3

2.657	2.712	(0.325)	50	1959405	51.1952	51.195	80.00- 120.00	100.00
2.657	2.712	(0.325)	52	587629			0.00- 59.51	29.99

5 Vinyl Chloride

CAS #: 75-01-4

2.850	2.878	(0.348)	62	1674809	53.8143	53.814	80.00- 120.00	100.00
2.850	2.878	(0.348)	64	486276			0.00- 59.15	29.03

6 1,3-Butadiene

CAS #: 106-99-0

2.823	2.850	(0.345)	54	1576385	51.0288	51.029	80.00- 120.00	100.00
2.823	2.850	(0.345)	39	1830395			92.11- 152.11	116.11

7 Bromomethane

CAS #: 74-83-9

3.376	3.403	(0.412)	94	1065162	57.6117	57.612	80.00- 120.00	100.00
3.376	3.403	(0.412)	96	1015596			60.71- 120.71	95.35

8 Chloroethane

CAS #: 75-00-3

3.486	3.542	(0.426)	64	815269	49.3998	49.400	80.00- 120.00	100.00
3.486	3.542	(0.426)	49	281064			1.83- 61.83	34.48
3.486	3.542	(0.426)	66	240915			0.00- 57.39	29.55

9 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.818	3.846	(0.466)	101	2678711	62.6860	62.686	80.00- 120.00	100.00
3.818	3.846	(0.466)	103	1712745			34.63- 94.63	63.94

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

13 Ethanol CAS #: 64-17-5
 4.178 4.205 (0.510) 45 709096 54.0890 54.089 80.00- 120.00 100.00
 4.178 4.205 (0.510) 43 141184 0.00- 49.45 19.91
 4.178 4.205 (0.510) 46 308179 11.95- 71.95 43.46

19 Freon 113 CAS #: 76-13-1
 4.648 4.675 (0.568) 151 1673997 63.9808 63.981 80.00- 120.00 100.00
 4.648 4.675 (0.568) 153 1049151 30.80- 90.80 62.67
 4.620 4.648 (0.564) 101 2142953 97.29- 157.29 128.01

20 1,1-Dichloroethene CAS #: 75-35-4
 4.675 4.703 (0.571) 61 2233903 54.7556 54.756 80.00- 120.00 100.00
 4.675 4.703 (0.571) 96 1182503 21.13- 81.13 52.93
 4.675 4.703 (0.571) 98 751329 2.38- 62.38 33.63

22 Acetone CAS #: 67-64-1
 4.814 4.841 (0.588) 58 730305 47.9891 47.989 80.00- 120.00 100.00
 4.814 4.841 (0.588) 43 2762335 327.94- 387.94 378.24

26 2-Propanol CAS #: 67-63-0
 5.035 5.062 (0.615) 45 3123616 47.0974 47.097 80.00- 120.00 100.00
 5.035 5.035 (0.615) 43 645448 0.00- 49.24 20.66
 5.035 5.062 (0.615) 59 94743 0.00- 33.25 3.03

25 Carbon Disulfide CAS #: 75-15-0
 5.007 5.035 (0.612) 76 2885394 51.3701 51.370 80.00- 120.00 100.00

28 3-Chloropropene CAS #: 107-05-1
 5.311 5.311 (0.649) 76 481205 50.7076 50.708 80.00- 120.00 100.00
 5.311 5.311 (0.649) 41 2399196 480.64- 540.64 498.58

29 Methylene Chloride CAS #: 75-09-2
 5.560 5.588 (0.679) 49 1995366 52.1493 52.149 80.00- 120.00 100.00
 5.560 5.588 (0.679) 84 886342 14.93- 74.93 44.42
 5.560 5.588 (0.679) 51 580728 0.00- 59.58 29.10

31 MTBE CAS #: 1634-04-4
 5.892 5.920 (0.720) 73 1057138 35.4133 35.413 80.00- 120.00 100.00
 5.892 5.920 (0.720) 57 360069 1.76- 61.76 34.06
 5.892 5.892 (0.720) 41 409622 10.34- 70.34 38.75

32 trans-1,2-Dichloroethene CAS #: 156-60-5
 5.947 5.975 (0.726) 96 1027243 50.4955 50.496 80.00- 120.00 100.00
 5.947 5.947 (0.726) 61 1898045 143.11- 203.11 184.77
 5.947 5.975 (0.726) 98 679367 32.40- 92.40 66.13

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

38 Hexane CAS #: 110-54-3
 6.279 6.307 (0.767) 57 2198596 42.9847 42.985 80.00- 120.00 100.00
 6.279 6.307 (0.767) 43 1747190 46.14- 106.14 79.47
 6.279 6.307 (0.767) 86 293543 0.00- 41.50 13.35

43 1,1-Dichloroethane CAS #: 75-34-3
 6.721 6.749 (0.821) 63 2092308 51.4229 51.423 80.00- 120.00 100.00
 6.721 6.749 (0.821) 65 605725 0.00- 58.60 28.95

53 2-Butanone CAS #: 78-93-3
 7.800 7.800 (0.953) 72 407188 51.8027 51.803 80.00- 120.00 100.00
 7.800 7.800 (0.953) 43 3077172 710.69- 770.69 755.71
 7.800 7.800 (0.953) 57 200699 23.20- 83.20 49.29

52 cis-1,2-Dichloroethene CAS #: 156-59-2
 7.744 7.772 (0.946) 61 1540431 48.7457 48.746 80.00- 120.00 100.00
 7.772 7.772 (0.949) 96 892925 29.80- 89.80 57.97
 7.772 7.772 (0.949) 98 567923 6.61- 66.61 36.87

56 Tetrahydrofuran CAS #: 109-99-9
 8.187 8.187 (1.000) 42 1724022 42.2928 42.293 80.00- 120.00 100.00
 8.187 8.187 (1.000) 71 357643 0.00- 49.86 20.74
 8.187 8.187 (1.000) 72 372542 0.00- 49.73 21.61

58 Chloroform CAS #: 67-66-3
 8.325 8.325 (1.017) 83 1733450 59.4716 59.472 80.00- 120.00 100.00
 8.325 8.325 (1.017) 85 1111407 35.17- 95.17 64.12

62 1,1,1-Trichloroethane CAS #: 71-55-6
 8.574 8.574 (1.047) 97 1923634 60.5931 60.593 80.00- 120.00 100.00
 8.574 8.574 (1.047) 99 1212060 32.85- 92.85 63.01

61 Cyclohexane CAS #: 110-82-7
 8.546 8.574 (1.044) 84 1101352 51.0832 51.083 80.00- 120.00 100.00
 8.546 8.574 (1.044) 56 2037413 146.57- 206.57 184.99
 8.546 8.546 (1.044) 41 1352454 89.91- 149.91 122.80

63 Vinyl Acetate CAS #: 108-05-4
 6.777 6.804 (0.828) 86 254488 53.6976 53.698 80.00- 120.00 100.00
 6.777 6.804 (0.828) 43 4170621 1767.50-1827.50 1638.83
 6.777 6.804 (0.828) 42 348501 104.58- 164.58 136.94

65 Carbon Tetrachloride CAS #: 56-23-5
 8.795 8.823 (1.074) 119 1769791 63.9871 63.987 80.00- 120.00 100.00
 8.795 8.823 (1.074) 117 1839536 75.68- 135.68 103.94

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPEV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

68	2,2,4-Trimethylpentane						CAS #: 540-84-1		
9.237	9.237	(1.128)	57	5129183	42.1980	42.198	80.00-	120.00	100.00
9.237	9.237	(1.128)	56	1680523			2.91-	62.91	32.76
9.237	9.237	(1.128)	41	1849147			0.00-	59.75	36.05

69	Benzene						CAS #: 71-43-2		
9.237	9.237	(0.918)	78	2167476	52.3824	52.382	80.00-	120.00	100.00
9.237	9.237	(0.918)	77	511580			0.00-	53.04	23.60

72	1,2-Dichloroethane						CAS #: 107-06-2		
9.403	9.431	(0.934)	62	1731806	61.5281	61.528	80.00-	120.00	100.00
9.403	9.431	(0.934)	64	507625			0.57-	60.57	29.31

75	Heptane						CAS #: 142-82-5		
9.625	9.625	(0.956)	100	274914	48.8889	48.889	80.00-	120.00	100.00
9.625	9.625	(0.956)	43	2525504			1063.83-	1123.83	918.65
9.625	9.625	(0.956)	71	783507			257.42-	317.42	285.00

80	Trichloroethene						CAS #: 79-01-6		
10.482	10.482	(1.041)	95	975420	56.2352	56.235	80.00-	120.00	100.00
10.482	10.482	(1.041)	130	872592			61.39-	121.39	89.46
10.482	10.482	(1.041)	97	619239			35.51-	95.51	63.48

82	1,2-Dichloropropane						CAS #: 78-87-5		
10.979	11.007	(1.091)	63	863365	47.9008	47.901	80.00-	120.00	100.00
10.979	11.007	(1.091)	62	625560			43.42-	103.42	72.46
10.979	10.979	(1.091)	41	940599			81.84-	141.84	108.95

84	1,4-Dioxane						CAS #: 123-91-1		
11.201	11.228	(1.113)	88	473846	51.0870	51.087	80.00-	120.00	100.00
11.201	11.228	(1.113)	58	495880			71.71-	131.71	104.65
11.201	11.201	(1.113)	57	163890			11.42-	71.42	34.59

85	Bromodichloromethane						CAS #: 75-27-4		
11.532	11.560	(1.146)	83	1630569	63.6349	63.635	80.00-	120.00	100.00
11.532	11.560	(1.146)	85	1059377			34.42-	94.42	64.97

90	cis-1,3-Dichloropropene						CAS #: 10061-01-5		
12.445	12.445	(1.236)	75	1057926	57.2239	57.224	80.00-	120.00	100.00
12.445	12.445	(1.236)	77	342775			0.00-	59.92	32.40
12.445	12.445	(1.236)	39	1164495			81.27-	141.27	110.07

91	4-Methyl-2-pentanone						CAS #: 108-10-1		
12.721	12.749	(1.264)	58	860976	48.5565	48.556	80.00-	120.00	100.00
12.721	12.721	(1.264)	43	2889334			296.95-	356.95	335.59
12.721	12.749	(1.264)	85	284168			0.00-	57.61	33.01

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
99 Toluene						CAS #:	108-88-3			
12.942	12.942	(1.286)	91	2318346	58.3421	58.342	80.00-	120.00	100.00	
12.942	12.942	(1.286)	92	1360929			29.80-	89.80	58.70	

100 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.468	13.468	(0.892)	75	1269222	63.3598	63.360	80.00-	120.00	100.00	
13.468	13.468	(0.892)	77	393539			0.57-	60.57	31.01	
13.468	13.468	(0.892)	39	1175566			62.75-	122.75	92.62	

101 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.744	13.744	(0.910)	97	756708	55.9536	55.954	80.00-	120.00	100.00	
13.744	13.744	(0.910)	99	452857			31.58-	91.58	59.85	
13.744	13.744	(0.910)	83	603044			51.83-	111.83	79.69	

102 Tetrachloroethene						CAS #:	127-18-4			
13.800	13.800	(0.914)	166	957179	56.5923	56.592	80.00-	120.00	100.00	
13.800	13.800	(0.914)	129	829916			54.34-	114.34	86.70	
13.800	13.800	(0.914)	131	789833			52.01-	112.01	82.52	

103 2-Hexanone						CAS #:	591-78-6			
14.131	14.131	(0.936)	58	1148943	45.4368	45.437	80.00-	120.00	100.00	
14.131	14.131	(0.936)	43	2840422			212.26-	272.26	247.22	
14.131	14.131	(0.936)	100	178727			0.00-	42.78	15.56	

105 Dibromochloromethane						CAS #:	124-48-1			
14.297	14.297	(0.947)	129	1410959	64.0880	64.088	80.00-	120.00	100.00	
14.297	14.297	(0.947)	127	1079834			48.77-	108.77	76.53	

106 1,2-Dibromoethane						CAS #:	106-93-4			
14.463	14.463	(0.958)	107	1138881	55.0991	55.099	80.00-	120.00	100.00	
14.463	14.463	(0.958)	109	1076614			63.06-	123.06	94.53	

109 Chlorobenzene						CAS #:	108-90-7			
15.154	15.154	(1.004)	112	1762848	53.9943	53.994	80.00-	120.00	100.00	
15.154	15.154	(1.004)	114	549032			1.82-	61.82	31.14	
15.154	15.154	(1.004)	77	1193514			36.53-	96.53	67.70	

111 Ethyl Benzene						CAS #:	100-41-4			
15.265	15.265	(1.011)	106	925418	57.6770	57.677	80.00-	120.00	100.00	
15.265	15.265	(1.011)	91	3288942			322.22-	382.22	355.40	

113 m,p-Xylene						CAS #:	108-38-3			
15.431	15.431	(1.022)	106	1153308	55.2104	55.210	80.00-	120.00	100.00	
15.431	15.431	(1.022)	91	2760665			202.98-	262.98	239.37	

114 o-Xylene						CAS #:	95-47-6			
15.956	15.956	(1.057)	106	1065180	53.9194	53.919	80.00-	120.00	100.00	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
114 o-Xylene (continued)									
15.956	15.956	(1.057)	91	2781167			222.10- 282.10	261.10	

115 Styrene CAS #: 100-42-5									
16.012	16.012	(1.060)	104	1677103	58.0825	58.082	80.00- 120.00	100.00	
16.012	16.012	(1.060)	78	1146526			35.14- 95.14	68.36	

118 Bromoform CAS #: 75-25-2									
16.260	16.260	(1.077)	173	1224808	64.9153	64.915	80.00- 120.00	100.00	
16.260	16.260	(1.077)	171	627452			21.42- 81.42	51.23	

123 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.896	16.896	(1.119)	83	1588729	51.4885	51.488	80.00- 120.00	100.00	
16.896	16.896	(1.119)	85	1061887			35.14- 95.14	66.84	

126 4-Ethyltoluene CAS #: 622-96-8									
17.062	17.062	(1.130)	105	4095414	60.3780	60.378	80.00- 120.00	100.00	
17.062	17.062	(1.130)	120	1123046			0.00- 58.08	27.42	

128 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.145	17.145	(1.135)	105	3274766	57.5817	57.582	80.00- 120.00	100.00	
17.145	17.145	(1.135)	120	1459617			16.58- 76.58	44.57	

131 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.532	17.532	(1.161)	105	3647744	59.7380	59.738	80.00- 120.00	100.00	
17.532	17.532	(1.161)	120	1541296			12.44- 72.44	42.25	

138 1,3-Dichlorobenzene CAS #: 541-73-1									
17.836	17.836	(1.181)	146	2140919	53.4897	53.490	80.00- 120.00	100.00	
17.836	17.836	(1.181)	148	1387363			33.12- 93.12	64.80	
17.836	17.836	(1.181)	111	1009504			15.78- 75.78	47.15	

141 1,4-Dichlorobenzene CAS #: 106-46-7									
17.919	17.919	(1.187)	146	1745478	55.1480	55.148	80.00- 120.00	100.00	
17.919	17.919	(1.187)	148	1108635			34.33- 94.33	63.51	
17.919	17.919	(1.187)	111	863073			18.49- 78.49	49.45	

143 alpha-Chlorotoluene CAS #: 100-44-7									
18.058	18.058	(1.196)	91	3583114	67.8535	67.854	80.00- 120.00	100.00(R)	
18.058	18.058	(1.196)	126	587594			0.00- 47.06	16.40	

146 1,2-Dichlorobenzene CAS #: 95-50-1									
18.279	18.279	(1.211)	146	2140217	51.5482	51.548	80.00- 120.00	100.00	
18.279	18.279	(1.211)	148	1357156			32.04- 92.04	63.41	
18.279	18.279	(1.211)	111	1014397			18.51- 78.51	47.40	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

154	1,2,4-Trichlorobenzene					CAS #:	120-82-1			
19.578	19.578	(1.297)	180	1437533	49.2347	49.235	80.00-	120.00	100.00	
19.578	19.578	(1.297)	182	1418219			64.91-	124.91	98.66	

155	Hexachlorobutadiene					CAS #:	87-68-3			
19.661	19.661	(1.302)	225	1323155	54.6863	54.686	80.00-	120.00	100.00	
19.661	19.661	(1.302)	223	851975			32.04-	92.04	64.39	

124	Propylbenzene					CAS #:	103-65-1			
16.924	16.924	(1.121)	91	4814199	61.3445	61.344	80.00-	120.00	100.00	
16.924	16.924	(1.121)	120	959905			0.00-	50.53	19.94	
16.924	16.924	(1.121)	105	170868			0.00-	33.52	3.55	

119	Cumene					CAS #:	98-82-8			
16.426	16.426	(1.088)	105	3667168	60.7582	60.758	80.00-	120.00	100.00	
16.426	16.426	(1.088)	120	873976			0.00-	55.50	23.83	
16.426	16.426	(1.088)	51	707310			0.00-	50.84	19.29	

156	Naphthalene					CAS #:	91-20-3			
19.744	19.744	(1.308)	128	4052641	46.7580	46.758	80.00-	120.00	100.00	
19.744	19.744	(1.308)	127	535767			0.00-	42.90	13.22	

30	Isopentane					CAS #:	78-78-4			
3.514	3.542	(0.429)	43	2629690	48.6703	48.670	80.00-	120.00	100.00	
3.514	3.542	(0.429)	57	1522829			30.33-	90.33	57.91	
3.514	3.542	(0.429)	72	131250			0.00-	34.69	4.99	

21	Butane					CAS #:	106-97-8			
2.740	2.767	(0.335)	58	445104	50.4983	50.498	80.00-	120.00	100.00	
2.740	2.767	(0.335)	43	3501210			773.30-	833.30	786.60	

96	Methyl Cyclohexane					CAS #:	108-87-2			
10.703	10.703	(1.063)	83	1264675	51.5598	51.560	80.00-	120.00	100.00	
10.703	10.703	(1.063)	98	647715			20.58-	80.58	51.22	
10.703	10.703	(1.063)	55	1756123			125.23-	185.23	138.86	

QC Flag Legend

R - Spike/Surrogate failed recovery limits.

Report Date: 07-Jun-2007 15:25

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 07-JUN-2007

Lab File ID: 5060711.d

Calibration Time: 13:20

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /var/chem/msd5.i/5-07jun.b/t14q529a.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	292964	175778	410150	238932	-18.44
79 1,4-Difluorobenze	1106143	663686	1548600	921544	-16.69
108 Chlorobenzene-d5	855448	513269	1197627	712923	-16.66

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
57 Bromochloromethan	8.21	7.88	8.54	8.19	-0.34
79 1,4-Difluorobenze	10.07	9.74	10.40	10.07	0.00
108 Chlorobenzene-d5	15.10	14.77	15.43	15.10	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msds.1/5-07jun.b/5060711.d
Date: 07-JUN-2007 14:35
Client ID: LCS-1
Sample Info: 50mL #1487-275

Column phase: RTX-624

Instrument: msds.1
Operator: JG
Column diameter: 0.53

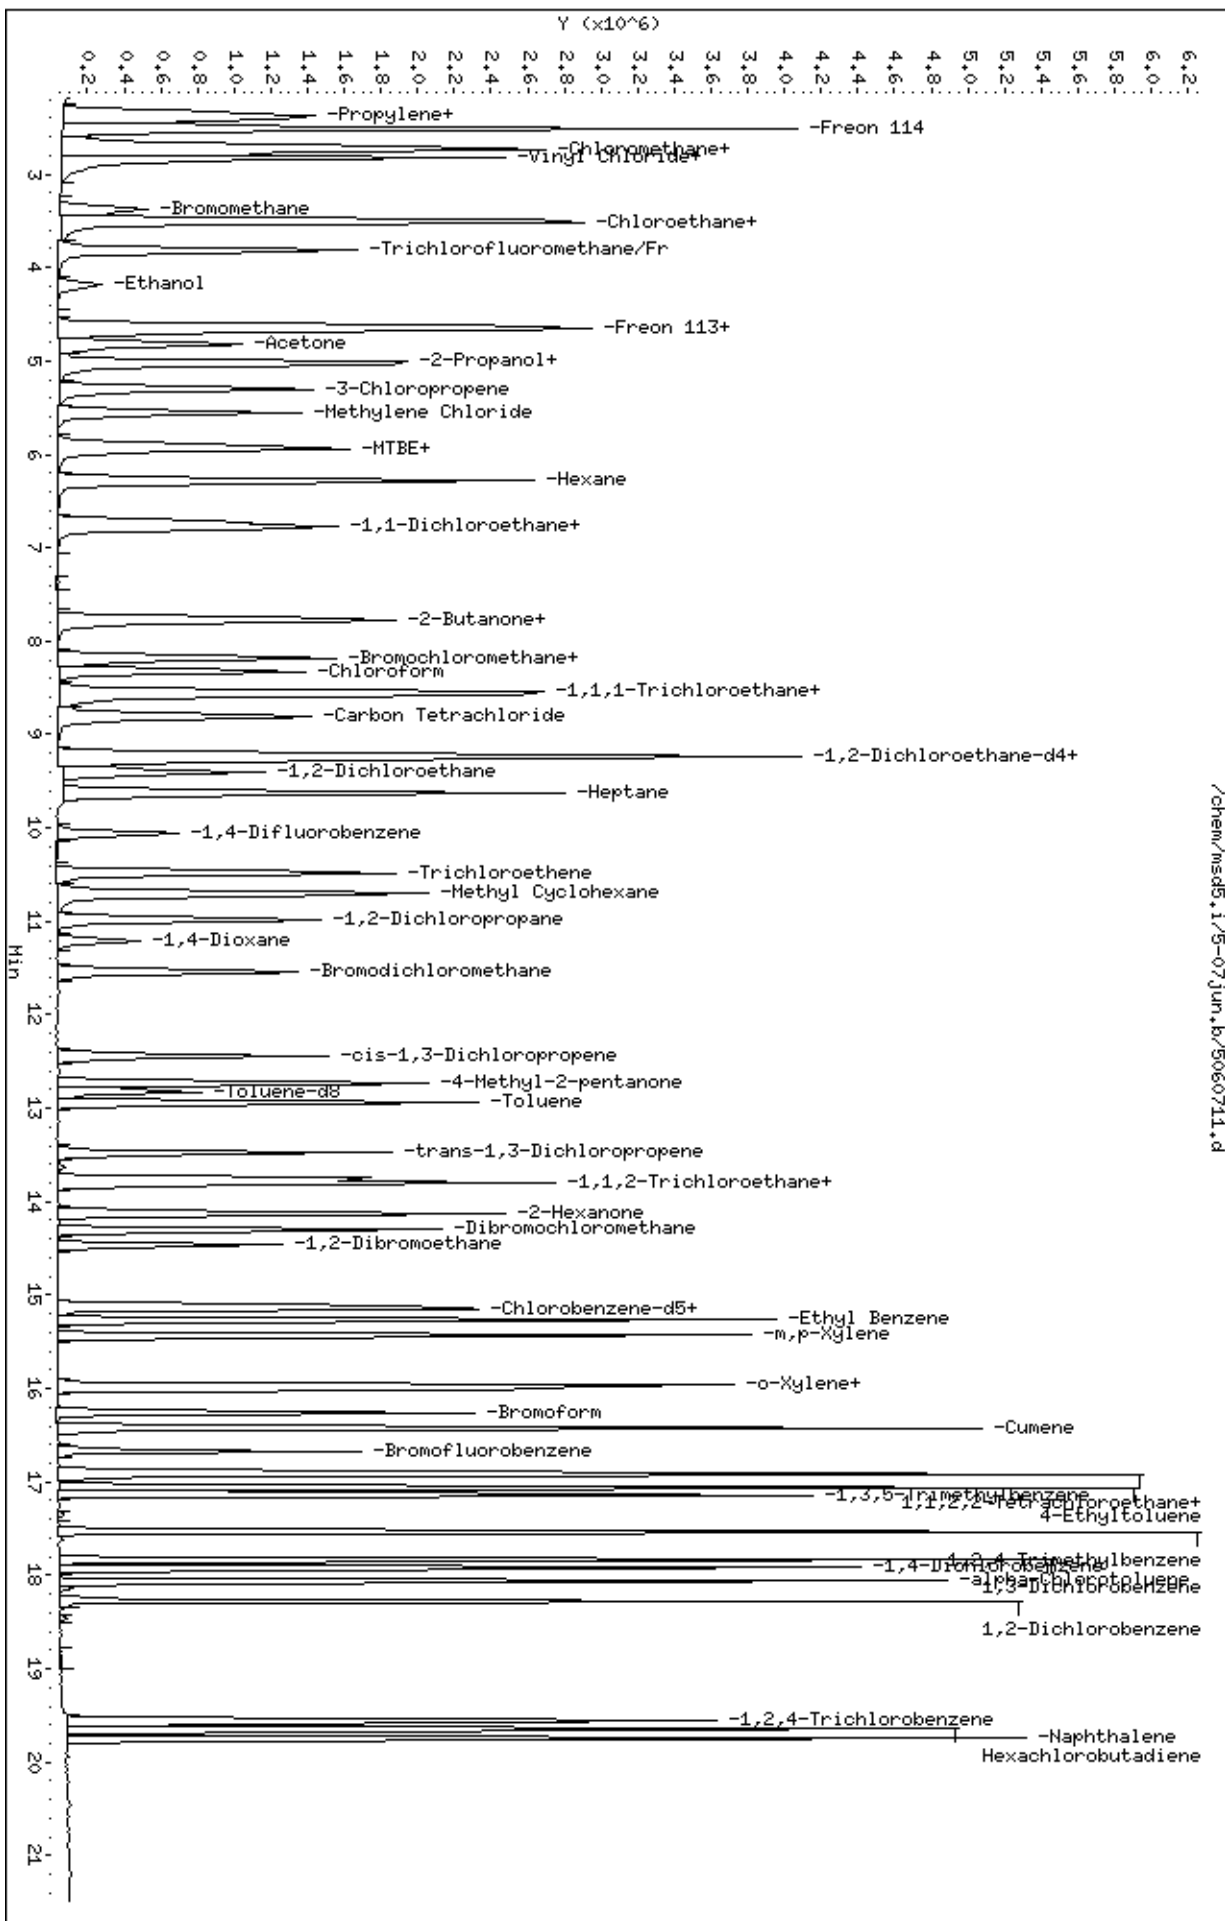

/chem/msds.1/5-07jun.b/5060711.d

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	36.21
75	30.0 - 60.0% of mass 95	54.28
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.61
173	Less than 2.0% of mass 174	(1.00) ¹
174	Greater than 50.0% of mass 95	56.03
175	5.0 - 9.0% of mass 174	(7.24) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(97.75) ¹
177	5.0 - 9.0% of mass 176	(6.58) ²

BFB Injection Date: 6/7/07
 BFB Injection Time: 12:51
 BFB File ID: SD00708
 Tekmar Purge Flow:
 Vacuum:
 ISS Std #: 1402-259 Exp. Date: 9/10/07
 BCM: 202064
 14-DFB: 106143
 CB-d5: 855448
 Verified CCV IS vs ICAL mid-point (-40%^d) Q-

Verify 176/174 m/z Ratio: $\frac{100}{100} = 1.00 = 97.75\%$

NOAH Cart #: 15/10 File #: SD00708/ F060708

Calculation Check:

$$\frac{\text{Area}_{\text{m/z 176}}}{\text{Area}_{\text{m/z 174}}} \times \frac{\text{Conc.}_{\text{m/z 174}}}{\text{RRF}} = \frac{(104922)}{(106143)} \times \frac{(25)}{(2.90997)} = 26.077$$

Reported Result 26.077

File ID: SD00708
 Compound: 71-48
 Initials: Q-

eg	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Loader Init.	Date Analyzed	Time Analyzed	Review Init.	Comments
1	✓ SD00708	BFB Tare Check	643-2286	SDing	2g	1.00	Q-	6/7/07	12:51	Q-	
2	✓ 09	CV # 1487-286	200g	SDing	SDing				13:20	Q-	UTBE out
3	X 10	LC # 1489-225							13:48	Q-	
4	✓ 11	LC # 1489-225							14:35	Q-	
5	✓ 12	LAB Blank	13073	Humid	200ul	1.00	Q-		16:10	Q-	
6	✓ 13	0706057 - 01A	11006	6.0% Spis		1.00	KR		17:42	KR	
7	✓ 14	↓ - 02A	70-1900	↓		1.00			18:14	KR	
8	✓ 15	0705649 - 01A	1418	10.1% Spis		2.00			18:46	KR	
9	✓ 16	↓ - 01A	↓	↓		↓			19:18	KR	

Signature

[Signature]

Date: 6/7/07

Report Date: 29-May-2007 14:40

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-29may.b/5052909.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 29-MAY-2007 14:47
 Operator : JG Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2ul #843-2980;50 ng
 Comment :
 Method : /var/chem/msd5.i/5-29may.b/bfb30.m
 Meth Date : 29-May-2007 14:40 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb								
3.860	3.900	-0.040	95	1533988			100.00- 100.00	100.00
3.860	3.900	-0.040	50	589973			15.00- 40.00	38.46
3.860	3.900	-0.040	75	819322			30.00- 60.00	53.41
3.860	3.900	-0.040	96	98444			5.00- 9.00	6.42
3.860	3.900	-0.040	173	7499			0.00- 2.00	0.83
3.860	3.900	-0.040	174	907809			50.00- 100.00	59.18
3.860	3.900	-0.040	175	64122			5.00- 9.00	7.06
3.860	3.900	-0.040	176	878321			95.00- 101.00	96.75
3.860	3.900	-0.040	177	56933			5.00- 9.00	6.48

Data File: /var/chem/msd5.i/5-29may.b/5052909.d

Page 1

Date : 29-MAY-2007 14:47

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

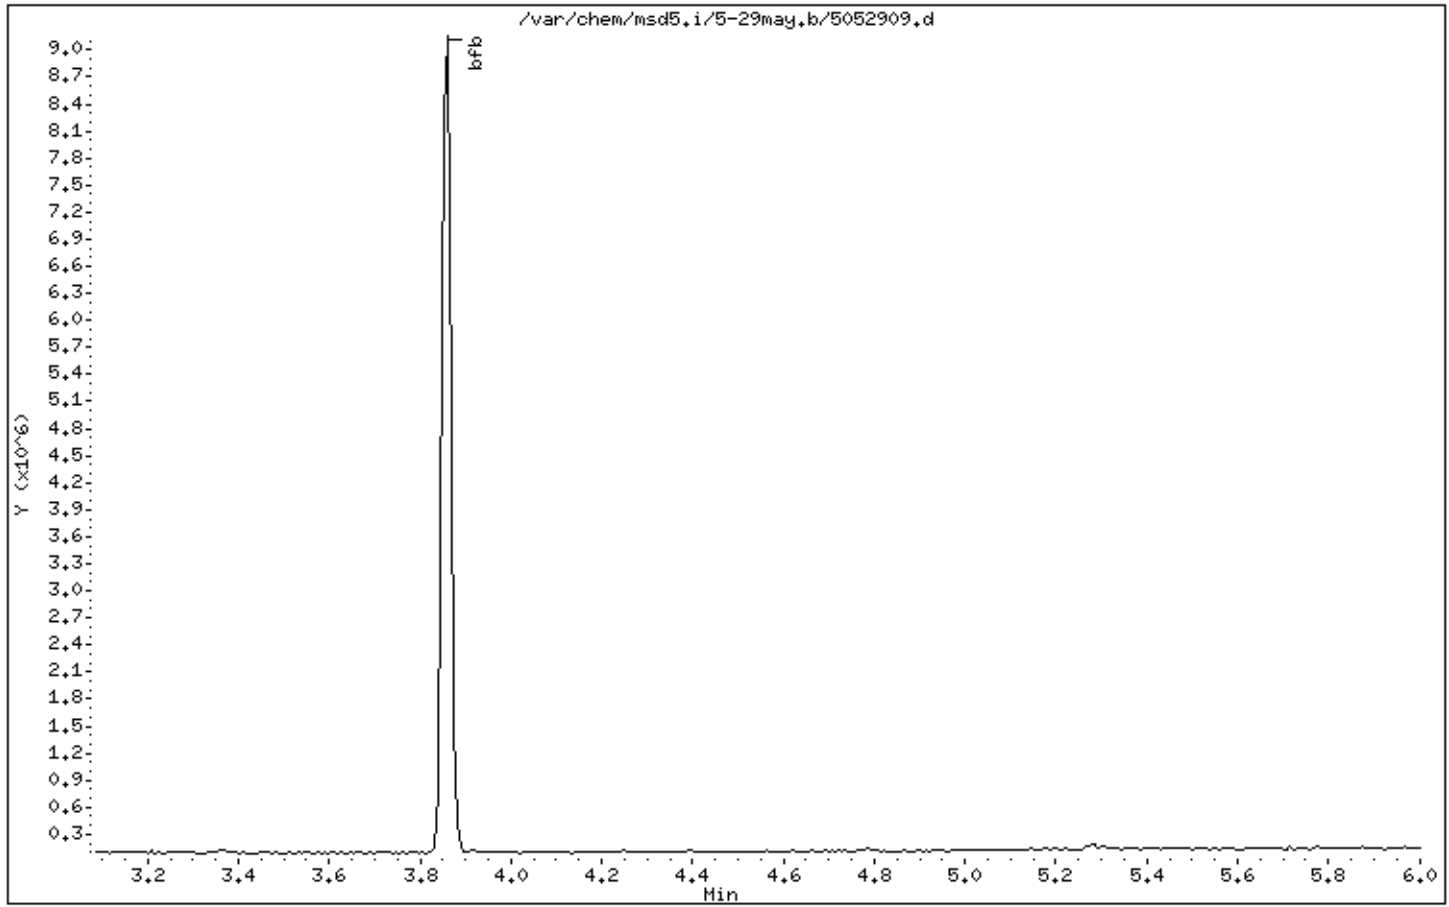

Date : 29-MAY-2007 14:47

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

1 bfb

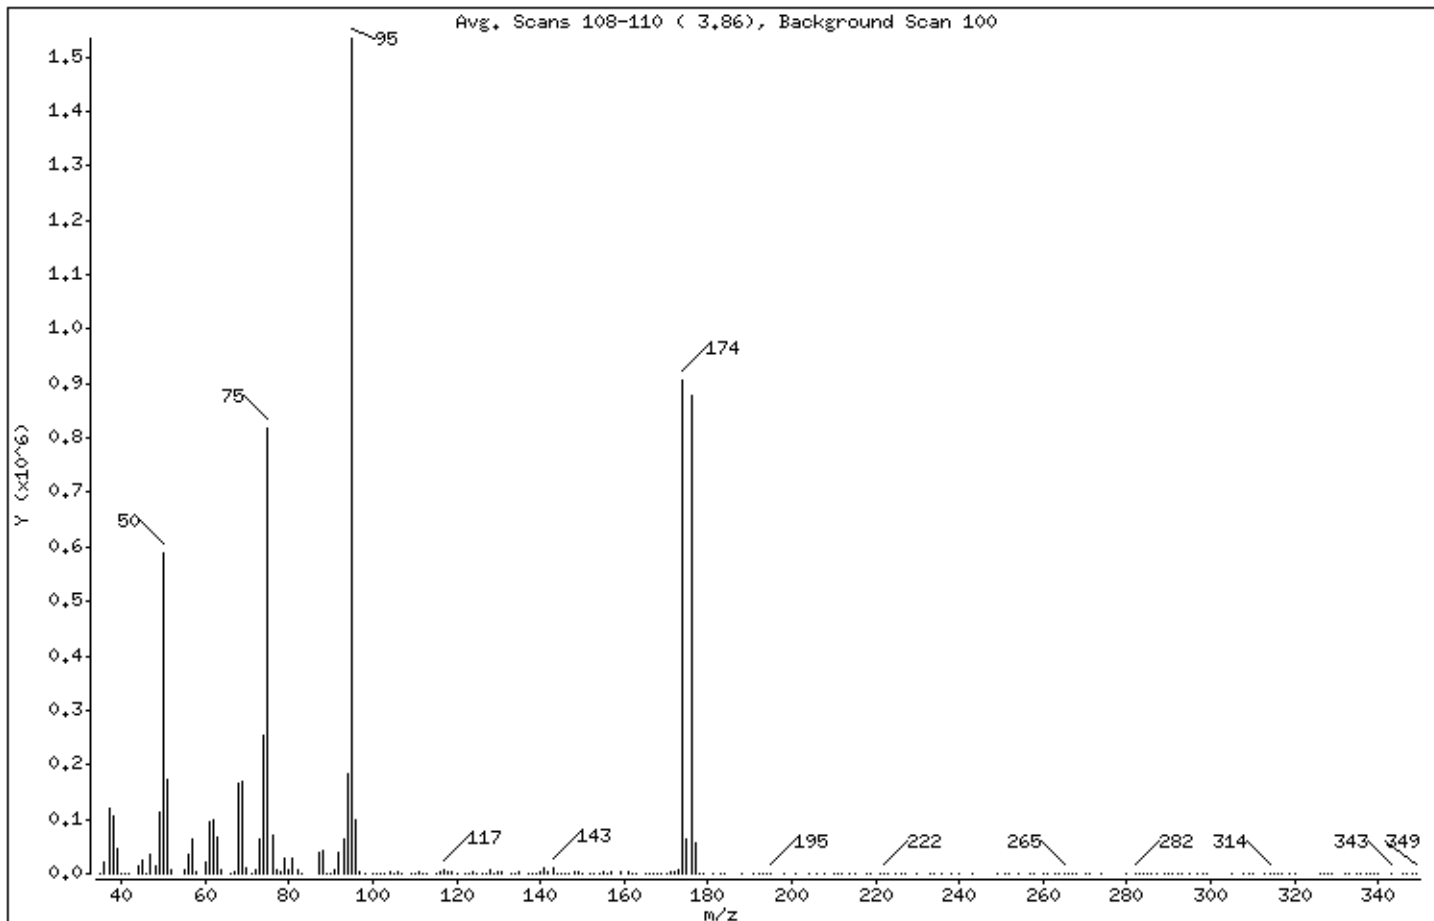

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	38.46
75	30.00 - 60.00% of mass 95	53.41
96	5.00 - 9.00% of mass 95	6.42
173	Less than 2.00% of mass 174	0.49 (0.83)
174	50.00 - 100.00% of mass 95	59.18
175	5.00 - 9.00% of mass 174	4.18 (7.06)
176	95.00 - 101.00% of mass 174	57.26 (96.75)
177	5.00 - 9.00% of mass 176	3.71 (6.48)

Date : 29-MAY-2007 14:47

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

Data File: 5052909.d

Spectrum: Avg. Scans 108-110 (3.86), Background Scan 100

Location of Maximum: 95.00

Number of points: 222

m/z	Y	m/z	Y	m/z	Y	m/z	Y
35,00	479	100,00	176	165,00	605	261,00	165
36,00	22232	101,00	382	166,00	317	263,00	59
37,00	118808	102,00	409	167,00	163	264,00	85
38,00	104848	103,00	1002	168,00	1385	265,00	457
39,00	45304	104,00	3980	169,00	692	266,00	73
40,00	1683	105,00	771	170,00	1428	267,00	70
41,00	826	106,00	3461	171,00	1929	268,00	455
42,00	63	107,00	522	172,00	2697	270,00	81
44,00	12641	109,00	505	173,00	7499	271,00	117
45,00	23448	110,00	683	174,00	907776	274,00	287
46,00	1365	111,00	1785	175,00	64120	280,00	416
47,00	36048	112,00	1016	176,00	878272	282,00	1234
48,00	13962	113,00	811	177,00	56928	283,00	166
49,00	111736	115,00	1590	178,00	813	284,00	135
50,00	589952	116,00	3772	179,00	275	285,00	98
51,00	173760	117,00	7445	181,00	181	286,00	120
52,00	7870	118,00	4285	183,00	97	287,00	589
55,00	5532	119,00	4130	184,00	162	289,00	71
56,00	34816	120,00	1072	188,00	80	290,00	332
57,00	62184	122,00	144	191,00	206	291,00	140
58,00	3043	123,00	735	192,00	494	292,00	129
60,00	20064	124,00	1969	193,00	130	293,00	363
61,00	96184	125,00	311	194,00	388	295,00	56
62,00	98712	126,00	1634	195,00	615	297,00	137
63,00	67864	127,00	1282	198,00	237	298,00	17
64,00	6220	128,00	5579	201,00	309	299,00	319
66,00	330	129,00	1655	204,00	214	305,00	99
67,00	2772	130,00	4538	206,00	186	308,00	298
68,00	164864	131,00	2085	208,00	10	309,00	171
69,00	169664	133,00	759	210,00	197	310,00	216
70,00	9514	134,00	679	211,00	425	313,00	61
71,00	478	135,00	2066	212,00	156	314,00	406
72,00	7983	137,00	1448	214,00	397	315,00	254
73,00	62656	138,00	177	215,00	452	316,00	325
74,00	253440	139,00	539	218,00	90	317,00	79

Date : 29-MAY-2007 14:47

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

Data File: 5052909.d

Spectrum: Avg. Scans 108-110 (3.86), Background Scan 100

Location of Maximum: 95.00

Number of points: 222

m/z	Y	m/z	Y	m/z	Y	m/z	Y
75.00	819264	140.00	2098	219.00	257	319.00	60
76.00	71520	141.00	11134	221.00	160	320.00	311
77.00	6450	142.00	2300	222.00	399	326.00	208
78.00	1931	143.00	11275	223.00	378	327.00	378
79.00	29040	144.00	1040	225.00	247	328.00	104
80.00	8677	145.00	1043	226.00	29	329.00	56
81.00	28520	146.00	1538	227.00	144	332.00	125
82.00	5512	147.00	488	230.00	290	333.00	107
83.00	1215	148.00	3775	233.00	38	335.00	197
87.00	38280	149.00	1829	234.00	171	336.00	220
88.00	42544	150.00	1608	236.00	200	337.00	171
89.00	343	152.00	1035	238.00	112	338.00	113
90.00	369	153.00	880	240.00	137	339.00	342
91.00	5755	154.00	1506	243.00	53	340.00	77
92.00	38480	155.00	2500	249.00	158	343.00	459
93.00	63096	156.00	252	251.00	308	346.00	7
94.00	181760	157.00	2201	252.00	349	347.00	415
95.00	1533952	159.00	1839	254.00	343	348.00	96
96.00	98440	161.00	1892	257.00	254	349.00	264
97.00	3364	162.00	299	258.00	62		
98.00	177	163.00	642	260.00	79		

Report Date: 07-Jun-2007 12:44

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-07jun.b/5060708.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 07-JUN-2007 12:51
 Operator : JG Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2ul #843-2980;50 ng
 Comment :
 Method : /var/chem/msd5.i/5-07jun.b/bfb30.m
 Meth Date : 07-Jun-2007 12:44 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb							
3.860	3.900	-0.040	95	1245119		100.00- 100.00	100.00
3.860	3.900	-0.040	50	450798		15.00- 40.00	36.21
3.860	3.900	-0.040	75	675791		30.00- 60.00	54.28
3.860	3.900	-0.040	96	82285		5.00- 9.00	6.61
3.860	3.900	-0.040	173	7385		0.00- 2.00	1.06
3.860	3.900	-0.040	174	697589		50.00- 100.00	56.03
3.860	3.900	-0.040	175	50517		5.00- 9.00	7.24
3.860	3.900	-0.040	176	681877		95.00- 101.00	97.75
3.860	3.900	-0.040	177	44855		5.00- 9.00	6.58

Data File: /var/chem/msd5.i/5-07jun.b/5060708.d

Page 1

Date : 07-JUN-2007 12:51

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

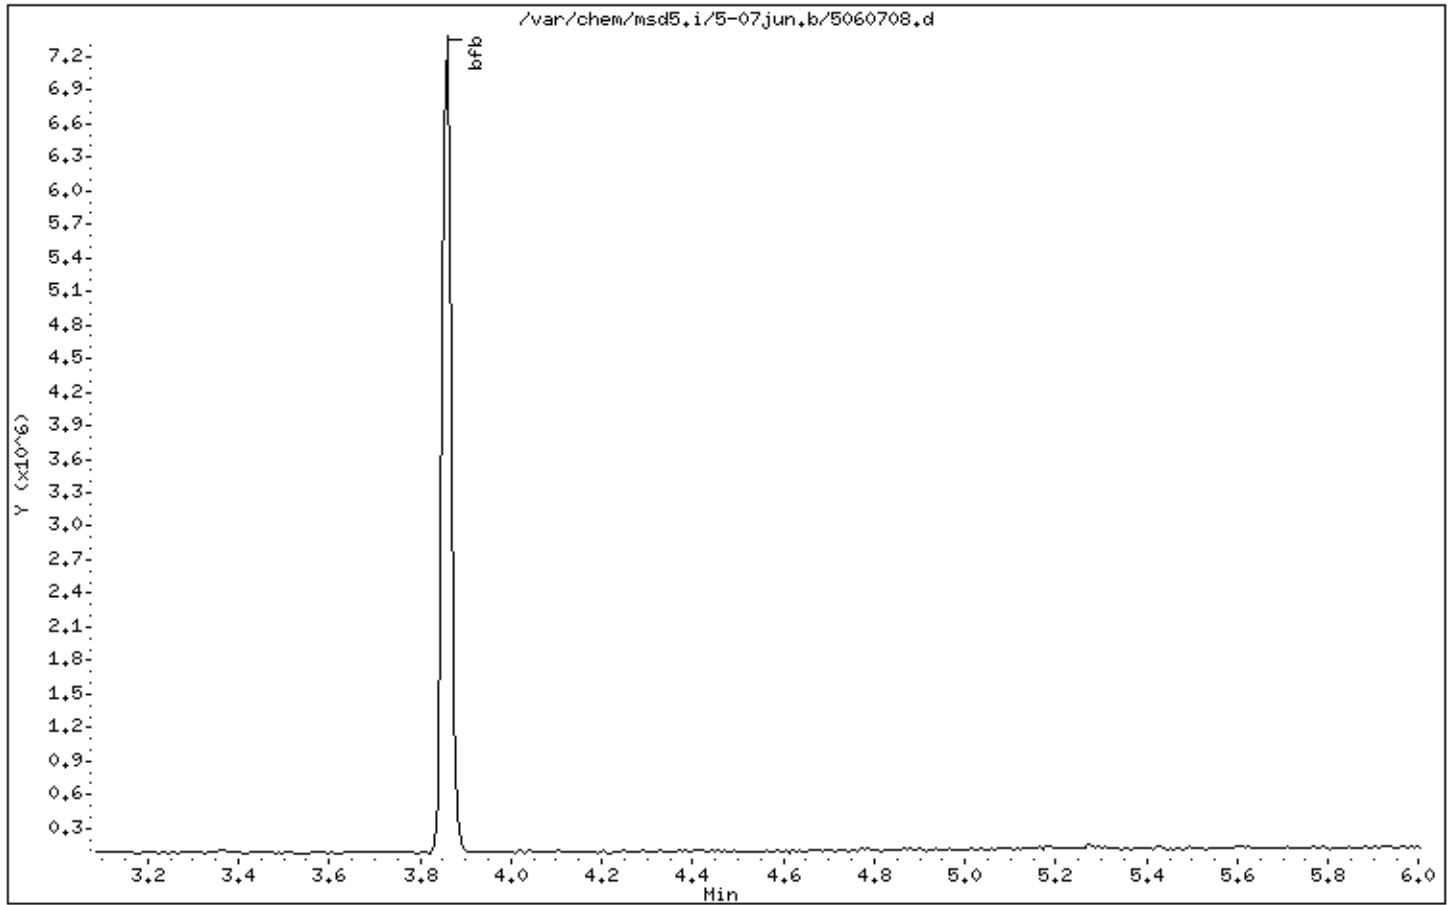

Date : 07-JUN-2007 12:51

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

1 bfb

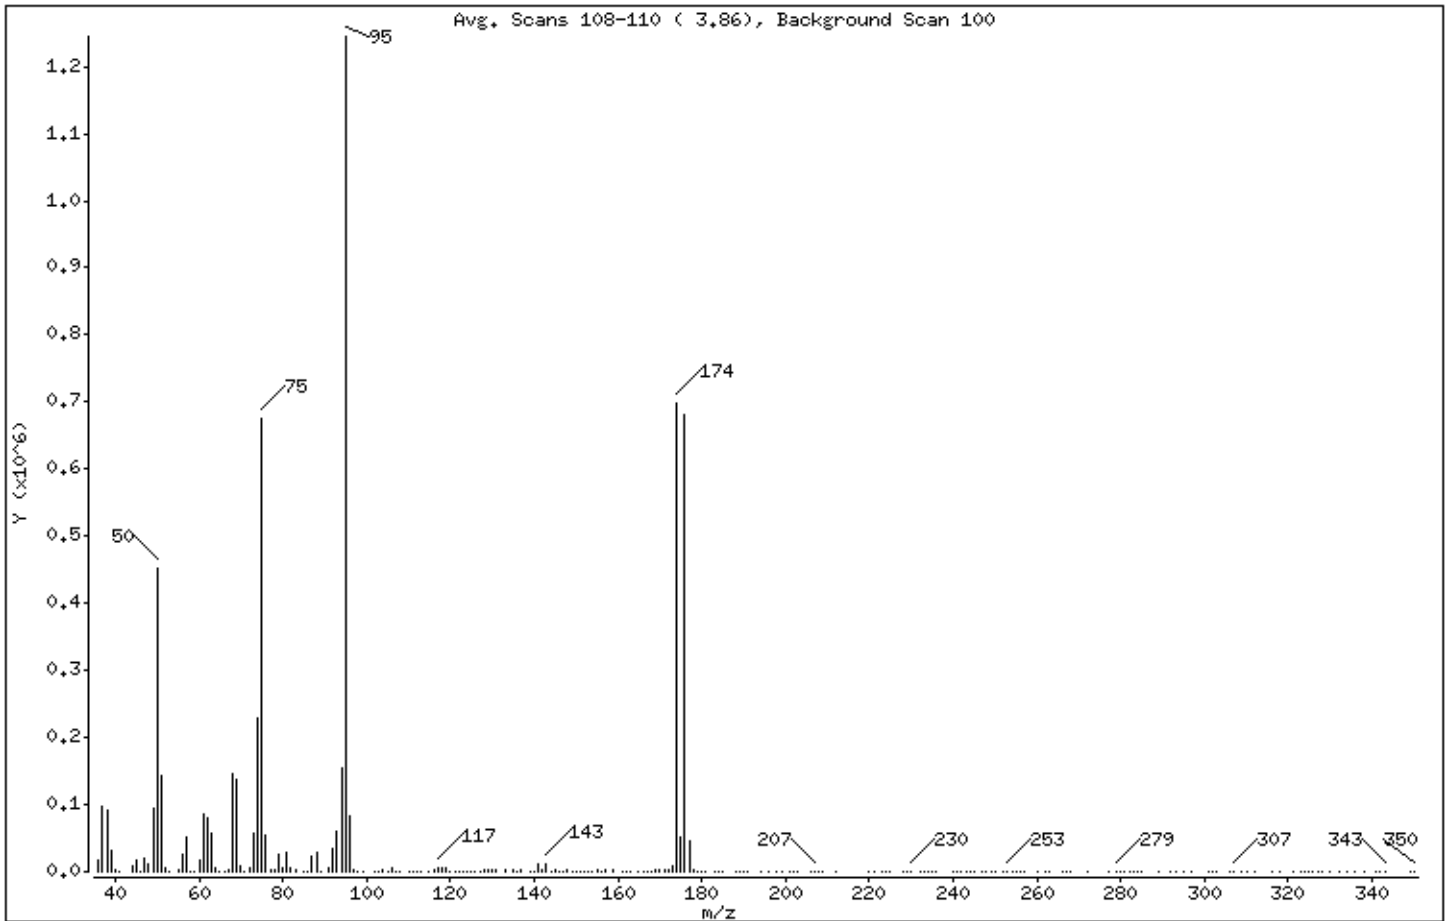

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	36.21
75	30.00 - 60.00% of mass 95	54.28
96	5.00 - 9.00% of mass 95	6.61
173	Less than 2.00% of mass 174	0.59 (1.06)
174	50.00 - 100.00% of mass 95	56.03
175	5.00 - 9.00% of mass 174	4.06 (7.24)
176	95.00 - 101.00% of mass 174	54.76 (97.75)
177	5.00 - 9.00% of mass 176	3.60 (6.58)

Date : 07-JUN-2007 12:51

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

Data File: 5060708.d

Spectrum: Avg. Scans 108-110 (3.86), Background Scan 100

Location of Maximum: 95.00

Number of points: 226

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	17360	98.00	186	165.00	63	249.00	238
37.00	98264	99.00	546	166.00	582	250.00	229
38.00	90200	102.00	353	167.00	247	252.00	266
39.00	32744	103.00	394	168.00	208	253.00	1226
40.00	1868	104.00	3485	169.00	1536	254.00	310
41.00	360	105.00	979	170.00	2040	255.00	354
44.00	9883	106.00	5337	171.00	2987	256.00	76
45.00	17984	107.00	958	172.00	2894	257.00	234
46.00	1173	108.00	74	173.00	7385	260.00	10
47.00	18912	110.00	953	174.00	697536	262.00	206
48.00	10492	111.00	942	175.00	50512	263.00	150
49.00	94568	112.00	985	176.00	681856	266.00	185
50.00	450752	113.00	1106	177.00	44848	267.00	132
51.00	142464	115.00	854	178.00	1767	268.00	218
52.00	4920	116.00	3283	179.00	491	272.00	68
53.00	760	117.00	6373	180.00	69	277.00	4
55.00	3814	118.00	4331	181.00	170	279.00	913
56.00	26112	119.00	5659	183.00	428	280.00	80
57.00	51424	120.00	569	184.00	14	281.00	173
58.00	1327	121.00	339	185.00	317	282.00	23
59.00	287	122.00	817	188.00	127	283.00	180
60.00	16696	123.00	231	189.00	695	284.00	194
61.00	85480	124.00	516	190.00	539	285.00	142
62.00	81424	125.00	321	191.00	659	289.00	284
63.00	56408	126.00	222	194.00	59	292.00	119
64.00	5434	127.00	549	196.00	296	293.00	229
65.00	69	128.00	3982	198.00	56	295.00	612
66.00	46	129.00	2499	199.00	277	297.00	60
67.00	3383	130.00	3825	201.00	77	301.00	161
68.00	145216	131.00	1910	202.00	346	302.00	132
69.00	137600	133.00	1616	203.00	55	303.00	65
70.00	8207	135.00	1593	206.00	86	306.00	174
71.00	202	136.00	1151	207.00	737	307.00	292
72.00	6564	137.00	2674	208.00	369	309.00	143
73.00	56496	139.00	733	209.00	550	310.00	204

Date : 07-JUN-2007 12:51

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: JG

Column phase:

Column diameter: 2.00

Data File: 5060708.d

Spectrum: Avg. Scans 108-110 (3.86), Background Scan 100

Location of Maximum: 95.00

Number of points: 226

m/z	Y	m/z	Y	m/z	Y	m/z	Y
74.00	229824	140.00	1067	212.00	192	312.00	102
75.00	675776	141.00	11630	220.00	351	316.00	90
76.00	55544	142.00	1688	221.00	66	318.00	269
77.00	2976	143.00	12237	223.00	163	321.00	220
78.00	2365	144.00	459	224.00	47	323.00	60
79.00	27096	145.00	2101	225.00	140	324.00	209
80.00	6805	146.00	1426	228.00	79	325.00	155
81.00	27376	147.00	610	229.00	162	326.00	92
82.00	5574	148.00	2909	230.00	519	327.00	109
83.00	1543	149.00	774	232.00	100	328.00	143
85.00	357	150.00	1332	233.00	363	330.00	55
86.00	1149	151.00	441	234.00	472	332.00	194
87.00	23136	152.00	296	235.00	171	334.00	268
88.00	27960	153.00	461	236.00	3	336.00	178
89.00	326	154.00	1373	240.00	237	338.00	196
91.00	4727	155.00	2656	241.00	319	341.00	77
92.00	34744	156.00	2	242.00	236	342.00	62
93.00	59880	157.00	1925	243.00	146	343.00	405
94.00	155648	159.00	1716	244.00	449	349.00	291
95.00	1244672	161.00	1386	245.00	45	350.00	225
96.00	82280	162.00	256	247.00	180		
97.00	2014	163.00	90	248.00	170		

Shipping/ Receiving Documents



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: _____ GEI Consultants, Inc.
ATTENTION: _____ Ms. Sarah Aldridge
FAX #: _____ 860-368-5307
FROM: _____ Sample Receiving
Workorder #: _____ 0706057
of pages (Including Cover): _____ 1

6/20/2007

Thank you for selecting Air Toxics Ltd. We have received your samples and have found discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Alicia Sullivan at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

The following discrepancy has been observed:

We have found a discrepancy between the Chain of Custody (COC) and the sample tags. The samples labeled AMS6-UW and AMS2-DW on the COC are labeled as 053007 AMS6-UW and 053007 AMS2-DW on the sample tags. ATL will report the sample identifications on the COC unless otherwise notified.

Your prompt response is appreciated.



AN ENVIRONMENTAL ANALYTICAL LABORATORY

SAMPLE RECEIPT SUMMARY

WORKORDER 0706057

Client

Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Dr. Suite 201
Glastonbury, CT 06033

Phone

860-368-5300

Fax

860-368-5307

Date Promised: 06/18/07

Date Completed: 6/15/07

Date Received: 6/4/07

PO#: NR

Project#: 061140-8-1703 Bay Barrier Wall Installation

Sales Rep: ANS

Total \$: \$ 676.00

Logged By: MW

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A	AMS6-UW	Modified TO-15	5/30/2007	6.0 "Hg	\$225.00
02A	AMS2-DW	Modified TO-15	5/30/2007	6.0 "Hg	\$225.00
03A	Lab Blank	Modified TO-15	NA	NA	\$0.00
04A	CCV	Modified TO-15	NA	NA	\$0.00
05A	LCS	Modified TO-15	NA	NA	\$0.00
Misc. Charges 6 Liter Summa Canister (3) @ \$50.00 each.					\$150.00
Blue Body Flow Controller (2) @ \$35.00 each.					\$70.00
Fuel Surcharge (3) @ \$2.00 each.					\$6.00

Note: Samples received after 3 P.M. PST are considered to be received on the following work day.
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

BILL TO: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Dr. Suite 201
Glastonbury, CT 06033

Analysis Code: TO-14A

TERMS:

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

Sample Discrepancy Report

Identification

Initiated By: MW Date: 6/4

Discrepancy Type: I. II. III.
(circle all that apply)

Workorder(s) affected: 0706057 Sample(s) affected: all

I. Sample Receipt Discrepancies

Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative

Narration not required:

- COC was not filled out in ink.
- Sample container (cartridge/tube/VOA vial) was received broken, however sample was intact.
- Flow controller used - canister samples received at ambient or under pressure.
- No brass cap on canister. OIA + O2A
- VOA vial for RSK-175 analysis received with headspace bubble <5mm.

Narration Required:

- COC improperly relinquished / received.
- Sample tags / can numbers do not match the COC.
- Samples received at wrong temperature (up to 10°C); ice / blue ice (circle one) was present. A temp. blank was / was not present (circle one).
- Custody Seal on the outside of the container was broken / improperly placed (circle one).
- Other (describe below).

Describe the Discrepancy: OIA 053007 AMS 6 VW O2A: 053007 AMS 2 DW
Can catalog # over is 24174 (client used this # as can # - ok)

II. Sample Receipt/Screening Discrepancies requiring CSR notification

Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative

If Section II. is filled out CSR must be notified within 24 hrs of Initiation

- COC was not received with samples.
- Analysis method(s) is not specified / incorrectly specified (circle one) on the COC.
- Number of samples on the COC does not match the number of samples that were received.
- Samples were received expired.
- Sampling date / time (sulfur only) is not documented for some / any samples (circle one).
- Sample received with significant (pooling) volume of H₂O in the Tedlar Bag.
- Sample container (cartridge/tube/VOA vial/DNPH Bottle, etc.) was received broken / leaking (circle one); sample can / cannot be analyzed (circle one).
- VOA vial for RSK-175 analysis received with headspace bubble >5mm.
- Samples for RSK-175 CO₂ analysis received preserved with HCl.
- Tedlar Bag received leaking / flat (circle one). Sample can / cannot (circle one) be analyzed.
- Canister was at ambient pressure at time of pressurization and (check all that apply): canister failed leak check on two manifolds, canister valve was open, brass nut was loose. Sample can / cannot be analyzed (circle one).
- Tedlar bag / canister received emitting a strong odor; sample can / cannot (circle one) be analyzed.
- Canister sample received with a vacuum difference >7.0"Hg between the receipt vac. and the final vac. reported on the COC, indicating loss of vacuum.
- Canister sample received at >15"Hg (not identified as a Trip/Field Blank).
- Trip Blank received at low vacuum (< 25"Hg).
- Tedlar Bag for Sulfur analysis has metal fitting.
- Incorrect sampling media / container for analysis requested.
- Sample was received at ≥ 10°C.
- Other (describe below)

Initials: _____ Date: _____
(if not the original initiator)

CSR Notified
(see section below)

Describe the Discrepancy: _____

Other Records

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	

DATA REVIEW CHECKLIST

Work Order #:

0700057

A R T M Q
[] [] [] [] []
[] [] [] [] []
[] [] [] [] []
QA NA QA NA
[] [] [] [] []
[] [] [] [] []

- Analysis/Reporting vs. Project Profile/SOP requirements checked (i.e. 100% Dups, J-Flag to MDL, etc)
The final report has the correct reporting list, special units, and header info.
Lab Narrative is correct (proper method & description/Receiving & Analytical notes correct)
Corrective Action issued - #
Unusual circumstances have been documented in the notes section below

LUMEN validation report present and initialed

CIRCLE (YES) / NO

- Lab Blank, CCV, LCS and DUP met QC criteria
Hold time is met for all samples
Appropriate data qualifier flags are applied
Manual integrations for samples and QC are properly documented
Samples analyzed within the project or method specific clock
Retention times have been verified
Appropriate ICAL(s) included
At least one result per sample is verified against the target quant sheets/raw data

- Dilution factor correctly calculated (sample load volume, syringe and bag dilutions, can pressurization(s))
Correct amount of sample analyzed (i.e. sample not over-diluted)
Spectra verified - documentation of spectral defense included (Section 5A of eCVP pkg)
TICs resemble reference spectra
TICs between duplicate samples are consistent
Checked samples for trends (i.e. Influent>Effluent, Landfill or Ambient etc)
Special units for all samples in the final report are correctly calculated
Manually entered results checked (i.e. special CCV compounds)
TPH/NMOC (verify calculations and correct reference compound used)
Chain of Custody scanned correctly
Verify sample id's vs. chain of custody
Samples pressurized w/ appropriate gas (N2 or He)
Final pressure consistent with canister size (6L vs. 1L)
Verify receipt pressures against logbook and target
Verify canister ID #'s
Extra printed copies are provided per client profile
Final invoice amount correct (adjusted for TAT, Penalties, Re-issue Charges etc.)
Client LUMEN report reviewed for accuracy and completeness

Notes: (to include: noting samples with QA/QC problems, Blanks with positive hits, narratives, etc.)

A/R: 1 hit in CCV, 1 hit in LCS

M/Q:

A (Analytical Review/Date) R/T (Reporting Review/Date) M (Management Review/Date) Q (QA Review/Date)
[Signature] 6/18/07 [Signature] 6/19/07 [Signature] 6/20/07

T: 6/15/07

Not Applicable