



**Air
Toxics LTD.**
Laboratory Services Since 1989

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

COMPREHENSIVE VALIDATION PACKAGE

Modified TO-15

INVENTORY SHEET

Work Order #: 0706310

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	22
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	23	30
b. Surrogate Recover Summary Form (If Applicable)	31	31
c. Internal Standard Summary Form (If Applicable)	32	32
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	33	150
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	151	165
i. Second Source LCS(Summary + Raw Data)	166	179
j. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	180	181
l. GC/MS Tune (Results + Raw Data)	182	201
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	202	203
b. Chain-of-Custody Records	204	204
c. Sample Log-In Sheet	205	205
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	206	206
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	207	209
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	210	211
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	--	--
i. <u>Data Review Check Sheet</u>	212	212

Comments:

Completed by:

Judy Lee

(Signature)

Judy Lee / Document Control

(Print Name & Title)

7/3/07

(Date)




AN ENVIRONMENTAL ANALYTICAL LABORATORY

WORK ORDER #: 0706310

Work Order Summary

CLIENT:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Dr. Suite 201 Glastonbury, CT 06033	BILL TO:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Dr. Suite 201 Glastonbury, CT 06033
PHONE:	860-368-5300	P.O. #	NR
FAX:	860-368-5307	PROJECT #	061140-8-1703 BayShore OU1 Southern
DATE RECEIVED:	06/15/2007	CONTACT:	cell Air Monitorin Bryanna Langley
DATE COMPLETED:	06/27/2007		

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>
01A	AMS2-UW	Modified TO-15	12.5 "Hg
02A	AMS4+60N-DW	Modified TO-15	5.5 "Hg
03A	Lab Blank	Modified TO-15	NA
04A	CCV	Modified TO-15	NA
05A	LCS	Modified TO-15	NA

CERTIFIED BY:  DATE: 06/27/07

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004
 NY NELAP - 11291, UT NELAP - 9166389892
 Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,
 Accreditation number: E87680, Effective date: 07/01/06, Expiration date: 06/30/07
 Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards
 This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.
 180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
 (916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

**LABORATORY NARRATIVE
Modified TO-15
GEI Consultants, Inc.
Workorder# 0706310**

Two 6 Liter Summa Canister samples were received on June 15, 2007. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

This workorder was independently validated prior to submittal using 'USEPA National Functional Guidelines' as generally applied to the analysis of volatile organic compounds in air. A rules-based, logic driven, independent validation engine was employed to assess completeness, evaluate pass/fail of relevant project quality control requirements and verification of all quantified amounts.

Method modifications taken to run these samples are summarized in the below table. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	+/- 30% Difference	<= 30% Difference with two allowed out up to <=40%.; flag and narrate outliers
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

Receiving Notes

The Chain of Custody (COC) information for samples AMS2-UW and AMS4+60N-DW did not match the entries on the sample tags with regard to sample identification. Therefore the information on the COC was used to process and report the samples.

Analytical Notes

There were no analytical discrepancies.

Definition of Data Qualifying Flags

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

- B - Compound present in laboratory blank greater than reporting limit (background subtraction no performed).
- J - Estimated value.
- E - Exceeds instrument calibration range.

S - Saturated peak.

Q - Exceeds quality control limits.

U - Compound analyzed for but not detected above the reporting limit.

UJ- Non-detected compound associated with low bias in the CCV

N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

a-File was requantified

b-File was quantified by a second column and detector

r1-File was requantified for the purpose of reissue

Table 1

Client Sample ID	Lab Sample ID	Date Collected	Date Received	Date Extracted	Sample Holding Time (Days)	Date Analyzed	Sample Extract Holding Time (Days)	Sample Condition
AMS2-UW	0706310-01A	6/13/2007	6/15/2007	NA	9	6/22/2007	NA	Good
AMS4+60N-DW	0706310-02A	6/13/2007	6/15/2007	NA	10	6/23/2007	NA	Good
Lab Blank	0706310-03A	NA	NA	NA	NA	6/22/2007	NA	Good
CCV	0706310-04A	NA	NA	NA	NA	6/22/2007	NA	Good
LCS	0706310-05A	NA	NA	NA	NA	6/22/2007	NA	Good

Sample Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds
MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: AMS2-UW

Lab ID#: 0706310-01A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Acetone	4.6	5.9	11	14



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS2-UW

Lab ID#: 0706310-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062219	Date of Collection:	6/13/07
Dil. Factor:	2.30	Date of Analysis:	6/22/07 11:38 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	1.2	Not Detected	5.7	Not Detected
Freon 114	1.2	Not Detected	8.0	Not Detected
Vinyl Chloride	1.2	Not Detected	2.9	Not Detected
Bromomethane	1.2	Not Detected	4.5	Not Detected
Chloroethane	1.2	Not Detected	3.0	Not Detected
Freon 11	1.2	Not Detected	6.5	Not Detected
1,1-Dichloroethene	1.2	Not Detected	4.6	Not Detected
Freon 113	1.2	Not Detected	8.8	Not Detected
Methylene Chloride	1.2	Not Detected	4.0	Not Detected
1,1-Dichloroethane	1.2	Not Detected	4.6	Not Detected
cis-1,2-Dichloroethene	1.2	Not Detected	4.6	Not Detected
Chloroform	1.2	Not Detected	5.6	Not Detected
1,1,1-Trichloroethane	1.2	Not Detected	6.3	Not Detected
Carbon Tetrachloride	1.2	Not Detected	7.2	Not Detected
Benzene	1.2	Not Detected	3.7	Not Detected
1,2-Dichloroethane	1.2	Not Detected	4.6	Not Detected
Trichloroethene	1.2	Not Detected	6.2	Not Detected
1,2-Dichloropropane	1.2	Not Detected	5.3	Not Detected
cis-1,3-Dichloropropene	1.2	Not Detected	5.2	Not Detected
Toluene	1.2	Not Detected	4.3	Not Detected
trans-1,3-Dichloropropene	1.2	Not Detected	5.2	Not Detected
1,1,2-Trichloroethane	1.2	Not Detected	6.3	Not Detected
Tetrachloroethene	1.2	Not Detected	7.8	Not Detected
1,2-Dibromoethane (EDB)	1.2	Not Detected	8.8	Not Detected
Chlorobenzene	1.2	Not Detected	5.3	Not Detected
Ethyl Benzene	1.2	Not Detected	5.0	Not Detected
m,p-Xylene	1.2	Not Detected	5.0	Not Detected
o-Xylene	1.2	Not Detected	5.0	Not Detected
Styrene	1.2	Not Detected	4.9	Not Detected
1,1,2,2-Tetrachloroethane	1.2	Not Detected	7.9	Not Detected
1,3,5-Trimethylbenzene	1.2	Not Detected	5.6	Not Detected
1,2,4-Trimethylbenzene	1.2	Not Detected	5.6	Not Detected
1,3-Dichlorobenzene	1.2	Not Detected	6.9	Not Detected
1,4-Dichlorobenzene	1.2	Not Detected	6.9	Not Detected
alpha-Chlorotoluene	1.2	Not Detected	6.0	Not Detected
1,2-Dichlorobenzene	1.2	Not Detected	6.9	Not Detected
1,3-Butadiene	1.2	Not Detected	2.5	Not Detected
Hexane	1.2	Not Detected	4.0	Not Detected
Cyclohexane	1.2	Not Detected	4.0	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS2-UW

Lab ID#: 0706310-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062219	Date of Collection:	6/13/07
Dil. Factor:	2.30	Date of Analysis:	6/22/07 11:38 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	1.2	Not Detected	4.7	Not Detected
Bromodichloromethane	1.2	Not Detected	7.7	Not Detected
Dibromochloromethane	1.2	Not Detected	9.8	Not Detected
Cumene	1.2	Not Detected	5.6	Not Detected
Propylbenzene	1.2	Not Detected	5.6	Not Detected
Chloromethane	4.6	Not Detected	9.5	Not Detected
1,2,4-Trichlorobenzene	4.6	Not Detected	34	Not Detected
Hexachlorobutadiene	4.6	Not Detected	49	Not Detected
Acetone	4.6	5.9	11	14
Carbon Disulfide	1.2	Not Detected	3.6	Not Detected
2-Propanol	4.6	Not Detected	11	Not Detected
trans-1,2-Dichloroethene	1.2	Not Detected	4.6	Not Detected
2-Butanone (Methyl Ethyl Ketone)	1.2	Not Detected	3.4	Not Detected
Tetrahydrofuran	1.2	Not Detected	3.4	Not Detected
1,4-Dioxane	4.6	Not Detected	16	Not Detected
4-Methyl-2-pentanone	1.2	Not Detected	4.7	Not Detected
2-Hexanone	4.6	Not Detected	19	Not Detected
Bromoform	1.2	Not Detected	12	Not Detected
4-Ethyltoluene	1.2	Not Detected	5.6	Not Detected
Ethanol	4.6	Not Detected	8.7	Not Detected
Methyl tert-butyl ether	1.2	Not Detected	4.1	Not Detected
3-Chloropropene	4.6	Not Detected	14	Not Detected
2,2,4-Trimethylpentane	1.2	Not Detected	5.4	Not Detected
Naphthalene	4.6	Not Detected	24	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	99	70-130
1,2-Dichloroethane-d4	102	70-130
4-Bromofluorobenzene	101	70-130

Report Date: 27-Jun-2007 15:54

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22jun.b/8062219.d
 Lab Smp Id: 0706310-01A
 Inj Date : 22-JUN-2007 23:38
 Operator : kr Inst ID: msd8.i
 Smp Info : 200mL #3717
 Misc Info : 12.5"Hg-5psi
 Comment :
 Method : /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Meth Date : 22-Jun-2007 10:48 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 12:08 Cal File: 8060706.d
 Als bottle: 1
 Dil Factor: 2.30000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.414 (1.000)	130	265126	25.0000		80.00-	120.00	100.00	
7.387	7.414 (1.000)	128	204637			47.85-	107.85	77.18	
7.387	7.387 (1.000)	49	398381			115.74-	175.74	150.26	

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267 (1.000)	114	1141082	25.0000		80.00-	120.00	100.00	
9.267	9.267 (1.000)	88	171750			0.00-	44.74	15.05	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576 (1.000)	117	875431	25.0000		80.00-	120.00	100.00	
14.576	14.576 (1.000)	82	490146			0.00-	30.00	55.99	

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465 (1.146)	65	354742	25.5653	25.565	80.00-	120.00	100.00	
8.465	8.465 (1.146)	67	188393			0.00-	30.00	53.11	

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115 (1.307)	98	982351	24.8672	24.867	80.00-	120.00	100.00	
12.115	12.115 (1.307)	70	101587			0.00-	30.00	10.34	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 104 Toluene-d8 (continued)

12.115 12.115 (1.307) 100 639230 0.00- 30.00 65.07

\$ 140 Bromofluorobenzene

CAS #: 460-00-4

16.207 16.207 (1.112) 174 526498 25.2770 25.277 80.00- 120.00 100.00

16.207 16.207 (1.112) 95 658853 91.37- 151.37 125.14

16.207 16.207 (1.112) 176 506603 68.43- 128.43 96.22

30 Acetone

CAS #: 67-64-1

4.152 4.124 (0.562) 58 23443 2.58026 5.934 80.00- 120.00 100.00

4.124 4.124 (0.558) 43 67892 0.00- 30.00 289.60

Report Date: 27-Jun-2007 15:54

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msd8.i
Lab File ID: 8062219.d
Lab Smp Id: 0706310-01ACalibration Date: 22-JUN-2007
Calibration Time: 10:27

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m

Misc Info: 12.5"Hg-5psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	307449	184469	430429	265126	-13.77
88 1,4-Difluorobenze	1381560	828936	1934184	1141082	-17.41
125 Chlorobenzene-d5	1041151	624691	1457611	875431	-15.92

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.41	7.08	7.74	7.39	-0.37
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-22jun
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0706310-01A
Level: LOW Operator: kr
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m
Misc Info: 12.5"Hg-5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 82 1,2-Dichloroethane	25.000	25.565	102.26	70-130
\$ 104 Toluene-d8	25.000	24.867	99.47	70-130
\$ 140 Bromofluorobenzene	25.000	25.277	101.11	70-130

Data File: /chem/msd8.1/8-22jun.b/8062219.d

Date: 22-JUN-2007 23:38

Client ID:

Sample Info: 200mL #3717


Column phase: RTX-624

Instrument: msd8.1

Operator: kp

Column diameter: 0.53

/chem/msd8.1/8-22jun.b/8062219.d



Date : 22-JUN-2007 23:38

Client ID:

Instrument: msd8,i

Sample Info: 200mL #3717







Operator: kr

Column phase: RTX-624

Column diameter: 0.53

30 Acetone

Concentration: 5.934 PPBV

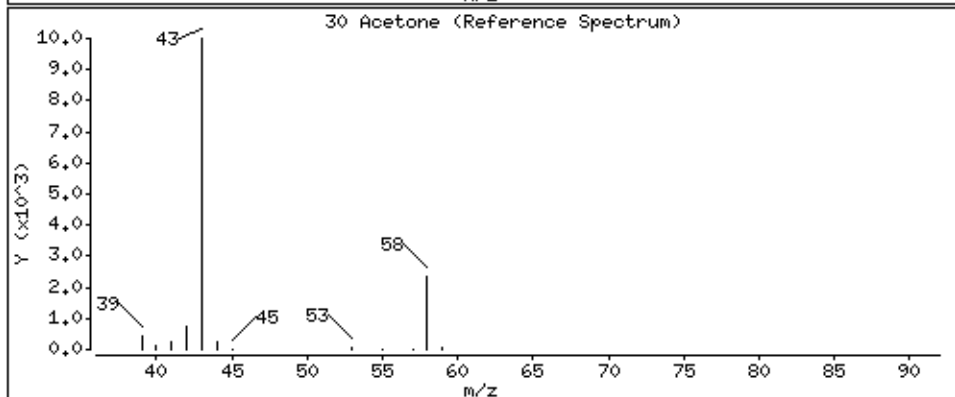



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds
MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: AMS4+60N-DW

Lab ID#: 0706310-02A

No Detections Were Found.



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS4+60N-DW

Lab ID#: 0706310-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062220	Date of Collection:	6/13/07
Dil. Factor:	1.64	Date of Analysis:	6/23/07 12:21 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.82	Not Detected	4.0	Not Detected
Freon 114	0.82	Not Detected	5.7	Not Detected
Vinyl Chloride	0.82	Not Detected	2.1	Not Detected
Bromomethane	0.82	Not Detected	3.2	Not Detected
Chloroethane	0.82	Not Detected	2.2	Not Detected
Freon 11	0.82	Not Detected	4.6	Not Detected
1,1-Dichloroethene	0.82	Not Detected	3.2	Not Detected
Freon 113	0.82	Not Detected	6.3	Not Detected
Methylene Chloride	0.82	Not Detected	2.8	Not Detected
1,1-Dichloroethane	0.82	Not Detected	3.3	Not Detected
cis-1,2-Dichloroethene	0.82	Not Detected	3.2	Not Detected
Chloroform	0.82	Not Detected	4.0	Not Detected
1,1,1-Trichloroethane	0.82	Not Detected	4.5	Not Detected
Carbon Tetrachloride	0.82	Not Detected	5.2	Not Detected
Benzene	0.82	Not Detected	2.6	Not Detected
1,2-Dichloroethane	0.82	Not Detected	3.3	Not Detected
Trichloroethene	0.82	Not Detected	4.4	Not Detected
1,2-Dichloropropane	0.82	Not Detected	3.8	Not Detected
cis-1,3-Dichloropropene	0.82	Not Detected	3.7	Not Detected
Toluene	0.82	Not Detected	3.1	Not Detected
trans-1,3-Dichloropropene	0.82	Not Detected	3.7	Not Detected
1,1,2-Trichloroethane	0.82	Not Detected	4.5	Not Detected
Tetrachloroethene	0.82	Not Detected	5.6	Not Detected
1,2-Dibromoethane (EDB)	0.82	Not Detected	6.3	Not Detected
Chlorobenzene	0.82	Not Detected	3.8	Not Detected
Ethyl Benzene	0.82	Not Detected	3.6	Not Detected
m,p-Xylene	0.82	Not Detected	3.6	Not Detected
o-Xylene	0.82	Not Detected	3.6	Not Detected
Styrene	0.82	Not Detected	3.5	Not Detected
1,1,2,2-Tetrachloroethane	0.82	Not Detected	5.6	Not Detected
1,3,5-Trimethylbenzene	0.82	Not Detected	4.0	Not Detected
1,2,4-Trimethylbenzene	0.82	Not Detected	4.0	Not Detected
1,3-Dichlorobenzene	0.82	Not Detected	4.9	Not Detected
1,4-Dichlorobenzene	0.82	Not Detected	4.9	Not Detected
alpha-Chlorotoluene	0.82	Not Detected	4.2	Not Detected
1,2-Dichlorobenzene	0.82	Not Detected	4.9	Not Detected
1,3-Butadiene	0.82	Not Detected	1.8	Not Detected
Hexane	0.82	Not Detected	2.9	Not Detected
Cyclohexane	0.82	Not Detected	2.8	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS4+60N-DW

Lab ID#: 0706310-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062220	Date of Collection:	6/13/07
Dil. Factor:	1.64	Date of Analysis:	6/23/07 12:21 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.82	Not Detected	3.4	Not Detected
Bromodichloromethane	0.82	Not Detected	5.5	Not Detected
Dibromochloromethane	0.82	Not Detected	7.0	Not Detected
Cumene	0.82	Not Detected	4.0	Not Detected
Propylbenzene	0.82	Not Detected	4.0	Not Detected
Chloromethane	3.3	Not Detected	6.8	Not Detected
1,2,4-Trichlorobenzene	3.3	Not Detected	24	Not Detected
Hexachlorobutadiene	3.3	Not Detected	35	Not Detected
Acetone	3.3	Not Detected	7.8	Not Detected
Carbon Disulfide	0.82	Not Detected	2.6	Not Detected
2-Propanol	3.3	Not Detected	8.1	Not Detected
trans-1,2-Dichloroethene	0.82	Not Detected	3.2	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.82	Not Detected	2.4	Not Detected
Tetrahydrofuran	0.82	Not Detected	2.4	Not Detected
1,4-Dioxane	3.3	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.82	Not Detected	3.4	Not Detected
2-Hexanone	3.3	Not Detected	13	Not Detected
Bromoform	0.82	Not Detected	8.5	Not Detected
4-Ethyltoluene	0.82	Not Detected	4.0	Not Detected
Ethanol	3.3	Not Detected	6.2	Not Detected
Methyl tert-butyl ether	0.82	Not Detected	3.0	Not Detected
3-Chloropropene	3.3	Not Detected	10	Not Detected
2,2,4-Trimethylpentane	0.82	Not Detected	3.8	Not Detected
Naphthalene	3.3	Not Detected	17	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	96	70-130
1,2-Dichloroethane-d4	103	70-130
4-Bromofluorobenzene	101	70-130

Report Date: 27-Jun-2007 15:54

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22jun.b/8062220.d
 Lab Smp Id: 0706310-02A
 Inj Date : 23-JUN-2007 00:21
 Operator : kr Inst ID: msd8.i
 Smp Info : 200mL #4068
 Misc Info : 5.5"Hg-5psi
 Comment :
 Method : /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Meth Date : 22-Jun-2007 10:48 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 12:08 Cal File: 8060706.d
 Als bottle: 1
 Dil Factor: 1.64000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.414	(1.000)	130	248843	25.0000		80.00- 120.00	100.00	
7.387	7.414	(1.000)	128	192414			47.85- 107.85	77.32	
7.387	7.387	(1.000)	49	369734			115.74- 175.74	148.58	

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	1088816	25.0000		80.00- 120.00	100.00	
9.267	9.267	(1.000)	88	160762			0.00- 44.74	14.76	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	816208	25.0000		80.00- 120.00	100.00	
14.576	14.576	(1.000)	82	454276			0.00- 30.00	55.66	

§ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.146)	65	334723	25.7010	25.701	80.00- 120.00	100.00	
8.465	8.465	(1.146)	67	178087			0.00- 30.00	53.20	

§ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	901328	23.9114	23.911	80.00- 120.00	100.00	
12.115	12.115	(1.307)	70	92640			0.00- 30.00	10.28	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
----	--------	----------	------	----------	---------	---------	--------------	-------

\$ 104 Toluene-d8 (continued)

12.115	12.115	(1.307)	100	597442			0.00- 30.00	66.28
--------	--------	---------	-----	--------	--	--	-------------	-------

\$ 140 Bromofluorobenzene

CAS #: 460-00-4

16.207	16.207	(1.112)	174	490841	25.2750	25.275	80.00- 120.00	100.00
16.207	16.207	(1.112)	95	613413			91.37- 151.37	124.97
16.207	16.207	(1.112)	176	472621			68.43- 128.43	96.29

Report Date: 27-Jun-2007 15:54

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i
 Lab File ID: 8062220.d
 Lab Smp Id: 0706310-02A
 Analysis Type: VOA
 Quant Type: ISTD
 Operator: kr
 Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Misc Info: 5.5"Hg-5psi

Calibration Date: 22-JUN-2007
 Calibration Time: 10:27
 Level: LOW
 Sample Type: AIR

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	307449	184469	430429	248843	-19.06
88 1,4-Difluorobenze	1381560	828936	1934184	1088816	-21.19
125 Chlorobenzene-d5	1041151	624691	1457611	816208	-21.61

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.41	7.08	7.74	7.39	-0.37
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-22jun
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0706310-02A
Level: LOW Operator: kr
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m
Misc Info: 5.5"Hg-5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 82 1,2-Dichloroethane	25.000	25.701	102.80	70-130
\$ 104 Toluene-d8	25.000	23.911	95.65	70-130
\$ 140 Bromofluorobenzene	25.000	25.275	101.10	70-130

Data File: /chem/msd8.1/8-22jun.b/8062220.d

Date : 23-JUN-2007 00:21

Client ID:

Sample Info: 200mL #4068


Column phase: RTX-624

Instrument: msd8.1

Operator: kp

Column diameter: 0.53

/chem/msd8.1/8-22jun.b/8062220.d



QC Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0706310-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062206	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/22/07 01:39 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0706310-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062206	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/22/07 01:39 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected	2.0	Not Detected
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	97	70-130
1,2-Dichloroethane-d4	103	70-130
4-Bromofluorobenzene	102	70-130

Report Date: 22-Jun-2007 14:01

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22jun.b/8062206.d
 Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
 Inj Date : 22-JUN-2007 13:39
 Operator : jdg Inst ID: msd8.i
 Smp Info : 200mL #13673
 Misc Info : Humid
 Comment :
 Method : /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Meth Date : 22-Jun-2007 10:48 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 12:08 Cal File: 8060706.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.414	(1.000)	130	259754	25.0000		80.00- 120.00	100.00	
7.387	7.414	(1.000)	128	203366			47.85- 107.85	78.29	
7.387	7.387	(1.000)	49	392099			115.74- 175.74	150.95	

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	1173930	25.0000		80.00- 120.00	100.00	
9.267	9.267	(1.000)	88	176668			0.00- 44.74	15.05	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	874596	25.0000		80.00- 120.00	100.00	
14.576	14.576	(1.000)	82	484033			0.00- 30.00	55.34	

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.146)	65	350180	25.7584	25.758	80.00- 120.00	100.00	
8.465	8.465	(1.146)	67	185531			0.00- 30.00	52.98	

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	982103	24.1653	24.165	80.00- 120.00	100.00	
12.115	12.115	(1.307)	70	103494			0.00- 30.00	10.54	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== ===== ===== ===== ===== ===== =====

\$ 104 Toluene-d8 (continued)

12.115 12.115 (1.307) 100 647501 0.00- 30.00 65.93

\$ 140 Bromofluorobenzene

CAS #: 460-00-4

16.207 16.207 (1.112) 174 529130 25.4276 25.428 80.00- 120.00 100.00

16.207 16.207 (1.112) 95 669570 91.37- 151.37 126.54

16.207 16.207 (1.112) 176 504977 68.43- 128.43 95.44

Report Date: 22-Jun-2007 14:01

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-JUN-2007

Lab File ID: 8062206.d

Calibration Time: 10:27

Lab Smp Id: Lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: jdg

Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m

Misc Info: Humid

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	307449	184469	430429	259754	-15.51
88 1,4-Difluorobenze	1381560	828936	1934184	1173930	-15.03
125 Chlorobenzene-d5	1041151	624691	1457611	874596	-16.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.41	7.08	7.74	7.39	-0.37
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-22jun
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
Level: LOW Operator: jdg
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: AT04+NA-2.spk Quant Type: ISTD
Sublist File: AT04+ENSR.sub
Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m
Misc Info: Humid

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 82 1,2-Dichloroethane	25.000	25.758	103.03	70-130
\$ 104 Toluene-d8	25.000	24.165	96.66	70-130
\$ 140 Bromofluorobenzene	25.000	25.428	101.71	70-130

Data File: /chem/msd8.1/8-22jun.b/8062206.d

Date: 22-JUN-2007 13:39

Client ID: Lab Blank

Sample Info: 200mL #13673


Column phase: RTX-624

Instrument: msd8.1

Operator: jdg

Column diameter: 0.53

/chem/msd8.1/8-22jun.b/8062206.d



LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0706310

	CLIENT SAMPLE NO.	SURROGATE % RECOVERY						TOTAL OUT
		1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#	
01	AMS2-UW	102		99		101		0
02	AMS4+60N-DW	103		96		101		0
03	Lab Blank	103		97		102		0
04	CCV	99		98		104		0
05	LCS	101		99		105		0
06								0
07								0
08								0
09								0
10								0
11								0
12								0
13								0
14								0
15								0
16								0
17								0
18								0
19								0
20								0
21								0
22								0
23								0
24								0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

* Designates values outside of QC limits

LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan

INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD
 Lab File ID: 8062202.d
 Instrument ID: msd8.i

SDG No: 0706310
 Date Analyzed: 06/22/2007
 Time Analyzed: 10:27 AM

	Chlorobenzene-d5			1,4-Difluorobenzene			Bromochloromethane		
	Area	#	RT	Area	#	RT	Area	#	RT
24-HOUR STD	1041151		14.58	1381560		9.27	307449		7.41
UPPER LIMIT	1457611		14.91	1934184		09.60	430429		07.74
LOWER LIMIT	624691		14.25	828936		08.94	184469		07.08
CLIENT SAMPLE NO									
01	AMS2-UW		14.58	1141082		9.27	265126		7.39
02	AMS4+60N-DW		14.58	1088816		9.27	248843		7.39
03	Lab Blank		14.58	1173930		9.27	259754		7.39
04	CCV		14.58	1381560		9.27	307449		7.41
05	LCS		14.58	1231802		9.27	277791		7.39
06									
07									
08									
09									
10									
11									
12									
13									
14									
15									
16									
17									
18									
19									
20									
21									
22									

'Area Upper Limit=+40% of internal standard area'
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT
 RT Lower Limit=-0.33 minutes of internal standard RT

* Designates values outside of QC limits

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Calibration File Names:

- Level 1: /chem/msd8.i/8-30may.b/8053003.d
- Level 2: /chem/msd8.i/8-30may.b/8053004.d
- Level 3: /chem/msd8.i/8-07jun.b/8060704.d
- Level 4: /chem/msd8.i/8-30may.b/8053006.d
- Level 5: /chem/msd8.i/8-07jun.b/8060705.d
- Level 6: /chem/msd8.i/8-30may.b/8053008.d
- Level 7: /chem/msd8.i/8-07jun.b/8060706.d

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	___	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
1 Freon 152a	+++++	+++++	0.98763	+++++	0.78978	+++++		
	0.82069						0.86603	12.290
2 Freon 22	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
3 Propylene	+++++	+++++	1.92982	1.31817	1.20253	1.15722		
	1.15784						1.35311	24.315
4 Dichlorodifluoromethane/Fr12	+++++	4.22735	4.02658	3.34137	3.02222	2.98122		
	2.95137						3.42502	16.496
5 Freon134a	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
6 Freon 114	+++++	3.61995	3.07946	3.11187	3.01070	2.87973		
	2.86380						3.09425	8.944
7 Isobutane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
8 Chloromethane	200.000 1.41963	+++++	1.76358	1.64915	1.55747	1.49684		1.57733	8.482
9 Butane	0.37508	+++++	0.49593	0.43121	0.39247	0.36498		0.41193	12.942
10 1,3-Butadiene	1.37941	2.12647	1.72912	1.45627	1.41158	1.30372		1.56776	19.767
11 Vinyl Chloride	1.64028	2.34753	1.85221	1.78079	1.74379	1.63245		1.83284	14.500
12 Methanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
13 Bromomethane	1.20683	1.25815	1.19877	1.26616	1.22534	1.19166		1.22449	2.562
14 Vinyl Bromide	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
15 Isopentane	2.24216	+++++	2.38563	2.37944	2.25961	2.17613		2.28859	3.988
16 Chloroethane	0.87782	1.10636	1.03490	0.98458	0.94664	0.86976		0.97001	9.461
17 Dichlorofluoromethane/Fr21	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
18 Trichlorofluoromethane/Fr11	+++++	4.06616	4.21652	3.95963	3.78415	3.62588		
	3.70548						3.89297	5.829
19 Pentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
20 Freon123a	+++++	+++++	1.38653	+++++	1.32725	+++++		
	1.29778						1.33719	3.380
21 Freon123	+++++	+++++	0.86166	+++++	0.84444	+++++		
	0.82221						0.84277	2.347
22 Dimethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
23 Ethanol	+++++	+++++	0.67753	0.66346	0.60794	0.58208		
	0.57722						0.62165	7.458
24 Freon 13	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
25 Acrolein	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
26 Isobutylene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
27 Freon142b	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
28 Freon 113	+++++	2.88068	2.79775	2.60107	2.43015	2.35327		
	2.39146						2.57573	8.639
29 1,1-Dichloroethene	+++++	2.86789	2.72869	2.56996	2.43351	2.34903		
	2.39867						2.55796	8.009
30 Acetone	+++++	+++++	0.98245	0.85434	0.84281	0.79818		
	0.80581						0.85672	8.662
31 Acetaldehyde	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++							
32 Freon143a	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++							
33 Carbon Disulfide	+++++	5.58896	4.86914	4.79052	4.54598	4.41760		
	4.55167						4.79398	8.848
34 2-Propanol	+++++	+++++	3.63428	3.09423	2.96019	2.88102		
	2.91819						3.09759	10.029
35 Acetonitrile	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++							
36 Cyclopentene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++							
37 3-Chloropropene	+++++	+++++	0.72576	0.81455	0.78451	0.74233		
	0.75685						0.76480	4.602

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
48 Ethanol-high	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
49 Isopropyl ether	+++++	+++++	4.44068	+++++	4.38024	+++++		4.35768	2.209
50 Propanal	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
51 Chloroprene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
52 1-Propanol	+++++	+++++	0.33412	+++++	0.29773	+++++		0.31408	5.881
53 Bromoethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
54 1,1-Dichloroethane	+++++	2.90490	3.23579	2.99995	2.89542	2.78581		2.95068	5.266
55 Vinyl Acetate	+++++	+++++	0.40978	0.42041	0.40294	0.41753		0.41654	2.650
56 Iodomethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
57 2,3-Dimethylbutane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
58 Ethyl-tert-butyl Ether	+++++	+++++	2.61890	+++++	3.32619	+++++		
	2.78316						2.90942	12.723
59 Methyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
60 2,2-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
61 Ethyl Acetate	+++++	+++++	0.39734	+++++	0.37435	+++++		
	0.36735						0.37968	4.133
62 1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
63 Methyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
64 cis-1,2-Dichloroethene	+++++	3.03723	2.36908	2.27992	2.14250	2.06765		
	2.11545						2.33530	15.487
65 2-Butanone	+++++	1.00709	0.85028	0.78676	0.77311	0.76198		
	0.79178						0.82850	11.187
66 2,4-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
67 Tetrahydrofuran	+++++	2.62724	2.20335	2.11722	2.03416	1.93041		
	2.00841						2.15347	11.624

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000		
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	% RSD
	200.000							
	Level 7							
69 Butanal	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
70 Chloroform	4.52339 2.82903	3.38269	2.97755	2.93420	2.84544	2.73693	3.17561	19.826
71 2-Butanol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
72 1,1-Dichloropropene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
73 Cyclohexane	+++++ 2.27273	3.13955	2.37507	2.38858	2.29135	2.22343	2.44845	14.063
74 3-Methyl-1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
75 1,1,1-Trichloroethane	+++++ 2.95670	3.69058	3.04827	3.03489	2.94955	2.87166	3.09194	9.709
76 2,3-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
77 Carbon Tetrachloride	+++++ 2.87341	2.95018	2.47054	2.94416	2.84417	2.79886	2.81355	6.321
78 Isobutanol	+++++ 0.29396	+++++	0.27113	+++++	0.29573	+++++	0.28694	4.783

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
79 tert-amyl-Methyl Ether	200.000 2.39754	+++++	2.60292	+++++	2.98159	+++++		2.66068	11.136
80 2,2,4-Trimethylpentane	7.40163	7.83756	7.57621	7.24629	6.93326	6.86073		7.30928	5.139
81 Benzene	1.46711 1.09326	1.32521	1.13921	1.09388	1.07898	1.04564		1.17761	13.352
83 1,2-Dichloroethane	0.43142	0.56444	0.46007	0.44951	0.43040	0.41345		0.45822	11.897
84 Thiopene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
85 Heptane	0.10755	0.19081	0.11421	0.11021	0.10683	0.10369		0.12222	27.645
86 1-Methoxy-2-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
87 2,3,4-Trimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
89 1-Butanol	0.26464	+++++	0.22243	+++++	0.24711	+++++		0.24472	8.665
90 Methyl Methacrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000		
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	% RSD
	200.000							
	Level 7							
91 2-Pentanone	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
92 Pentanal	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
93 Ethyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
94 Trichloroethene	+++++	0.53286	0.44939	0.44327	0.42705	0.41017	0.44757	9.860
95 Methyl Cyclohexane	+++++	3.26599	3.09517	3.05667	2.96150	2.88311	3.05031	4.263
96 Dibromomethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
97 1,2-Dichloropropane	+++++	0.42737	0.43013	0.38160	0.37306	0.36109	0.39140	7.588
98 1,4-Dioxane	+++++	+++++	0.24770	0.24197	0.23695	0.23009	0.23873	2.747
99 Octane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
100 Bromodichloromethane	+++++	0.73233	0.64459	0.64531	0.63931	0.61664	0.65370	6.123

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
101 1-Nitropropane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++						+++++	+++++
102 cis-1,3-Dichloropropene	+++++	0.61851	0.52709	0.53649	0.53068	0.51575		
	0.53501						0.54392	6.854
103 4-Methyl-2-pentanone	+++++	0.28397	0.30418	0.29328	0.29702	0.29012		
	0.29696						0.29426	2.342
105 Toluene	+++++	1.25780	1.14795	1.11923	1.10994	1.09416		
	1.15787						1.14782	5.129
106 1-Methoxy-2-propyl acetate	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
107 Epichlorohydrin	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
108 trans-1,3-Dichloropropene	+++++	0.75878	0.70145	0.71553	0.72836	0.71539		
	0.72913						0.72478	2.694
109 1,3-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
110 1,1,2-Trichloroethane	+++++	0.66231	0.52902	0.51019	0.50076	0.48912		
	0.49787						0.53155	12.321
111 alpha-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	---	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
122 Dicyclopentadiene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
123 1,1,1,2-Tetrachloroethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
124 D-Limonene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
126 Chlorobenzene	+++++	1.22227	1.44203	1.24119	1.25172	1.24989	1.28368	6.323
127 Bis(2-chloroethyl) ether	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
128 Nonane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
129 Ethyl Benzene	+++++	0.80931	0.66703	0.64128	0.64323	0.65061	0.67934	9.504
130 m,p-Xylene	+++++	0.84552	0.85011	0.79451	0.81241	0.81316	0.82782	2.919
131 Undecane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
132 o-Xylene	+++++	0.91319	0.84572	0.80595	0.81315	0.80154	0.83535	4.986

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
133 2-Heptanone	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++						+++++	+++++
134 Styrene	1.11092	1.18281	1.11362	1.12817	1.19071	1.22490		
	1.30443						1.17936	5.944
135 Bromoform	+++++	0.63208	0.65434	0.73553	0.76857	0.78441		
	0.82156						0.73275	10.236
136 Cyclohexanone	+++++	+++++	0.55672	+++++	0.57050	+++++		
	0.58931						0.57218	2.859
137 Cumene	2.79880	2.40146	2.35517	2.21000	2.28171	2.31208		
	2.13898						2.35689	9.067
138 1-chloro-2-Bromopropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
139 Bromobenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
141 1,2,3-Trichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
142 Dodecane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
143 2-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
144 1,1,2,2-Tetrachloroethane	200.000 1.22319	1.33097	1.23407	1.15272	1.19774	1.19102	1.22162	4.962
145 Propylbenzene	1.94674	2.82083	2.74232	2.62546	2.75408	2.80075	2.61503	12.788
146 4-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
147 4-Ethyltoluene	1.73174	2.24895	2.26379	2.34932	2.40819	2.44980	2.24196	11.686
148 1,3,5-Trimethylbenzene	1.49096	2.38847	2.33379	2.17383	2.24009	2.30283	2.15500	15.486
149 2,6-Dimethyl-1-propanol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
150 tert-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
151 Pentachloroethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
152 sec-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
153 1,2,4-Trimethylbenzene	1.33793	2.40359	2.29481	2.25241	2.34010	2.38632	2.16919	18.952

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
164 Aniline	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
165 1,2-Dibromo-3-Chloropropane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
166 Isooctyl Alcohol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
167 1,2,4-Trichlorobenzene	+++++ 1.22253	+++++	1.48368	1.26108	1.43814	1.47814	1.37671	9.090
168 Hexachlorobutadiene	+++++ 0.73297	+++++	0.95260	0.75132	0.77092	0.74328	0.79022	11.621
169 Naphthalene	+++++ 1.31458	+++++	3.90045	3.19414	3.61060	2.49731	2.90342	35.577 <-
170 1,2,3-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
171 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
172 Isooctyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
\$ 82 1,2-Dichloroethane-d4	1.29108 1.39339	1.28164	1.33015	1.25825	1.26386	1.34062	1.30843	3.724

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 30-MAY-2007 14:12
 End Cal Date : 07-JUN-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd8.i/8-07jun.b/t14q530b.m
 Cal Date : 07-Jun-2007 14:14 jgray
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
\$ 104 Toluene-d8	0.89493	0.88890	0.87548	0.83261	0.85871	0.85180		0.86549	2.548
\$ 140 Bromofluorobenzene	0.57145	0.56913	0.58528	0.59982	0.61223	0.61820		0.59482	3.318

Calibration History

Method : /chem/msd8.i/8-07jun.b/t14q530b.m
Start Cal Date: 30-MAY-2007 14:12
End Cal Date : 07-JUN-2007 12:08

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.20000		
30-MAY-2007 14:12	AFCEElow	/chem/msd8.i/8-30may.b/8053003.d
Cal Level: 2 , Cal Amount: 0.50000		
30-MAY-2007 14:39	AT04Low+ENSR	/chem/msd8.i/8-30may.b/8053004.d
Cal Level: 3 , Cal Amount: 2.00000		
07-JUN-2007 11:09	sp16b	/chem/msd8.i/8-07jun.b/8060704.d
30-MAY-2007 15:07	AT04mdl+ENSR	/chem/msd8.i/8-30may.b/8053005.d
Cal Level: 4 , Cal Amount: 25.00000		
30-MAY-2007 15:35	AT04mdl+ENSR	/chem/msd8.i/8-30may.b/8053006.d
Cal Level: 5 , Cal Amount: 50.00000		
07-JUN-2007 11:37	sp16b	/chem/msd8.i/8-07jun.b/8060705.d
30-MAY-2007 16:03	AT04mdl+ENSR	/chem/msd8.i/8-30may.b/8053007.d
Cal Level: 6 , Cal Amount: 100.00000		
30-MAY-2007 16:31	AT04mdl+ENSR	/chem/msd8.i/8-30may.b/8053008.d
Cal Level: 7 , Cal Amount: 200.00000		
07-JUN-2007 12:08	sp16b	/chem/msd8.i/8-07jun.b/8060706.d
30-MAY-2007 17:02	AT04mdl+ENSR	/chem/msd8.i/8-30may.b/8053009.d

Continuing Calibration
Ccal Level Mode: GLOBAL LEVEL 5

+-----+-----+-----+-----+-----+		
Ccal Level: 5 , Ccal Amount: 50.000		
+-----+-----+-----+-----+-----+		
07-JUN-2007 10:01 AT04+ENSR	/chem/msd8.i/8-07jun.b/8060702.d	
+-----+-----+-----+-----+-----+		
Ccal Level: 5 , Ccal Amount: 50.000		
+-----+-----+-----+-----+-----+		
07-JUN-2007 11:37 sp16bCCV	/chem/msd8.i/8-07jun.b/8060705a.d	
+-----+-----+-----+-----+-----+		
Ccal Level: 5 , Ccal Amount: 50.000		
+-----+-----+-----+-----+-----+		
07-JUN-2007 11:37 sp16b	/chem/msd8.i/8-07jun.b/8060705.d	
+-----+-----+-----+-----+-----+		
Ccal Level: 5 , Ccal Amount: 50.000		
+-----+-----+-----+-----+-----+		
07-JUN-2007 11:37 sp16bCCV	/chem/msd8.i/8-07jun.b/8060705a.d	
+-----+-----+-----+-----+-----+		

@ Air Toxics Ltd.

MSD-8

ION ABUNDANCE CRITERIA

% REL. ABUNDANCE

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	17.60
75	30.0 - 60.0% of mass 95	44.95
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.34
173	Less than 2.0% of mass 174	(0.00) ¹
174	Greater than 50.0% of mass 95	82.17
175	5.0 - 9.0% of mass 174	(7.22) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(97.95) ¹
177	5.0 - 9.0% of mass 176	(6.12) ²

¹ - value in parenthesis is % mass 174

² - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio: ~~16.80876~~ 1646880/1680596 x 100 = 97.93

DB 5/31/07

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} \times \text{RRF}$

DB 5/31/07

Reported Result

05/31/07

Logbook #: 1478

BFB Injection Date: 5/30/07

BFB Injection Time: 1320

BFB File ID: 8053001

Tekmar Purge Flow: 16.3 ml/min

Vacuum: 8.1 x 10⁻⁶

IS/Std #: 1443-64 Exp. Date: 7/30/07

BCM 441133

1,4-DFB 1992312

CB-d5 1475337

Verified CCVIS vs ICAL mid-point (-40%D) NA

NOAH Cart #: _____

File #: _____

File ID: _____
 Compound: _____
 Initials: _____

Sample/Client Name	Can #	Pressure	Am't Loaded	DF	Loader Init.	Date Analyzed	Time Analyzed	Review Init.	Comments
BFB Tune Check	843-2981	50mg	200ul	10	DB	5-30-07	1320	DB	
System Blank	34190	-	200ul				1344		
ICAL Level 1	1187289	0.2ppbv	0.2ul				1412		
04		0.5ppbv	0.5ul				1439		
05		20ppbv	2.0ul				1567		
06		25ppbv	2.5ul				1535		
07		50ppbv	5.0ul				1603		
08		100ppbv	10.0ul				1631		
09		200ppbv	20.0ul				1702		

Signature


Deane Burton

5/31/07

Date

Revision 05/2005

Page 299



Comments: 1st Flow Meter: 05E 27601 exp 8/19/07

220 ml/min → 25 ml/min

Flow meter: AA 9506172

X	805 3010	System Blank	34190	-	200ml	10	08	5-30-07	1732	08
X				-					1803	
X				-				5-31-07	0909	
X				-					0941	

08 5/31/07

Signature Laurie Boston

Date 5/31/07

Revision 05/2005
Page 300

@ Air Toxics Ltd.

MSD-8

Logbook #: 1478

ION ABUNDANCE CRITERIA

m/z	REL. ABUNDANCE	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	16.87
75	30.0 - 60.0% of mass 95	44.35
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.50
173	Less than 2.0% of mass 174	(0.60) ¹
174	Greater than 50.0% of mass 95	82.10
175	5.0 - 9.0% of mass 174	(7.18) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(47.50) ¹
177	5.0 - 9.0% of mass 176	(6.44) ²

¹ - value in parenthesis is % mass 174
² - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio: $\frac{123.806}{126.976} \cdot 100 = 97.50\%$

NOAH Cart #: _____

File #: _____

BFB Injection Date: 1/21/07

BFB Injection Time: 0944

BFB File ID: 80e0701

Tekmar Purge Flow: 2

Vacuum: 0.61362

IS/S Std #: 1493-64 Exp. Date: 3/31/07

BCM: 437026

1,4-DFB: 1441557

CB-d5: 1439615

Verified CCV IS vs ICAL mid-point (-40% D) DL

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{sample}}}{\text{Areas}} \times \text{Conc.}_{\text{is}} \times \text{RRF}$

$= \frac{(1666776)}{(1441557)} \times (25) = 29.208$

Reported Result: 29.728

File ID: 80e0702

Compound: T61-28

Initials: DL

File #	Sample / Client Name	Cart #	Pressure	Ampl. Loaded	DF	Loader Int.	Date Analyzed	Time Analyzed	Review Int.	Comments
1	BFB Tone Check	2481	50mg	2µl	100	DL	1/21/07	0944	DL	
2	DL CAS # 1489-289	200 ppbv	50 ppbv	50µl				1001	DL	
3	DL CAS # 1489-289	200 ppbv	50 ppbv	50µl				1029	DL	
4	DL IPRC Level 3	1493-64	2 ppbv	2µl				1109	DL	splide
5	DL OS	5	50 ppbv	50µl				1137	DL	
6	DL OS	7	200 ppbv	200µl				1208	DL	
7	DL System Blank	131023	Humid	200µl	100	DL		1326	DL	
8	DL OS	DL	Lab Blank	1				1356	DL	
9	DL OS	DL	DL	DL						

Signature: AG

Date: 1/21/07

Initial Calibration Narrative

A seven-point initial calibration was analyzed on MSD-8 on May 30, 2007.

The following compounds used 0.2 as the lowest calibration concentration:
Benzene, Chloroform, Styrene and Cumene.

before

File Security Edit Display Process Spectra Help

Sample: ICAL Type: CALIB_3 Inj.Date: 30-MAY-2007 15:07

- + 67 Tetrahydrofuran
- + 70 Chloroform
- + 73 Cyclohexane
- + 75 1,1,1-Trichloroethane
- + 77 Carbon Tetrachloride
- + 81 Benzene
- + 80 2,2,4-Trimethylpentane
- + 83 1,2-Dichloroethane
- + 85 Heptane
- + 94 Trichloroethylene
- + 95 Methyl Cyclohexane
- + 97 1,2-Dichloropropane
- + 98 1,4-Dioxane
- + 100 Bromodichloromethane
- + 102 cis-1,3-Dichlorobenzene
- + 103 4-Methyl-2-pentanone**
- + 105 Toluene
- + 108 trans-1,3-Dichlorobenzene
- + 110 1,1,2-Trichloroethane
- + 112 Tetrachloroethane
- + 114 2-Hexanone
- + 116 Dibromochloromethane
- + 117 1,2-Dibromoethane
- + 126 Chlorobenzene
- + 129 Ethyl Benzene

HP MS 8053005.d, Scan 368: 12.032 min. (SUB)

Reference Spectrum for 4-Methyl-2-pentanone

Ion 58.00

Ion 43.00

Ion 85.00

Hit#	RT(min)	Response	Amount	Conc	Ratio	Flags	Report:
1	11.645	2880			234		
2	12.032	63447	2.526	2.526	100		
	12.032	123002			194		
	12.032	21458			34		
3	12.364	2625	0.1045	0.1045	100	T	

8053005.d

Jun 1 2007






... / Initial	6/11/07 DL
Poor Integration	
Split Peak	✓
Peak Tailing	
Background Subtraction	
Zoom In	
Missed Peak	

after
re 6/11/07

File Security Edit Display Process Spectra Help

Sample: ICAL Type: CALIB_3 Inj.Date: 30-MAY-2007 15:07

- + 67 Tetrahydrofuran
- + 70 Chloroform
- + 73 Cyclohexane
- + 75 1,1,1-Trichloroethane
- + 77 Carbon Tetrachloride
- + 81 Benzene
- + 80 2,2,4-Trimethylpentane
- + 83 1,2-Dichloroethane
- + 85 Heptane
- + 94 Trichloroethylene
- + 95 Methyl Cyclohexane
- + 97 1,2-Dichloropropane
- + 98 1,4-Dioxane
- + 100 Bromodichloromethane
- + 102 cis-1,3-Dichloropropane
- + 103 4-Methyl-2-pentanone
- + 105 Toluene
- + 108 trans-1,3-Dichloropropane
- + 110 1,1,2-Trichloroethane
- + 112 Tetrachloroethane
- + 114 2-Hexanone
- + 116 Dibromochloromethane
- + 117 1,2-Dibromoethane
- + 126 Chlorobenzene
- + 129 Ethyl Benzene



8053005.d

Hit#	RT(min)	Response	Amount	Conc	Ratio	Flags	Report:
1	12.032	49522	2.067	2.067	100	M	
	12.032	123001			248		
	12.032	21457			43		

- Mark 4-Methyl-2-pentanone Undetected.



Air Toxics Ltd.
 Modified EPA Methods TO-14A/TO-15
 Internal Standard and Associated Target Compounds and Surrogates

Bromochloromethane
Target Compounds:
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
3-Chloropropene
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
2,2,4-Trimethylpentane
Surrogates:
1,2-Dichloroethane-d4

1,4-Difluorobenzene
Target Compounds:
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
Surrogates:
Toluene-d8

Chlorobenzene-d5
Target Compounds:
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
Surrogates:
Bromofluorobenzene

Report Date: 01-Jun-2007 10:48

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-31may.b/8053103.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 31-MAY-2007 11:48
 Operator : JG Inst ID: msd8.i
 Smp Info : 50ml #1487-275
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /chem/msd8.i/8-31may.b/t14q530a.m
 Meth Date : 01-Jun-2007 10:48 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 17:02 Cal File: 8053009.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
		ON-COL		FINAL		TARGET RANGE		RATIO
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====

* 68	Bromochloromethane				CAS #: 74-97-5			
7.387	7.415 (1.000)	130	440756	25.0000		80.00- 120.00	100.00	
7.387	7.415 (1.000)	128	346888			48.60- 108.60	78.70	
7.387	7.387 (1.000)	49	625716			114.98- 174.98	141.96	

* 88	1,4-Difluorobenzene				CAS #: 540-36-3			
9.267	9.267 (1.000)	114	2010798	25.0000		80.00- 120.00	100.00	
9.267	9.267 (1.000)	88	311662			0.00- 45.16	15.50	

* 125	Chlorobenzene-d5				CAS #: 3114-55-4			
14.576	14.576 (1.000)	117	1506758	25.0000		80.00- 120.00	100.00	
14.576	14.576 (1.000)	82	856520			0.00- 30.00	56.85	

\$ 82	1,2-Dichloroethane-d4				CAS #: 17060-07-0			
8.465	8.465 (1.146)	65	572200	24.8051	24.805	80.00- 120.00	100.00	
8.465	8.465 (1.146)	67	351230			0.00- 30.00	61.38	

\$ 104	Toluene-d8				CAS #: 2037-26-5			
12.115	12.115 (1.307)	98	1737699	24.9622	24.962	80.00- 120.00	100.00	
12.115	12.115 (1.307)	70	186801			0.00- 30.00	10.75	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT (REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

\$ 104 Toluene-d8 (continued)

12.115	12.115 (1.307)	100	1549990			0.00- 30.00	89.20
--------	----------------	-----	---------	--	--	-------------	-------

\$ 140 Bromofluorobenzene

CAS #: 460-00-4

16.207	16.207 (1.112)	174	897285	25.0287	25.029	80.00- 120.00	100.00
16.207	16.207 (1.112)	95	1158459			105.65- 165.65	129.11
16.207	16.207 (1.112)	176	894688			66.34- 126.34	99.71

4 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.050	2.078 (0.278)	85	2778941	46.0212	46.021	80.00- 120.00	100.00
2.050	2.078 (0.278)	87	891336			0.00- 30.00	32.07

6 Freon 114

CAS #: 76-14-2

2.161	2.189 (0.293)	135	2562967	46.9817	46.982	80.00- 120.00	100.00
2.161	2.189 (0.293)	137	809100			0.71- 60.71	31.57

8 Chloromethane

CAS #: 74-87-3

2.272	2.299 (0.308)	50	1366974	49.1562	49.156	80.00- 120.00	100.00
2.272	2.299 (0.308)	52	419326			0.00- 30.00	30.68

11 Vinyl Chloride

CAS #: 75-01-4

2.410	2.438 (0.326)	62	1506942	46.6352	46.635	80.00- 120.00	100.00
2.410	2.438 (0.326)	64	471709			0.00- 30.00	31.30

10 1,3-Butadiene

CAS #: 106-99-0

2.382	2.410 (0.322)	54	1138555	41.1922	41.192	80.00- 120.00	100.00
2.382	2.410 (0.322)	39	1152974			0.00- 30.00	101.27

13 Bromomethane

CAS #: 74-83-9

2.852	2.880 (0.386)	94	1047024	48.5003	48.500	80.00- 120.00	100.00
2.852	2.880 (0.386)	96	1003279			63.65- 123.65	95.82

16 Chloroethane

CAS #: 75-00-3

2.963	2.991 (0.401)	64	798701	46.7036	46.704	80.00- 120.00	100.00
2.935	2.963 (0.397)	49	208062			0.00- 30.00	26.05
2.963	2.991 (0.401)	66	241751			0.00- 30.00	30.27

18 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.212	3.239 (0.435)	101	3306964	48.1826	48.183	80.00- 120.00	100.00
3.212	3.239 (0.435)	103	2152698			34.50- 94.50	65.10

23 Ethanol

CAS #: 64-17-5

3.516	3.544 (0.476)	45	588478	53.6942	53.694	80.00- 120.00	100.00
3.516	3.544 (0.476)	43	117595			0.00- 30.00	19.98
3.516	3.544 (0.476)	46	241557			0.00- 30.00	41.05

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

28 Freon 113 CAS #: 76-13-1
 3.931 3.958 (0.532) 151 2312964 50.9343 50.934 80.00- 120.00 100.00
 3.931 3.958 (0.532) 153 1528932 34.32- 94.32 66.10
 3.931 3.958 (0.532) 101 2826353 85.50- 145.50 122.20

29 1,1-Dichloroethene CAS #: 75-35-4
 3.958 3.986 (0.536) 61 2385056 52.8867 52.887 80.00- 120.00 100.00
 3.958 3.986 (0.536) 96 1431121 29.81- 89.81 60.00
 3.958 3.986 (0.536) 98 913818 9.00- 69.00 38.31

30 Acetone CAS #: 67-64-1
 4.124 4.124 (0.558) 58 750144 49.6648 49.665 80.00- 120.00 100.00
 4.124 4.124 (0.558) 43 2233113 0.00- 30.00 297.69

34 2-Propanol CAS #: 67-63-0
 4.318 4.318 (0.584) 45 2687206 49.2062 49.206 80.00- 120.00 100.00
 4.318 4.318 (0.584) 43 509221 0.00- 30.00 18.95
 4.318 4.318 (0.584) 59 100187 0.00- 30.00 3.73

33 Carbon Disulfide CAS #: 75-15-0
 4.290 4.290 (0.581) 76 4015505 47.5101 47.510 80.00- 120.00 100.00

37 3-Chloropropene CAS #: 107-05-1
 4.566 4.594 (0.618) 76 692936 51.3911 51.391 80.00- 120.00 100.00
 4.566 4.594 (0.618) 41 2090707 0.00- 30.00 301.72

40 Methylene Chloride CAS #: 75-09-2
 4.815 4.815 (0.652) 49 1736664 51.4364 51.436 80.00- 120.00 100.00
 4.815 4.843 (0.652) 84 1236611 40.47- 100.47 71.21
 4.815 4.815 (0.652) 51 518270 0.00- 30.00 29.84

43 MTBE CAS #: 1634-04-4
 5.147 5.175 (0.697) 73 2334781 48.6230 48.623 80.00- 120.00 100.00
 5.147 5.175 (0.697) 57 526586 0.00- 52.63 22.55
 5.147 5.175 (0.697) 41 546280 0.00- 30.00 23.40

45 trans-1,2-Dichloroethene CAS #: 156-60-5
 5.175 5.203 (0.701) 96 1480166 46.3832 46.383 80.00- 120.00 100.00
 5.175 5.203 (0.701) 61 2223377 119.47- 179.47 150.21
 5.175 5.203 (0.701) 98 951148 0.00- 30.00 64.26

46 Hexane CAS #: 110-54-3
 5.534 5.534 (0.749) 57 2449048 50.6003 50.600 80.00- 120.00 100.00
 5.534 5.534 (0.749) 43 1575746 0.00- 30.00 64.34
 5.534 5.534 (0.749) 86 364966 0.00- 30.00 14.90

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

54 1,1-Dichloroethane CAS #: 75-34-3
 5.949 5.949 (0.805) 63 2639497 50.7389 50.739 80.00- 120.00 100.00
 5.949 5.949 (0.805) 65 834971 1.86- 61.86 31.63

65 2-Butanone CAS #: 78-93-3
 7.027 7.027 (0.951) 72 692091 47.3821 47.382 80.00- 120.00 100.00
 7.027 7.027 (0.951) 43 2937806 409.65- 469.65 424.48
 7.027 7.027 (0.951) 57 229143 0.00- 30.00 33.11

64 cis-1,2-Dichloroethene CAS #: 156-59-2
 6.972 6.972 (0.944) 61 1927506 46.8160 46.816 80.00- 120.00 100.00
 6.972 6.972 (0.944) 96 1448922 43.20- 103.20 75.17
 6.972 6.972 (0.944) 98 903977 17.85- 77.85 46.90

67 Tetrahydrofuran CAS #: 109-99-9
 7.387 7.415 (1.000) 42 1762470 46.4222 46.422 80.00- 120.00 100.00
 7.387 7.415 (1.000) 71 616972 5.48- 65.48 35.01
 7.387 7.415 (1.000) 72 683813 0.00- 30.00 38.80

70 Chloroform CAS #: 67-66-3
 7.525 7.553 (1.019) 83 2568490 45.8768 45.877 80.00- 120.00 100.00
 7.525 7.553 (1.019) 85 1587019 32.67- 92.67 61.79

75 1,1,1-Trichloroethane CAS #: 71-55-6
 7.774 7.774 (1.052) 97 2636611 48.3678 48.368 80.00- 120.00 100.00
 7.774 7.774 (1.052) 99 1692005 34.55- 94.55 64.17

73 Cyclohexane CAS #: 110-82-7
 7.746 7.746 (1.049) 84 2011710 46.6032 46.603 80.00- 120.00 100.00
 7.746 7.746 (1.049) 56 2573375 96.25- 156.25 127.92
 7.746 7.746 (1.049) 41 1297745 32.28- 92.28 64.51

77 Carbon Tetrachloride CAS #: 56-23-5
 7.995 8.023 (1.082) 119 2542777 51.2619 51.262 80.00- 120.00 100.00
 7.995 8.023 (1.082) 117 2618298 73.30- 133.30 102.97

80 2,2,4-Trimethylpentane CAS #: 540-84-1
 8.465 8.465 (1.146) 57 6011320 46.6484 46.648 80.00- 120.00 100.00
 8.465 8.465 (1.146) 56 1918609 0.00- 30.00 31.92
 8.465 8.465 (1.146) 41 1389836 0.00- 30.00 23.12

81 Benzene CAS #: 71-43-2
 8.437 8.438 (0.910) 78 4287698 45.2681 45.268 80.00- 120.00 100.00
 8.437 8.438 (0.910) 77 959130 0.00- 30.00 22.37

83 1,2-Dichloroethane CAS #: 107-06-2
 8.603 8.603 (0.928) 62 1763231 47.8421 47.842 80.00- 120.00 100.00

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
83 1,2-Dichloroethane (continued)									
8.603	8.603	(0.928)	64	570080			0.00- 30.00	32.33	

85 Heptane CAS #: 142-82-5									
8.852	8.852	(0.955)	100	422399	42.9697	42.970	80.00- 120.00	100.00	
8.852	8.852	(0.955)	43	2420809			0.00- 30.00	573.11	
8.852	8.852	(0.955)	71	1375374			0.00- 30.00	325.61	

94 Trichloroethene CAS #: 79-01-6									
9.682	9.682	(1.045)	95	1722090	47.8377	47.838	80.00- 120.00	100.00	
9.682	9.682	(1.045)	130	1803299			78.57- 138.57	104.72	
9.682	9.682	(1.045)	97	1080675			34.08- 94.08	62.75	

97 1,2-Dichloropropane CAS #: 78-87-5									
10.179	10.179	(1.098)	63	1484383	47.1518	47.152	80.00- 120.00	100.00	
10.179	10.179	(1.098)	62	1055399			42.26- 102.26	71.10	
10.179	10.179	(1.098)	41	846166			26.77- 86.77	57.00	

98 1,4-Dioxane CAS #: 123-91-1									
10.428	10.428	(1.125)	88	953301	49.6479	49.648	80.00- 120.00	100.00	
10.428	10.428	(1.125)	58	672923			41.45- 101.45	70.59	
10.428	10.428	(1.125)	57	202353			0.00- 30.00	21.23	

100 Bromodichloromethane CAS #: 75-27-4									
10.732	10.732	(1.158)	83	2523493	47.9946	47.995	80.00- 120.00	100.00	
10.732	10.732	(1.158)	85	1562917			31.75- 91.75	61.93	

102 cis-1,3-Dichloropropene CAS #: 10061-01-5									
11.672	11.673	(1.260)	75	2069212	47.2977	47.298	80.00- 120.00	100.00	
11.672	11.673	(1.260)	77	655311			1.36- 61.36	31.67	
11.672	11.673	(1.260)	39	1004071			17.70- 77.70	48.52	

103 4-Methyl-2-pentanone CAS #: 108-10-1									
12.032	12.032	(1.298)	58	1179076	49.8183	49.818	80.00- 120.00	100.00	
12.032	12.032	(1.298)	43	2851980			0.00- 30.00	241.88	
12.032	12.032	(1.298)	85	496153			0.00- 30.00	42.08	

105 Toluene CAS #: 108-88-3									
12.253	12.253	(1.322)	91	4606596	49.8972	49.897	80.00- 120.00	100.00	
12.253	12.253	(1.322)	92	2757068			29.69- 89.69	59.85	

108 trans-1,3-Dichloropropene CAS #: 10061-02-6									
12.834	12.861	(0.880)	75	2120788	48.5501	48.550	80.00- 120.00	100.00	
12.834	12.861	(0.880)	77	642673			0.08- 60.08	30.30	
12.834	12.834	(0.880)	39	956206			15.97- 75.97	45.09	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	ON-COL		FINAL	TARGET RANGE	RATIO		
				RESPONSE	(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	

110	1,1,2-Trichloroethane					CAS #:	79-00-5			
13.138	13.138	(0.901)	97	1450072	45.2633	45.263	80.00-	120.00	100.00	
13.138	13.138	(0.901)	99	903189			29.85-	89.85	62.29	
13.138	13.138	(0.901)	83	1268499			54.93-	114.93	87.48	

112	Tetrachloroethene					CAS #:	127-18-4			
13.193	13.193	(0.905)	166	2052640	47.3396	47.340	80.00-	120.00	100.00	
13.193	13.193	(0.905)	129	1598570			45.08-	105.08	77.88	
13.193	13.193	(0.905)	131	1573037			44.22-	104.22	76.63	

114	2-Hexanone					CAS #:	591-78-6			
13.580	13.580	(0.932)	58	1578878	49.7385	49.738	80.00-	120.00	100.00	
13.580	13.580	(0.932)	43	2839029			148.62-	208.62	179.81	
13.580	13.580	(0.932)	100	328947			0.00-	30.00	20.83	

116	Dibromochloromethane					CAS #:	124-48-1			
13.718	13.719	(0.941)	129	2441815	48.6342	48.634	80.00-	120.00	100.00	
13.718	13.719	(0.941)	127	1862028			0.00-	30.00	76.26	

117	1,2-Dibromoethane					CAS #:	106-93-4			
13.884	13.884	(0.953)	107	2264782	46.3953	46.395	80.00-	120.00	100.00	
13.884	13.884	(0.953)	109	2141958			63.81-	123.81	94.58	

126	Chlorobenzene					CAS #:	108-90-7			
14.603	14.631	(1.002)	112	3600449	46.5367	46.537	80.00-	120.00	100.00	
14.603	14.631	(1.002)	114	1156467			1.84-	61.84	32.12	
14.603	14.603	(1.002)	77	2040419			26.78-	86.78	56.67	

129	Ethyl Benzene					CAS #:	100-41-4			
14.769	14.769	(1.013)	106	1875253	45.8007	45.801	80.00-	120.00	100.00	
14.769	14.769	(1.013)	91	5813094			0.00-	30.00	309.99	

130	m,p-Xylene					CAS #:	108-38-3			
14.935	14.935	(1.025)	106	2373682	47.5756	47.576	80.00-	120.00	100.00	
14.935	14.935	(1.025)	91	4516302			0.00-	30.00	190.27	

132	o-Xylene					CAS #:	95-47-6			
15.488	15.488	(1.063)	106	2318082	46.0425	46.042	80.00-	120.00	100.00	
15.488	15.488	(1.063)	91	4803654			178.74-	238.74	207.23	

134	Styrene					CAS #:	100-42-5			
15.516	15.516	(1.064)	104	3405235	47.9066	47.907	80.00-	120.00	100.00	
15.516	15.516	(1.064)	78	1716218			20.27-	80.27	50.40	

135	Bromoform					CAS #:	75-25-2			
15.764	15.765	(1.082)	173	2241846	50.7630	50.763	80.00-	120.00	100.00	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
135 Bromoform (continued)									
15.764	15.765	(1.082)	171	1157469			20.67-	80.67	51.63

144 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.456	16.456	(1.129)	83	3338269	45.3401	45.340	80.00-	120.00	100.00
16.456	16.456	(1.129)	85	2060617			31.59-	91.59	61.73

147 4-Ethyltoluene CAS #: 622-96-8									
16.649	16.649	(1.142)	105	6752548	49.9730	49.973	80.00-	120.00	100.00
16.649	16.649	(1.142)	120	2056264			0.00-	59.85	30.45

148 1,3,5-Trimethylbenzene CAS #: 108-67-8									
16.732	16.732	(1.148)	105	6260050	48.1979	48.198	80.00-	120.00	100.00
16.732	16.732	(1.148)	120	3095852			0.00-	30.00	49.45

153 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.147	17.147	(1.176)	105	6608084	50.5445	50.544	80.00-	120.00	100.00
17.147	17.147	(1.176)	120	2956336			15.22-	75.22	44.74

156 1,3-Dichlorobenzene CAS #: 541-73-1									
17.451	17.451	(1.197)	146	4297022	50.4188	50.419	80.00-	120.00	100.00
17.451	17.451	(1.197)	148	2703733			0.00-	30.00	62.92
17.451	17.451	(1.197)	111	1752089			0.00-	30.00	40.77

157 1,4-Dichlorobenzene CAS #: 106-46-7									
17.562	17.562	(1.205)	146	3673574	45.4817	45.482	80.00-	120.00	100.00
17.562	17.562	(1.205)	148	2397507			0.00-	30.00	65.26
17.562	17.562	(1.205)	111	1301488			0.00-	30.00	35.43

158 alpha-Chlorotoluene CAS #: 100-44-7									
17.700	17.700	(1.214)	91	6425001	54.7247	54.725	80.00-	120.00	100.00
17.700	17.700	(1.214)	126	1322597			0.00-	30.00	20.59

161 1,2-Dichlorobenzene CAS #: 95-50-1									
17.921	17.921	(1.230)	146	3730128	45.4352	45.435	80.00-	120.00	100.00
17.921	17.921	(1.230)	148	2410442			33.37-	93.37	64.62
17.921	17.921	(1.230)	111	1412557			7.65-	67.65	37.87

167 1,2,4-Trichlorobenzene CAS #: 120-82-1									
19.276	19.276	(1.322)	180	3988477	48.0685	48.068	80.00-	120.00	100.00
19.276	19.276	(1.322)	182	3802153			64.68-	124.68	95.33

168 Hexachlorobutadiene CAS #: 87-68-3									
19.359	19.359	(1.328)	225	2159382	45.3397	45.340	80.00-	120.00	100.00
19.359	19.359	(1.328)	223	1379410			33.22-	93.22	63.88

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
145 Propylbenzene						CAS #: 103-65-1			
16.483	16.484	(1.131)	91	8066062	51.1778	51.178	80.00- 120.00	100.00	
16.483	16.484	(1.131)	120	1852431			0.00- 30.00	22.97	
16.483	16.484	(1.131)	105	285850			0.00- 30.00	3.54	

137 Cumene						CAS #: 98-82-8			
15.958	15.958	(1.095)	105	6813817	47.9676	47.968	80.00- 120.00	100.00	
15.958	15.986	(1.095)	120	1785636			0.00- 30.00	26.21	
15.958	15.958	(1.095)	51	636171			0.00- 30.00	9.34	

169 Naphthalene						CAS #: 91-20-3			
19.470	19.470	(1.336)	128	9185790	52.4933	52.493	80.00- 120.00	100.00	
19.470	19.470	(1.336)	127	1071085			0.00- 30.00	11.66	

9 Butane						CAS #: 106-97-8			
2.327	2.355	(0.315)	58	350243	48.2264	48.226	70.00- 130.00	100.00	
2.327	2.355	(0.315)	43	2575697			0.00- 30.00	735.40	

15 Isopentane						CAS #: 78-78-4			
2.963	2.963	(0.401)	43	1966389	48.7352	48.735	70.00- 130.00	100.00	
2.963	2.963	(0.401)	57	1333134			0.00- 30.00	67.80	
2.963	2.963	(0.401)	72	143213			0.00- 30.00	7.28	

95 Methyl Cyclohexane						CAS #: 108-87-2			
9.903	9.903	(1.341)	83	2603625	48.4146	48.414	70.00- 130.00	100.00	
9.903	9.903	(1.341)	98	1166714			0.00- 30.00	44.81	
9.903	9.903	(1.341)	55	2051809			0.00- 30.00	78.81	

Report Date: 01-Jun-2007 10:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 31-MAY-2007

Lab File ID: 8053103.d

Calibration Time: 11:20

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd8.i/8-31may.b/t14q530a.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	510079	306047	714111	440756	-13.59
88 1,4-Difluorobenze	2335966	1401580	3270352	2010798	-13.92
125 Chlorobenzene-d5	1717992	1030795	2405189	1506758	-12.30

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.41	7.08	7.74	7.39	-0.37
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-31may
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: JG
 Data Type: MS DATA SampleType: LCS
 SpikeList File: Spectra.spk Quant Type: ISTD
 Sublist File: AT04+ENSR.sub
 Method File: /chem/msd8.i/8-31may.b/t14q530a.m
 Misc Info: 200ppbv-50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
134 Styrene	50.000	47.907	95.81	70-130
108 trans-1,3-Dichloro	50.000	48.550	97.10	70-130
4 Dichlorodifluorome	50.000	46.021	92.04	70-130
6 Freon 114	50.000	46.982	93.96	70-130
8 Chloromethane	50.000	49.156	98.31	70-130
11 Vinyl Chloride	50.000	46.635	93.27	70-130
10 1,3-Butadiene	50.000	41.192	82.38	60-140
13 Bromomethane	50.000	48.500	97.00	70-130
16 Chloroethane	50.000	46.704	93.41	70-130
18 Trichlorofluoromet	50.000	48.183	96.37	70-130
23 Ethanol	50.000	53.694	107.39	60-140
28 Freon 113	50.000	50.934	101.87	70-130
29 1,1-Dichloroethene	50.000	52.887	105.77	70-130
30 Acetone	50.000	49.665	99.33	60-140
33 Carbon Disulfide	50.000	47.510	95.02	60-140
34 2-Propanol	50.000	49.206	98.41	60-140
40 Methylene Chloride	50.000	51.436	102.87	70-130
43 MTBE	50.000	48.623	97.25	60-140
45 trans-1,2-Dichloro	50.000	46.383	92.77	60-140
46 Hexane	50.000	50.600	101.20	60-140
54 1,1-Dichloroethane	50.000	50.739	101.48	70-130
64 cis-1,2-Dichloroet	50.000	46.816	93.63	70-130
65 2-Butanone	50.000	47.382	94.76	60-140
67 Tetrahydrofuran	50.000	46.422	92.84	60-140
70 Chloroform	50.000	45.877	91.75	70-130
73 Cyclohexane	50.000	46.603	93.21	60-140
75 1,1,1-Trichloroeth	50.000	48.368	96.74	70-130
77 Carbon Tetrachlori	50.000	51.262	102.52	70-130
81 Benzene	50.000	45.268	90.54	70-130
83 1,2-Dichloroethane	50.000	47.842	95.68	70-130
85 Heptane	50.000	42.970	85.94	60-140
94 Trichloroethene	50.000	47.838	95.68	70-130
97 1,2-Dichloropropan	50.000	47.152	94.30	70-130

Report Date: 01-Jun-2007 10:48

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
98 1,4-Dioxane	50.000	49.648	99.30	60-140
100 Bromodichlorometha	50.000	47.995	95.99	60-140
102 cis-1,3-Dichloropr	50.000	47.298	94.60	70-130
103 4-Methyl-2-pentano	50.000	49.818	99.64	60-140
105 Toluene	50.000	49.897	99.79	70-130
110 1,1,2-Trichloroeth	50.000	45.263	90.53	70-130
112 Tetrachloroethene	50.000	47.340	94.68	70-130
114 2-Hexanone	50.000	49.738	99.48	60-140
116 Dibromochlorometha	50.000	48.634	97.27	60-140
117 1,2-Dibromoethane	50.000	46.395	92.79	70-130
126 Chlorobenzene	50.000	46.537	93.07	70-130
129 Ethyl Benzene	50.000	45.801	91.60	70-130
130 m,p-Xylene	50.000	47.576	95.15	70-130
132 o-Xylene	50.000	46.042	92.08	70-130
135 Bromoform	50.000	50.763	101.53	60-140
144 1,1,2,2-Tetrachlor	50.000	45.340	90.68	70-130
147 4-Ethyltoluene	50.000	49.973	99.95	60-140
148 1,3,5-Trimethylben	50.000	48.198	96.40	70-130
153 1,2,4-Trimethylben	50.000	50.544	101.09	70-130
156 1,3-Dichlorobenzen	50.000	50.419	100.84	70-130
157 1,4-Dichlorobenzen	50.000	45.482	90.96	70-130
158 alpha-Chlorotoluen	50.000	54.725	109.45	70-130
161 1,2-Dichlorobenzen	50.000	45.435	90.87	70-130
167 1,2,4-Trichloroben	50.000	48.068	96.14	70-130
168 Hexachlorobutadien	50.000	45.340	90.68	70-130
137 Cumene	50.000	47.968	95.94	60-140
145 Propylbenzene	50.000	51.178	102.36	60-140
37 3-Chloropropene	50.000	51.391	102.78	60-140
80 2,2,4-Trimethylpen	50.000	46.648	93.30	60-140
169 Naphthalene	50.000	52.493	104.99	60-140
9 Butane	50.000	48.226	96.45	70-130
15 Isopentane	50.000	48.735	97.47	70-130
95 Methyl Cyclohexane	50.000	48.414	96.83	70-130


SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 82 1,2-Dichloroethane	25.000	24.805	99.22	70-130
\$ 104 Toluene-d8	25.000	24.962	99.85	70-130
\$ 140 Bromofluorobenzene	25.000	25.029	100.11	70-130

Data File: /chem/msd8.1/8-31may.b/8053103.d
Date: 31-May-2007 11:48
Client ID: LCS-1
Sample Info: 50ml #1487-275

Column phase: RTX-624

Instrument: msd8.1
Operator: JG
Column diameter: 0.53

/chem/msd8.1/8-31may.b/8053103.d



Report Date: 31-May-2007 14:52

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053003.d
 Lab Smp Id: ICAL Client Smp ID: Level 1
 Inj Date : 30-MAY-2007 14:12
 Operator : db Inst ID: msd8.i
 Smp Info : 0.2ml #1487-289
 Misc Info : 200ppbv-0.2ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 31-May-2007 14:52 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 14:12 Cal File: 8053003.d
 Als bottle: 1 Calibration Sample, Level: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AFCEElow.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.387	(1.000)	130	449663	25.0000			70.00- 130.00	100.00
7.387	7.387	(1.000)	128	347373				47.57- 107.57	77.25
7.387	7.387	(1.000)	49	653261				113.47- 173.47	145.28

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	2011611	25.0000			70.00- 130.00	100.00
9.267	9.267	(1.000)	88	307684				0.00- 45.68	15.30

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	1511139	25.0000			70.00- 130.00	100.00
14.576	14.576	(1.000)	82	870029				0.00- 30.00	57.57

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.146)	65	580550	25.0000	24.668		70.00- 130.00	100.00
8.465	8.465	(1.146)	67	304406				0.00- 30.00	52.43

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	1800242	25.0000	25.850		70.00- 130.00	100.00
12.115	12.115	(1.307)	70	162095				0.00- 30.00	9.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 104 Toluene-d8 (continued)									
12.115	12.115	(1.307)	100	1155287			0.00- 30.00	64.17	

\$ 140 Bromofluorobenzene									
						CAS #: 460-00-4			
16.207	16.207	(1.112)	174	863540	25.0000	24.018	70.00- 130.00	100.00	
16.207	16.207	(1.112)	95	1149176			102.16- 162.16	133.08	
16.207	16.207	(1.112)	176	834188			64.31- 124.31	96.60	

70 Chloroform									
						CAS #: 67-66-3			
7.525	7.525	(1.019)	83	16272	0.20000	0.3066	70.00- 130.00	100.00(a)	
7.525	7.525	(1.019)	85	9678			31.98- 91.98	59.48	

81 Benzene									
						CAS #: 71-43-2			
8.437	8.437	(0.910)	78	23610	0.20000	0.2598	70.00- 130.00	100.00(a)	
8.437	8.437	(0.910)	77	8272			0.00- 30.00	35.04	

134 Styrene									
						CAS #: 100-42-5			
15.516	15.516	(1.064)	104	13430	0.20000	0.1866	70.00- 130.00	100.00(a)	
15.516	15.516	(1.064)	78	8927			20.25- 80.25	66.47	

137 Cumene									
						CAS #: 98-82-8			
15.958	15.958	(1.095)	105	33835	0.20000	0.2452	70.00- 130.00	100.00(a)	
15.958	15.958	(1.095)	120	10282			0.00- 30.00	30.39	
15.958	15.958	(1.095)	51	4623			0.00- 30.00	13.66	

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 31-May-2007 14:52

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053003.d

Calibration Time: 16:03

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-0.2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	441133	264680	617586	449663	1.93
88 1,4-Difluorobenze	1992312	1195387	2789237	2011611	0.97
125 Chlorobenzene-d5	1475337	885202	2065472	1511139	2.43

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-30may.b/8053003.d

Date: 30-May-2007 14:12

Client ID: Level 1

Sample Info: 0.2ml #1487-289


Column phase: RTX-624

Instrument: msd8.1

Operator: db

Column diameter: 0.53

/chem/msd8.1/8-30may.b/8053003.d



Report Date: 01-Jun-2007 13:36

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053004.d
 Lab Smp Id: ICAL Client Smp ID: Level 2
 Inj Date : 30-MAY-2007 14:39
 Operator : db Inst ID: msd8.i
 Smp Info : 0.5ml #1487-289
 Misc Info : 200ppbv-0.5ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 01-Jun-2007 10:56 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 14:39 Cal File: 8053004.d
 Als bottle: 1 Calibration Sample, Level: 2
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04Low+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5								
7.387	7.415	(1.000)	130	441719	25.0000		80.00- 120.00	100.00
7.387	7.415	(1.000)	128	338788			48.60- 108.60	76.70
7.387	7.415	(1.000)	49	651629			114.98- 174.98	147.52

* 88 1,4-Difluorobenzene CAS #: 540-36-3								
9.267	9.267	(1.000)	114	1974518	25.0000		80.00- 120.00	100.00
9.267	9.267	(1.000)	88	311817			0.00- 45.16	15.79

* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.576	14.576	(1.000)	117	1505104	25.0000		80.00- 120.00	100.00
14.576	14.576	(1.000)	82	859236			0.00- 30.00	57.09

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
8.465	8.465	(1.146)	65	566125	25.0000	24.488	80.00- 120.00	100.00
8.465	8.465	(1.146)	67	303961			0.00- 30.00	53.69

\$ 104 Toluene-d8 CAS #: 2037-26-5								
12.115	12.115	(1.307)	98	1755155	25.0000	25.676	80.00- 120.00	100.00
12.115	12.115	(1.307)	70	183881			0.00- 30.00	10.48

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 104 Toluene-d8 (continued)									
12.115	12.115	(1.307)	100	1118700			0.00- 30.00	63.74	

\$ 140 Bromofluorobenzene CAS #: 460-00-4									
16.207	16.207	(1.112)	174	856607	25.0000	23.920	80.00- 120.00	100.00	
16.207	16.207	(1.112)	95	1122836			105.65- 165.65	131.08	
16.207	16.207	(1.112)	176	830280			66.34- 126.34	96.93	

4 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.050	2.078	(0.278)	85	37346	0.50000	0.6171	80.00- 120.00	100.00	
2.050	2.078	(0.278)	87	12534			0.00- 30.00	33.56	

6 Freon 114 CAS #: 76-14-2									
2.216	2.189	(0.300)	135	31980	0.50000	0.5849	80.00- 120.00	100.00(H)	
2.216	2.189	(0.300)	137	10844			0.71- 60.71	33.91	

11 Vinyl Chloride CAS #: 75-01-4									
2.438	2.438	(0.330)	62	20739	0.50000	0.6404	80.00- 120.00	100.00	
2.438	2.438	(0.330)	64	16204			0.00- 30.00	78.13	

10 1,3-Butadiene CAS #: 106-99-0									
2.438	2.410	(0.330)	54	18786	0.50000	0.6782	80.00- 120.00	100.00	
2.410	2.410	(0.326)	39	32703			0.00- 30.00	174.08	

13 Bromomethane CAS #: 74-83-9									
2.852	2.880	(0.386)	94	11115	0.50000	0.5137	80.00- 120.00	100.00	
2.852	2.880	(0.386)	96	7716			63.65- 123.65	69.42	

16 Chloroethane CAS #: 75-00-3									
2.991	2.991	(0.405)	64	9774	0.50000	0.5703	80.00- 120.00	100.00	
2.991	2.991	(0.405)	49	2239			0.00- 30.00	22.91	
2.963	2.991	(0.401)	66	2848			0.00- 30.00	29.14	

18 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
3.239	3.239	(0.439)	101	35922	0.50000	0.5222	80.00- 120.00	100.00	
3.239	3.239	(0.439)	103	24332			34.50- 94.50	67.74	

28 Freon 113 CAS #: 76-13-1									
3.931	3.958	(0.532)	151	25449	0.50000	0.5592	80.00- 120.00	100.00	
3.931	3.958	(0.532)	153	17314			34.32- 94.32	68.03	
3.931	3.958	(0.532)	101	27551			85.50- 145.50	108.26	

29 1,1-Dichloroethene CAS #: 75-35-4									
3.986	3.986	(0.540)	61	25336	0.50000	0.5606	80.00- 120.00	100.00	
3.986	3.986	(0.540)	96	14575			29.81- 89.81	57.53	
3.986	3.986	(0.540)	98	11440			9.00- 69.00	45.15	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

33	Carbon Disulfide					CAS #:	75-15-0			
4.318	4.290	(0.585)	76	49375	0.50000	0.5829	80.00-	120.00	100.00	

40	Methylene Chloride					CAS #:	75-09-2			
4.843	4.815	(0.656)	49	19995	0.50000	0.5909	80.00-	120.00	100.00	
4.871	4.815	(0.659)	84	18154			40.47-	100.47	90.79	
4.843	4.815	(0.656)	51	6239			0.00-	30.00	31.20	

43	MTBE					CAS #:	1634-04-4			
5.175	5.175	(0.701)	73	22887	0.50000	0.4756	80.00-	120.00	100.00(a)	
5.147	5.175	(0.697)	57	8958			0.00-	52.63	39.14	
5.175	5.175	(0.701)	41	6914			0.00-	30.00	30.21	

45	trans-1,2-Dichloroethene					CAS #:	156-60-5			
5.203	5.203	(0.704)	96	19355	0.50000	0.6052	80.00-	120.00	100.00	
5.203	5.203	(0.704)	61	29045			119.47-	179.47	150.06	
5.203	5.203	(0.704)	98	12410			0.00-	30.00	64.12	

46	Hexane					CAS #:	110-54-3			
5.534	5.534	(0.749)	57	24684	0.50000	0.5089	80.00-	120.00	100.00	
5.534	5.534	(0.749)	43	18247			0.00-	30.00	73.92	
5.534	5.534	(0.749)	86	4409			0.00-	30.00	17.86	

54	1,1-Dichloroethane					CAS #:	75-34-3			
5.949	5.949	(0.805)	63	25663	0.50000	0.4922	80.00-	120.00	100.00(a)	
5.949	5.949	(0.805)	65	13490			1.86-	61.86	52.57	

65	2-Butanone					CAS #:	78-93-3			
7.027	7.027	(0.951)	72	8897	0.50000	0.6078	80.00-	120.00	100.00	
7.027	7.027	(0.951)	43	35422			409.65-	469.65	398.13	
7.055	7.027	(0.955)	57	4439			0.00-	30.00	49.89	

64	cis-1,2-Dichloroethene					CAS #:	156-59-2			
6.972	6.972	(0.944)	61	26832	0.50000	0.6503	80.00-	120.00	100.00	
6.972	6.972	(0.944)	96	19889			43.20-	103.20	74.12	
6.972	6.972	(0.944)	98	13061			17.85-	77.85	48.68	

67	Tetrahydrofuran					CAS #:	109-99-9			
7.415	7.415	(1.004)	42	23210	0.50000	0.6100	80.00-	120.00	100.00	
7.415	7.415	(1.004)	71	9141			5.48-	65.48	39.38	
7.415	7.415	(1.004)	72	10737			0.00-	30.00	46.26	

70	Chloroform					CAS #:	67-66-3			
7.525	7.553	(1.019)	83	29884	0.50000	0.5731	80.00-	120.00	100.00	
7.525	7.553	(1.019)	85	17860			32.67-	92.67	59.76	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

75	1,1,1-Trichloroethane					CAS #:	71-55-6			
7.774	7.774	(1.052)	97	32604	0.50000	0.5968	80.00-	120.00	100.00	
7.774	7.774	(1.052)	99	18613			34.55-	94.55	57.09	

73	Cyclohexane					CAS #:	110-82-7			
7.746	7.746	(1.049)	84	27736	0.50000	0.6411	80.00-	120.00	100.00	
7.746	7.746	(1.049)	56	29634			96.25-	156.25	106.84	
7.746	7.746	(1.049)	41	14639			32.28-	92.28	52.78	

77	Carbon Tetrachloride					CAS #:	56-23-5			
7.995	8.023	(1.082)	119	26063	0.50000	0.5243	80.00-	120.00	100.00	
7.995	8.023	(1.082)	117	24950			73.30-	133.30	95.73	

81	Benzene					CAS #:	71-43-2			
8.438	8.438	(0.910)	78	52333	0.50000	0.5867	80.00-	120.00	100.00	
8.438	8.438	(0.910)	77	11248			0.00-	30.00	21.49	

83	1,2-Dichloroethane					CAS #:	107-06-2			
8.603	8.603	(0.928)	62	22290	0.50000	0.6159	80.00-	120.00	100.00	
8.603	8.603	(0.928)	64	6977			0.00-	30.00	31.30	

85	Heptane					CAS #:	142-82-5			
8.852	8.852	(0.955)	100	7535	0.50000	0.7806	80.00-	120.00	100.00	
8.852	8.852	(0.955)	43	29890			0.00-	30.00	396.68	
8.852	8.852	(0.955)	71	17485			0.00-	30.00	232.05	

94	Trichloroethene					CAS #:	79-01-6			
9.682	9.682	(1.045)	95	21043	0.50000	0.5953	80.00-	120.00	100.00	
9.682	9.682	(1.045)	130	22414			78.57-	138.57	106.52	
9.682	9.682	(1.045)	97	14838			34.08-	94.08	70.51	

97	1,2-Dichloropropane					CAS #:	78-87-5			
10.179	10.179	(1.098)	63	16877	0.50000	0.5460	80.00-	120.00	100.00	
10.179	10.179	(1.098)	62	13213			42.26-	102.26	78.29	
10.179	10.179	(1.098)	41	10990			26.77-	86.77	65.12	

100	Bromodichloromethane					CAS #:	75-27-4			
10.732	10.732	(1.158)	83	28920	0.50000	0.5601	80.00-	120.00	100.00	
10.732	10.732	(1.158)	85	18413			31.75-	91.75	63.67	

102	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
11.672	11.673	(1.260)	75	24425	0.50000	0.5686	80.00-	120.00	100.00	
11.672	11.673	(1.260)	77	6970			1.36-	61.36	28.54	
11.700	11.673	(1.263)	39	8862			17.70-	77.70	36.28	

103	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.032	12.032	(1.298)	58	11214	0.50000	0.4825	80.00-	120.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
103 4-Methyl-2-pentanone (continued)									
12.032	12.032	(1.298)	43	37485			0.00- 30.00	334.27	
12.032	12.032	(1.298)	85	6047			0.00- 30.00	53.92	

105 Toluene CAS #: 108-88-3									
12.253	12.253	(1.322)	91	49671	0.50000	0.5479	80.00- 120.00	100.00	
12.253	12.253	(1.322)	92	32962			29.69- 89.69	66.36	

108 trans-1,3-Dichloropropene CAS #: 10061-02-6									
12.861	12.861	(0.882)	75	22841	0.50000	0.5235	80.00- 120.00	100.00	
12.834	12.861	(0.880)	77	6413			0.08- 60.08	28.08	
12.834	12.861	(0.880)	39	12864			15.97- 75.97	56.32	

110 1,1,2-Trichloroethane CAS #: 79-00-5									
13.138	13.138	(0.901)	97	19937	0.50000	0.6230	80.00- 120.00	100.00	
13.138	13.138	(0.901)	99	10911			29.85- 89.85	54.73	
13.138	13.138	(0.901)	83	15123			54.93- 114.93	75.85	

112 Tetrachloroethene CAS #: 127-18-4									
13.193	13.193	(0.905)	166	23583	0.50000	0.5445	80.00- 120.00	100.00	
13.193	13.193	(0.905)	129	18864			45.08- 105.08	79.99	
13.193	13.193	(0.905)	131	17800			44.22- 104.22	75.48	

114 2-Hexanone CAS #: 591-78-6									
13.580	13.580	(0.932)	58	16251	0.50000	0.5125	80.00- 120.00	100.00	
13.580	13.580	(0.932)	43	29468			148.62- 208.62	181.33	
13.580	13.580	(0.932)	100	5765			0.00- 30.00	35.47	

116 Dibromochloromethane CAS #: 124-48-1									
13.719	13.719	(0.941)	129	25600	0.50000	0.5104	80.00- 120.00	100.00	
13.719	13.719	(0.941)	127	16875			0.00- 30.00	65.92	

117 1,2-Dibromoethane CAS #: 106-93-4									
13.884	13.884	(0.953)	107	26910	0.50000	0.5519	80.00- 120.00	100.00	
13.884	13.884	(0.953)	109	23468			63.81- 123.81	87.21	

126 Chlorobenzene CAS #: 108-90-7									
14.631	14.631	(1.004)	112	36793	0.50000	0.4761	80.00- 120.00	100.00(a)	
14.631	14.631	(1.004)	114	11501			1.84- 61.84	31.26	
14.603	14.631	(1.002)	77	32356			26.78- 86.78	87.94	

129 Ethyl Benzene CAS #: 100-41-4									
14.769	14.769	(1.013)	106	24362	0.50000	0.5957	80.00- 120.00	100.00	
14.769	14.769	(1.013)	91	64080			0.00- 30.00	263.03	

130 m,p-Xylene CAS #: 108-38-3									
14.935	14.935	(1.025)	106	25452	0.50000	0.5107	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 m,p-Xylene (continued)									
14.935	14.935	(1.025)	91	55732			0.00- 30.00	218.97	

132 o-Xylene CAS #: 95-47-6									
15.488	15.488	(1.063)	106	27489	0.50000	0.5466	80.00- 120.00	100.00	
15.488	15.488	(1.063)	91	51508			178.74- 238.74	187.38	

134 Styrene CAS #: 100-42-5									
15.516	15.516	(1.064)	104	35605	0.50000	0.4966	80.00- 120.00	100.00(a)	
15.516	15.516	(1.064)	78	18620			20.27- 80.27	52.30	

135 Bromoform CAS #: 75-25-2									
15.765	15.765	(1.082)	173	19027	0.50000	0.4313	80.00- 120.00	100.00(a)	
15.765	15.765	(1.082)	171	11415			20.67- 80.67	59.99	

144 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.456	16.456	(1.129)	83	40065	0.50000	0.5448	80.00- 120.00	100.00	
16.456	16.456	(1.129)	85	25337			31.59- 91.59	63.24	

147 4-Ethyltoluene CAS #: 622-96-8									
16.649	16.649	(1.142)	105	67698	0.50000	0.5016	80.00- 120.00	100.00	
16.649	16.649	(1.142)	120	22846			0.00- 59.85	33.75	

148 1,3,5-Trimethylbenzene CAS #: 108-67-8									
16.732	16.732	(1.148)	105	71898	0.50000	0.5542	80.00- 120.00	100.00	
16.732	16.732	(1.148)	120	34076			0.00- 30.00	47.39	

153 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.147	17.147	(1.176)	105	72353	0.50000	0.5540	80.00- 120.00	100.00	
17.147	17.147	(1.176)	120	33530			15.22- 75.22	46.34	

156 1,3-Dichlorobenzene CAS #: 541-73-1									
17.451	17.451	(1.197)	146	40043	0.50000	0.4704	80.00- 120.00	100.00(a)	
17.451	17.451	(1.197)	148	25065			0.00- 30.00	62.60	
17.451	17.451	(1.197)	111	16317			0.00- 30.00	40.75	

157 1,4-Dichlorobenzene CAS #: 106-46-7									
17.562	17.562	(1.205)	146	46404	0.50000	0.5751	80.00- 120.00	100.00	
17.562	17.562	(1.205)	148	26549			0.00- 30.00	57.21	
17.562	17.562	(1.205)	111	15041			0.00- 30.00	32.41	

158 alpha-Chlorotoluene CAS #: 100-44-7									
17.700	17.700	(1.214)	91	56800	0.50000	0.4843	80.00- 120.00	100.00(a)	
17.700	17.700	(1.214)	126	13675			0.00- 30.00	24.08	

161 1,2-Dichlorobenzene CAS #: 95-50-1									
17.921	17.921	(1.230)	146	44406	0.50000	0.5415	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
161 1,2-Dichlorobenzene (continued)									
17.921	17.921	(1.230)	148	29125			33.37- 93.37	65.59	
17.921	17.921	(1.230)	111	15806			7.65- 67.65	35.59	

137 Cumene CAS #: 98-82-8									
15.958	15.958	(1.095)	105	72289	0.50000	0.5259	80.00- 120.00	100.00	
15.958	15.958	(1.095)	120	21844			0.00- 30.00	30.22	
15.958	15.958	(1.095)	51	7145			0.00- 30.00	9.88	

145 Propylbenzene CAS #: 103-65-1									
16.484	16.484	(1.131)	91	84913	0.50000	0.5394	80.00- 120.00	100.00	
16.484	16.484	(1.131)	120	21938			0.00- 30.00	25.84	
16.484	16.484	(1.131)	105	3685			0.00- 30.00	4.34	

80 2,2,4-Trimethylpentane CAS #: 540-84-1									
8.465	8.465	(1.146)	57	69240	0.50000	0.5361	80.00- 120.00	100.00	
8.465	8.465	(1.146)	56	27170			0.00- 30.00	39.24	
8.465	8.465	(1.146)	41	17762			0.00- 30.00	25.65	

95 Methyl Cyclohexane CAS #: 108-87-2									
9.903	9.903	(1.341)	83	28853	0.50000	0.5354	70.00- 130.00	100.00	
9.903	9.903	(1.341)	98	14551			0.00- 30.00	50.43	
9.903	9.903	(1.341)	55	24257			0.00- 30.00	84.07	

QC Flag Legend

- a - Target compound detected but, quantitated amount Below Limit Of Quantitation(BLOQ).
- H - Operator selected an alternate compound hit.

Report Date: 01-Jun-2007 13:36

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053004.d

Calibration Time: 14:39

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-0.5ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	448309	268985	627633	441719	-1.47
88 1,4-Difluorobenze	2033490	1220094	2846886	1974518	-2.90
125 Chlorobenzene-d5	1524596	914758	2134434	1505104	-1.28

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-30may.b/8053004.d

Date: 30-May-2007 14:39

Client ID: Level 2

Sample Info: 0.5ml #1487-289


Column phase: RTX-624

Instrument: msd8.1

Operator: db

Column diameter: 0.53

Page 1



/chem/msd8.1/8-30may.b/8053004.d

Chlorobenzene-d5+

Bromofluorobenzene

Report Date: 07-Jun-2007 13:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-07jun.b/8060704.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 07-JUN-2007 11:09
 Operator : JG Inst ID: msd8.i
 Smp Info : 2mL #1443-96
 Misc Info : 200ppbv-2ppbv
 Comment :
 Method : /chem/msd8.i/8-07jun.b/t14q530b.m
 Meth Date : 07-Jun-2007 13:41 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 11:09 Cal File: 8060704.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp16b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	CAL-AMT		ON-COL	TARGET RANGE	RATIO	
				RESPONSE	(PPBV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

* 68	Bromochloromethane					CAS #:	74-97-5		
7.387	7.387	(1.000)	130	359827	25.0000		70.00-	130.00	100.00
7.387	7.387	(1.000)	128	276445			42.98-	102.98	76.83
7.387	7.387	(1.000)	49	515800			112.53-	172.53	143.35

* 88	1,4-Difluorobenzene					CAS #:	540-36-3		
9.267	9.267	(1.000)	114	1618571	25.0000		70.00-	130.00	100.00
9.267	9.267	(1.000)	88	239337			0.00-	44.58	14.79

* 125	Chlorobenzene-d5					CAS #:	3114-55-4		
14.576	14.576	(1.000)	117	1231123	25.0000		70.00-	130.00	100.00
14.576	14.576	(1.000)	82	682772			0.00-	30.00	55.46

1	Freon 152a					CAS #:	75-37-6		
2.050	2.050	(0.278)	65	28430	2.00000	2.281	70.00-	130.00	100.00
2.078	2.078	(0.281)	51	113235			0.00-	30.00	398.29

20	Freon123a					CAS #:	354-23-4		
3.682	3.682	(0.498)	67	39913	2.00000	2.074	70.00-	130.00	100.00
3.709	3.709	(0.502)	117	33578			0.00-	30.00	84.13

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
21 Freon123						CAS #:	306-83-2			
3.792	3.792	(0.513)	83	24804	2.00000	2.045	70.00- 130.00	100.00		
3.792	3.792	(0.513)	133	7379			0.00- 30.00	29.75		
3.792	3.792	(0.513)	85	18073			0.00- 30.00	72.86		

38 tert-Butyl-Alcohol						CAS #:	75-65-0			
4.954	4.954	(0.671)	59	67488	2.00000	2.691	70.00- 130.00	100.00		
4.954	4.954	(0.671)	41	16170			0.00- 30.00	23.96		
4.954	4.954	(0.671)	57	7979			0.00- 30.00	11.82		

49 Isopropyl ether						CAS #:	108-20-3			
5.949	5.949	(0.805)	45	127830	2.00000	2.038	70.00- 130.00	100.00		
5.977	5.977	(0.809)	87	31904			0.00- 30.00	24.96		
5.977	5.977	(0.809)	59	14776			0.00- 30.00	11.56		

52 1-Propanol						CAS #:	71-23-8			
6.170	6.170	(0.835)	42	9618	2.00000	2.128	70.00- 130.00	100.00		
6.170	6.170	(0.835)	59	11102			0.00- 30.00	115.43		
6.170	6.170	(0.835)	41	10796			0.00- 30.00	112.25		

58 Ethyl-tert-butyl Ether						CAS #:	637-92-3			
6.585	6.585	(0.891)	59	75388	2.00000	1.800	70.00- 130.00	100.00(a)		
6.585	6.585	(0.891)	87	27007			0.00- 30.00	35.82		
6.585	6.585	(0.891)	41	10624			0.00- 30.00	14.09		

61 Ethyl Acetate						CAS #:	141-78-6			
7.083	7.083	(0.959)	70	11438	2.00000	2.093	70.00- 130.00	100.00		
7.083	7.083	(0.959)	43	92650			0.00- 30.00	810.02		
7.083	7.083	(0.959)	61	15040			0.00- 30.00	131.49		

78 Isobutanol						CAS #:	78-83-1			
8.437	8.437	(0.910)	43	35107	2.00000	1.890	70.00- 130.00	100.00		
8.437	8.437	(0.910)	41	23753			0.00- 30.00	67.66		

79 tert-amyl-Methyl Ether						CAS #:	994-05-8			
8.631	8.631	(1.168)	73	74928	2.00000	1.956	70.00- 130.00	100.00(a)		
8.631	8.631	(1.168)	87	18030			0.00- 30.00	24.06		
8.631	8.631	(1.168)	55	22510			0.00- 30.00	30.04		

89 1-Butanol						CAS #:	71-36-3			
9.737	9.737	(1.051)	56	28801	2.00000	1.818	70.00- 130.00	100.00(a)		
9.737	9.737	(1.051)	41	18725			0.00- 30.00	65.02		
9.737	9.737	(1.051)	43	17406			0.00- 30.00	60.44		

136 Cyclohexanone						CAS #:	108-94-1			
16.152	16.152	(1.108)	55	54831	2.00000	1.946	70.00- 130.00	100.00(a)		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
136 Cyclohexanone (continued)									
16.152	16.152	(1.108)	98	24425			0.00- 30.00	44.55	
16.152	16.152	(1.108)	42	35102			0.00- 30.00	64.02	

QC Flag Legend

a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).

Report Date: 07-Jun-2007 13:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 07-JUN-2007

Lab File ID: 8060704.d

Calibration Time: 11:37

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd8.i/8-07jun.b/t14q530b.m

Misc Info: 200ppbv-2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	350593	210356	490830	359827	2.63
88 1,4-Difluorobenze	1524282	914569	2133995	1618571	6.19
125 Chlorobenzene-d5	1168126	700876	1635376	1231123	5.39

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-07jun.b/8060704.d

Date: 07-JUN-2007 11:09

Client ID: Level 3

Sample Info: 2mL #1443-96


Column phase: RTX-624

Instrument: msd8.1

Operator: JG

Column diameter: 0.53

/chem/msd8.1/8-07jun.b/8060704.d



Report Date: 31-May-2007 14:52

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053005.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 30-MAY-2007 15:07
 Operator : db Inst ID: msd8.i
 Smp Info : 2.0ml #1487-289
 Misc Info : 200ppbv-2.0ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 31-May-2007 14:52 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 15:07 Cal File: 8053005.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO
==	=====	=====	====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5								
7.387	7.387	(1.000)	130	444018	25.0000		70.00- 130.00	100.00
7.387	7.387	(1.000)	128	343097			47.57- 107.57	77.27
7.387	7.387	(1.000)	49	663820			113.47- 173.47	149.50

* 88 1,4-Difluorobenzene CAS #: 540-36-3								
9.267	9.267	(1.000)	114	2035031	25.0000		70.00- 130.00	100.00
9.267	9.267	(1.000)	88	289330			0.00- 45.68	14.22

* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.576	14.576	(1.000)	117	1499190	25.0000		70.00- 130.00	100.00
14.576	14.576	(1.000)	82	846297			0.00- 30.00	56.45

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
8.465	8.465	(1.146)	65	590610	25.0000	25.415	70.00- 130.00	100.00
8.465	8.465	(1.146)	67	303638			0.00- 30.00	51.41

\$ 104 Toluene-d8 CAS #: 2037-26-5								
12.115	12.115	(1.307)	98	1781631	25.0000	25.288	70.00- 130.00	100.00
12.115	12.115	(1.307)	70	175095			0.00- 30.00	9.83

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 104 Toluene-d8 (continued)										
12.115	12.115	(1.307)	100	1161193			0.00- 30.00	65.18		

\$ 140 Bromofluorobenzene										
						CAS #: 460-00-4				
16.207	16.207	(1.112)	174	877440	25.0000	24.599	70.00- 130.00	100.00		
16.207	16.207	(1.112)	95	1139577			102.16- 162.16	129.88		
16.207	16.207	(1.112)	176	835648			64.31- 124.31	95.24		

3 Propylene										
						CAS #: 115-07-1				
2.023	2.023	(0.274)	41	68550	2.00000	2.852	70.00- 130.00	100.00		
2.023	2.023	(0.274)	42	32909			0.00- 30.00	48.01		
2.023	2.023	(0.274)	39	33753			0.00- 30.00	49.24		

4 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.050	2.050	(0.278)	85	143030	2.00000	2.351	70.00- 130.00	100.00		
2.050	2.050	(0.278)	87	45048			0.00- 30.00	31.50		

6 Freon 114										
						CAS #: 76-14-2				
2.216	2.216	(0.300)	135	109387	2.00000	1.990	70.00- 130.00	100.00		
2.216	2.216	(0.300)	137	29718			1.53- 61.53	27.17		

8 Chloromethane										
						CAS #: 74-87-3				
2.299	2.299	(0.311)	50	62645	2.00000	2.236	70.00- 130.00	100.00		
2.299	2.299	(0.311)	52	20724			0.00- 30.00	33.08		

9 Butane										
						CAS #: 106-97-8				
2.382	2.382	(0.322)	58	17616	2.00000	2.408	70.00- 130.00	100.00		
2.382	2.382	(0.322)	43	128408			0.00- 30.00	728.93		

11 Vinyl Chloride										
						CAS #: 75-01-4				
2.410	2.410	(0.326)	62	65793	2.00000	2.021	70.00- 130.00	100.00		
2.437	2.437	(0.330)	64	27327			0.00- 30.00	41.53		

10 1,3-Butadiene										
						CAS #: 106-99-0				
2.410	2.410	(0.326)	54	61421	2.00000	2.206	70.00- 130.00	100.00		
2.410	2.410	(0.326)	39	64322			0.00- 30.00	104.72		

13 Bromomethane										
						CAS #: 74-83-9				
2.852	2.852	(0.386)	94	42582	2.00000	1.958	70.00- 130.00	100.00		
2.852	2.852	(0.386)	96	42273			65.03- 125.03	99.27		

16 Chloroethane										
						CAS #: 75-00-3				
2.990	2.990	(0.405)	64	36761	2.00000	2.134	70.00- 130.00	100.00		
2.990	2.990	(0.405)	49	9519			0.00- 30.00	25.89		
2.990	2.990	(0.405)	66	10406			0.00- 30.00	28.31		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
15 Isopentane						CAS #:	78-78-4		
2.963	2.963	(0.401)	43	84741	2.00000	2.085	70.00-	130.00	100.00
2.963	2.963	(0.401)	57	57480			0.00-	30.00	67.83
2.963	2.963	(0.401)	72	7193			0.00-	30.00	8.49

18 Trichlorofluoromethane/Fr11						CAS #:	75-69-4		
3.239	3.239	(0.439)	101	149777	2.00000	2.166	70.00-	130.00	100.00
3.239	3.239	(0.439)	103	91623			34.97-	94.97	61.17

23 Ethanol						CAS #:	64-17-5		
3.516	3.516	(0.476)	45	24067	2.00000	2.180	70.00-	130.00	100.00
3.516	3.516	(0.476)	43	13031			0.00-	30.00	54.14
3.516	3.516	(0.476)	46	11087			0.00-	30.00	46.07

28 Freon 113						CAS #:	76-13-1		
3.931	3.931	(0.532)	151	99380	2.00000	2.172	70.00-	130.00	100.00
3.931	3.931	(0.532)	153	59189			33.71-	93.71	59.56
3.931	3.931	(0.532)	101	109122			86.34-	146.34	109.80

29 1,1-Dichloroethene						CAS #:	75-35-4		
3.986	3.986	(0.540)	61	96927	2.00000	2.133	70.00-	130.00	100.00
3.986	3.986	(0.540)	96	59254			30.42-	90.42	61.13
3.986	3.986	(0.540)	98	44431			8.39-	68.39	45.84

30 Acetone						CAS #:	67-64-1		
4.124	4.124	(0.558)	58	34898	2.00000	2.294	70.00-	130.00	100.00
4.124	4.124	(0.558)	43	95643			0.00-	30.00	274.06

33 Carbon Disulfide						CAS #:	75-15-0		
4.318	4.318	(0.584)	76	172959	2.00000	2.031	70.00-	130.00	100.00

34 2-Propanol						CAS #:	67-63-0		
4.318	4.318	(0.584)	45	129095	2.00000	2.346	70.00-	130.00	100.00
4.318	4.318	(0.584)	43	34823			0.00-	30.00	26.97
4.318	4.318	(0.584)	59	7801			0.00-	30.00	6.04

37 3-Chloropropene						CAS #:	107-05-1		
4.566	4.566	(0.618)	76	25780	2.00000	1.898	70.00-	130.00	100.00(a)
4.566	4.566	(0.618)	41	78835			0.00-	30.00	305.80

40 Methylene Chloride						CAS #:	75-09-2		
4.843	4.843	(0.656)	49	72037	2.00000	2.118	70.00-	130.00	100.00
4.843	4.843	(0.656)	84	56488			41.01-	101.01	78.42
4.843	4.843	(0.656)	51	22744			0.00-	30.00	31.57

43 MTBE						CAS #:	1634-04-4		
5.175	5.175	(0.701)	73	78059	2.00000	1.614	70.00-	130.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
43 MTBE (continued)									
5.147	5.147	(0.697)	57	21684			0.00- 53.82	27.78	
5.147	5.147	(0.697)	41	16336			0.00- 30.00	20.93	

45 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.202	5.202	(0.704)	96	70934	2.00000	2.206	70.00- 130.00	100.00	
5.202	5.202	(0.704)	61	94977			119.04- 179.04	133.89	
5.202	5.202	(0.704)	98	40611			0.00- 30.00	57.25	

46 Hexane						CAS #: 110-54-3			
5.534	5.534	(0.749)	57	95925	2.00000	1.967	70.00- 130.00	100.00	
5.534	5.534	(0.749)	43	60460			0.00- 30.00	63.03	
5.534	5.534	(0.749)	86	15672			0.00- 30.00	16.34	

54 1,1-Dichloroethane						CAS #: 75-34-3			
5.949	5.949	(0.805)	63	114940	2.00000	2.193	70.00- 130.00	100.00	
5.949	5.949	(0.805)	65	34286			1.22- 61.22	29.83	

55 Vinyl Acetate						CAS #: 108-05-4			
6.032	6.032	(0.817)	86	14556	2.00000	1.968	70.00- 130.00	100.00(a)	
6.032	6.032	(0.817)	43	135869			0.00- 30.00	933.42	
6.032	6.032	(0.817)	42	12791			0.00- 30.00	87.87	

64 cis-1,2-Dichloroethene						CAS #: 156-59-2			
6.972	6.972	(0.944)	61	84153	2.00000	2.029	70.00- 130.00	100.00	
6.972	6.972	(0.944)	96	66205			45.09- 105.09	78.67	
6.972	6.972	(0.944)	98	40871			17.66- 77.66	48.57	

65 2-Butanone						CAS #: 78-93-3			
7.027	7.027	(0.951)	72	30203	2.00000	2.052	70.00- 130.00	100.00	
7.027	7.027	(0.951)	43	124260			398.56- 458.56	411.42	
7.027	7.027	(0.951)	57	9637			0.00- 30.00	31.91	

67 Tetrahydrofuran						CAS #: 109-99-9			
7.414	7.414	(1.004)	42	78266	2.00000	2.046	70.00- 130.00	100.00	
7.414	7.414	(1.004)	71	36816			5.14- 65.14	47.04	
7.414	7.414	(1.004)	72	33830			0.00- 30.00	43.22	

70 Chloroform						CAS #: 67-66-3			
7.525	7.525	(1.019)	83	105767	2.00000	2.018	70.00- 130.00	100.00	
7.525	7.525	(1.019)	85	69135			31.98- 91.98	65.37	

73 Cyclohexane						CAS #: 110-82-7			
7.746	7.746	(1.049)	84	84366	2.00000	1.940	70.00- 130.00	100.00	
7.746	7.746	(1.049)	56	109014			99.30- 159.30	129.22	
7.746	7.746	(1.049)	41	61541			33.84- 93.84	72.95	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

75	1,1,1-Trichloroethane					CAS #:	71-55-6			
7.774	7.774	(1.052)	97	108279	2.00000	1.972	70.00-	130.00	100.00	
7.774	7.774	(1.052)	99	66999			34.73-	94.73	61.88	

77	Carbon Tetrachloride					CAS #:	56-23-5			
7.995	7.995	(1.082)	119	87757	2.00000	1.756	70.00-	130.00	100.00	
7.995	7.995	(1.082)	117	99969			74.04-	134.04	113.92	

81	Benzene					CAS #:	71-43-2			
8.437	8.437	(0.910)	78	185467	2.00000	2.017	70.00-	130.00	100.00	
8.437	8.437	(0.910)	77	44486			0.00-	30.00	23.99	

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
8.465	8.465	(1.146)	57	269118	2.00000	2.073	70.00-	130.00	100.00	
8.465	8.465	(1.146)	56	84149			0.00-	30.00	31.27	
8.465	8.465	(1.146)	41	62827			0.00-	30.00	23.35	

83	1,2-Dichloroethane					CAS #:	107-06-2			
8.603	8.603	(0.928)	62	74900	2.00000	2.008	70.00-	130.00	100.00	
8.603	8.603	(0.928)	64	24637			0.00-	30.00	32.89	

85	Heptane					CAS #:	142-82-5			
8.852	8.852	(0.955)	100	18594	2.00000	1.869	70.00-	130.00	100.00	
8.852	8.852	(0.955)	43	110807			0.00-	30.00	595.93	
8.852	8.852	(0.955)	71	61004			0.00-	30.00	328.08	

94	Trichloroethene					CAS #:	79-01-6			
9.682	9.682	(1.045)	95	73161	2.00000	2.008	70.00-	130.00	100.00	
9.682	9.682	(1.045)	130	72926			77.84-	137.84	99.68	
9.682	9.682	(1.045)	97	48621			34.22-	94.22	66.46	

95	Methyl Cyclohexane					CAS #:	108-87-2			
9.903	9.903	(1.341)	83	109945	2.00000	2.029	70.00-	130.00	100.00	
9.903	9.903	(1.341)	98	54584			0.00-	30.00	49.65	
9.903	9.903	(1.341)	55	89274			0.00-	30.00	81.20	

97	1,2-Dichloropropane					CAS #:	78-87-5			
10.179	10.179	(1.098)	63	70027	2.00000	2.198	70.00-	130.00	100.00	
10.179	10.179	(1.098)	62	47177			42.15-	102.15	67.37	
10.179	10.179	(1.098)	41	36977			26.47-	86.47	52.80	

98	1,4-Dioxane					CAS #:	123-91-1			
10.428	10.428	(1.125)	88	40326	2.00000	2.075	70.00-	130.00	100.00	
10.428	10.428	(1.125)	58	27930			44.03-	104.03	69.26	
10.428	10.428	(1.125)	57	7847			0.00-	30.00	19.46	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
					(PPEV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

100	Bromodichloromethane				CAS #:		75-27-4		
10.732	10.732	(1.158)	83	104941	2.00000	1.972	70.00-	130.00	100.00
10.732	10.732	(1.158)	85	62504			31.03-	91.03	59.56

102	cis-1,3-Dichloropropene				CAS #:		10061-01-5		
11.672	11.672	(1.260)	75	85811	2.00000	1.938	70.00-	130.00	100.00
11.672	11.672	(1.260)	77	26235			1.19-	61.19	30.57
11.672	11.672	(1.260)	39	39774			16.93-	76.93	46.35

103	4-Methyl-2-pentanone				CAS #:		108-10-1		
12.032	12.032	(1.298)	58	49522	2.00000	2.067	70.00-	130.00	100.00(M)
12.032	12.032	(1.298)	43	123001			0.00-	30.00	248.38
12.032	12.032	(1.298)	85	21457			0.00-	30.00	43.33

105	Toluene				CAS #:		108-88-3		
12.253	12.253	(1.322)	91	186889	2.00000	2.000	70.00-	130.00	100.00
12.253	12.253	(1.322)	92	110346			30.46-	90.46	59.04

108	trans-1,3-Dichloropropene				CAS #:		10061-02-6		
12.861	12.861	(0.882)	75	84129	2.00000	1.936	70.00-	130.00	100.00
12.861	12.861	(0.882)	77	21596			0.11-	60.11	25.67
12.834	12.834	(0.880)	39	40030			15.75-	75.75	47.58

110	1,1,2-Trichloroethane				CAS #:		79-00-5		
13.138	13.138	(0.901)	97	63448	2.00000	1.990	70.00-	130.00	100.00
13.138	13.138	(0.901)	99	41614			31.47-	91.47	65.59
13.138	13.138	(0.901)	83	50435			58.25-	118.25	79.49

112	Tetrachloroethene				CAS #:		127-18-4		
13.193	13.193	(0.905)	166	89856	2.00000	2.083	70.00-	130.00	100.00
13.193	13.193	(0.905)	129	69545			45.90-	105.90	77.40
13.193	13.193	(0.905)	131	66172			43.88-	103.88	73.64

114	2-Hexanone				CAS #:		591-78-6		
13.580	13.580	(0.932)	58	52105	2.00000	1.650	70.00-	130.00	100.00(a)
13.580	13.580	(0.932)	43	110802			147.03-	207.03	212.65
13.580	13.580	(0.932)	100	12762			0.00-	30.00	24.49

116	Dibromochloromethane				CAS #:		124-48-1		
13.718	13.718	(0.941)	129	95939	2.00000	1.920	70.00-	130.00	100.00
13.718	13.718	(0.941)	127	73156			0.00-	30.00	76.25

117	1,2-Dibromoethane				CAS #:		106-93-4		
13.884	13.884	(0.953)	107	96620	2.00000	1.989	70.00-	130.00	100.00
13.884	13.884	(0.953)	109	96596			65.18-	125.18	99.98

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
126 Chlorobenzene						CAS #:	108-90-7		
14.631	14.631	(1.004)	112	172950	2.00000	2.247	70.00-	130.00	100.00
14.631	14.631	(1.004)	114	49642			1.91-	61.91	28.70
14.603	14.603	(1.002)	77	98312			26.50-	86.50	56.84

129 Ethyl Benzene						CAS #:	100-41-4		
14.769	14.769	(1.013)	106	80000	2.00000	1.964	70.00-	130.00	100.00
14.769	14.769	(1.013)	91	248489			0.00-	30.00	310.61

130 m,p-Xylene						CAS #:	108-38-3		
14.935	14.935	(1.025)	106	101958	2.00000	2.054	70.00-	130.00	100.00
14.935	14.935	(1.025)	91	191884			0.00-	30.00	188.20

132 o-Xylene						CAS #:	95-47-6		
15.488	15.488	(1.063)	106	101432	2.00000	2.025	70.00-	130.00	100.00
15.488	15.488	(1.063)	91	208881			177.47-	237.47	205.93

134 Styrene						CAS #:	100-42-5		
15.516	15.516	(1.064)	104	133562	2.00000	1.870	70.00-	130.00	100.00
15.516	15.516	(1.064)	78	71778			20.25-	80.25	53.74

135 Bromoform						CAS #:	75-25-2		
15.764	15.764	(1.082)	173	78478	2.00000	1.786	70.00-	130.00	100.00
15.764	15.764	(1.082)	171	40496			21.05-	81.05	51.60

137 Cumene						CAS #:	98-82-8		
15.958	15.958	(1.095)	105	282468	2.00000	2.063	70.00-	130.00	100.00
15.958	15.958	(1.095)	120	74218			0.00-	30.00	26.27
15.958	15.958	(1.095)	51	28040			0.00-	30.00	9.93

144 1,1,2,2-Tetrachloroethane						CAS #:	79-34-5		
16.456	16.456	(1.129)	83	148008	2.00000	2.020	70.00-	130.00	100.00
16.456	16.456	(1.129)	85	94627			31.99-	91.99	63.93

145 Propylbenzene						CAS #:	103-65-1		
16.483	16.483	(1.131)	91	328901	2.00000	2.097	70.00-	130.00	100.00
16.483	16.483	(1.131)	120	75360			0.00-	30.00	22.91
16.483	16.483	(1.131)	105	9519			0.00-	30.00	2.89

147 4-Ethyltoluene						CAS #:	622-96-8		
16.649	16.649	(1.142)	105	271508	2.00000	2.019	70.00-	130.00	100.00
16.649	16.649	(1.142)	120	87836			0.00-	59.60	32.35

148 1,3,5-Trimethylbenzene						CAS #:	108-67-8		
16.732	16.732	(1.148)	105	279904	2.00000	2.166	70.00-	130.00	100.00
16.732	16.732	(1.148)	120	137880			0.00-	30.00	49.26

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

153	17.147	17.147 (1.176)	105	275228	2.00000	2.116	70.00- 130.00	100.00	
	17.147	17.147 (1.176)	120	129173			15.41- 75.41	46.93	

156	17.451	17.451 (1.197)	146	167109	2.00000	1.971	70.00- 130.00	100.00	
	17.451	17.451 (1.197)	148	106537			0.00- 30.00	63.75	
	17.451	17.451 (1.197)	111	73203			0.00- 30.00	43.81	

157	17.562	17.562 (1.205)	146	138434	2.00000	1.722	70.00- 130.00	100.00	
	17.562	17.562 (1.205)	148	127853			0.00- 30.00	92.36	
	17.562	17.562 (1.205)	111	69398			0.00- 30.00	50.13	

158	17.700	17.700 (1.214)	91	230635	2.00000	1.974	70.00- 130.00	100.00	
	17.700	17.700 (1.214)	126	47342			0.00- 30.00	20.53	

161	17.921	17.921 (1.230)	146	165520	2.00000	2.026	70.00- 130.00	100.00	
	17.921	17.921 (1.230)	148	106977			32.70- 92.70	64.63	
	17.921	17.921 (1.230)	111	68354			7.07- 67.07	41.30	

167	19.276	19.276 (1.322)	180	177945	2.00000	2.155	70.00- 130.00	100.00	
	19.276	19.276 (1.322)	182	166734			65.19- 125.19	93.70	

168	19.359	19.359 (1.328)	225	114250	2.00000	2.411	70.00- 130.00	100.00	
	19.359	19.359 (1.328)	223	74622			33.26- 93.26	65.31	

169	19.470	19.470 (1.336)	128	467801	2.00000	2.687	70.00- 130.00	100.00	
	19.470	19.470 (1.336)	127	67084			0.00- 30.00	14.34	

QC Flag Legend

- a - Target compound detected but, quantitated amount Below Limit Of Quantitation(BLOQ).
- M - Compound response manually integrated.

Report Date: 31-May-2007 14:52

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053005.d

Calibration Time: 16:03

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	441133	264680	617586	444018	0.65
88 1,4-Difluorobenze	1992312	1195387	2789237	2035031	2.14
125 Chlorobenzene-d5	1475337	885202	2065472	1499190	1.62

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.


AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-30may.b/8053005.d
 Date: 30-MAY-2007 15:07
 Client ID: Level 3
 Sample Info: 2.0ml #1487-289
 Column phase: RTX-624

Instrument: msd8.1
 Operator: db
 Column diameter: 0.53



Report Date: 01-Jun-2007 13:51

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053006.d
 Lab Smp Id: ICAL Client Smp ID: Level 4
 Inj Date : 30-MAY-2007 15:35
 Operator : db Inst ID: msd8.i
 Smp Info : 25ml #1487-289
 Misc Info : 200ppbv-25ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 01-Jun-2007 10:56 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 15:35 Cal File: 8053006.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.415	(1.000)	130	442807	25.0000			80.00- 120.00	100.00
7.387	7.415	(1.000)	128	348882				48.60- 108.60	78.79
7.387	7.415	(1.000)	49	642051				114.98- 174.98	145.00

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	2029767	25.0000			80.00- 120.00	100.00
9.267	9.267	(1.000)	88	305336				0.00- 45.16	15.04

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	1539410	25.0000			80.00- 120.00	100.00
14.576	14.576	(1.000)	82	880295				0.00- 30.00	57.18

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.146)	65	557163	25.0000	24.041		80.00- 120.00	100.00
8.465	8.465	(1.146)	67	328511				0.00- 30.00	58.96

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	1689996	25.0000	24.050		80.00- 120.00	100.00
12.115	12.115	(1.307)	70	173996				0.00- 30.00	10.30

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 104 Toluene-d8 (continued)										
12.115	12.115	(1.307)	100	1337051			0.00- 30.00	79.12		

\$ 140 Bromofluorobenzene										
						CAS #: 460-00-4				
16.207	16.207	(1.112)	174	923372	25.0000	25.210	80.00- 120.00	100.00		
16.207	16.207	(1.112)	95	1221505			105.65- 165.65	132.29		
16.207	16.207	(1.112)	176	870157			66.34- 126.34	94.24		

3 Propylene						CAS #: 115-07-1				
1.995	1.995	(0.270)	41	583695	25.0000	24.354	70.00- 130.00	100.00		
1.995	1.995	(0.270)	42	385435			0.00- 30.00	66.03		
1.995	1.995	(0.270)	39	385271			0.00- 30.00	66.01		

4 Dichlorodifluoromethane/Fr12						CAS #: 75-71-8				
2.050	2.078	(0.278)	85	1479581	25.0000	24.389	80.00- 120.00	100.00		
2.050	2.078	(0.278)	87	460934			0.00- 30.00	31.15		

6 Freon 114						CAS #: 76-14-2				
2.161	2.189	(0.293)	135	1377957	25.0000	25.142	80.00- 120.00	100.00		
2.161	2.189	(0.293)	137	436681			0.71- 60.71	31.69		

8 Chloromethane						CAS #: 74-87-3				
2.272	2.299	(0.308)	50	730257	25.0000	26.138	80.00- 120.00	100.00		
2.272	2.299	(0.308)	52	232404			0.00- 30.00	31.82		

9 Butane						CAS #: 106-97-8				
2.327	2.355	(0.315)	58	190942	25.0000	26.170	70.00- 130.00	100.00		
2.327	2.355	(0.315)	43	1372202			0.00- 30.00	718.65		

11 Vinyl Chloride						CAS #: 75-01-4				
2.410	2.438	(0.326)	62	788546	25.0000	24.290	80.00- 120.00	100.00		
2.410	2.438	(0.326)	64	250595			0.00- 30.00	31.78		

10 1,3-Butadiene						CAS #: 106-99-0				
2.382	2.410	(0.322)	54	644846	25.0000	23.222	80.00- 120.00	100.00		
2.382	2.410	(0.322)	39	672011			0.00- 30.00	104.21		

13 Bromomethane						CAS #: 74-83-9				
2.852	2.880	(0.386)	94	560666	25.0000	25.851	80.00- 120.00	100.00		
2.852	2.880	(0.386)	96	514411			63.65- 123.65	91.75		

16 Chloroethane						CAS #: 75-00-3				
2.935	2.991	(0.397)	64	435981	25.0000	25.376	80.00- 120.00	100.00		
2.935	2.991	(0.397)	49	106716			0.00- 30.00	24.48		
2.935	2.991	(0.397)	66	126764			0.00- 30.00	29.08		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
15 Isopentane						CAS #: 78-78-4			
2.935	2.963	(0.397)	43	1053632	25.0000	25.992	70.00- 130.00	100.00	
2.963	2.963	(0.401)	57	687436			0.00- 30.00	65.24	
2.963	2.963	(0.401)	72	78712			0.00- 30.00	7.47	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.212	3.239	(0.435)	101	1753350	25.0000	25.428	80.00- 120.00	100.00	
3.212	3.239	(0.435)	103	1132129			34.50- 94.50	64.57	

23 Ethanol						CAS #: 64-17-5			
3.516	3.544	(0.476)	45	293783	25.0000	26.681	80.00- 120.00	100.00	
3.516	3.544	(0.476)	43	57563			0.00- 30.00	19.59	
3.516	3.544	(0.476)	46	113176			0.00- 30.00	38.52	

28 Freon 113						CAS #: 76-13-1			
3.930	3.958	(0.532)	151	1151774	25.0000	25.246	80.00- 120.00	100.00	
3.930	3.958	(0.532)	153	703274			34.32- 94.32	61.06	
3.930	3.958	(0.532)	101	1334210			85.50- 145.50	115.84	

29 1,1-Dichloroethene						CAS #: 75-35-4			
3.958	3.986	(0.536)	61	1137998	25.0000	25.117	80.00- 120.00	100.00	
3.958	3.986	(0.536)	96	688816			29.81- 89.81	60.53	
3.958	3.986	(0.536)	98	424092			9.00- 69.00	37.27	

30 Acetone						CAS #: 67-64-1			
4.124	4.124	(0.558)	58	378307	25.0000	24.930	80.00- 120.00	100.00	
4.124	4.124	(0.558)	43	1131658			0.00- 30.00	299.14	

33 Carbon Disulfide						CAS #: 75-15-0			
4.290	4.290	(0.581)	76	2121278	25.0000	24.982	80.00- 120.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
4.318	4.318	(0.584)	45	1370148	25.0000	24.973	80.00- 120.00	100.00	
4.318	4.318	(0.584)	43	262313			0.00- 30.00	19.14	
4.318	4.318	(0.584)	59	54411			0.00- 30.00	3.97	

37 3-Chloropropene						CAS #: 107-05-1			
4.566	4.594	(0.618)	76	360688	25.0000	26.626	80.00- 120.00	100.00	
4.566	4.594	(0.618)	41	1082431			0.00- 30.00	300.10	

40 Methylene Chloride						CAS #: 75-09-2			
4.815	4.815	(0.652)	49	845544	25.0000	24.927	80.00- 120.00	100.00	
4.815	4.815	(0.652)	84	605378			40.47- 100.47	71.60	
4.815	4.815	(0.652)	51	259145			0.00- 30.00	30.65	

43 MTBE						CAS #: 1634-04-4			
5.147	5.175	(0.697)	73	1407624	25.0000	29.179	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
43 MTBE (continued)									
5.147	5.175	(0.697)	57	327200			0.00- 52.63	23.24	
5.147	5.175	(0.697)	41	310806			0.00- 30.00	22.08	

45 trans-1,2-Dichloroethene CAS #: 156-60-5									
5.175	5.203	(0.701)	96	762528	25.0000	23.784	80.00- 120.00	100.00	
5.175	5.203	(0.701)	61	1150624			119.47- 179.47	150.90	
5.175	5.203	(0.701)	98	496217			0.00- 30.00	65.08	

46 Hexane CAS #: 110-54-3									
5.534	5.534	(0.749)	57	1205663	25.0000	24.795	80.00- 120.00	100.00	
5.534	5.534	(0.749)	43	773376			0.00- 30.00	64.15	
5.534	5.534	(0.749)	86	198943			0.00- 30.00	16.50	

54 1,1-Dichloroethane CAS #: 75-34-3									
5.949	5.949	(0.805)	63	1328399	25.0000	25.417	80.00- 120.00	100.00	
5.949	5.949	(0.805)	65	419788			1.86- 61.86	31.60	

55 Vinyl Acetate CAS #: 108-05-4									
6.032	6.032	(0.817)	86	186162	25.0000	25.232	70.00- 130.00	100.00	
6.032	6.032	(0.817)	43	2005122			0.00- 30.00	1077.08	
6.032	6.032	(0.817)	42	151750			0.00- 30.00	81.52	

64 cis-1,2-Dichloroethene CAS #: 156-59-2									
6.972	6.972	(0.944)	61	1009566	25.0000	24.407	80.00- 120.00	100.00	
6.972	6.972	(0.944)	96	744531			43.20- 103.20	73.75	
6.972	6.972	(0.944)	98	478476			17.85- 77.85	47.39	

65 2-Butanone CAS #: 78-93-3									
7.027	7.027	(0.951)	72	348381	25.0000	23.740	80.00- 120.00	100.00	
7.027	7.027	(0.951)	43	1511122			409.65- 469.65	433.76	
7.027	7.027	(0.951)	57	115798			0.00- 30.00	33.24	

67 Tetrahydrofuran CAS #: 109-99-9									
7.387	7.415	(1.000)	42	937522	25.0000	24.579	80.00- 120.00	100.00	
7.387	7.415	(1.000)	71	331869			5.48- 65.48	35.40	
7.414	7.415	(1.004)	72	366437			0.00- 30.00	39.09	

70 Chloroform CAS #: 67-66-3									
7.525	7.553	(1.019)	83	1299284	25.0000	24.858	80.00- 120.00	100.00	
7.525	7.553	(1.019)	85	810995			32.67- 92.67	62.42	

73 Cyclohexane CAS #: 110-82-7									
7.746	7.746	(1.049)	84	1057678	25.0000	24.389	80.00- 120.00	100.00	
7.746	7.746	(1.049)	56	1367225			96.25- 156.25	129.27	
7.746	7.746	(1.049)	41	682191			32.28- 92.28	64.50	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

75	1,1,1-Trichloroethane					CAS #:	71-55-6			
7.774	7.774	(1.052)	97	1343871	25.0000	24.539	80.00-	120.00	100.00	
7.774	7.774	(1.052)	99	876393			34.55-	94.55	65.21	

77	Carbon Tetrachloride					CAS #:	56-23-5			
7.995	8.023	(1.082)	119	1303695	25.0000	26.160	80.00-	120.00	100.00	
7.995	8.023	(1.082)	117	1329642			73.30-	133.30	101.99	

81	Benzene					CAS #:	71-43-2			
8.437	8.438	(0.910)	78	2220324	25.0000	24.214	80.00-	120.00	100.00	
8.437	8.438	(0.910)	77	477752			0.00-	30.00	21.52	

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
8.465	8.465	(1.146)	57	3208710	25.0000	24.784	80.00-	120.00	100.00	
8.465	8.465	(1.146)	56	1043397			0.00-	30.00	32.52	
8.465	8.465	(1.146)	41	660582			0.00-	30.00	20.59	

83	1,2-Dichloroethane					CAS #:	107-06-2			
8.603	8.603	(0.928)	62	912402	25.0000	24.525	80.00-	120.00	100.00	
8.603	8.603	(0.928)	64	284806			0.00-	30.00	31.21	

85	Heptane					CAS #:	142-82-5			
8.852	8.852	(0.955)	100	223706	25.0000	22.544	80.00-	120.00	100.00	
8.852	8.852	(0.955)	43	1246808			0.00-	30.00	557.34	
8.852	8.852	(0.955)	71	718610			0.00-	30.00	321.23	

94	Trichloroethene					CAS #:	79-01-6			
9.682	9.682	(1.045)	95	899732	25.0000	24.760	80.00-	120.00	100.00	
9.682	9.682	(1.045)	130	950218			78.57-	138.57	105.61	
9.682	9.682	(1.045)	97	567162			34.08-	94.08	63.04	

95	Methyl Cyclohexane					CAS #:	108-87-2			
9.903	9.903	(1.341)	83	1353516	25.0000	25.052	70.00-	130.00	100.00	
9.903	9.903	(1.341)	98	623110			0.00-	30.00	46.04	
9.903	9.903	(1.341)	55	1057240			0.00-	30.00	78.11	

97	1,2-Dichloropropane					CAS #:	78-87-5			
10.179	10.179	(1.098)	63	774557	25.0000	24.374	80.00-	120.00	100.00	
10.179	10.179	(1.098)	62	537358			42.26-	102.26	69.38	
10.179	10.179	(1.098)	41	444960			26.77-	86.77	57.45	

98	1,4-Dioxane					CAS #:	123-91-1			
10.428	10.428	(1.125)	88	491146	25.0000	25.340	80.00-	120.00	100.00	
10.428	10.428	(1.125)	58	356106			41.45-	101.45	72.51	
10.428	10.428	(1.125)	57	107866			0.00-	30.00	21.96	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
100 Bromodichloromethane									
						CAS #:	75-27-4		
10.732	10.732	(1.158)	83	1309837	25.0000	24.679	80.00-	120.00	100.00
10.732	10.732	(1.158)	85	812676			31.75-	91.75	62.04

102 cis-1,3-Dichloropropene									
						CAS #:	10061-01-5		
11.672	11.673	(1.260)	75	1088954	25.0000	24.658	80.00-	120.00	100.00
11.672	11.673	(1.260)	77	332460			1.36-	61.36	30.53
11.672	11.673	(1.260)	39	522028			17.70-	77.70	47.94

103 4-Methyl-2-pentanone									
						CAS #:	108-10-1		
12.032	12.032	(1.298)	58	595289	25.0000	24.917	80.00-	120.00	100.00
12.032	12.032	(1.298)	43	1462778			0.00-	30.00	245.73
12.032	12.032	(1.298)	85	250389			0.00-	30.00	42.06

105 Toluene									
						CAS #:	108-88-3		
12.253	12.253	(1.322)	91	2271771	25.0000	24.377	80.00-	120.00	100.00
12.253	12.253	(1.322)	92	1302497			29.69-	89.69	57.33

108 trans-1,3-Dichloropropene									
						CAS #:	10061-02-6		
12.834	12.861	(0.880)	75	1101495	25.0000	24.681	80.00-	120.00	100.00
12.834	12.861	(0.880)	77	341616			0.08-	60.08	31.01
12.834	12.861	(0.880)	39	503742			15.97-	75.97	45.73

110 1,1,2-Trichloroethane									
						CAS #:	79-00-5		
13.138	13.138	(0.901)	97	785392	25.0000	23.996	80.00-	120.00	100.00
13.138	13.138	(0.901)	99	476630			29.85-	89.85	60.69
13.138	13.138	(0.901)	83	661660			54.93-	114.93	84.25

112 Tetrachloroethene									
						CAS #:	127-18-4		
13.193	13.193	(0.905)	166	1075849	25.0000	24.286	80.00-	120.00	100.00
13.193	13.193	(0.905)	129	832653			45.08-	105.08	77.39
13.193	13.193	(0.905)	131	811520			44.22-	104.22	75.43

114 2-Hexanone									
						CAS #:	591-78-6		
13.580	13.580	(0.932)	58	818770	25.0000	25.246	80.00-	120.00	100.00
13.580	13.580	(0.932)	43	1453939			148.62-	208.62	177.58
13.580	13.580	(0.932)	100	165065			0.00-	30.00	20.16

116 Dibromochloromethane									
						CAS #:	124-48-1		
13.718	13.719	(0.941)	129	1251408	25.0000	24.396	80.00-	120.00	100.00
13.718	13.719	(0.941)	127	988822			0.00-	30.00	79.02

117 1,2-Dibromoethane									
						CAS #:	106-93-4		
13.884	13.884	(0.953)	107	1209824	25.0000	24.258	80.00-	120.00	100.00
13.884	13.884	(0.953)	109	1141289			63.81-	123.81	94.34

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
126 Chlorobenzene						CAS #:	108-90-7		
14.603	14.631	(1.002)	112	1910705	25.0000	24.172	80.00-	120.00	100.00
14.631	14.631	(1.004)	114	623141			1.84-	61.84	32.61
14.603	14.631	(1.002)	77	1069076			26.78-	86.78	55.95

129 Ethyl Benzene						CAS #:	100-41-4		
14.769	14.769	(1.013)	106	987199	25.0000	23.600	80.00-	120.00	100.00
14.769	14.769	(1.013)	91	3031265			0.00-	30.00	307.06

130 m,p-Xylene						CAS #:	108-38-3		
14.935	14.935	(1.025)	106	1223079	25.0000	23.994	80.00-	120.00	100.00
14.935	14.935	(1.025)	91	2365743			0.00-	30.00	193.43

132 o-Xylene						CAS #:	95-47-6		
15.488	15.488	(1.063)	106	1240684	25.0000	24.120	80.00-	120.00	100.00
15.488	15.488	(1.063)	91	2526182			178.74-	238.74	203.61

134 Styrene						CAS #:	100-42-5		
15.516	15.516	(1.064)	104	1736719	25.0000	23.686	80.00-	120.00	100.00
15.516	15.516	(1.064)	78	866978			20.27-	80.27	49.92

135 Bromoform						CAS #:	75-25-2		
15.764	15.765	(1.082)	173	1132279	25.0000	25.095	80.00-	120.00	100.00
15.764	15.765	(1.082)	171	579428			20.67-	80.67	51.17

137 Cumene						CAS #:	98-82-8		
15.958	15.958	(1.095)	105	3402095	25.0000	24.198	80.00-	120.00	100.00
15.958	15.958	(1.095)	120	915816			0.00-	30.00	26.92
15.958	15.958	(1.095)	51	322973			0.00-	30.00	9.49

144 1,1,2,2-Tetrachloroethane						CAS #:	79-34-5		
16.456	16.456	(1.129)	83	1774511	25.0000	23.590	80.00-	120.00	100.00
16.456	16.456	(1.129)	85	1091597			31.59-	91.59	61.52

145 Propylbenzene						CAS #:	103-65-1		
16.483	16.484	(1.131)	91	4041657	25.0000	25.100	80.00-	120.00	100.00
16.483	16.484	(1.131)	120	954510			0.00-	30.00	23.62
16.483	16.484	(1.131)	105	145225			0.00-	30.00	3.59

147 4-Ethyltoluene						CAS #:	622-96-8		
16.649	16.649	(1.142)	105	3616568	25.0000	26.197	80.00-	120.00	100.00
16.649	16.649	(1.142)	120	1114974			0.00-	59.85	30.83

148 1,3,5-Trimethylbenzene						CAS #:	108-67-8		
16.732	16.732	(1.148)	105	3346408	25.0000	25.218	80.00-	120.00	100.00
16.732	16.732	(1.148)	120	1670014			0.00-	30.00	49.90

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

153	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
17.147	17.147	(1.176)	105	3467382	25.0000	25.959	80.00- 120.00	100.00	
17.147	17.147	(1.176)	120	1561865			15.22- 75.22	45.04	

156	1,3-Dichlorobenzene					CAS #: 541-73-1			
17.451	17.451	(1.197)	146	2193262	25.0000	25.189	80.00- 120.00	100.00	
17.451	17.451	(1.197)	148	1371901			0.00- 30.00	62.55	
17.451	17.451	(1.197)	111	918858			0.00- 30.00	41.89	

157	1,4-Dichlorobenzene					CAS #: 106-46-7			
17.562	17.562	(1.205)	146	1979487	25.0000	23.988	80.00- 120.00	100.00	
17.562	17.562	(1.205)	148	1208680			0.00- 30.00	61.06	
17.562	17.562	(1.205)	111	686076			0.00- 30.00	34.66	

158	alpha-Chlorotoluene					CAS #: 100-44-7			
17.700	17.700	(1.214)	91	3074757	25.0000	25.634	80.00- 120.00	100.00	
17.700	17.700	(1.214)	126	653675			0.00- 30.00	21.26	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
17.921	17.921	(1.230)	146	1978729	25.0000	23.591	80.00- 120.00	100.00	
17.921	17.921	(1.230)	148	1274964			33.37- 93.37	64.43	
17.921	17.921	(1.230)	111	743013			7.65- 67.65	37.55	

167	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.276	19.276	(1.322)	180	1941314	25.0000	22.900	80.00- 120.00	100.00	
19.276	19.276	(1.322)	182	1852644			64.68- 124.68	95.43	

168	Hexachlorobutadiene					CAS #: 87-68-3			
19.359	19.359	(1.328)	225	1156590	25.0000	23.769	80.00- 120.00	100.00	
19.359	19.359	(1.328)	223	748967			33.22- 93.22	64.76	

169	Naphthalene					CAS #: 91-20-3			
19.469	19.470	(1.336)	128	4917090	25.0000	27.503	80.00- 120.00	100.00	
19.469	19.470	(1.336)	127	601613			0.00- 30.00	12.24	

Report Date: 01-Jun-2007 13:51

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053006.d

Calibration Time: 15:35

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	448309	268985	627633	442807	-1.23
88 1,4-Difluorobenze	2033490	1220094	2846886	2029767	-0.18
125 Chlorobenzene-d5	1524596	914758	2134434	1539410	0.97

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-30may.b/8053006.d
Date: 30-May-2007 15:35
Client ID: Level 4
Sample Info: 25ml #1487-289

Column phase: RTX-624

Instrument: msd8.1
Operator: db
Column diameter: 0.53

/chem/msd8.1/8-30may.b/8053006.d



Report Date: 07-Jun-2007 13:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-07jun.b/8060705.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 07-JUN-2007 11:37
 Operator : JG Inst ID: msd8.i
 Smp Info : 50ml #1443-96
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /chem/msd8.i/8-07jun.b/t14q530b.m
 Meth Date : 07-Jun-2007 13:41 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 11:37 Cal File: 8060705.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp16b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
		CAL-AMT		ON-COL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.387 (1.000)	130	350593 25.0000			80.00-	120.00	100.00	
7.387	7.387 (1.000)	128	255876			42.98-	102.98	72.98	
7.387	7.387 (1.000)	49	499697			112.53-	172.53	142.53	

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267 (1.000)	114	1524282 25.0000			80.00-	120.00	100.00	
9.267	9.267 (1.000)	88	222191			0.00-	44.58	14.58	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576 (1.000)	117	1168126 25.0000			80.00-	120.00	100.00	
14.576	14.576 (1.000)	82	655064			26.08-	86.08	56.08	

1 Freon 152a CAS #: 75-37-6									
1.995	1.995 (0.270)	65	553785 50.0000	45.598		80.00-	120.00	100.00	
2.050	2.050 (0.278)	51	2608865			441.10-	501.10	471.10	

20 Freon123a CAS #: 354-23-4									
3.682	3.682 (0.498)	67	930646 50.0000	49.628		80.00-	120.00	100.00	
3.682	3.682 (0.498)	117	739080			49.42-	109.42	79.42	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
21 Freon123						CAS #: 306-83-2			
3.792	3.792	(0.513)	83	592112	50.0000	50.099	80.00- 120.00	100.00	
3.792	3.792	(0.513)	133	115001			0.00- 49.42	19.42	
3.792	3.792	(0.513)	85	439319			44.20- 104.20	74.20	

38 tert-Butyl-Alcohol						CAS #: 75-65-0			
4.954	4.954	(0.671)	59	1213562	50.0000	49.665	80.00- 120.00	100.00	
4.954	4.954	(0.671)	41	281263			0.00- 53.18	23.18	
4.954	4.954	(0.671)	57	119569			0.00- 39.85	9.85	

49 Isopropyl ether						CAS #: 108-20-3			
5.949	5.949	(0.805)	45	3071363	50.0000	50.259	80.00- 120.00	100.00	
5.949	5.949	(0.805)	87	793048			0.00- 55.82	25.82	
5.949	5.949	(0.805)	59	334819			0.00- 40.90	10.90	

52 1-Propanol						CAS #: 71-23-8			
6.170	6.170	(0.835)	42	208766	50.0000	47.398	80.00- 120.00	100.00	
6.170	6.170	(0.835)	59	279123			103.70- 163.70	133.70	
6.170	6.170	(0.835)	41	166970			49.98- 109.98	79.98	

58 Ethyl-tert-butyl Ether						CAS #: 637-92-3			
6.585	6.585	(0.891)	59	2332280	50.0000	57.162	80.00- 120.00	100.00	
6.585	6.585	(0.891)	87	900443			8.61- 68.61	38.61	
6.585	6.585	(0.891)	41	405190			0.00- 47.37	17.37	

61 Ethyl Acetate						CAS #: 141-78-6			
7.083	7.083	(0.959)	70	262488	50.0000	49.298	80.00- 120.00	100.00	
7.083	7.083	(0.959)	43	2435365			897.80- 957.80	927.80	
7.083	7.083	(0.959)	61	345569			101.65- 161.65	131.65	

78 Isobutanol						CAS #: 78-83-1			
8.437	8.437	(0.910)	43	901547	50.0000	51.531	80.00- 120.00	100.00	
8.437	8.437	(0.910)	41	603783			36.97- 96.97	66.97	

79 tert-amyl-Methyl Ether						CAS #: 994-05-8			
8.631	8.631	(1.168)	73	2090649	50.0000	56.030	80.00- 120.00	100.00	
8.631	8.631	(1.168)	87	519620			0.00- 54.85	24.85	
8.631	8.631	(1.168)	55	584782			0.00- 57.97	27.97	

89 1-Butanol						CAS #: 71-36-3			
9.709	9.709	(1.048)	56	753331	50.0000	50.488	80.00- 120.00	100.00	
9.709	9.709	(1.048)	41	501173			36.53- 96.53	66.53	
9.709	9.709	(1.048)	43	411551			24.63- 84.63	54.63	

136 Cyclohexanone						CAS #: 108-94-1			
16.152	16.152	(1.108)	55	1332835	50.0000	49.854	80.00- 120.00	100.00	

AMOUNTS

RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
136 Cyclohexanone (continued)								
16.152	16.152	(1.108)	98	595161			14.65- 74.65	44.65
16.124	16.124	(1.106)	42	881662			36.15- 96.15	66.15

Report Date: 07-Jun-2007 13:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 07-JUN-2007

Lab File ID: 8060705.d

Calibration Time: 11:37

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd8.i/8-07jun.b/t14q530b.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	350593	210356	490830	350593	0.00
88 1,4-Difluorobenze	1524282	914569	2133995	1524282	0.00
125 Chlorobenzene-d5	1168126	700876	1635376	1168126	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-07jun.b/8060705.d

Date: 07-JUN-2007 11:37

Client ID: Level 5

Sample Info: 50ml #1443-96


Column phase: RTX-624

Instrument: msd8.1

Operator: JG

Column diameter: 0.53

/chem/msd8.1/8-07jun.b/8060705.d



Report Date: 31-May-2007 14:53

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053007.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 30-MAY-2007 16:03
 Operator : db Inst ID: msd8.i
 Smp Info : 50ml #1487-289
 Misc Info : 200ppbv-50ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 31-May-2007 14:53 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 16:03 Cal File: 8053007.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.387	(1.000)	130	441133	25.0000		80.00- 120.00	100.00	
7.387	7.387	(1.000)	128	342185			47.57- 107.57	77.57	
7.387	7.387	(1.000)	49	632872			113.47- 173.47	143.47	

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	1992312	25.0000		80.00- 120.00	100.00	
9.267	9.267	(1.000)	88	312375			0.00- 45.68	15.68	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	1475337	25.0000		80.00- 120.00	100.00	
14.576	14.576	(1.000)	82	860714			28.34- 88.34	58.34	

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.146)	65	557531	25.0000	24.148	80.00- 120.00	100.00	
8.465	8.465	(1.146)	67	334456			29.99- 89.99	59.99	

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	1710823	25.0000	24.804	80.00- 120.00	100.00	
12.115	12.115	(1.307)	70	174905			0.00- 40.22	10.22	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 104 Toluene-d8 (continued)									
12.115	12.115	(1.307)	100	1606916			63.93- 123.93	93.93	

\$ 140 Bromofluorobenzene									
						CAS #: 460-00-4			
16.207	16.207	(1.112)	174	903252	25.0000	25.732	80.00- 120.00	100.00	
16.207	16.207	(1.112)	95	1193763			102.16- 162.16	132.16	
16.207	16.207	(1.112)	176	851833			64.31- 124.31	94.31	

3 Propylene									
						CAS #: 115-07-1			
1.995	1.995	(0.270)	41	1060951	50.0000	44.436	80.00- 120.00	100.00	
1.995	1.995	(0.270)	42	724676			38.30- 98.30	68.30	
1.995	1.995	(0.270)	39	723770			38.22- 98.22	68.22	

4 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
2.050	2.050	(0.278)	85	2666402	50.0000	44.120	80.00- 120.00	100.00	
2.050	2.050	(0.278)	87	867034			2.52- 62.52	32.52	

6 Freon 114									
						CAS #: 76-14-2			
2.161	2.161	(0.293)	135	2656241	50.0000	48.650	80.00- 120.00	100.00	
2.161	2.161	(0.293)	137	837548			1.53- 61.53	31.53	

8 Chloromethane									
						CAS #: 74-87-3			
2.272	2.272	(0.308)	50	1374103	50.0000	49.370	80.00- 120.00	100.00	
2.272	2.272	(0.308)	52	422135			0.72- 60.72	30.72	

9 Butane									
						CAS #: 106-97-8			
2.327	2.327	(0.315)	58	346263	50.0000	47.638	80.00- 120.00	100.00	
2.327	2.327	(0.315)	43	2556532			708.32- 768.32	738.32	

11 Vinyl Chloride									
						CAS #: 75-01-4			
2.410	2.410	(0.326)	62	1538485	50.0000	47.571	80.00- 120.00	100.00	
2.410	2.410	(0.326)	64	484291			1.48- 61.48	31.48	

10 1,3-Butadiene									
						CAS #: 106-99-0			
2.382	2.382	(0.322)	54	1245393	50.0000	45.019	80.00- 120.00	100.00	
2.382	2.382	(0.322)	39	1201450			66.47- 126.47	96.47	

13 Bromomethane									
						CAS #: 74-83-9			
2.852	2.852	(0.386)	94	1081074	50.0000	50.035	80.00- 120.00	100.00	
2.852	2.852	(0.386)	96	1027301			65.03- 125.03	95.03	

16 Chloroethane									
						CAS #: 75-00-3			
2.963	2.963	(0.401)	64	835185	50.0000	48.795	80.00- 120.00	100.00	
2.963	2.963	(0.401)	49	206572			0.00- 54.73	24.73	
2.963	2.963	(0.401)	66	259149			1.03- 61.03	31.03	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
15 Isopentane						CAS #: 78-78-4			
2.963	2.963	(0.401)	43	1993575	50.0000	49.367	80.00- 120.00	100.00	
2.963	2.963	(0.401)	57	1377018			39.07- 99.07	69.07	
2.963	2.963	(0.401)	72	149398			0.00- 37.49	7.49	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.212	3.212	(0.435)	101	3338623	50.0000	48.602	80.00- 120.00	100.00	
3.212	3.212	(0.435)	103	2168945			34.97- 94.97	64.97	

23 Ethanol						CAS #: 64-17-5			
3.516	3.516	(0.476)	45	536367	50.0000	48.898	80.00- 120.00	100.00	
3.516	3.516	(0.476)	43	110348			0.00- 50.57	20.57	
3.516	3.516	(0.476)	46	225695			12.08- 72.08	42.08	

28 Freon 113						CAS #: 76-13-1			
3.931	3.931	(0.532)	151	2144041	50.0000	47.174	80.00- 120.00	100.00	
3.931	3.931	(0.532)	153	1365964			33.71- 93.71	63.71	
3.931	3.931	(0.532)	101	2494396			86.34- 146.34	116.34	

29 1,1-Dichloroethene						CAS #: 75-35-4			
3.958	3.958	(0.536)	61	2147006	50.0000	47.567	80.00- 120.00	100.00	
3.958	3.958	(0.536)	96	1297826			30.45- 90.45	60.45	
3.958	3.958	(0.536)	98	824285			8.39- 68.39	38.39	

30 Acetone						CAS #: 67-64-1			
4.124	4.124	(0.558)	58	743587	50.0000	49.188	80.00- 120.00	100.00	
4.124	4.124	(0.558)	43	2174812			262.48- 322.48	292.48	

33 Carbon Disulfide						CAS #: 75-15-0			
4.290	4.290	(0.581)	76	4010765	50.0000	47.413	80.00- 120.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
4.318	4.318	(0.584)	45	2611678	50.0000	47.782	80.00- 120.00	100.00	
4.318	4.318	(0.584)	43	497434			0.00- 49.05	19.05	
4.318	4.318	(0.584)	59	105698			0.00- 34.05	4.05	

37 3-Chloropropene						CAS #: 107-05-1			
4.566	4.566	(0.618)	76	692146	50.0000	51.289	80.00- 120.00	100.00	
4.566	4.566	(0.618)	41	2087482			271.60- 331.60	301.60	

40 Methylene Chloride						CAS #: 75-09-2			
4.815	4.815	(0.652)	49	1613264	50.0000	47.741	80.00- 120.00	100.00	
4.815	4.815	(0.652)	84	1145605			41.01- 101.01	71.01	
4.815	4.815	(0.652)	51	477098			0.00- 59.57	29.57	

43 MTBE						CAS #: 1634-04-4			
5.147	5.147	(0.697)	73	2615636	50.0000	54.425	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
43 MTBE (continued)									
5.147	5.147	(0.697)	57	623120			0.00- 53.82	23.82	
5.147	5.147	(0.697)	41	585377			0.00- 52.38	22.38	

45 trans-1,2-Dichloroethene					CAS #: 156-60-5				
5.175	5.175	(0.701)	96	1487814	50.0000	46.583	80.00- 120.00	100.00	
5.175	5.175	(0.701)	61	2217443			119.04- 179.04	149.04	
5.202	5.202	(0.704)	98	952041			33.99- 93.99	63.99	

46 Hexane					CAS #: 110-54-3				
5.534	5.534	(0.749)	57	2496765	50.0000	51.542	80.00- 120.00	100.00	
5.534	5.534	(0.749)	43	1570026			32.88- 92.88	62.88	
5.534	5.534	(0.749)	86	367327			0.00- 44.71	14.71	

54 1,1-Dichloroethane					CAS #: 75-34-3				
5.949	5.949	(0.805)	63	2554528	50.0000	49.064	80.00- 120.00	100.00	
5.949	5.949	(0.805)	65	797507			1.22- 61.22	31.22	

55 Vinyl Acetate					CAS #: 108-05-4				
6.032	6.032	(0.817)	86	355502	50.0000	48.367	80.00- 120.00	100.00	
6.032	6.032	(0.817)	43	3900404			1067.15-1127.15	1097.15	
6.032	6.032	(0.817)	42	297238			53.61- 113.61	83.61	

64 cis-1,2-Dichloroethene					CAS #: 156-59-2				
6.972	6.972	(0.944)	61	1890254	50.0000	45.872	80.00- 120.00	100.00	
6.972	6.972	(0.944)	96	1419326			45.09- 105.09	75.09	
6.972	6.972	(0.944)	98	900856			17.66- 77.66	47.66	

65 2-Butanone					CAS #: 78-93-3				
7.027	7.027	(0.951)	72	682086	50.0000	46.657	80.00- 120.00	100.00	
7.027	7.027	(0.951)	43	2923118			398.56- 458.56	428.56	
7.027	7.027	(0.951)	57	230736			3.83- 63.83	33.83	

67 Tetrahydrofuran					CAS #: 109-99-9				
7.387	7.387	(1.000)	42	1794674	50.0000	47.230	80.00- 120.00	100.00	
7.387	7.387	(1.000)	71	630736			5.14- 65.14	35.14	
7.387	7.387	(1.000)	72	683952			8.11- 68.11	38.11	

70 Chloroform					CAS #: 67-66-3				
7.525	7.525	(1.019)	83	2510438	50.0000	48.212	80.00- 120.00	100.00	
7.525	7.525	(1.019)	85	1556022			31.98- 91.98	61.98	

73 Cyclohexane					CAS #: 110-82-7				
7.746	7.746	(1.049)	84	2021584	50.0000	46.792	80.00- 120.00	100.00	
7.746	7.746	(1.049)	56	2613838			99.30- 159.30	129.30	
7.746	7.746	(1.049)	41	1290550			33.84- 93.84	63.84	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

75	1,1,1-Trichloroethane					CAS #:	71-55-6			
7.774	7.774	(1.052)	97	2602285	50.0000	47.697	80.00-	120.00	100.00	
7.774	7.774	(1.052)	99	1684374			34.73-	94.73	64.73	

77	Carbon Tetrachloride					CAS #:	56-23-5			
7.995	7.995	(1.082)	119	2509316	50.0000	50.544	80.00-	120.00	100.00	
7.995	7.995	(1.082)	117	2610640			74.04-	134.04	104.04	

81	Benzene					CAS #:	71-43-2			
8.437	8.437	(0.910)	78	4299343	50.0000	47.769	80.00-	120.00	100.00	
8.437	8.437	(0.910)	77	953019			0.00-	52.17	22.17	

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
8.465	8.465	(1.146)	57	6116976	50.0000	47.428	80.00-	120.00	100.00	
8.465	8.465	(1.146)	56	1934694			1.63-	61.63	31.63	
8.465	8.465	(1.146)	41	1435732			0.00-	53.47	23.47	

83	1,2-Dichloroethane					CAS #:	107-06-2			
8.603	8.603	(0.928)	62	1714995	50.0000	46.965	80.00-	120.00	100.00	
8.603	8.603	(0.928)	64	541369			1.57-	61.57	31.57	

85	Heptane					CAS #:	142-82-5			
8.852	8.852	(0.955)	100	425691	50.0000	43.706	80.00-	120.00	100.00	
8.852	8.852	(0.955)	43	2479146			552.38-	612.38	582.38	
8.852	8.852	(0.955)	71	1375573			293.14-	353.14	323.14	

94	Trichloroethene					CAS #:	79-01-6			
9.682	9.682	(1.045)	95	1701628	50.0000	47.708	80.00-	120.00	100.00	
9.682	9.682	(1.045)	130	1834985			77.84-	137.84	107.84	
9.682	9.682	(1.045)	97	1092814			34.22-	94.22	64.22	

95	Methyl Cyclohexane					CAS #:	108-87-2			
9.903	9.903	(1.341)	83	2612830	50.0000	48.544	80.00-	120.00	100.00	
9.903	9.903	(1.341)	98	1224638			16.87-	76.87	46.87	
9.903	9.903	(1.341)	55	2044095			48.23-	108.23	78.23	

97	1,2-Dichloropropane					CAS #:	78-87-5			
10.179	10.179	(1.098)	63	1486513	50.0000	47.658	80.00-	120.00	100.00	
10.179	10.179	(1.098)	62	1072565			42.15-	102.15	72.15	
10.179	10.179	(1.098)	41	839449			26.47-	86.47	56.47	

98	1,4-Dioxane					CAS #:	123-91-1			
10.428	10.428	(1.125)	88	944170	50.0000	49.629	80.00-	120.00	100.00	
10.428	10.428	(1.125)	58	698982			44.03-	104.03	74.03	
10.428	10.428	(1.125)	57	215615			0.00-	52.84	22.84	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	CAL-AMT		ON-COL	TARGET RANGE	RATIO		
				RESPONSE	(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	

100	Bromodichloromethane					CAS #:	75-27-4			
10.732	10.732	(1.158)	83	2547396	50.0000	48.899	80.00-	120.00	100.00	
10.732	10.732	(1.158)	85	1554700			31.03-	91.03	61.03	

102	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
11.672	11.672	(1.260)	75	2114572	50.0000	48.783	80.00-	120.00	100.00	
11.672	11.672	(1.260)	77	659599			1.19-	61.19	31.19	
11.672	11.672	(1.260)	39	992332			16.93-	76.93	46.93	

103	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.032	12.032	(1.298)	58	1183517	50.0000	50.470	80.00-	120.00	100.00	
12.032	12.032	(1.298)	43	2867386			212.28-	272.28	242.28	
12.032	12.032	(1.298)	85	492895			11.65-	71.65	41.65	

105	Toluene					CAS #:	108-88-3			
12.253	12.253	(1.322)	91	4422713	50.0000	48.350	80.00-	120.00	100.00	
12.253	12.253	(1.322)	92	2673976			30.46-	90.46	60.46	

108	trans-1,3-Dichloropropene					CAS #:	10061-02-6			
12.834	12.834	(0.880)	75	2149165	50.0000	50.248	80.00-	120.00	100.00	
12.834	12.834	(0.880)	77	647075			0.11-	60.11	30.11	
12.834	12.834	(0.880)	39	983279			15.75-	75.75	45.75	

110	1,1,2-Trichloroethane					CAS #:	79-00-5			
13.138	13.138	(0.901)	97	1477573	50.0000	47.104	80.00-	120.00	100.00	
13.138	13.138	(0.901)	99	908334			31.47-	91.47	61.47	
13.138	13.138	(0.901)	83	1303964			58.25-	118.25	88.25	

112	Tetrachloroethene					CAS #:	127-18-4			
13.193	13.193	(0.905)	166	2055564	50.0000	48.417	80.00-	120.00	100.00	
13.193	13.193	(0.905)	129	1560241			45.90-	105.90	75.90	
13.193	13.193	(0.905)	131	1518741			43.88-	103.88	73.88	

114	2-Hexanone					CAS #:	591-78-6			
13.580	13.580	(0.932)	58	1624483	50.0000	52.265	80.00-	120.00	100.00	
13.580	13.580	(0.932)	43	2875801			147.03-	207.03	177.03	
13.580	13.580	(0.932)	100	334216			0.00-	50.57	20.57	

116	Dibromochloromethane					CAS #:	124-48-1			
13.718	13.718	(0.941)	129	2439103	50.0000	49.615	80.00-	120.00	100.00	
13.718	13.718	(0.941)	127	1880746			47.11-	107.11	77.11	

117	1,2-Dibromoethane					CAS #:	106-93-4			
13.884	13.884	(0.953)	107	2349832	50.0000	49.163	80.00-	120.00	100.00	
13.884	13.884	(0.953)	109	2236461			65.18-	125.18	95.18	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
126 Chlorobenzene						CAS #:	108-90-7			
14.631	14.631	(1.004)	112	3693405	50.0000	48.755	80.00-	120.00	100.00	
14.631	14.631	(1.004)	114	1178415			1.91-	61.91	31.91	
14.603	14.603	(1.002)	77	2086900			26.50-	86.50	56.50	

129 Ethyl Benzene						CAS #:	100-41-4			
14.769	14.769	(1.013)	106	1897967	50.0000	47.343	80.00-	120.00	100.00	
14.769	14.769	(1.013)	91	5944387			283.20-	343.20	313.20	

130 m,p-Xylene						CAS #:	108-38-3			
14.935	14.935	(1.025)	106	2397145	50.0000	49.069	80.00-	120.00	100.00	
14.935	14.935	(1.025)	91	4593983			161.64-	221.64	191.64	

132 o-Xylene						CAS #:	95-47-6			
15.488	15.488	(1.063)	106	2399345	50.0000	48.671	80.00-	120.00	100.00	
15.488	15.488	(1.063)	91	4977982			177.47-	237.47	207.47	

134 Styrene						CAS #:	100-42-5			
15.516	15.516	(1.064)	104	3513401	50.0000	49.997	80.00-	120.00	100.00	
15.516	15.516	(1.064)	78	1765544			20.25-	80.25	50.25	

135 Bromoform						CAS #:	75-25-2			
15.764	15.764	(1.082)	173	2267799	50.0000	52.444	80.00-	120.00	100.00	
15.764	15.764	(1.082)	171	1157789			21.05-	81.05	51.05	

137 Cumene						CAS #:	98-82-8			
15.958	15.958	(1.095)	105	6732590	50.0000	49.967	80.00-	120.00	100.00	
15.958	15.958	(1.095)	120	1777182			0.00-	56.40	26.40	
15.958	15.958	(1.095)	51	616754			0.00-	39.16	9.16	

144 1,1,2,2-Tetrachloroethane						CAS #:	79-34-5			
16.456	16.456	(1.129)	83	3534141	50.0000	49.023	80.00-	120.00	100.00	
16.456	16.456	(1.129)	85	2190780			31.99-	91.99	61.99	

145 Propylbenzene						CAS #:	103-65-1			
16.483	16.483	(1.131)	91	8126384	50.0000	52.659	80.00-	120.00	100.00	
16.483	16.483	(1.131)	120	1859596			0.00-	52.88	22.88	
16.483	16.483	(1.131)	105	291527			0.00-	33.59	3.59	

147 4-Ethyltoluene						CAS #:	622-96-8			
16.649	16.649	(1.142)	105	7105769	50.0000	53.707	80.00-	120.00	100.00	
16.649	16.649	(1.142)	120	2103349			0.00-	59.60	29.60	

148 1,3,5-Trimethylbenzene						CAS #:	108-67-8			
16.732	16.732	(1.148)	105	6609789	50.0000	51.974	80.00-	120.00	100.00	
16.732	16.732	(1.148)	120	3263943			19.38-	79.38	49.38	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

153	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
17.147	17.147	(1.176)	105	6904880	50.0000	53.940	80.00- 120.00	100.00	
17.147	17.147	(1.176)	120	3135375			15.41- 75.41	45.41	

156	1,3-Dichlorobenzene					CAS #: 541-73-1			
17.451	17.451	(1.197)	146	4379647	50.0000	52.483	80.00- 120.00	100.00	
17.451	17.451	(1.197)	148	2790179			33.71- 93.71	63.71	
17.451	17.451	(1.197)	111	1812557			11.39- 71.39	41.39	

157	1,4-Dichlorobenzene					CAS #: 106-46-7			
17.562	17.562	(1.205)	146	3953538	50.0000	49.990	80.00- 120.00	100.00	
17.562	17.562	(1.205)	148	2487194			32.91- 92.91	62.91	
17.562	17.562	(1.205)	111	1393312			5.24- 65.24	35.24	

158	alpha-Chlorotoluene					CAS #: 100-44-7			
17.700	17.700	(1.214)	91	6430403	50.0000	55.937	80.00- 120.00	100.00	
17.700	17.700	(1.214)	126	1298111			0.00- 50.19	20.19	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
17.921	17.921	(1.230)	146	3963669	50.0000	49.308	80.00- 120.00	100.00	
17.921	17.921	(1.230)	148	2485367			32.70- 92.70	62.70	
17.921	17.921	(1.230)	111	1469135			7.07- 67.07	37.07	

167	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.276	19.276	(1.322)	180	4243469	50.0000	52.231	80.00- 120.00	100.00	
19.276	19.276	(1.322)	182	4039439			65.19- 125.19	95.19	

168	Hexachlorobutadiene					CAS #: 87-68-3			
19.359	19.359	(1.328)	225	2274747	50.0000	48.779	80.00- 120.00	100.00	
19.359	19.359	(1.328)	223	1438980			33.26- 93.26	63.26	

169	Naphthalene					CAS #: 91-20-3			
19.470	19.470	(1.336)	128	10653699	50.0000	62.178	80.00- 120.00	100.00	
19.470	19.470	(1.336)	127	1203008			0.00- 41.29	11.29	

Report Date: 31-May-2007 14:53

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053007.d

Calibration Time: 16:03

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	441133	264680	617586	441133	0.00
88 1,4-Difluorobenze	1992312	1195387	2789237	1992312	0.00
125 Chlorobenzene-d5	1475337	885202	2065472	1475337	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-30may.b/8053007.d
Date: 30-May-2007 16:03
Client ID: Level 5
Sample Info: 50ml #1487-289

Column phase: RTX-624

Instrument: msd8.1
Operator: db
Column diameter: 0.53

/chem/msd8.1/8-30may.b/8053007.d



Report Date: 31-May-2007 14:53

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053008.d
 Lab Smp Id: ICAL Client Smp ID: Level 6
 Inj Date : 30-MAY-2007 16:31
 Operator : db Inst ID: msd8.i
 Smp Info : 100ml #1487-289
 Misc Info : 200ppbv-100ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 31-May-2007 14:53 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 16:31 Cal File: 8053008.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5									
7.387	7.387	(1.000)	130	456242	25.0000			70.00- 130.00	100.00
7.387	7.387	(1.000)	128	338679				47.57- 107.57	74.23
7.387	7.387	(1.000)	49	641995				113.47- 173.47	140.71

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	2079239	25.0000			70.00- 130.00	100.00
9.267	9.267	(1.000)	88	315764				0.00- 45.68	15.19

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	1515229	25.0000			70.00- 130.00	100.00
14.576	14.576	(1.000)	82	883171				0.00- 30.00	58.29

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.146)	65	611646	25.0000	25.615		70.00- 130.00	100.00
8.465	8.465	(1.146)	67	381750				0.00- 30.00	62.41

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	1771106	25.0000	24.605		70.00- 130.00	100.00
12.115	12.115	(1.307)	70	167250				0.00- 30.00	9.44

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 104 Toluene-d8 (continued)										
12.115	12.115	(1.307)	100	1418894			0.00- 30.00	80.11		

\$ 140 Bromofluorobenzene										
						CAS #: 460-00-4				
16.207	16.207	(1.112)	174	936709	25.0000	25.982	70.00- 130.00	100.00		
16.207	16.207	(1.112)	95	1233267			102.16- 162.16	131.66		
16.207	16.207	(1.112)	176	887102			64.31- 124.31	94.70		

3 Propylene						CAS #: 115-07-1				
1.995	1.995	(0.270)	41	2111882	100.000	85.522	70.00- 130.00	100.00		
1.995	1.995	(0.270)	42	1405317			0.00- 30.00	66.54		
1.995	1.995	(0.270)	39	1426212			0.00- 30.00	67.53		

4 Dichlorodifluoromethane/Fr12						CAS #: 75-71-8				
2.050	2.050	(0.278)	85	5440637	100.000	87.042	70.00- 130.00	100.00		
2.050	2.050	(0.278)	87	1735219			0.00- 30.00	31.89		

6 Freon 114						CAS #: 76-14-2				
2.161	2.161	(0.293)	135	5255420	100.000	93.067	70.00- 130.00	100.00		
2.161	2.161	(0.293)	137	1643521			1.53- 61.53	31.27		

8 Chloromethane						CAS #: 74-87-3				
2.272	2.272	(0.308)	50	2731679	100.000	94.896	70.00- 130.00	100.00		
2.272	2.272	(0.308)	52	810595			0.00- 30.00	29.67		

9 Butane						CAS #: 106-97-8				
2.327	2.327	(0.315)	58	666073	100.000	88.601	70.00- 130.00	100.00		
2.327	2.327	(0.315)	43	5010913			0.00- 30.00	752.31		

11 Vinyl Chloride						CAS #: 75-01-4				
2.410	2.410	(0.326)	62	2979171	100.000	89.067	70.00- 130.00	100.00		
2.410	2.410	(0.326)	64	906402			0.00- 30.00	30.42		

10 1,3-Butadiene						CAS #: 106-99-0				
2.410	2.410	(0.326)	54	2379256	100.000	83.158	70.00- 130.00	100.00		
2.382	2.382	(0.322)	39	2438472			0.00- 30.00	102.49		

13 Bromomethane						CAS #: 74-83-9				
2.852	2.852	(0.386)	94	2174749	100.000	97.320	70.00- 130.00	100.00		
2.852	2.852	(0.386)	96	2040837			65.03- 125.03	93.84		

16 Chloroethane						CAS #: 75-00-3				
2.963	2.963	(0.401)	64	1587282	100.000	89.665	70.00- 130.00	100.00		
2.963	2.963	(0.401)	49	396910			0.00- 30.00	25.01		
2.963	2.963	(0.401)	66	488935			0.00- 30.00	30.80		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

15 Isopentane						CAS #: 78-78-4			
2.963	2.963	(0.401)	43	3971363	100.000	95.086	70.00- 130.00	100.00	
2.963	2.963	(0.401)	57	2686310			0.00- 30.00	67.64	
2.963	2.963	(0.401)	72	284025			0.00- 30.00	7.15	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.212	3.212	(0.435)	101	6617115	100.000	93.139	70.00- 130.00	100.00	
3.212	3.212	(0.435)	103	4259322			34.97- 94.97	64.37	

23 Ethanol						CAS #: 64-17-5			
3.543	3.543	(0.480)	45	1062280	100.000	93.635	70.00- 130.00	100.00	
3.516	3.516	(0.476)	43	191015			0.00- 30.00	17.98	
3.516	3.516	(0.476)	46	431356			0.00- 30.00	40.61	

28 Freon 113						CAS #: 76-13-1			
3.930	3.930	(0.532)	151	4294641	100.000	91.363	70.00- 130.00	100.00	
3.930	3.930	(0.532)	153	2715258			33.71- 93.71	63.22	
3.930	3.930	(0.532)	101	5038552			86.34- 146.34	117.32	

29 1,1-Dichloroethene						CAS #: 75-35-4			
3.958	3.958	(0.536)	61	4286913	100.000	91.832	70.00- 130.00	100.00	
3.958	3.958	(0.536)	96	2549826			30.45- 90.45	59.48	
3.958	3.958	(0.536)	98	1633650			8.39- 68.39	38.11	

30 Acetone						CAS #: 67-64-1			
4.124	4.124	(0.558)	58	1456647	100.000	93.167	70.00- 130.00	100.00	
4.124	4.124	(0.558)	43	4343030			0.00- 30.00	298.15	

33 Carbon Disulfide						CAS #: 75-15-0			
4.290	4.290	(0.581)	76	8061972	100.000	92.149	70.00- 130.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
4.318	4.318	(0.584)	45	5257774	100.000	93.009	70.00- 130.00	100.00	
4.318	4.318	(0.584)	43	986622			0.00- 30.00	18.77	
4.318	4.318	(0.584)	59	208508			0.00- 30.00	3.97	

37 3-Chloropropene						CAS #: 107-05-1			
4.566	4.566	(0.618)	76	1354721	100.000	97.062	70.00- 130.00	100.00	
4.566	4.566	(0.618)	41	4132615			0.00- 30.00	305.05	

40 Methylene Chloride						CAS #: 75-09-2			
4.815	4.815	(0.652)	49	3152614	100.000	90.205	70.00- 130.00	100.00	
4.815	4.815	(0.652)	84	2300704			41.01- 101.01	72.98	
4.815	4.815	(0.652)	51	949529			0.00- 30.00	30.12	

43 MTBE						CAS #: 1634-04-4			
5.147	5.147	(0.697)	73	5123497	100.000	103.08	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
43 MTBE (continued)									
5.147	5.147	(0.697)	57	1222306			0.00- 53.82	23.86	
5.147	5.147	(0.697)	41	1170037			0.00- 30.00	22.84	

45 trans-1,2-Dichloroethene					CAS #: 156-60-5				
5.175	5.175	(0.701)	96	2948613	100.000	89.263	70.00- 130.00	100.00	
5.175	5.175	(0.701)	61	4422228			119.04- 179.04	149.98	
5.175	5.175	(0.701)	98	1894246			0.00- 30.00	64.24	

46 Hexane					CAS #: 110-54-3				
5.534	5.534	(0.749)	57	4711392	100.000	94.039	70.00- 130.00	100.00	
5.534	5.534	(0.749)	43	2957338			0.00- 30.00	62.77	
5.534	5.534	(0.749)	86	725012			0.00- 30.00	15.39	

54 1,1-Dichloroethane					CAS #: 75-34-3				
5.949	5.949	(0.805)	63	5084008	100.000	94.412	70.00- 130.00	100.00	
5.949	5.949	(0.805)	65	1596380			1.22- 61.22	31.40	

55 Vinyl Acetate					CAS #: 108-05-4				
6.032	6.032	(0.817)	86	761982	100.000	100.24	70.00- 130.00	100.00	
6.032	6.032	(0.817)	43	8054687			0.00- 30.00	1057.07	
6.032	6.032	(0.817)	42	616418			0.00- 30.00	80.90	

64 cis-1,2-Dichloroethene					CAS #: 156-59-2				
6.972	6.972	(0.944)	61	3773397	100.000	88.539	70.00- 130.00	100.00	
6.972	6.972	(0.944)	96	2782950			45.09- 105.09	73.75	
6.972	6.972	(0.944)	98	1774497			17.66- 77.66	47.03	

65 2-Butanone					CAS #: 78-93-3				
7.027	7.027	(0.951)	72	1390585	100.000	91.971	70.00- 130.00	100.00	
7.027	7.027	(0.951)	43	5954215			398.56- 458.56	428.18	
7.027	7.027	(0.951)	57	451831			0.00- 30.00	32.49	

67 Tetrahydrofuran					CAS #: 109-99-9				
7.387	7.387	(1.000)	42	3522933	100.000	89.642	70.00- 130.00	100.00	
7.387	7.387	(1.000)	71	1272954			5.14- 65.14	36.13	
7.387	7.387	(1.000)	72	1374375			0.00- 30.00	39.01	

70 Chloroform					CAS #: 67-66-3				
7.525	7.525	(1.019)	83	4994804	100.000	92.746	70.00- 130.00	100.00	
7.525	7.525	(1.019)	85	3098846			31.98- 91.98	62.04	

73 Cyclohexane					CAS #: 110-82-7				
7.746	7.746	(1.049)	84	4057695	100.000	90.810	70.00- 130.00	100.00	
7.746	7.746	(1.049)	56	5201149			99.30- 159.30	128.18	
7.746	7.746	(1.049)	41	2605789			33.84- 93.84	64.22	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

75	1,1,1-Trichloroethane					CAS #:	71-55-6			
7.774	7.774	(1.052)	97	5240694	100.000	92.876	70.00-	130.00	100.00	
7.774	7.774	(1.052)	99	3350182			34.73-	94.73	63.93	

77	Carbon Tetrachloride					CAS #:	56-23-5			
7.995	7.995	(1.082)	119	5107823	100.000	99.478	70.00-	130.00	100.00	
7.995	7.995	(1.082)	117	5255553			74.04-	134.04	102.89	

81	Benzene					CAS #:	71-43-2			
8.437	8.437	(0.910)	78	8696555	100.000	92.587	70.00-	130.00	100.00	
8.437	8.437	(0.910)	77	1944596			0.00-	30.00	22.36	

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
8.465	8.465	(1.146)	57	12520618	100.000	93.863	70.00-	130.00	100.00	
8.465	8.465	(1.146)	56	3975572			0.00-	30.00	31.75	
8.465	8.465	(1.146)	41	2931448			0.00-	30.00	23.41	

83	1,2-Dichloroethane					CAS #:	107-06-2			
8.603	8.603	(0.928)	62	3438647	100.000	90.230	70.00-	130.00	100.00	
8.603	8.603	(0.928)	64	1083383			0.00-	30.00	31.51	

85	Heptane					CAS #:	142-82-5			
8.852	8.852	(0.955)	100	862354	100.000	84.838	70.00-	130.00	100.00	
8.852	8.852	(0.955)	43	4963883			0.00-	30.00	575.62	
8.852	8.852	(0.955)	71	2771790			0.00-	30.00	321.42	

94	Trichloroethene					CAS #:	79-01-6			
9.682	9.682	(1.045)	95	3411326	100.000	91.643	70.00-	130.00	100.00	
9.682	9.682	(1.045)	130	3669068			77.84-	137.84	107.56	
9.682	9.682	(1.045)	97	2155039			34.22-	94.22	63.17	

95	Methyl Cyclohexane					CAS #:	108-87-2			
9.903	9.903	(1.341)	83	5261578	100.000	94.518	70.00-	130.00	100.00	
9.903	9.903	(1.341)	98	2392828			0.00-	30.00	45.48	
9.903	9.903	(1.341)	55	4199922			0.00-	30.00	79.82	

97	1,2-Dichloropropane					CAS #:	78-87-5			
10.179	10.179	(1.098)	63	3003131	100.000	92.255	70.00-	130.00	100.00	
10.179	10.179	(1.098)	62	2137034			42.15-	102.15	71.16	
10.179	10.179	(1.098)	41	1697497			26.47-	86.47	56.52	

98	1,4-Dioxane					CAS #:	123-91-1			
10.428	10.428	(1.125)	88	1913662	100.000	96.383	70.00-	130.00	100.00	
10.428	10.428	(1.125)	58	1398870			44.03-	104.03	73.10	
10.428	10.428	(1.125)	57	419838			0.00-	30.00	21.94	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

100	Bromodichloromethane					CAS #:	75-27-4			
10.732	10.732	(1.158)	83	5128594	100.000	94.331	70.00- 130.00	100.00		
10.732	10.732	(1.158)	85	3168965			31.03- 91.03	61.79		

102	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
11.672	11.672	(1.260)	75	4289445	100.000	94.820	70.00- 130.00	100.00		
11.672	11.672	(1.260)	77	1336780			1.19- 61.19	31.16		
11.672	11.672	(1.260)	39	1995148			16.93- 76.93	46.51		

103	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.032	12.032	(1.298)	58	2412926	100.000	98.595	70.00- 130.00	100.00		
12.032	12.032	(1.298)	43	5915330			0.00- 30.00	245.15		
12.032	12.032	(1.298)	85	996247			0.00- 30.00	41.29		

105	Toluene					CAS #:	108-88-3			
12.253	12.253	(1.322)	91	9100045	100.000	95.324	70.00- 130.00	100.00		
12.253	12.253	(1.322)	92	5435801			30.46- 90.46	59.73		

108	trans-1,3-Dichloropropene					CAS #:	10061-02-6			
12.834	12.834	(0.880)	75	4335904	100.000	98.705	70.00- 130.00	100.00		
12.834	12.834	(0.880)	77	1335466			0.11- 60.11	30.80		
12.834	12.834	(0.880)	39	2001936			15.75- 75.75	46.17		

110	1,1,2-Trichloroethane					CAS #:	79-00-5			
13.138	13.138	(0.901)	97	2964497	100.000	92.018	70.00- 130.00	100.00		
13.138	13.138	(0.901)	99	1840259			31.47- 91.47	62.08		
13.138	13.138	(0.901)	83	2551394			58.25- 118.25	86.06		

112	Tetrachloroethene					CAS #:	127-18-4			
13.193	13.193	(0.905)	166	4186065	100.000	96.002	70.00- 130.00	100.00		
13.193	13.193	(0.905)	129	3258954			45.90- 105.90	77.85		
13.193	13.193	(0.905)	131	3031301			43.88- 103.88	72.41		

114	2-Hexanone					CAS #:	591-78-6			
13.580	13.580	(0.932)	58	3291331	100.000	103.10	70.00- 130.00	100.00		
13.580	13.580	(0.932)	43	6040547			147.03- 207.03	183.53		
13.580	13.580	(0.932)	100	705295			0.00- 30.00	21.43		

116	Dibromochloromethane					CAS #:	124-48-1			
13.718	13.718	(0.941)	129	5095518	100.000	100.92	70.00- 130.00	100.00		
13.718	13.718	(0.941)	127	3903792			0.00- 30.00	76.61		

117	1,2-Dibromoethane					CAS #:	106-93-4			
13.884	13.884	(0.953)	107	4784702	100.000	97.469	70.00- 130.00	100.00		
13.884	13.884	(0.953)	109	4502499			65.18- 125.18	94.10		

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
126 Chlorobenzene						CAS #:	108-90-7	
14.631	14.631	(1.004)	112	7575451	100.000	97.367	70.00- 130.00	100.00
14.631	14.631	(1.004)	114	2379711			1.91- 61.91	31.41
14.603	14.603	(1.002)	77	4237044			26.50- 86.50	55.93

129 Ethyl Benzene						CAS #:	100-41-4	
14.769	14.769	(1.013)	106	3943287	100.000	95.771	70.00- 130.00	100.00
14.769	14.769	(1.013)	91	12558154			0.00- 30.00	318.47

130 m,p-Xylene						CAS #:	108-38-3	
14.935	14.935	(1.025)	106	4928477	100.000	98.229	70.00- 130.00	100.00
14.935	14.935	(1.025)	91	9732569			0.00- 30.00	197.48

132 o-Xylene						CAS #:	95-47-6	
15.488	15.488	(1.063)	106	4858089	100.000	95.953	70.00- 130.00	100.00
15.488	15.488	(1.063)	91	10291979			177.47- 237.47	211.85

134 Styrene						CAS #:	100-42-5	
15.516	15.516	(1.064)	104	7423994	100.000	102.86	70.00- 130.00	100.00
15.516	15.516	(1.064)	78	3649528			20.25- 80.25	49.16

135 Bromoform						CAS #:	75-25-2	
15.764	15.764	(1.082)	173	4754269	100.000	107.05	70.00- 130.00	100.00
15.764	15.764	(1.082)	171	2426878			21.05- 81.05	51.05

137 Cumene						CAS #:	98-82-8	
15.958	15.958	(1.095)	105	14013350	100.000	101.26	70.00- 130.00	100.00
15.958	15.958	(1.095)	120	3600114			0.00- 30.00	25.69
15.958	15.958	(1.095)	51	1268255			0.00- 30.00	9.05

144 1,1,2,2-Tetrachloroethane						CAS #:	79-34-5	
16.456	16.456	(1.129)	83	7218673	100.000	97.495	70.00- 130.00	100.00
16.456	16.456	(1.129)	85	4420519			31.99- 91.99	61.24

145 Propylbenzene						CAS #:	103-65-1	
16.483	16.483	(1.131)	91	16975123	100.000	107.10	70.00- 130.00	100.00
16.483	16.483	(1.131)	120	3752339			0.00- 30.00	22.10
16.483	16.483	(1.131)	105	582164			0.00- 30.00	3.43

147 4-Ethyltoluene						CAS #:	622-96-8	
16.649	16.649	(1.142)	105	14848016	100.000	109.27	70.00- 130.00	100.00
16.649	16.649	(1.142)	120	4383266			0.00- 59.60	29.52

148 1,3,5-Trimethylbenzene						CAS #:	108-67-8	
16.732	16.732	(1.148)	105	13957272	100.000	106.86	70.00- 130.00	100.00
16.732	16.732	(1.148)	120	6759537			0.00- 30.00	48.43

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

153	17.147	17.147 (1.176)	105	14463263	100.000	110.01	70.00- 130.00	100.00	
	17.147	17.147 (1.176)	120	6341397			15.41- 75.41	43.84	

156	17.451	17.451 (1.197)	146	9209832	100.000	107.46	70.00- 130.00	100.00	
	17.451	17.451 (1.197)	148	5794867			0.00- 30.00	62.92	
	17.451	17.451 (1.197)	111	3806522			0.00- 30.00	41.33	

157	17.562	17.562 (1.205)	146	8545658	100.000	105.21	70.00- 130.00	100.00	
	17.562	17.562 (1.205)	148	5364507			0.00- 30.00	62.77	
	17.562	17.562 (1.205)	111	2979869			0.00- 30.00	34.87	

158	17.700	17.700 (1.214)	91	14388865	100.000	121.87	70.00- 130.00	100.00	
	17.700	17.700 (1.214)	126	2812628			0.00- 30.00	19.55	

161	17.921	17.921 (1.230)	146	8345519	100.000	101.08	70.00- 130.00	100.00	
	17.921	17.921 (1.230)	148	5277126			32.70- 92.70	63.23	
	17.921	17.921 (1.230)	111	3065390			7.07- 67.07	36.73	

167	19.276	19.276 (1.322)	180	8958905	100.000	107.37	70.00- 130.00	100.00	
	19.276	19.276 (1.322)	182	8611749			65.19- 125.19	96.13	

168	19.359	19.359 (1.328)	225	4504987	100.000	94.060	70.00- 130.00	100.00	
	19.359	19.359 (1.328)	223	2843237			33.26- 93.26	63.11	

169	19.469	19.469 (1.336)	128	15136012	100.000	86.013	70.00- 130.00	100.00	
	19.469	19.469 (1.336)	127	2518408			0.00- 30.00	16.64	

Report Date: 31-May-2007 14:53

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053008.d

Calibration Time: 16:03

Lab Smp Id: ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	441133	264680	617586	456242	3.43
88 1,4-Difluorobenze	1992312	1195387	2789237	2079239	4.36
125 Chlorobenzene-d5	1475337	885202	2065472	1515229	2.70


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 07-Jun-2007 13:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-07jun.b/8060706.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 07-JUN-2007 12:08
 Operator : JG Inst ID: msd8.i
 Smp Info : 200ml #1443-96
 Misc Info : 200ppbv-200ppbv
 Comment :
 Method : /chem/msd8.i/8-07jun.b/t14q530b.m
 Meth Date : 07-Jun-2007 13:41 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 12:08 Cal File: 8060706.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp16b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

* 68	Bromochloromethane			CAS #: 74-97-5				
7.387	7.387	(1.000)	130	361211	25.0000		70.00- 130.00	100.00
7.387	7.387	(1.000)	128	275936			42.98- 102.98	76.39
7.387	7.387	(1.000)	49	511706			112.53- 172.53	141.66

* 88	1,4-Difluorobenzene			CAS #: 540-36-3				
9.267	9.267	(1.000)	114	1595379	25.0000		70.00- 130.00	100.00
9.267	9.267	(1.000)	88	244093			0.00- 44.58	15.30

* 125	Chlorobenzene-d5			CAS #: 3114-55-4				
14.576	14.576	(1.000)	117	1171779	25.0000		70.00- 130.00	100.00
14.576	14.576	(1.000)	82	674436			0.00- 30.00	57.56

1	Freon 152a			CAS #: 75-37-6				
2.023	2.023	(0.274)	65	2371527	200.000	189.53	70.00- 130.00	100.00
2.078	2.078	(0.281)	51	10140161			0.00- 30.00	427.58

20	Freon123a			CAS #: 354-23-4				
3.682	3.682	(0.498)	67	3750189	200.000	194.11	70.00- 130.00	100.00
3.710	3.710	(0.502)	117	2671033			0.00- 30.00	71.22

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
21 Freon123						CAS #: 306-83-2			
3.792	3.792	(0.513)	83	2375930	200.000	195.12	70.00- 130.00	100.00	
3.792	3.792	(0.513)	133	448165			0.00- 30.00	18.86	
3.792	3.792	(0.513)	85	1758646			0.00- 30.00	74.02	

38 tert-Butyl-Alcohol						CAS #: 75-65-0			
4.954	4.954	(0.671)	59	3329003	200.000	132.23	70.00- 130.00	100.00	
4.954	4.954	(0.671)	41	767923			0.00- 30.00	23.07	
4.954	4.954	(0.671)	57	334446			0.00- 30.00	10.05	

49 Isopropyl ether						CAS #: 108-20-3			
5.949	5.949	(0.805)	45	12287330	200.000	195.16	70.00- 130.00	100.00	
5.949	5.949	(0.805)	87	3425229			0.00- 30.00	27.88	
5.949	5.949	(0.805)	59	1325426			0.00- 30.00	10.79	

52 1-Propanol						CAS #: 71-23-8			
6.170	6.170	(0.835)	42	896926	200.000	197.65	70.00- 130.00	100.00	
6.170	6.170	(0.835)	59	1152290			0.00- 30.00	128.47	
6.143	6.143	(0.832)	41	735160			0.00- 30.00	81.96	

58 Ethyl-tert-butyl Ether						CAS #: 637-92-3			
6.585	6.585	(0.891)	59	8042475	200.000	191.32	70.00- 130.00	100.00	
6.585	6.585	(0.891)	87	3100400			0.00- 30.00	38.55	
6.585	6.585	(0.891)	41	1355089			0.00- 30.00	16.85	

61 Ethyl Acetate						CAS #: 141-78-6			
7.083	7.083	(0.959)	70	1061516	200.000	193.50	70.00- 130.00	100.00	
7.083	7.083	(0.959)	43	9985386			0.00- 30.00	940.67	
7.083	7.083	(0.959)	61	1428422			0.00- 30.00	134.56	

78 Isobutanol						CAS #: 78-83-1			
8.438	8.438	(0.910)	43	3751872	200.000	204.90	70.00- 130.00	100.00(A)	
8.438	8.438	(0.910)	41	2497173			0.00- 30.00	66.56	

79 tert-amyl-Methyl Ether						CAS #: 994-05-8			
8.631	8.631	(1.168)	73	6928131	200.000	180.22	70.00- 130.00	100.00	
8.631	8.631	(1.168)	87	1658341			0.00- 30.00	23.94	
8.631	8.631	(1.168)	55	1860950			0.00- 30.00	26.86	

89 1-Butanol						CAS #: 71-36-3			
9.709	9.709	(1.048)	56	3377553	200.000	216.27	70.00- 130.00	100.00(A)	
9.709	9.709	(1.048)	41	2212090			0.00- 30.00	65.49	
9.709	9.709	(1.048)	43	1815594			0.00- 30.00	53.75	

136 Cyclohexanone						CAS #: 108-94-1			
16.152	16.152	(1.108)	55	5524328	200.000	205.99	70.00- 130.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
136 Cyclohexanone (continued)									
16.152	16.152	(1.108)	98	2497048			0.00- 30.00	45.20	
16.124	16.124	(1.106)	42	3645343			0.00- 30.00	65.99	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 07-Jun-2007 13:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 07-JUN-2007

Lab File ID: 8060706.d

Calibration Time: 11:37

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: JG

Method File: /chem/msd8.i/8-07jun.b/t14q530b.m

Misc Info: 200ppbv-200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	350593	210356	490830	361211	3.03
88 1,4-Difluorobenze	1524282	914569	2133995	1595379	4.66
125 Chlorobenzene-d5	1168126	700876	1635376	1171779	0.31

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-07jun.b/8060706.d
Date : 07-JUN-2007 12:08
Client ID: Level 7
Sample Info: 200ml #1443-96

Column phase: RTX-624

Instrument: msd8.1
Operator: JG
Column diameter: 0.53

/chem/msd8.1/8-07jun.b/8060706.d



Report Date: 31-May-2007 14:53

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-30may.b/8053009.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 30-MAY-2007 17:02
 Operator : db Inst ID: msd8.i
 Smp Info : 200ml #1487-289
 Misc Info : 200ppbv-200ppbv
 Comment :
 Method : /chem/msd8.i/8-30may.b/t14q530a.m
 Meth Date : 31-May-2007 14:53 jgray Quant Type: ISTD
 Cal Date : 30-MAY-2007 17:02 Cal File: 8053009.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5								
7.387	7.387	(1.000)	130	448309	25.0000		70.00- 130.00	100.00
7.387	7.387	(1.000)	128	332770			47.57- 107.57	74.23
7.387	7.387	(1.000)	49	652713			113.47- 173.47	145.59

* 88 1,4-Difluorobenzene CAS #: 540-36-3								
9.267	9.267	(1.000)	114	2033490	25.0000		70.00- 130.00	100.00
9.267	9.267	(1.000)	88	307791			0.00- 45.68	15.14

* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.576	14.576	(1.000)	117	1524596	25.0000		70.00- 130.00	100.00
14.576	14.576	(1.000)	82	864175			0.00- 30.00	56.68

§ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
8.465	8.465	(1.146)	65	624669	25.0000	26.623	70.00- 130.00	100.00
8.465	8.465	(1.146)	67	466938			0.00- 30.00	74.75

§ 104 Toluene-d8 CAS #: 2037-26-5								
12.115	12.115	(1.307)	98	1740690	25.0000	24.726	70.00- 130.00	100.00
12.115	12.115	(1.307)	70	177697			0.00- 30.00	10.21

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 104 Toluene-d8 (continued)										
12.115	12.115	(1.307)	100	1188238			0.00- 30.00	68.26		

\$ 140 Bromofluorobenzene										
						CAS #: 460-00-4				
16.207	16.207	(1.112)	174	926433	25.0000	25.539	70.00- 130.00	100.00		
16.207	16.207	(1.112)	95	1239953			102.16- 162.16	133.84		
16.207	16.207	(1.112)	176	905386			64.31- 124.31	97.73		

3 Propylene						CAS #: 115-07-1				
1.995	1.995	(0.270)	41	4152556	200.000	171.14	70.00- 130.00	100.00		
1.995	1.995	(0.270)	42	2781935			0.00- 30.00	66.99		
1.995	1.995	(0.270)	39	2816950			0.00- 30.00	67.84		

4 Dichlorodifluoromethane/Fr12						CAS #: 75-71-8				
2.050	2.050	(0.278)	85	10585010	200.000	172.34	70.00- 130.00	100.00		
2.050	2.050	(0.278)	87	3334935			0.00- 30.00	31.51		

6 Freon 114						CAS #: 76-14-2				
2.189	2.189	(0.296)	135	10270951	200.000	185.10	70.00- 130.00	100.00		
2.189	2.189	(0.296)	137	3216633			1.53- 61.53	31.32		

8 Chloromethane						CAS #: 74-87-3				
2.299	2.299	(0.311)	50	5091461	200.000	180.00	70.00- 130.00	100.00		
2.299	2.299	(0.311)	52	1478081			0.00- 30.00	29.03		

9 Butane						CAS #: 106-97-8				
2.355	2.355	(0.319)	58	1345216	200.000	182.11	70.00- 130.00	100.00		
2.355	2.355	(0.319)	43	9990258			0.00- 30.00	742.65		

11 Vinyl Chloride						CAS #: 75-01-4				
2.410	2.410	(0.326)	62	5882802	200.000	178.99	70.00- 130.00	100.00		
2.410	2.410	(0.326)	64	1795563			0.00- 30.00	30.52		

10 1,3-Butadiene						CAS #: 106-99-0				
2.410	2.410	(0.326)	54	4947217	200.000	175.97	70.00- 130.00	100.00		
2.410	2.410	(0.326)	39	5464185			0.00- 30.00	110.45		

13 Bromomethane						CAS #: 74-83-9				
2.852	2.852	(0.386)	94	4328268	200.000	197.12	70.00- 130.00	100.00		
2.852	2.852	(0.386)	96	4126213			65.03- 125.03	95.33		

16 Chloroethane						CAS #: 75-00-3				
2.963	2.963	(0.401)	64	3148287	200.000	180.99	70.00- 130.00	100.00		
2.963	2.963	(0.401)	49	753176			0.00- 30.00	23.92		
2.963	2.963	(0.401)	66	936359			0.00- 30.00	29.74		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

15 Isopentane						CAS #: 78-78-4			
2.963	2.963	(0.401)	43	8041442	200.000	195.94	70.00- 130.00	100.00	
2.963	2.963	(0.401)	57	5344427			0.00- 30.00	66.46	
2.963	2.963	(0.401)	72	583435			0.00- 30.00	7.26	

18 Trichlorofluoromethane/Fr11						CAS #: 75-69-4			
3.212	3.212	(0.435)	101	13289588	200.000	190.37	70.00- 130.00	100.00	
3.212	3.212	(0.435)	103	8582872			34.97- 94.97	64.58	

23 Ethanol						CAS #: 64-17-5			
3.571	3.571	(0.483)	45	2070197	200.000	185.71	70.00- 130.00	100.00	
3.571	3.571	(0.483)	43	359833			0.00- 30.00	17.38	
3.571	3.571	(0.483)	46	831102			0.00- 30.00	40.15	

28 Freon 113						CAS #: 76-13-1			
3.931	3.931	(0.532)	151	8576901	200.000	185.69	70.00- 130.00	100.00	
3.931	3.931	(0.532)	153	5456307			33.71- 93.71	63.62	
3.931	3.931	(0.532)	101	10076601			86.34- 146.34	117.49	

29 1,1-Dichloroethene						CAS #: 75-35-4			
3.958	3.958	(0.536)	61	8602773	200.000	187.54	70.00- 130.00	100.00	
3.958	3.958	(0.536)	96	5115455			30.45- 90.45	59.46	
3.958	3.958	(0.536)	98	3278527			8.39- 68.39	38.11	

30 Acetone						CAS #: 67-64-1			
4.124	4.124	(0.558)	58	2890019	200.000	188.12	70.00- 130.00	100.00	
4.124	4.124	(0.558)	43	8716480			0.00- 30.00	301.61	

33 Carbon Disulfide						CAS #: 75-15-0			
4.290	4.290	(0.581)	76	16324453	200.000	189.89	70.00- 130.00	100.00	

34 2-Propanol						CAS #: 67-63-0			
4.318	4.318	(0.584)	45	10466020	200.000	188.42	70.00- 130.00	100.00	
4.318	4.318	(0.584)	43	1932601			0.00- 30.00	18.47	
4.318	4.318	(0.584)	59	413505			0.00- 30.00	3.95	

37 3-Chloropropene						CAS #: 107-05-1			
4.566	4.566	(0.618)	76	2714411	200.000	197.92	70.00- 130.00	100.00	
4.566	4.566	(0.618)	41	8255613			0.00- 30.00	304.14	

40 Methylene Chloride						CAS #: 75-09-2			
4.815	4.815	(0.652)	49	6217595	200.000	181.05	70.00- 130.00	100.00	
4.815	4.815	(0.652)	84	4498494			41.01- 101.01	72.35	
4.815	4.815	(0.652)	51	1878140			0.00- 30.00	30.21	

43 MTBE						CAS #: 1634-04-4			
5.147	5.147	(0.697)	73	9333899	200.000	191.11	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
43 MTBE (continued)									
5.147	5.147	(0.697)	57	2192207			0.00- 53.82	23.49	
5.147	5.147	(0.697)	41	2086738			0.00- 30.00	22.36	

45 trans-1,2-Dichloroethene					CAS #: 156-60-5				
5.175	5.175	(0.701)	96	5912048	200.000	182.14	70.00- 130.00	100.00	
5.175	5.175	(0.701)	61	8855088			119.04- 179.04	149.78	
5.175	5.175	(0.701)	98	3761119			0.00- 30.00	63.62	

46 Hexane					CAS #: 110-54-3				
5.534	5.534	(0.749)	57	10195455	200.000	207.10	70.00- 130.00	100.00(A)	
5.534	5.534	(0.749)	43	6386604			0.00- 30.00	62.64	
5.534	5.534	(0.749)	86	1626253			0.00- 30.00	15.95	

54 1,1-Dichloroethane					CAS #: 75-34-3				
5.949	5.949	(0.805)	63	10336900	200.000	195.36	70.00- 130.00	100.00	
5.949	5.949	(0.805)	65	3213837			1.22- 61.22	31.09	

55 Vinyl Acetate					CAS #: 108-05-4				
6.032	6.032	(0.817)	86	1549543	200.000	207.45	70.00- 130.00	100.00(A)	
6.032	6.032	(0.817)	43	16691748			0.00- 30.00	1077.20	
6.032	6.032	(0.817)	42	1228627			0.00- 30.00	79.29	

64 cis-1,2-Dichloroethene					CAS #: 156-59-2				
6.972	6.972	(0.944)	61	7586985	200.000	181.17	70.00- 130.00	100.00	
6.972	6.972	(0.944)	96	5613120			45.09- 105.09	73.98	
6.972	6.972	(0.944)	98	3566701			17.66- 77.66	47.01	

65 2-Butanone					CAS #: 78-93-3				
7.027	7.027	(0.951)	72	2839689	200.000	191.14	70.00- 130.00	100.00	
7.027	7.027	(0.951)	43	12152318			398.56- 458.56	427.95	
7.027	7.027	(0.951)	57	913237			0.00- 30.00	32.16	

67 Tetrahydrofuran					CAS #: 109-99-9				
7.387	7.387	(1.000)	42	7203120	200.000	186.53	70.00- 130.00	100.00	
7.387	7.387	(1.000)	71	2561625			5.14- 65.14	35.56	
7.387	7.387	(1.000)	72	2765395			0.00- 30.00	38.39	

70 Chloroform					CAS #: 67-66-3				
7.525	7.525	(1.019)	83	10146243	200.000	191.74	70.00- 130.00	100.00	
7.525	7.525	(1.019)	85	6278598			31.98- 91.98	61.88	

73 Cyclohexane					CAS #: 110-82-7				
7.746	7.746	(1.049)	84	8151077	200.000	185.65	70.00- 130.00	100.00	
7.746	7.746	(1.049)	56	10487225			99.30- 159.30	128.66	
7.746	7.746	(1.049)	41	5082554			33.84- 93.84	62.35	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

75	1,1,1-Trichloroethane				CAS #: 71-55-6				
7.774	7.774	(1.052)	97	10604133	200.000	191.25	70.00- 130.00	100.00	
7.774	7.774	(1.052)	99	6750218			34.73- 94.73	63.66	

77	Carbon Tetrachloride				CAS #: 56-23-5				
7.995	7.995	(1.082)	119	10305397	200.000	204.25	70.00- 130.00	100.00(A)	
7.995	7.995	(1.082)	117	10656606			74.04- 134.04	103.41	

81	Benzene				CAS #: 71-43-2				
8.437	8.437	(0.910)	78	17785145	200.000	193.61	70.00- 130.00	100.00	
8.437	8.437	(0.910)	77	3896089			0.00- 30.00	21.91	

80	2,2,4-Trimethylpentane				CAS #: 540-84-1				
8.465	8.465	(1.146)	57	26545736	200.000	202.53	70.00- 130.00	100.00(A)	
8.465	8.465	(1.146)	56	8248292			0.00- 30.00	31.07	
8.465	8.465	(1.146)	41	6074066			0.00- 30.00	22.88	

83	1,2-Dichloroethane				CAS #: 107-06-2				
8.603	8.603	(0.928)	62	7018378	200.000	188.31	70.00- 130.00	100.00	
8.603	8.603	(0.928)	64	2171145			0.00- 30.00	30.94	

85	Heptane				CAS #: 142-82-5				
8.852	8.852	(0.955)	100	1749662	200.000	176.00	70.00- 130.00	100.00	
8.852	8.852	(0.955)	43	10101737			0.00- 30.00	577.35	
8.852	8.852	(0.955)	71	5661505			0.00- 30.00	323.58	

94	Trichloroethene				CAS #: 79-01-6				
9.682	9.682	(1.045)	95	6875905	200.000	188.87	70.00- 130.00	100.00	
9.682	9.682	(1.045)	130	7400546			77.84- 137.84	107.63	
9.682	9.682	(1.045)	97	4412159			34.22- 94.22	64.17	

95	Methyl Cyclohexane				CAS #: 108-87-2				
9.903	9.903	(1.341)	83	10900787	200.000	199.28	70.00- 130.00	100.00	
9.903	9.903	(1.341)	98	4807211			0.00- 30.00	44.10	
9.903	9.903	(1.341)	55	8581305			0.00- 30.00	78.72	

97	1,2-Dichloropropane				CAS #: 78-87-5				
10.179	10.179	(1.098)	63	6102724	200.000	191.69	70.00- 130.00	100.00	
10.179	10.179	(1.098)	62	4318168			42.15- 102.15	70.76	
10.179	10.179	(1.098)	41	3413820			26.47- 86.47	55.94	

98	1,4-Dioxane				CAS #: 123-91-1				
10.428	10.428	(1.125)	88	3854134	200.000	198.48	70.00- 130.00	100.00	
10.428	10.428	(1.125)	58	2794898			44.03- 104.03	72.52	
10.428	10.428	(1.125)	57	841647			0.00- 30.00	21.84	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

100	Bromodichloromethane					CAS #: 75-27-4				
10.732	10.732	(1.158)	83	10477147	200.000	197.04	70.00- 130.00	100.00		
10.732	10.732	(1.158)	85	6434109			31.03- 91.03	61.41		

102	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
11.672	11.672	(1.260)	75	8703573	200.000	196.72	70.00- 130.00	100.00		
11.672	11.672	(1.260)	77	2719406			1.19- 61.19	31.24		
11.672	11.672	(1.260)	39	4066285			16.93- 76.93	46.72		

103	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.032	12.032	(1.298)	58	4830872	200.000	201.84	70.00- 130.00	100.00(A)		
12.032	12.032	(1.298)	43	12195996			0.00- 30.00	252.46		
12.032	12.032	(1.298)	85	2017678			0.00- 30.00	41.77		

105	Toluene					CAS #: 108-88-3				
12.253	12.253	(1.322)	91	18836110	200.000	201.75	70.00- 130.00	100.00(A)		
12.253	12.253	(1.322)	92	11087412			30.46- 90.46	58.86		

108	trans-1,3-Dichloropropene					CAS #: 10061-02-6				
12.834	12.834	(0.880)	75	8893044	200.000	201.20	70.00- 130.00	100.00(A)		
12.834	12.834	(0.880)	77	2758588			0.11- 60.11	31.02		
12.834	12.834	(0.880)	39	4059278			15.75- 75.75	45.65		

110	1,1,2-Trichloroethane					CAS #: 79-00-5				
13.138	13.138	(0.901)	97	6072445	200.000	187.33	70.00- 130.00	100.00		
13.138	13.138	(0.901)	99	3749841			31.47- 91.47	61.75		
13.138	13.138	(0.901)	83	5216234			58.25- 118.25	85.90		

112	Tetrachloroethene					CAS #: 127-18-4				
13.193	13.193	(0.905)	166	8509996	200.000	193.97	70.00- 130.00	100.00		
13.193	13.193	(0.905)	129	6421962			45.90- 105.90	75.46		
13.193	13.193	(0.905)	131	6172896			43.88- 103.88	72.54		

114	2-Hexanone					CAS #: 591-78-6				
13.580	13.580	(0.932)	58	6995194	200.000	217.79	70.00- 130.00	100.00(A)		
13.580	13.580	(0.932)	43	12710091			147.03- 207.03	181.70		
13.580	13.580	(0.932)	100	1440713			0.00- 30.00	20.60		

116	Dibromochloromethane					CAS #: 124-48-1				
13.718	13.718	(0.941)	129	10582353	200.000	208.30	70.00- 130.00	100.00(A)		
13.718	13.718	(0.941)	127	8100146			0.00- 30.00	76.54		

117	1,2-Dibromoethane					CAS #: 106-93-4				
13.884	13.884	(0.953)	107	9615029	200.000	194.66	70.00- 130.00	100.00		
13.884	13.884	(0.953)	109	9190853			65.18- 125.18	95.59		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
126 Chlorobenzene						CAS #: 108-90-7			
14.603	14.603	(1.002)	112	15794834	200.000	201.76	70.00- 130.00	100.00(A)	
14.631	14.631	(1.004)	114	4886367			1.91- 61.91	30.94	
14.603	14.603	(1.002)	77	8721903			26.50- 86.50	55.22	

129 Ethyl Benzene						CAS #: 100-41-4			
14.769	14.769	(1.013)	106	8105324	200.000	195.65	70.00- 130.00	100.00	
14.769	14.769	(1.013)	91	22645192			0.00- 30.00	279.39	

130 m,p-Xylene						CAS #: 108-38-3			
14.935	14.935	(1.025)	106	10381915	200.000	205.65	70.00- 130.00	100.00(A)	
14.935	14.935	(1.025)	91	19724408			0.00- 30.00	189.99	

132 o-Xylene						CAS #: 95-47-6			
15.488	15.488	(1.063)	106	10154080	200.000	199.32	70.00- 130.00	100.00	
15.488	15.488	(1.063)	91	18196909			177.47- 237.47	179.21	

134 Styrene						CAS #: 100-42-5			
15.516	15.516	(1.064)	104	15909823	200.000	219.09	70.00- 130.00	100.00(A)	
15.516	15.516	(1.064)	78	7701877			20.25- 80.25	48.41	

135 Bromoform						CAS #: 75-25-2			
15.765	15.765	(1.082)	173	10020398	200.000	224.24	70.00- 130.00	100.00(A)	
15.765	15.765	(1.082)	171	5036697			21.05- 81.05	50.26	

137 Cumene						CAS #: 98-82-8			
15.958	15.958	(1.095)	105	26088631	200.000	187.36	70.00- 130.00	100.00	
15.958	15.958	(1.095)	120	7362914			0.00- 30.00	28.22	
15.958	15.958	(1.095)	51	2543543			0.00- 30.00	9.75	

144 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5			
16.456	16.456	(1.129)	83	14918929	200.000	200.26	70.00- 130.00	100.00(A)	
16.456	16.456	(1.129)	85	9007640			31.99- 91.99	60.38	

145 Propylbenzene						CAS #: 103-65-1			
16.483	16.483	(1.131)	91	23743906	200.000	148.89	70.00- 130.00	100.00	
16.483	16.483	(1.131)	120	7677511			0.00- 30.00	32.33	
16.483	16.483	(1.131)	105	1188043			0.00- 30.00	5.00	

147 4-Ethyltoluene						CAS #: 622-96-8			
16.649	16.649	(1.142)	105	21121664	200.000	154.48	70.00- 130.00	100.00	
16.649	16.649	(1.142)	120	9170339			0.00- 59.60	43.42	

148 1,3,5-Trimethylbenzene						CAS #: 108-67-8			
16.732	16.732	(1.148)	105	18184900	200.000	138.37	70.00- 130.00	100.00	
16.732	16.732	(1.148)	120	14177241			0.00- 30.00	77.96	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

153	17.147	17.147 (1.176)	105	16318393	200.000	123.36	70.00- 130.00	100.00	
	17.147	17.147 (1.176)	120	12694037			15.41- 75.41	77.79	

156	17.451	17.451 (1.197)	146	16249745	200.000	188.43	70.00- 130.00	100.00	
	17.451	17.451 (1.197)	148	12045123			0.00- 30.00	74.12	
	17.451	17.451 (1.197)	111	7776993			0.00- 30.00	47.86	

157	17.562	17.562 (1.205)	146	15969247	200.000	195.40	70.00- 130.00	100.00	
	17.562	17.562 (1.205)	148	11683869			0.00- 30.00	73.16	
	17.562	17.562 (1.205)	111	6235138			0.00- 30.00	39.04	

158	17.700	17.700 (1.214)	91	16188926	200.000	136.28	70.00- 130.00	100.00	
	17.700	17.700 (1.214)	126	5969592			0.00- 30.00	36.87	

161	17.921	17.921 (1.230)	146	16002972	200.000	192.64	70.00- 130.00	100.00	
	17.921	17.921 (1.230)	148	10877445			32.70- 92.70	67.97	
	17.921	17.921 (1.230)	111	6353120			7.07- 67.07	39.70	

167	19.276	19.276 (1.322)	180	14910912	200.000	177.60	70.00- 130.00	100.00	
	19.276	19.276 (1.322)	182	14865436			65.19- 125.19	99.70	

168	19.359	19.359 (1.328)	225	8939871	200.000	185.51	70.00- 130.00	100.00	
	19.359	19.359 (1.328)	223	5565949			33.26- 93.26	62.26	

169	19.470	19.470 (1.336)	128	16033683	200.000	90.554	70.00- 130.00	100.00	
	19.470	19.470 (1.336)	127	5377959			0.00- 30.00	33.54	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 31-May-2007 14:53

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 30-MAY-2007

Lab File ID: 8053009.d

Calibration Time: 16:03

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: db

Method File: /chem/msd8.i/8-30may.b/t14q530a.m

Misc Info: 200ppbv-200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	441133	264680	617586	448309	1.63
88 1,4-Difluorobenze	1992312	1195387	2789237	2033490	2.07
125 Chlorobenzene-d5	1475337	885202	2065472	1524596	3.34

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.39	7.06	7.72	7.39	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-30may.b/8053009.d
Date: 30-May-2007 17:02
Client ID: Level 7
Sample Info: 200ml #1487-289

Column phase: RTX-624

Instrument: msd8.i
Operator: db
Column diameter: 0.53





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0706310-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062202	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/22/07 10:27 AM

Compound	%Recovery
Freon 12	92
Freon 114	88
Vinyl Chloride	86
Bromomethane	92
Chloroethane	85
Freon 11	90
1,1-Dichloroethene	86
Freon 113	89
Methylene Chloride	89
1,1-Dichloroethane	89
cis-1,2-Dichloroethene	83
Chloroform	81
1,1,1-Trichloroethane	87
Carbon Tetrachloride	93
Benzene	81
1,2-Dichloroethane	88
Trichloroethene	85
1,2-Dichloropropane	85
cis-1,3-Dichloropropene	84
Toluene	86
trans-1,3-Dichloropropene	83
1,1,2-Trichloroethane	80
Tetrachloroethene	87
1,2-Dibromoethane (EDB)	86
Chlorobenzene	84
Ethyl Benzene	83
m,p-Xylene	86
o-Xylene	83
Styrene	84
1,1,2,2-Tetrachloroethane	77
1,3,5-Trimethylbenzene	84
1,2,4-Trimethylbenzene	90
1,3-Dichlorobenzene	89
1,4-Dichlorobenzene	79
alpha-Chlorotoluene	83
1,2-Dichlorobenzene	78
1,3-Butadiene	85
Hexane	90
Cyclohexane	80



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0706310-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062202	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/22/07 10:27 AM

Compound	%Recovery
Heptane	87
Bromodichloromethane	86
Dibromochloromethane	86
Cumene	86
Propylbenzene	91
Chloromethane	92
1,2,4-Trichlorobenzene	79
Hexachlorobutadiene	107
Acetone	87
Carbon Disulfide	86
2-Propanol	84
trans-1,2-Dichloroethene	84
2-Butanone (Methyl Ethyl Ketone)	82
Tetrahydrofuran	86
1,4-Dioxane	86
4-Methyl-2-pentanone	88
2-Hexanone	85
Bromoform	92
4-Ethyltoluene	86
Ethanol	84
Methyl tert-butyl ether	114
3-Chloropropene	92
2,2,4-Trimethylpentane	81
Naphthalene	83

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	98	70-130
1,2-Dichloroethane-d4	99	70-130
4-Bromofluorobenzene	104	70-130

Report Date: 22-Jun-2007 10:48

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd8.i Injection Date: 22-JUN-2007 10:27
 Lab File ID: 8062202.d Init. Cal. Date(s): 30-MAY-2007 07-JUN-2007
 Analysis Type: AIR Init. Cal. Times: 14:12 12:08
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /var/chem/msd8.i/8-22jun.b/t14q530b.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 82 1,2-Dichloroethane-d4	1.30843	1.29527	0.010	1.00517	30.00000	Averaged
\$ 104 Toluene-d8	0.86549	0.85289	0.010	1.45594	30.00000	Averaged
\$ 140 Bromofluorobenzene	0.59482	0.61784	0.010	-3.86950	30.00000	Averaged
3 Propylene	1.35311	1.17024	0.010	13.51526	30.00000	Averaged
4 Dichlorodifluoromethane/Fr1	3.42502	3.15343	0.010	7.92950	30.00000	Averaged
6 Freon 114	3.09425	2.70795	0.010	12.48454	30.00000	Averaged
8 Chloromethane	1.57733	1.44691	0.010	8.26899	30.00000	Averaged
11 Vinyl Chloride	1.83284	1.57009	0.010	14.33589	30.00000	Averaged
10 1,3-Butadiene	1.56776	1.33314	0.010	14.96558	30.00000	Averaged
13 Bromomethane	1.22449	1.12090	0.010	8.45961	30.00000	Averaged
16 Chloroethane	0.97001	0.82339	0.010	15.11543	30.00000	Averaged
18 Trichlorofluoromethane/Fr11	3.89297	3.48913	0.010	10.37367	30.00000	Averaged
23 Ethanol	0.62165	0.51915	0.010	16.48762	30.00000	Averaged
28 Freon 113	2.57573	2.28978	0.010	11.10178	30.00000	Averaged
29 1,1-Dichloroethene	2.55796	2.21296	0.010	13.48736	30.00000	Averaged
30 Acetone	0.85672	0.74508	0.010	13.03112	30.00000	Averaged
34 2-Propanol	3.09759	2.59499	0.010	16.22540	30.00000	Averaged
33 Carbon Disulfide	4.79398	4.11545	0.010	14.15386	30.00000	Averaged
37 3-Chloropropene	0.76480	0.70395	0.010	7.95662	30.00000	Averaged
40 Methylene Chloride	1.91508	1.70445	0.010	10.99843	30.00000	Averaged
43 MTBE	2.72362	3.10122	0.010	-13.86390	30.00000	Averaged
45 trans-1,2-Dichloroethene	1.81006	1.51375	0.010	16.37003	30.00000	Averaged
46 Hexane	2.74528	2.46899	0.010	10.06412	30.00000	Averaged
54 1,1-Dichloroethane	2.95068	2.63390	0.010	10.73572	30.00000	Averaged
55 Vinyl Acetate	0.41654	0.35888	0.010	13.84288	30.00000	Averaged
65 2-Butanone	0.82850	0.67766	0.010	18.20625	30.00000	Averaged
64 cis-1,2-Dichloroethene	2.33530	1.93071	0.010	17.32514	30.00000	Averaged
67 Tetrahydrofuran	2.15347	1.86325	0.010	13.47657	30.00000	Averaged
70 Chloroform	3.17561	2.56706	0.010	19.16297	30.00000	Averaged
75 1,1,1-Trichloroethane	3.09194	2.68455	0.010	13.17603	30.00000	Averaged
73 Cyclohexane	2.44845	1.96003	0.010	19.94806	30.00000	Averaged
77 Carbon Tetrachloride	2.81355	2.62304	0.010	6.77140	30.00000	Averaged
80 2,2,4-Trimethylpentane	7.30928	5.91824	0.010	19.03123	30.00000	Averaged
81 Benzene	1.17761	0.95586	0.010	18.83071	30.00000	Averaged
83 1,2-Dichloroethane	0.45822	0.40301	0.010	12.04845	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd8.i Injection Date: 22-JUN-2007 10:27
 Lab File ID: 8062202.d Init. Cal. Date(s): 30-MAY-2007 07-JUN-2007
 Analysis Type: AIR Init. Cal. Times: 14:12 12:08
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /var/chem/msd8.i/8-22jun.b/t14q530b.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE
			RRF %D / %DRIFT	%D / %DRIFT	
85 Heptane	0.12222	0.10684	0.010 12.57854	30.00000	Averaged
94 Trichloroethene	0.44757	0.38226	0.010 14.59227	30.00000	Averaged
97 1,2-Dichloropropane	0.39140	0.33178	0.010 15.23306	30.00000	Averaged
98 1,4-Dioxane	0.23873	0.20604	0.010 13.69322	30.00000	Averaged
100 Bromodichloromethane	0.65370	0.56332	0.010 13.82695	30.00000	Averaged
102 cis-1,3-Dichloropropene	0.54392	0.45644	0.010 16.08337	30.00000	Averaged
103 4-Methyl-2-pentanone	0.29426	0.26003	0.010 11.62955	30.00000	Averaged
105 Toluene	1.14782	0.98342	0.010 14.32305	30.00000	Averaged
108 trans-1,3-Dichloropropene	0.72478	0.60274	0.010 16.83739	30.00000	Averaged
110 1,1,2-Trichloroethane	0.53155	0.42628	0.010 19.80312	30.00000	Averaged
112 Tetrachloroethene	0.71942	0.62358	0.010 13.32229	30.00000	Averaged
114 2-Hexanone	0.52669	0.44883	0.010 14.78228	30.00000	Averaged
116 Dibromochloromethane	0.83304	0.71649	0.010 13.99066	30.00000	Averaged
117 1,2-Dibromoethane	0.80993	0.69259	0.010 14.48777	30.00000	Averaged
126 Chlorobenzene	1.28368	1.08077	0.010 15.80720	30.00000	Averaged
129 Ethyl Benzene	0.67934	0.56441	0.010 16.91767	30.00000	Averaged
130 m,p-Xylene	0.82782	0.71342	0.010 13.81923	30.00000	Averaged
132 o-Xylene	0.83535	0.69374	0.010 16.95170	30.00000	Averaged
134 Styrene	1.17936	0.99062	0.010 16.00413	30.00000	Averaged
135 Bromoform	0.73275	0.67110	0.010 8.41290	30.00000	Averaged
144 1,1,2,2-Tetrachloroethane	1.22162	0.93593	0.010 23.38590	30.00000	Averaged
147 4-Ethyltoluene	2.24196	1.92317	0.010 14.21950	30.00000	Averaged
148 1,3,5-Trimethylbenzene	2.15500	1.81902	0.010 15.59036	30.00000	Averaged
153 1,2,4-Trimethylbenzene	2.16919	1.94322	0.010 10.41712	30.00000	Averaged
156 1,3-Dichlorobenzene	1.41407	1.26512	0.010 10.53374	30.00000	Averaged
157 1,4-Dichlorobenzene	1.34013	1.06002	0.010 20.90161	30.00000	Averaged
158 alpha-Chlorotoluene	1.94799	1.61026	0.010 17.33748	30.00000	Averaged
161 1,2-Dichlorobenzene	1.36216	1.06273	0.010 21.98175	30.00000	Averaged
167 1,2,4-Trichlorobenzene	1.37671	1.08946	0.010 20.86495	30.00000	Averaged
168 Hexachlorobutadiene	0.79022	0.84828	0.010 -7.34786	30.00000	Averaged
145 Propylbenzene	2.61503	2.38523	0.010 8.78785	30.00000	Averaged
137 Cumene	2.35689	2.02309	0.010 14.16271	30.00000	Averaged
169 Naphthalene	2.90342	2.42378	0.010 16.51974	30.00000	Averaged
9 Butane	0.41193	0.36555	0.010 11.26051	30.00000	Averaged
15 Isopentane	2.28859	2.17830	0.010 4.81925	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd8.i Injection Date: 22-JUN-2007 10:27
Lab File ID: 8062202.d Init. Cal. Date(s): 30-MAY-2007 07-JUN-2007
Analysis Type: AIR Init. Cal. Times: 14:12 12:08
Lab Sample ID: CCV-1 Quant Type: ISTD
Method: /var/chem/msd8.i/8-22jun.b/t14q530b.m

COMPOUND	RRF / AMOUNT	RF50	MIN RRF	%D / %DRIFT	MAX RRF	%D / %DRIFT	CURVE TYPE
95 Methyl Cyclohexane	3.05031	2.53112	0.010	17.02093	30.00000		Averaged

Report Date: 22-Jun-2007 10:48

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22jun.b/8062202.d
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1
 Inj Date : 22-JUN-2007 10:27
 Operator : jdg Inst ID: msd8.i
 Smp Info : 100ml #1487-286A
 Misc Info : 100ppbv-50ppbv
 Comment :
 Method : /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Meth Date : 22-Jun-2007 10:48 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 12:08 Cal File: 8060706.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 68 Bromochloromethane CAS #: 74-97-5									
7.414	7.414	(1.000)	130	307449	25.0000			80.00- 120.00	100.00
7.414	7.414	(1.000)	128	239355				47.85- 107.85	77.85
7.387	7.387	(1.000)	49	448072				115.74- 175.74	145.74

* 88 1,4-Difluorobenzene CAS #: 540-36-3									
9.267	9.267	(1.000)	114	1381560	25.0000			80.00- 120.00	100.00
9.267	9.267	(1.000)	88	203647				0.00- 44.74	14.74

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.576	14.576	(1.000)	117	1041151	25.0000			80.00- 120.00	100.00
14.576	14.576	(1.000)	82	572167				0.00- 30.00	54.96

\$ 82 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
8.465	8.465	(1.142)	65	398231	25.0000	24.749		80.00- 120.00	100.00
8.465	8.465	(1.142)	67	239277				0.00- 30.00	60.08

\$ 104 Toluene-d8 CAS #: 2037-26-5									
12.115	12.115	(1.307)	98	1178320	25.0000	24.636		80.00- 120.00	100.00
12.115	12.115	(1.307)	70	117884				0.00- 30.00	10.00

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 104 Toluene-d8 (continued)										
12.115	12.115	(1.307)	100	1031243			0.00- 30.00	87.52		

\$ 140 Bromofluorobenzene										
						CAS #:	460-00-4			
16.207	16.207	(1.112)	174	643266	25.0000	25.967	80.00- 120.00	100.00		
16.207	16.207	(1.112)	95	780751			91.37- 151.37	121.37		
16.207	16.207	(1.112)	176	633136			68.43- 128.43	98.43		

3 Propylene										
						CAS #:	115-07-1			
2.023	2.023	(0.273)	41	719577	50.0000	43.242	80.00- 120.00	100.00		
2.023	2.023	(0.273)	42	481914			0.00- 30.00	66.97		
2.023	2.023	(0.273)	39	483333			0.00- 30.00	67.17		

4 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.078	2.078	(0.280)	85	1939039	50.0000	46.035	80.00- 120.00	100.00		
2.078	2.078	(0.280)	87	605340			0.00- 30.00	31.22		

6 Freon 114										
						CAS #:	76-14-2			
2.161	2.161	(0.291)	135	1665113	50.0000	43.758	80.00- 120.00	100.00		
2.161	2.161	(0.291)	137	534602			2.11- 62.11	32.11		

8 Chloromethane										
						CAS #:	74-87-3			
2.299	2.299	(0.310)	50	889699	50.0000	45.866	80.00- 120.00	100.00		
2.327	2.327	(0.314)	52	276287			0.00- 30.00	31.05		

11 Vinyl Chloride										
						CAS #:	75-01-4			
2.437	2.437	(0.329)	62	965443	50.0000	42.832	80.00- 120.00	100.00		
2.437	2.437	(0.329)	64	303258			0.00- 30.00	31.41		

10 1,3-Butadiene										
						CAS #:	106-99-0			
2.410	2.410	(0.325)	54	819744	50.0000	42.517	80.00- 120.00	100.00		
2.410	2.410	(0.325)	39	856258			0.00- 30.00	104.45		

13 Bromomethane										
						CAS #:	74-83-9			
2.880	2.880	(0.388)	94	689239	50.0000	45.770	80.00- 120.00	100.00		
2.880	2.880	(0.388)	96	651123			64.47- 124.47	94.47		

16 Chloroethane										
						CAS #:	75-00-3			
2.963	2.963	(0.400)	64	506300	50.0000	42.442	80.00- 120.00	100.00		
2.963	2.963	(0.400)	49	130338			0.00- 30.00	25.74		
2.963	2.963	(0.400)	66	154119			0.00- 30.00	30.44		

18 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.239	3.239	(0.437)	101	2145456	50.0000	44.813	80.00- 120.00	100.00		
3.239	3.239	(0.437)	103	1392395			34.90- 94.90	64.90		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
23 Ethanol						CAS #: 64-17-5			
3.543	3.543	(0.478)	45	319226	50.0000	41.756	80.00- 120.00	100.00	
3.543	3.543	(0.478)	43	63496			0.00- 30.00	19.89	
3.571	3.571	(0.482)	46	126375			0.00- 30.00	39.59	

28 Freon 113						CAS #: 76-13-1			
3.958	3.958	(0.534)	151	1407980	50.0000	44.449	80.00- 120.00	100.00	
3.958	3.958	(0.534)	153	891418			33.31- 93.31	63.31	
3.958	3.958	(0.534)	101	1617335			84.87- 144.87	114.87	

29 1,1-Dichloroethene						CAS #: 75-35-4			
3.986	3.986	(0.538)	61	1360744	50.0000	43.256	80.00- 120.00	100.00	
3.986	3.986	(0.538)	96	818495			30.15- 90.15	60.15	
3.986	3.986	(0.538)	98	523802			8.49- 68.49	38.49	

30 Acetone						CAS #: 67-64-1			
4.124	4.124	(0.556)	58	458147	50.0000	43.484	80.00- 120.00	100.00	
4.124	4.124	(0.556)	43	1398123			0.00- 30.00	305.17	

34 2-Propanol						CAS #: 67-63-0			
4.318	4.318	(0.582)	45	1595654	50.0000	41.887	80.00- 120.00	100.00	
4.318	4.318	(0.582)	43	326637			0.00- 30.00	20.47	
4.318	4.318	(0.582)	59	63461			0.00- 30.00	3.98	

33 Carbon Disulfide						CAS #: 75-15-0			
4.318	4.318	(0.582)	76	2530580	50.0000	42.923	80.00- 120.00	100.00	

37 3-Chloropropene						CAS #: 107-05-1			
4.594	4.594	(0.620)	76	432855	50.0000	46.022	80.00- 120.00	100.00	
4.594	4.594	(0.620)	41	1310773			0.00- 30.00	302.82	

40 Methylene Chloride						CAS #: 75-09-2			
4.815	4.815	(0.649)	49	1048063	50.0000	44.501	80.00- 120.00	100.00	
4.843	4.843	(0.653)	84	727618			39.43- 99.43	69.43	
4.815	4.815	(0.649)	51	312071			0.00- 30.00	29.78	

43 MTBE						CAS #: 1634-04-4			
5.175	5.175	(0.698)	73	1906933	50.0000	56.932	80.00- 120.00	100.00	
5.175	5.175	(0.698)	57	447344			0.00- 53.46	23.46	
5.175	5.175	(0.698)	41	445103			0.00- 30.00	23.34	

45 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.202	5.202	(0.702)	96	930801	50.0000	41.815	80.00- 120.00	100.00	
5.202	5.202	(0.702)	61	1418457			122.39- 182.39	152.39	
5.202	5.202	(0.702)	98	592426			0.00- 30.00	63.65	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
46 Hexane						CAS #: 110-54-3			
5.534	5.534	(0.746)	57	1518177	50.0000	44.968	80.00- 120.00	100.00	
5.534	5.534	(0.746)	43	999797			0.00- 30.00	65.86	
5.534	5.534	(0.746)	86	253726			0.00- 30.00	16.71	

54 1,1-Dichloroethane						CAS #: 75-34-3			
5.949	5.949	(0.802)	63	1619580	50.0000	44.632	80.00- 120.00	100.00	
5.949	5.949	(0.802)	65	505226			1.19- 61.19	31.19	

55 Vinyl Acetate						CAS #: 108-05-4			
6.032	6.032	(0.814)	86	220676	50.0000	43.078	80.00- 120.00	100.00	
6.032	6.032	(0.814)	43	2473867			0.00- 30.00	1121.04	
6.032	6.032	(0.814)	42	192311			0.00- 30.00	87.15	

65 2-Butanone						CAS #: 78-93-3			
7.027	7.027	(0.948)	72	416691	50.0000	40.897	80.00- 120.00	100.00	
7.027	7.027	(0.948)	43	1866611			417.96- 477.96	447.96	
7.027	7.027	(0.948)	57	146811			0.00- 30.00	35.23	

64 cis-1,2-Dichloroethene						CAS #: 156-59-2			
6.972	6.972	(0.940)	61	1187189	50.0000	41.337	80.00- 120.00	100.00	
6.972	6.972	(0.940)	96	873681			43.59- 103.59	73.59	
6.972	6.972	(0.940)	98	561130			17.27- 77.27	47.27	

67 Tetrahydrofuran						CAS #: 109-99-9			
7.387	7.387	(0.996)	42	1145710	50.0000	43.262	80.00- 120.00	100.00	
7.387	7.387	(0.996)	71	392814			4.29- 64.29	34.29	
7.387	7.387	(0.996)	72	418715			0.00- 30.00	36.55	

70 Chloroform						CAS #: 67-66-3			
7.525	7.525	(1.015)	83	1578483	50.0000	40.418	80.00- 120.00	100.00	
7.525	7.525	(1.015)	85	998946			33.29- 93.29	63.29	

75 1,1,1-Trichloroethane						CAS #: 71-55-6			
7.774	7.774	(1.048)	97	1650723	50.0000	43.412	80.00- 120.00	100.00	
7.774	7.774	(1.048)	99	1042665			33.16- 93.16	63.16	

73 Cyclohexane						CAS #: 110-82-7			
7.746	7.746	(1.045)	84	1205221	50.0000	40.026	80.00- 120.00	100.00	
7.746	7.746	(1.045)	56	1616407			104.12- 164.12	134.12	
7.746	7.746	(1.045)	41	798890			36.29- 96.29	66.29	

77 Carbon Tetrachloride						CAS #: 56-23-5			
8.023	8.023	(1.082)	119	1612899	50.0000	46.614	80.00- 120.00	100.00	
7.995	7.995	(1.078)	117	1659279			72.88- 132.88	102.88	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
8.465	8.465	(1.142)	57	3639111	50.0000	40.484	80.00- 120.00	100.00		
8.465	8.465	(1.142)	56	1171915			0.00- 30.00	32.20		
8.465	8.465	(1.142)	41	899455			0.00- 30.00	24.72		

81	Benzene					CAS #: 71-43-2				
8.437	8.437	(0.910)	78	2641160	50.0000	40.585	80.00- 120.00	100.00		
8.437	8.437	(0.910)	77	607655			0.00- 30.00	23.01		

83	1,2-Dichloroethane					CAS #: 107-06-2				
8.603	8.603	(0.928)	62	1113560	50.0000	43.976	80.00- 120.00	100.00		
8.603	8.603	(0.928)	64	347840			0.00- 30.00	31.24		

85	Heptane					CAS #: 142-82-5				
8.852	8.852	(0.955)	100	295223	50.0000	43.711	80.00- 120.00	100.00		
8.852	8.852	(0.955)	43	1693383			0.00- 30.00	573.59		
8.852	8.852	(0.955)	71	918363			0.00- 30.00	311.07		

94	Trichloroethene					CAS #: 79-01-6				
9.682	9.682	(1.045)	95	1056220	50.0000	42.704	80.00- 120.00	100.00		
9.682	9.682	(1.045)	130	1127782			76.78- 136.78	106.78		
9.682	9.682	(1.045)	97	679898			34.37- 94.37	64.37		

97	1,2-Dichloropropane					CAS #: 78-87-5				
10.179	10.179	(1.098)	63	916738	50.0000	42.383	80.00- 120.00	100.00		
10.179	10.179	(1.098)	62	650452			40.95- 100.95	70.95		
10.179	10.179	(1.098)	41	560864			31.18- 91.18	61.18		

98	1,4-Dioxane					CAS #: 123-91-1				
10.428	10.428	(1.125)	88	569305	50.0000	43.153	80.00- 120.00	100.00		
10.428	10.428	(1.125)	58	423798			44.44- 104.44	74.44		
10.428	10.428	(1.125)	57	125364			0.00- 30.00	22.02		

100	Bromodichloromethane					CAS #: 75-27-4				
10.732	10.732	(1.158)	83	1556511	50.0000	43.086	80.00- 120.00	100.00		
10.732	10.732	(1.158)	85	960386			31.70- 91.70	61.70		

102	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
11.672	11.672	(1.260)	75	1261200	50.0000	41.958	80.00- 120.00	100.00		
11.672	11.672	(1.260)	77	397403			1.51- 61.51	31.51		
11.672	11.672	(1.260)	39	641868			20.89- 80.89	50.89		

103	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.032	12.032	(1.298)	58	718507	50.0000	44.185	80.00- 120.00	100.00		
12.032	12.032	(1.298)	43	1799791			0.00- 30.00	250.49		
12.032	12.032	(1.298)	85	294391			0.00- 30.00	40.97		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
105 Toluene						CAS #: 108-88-3			
12.253	12.253	(1.322)	91	2717310	50.0000	42.838	80.00- 120.00	100.00	
12.253	12.253	(1.322)	92	1636082			30.21- 90.21	60.21	

108 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
12.834	12.834	(0.880)	75	1255091	50.0000	41.581	80.00- 120.00	100.00	
12.834	12.834	(0.880)	77	400493			1.91- 61.91	31.91	
12.834	12.834	(0.880)	39	617000			19.16- 79.16	49.16	

110 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.138	13.138	(0.901)	97	887649	50.0000	40.098	80.00- 120.00	100.00	
13.138	13.138	(0.901)	99	562231			33.34- 93.34	63.34	
13.138	13.138	(0.901)	83	775401			57.35- 117.35	87.35	

112 Tetrachloroethene						CAS #: 127-18-4			
13.193	13.193	(0.905)	166	1298482	50.0000	43.339	80.00- 120.00	100.00	
13.193	13.193	(0.905)	129	991416			46.35- 106.35	76.35	
13.193	13.193	(0.905)	131	956045			43.63- 103.63	73.63	

114 2-Hexanone						CAS #: 591-78-6			
13.580	13.580	(0.932)	58	934600	50.0000	42.609	80.00- 120.00	100.00	
13.580	13.580	(0.932)	43	1741943			156.38- 216.38	186.38	
13.580	13.580	(0.932)	100	196484			0.00- 30.00	21.02	

116 Dibromochloromethane						CAS #: 124-48-1			
13.718	13.718	(0.941)	129	1491958	50.0000	43.005	80.00- 120.00	100.00	
13.718	13.718	(0.941)	127	1148185			0.00- 30.00	76.96	

117 1,2-Dibromoethane						CAS #: 106-93-4			
13.884	13.884	(0.953)	107	1442184	50.0000	42.756	80.00- 120.00	100.00	
13.884	13.884	(0.953)	109	1367491			64.82- 124.82	94.82	

126 Chlorobenzene						CAS #: 108-90-7			
14.603	14.603	(1.002)	112	2250487	50.0000	42.096	80.00- 120.00	100.00	
14.603	14.603	(1.002)	114	728256			2.36- 62.36	32.36	
14.603	14.603	(1.002)	77	1258816			25.94- 85.94	55.94	

129 Ethyl Benzene						CAS #: 100-41-4			
14.769	14.769	(1.013)	106	1175267	50.0000	41.541	80.00- 120.00	100.00	
14.769	14.769	(1.013)	91	3603014			0.00- 30.00	306.57	

130 m,p-Xylene						CAS #: 108-38-3			
14.935	14.935	(1.025)	106	1485556	50.0000	43.090	80.00- 120.00	100.00	
14.935	14.935	(1.025)	91	2876195			0.00- 30.00	193.61	

132 o-Xylene						CAS #: 95-47-6			
15.488	15.488	(1.063)	106	1444579	50.0000	41.524	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.488	15.488	(1.063)	91	2916130			171.87- 231.87	201.87	

134 Styrene CAS #: 100-42-5									
15.516	15.516	(1.064)	104	2062765	50.0000	41.998	80.00- 120.00	100.00	
15.516	15.516	(1.064)	78	1099516			23.30- 83.30	53.30	

135 Bromoform CAS #: 75-25-2									
15.765	15.765	(1.082)	173	1397440	50.0000	45.794	80.00- 120.00	100.00	
15.765	15.765	(1.082)	171	714214			21.11- 81.11	51.11	

144 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.456	16.456	(1.129)	83	1948892	50.0000	38.307	80.00- 120.00	100.00	
16.456	16.456	(1.129)	85	1212072			32.19- 92.19	62.19	

147 4-Ethyltoluene CAS #: 622-96-8									
16.649	16.649	(1.142)	105	4004616	50.0000	42.890	80.00- 120.00	100.00	
16.649	16.649	(1.142)	120	1231777			0.76- 60.76	30.76	

148 1,3,5-Trimethylbenzene CAS #: 108-67-8									
16.732	16.732	(1.148)	105	3787759	50.0000	42.205	80.00- 120.00	100.00	
16.732	16.732	(1.148)	120	1919443			0.00- 30.00	50.67	

153 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.147	17.147	(1.176)	105	4046380	50.0000	44.791	80.00- 120.00	100.00	
17.147	17.147	(1.176)	120	1854873			15.84- 75.84	45.84	

156 1,3-Dichlorobenzene CAS #: 541-73-1									
17.451	17.451	(1.197)	146	2634359	50.0000	44.733	80.00- 120.00	100.00	
17.451	17.451	(1.197)	148	1679797			0.00- 30.00	63.76	
17.451	17.451	(1.197)	111	1052350			0.00- 30.00	39.95	

157 1,4-Dichlorobenzene CAS #: 106-46-7									
17.562	17.562	(1.205)	146	2207292	50.0000	39.549	80.00- 120.00	100.00	
17.562	17.562	(1.205)	148	1412857			0.00- 30.00	64.01	
17.562	17.562	(1.205)	111	825860			0.00- 30.00	37.42	

158 alpha-Chlorotoluene CAS #: 100-44-7									
17.700	17.700	(1.214)	91	3353038	50.0000	41.331	80.00- 120.00	100.00	
17.700	17.700	(1.214)	126	728826			0.00- 30.00	21.74	

161 1,2-Dichlorobenzene CAS #: 95-50-1									
17.921	17.921	(1.230)	146	2212931	50.0000	39.009	80.00- 120.00	100.00	
17.921	17.921	(1.230)	148	1430214			34.63- 94.63	64.63	
17.921	17.921	(1.230)	111	864895			9.08- 69.08	39.08	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

167	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.276	19.276	(1.322)	180	2268589	50.0000	39.568	80.00- 120.00	100.00	
19.276	19.276	(1.322)	182	2165957			65.48- 125.48	95.48	

168	Hexachlorobutadiene					CAS #: 87-68-3			
19.359	19.359	(1.328)	225	1766383	50.0000	53.674	80.00- 120.00	100.00	
19.359	19.359	(1.328)	223	1138347			34.45- 94.45	64.45	

145	Propylbenzene					CAS #: 103-65-1			
16.483	16.483	(1.131)	91	4966760	50.0000	45.606	80.00- 120.00	100.00	
16.483	16.483	(1.131)	120	1165920			0.00- 30.00	23.47	
16.483	16.483	(1.131)	105	182446			0.00- 30.00	3.67	

137	Cumene					CAS #: 98-82-8			
15.958	15.958	(1.095)	105	4212680	50.0000	42.919	80.00- 120.00	100.00	
15.958	15.958	(1.095)	120	1104962			0.00- 30.00	26.23	
15.958	15.958	(1.095)	51	414897			0.00- 30.00	9.85	

169	Naphthalene					CAS #: 91-20-3			
19.470	19.470	(1.336)	128	5047042	50.0000	41.740	80.00- 120.00	100.00	
19.470	19.470	(1.336)	127	605911			0.00- 30.00	12.01	

9	Butane					CAS #: 106-97-8			
2.355	2.355	(0.318)	58	224774	50.0000	44.370	80.00- 120.00	100.00	
2.355	2.355	(0.318)	43	1706840			0.00- 30.00	759.36	

15	Isopentane					CAS #: 78-78-4			
2.963	2.963	(0.400)	43	1339432	50.0000	47.590	80.00- 120.00	100.00	
2.963	2.963	(0.400)	57	887974			0.00- 30.00	66.29	
2.963	2.963	(0.400)	72	89127			0.00- 30.00	6.65	

95	Methyl Cyclohexane					CAS #: 108-87-2			
9.903	9.903	(1.336)	83	1556380	50.0000	41.490	80.00- 120.00	100.00	
9.903	9.903	(1.336)	98	707424			0.00- 30.00	45.45	
9.903	9.903	(1.336)	55	1272499			0.00- 30.00	81.76	

Report Date: 22-Jun-2007 10:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-JUN-2007

Lab File ID: 8062202.d

Calibration Time: 10:27

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: jdg

Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m

Misc Info: 100ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	307449	184469	430429	307449	0.00
88 1,4-Difluorobenze	1381560	828936	1934184	1381560	0.00
125 Chlorobenzene-d5	1041151	624691	1457611	1041151	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.41	7.08	7.74	7.41	0.00
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22jun.b/8062202.d
Date: 22-JUN-2007 10:27
Client ID: CCV-1
Sample Info: 100ml #1487-286A

Column phase: RTX-624

Instrument: msd8.1
Operator: jdg
Column diameter: 0.53

/chem/msd8.1/8-22jun.b/8062202.d





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0706310-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062203	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/22/07 10:54 AM

Compound	%Recovery
Freon 12	83
Freon 114	83
Vinyl Chloride	82
Bromomethane	88
Chloroethane	83
Freon 11	85
1,1-Dichloroethene	94
Freon 113	95
Methylene Chloride	94
1,1-Dichloroethane	90
cis-1,2-Dichloroethene	84
Chloroform	80
1,1,1-Trichloroethane	86
Carbon Tetrachloride	92
Benzene	80
1,2-Dichloroethane	89
Trichloroethene	85
1,2-Dichloropropane	84
cis-1,3-Dichloropropene	83
Toluene	89
trans-1,3-Dichloropropene	85
1,1,2-Trichloroethane	82
Tetrachloroethene	87
1,2-Dibromoethane (EDB)	82
Chlorobenzene	85
Ethyl Benzene	80
m,p-Xylene	86
o-Xylene	80
Styrene	81
1,1,2,2-Tetrachloroethane	76
1,3,5-Trimethylbenzene	80
1,2,4-Trimethylbenzene	88
1,3-Dichlorobenzene	90
1,4-Dichlorobenzene	76
alpha-Chlorotoluene	87
1,2-Dichlorobenzene	74
1,3-Butadiene	76
Hexane	94
Cyclohexane	79



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0706310-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	8062203	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 6/22/07 10:54 AM

Compound	%Recovery
Heptane	85
Bromodichloromethane	85
Dibromochloromethane	87
Cumene	89
Propylbenzene	95
Chloromethane	89
1,2,4-Trichlorobenzene	78
Hexachlorobutadiene	106
Acetone	89
Carbon Disulfide	83
2-Propanol	86
trans-1,2-Dichloroethene	82
2-Butanone (Methyl Ethyl Ketone)	84
Tetrahydrofuran	83
1,4-Dioxane	86
4-Methyl-2-pentanone	88
2-Hexanone	80
Bromoform	94
4-Ethyltoluene	86
Ethanol	94
Methyl tert-butyl ether	95
3-Chloropropene	93
2,2,4-Trimethylpentane	81
Naphthalene	76

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	99	70-130
1,2-Dichloroethane-d4	101	70-130
4-Bromofluorobenzene	105	70-130

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 8-22jun
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: jdg
 Data Type: MS DATA SampleType: LCS
 SpikeList File: Spectra.spk Quant Type: ISTD
 Sublist File: AT04+ENSR.sub
 Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Misc Info: 100ppbv-50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
134 Styrene	50.000	40.679	81.36	70-130
108 trans-1,3-Dichloro	50.000	42.305	84.61	70-130
3 Propylene	50.000	44.227	88.45	60-140
4 Dichlorodifluorome	50.000	41.491	82.98	70-130
6 Freon 114	50.000	41.504	83.01	70-130
8 Chloromethane	50.000	44.571	89.14	70-130
11 Vinyl Chloride	50.000	41.282	82.56	70-130
10 1,3-Butadiene	50.000	38.166	76.33	60-140
13 Bromomethane	50.000	44.059	88.12	70-130
16 Chloroethane	50.000	41.631	83.26	70-130
18 Trichlorofluoromet	50.000	42.704	85.41	70-130
23 Ethanol	50.000	47.268	94.54	60-140
28 Freon 113	50.000	47.311	94.62	70-130
29 1,1-Dichloroethene	50.000	47.071	94.14	70-130
30 Acetone	50.000	44.303	88.61	60-140
33 Carbon Disulfide	50.000	41.662	83.32	60-140
34 2-Propanol	50.000	43.045	86.09	60-140
40 Methylene Chloride	50.000	46.900	93.80	70-130
43 MTBE	50.000	47.434	94.87	60-140
45 trans-1,2-Dichloro	50.000	40.962	81.92	60-140
46 Hexane	50.000	46.878	93.76	60-140
54 1,1-Dichloroethane	50.000	44.872	89.74	70-130
55 Vinyl Acetate	50.000	42.703	85.41	60-140
64 cis-1,2-Dichloroet	50.000	42.068	84.14	70-130
65 2-Butanone	50.000	42.045	84.09	60-140
67 Tetrahydrofuran	50.000	41.513	83.03	60-140
70 Chloroform	50.000	40.298	80.60	70-130
73 Cyclohexane	50.000	39.355	78.71	60-140
75 1,1,1-Trichloroeth	50.000	43.075	86.15	70-130
77 Carbon Tetrachlori	50.000	45.932	91.87	70-130
81 Benzene	50.000	40.295	80.59	70-130
83 1,2-Dichloroethane	50.000	44.703	89.41	70-130
85 Heptane	50.000	42.427	84.85	60-140

Report Date: 22-Jun-2007 11:20

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
94 Trichloroethene	50.000	42.364	84.73	70-130
97 1,2-Dichloropropan	50.000	41.933	83.87	70-130
98 1,4-Dioxane	50.000	42.824	85.65	60-140
100 Bromodichlorometha	50.000	42.662	85.32	60-140
102 cis-1,3-Dichloropr	50.000	41.318	82.64	70-130
103 4-Methyl-2-pentano	50.000	43.867	87.73	60-140
105 Toluene	50.000	44.455	88.91	70-130
110 1,1,2-Trichloroeth	50.000	40.760	81.52	70-130
112 Tetrachloroethene	50.000	43.539	87.08	70-130
114 2-Hexanone	50.000	40.019	80.04	60-140
116 Dibromochlorometha	50.000	43.744	87.49	60-140
117 1,2-Dibromoethane	50.000	41.048	82.10	70-130
126 Chlorobenzene	50.000	42.665	85.33	70-130
129 Ethyl Benzene	50.000	39.839	79.68	70-130
130 m,p-Xylene	50.000	43.185	86.37	70-130
132 o-Xylene	50.000	39.854	79.71	70-130
135 Bromoform	50.000	46.962	93.92	60-140
144 1,1,2,2-Tetrachlor	50.000	37.858	75.72	70-130
147 4-Ethyltoluene	50.000	43.298	86.60	60-140
148 1,3,5-Trimethylben	50.000	40.027	80.05	70-130
153 1,2,4-Trimethylben	50.000	43.796	87.59	70-130
156 1,3-Dichlorobenzen	50.000	45.286	90.57	70-130
157 1,4-Dichlorobenzen	50.000	37.858	75.72	70-130
158 alpha-Chlorotoluen	50.000	43.526	87.05	70-130
161 1,2-Dichlorobenzen	50.000	36.915	73.83	70-130
167 1,2,4-Trichloroben	50.000	39.104	78.21	70-130
168 Hexachlorobutadien	50.000	52.780	105.56	70-130
137 Cumene	50.000	44.392	88.78	60-140
145 Propylbenzene	50.000	47.671	95.34	60-140
37 3-Chloropropene	50.000	46.676	93.35	60-140
80 2,2,4-Trimethylpen	50.000	40.580	81.16	60-140
169 Naphthalene	50.000	38.016	76.03	60-140
9 Butane	50.000	43.806	87.61	70-130
15 Isopentane	50.000	45.002	90.00	70-130
95 Methyl Cyclohexane	50.000	41.749	83.50	70-130

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 82 1,2-Dichloroethane	25.000	25.188	100.75	70-130
\$ 104 Toluene-d8	25.000	24.755	99.02	70-130
\$ 140 Bromofluorobenzene	25.000	26.324	105.30	70-130

Report Date: 22-Jun-2007 11:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd8.i/8-22jun.b/8062203.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 22-JUN-2007 10:54
 Operator : jdg Inst ID: msd8.i
 Smp Info : 100ml #1487-275A
 Misc Info : 100ppbv-50ppbv
 Comment :
 Method : /var/chem/msd8.i/8-22jun.b/t14q530b.m
 Meth Date : 22-Jun-2007 10:48 jgray Quant Type: ISTD
 Cal Date : 07-JUN-2007 12:08 Cal File: 8060706.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				(PPBV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====

* 68	Bromochloromethane					CAS #: 74-97-5		
7.387	7.414	(1.000)	130	277791	25.0000	80.00- 120.00	100.00	
7.387	7.414	(1.000)	128	214140		47.85- 107.85	77.09	
7.387	7.387	(1.000)	49	410466		115.74- 175.74	147.76	

* 88	1,4-Difluorobenzene					CAS #: 540-36-3		
9.267	9.267	(1.000)	114	1231802	25.0000	80.00- 120.00	100.00	
9.267	9.267	(1.000)	88	187762		0.00- 44.74	15.24	

* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.576	14.576	(1.000)	117	926071	25.0000	80.00- 120.00	100.00	
14.576	14.576	(1.000)	82	501546		0.00- 30.00	54.16	

\$ 82	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
8.465	8.465	(1.146)	65	366201	25.1879	80.00- 120.00	100.00	
8.465	8.465	(1.146)	67	216718		0.00- 30.00	59.18	

\$ 104	Toluene-d8					CAS #: 2037-26-5		
12.115	12.115	(1.307)	98	1055688	24.7555	80.00- 120.00	100.00	
12.115	12.115	(1.307)	70	105294		0.00- 30.00	9.97	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 104 Toluene-d8 (continued)

12.115	12.115	(1.307)	100	732173			0.00- 30.00	69.36
--------	--------	---------	-----	--------	--	--	-------------	-------

\$ 140 Bromofluorobenzene

CAS #: 460-00-4

16.207	16.207	(1.112)	174	580019	26.3238	26.324	80.00- 120.00	100.00
16.207	16.207	(1.112)	95	705419			91.37- 151.37	121.62
16.207	16.207	(1.112)	176	567489			68.43- 128.43	97.84

3 Propylene

CAS #: 115-07-1

1.995	2.023	(0.270)	41	664970	44.2272	44.227	80.00- 120.00	100.00
1.995	2.023	(0.270)	42	442847			0.00- 30.00	66.60
1.995	2.023	(0.270)	39	450312			0.00- 30.00	67.72

4 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.050	2.078	(0.278)	85	1579062	41.4914	41.491	80.00- 120.00	100.00
2.050	2.078	(0.278)	87	513309			0.00- 30.00	32.51

6 Freon 114

CAS #: 76-14-2

2.161	2.161	(0.293)	135	1426984	41.5035	41.504	80.00- 120.00	100.00
2.161	2.161	(0.293)	137	460421			2.11- 62.11	32.27

8 Chloromethane

CAS #: 74-87-3

2.272	2.299	(0.308)	50	781189	44.5712	44.571	80.00- 120.00	100.00
2.272	2.327	(0.308)	52	242844			0.00- 30.00	31.09

11 Vinyl Chloride

CAS #: 75-01-4

2.410	2.437	(0.326)	62	840752	41.2824	41.282	80.00- 120.00	100.00
2.410	2.437	(0.326)	64	260255			0.00- 30.00	30.96

10 1,3-Butadiene

CAS #: 106-99-0

2.382	2.410	(0.322)	54	664872	38.1662	38.166	80.00- 120.00	100.00
2.382	2.410	(0.322)	39	651034			0.00- 30.00	97.92

13 Bromomethane

CAS #: 74-83-9

2.852	2.880	(0.386)	94	599473	44.0593	44.059	80.00- 120.00	100.00
2.852	2.880	(0.386)	96	567403			64.47- 124.47	94.65

16 Chloroethane

CAS #: 75-00-3

2.935	2.963	(0.397)	64	448715	41.6310	41.631	80.00- 120.00	100.00
2.935	2.963	(0.397)	49	118231			0.00- 30.00	26.35
2.935	2.963	(0.397)	66	140046			0.00- 30.00	31.21

18 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.212	3.239	(0.435)	101	1847243	42.7036	42.704	80.00- 120.00	100.00
3.212	3.239	(0.435)	103	1216670			34.90- 94.90	65.86

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

23 Ethanol CAS #: 64-17-5
 3.516 3.543 (0.476) 45 326509 47.2686 47.268 80.00- 120.00 100.00
 3.516 3.543 (0.476) 43 65585 0.00- 30.00 20.09
 3.516 3.571 (0.476) 46 135105 0.00- 30.00 41.38

28 Freon 113 CAS #: 76-13-1
 3.931 3.958 (0.532) 151 1354067 47.3109 47.311 80.00- 120.00 100.00
 3.931 3.958 (0.532) 153 869792 33.31- 93.31 64.24
 3.931 3.958 (0.532) 101 1554053 84.87- 144.87 114.77

29 1,1-Dichloroethene CAS #: 75-35-4
 3.958 3.986 (0.536) 61 1337914 47.0713 47.071 80.00- 120.00 100.00
 3.958 3.986 (0.536) 96 789313 30.15- 90.15 59.00
 3.958 3.986 (0.536) 98 516697 8.49- 68.49 38.62

30 Acetone CAS #: 67-64-1
 4.124 4.124 (0.558) 58 421749 44.3035 44.303 80.00- 120.00 100.00
 4.124 4.124 (0.558) 43 1276403 0.00- 30.00 302.65

34 2-Propanol CAS #: 67-63-0
 4.290 4.318 (0.581) 45 1481565 43.0447 43.045 80.00- 120.00 100.00
 4.290 4.318 (0.581) 43 292108 0.00- 30.00 19.72
 4.318 4.318 (0.585) 59 58456 0.00- 30.00 3.95

33 Carbon Disulfide CAS #: 75-15-0
 4.290 4.318 (0.581) 76 2219292 41.6620 41.662 80.00- 120.00 100.00

37 3-Chloropropene CAS #: 107-05-1
 4.567 4.594 (0.618) 76 396659 46.6759 46.676 80.00- 120.00 100.00
 4.567 4.594 (0.618) 41 1210551 0.00- 30.00 305.19

40 Methylene Chloride CAS #: 75-09-2
 4.815 4.815 (0.652) 49 998027 46.9005 46.900 80.00- 120.00 100.00
 4.815 4.843 (0.652) 84 691751 39.43- 99.43 69.31
 4.815 4.815 (0.652) 51 296204 0.00- 30.00 29.68

43 MTBE CAS #: 1634-04-4
 5.147 5.175 (0.697) 73 1435526 47.4337 47.434 80.00- 120.00 100.00
 5.147 5.175 (0.697) 57 359896 0.00- 53.46 25.07
 5.147 5.175 (0.697) 41 343700 0.00- 30.00 23.94

45 trans-1,2-Dichloroethene CAS #: 156-60-5
 5.175 5.202 (0.701) 96 823852 40.9618 40.962 80.00- 120.00 100.00
 5.175 5.202 (0.701) 61 1244250 122.39- 182.39 151.03
 5.175 5.202 (0.701) 98 535861 0.00- 30.00 65.04

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
46 Hexane						CAS #:	110-54-3			
5.534	5.534	(0.749)	57	1430005	46.8784	46.878	80.00- 120.00	100.00		
5.534	5.534	(0.749)	43	914545			0.00- 30.00	63.95		
5.534	5.534	(0.749)	86	211476			0.00- 30.00	14.79		

54 1,1-Dichloroethane						CAS #:	75-34-3			
5.949	5.949	(0.805)	63	1471207	44.8719	44.872	80.00- 120.00	100.00		
5.949	5.949	(0.805)	65	472158			1.19- 61.19	32.09		

55 Vinyl Acetate						CAS #:	108-05-4			
6.032	6.032	(0.817)	86	197651	42.7032	42.703	80.00- 120.00	100.00		
6.032	6.032	(0.817)	43	2226650			0.00- 30.00	1126.56		
6.032	6.032	(0.817)	42	175140			0.00- 30.00	88.61		

65 2-Butanone						CAS #:	78-93-3			
7.027	7.027	(0.951)	72	387069	42.0455	42.045	80.00- 120.00	100.00		
7.000	7.027	(0.948)	43	1668799			417.96- 477.96	431.14		
7.027	7.027	(0.951)	57	127771			0.00- 30.00	33.01		

64 cis-1,2-Dichloroethene						CAS #:	156-59-2			
6.972	6.972	(0.944)	61	1091631	42.0682	42.068	80.00- 120.00	100.00		
6.972	6.972	(0.944)	96	793599			43.59- 103.59	72.70		
6.972	6.972	(0.944)	98	506946			17.27- 77.27	46.44		

67 Tetrahydrofuran						CAS #:	109-99-9			
7.387	7.387	(1.000)	42	993336	41.5126	41.513	80.00- 120.00	100.00		
7.387	7.387	(1.000)	71	340236			4.29- 64.29	34.25		
7.387	7.387	(1.000)	72	371731			0.00- 30.00	37.42		

70 Chloroform						CAS #:	67-66-3			
7.525	7.525	(1.019)	83	1421947	40.2976	40.298	80.00- 120.00	100.00		
7.525	7.525	(1.019)	85	886042			33.29- 93.29	62.31		

75 1,1,1-Trichloroethane						CAS #:	71-55-6			
7.774	7.774	(1.052)	97	1479916	43.0752	43.075	80.00- 120.00	100.00		
7.774	7.774	(1.052)	99	938987			33.16- 93.16	63.45		

73 Cyclohexane						CAS #:	110-82-7			
7.746	7.746	(1.049)	84	1070697	39.3547	39.355	80.00- 120.00	100.00		
7.746	7.746	(1.049)	56	1445130			104.12- 164.12	134.97		
7.746	7.746	(1.049)	41	725693			36.29- 96.29	67.78		

77 Carbon Tetrachloride						CAS #:	56-23-5			
7.995	8.023	(1.082)	119	1435997	45.9325	45.932	80.00- 120.00	100.00		
7.995	7.995	(1.082)	117	1455929			72.88- 132.88	101.39		

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPEV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

80	2,2,4-Trimethylpentane					CAS #: 540-84-1			
8.465	8.465	(1.146)	57	3295794	40.5795	40.580	80.00-	120.00	100.00
8.465	8.465	(1.146)	56	1060237			0.00-	30.00	32.17
8.465	8.465	(1.146)	41	787890			0.00-	30.00	23.91

81	Benzene					CAS #: 71-43-2			
8.410	8.437	(0.908)	78	2338074	40.2953	40.295	80.00-	120.00	100.00
8.410	8.437	(0.908)	77	527590			0.00-	30.00	22.57

83	1,2-Dichloroethane					CAS #: 107-06-2			
8.603	8.603	(0.928)	62	1009278	44.7033	44.703	80.00-	120.00	100.00
8.603	8.603	(0.928)	64	309770			0.00-	30.00	30.69

85	Heptane					CAS #: 142-82-5			
8.852	8.852	(0.955)	100	255491	42.4270	42.427	80.00-	120.00	100.00
8.852	8.852	(0.955)	43	1543141			0.00-	30.00	603.99
8.852	8.852	(0.955)	71	817951			0.00-	30.00	320.15

94	Trichloroethene					CAS #: 79-01-6			
9.654	9.682	(1.042)	95	934224	42.3636	42.364	80.00-	120.00	100.00
9.682	9.682	(1.045)	130	1000542			76.78-	136.78	107.10
9.654	9.682	(1.042)	97	594063			34.37-	94.37	63.59

97	1,2-Dichloropropane					CAS #: 78-87-5			
10.179	10.179	(1.098)	63	808687	41.9334	41.933	80.00-	120.00	100.00
10.179	10.179	(1.098)	62	572107			40.95-	100.95	70.75
10.179	10.179	(1.098)	41	472555			31.18-	91.18	58.43

98	1,4-Dioxane					CAS #: 123-91-1			
10.428	10.428	(1.125)	88	503724	42.8244	42.824	80.00-	120.00	100.00
10.401	10.428	(1.122)	58	374481			44.44-	104.44	74.34
10.428	10.428	(1.125)	57	115647			0.00-	30.00	22.96

100	Bromodichloromethane					CAS #: 75-27-4			
10.732	10.732	(1.158)	83	1374123	42.6622	42.662	80.00-	120.00	100.00
10.732	10.732	(1.158)	85	853114			31.70-	91.70	62.08

102	cis-1,3-Dichloropropene					CAS #: 10061-01-5			
11.672	11.672	(1.260)	75	1107341	41.3185	41.318	80.00-	120.00	100.00
11.672	11.672	(1.260)	77	347603			1.51-	61.51	31.39
11.672	11.672	(1.260)	39	568431			20.89-	80.89	51.33

103	4-Methyl-2-pentanone					CAS #: 108-10-1			
12.032	12.032	(1.298)	58	636003	43.8666	43.867	80.00-	120.00	100.00
12.032	12.032	(1.298)	43	1595352			0.00-	30.00	250.84
12.032	12.032	(1.298)	85	262555			0.00-	30.00	41.28

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
105 Toluene						CAS #:	108-88-3			
12.225	12.253	(1.319)	91	2514176	44.4549	44.455	80.00-	120.00	100.00	
12.225	12.253	(1.319)	92	1519605			30.21-	90.21	60.44	

108 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
12.834	12.834	(0.880)	75	1135800	42.3052	42.305	80.00-	120.00	100.00	
12.834	12.834	(0.880)	77	349491			1.91-	61.91	30.77	
12.834	12.834	(0.880)	39	546451			19.16-	79.16	48.11	

110 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.138	13.138	(0.901)	97	802566	40.7602	40.760	80.00-	120.00	100.00	
13.138	13.138	(0.901)	99	502891			33.34-	93.34	62.66	
13.138	13.138	(0.901)	83	689007			57.35-	117.35	85.85	

112 Tetrachloroethene						CAS #:	127-18-4			
13.193	13.193	(0.905)	166	1160283	43.5386	43.539	80.00-	120.00	100.00	
13.193	13.193	(0.905)	129	875139			46.35-	106.35	75.42	
13.193	13.193	(0.905)	131	847007			43.63-	103.63	73.00	

114 2-Hexanone						CAS #:	591-78-6			
13.580	13.580	(0.932)	58	780778	40.0195	40.019	80.00-	120.00	100.00	
13.580	13.580	(0.932)	43	1459243			156.38-	216.38	186.90	
13.580	13.580	(0.932)	100	165092			0.00-	30.00	21.14	

116 Dibromochloromethane						CAS #:	124-48-1			
13.719	13.718	(0.941)	129	1349882	43.7446	43.744	80.00-	120.00	100.00	
13.719	13.718	(0.941)	127	1072418			0.00-	30.00	79.45	

117 1,2-Dibromoethane						CAS #:	106-93-4			
13.884	13.884	(0.953)	107	1231520	41.0477	41.048	80.00-	120.00	100.00	
13.884	13.884	(0.953)	109	1165311			64.82-	124.82	94.62	

126 Chlorobenzene						CAS #:	108-90-7			
14.603	14.603	(1.002)	112	2028757	42.6646	42.665	80.00-	120.00	100.00	
14.603	14.603	(1.002)	114	646421			2.36-	62.36	31.86	
14.603	14.603	(1.002)	77	1139409			25.94-	85.94	56.16	

129 Ethyl Benzene						CAS #:	100-41-4			
14.769	14.769	(1.013)	106	1002535	39.8392	39.839	80.00-	120.00	100.00	
14.769	14.769	(1.013)	91	3069629			0.00-	30.00	306.19	

130 m,p-Xylene						CAS #:	108-38-3			
14.935	14.935	(1.025)	106	1324248	43.1847	43.185	80.00-	120.00	100.00	
14.935	14.935	(1.025)	91	2562741			0.00-	30.00	193.52	

132 o-Xylene						CAS #:	95-47-6			
15.488	15.488	(1.063)	106	1233222	39.8538	39.854	80.00-	120.00	100.00	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.488	15.488	(1.063)	91	2534376			171.87- 231.87	205.51	

134 Styrene CAS #: 100-42-5									
15.516	15.516	(1.064)	104	1777153	40.6792	40.679	80.00- 120.00	100.00	
15.516	15.516	(1.064)	78	953637			23.30- 83.30	53.66	

135 Bromoform CAS #: 75-25-2									
15.765	15.765	(1.082)	173	1274689	46.9618	46.962	80.00- 120.00	100.00	
15.765	15.765	(1.082)	171	644689			21.11- 81.11	50.58	

144 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.456	16.456	(1.129)	83	1713159	37.8580	37.858	80.00- 120.00	100.00	
16.456	16.456	(1.129)	85	1048906			32.19- 92.19	61.23	

147 4-Ethyltoluene CAS #: 622-96-8									
16.649	16.649	(1.142)	105	3595836	43.2979	43.298	80.00- 120.00	100.00	
16.649	16.649	(1.142)	120	1101388			0.76- 60.76	30.63	

148 1,3,5-Trimethylbenzene CAS #: 108-67-8									
16.732	16.732	(1.148)	105	3195216	40.0267	40.027	80.00- 120.00	100.00	
16.732	16.732	(1.148)	120	1609976			0.00- 30.00	50.39	

153 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.147	17.147	(1.176)	105	3519110	43.7956	43.796	80.00- 120.00	100.00	
17.147	17.147	(1.176)	120	1673288			15.84- 75.84	47.55	

156 1,3-Dichlorobenzene CAS #: 541-73-1									
17.451	17.451	(1.197)	146	2372157	45.2863	45.286	80.00- 120.00	100.00	
17.451	17.451	(1.197)	148	1526425			0.00- 30.00	64.35	
17.451	17.451	(1.197)	111	913883			0.00- 30.00	38.53	

157 1,4-Dichlorobenzene CAS #: 106-46-7									
17.562	17.562	(1.205)	146	1879351	37.8578	37.858	80.00- 120.00	100.00	
17.562	17.562	(1.205)	148	1199576			0.00- 30.00	63.83	
17.562	17.562	(1.205)	111	715447			0.00- 30.00	38.07	

158 alpha-Chlorotoluene CAS #: 100-44-7									
17.700	17.700	(1.214)	91	3140805	43.5262	43.526	80.00- 120.00	100.00	
17.700	17.700	(1.214)	126	690082			0.00- 30.00	21.97	

161 1,2-Dichlorobenzene CAS #: 95-50-1									
17.921	17.921	(1.230)	146	1862682	36.9153	36.915	80.00- 120.00	100.00	
17.921	17.921	(1.230)	148	1197875			34.63- 94.63	64.31	
17.921	17.921	(1.230)	111	744175			9.08- 69.08	39.95	

CONCENTRATIONS

RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

167	1,2,4-Trichlorobenzene					CAS #: 120-82-1		
19.276	19.276	(1.322)	180	1994190	39.1038	39.104	80.00- 120.00	100.00
19.276	19.276	(1.322)	182	1923557			65.48- 125.48	96.46

168	Hexachlorobutadiene					CAS #: 87-68-3		
19.359	19.359	(1.328)	225	1544965	52.7797	52.780	80.00- 120.00	100.00
19.359	19.359	(1.328)	223	974103			34.45- 94.45	63.05

145	Propylbenzene					CAS #: 103-65-1		
16.483	16.483	(1.131)	91	4617828	47.6713	47.671	80.00- 120.00	100.00
16.483	16.483	(1.131)	120	1089632			0.00- 30.00	23.60
16.483	16.483	(1.131)	105	173919			0.00- 30.00	3.77

137	Cumene					CAS #: 98-82-8		
15.958	15.958	(1.095)	105	3875674	44.3919	44.392	80.00- 120.00	100.00
15.958	15.958	(1.095)	120	1041506			0.00- 30.00	26.87
15.958	15.958	(1.095)	51	375652			0.00- 30.00	9.69

169	Naphthalene					CAS #: 91-20-3		
19.470	19.470	(1.336)	128	4088712	38.0166	38.016	80.00- 120.00	100.00
19.470	19.470	(1.336)	127	505514			0.00- 30.00	12.36

9	Butane					CAS #: 106-97-8		
2.327	2.355	(0.315)	58	200513	43.8065	43.806	80.00- 120.00	100.00
2.327	2.355	(0.315)	43	1522207			0.00- 30.00	759.16

15	Isopentane					CAS #: 78-78-4		
2.935	2.963	(0.397)	43	1144408	45.0023	45.002	80.00- 120.00	100.00
2.963	2.963	(0.401)	57	756383			0.00- 30.00	66.09
2.963	2.963	(0.401)	72	72865			0.00- 30.00	6.37

95	Methyl Cyclohexane					CAS #: 108-87-2		
9.903	9.903	(1.341)	83	1415025	41.7486	41.749	80.00- 120.00	100.00
9.903	9.903	(1.341)	98	644659			0.00- 30.00	45.56
9.903	9.903	(1.341)	55	1156633			0.00- 30.00	81.74

Report Date: 22-Jun-2007 11:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd8.i

Calibration Date: 22-JUN-2007

Lab File ID: 8062203.d

Calibration Time: 10:27

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: jdg

Method File: /var/chem/msd8.i/8-22jun.b/t14q530b.m

Misc Info: 100ppbv-50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	307449	184469	430429	277791	-9.65
88 1,4-Difluorobenze	1381560	828936	1934184	1231802	-10.84
125 Chlorobenzene-d5	1041151	624691	1457611	926071	-11.05

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
68 Bromochloromethan	7.41	7.08	7.74	7.39	-0.37
88 1,4-Difluorobenze	9.27	8.94	9.60	9.27	0.00
125 Chlorobenzene-d5	14.58	14.25	14.91	14.58	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd8.1/8-22jun.b/8062203.d
Date: 22-JUN-2007 10:54
Client ID: LCS-1
Sample Info: 100ml #1487-275A

Column phase: RTX-624

Instrument: msd8.1
Operator: jdg
Column diameter: 0.53

/chem/msd8.1/8-22jun.b/8062203.d



10	X	B012210	0700312-03A	33923	160 ^{1/4} Sp	30ml	3835	OK	6/22/07	1914	OK	200x
11	X			1662	170 ^{1/4} Sp	20ml	15100	↓		1749	LR	500x REPR
12	X			31157	2.5 ^{1/4} Sp	36ml	9930	↓		1825	BR	1000x
13	✓			33923	160 ^{1/4} Sp	2.5ml	230	KR		1925	KR	1/8" 224-TMP
14	✓			1602	170 ^{1/4} Sp	0.5ml	1210	↓		1953	KR	1/8" 224-TMP
15	✓			31157	2.5 ^{1/4} Sp	0.5ml	584	↓		2021	KR	1/8" 224-TMP
16	✓			34393	Humistyl	200ml	1000	↓		2106	KR	
17	✓			25301	60 ^{1/4} Sp	↓	168	↓		2213	LR	
18	✓			12678	60 ^{1/4} Sp	↓	168	↓		2256	OK	
19	✓			3717	125 ^{1/4} Sp	↓	230	↓		2338	OK	
20	✓			4068	55 ^{1/4} Sp	↓	164	↓		0021	OK	
21	✓			13842	40 ^{1/4} Sp	↓	155	↓		6103	OK	
22	X			35745	10 ^{1/4} Sp	0.5ml	5560	↓		6138	OK	500x REPR
23	X			04586	55 ^{1/4} Sp	1.0ml	32100	↓		6214	OK	1000x REPR
24	X			36639	20 ^{1/4} Sp	1.0ml	35000	↓		0242	OK	1000x REPR
25												
26												
27												
28												
29												
30												
31												
32												

Comments:

~~6/25/07~~

Signature *AS*

Date 6/25/07

Report Date: 30-May-2007 13:12

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-30may.b/8053001.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 30-MAY-2007 13:20
 Operator : db Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2981
 Comment :
 Method : /var/chem/msd8.i/8-30may.b/bfb30.m
 Meth Date : 30-May-2007 13:12 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb						CAS #: 460-00-4	
3.693	3.748	-0.055	95	2045811			100.00- 100.00	100.00
3.693	3.748	-0.055	50	359998			15.00- 40.00	17.60
3.693	3.748	-0.055	75	919533			30.00- 60.00	44.95
3.693	3.748	-0.055	96	129781			5.00- 9.00	6.34
3.693	3.748	-0.055	173	0			0.00- 2.00	0.00
3.693	3.748	-0.055	174	1680993			50.00- 100.00	82.17
3.693	3.748	-0.055	175	121284			5.00- 9.00	7.22
3.693	3.748	-0.055	176	1646565			95.00- 101.00	97.95
3.693	3.748	-0.055	177	100750			5.00- 9.00	6.12

Date : 30-MAY-2007 13:20

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: db

Column phase:

Column diameter: 0.53



Date : 30-MAY-2007 13:20

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: db

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	17.60
75	30.00 - 60.00% of mass 95	44.95
96	5.00 - 9.00% of mass 95	6.34
173	Less than 2.00% of mass 174	0.00 (0.00)
174	50.00 - 100.00% of mass 95	82.17
175	5.00 - 9.00% of mass 174	5.93 (7.22)
176	95.00 - 101.00% of mass 174	80.48 (97.95)
177	5.00 - 9.00% of mass 176	4.92 (6.12)

Date : 30-MAY-2007 13:20

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: db

Column phase:

Column diameter: 0.53

Data File: 8053001.d

Spectrum: Avg. Scans 22-24 (3.69), Background Scan 20

Location of Maximum: 95.00

Number of points: 203

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	14576	88.00	69600	146.00	2289	224.00	96
37.00	81912	90.00	71	147.00	735	226.00	106
38.00	72104	91.00	5332	148.00	3537	227.00	79
39.00	27744	92.00	45488	149.00	517	230.00	71
40.00	666	93.00	72336	150.00	1526	232.00	7
41.00	282	94.00	200896	151.00	3455	233.00	69
42.00	266	95.00	2045440	152.00	1099	234.00	53
43.00	1037	96.00	129776	153.00	1348	236.00	162
44.00	8880	97.00	3615	154.00	793	237.00	106
45.00	14430	99.00	151	155.00	3949	239.00	128
46.00	773	100.00	254	156.00	1096	241.00	12
47.00	25872	104.00	5055	157.00	2094	246.00	153
48.00	9871	105.00	596	158.00	402	249.00	187
49.00	74368	106.00	4503	159.00	2163	253.00	2495
50.00	359936	107.00	988	160.00	268	254.00	409
51.00	108176	108.00	555	161.00	1464	256.00	228
52.00	4377	110.00	383	165.00	310	260.00	2065
53.00	38	111.00	999	166.00	280	261.00	288
54.00	179	112.00	318	167.00	31	262.00	141
55.00	3691	113.00	871	168.00	406	263.00	49
56.00	23056	114.00	168	169.00	116	271.00	132
57.00	42176	115.00	1417	170.00	525	272.00	213
58.00	1681	116.00	4417	171.00	529	274.00	165
59.00	870	117.00	7444	172.00	147	277.00	227
60.00	14254	118.00	4536	174.00	1680896	278.00	250
61.00	78008	119.00	5766	175.00	121280	280.00	96
62.00	77280	120.00	141	176.00	1646080	283.00	9
63.00	54928	121.00	37	177.00	100744	286.00	82
64.00	4760	122.00	334	178.00	2548	293.00	62
65.00	299	123.00	262	179.00	303	294.00	193
66.00	139	124.00	1026	180.00	158	306.00	23
67.00	4680	125.00	80	181.00	28	307.00	84
68.00	174208	126.00	853	182.00	414	312.00	77
69.00	170368	127.00	1542	185.00	250	313.00	20
70.00	12581	128.00	6593	190.00	92	314.00	35

Date : 30-MAY-2007 13:20

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: db

Column phase:

Column diameter: 0.53

Data File: 8053001.d

Spectrum: Avg. Scans 22-24 (3.69), Background Scan 20

Location of Maximum: 95.00

Number of points: 203

m/z	Y	m/z	Y	m/z	Y	m/z	Y
71.00	479	129.00	2422	191.00	1655	315.00	123
72.00	8178	130.00	5089	193.00	1111	316.00	69
73.00	70936	131.00	2310	195.00	988	317.00	75
74.00	282304	132.00	264	196.00	87	324.00	162
75.00	919488	133.00	5559	198.00	244	327.00	112
76.00	77456	134.00	717	200.00	181	328.00	238
77.00	9607	135.00	3857	202.00	196	331.00	341
78.00	6315	137.00	2383	204.00	252	337.00	8
79.00	28224	138.00	384	205.00	48	338.00	80
80.00	10980	139.00	23	207.00	1232	341.00	15
81.00	30280	140.00	1176	209.00	15	342.00	184
82.00	8002	141.00	14199	217.00	163	343.00	1020
83.00	870	142.00	1290	218.00	108	344.00	224
85.00	271	143.00	13753	219.00	292	345.00	257
86.00	2288	144.00	540	222.00	218	347.00	112
87.00	76888	145.00	517	223.00	143		

Report Date: 31-May-2007 10:40

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-31may.b/8053101.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 31-MAY-2007 10:48
 Operator : JG Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2981
 Comment :
 Method : /var/chem/msd8.i/8-31may.b/bfb30.m
 Meth Date : 31-May-2007 10:40 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb					CAS #: 460-00-4		
3.665	3.748	-0.083	95	2098550			100.00- 100.00	100.00
3.665	3.748	-0.083	50	381786			15.00- 40.00	18.19
3.665	3.748	-0.083	75	968533			30.00- 60.00	46.15
3.665	3.748	-0.083	96	132439			5.00- 9.00	6.31
3.665	3.748	-0.083	173	0			0.00- 2.00	0.00
3.665	3.748	-0.083	174	1305650			50.00- 100.00	62.22
3.665	3.748	-0.083	175	94421			5.00- 9.00	7.23
3.665	3.748	-0.083	176	1269961			95.00- 101.00	97.27
3.665	3.748	-0.083	177	79443			5.00- 9.00	6.26

Date : 31-MAY-2007 10:48

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53



Date : 31-MAY-2007 10:48

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	18.19
75	30.00 - 60.00% of mass 95	46.15
96	5.00 - 9.00% of mass 95	6.31
173	Less than 2.00% of mass 174	0.00 (0.00)
174	50.00 - 100.00% of mass 95	62.22
175	5.00 - 9.00% of mass 174	4.50 (7.23)
176	95.00 - 101.00% of mass 174	60.52 (97.27)
177	5.00 - 9.00% of mass 176	3.79 (6.26)

Date : 31-MAY-2007 10:48

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8053101.d

Spectrum: Avg. Scans 21-23 (3.67), Background Scan 19

Location of Maximum: 95.00

Number of points: 214

m/z	Y	m/z	Y	m/z	Y	m/z	Y
35,00	137	94,00	205184	151,00	3262	228,00	71
36,00	14156	95,00	2098176	152,00	1052	231,00	253
37,00	84784	96,00	132416	153,00	1057	234,00	294
38,00	75080	97,00	3341	154,00	736	239,00	62
39,00	28376	99,00	48	155,00	3200	240,00	97
40,00	1047	101,00	315	156,00	909	242,00	73
41,00	106	102,00	203	157,00	2816	244,00	149
42,00	55	103,00	657	158,00	559	247,00	572
43,00	211	104,00	5350	159,00	1429	248,00	254
44,00	7388	105,00	2049	160,00	60	249,00	409
45,00	14858	106,00	5376	161,00	1271	253,00	1015
46,00	633	107,00	1173	162,00	125	254,00	514
47,00	26592	108,00	2447	164,00	421	255,00	420
48,00	10731	110,00	632	165,00	504	260,00	2797
49,00	76568	111,00	502	166,00	207	261,00	644
50,00	381760	112,00	639	168,00	29	262,00	211
51,00	113200	113,00	462	169,00	293	263,00	573
52,00	4745	114,00	191	170,00	825	266,00	105
54,00	329	115,00	1370	171,00	202	268,00	539
55,00	4012	116,00	4406	172,00	1168	269,00	2080
56,00	23784	117,00	7635	174,00	1305600	271,00	417
57,00	44856	118,00	4301	175,00	94416	272,00	226
58,00	1605	119,00	5713	176,00	1269760	276,00	73
59,00	94	120,00	206	177,00	79440	277,00	70
60,00	15955	121,00	85	178,00	2019	280,00	67
61,00	80456	122,00	442	179,00	232	284,00	33
62,00	80808	123,00	276	182,00	265	286,00	285
63,00	59272	124,00	626	184,00	73	290,00	69
64,00	4612	125,00	654	187,00	309	294,00	279
65,00	347	126,00	665	189,00	56	297,00	97
67,00	4333	127,00	383	190,00	468	304,00	67
68,00	183360	128,00	6237	192,00	470	305,00	75
69,00	178944	129,00	2514	194,00	219	308,00	6
70,00	12538	130,00	5415	195,00	187	312,00	97
71,00	154	131,00	1580	196,00	51	313,00	93

Date : 31-MAY-2007 10:48

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8053101.d
Spectrum: Avg. Scans 21-23 (3.67), Background Scan 19
Location of Maximum: 95.00
Number of points: 214

m/z	Y	m/z	Y	m/z	Y	m/z	Y
72.00	9221	132.00	642	197.00	155	320.00	79
73.00	77056	133.00	4651	198.00	68	321.00	66
74.00	293888	134.00	94	201.00	293	322.00	31
75.00	968512	135.00	3077	202.00	2	325.00	87
76.00	80984	136.00	556	204.00	196	326.00	336
77.00	10372	137.00	1762	207.00	4437	327.00	374
78.00	6903	138.00	535	209.00	907	329.00	379
79.00	30680	139.00	313	210.00	269	330.00	28
80.00	11058	140.00	959	211.00	98	331.00	523
81.00	32776	141.00	12035	212.00	77	332.00	108
82.00	7583	142.00	1761	215.00	383	333.00	61
83.00	817	143.00	13357	216.00	126	336.00	57
85.00	193	144.00	630	217.00	405	337.00	293
86.00	1722	145.00	1013	218.00	98	340.00	72
87.00	76424	146.00	1173	219.00	148	345.00	27
88.00	75128	147.00	1632	220.00	54	346.00	86
91.00	5521	148.00	3013	221.00	230	347.00	328
92.00	47968	149.00	1108	223.00	29		
93.00	70904	150.00	1355	226.00	7		

Report Date: 07-Jun-2007 09:36

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-07jun.b/8060701.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 07-JUN-2007 09:44
 Operator : JG Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2981
 Comment :
 Method : /var/chem/msd8.i/8-07jun.b/bfb30.m
 Meth Date : 07-Jun-2007 09:36 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb						CAS #: 460-00-4	
3.693	3.748	-0.055	95	1547009			100.00- 100.00	100.00
3.693	3.748	-0.055	50	260935			15.00- 40.00	16.87
3.693	3.748	-0.055	75	686126			30.00- 60.00	44.35
3.693	3.748	-0.055	96	100570			5.00- 9.00	6.50
3.693	3.748	-0.055	173	0			0.00- 2.00	0.00
3.693	3.748	-0.055	174	1270075			50.00- 100.00	82.10
3.693	3.748	-0.055	175	91158			5.00- 9.00	7.18
3.693	3.748	-0.055	176	1238372			95.00- 101.00	97.50
3.693	3.748	-0.055	177	79712			5.00- 9.00	6.44

Data File: /var/chem/msd8.i/8-07jun,b/8060701.d

Page 1

Date : 07-JUN-2007 09:44

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53



Date : 07-JUN-2007 09:44

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	16.87
75	30.00 - 60.00% of mass 95	44.35
96	5.00 - 9.00% of mass 95	6.50
173	Less than 2.00% of mass 174	0.00 (0.00)
174	50.00 - 100.00% of mass 95	82.10
175	5.00 - 9.00% of mass 174	5.89 (7.18)
176	95.00 - 101.00% of mass 174	80.05 (97.50)
177	5.00 - 9.00% of mass 176	5.15 (6.44)

Date : 07-JUN-2007 09:44

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8060701.d

Spectrum: Avg. Scans 22-24 (3.69), Background Scan 19

Location of Maximum: 95.00

Number of points: 200

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	9970	95.00	1546752	151.00	1962	239.00	118
37.00	57896	96.00	100568	152.00	814	240.00	95
38.00	52136	97.00	2753	153.00	984	241.00	353
39.00	19648	98.00	161	154.00	1010	243.00	71
40.00	588	100.00	167	155.00	3800	244.00	176
43.00	197	101.00	285	157.00	2246	246.00	120
44.00	4251	102.00	16	158.00	327	247.00	6
45.00	9185	103.00	22	159.00	1499	248.00	11
46.00	342	104.00	4146	161.00	1320	253.00	36
47.00	19488	105.00	117	163.00	412	260.00	741
48.00	7926	106.00	4264	164.00	210	262.00	130
49.00	52552	107.00	1026	165.00	348	264.00	100
50.00	260928	108.00	312	167.00	140	265.00	313
51.00	78664	109.00	104	168.00	485	266.00	130
52.00	3036	110.00	448	169.00	66	267.00	225
53.00	118	111.00	533	170.00	415	269.00	1562
55.00	2142	112.00	413	171.00	196	270.00	1087
56.00	15891	113.00	724	172.00	123	273.00	281
57.00	28648	115.00	1346	174.00	1269760	277.00	76
58.00	1367	116.00	3207	175.00	91152	279.00	262
60.00	10831	117.00	5498	176.00	1238016	280.00	71
61.00	56968	118.00	4049	177.00	79712	283.00	90
62.00	56216	119.00	5853	178.00	2338	291.00	69
63.00	41432	121.00	1635	180.00	88	293.00	255
64.00	3731	122.00	373	183.00	322	294.00	81
65.00	363	123.00	369	186.00	156	295.00	90
66.00	70	124.00	635	188.00	13	296.00	257
67.00	2845	125.00	463	189.00	96	297.00	347
68.00	125112	126.00	226	191.00	373	298.00	75
69.00	129024	127.00	748	192.00	133	306.00	333
70.00	8669	128.00	3748	193.00	163	307.00	133
72.00	6050	129.00	2217	194.00	325	309.00	140
73.00	53624	130.00	4252	196.00	3	311.00	123
74.00	208320	131.00	1446	197.00	94	312.00	69
75.00	686080	133.00	2990	201.00	184	313.00	385

Date : 07-JUN-2007 09:44

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8060701.d

Spectrum: Avg. Scans 22-24 (3.69), Background Scan 19

Location of Maximum: 95.00

Number of points: 200

m/z	Y	m/z	Y	m/z	Y	m/z	Y
76.00	57288	134.00	774	203.00	75	314.00	315
77.00	7929	135.00	3276	204.00	97	316.00	128
78.00	5211	136.00	534	208.00	463	323.00	154
79.00	20992	137.00	1598	210.00	12	324.00	52
80.00	8519	138.00	533	213.00	69	328.00	104
81.00	22688	140.00	855	216.00	79	331.00	184
82.00	6628	141.00	10503	217.00	7	332.00	155
83.00	282	142.00	1289	220.00	40	334.00	738
86.00	1293	143.00	10201	222.00	82	335.00	292
87.00	57576	144.00	550	224.00	74	336.00	256
88.00	55552	145.00	522	225.00	34	337.00	184
90.00	170	146.00	1223	233.00	391	347.00	72
91.00	4158	147.00	355	235.00	251		
92.00	33184	148.00	2820	236.00	228		
93.00	54200	149.00	926	237.00	151		
94.00	153536	150.00	1082	238.00	199		

Report Date: 22-Jun-2007 09:50

Air Toxics Ltd.

Data file : /var/chem/msd8.i/8-22jun.b/8062201.d
 Lab Smp Id: BFB Client Smp ID: BFB
 Inj Date : 22-JUN-2007 09:57
 Operator : JG Inst ID: msd8.i
 Smp Info : BFB Tune Check
 Misc Info : 50ng 2uL #843-2980
 Comment :
 Method : /var/chem/msd8.i/8-22jun.b/bfb30.m
 Meth Date : 22-Jun-2007 09:50 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	2.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE	(ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb								
3.693	3.748	-0.055	95	1146282			100.00- 100.00	100.00
3.693	3.748	-0.055	50	219957			15.00- 40.00	19.19
3.693	3.748	-0.055	75	539674			30.00- 60.00	47.08
3.693	3.748	-0.055	96	75837			5.00- 9.00	6.62
3.693	3.748	-0.055	173	2471			0.00- 2.00	0.29
3.693	3.748	-0.055	174	862336			50.00- 100.00	75.23
3.693	3.748	-0.055	175	63362			5.00- 9.00	7.35
3.693	3.748	-0.055	176	846852			95.00- 101.00	98.20
3.693	3.748	-0.055	177	54888			5.00- 9.00	6.48

Date : 22-JUN-2007 09:57

Client ID: BFB

Instrument: msd8.i


Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53



Date : 22-JUN-2007 09:57

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check


Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	19.19
75	30.00 - 60.00% of mass 95	47.08
96	5.00 - 9.00% of mass 95	6.62
173	Less than 2.00% of mass 174	0.22 (0.29)
174	50.00 - 100.00% of mass 95	75.23
175	5.00 - 9.00% of mass 174	5.53 (7.35)
176	95.00 - 101.00% of mass 174	73.88 (98.20)
177	5.00 - 9.00% of mass 176	4.79 (6.48)

Date : 22-JUN-2007 09:57

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8062201.d

Spectrum: Avg. Scans 22-24 (3.69), Background Scan 19

Location of Maximum: 95.00

Number of points: 168

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	8621	87.00	42416	137.00	1416	203.00	83
37.00	49984	88.00	42304	138.00	98	204.00	98
38.00	44200	90.00	67	139.00	230	207.00	565
39.00	17528	91.00	2909	140.00	615	208.00	203
40.00	785	92.00	27424	141.00	7939	221.00	2
44.00	3789	93.00	42120	142.00	1059	233.00	10
45.00	8070	94.00	119496	143.00	8779	236.00	71
46.00	509	95.00	1145856	144.00	540	237.00	68
47.00	15359	96.00	75832	145.00	947	239.00	68
48.00	6567	97.00	2356	146.00	1255	240.00	66
49.00	45024	101.00	239	147.00	791	247.00	160
50.00	219904	103.00	110	148.00	2078	248.00	83
51.00	65416	104.00	3151	149.00	866	251.00	123
52.00	2404	105.00	777	150.00	1051	252.00	96
55.00	1613	106.00	3261	151.00	749	253.00	481
56.00	13780	107.00	902	152.00	684	254.00	187
57.00	24256	108.00	40	153.00	504	255.00	52
58.00	939	110.00	176	154.00	751	261.00	221
59.00	314	111.00	418	155.00	2463	266.00	211
60.00	9231	112.00	551	156.00	384	267.00	237
61.00	46728	113.00	558	157.00	1672	269.00	1165
62.00	46640	115.00	806	158.00	454	270.00	372
63.00	33600	116.00	2560	159.00	1272	271.00	70
64.00	3180	117.00	4955	161.00	944	282.00	1
65.00	274	118.00	2580	162.00	198	284.00	5
66.00	218	119.00	3898	169.00	317	297.00	75
67.00	2354	120.00	147	170.00	275	311.00	76
68.00	104272	121.00	74	171.00	580	322.00	67
69.00	102536	122.00	218	172.00	148	326.00	70
70.00	6744	123.00	457	173.00	2471	327.00	39
72.00	4860	124.00	685	174.00	862336	329.00	264
73.00	43552	125.00	542	175.00	63360	331.00	433
74.00	166144	126.00	379	176.00	846848	334.00	114
75.00	539648	127.00	454	177.00	54888	335.00	67
76.00	44888	128.00	3185	178.00	1266	336.00	81

Date : 22-JUN-2007 09:57

Client ID: BFB

Instrument: msd8.i

Sample Info: BFB Tune Check

Volume Injected (uL): 2.0

Operator: JG

Column phase:

Column diameter: 0.53

Data File: 8062201.d

Spectrum: Avg. Scans 22-24 (3.69), Background Scan 19

Location of Maximum: 95.00

Number of points: 168

m/z	Y	m/z	Y	m/z	Y	m/z	Y
77.00	5884	129.00	1631	179.00	53	343.00	470
78.00	3922	130.00	3535	181.00	75	344.00	14
79.00	17616	131.00	1476	187.00	86	345.00	22
80.00	6502	132.00	325	190.00	157	346.00	255
81.00	18296	133.00	946	191.00	89		
82.00	4378	134.00	333	192.00	111		
83.00	417	135.00	1461	193.00	69		
86.00	1261	136.00	207	197.00	67		

Shipping/ Receiving Documents



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: _____ GEI Consultants, Inc.
ATTENTION: _____ Ms. Sarah Aldridge
FAX #: _____ 860-368-5307
FROM: _____ Sample Receiving
Workorder #: _____ 0706310
of pages (Including Cover): _____ 1

7/3/2007

Thank you for selecting Air Toxics Ltd. We have received your samples and have found discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Alicia Sullivan at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

The following discrepancy has been observed:

We have found a discrepancy between the Chain of Custody (COC) and the sample tags. The samples labeled AMS2-UW and AMS4+60N-DW on the COC are labeled as 061307AMS2-UW and 061307AMS4+60N-DW on the sample tags. ATL will report the sample identifications on the COC unless otherwise notified.

Your prompt response is appreciated.

Receipt VRL 6/16/07

AIR TOXICS LTD.

AN ENVIRONMENTAL ANALYTICAL LABORATORY

CHAIN-OF-CUSTODY RECORD

Sample Transportation Notice

Relinquishing signature on this document indicates that sample is being shipped in compliance with all applicable local, State, Federal, National, and international laws, regulations and ordinances of any kind. Air Toxics Limited assumes no liability with respect to the collection, handling, or shipping of these samples. Relinquishing signature also indicates agreement to hold harmless, defend, and indemnify Air Toxics Limited against any claim, demand, or action of any kind, related to the collection, handling, or shipping of samples. D.O.T. Hotline (800) 457-4922

180 BLUE RAVINE ROAD, SUITE B
 FOLSOM, CA 95630-4719
 (916) 985-1000 FAX: (916) 985-1020

Contact	Project Info:	Turn Around Time:
Company: GEI Consultants, Inc.	P.O. #	<input checked="" type="checkbox"/> Normal
Address: 455 Winding Brook Glastonbury CT 06033	Project #	<input type="checkbox"/> Rush
Phone: 860-368-5300 Cell:	Project Name	Specify _____
Collected By: Signature: <i>[Signature]</i>	BayShore OVI Southern cell Air Monitoring	

Lab I.D.	Field Sample I.D.	Date & Time	Analyses Requested	Canister Pressure/Vacuum Initial	Final	Receipt
01A	PM542-UW	6/13/07 6:30-1:50P	TO-15 + Naphthalene	-30	-14.5	12.05/11.6
02A	PM544+100N-DW	6/13/07 6:55-1:50P	TO-15 + Naphthalene	-30	-7.5	5.54/4.9

Relinquished By: (Signature) Date/Time	Received By: (Signature) Date/Time	Notes: used flow controllers included
Relinquished By: (Signature) Date/Time	Received By: (Signature) Date/Time	Initial and final can pressures in inches Hg
Relinquished By: (Signature) Date/Time	Received By: (Signature) Date/Time	Send Data Pack to Lisa McDonough and EDD to datagroup@geiconsultants.com

LAB	Shipper Name	Alt. Bill #	Opened By	Temp (C)	Condition	Customs Seal/Mark	Matl. Order #
Use Only	FedEx	8617 5870 7653	MG	N/A	Good	Yes No None	070631



AN ENVIRONMENTAL ANALYTICAL LABORATORY

SAMPLE RECEIPT SUMMARY

WORKORDER 0706310

Client

Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Dr. Suite 201
Glastonbury, CT 06033

Phone

860-368-5300

Fax

860-368-5307

Date Promised: 06/29/07

Date Completed: 6/27/07

Date Received: 6/15/07

PO#: NR

Project#: 061140-8-1703 BayShore OU1 Southern cell
Air Monitorin

Total \$: \$ 624.00

Logged By: MG

Sales Rep: ANS

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A	AMS2-UW	Modified TO-15	6/13/2007	12.5 "Hg	\$225.00
02A	AMS4+60N-DW	Modified TO-15	6/13/2007	5.5 "Hg	\$225.00
03A	Lab Blank	Modified TO-15	NA	NA	\$0.00
04A	CCV	Modified TO-15	NA	NA	\$0.00
05A	LCS	Modified TO-15	NA	NA	\$0.00
Misc. Charges 6 Liter Summa Canister (2) @ \$50.00 each.					\$100.00
Blue Body Flow Controller (2) @ \$35.00 each.					\$70.00
Fuel Surcharge (2) @ \$2.00 each.					\$4.00

Note: Samples received after 3 P.M. PST are considered to be received on the following work day.
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

BILL TO: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Dr. Suite 201
Glastonbury, CT 06033

Analysis Code: TO-14A

TERMS:

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

Sample Discrepancy Report

Identification

Initiated By: MG

Date: 6/15/07

Discrepancy Type: I. II. III.
(circle all that apply)

Workorder(s) affected: 0706310

Sample(s) affected: all

I. Sample Receipt Discrepancies

Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative

Narration not required:

- COC was not filled out in Ink.
- Sample container (cartridge/tube/VOA vial) was received broken, however sample was intact.
- Flow controller used - canister samples received at ambient or under pressure.
- No brass cap on canister.
- VOA vial for RSK-175 analysis received with headspace bubble <5mm.

Narration Required:

- COC improperly relinquished / received.
- Sample tags / can numbers do not match the COC.
- Samples received at wrong temperature (up to 10°C); ice / blue ice (circle one) was present. A temp. blank was / was not present (circle one).
- Custody Seal on the outside of the container was broken / improperly placed (circle one).
- Other (describe below).

Describe the Discrepancy: ID tags for OIA read "061307AMS2-UW" and "02A" "061307AMS4-DW" + 60N-DW"
MG 4/15

II. Sample Receipt/Screening Discrepancies requiring CSR notification

Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative

If Section II. is filled out CSR must be notified within 24 hrs of initiation

- COC was not received with samples.
- Analysis method(s) is not specified / incorrectly specified (circle one) on the COC.
- Number of samples on the COC does not match the number of samples that were received.
- Samples were received expired.
- Sampling date / time (sulfur only) is not documented for some / any samples (circle one).
- Sample received with significant (pooling) volume of H₂O in the Tedlar Bag.
- Sample container (cartridge/tube/VOA vial/DNPH Bottle, etc.) was received broken / leaking (circle one); sample can / cannot be analyzed (circle one).
- VOA vial for RSK-175 analysis received with headspace bubble >5mm.
- Samples for RSK-175 CO₂ analysis received preserved with HCl.
- Tedlar Bag received leaking / flat (circle one). Sample can / cannot (circle one) be analyzed.
- Canister was at ambient pressure at time of pressurization and (check all that apply): canister failed leak check on two manifolds, canister valve was open, brass nut was loose. Sample can / cannot be analyzed (circle one).
- Tedlar bag / canister received emitting a strong odor; sample can / cannot (circle one) be analyzed.
- Canister sample received with a vacuum difference >7.0"Hg between the receipt vac. and the final vac. reported on the COC, indicating loss of vacuum.
- Canister sample received at >15"Hg (not identified as a Trip/Field Blank).
- Trip Blank received at low vacuum (< 25"Hg).
- Tedlar Bag for Sulfur analysis has metal fitting.
- Incorrect sampling media / container for analysis requested.
- Sample was received at ≥ 10°C.
- Other (describe below)

Initials: _____
(if not the original initiator)

Date: _____

CSR Notified
(see section below)

Describe the Discrepancy: _____

Other Records

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	

DATA REVIEW CHECKLIST

Work Order #:

0700310

- Analysis/Reporting vs. Project Profile/SOP requirements checked (i.e. 100% Dups, J-Flag to MDL, etc)
- The final report has the correct reporting list, special units, and header info.
- Lab Narrative is correct (proper method & description/Receiving & Analytical notes correct)
- Corrective Action issued - #
- Unusual circumstances have been documented in the notes section below

LUMEN validation report present and initialed

CIRCLE (YES / NO)

- Lab Blank, CCV, LCS and DUP met QC criteria
- Hold time is met for all samples
- Appropriate data qualifier flags are applied
- Manual integrations for samples and QC are properly documented
- Samples analyzed within the project or method specific clock
- Retention times have been verified
- Appropriate ICAL(s) included
- At least one result per sample is verified against the target quant sheets/raw data

- Dilution factor correctly calculated (sample load volume, syringe and bag dilutions, can pressurization(s))
- Correct amount of sample analyzed (i.e. sample not over-diluted)
- Spectra verified - documentation of spectral defense included (Section 5A of eCVP pkg)
- TICs resemble reference spectra
- TICs between duplicate samples are consistent
- Checked samples for trends (i.e. Influent>Effluent, Landfill or Ambient etc)
- Special units for all samples in the final report are correctly calculated
- Manually entered results checked (i.e. special CCV compounds)
- TPH/NMOC (verify calculations and correct reference compound used)
- Chain of Custody scanned correctly
- Verify sample id's vs. chain of custody
- Samples pressurized w/ appropriate gas (N₂ or He) Tedlar Bag only
- Final pressure consistent with canister size (6L vs. 1L)
- Verify receipt pressures against logbook and Target
- Verify canister ID #'s
- Extra printed copies are provided per client profile
- Final invoice amount correct (adjusted for TAT, Penalties, Re-issue Charges etc.)
- Client LUMEN report reviewed for accuracy and completeness

Notes: (to include: noting samples with QA/QC problems, Blanks with positive hits, narratives, etc.)

A/R: *NA out in CCV, LCS*

M/O:

A (Analytical Review/Date)	R/T (Reporting Review/Date)	M (Management Review/Date)	Q (QA Review/Date)
<i>Out 6/25/07</i>	R: <i>[Signature] 6-27-07</i>	<i>[Signature] 6/27/07</i>	
	T: _____		

Not Applicable