



**Air
Toxics LTD.**
Laboratory Services Since 1989

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

COMPREHENSIVE VALIDATION PACKAGE

Modified TO-15

INVENTORY SHEET

Work Order #: 0712439

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	19
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	20	27
b. Surrogate Recover Summary Form (If Applicable)	28	28
c. Internal Standard Summary Form (If Applicable)	29	29
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	30	182
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	183	197
i. Second Source LCS(Summary + Raw Data)	198	211
j. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	212	213
l. GC/MS Tune (Results + Raw Data)	214	238
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	239	240
b. Chain-of-Custody Records	241	241
c. Sample Log-In Sheet	242	242
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	243	244
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	245	247
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	248	249
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	--	--
i. <u>Data Review Check Sheet</u>	250	250

Comments:

Completed by:

Kara McKiernan

Kara McKiernan / Document Control

1/9/08

(Signature)

(Print Name & Title)

(Date)




AN ENVIRONMENTAL ANALYTICAL LABORATORY

WORK ORDER #: 0712439

Work Order Summary

CLIENT:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Drive Suite 201 Glastonbury, CT 06033	BILL TO:	Ms. Sarah Aldridge GEI Consultants, Inc. 455 Winding Brook Drive Suite 201 Glastonbury, CT 06033
PHONE:	860-368-5300	P.O. #	NR
FAX:	860-368-5307	PROJECT #	061140-8-1703 BayShore OU1 Southern
DATE RECEIVED:	12/20/2007	CONTACT:	cell Air Monitorin Bryanna Langley
DATE COMPLETED:	01/07/2008		

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>	<u>FINAL PRESSURE</u>
01A(cancelled)	UW AMS5	Modified TO-15	0.0 "Hg	5 psi
02A	DW AMS3	Modified TO-15	4.5 "Hg	5 psi
03A	Lab Blank	Modified TO-15	NA	NA
04A	CCV	Modified TO-15	NA	NA
05A	LCS	Modified TO-15	NA	NA

CERTIFIED BY:  DATE: 01/07/08

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004
NY NELAP - 11291, UT NELAP - 9166389892

Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,
Accreditation number: E87680, Effective date: 07/01/07, Expiration date: 06/30/08

Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards

This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

LABORATORY NARRATIVE
Modified TO-15
GEI Consultants, Inc.
Workorder# 0712439



Two 6 Liter Summa Canister samples were received on December 20, 2007. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

This workorder was independently validated prior to submittal using 'USEPA National Functional Guidelines' as generally applied to the analysis of volatile organic compounds in air. A rules-based, logic driven, independent validation engine was employed to assess completeness, evaluate pass/fail of relevant project quality control requirements and verification of all quantified amounts.

Method modifications taken to run these samples are summarized in the table below. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	+/- 30% Difference	<= 30% Difference with two allowed out up to <=40%.; flag and narrate outliers
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

Receiving Notes

The canister valve on sample UW AMS5 was received open and a brass plug used to seal the canister was loose. Sample vented to ambient pressure during shipment. At the client's request, the sample was cancelled.

Analytical Notes

There were no analytical discrepancies.

Definition of Data Qualifying Flags

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

B - Compound present in laboratory blank greater than reporting limit (background subtraction no performed).

J - Estimated value.

E - Exceeds instrument calibration range.

S - Saturated peak.

- Q - Exceeds quality control limits.
- U - Compound analyzed for but not detected above the reporting limit.
- UJ- Non-detected compound associated with low bias in the CCV
- N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

- a-File was requantified
- b-File was quantified by a second column and detector
- r1-File was requantified for the purpose of reissue

Table 1

Client Sample ID	Lab Sample ID	Date Collected	Date Received	Date Extracted	Sample Holding Time (Days)	Date Analyzed	Sample Extract Holding Time (Days)	Sample Condition
DW AMS3	0712439-02A	12/19/2007	12/20/2007	NA	10	12/29/2007	NA	Good
Lab Blank	0712439-03A	NA	NA	NA	NA	12/28/2007	NA	Good
CCV	0712439-04A	NA	NA	NA	NA	12/28/2007	NA	Good
LCS	0712439-05A	NA	NA	NA	NA	12/28/2007	NA	Good

Sample Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: DW AMS3

Lab ID#: 0712439-02A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Benzene	0.79	1.3	2.5	4.0
Toluene	0.79	3.2	3.0	12
m,p-Xylene	0.79	1.3	3.4	5.8
Hexane	0.79	0.95	2.8	3.3
2-Butanone (Methyl Ethyl Ketone)	0.79	0.88	2.3	2.6
Ethanol	3.2	4.0	6.0	7.6



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: DW AMS3

Lab ID#: 0712439-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122825	Date of Collection:	12/19/07
Dil. Factor:	1.58	Date of Analysis:	12/29/07 12:08 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.79	Not Detected	3.9	Not Detected
Freon 114	0.79	Not Detected	5.5	Not Detected
Vinyl Chloride	0.79	Not Detected	2.0	Not Detected
Bromomethane	0.79	Not Detected	3.1	Not Detected
Chloroethane	0.79	Not Detected	2.1	Not Detected
Freon 11	0.79	Not Detected	4.4	Not Detected
1,1-Dichloroethene	0.79	Not Detected	3.1	Not Detected
Freon 113	0.79	Not Detected	6.0	Not Detected
Methylene Chloride	0.79	Not Detected	2.7	Not Detected
1,1-Dichloroethane	0.79	Not Detected	3.2	Not Detected
cis-1,2-Dichloroethene	0.79	Not Detected	3.1	Not Detected
Chloroform	0.79	Not Detected	3.8	Not Detected
1,1,1-Trichloroethane	0.79	Not Detected	4.3	Not Detected
Carbon Tetrachloride	0.79	Not Detected	5.0	Not Detected
Benzene	0.79	1.3	2.5	4.0
1,2-Dichloroethane	0.79	Not Detected	3.2	Not Detected
Trichloroethene	0.79	Not Detected	4.2	Not Detected
1,2-Dichloropropane	0.79	Not Detected	3.6	Not Detected
cis-1,3-Dichloropropene	0.79	Not Detected	3.6	Not Detected
Toluene	0.79	3.2	3.0	12
trans-1,3-Dichloropropene	0.79	Not Detected	3.6	Not Detected
1,1,2-Trichloroethane	0.79	Not Detected	4.3	Not Detected
Tetrachloroethene	0.79	Not Detected	5.4	Not Detected
1,2-Dibromoethane (EDB)	0.79	Not Detected	6.1	Not Detected
Chlorobenzene	0.79	Not Detected	3.6	Not Detected
Ethyl Benzene	0.79	Not Detected	3.4	Not Detected
m,p-Xylene	0.79	1.3	3.4	5.8
o-Xylene	0.79	Not Detected	3.4	Not Detected
Styrene	0.79	Not Detected	3.4	Not Detected
1,1,2,2-Tetrachloroethane	0.79	Not Detected	5.4	Not Detected
1,3,5-Trimethylbenzene	0.79	Not Detected	3.9	Not Detected
1,2,4-Trimethylbenzene	0.79	Not Detected	3.9	Not Detected
1,3-Dichlorobenzene	0.79	Not Detected	4.8	Not Detected
1,4-Dichlorobenzene	0.79	Not Detected	4.8	Not Detected
alpha-Chlorotoluene	0.79	Not Detected	4.1	Not Detected
1,2-Dichlorobenzene	0.79	Not Detected	4.7	Not Detected
1,3-Butadiene	0.79	Not Detected	1.7	Not Detected
Hexane	0.79	0.95	2.8	3.3
Cyclohexane	0.79	Not Detected	2.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: DW AMS3

Lab ID#: 0712439-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122825	Date of Collection:	12/19/07
Dil. Factor:	1.58	Date of Analysis:	12/29/07 12:08 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.79	Not Detected	3.2	Not Detected
Bromodichloromethane	0.79	Not Detected	5.3	Not Detected
Dibromochloromethane	0.79	Not Detected	6.7	Not Detected
Cumene	0.79	Not Detected	3.9	Not Detected
Propylbenzene	0.79	Not Detected	3.9	Not Detected
Chloromethane	3.2	Not Detected	6.5	Not Detected
1,2,4-Trichlorobenzene	3.2	Not Detected	23	Not Detected
Hexachlorobutadiene	3.2	Not Detected	34	Not Detected
Acetone	3.2	Not Detected	7.5	Not Detected
Carbon Disulfide	0.79	Not Detected	2.5	Not Detected
2-Propanol	3.2	Not Detected	7.8	Not Detected
trans-1,2-Dichloroethene	0.79	Not Detected	3.1	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.79	0.88	2.3	2.6
Tetrahydrofuran	0.79	Not Detected	2.3	Not Detected
1,4-Dioxane	3.2	Not Detected	11	Not Detected
4-Methyl-2-pentanone	0.79	Not Detected	3.2	Not Detected
2-Hexanone	3.2	Not Detected	13	Not Detected
Bromoform	0.79	Not Detected	8.2	Not Detected
4-Ethyltoluene	0.79	Not Detected	3.9	Not Detected
Ethanol	3.2	4.0	6.0	7.6
Methyl tert-butyl ether	0.79	Not Detected	2.8	Not Detected
3-Chloropropene	3.2	Not Detected	9.9	Not Detected
2,2,4-Trimethylpentane	0.79	Not Detected	3.7	Not Detected
Naphthalene	3.2	Not Detected	16	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	95	70-130
1,2-Dichloroethane-d4	101	70-130
4-Bromofluorobenzene	96	70-130

Report Date: 07-Jan-2008 12:36

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-28dec.b/5122825.d
 Lab Smp Id: 0712439-02A
 Inj Date : 29-DEC-2007 00:08
 Operator : cb Inst ID: msd5.i
 Smp Info : 200mL #34317
 Misc Info : 4.5"Hg --> 5psi CEI
 Comment :
 Method : /chem/msd5.i/5-28dec.b/t14qn12c.m
 Meth Date : 04-Jan-2008 14:12 ctaylor Quant Type: ISTD
 Cal Date : 27-NOV-2007 12:08 Cal File: 5112707.d
 Als bottle: 1
 Dil Factor: 1.58000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	253633	25.0000		80.00- 120.00	100.00	
8.059	8.059	(1.000)	128	195777			50.29- 110.29	77.19	
8.059	8.059	(1.000)	49	582486			207.42- 267.42	229.66	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.912	(1.000)	114	875925	25.0000		80.00- 120.00	100.00	
9.911	9.912	(1.000)	88	147576			0.00- 47.33	16.85	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	689407	25.0000		80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	398095			0.00- 30.00	57.74	

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.137	9.110	(1.134)	65	384320	25.3152	25.315	80.00- 120.00	100.00	
9.137	9.110	(1.134)	67	183651			27.88- 87.88	47.79	

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.677	(1.282)	98	735248	23.7755	23.775	80.00- 120.00	100.00	
12.676	12.677	(1.279)	70	84117			0.00- 40.29	11.44	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT (REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

\$ 107 Toluene-d8 (continued)

12.704	12.677 (1.282)	100	455390			37.87- 97.87	61.94
--------	----------------	-----	--------	--	--	--------------	-------

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575	16.575 (1.105)	174	386264	24.0125	24.012	80.00- 120.00	100.00
16.575	16.575 (1.105)	95	598192			122.99- 182.99	154.87
16.575	16.575 (1.105)	176	377969			64.86- 124.86	97.85

26 Ethanol

CAS #: 64-17-5

4.133	4.078 (0.513)	45	18229	2.56621	4.055	80.00- 120.00	100.00
4.105	4.078 (0.509)	43	2810			0.00- 30.00	15.42
4.133	4.078 (0.513)	46	4854			0.00- 30.00	26.63

51 Hexane

CAS #: 110-54-3

6.151	6.151 (0.763)	57	19873	0.59970	0.9475	80.00- 120.00	100.00
6.151	6.151 (0.763)	43	15277			0.00- 30.00	76.88
6.179	6.151 (0.767)	86	2599			0.00- 30.00	13.08

67 2-Butanone

CAS #: 78-93-3

7.699	7.644 (0.955)	72	3983	0.55934	0.8838	80.00- 120.00	100.00
7.727	7.644 (0.959)	43	191064			590.40- 650.40	4796.69
7.699	7.644 (0.955)	57	1534			0.00- 30.00	38.53

81 Benzene

CAS #: 71-43-2

9.082	9.082 (0.916)	78	30316	0.80298	1.269	80.00- 120.00	100.00
9.082	9.082 (0.916)	77	10295			0.00- 30.00	33.96

108 Toluene

CAS #: 108-88-3

12.815	12.815 (1.293)	91	80018	2.05447	3.246	80.00- 120.00	100.00
12.815	12.815 (1.293)	92	46377			28.40- 88.40	57.96

130 m,p-Xylene

CAS #: 108-38-3

15.331	15.331 (1.022)	106	16699	0.84829	1.340	80.00- 120.00	100.00
15.331	15.331 (1.022)	91	31084			0.00- 30.00	186.14

Report Date: 07-Jan-2008 12:36

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msd5.i
Lab File ID: 5122825.d
Lab Smp Id: 0712439-02ACalibration Date: 28-DEC-2007
Calibration Time: 09:33

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-28dec.b/t14qn12c.m

Misc Info: 4.5"Hg --> 5psi CEI

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	269712	161827	377597	253633	-5.96
92 1,4-Difluorobenze	1058104	634862	1481346	875925	-17.22
125 Chlorobenzene-d5	829571	497743	1161399	689407	-16.90

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-28dec
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0712439-02A
Level: LOW Operator: cb
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 2926Spectra.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /chem/msd5.i/5-28dec.b/t14qn12c.m
Misc Info: 4.5"Hg --> 5psi CEI

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	25.315	101.26	70-130
\$ 107 Toluene-d8	25.000	23.775	95.10	70-130
\$ 138 Bromofluorobenzene	25.000	24.012	96.05	70-130

Data File: /chem/msd5.1/5-28dec.b/5122825.d

Date : 29-DEC-2007 00:08

Client ID:

Sample Info: 200ML #34317


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-28dec.b/5122825.d



Date : 29-DEC-2007 00:08

Client ID:

Instrument: msd5.i

Sample Info: 200mL #34317








Operator: cb

Column phase: RTX-624

Column diameter: 0.53

26 Ethanol

Concentration: 4.055 PPBV



Date : 29-DEC-2007 00:08

Client ID:

Instrument: msd5.i

Sample Info: 200mL #34317








Operator: cb

Column phase: RTX-624

Column diameter: 0.53

51 Hexane

Concentration: 0.9475 PPBV



Date : 29-DEC-2007 00:08

Client ID:

Instrument: msd5,i

Sample Info: 200mL #34317








Operator: cb

Column phase: RTX-624

Column diameter: 0.53

67 2-Butanone

Concentration: 0.8838 PPBV



Date : 29-DEC-2007 00:08

Client ID:

Instrument: msd5.i

Sample Info: 200mL #34317







Operator: cb

Column phase: RTX-624

Column diameter: 0.53

81 Benzene

Concentration: 1.269 PPBV



Date : 29-DEC-2007 00:08

Client ID:

Instrument: msd5.i

Sample Info: 200mL #34317







Operator: cb

Column phase: RTX-624

Column diameter: 0.53

108 Toluene

Concentration: 3.246 PPBV



Date : 29-DEC-2007 00:08

Client ID:

Instrument: msd5.i

Sample Info: 200mL #34317







Operator: cb

Column phase: RTX-624

Column diameter: 0.53

130 m,p-Xylene

Concentration: 1,340 PPBV



QC Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0712439-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122805	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 12/28/07 10:58 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0712439-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122805	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 12/28/07 10:58 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected	2.0	Not Detected
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	98	70-130
1,2-Dichloroethane-d4	108	70-130
4-Bromofluorobenzene	100	70-130

Report Date: 28-Dec-2007 11:04

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-28dec.b/5122805.d
 Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
 Inj Date : 28-DEC-2007 10:58
 Operator : cb Inst ID: msd5.i
 Smp Info : 200mL #13673
 Misc Info : Humid Cert Cart #8 Leg 3
 Comment :
 Method : /var/chem/msd5.i/5-28dec.b/t14qn12c.m
 Meth Date : 28-Dec-2007 09:47 cbond Quant Type: ISTD
 Cal Date : 27-NOV-2007 12:08 Cal File: 5112707.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059 (1.000)	130	269726	25.0000		80.00-	120.00	100.00	
8.059	8.059 (1.000)	128	221919			50.29-	110.29	82.28	
8.059	8.031 (1.000)	49	641892			207.42-	267.42	237.98	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.912 (1.000)	114	995980	25.0000		80.00-	120.00	100.00	
9.911	9.912 (1.000)	88	166105			0.00-	47.33	16.68	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999 (1.000)	117	792086	25.0000		80.00-	120.00	100.00	
14.999	14.999 (1.000)	82	464768			0.00-	30.00	58.68	

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.137	9.110 (1.134)	65	435877	26.9983	26.998	80.00-	120.00	100.00	
9.110	9.110 (1.130)	67	205497			27.88-	87.88	47.15	

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.677 (1.282)	98	862002	24.5143	24.514	80.00-	120.00	100.00	
12.676	12.677 (1.279)	70	92847			0.00-	40.29	10.77	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 107 Toluene-d8 (continued)

12.704 12.677 (1.282) 100 547335 37.87- 97.87 63.50

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575 16.575 (1.105) 174 464201 25.1167 25.117 80.00- 120.00 100.00

16.575 16.575 (1.105) 95 713434 122.99- 182.99 153.69

16.575 16.575 (1.105) 176 437846 64.86- 124.86 94.32

Report Date: 28-Dec-2007 11:04

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 28-DEC-2007

Lab File ID: 5122805.d

Calibration Time: 09:33

Lab Smp Id: Lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /var/chem/msd5.i/5-28dec.b/t14qn12c.m

Misc Info: Humid Cert Cart #8 Leg 3

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	269712	161827	377597	269726	0.01
92 1,4-Difluorobenze	1058104	634862	1481346	995980	-5.87
125 Chlorobenzene-d5	829571	497743	1161399	792086	-4.52

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-28dec
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: Lab Blank Client Smp ID: Lab Blank
Level: LOW Operator: cb
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 2926Spectra.spk Quant Type: ISTD
Sublist File: AT04ENSR.sub
Method File: /var/chem/msd5.i/5-28dec.b/t14qn12c.m
Misc Info: Humid Cert Cart #8 Leg 3

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	26.998	107.99	70-130
\$ 107 Toluene-d8	25.000	24.514	98.06	70-130
\$ 138 Bromofluorobenzene	25.000	25.117	100.47	70-130

Data File: /chem/msd5.1/5-28dec.b/5122805.d

Date: 28-DEC-2007 10:58

Client ID: Lab Blank

Sample Info: 200mL #13673


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-28dec.b/5122805.d



LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0712439

CLIENT SAMPLE NO.	SURROGATE % RECOVERY							TOTAL OUT	
	1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#			#
01	DW AMS3	101		95		96			0
02	Lab Blank	108		98		100			0
03	CCV	111		101		105			0
04	LCS	108		102		105			0
05									0
06									0
07									0
08									0
09									0
10									0
11									0
12									0
13									0
14									0
15									0
16									0
17									0
18									0
19									0
20									0
21									0
22									0
23									0
24									0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

* Designates values outside of QC limits

LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan

INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD
 Lab File ID: 5122803.d
 Instrument ID: msd5.i

SDG No: 0712439
 Date Analyzed: 12/28/2007
 Time Analyzed: 09:33 AM

	Chlorobenzene-d5			1,4-Difluorobenzene			Bromochloromethane		
	Area	#	RT	Area	#	RT	Area	#	RT
24-HOUR STD	829571		15	1058104		9.91	269712		8.06
UPPER LIMIT	1161399		15.33	1481346		10.24	377597		08.39
LOWER LIMIT	497743		14.67	634862		09.58	161827		07.73
CLIENT SAMPLE NO									
01 DW AMS3	689407		15	875925		9.91	253633		8.06
02 Lab Blank	792086		15	995980		9.91	269726		8.06
03 CCV	829571		15	1058104		9.91	269712		8.06
04 LCS	838490		15	1061667		9.91	276210		8.06
05									
06									
07									
08									
09									
10									
11									
12									
13									
14									
15									
16									
17									
18									
19									
20									
21									
22									

'Area Upper Limit=+40% of internal standard area'
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT
 RT Lower Limit=-0.33 minutes of internal standard RT

* Designates values outside of QC limits

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Calibration File Names:

Level 1: /chem/msd5.i/5-12nov.b/5111207.d
 Level 2: /chem/msd5.i/5-12nov.b/5111232.d
 Level 3: /chem/msd5.i/5-27nov.b/5112706.d
 Level 4: /chem/msd5.i/5-12nov.b/5111210.d
 Level 5: /chem/msd5.i/5-27nov.b/5112702.d
 Level 6: /chem/msd5.i/5-12nov.b/5111212.d
 Level 7: /chem/msd5.i/5-27nov.b/5112707.d
 Level 8: /chem/msd5.i/5-13nov.b/5111303.d

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
1 Freon134a	200.000	250.000	0.94452	0.94452	1.13299	1.13299	1.03523	9.122
2 Propane	0.98320	0.98320	0.98320	0.98320	0.98320	0.98320	0.98320	0.98320
3 Freon 152a	0.98320	0.98320	0.75951	0.75951	1.05087	1.05087	0.93120	16.375
4 Freon 22	0.27887	0.27887	0.29507	0.29507	0.29162	0.29162	0.28852	2.957
5 Freon142b	2.06052	2.06052	1.28221	1.28221	2.22653	2.22653	1.85642	27.158
6 Propylene	1.77133	1.77133	1.33663	1.98098	1.84757	1.78835	1.74497	13.907
7 Isobutane	4.69001	4.69001	3.76183	3.76183	5.30591	5.30591	4.58592	16.949

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	RRF	% RSD
8 Dichlorodifluoromethane/Fr12	200.000 Level 7	250.000 Level 8						
	+++++	2.14296	2.41813	3.42716	3.06268	3.40660		
	3.27897	+++++					2.95608	18.473
9 Freon 114	+++++	2.35572	2.34787	3.13944	2.87726	2.78949		
	2.67692	+++++					2.69778	11.432
10 Chloromethane	+++++	+++++	1.60683	2.55808	2.34986	2.35020		
	2.23347	+++++					2.21969	16.310
11 Butane	+++++	+++++	0.42153	0.59949	0.55149	0.53532		
	0.53045	+++++					0.52766	12.376
12 1,3-Butadiene	+++++	1.36769	1.32470	2.25041	2.03875	2.02523		
	1.94101	+++++					1.82463	21.079
13 Vinyl Chloride	+++++	1.94068	1.71199	2.50747	2.31038	2.22243		
	2.12601	+++++					2.13649	13.137
14 Methanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
15 Bromomethane	+++++	1.17885	1.02592	1.63273	1.51216	1.48575		
	1.44040	+++++					1.37930	16.596
16 Dichlorofluoromethane/Fr21	+++++	+++++	1.96732	+++++	2.44556	+++++		
	2.29871	+++++					2.23719	10.950
17 Isopentane	+++++	+++++	2.50260	3.49372	3.22831	3.19381		
	3.05601	+++++					3.09489	11.861

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	RRF	% RSD
18 Pentane	200.000 Level 7	250.000 Level 8	3.62243	5.34445	4.68401	19.822		
19 Chloroethane	1.13285	0.86045	1.28504	1.09440	1.08050	1.08675	12.558	
20 Trichlorofluoromethane/Fr11	2.87555	2.52189	3.78007	3.49996	3.38902	3.22295	14.077	
21 Dimethyl Ether	1.16671	1.25309	1.23982	5.441				
22 Freon123a	1.29965	1.96506	2.55391	2.32714	13.617			
23 Freon 13	0.33707	0.72341	0.58368	36.699				
24 Freon123	2.46247	0.52661	0.83695	0.76785	0.72130	0.70017	16.984	
25 Acrolein	0.69057	0.33707	0.72341	0.58368	36.699			
26 Ethanol	0.64815	0.52661	0.83695	0.76785	0.72130	0.70017	16.984	
27 Isobutylene	0.64815	0.52661	0.83695	0.76785	0.72130	0.70017	16.984	

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
28 Acetaldehyde	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
29 Freon143a	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
30 Freon 113	+++++	1.91659	1.56182	2.37148	2.10219	2.07645	2.00401	13.262
31 1,1-Dichloroethene	+++++	2.21687	2.16206	3.06675	2.86001	2.81451	2.65222	14.016
32 Acetone	+++++	+++++	0.61101	1.11948	1.08688	1.08129	0.99203	21.573
33 Methyl Acetate	+++++	+++++	2.71505	+++++	4.34600	+++++	3.69644	23.391
34 Acetonitrile	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
35 Carbon Disulfide	+++++	3.32414	3.49304	5.41847	4.96922	4.94551	4.49145	19.275
36 2-Propanol	+++++	+++++	2.31777	3.85058	3.80252	3.87240	3.53043	19.219
37 tert-Butyl-Alcohol	+++++	+++++	1.68840	+++++	1.36172	+++++	1.29917	32.635

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
38 3-Chloropropene	+++++	+++++	0.53986	0.82084	0.81735	0.79617		
	0.76493	+++++					0.74783	15.828
39 Acrylonitrile	+++++	+++++	1.31733	+++++	2.12469	+++++		
	2.08501	+++++					1.84234	24.702
40 2-Methyl-1-Butene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
41 Vinyl Bromide	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
42 1-Pentene	+++++	+++++	2.00220	+++++	2.87804	+++++		
	2.70156	+++++					2.52727	18.328
43 Methylene Chloride	+++++	2.18980	1.79922	2.58303	2.37732	2.36058		
	2.29716	+++++					2.26785	11.608
44 Ethyl Ether	+++++	+++++	0.73961	+++++	1.09163	+++++		
	1.03698	+++++					0.95607	19.815
45 Ethanol-high	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
46 MTBE	+++++	2.26968	1.51670	1.87823	1.71311	1.57976		
	1.28551	+++++					1.70717	19.882
47 trans-1,2-Dichloroethene	+++++	1.16025	1.27834	1.92147	1.76911	1.77243		
	1.73593	+++++					1.60625	19.224

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	RRF	% RSD
48 Propanal	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
49 Isopropyl ether	+++++	+++++	4.92934	+++++	6.87591	+++++	6.24593	18.261
50 Bromoethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
51 Hexane	+++++	2.46682	2.43567	3.86592	3.61363	3.63581	3.26636	19.577
52 Chloroprene	+++++	+++++	2.08646	+++++	3.48132	+++++	2.95915	25.704
53 Iodomethane	+++++	+++++	2.27666	+++++	4.12055	+++++	3.31677	28.473
54 2,3-Dimethylbutane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
55 1,1-Dichloroethane	+++++	2.10360	2.41092	3.46585	3.17790	3.17315	2.90836	18.148
56 Vinyl Acetate	+++++	+++++	0.16492	0.41424	0.40332	0.42711	0.36845	31.034 <-
57 Ethyl-tert-butyl Ether	+++++	+++++	1.77550	+++++	3.01750	+++++	2.39046	25.982

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000	250.000						
	Level 7	Level 8						
58 1-Hexene	+++++	+++++	1.01069	+++++	1.69978	+++++		
	1.68542	+++++					1.46530	26.873
59 1,3-Dichloropropane	+++++	+++++	0.35918	+++++	0.55397	+++++		
	0.51750	+++++					0.47688	21.715
60 2,2-Dichloropropane	+++++	+++++	1.26874	+++++	1.99847	+++++		
	1.92216	+++++					1.72979	23.188
61 Ethyl Acetate	+++++	+++++	0.21783	+++++	0.31814	+++++		
	0.33777	+++++					0.29125	22.090
62 Methyl Acrylate	+++++	+++++	1.65144	+++++	3.50217	+++++		
	3.66577	+++++					2.93979	38.055
63 2,4-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
64 1-Propanol	+++++	+++++	0.12700	+++++	0.30625	+++++		
	0.34871	+++++					0.26065	45.147 <-
65 Butanal	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
66 cis-1,2-Dichloroethene	+++++	1.79718	1.78128	2.54908	2.33516	2.32726		
	2.31230	+++++					2.18371	14.552
67 2-Butanone	+++++	0.64058	0.42684	0.77906	0.78663	0.78694		
	0.79131	+++++					0.70189	20.918

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
68 2-Butanol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
69 3-Methyl-1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
70 Tetrahydrofuran	+++++	2.89615	2.01569	2.81384	2.66945	2.66508		
	2.62003	+++++					2.61338	11.896
72 Chloroform	+++++	1.85697	2.01228	2.91307	2.70085	2.66696		
	2.63482	+++++					2.46416	17.224
73 1,1-Dichloropropene	+++++	+++++	0.50371	+++++	0.76357	+++++		
	0.70852	+++++					0.65860	20.792
74 Cyclohexane	+++++	1.48727	1.55950	2.36916	2.18953	2.16867		
	2.13124	+++++					1.98423	18.494
75 1,1,1-Trichloroethane	+++++	2.14462	1.90906	2.79475	2.68520	2.63285		
	2.61196	+++++					2.46307	14.281
76 Isobutanol	+++++	+++++	0.26685	+++++	0.39129	+++++		
	0.42205	+++++					0.36006	22.823
77 Carbon Tetrachloride	+++++	1.39443	1.55958	2.42097	2.25001	2.29409		
	2.28291	+++++					2.03366	21.548
78 tert-amyl-Methyl Ether	+++++	+++++	1.56158	+++++	2.40734	+++++		
	1.78316	+++++					1.91736	22.873

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000	250.000						
	Level 7	Level 8						
79 2,3-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
80 2,2,4-Trimethylpentane	+++++	6.46742	6.43483	10.79687	9.93119	10.12077		
	9.98846	+++++					8.95659	21.942
81 Benzene	+++++	0.86714	0.83488	1.27550	1.21675	1.15483		
	1.11627	+++++					1.07756	17.071
82 1-Methoxy-2-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
83 2,3,4-Trimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
85 1,2-Dichloroethane	+++++	0.40590	0.38967	0.56859	0.54489	0.53423		
	0.51864	+++++					0.49365	15.434
86 2-Pentanone	+++++	+++++	0.71310	+++++	1.48585	+++++		
	1.53779	+++++					1.24558	37.081
87 Pentanal	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
88 Ethyl Acrylate	+++++	+++++	0.58998	+++++	1.13179	+++++		
	1.15887	+++++					0.96022	33.421
89 Octane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
90 Heptane	+++++	0.08116	0.08418	0.14505	0.14238	0.13769		
	0.13168	+++++					0.12036	24.559
91 1-Butanol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
93 Trichloroethene	+++++	0.42639	0.32876	0.49891	0.47147	0.45370		
	0.44315	+++++					0.43706	13.406
94 Methyl Cyclohexane	+++++	0.48944	0.48701	0.73738	0.69656	0.66783		
	0.65602	+++++					0.62237	17.293
95 Dibromomethane	+++++	+++++	0.24775	+++++	0.35521	+++++		
	0.33362	+++++					0.31219	18.207
96 Methyl Methacrylate	+++++	+++++	0.41367	+++++	0.79182	+++++		
	0.80096	+++++					0.66882	33.045
97 1-Nitropropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
98 1,2-Dichloropropane	+++++	0.38729	0.35186	0.46911	0.46335	0.43802		
	0.43292	+++++					0.42376	10.768
99 1,4-Dioxane	+++++	+++++	0.18537	0.25698	0.27094	0.25881		
	0.25845	+++++					0.24611	13.984
100 Bromodichloromethane	+++++	0.49548	0.48012	0.69796	0.67917	0.66072		
	0.65298	+++++					0.61107	15.852

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
112 Alphamethylstyrene	+++++	+++++	0.37209	+++++	0.87896	+++++		
	0.91363	+++++					0.72156	42.013<-
113 trans-1,3-Dichloropropene	+++++	0.18296	0.29498	0.61567	0.62632	0.62490		
	0.64674	0.70569					0.52818	38.318<-
114 1,1,2-Trichloroethane	+++++	0.39610	0.39469	0.54509	0.51796	0.49373		
	0.47937	+++++					0.47116	13.327
115 D-Limonene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
116 Tetrachloroethene	+++++	0.45111	0.49434	0.64278	0.59961	0.56072		
	0.53734	+++++					0.54765	12.700
117 Bis(2-chloroethyl) ether	+++++	+++++	0.62771	+++++	0.92422	+++++		
	1.00285	+++++					0.85159	23.231
118 Butyl Acetate	+++++	+++++	0.25494	+++++	0.44184	+++++		
	0.43981	+++++					0.37886	28.327
119 2-Hexanone	+++++	+++++	0.38705	0.70746	0.73728	0.72182		
	0.73265	+++++					0.65725	23.048
120 Dibromochloromethane	+++++	0.48543	0.46005	0.78337	0.75484	0.73819		
	0.73361	+++++					0.65925	22.107
121 Undecane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
122 1,2-Dibromoethane	+++++	0.52523	0.51112	0.81252	0.78864	0.75350		
	0.75279	+++++					0.69063	19.626
123 1,1,1,2-Tetrachloroethane	+++++	+++++	0.33132	+++++	0.52257	+++++		
	0.48676	+++++					0.44688	22.752
124 1-chloro-2-Bromopropane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
126 Chlorobenzene	+++++	0.88825	0.94525	1.24714	1.18342	1.10891		
	1.08181	+++++					1.07580	12.765
127 Nonane	+++++	+++++	0.86684	+++++	1.69464	+++++		
	1.64249	+++++					1.40132	33.084
128 Ethyl Benzene	+++++	0.53437	0.38875	0.68425	0.66879	0.60711		
	0.60394	+++++					0.58120	18.645
129 Dodecane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
130 m,p-Xylene	+++++	0.54044	0.51688	0.87274	0.82250	0.77957		
	0.75100	+++++					0.71385	20.930
131 2-Heptanone	+++++	+++++	0.52167	+++++	0.79118	+++++		
	0.91641	+++++					0.74309	27.146
132 o-Xylene	+++++	0.56408	0.52558	0.79941	0.76308	0.73032		
	0.69050	+++++					0.67883	16.282

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
133 Styrene	1.01812	0.58973	0.60689	1.26959	1.21344	1.16476		
	1.14342	++++					1.00085	28.528
134 Bromoform	++++	0.48390	0.40330	0.67685	0.68425	0.64213		
	0.63460	++++					0.58750	19.734
135 Cyclohexanone	++++	++++	0.53372	++++	0.71042	++++		
	0.75222	++++					0.66546	17.429
136 Cumene	2.76185	1.36519	1.48674	2.40147	2.32384	2.19490		
	1.87373	++++					2.05825	24.639
137 Bromobenzene	++++	++++	0.43766	++++	0.64466	++++		
	0.57640	++++					0.55291	19.077
139 1,2,3-Trichloropropane	++++	++++	0.24503	++++	0.34523	++++		
	0.31982	++++					0.30336	17.170
140 2-Chlorotoluene	++++	++++	0.32740	++++	0.54839	++++		
	0.51453	++++					0.46344	25.683
141 1,1,2,2-Tetrachloroethane	++++	0.76674	0.86441	1.23496	1.15323	1.08107		
	1.04200	++++					1.02374	17.278
142 Propylbenzene	++++	1.52345	1.84115	2.86189	2.84745	2.63995		
	2.43007	++++					2.35732	23.556
143 4-Chlorotoluene	++++	++++	0.35794	++++	0.54350	++++		
	0.52520	++++					0.47555	21.503

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	RRF	% RSD
144 4-Ethyltoluene	200.000 Level 7	250.000 Level 8						
144 4-Ethyltoluene	+++++	1.26455	1.45132	2.47094	2.39413	2.28584		
	2.15067	+++++					2.00291	25.686
145 Aniline	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
146 Diisobutyl Ketone	+++++	+++++	1.47619	+++++	1.90111	+++++		
	1.88785	+++++					1.75505	13.766
147 1,3,5-Trimethylbenzene	+++++	1.25900	1.34770	2.28575	2.15752	2.06450		
	1.74793	+++++					1.81040	23.861
148 Isooctyl Alcohol	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
149 tert-Butylbenzene	+++++	+++++	1.47499	+++++	2.12146	+++++		
	2.17492	+++++					1.92379	20.251
150 Pentachloroethane	+++++	+++++	0.21671	+++++	0.39389	+++++		
	0.40303	+++++					0.33788	31.085
151 sec-Butylbenzene	+++++	+++++	1.76154	+++++	2.70134	+++++		
	2.38802	+++++					2.28363	20.954
152 1,2,4-Trimethylbenzene	+++++	1.00582	1.15157	1.83029	1.81563	1.72281		
	1.68855	+++++					1.53578	23.510
153 p-Cymene	+++++	+++++	0.33781	+++++	0.56323	+++++		
	0.58177	+++++					0.49427	27.477

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000	250.000						
	Level 7	Level 8						
154 1,2,3-Trimethylbenzene	+++++	+++++	0.48220	+++++	0.82940	+++++		
	0.81804	+++++					0.70988	27.788
155 1,3-Dichlorobenzene	+++++	0.99769	0.86656	1.24394	1.19375	1.12009		
	1.10147	+++++					1.08725	12.604
156 1,4-Dichlorobenzene	+++++	0.94834	1.10360	1.51808	1.44770	1.37048		
	1.25731	+++++					1.27425	16.993
157 alpha-Chlorotoluene	1.60406	0.82175	0.79269	1.98425	2.19183	2.23850		
	1.59858	+++++					1.60452	37.419 <-
158 Butylbenzene	+++++	+++++	0.31099	+++++	0.50442	+++++		
	0.52164	+++++					0.44568	26.243
159 1,2-Dichlorobenzene	+++++	1.01178	1.08493	1.26153	1.21775	1.17597		
	1.10932	+++++					1.14355	8.057
160 Hexachloroethane	+++++	+++++	0.45089	+++++	0.75661	+++++		
	0.77025	+++++					0.65925	27.391
161 1,2-Dibromo-3-Chloropropane	+++++	+++++	0.29642	+++++	0.50709	+++++		
	0.56221	+++++					0.45524	30.813
162 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++	+++++					+++++	+++++
163 1,2,4-Trichlorobenzene	+++++	+++++	0.77054	0.82814	0.85214	0.80829		
	0.79944	+++++					0.81171	3.778

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 12-NOV-2007 13:22
 End Cal Date : 27-NOV-2007 12:08
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Cal Date : 27-Nov-2007 15:32 cbond
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	RRF	% RSD
164 Hexachlorobutadiene	+++++ 0.53576	+++++ +++++	0.53651	0.60902	0.60706	0.56299	0.57027	6.346
165 Naphthalene	+++++ 1.69291	+++++ +++++	2.57361	3.03888	3.14450	3.06743	2.70346	22.481
166 1,2,3-Trichlorobenzene	+++++ 1.08304	+++++ +++++	0.83081	+++++	1.04576	+++++	0.98654	13.801
167 Isooctyl Acrylate	+++++ +++++	+++++ +++++	+++++	+++++	+++++	+++++	+++++	+++++
192 Cyclopentene	+++++ 3.86686	+++++ +++++	2.78953	+++++	4.17550	+++++	3.61063	20.153
\$ 84 1,2-Dichloroethane-d4	+++++ 1.57317	1.40375 1.68718	1.44058	1.44597	1.38908	1.53501	1.49639	7.195
\$ 107 Toluene-d8	+++++ 0.90672	0.84718 0.88771	0.87004	0.89425	0.89966	0.87285	0.88263	2.332
\$ 138 Bromofluorobenzene	+++++ 0.59244	0.56787 0.61468	0.55601	0.59299	0.58759	0.57170	0.58333	3.355

Calibration History

Method : /chem/msd5.i/5-27nov.b/t14qn12c.m
Start Cal Date: 12-NOV-2007 13:22
End Cal Date : 27-NOV-2007 12:08

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.20000		
12-NOV-2007 13:22	AFCEElow	/chem/msd5.i/5-12nov.b/5111207.d
Cal Level: 2 , Cal Amount: 0.50000		
13-NOV-2007 10:41	AT04Low+ENSR	/chem/msd5.i/5-12nov.b/5111232.d
Cal Level: 3 , Cal Amount: 2.00000		
27-NOV-2007 11:36	sp19b	/chem/msd5.i/5-27nov.b/5112706.d
19-NOV-2007 01:56	sp21b	/chem/msd5.i/5-19nov.b/5111902.d
12-NOV-2007 19:20	sp20a	/chem/msd5.i/5-12nov.b/5111216.d
12-NOV-2007 14:17	AT04MDL+ENSR	/chem/msd5.i/5-12nov.b/5111209.d
Cal Level: 4 , Cal Amount: 25.00000		
12-NOV-2007 14:45	AT04MDL+ENSR	/chem/msd5.i/5-12nov.b/5111210.d
Cal Level: 5 , Cal Amount: 50.00000		
27-NOV-2007 09:21	sp19b	/chem/msd5.i/5-27nov.b/5112702.d
19-NOV-2007 02:24	sp21b	/chem/msd5.i/5-19nov.b/5111903.d
12-NOV-2007 19:48	sp20a	/chem/msd5.i/5-12nov.b/5111217.d
12-NOV-2007 15:12	AT04MDL+ENSR	/chem/msd5.i/5-12nov.b/5111211.d
Cal Level: 6 , Cal Amount: 100.00000		
12-NOV-2007 15:41	AT04MDL+ENSR	/chem/msd5.i/5-12nov.b/5111212.d
Cal Level: 7 , Cal Amount: 200.00000		
27-NOV-2007 12:08	sp19b	/chem/msd5.i/5-27nov.b/5112707.d

```
|19-NOV-2007 02:57 |sp21b |/chem/msd5.i/5-19nov.b/5111904.d |
|12-NOV-2007 20:20 |sp20a |/chem/msd5.i/5-12nov.b/5111218.d |
|12-NOV-2007 16:13 |AT04MDL+ENSR |/chem/msd5.i/5-12nov.b/5111213.d |
+-----+-----+-----+-----+
```

```
+-----+-----+-----+-----+
| Cal Level: 8 , Cal Amount: 250.00000 |
+=====+
|13-NOV-2007 12:52 |Level8 |/chem/msd5.i/5-13nov.b/5111303.d |
+-----+-----+-----+-----+
```

Continuing Calibration
Ccal Level Mode: GLOBAL LEVEL 5

```
+-----+-----+-----+-----+
| Ccal Level: 5 , Ccal Amount: 50.000 |
+=====+
|27-NOV-2007 09:49 |AT04ENSR |/chem/msd5.i/5-27nov.b/5112703.d |
+-----+-----+-----+-----+
| Ccal Level: 5 , Ccal Amount: 50.000 |
+=====+
|27-NOV-2007 09:21 |sp19b |/chem/msd5.i/5-27nov.b/5112702.d |
+-----+-----+-----+-----+
| Ccal Level: 5 , Ccal Amount: 50.000 |
+=====+
|27-NOV-2007 09:21 |sp19bCCV |/chem/msd5.i/5-27nov.b/5112702a.d |
+-----+-----+-----+-----+
```

Initial Calibration Narrative

A seven point initial calibration was analyzed on MSD-5 on 11/12/2007 and 11/13/2007. As noted on the accompanying analytical run logs, the following point calibration level 2 was re-analyzed due to:

- a. unacceptable peak resolution and/or integration of 2-Butanone

The following compounds used either 0.2 or 0.25 ppbv as the lowest calibration concentration:

Cumene, alpha-Chlorotoluene, trans-1,3-Dichloropropene, and Styrene.

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	26.19
75	30.0 - 60.0% of mass 95	42.68
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.38
173	Less than 2.0% of mass 174	(0.85) ¹
174	Greater than 50.0% of mass 95	70.79
175	5.0 - 9.0% of mass 174	(7.30) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(96.59) ¹
177	5.0 - 9.0% of mass 176	(6.30) ²

BFB Injection Date: 11/12/07
 BFB Injection Time: 1201
 BFB File ID: 5111205
 Tekmar Purge Flow: 12.5 mL/min
 Vacuum: 5.58 x 10⁻⁵ Torr
 IS/S Std #: 1487-401 Exp. Date: 01/24/08
 BCM 355243
 1,4-DFB 1306315
 CB-d5 1073463
 Verified CCV IS vs ICAL mid-point (-40%^D) 55
INITIALS

Verify 176/174 m/z Ratio: $\frac{681408}{705472} \times 100 = 96.599\%$

NOAH Cart #: 0 File #: F111209d
11-13-02 CF

Calculation Check:

$$\frac{\text{ppbv of compound}}{\text{Area}_{\text{sample}}} = \frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} \times \text{RRF}$$

$$= \frac{(493461)}{(355243)} \times (25) \times (1.49639) = 23.207$$

Reported Result 23.207

File ID: 5111205
 Compound: 1,4-DFB-d4
 Initials: CF

#	File #	Sample / Client Name	Can #	Pressure	Am't Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
1	✓ 5111205	BFB Tune Check	1476-65	50mg Humid	2ul	1.00	11/12/07	1201	CB	Single scan 102 Area +1
2	✓ 06	System Blank	13673	200 ppbv - 0.2 ppbv	200mL			1254	CB	
3	✓ 07	ICAL Level 1	1576-89	200 ppbv - 0.2 ppbv	0.2mL			1322	CB	THERMURA
4	✓ 08			200 ppbv - 0.5 ppbv	0.5mL			1349	CB	
5	✓ 09			200 ppbv - 2 ppbv	2mL			1477	CB	
6	✓ 10			200 ppbv - 25 ppbv	25mL			1445	CB	CCV
7	✓ 11			200 ppbv - 50 ppbv	50mL			1512	CB	
8	✓ 12			200 ppbv - 100 ppbv	100mL			1541	CB	
9	✓ 13			200 ppbv	200mL			1613	CB	
10	✓ 14	System Blank	125142	Humid	200mL			1758	CB	

11-13-02 CF

11	X	511215	ICAL Level 3	1510-88	20 ppbv	2.0 mL	1.00	1/12/07	12881831	145	Not Needed
12	✓	511216	ICAL Level 3	1487424	20 ppbv	2.0 mL	1.00	1/12/07	1920	145	SP200
13	✓	17	↓	↓	50 ppbv	5.0 mL	1.00	1/12/07	1948	145	CLV200
14	✓	18	↓	↓	200 ppbv	200 μL	1.00	1/12/07	0020	145	↓
15	X	19	ICAL Lcs	1570-113	20 ppbv	2.0 μL	1.00	1/12/07	2144	145	Not Used
16	X	20	↓	↓	↓	↓	↓	1/12/07	2333	145	↓
17	X	21	System Blank	12941	Humid	200 μL	1.00	1/12/07	0028	145	↓
18	X	22	Lab Blank	↓	↓	↓	↓	1/12/07	0113	145	↓
19	X	23	OP11016A-DUA	SC48	6.5 (11/15/07)	↓	2.58	1/12/07	0228	145	↓
20	X	24	-07A	2122	0.2 (11/15/07)	↓	1.99	1/12/07	0300	145	↓
21	X	25	-08A	34594	5.5 (11/15/07)	↓	4.99	1/12/07	0333	145	↓
22	X	26	-09A	1742	5.0	↓	2.42	1/12/07	0405	145	↓
23	X	27	-10A	1737	5.5	↓	2.47	1/12/07	0437	145	↓
24	X	28	-11A	30829	8.5	↓	2.82	1/12/07	0509	145	↓
25	X	29	-12A	34628	5.0	100 μL	4.84	1/12/07	0538	145	↓
26	X	30	↓	SC59	6.5	200 μL	2.58	1/12/07	0610	145	↓
27	✓	31	Lab Blank	12941	Humid	200 μL	1.00	1/12/07	1014	145	CF
28	✓	32	ICAL Level 2 (Accepted)	157089	0.5 ppbv	0.5 mL	1.00	1/12/07	1041	145	CF
29											
30											
31											
32											

Comments:

Actual 25.0 Nominal 22.6 11-13-07 CF

Flow controller Serial # AA920318

Dist Flow Meter Serial # 200-74116 Exp 8-31-08

Signature *CF*

Date 11-13-07

Date

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	26.36
75	30.0 - 60.0% of mass 95	47.51
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.69
173	Less than 2.0% of mass 174	(0.76) ¹
174	Greater than 50.0% of mass 95	64.09
175	5.0 - 9.0% of mass 174	(2.32) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(97.32) ¹
177	5.0 - 9.0% of mass 176	(6.11) ²

Verify 176/174 m/z Ratio: $\frac{619498}{1636565} \times 100 = 97.32\%$

BFB Injection Date: 11/19/07
 BFB Injection Time: 0033
 BFB File ID: 5111901
 Tekmar Purge Flow: 11/19/07
 Vacuum:
 IS/S Std #: 1487-461 Exp. Date: 1/24/08
 BCM 345866
 1,4-DFB 1304928
 CB-d5 994233
 Verified CCV IS vs ICAL mid-point (-40%^D)

NOAH Cart #: 14/11 File #: 5111901/5111911

Calculation Check: $\frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} = \text{Conc.}_{\text{sample}}$


$\frac{(1130502)}{(1304928)} \times (25.0) = 21.538$

File ID: 5111906
 Compound: Tol-d8
 Initials: R

%	File #	Sample / Client Name	Can #	Pressure	Am't Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	5111901	BFB Tune Check	1486-65	50mg	2µL	1.00	11/19/07	0033	CB	
✓	02	ICAL Sp level 3	1487-405	200-50µhr	2.0mL			0156	CB	T140126
✓	03	ICAL Sp level 5		200-50µhr	5.0mL			0224	CB	Sp216 CCV50
✓	04	ICAL Sp level 7		200µhr	300mL			0257	CB	
✓	05	System Blank	34190	Humid	200mL			0411	CB	
✓	06	CCV-1	1576-89	200-50µhr	5.0mL			0502	CB	
✓	07	ACS-1	1443-3024	100-50µhr	100mL			0530	CB	
✓	08	CCV-50	1487-404	200-50µhr	5.0mL			0605	CB	
X	09	Lab Blank	34190	Humid	200mL			0929	CB	Cart 7 8 Log 8
✓	10	Lab Blank						1051	CB	Cart 14 Log 4

11	✓	S111911	ICRL Level 1 3	1443-361	200µg/ml 7 µg/ml	2ml	1.00	11/19/07	1224	CB	T1401126
12	✓	12	5	↓	200µg/ml 50µg/ml	50ml			1252	CB	SPI90000 CNGP
13	✓	13	7	↓	200µg/ml	200ml			1324	CB	
14	✓	14	CNGP (200µg/ml)	1487-404	50µg/ml	50ml			1443	CB	SPI20000
15	✓	15	Lab Blank	34190	Humid	200ml			1555	CB	Cart Cart 5 Log 1
16	X	16	Lab Blank						1703	SC	Cart Cart 8 Log 8
17	✓	S111917	0211102A-01A	35746	6.0µg-5µg	200µl	1.68		1811	SC	
18	✓	18	02A	↓	↓		1.68		1843	SC	
19	✓	19	02A	4339	4.5µg		1.58		1915	SC	
20	✓	20	02A	15286	5.5µg		1.04		1942	SC	
21	✓	21	0-1A	1588	6.0µg		1.68		2019	SC	
22	✓	22	05A	4059	5.0µg		1.61		2051	SC	
23	X	23	0211102A-01A	94902	11.5µg-15µg	150µl	4.37		2122	SC	PR @ 200µl
24	✓	24	02A	9368	2.5µg	200µl	2.08		2154	SC	
25	✓	25	03A	3246	17.0µg	3.0µl	3.1		2221	SC	
26	✓	26	01A	94902	11.5µg-15µg	8.00ml	3.28		2312	SC	
27	✓	27	0711123A-01A	25381	0.2µg-0.5µg	20ml	13.2	11/20/07	0000	SC	
28	X	28	-02A	70-15W	0.5µg-0.5µg	200ml	1.36	↓	0033	SC	out of clock
29											
30											
31											
32											

Comments:

Signature 

Date 11/19/07

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	29.14
75	30.0 - 60.0% of mass 95	48.74
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.55
173	Less than 2.0% of mass 174	(0.65) ¹
174	Greater than 50.0% of mass 95	69.70
175	5.0 - 9.0% of mass 174	(7.32) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(98.44) ¹
177	5.0 - 9.0% of mass 176	(5.92) ²

¹ - value in parenthesis is % mass 174 ² - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio: $\frac{412821}{419349} \times 100 = 98.44\%$

BFB Injection Date: 11/27/07
 BFB Injection Time: 0856
 BFB File ID: 5112701
 Tekmar Purge Flow: 12.8 mL/min
 Vacuum: 6.24 x 10⁻⁵ Torr
 IS/S Std #: 1576-131 Exp. Date: 2-26-07
 BCM: 295766
 1,4-DFB: 1044114
 CB-d5: 825609
 Verified CCV IS vs ICAL mid-point (-40% D) CB

NOAH Cart #: 11/ File #: 5112602/

File ID: 5112703
 Compound: toluene-d8
 Initials: CB

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{Sample}}}{\text{Area}_{\text{std}}} \times \text{Conc}_{\text{std}} \times \text{RRF}$

= $\frac{900442}{1044114} \times (25.0) \times (0.88263)$

Reported Result 24.427

Sl. #	File #	Sample / Client Name	Can #	Pressure	Am't Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
1	5112701	BFB Tune Check	1476-65	50ps	2uL	1.00	11/27/07	0856	CB	
2	02	ICAL Level 2 (200 ppbv)	1443-574	50ppbv	50uL			0921	CB	4/14 g/n/2c 30 ppb CCV
3	03	CCV-1 (100 ppbv)	1576-90A		100uL			0949	CB	
4	04	LS-1 (200 ppbv)	1576-111		50uL			1017	CB	
5	05	System Blank	12941	Humid	200uL			1108	CB	
6	06	ICAL Level 3	1443-377	2ppbv	2uL			1136	CB	4/14 g/n/2c 30 ppb
7	07	ICAL Level 7			200uL			1208	CB	
8	08	Lab Blank	13673	Humid	200uL			310	CB	
9	09	0711308-014	94485	60%b-15ps	100uL	5.06		409	CB	ICAL Cart #14 Log 2
10	10	0711207-01A	1575	7ppb-9.6ps	200uL	1.00			CB	IC-1/2 PCA @ 400 KPa @ 35 mL

Air Toxics Ltd.
 Modified EPA Methods TO-14A/TO-15
 Internal Standard and Associated Target Compounds and Surrogates

Bromochloromethane
Target Compounds:
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
3-Chloropropene
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
2,2,4-Trimethylpentane
Surrogates:
1,2-Dichloroethane-d4

1,4-Difluorobenzene
Target Compounds:
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
Surrogates:
Toluene-d8

Chlorobenzene-d5
Target Compounds:
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
Surrogates:
Bromofluorobenzene

Report Date: 13-Nov-2007 14:27

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-13nov.b/5111306.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 13-NOV-2007 14:19
 Operator : ct Inst ID: msd5.i
 Smp Info : 50mL #1576-113
 Misc Info : 50ppbv (200ppbv)
 Comment :
 Method : /chem/msd5.i/5-13nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 14:10 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 20:20 Cal File: 5111218.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				(PPBV)	(PPBV)			
==	=====	=====	====	=====	=====	=====	=====	=====

* 71	Bromochloromethane					CAS #: 74-97-5		
8.059	8.059	(1.000)	130	329578	25.0000	80.00- 120.00	100.00	
8.059	8.059	(1.000)	128	255291		44.59- 104.59	77.46	
8.032	8.059	(1.000)	49	712129		179.89- 239.89	216.07	

* 92	1,4-Difluorobenzene					CAS #: 540-36-3		
9.912	9.912	(1.000)	114	1265824	25.0000	80.00- 120.00	100.00	
9.912	9.912	(1.000)	88	211923		0.00- 46.50	16.74	

* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.999	14.999	(1.000)	117	985864	25.0000	80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	591551		0.00- 30.00	60.00	

\$ 84	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.110	9.110	(1.130)	65	494884	25.0865	25.086 80.00- 120.00	100.00	
9.110	9.110	(1.130)	67	275885		0.00- 30.00	55.75	

\$ 107	Toluene-d8					CAS #: 2037-26-5		
12.704	12.704	(1.282)	98	1130598	25.2986	25.299 80.00- 120.00	100.00	
12.677	12.704	(1.279)	70	113531		0.00- 30.00	10.04	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 107 Toluene-d8 (continued)

12.704	12.704	(1.282)	100	729210			0.00- 30.00	64.50
--------	--------	---------	-----	--------	--	--	-------------	-------

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575	16.575	(1.105)	174	573073	24.9127	24.913	80.00- 120.00	100.00
16.575	16.575	(1.105)	95	940083			133.48- 193.48	164.04
16.575	16.575	(1.105)	176	557005			70.11- 130.11	97.20

6 Propylene

CAS #: 115-07-1

2.280	2.280	(0.283)	41	1390096	60.4280	60.428	80.00- 120.00	100.00
2.280	2.280	(0.283)	42	935654			0.00- 30.00	67.31
2.280	2.280	(0.283)	39	946796			0.00- 30.00	68.11

8 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.336	2.336	(0.290)	85	2194755	56.3185	56.318	80.00- 120.00	100.00
2.336	2.336	(0.290)	87	706954			0.00- 30.00	32.21

9 Freon 114

CAS #: 76-14-2

2.446	2.446	(0.304)	135	2054336	57.7626	57.762	80.00- 120.00	100.00
2.446	2.446	(0.304)	137	652867			1.61- 61.61	31.78

10 Chloromethane

CAS #: 74-87-3

2.585	2.585	(0.321)	50	1613808	55.1495	55.149	80.00- 120.00	100.00
2.585	2.585	(0.321)	52	516287			0.00- 30.00	31.99

13 Vinyl Chloride

CAS #: 75-01-4

2.778	2.778	(0.345)	62	1597055	56.7023	56.702	80.00- 120.00	100.00
2.778	2.778	(0.345)	64	502731			0.00- 30.00	31.48

12 1,3-Butadiene

CAS #: 106-99-0

2.750	2.750	(0.341)	54	1419547	59.0142	59.014	80.00- 120.00	100.00
2.750	2.750	(0.341)	39	1537627			0.00- 30.00	108.32

15 Bromomethane

CAS #: 74-83-9

3.276	3.276	(0.406)	94	1074167	59.0738	59.074	80.00- 120.00	100.00
3.276	3.276	(0.406)	96	994884			64.51- 124.51	92.62

19 Chloroethane

CAS #: 75-00-3

3.386	3.386	(0.420)	64	789236	55.0880	55.088	80.00- 120.00	100.00
3.386	3.386	(0.420)	49	223113			0.00- 30.00	28.27
3.386	3.386	(0.420)	66	232780			0.00- 30.00	29.49

20 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.718	3.718	(0.461)	101	2404031	56.5807	56.581	80.00- 120.00	100.00
3.718	3.718	(0.461)	103	1562591			35.79- 95.79	65.00

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

26 Ethanol CAS #: 64-17-5
 4.078 4.078 (0.506) 45 617839 66.9348 66.935 80.00- 120.00 100.00
 4.078 4.078 (0.506) 43 114972 0.00- 30.00 18.61
 4.078 4.078 (0.506) 46 261005 0.00- 30.00 42.24

30 Freon 113 CAS #: 76-13-1
 4.520 4.520 (0.561) 151 1654470 62.6241 62.624 80.00- 120.00 100.00
 4.520 4.520 (0.561) 153 1049272 32.44- 92.44 63.42
 4.520 4.520 (0.561) 101 2296302 106.77- 166.77 138.79

31 1,1-Dichloroethene CAS #: 75-35-4
 4.575 4.548 (0.568) 61 2222648 63.5687 63.569 80.00- 120.00 100.00
 4.575 4.548 (0.568) 96 1252491 25.42- 85.42 56.35
 4.575 4.548 (0.568) 98 803129 5.54- 65.54 36.13

32 Acetone CAS #: 67-64-1
 4.714 4.714 (0.585) 58 757570 57.9269 57.927 80.00- 120.00 100.00
 4.714 4.714 (0.585) 43 2299307 0.00- 30.00 303.51

36 2-Propanol CAS #: 67-63-0
 4.907 4.907 (0.609) 45 2726787 58.5876 58.588 80.00- 120.00 100.00
 4.907 4.907 (0.609) 43 578881 0.00- 30.00 21.23
 4.907 4.907 (0.609) 59 104526 0.00- 30.00 3.83

35 Carbon Disulfide CAS #: 75-15-0
 4.907 4.907 (0.609) 76 3464610 58.5126 58.513 80.00- 120.00 100.00

38 3-Chloropropene CAS #: 107-05-1
 5.184 5.184 (0.643) 76 568549 57.6695 57.670 80.00- 120.00 100.00
 5.184 5.184 (0.643) 41 2168064 0.00- 30.00 381.33

43 Methylene Chloride CAS #: 75-09-2
 5.432 5.432 (0.674) 49 1841524 61.5949 61.595 80.00- 120.00 100.00
 5.432 5.432 (0.674) 84 1049480 26.07- 86.07 56.99
 5.432 5.432 (0.674) 51 562086 0.00- 30.00 30.52

46 MTBE CAS #: 1634-04-4
 5.764 5.764 (0.715) 73 1236681 54.9495 54.949 80.00- 120.00 100.00
 5.764 5.764 (0.715) 57 394002 2.42- 62.42 31.86
 5.764 5.764 (0.715) 41 414743 0.00- 30.00 33.54

47 trans-1,2-Dichloroethene CAS #: 156-60-5
 5.820 5.820 (0.722) 96 1255521 59.2914 59.291 80.00- 120.00 100.00
 5.820 5.820 (0.722) 61 2028708 128.85- 188.85 161.58
 5.820 5.820 (0.722) 98 786800 0.00- 30.00 62.67

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

51 Hexane CAS #: 110-54-3
 6.151 6.151 (0.763) 57 2564369 59.5522 59.552 80.00- 120.00 100.00
 6.151 6.151 (0.763) 43 1789596 0.00- 30.00 69.79
 6.151 6.151 (0.763) 86 368027 0.00- 30.00 14.35

55 1,1-Dichloroethane CAS #: 75-34-3
 6.594 6.594 (0.818) 63 2312589 60.3159 60.316 80.00- 120.00 100.00
 6.594 6.594 (0.818) 65 689212 0.00- 59.87 29.80

67 2-Butanone CAS #: 78-93-3
 7.672 7.672 (0.952) 72 544183 58.8106 58.810 80.00- 120.00 100.00
 7.644 7.672 (0.949) 43 3022181 561.22- 621.22 555.36
 7.644 7.672 (0.949) 57 217616 0.00- 30.00 39.99

66 cis-1,2-Dichloroethene CAS #: 156-59-2
 7.617 7.617 (0.945) 61 1682856 58.4566 58.456 80.00- 120.00 100.00
 7.617 7.617 (0.945) 96 1133257 38.38- 98.38 67.34
 7.617 7.617 (0.945) 98 720000 14.09- 74.09 42.78

70 Tetrahydrofuran CAS #: 109-99-9
 8.032 8.031 (0.997) 42 1849537 53.6838 53.684 80.00- 120.00 100.00
 8.032 8.031 (0.997) 71 479708 0.00- 55.17 25.94
 8.032 8.031 (0.997) 72 529224 0.00- 30.00 28.61

72 Chloroform CAS #: 67-66-3
 8.197 8.197 (1.017) 83 1933667 59.5243 59.524 80.00- 120.00 100.00
 8.197 8.197 (1.017) 85 1237413 34.62- 94.62 63.99

75 1,1,1-Trichloroethane CAS #: 71-55-6
 8.419 8.419 (1.045) 97 1910343 58.8323 58.832 80.00- 120.00 100.00
 8.419 8.419 (1.045) 99 1227419 33.24- 93.24 64.25

74 Cyclohexane CAS #: 110-82-7
 8.419 8.419 (1.045) 84 1515378 57.9311 57.931 80.00- 120.00 100.00
 8.391 8.419 (1.041) 56 2394553 126.47- 186.47 158.02
 8.391 8.419 (1.041) 41 1346348 58.16- 118.16 88.85

56 Vinyl Acetate CAS #: 108-05-4
 6.649 6.649 (0.825) 86 284978 58.6702 58.670 80.00- 120.00 100.00
 6.649 6.649 (0.825) 43 3788471 0.00- 30.00 1329.39
 6.649 6.649 (0.825) 42 277519 0.00- 30.00 97.38

77 Carbon Tetrachloride CAS #: 56-23-5
 8.667 8.667 (1.075) 119 1606399 59.9179 59.918 80.00- 120.00 100.00
 8.667 8.667 (1.075) 117 1673357 74.63- 134.63 104.17

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.110	9.110	(1.130)	57	6983920	59.1478	59.148	80.00-	120.00	100.00	
9.110	9.110	(1.130)	56	2282176			0.00-	30.00	32.68	
9.110	9.110	(1.130)	41	1794142			0.00-	30.00	25.69	

81	Benzene					CAS #:	71-43-2			
9.082	9.082	(0.916)	78	3120968	57.2023	57.202	80.00-	120.00	100.00	
9.082	9.082	(0.916)	77	720584			0.00-	30.00	23.09	

85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	1483218	59.3403	59.340	80.00-	120.00	100.00	
9.276	9.276	(0.936)	64	462703			0.00-	30.00	31.20	

90	Heptane					CAS #:	142-82-5			
9.497	9.469	(0.958)	100	360524	59.1602	59.160	80.00-	120.00	100.00	
9.469	9.469	(0.955)	43	2886916			0.00-	30.00	800.76	
9.469	9.469	(0.955)	71	1119378			0.00-	30.00	310.49	

93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	1219788	55.1199	55.120	80.00-	120.00	100.00	
10.326	10.326	(1.042)	130	1163570			63.34-	123.34	95.39	
10.326	10.326	(1.042)	97	789093			34.39-	94.39	64.69	

98	1,2-Dichloropropane					CAS #:	78-87-5			
10.824	10.824	(1.092)	63	1198025	55.8359	55.836	80.00-	120.00	100.00	
10.824	10.824	(1.092)	62	834206			40.55-	100.55	69.63	
10.824	10.824	(1.092)	41	818464			41.13-	101.13	68.32	

99	1,4-Dioxane					CAS #:	123-91-1			
11.073	11.073	(1.117)	88	665226	53.3833	53.383	80.00-	120.00	100.00	
11.045	11.073	(1.114)	58	640313			62.89-	122.89	96.25	
11.045	11.073	(1.114)	57	203792			0.00-	30.00	30.64	

100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	1786670	57.7457	57.746	80.00-	120.00	100.00	
11.405	11.405	(1.151)	85	1146088			33.46-	93.46	64.15	

103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	1277421	58.2532	58.253	80.00-	120.00	100.00	
12.317	12.317	(1.243)	77	409273			2.37-	62.37	32.04	
12.290	12.317	(1.240)	39	946560			44.56-	104.56	74.10	

106	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.594	12.594	(1.271)	58	1081560	60.5091	60.509	80.00-	120.00	100.00	
12.594	12.594	(1.271)	43	3066032			0.00-	30.00	283.48	
12.594	12.594	(1.271)	85	360057			0.00-	30.00	33.29	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
108 Toluene						CAS #:	108-88-3			
12.815	12.815	(1.293)	91	3221255	57.2310	57.231	80.00- 120.00	100.00		
12.815	12.815	(1.293)	92	1904763			30.01- 90.01	59.13		

113 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.368	13.368	(0.891)	75	1274370	61.1838	61.184	80.00- 120.00	100.00		
13.368	13.368	(0.891)	77	409356			1.79- 61.79	32.12		
13.340	13.368	(0.889)	39	886762			40.58- 100.58	69.58		

114 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.644	13.644	(0.910)	97	1067431	57.4509	57.451	80.00- 120.00	100.00		
13.644	13.644	(0.910)	99	656158			32.34- 92.34	61.47		
13.644	13.644	(0.910)	83	866152			52.84- 112.84	81.14		

116 Tetrachloroethene						CAS #:	127-18-4			
13.700	13.700	(0.913)	166	1235329	57.2010	57.201	80.00- 120.00	100.00		
13.672	13.700	(0.912)	129	970748			50.58- 110.58	78.58		
13.672	13.700	(0.912)	131	954865			48.33- 108.33	77.30		

119 2-Hexanone						CAS #:	591-78-6			
14.004	14.004	(0.934)	58	1433868	55.3223	55.322	80.00- 120.00	100.00		
14.004	14.004	(0.934)	43	2914899			176.65- 236.65	203.29		
14.031	14.004	(0.935)	100	208571			0.00- 30.00	14.55		

120 Dibromochloromethane						CAS #:	124-48-1			
14.197	14.197	(0.947)	129	1549883	59.6173	59.617	80.00- 120.00	100.00		
14.197	14.197	(0.947)	127	1203853			0.00- 30.00	77.67		

122 1,2-Dibromoethane						CAS #:	106-93-4			
14.363	14.363	(0.958)	107	1517022	55.7017	55.702	80.00- 120.00	100.00		
14.363	14.363	(0.958)	109	1435652			64.70- 124.70	94.64		

126 Chlorobenzene						CAS #:	108-90-7			
15.027	15.027	(1.002)	112	2351199	55.4220	55.422	80.00- 120.00	100.00		
15.027	15.027	(1.002)	114	749667			1.03- 61.03	31.88		
15.027	15.027	(1.002)	77	1452071			31.90- 91.90	61.76		

128 Ethyl Benzene						CAS #:	100-41-4			
15.165	15.165	(1.011)	106	1300388	56.7372	56.737	80.00- 120.00	100.00		
15.165	15.165	(1.011)	91	4332438			0.00- 30.00	333.17		

130 m,p-Xylene						CAS #:	108-38-3			
15.331	15.331	(1.022)	106	1634742	58.0715	58.071	80.00- 120.00	100.00		
15.331	15.331	(1.022)	91	3490965			0.00- 30.00	213.55		

132 o-Xylene						CAS #:	95-47-6			
15.856	15.856	(1.057)	106	1551490	57.9579	57.958	80.00- 120.00	100.00		

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	3470165			198.40- 258.40	223.67	

133 Styrene CAS #: 100-42-5									
15.912	15.912	(1.061)	104	2405394	60.9453	60.945	80.00- 120.00	100.00	
15.912	15.912	(1.061)	78	1281079			22.91- 82.91	53.26	

134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1372663	59.2484	59.248	80.00- 120.00	100.00	
16.160	16.160	(1.077)	171	717398			21.91- 81.91	52.26	

141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	2257364	55.9161	55.916	80.00- 120.00	100.00	
16.796	16.796	(1.120)	85	1428065			34.08- 94.08	63.26	

144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	4826213	61.1039	61.104	80.00- 120.00	100.00	
16.962	16.962	(1.131)	120	1403150			0.00- 59.53	29.07	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	4304136	60.2885	60.288	80.00- 120.00	100.00	
17.045	17.045	(1.136)	120	2019971			0.00- 30.00	46.93	

152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	3520245	58.1256	58.126	80.00- 120.00	100.00	
17.460	17.460	(1.164)	120	1622961			16.07- 76.07	46.10	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	2295165	53.5312	53.531	80.00- 120.00	100.00	
17.764	17.764	(1.184)	148	1480562			0.00- 30.00	64.51	
17.764	17.764	(1.184)	111	941672			0.00- 30.00	41.03	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	2801549	55.7527	55.753	80.00- 120.00	100.00	
17.847	17.847	(1.190)	148	1748952			0.00- 30.00	62.43	
17.847	17.847	(1.190)	111	1187423			0.00- 30.00	42.38	

157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	4403553	69.5954	69.595	80.00- 120.00	100.00(R)	
17.985	17.985	(1.199)	126	864941			0.00- 30.00	19.64	

159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.207	18.206	(1.214)	146	2361508	52.3671	52.367	80.00- 120.00	100.00	
18.207	18.206	(1.214)	148	1497823			34.60- 94.60	63.43	
18.207	18.206	(1.214)	111	963711			10.93- 70.93	40.81	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

163	1,2,4-Trichlorobenzene					CAS #:	120-82-1		
19.506	19.506	(1.300)	180	1572894	49.1385	49.138	80.00-	120.00	100.00
19.506	19.506	(1.300)	182	1493992			63.79-	123.79	94.98

164	Hexachlorobutadiene					CAS #:	87-68-3		
19.589	19.589	(1.306)	225	1120526	49.8270	49.827	80.00-	120.00	100.00
19.589	19.589	(1.306)	223	722204			29.99-	89.99	64.45

142	Propylbenzene					CAS #:	103-65-1		
16.824	16.824	(1.122)	91	5736153	61.7056	61.706	80.00-	120.00	100.00
16.824	16.824	(1.122)	120	1198962			0.00-	30.00	20.90
16.824	16.824	(1.122)	105	195355			0.00-	30.00	3.41

136	Cumene					CAS #:	98-82-8		
16.326	16.326	(1.088)	105	4762001	58.6699	58.670	80.00-	120.00	100.00
16.326	16.326	(1.088)	120	1255353			0.00-	30.00	26.36
16.326	16.326	(1.088)	51	683771			0.00-	30.00	14.36

165	Naphthalene					CAS #:	91-20-3		
19.672	19.672	(1.312)	128	5933474	55.6559	55.656	80.00-	120.00	100.00
19.672	19.672	(1.312)	127	733755			0.00-	30.00	12.37

17	Isopentane					CAS #:	78-78-4		
3.414	3.414	(0.424)	43	2280331	55.8901	55.890	80.00-	120.00	100.00
3.414	3.414	(0.424)	57	1478618			0.00-	30.00	64.84
3.414	3.414	(0.424)	72	138916			0.00-	30.00	6.09

11	Butane					CAS #:	106-97-8		
2.668	2.667	(0.331)	58	395221	56.8161	56.816	80.00-	120.00	100.00
2.668	2.667	(0.331)	43	2997680			0.00-	30.00	758.48

94	Methyl Cyclohexane					CAS #:	108-87-2		
10.548	10.548	(1.064)	83	1837040	58.2953	58.295	80.00-	120.00	100.00
10.548	10.548	(1.064)	98	917043			0.00-	30.00	49.92
10.548	10.548	(1.064)	55	2039352			0.00-	30.00	111.01

QC Flag Legend

R - Spike/Surrogate failed recovery limits.

Report Date: 13-Nov-2007 14:27

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 13-NOV-2007

Lab File ID: 5111306.d

Calibration Time: 13:51

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /chem/msd5.i/5-13nov.b/t14qn12a.m

Misc Info: 50ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	332179	199307	465051	329578	-0.78
92 1,4-Difluorobenze	1233793	740276	1727310	1265824	2.60
125 Chlorobenzene-d5	987199	592319	1382079	985864	-0.14

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT


Client Name: Client SDG: 5-13nov
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: ct
 Data Type: MS DATA SampleType: LCS
 SpikeList File: 2926Spectra.spk Quant Type: ISTD
 Sublist File: AT04ENSR.sub
 Method File: /chem/msd5.i/5-13nov.b/t14qn12a.m
 Misc Info: 50ppbv (200ppbv)

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
8 Dichlorodifluorome	50.000	56.318	112.64	70-130
9 Freon 114	50.000	57.762	115.53	70-130
10 Chloromethane	50.000	55.149	110.30	70-130
13 Vinyl Chloride	50.000	56.702	113.40	70-130
12 1,3-Butadiene	50.000	59.014	118.03	60-140
15 Bromomethane	50.000	59.074	118.15	70-130
19 Chloroethane	50.000	55.088	110.18	70-130
20 Trichlorofluoromet	50.000	56.581	113.16	70-130
26 Ethanol	50.000	66.935	133.87	60-140
30 Freon 113	50.000	62.624	125.25	70-130
31 1,1-Dichloroethene	50.000	63.569	127.14	70-130
35 Carbon Disulfide	50.000	58.513	117.03	60-140
32 Acetone	50.000	57.927	115.85	60-140
36 2-Propanol	50.000	58.588	117.18	60-140
38 3-Chloropropene	50.000	57.670	115.34	60-140
43 Methylene Chloride	50.000	61.595	123.19	70-130
46 MTBE	50.000	54.949	109.90	60-140
47 trans-1,2-Dichloro	50.000	59.291	118.58	60-140
51 Hexane	50.000	59.552	119.10	60-140
55 1,1-Dichloroethane	50.000	60.316	120.63	70-130
66 cis-1,2-Dichloroet	50.000	58.456	116.91	70-130
67 2-Butanone	50.000	58.810	117.62	60-140
70 Tetrahydrofuran	50.000	53.684	107.37	60-140
72 Chloroform	50.000	59.524	119.05	70-130
74 Cyclohexane	50.000	57.931	115.86	60-140
75 1,1,1-Trichloroeth	50.000	58.832	117.66	70-130
56 Vinyl Acetate	50.000	58.670	117.34	60-140
77 Carbon Tetrachlori	50.000	59.918	119.84	70-130
80 2,2,4-Trimethylpen	50.000	59.148	118.30	60-140
81 Benzene	50.000	57.202	114.40	70-130
85 1,2-Dichloroethane	50.000	59.340	118.68	70-130
90 Heptane	50.000	59.160	118.32	60-140
93 Trichloroethene	50.000	55.120	110.24	70-130

Report Date: 13-Nov-2007 14:27

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
98 1,2-Dichloropropan	50.000	55.836	111.67	70-130
99 1,4-Dioxane	50.000	53.383	106.77	60-140
100 Bromodichlorometha	50.000	57.746	115.49	60-140
103 cis-1,3-Dichloropr	50.000	58.253	116.51	70-130
106 4-Methyl-2-pentano	50.000	60.509	121.02	60-140
108 Toluene	50.000	57.231	114.46	70-130
113 trans-1,3-Dichloro	50.000	61.184	122.37	70-130
114 1,1,2-Trichloroeth	50.000	57.451	114.90	70-130
116 Tetrachloroethene	50.000	57.201	114.40	70-130
119 2-Hexanone	50.000	55.322	110.64	60-140
120 Dibromochlorometha	50.000	59.617	119.23	60-140
122 1,2-Dibromoethane	50.000	55.702	111.40	70-130
126 Chlorobenzene	50.000	55.422	110.84	70-130
128 Ethyl Benzene	50.000	56.737	113.47	70-130
130 m,p-Xylene	50.000	58.071	116.14	70-130
132 o-Xylene	50.000	57.958	115.92	70-130
133 Styrene	50.000	60.945	121.89	70-130
134 Bromoform	50.000	59.248	118.50	60-140
136 Cumene	50.000	58.670	117.34	60-140
141 1,1,2,2-Tetrachlor	50.000	55.916	111.83	70-130
142 Propylbenzene	50.000	61.706	123.41	60-140
144 4-Ethyltoluene	50.000	61.104	122.21	60-140
147 1,3,5-Trimethylben	50.000	60.288	120.58	70-130
152 1,2,4-Trimethylben	50.000	58.126	116.25	70-130
155 1,3-Dichlorobenzen	50.000	53.531	107.06	70-130
156 1,4-Dichlorobenzen	50.000	55.753	111.51	70-130
157 alpha-Chlorotoluen	50.000	69.595	139.19*	70-130
159 1,2-Dichlorobenzen	50.000	52.367	104.73	70-130
163 1,2,4-Trichloroben	50.000	49.138	98.28	70-130
164 Hexachlorobutadien	50.000	49.827	99.65	70-130
6 Propylene	50.000	60.428	120.86	70-130
165 Naphthalene	50.000	55.656	111.31	60-140
11 Butane	50.000	56.816	113.63	70-130
17 Isopentane	50.000	55.890	111.78	70-130
94 Methyl Cyclohexane	50.000	58.295	116.59	70-130

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	25.086	100.35	70-130
\$ 107 Toluene-d8	25.000	25.299	101.19	70-130
\$ 138 Bromofluorobenzene	25.000	24.913	99.65	70-130



Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111207.d
 Lab Smp Id: ICAL Client Smp ID: Level 1
 Inj Date : 12-NOV-2007 13:22
 Operator : cb Inst ID: msd5.i
 Smp Info : 0.2mL #1576-89
 Misc Info : 200ppbv -> 0.2ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 13:22 Cal File: 5111207.d
 Als bottle: 1 Calibration Sample, Level: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AFCEElow.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	324865	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	255197				42.76- 102.76	78.55
8.031	8.031	(1.000)	49	723656				173.18- 233.18	222.76

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.911	(1.000)	114	1268973	25.0000			70.00- 130.00	100.00
9.911	9.911	(1.000)	88	206541				0.00- 46.42	16.28

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	967469	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	578503				0.00- 30.00	59.80

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.110	9.110	(1.130)	65	466593	25.0000	23.996		70.00- 130.00	100.00
9.110	9.110	(1.130)	67	236655				0.00- 30.00	50.72

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	1063579	25.0000	23.740		70.00- 130.00	100.00
12.676	12.676	(1.279)	70	108141				0.00- 30.00	10.17

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	693173			0.00- 30.00	65.17		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	542906	25.0000	24.050	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	853089			128.71- 188.71	157.13		
16.575	16.575	(1.105)	176	514238			68.26- 128.26	94.72		

72 Chloroform										
						CAS #: 67-66-3				
8.197	8.197	(1.017)	83	10780	0.20000	0.3366	70.00- 130.00	100.00		
8.197	8.197	(1.017)	85	7440			35.19- 95.19	69.02		

81 Benzene										
						CAS #: 71-43-2				
9.082	9.082	(0.916)	78	19738	0.20000	0.3609	70.00- 130.00	100.00		
9.082	9.082	(0.916)	77	5003			0.00- 30.00	25.35		

133 Styrene										
						CAS #: 100-42-5				
15.911	15.911	(1.061)	104	7880	0.20000	0.2034	70.00- 130.00	100.00		
15.911	15.911	(1.061)	78	5297			22.39- 82.39	67.22		

136 Cumene										
						CAS #: 98-82-8				
16.326	16.326	(1.088)	105	21376	0.20000	0.2684	70.00- 130.00	100.00		
16.326	16.326	(1.088)	120	5275			0.00- 30.00	24.68		
16.326	16.326	(1.088)	51	3186			0.00- 30.00	14.90		

157 alpha-Chlorotoluene										
						CAS #: 100-44-7				
17.985	17.985	(1.199)	91	12415	0.20000	0.1999	70.00- 130.00	100.00(a)		
17.985	17.985	(1.199)	126	2022			0.00- 30.00	16.29		

106 4-Methyl-2-pentanone										
						CAS #: 108-10-1				
12.621	12.621	(1.273)	58	4383	0.20000	0.2446	70.00- 130.00	100.00(a)		
12.593	12.593	(1.271)	43	10942			0.00- 30.00	249.65		
12.621	12.621	(1.273)	85	1921			0.00- 30.00	43.83		

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111207.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 0.2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	324865	-8.55
92 1,4-Difluorobenze	1306915	784149	1829681	1268973	-2.90
125 Chlorobenzene-d5	1023463	614078	1432848	967469	-5.47

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111207.d

Date: 12-NOV-2007 13:22

Client ID: Level 1

Sample Info: 0.2mL #1576-89


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-12nov.b/5111207.d



Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111232.d
 Lab Smp Id: ICAL Client Smp ID: Level 2
 Inj Date : 13-NOV-2007 10:41
 Operator : ct Inst ID: msd5.i
 Smp Info : 0.5mL #1576-89
 Misc Info : 0.5ppbv (200ppbv)
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 13-NOV-2007 10:41 Cal File: 5111232.d
 Als bottle: 1 Calibration Sample, Level: 2
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04Low+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	301055	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	241588				42.76- 102.76	80.25
8.059	8.059	(1.000)	49	676243				173.18- 233.18	224.62

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.911	(1.000)	114	1093486	25.0000			70.00- 130.00	100.00
9.911	9.911	(1.000)	88	186745				0.00- 46.42	17.08

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	848011	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	511706				0.00- 30.00	60.34

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.110	9.110	(1.130)	65	422605	25.0000	23.452		70.00- 130.00	100.00
9.110	9.110	(1.130)	67	209734				0.00- 30.00	49.63

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	926376	25.0000	23.996		70.00- 130.00	100.00
12.676	12.676	(1.279)	70	99400				0.00- 30.00	10.73

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	600305			0.00- 30.00	64.80		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	481562	25.0000	24.338	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	749901			128.71- 188.71	155.72		
16.575	16.575	(1.105)	176	460138			68.26- 128.26	95.55		

8 Dichlorodifluoromethane/Fr12						CAS #: 75-71-8				
2.336	2.336	(0.290)	85	12903	0.50000	0.3625	70.00- 130.00	100.00(a)		
2.308	2.308	(0.286)	87	4793			0.00- 30.00	37.15		

9 Freon 114						CAS #: 76-14-2				
2.446	2.446	(0.304)	135	14184	0.50000	0.4366	70.00- 130.00	100.00(a)		
2.446	2.446	(0.304)	137	5692			2.29- 62.29	40.13		

13 Vinyl Chloride						CAS #: 75-01-4				
2.778	2.778	(0.345)	62	11685	0.50000	0.4542	70.00- 130.00	100.00(a)		
2.750	2.750	(0.341)	64	3659			0.00- 30.00	31.31		

12 1,3-Butadiene						CAS #: 106-99-0				
2.750	2.750	(0.341)	54	8235	0.50000	0.3748	70.00- 130.00	100.00(a)		
2.750	2.750	(0.341)	39	10174			0.00- 30.00	123.55		

15 Bromomethane						CAS #: 74-83-9				
3.276	3.276	(0.406)	94	7098	0.50000	0.4273	70.00- 130.00	100.00(a)		
3.276	3.276	(0.406)	96	6564			65.07- 125.07	92.48		

19 Chloroethane						CAS #: 75-00-3				
3.414	3.414	(0.424)	64	6821	0.50000	0.5212	70.00- 130.00	100.00		
3.386	3.386	(0.420)	49	1821			0.00- 30.00	26.70		
3.414	3.414	(0.424)	66	2050			0.00- 30.00	30.05		

20 Trichlorofluoromethane/Fr11						CAS #: 75-69-4				
3.718	3.718	(0.461)	101	17314	0.50000	0.4461	70.00- 130.00	100.00(a)		
3.718	3.718	(0.461)	103	10722			34.56- 94.56	61.93		

30 Freon 113						CAS #: 76-13-1				
4.520	4.520	(0.561)	151	11540	0.50000	0.4782	70.00- 130.00	100.00(a)		
4.520	4.520	(0.561)	153	5960			33.43- 93.43	51.65		
4.520	4.520	(0.561)	101	14065			108.48- 168.48	121.88		

31 1,1-Dichloroethene						CAS #: 75-35-4				
4.547	4.547	(0.564)	61	13348	0.50000	0.4179	70.00- 130.00	100.00(a)		
4.547	4.547	(0.564)	96	6903			27.13- 87.13	51.72		
4.575	4.575	(0.568)	98	6347			5.60- 65.60	47.55		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

35	Carbon Disulfide					CAS #:	75-15-0		
4.907	4.907	(0.609)	76	20015	0.50000	0.3700	70.00- 130.00	100.00(a)	

43	Methylene Chloride					CAS #:	75-09-2		
5.432	5.432	(0.674)	49	13185	0.50000	0.4828	70.00- 130.00	100.00(a)	
5.432	5.432	(0.674)	84	7588			29.81- 89.81	57.55	
5.432	5.432	(0.674)	51	5074			0.00- 30.00	38.48	

46	MTBE					CAS #:	1634-04-4		
5.764	5.764	(0.715)	73	13666	0.50000	0.6648	70.00- 130.00	100.00	
5.764	5.764	(0.715)	57	4935			1.68- 61.68	36.11	
5.764	5.764	(0.715)	41	6421			0.00- 30.00	46.99	

47	trans-1,2-Dichloroethene					CAS #:	156-60-5		
5.819	5.819	(0.722)	96	6986	0.50000	0.3612	70.00- 130.00	100.00(a)	
5.819	5.819	(0.722)	61	14051			133.65- 193.65	201.13	
5.819	5.819	(0.722)	98	5355			0.00- 30.00	76.65	

51	Hexane					CAS #:	110-54-3		
6.151	6.151	(0.763)	57	14853	0.50000	0.3776	70.00- 130.00	100.00(a)	
6.151	6.151	(0.763)	43	13512			0.00- 30.00	90.97	
6.179	6.179	(0.767)	86	3050			0.00- 30.00	20.53	

55	1,1-Dichloroethane					CAS #:	75-34-3		
6.594	6.594	(0.818)	63	12666	0.50000	0.3616	70.00- 130.00	100.00(a)	
6.594	6.594	(0.818)	65	5023			0.52- 60.52	39.66	

67	2-Butanone					CAS #:	78-93-3		
7.700	7.700	(0.955)	72	3857	0.50000	0.4563	70.00- 130.00	100.00(a)	
7.700	7.700	(0.955)	43	13510			536.33- 596.33	350.27	
7.700	7.700	(0.955)	57	1285			0.00- 30.00	33.32	

66	cis-1,2-Dichloroethene					CAS #:	156-59-2		
7.617	7.617	(0.945)	61	10821	0.50000	0.4115	70.00- 130.00	100.00(a)	
7.617	7.617	(0.945)	96	7971			37.56- 97.56	73.66	
7.617	7.617	(0.945)	98	4824			14.52- 74.52	44.58	

70	Tetrahydrofuran					CAS #:	109-99-9		
8.059	8.059	(1.000)	42	17438	0.50000	0.5541	70.00- 130.00	100.00	
8.087	8.087	(1.003)	71	4573			0.00- 55.74	26.22	
8.059	8.059	(1.000)	72	6854			0.00- 30.00	39.30	

72	Chloroform					CAS #:	67-66-3		
8.197	8.197	(1.017)	83	11181	0.50000	0.3768	70.00- 130.00	100.00(a)	
8.197	8.197	(1.017)	85	6949			35.19- 95.19	62.15	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

75	1,1,1-Trichloroethane					CAS #:	71-55-6		
8.418	8.418	(1.045)	97	12913	0.50000	0.4354	70.00-	130.00	100.00(a)
8.446	8.446	(1.048)	99	6490			33.02-	93.02	50.26

74	Cyclohexane					CAS #:	110-82-7		
8.418	8.418	(1.045)	84	8955	0.50000	0.3748	70.00-	130.00	100.00(a)
8.391	8.391	(1.041)	56	15410			126.11-	186.11	172.08
8.391	8.391	(1.041)	41	11390			55.82-	115.82	127.19

77	Carbon Tetrachloride					CAS #:	56-23-5		
8.667	8.667	(1.075)	119	8396	0.50000	0.3428	70.00-	130.00	100.00(a)
8.667	8.667	(1.075)	117	10748			75.98-	135.98	128.01

80	2,2,4-Trimethylpentane					CAS #:	540-84-1		
9.082	9.082	(1.127)	57	38941	0.50000	0.3610	70.00-	130.00	100.00(a)
9.082	9.082	(1.127)	56	14187			0.00-	30.00	36.43
9.082	9.082	(1.127)	41	12183			0.00-	30.00	31.29

81	Benzene					CAS #:	71-43-2		
9.082	9.082	(0.916)	78	18964	0.50000	0.4024	70.00-	130.00	100.00(a)
9.082	9.082	(0.916)	77	4842			0.00-	30.00	25.53

85	1,2-Dichloroethane					CAS #:	107-06-2		
9.276	9.276	(0.936)	62	8877	0.50000	0.4111	70.00-	130.00	100.00(a)
9.276	9.276	(0.936)	64	2677			0.00-	30.00	30.16

90	Heptane					CAS #:	142-82-5		
9.469	9.469	(0.955)	100	1775	0.50000	0.3372	70.00-	130.00	100.00(a)
9.469	9.469	(0.955)	43	15642			0.00-	30.00	881.24
9.469	9.469	(0.955)	71	5645			0.00-	30.00	318.03

93	Trichloroethene					CAS #:	79-01-6		
10.326	10.326	(1.042)	95	9325	0.50000	0.4878	70.00-	130.00	100.00(a)
10.326	10.326	(1.042)	130	7696			64.49-	124.49	82.53
10.354	10.354	(1.045)	97	5987			34.72-	94.72	64.20

98	1,2-Dichloropropane					CAS #:	78-87-5		
10.824	10.824	(1.092)	63	8470	0.50000	0.4570	70.00-	130.00	100.00(a)
10.852	10.852	(1.095)	62	5511			39.05-	99.05	65.06
10.852	10.852	(1.095)	41	5947			36.65-	96.65	70.21

100	Bromodichloromethane					CAS #:	75-27-4		
11.405	11.405	(1.151)	83	10836	0.50000	0.4054	70.00-	130.00	100.00(a)
11.405	11.405	(1.151)	85	7777			34.72-	94.72	71.77

103	cis-1,3-Dichloropropene					CAS #:	10061-01-5		
12.317	12.317	(1.243)	75	6503	0.50000	0.3433	70.00-	130.00	100.00(a)

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
103 cis-1,3-Dichloropropene (continued)									
12.317	12.317	(1.243)	77	1501			0.28- 60.28	23.08	
12.317	12.317	(1.243)	39	6582			43.30- 103.30	101.21	

106 4-Methyl-2-pentanone CAS #: 108-10-1									
12.593	12.593	(1.271)	58	3651	0.50000	0.2364	70.00- 130.00	100.00(a)	
12.593	12.593	(1.271)	43	14600			0.00- 30.00	399.89	
12.593	12.593	(1.271)	85	1498			0.00- 30.00	41.03	

108 Toluene CAS #: 108-88-3									
12.815	12.815	(1.293)	91	23962	0.50000	0.4928	70.00- 130.00	100.00(a)	
12.815	12.815	(1.293)	92	10275			29.65- 89.65	42.88	

113 trans-1,3-Dichloropropene CAS #: 10061-02-6									
13.368	13.368	(0.891)	75	3103	0.50000	0.1732	70.00- 130.00	100.00(a)	
13.340	13.340	(0.889)	77	2407			1.96- 61.96	77.57	
13.368	13.368	(0.891)	39	3144			38.82- 98.82	101.32	

114 1,1,2-Trichloroethane CAS #: 79-00-5									
13.644	13.644	(0.910)	97	6718	0.50000	0.4204	70.00- 130.00	100.00(a)	
13.644	13.644	(0.910)	99	4190			33.63- 93.63	62.37	
13.644	13.644	(0.910)	83	6314			55.73- 115.73	93.99	

116 Tetrachloroethene CAS #: 127-18-4									
13.699	13.699	(0.913)	166	7651	0.50000	0.4119	70.00- 130.00	100.00(a)	
13.672	13.672	(0.912)	129	7468			50.24- 110.24	97.61	
13.699	13.699	(0.913)	131	6779			48.42- 108.42	88.60	

120 Dibromochloromethane CAS #: 124-48-1									
14.197	14.197	(0.947)	129	8233	0.50000	0.3682	70.00- 130.00	100.00(a)	
14.197	14.197	(0.947)	127	6244			0.00- 30.00	75.84	

122 1,2-Dibromoethane CAS #: 106-93-4									
14.363	14.363	(0.958)	107	8908	0.50000	0.3802	70.00- 130.00	100.00(a)	
14.363	14.363	(0.958)	109	9791			63.74- 123.74	109.91	

126 Chlorobenzene CAS #: 108-90-7									
15.027	15.027	(1.002)	112	15065	0.50000	0.4128	70.00- 130.00	100.00(a)	
15.054	15.054	(1.004)	114	4670			1.82- 61.82	31.00	
14.999	14.999	(1.000)	77	17996			31.79- 91.79	119.46	

128 Ethyl Benzene CAS #: 100-41-4									
15.165	15.165	(1.011)	106	9063	0.50000	0.4597	70.00- 130.00	100.00(a)	
15.165	15.165	(1.011)	91	23494			0.00- 30.00	259.23	

130 m,p-Xylene CAS #: 108-38-3									
15.331	15.331	(1.022)	106	9166	0.50000	0.3785	70.00- 130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 m,p-Xylene (continued)									
15.331	15.331	(1.022)	91	18014			0.00- 30.00	196.53	

132 o-Xylene CAS #: 95-47-6									
15.856	15.856	(1.057)	106	9567	0.50000	0.4155	70.00- 130.00	100.00(a)	
15.856	15.856	(1.057)	91	16804			195.49- 255.49	175.65	

133 Styrene CAS #: 100-42-5									
15.911	15.911	(1.061)	104	10002	0.50000	0.2946	70.00- 130.00	100.00(a)	
15.911	15.911	(1.061)	78	6410			22.39- 82.39	64.09	

134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	8207	0.50000	0.4118	70.00- 130.00	100.00(a)	
16.160	16.160	(1.077)	171	3326			21.21- 81.21	40.53	

141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	13004	0.50000	0.3745	70.00- 130.00	100.00(a)	
16.796	16.796	(1.120)	85	8980			33.63- 93.63	69.06	

144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	21447	0.50000	0.3157	70.00- 130.00	100.00(a)	
16.962	16.962	(1.131)	120	8273			0.00- 59.46	38.57	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	21353	0.50000	0.3477	70.00- 130.00	100.00(a)	
17.045	17.045	(1.136)	120	12086			0.00- 30.00	56.60	

152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	17059	0.50000	0.3275	70.00- 130.00	100.00(a)	
17.460	17.460	(1.164)	120	9403			16.11- 76.11	55.12	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	16921	0.50000	0.4588	70.00- 130.00	100.00(a)	
17.764	17.764	(1.184)	148	11100			0.00- 30.00	65.60	
17.764	17.764	(1.184)	111	8925			0.00- 30.00	52.75	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	16084	0.50000	0.3721	70.00- 130.00	100.00(a)	
17.847	17.847	(1.190)	148	12317			0.00- 30.00	76.58	
17.847	17.847	(1.190)	111	6845			0.00- 30.00	42.56	

157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	13937	0.50000	0.2561	70.00- 130.00	100.00(a)	
17.985	17.985	(1.199)	126	2588			0.00- 30.00	18.57	

159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	17160	0.50000	0.4424	70.00- 130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
159 1,2-Dichlorobenzene (continued)									
18.206	18.206	(1.214)	148	11130			32.64- 92.64	64.86	
18.206	18.206	(1.214)	111	5360			11.53- 71.53	31.24	

142 Propylbenzene CAS #: 103-65-1									
16.824	16.824	(1.122)	91	25838	0.50000	0.3231	70.00- 130.00	100.00(a)	
16.824	16.824	(1.122)	120	6184			0.00- 30.00	23.93	
16.851	16.851	(1.123)	105	1630			0.00- 30.00	6.31	

136 Cumene CAS #: 98-82-8									
16.326	16.326	(1.088)	105	23154	0.50000	0.3316	70.00- 130.00	100.00(a)	
16.326	16.326	(1.088)	120	7767			0.00- 30.00	33.54	
16.326	16.326	(1.088)	51	4373			0.00- 30.00	18.89	

94 Methyl Cyclohexane CAS #: 108-87-2									
10.547	10.547	(1.064)	83	10704	0.50000	0.3932	70.00- 130.00	100.00(a)	
10.547	10.547	(1.064)	98	6673			0.00- 30.00	62.34	
10.547	10.547	(1.064)	55	11258			0.00- 30.00	105.18	

QC Flag Legend

a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111232.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 0.5ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	301055	-15.25
92 1,4-Difluorobenze	1306915	784149	1829681	1093486	-16.33
125 Chlorobenzene-d5	1023463	614078	1432848	848011	-17.14

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111232.d

Date: 13-NOV-2007 10:41

Client ID: Level 2

Sample Info: 0.5mL #1576-89


Column phase: RTX-624

Instrument: msd5.1

Operator: ct

Column diameter: 0.53

/chem/msd5.1/5-12nov.b/5111232.d



Report Date: 27-Nov-2007 15:31

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-27nov.b/5112706.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 27-NOV-2007 11:36
 Operator : cb Inst ID: msd5.i
 Smp Info : 2mL #1443-374
 Misc Info : 200ppbv --> 2ppbv
 Comment :
 Method : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Meth Date : 27-Nov-2007 15:31 cbond Quant Type: ISTD
 Cal Date : 27-NOV-2007 11:36 Cal File: 5112706.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp19b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	270347	25.0000		70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	205832			47.29- 107.29	76.14	
8.059	8.059	(1.000)	49	577575			183.28- 243.28	213.64	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.911	(1.000)	114	930111	25.0000		70.00- 130.00	100.00	
9.911	9.911	(1.000)	88	148339			0.00- 46.71	15.95	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	772234	25.0000		70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	425390			0.00- 30.00	55.09	

7 Isobutane CAS #: 75-28-5									
2.501	2.501	(0.310)	43	81360	2.00000	1.641	70.00- 130.00	100.00(a)	
2.501	2.501	(0.310)	42	25417			0.00- 30.00	31.24	
2.474	2.474	(0.307)	58	1783			0.00- 30.00	2.19	

18 Pentane CAS #: 109-66-0									
3.801	3.801	(0.472)	43	78345	2.00000	1.547	70.00- 130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
18 Pentane (continued)									
3.801	3.801	(0.472)	57	12726			0.00- 30.00	16.24	
3.828	3.828	(0.475)	72	6543			0.00- 30.00	8.35	

25 Acrolein						CAS #: 107-02-8			
4.520	4.520	(0.561)	55	7290	2.00000	1.155	70.00- 130.00	100.00(a)	
4.520	4.520	(0.561)	56	10702			0.00- 30.00	146.80	

39 Acrylonitrile						CAS #: 107-13-1			
5.957	5.957	(0.739)	53	28491	2.00000	1.430	70.00- 130.00	100.00(a)	
5.957	5.957	(0.739)	52	17172			0.00- 30.00	60.27	

42 1-Pentene						CAS #: 109-67-1			
3.718	3.718	(0.461)	55	43303	2.00000	1.584	70.00- 130.00	100.00(Ta)	
3.746	3.746	(0.465)	42	56497			0.00- 30.00	130.47	
0.000	1.000	(0.000)	0	0			0.00- 30.00	0.00	

44 Ethyl Ether						CAS #: 60-29-7			
4.188	4.188	(0.520)	74	15996	2.00000	1.547	70.00- 130.00	100.00(Ta)	
4.160	4.160	(0.516)	59	26794			0.00- 30.00	167.50	
0.000	1.000	(0.000)	31	0			0.00- 30.00	0.00	

53 Iodomethane						CAS #: 74-88-4			
4.851	4.851	(0.602)	142	49239	2.00000	1.373	70.00- 130.00	100.00(a)	
4.851	4.851	(0.602)	127	15294			0.00- 30.00	31.06	

58 1-Hexene						CAS #: 592-41-6			
6.040	6.040	(0.750)	55	21859	2.00000	1.380	70.00- 130.00	100.00(a)	
6.040	6.040	(0.750)	41	37770			0.00- 30.00	172.79	
6.040	6.040	(0.750)	84	8721			0.00- 30.00	39.90	

62 Methyl Acrylate						CAS #: 96-33-3			
7.838	7.838	(0.973)	55	35717	2.00000	1.124	70.00- 130.00	100.00(a)	
7.810	7.810	(0.969)	85	4774			0.00- 30.00	13.37	
7.810	7.810	(0.969)	58	3247			0.00- 30.00	9.09	

86 2-Pentanone						CAS #: 107-87-9			
10.824	10.824	(1.092)	43	53061	2.00000	1.145	70.00- 130.00	100.00(a)	
10.796	10.796	(1.089)	58	4329			0.00- 30.00	8.16	
10.824	10.824	(1.092)	86	8341			0.00- 30.00	15.72	

88 Ethyl Acrylate						CAS #: 140-88-5			
10.630	10.630	(1.073)	55	43900	2.00000	1.229	70.00- 130.00	100.00(a)	
10.630	10.630	(1.073)	99	1675			0.00- 30.00	3.82	
10.630	10.630	(1.073)	45	4505			0.00- 30.00	10.26	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
95 Dibromomethane						CAS #: 74-95-3			
11.073	11.073	(1.117)	174	18435	2.00000	1.587	70.00- 130.00	100.00(a)	
11.073	11.073	(1.117)	93	20667			0.00- 30.00	112.11	
11.073	11.073	(1.117)	95	16529			0.00- 30.00	89.66	

96 Methyl Methacrylate						CAS #: 80-62-6			
11.073	11.073	(1.117)	41	30781	2.00000	1.237	70.00- 130.00	100.00(a)	
11.073	11.073	(1.117)	69	14833			0.00- 30.00	48.19	
11.073	11.073	(1.117)	100	5367			0.00- 30.00	17.44	

112 Alphamethylstyrene						CAS #: 98-83-9			
17.294	17.294	(1.153)	118	22987	2.00000	1.031	70.00- 130.00	100.00(a)	
17.294	17.294	(1.153)	103	13393			0.00- 30.00	58.26	

117 Bis(2-chloroethyl) ether						CAS #: 111-44-4			
17.708	17.708	(1.181)	93	38779	2.00000	1.474	70.00- 130.00	100.00(a)	
17.708	17.708	(1.181)	95	13596			0.00- 30.00	35.06	
17.708	17.708	(1.181)	63	36316			0.00- 30.00	93.65	

127 Nonane						CAS #: 111-84-2			
15.331	15.331	(1.022)	43	53552	2.00000	1.237	70.00- 130.00	100.00(a)	
15.331	15.331	(1.022)	57	41083			0.00- 30.00	76.72	
15.331	15.331	(1.022)	85	11561			0.00- 30.00	21.59	

QC Flag Legend

T - Target compound detected outside RT window.
 a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 27-Nov-2007 15:31

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 27-NOV-2007

Lab File ID: 5112706.d

Calibration Time: 09:21

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-27nov.b/t14qn12c.m

Misc Info: 200ppbv --> 2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	351932	211159	492705	270347	-23.18
92 1,4-Difluorobenze	1207474	724484	1690464	930111	-22.97
125 Chlorobenzene-d5	945809	567485	1324133	772234	-18.35

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.94	9.61	10.27	9.91	-0.28
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-27nov.b/5112706.d

Date: 27-NOV-2007 11:36

Client ID: Level 3

Sample Info: 2mL #1443-374


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-27nov.b/5112706.d



Report Date: 20-Nov-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-19nov.b/5111902.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 19-NOV-2007 01:56
 Operator : sjr Inst ID: msd5.i
 Smp Info : 2.0mL #1487-405
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msd5.i/5-19nov.b/t14qn12b.m
 Meth Date : 20-Nov-2007 15:39 ctaylor Quant Type: ISTD
 Cal Date : 19-NOV-2007 01:56 Cal File: 5111902.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp21b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	409441	25.0000		70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	329261			47.38- 107.38	80.42	
8.059	8.059	(1.000)	49	912391			197.25- 257.25	222.84	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.939	9.939	(1.000)	114	1547444	25.0000		70.00- 130.00	100.00	
9.939	9.939	(1.000)	88	252732			0.00- 47.51	16.33	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	1175868	25.0000		70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	671079			0.00- 30.00	57.07	

1 Freon134a CAS #: 811-97-2									
2.253	2.253	(0.280)	83	30938	2.00000	2.000	70.00- 130.00	100.00	
2.253	2.253	(0.280)	69	158131			0.00- 30.00	511.12	

3 Freon 152a CAS #: 75-37-6									
2.336	2.336	(0.290)	65	24878	2.00000	2.000	70.00- 130.00	100.00	
2.391	2.391	(0.297)	51	151737			0.00- 30.00	609.92	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
4 Freon 22						CAS #: 75-45-6			
2.391	2.391	(0.297)	67	9665	2.00000	2.000	70.00- 130.00	100.00	
2.391	2.391	(0.297)	51	149706			0.00- 30.00	1548.95	

5 Freon142b						CAS #: 75-68-3			
2.612	2.612	(0.324)	65	41999	2.00000	2.000	70.00- 130.00	100.00	
2.612	2.612	(0.324)	45	14040			0.00- 30.00	33.43	

16 Dichlorofluoromethane/Fr21						CAS #: 75-43-4			
3.773	3.773	(0.468)	67	64440	2.00000	2.000	70.00- 130.00	100.00	
3.773	3.773	(0.468)	69	21205			0.00- 30.00	32.91	
3.746	3.746	(0.465)	35	1461			0.00- 30.00	2.27	

22 Freon123a						CAS #: 354-23-4			
4.327	4.327	(0.537)	117	38216	2.00000	2.000	70.00- 130.00	100.00	
4.299	4.299	(0.533)	67	50149			0.00- 30.00	131.23	

24 Freon123						CAS #: 306-83-2			
4.437	4.437	(0.551)	83	64366	2.00000	2.000	70.00- 130.00	100.00	
4.437	4.437	(0.551)	133	10230			0.00- 30.00	15.89	
4.437	4.437	(0.551)	85	50869			0.00- 30.00	79.03	

37 tert-Butyl-Alcohol						CAS #: 75-65-0			
5.598	5.598	(0.695)	59	55304	2.00000	2.000	70.00- 130.00	100.00	
5.598	5.598	(0.695)	41	21376			0.00- 30.00	38.65	
5.598	5.598	(0.695)	57	5625			0.00- 30.00	10.17	

49 Isopropyl ether						CAS #: 108-20-3			
6.594	6.594	(0.818)	45	161462	2.00000	2.000	70.00- 130.00	100.00	
6.621	6.621	(0.822)	87	28999			0.00- 30.00	17.96	
6.594	6.594	(0.818)	59	15860			0.00- 30.00	9.82	

57 Ethyl-tert-butyl Ether						CAS #: 637-92-3			
7.230	7.230	(0.897)	59	58157	2.00000	2.000	70.00- 130.00	100.00	
7.230	7.230	(0.897)	87	18728			0.00- 30.00	32.20	
7.230	7.230	(0.897)	41	14279			0.00- 30.00	24.55	

61 Ethyl Acetate						CAS #: 141-78-6			
7.727	7.727	(0.959)	70	7135	2.00000	2.000	70.00- 130.00	100.00	
7.755	7.755	(0.962)	43	63008			0.00- 30.00	883.08	
7.727	7.727	(0.959)	61	7037			0.00- 30.00	98.63	

64 1-Propanol						CAS #: 71-23-8			
6.870	6.870	(0.852)	42	4160	2.00000	2.000	70.00- 130.00	100.00	
6.843	6.843	(0.849)	59	5134			0.00- 30.00	123.41	
6.870	6.870	(0.852)	41	5256			0.00- 30.00	126.35	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

76 Isobutanol						CAS #: 78-83-1			
9.110	9.110	(0.917)	43	33035	2.00000	2.000	70.00- 130.00	100.00	
9.082	9.082	(0.914)	41	22733			0.00- 30.00	68.81	

78 tert-amyl-Methyl Ether						CAS #: 994-05-8			
9.276	9.276	(1.151)	73	51150	2.00000	2.000	70.00- 130.00	100.00	
9.303	9.303	(1.154)	87	15256			0.00- 30.00	29.83	
9.276	9.276	(1.151)	55	24944			0.00- 30.00	48.77	

118 Butyl Acetate						CAS #: 123-86-4			
14.197	14.197	(1.428)	56	31561	2.00000	2.000	70.00- 130.00	100.00	
14.197	14.197	(1.428)	73	9197			0.00- 30.00	29.14	
14.197	14.197	(1.428)	43	79367			0.00- 30.00	251.47	

131 2-Heptanone						CAS #: 110-43-0			
16.105	16.105	(1.074)	58	49073	2.00000	2.000	70.00- 130.00	100.00	
16.105	16.105	(1.074)	43	74991			0.00- 30.00	152.82	

135 Cyclohexanone						CAS #: 108-94-1			
16.520	16.520	(1.101)	55	50207	2.00000	2.000	70.00- 130.00	100.00	
16.520	16.520	(1.101)	98	16347			0.00- 30.00	32.56	
16.520	16.520	(1.101)	42	35309			0.00- 30.00	70.33	

146 Diisobutyl Ketone						CAS #: 108-83-8			
17.211	17.211	(1.147)	57	138864	2.00000	2.000	70.00- 130.00	100.00	
17.211	17.211	(1.147)	85	79860			30.87- 90.87	57.51	

Report Date: 20-Nov-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 19-NOV-2007

Lab File ID: 5111902.d

Calibration Time: 02:24

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd5.i/5-19nov.b/t14qn12b.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	320182	192109	448255	409441	27.88
92 1,4-Difluorobenze	1222930	733758	1712102	1547444	26.54
125 Chlorobenzene-d5	969063	581438	1356688	1175868	21.34

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.94	0.28
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-19nov.b/5111902.d

Date: 19-NOV-2007 01:56

Client ID: Level 3


Sample Info: 2.0mL #1487-405

Column phase: RTX-624

Instrument: msd5.1

Operator: sjr

Column diameter: 0.53



Report Date: 13-Nov-2007 13:24

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111216.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 12-NOV-2007 19:20
 Operator : cb Inst ID: msd5.i
 Smp Info : 2.0mL #1487-404
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:24 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 19:20 Cal File: 5111216.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp20a.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	333304	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	268129				47.79- 107.79	80.45
8.059	8.059	(1.000)	49	749174				186.23- 246.23	224.77

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1294039	25.0000			70.00- 130.00	100.00
9.912	9.912	(1.000)	88	205628				0.00- 46.01	15.89

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	982975	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	582405				0.00- 30.00	59.25

33 Methyl Acetate CAS #: 79-20-9									
5.239	5.239	(0.650)	43	72395	2.00000	1.469		70.00- 130.00	100.00(a)
5.239	5.239	(0.650)	74	13849				0.00- 30.00	19.13
5.239	5.239	(0.650)	59	4835				0.00- 30.00	6.68

52 Chloroprene CAS #: 126-99-8									
6.677	6.677	(0.828)	53	55634	2.00000	1.410		70.00- 130.00	100.00(a)

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
52 Chloroprene (continued)									
6.704	6.704	(0.832)	88	24677			12.60- 72.60	44.36	
6.677	6.677	(0.828)	50	14078			0.00- 52.95	25.30	

59 1,3-Dichloropropane CAS #: 142-28-9									
13.893	13.893	(1.402)	76	37183	2.00000	1.506	70.00- 130.00	100.00(a)	
13.893	13.893	(1.402)	41	36632			68.80- 128.80	98.52	
13.893	13.893	(1.402)	78	14474			0.00- 30.00	38.93	

60 2,2-Dichloropropane CAS #: 594-20-7									
7.561	7.561	(0.938)	77	33830	2.00000	1.467	70.00- 130.00	100.00(a)	
7.561	7.561	(0.938)	79	10723			2.86- 62.86	31.70	
7.561	7.561	(0.938)	97	7959			0.00- 30.00	23.53	

73 1,1-Dichloropropene CAS #: 563-58-6									
8.723	8.723	(1.082)	110	13431	2.00000	1.530	70.00- 130.00	100.00(a)	
8.723	8.723	(1.082)	75	38422			0.00- 30.00	286.07	

123 1,1,1,2-Tetrachloroethane CAS #: 630-20-6									
15.193	15.193	(1.013)	131	26054	2.00000	1.483	70.00- 130.00	100.00(a)	
15.165	15.165	(1.011)	117	19617			0.00- 30.00	75.29	
15.165	15.165	(1.011)	95	13111			0.00- 30.00	50.32	

137 Bromobenzene CAS #: 108-86-1									
16.741	16.741	(1.116)	156	34417	2.00000	1.583	70.00- 130.00	100.00(a)	
16.741	16.741	(1.116)	77	63144			151.57- 211.57	183.47	
16.741	16.741	(1.116)	158	36862			0.00- 30.00	107.10	

139 1,2,3-Trichloropropane CAS #: 96-18-4									
16.852	16.852	(1.123)	110	19269	2.00000	1.615	70.00- 130.00	100.00(a)	
16.852	16.852	(1.123)	61	17041			0.00- 30.00	88.44	
16.852	16.852	(1.123)	112	14352			0.00- 30.00	74.48	

140 2-Chlorotoluene CAS #: 95-49-8									
16.962	16.962	(1.131)	126	25746	2.00000	1.413	70.00- 130.00	100.00(a)	
16.962	16.962	(1.131)	91	89078			287.64- 347.64	345.99	
16.962	16.962	(1.131)	65	10756			0.00- 30.00	41.78	

143 4-Chlorotoluene CAS #: 106-43-4									
17.100	17.100	(1.140)	126	28148	2.00000	1.505	70.00- 130.00	100.00(a)	
17.100	17.100	(1.140)	91	88953			287.83- 347.83	316.02	
17.100	17.100	(1.140)	63	13716			0.00- 30.00	48.73	

149 tert-Butylbenzene CAS #: 98-06-6									
17.377	17.377	(1.159)	119	115990	2.00000	1.533	70.00- 130.00	100.00(a)	
17.377	17.377	(1.159)	134	24294			0.00- 53.69	20.94	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
149 tert-Butylbenzene (continued)									
17.377	17.377	(1.159)	91	68058			0.00- 30.00	58.68	

150 Pentachloroethane CAS #: 76-01-7									
17.460	17.460	(1.164)	167	17042	2.00000	1.283	70.00- 130.00	100.00(a)	
17.432	17.432	(1.162)	117	21565			0.00- 30.00	126.54	

151 sec-Butylbenzene CAS #: 135-98-8									
17.598	17.598	(1.173)	105	138524	2.00000	1.543	70.00- 130.00	100.00(a)	
17.598	17.598	(1.173)	134	21366			0.00- 49.07	15.42	
17.598	17.598	(1.173)	91	26208			0.00- 30.00	18.92	

153 p-Cymene CAS #: 99-87-6									
17.764	17.764	(1.184)	134	26565	2.00000	1.367	70.00- 130.00	100.00(a)	
17.764	17.764	(1.184)	119	95739			341.15- 401.15	360.40	
17.764	17.764	(1.184)	91	23297			0.00- 30.00	87.70	

154 1,2,3-Trimethylbenzene CAS #: 526-73-8									
17.875	17.875	(1.192)	120	37919	2.00000	1.358	70.00- 130.00	100.00(a)	
17.875	17.875	(1.192)	105	93862			197.36- 257.36	247.53	
17.875	17.875	(1.192)	77	10501			0.00- 30.00	27.69	

158 Butylbenzene CAS #: 104-51-8									
18.151	18.151	(1.210)	134	24456	2.00000	1.396	70.00- 130.00	100.00(a)	
18.123	18.123	(1.208)	91	104158			393.82- 453.82	425.90	
18.123	18.123	(1.208)	92	50355			0.00- 30.00	205.90	

160 Hexachloroethane CAS #: 67-72-1									
18.372	18.372	(1.225)	117	35457	2.00000	1.368	70.00- 130.00	100.00(a)	
18.400	18.400	(1.227)	201	21688			0.00- 30.00	61.17	
Sum of Peak Amounts =					1.37				

161 1,2-Dibromo-3-Chloropropane CAS #: 96-12-8									
18.898	18.898	(1.260)	157	23310	2.00000	1.302	70.00- 130.00	100.00(a)	
18.870	18.870	(1.258)	75	30534			92.49- 152.49	130.99	
18.898	18.898	(1.260)	155	18218			0.00- 30.00	78.16	

166 1,2,3-Trichlorobenzene CAS #: 87-61-6									
19.865	19.865	(1.324)	180	65333	2.00000	1.684	70.00- 130.00	100.00(a)	
19.865	19.865	(1.324)	182	62516			0.00- 30.00	95.69	
19.865	19.865	(1.324)	145	19587			0.00- 30.00	29.98	

192 Cyclopentene CAS #: 142-29-0									
5.239	5.239	(0.650)	67	74381	2.00000	1.545	70.00- 130.00	100.00(a)	
5.239	5.239	(0.650)	68	26258			0.00- 30.00	35.30	
5.239	5.239	(0.650)	53	16468			0.00- 30.00	22.14	

QC Flag Legend

a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).

Report Date: 13-Nov-2007 13:24

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111216.d

Calibration Time: 19:48

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	345466	207280	483652	333304	-3.52
92 1,4-Difluorobenze	1312181	787309	1837053	1294039	-1.38
125 Chlorobenzene-d5	1008754	605252	1412256	982975	-2.56

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111216.d

Date: 12-NOV-2007 19:20

Client ID: Level 3

Sample Info: 2.0mL #1487-404


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-12nov.b/5111216.d



Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111209.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 12-NOV-2007 14:17
 Operator : cb Inst ID: msd5.i
 Smp Info : 2mL #1576-89
 Misc Info : 200ppbv -> 2ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 14:17 Cal File: 5111209.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	322724	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	256512				42.76- 102.76	79.48
8.059	8.059	(1.000)	49	726685				173.18- 233.18	225.17

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1214211	25.0000			70.00- 130.00	100.00
9.912	9.912	(1.000)	88	205951				0.00- 46.42	16.96

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	958757	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	568356				0.00- 30.00	59.28

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.137	9.137	(1.134)	65	464909	25.0000	24.068		70.00- 130.00	100.00
9.110	9.110	(1.130)	67	229742				0.00- 30.00	49.42

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	1056409	25.0000	24.643		70.00- 130.00	100.00
12.676	12.676	(1.279)	70	110980				0.00- 30.00	10.51

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	688251			0.00- 30.00	65.15		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	533075	25.0000	23.829	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	889818			128.71- 188.71	166.92		
16.575	16.575	(1.105)	176	520587			68.26- 128.26	97.66		

6 Propylene										
						CAS #: 115-07-1				
2.280	2.280	(0.283)	41	34509	2.00000	1.532	70.00- 130.00	100.00(a)		
2.280	2.280	(0.283)	42	30676			0.00- 30.00	88.89		
2.280	2.280	(0.283)	39	24651			0.00- 30.00	71.43		

8 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.336	2.336	(0.290)	85	62431	2.00000	1.636	70.00- 130.00	100.00		
2.336	2.336	(0.290)	87	24055			0.00- 30.00	38.53		

9 Freon 114										
						CAS #: 76-14-2				
2.474	2.474	(0.307)	135	60617	2.00000	1.740	70.00- 130.00	100.00		
2.474	2.474	(0.307)	137	17640			2.29- 62.29	29.10		

10 Chloromethane										
						CAS #: 74-87-3				
2.584	2.584	(0.321)	50	41485	2.00000	1.448	70.00- 130.00	100.00(a)		
2.612	2.612	(0.324)	52	14778			0.00- 30.00	35.62		

13 Vinyl Chloride										
						CAS #: 75-01-4				
2.778	2.778	(0.345)	62	44200	2.00000	1.603	70.00- 130.00	100.00		
2.778	2.778	(0.345)	64	12716			0.00- 30.00	28.77		

12 1,3-Butadiene										
						CAS #: 106-99-0				
2.750	2.750	(0.341)	54	34201	2.00000	1.452	70.00- 130.00	100.00		
2.750	2.750	(0.341)	39	38518			0.00- 30.00	112.62		

15 Bromomethane										
						CAS #: 74-83-9				
3.276	3.276	(0.406)	94	26487	2.00000	1.488	70.00- 130.00	100.00		
3.276	3.276	(0.406)	96	25693			65.07- 125.07	97.00		

19 Chloroethane										
						CAS #: 75-00-3				
3.414	3.414	(0.424)	64	22215	2.00000	1.584	70.00- 130.00	100.00		
3.414	3.414	(0.424)	49	6499			0.00- 30.00	29.26		
3.414	3.414	(0.424)	66	5751			0.00- 30.00	25.89		

20 Trichlorofluoromethane/Fr11										
						CAS #: 75-69-4				
3.718	3.718	(0.461)	101	65110	2.00000	1.565	70.00- 130.00	100.00		
3.718	3.718	(0.461)	103	47734			34.56- 94.56	73.31		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.105	4.105	(0.509)	45	13596	2.00000	1.504	70.00- 130.00	100.00(a)	
4.105	4.105	(0.509)	43	3872			0.00- 30.00	28.48	
4.105	4.105	(0.509)	46	4661			0.00- 30.00	34.28	

30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	40323	2.00000	1.559	70.00- 130.00	100.00	
4.520	4.520	(0.561)	153	25890			33.43- 93.43	64.21	
4.520	4.520	(0.561)	101	61129			108.48- 168.48	151.60	

31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	55820	2.00000	1.630	70.00- 130.00	100.00	
4.575	4.575	(0.568)	96	30966			27.13- 87.13	55.47	
4.575	4.575	(0.568)	98	20802			5.60- 65.60	37.27	

32 Acetone						CAS #: 67-64-1			
4.741	4.741	(0.588)	58	15775	2.00000	1.232	70.00- 130.00	100.00(a)	
4.741	4.741	(0.588)	43	53793			0.00- 30.00	341.00	

36 2-Propanol						CAS #: 67-63-0			
4.935	4.935	(0.612)	45	59840	2.00000	1.313	70.00- 130.00	100.00(a)	
4.935	4.935	(0.612)	43	22325			0.00- 30.00	37.31	
4.935	4.935	(0.612)	59	2440			0.00- 30.00	4.08	

35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	90183	2.00000	1.555	70.00- 130.00	100.00	

38 3-Chloropropene						CAS #: 107-05-1			
5.183	5.183	(0.643)	76	13938	2.00000	1.444	70.00- 130.00	100.00(a)	
5.183	5.183	(0.643)	41	46871			0.00- 30.00	336.28	

43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	46452	2.00000	1.587	70.00- 130.00	100.00	
5.432	5.432	(0.674)	84	27786			29.81- 89.81	59.82	
5.432	5.432	(0.674)	51	15672			0.00- 30.00	33.74	

46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	39158	2.00000	1.777	70.00- 130.00	100.00	
5.792	5.792	(0.719)	57	11612			1.68- 61.68	29.65	
5.792	5.792	(0.719)	41	16143			0.00- 30.00	41.23	

47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	33004	2.00000	1.592	70.00- 130.00	100.00	
5.819	5.819	(0.722)	61	57452			133.65- 193.65	174.08	
5.819	5.819	(0.722)	98	21915			0.00- 30.00	66.40	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
51 Hexane						CAS #:	110-54-3			
6.151	6.151	(0.763)	57	62884	2.00000	1.491	70.00- 130.00	100.00		
6.151	6.151	(0.763)	43	45994			0.00- 30.00	73.14		
6.179	6.179	(0.767)	86	7888			0.00- 30.00	12.54		

55 1,1-Dichloroethane						CAS #:	75-34-3			
6.594	6.594	(0.818)	63	62245	2.00000	1.658	70.00- 130.00	100.00		
6.594	6.594	(0.818)	65	19845			0.52- 60.52	31.88		

67 2-Butanone						CAS #:	78-93-3			
7.672	7.672	(0.952)	72	11020	2.00000	1.216	70.00- 130.00	100.00		
7.672	7.672	(0.952)	43	61049			536.33- 596.33	553.98		
7.700	7.700	(0.955)	57	5393			0.00- 30.00	48.94		

66 cis-1,2-Dichloroethene						CAS #:	156-59-2			
7.617	7.617	(0.945)	61	45989	2.00000	1.631	70.00- 130.00	100.00		
7.644	7.644	(0.949)	96	27458			37.56- 97.56	59.71		
7.617	7.617	(0.945)	98	20458			14.52- 74.52	44.48		

70 Tetrahydrofuran						CAS #:	109-99-9			
8.059	8.059	(1.000)	42	52041	2.00000	1.542	70.00- 130.00	100.00		
8.059	8.059	(1.000)	71	14250			0.00- 55.74	27.38		
8.059	8.059	(1.000)	72	13170			0.00- 30.00	25.31		

72 Chloroform						CAS #:	67-66-3			
8.197	8.197	(1.017)	83	51953	2.00000	1.633	70.00- 130.00	100.00		
8.197	8.197	(1.017)	85	34726			35.19- 95.19	66.84		

75 1,1,1-Trichloroethane						CAS #:	71-55-6			
8.418	8.418	(1.045)	97	49288	2.00000	1.550	70.00- 130.00	100.00		
8.418	8.418	(1.045)	99	27424			33.02- 93.02	55.64		

74 Cyclohexane						CAS #:	110-82-7			
8.418	8.418	(1.045)	84	40263	2.00000	1.572	70.00- 130.00	100.00		
8.391	8.391	(1.041)	56	59986			126.11- 186.11	148.99		
8.391	8.391	(1.041)	41	35277			55.82- 115.82	87.62		

56 Vinyl Acetate						CAS #:	108-05-4			
6.677	6.677	(0.828)	86	4258	2.00000	0.8952	70.00- 130.00	100.00(a)		
6.677	6.677	(0.828)	43	46710			0.00- 30.00	1096.99		
6.677	6.677	(0.828)	42	6522			0.00- 30.00	153.17		

77 Carbon Tetrachloride						CAS #:	56-23-5			
8.667	8.667	(1.075)	119	40265	2.00000	1.534	70.00- 130.00	100.00		
8.667	8.667	(1.075)	117	46330			75.98- 135.98	115.06		

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.082	9.082	(1.127)	57	166134	2.00000	1.437	70.00-	130.00	100.00	
9.082	9.082	(1.127)	56	53643			0.00-	30.00	32.29	
9.082	9.082	(1.127)	41	48146			0.00-	30.00	28.98	

81	Benzene					CAS #:	71-43-2			
9.082	9.082	(0.916)	78	81098	2.00000	1.550	70.00-	130.00	100.00	
9.082	9.082	(0.916)	77	19267			0.00-	30.00	23.76	

85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	37851	2.00000	1.579	70.00-	130.00	100.00	
9.276	9.276	(0.936)	64	14265			0.00-	30.00	37.69	

90	Heptane					CAS #:	142-82-5			
9.497	9.497	(0.958)	100	8177	2.00000	1.399	70.00-	130.00	100.00	
9.469	9.469	(0.955)	43	68554			0.00-	30.00	838.38	
9.469	9.469	(0.955)	71	25465			0.00-	30.00	311.42	

93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	31935	2.00000	1.504	70.00-	130.00	100.00	
10.326	10.326	(1.042)	130	35650			64.49-	124.49	111.63	
10.326	10.326	(1.042)	97	22195			34.72-	94.72	69.50	

98	1,2-Dichloropropane					CAS #:	78-87-5			
10.824	10.824	(1.092)	63	34179	2.00000	1.661	70.00-	130.00	100.00	
10.852	10.852	(1.095)	62	22975			39.05-	99.05	67.22	
10.852	10.852	(1.095)	41	22269			36.65-	96.65	65.15	

99	1,4-Dioxane					CAS #:	123-91-1			
11.073	11.073	(1.117)	88	18006	2.00000	1.506	70.00-	130.00	100.00(a)	
11.073	11.073	(1.117)	58	18328			62.00-	122.00	101.79	
11.073	11.073	(1.117)	57	7210			0.00-	30.00	40.04	

100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	46637	2.00000	1.571	70.00-	130.00	100.00	
11.405	11.405	(1.151)	85	25261			34.72-	94.72	54.17	

103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	31732	2.00000	1.508	70.00-	130.00	100.00	
12.317	12.317	(1.243)	77	9531			0.28-	60.28	30.04	
12.317	12.317	(1.243)	39	23919			43.30-	103.30	75.38	

106	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.594	12.594	(1.271)	58	22957	2.00000	1.339	70.00-	130.00	100.00	
12.594	12.594	(1.271)	43	75333			0.00-	30.00	328.15	
12.621	12.621	(1.273)	85	8223			0.00-	30.00	35.82	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #:	108-88-3		
12.815	12.815	(1.293)	91	84031	2.00000	1.556	70.00-	130.00	100.00
12.815	12.815	(1.293)	92	49902			29.65-	89.65	59.39

113 trans-1,3-Dichloropropene						CAS #:	10061-02-6		
13.368	13.368	(0.891)	75	22625	2.00000	1.117	70.00-	130.00	100.00
13.368	13.368	(0.891)	77	8200			1.96-	61.96	36.24
13.368	13.368	(0.891)	39	16458			38.82-	98.82	72.74

114 1,1,2-Trichloroethane						CAS #:	79-00-5		
13.644	13.644	(0.910)	97	30273	2.00000	1.675	70.00-	130.00	100.00
13.644	13.644	(0.910)	99	19956			33.63-	93.63	65.92
13.644	13.644	(0.910)	83	24520			55.73-	115.73	81.00

116 Tetrachloroethene						CAS #:	127-18-4		
13.699	13.699	(0.913)	166	37916	2.00000	1.805	70.00-	130.00	100.00
13.672	13.672	(0.912)	129	24639			50.24-	110.24	64.98
13.699	13.699	(0.913)	131	24276			48.42-	108.42	64.03

119 2-Hexanone						CAS #:	591-78-6		
14.031	14.031	(0.935)	58	29687	2.00000	1.178	70.00-	130.00	100.00(a)
14.031	14.031	(0.935)	43	64036			168.65-	228.65	215.70
14.031	14.031	(0.935)	100	4239			0.00-	30.00	14.28

120 Dibromochloromethane						CAS #:	124-48-1		
14.197	14.197	(0.947)	129	35286	2.00000	1.396	70.00-	130.00	100.00
14.197	14.197	(0.947)	127	26625			0.00-	30.00	75.45

122 1,2-Dibromoethane						CAS #:	106-93-4		
14.363	14.363	(0.958)	107	39203	2.00000	1.480	70.00-	130.00	100.00
14.363	14.363	(0.958)	109	34913			63.74-	123.74	89.06

126 Chlorobenzene						CAS #:	108-90-7		
15.027	15.027	(1.002)	112	72501	2.00000	1.757	70.00-	130.00	100.00
15.027	15.027	(1.002)	114	21533			1.82-	61.82	29.70
15.027	15.027	(1.002)	77	47947			31.79-	91.79	66.13

128 Ethyl Benzene						CAS #:	100-41-4		
15.165	15.165	(1.011)	106	29817	2.00000	1.338	70.00-	130.00	100.00
15.165	15.165	(1.011)	91	112702			0.00-	30.00	377.98

130 m,p-Xylene						CAS #:	108-38-3		
15.331	15.331	(1.022)	106	39645	2.00000	1.448	70.00-	130.00	100.00
15.331	15.331	(1.022)	91	85232			0.00-	30.00	214.99

132 o-Xylene						CAS #:	95-47-6		
15.856	15.856	(1.057)	106	40312	2.00000	1.548	70.00-	130.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	83837			195.49- 255.49	207.97	

133 Styrene									
15.911	15.911	(1.061)	104	46549	2.00000	1.213	70.00- 130.00	100.00	
15.911	15.911	(1.061)	78	26850			22.39- 82.39	57.68	

134 Bromoform									
16.160	16.160	(1.077)	173	30933	2.00000	1.373	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	16221			21.21- 81.21	52.44	

141 1,1,2,2-Tetrachloroethane									
16.796	16.796	(1.120)	83	66301	2.00000	1.689	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	42929			33.63- 93.63	64.75	

144 4-Ethyltoluene									
16.962	16.962	(1.131)	105	111317	2.00000	1.449	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	31652			0.00- 59.46	28.43	

147 1,3,5-Trimethylbenzene									
17.045	17.045	(1.136)	105	103369	2.00000	1.489	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	52144			0.00- 30.00	50.44	

152 1,2,4-Trimethylbenzene									
17.460	17.460	(1.164)	105	88326	2.00000	1.500	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	40529			16.11- 76.11	45.89	

155 1,3-Dichlorobenzene									
17.764	17.764	(1.184)	146	66466	2.00000	1.594	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	46072			0.00- 30.00	69.32	
17.764	17.764	(1.184)	111	29558			0.00- 30.00	44.47	

156 1,4-Dichlorobenzene									
17.847	17.847	(1.190)	146	84647	2.00000	1.732	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	47850			0.00- 30.00	56.53	
17.847	17.847	(1.190)	111	35983			0.00- 30.00	42.51	

157 alpha-Chlorotoluene									
17.985	17.985	(1.199)	91	60800	2.00000	0.9881	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	12615			0.00- 30.00	20.75	

159 1,2-Dichlorobenzene									
18.206	18.206	(1.214)	146	83215	2.00000	1.897	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	48015			32.64- 92.64	57.70	
18.206	18.206	(1.214)	111	30589			11.53- 71.53	36.76	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.506	19.506	(1.300)	180	59101	2.00000	1.898	70.00- 130.00	100.00(a)	
19.506	19.506	(1.300)	182	53267			63.93- 123.93	90.13	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.589	19.589	(1.306)	225	41151	2.00000	1.882	70.00- 130.00	100.00(a)	
19.589	19.589	(1.306)	223	24876			32.69- 92.69	60.45	

142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	141217	2.00000	1.562	70.00- 130.00	100.00	
16.852	16.852	(1.123)	120	31026			0.00- 30.00	21.97	
16.852	16.852	(1.123)	105	4167			0.00- 30.00	2.95	

136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	114034	2.00000	1.445	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	27668			0.00- 30.00	24.26	
16.326	16.326	(1.088)	51	17582			0.00- 30.00	15.42	

165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	197397	2.00000	1.904	70.00- 130.00	100.00(a)	
19.672	19.672	(1.312)	127	24023			0.00- 30.00	12.17	

17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	64612	2.00000	1.617	70.00- 130.00	100.00(a)	
3.414	3.414	(0.424)	57	43012			0.00- 30.00	66.57	
3.414	3.414	(0.424)	72	3775			0.00- 30.00	5.84	

11	Butane					CAS #: 106-97-8			
2.667	2.667	(0.331)	58	10883	2.00000	1.598	70.00- 130.00	100.00(a)	
2.667	2.667	(0.331)	43	85425			0.00- 30.00	784.94	

94	Methyl Cyclohexane					CAS #: 108-87-2			
10.547	10.547	(1.064)	83	47307	2.00000	1.565	70.00- 130.00	100.00	
10.547	10.547	(1.064)	98	22026			0.00- 30.00	46.56	
10.547	10.547	(1.064)	55	54868			0.00- 30.00	115.98	

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111209.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	322724	-9.15
92 1,4-Difluorobenze	1306915	784149	1829681	1214211	-7.09
125 Chlorobenzene-d5	1023463	614078	1432848	958757	-6.32

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111209.d

Date: 12-NOV-2007 14:17

Client ID: Level 3

Sample Info: 2mL #1576-89


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-12nov.b/5111209.d

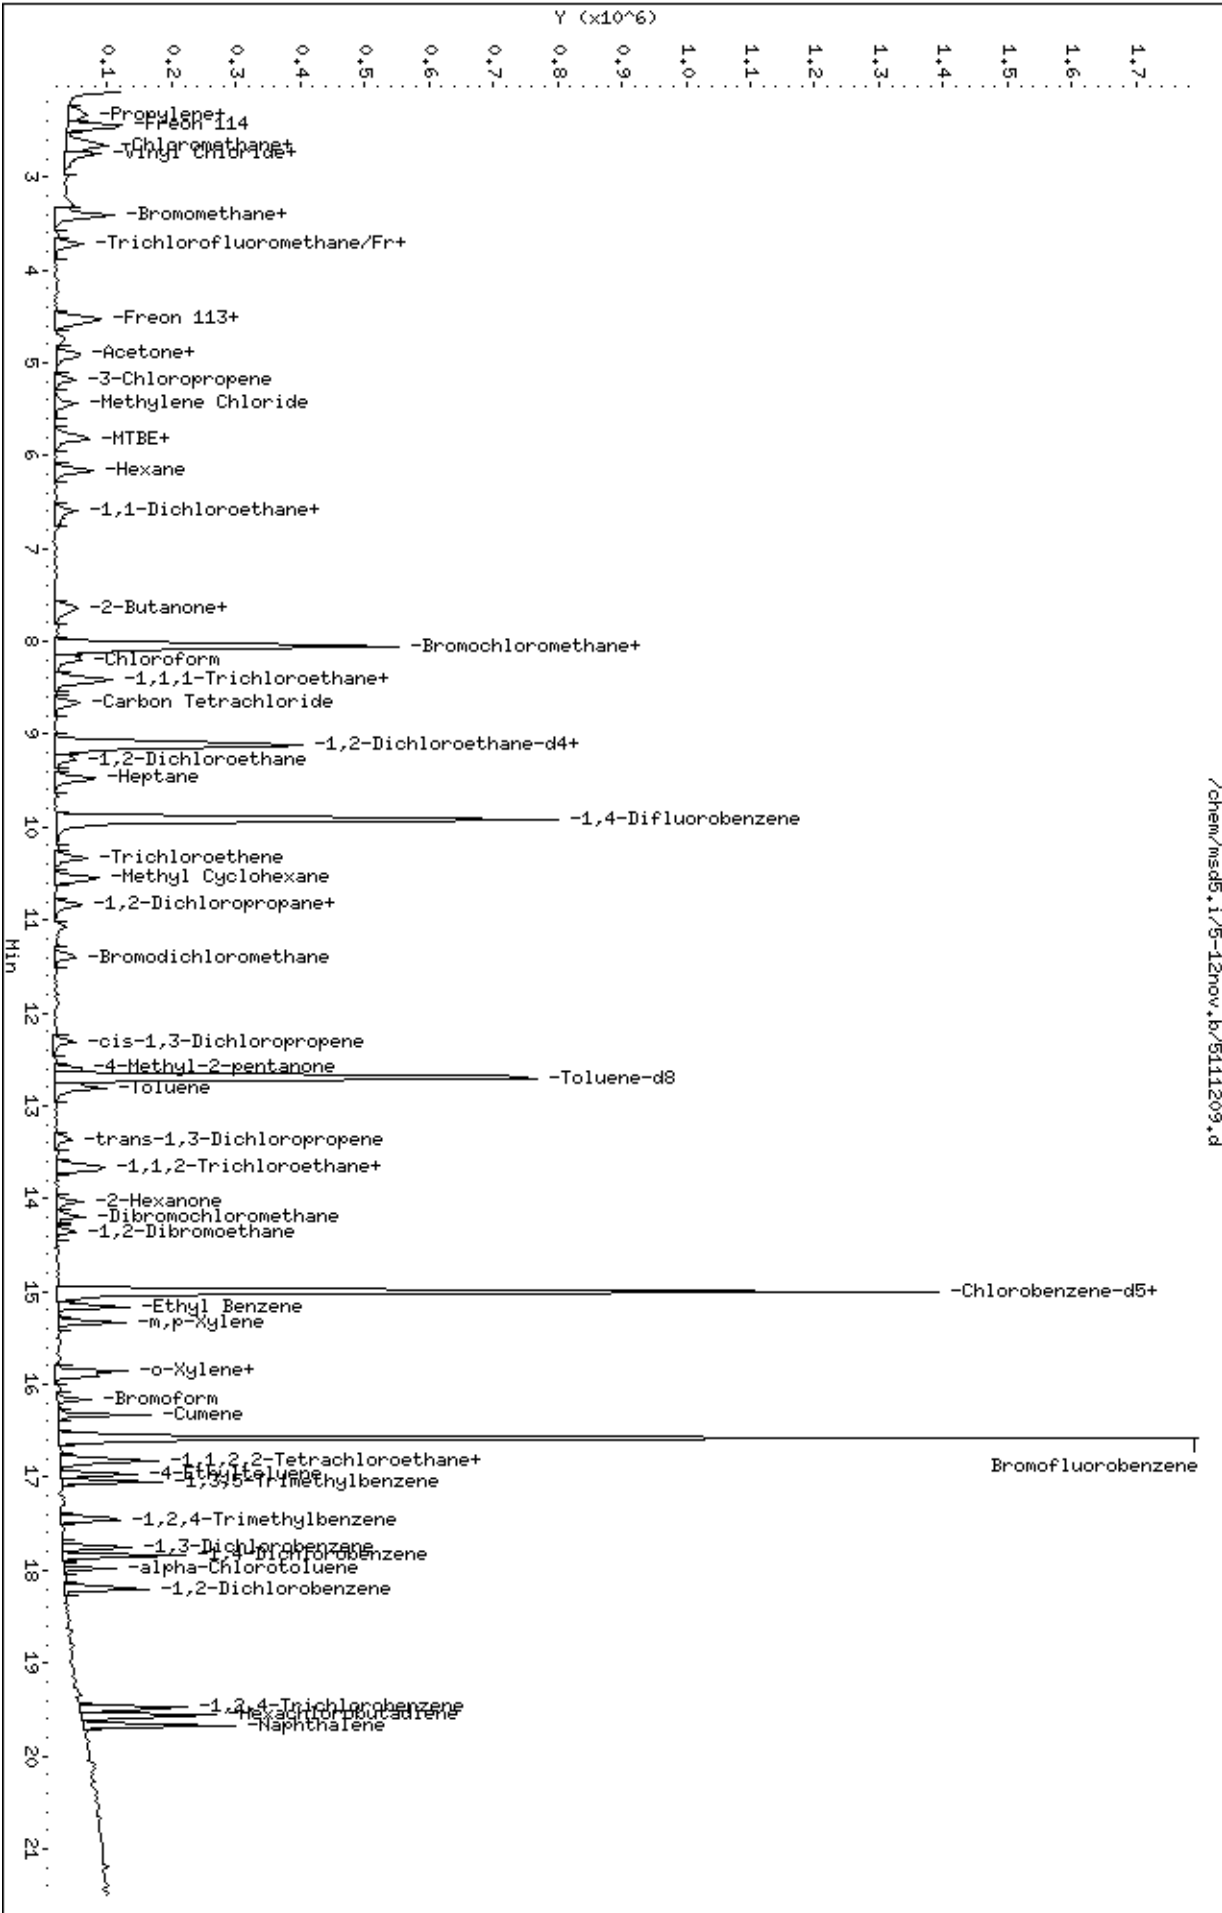

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111210.d
 Lab Smp Id: ICAL Client Smp ID: Level 4
 Inj Date : 12-NOV-2007 14:45
 Operator : cb Inst ID: msd5.i
 Smp Info : 25mL #1576-89
 Misc Info : 200ppbv -> 25ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 14:45 Cal File: 5111210.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	334527	25.0000		70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	260785			42.76- 102.76	77.96	
8.031	8.031	(1.000)	49	727160			173.18- 233.18	217.37	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1289908	25.0000		70.00- 130.00	100.00	
9.912	9.912	(1.000)	88	199765			0.00- 46.42	15.49	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	997843	25.0000		70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	587344			0.00- 30.00	58.86	

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.110	9.110	(1.130)	65	483717	25.0000	24.158	70.00- 130.00	100.00	
9.137	9.137	(1.134)	67	270045			0.00- 30.00	55.83	

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	1153506	25.0000	25.329	70.00- 130.00	100.00	
12.704	12.704	(1.282)	70	115740			0.00- 30.00	10.03	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	758692			0.00- 30.00	65.77		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	591715	25.0000	25.414	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	932598			128.71- 188.71	157.61		
16.575	16.575	(1.105)	176	571616			68.26- 128.26	96.60		

6 Propylene										
						CAS #: 115-07-1				
2.280	2.280	(0.283)	41	662690	25.0000	28.381	70.00- 130.00	100.00		
2.280	2.280	(0.283)	42	450921			0.00- 30.00	68.04		
2.280	2.280	(0.283)	39	450789			0.00- 30.00	68.02		

8 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.336	2.336	(0.290)	85	1146478	25.0000	28.984	70.00- 130.00	100.00		
2.336	2.336	(0.290)	87	378796			0.00- 30.00	33.04		

9 Freon 114										
						CAS #: 76-14-2				
2.446	2.446	(0.304)	135	1050229	25.0000	29.093	70.00- 130.00	100.00		
2.446	2.446	(0.304)	137	322619			2.29- 62.29	30.72		

10 Chloromethane										
						CAS #: 74-87-3				
2.585	2.585	(0.321)	50	855747	25.0000	28.811	70.00- 130.00	100.00		
2.585	2.585	(0.321)	52	260182			0.00- 30.00	30.40		

13 Vinyl Chloride										
						CAS #: 75-01-4				
2.778	2.778	(0.345)	62	838816	25.0000	29.341	70.00- 130.00	100.00		
2.778	2.778	(0.345)	64	261204			0.00- 30.00	31.14		

12 1,3-Butadiene										
						CAS #: 106-99-0				
2.750	2.750	(0.341)	54	752822	25.0000	30.834	70.00- 130.00	100.00		
2.750	2.750	(0.341)	39	795006			0.00- 30.00	105.60		

15 Bromomethane										
						CAS #: 74-83-9				
3.276	3.276	(0.406)	94	546191	25.0000	29.593	70.00- 130.00	100.00		
3.276	3.276	(0.406)	96	523940			65.07- 125.07	95.93		

19 Chloroethane										
						CAS #: 75-00-3				
3.386	3.386	(0.420)	64	429880	25.0000	29.561	70.00- 130.00	100.00		
3.386	3.386	(0.420)	49	120010			0.00- 30.00	27.92		
3.386	3.386	(0.420)	66	127147			0.00- 30.00	29.58		

20 Trichlorofluoromethane/Fr11										
						CAS #: 75-69-4				
3.718	3.718	(0.461)	101	1264537	25.0000	29.322	70.00- 130.00	100.00		
3.718	3.718	(0.461)	103	819011			34.56- 94.56	64.77		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.078	4.078	(0.506)	45	279983	25.0000	29.884	70.00- 130.00	100.00	
4.078	4.078	(0.506)	43	55168			0.00- 30.00	19.70	
4.078	4.078	(0.506)	46	117750			0.00- 30.00	42.06	

30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	793323	25.0000	29.584	70.00- 130.00	100.00	
4.520	4.520	(0.561)	153	486250			33.43- 93.43	61.29	
4.520	4.520	(0.561)	101	1063047			108.48- 168.48	134.00	

31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	1025912	25.0000	28.907	70.00- 130.00	100.00	
4.575	4.575	(0.568)	96	579347			27.13- 87.13	56.47	
4.575	4.575	(0.568)	98	379018			5.60- 65.60	36.94	

32 Acetone						CAS #: 67-64-1			
4.714	4.714	(0.585)	58	374495	25.0000	28.212	70.00- 130.00	100.00	
4.714	4.714	(0.585)	43	1138367			0.00- 30.00	303.97	

36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	1288123	25.0000	27.267	70.00- 130.00	100.00	
4.907	4.907	(0.609)	43	286038			0.00- 30.00	22.21	
4.935	4.935	(0.612)	59	48259			0.00- 30.00	3.75	

35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	1812623	25.0000	30.160	70.00- 130.00	100.00	

38 3-Chloropropene						CAS #: 107-05-1			
5.184	5.184	(0.643)	76	274594	25.0000	27.441	70.00- 130.00	100.00	
5.184	5.184	(0.643)	41	1080424			0.00- 30.00	393.46	

43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	864094	25.0000	28.474	70.00- 130.00	100.00	
5.432	5.432	(0.674)	84	511783			29.81- 89.81	59.23	
5.432	5.432	(0.674)	51	267550			0.00- 30.00	30.96	

46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	628320	25.0000	27.505	70.00- 130.00	100.00	
5.764	5.764	(0.715)	57	190297			1.68- 61.68	30.29	
5.764	5.764	(0.715)	41	220926			0.00- 30.00	35.16	

47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.820	5.820	(0.722)	96	642782	25.0000	29.906	70.00- 130.00	100.00	
5.820	5.820	(0.722)	61	1038046			133.65- 193.65	161.49	
5.820	5.820	(0.722)	98	412618			0.00- 30.00	64.19	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	1293253	25.0000	29.589	70.00- 130.00	100.00	
6.151	6.151	(0.763)	43	912632			0.00- 30.00	70.57	
6.151	6.151	(0.763)	86	175618			0.00- 30.00	13.58	

55 1,1-Dichloroethane						CAS #: 75-34-3			
6.594	6.594	(0.818)	63	1159420	25.0000	29.792	70.00- 130.00	100.00	
6.594	6.594	(0.818)	65	353585			0.52- 60.52	30.50	

67 2-Butanone						CAS #: 78-93-3			
7.672	7.672	(0.952)	72	260618	25.0000	27.749	70.00- 130.00	100.00	
7.672	7.672	(0.952)	43	1556458			536.33- 596.33	597.22	
7.672	7.672	(0.952)	57	108815			0.00- 30.00	41.75	

66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	852737	25.0000	29.183	70.00- 130.00	100.00	
7.617	7.617	(0.945)	96	579802			37.56- 97.56	67.99	
7.617	7.617	(0.945)	98	374515			14.52- 74.52	43.92	

70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	941307	25.0000	26.918	70.00- 130.00	100.00	
8.031	8.031	(0.997)	71	243549			0.00- 55.74	25.87	
8.031	8.031	(0.997)	72	276695			0.00- 30.00	29.39	

72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	974502	25.0000	29.554	70.00- 130.00	100.00	
8.197	8.197	(1.017)	85	633277			35.19- 95.19	64.98	

75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.419	8.419	(1.045)	97	934919	25.0000	28.366	70.00- 130.00	100.00	
8.419	8.419	(1.045)	99	613886			33.02- 93.02	65.66	

74 Cyclohexane						CAS #: 110-82-7			
8.419	8.419	(1.045)	84	792547	25.0000	29.850	70.00- 130.00	100.00	
8.391	8.391	(1.041)	56	1226244			126.11- 186.11	154.72	
8.391	8.391	(1.041)	41	701484			55.82- 115.82	88.51	

56 Vinyl Acetate						CAS #: 108-05-4			
6.677	6.677	(0.828)	86	138576	25.0000	28.107	70.00- 130.00	100.00	
6.649	6.649	(0.825)	43	1704333			0.00- 30.00	1229.89	
6.649	6.649	(0.825)	42	130423			0.00- 30.00	94.12	

77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	809879	25.0000	29.761	70.00- 130.00	100.00	
8.667	8.667	(1.075)	117	859338			75.98- 135.98	106.11	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.110	9.110	(1.130)	57	3611843	25.0000	30.137	70.00- 130.00	100.00		
9.110	9.110	(1.130)	56	1138268			0.00- 30.00	31.51		
9.110	9.110	(1.130)	41	934324			0.00- 30.00	25.87		

81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	1645273	25.0000	29.592	70.00- 130.00	100.00		
9.082	9.082	(0.916)	77	374414			0.00- 30.00	22.76		

85	1,2-Dichloroethane					CAS #: 107-06-2				
9.276	9.276	(0.936)	62	733430	25.0000	28.795	70.00- 130.00	100.00		
9.276	9.276	(0.936)	64	229542			0.00- 30.00	31.30		

90	Heptane					CAS #: 142-82-5				
9.497	9.497	(0.958)	100	187102	25.0000	30.129	70.00- 130.00	100.00		
9.469	9.469	(0.955)	43	1432521			0.00- 30.00	765.64		
9.469	9.469	(0.955)	71	558888			0.00- 30.00	298.71		

93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	643545	25.0000	28.538	70.00- 130.00	100.00		
10.326	10.326	(1.042)	130	606528			64.49- 124.49	94.25		
10.326	10.326	(1.042)	97	408553			34.72- 94.72	63.48		

98	1,2-Dichloropropane					CAS #: 78-87-5				
10.824	10.824	(1.092)	63	605108	25.0000	27.675	70.00- 130.00	100.00		
10.852	10.852	(1.095)	62	432166			39.05- 99.05	71.42		
10.824	10.824	(1.092)	41	428434			36.65- 96.65	70.80		

99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.117)	88	331486	25.0000	26.104	70.00- 130.00	100.00		
11.073	11.073	(1.117)	58	317598			62.00- 122.00	95.81		
11.073	11.073	(1.117)	57	103554			0.00- 30.00	31.24		

100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.151)	83	900304	25.0000	28.555	70.00- 130.00	100.00		
11.405	11.405	(1.151)	85	563113			34.72- 94.72	62.55		

103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	629894	25.0000	28.188	70.00- 130.00	100.00		
12.317	12.317	(1.243)	77	201792			0.28- 60.28	32.04		
12.289	12.289	(1.240)	39	478334			43.30- 103.30	75.94		

106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.594	12.594	(1.271)	58	530758	25.0000	29.139	70.00- 130.00	100.00		
12.594	12.594	(1.271)	43	1509968			0.00- 30.00	284.49		
12.594	12.594	(1.271)	85	169679			0.00- 30.00	31.97		

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
108 Toluene						CAS #:	108-88-3			
12.815	12.815	(1.293)	91	1600261	25.0000	27.900	70.00-	130.00	100.00	
12.815	12.815	(1.293)	92	944522			29.65-	89.65	59.02	

113 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.368	13.368	(0.891)	75	614344	25.0000	29.141	70.00-	130.00	100.00	
13.368	13.368	(0.891)	77	195343			1.96-	61.96	31.80	
13.368	13.368	(0.891)	39	433660			38.82-	98.82	70.59	

114 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.644	13.644	(0.910)	97	543918	25.0000	28.923	70.00-	130.00	100.00	
13.644	13.644	(0.910)	99	333845			33.63-	93.63	61.38	
13.644	13.644	(0.910)	83	469329			55.73-	115.73	86.29	

116 Tetrachloroethene						CAS #:	127-18-4			
13.700	13.700	(0.913)	166	641390	25.0000	29.342	70.00-	130.00	100.00	
13.672	13.672	(0.912)	129	519336			50.24-	110.24	80.97	
13.700	13.700	(0.913)	131	465809			48.42-	108.42	72.62	

119 2-Hexanone						CAS #:	591-78-6			
14.004	14.004	(0.934)	58	705936	25.0000	26.910	70.00-	130.00	100.00	
14.004	14.004	(0.934)	43	1449745			168.65-	228.65	205.36	
14.031	14.031	(0.935)	100	106081			0.00-	30.00	15.03	

120 Dibromochloromethane						CAS #:	124-48-1			
14.197	14.197	(0.947)	129	781679	25.0000	29.707	70.00-	130.00	100.00	
14.197	14.197	(0.947)	127	629962			0.00-	30.00	80.59	

122 1,2-Dibromoethane						CAS #:	106-93-4			
14.363	14.363	(0.958)	107	810766	25.0000	29.412	70.00-	130.00	100.00	
14.363	14.363	(0.958)	109	766083			63.74-	123.74	94.49	

126 Chlorobenzene						CAS #:	108-90-7			
15.027	15.027	(1.002)	112	1244447	25.0000	28.982	70.00-	130.00	100.00	
15.027	15.027	(1.002)	114	386814			1.82-	61.82	31.08	
15.027	15.027	(1.002)	77	775823			31.79-	91.79	62.34	

128 Ethyl Benzene						CAS #:	100-41-4			
15.165	15.165	(1.011)	106	682779	25.0000	29.433	70.00-	130.00	100.00	
15.165	15.165	(1.011)	91	2277047			0.00-	30.00	333.50	

130 m,p-Xylene						CAS #:	108-38-3			
15.331	15.331	(1.022)	106	870860	25.0000	30.564	70.00-	130.00	100.00	
15.331	15.331	(1.022)	91	1817374			0.00-	30.00	208.69	

132 o-Xylene						CAS #:	95-47-6			
15.856	15.856	(1.057)	106	797683	25.0000	29.441	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	1777338			195.49- 255.49	222.81	

133 Styrene									
15.912	15.912	(1.061)	104	1266850	25.0000	31.713	70.00- 130.00	100.00	
15.912	15.912	(1.061)	78	629233			22.39- 82.39	49.67	

134 Bromoform									
16.160	16.160	(1.077)	173	675390	25.0000	28.802	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	359161			21.21- 81.21	53.18	

141 1,1,2,2-Tetrachloroethane									
16.796	16.796	(1.120)	83	1232295	25.0000	30.158	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	772986			33.63- 93.63	62.73	

144 4-Ethyltoluene									
16.962	16.962	(1.131)	105	2465606	25.0000	30.842	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	715161			0.00- 59.46	29.01	

147 1,3,5-Trimethylbenzene									
17.045	17.045	(1.136)	105	2280818	25.0000	31.564	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	1072498			0.00- 30.00	47.02	

152 1,2,4-Trimethylbenzene									
17.460	17.460	(1.164)	105	1826338	25.0000	29.794	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	851499			16.11- 76.11	46.62	

155 1,3-Dichlorobenzene									
17.764	17.764	(1.184)	146	1241257	25.0000	28.603	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	812078			0.00- 30.00	65.42	
17.764	17.764	(1.184)	111	499022			0.00- 30.00	40.20	

156 1,4-Dichlorobenzene									
17.847	17.847	(1.190)	146	1514808	25.0000	29.784	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	963066			0.00- 30.00	63.58	
17.847	17.847	(1.190)	111	647676			0.00- 30.00	42.76	

157 alpha-Chlorotoluene									
17.985	17.985	(1.199)	91	1979971	25.0000	30.916	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	394352			0.00- 30.00	19.92	

159 1,2-Dichlorobenzene									
18.206	18.206	(1.214)	146	1258812	25.0000	27.579	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	803161			32.64- 92.64	63.80	
18.206	18.206	(1.214)	111	506882			11.53- 71.53	40.27	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.506	19.506	(1.300)	180	826354	25.0000	25.506	70.00- 130.00	100.00	
19.506	19.506	(1.300)	182	806386			63.93- 123.93	97.58	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.589	19.589	(1.306)	225	607708	25.0000	26.699	70.00- 130.00	100.00	
19.589	19.589	(1.306)	223	380207			32.69- 92.69	62.56	

142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	2855716	25.0000	30.351	70.00- 130.00	100.00	
16.824	16.824	(1.122)	120	608220			0.00- 30.00	21.30	
16.824	16.824	(1.122)	105	99037			0.00- 30.00	3.47	

136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	2396295	25.0000	29.169	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	632802			0.00- 30.00	26.41	
16.326	16.326	(1.088)	51	340331			0.00- 30.00	14.20	

165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	3032327	25.0000	28.102	70.00- 130.00	100.00	
19.672	19.672	(1.312)	127	372568			0.00- 30.00	12.29	

17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	1168743	25.0000	28.222	70.00- 130.00	100.00	
3.414	3.414	(0.424)	57	771876			0.00- 30.00	66.04	
3.414	3.414	(0.424)	72	70331			0.00- 30.00	6.02	

11	Butane					CAS #: 106-97-8			
2.667	2.667	(0.331)	58	200544	25.0000	28.403	70.00- 130.00	100.00	
2.667	2.667	(0.331)	43	1493932			0.00- 30.00	744.94	

94	Methyl Cyclohexane					CAS #: 108-87-2			
10.548	10.548	(1.064)	83	951148	25.0000	29.620	70.00- 130.00	100.00	
10.548	10.548	(1.064)	98	442883			0.00- 30.00	46.56	
10.548	10.548	(1.064)	55	1041822			0.00- 30.00	109.53	

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111210.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	334527	-5.83
92 1,4-Difluorobenze	1306915	784149	1829681	1289908	-1.30
125 Chlorobenzene-d5	1023463	614078	1432848	997843	-2.50


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 27-Nov-2007 15:31

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-27nov.b/5112702.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 27-NOV-2007 09:21
 Operator : cb Inst ID: msd5.i
 Smp Info : 50mL #1443-374
 Misc Info : 50ppbv (200ppbv)
 Comment :
 Method : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Meth Date : 27-Nov-2007 15:31 cbond Quant Type: ISTD
 Cal Date : 27-NOV-2007 09:21 Cal File: 5112702.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp19b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	351932	25.0000			80.00- 120.00	100.00
8.059	8.059	(1.000)	128	271999				47.29- 107.29	77.29
8.059	8.059	(1.000)	49	750615				183.28- 243.28	213.28

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.939	9.939	(1.000)	114	1207474	25.0000			80.00- 120.00	100.00
9.912	9.912	(1.000)	88	201712				0.00- 46.71	16.71

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	945809	25.0000			80.00- 120.00	100.00
14.999	14.999	(1.000)	82	538652				26.95- 86.95	56.95

7 Isobutane CAS #: 75-28-5									
2.502	2.502	(0.310)	43	3734639	50.0000	57.850		80.00- 120.00	100.00
2.502	2.502	(0.310)	42	1231328				2.97- 62.97	32.97
2.502	2.502	(0.310)	58	103831				0.00- 32.78	2.78

18 Pentane CAS #: 109-66-0									
3.829	3.829	(0.475)	43	3761769	50.0000	57.050		80.00- 120.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
18 Pentane (continued)									
3.829	3.829	(0.475)	57	554812			0.00- 44.75	14.75	
3.829	3.829	(0.475)	72	320049			0.00- 38.51	8.51	

25 Acrolein					CAS #: 107-02-8				
4.492	4.492	(0.557)	55	509181	50.0000	61.969	80.00- 120.00	100.00	
4.492	4.492	(0.557)	56	732493			113.86- 173.86	143.86	

39 Acrylonitrile					CAS #: 107-13-1				
5.958	5.958	(0.739)	53	1495490	50.0000	57.662	80.00- 120.00	100.00	
5.958	5.958	(0.739)	52	1118902			44.82- 104.82	74.82	

42 1-Pentene					CAS #: 109-67-1				
3.746	3.746	(0.465)	55	2025749	50.0000	56.940	80.00- 120.00	100.00(T)	
3.746	3.746	(0.465)	42	3115059			123.77- 183.77	153.77	
0.000	1.000	(0.000)	0	0			0.00- 30.00	0.00	

44 Ethyl Ether					CAS #: 60-29-7				
4.188	4.188	(0.520)	74	768359	50.0000	57.089	80.00- 120.00	100.00(T)	
4.188	4.188	(0.520)	59	1292702			138.24- 198.24	168.24	
0.000	1.000	(0.000)	31	0			0.00- 30.00	0.00	

53 Iodomethane					CAS #: 74-88-4				
4.852	4.852	(0.602)	142	2900304	50.0000	62.117	80.00- 120.00	100.00	
4.852	4.852	(0.602)	127	938980			2.38- 62.38	32.38	

58 1-Hexene					CAS #: 592-41-6				
6.068	6.068	(0.753)	55	1196417	50.0000	58.001	80.00- 120.00	100.00	
6.068	6.068	(0.753)	41	1853146			124.89- 184.89	154.89	
6.068	6.068	(0.753)	84	388707			2.49- 62.49	32.49	

62 Methyl Acrylate					CAS #: 96-33-3				
7.810	7.810	(0.969)	55	2465050	50.0000	59.565	80.00- 120.00	100.00	
7.810	7.810	(0.969)	85	288166			0.00- 41.69	11.69	
7.810	7.810	(0.969)	58	209426			0.00- 38.50	8.50	

86 2-Pentanone					CAS #: 107-87-9				
10.796	10.796	(1.086)	43	3588242	50.0000	59.645	80.00- 120.00	100.00	
10.796	10.796	(1.086)	58	248284			0.00- 36.92	6.92	
10.796	10.796	(1.086)	86	450773			0.00- 42.56	12.56	

88 Ethyl Acrylate					CAS #: 140-88-5				
10.630	10.630	(1.070)	55	2733225	50.0000	58.934	80.00- 120.00	100.00	
10.630	10.630	(1.070)	99	141739			0.00- 35.19	5.19	
10.630	10.630	(1.070)	45	270556			0.00- 39.90	9.90	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

95 Dibromomethane						CAS #: 74-95-3			
11.073	11.073	(1.114)	174	857804	50.0000	56.889	80.00- 120.00	100.00	
11.073	11.073	(1.114)	93	941910			79.80- 139.80	109.80	
11.073	11.073	(1.114)	95	789916			62.09- 122.09	92.09	

96 Methyl Methacrylate						CAS #: 80-62-6			
11.073	11.073	(1.114)	41	1912198	50.0000	59.195	80.00- 120.00	100.00	
11.073	11.073	(1.114)	69	901405			17.14- 77.14	47.14	
11.073	11.073	(1.114)	100	360526			0.00- 48.85	18.85	

112 Alphamethylstyrene						CAS #: 98-83-9			
17.294	17.294	(1.153)	118	1662649	50.0000	60.907	80.00- 120.00	100.00	
17.294	17.294	(1.153)	103	969695			28.32- 88.32	58.32	

117 Bis(2-chloroethyl) ether						CAS #: 111-44-4			
17.709	17.709	(1.181)	93	1748274	50.0000	54.264	80.00- 120.00	100.00	
17.709	17.709	(1.181)	95	550087			1.46- 61.46	31.46	
17.709	17.709	(1.181)	63	1420888			51.27- 111.27	81.27	

127 Nonane						CAS #: 111-84-2			
15.331	15.331	(1.022)	43	3205620	50.0000	60.466	80.00- 120.00	100.00	
15.331	15.331	(1.022)	57	2399225			44.84- 104.84	74.84	
15.331	15.331	(1.022)	85	723428			0.00- 52.57	22.57	

QC Flag Legend

T - Target compound detected outside RT window.

Report Date: 27-Nov-2007 15:31

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 27-NOV-2007

Lab File ID: 5112702.d

Calibration Time: 09:21

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-27nov.b/t14qn12c.m

Misc Info: 50ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	351932	211159	492705	351932	0.00
92 1,4-Difluorobenze	1207474	724484	1690464	1207474	0.00
125 Chlorobenzene-d5	945809	567485	1324133	945809	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.94	9.61	10.27	9.94	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-27nov.b/5112702.d

Date: 27-NOV-2007 09:21

Client ID: Level 5

Sample Info: 50mL #1443-374


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-27nov.b/5112702.d

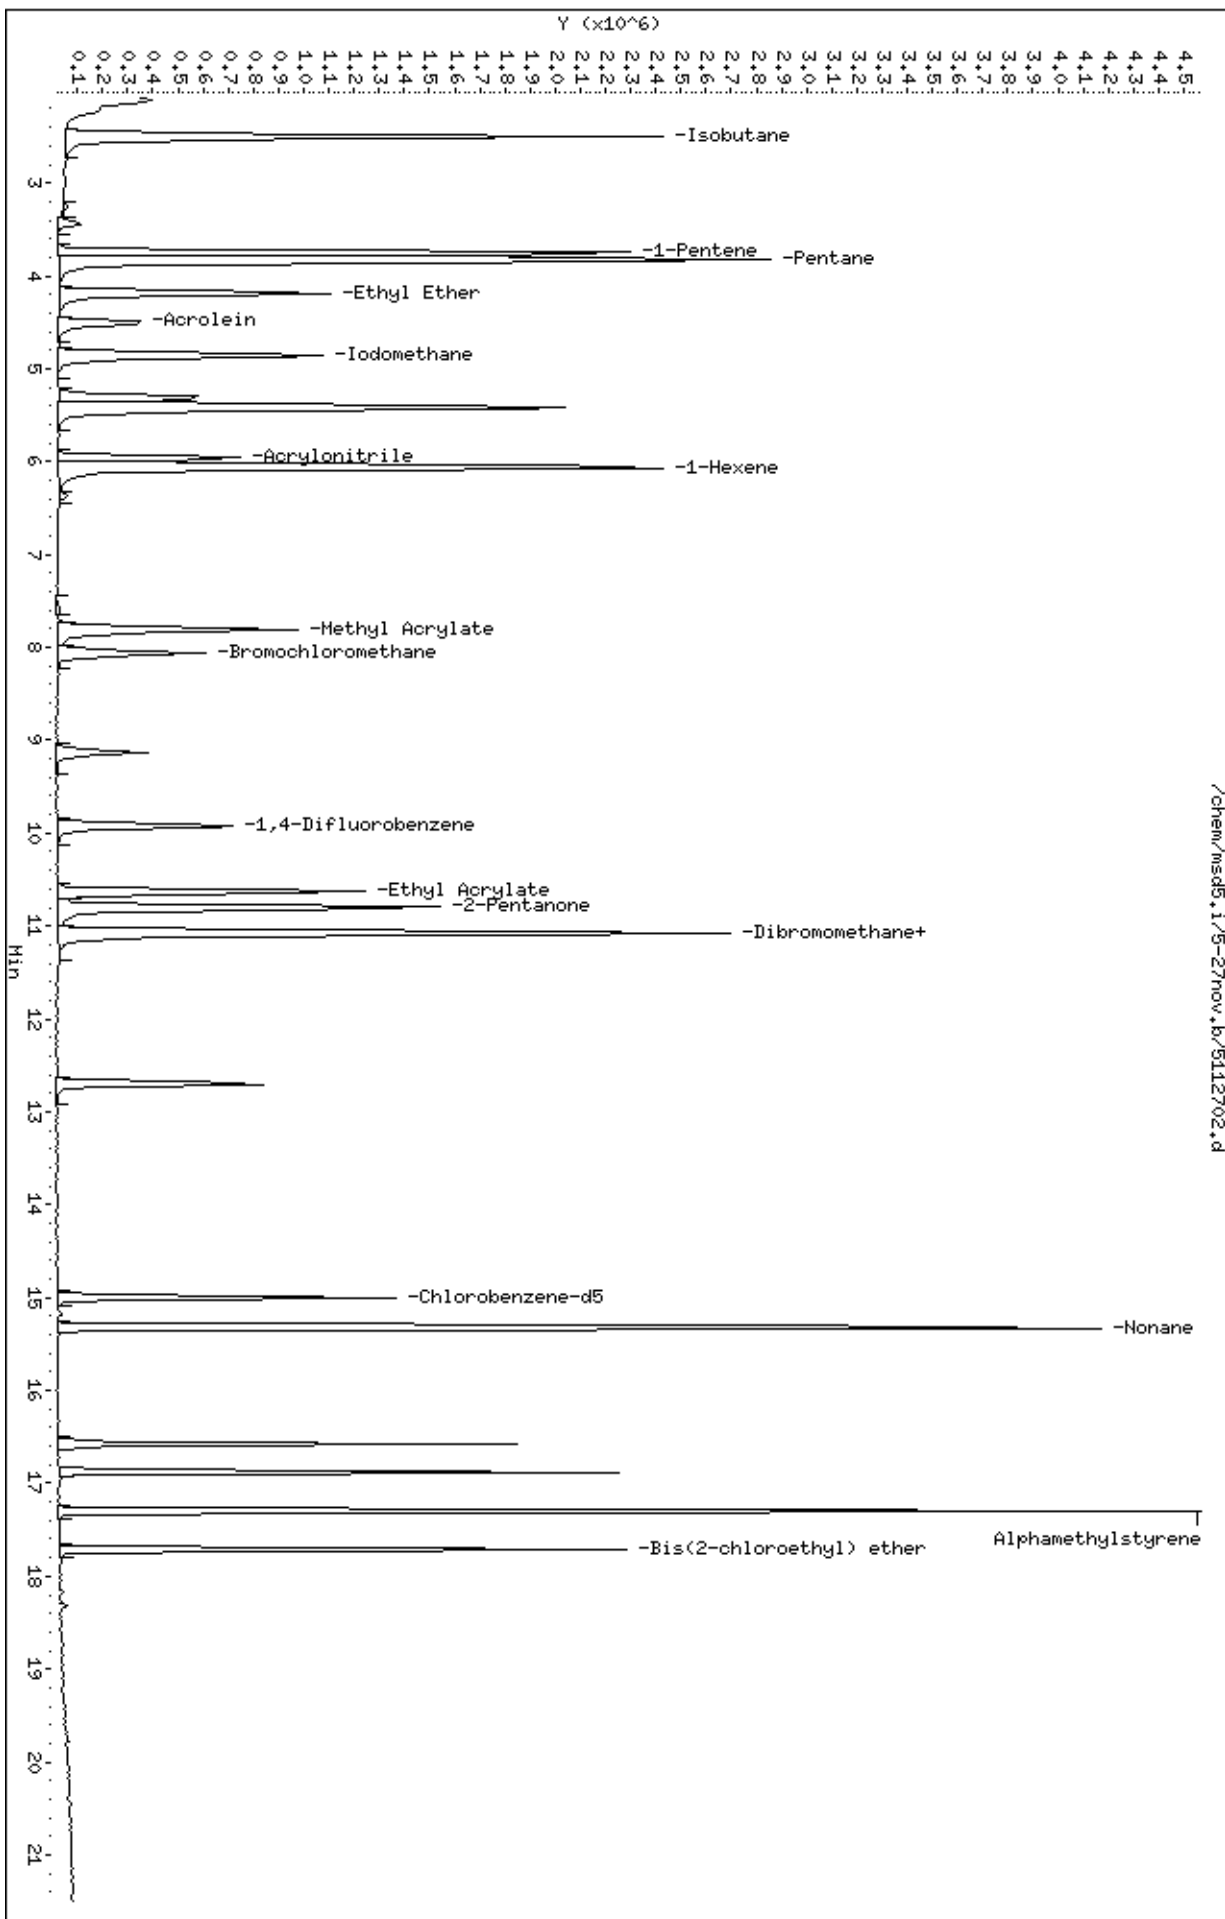

Report Date: 20-Nov-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-19nov.b/5111903.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 19-NOV-2007 02:24
 Operator : sjr Inst ID: msd5.i
 Smp Info : 50mL #1487-405
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msd5.i/5-19nov.b/t14qn12b.m
 Meth Date : 20-Nov-2007 15:39 ctaylor Quant Type: ISTD
 Cal Date : 19-NOV-2007 02:24 Cal File: 5111903.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp21b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	320182	25.0000			80.00- 120.00	100.00
8.059	8.059	(1.000)	128	247757				47.38- 107.38	77.38
8.059	8.059	(1.000)	49	727629				197.25- 257.25	227.25

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.911	(1.000)	114	1222930	25.0000			80.00- 120.00	100.00
9.911	9.911	(1.000)	88	214130				0.00- 47.51	17.51

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	969063	25.0000			80.00- 120.00	100.00
14.999	14.999	(1.000)	82	569146				28.73- 88.73	58.73

1 Freon134a CAS #: 811-97-2									
2.197	2.197	(0.273)	83	725525	50.0000	54.536		80.00- 120.00	100.00
2.335	2.335	(0.290)	69	86258				0.00- 41.89	11.89

3 Freon 152a CAS #: 75-37-6									
2.280	2.280	(0.283)	65	672942	50.0000	58.047		80.00- 120.00	100.00
2.335	2.335	(0.290)	51	3505165				490.87- 550.87	520.87

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

4 Freon 22						CAS #: 75-45-6			
2.335	2.335	(0.290)	67	186741	50.0000	49.706	80.00- 120.00	100.00	
2.335	2.335	(0.290)	51	3481504			1834.35-1894.35	1864.35	

5 Freon142b						CAS #: 75-68-3			
2.557	2.557	(0.317)	65	1425792	50.0000	63.457	80.00- 120.00	100.00	
2.529	2.529	(0.314)	45	439299			0.81- 60.81	30.81	

16 Dichlorofluoromethane/Fr21						CAS #: 75-43-4			
3.718	3.718	(0.461)	67	1566047	50.0000	55.419	80.00- 120.00	100.00	
3.718	3.718	(0.461)	69	474287			0.29- 60.29	30.29	
3.773	3.773	(0.468)	35	4459			0.00- 30.28	0.28	

22 Freon123a						CAS #: 354-23-4			
4.271	4.271	(0.530)	117	802431	50.0000	51.785	80.00- 120.00	100.00	
4.271	4.271	(0.530)	67	1266245			127.80- 187.80	157.80	

24 Freon123						CAS #: 306-83-2			
4.409	4.409	(0.547)	83	1635430	50.0000	56.515	80.00- 120.00	100.00	
4.409	4.409	(0.547)	133	249822			0.00- 45.28	15.28	
4.409	4.409	(0.547)	85	1130542			39.13- 99.13	69.13	

37 tert-Butyl-Alcohol						CAS #: 75-65-0			
5.570	5.570	(0.691)	59	871998	50.0000	44.645	80.00- 120.00	100.00	
5.570	5.570	(0.691)	41	287836			3.01- 63.01	33.01	
5.570	5.570	(0.691)	57	89186			0.00- 40.23	10.23	

49 Isopropyl ether						CAS #: 108-20-3			
6.593	6.593	(0.818)	45	4403085	50.0000	58.244	80.00- 120.00	100.00	
6.593	6.593	(0.818)	87	831467			0.00- 48.88	18.88	
6.593	6.593	(0.818)	59	440147			0.00- 40.00	10.00	

57 Ethyl-tert-butyl Ether						CAS #: 637-92-3			
7.202	7.202	(0.894)	59	1932300	50.0000	62.956	80.00- 120.00	100.00	
7.202	7.202	(0.894)	87	624017			2.29- 62.29	32.29	
7.202	7.202	(0.894)	41	425510			0.00- 52.02	22.02	

61 Ethyl Acetate						CAS #: 141-78-6			
7.699	7.699	(0.955)	70	203725	50.0000	59.358	80.00- 120.00	100.00	
7.699	7.699	(0.955)	43	2599138			1245.81-1305.81	1275.81	
7.699	7.699	(0.955)	61	314227			124.24- 184.24	154.24	

64 1-Propanol						CAS #: 71-23-8			
6.815	6.815	(0.846)	42	196110	50.0000	70.686	80.00- 120.00	100.00	
6.815	6.815	(0.846)	59	196448			70.17- 130.17	100.17	
6.815	6.815	(0.846)	41	119724			31.05- 91.05	61.05	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

76 Isobutanol						CAS #: 78-83-1			
9.082	9.082	(0.916)	43	957047	50.0000	59.454	80.00- 120.00	100.00	
9.082	9.082	(0.916)	41	676060			40.64- 100.64	70.64	

78 tert-amyl-Methyl Ether						CAS #: 994-05-8			
9.275	9.275	(1.151)	73	1541577	50.0000	60.655	80.00- 120.00	100.00	
9.275	9.275	(1.151)	87	383472			0.00- 54.88	24.88	
9.275	9.275	(1.151)	55	715772			16.43- 76.43	46.43	

118 Butyl Acetate						CAS #: 123-86-4			
14.197	14.197	(1.432)	56	1080669	50.0000	63.411	80.00- 120.00	100.00	
14.197	14.197	(1.432)	73	298763			0.00- 57.65	27.65	
14.197	14.197	(1.432)	43	2701863			220.02- 280.02	250.02	

131 2-Heptanone						CAS #: 110-43-0			
16.077	16.077	(1.072)	58	1533405	50.0000	60.264	80.00- 120.00	100.00	
16.077	16.077	(1.072)	43	2665724			143.84- 203.84	173.84	

135 Cyclohexanone						CAS #: 108-94-1			
16.520	16.520	(1.101)	55	1376890	50.0000	57.101	80.00- 120.00	100.00	
16.520	16.520	(1.101)	98	447407			2.49- 62.49	32.49	
16.520	16.520	(1.101)	42	988900			41.82- 101.82	71.82	

146 Diisobutyl Ketone						CAS #: 108-83-8			
17.211	17.211	(1.147)	57	3684582	50.0000	56.291	80.00- 120.00	100.00	
17.211	17.211	(1.147)	85	2242699			30.87- 90.87	60.87	

Report Date: 20-Nov-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 19-NOV-2007

Lab File ID: 5111903.d

Calibration Time: 02:24

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd5.i/5-19nov.b/t14qn12b.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	320182	192109	448255	320182	0.00
92 1,4-Difluorobenze	1222930	733758	1712102	1222930	0.00
125 Chlorobenzene-d5	969063	581438	1356688	969063	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-19nov.b/5111903.d

Date: 19-NOV-2007 02:24

Client ID: Level 5

Sample Info: 50mL #1487-405


Column phase: RTX-624

Instrument: msd5.1

Operator: sjr

Column diameter: 0.53

/chem/msd5.1/5-19nov.b/5111903.d



Report Date: 13-Nov-2007 13:25

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111217.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 12-NOV-2007 19:48
 Operator : cb Inst ID: msd5.i
 Smp Info : 50mL #1487-404
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:25 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 19:48 Cal File: 5111217.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp20a.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

* 71	Bromochloromethane						CAS #:	74-97-5	
8.059	8.059	(1.000)	130	345466	25.0000			80.00- 120.00	100.00
8.059	8.059	(1.000)	128	268730				47.79- 107.79	77.79
8.031	8.031	(1.000)	49	746996				186.23- 246.23	216.23

* 92	1,4-Difluorobenzene						CAS #:	540-36-3	
9.912	9.912	(1.000)	114	1312181	25.0000			80.00- 120.00	100.00
9.912	9.912	(1.000)	88	210064				0.00- 46.01	16.01

* 125	Chlorobenzene-d5						CAS #:	3114-55-4	
14.999	14.999	(1.000)	117	1008754	25.0000			80.00- 120.00	100.00
14.999	14.999	(1.000)	82	607985				30.27- 90.27	60.27

33	Methyl Acetate						CAS #:	79-20-9	
5.211	5.211	(0.647)	43	3002789	50.0000	58.786		80.00- 120.00	100.00
5.211	5.211	(0.647)	74	493386				0.00- 46.43	16.43
5.211	5.211	(0.647)	59	206971				0.00- 36.89	6.89

52	Chloroprene						CAS #:	126-99-8	
6.677	6.677	(0.828)	53	2405354	50.0000	58.823		80.00- 120.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
52 Chloroprene (continued)									
6.677	6.677	(0.828)	88	1024721			12.60- 72.60	42.60	
6.677	6.677	(0.828)	50	551998			0.00- 52.95	22.95	

59 1,3-Dichloropropane					CAS #: 142-28-9				
13.893	13.893	(1.402)	76	1453809	50.0000	58.082	80.00- 120.00	100.00	
13.893	13.893	(1.402)	41	1436383			68.80- 128.80	98.80	
13.893	13.893	(1.402)	78	465938			2.05- 62.05	32.05	

60 2,2-Dichloropropane					CAS #: 594-20-7				
7.561	7.561	(0.938)	77	1380807	50.0000	57.766	80.00- 120.00	100.00	
7.561	7.561	(0.938)	79	453796			2.86- 62.86	32.86	
7.561	7.561	(0.938)	97	311903			0.00- 52.59	22.59	

73 1,1-Dichloropropene					CAS #: 563-58-6				
8.723	8.723	(1.082)	110	527576	50.0000	57.969	80.00- 120.00	100.00	
8.723	8.723	(1.082)	75	1429533			240.96- 300.96	270.96	

123 1,1,1,2-Tetrachloroethane					CAS #: 630-20-6				
15.193	15.193	(1.013)	131	1054297	50.0000	58.469	80.00- 120.00	100.00	
15.193	15.193	(1.013)	117	721225			38.41- 98.41	68.41	
15.165	15.165	(1.011)	95	427459			10.54- 70.54	40.54	

137 Bromobenzene					CAS #: 108-86-1				
16.741	16.741	(1.116)	156	1300604	50.0000	58.297	80.00- 120.00	100.00	
16.741	16.741	(1.116)	77	2361550			151.57- 211.57	181.57	
16.741	16.741	(1.116)	158	1239903			65.33- 125.33	95.33	

139 1,2,3-Trichloropropane					CAS #: 96-18-4				
16.852	16.852	(1.123)	110	696512	50.0000	56.901	80.00- 120.00	100.00	
16.852	16.852	(1.123)	61	577248			52.88- 112.88	82.88	
16.852	16.852	(1.123)	112	428340			31.50- 91.50	61.50	

140 2-Chlorotoluene					CAS #: 95-49-8				
16.962	16.962	(1.131)	126	1106391	50.0000	59.165	80.00- 120.00	100.00	
16.962	16.962	(1.131)	91	3514345			287.64- 347.64	317.64	
16.962	16.962	(1.131)	65	354394			2.03- 62.03	32.03	

143 4-Chlorotoluene					CAS #: 106-43-4				
17.100	17.100	(1.140)	126	1096512	50.0000	57.144	80.00- 120.00	100.00	
17.100	17.100	(1.140)	91	3485044			287.83- 347.83	317.83	
17.100	17.100	(1.140)	63	442755			10.38- 70.38	40.38	

149 tert-Butylbenzene					CAS #: 98-06-6				
17.377	17.377	(1.159)	119	4280060	50.0000	55.137	80.00- 120.00	100.00	
17.377	17.377	(1.159)	134	1013841			0.00- 53.69	23.69	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
149 tert-Butylbenzene (continued)									
17.377	17.377	(1.159)	91	2758688			34.45- 94.45	64.45	

150 Pentachloroethane CAS #: 76-01-7									
17.460	17.460	(1.164)	167	794680	50.0000	58.289	80.00- 120.00	100.00	
17.432	17.432	(1.162)	117	894688			82.58- 142.58	112.58	

151 sec-Butylbenzene CAS #: 135-98-8									
17.598	17.598	(1.173)	105	5449977	50.0000	59.146	80.00- 120.00	100.00	
17.598	17.598	(1.173)	134	1039049			0.00- 49.07	19.07	
17.598	17.598	(1.173)	91	915072			0.00- 46.79	16.79	

153 p-Cymene CAS #: 99-87-6									
17.764	17.764	(1.184)	134	1136321	50.0000	56.976	80.00- 120.00	100.00	
17.764	17.764	(1.184)	119	4217404			341.15- 401.15	371.15	
17.764	17.764	(1.184)	91	1020158			59.78- 119.78	89.78	

154 1,2,3-Trimethylbenzene CAS #: 526-73-8									
17.875	17.875	(1.192)	120	1673326	50.0000	58.418	80.00- 120.00	100.00	
17.875	17.875	(1.192)	105	3804482			197.36- 257.36	227.36	
17.875	17.875	(1.192)	77	419654			0.00- 55.08	25.08	

158 Butylbenzene CAS #: 104-51-8									
18.151	18.151	(1.210)	134	1017669	50.0000	56.589	80.00- 120.00	100.00	
18.123	18.123	(1.208)	91	4313119			393.82- 453.82	423.82	
18.123	18.123	(1.208)	92	2356714			201.58- 261.58	231.58	

160 Hexachloroethane CAS #: 67-72-1									
18.372	18.372	(1.225)	117	1526467	50.0000	57.384	80.00- 120.00	100.00	
18.400	18.400	(1.227)	201	960023			32.89- 92.89	62.89	
Sum of Peak Amounts =					57.4				

161 1,2-Dibromo-3-Chloropropane CAS #: 96-12-8									
18.870	18.870	(1.258)	157	1023062	50.0000	55.695	80.00- 120.00	100.00	
18.870	18.870	(1.258)	75	1253152			92.49- 152.49	122.49	
18.870	18.870	(1.258)	155	805144			48.70- 108.70	78.70	

166 1,2,3-Trichlorobenzene CAS #: 87-61-6									
19.865	19.865	(1.324)	180	2109836	50.0000	53.002	80.00- 120.00	100.00	
19.865	19.865	(1.324)	182	1992366			64.43- 124.43	94.43	
19.865	19.865	(1.324)	145	683997			2.42- 62.42	32.42	

192 Cyclopentene CAS #: 142-29-0									
5.239	5.239	(0.650)	67	2884987	50.0000	57.822	80.00- 120.00	100.00	
5.239	5.239	(0.650)	68	1097704			8.05- 68.05	38.05	
5.239	5.239	(0.650)	53	689669			0.00- 53.91	23.91	

Report Date: 13-Nov-2007 13:25

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111217.d

Calibration Time: 19:48

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	345466	207280	483652	345466	0.00
92 1,4-Difluorobenze	1312181	787309	1837053	1312181	0.00
125 Chlorobenzene-d5	1008754	605252	1412256	1008754	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111217.d

Date: 12-NOV-2007 19:48

Client ID: Level 5

Sample Info: 50mL #1487-404


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-12nov.b/5111217.d



Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111211.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 12-NOV-2007 15:12
 Operator : cb Inst ID: msd5.i
 Smp Info : 50mL #1576-89
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 15:12 Cal File: 5111211.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	355243	25.0000		80.00- 120.00	100.00	
8.059	8.059	(1.000)	128	258473			42.76- 102.76	72.76	
8.059	8.059	(1.000)	49	721775			173.18- 233.18	203.18	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.911	(1.000)	114	1306915	25.0000		80.00- 120.00	100.00	
9.911	9.911	(1.000)	88	214533			0.00- 46.42	16.42	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	1023463	25.0000		80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	610449			29.65- 89.65	59.65	

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.110	9.110	(1.130)	65	493461	25.0000	23.207	80.00- 120.00	100.00	
9.110	9.110	(1.130)	67	285594			27.88- 87.88	57.88	

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	1175775	25.0000	25.482	80.00- 120.00	100.00	
12.676	12.676	(1.279)	70	120943			0.00- 40.29	10.29	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	797977			37.87- 97.87	67.87		

\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.575	16.575	(1.105)	174	601379	25.0000	25.183	80.00- 120.00	100.00		
16.575	16.575	(1.105)	95	954444			128.71- 188.71	158.71		
16.575	16.575	(1.105)	176	590897			68.26- 128.26	98.26		

6 Propylene										
						CAS #:	115-07-1			
2.280	2.280	(0.283)	41	1312675	50.0000	52.940	80.00- 120.00	100.00		
2.280	2.280	(0.283)	42	859227			35.46- 95.46	65.46		
2.280	2.280	(0.283)	39	905799			39.00- 99.00	69.00		

8 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.336	2.336	(0.290)	85	2175989	50.0000	51.803	80.00- 120.00	100.00		
2.336	2.336	(0.290)	87	699568			2.15- 62.15	32.15		

9 Freon 114										
						CAS #:	76-14-2			
2.474	2.474	(0.307)	135	2044251	50.0000	53.326	80.00- 120.00	100.00		
2.474	2.474	(0.307)	137	660064			2.29- 62.29	32.29		

10 Chloromethane										
						CAS #:	74-87-3			
2.584	2.584	(0.321)	50	1669546	50.0000	52.932	80.00- 120.00	100.00		
2.584	2.584	(0.321)	52	492673			0.00- 59.51	29.51		

13 Vinyl Chloride										
						CAS #:	75-01-4			
2.778	2.778	(0.345)	62	1641494	50.0000	54.070	80.00- 120.00	100.00		
2.778	2.778	(0.345)	64	510794			1.12- 61.12	31.12		

12 1,3-Butadiene										
						CAS #:	106-99-0			
2.750	2.750	(0.341)	54	1448503	50.0000	55.867	80.00- 120.00	100.00		
2.750	2.750	(0.341)	39	1594739			80.10- 140.10	110.10		

15 Bromomethane										
						CAS #:	74-83-9			
3.276	3.276	(0.406)	94	1074369	50.0000	54.816	80.00- 120.00	100.00		
3.276	3.276	(0.406)	96	1021436			65.07- 125.07	95.07		

19 Chloroethane										
						CAS #:	75-00-3			
3.386	3.386	(0.420)	64	777558	50.0000	50.352	80.00- 120.00	100.00		
3.386	3.386	(0.420)	49	221791			0.00- 58.52	28.52		
3.386	3.386	(0.420)	66	235947			0.34- 60.34	30.34		

20 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.718	3.718	(0.461)	101	2486676	50.0000	54.298	80.00- 120.00	100.00		
3.718	3.718	(0.461)	103	1605442			34.56- 94.56	64.56		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
26 Ethanol						CAS #: 64-17-5			
4.077	4.077	(0.506)	45	545546	50.0000	54.833	80.00- 120.00	100.00	
4.077	4.077	(0.506)	43	108744			0.00- 49.93	19.93	
4.077	4.077	(0.506)	46	228599			11.90- 71.90	41.90	

30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	1493574	50.0000	52.450	80.00- 120.00	100.00	
4.520	4.520	(0.561)	153	947418			33.43- 93.43	63.43	
4.520	4.520	(0.561)	101	2068318			108.48- 168.48	138.48	

31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	2031999	50.0000	53.917	80.00- 120.00	100.00	
4.575	4.575	(0.568)	96	1160823			27.13- 87.13	57.13	
4.575	4.575	(0.568)	98	723443			5.60- 65.60	35.60	

32 Acetone						CAS #: 67-64-1			
4.713	4.713	(0.585)	58	772213	50.0000	54.781	80.00- 120.00	100.00	
4.713	4.713	(0.585)	43	2262129			262.94- 322.94	292.94	

36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	2701635	50.0000	53.853	80.00- 120.00	100.00	
4.907	4.907	(0.609)	43	607237			0.00- 52.48	22.48	
4.907	4.907	(0.609)	59	97529			0.00- 33.61	3.61	

35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	3530562	50.0000	55.319	80.00- 120.00	100.00	

38 3-Chloropropene						CAS #: 107-05-1			
5.183	5.183	(0.643)	76	580717	50.0000	54.648	80.00- 120.00	100.00	
5.183	5.183	(0.643)	41	2113664			333.97- 393.97	363.97	

43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	1689054	50.0000	52.414	80.00- 120.00	100.00	
5.432	5.432	(0.674)	84	1010161			29.81- 89.81	59.81	
5.432	5.432	(0.674)	51	516265			0.57- 60.57	30.57	

46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	1217142	50.0000	50.174	80.00- 120.00	100.00	
5.764	5.764	(0.715)	57	385552			1.68- 61.68	31.68	
5.764	5.764	(0.715)	41	417118			4.27- 64.27	34.27	

47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	1256929	50.0000	55.069	80.00- 120.00	100.00	
5.819	5.819	(0.722)	61	2056986			133.65- 193.65	163.65	
5.819	5.819	(0.722)	98	806007			34.13- 94.13	64.13	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	2567435	50.0000	55.316	80.00- 120.00	100.00	
6.151	6.151	(0.763)	43	1763419			38.68- 98.68	68.68	
6.151	6.151	(0.763)	86	368536			0.00- 44.35	14.35	

55 1,1-Dichloroethane						CAS #: 75-34-3			
6.594	6.594	(0.818)	63	2257850	50.0000	54.634	80.00- 120.00	100.00	
6.594	6.594	(0.818)	65	689178			0.52- 60.52	30.52	

67 2-Butanone						CAS #: 78-93-3			
7.672	7.672	(0.952)	72	558891	50.0000	56.036	80.00- 120.00	100.00	
7.644	7.644	(0.949)	43	3165141			536.33- 596.33	566.33	
7.644	7.644	(0.949)	57	216333			8.71- 68.71	38.71	

66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	1659102	50.0000	53.468	80.00- 120.00	100.00	
7.617	7.617	(0.945)	96	1120921			37.56- 97.56	67.56	
7.617	7.617	(0.945)	98	738627			14.52- 74.52	44.52	

70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	1896605	50.0000	51.073	80.00- 120.00	100.00	
8.031	8.031	(0.997)	71	488200			0.00- 55.74	25.74	
8.031	8.031	(0.997)	72	523776			0.00- 57.62	27.62	

72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	1918915	50.0000	54.803	80.00- 120.00	100.00	
8.197	8.197	(1.017)	85	1250945			35.19- 95.19	65.19	

75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.418	8.418	(1.045)	97	1907795	50.0000	54.509	80.00- 120.00	100.00	
8.418	8.418	(1.045)	99	1202373			33.02- 93.02	63.02	

74 Cyclohexane						CAS #: 110-82-7			
8.418	8.418	(1.045)	84	1555633	50.0000	55.173	80.00- 120.00	100.00	
8.391	8.391	(1.041)	56	2428435			126.11- 186.11	156.11	
8.391	8.391	(1.041)	41	1335097			55.82- 115.82	85.82	

56 Vinyl Acetate						CAS #: 108-05-4			
6.649	6.649	(0.825)	86	286552	50.0000	54.732	80.00- 120.00	100.00	
6.649	6.649	(0.825)	43	3665493			1249.17-1309.17	1279.17	
6.649	6.649	(0.825)	42	271666			64.81- 124.81	94.81	

77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	1598598	50.0000	55.319	80.00- 120.00	100.00	
8.667	8.667	(1.075)	117	1694265			75.98- 135.98	105.98	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

80	2,2,4-Trimethylpentane				CAS #: 540-84-1				
9.110	9.110	(1.130)	57	7055970	50.0000	55.441	80.00-	120.00	100.00
9.110	9.110	(1.130)	56	2339543			3.16-	63.16	33.16
9.110	9.110	(1.130)	41	1821506			0.00-	55.82	25.82

81	Benzene				CAS #: 71-43-2				
9.082	9.082	(0.916)	78	3180389	50.0000	56.459	80.00-	120.00	100.00
9.082	9.082	(0.916)	77	713793			0.00-	52.44	22.44

85	1,2-Dichloroethane				CAS #: 107-06-2				
9.275	9.275	(0.936)	62	1424249	50.0000	55.189	80.00-	120.00	100.00
9.275	9.275	(0.936)	64	475387			3.38-	63.38	33.38

90	Heptane				CAS #: 142-82-5				
9.469	9.469	(0.955)	100	372161	50.0000	59.150	80.00-	120.00	100.00
9.469	9.469	(0.955)	43	2908022			751.39-	811.39	781.39
9.469	9.469	(0.955)	71	1125638			272.46-	332.46	302.46

93	Trichloroethene				CAS #: 79-01-6				
10.326	10.326	(1.042)	95	1232331	50.0000	53.936	80.00-	120.00	100.00
10.326	10.326	(1.042)	130	1164486			64.49-	124.49	94.49
10.326	10.326	(1.042)	97	797550			34.72-	94.72	64.72

98	1,2-Dichloropropane				CAS #: 78-87-5				
10.852	10.852	(1.095)	63	1211107	50.0000	54.671	80.00-	120.00	100.00
10.824	10.824	(1.092)	62	836213			39.05-	99.05	69.05
10.824	10.824	(1.092)	41	807190			36.65-	96.65	66.65

99	1,4-Dioxane				CAS #: 123-91-1				
11.073	11.073	(1.117)	88	708188	50.0000	55.044	80.00-	120.00	100.00
11.073	11.073	(1.117)	58	651545			62.00-	122.00	92.00
11.073	11.073	(1.117)	57	203324			0.00-	58.71	28.71

100	Bromodichloromethane				CAS #: 75-27-4				
11.405	11.405	(1.151)	83	1775227	50.0000	55.572	80.00-	120.00	100.00
11.405	11.405	(1.151)	85	1148990			34.72-	94.72	64.72

103	cis-1,3-Dichloropropene				CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	1313299	50.0000	58.006	80.00-	120.00	100.00
12.317	12.317	(1.243)	77	397718			0.28-	60.28	30.28
12.317	12.317	(1.243)	39	962609			43.30-	103.30	73.30

106	4-Methyl-2-pentanone				CAS #: 108-10-1				
12.593	12.593	(1.271)	58	1089972	50.0000	59.062	80.00-	120.00	100.00
12.593	12.593	(1.271)	43	3042244			249.11-	309.11	279.11
12.593	12.593	(1.271)	85	356294			2.69-	62.69	32.69

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	3149555	50.0000	54.198	80.00- 120.00	100.00	
12.815	12.815	(1.293)	92	1878571			29.65- 89.65	59.65	

113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	1282039	50.0000	59.291	80.00- 120.00	100.00	
13.368	13.368	(0.891)	77	409698			1.96- 61.96	31.96	
13.368	13.368	(0.891)	39	882256			38.82- 98.82	68.82	

114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	1060223	50.0000	54.967	80.00- 120.00	100.00	
13.644	13.644	(0.910)	99	674672			33.63- 93.63	63.63	
13.644	13.644	(0.910)	83	908942			55.73- 115.73	85.73	

116 Tetrachloroethene						CAS #: 127-18-4			
13.699	13.699	(0.913)	166	1227356	50.0000	54.744	80.00- 120.00	100.00	
13.699	13.699	(0.913)	129	984805			50.24- 110.24	80.24	
13.699	13.699	(0.913)	131	962472			48.42- 108.42	78.42	

119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	1509153	50.0000	56.088	80.00- 120.00	100.00	
14.004	14.004	(0.934)	43	2997890			168.65- 228.65	198.65	
14.031	14.031	(0.935)	100	225645			0.00- 44.95	14.95	

120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	1545103	50.0000	57.250	80.00- 120.00	100.00	
14.197	14.197	(0.947)	127	1216596			48.74- 108.74	78.74	

122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	1614283	50.0000	57.095	80.00- 120.00	100.00	
14.363	14.363	(0.958)	109	1513177			63.74- 123.74	93.74	

126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	2422375	50.0000	55.002	80.00- 120.00	100.00	
15.027	15.027	(1.002)	114	770695			1.82- 61.82	31.82	
15.027	15.027	(1.002)	77	1496728			31.79- 91.79	61.79	

128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	1368971	50.0000	57.535	80.00- 120.00	100.00	
15.165	15.165	(1.011)	91	4502915			298.93- 358.93	328.93	

130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	1683589	50.0000	57.610	80.00- 120.00	100.00	
15.331	15.331	(1.022)	91	3631728			185.71- 245.71	215.71	

132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	1561970	50.0000	56.206	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	3522055			195.49- 255.49	225.49	

133 Styrene CAS #: 100-42-5									
15.911	15.911	(1.061)	104	2483828	50.0000	60.620	80.00- 120.00	100.00	
15.911	15.911	(1.061)	78	1301372			22.39- 82.39	52.39	

134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1400605	50.0000	58.234	80.00- 120.00	100.00	
16.160	16.160	(1.077)	171	717301			21.21- 81.21	51.21	

141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	2360572	50.0000	56.324	80.00- 120.00	100.00	
16.796	16.796	(1.120)	85	1502138			33.63- 93.63	63.63	

144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	4900605	50.0000	59.766	80.00- 120.00	100.00	
16.962	16.962	(1.131)	120	1443784			0.00- 59.46	29.46	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	4416287	50.0000	59.587	80.00- 120.00	100.00	
17.045	17.045	(1.136)	120	2089426			17.31- 77.31	47.31	

152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	3716466	50.0000	59.111	80.00- 120.00	100.00	
17.460	17.460	(1.164)	120	1713727			16.11- 76.11	46.11	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	2443521	50.0000	54.898	80.00- 120.00	100.00	
17.764	17.764	(1.184)	148	1563539			33.99- 93.99	63.99	
17.764	17.764	(1.184)	111	1008640			11.28- 71.28	41.28	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	2963344	50.0000	56.806	80.00- 120.00	100.00	
17.847	17.847	(1.190)	148	1875291			33.28- 93.28	63.28	
17.847	17.847	(1.190)	111	1248063			12.12- 72.12	42.12	

157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	4486516	50.0000	68.302	80.00- 120.00	100.00	
17.985	17.985	(1.199)	126	846690			0.00- 48.87	18.87	

159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	2492645	50.0000	53.244	80.00- 120.00	100.00	
18.206	18.206	(1.214)	148	1561440			32.64- 92.64	62.64	
18.206	18.206	(1.214)	111	1035282			11.53- 71.53	41.53	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.506	19.506	(1.300)	180	1744262	50.0000	52.490	80.00- 120.00	100.00	
19.506	19.506	(1.300)	182	1638315			63.93- 123.93	93.93	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.589	19.589	(1.306)	225	1242599	50.0000	53.225	80.00- 120.00	100.00	
19.589	19.589	(1.306)	223	778986			32.69- 92.69	62.69	

142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	5828519	50.0000	60.396	80.00- 120.00	100.00	
16.824	16.824	(1.122)	120	1254651			0.00- 51.53	21.53	
16.824	16.824	(1.122)	105	202539			0.00- 33.47	3.47	

136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	4756734	50.0000	56.452	80.00- 120.00	100.00	
16.326	16.326	(1.088)	120	1291385			0.00- 57.15	27.15	
16.326	16.326	(1.088)	51	661182			0.00- 43.90	13.90	

165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	6436561	50.0000	58.157	80.00- 120.00	100.00	
19.672	19.672	(1.312)	127	794729			0.00- 42.35	12.35	

17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	2293671	50.0000	52.156	80.00- 120.00	100.00	
3.414	3.414	(0.424)	57	1474529			34.29- 94.29	64.29	
3.414	3.414	(0.424)	72	150731			0.00- 36.57	6.57	

11	Butane					CAS #: 106-97-8			
2.667	2.667	(0.331)	58	391826	50.0000	52.258	80.00- 120.00	100.00	
2.667	2.667	(0.331)	43	2841502			695.19- 755.19	725.19	

94	Methyl Cyclohexane					CAS #: 108-87-2			
10.547	10.547	(1.064)	83	1820696	50.0000	55.960	80.00- 120.00	100.00	
10.547	10.547	(1.064)	98	909326			19.94- 79.94	49.94	
10.547	10.547	(1.064)	55	1974573			78.45- 138.45	108.45	

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111211.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	355243	0.00
92 1,4-Difluorobenze	1306915	784149	1829681	1306915	0.00
125 Chlorobenzene-d5	1023463	614078	1432848	1023463	0.00


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111212.d
 Lab Smp Id: ICAL Client Smp ID: Level 6
 Inj Date : 12-NOV-2007 15:41
 Operator : cb Inst ID: msd5.i
 Smp Info : 100mL #1576-89
 Misc Info : 200ppbv -> 100ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 15:41 Cal File: 5111212.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	362309	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	281606				42.76- 102.76	77.73
8.059	8.059	(1.000)	49	764495				173.18- 233.18	211.01

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.911	9.911	(1.000)	114	1394945	25.0000			70.00- 130.00	100.00
9.911	9.911	(1.000)	88	227570				0.00- 46.42	16.31

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	1101731	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	629454				0.00- 30.00	57.13

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.137	9.137	(1.134)	65	556149	25.0000	25.645		70.00- 130.00	100.00
9.110	9.110	(1.130)	67	330557				0.00- 30.00	59.44

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	1217578	25.0000	24.723		70.00- 130.00	100.00
12.704	12.704	(1.282)	70	125916				0.00- 30.00	10.34

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	850099			0.00- 30.00	69.82		

\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.575	16.575	(1.105)	174	629857	25.0000	24.502	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	1021545			128.71- 188.71	162.19		
16.575	16.575	(1.105)	176	610035			68.26- 128.26	96.85		

6 Propylene										
						CAS #:	115-07-1			
2.280	2.280	(0.283)	41	2591741	100.000	102.48	70.00- 130.00	100.00		
2.280	2.280	(0.283)	42	1728444			0.00- 30.00	66.69		
2.280	2.280	(0.283)	39	1780659			0.00- 30.00	68.71		

8 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.335	2.335	(0.290)	85	4936969	100.000	115.24	70.00- 130.00	100.00		
2.335	2.335	(0.290)	87	1597861			0.00- 30.00	32.37		

9 Freon 114										
						CAS #:	76-14-2			
2.474	2.474	(0.307)	135	4042630	100.000	103.40	70.00- 130.00	100.00		
2.474	2.474	(0.307)	137	1282118			2.29- 62.29	31.71		

10 Chloromethane										
						CAS #:	74-87-3			
2.612	2.612	(0.324)	50	3405993	100.000	105.88	70.00- 130.00	100.00		
2.612	2.612	(0.324)	52	1041620			0.00- 30.00	30.58		

13 Vinyl Chloride										
						CAS #:	75-01-4			
2.778	2.778	(0.345)	62	3220830	100.000	104.02	70.00- 130.00	100.00		
2.778	2.778	(0.345)	64	1008251			0.00- 30.00	31.30		

12 1,3-Butadiene										
						CAS #:	106-99-0			
2.750	2.750	(0.341)	54	2935038	100.000	110.99	70.00- 130.00	100.00		
2.750	2.750	(0.341)	39	2947538			0.00- 30.00	100.43		

15 Bromomethane										
						CAS #:	74-83-9			
3.276	3.276	(0.406)	94	2153199	100.000	107.72	70.00- 130.00	100.00		
3.276	3.276	(0.406)	96	2023282			65.07- 125.07	93.97		

19 Chloroethane										
						CAS #:	75-00-3			
3.414	3.414	(0.424)	64	1565896	100.000	99.424	70.00- 130.00	100.00		
3.414	3.414	(0.424)	49	445169			0.00- 30.00	28.43		
3.414	3.414	(0.424)	66	461281			0.00- 30.00	29.46		

20 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.718	3.718	(0.461)	101	4911495	100.000	105.15	70.00- 130.00	100.00		
3.718	3.718	(0.461)	103	3183710			34.56- 94.56	64.82		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.105	4.105	(0.509)	45	1045340	100.000	103.02	70.00- 130.00	100.00	
4.077	4.077	(0.506)	43	190328			0.00- 30.00	18.21	
4.105	4.105	(0.509)	46	413290			0.00- 30.00	39.54	

30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	3009266	100.000	103.61	70.00- 130.00	100.00	
4.520	4.520	(0.561)	153	1866918			33.43- 93.43	62.04	
4.520	4.520	(0.561)	101	4188633			108.48- 168.48	139.19	

31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	4078882	100.000	106.12	70.00- 130.00	100.00	
4.575	4.575	(0.568)	96	2277835			27.13- 87.13	55.84	
4.575	4.575	(0.568)	98	1453379			5.60- 65.60	35.63	

32 Acetone						CAS #: 67-64-1			
4.713	4.713	(0.585)	58	1567044	100.000	109.00	70.00- 130.00	100.00	
4.713	4.713	(0.585)	43	4681900			0.00- 30.00	298.77	

36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	5612024	100.000	109.69	70.00- 130.00	100.00	
4.907	4.907	(0.609)	43	1154075			0.00- 30.00	20.56	
4.935	4.935	(0.612)	59	198977			0.00- 30.00	3.55	

35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	7167211	100.000	110.11	70.00- 130.00	100.00	

38 3-Chloropropene						CAS #: 107-05-1			
5.183	5.183	(0.643)	76	1153842	100.000	106.46	70.00- 130.00	100.00	
5.183	5.183	(0.643)	41	4405012			0.00- 30.00	381.77	

43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	3421033	100.000	104.09	70.00- 130.00	100.00	
5.460	5.460	(0.677)	84	1995352			29.81- 89.81	58.33	
5.432	5.432	(0.674)	51	1046132			0.00- 30.00	30.58	

46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	2289440	100.000	92.537	70.00- 130.00	100.00	
5.764	5.764	(0.715)	57	733908			1.68- 61.68	32.06	
5.764	5.764	(0.715)	41	781870			0.00- 30.00	34.15	

47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	2568670	100.000	110.34	70.00- 130.00	100.00	
5.819	5.819	(0.722)	61	4104175			133.65- 193.65	159.78	
5.819	5.819	(0.722)	98	1632808			0.00- 30.00	63.57	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	5269145	100.000	111.31	70.00- 130.00	100.00	
6.151	6.151	(0.763)	43	3621749			0.00- 30.00	68.74	
6.151	6.151	(0.763)	86	743039			0.00- 30.00	14.10	

55 1,1-Dichloroethane						CAS #: 75-34-3			
6.593	6.593	(0.818)	63	4598639	100.000	109.10	70.00- 130.00	100.00	
6.593	6.593	(0.818)	65	1401480			0.52- 60.52	30.48	

67 2-Butanone						CAS #: 78-93-3			
7.644	7.644	(0.949)	72	1140456	100.000	112.12	70.00- 130.00	100.00	
7.644	7.644	(0.949)	43	6545068			536.33- 596.33	573.90	
7.644	7.644	(0.949)	57	442595			0.00- 30.00	38.81	

66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	3372749	100.000	106.57	70.00- 130.00	100.00	
7.617	7.617	(0.945)	96	2273619			37.56- 97.56	67.41	
7.617	7.617	(0.945)	98	1458637			14.52- 74.52	43.25	

70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	3862336	100.000	101.98	70.00- 130.00	100.00	
8.031	8.031	(0.997)	71	1005813			0.00- 55.74	26.04	
8.031	8.031	(0.997)	72	1059045			0.00- 30.00	27.42	

72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	3865056	100.000	108.23	70.00- 130.00	100.00	
8.197	8.197	(1.017)	85	2482837			35.19- 95.19	64.24	

75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.446	8.446	(1.048)	97	3815620	100.000	106.89	70.00- 130.00	100.00	
8.418	8.418	(1.045)	99	2483612			33.02- 93.02	65.09	

74 Cyclohexane						CAS #: 110-82-7			
8.418	8.418	(1.045)	84	3142908	100.000	109.30	70.00- 130.00	100.00	
8.418	8.418	(1.045)	56	5009806			126.11- 186.11	159.40	
8.391	8.391	(1.041)	41	2756840			55.82- 115.82	87.72	

56 Vinyl Acetate						CAS #: 108-05-4			
6.649	6.649	(0.825)	86	618984	100.000	115.92	70.00- 130.00	100.00	
6.649	6.649	(0.825)	43	7909568			0.00- 30.00	1277.83	
6.649	6.649	(0.825)	42	576336			0.00- 30.00	93.11	

77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	3324674	100.000	112.80	70.00- 130.00	100.00	
8.667	8.667	(1.075)	117	3444612			75.98- 135.98	103.61	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.110	9.110	(1.130)	57	14667384	100.000	113.00	70.00- 130.00	100.00		
9.110	9.110	(1.130)	56	4774429			0.00- 30.00	32.55		
9.110	9.110	(1.130)	41	3713992			0.00- 30.00	25.32		

81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	6443717	100.000	107.17	70.00- 130.00	100.00		
9.082	9.082	(0.916)	77	1479096			0.00- 30.00	22.95		

85	1,2-Dichloroethane					CAS #: 107-06-2				
9.275	9.275	(0.936)	62	2980908	100.000	108.22	70.00- 130.00	100.00		
9.275	9.275	(0.936)	64	935537			0.00- 30.00	31.38		

90	Heptane					CAS #: 142-82-5				
9.497	9.497	(0.958)	100	768289	100.000	114.40	70.00- 130.00	100.00		
9.469	9.469	(0.955)	43	5921486			0.00- 30.00	770.74		
9.469	9.469	(0.955)	71	2319652			0.00- 30.00	301.92		

93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	2531522	100.000	103.80	70.00- 130.00	100.00		
10.326	10.326	(1.042)	130	2370571			64.49- 124.49	93.64		
10.326	10.326	(1.042)	97	1632142			34.72- 94.72	64.47		

98	1,2-Dichloropropane					CAS #: 78-87-5				
10.851	10.851	(1.095)	63	2444067	100.000	103.36	70.00- 130.00	100.00		
10.851	10.851	(1.095)	62	1742633			39.05- 99.05	71.30		
10.824	10.824	(1.092)	41	1706739			36.65- 96.65	69.83		

99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.117)	88	1444101	100.000	105.16	70.00- 130.00	100.00		
11.045	11.045	(1.114)	58	1358709			62.00- 122.00	94.09		
11.045	11.045	(1.114)	57	421008			0.00- 30.00	29.15		

100	Bromodichloromethane					CAS #: 75-27-4				
11.404	11.404	(1.151)	83	3686686	100.000	108.12	70.00- 130.00	100.00		
11.404	11.404	(1.151)	85	2353475			34.72- 94.72	63.84		

103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	2762200	100.000	114.30	70.00- 130.00	100.00		
12.317	12.317	(1.243)	77	825604			0.28- 60.28	29.89		
12.289	12.289	(1.240)	39	1995795			43.30- 103.30	72.25		

106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.593	12.593	(1.271)	58	2267876	100.000	115.13	70.00- 130.00	100.00		
12.593	12.593	(1.271)	43	6376954			0.00- 30.00	281.19		
12.593	12.593	(1.271)	85	737054			0.00- 30.00	32.50		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	6367014	100.000	102.65	70.00- 130.00	100.00	
12.815	12.815	(1.293)	92	3757228			29.65- 89.65	59.01	

113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	2753871	100.000	118.31	70.00- 130.00	100.00	
13.368	13.368	(0.891)	77	862721			1.96- 61.96	31.33	
13.340	13.340	(0.889)	39	1883829			38.82- 98.82	68.41	

114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	2175838	100.000	104.79	70.00- 130.00	100.00	
13.644	13.644	(0.910)	99	1345223			33.63- 93.63	61.83	
13.644	13.644	(0.910)	83	1807881			55.73- 115.73	83.09	

116 Tetrachloroethene						CAS #: 127-18-4			
13.699	13.699	(0.913)	166	2471030	100.000	102.39	70.00- 130.00	100.00	
13.699	13.699	(0.913)	129	1991710			50.24- 110.24	80.60	
13.699	13.699	(0.913)	131	1942785			48.42- 108.42	78.62	

119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	3181008	100.000	109.82	70.00- 130.00	100.00	
14.004	14.004	(0.934)	43	6436176			168.65- 228.65	202.33	
14.031	14.031	(0.935)	100	503002			0.00- 30.00	15.81	

120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	3253162	100.000	111.97	70.00- 130.00	100.00	
14.197	14.197	(0.947)	127	2514914			0.00- 30.00	77.31	

122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	3320619	100.000	109.10	70.00- 130.00	100.00	
14.363	14.363	(0.958)	109	3107302			63.74- 123.74	93.58	

126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	4886903	100.000	103.08	70.00- 130.00	100.00	
15.027	15.027	(1.002)	114	1546858			1.82- 61.82	31.65	
15.027	15.027	(1.002)	77	3017918			31.79- 91.79	61.76	

128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	2675495	100.000	104.46	70.00- 130.00	100.00	
15.165	15.165	(1.011)	91	9072718			0.00- 30.00	339.10	

130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	3435495	100.000	109.20	70.00- 130.00	100.00	
15.331	15.331	(1.022)	91	7334004			0.00- 30.00	213.48	

132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	3218448	100.000	107.58	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	7280732			195.49- 255.49	226.22	

133 Styrene									
15.911	15.911	(1.061)	104	5132999	100.000	116.38	70.00- 130.00	100.00	
15.911	15.911	(1.061)	78	2701016			22.39- 82.39	52.62	

134 Bromoform									
16.160	16.160	(1.077)	173	2829830	100.000	109.30	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	1476899			21.21- 81.21	52.19	

141 1,1,2,2-Tetrachloroethane									
16.796	16.796	(1.120)	83	4764204	100.000	105.60	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	3047016			33.63- 93.63	63.96	

144 4-Ethyltoluene									
16.962	16.962	(1.131)	105	10073530	100.000	114.13	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	2874204			0.00- 59.46	28.53	

147 1,3,5-Trimethylbenzene									
17.045	17.045	(1.136)	105	9098092	100.000	114.04	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	4188565			0.00- 30.00	46.04	

152 1,2,4-Trimethylbenzene									
17.460	17.460	(1.164)	105	7592274	100.000	112.18	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	3445930			16.11- 76.11	45.39	

155 1,3-Dichlorobenzene									
17.764	17.764	(1.184)	146	4936158	100.000	103.02	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	3149621			0.00- 30.00	63.81	
17.764	17.764	(1.184)	111	2021086			0.00- 30.00	40.94	

156 1,4-Dichlorobenzene									
17.847	17.847	(1.190)	146	6039588	100.000	107.55	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	3761986			0.00- 30.00	62.29	
17.847	17.847	(1.190)	111	2601264			0.00- 30.00	43.07	

157 alpha-Chlorotoluene									
17.985	17.985	(1.199)	91	9864888	100.000	139.51	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	1849741			0.00- 30.00	18.75	

159 1,2-Dichlorobenzene									
18.206	18.206	(1.214)	146	5182397	100.000	102.84	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	3320571			32.64- 92.64	64.07	
18.206	18.206	(1.214)	111	2125741			11.53- 71.53	41.02	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.506	19.506	(1.300)	180	3562078	100.000	99.579	70.00- 130.00	100.00	
19.506	19.506	(1.300)	182	3343294			63.93- 123.93	93.86	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.589	19.589	(1.306)	225	2481075	100.000	98.724	70.00- 130.00	100.00	
19.589	19.589	(1.306)	223	1537358			32.69- 92.69	61.96	

142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	11634048	100.000	111.99	70.00- 130.00	100.00	
16.824	16.824	(1.122)	120	2469759			0.00- 30.00	21.23	
16.824	16.824	(1.122)	105	398750			0.00- 30.00	3.43	

136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	9672736	100.000	106.64	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	2545654			0.00- 30.00	26.32	
16.326	16.326	(1.088)	51	1381671			0.00- 30.00	14.28	

165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	13517916	100.000	113.46	70.00- 130.00	100.00	
19.672	19.672	(1.312)	127	1684760			0.00- 30.00	12.46	

17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	4628579	100.000	103.20	70.00- 130.00	100.00	
3.414	3.414	(0.424)	57	2949004			0.00- 30.00	63.71	
3.414	3.414	(0.424)	72	289136			0.00- 30.00	6.25	

11	Butane					CAS #: 106-97-8			
2.695	2.695	(0.334)	58	775812	100.000	101.45	70.00- 130.00	100.00	
2.695	2.695	(0.334)	43	5714173			0.00- 30.00	736.54	

94	Methyl Cyclohexane					CAS #: 108-87-2			
10.547	10.547	(1.064)	83	3726328	100.000	107.30	70.00- 130.00	100.00	
10.547	10.547	(1.064)	98	1818897			0.00- 30.00	48.81	
10.547	10.547	(1.064)	55	4140939			0.00- 30.00	111.13	

Report Date: 13-Nov-2007 13:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111212.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	362309	1.99
92 1,4-Difluorobenze	1306915	784149	1829681	1394945	6.74
125 Chlorobenzene-d5	1023463	614078	1432848	1101731	7.65

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111212.d
Date: 12-NOV-2007 15:41
Client ID: Level 6
Sample Info: 100mL #1576-89

Column phase: RTX-624

Instrument: msd5.1
Operator: cb
Column diameter: 0.53

/chem/msd5.1/5-12nov.b/5111212.d



Report Date: 27-Nov-2007 15:31

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-27nov.b/5112707.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 27-NOV-2007 12:08
 Operator : cb Inst ID: msd5.i
 Smp Info : 200mL #1443-374
 Misc Info : 200ppbv
 Comment :
 Method : /chem/msd5.i/5-27nov.b/t14qn12c.m
 Meth Date : 27-Nov-2007 15:31 cbond Quant Type: ISTD
 Cal Date : 27-NOV-2007 12:08 Cal File: 5112707.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp19b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	292008	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	228611				47.29- 107.29	78.29
8.059	8.059	(1.000)	49	634506				183.28- 243.28	217.29

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1011912	25.0000			70.00- 130.00	100.00
9.912	9.912	(1.000)	88	161742				0.00- 46.71	15.98

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	815306	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	457661				0.00- 30.00	56.13

7 Isobutane CAS #: 75-28-5									
2.502	2.502	(0.310)	43	10956154	200.000	204.54		70.00- 130.00	100.00(A)
2.502	2.502	(0.310)	42	3649588				0.00- 30.00	33.31
2.502	2.502	(0.310)	58	324251				0.00- 30.00	2.96

18 Pentane CAS #: 109-66-0									
3.801	3.801	(0.472)	43	11879225	200.000	217.13		70.00- 130.00	100.00(A)

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
18 Pentane (continued)									
3.801	3.801	(0.472)	57	1697893			0.00- 30.00	14.29	
3.801	3.801	(0.472)	72	987894			0.00- 30.00	8.32	

25 Acrolein						CAS #: 107-02-8			
4.492	4.492	(0.557)	55	1613223	200.000	236.63	70.00- 130.00	100.00(A)	
4.492	4.492	(0.557)	56	2291472			0.00- 30.00	142.04	

39 Acrylonitrile						CAS #: 107-13-1			
5.930	5.930	(0.736)	53	4870715	200.000	226.34	70.00- 130.00	100.00(A)	
5.930	5.930	(0.736)	52	3665944			0.00- 30.00	75.27	

42 1-Pentene						CAS #: 109-67-1			
3.746	3.746	(0.465)	55	6311026	200.000	213.79	70.00- 130.00	100.00(TA)	
3.746	3.746	(0.465)	42	8977985			0.00- 30.00	142.26	
0.000	1.000	(0.000)	0	0			0.00- 30.00	0.00	

44 Ethyl Ether						CAS #: 60-29-7			
4.160	4.160	(0.516)	74	2422443	200.000	216.92	70.00- 130.00	100.00(TA)	
4.160	4.160	(0.516)	59	4103622			0.00- 30.00	169.40	
0.000	1.000	(0.000)	31	0			0.00- 30.00	0.00	

53 Iodomethane						CAS #: 74-88-4			
4.852	4.852	(0.602)	142	8300306	200.000	214.25	70.00- 130.00	100.00(A)	
4.852	4.852	(0.602)	127	2702327			0.00- 30.00	32.56	

58 1-Hexene						CAS #: 592-41-6			
6.041	6.041	(0.750)	55	3937252	200.000	230.04	70.00- 130.00	100.00(A)	
6.041	6.041	(0.750)	41	6021255			0.00- 30.00	152.93	
6.041	6.041	(0.750)	84	1242160			0.00- 30.00	31.55	

62 Methyl Acrylate						CAS #: 96-33-3			
7.783	7.783	(0.966)	55	8563472	200.000	249.39	70.00- 130.00	100.00(A)	
7.783	7.783	(0.966)	85	1022521			0.00- 30.00	11.94	
7.783	7.783	(0.966)	58	775887			0.00- 30.00	9.06	

86 2-Pentanone						CAS #: 107-87-9			
10.796	10.796	(1.089)	43	12448831	200.000	246.92	70.00- 130.00	100.00(A)	
10.796	10.796	(1.089)	58	864970			0.00- 30.00	6.95	
10.796	10.796	(1.089)	86	1531382			0.00- 30.00	12.30	

88 Ethyl Acrylate						CAS #: 140-88-5			
10.603	10.603	(1.070)	55	9381427	200.000	241.38	70.00- 130.00	100.00(A)	
10.630	10.630	(1.073)	99	504390			0.00- 30.00	5.38	
10.603	10.603	(1.070)	45	999353			0.00- 30.00	10.65	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
95 Dibromomethane			CAS #: 74-95-3						
11.073	11.073	(1.117)	174	2700745	200.000	213.73	70.00- 130.00	100.00(A)	
11.073	11.073	(1.117)	93	3037775			0.00- 30.00	112.48	
11.073	11.073	(1.117)	95	2547353			0.00- 30.00	94.32	

96 Methyl Methacrylate			CAS #: 80-62-6						
11.073	11.073	(1.117)	41	6484005	200.000	239.52	70.00- 130.00	100.00(A)	
11.073	11.073	(1.117)	69	3076497			0.00- 30.00	47.45	
11.073	11.073	(1.117)	100	1197569			0.00- 30.00	18.47	

112 Alphamethylstyrene			CAS #: 98-83-9						
17.294	17.294	(1.153)	118	5959126	200.000	253.24	70.00- 130.00	100.00(A)	
17.294	17.294	(1.153)	103	3515220			0.00- 30.00	58.99	

117 Bis(2-chloroethyl) ether			CAS #: 111-44-4						
17.709	17.709	(1.181)	93	6541008	200.000	235.52	70.00- 130.00	100.00(A)	
17.709	17.709	(1.181)	95	2074279			0.00- 30.00	31.71	
17.709	17.709	(1.181)	63	5507058			0.00- 30.00	84.19	

127 Nonane			CAS #: 111-84-2						
15.303	15.303	(1.020)	43	10713070	200.000	234.42	70.00- 130.00	100.00(A)	
15.331	15.331	(1.022)	57	8243126			0.00- 30.00	76.94	
15.331	15.331	(1.022)	85	2319331			0.00- 30.00	21.65	

QC Flag Legend

- T - Target compound detected outside RT window.
- A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 27-Nov-2007 15:31

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 27-NOV-2007

Lab File ID: 5112707.d

Calibration Time: 09:21

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-27nov.b/t14qn12c.m

Misc Info: 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	351932	211159	492705	292008	-17.03
92 1,4-Difluorobenze	1207474	724484	1690464	1011912	-16.20
125 Chlorobenzene-d5	945809	567485	1324133	815306	-13.80

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.94	9.61	10.27	9.91	-0.28
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-27nov.b/5112707.d

Date: 27-NOV-2007 12:08

Client ID: Level 7

Sample Info: 200mL #1443-374


Column phase: RTX-624

Instrument: msd5.1

Operator: cb

Column diameter: 0.53

/chem/msd5.1/5-27nov.b/5112707.d

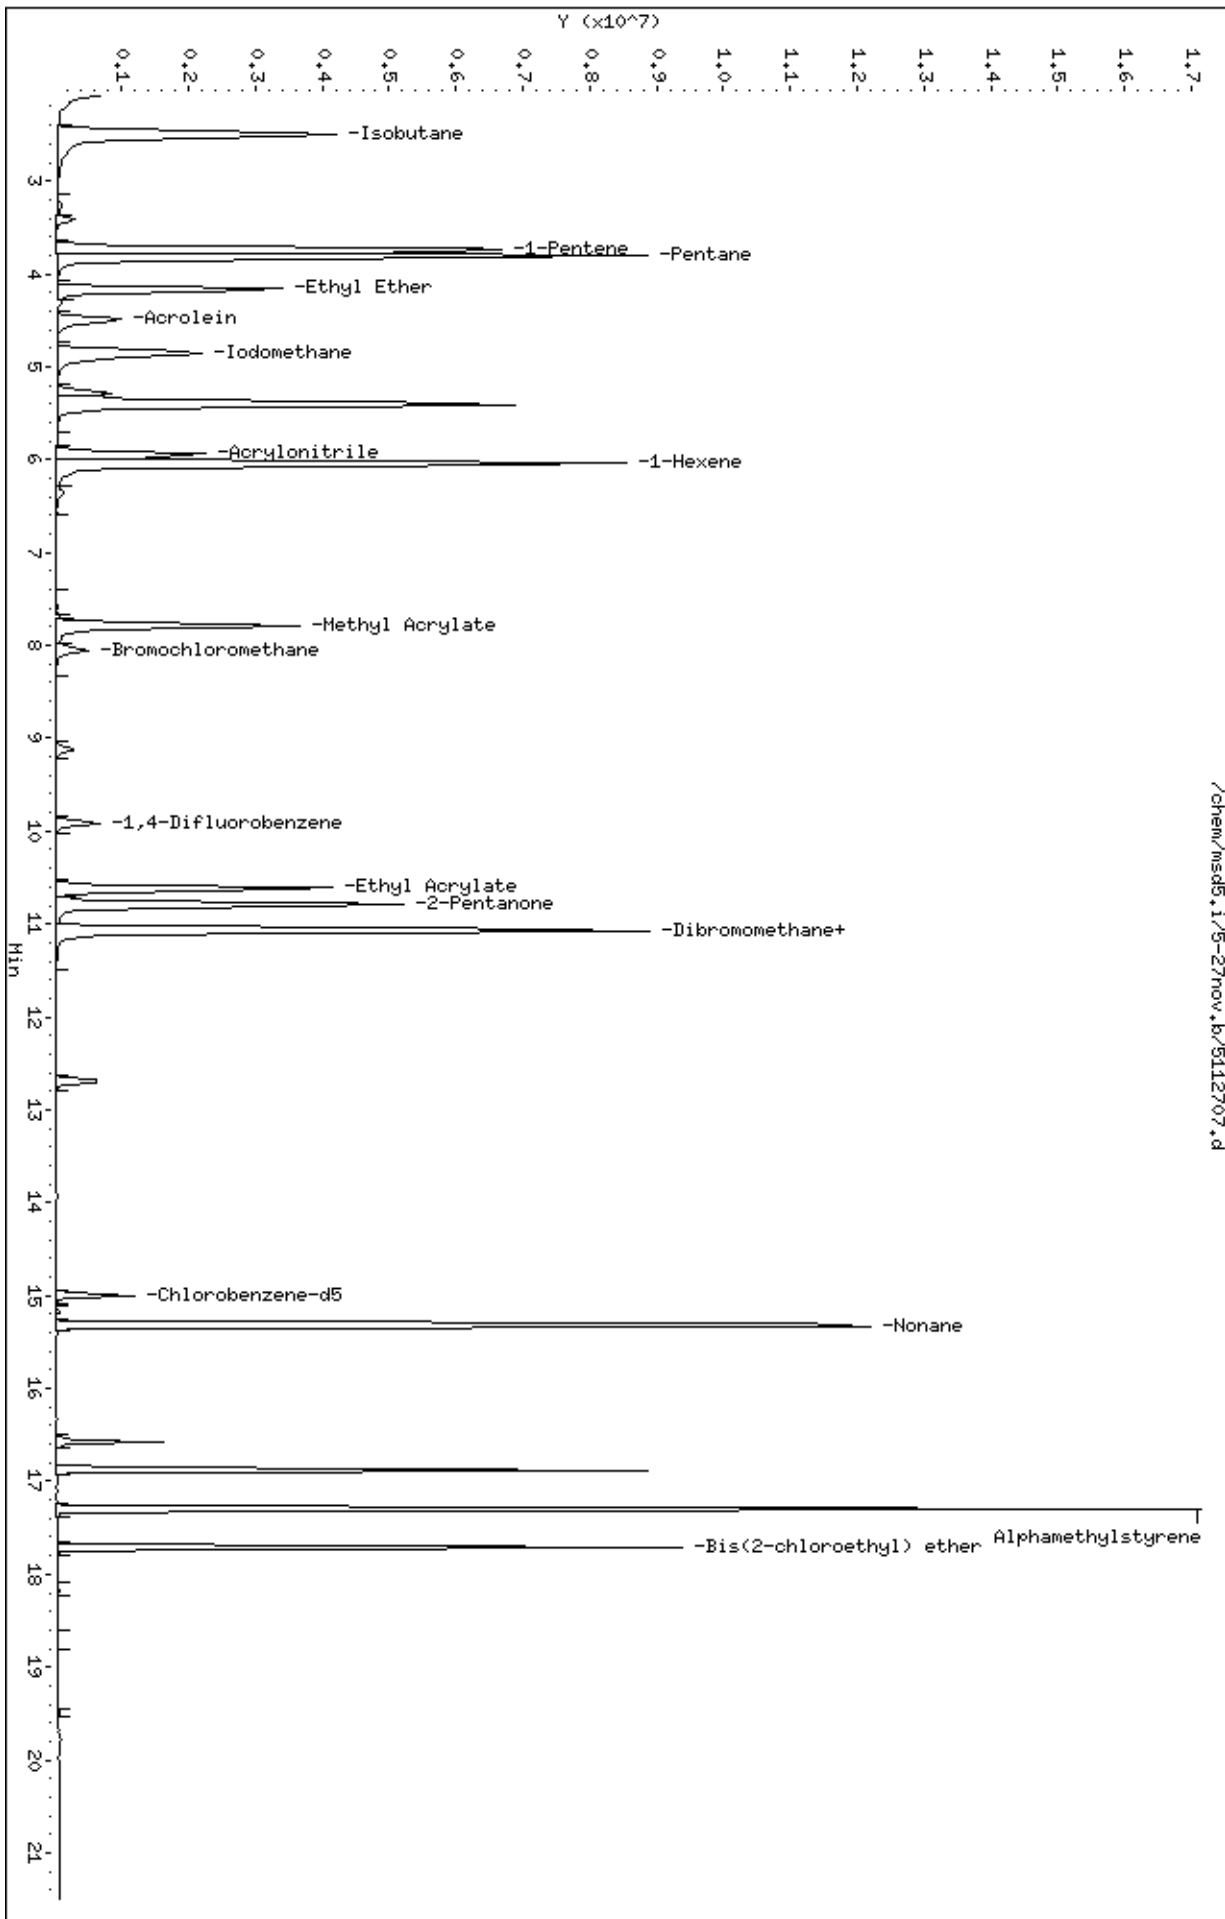

Report Date: 20-Nov-2007 15:39

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-19nov.b/5111904.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 19-NOV-2007 02:57
 Operator : sjr Inst ID: msd5.i
 Smp Info : 200mL #1487-405
 Misc Info : 200ppbv -> 200ppbv
 Comment :
 Method : /chem/msd5.i/5-19nov.b/t14qn12b.m
 Meth Date : 20-Nov-2007 15:39 ctaylor Quant Type: ISTD
 Cal Date : 19-NOV-2007 02:57 Cal File: 5111904.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp21b.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	343138	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	270425				47.38- 107.38	78.81
8.059	8.059	(1.000)	49	766186				197.25- 257.25	223.29

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1331702	25.0000			70.00- 130.00	100.00
9.912	9.912	(1.000)	88	197405				0.00- 47.51	14.82

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	994154	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	589200				0.00- 30.00	59.27

1 Freon134a CAS #: 811-97-2									
2.225	2.225	(0.276)	83	2822475	200.000	198.64		70.00- 130.00	100.00
2.197	2.197	(0.273)	69	12292152				0.00- 30.00	435.51

3 Freon 152a CAS #: 75-37-6									
2.280	2.280	(0.283)	65	2698998	200.000	211.17		70.00- 130.00	100.00(A)
2.363	2.363	(0.293)	51	13971311				0.00- 30.00	517.65

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

4 Freon 22						CAS #: 75-45-6			
2.363	2.363	(0.293)	67	765522	200.000	193.31	70.00- 130.00	100.00	
2.363	2.363	(0.293)	51	13848942			0.00- 30.00	1809.08	

5 Freon142b						CAS #: 75-68-3			
2.557	2.557	(0.317)	65	5656340	200.000	221.99	70.00- 130.00	100.00(A)	
2.557	2.557	(0.317)	45	1828730			0.00- 30.00	32.33	

16 Dichlorofluoromethane/Fr21						CAS #: 75-43-4			
3.746	3.746	(0.465)	67	6310190	200.000	205.50	70.00- 130.00	100.00(TA)	
3.746	3.746	(0.465)	69	1881367			0.00- 30.00	29.81	
0.000	1.000	(0.000)	35	0			0.00- 30.00	0.00	

22 Freon123a						CAS #: 354-23-4			
4.299	4.299	(0.533)	117	3567672	200.000	209.65	70.00- 130.00	100.00(A)	
4.299	4.299	(0.533)	67	5067373			0.00- 30.00	142.04	

24 Freon123						CAS #: 306-83-2			
4.409	4.409	(0.547)	83	6759738	200.000	211.63	70.00- 130.00	100.00(A)	
4.409	4.409	(0.547)	133	1059607			0.00- 30.00	15.68	
4.409	4.409	(0.547)	85	4429960			0.00- 30.00	65.53	

37 tert-Butyl-Alcohol						CAS #: 75-65-0			
5.571	5.571	(0.691)	59	2326170	200.000	130.45	70.00- 130.00	100.00	
5.571	5.571	(0.691)	41	747973			0.00- 30.00	32.15	
5.571	5.571	(0.691)	57	252239			0.00- 30.00	10.84	

49 Isopropyl ether						CAS #: 108-20-3			
6.594	6.594	(0.818)	45	19030534	200.000	221.98	70.00- 130.00	100.00(A)	
6.594	6.594	(0.818)	87	3450126			0.00- 30.00	18.13	
6.594	6.594	(0.818)	59	1842568			0.00- 30.00	9.68	

57 Ethyl-tert-butyl Ether						CAS #: 637-92-3			
7.202	7.202	(0.894)	59	6528854	200.000	198.99	70.00- 130.00	100.00	
7.202	7.202	(0.894)	87	2135083			0.00- 30.00	32.70	
7.202	7.202	(0.894)	41	1374641			0.00- 30.00	21.05	

61 Ethyl Acetate						CAS #: 141-78-6			
7.700	7.700	(0.955)	70	927220	200.000	231.95	70.00- 130.00	100.00(A)	
7.700	7.700	(0.955)	43	11648831			0.00- 30.00	1256.32	
7.700	7.700	(0.955)	61	1400945			0.00- 30.00	151.09	

64 1-Propanol						CAS #: 71-23-8			
6.787	6.787	(0.842)	42	957247	200.000	267.57	70.00- 130.00	100.00(A)	
6.787	6.787	(0.842)	59	954733			0.00- 30.00	99.74	
6.787	6.787	(0.842)	41	583962			0.00- 30.00	61.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

76 Isobutanol					CAS #: 78-83-1				
9.082	9.082	(0.916)	43	4496367	200.000	234.43	70.00- 130.00	100.00(A)	
9.082	9.082	(0.916)	41	3057760			0.00- 30.00	68.01	

78 tert-amyl-Methyl Ether					CAS #: 994-05-8				
9.276	9.276	(1.151)	73	4894950	200.000	186.00	70.00- 130.00	100.00	
9.276	9.276	(1.151)	87	1188343			0.00- 30.00	24.28	
9.276	9.276	(1.151)	55	2091139			0.00- 30.00	42.72	

118 Butyl Acetate					CAS #: 123-86-4				
14.197	14.197	(1.432)	56	4685613	200.000	232.17	70.00- 130.00	100.00(A)	
14.197	14.197	(1.432)	73	1304433			0.00- 30.00	27.84	
14.197	14.197	(1.432)	43	12061971			0.00- 30.00	257.43	

131 2-Heptanone					CAS #: 110-43-0				
16.077	16.077	(1.072)	58	7288423	200.000	246.65	70.00- 130.00	100.00(A)	
16.077	16.077	(1.072)	43	12754387			0.00- 30.00	175.00	

135 Cyclohexanone					CAS #: 108-94-1				
16.520	16.520	(1.101)	55	5982602	200.000	226.08	70.00- 130.00	100.00(A)	
16.520	16.520	(1.101)	98	1904727			0.00- 30.00	31.84	
16.520	16.520	(1.101)	42	4318876			0.00- 30.00	72.19	

146 Diisobutyl Ketone					CAS #: 108-83-8				
17.211	17.211	(1.147)	57	15014507	200.000	215.13	70.00- 130.00	100.00(A)	
17.211	17.211	(1.147)	85	9264937			30.87- 90.87	61.71	

QC Flag Legend

- T - Target compound detected outside RT window.
- A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 20-Nov-2007 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 19-NOV-2007

Lab File ID: 5111904.d

Calibration Time: 02:24

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msd5.i/5-19nov.b/t14qn12b.m

Misc Info: 200ppbv -> 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	320182	192109	448255	343138	7.17
92 1,4-Difluorobenze	1222930	733758	1712102	1331702	8.89
125 Chlorobenzene-d5	969063	581438	1356688	994154	2.59

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-19nov.b/5111904.d

Date: 19-NOV-2007 02:57

Client ID: Level 7

Sample Info: 200mL #1487-405


Column phase: RTX-624

Instrument: msd5.1

Operator: sjr

Column diameter: 0.53

/chem/msd5.1/5-19nov.b/5111904.d



Report Date: 13-Nov-2007 13:25

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111218.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 12-NOV-2007 20:20
 Operator : cb Inst ID: msd5.i
 Smp Info : 200mL #1487-404
 Misc Info : 200ppbv -> 200ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:25 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 20:20 Cal File: 5111218.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp20a.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	380418	25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	291580				47.79- 107.79	76.65
8.031	8.031	(1.000)	49	799092				186.23- 246.23	210.06

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1363143	25.0000			70.00- 130.00	100.00
9.912	9.912	(1.000)	88	229507				0.00- 46.01	16.84

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	1062928	25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	616683				0.00- 30.00	58.02

33 Methyl Acetate CAS #: 79-20-9									
5.211	5.211	(0.647)	43	12259393	200.000	217.95		70.00- 130.00	100.00(A)
5.211	5.211	(0.647)	74	2047380				0.00- 30.00	16.70
5.211	5.211	(0.647)	59	866635				0.00- 30.00	7.07

52 Chloroprene CAS #: 126-99-8									
6.677	6.677	(0.828)	53	10072516	200.000	223.69		70.00- 130.00	100.00(A)

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
52 Chloroprene (continued)									
6.677	6.677	(0.828)	88	4358164			12.60- 72.60	43.27	
6.677	6.677	(0.828)	50	2391088			0.00- 52.95	23.74	

59 1,3-Dichloropropane CAS #: 142-28-9									
13.893	13.893	(1.402)	76	5643367	200.000	217.03	70.00- 130.00	100.00(A)	
13.893	13.893	(1.402)	41	5633681			68.80- 128.80	99.83	
13.893	13.893	(1.402)	78	1790220			0.00- 30.00	31.72	

60 2,2-Dichloropropane CAS #: 594-20-7									
7.561	7.561	(0.938)	77	5849796	200.000	222.24	70.00- 130.00	100.00(A)	
7.561	7.561	(0.938)	79	1862935			2.86- 62.86	31.85	
7.561	7.561	(0.938)	97	1314683			0.00- 30.00	22.47	

73 1,1-Dichloropropene CAS #: 563-58-6									
8.723	8.723	(1.082)	110	2156285	200.000	215.16	70.00- 130.00	100.00(A)	
8.723	8.723	(1.082)	75	5802969			0.00- 30.00	269.12	

123 1,1,1,2-Tetrachloroethane CAS #: 630-20-6									
15.193	15.193	(1.013)	131	4139143	200.000	217.85	70.00- 130.00	100.00(A)	
15.193	15.193	(1.013)	117	2866073			0.00- 30.00	69.24	
15.165	15.165	(1.011)	95	1719696			0.00- 30.00	41.55	

137 Bromobenzene CAS #: 108-86-1									
16.741	16.741	(1.116)	156	4901390	200.000	208.50	70.00- 130.00	100.00(A)	
16.741	16.741	(1.116)	77	9195353			151.57- 211.57	187.61	
16.741	16.741	(1.116)	158	4720437			0.00- 30.00	96.31	

139 1,2,3-Trichloropropane CAS #: 96-18-4									
16.852	16.852	(1.123)	110	2719560	200.000	210.85	70.00- 130.00	100.00(A)	
16.852	16.852	(1.123)	61	2348836			0.00- 30.00	86.37	
16.852	16.852	(1.123)	112	1719588			0.00- 30.00	63.23	

140 2-Chlorotoluene CAS #: 95-49-8									
16.962	16.962	(1.131)	126	4375302	200.000	222.05	70.00- 130.00	100.00(A)	
16.962	16.962	(1.131)	91	14275120			287.64- 347.64	326.27	
16.962	16.962	(1.131)	65	1397486			0.00- 30.00	31.94	

143 4-Chlorotoluene CAS #: 106-43-4									
17.100	17.100	(1.140)	126	4466011	200.000	220.88	70.00- 130.00	100.00(A)	
17.100	17.100	(1.140)	91	14535401			287.83- 347.83	325.47	
17.100	17.100	(1.140)	63	1857348			0.00- 30.00	41.59	

149 tert-Butylbenzene CAS #: 98-06-6									
17.377	17.377	(1.159)	119	18494291	200.000	226.11	70.00- 130.00	100.00(A)	
17.377	17.377	(1.159)	134	3933766			0.00- 53.69	21.27	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
149 tert-Butylbenzene (continued)									
17.377	17.377	(1.159)	91	11227307			0.00- 30.00	60.71	

150 Pentachloroethane CAS #: 76-01-7									
17.460	17.460	(1.164)	167	3427155	200.000	238.56	70.00- 130.00	100.00(A)	
17.432	17.432	(1.162)	117	3887356			0.00- 30.00	113.43	

151 sec-Butylbenzene CAS #: 135-98-8									
17.598	17.598	(1.173)	105	20306305	200.000	209.14	70.00- 130.00	100.00(A)	
17.598	17.598	(1.173)	134	4363727			0.00- 49.07	21.49	
17.598	17.598	(1.173)	91	3819852			0.00- 30.00	18.81	

153 p-Cymene CAS #: 99-87-6									
17.764	17.764	(1.184)	134	4947028	200.000	235.40	70.00- 130.00	100.00(A)	
17.764	17.764	(1.184)	119	18479267			341.15- 401.15	373.54	
17.764	17.764	(1.184)	91	4493393			0.00- 30.00	90.83	

154 1,2,3-Trimethylbenzene CAS #: 526-73-8									
17.875	17.875	(1.192)	120	6956133	200.000	230.47	70.00- 130.00	100.00(A)	
17.875	17.875	(1.192)	105	16213534			197.36- 257.36	233.08	
17.875	17.875	(1.192)	77	1812902			0.00- 30.00	26.06	

158 Butylbenzene CAS #: 104-51-8									
18.151	18.151	(1.210)	134	4435716	200.000	234.08	70.00- 130.00	100.00(A)	
18.123	18.123	(1.208)	91	18354905			393.82- 453.82	413.80	
18.123	18.123	(1.208)	92	10202168			0.00- 30.00	230.00	

160 Hexachloroethane CAS #: 67-72-1									
18.372	18.372	(1.225)	117	6549758	200.000	233.67	70.00- 130.00	100.00(A)	
18.400	18.400	(1.227)	201	4183292			0.00- 30.00	63.87	
Sum of Peak Amounts =					234				

161 1,2-Dibromo-3-Chloropropane CAS #: 96-12-8									
18.870	18.870	(1.258)	157	4780713	200.000	246.99	70.00- 130.00	100.00(A)	
18.870	18.870	(1.258)	75	5676066			92.49- 152.49	118.73	
18.870	18.870	(1.258)	155	3766945			0.00- 30.00	78.79	

166 1,2,3-Trichlorobenzene CAS #: 87-61-6									
19.865	19.865	(1.324)	180	9209537	200.000	219.56	70.00- 130.00	100.00(A)	
19.865	19.865	(1.324)	182	8636309			0.00- 30.00	93.78	
19.865	19.865	(1.324)	145	3064881			0.00- 30.00	33.28	

192 Cyclopentene CAS #: 142-29-0									
5.211	5.211	(0.647)	67	11768190	200.000	214.19	70.00- 130.00	100.00(A)	
5.211	5.211	(0.647)	68	4482374			0.00- 30.00	38.09	
5.211	5.211	(0.647)	53	2799572			0.00- 30.00	23.79	

QC Flag Legend

A - Target compound detected but, quantitated amount
exceeded maximum amount.

Report Date: 13-Nov-2007 13:25

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111218.d

Calibration Time: 19:48

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv -> 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	345466	207280	483652	380418	10.12
92 1,4-Difluorobenze	1312181	787309	1837053	1363143	3.88
125 Chlorobenzene-d5	1008754	605252	1412256	1062928	5.37


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 13-Nov-2007 13:21

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-12nov.b/5111213.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 12-NOV-2007 16:13
 Operator : cb Inst ID: msd5.i
 Smp Info : 200mL #1576-89
 Misc Info : 200ppbv
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:20 ctaylor Quant Type: ISTD
 Cal Date : 12-NOV-2007 16:13 Cal File: 5111213.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04MDL+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

* 71	Bromochloromethane						CAS #: 74-97-5	
8.059	8.059	(1.000)	130	379428 25.0000			70.00- 130.00	100.00
8.059	8.059	(1.000)	128	296624			42.76- 102.76	78.18
8.059	8.059	(1.000)	49	802235			173.18- 233.18	211.43

* 92	1,4-Difluorobenzene						CAS #: 540-36-3	
9.912	9.912	(1.000)	114	1473899 25.0000			70.00- 130.00	100.00
9.912	9.912	(1.000)	88	238341			0.00- 46.42	16.17

* 125	Chlorobenzene-d5						CAS #: 3114-55-4	
14.999	14.999	(1.000)	117	1158184 25.0000			70.00- 130.00	100.00
14.999	14.999	(1.000)	82	685651			0.00- 30.00	59.20

\$ 84	1,2-Dichloroethane-d4						CAS #: 17060-07-0	
9.137	9.137	(1.134)	65	596904 25.0000	26.283		70.00- 130.00	100.00
9.110	9.110	(1.130)	67	414836			0.00- 30.00	69.50

\$ 107	Toluene-d8						CAS #: 2037-26-5	
12.704	12.704	(1.282)	98	1336408 25.0000	25.682		70.00- 130.00	100.00
12.704	12.704	(1.282)	70	133913			0.00- 30.00	10.02

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	940191			0.00- 30.00	70.35		

\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	686157	25.0000	25.391	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	1078230			128.71- 188.71	157.14		
16.575	16.575	(1.105)	176	661942			68.26- 128.26	96.47		

6 Propylene										
						CAS #: 115-07-1				
2.280	2.280	(0.283)	41	5376726	200.000	203.02	70.00- 130.00	100.00(A)		
2.280	2.280	(0.283)	42	3639937			0.00- 30.00	67.70		
2.280	2.280	(0.283)	39	3684723			0.00- 30.00	68.53		

8 Dichlorodifluoromethane/Fr12										
						CAS #: 75-71-8				
2.336	2.336	(0.290)	85	9953066	200.000	221.84	70.00- 130.00	100.00(A)		
2.336	2.336	(0.290)	87	3204362			0.00- 30.00	32.19		

9 Freon 114										
						CAS #: 76-14-2				
2.502	2.502	(0.310)	135	8125587	200.000	198.45	70.00- 130.00	100.00		
2.502	2.502	(0.310)	137	2547872			2.29- 62.29	31.36		

10 Chloromethane										
						CAS #: 74-87-3				
2.640	2.640	(0.328)	50	6779536	200.000	201.24	70.00- 130.00	100.00(A)		
2.640	2.640	(0.328)	52	2029289			0.00- 30.00	29.93		

13 Vinyl Chloride										
						CAS #: 75-01-4				
2.778	2.778	(0.345)	62	6453329	200.000	199.02	70.00- 130.00	100.00		
2.778	2.778	(0.345)	64	2007029			0.00- 30.00	31.10		

12 1,3-Butadiene										
						CAS #: 106-99-0				
2.778	2.778	(0.345)	54	5891794	200.000	212.76	70.00- 130.00	100.00(A)		
2.778	2.778	(0.345)	39	6841437			0.00- 30.00	116.12		

15 Bromomethane										
						CAS #: 74-83-9				
3.276	3.276	(0.406)	94	4372221	200.000	208.86	70.00- 130.00	100.00(A)		
3.276	3.276	(0.406)	96	4138619			65.07- 125.07	94.66		

19 Chloroethane										
						CAS #: 75-00-3				
3.442	3.442	(0.427)	64	3239683	200.000	196.42	70.00- 130.00	100.00		
3.442	3.442	(0.427)	49	869249			0.00- 30.00	26.83		
3.442	3.442	(0.427)	66	945867			0.00- 30.00	29.20		

20 Trichlorofluoromethane/Fr11										
						CAS #: 75-69-4				
3.746	3.746	(0.465)	101	9929412	200.000	202.99	70.00- 130.00	100.00(A)		
3.746	3.746	(0.465)	103	6390218			34.56- 94.56	64.36		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.133	4.133	(0.513)	45	1967404	200.000	185.14	70.00- 130.00	100.00	
4.133	4.133	(0.513)	43	362712			0.00- 30.00	18.44	
4.133	4.133	(0.513)	46	816407			0.00- 30.00	41.50	

30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	6057243	200.000	199.15	70.00- 130.00	100.00	
4.548	4.548	(0.564)	153	3827738			33.43- 93.43	63.19	
4.520	4.520	(0.561)	101	8431386			108.48- 168.48	139.20	

31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	8478221	200.000	210.62	70.00- 130.00	100.00(A)	
4.575	4.575	(0.568)	96	4763041			27.13- 87.13	56.18	
4.575	4.575	(0.568)	98	3012899			5.60- 65.60	35.54	

32 Acetone						CAS #: 67-64-1			
4.713	4.713	(0.585)	58	3222078	200.000	214.00	70.00- 130.00	100.00(A)	
4.713	4.713	(0.585)	43	9448686			0.00- 30.00	293.25	

36 2-Propanol						CAS #: 67-63-0			
4.935	4.935	(0.612)	45	11561568	200.000	215.77	70.00- 130.00	100.00(A)	
4.935	4.935	(0.612)	43	2331834			0.00- 30.00	20.17	
4.935	4.935	(0.612)	59	426669			0.00- 30.00	3.69	

35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	14564959	200.000	213.66	70.00- 130.00	100.00(A)	

38 3-Chloropropene						CAS #: 107-05-1			
5.184	5.184	(0.643)	76	2321881	200.000	204.57	70.00- 130.00	100.00(A)	
5.184	5.184	(0.643)	41	8708129			0.00- 30.00	375.05	

43 Methylene Chloride						CAS #: 75-09-2			
5.460	5.460	(0.678)	49	6972846	200.000	202.58	70.00- 130.00	100.00(A)	
5.460	5.460	(0.678)	84	4089078			29.81- 89.81	58.64	
5.460	5.460	(0.678)	51	2112801			0.00- 30.00	30.30	

46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	3902079	200.000	150.60	70.00- 130.00	100.00	
5.764	5.764	(0.715)	57	1232072			1.68- 61.68	31.57	
5.764	5.764	(0.715)	41	1256752			0.00- 30.00	32.21	

47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	5269287	200.000	216.15	70.00- 130.00	100.00(A)	
5.819	5.819	(0.722)	61	8491435			133.65- 193.65	161.15	
5.819	5.819	(0.722)	98	3350199			0.00- 30.00	63.58	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	10867838	200.000	219.22	70.00- 130.00	100.00(A)	
6.151	6.151	(0.763)	43	7427006			0.00- 30.00	68.34	
6.179	6.179	(0.767)	86	1502171			0.00- 30.00	13.82	

55 1,1-Dichloroethane						CAS #: 75-34-3			
6.594	6.594	(0.818)	63	9466761	200.000	214.47	70.00- 130.00	100.00(A)	
6.594	6.594	(0.818)	65	2873484			0.52- 60.52	30.35	

67 2-Butanone						CAS #: 78-93-3			
7.644	7.644	(0.949)	72	2401975	200.000	225.48	70.00- 130.00	100.00(A)	
7.644	7.644	(0.949)	43	13592738			536.33- 596.33	565.90	
7.644	7.644	(0.949)	57	970844			0.00- 30.00	40.42	

66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	7018804	200.000	211.78	70.00- 130.00	100.00(A)	
7.617	7.617	(0.945)	96	4681675			37.56- 97.56	66.70	
7.617	7.617	(0.945)	98	2974274			14.52- 74.52	42.38	

70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	7952915	200.000	200.51	70.00- 130.00	100.00(A)	
8.031	8.031	(0.997)	71	2097817			0.00- 55.74	26.38	
8.031	8.031	(0.997)	72	2268304			0.00- 30.00	28.52	

72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	7997810	200.000	213.85	70.00- 130.00	100.00(A)	
8.197	8.197	(1.017)	85	5151553			35.19- 95.19	64.41	

75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.446	8.446	(1.048)	97	7928397	200.000	212.09	70.00- 130.00	100.00(A)	
8.446	8.446	(1.048)	99	5100696			33.02- 93.02	64.33	

74 Cyclohexane						CAS #: 110-82-7			
8.418	8.418	(1.045)	84	6469207	200.000	214.82	70.00- 130.00	100.00(A)	
8.418	8.418	(1.045)	56	10311383			126.11- 186.11	159.39	
8.391	8.391	(1.041)	41	5608294			55.82- 115.82	86.69	

56 Vinyl Acetate						CAS #: 108-05-4			
6.649	6.649	(0.825)	86	1313244	200.000	234.84	70.00- 130.00	100.00(A)	
6.649	6.649	(0.825)	43	16877699			0.00- 30.00	1285.19	
6.649	6.649	(0.825)	42	1237902			0.00- 30.00	94.26	

77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	6929597	200.000	224.51	70.00- 130.00	100.00(A)	
8.667	8.667	(1.075)	117	7148759			75.98- 135.98	103.16	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.110	9.110	(1.130)	57	30319210	200.000	223.04	70.00-	130.00	100.00(A)	
9.110	9.110	(1.130)	56	9915225			0.00-	30.00	32.70	
9.110	9.110	(1.130)	41	7628319			0.00-	30.00	25.16	

81	Benzene					CAS #:	71-43-2			
9.082	9.082	(0.916)	78	13162200	200.000	207.18	70.00-	130.00	100.00(A)	
9.082	9.082	(0.916)	77	3019769			0.00-	30.00	22.94	

85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	6115333	200.000	210.12	70.00-	130.00	100.00(A)	
9.276	9.276	(0.936)	64	1907292			0.00-	30.00	31.19	

90	Heptane					CAS #:	142-82-5			
9.497	9.497	(0.958)	100	1552617	200.000	218.81	70.00-	130.00	100.00(A)	
9.469	9.469	(0.955)	43	12168235			0.00-	30.00	783.72	
9.469	9.469	(0.955)	71	4755038			0.00-	30.00	306.26	

93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	5225261	200.000	202.78	70.00-	130.00	100.00(A)	
10.326	10.326	(1.042)	130	4874779			64.49-	124.49	93.29	
10.326	10.326	(1.042)	97	3343656			34.72-	94.72	63.99	

98	1,2-Dichloropropane					CAS #:	78-87-5			
10.852	10.852	(1.095)	63	5104635	200.000	204.32	70.00-	130.00	100.00(A)	
10.852	10.852	(1.095)	62	3646628			39.05-	99.05	71.44	
10.824	10.824	(1.092)	41	3449628			36.65-	96.65	67.58	

99	1,4-Dioxane					CAS #:	123-91-1			
11.073	11.073	(1.117)	88	3047468	200.000	210.03	70.00-	130.00	100.00(A)	
11.045	11.045	(1.114)	58	2835408			62.00-	122.00	93.04	
11.045	11.045	(1.114)	57	881722			0.00-	30.00	28.93	

100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	7699387	200.000	213.72	70.00-	130.00	100.00(A)	
11.405	11.405	(1.151)	85	4904851			34.72-	94.72	63.70	

103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	5762675	200.000	225.69	70.00-	130.00	100.00(A)	
12.317	12.317	(1.243)	77	1837180			0.28-	60.28	31.88	
12.289	12.289	(1.240)	39	4130568			43.30-	103.30	71.68	

106	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.594	12.594	(1.271)	58	4730396	200.000	227.29	70.00-	130.00	100.00(A)	
12.594	12.594	(1.271)	43	13344863			0.00-	30.00	282.11	
12.594	12.594	(1.271)	85	1564460			0.00-	30.00	33.07	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	13234278	200.000	201.94	70.00- 130.00	100.00(A)	
12.815	12.815	(1.293)	92	7782172			29.65- 89.65	58.80	

113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	5992352	200.000	244.89	70.00- 130.00	100.00(A)	
13.368	13.368	(0.891)	77	1862914			1.96- 61.96	31.09	
13.340	13.340	(0.889)	39	4062607			38.82- 98.82	67.80	

114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	4441546	200.000	203.48	70.00- 130.00	100.00(A)	
13.644	13.644	(0.910)	99	2760199			33.63- 93.63	62.15	
13.644	13.644	(0.910)	83	3712821			55.73- 115.73	83.59	

116 Tetrachloroethene						CAS #: 127-18-4			
13.700	13.700	(0.913)	166	4978683	200.000	196.23	70.00- 130.00	100.00	
13.700	13.700	(0.913)	129	4049222			50.24- 110.24	81.33	
13.700	13.700	(0.913)	131	3856812			48.42- 108.42	77.47	

119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	6788322	200.000	222.94	70.00- 130.00	100.00(A)	
14.004	14.004	(0.934)	43	13564043			168.65- 228.65	199.81	
14.031	14.031	(0.935)	100	1021389			0.00- 30.00	15.05	

120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	6797279	200.000	222.56	70.00- 130.00	100.00(A)	
14.197	14.197	(0.947)	127	5288923			0.00- 30.00	77.81	

122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	6974912	200.000	218.00	70.00- 130.00	100.00(A)	
14.363	14.363	(0.958)	109	6501581			63.74- 123.74	93.21	

126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	10023472	200.000	201.12	70.00- 130.00	100.00(A)	
15.027	15.027	(1.002)	114	3208018			1.82- 61.82	32.01	
15.027	15.027	(1.002)	77	6285605			31.79- 91.79	62.71	

128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	5595835	200.000	207.82	70.00- 130.00	100.00(A)	
15.165	15.165	(1.011)	91	18264820			0.00- 30.00	326.40	

130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	6958327	200.000	210.40	70.00- 130.00	100.00(A)	
15.331	15.331	(1.022)	91	15132243			0.00- 30.00	217.47	

132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	6397817	200.000	203.44	70.00- 130.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	14678586			195.49- 255.49	229.43	

133 Styrene CAS #: 100-42-5									
15.911	15.911	(1.061)	104	10594301	200.000	228.49	70.00- 130.00	100.00(A)	
15.911	15.911	(1.061)	78	5603941			22.39- 82.39	52.90	

134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	5879832	200.000	216.03	70.00- 130.00	100.00(A)	
16.160	16.160	(1.077)	171	3042544			21.21- 81.21	51.75	

141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	9654646	200.000	203.57	70.00- 130.00	100.00(A)	
16.796	16.796	(1.120)	85	6137606			33.63- 93.63	63.57	

144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	19926988	200.000	214.75	70.00- 130.00	100.00(A)	
16.962	16.962	(1.131)	120	5796728			0.00- 59.46	29.09	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	16195440	200.000	193.10	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	8354342			0.00- 30.00	51.58	

152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	15645232	200.000	219.90	70.00- 130.00	100.00(A)	
17.460	17.460	(1.164)	120	7177069			16.11- 76.11	45.87	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	10205679	200.000	202.62	70.00- 130.00	100.00(A)	
17.764	17.764	(1.184)	148	6469217			0.00- 30.00	63.39	
17.764	17.764	(1.184)	111	4196257			0.00- 30.00	41.12	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	11649605	200.000	197.34	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	7316004			0.00- 30.00	62.80	
17.847	17.847	(1.190)	111	5090946			0.00- 30.00	43.70	

157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	14811552	200.000	199.26	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	3792145			0.00- 30.00	25.60	

159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	10278339	200.000	194.01	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	6561023			32.64- 92.64	63.83	
18.206	18.206	(1.214)	111	4303497			11.53- 71.53	41.87	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.506	19.506	(1.300)	180	7407149	200.000	196.98	70.00- 130.00	100.00	
19.506	19.506	(1.300)	182	6968403			63.93- 123.93	94.08	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.589	19.589	(1.306)	225	4964078	200.000	187.90	70.00- 130.00	100.00	
19.589	19.589	(1.306)	223	3098497			32.69- 92.69	62.42	

142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	22515730	200.000	206.17	70.00- 130.00	100.00(A)	
16.824	16.824	(1.122)	120	5037838			0.00- 30.00	22.37	
16.824	16.824	(1.122)	105	809839			0.00- 30.00	3.60	

136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	17361026	200.000	182.07	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	5128121			0.00- 30.00	29.54	
16.326	16.326	(1.088)	51	2810203			0.00- 30.00	16.19	

165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	15685584	200.000	125.24	70.00- 130.00	100.00	
19.672	19.672	(1.312)	127	3440644			0.00- 30.00	21.94	

17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	9276275	200.000	197.49	70.00- 130.00	100.00	
3.414	3.414	(0.424)	57	5992060			0.00- 30.00	64.60	
3.414	3.414	(0.424)	72	601448			0.00- 30.00	6.48	

11	Butane					CAS #: 106-97-8			
2.695	2.695	(0.334)	58	1610134	200.000	201.06	70.00- 130.00	100.00(A)	
2.695	2.695	(0.334)	43	11574318			0.00- 30.00	718.84	

94	Methyl Cyclohexane					CAS #: 108-87-2			
10.547	10.547	(1.064)	83	7735277	200.000	210.81	70.00- 130.00	100.00(A)	
10.547	10.547	(1.064)	98	3742413			0.00- 30.00	48.38	
10.547	10.547	(1.064)	55	8517231			0.00- 30.00	110.11	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 13-Nov-2007 13:21

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111213.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	379428	6.81
92 1,4-Difluorobenze	1306915	784149	1829681	1473899	12.78
125 Chlorobenzene-d5	1023463	614078	1432848	1158184	13.16

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-12nov.b/5111213.d
Date: 12-NOV-2007 16:13
Client ID: Level 7
Sample Info: 200mL #1576-89

Column phase: RTX-624

Instrument: msd5.1
Operator: cb
Column diameter: 0.53



Report Date: 13-Nov-2007 13:21

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-13nov.b/5111303.d
 Lab Smp Id: ICAL Client Smp ID: Level 8
 Inj Date : 13-NOV-2007 12:52
 Operator : ct Inst ID: msd5.i
 Smp Info : 50mL #1497-139
 Misc Info : 250ppbv (1000ppbv)
 Comment :
 Method : /chem/msd5.i/5-12nov.b/t14qn12a.m
 Meth Date : 13-Nov-2007 13:21 ctaylor Quant Type: ISTD
 Cal Date : 13-NOV-2007 12:52 Cal File: 5111303.d
 Als bottle: 1 Calibration Sample, Level: 8
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: Level8.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	351990	25.0000		70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	274795			42.76- 102.76	78.07	
8.031	8.031	(1.000)	49	788886			173.18- 233.18	224.12	

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1397135	25.0000		70.00- 130.00	100.00	
9.912	9.912	(1.000)	88	229663			0.00- 46.42	16.44	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	1075416	25.0000		70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	649768			0.00- 30.00	60.42	

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.110	9.110	(1.130)	65	593872	25.0000	28.188	70.00- 130.00	100.00	
9.110	9.110	(1.130)	67	443921			0.00- 30.00	74.75	

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.704	12.704	(1.282)	98	1240246	25.0000	25.144	70.00- 130.00	100.00	
12.677	12.677	(1.279)	70	124834			0.00- 30.00	10.07	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 107 Toluene-d8 (continued)									
12.704	12.704	(1.282)	100	913233			0.00- 30.00	73.63	

\$ 138 Bromofluorobenzene									
						CAS #: 460-00-4			
16.575	16.575	(1.105)	174	661035	25.0000	26.344	70.00- 130.00	100.00	
16.575	16.575	(1.105)	95	1017403			128.71- 188.71	153.91	
16.575	16.575	(1.105)	176	644249			68.26- 128.26	97.46	

113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	7589108	250.000	334.02	70.00- 130.00	100.00(A)	
13.368	13.368	(0.891)	77	2394908			1.96- 61.96	31.56	
13.340	13.340	(0.889)	39	5237247			38.82- 98.82	69.01	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 13-Nov-2007 13:21

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 12-NOV-2007

Lab File ID: 5111303.d

Calibration Time: 15:12

Lab Smp Id: ICAL

Client Smp ID: Level 8

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /chem/msd5.i/5-12nov.b/t14qn12a.m

Misc Info: 250ppbv (1000ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355243	213146	497340	351990	-0.92
92 1,4-Difluorobenze	1306915	784149	1829681	1397135	6.90
125 Chlorobenzene-d5	1023463	614078	1432848	1075416	5.08

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-13nov.b/5111303.d

Date: 13-NOV-2007 12:52

Client ID: Level 8

Sample Info: 50mL #1497-139


Column phase: RTX-624

Instrument: msd5.1

Operator: ct

Column diameter: 0.53

/chem/msd5.1/5-13nov.b/5111303.d





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0712439-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122803	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 12/28/07 09:33 AM

Compound	%Recovery
Freon 12	100
Freon 114	102
Vinyl Chloride	98
Bromomethane	97
Chloroethane	90
Freon 11	104
1,1-Dichloroethene	103
Freon 113	103
Methylene Chloride	110
1,1-Dichloroethane	105
cis-1,2-Dichloroethene	104
Chloroform	105
1,1,1-Trichloroethane	107
Carbon Tetrachloride	114
Benzene	94
1,2-Dichloroethane	111
Trichloroethene	96
1,2-Dichloropropane	97
cis-1,3-Dichloropropene	104
Toluene	94
trans-1,3-Dichloropropene	108
1,1,2-Trichloroethane	98
Tetrachloroethene	102
1,2-Dibromoethane (EDB)	102
Chlorobenzene	98
Ethyl Benzene	98
m,p-Xylene	101
o-Xylene	103
Styrene	101
1,1,2,2-Tetrachloroethane	98
1,3,5-Trimethylbenzene	109
1,2,4-Trimethylbenzene	104
1,3-Dichlorobenzene	93
1,4-Dichlorobenzene	105
alpha-Chlorotoluene	115
1,2-Dichlorobenzene	92
1,3-Butadiene	112
Hexane	110
Cyclohexane	98



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0712439-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122803	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 12/28/07 09:33 AM

Compound	%Recovery
Heptane	99
Bromodichloromethane	104
Dibromochloromethane	108
Cumene	102
Propylbenzene	110
Chloromethane	109
1,2,4-Trichlorobenzene	93
Hexachlorobutadiene	98
Acetone	97
Carbon Disulfide	97
2-Propanol	99
trans-1,2-Dichloroethene	99
2-Butanone (Methyl Ethyl Ketone)	98
Tetrahydrofuran	101
1,4-Dioxane	94
4-Methyl-2-pentanone	108
2-Hexanone	102
Bromoform	108
4-Ethyltoluene	112
Ethanol	100
Methyl tert-butyl ether	119
3-Chloropropene	92
2,2,4-Trimethylpentane	112
Naphthalene	112

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	101	70-130
1,2-Dichloroethane-d4	111	70-130
4-Bromofluorobenzene	105	70-130

Report Date: 28-Dec-2007 09:47

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i Injection Date: 28-DEC-2007 09:33
 Lab File ID: 5122803.d Init. Cal. Date(s): 12-NOV-2007 27-NOV-2007
 Analysis Type: AIR Init. Cal. Times: 13:22 12:08
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /var/chem/msd5.i/5-28dec.b/t14qn12c.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 84 1,2-Dichloroethane-d4	1.49639	1.66545	0.010	-11.29751	30.00000	Averaged
\$ 107 Toluene-d8	0.88263	0.89131	0.010	-0.98375	30.00000	Averaged
\$ 138 Bromofluorobenzene	0.58333	0.61467	0.010	-5.37341	30.00000	Averaged
6 Propylene	1.74497	1.81764	0.010	-4.16473	30.00000	Averaged
8 Dichlorodifluoromethane/Fr1	2.95608	2.97102	0.010	-0.50513	30.00000	Averaged
9 Freon 114	2.69778	2.75752	0.010	-2.21416	30.00000	Averaged
10 Chloromethane	2.21969	2.41326	0.010	-8.72059	30.00000	Averaged
13 Vinyl Chloride	2.13649	2.09674	0.010	1.86054	30.00000	Averaged
12 1,3-Butadiene	1.82463	2.04729	0.010	-12.20268	30.00000	Averaged
15 Bromomethane	1.37930	1.34131	0.010	2.75457	30.00000	Averaged
19 Chloroethane	1.08675	0.97940	0.010	9.87828	30.00000	Averaged
20 Trichlorofluoromethane/Fr11	3.22295	3.33810	0.010	-3.57293	30.00000	Averaged
26 Ethanol	0.70017	0.69816	0.010	0.28728	30.00000	Averaged
30 Freon 113	2.00401	2.06964	0.010	-3.27510	30.00000	Averaged
31 1,1-Dichloroethene	2.65222	2.72592	0.010	-2.77889	30.00000	Averaged
32 Acetone	0.99203	0.96075	0.010	3.15338	30.00000	Averaged
36 2-Propanol	3.53043	3.51153	0.010	0.53532	30.00000	Averaged
35 Carbon Disulfide	4.49145	4.37262	0.010	2.64572	30.00000	Averaged
38 3-Chloropropene	0.74783	0.68656	0.010	8.19284	30.00000	Averaged
43 Methylene Chloride	2.26785	2.50790	0.010	-10.58469	30.00000	Averaged
46 MTBE	1.70717	2.03595	0.010	-19.25920	30.00000	Averaged
47 trans-1,2-Dichloroethene	1.60625	1.59535	0.010	0.67879	30.00000	Averaged
51 Hexane	3.26636	3.57780	0.010	-9.53460	30.00000	Averaged
55 1,1-Dichloroethane	2.90836	3.04695	0.010	-4.76513	30.00000	Averaged
67 2-Butanone	0.70189	0.68465	0.010	2.45745	30.00000	Averaged
66 cis-1,2-Dichloroethene	2.18371	2.28155	0.010	-4.48049	30.00000	Averaged
70 Tetrahydrofuran	2.61338	2.64356	0.010	-1.15503	30.00000	Averaged
72 Chloroform	2.46416	2.59241	0.010	-5.20473	30.00000	Averaged
75 1,1,1-Trichloroethane	2.46307	2.64749	0.010	-7.48737	30.00000	Averaged
74 Cyclohexane	1.98423	1.95145	0.010	1.65205	30.00000	Averaged
56 Vinyl Acetate	0.36845	0.47390	0.010	-28.62179	30.00000	Averaged
77 Carbon Tetrachloride	2.03366	2.32551	0.010	-14.35093	30.00000	Averaged
80 2,2,4-Trimethylpentane	8.95659	9.99210	0.010	-11.56140	30.00000	Averaged
81 Benzene	1.07756	1.01081	0.010	6.19450	30.00000	Averaged
85 1,2-Dichloroethane	0.49365	0.54980	0.010	-11.37395	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i Injection Date: 28-DEC-2007 09:33
 Lab File ID: 5122803.d Init. Cal. Date(s): 12-NOV-2007 27-NOV-2007
 Analysis Type: AIR Init. Cal. Times: 13:22 12:08
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /var/chem/msd5.i/5-28dec.b/t14qn12c.m

COMPOUND	RRF / AMOUNT	RF50	MIN		MAX		CURVE TYPE
			RRF	%D / %DRIFT	%D / %DRIFT	%D / %DRIFT	
90 Heptane	0.12036	0.11927	0.010	0.90521	30.00000	Averaged	
93 Trichloroethene	0.43706	0.41921	0.010	4.08442	30.00000	Averaged	
98 1,2-Dichloropropane	0.42376	0.41187	0.010	2.80613	30.00000	Averaged	
99 1,4-Dioxane	0.24611	0.23210	0.010	5.69393	30.00000	Averaged	
100 Bromodichloromethane	0.61107	0.63501	0.010	-3.91700	30.00000	Averaged	
103 cis-1,3-Dichloropropene	0.43309	0.45295	0.010	-4.58440	30.00000	Averaged	
106 4-Methyl-2-pentanone	0.35302	0.38318	0.010	-8.54312	30.00000	Averaged	
108 Toluene	1.11163	1.04715	0.010	5.80094	30.00000	Averaged	
113 trans-1,3-Dichloropropene	0.52818	0.57053	0.010	-8.01730	30.00000	Averaged	
114 1,1,2-Trichloroethane	0.47116	0.46058	0.010	2.24529	30.00000	Averaged	
116 Tetrachloroethene	0.54765	0.56104	0.010	-2.44472	30.00000	Averaged	
119 2-Hexanone	0.65725	0.67287	0.010	-2.37679	30.00000	Averaged	
120 Dibromochloromethane	0.65925	0.70985	0.010	-7.67607	30.00000	Averaged	
122 1,2-Dibromoethane	0.69063	0.70363	0.010	-1.88177	30.00000	Averaged	
126 Chlorobenzene	1.07580	1.05346	0.010	2.07595	30.00000	Averaged	
128 Ethyl Benzene	0.58120	0.57208	0.010	1.57021	30.00000	Averaged	
130 m,p-Xylene	0.71385	0.72093	0.010	-0.99099	30.00000	Averaged	
132 o-Xylene	0.67883	0.69925	0.010	-3.00802	30.00000	Averaged	
133 Styrene	1.00085	1.01074	0.010	-0.98787	30.00000	Averaged	
134 Bromoform	0.58750	0.63244	0.010	-7.64900	30.00000	Averaged	
141 1,1,2,2-Tetrachloroethane	1.02374	1.00370	0.010	1.95699	30.00000	Averaged	
144 4-Ethyltoluene	2.00291	2.23474	0.010	-11.57495	30.00000	Averaged	
147 1,3,5-Trimethylbenzene	1.81040	1.96887	0.010	-8.75344	30.00000	Averaged	
152 1,2,4-Trimethylbenzene	1.53578	1.60393	0.010	-4.43753	30.00000	Averaged	
155 1,3-Dichlorobenzene	1.08725	1.01631	0.010	6.52528	30.00000	Averaged	
156 1,4-Dichlorobenzene	1.27425	1.33822	0.010	-5.01991	30.00000	Averaged	
157 alpha-Chlorotoluene	1.60452	1.84698	0.010	-15.11125	30.00000	Averaged	
159 1,2-Dichlorobenzene	1.14355	1.05869	0.010	7.42064	30.00000	Averaged	
163 1,2,4-Trichlorobenzene	0.81171	0.75285	0.010	7.25113	30.00000	Averaged	
164 Hexachlorobutadiene	0.57027	0.55909	0.010	1.95997	30.00000	Averaged	
142 Propylbenzene	2.35732	2.59327	0.010	-10.00897	30.00000	Averaged	
136 Cumene	2.05825	2.10620	0.010	-2.32992	30.00000	Averaged	
165 Naphthalene	2.70346	3.03215	0.010	-12.15784	30.00000	Averaged	
17 Isopentane	3.09489	3.37493	0.010	-9.04848	30.00000	Averaged	
11 Butane	0.52766	0.52971	0.010	-0.38964	30.00000	Averaged	

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i Injection Date: 28-DEC-2007 09:33
Lab File ID: 5122803.d Init. Cal. Date(s): 12-NOV-2007 27-NOV-2007
Analysis Type: AIR Init. Cal. Times: 13:22 12:08
Lab Sample ID: CCV-1 Quant Type: ISTD
Method: /var/chem/msd5.i/5-28dec.b/t14qn12c.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
94 Methyl Cyclohexane	0.62237	0.60966	0.010	2.04304	30.00000	Averaged

Report Date: 28-Dec-2007 09:47

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-28dec.b/5122803.d
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1
 Inj Date : 28-DEC-2007 09:33
 Operator : cb Inst ID: msd5.i
 Smp Info : 50mL #1443-379
 Misc Info : 50ppbv (200ppbv)
 Comment :
 Method : /var/chem/msd5.i/5-28dec.b/t14qn12c.m
 Meth Date : 28-Dec-2007 09:47 cbond Quant Type: ISTD
 Cal Date : 27-NOV-2007 12:08 Cal File: 5112707.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5									
8.059	8.059	(1.000)	130	269712	25.0000			80.00- 120.00	100.00
8.059	8.059	(1.000)	128	216539				50.29- 110.29	80.29
8.031	8.031	(1.000)	49	640352				207.42- 267.42	237.42

* 92 1,4-Difluorobenzene CAS #: 540-36-3									
9.912	9.912	(1.000)	114	1058104	25.0000			80.00- 120.00	100.00
9.912	9.912	(1.000)	88	183354				0.00- 47.33	17.33

* 125 Chlorobenzene-d5 CAS #: 3114-55-4									
14.999	14.999	(1.000)	117	829571	25.0000			80.00- 120.00	100.00
14.999	14.999	(1.000)	82	498833				0.00- 30.00	60.13

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.110	9.110	(1.130)	65	449191	25.0000	27.824		80.00- 120.00	100.00
9.110	9.110	(1.130)	67	235061				27.88- 87.88	52.33

\$ 107 Toluene-d8 CAS #: 2037-26-5									
12.677	12.677	(1.279)	98	943100	25.0000	25.246		80.00- 120.00	100.00
12.677	12.677	(1.279)	70	97730				0.00- 40.29	10.36

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 107 Toluene-d8 (continued)									
12.677	12.677	(1.279)	100	622229			37.87- 97.87	65.98	

\$ 138 Bromofluorobenzene									
						CAS #: 460-00-4			
16.575	16.575	(1.105)	174	509913	25.0000	26.343	80.00- 120.00	100.00	
16.575	16.575	(1.105)	95	780098			122.99- 182.99	152.99	
16.575	16.575	(1.105)	176	483688			64.86- 124.86	94.86	

6 Propylene									
						CAS #: 115-07-1			
2.280	2.280	(0.283)	41	980481	50.0000	52.082	80.00- 120.00	100.00	
2.280	2.280	(0.283)	42	659242			0.00- 30.00	67.24	
2.280	2.280	(0.283)	39	647155			0.00- 30.00	66.00	

8 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
2.336	2.336	(0.290)	85	1602637	50.0000	50.252	80.00- 120.00	100.00	
2.336	2.336	(0.290)	87	519988			0.00- 30.00	32.45	

9 Freon 114									
						CAS #: 76-14-2			
2.446	2.446	(0.304)	135	1487470	50.0000	51.107	80.00- 120.00	100.00	
2.446	2.446	(0.304)	137	474532			1.90- 61.90	31.90	

10 Chloromethane									
						CAS #: 74-87-3			
2.584	2.584	(0.321)	50	1301770	50.0000	54.360	80.00- 120.00	100.00	
2.584	2.584	(0.321)	52	391550			0.00- 30.00	30.08	

13 Vinyl Chloride									
						CAS #: 75-01-4			
2.778	2.778	(0.345)	62	1131033	50.0000	49.070	80.00- 120.00	100.00	
2.778	2.778	(0.345)	64	345105			0.00- 30.00	30.51	

12 1,3-Butadiene									
						CAS #: 106-99-0			
2.750	2.750	(0.341)	54	1104355	50.0000	56.101	80.00- 120.00	100.00	
2.750	2.750	(0.341)	39	1142808			0.00- 30.00	103.48	

15 Bromomethane									
						CAS #: 74-83-9			
3.276	3.276	(0.406)	94	723533	50.0000	48.623	80.00- 120.00	100.00	
3.276	3.276	(0.406)	96	695111			66.07- 126.07	96.07	

19 Chloroethane									
						CAS #: 75-00-3			
3.386	3.386	(0.420)	64	528313	50.0000	45.061	80.00- 120.00	100.00	
3.386	3.386	(0.420)	49	160158			0.00- 30.00	30.31	
3.386	3.386	(0.420)	66	155176			0.00- 30.00	29.37	

20 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
3.718	3.718	(0.461)	101	1800652	50.0000	51.786	80.00- 120.00	100.00	
3.718	3.718	(0.461)	103	1191201			36.15- 96.15	66.15	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.078	4.078	(0.506)	45	376605	50.0000	49.856	80.00- 120.00	100.00	
4.078	4.078	(0.506)	43	71167			0.00- 30.00	18.90	
4.078	4.078	(0.506)	46	162920			0.00- 30.00	43.26	

30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	1116414	50.0000	51.638	80.00- 120.00	100.00	
4.520	4.520	(0.561)	153	696975			32.43- 92.43	62.43	
4.520	4.520	(0.561)	101	1490283			103.49- 163.49	133.49	

31 1,1-Dichloroethene						CAS #: 75-35-4			
4.548	4.548	(0.564)	61	1470426	50.0000	51.389	80.00- 120.00	100.00	
4.575	4.575	(0.568)	96	794390			24.02- 84.02	54.02	
4.575	4.575	(0.568)	98	510884			4.74- 64.74	34.74	

32 Acetone						CAS #: 67-64-1			
4.713	4.713	(0.585)	58	518250	50.0000	48.423	80.00- 120.00	100.00	
4.713	4.713	(0.585)	43	1685948			0.00- 30.00	325.32	

36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	1894204	50.0000	49.732	80.00- 120.00	100.00	
4.907	4.907	(0.609)	43	427587			0.00- 30.00	22.57	
4.907	4.907	(0.609)	59	67768			0.00- 30.00	3.58	

35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	2358696	50.0000	48.677	80.00- 120.00	100.00	

38 3-Chloropropene						CAS #: 107-05-1			
5.184	5.184	(0.643)	76	370348	50.0000	45.904	80.00- 120.00	100.00	
5.184	5.184	(0.643)	41	1598103			0.00- 30.00	431.51	

43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	1352819	50.0000	55.292	80.00- 120.00	100.00	
5.432	5.432	(0.674)	84	676925			20.04- 80.04	50.04	
5.432	5.432	(0.674)	51	409791			0.00- 30.00	30.29	

46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	1098242	50.0000	59.630	80.00- 120.00	100.00	
5.764	5.764	(0.715)	57	365459			3.28- 63.28	33.28	
5.764	5.764	(0.715)	41	406766			0.00- 30.00	37.04	

47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	860571	50.0000	49.661	80.00- 120.00	100.00	
5.819	5.819	(0.722)	61	1463752			140.09- 200.09	170.09	
5.819	5.819	(0.722)	98	562091			0.00- 30.00	65.32	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	1929951	50.0000	54.767	80.00- 120.00	100.00	
6.151	6.151	(0.763)	43	1402702			0.00- 30.00	72.68	
6.151	6.151	(0.763)	86	255635			0.00- 30.00	13.25	

55 1,1-Dichloroethane						CAS #: 75-34-3			
6.594	6.594	(0.818)	63	1643598	50.0000	52.382	80.00- 120.00	100.00	
6.594	6.594	(0.818)	65	476170			0.00- 58.97	28.97	

67 2-Butanone						CAS #: 78-93-3			
7.644	7.644	(0.949)	72	369314	50.0000	48.771	80.00- 120.00	100.00	
7.644	7.644	(0.949)	43	2291218			590.40- 650.40	620.40	
7.672	7.672	(0.952)	57	154431			0.00- 30.00	41.82	

66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	1230724	50.0000	52.240	80.00- 120.00	100.00	
7.617	7.617	(0.945)	96	785083			33.79- 93.79	63.79	
7.617	7.617	(0.945)	98	500256			10.65- 70.65	40.65	

70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	1426000	50.0000	50.578	80.00- 120.00	100.00	
8.031	8.031	(0.997)	71	318833			0.00- 52.36	22.36	
8.031	8.031	(0.997)	72	344896			0.00- 30.00	24.19	

72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	1398410	50.0000	52.602	80.00- 120.00	100.00	
8.197	8.197	(1.017)	85	896421			34.10- 94.10	64.10	

75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.418	8.418	(1.045)	97	1428121	50.0000	53.744	80.00- 120.00	100.00	
8.418	8.418	(1.045)	99	935080			35.48- 95.48	65.48	

74 Cyclohexane						CAS #: 110-82-7			
8.391	8.391	(1.041)	84	1052657	50.0000	49.174	80.00- 120.00	100.00	
8.391	8.391	(1.041)	56	1837151			144.53- 204.53	174.53	
8.391	8.391	(1.041)	41	1045719			69.34- 129.34	99.34	

56 Vinyl Acetate						CAS #: 108-05-4			
6.151	6.151	(0.763)	86	255635	50.0000	64.311	80.00- 120.00	100.00	
6.151	6.151	(0.763)	43	1402702			0.00- 30.00	548.71	
6.151	6.151	(0.763)	42	690298			0.00- 30.00	270.03	

77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	1254437	50.0000	57.175	80.00- 120.00	100.00	
8.667	8.667	(1.075)	117	1335440			76.46- 136.46	106.46	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.082	9.082	(1.127)	57	5389977	50.0000	55.781	80.00- 120.00	100.00		
9.082	9.082	(1.127)	56	1737079			0.00- 30.00	32.23		
9.082	9.082	(1.127)	41	1404582			0.00- 30.00	26.06		

81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	2139091	50.0000	46.903	80.00- 120.00	100.00		
9.082	9.082	(0.916)	77	494834			0.00- 30.00	23.13		

85	1,2-Dichloroethane					CAS #: 107-06-2				
9.276	9.276	(0.936)	62	1163494	50.0000	55.687	80.00- 120.00	100.00		
9.276	9.276	(0.936)	64	357217			0.00- 30.00	30.70		

90	Heptane					CAS #: 142-82-5				
9.469	9.469	(0.955)	100	252395	50.0000	49.547	80.00- 120.00	100.00		
9.469	9.469	(0.955)	43	2195219			0.00- 30.00	869.76		
9.469	9.469	(0.955)	71	757338			0.00- 30.00	300.06		

93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	887136	50.0000	47.958	80.00- 120.00	100.00		
10.326	10.326	(1.042)	130	870346			68.11- 128.11	98.11		
10.326	10.326	(1.042)	97	572517			34.54- 94.54	64.54		

98	1,2-Dichloropropane					CAS #: 78-87-5				
10.824	10.824	(1.092)	63	871598	50.0000	48.597	80.00- 120.00	100.00		
10.824	10.824	(1.092)	62	613377			40.37- 100.37	70.37		
10.824	10.824	(1.092)	41	647710			44.31- 104.31	74.31		

99	1,4-Dioxane					CAS #: 123-91-1				
11.045	11.045	(1.114)	88	491166	50.0000	47.153	80.00- 120.00	100.00		
11.045	11.045	(1.114)	58	493587			70.49- 130.49	100.49		
11.045	11.045	(1.114)	57	155130			0.00- 30.00	31.58		

100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.151)	83	1343805	50.0000	51.958	80.00- 120.00	100.00		
11.405	11.405	(1.151)	85	854636			33.60- 93.60	63.60		

103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.289	12.289	(1.240)	75	958531	50.0000	52.292	80.00- 120.00	100.00		
12.289	12.289	(1.240)	77	292967			0.56- 60.56	30.56		
12.289	12.289	(1.240)	39	735296			46.71- 106.71	76.71		

106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.594	12.594	(1.271)	58	810881	50.0000	54.272	80.00- 120.00	100.00		
12.594	12.594	(1.271)	43	2334551			0.00- 30.00	287.90		
12.594	12.594	(1.271)	85	249132			0.00- 30.00	30.72		

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
108 Toluene						CAS #:	108-88-3			
12.815	12.815	(1.293)	91	2215977	50.0000	47.100	80.00-	120.00	100.00	
12.815	12.815	(1.293)	92	1294059			28.40-	88.40	58.40	

113 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.368	13.368	(0.891)	75	946583	50.0000	54.009	80.00-	120.00	100.00	
13.368	13.368	(0.891)	77	304258			2.14-	62.14	32.14	
13.340	13.340	(0.889)	39	672464			41.04-	101.04	71.04	

114 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.644	13.644	(0.910)	97	764165	50.0000	48.877	80.00-	120.00	100.00	
13.644	13.644	(0.910)	99	476637			32.37-	92.37	62.37	
13.644	13.644	(0.910)	83	627981			52.18-	112.18	82.18	

116 Tetrachloroethene						CAS #:	127-18-4			
13.700	13.700	(0.913)	166	930840	50.0000	51.222	80.00-	120.00	100.00	
13.672	13.672	(0.912)	129	731370			48.57-	108.57	78.57	
13.672	13.672	(0.912)	131	706433			45.89-	105.89	75.89	

119 2-Hexanone						CAS #:	591-78-6			
14.004	14.004	(0.934)	58	1116392	50.0000	51.188	80.00-	120.00	100.00	
14.004	14.004	(0.934)	43	2256460			172.12-	232.12	202.12	
14.004	14.004	(0.934)	100	160261			0.00-	30.00	14.36	

120 Dibromochloromethane						CAS #:	124-48-1			
14.197	14.197	(0.947)	129	1177748	50.0000	53.838	80.00-	120.00	100.00	
14.197	14.197	(0.947)	127	923737			0.00-	30.00	78.43	

122 1,2-Dibromoethane						CAS #:	106-93-4			
14.335	14.335	(0.956)	107	1167418	50.0000	50.941	80.00-	120.00	100.00	
14.335	14.335	(0.956)	109	1088061			63.20-	123.20	93.20	

126 Chlorobenzene						CAS #:	108-90-7			
15.027	15.027	(1.002)	112	1747847	50.0000	48.962	80.00-	120.00	100.00	
15.027	15.027	(1.002)	114	539579			0.87-	60.87	30.87	
15.027	15.027	(1.002)	77	1083318			31.98-	91.98	61.98	

128 Ethyl Benzene						CAS #:	100-41-4			
15.165	15.165	(1.011)	106	949157	50.0000	49.215	80.00-	120.00	100.00	
15.165	15.165	(1.011)	91	3206010			0.00-	30.00	337.77	

130 m,p-Xylene						CAS #:	108-38-3			
15.331	15.331	(1.022)	106	1196122	50.0000	50.495	80.00-	120.00	100.00	
15.331	15.331	(1.022)	91	2611630			0.00-	30.00	218.34	

132 o-Xylene						CAS #:	95-47-6			
15.856	15.856	(1.057)	106	1160150	50.0000	51.504	80.00-	120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	2590775			193.31- 253.31	223.31	

133 Styrene CAS #: 100-42-5									
15.911	15.911	(1.061)	104	1676957	50.0000	50.494	80.00- 120.00	100.00	
15.884	15.884	(1.059)	78	937291			25.89- 85.89	55.89	

134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1049310	50.0000	53.824	80.00- 120.00	100.00	
16.160	16.160	(1.077)	171	537657			21.24- 81.24	51.24	

141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	1665282	50.0000	49.022	80.00- 120.00	100.00	
16.796	16.796	(1.120)	85	1070476			34.28- 94.28	64.28	

144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	3707756	50.0000	55.787	80.00- 120.00	100.00	
16.962	16.962	(1.131)	120	1059561			0.00- 58.58	28.58	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	3266640	50.0000	54.377	80.00- 120.00	100.00	
17.045	17.045	(1.136)	120	1525075			0.00- 30.00	46.69	

152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	2661146	50.0000	52.219	80.00- 120.00	100.00	
17.460	17.460	(1.164)	120	1185597			14.55- 74.55	44.55	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	1686195	50.0000	46.737	80.00- 120.00	100.00	
17.764	17.764	(1.184)	148	1061901			0.00- 30.00	62.98	
17.736	17.736	(1.182)	111	732798			0.00- 30.00	43.46	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	2220296	50.0000	52.510	80.00- 120.00	100.00	
17.847	17.847	(1.190)	148	1393939			0.00- 30.00	62.78	
17.847	17.847	(1.190)	111	930025			0.00- 30.00	41.89	

157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	3064410	50.0000	57.556	80.00- 120.00	100.00	
17.985	17.985	(1.199)	126	611306			0.00- 30.00	19.95	

159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	1756514	50.0000	46.290	80.00- 120.00	100.00	
18.206	18.206	(1.214)	148	1110305			33.21- 93.21	63.21	
18.206	18.206	(1.214)	111	712635			10.57- 70.57	40.57	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.478	19.478	(1.299)	180	1249087	50.0000	46.374	80.00- 120.00	100.00	
19.478	19.478	(1.299)	182	1191180			65.36- 125.36	95.36	

164	Hexachlorobutadiene					CAS #: 87-68-3			
19.561	19.561	(1.304)	225	927614	50.0000	49.020	80.00- 120.00	100.00	
19.561	19.561	(1.304)	223	563285			30.72- 90.72	60.72	

142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	4302601	50.0000	55.004	80.00- 120.00	100.00	
16.824	16.824	(1.122)	120	909968			0.00- 30.00	21.15	
16.824	16.824	(1.122)	105	150046			0.00- 30.00	3.49	

136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	3494489	50.0000	51.165	80.00- 120.00	100.00	
16.326	16.326	(1.088)	120	916960			0.00- 30.00	26.24	
16.326	16.326	(1.088)	51	513188			0.00- 30.00	14.69	

165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	5030763	50.0000	56.079	80.00- 120.00	100.00	
19.672	19.672	(1.312)	127	621314			0.00- 30.00	12.35	

17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	1820518	50.0000	54.524	80.00- 120.00	100.00	
3.414	3.414	(0.424)	57	1122039			0.00- 30.00	61.63	
3.414	3.414	(0.424)	72	99749			0.00- 30.00	5.48	

11	Butane					CAS #: 106-97-8			
2.667	2.667	(0.331)	58	285739	50.0000	50.195	80.00- 120.00	100.00	
2.667	2.667	(0.331)	43	2284054			0.00- 30.00	799.35	

94	Methyl Cyclohexane					CAS #: 108-87-2			
10.547	10.547	(1.064)	83	1290165	50.0000	48.978	80.00- 120.00	100.00	
10.547	10.547	(1.064)	98	636626			0.00- 30.00	49.34	
10.547	10.547	(1.064)	55	1535923			0.00- 30.00	119.05	

Report Date: 28-Dec-2007 09:47

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 28-DEC-2007

Lab File ID: 5122803.d

Calibration Time: 09:05

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /var/chem/msd5.i/5-28dec.b/t14qn12c.m

Misc Info: 50ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	355417	213250	497584	269712	-24.11
92 1,4-Difluorobenze	1305801	783481	1828121	1058104	-18.97
125 Chlorobenzene-d5	1002859	601715	1404003	829571	-17.28

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-28dec.b/5122803.d
Date: 28-DEC-2007 09:33
Client ID: CCV-1
Sample Info: 50mL #1443-379

Column phase: RTX-624

Instrument: msd5.1
Operator: cb
Column diameter: 0.53

/chem/msd5.1/5-28dec.b/5122803.d





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0712439-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122804	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 12/28/07 10:01 AM

Compound	%Recovery
Freon 12	103
Freon 114	106
Vinyl Chloride	104
Bromomethane	101
Chloroethane	95
Freon 11	112
1,1-Dichloroethene	121
Freon 113	122
Methylene Chloride	124
1,1-Dichloroethane	115
cis-1,2-Dichloroethene	113
Chloroform	114
1,1,1-Trichloroethane	118
Carbon Tetrachloride	123
Benzene	104
1,2-Dichloroethane	121
Trichloroethene	105
1,2-Dichloropropane	104
cis-1,3-Dichloropropene	109
Toluene	108
trans-1,3-Dichloropropene	119
1,1,2-Trichloroethane	107
Tetrachloroethene	107
1,2-Dibromoethane (EDB)	105
Chlorobenzene	105
Ethyl Benzene	104
m,p-Xylene	110
o-Xylene	109
Styrene	111
1,1,2,2-Tetrachloroethane	105
1,3,5-Trimethylbenzene	119
1,2,4-Trimethylbenzene	114
1,3-Dichlorobenzene	100
1,4-Dichlorobenzene	111
alpha-Chlorotoluene	133 Q
1,2-Dichlorobenzene	97
1,3-Butadiene	114
Hexane	118
Cyclohexane	104



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0712439-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5122804	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 12/28/07 10:01 AM

Compound	%Recovery
Heptane	110
Bromodichloromethane	112
Dibromochloromethane	116
Cumene	111
Propylbenzene	118
Chloromethane	113
1,2,4-Trichlorobenzene	104
Hexachlorobutadiene	104
Acetone	115
Carbon Disulfide	102
2-Propanol	112
trans-1,2-Dichloroethene	108
2-Butanone (Methyl Ethyl Ketone)	97
Tetrahydrofuran	106
1,4-Dioxane	104
4-Methyl-2-pentanone	122
2-Hexanone	107
Bromoform	116
4-Ethyltoluene	121
Ethanol	126
Methyl tert-butyl ether	126
3-Chloropropene	102
2,2,4-Trimethylpentane	117
Naphthalene	116

Q = Exceeds Quality Control limits.

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	102	70-130
1,2-Dichloroethane-d4	108	70-130
4-Bromofluorobenzene	105	70-130

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-28dec
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: cb
 Data Type: MS DATA SampleType: LCS
 SpikeList File: 2926Spectra.spk Quant Type: ISTD
 Sublist File: AT04ENSR.sub
 Method File: /var/chem/msd5.i/5-28dec.b/t14qn12c.m
 Misc Info: 50ppbv (200ppbv)

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
8 Dichlorodifluorome	50.000	51.691	103.38	70-130
9 Freon 114	50.000	53.134	106.27	70-130
10 Chloromethane	50.000	56.634	113.27	70-130
13 Vinyl Chloride	50.000	52.094	104.19	70-130
12 1,3-Butadiene	50.000	57.154	114.31	60-140
15 Bromomethane	50.000	50.437	100.87	70-130
19 Chloroethane	50.000	47.603	95.21	70-130
20 Trichlorofluoromet	50.000	55.965	111.93	70-130
26 Ethanol	50.000	63.145	126.29	60-140
30 Freon 113	50.000	60.980	121.96	70-130
31 1,1-Dichloroethene	50.000	60.615	121.23	70-130
35 Carbon Disulfide	50.000	51.192	102.38	60-140
32 Acetone	50.000	57.554	115.11	60-140
36 2-Propanol	50.000	56.037	112.07	60-140
38 3-Chloropropene	50.000	51.222	102.44	60-140
43 Methylene Chloride	50.000	62.010	124.02	70-130
46 MTBE	50.000	63.189	126.38	60-140
47 trans-1,2-Dichloro	50.000	54.006	108.01	60-140
51 Hexane	50.000	59.276	118.55	60-140
55 1,1-Dichloroethane	50.000	57.492	114.98	70-130
66 cis-1,2-Dichloroet	50.000	56.456	112.91	70-130
67 2-Butanone	50.000	48.485	96.97	60-140
70 Tetrahydrofuran	50.000	52.766	105.53	60-140
72 Chloroform	50.000	57.081	114.16	70-130
74 Cyclohexane	50.000	52.064	104.13	60-140
75 1,1,1-Trichloroeth	50.000	58.973	117.95	70-130
56 Vinyl Acetate	50.000	64.281	128.56	60-140
77 Carbon Tetrachlori	50.000	61.645	123.29	70-130
80 2,2,4-Trimethylpen	50.000	58.670	117.34	60-140
81 Benzene	50.000	52.082	104.16	70-130
85 1,2-Dichloroethane	50.000	60.593	121.19	70-130
90 Heptane	50.000	55.016	110.03	60-140
93 Trichloroethene	50.000	52.412	104.82	70-130

Report Date: 28-Dec-2007 10:09

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
98 1,2-Dichloropropan	50.000	52.121	104.24	70-130
99 1,4-Dioxane	50.000	52.245	104.49	60-140
100 Bromodichlorometha	50.000	56.018	112.04	60-140
103 cis-1,3-Dichloropr	50.000	54.495	108.99	70-130
106 4-Methyl-2-pentano	50.000	61.108	122.22	60-140
108 Toluene	50.000	53.774	107.55	70-130
113 trans-1,3-Dichloro	50.000	59.412	118.82	70-130
114 1,1,2-Trichloroeth	50.000	53.567	107.13	70-130
116 Tetrachloroethene	50.000	53.597	107.19	70-130
119 2-Hexanone	50.000	53.695	107.39	60-140
120 Dibromochlorometha	50.000	58.078	116.16	60-140
122 1,2-Dibromoethane	50.000	52.429	104.86	70-130
126 Chlorobenzene	50.000	52.414	104.83	70-130
128 Ethyl Benzene	50.000	52.223	104.45	70-130
130 m,p-Xylene	50.000	55.175	110.35	70-130
132 o-Xylene	50.000	54.459	108.92	70-130
133 Styrene	50.000	55.529	111.06	70-130
134 Bromoform	50.000	58.089	116.18	60-140
136 Cumene	50.000	55.500	111.00	60-140
141 1,1,2,2-Tetrachlor	50.000	52.526	105.05	70-130
142 Propylbenzene	50.000	59.252	118.50	60-140
144 4-Ethyltoluene	50.000	60.621	121.24	60-140
147 1,3,5-Trimethylben	50.000	59.498	119.00	70-130
152 1,2,4-Trimethylben	50.000	56.799	113.60	70-130
155 1,3-Dichlorobenzen	50.000	50.141	100.28	70-130
156 1,4-Dichlorobenzen	50.000	55.601	111.20	70-130
157 alpha-Chlorotoluen	50.000	66.372	132.74*	70-130
159 1,2-Dichlorobenzen	50.000	48.390	96.78	70-130
163 1,2,4-Trichloroben	50.000	52.037	104.07	70-130
164 Hexachlorobutadien	50.000	51.856	103.71	70-130
6 Propylene	50.000	58.238	116.48	70-130
165 Naphthalene	50.000	57.800	115.60	60-140
11 Butane	50.000	54.806	109.61	70-130
17 Isopentane	50.000	55.860	111.72	70-130
94 Methyl Cyclohexane	50.000	54.062	108.12	70-130

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	27.032	108.13	70-130
\$ 107 Toluene-d8	25.000	25.558	102.23	70-130
\$ 138 Bromofluorobenzene	25.000	26.232	104.93	70-130

Report Date: 28-Dec-2007 10:09

Air Toxics Ltd.

AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-28dec.b/5122804.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 28-DEC-2007 10:01
 Operator : cb Inst ID: msd5.i
 Smp Info : 50mL #1576-171
 Misc Info : 50ppbv (200ppbv)
 Comment :
 Method : /var/chem/msd5.i/5-28dec.b/t14qn12c.m
 Meth Date : 28-Dec-2007 09:47 cbond Quant Type: ISTD
 Cal Date : 27-NOV-2007 12:08 Cal File: 5112707.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				(PPBV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5								
8.059	8.059	(1.000)	130	276210	25.0000	80.00- 120.00	100.00	
8.059	8.059	(1.000)	128	215940		50.29- 110.29	78.18	
8.031	8.031	(1.000)	49	638051		207.42- 267.42	231.00	

* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.911	9.912	(1.000)	114	1061667	25.0000	80.00- 120.00	100.00	
9.911	9.912	(1.000)	88	178724		0.00- 47.33	16.83	

* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	838490	25.0000	80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	483659		0.00- 30.00	57.68	

\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.110	9.110	(1.130)	65	446914	27.0321	27.032 80.00- 120.00	100.00	
9.110	9.110	(1.130)	67	246145		27.88- 87.88	55.08	

\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.676	12.677	(1.279)	98	957963	25.5577	25.558 80.00- 120.00	100.00	
12.676	12.677	(1.279)	70	97266		0.00- 40.29	10.15	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

\$ 107 Toluene-d8 (continued)

12.676 12.677 (1.279) 100 641724 37.87- 97.87 66.99

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575 16.575 (1.105) 174 513223 26.2323 26.232 80.00- 120.00 100.00

16.575 16.575 (1.105) 95 774952 122.99- 182.99 151.00

16.575 16.575 (1.105) 176 499760 64.86- 124.86 97.38

6 Propylene

CAS #: 115-07-1

2.280 2.280 (0.283) 41 1122786 58.2384 58.238 80.00- 120.00 100.00

2.280 2.280 (0.283) 42 754874 0.00- 30.00 67.23

2.280 2.280 (0.283) 39 724705 0.00- 30.00 64.55

8 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.335 2.336 (0.290) 85 1688238 51.6913 51.691 80.00- 120.00 100.00

2.335 2.336 (0.290) 87 540482 0.00- 30.00 32.01

9 Freon 114

CAS #: 76-14-2

2.446 2.446 (0.304) 135 1583721 53.1340 53.134 80.00- 120.00 100.00

2.446 2.446 (0.304) 137 486558 1.90- 61.90 30.72

10 Chloromethane

CAS #: 74-87-3

2.584 2.584 (0.321) 50 1388900 56.6343 56.634 80.00- 120.00 100.00

2.584 2.584 (0.321) 52 433136 0.00- 30.00 31.19

13 Vinyl Chloride

CAS #: 75-01-4

2.778 2.778 (0.345) 62 1229675 52.0942 52.094 80.00- 120.00 100.00

2.778 2.778 (0.345) 64 363901 0.00- 30.00 29.59

12 1,3-Butadiene

CAS #: 106-99-0

2.750 2.750 (0.341) 54 1152193 57.1545 57.154 80.00- 120.00 100.00

2.750 2.750 (0.341) 39 1206543 0.00- 30.00 104.72

15 Bromomethane

CAS #: 74-83-9

3.276 3.276 (0.406) 94 768616 50.4372 50.437 80.00- 120.00 100.00

3.276 3.276 (0.406) 96 742090 66.07- 126.07 96.55

19 Chloroethane

CAS #: 75-00-3

3.386 3.386 (0.420) 64 571570 47.6035 47.603 80.00- 120.00 100.00

3.386 3.386 (0.420) 49 175246 0.00- 30.00 30.66

3.386 3.386 (0.420) 66 169103 0.00- 30.00 29.59

20 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.718 3.718 (0.461) 101 1992816 55.9647 55.965 80.00- 120.00 100.00

3.718 3.718 (0.461) 103 1269853 36.15- 96.15 63.72

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPBV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

26 Ethanol CAS #: 64-17-5
 4.077 4.078 (0.506) 45 488475 63.1448 63.145 80.00- 120.00 100.00
 4.077 4.078 (0.506) 43 85249 0.00- 30.00 17.45
 4.077 4.078 (0.506) 46 203761 0.00- 30.00 41.71

30 Freon 113 CAS #: 76-13-1
 4.520 4.520 (0.561) 151 1350159 60.9798 60.980 80.00- 120.00 100.00
 4.520 4.520 (0.561) 153 867111 32.43- 92.43 64.22
 4.520 4.520 (0.561) 101 1781606 103.49- 163.49 131.96

31 1,1-Dichloroethene CAS #: 75-35-4
 4.547 4.548 (0.564) 61 1776181 60.6148 60.615 80.00- 120.00 100.00
 4.575 4.575 (0.568) 96 944257 24.02- 84.02 53.16
 4.575 4.575 (0.568) 98 612004 4.74- 64.74 34.46

32 Acetone CAS #: 67-64-1
 4.713 4.713 (0.585) 58 630807 57.5536 57.554 80.00- 120.00 100.00
 4.713 4.713 (0.585) 43 1874291 0.00- 30.00 297.13

36 2-Propanol CAS #: 67-63-0
 4.907 4.907 (0.609) 45 2185762 56.0371 56.037 80.00- 120.00 100.00
 4.907 4.907 (0.609) 43 496757 0.00- 30.00 22.73
 4.907 4.907 (0.609) 59 79704 0.00- 30.00 3.65

35 Carbon Disulfide CAS #: 75-15-0
 4.907 4.907 (0.609) 76 2540297 51.1916 51.192 80.00- 120.00 100.00

38 3-Chloropropene CAS #: 107-05-1
 5.183 5.184 (0.643) 76 423212 51.2219 51.222 80.00- 120.00 100.00
 5.183 5.184 (0.643) 41 1793395 0.00- 30.00 423.76

43 Methylene Chloride CAS #: 75-09-2
 5.432 5.432 (0.674) 49 1553736 62.0102 62.010 80.00- 120.00 100.00
 5.432 5.432 (0.674) 84 809996 20.04- 80.04 52.13
 5.432 5.432 (0.674) 51 477743 0.00- 30.00 30.75

46 MTBE CAS #: 1634-04-4
 5.764 5.764 (0.715) 73 1191842 63.1893 63.189 80.00- 120.00 100.00
 5.764 5.764 (0.715) 57 405848 3.28- 63.28 34.05
 5.764 5.764 (0.715) 41 427273 0.00- 30.00 35.85

47 trans-1,2-Dichloroethene CAS #: 156-60-5
 5.819 5.819 (0.722) 96 958430 54.0066 54.006 80.00- 120.00 100.00
 5.819 5.819 (0.722) 61 1622234 140.09- 200.09 169.26
 5.819 5.819 (0.722) 98 596327 0.00- 30.00 62.22

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

51 Hexane CAS #: 110-54-3
 6.151 6.151 (0.763) 57 2139151 59.2758 59.276 80.00- 120.00 100.00
 6.151 6.151 (0.763) 43 1508342 0.00- 30.00 70.51
 6.151 6.151 (0.763) 86 261671 0.00- 30.00 12.23

55 1,1-Dichloroethane CAS #: 75-34-3
 6.593 6.594 (0.818) 63 1847374 57.4919 57.492 80.00- 120.00 100.00
 6.593 6.594 (0.818) 65 554905 0.00- 58.97 30.04

67 2-Butanone CAS #: 78-93-3
 7.644 7.644 (0.949) 72 375994 48.4853 48.485 80.00- 120.00 100.00
 7.644 7.644 (0.949) 43 2510219 590.40- 650.40 667.62
 7.644 7.672 (0.949) 57 172818 0.00- 30.00 45.96

66 cis-1,2-Dichloroethene CAS #: 156-59-2
 7.617 7.617 (0.945) 61 1362077 56.4556 56.456 80.00- 120.00 100.00
 7.617 7.617 (0.945) 96 862087 33.79- 93.79 63.29
 7.617 7.617 (0.945) 98 548966 10.65- 70.65 40.30

70 Tetrahydrofuran CAS #: 109-99-9
 8.031 8.031 (0.997) 42 1523559 52.7665 52.766 80.00- 120.00 100.00
 8.031 8.031 (0.997) 71 336752 0.00- 52.36 22.10
 8.031 8.031 (0.997) 72 382968 0.00- 30.00 25.14

72 Chloroform CAS #: 67-66-3
 8.197 8.197 (1.017) 83 1554026 57.0808 57.081 80.00- 120.00 100.00
 8.197 8.197 (1.017) 85 1018199 34.10- 94.10 65.52

75 1,1,1-Trichloroethane CAS #: 71-55-6
 8.418 8.418 (1.045) 97 1604825 58.9727 58.973 80.00- 120.00 100.00
 8.418 8.418 (1.045) 99 1048638 35.48- 95.48 65.34

74 Cyclohexane CAS #: 110-82-7
 8.391 8.391 (1.041) 84 1141380 52.0642 52.064 80.00- 120.00 100.00
 8.391 8.391 (1.041) 56 1989624 144.53- 204.53 174.32
 8.391 8.391 (1.041) 41 1127486 69.34- 129.34 98.78

56 Vinyl Acetate CAS #: 108-05-4
 6.151 6.151 (0.763) 86 261671 64.2807 64.281 80.00- 120.00 100.00
 6.151 6.151 (0.763) 43 1508342 0.00- 30.00 576.43
 6.151 6.151 (0.763) 42 773024 0.00- 30.00 295.42

77 Carbon Tetrachloride CAS #: 56-23-5
 8.667 8.667 (1.075) 119 1385087 61.6451 61.645 80.00- 120.00 100.00
 8.667 8.667 (1.075) 117 1438696 76.46- 136.46 103.87

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO	
				(PPEV)	(PPEV)	(PPEV)	(PPEV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	

80	2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.082	9.082	(1.127)	57	5805748	58.6700	58.670	80.00-	120.00	100.00	
9.082	9.082	(1.127)	56	1914323			0.00-	30.00	32.97	
9.082	9.082	(1.127)	41	1551035			0.00-	30.00	26.72	

81	Benzene						CAS #: 71-43-2			
9.082	9.082	(0.916)	78	2383287	52.0817	52.082	80.00-	120.00	100.00	
9.082	9.082	(0.916)	77	547947			0.00-	30.00	22.99	

85	1,2-Dichloroethane						CAS #: 107-06-2			
9.248	9.276	(0.933)	62	1270262	60.5931	60.593	80.00-	120.00	100.00	
9.275	9.276	(0.936)	64	402766			0.00-	30.00	31.71	

90	Heptane						CAS #: 142-82-5			
9.469	9.469	(0.955)	100	281195	55.0158	55.016	80.00-	120.00	100.00	
9.469	9.469	(0.955)	43	2432908			0.00-	30.00	865.20	
9.469	9.469	(0.955)	71	823059			0.00-	30.00	292.70	

93	Trichloroethene						CAS #: 79-01-6			
10.326	10.326	(1.042)	95	972800	52.4122	52.412	80.00-	120.00	100.00	
10.326	10.326	(1.042)	130	924476			68.11-	128.11	95.03	
10.326	10.326	(1.042)	97	619102			34.54-	94.54	63.64	

98	1,2-Dichloropropane						CAS #: 78-87-5			
10.824	10.824	(1.092)	63	937958	52.1214	52.121	80.00-	120.00	100.00	
10.824	10.824	(1.092)	62	656414			40.37-	100.37	69.98	
10.824	10.824	(1.092)	41	692290			44.31-	104.31	73.81	

99	1,4-Dioxane						CAS #: 123-91-1			
11.045	11.045	(1.114)	88	546039	52.2450	52.245	80.00-	120.00	100.00	
11.045	11.045	(1.114)	58	527878			70.49-	130.49	96.67	
11.045	11.045	(1.114)	57	162471			0.00-	30.00	29.75	

100	Bromodichloromethane						CAS #: 75-27-4			
11.404	11.405	(1.151)	83	1453685	56.0184	56.018	80.00-	120.00	100.00	
11.404	11.405	(1.151)	85	936293			33.60-	93.60	64.41	

103	cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.317	12.289	(1.243)	75	1002266	54.4946	54.495	80.00-	120.00	100.00	
12.317	12.289	(1.243)	77	317897			0.56-	60.56	31.72	
12.289	12.289	(1.240)	39	803165			46.71-	106.71	80.13	

106	4-Methyl-2-pentanone						CAS #: 108-10-1			
12.593	12.594	(1.271)	58	916096	61.1077	61.108	80.00-	120.00	100.00	
12.593	12.594	(1.271)	43	2561364			0.00-	30.00	279.60	
12.593	12.594	(1.271)	85	272865			0.00-	30.00	29.79	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

108	Toluene					CAS #: 108-88-3			
12.815	12.815	(1.293)	91	2538527	53.7741	53.774	80.00- 120.00	100.00	
12.815	12.815	(1.293)	92	1489856			28.40- 88.40	58.69	

113	trans-1,3-Dichloropropene					CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	1052474	59.4117	59.412	80.00- 120.00	100.00	
13.368	13.368	(0.891)	77	340104			2.14- 62.14	32.31	
13.340	13.340	(0.889)	39	756437			41.04- 101.04	71.87	

114	1,1,2-Trichloroethane					CAS #: 79-00-5			
13.644	13.644	(0.910)	97	846496	53.5675	53.567	80.00- 120.00	100.00	
13.644	13.644	(0.910)	99	516703			32.37- 92.37	61.04	
13.644	13.644	(0.910)	83	677910			52.18- 112.18	80.08	

116	Tetrachloroethene					CAS #: 127-18-4			
13.699	13.700	(0.913)	166	984469	53.5972	53.597	80.00- 120.00	100.00	
13.672	13.672	(0.912)	129	808057			48.57- 108.57	82.08	
13.672	13.672	(0.912)	131	788066			45.89- 105.89	80.05	

119	2-Hexanone					CAS #: 591-78-6			
14.004	14.004	(0.934)	58	1183661	53.6955	53.695	80.00- 120.00	100.00	
14.004	14.004	(0.934)	43	2486505			172.12- 232.12	210.07	
14.004	14.004	(0.934)	100	166575			0.00- 30.00	14.07	

120	Dibromochloromethane					CAS #: 124-48-1			
14.197	14.197	(0.947)	129	1284167	58.0783	58.078	80.00- 120.00	100.00	
14.197	14.197	(0.947)	127	1011492			0.00- 30.00	78.77	

122	1,2-Dibromoethane					CAS #: 106-93-4			
14.335	14.335	(0.956)	107	1214441	52.4291	52.429	80.00- 120.00	100.00	
14.363	14.335	(0.958)	109	1156767			63.20- 123.20	95.25	

126	Chlorobenzene					CAS #: 108-90-7			
15.027	15.027	(1.002)	112	1891177	52.4136	52.414	80.00- 120.00	100.00	
15.027	15.027	(1.002)	114	605123			0.87- 60.87	32.00	
15.027	15.027	(1.002)	77	1170212			31.98- 91.98	61.88	

128	Ethyl Benzene					CAS #: 100-41-4			
15.165	15.165	(1.011)	106	1018009	52.2235	52.223	80.00- 120.00	100.00	
15.165	15.165	(1.011)	91	3421081			0.00- 30.00	336.06	

130	m,p-Xylene					CAS #: 108-38-3			
15.331	15.331	(1.022)	106	1321031	55.1754	55.175	80.00- 120.00	100.00	
15.331	15.331	(1.022)	91	2823795			0.00- 30.00	213.76	

132	o-Xylene					CAS #: 95-47-6			
15.856	15.856	(1.057)	106	1239908	54.4593	54.459	80.00- 120.00	100.00	

CONCENTRATIONS

RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
132 o-Xylene (continued)								
15.856	15.856	(1.057)	91	2847177			193.31- 253.31	229.63

133 Styrene CAS #: 100-42-5								
15.911	15.911	(1.061)	104	1864010	55.5292	55.529	80.00- 120.00	100.00
15.884	15.884	(1.059)	78	1043698			25.89- 85.89	55.99

134 Bromoform CAS #: 75-25-2								
16.160	16.160	(1.077)	173	1144618	58.0888	58.089	80.00- 120.00	100.00
16.160	16.160	(1.077)	171	592035			21.24- 81.24	51.72

141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5								
16.796	16.796	(1.120)	83	1803515	52.5260	52.526	80.00- 120.00	100.00
16.796	16.796	(1.120)	85	1146048			34.28- 94.28	63.55

144 4-Ethyltoluene CAS #: 622-96-8								
16.962	16.962	(1.131)	105	4072302	60.6207	60.621	80.00- 120.00	100.00
16.962	16.962	(1.131)	120	1174560			0.00- 58.58	28.84

147 1,3,5-Trimethylbenzene CAS #: 108-67-8								
17.045	17.045	(1.136)	105	3612751	59.4984	59.498	80.00- 120.00	100.00
17.045	17.045	(1.136)	120	1666850			0.00- 30.00	46.14

152 1,2,4-Trimethylbenzene CAS #: 95-63-6								
17.460	17.460	(1.164)	105	2925689	56.7991	56.799	80.00- 120.00	100.00
17.460	17.460	(1.164)	120	1317076			14.55- 74.55	45.02

155 1,3-Dichlorobenzene CAS #: 541-73-1								
17.764	17.764	(1.184)	146	1828457	50.1414	50.141	80.00- 120.00	100.00
17.764	17.764	(1.184)	148	1151647			0.00- 30.00	62.98
17.764	17.736	(1.184)	111	778174			0.00- 30.00	42.56

156 1,4-Dichlorobenzene CAS #: 106-46-7								
17.847	17.847	(1.190)	146	2376292	55.6015	55.601	80.00- 120.00	100.00
17.847	17.847	(1.190)	148	1512078			0.00- 30.00	63.63
17.847	17.847	(1.190)	111	990277			0.00- 30.00	41.67

157 alpha-Chlorotoluene CAS #: 100-44-7								
17.985	17.985	(1.199)	91	3571813	66.3721	66.372	80.00- 120.00	100.00(R)
17.985	17.985	(1.199)	126	716440			0.00- 30.00	20.06

159 1,2-Dichlorobenzene CAS #: 95-50-1								
18.206	18.206	(1.214)	146	1855954	48.3900	48.390	80.00- 120.00	100.00
18.206	18.206	(1.214)	148	1193706			33.21- 93.21	64.32
18.206	18.206	(1.214)	111	765737			10.57- 70.57	41.26

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

163	1,2,4-Trichlorobenzene					CAS #:	120-82-1			
19.478	19.478	(1.299)	180	1416673	52.0369	52.037	80.00- 120.00	100.00		
19.478	19.478	(1.299)	182	1308800			65.36- 125.36	92.39		

164	Hexachlorobutadiene					CAS #:	87-68-3			
19.589	19.561	(1.306)	225	991834	51.8562	51.856	80.00- 120.00	100.00		
19.589	19.561	(1.306)	223	617939			30.72- 90.72	62.30		

142	Propylbenzene					CAS #:	103-65-1			
16.824	16.824	(1.122)	91	4684653	59.2516	59.252	80.00- 120.00	100.00		
16.824	16.824	(1.122)	120	989056			0.00- 30.00	21.11		
16.824	16.824	(1.122)	105	163672			0.00- 30.00	3.49		

136	Cumene					CAS #:	98-82-8			
16.326	16.326	(1.088)	105	3831352	55.5005	55.500	80.00- 120.00	100.00		
16.326	16.326	(1.088)	120	1028868			0.00- 30.00	26.85		
16.326	16.326	(1.088)	51	581335			0.00- 30.00	15.17		

165	Naphthalene					CAS #:	91-20-3			
19.672	19.672	(1.312)	128	5240863	57.7995	57.800	80.00- 120.00	100.00		
19.672	19.672	(1.312)	127	641238			0.00- 30.00	12.24		

17	Isopentane					CAS #:	78-78-4			
3.414	3.414	(0.424)	43	1910054	55.8600	55.860	80.00- 120.00	100.00		
3.414	3.414	(0.424)	57	1192475			0.00- 30.00	62.43		
3.414	3.414	(0.424)	72	106146			0.00- 30.00	5.56		

11	Butane					CAS #:	106-97-8			
2.667	2.667	(0.331)	58	319505	54.8060	54.806	80.00- 120.00	100.00		
2.667	2.667	(0.331)	43	2510324			0.00- 30.00	785.69		

94	Methyl Cyclohexane					CAS #:	108-87-2			
10.547	10.547	(1.064)	83	1428863	54.0618	54.062	80.00- 120.00	100.00		
10.547	10.547	(1.064)	98	704323			0.00- 30.00	49.29		
10.547	10.547	(1.064)	55	1725061			0.00- 30.00	120.73		

QC Flag Legend

R - Spike/Surrogate failed recovery limits.

Report Date: 28-Dec-2007 10:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 28-DEC-2007

Lab File ID: 5122804.d

Calibration Time: 09:33

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: cb

Method File: /var/chem/msd5.i/5-28dec.b/t14qn12c.m

Misc Info: 50ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	269712	161827	377597	276210	2.41
92 1,4-Difluorobenze	1058104	634862	1481346	1061667	0.34
125 Chlorobenzene-d5	829571	497743	1161399	838490	1.08


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	28.29
75	30.0 - 60.0% of mass 95	47.21
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.42
173	Less than 2.0% of mass 174	(0.68) ¹
174	Greater than 50.0% of mass 95	60.73
175	5.0 - 9.0% of mass 174	(7.35) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(98.25) ¹
177	5.0 - 9.0% of mass 176	(6.51) ²

¹ - value in parenthesis is % mass 174 ² - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio: $\frac{100.00}{100.00} / \frac{100.00}{100.00} = 1.00 = 98.25\%$

BFB Injection Date: 12/28/07
 BFB Injection Time: 0840
 BFB File ID: 5122801
 Tekmar Purge Flow: 12.5 mL/min
 Vacuum: 3.20 x 10⁻⁶ Torr

IS/Std #:	<u>1576-131</u>	Exp. Date:	<u>2-26-08</u>
BCM	<u>269712</u>		
1,4-DFB	<u>1058104</u>		
CB-d5	<u>829571</u>		

Verified CCV IS vs ICAL mid-point (-40%AD) CB

NOAH Cart #: 8 /

File #: 5122805 /

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{Sample}}}{\text{Area}_{\text{Std}}} \times \frac{\text{Conc}_{\text{Std}}}{\text{RRF}}$

$= \frac{943100}{1058104} \times \frac{25.0}{0.98263} = 25.246$

Reported Result: 25.246

File ID:	<u>5122803</u>
Compound:	<u>Toluene-d8</u>
Initials:	<u>CB</u>

Sl. #	File #	Sample / Client Name	Can #	Pressure	Amnt Loaded	DR	Date Analyzed	Time Analyzed	Recovery Init	Comments
1	✓ 5122801	BFB Tune Check	1476-65	50mg	2ul	1.00	12/28/07	0840	CB	
2	✓ 02	CONSP (200µg)	1443-340	50µg	50µl			0905	CB	sp2lb con
3	✓ 03	CON-1 (200µg)	1443-374					0933	CB	
4	✓ 04	US-1 (200µg)	1574-171					1001	CB	
5	✓ 05	Lab Blank	13673	Hand	200µl			1058	CB	Car Cart #8 Log 3
6	X 06	Car Cart #7 Log 6	1					1144	CB	
7	✓ 07	Car Cart #14 Log 6						1350	CB	
8	✓ 08	8125224 - 02A	34455	35M 4µg	200µl	1.73		1445	CB	
9	✓ 09	04M	4385	70µg		1.75		1518	CB	
10	✓ 10	04M	4385	70µg		1.75		1548	CB	

11	✓	ST22811	0712522A-014A	91003	35 th -5 th	51002	310	12/29/17	1602	44
12	✓	12	08A	33871	115 th	90002	3E0		1600	44
13	✓	13	09A	4195	↓	30000	114		1378	44
14	✓	14	0712136A-01A	35973	135 th	REO00	244		1750	44
15	✓	15	01A	↓	↓		↓		1823	44
16	✓	16	02A	33509	205 th		423		1855	44
17	✓	17	03A	34202	120 th		124		1928	44
18	✓	18	07121402-01A	34721	35 th -5 th	20000	152		2010	44
19	✓	19	0712127A-01A	34407	115 th		141		2052	44
20	✓	20	01A	↓	↓		↓		2125	44
21	✓	21	02A	34407	20 th		141		2157	44
22	✓	22	03A	34202	10 th		139		2230	44
23	✓	23	04A	21008	45 th		158		2302	44
24	✓	24	07121431-01A	34208	02 th		134		2335	44
25	✓	25	02A	34312	45 th		158	12/29/17	0008	44
26	✓	26	07121351-01A	94191	85 th		153		0040	44
27	✓	27	01A	↓	↓		↓		0113	44
28										
29										
30										
31										
32										

Comments:

Signature

[Handwritten Signature]

Date

12/31/17

CG 12/31/17

Report Date: 12-Nov-2007 11:56

Air Toxics Ltd.

Data file : /chem/msd5.i/5-12nov.b/5111205.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 12-NOV-2007 12:01
 Operator : cb Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2ul #1476-65 50 ng
 Comment :
 Method : /var/chem/msd5.i/5-12nov.b/bfb30.m
 Meth Date : 12-Nov-2007 11:51 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	====	=====	=====	=====	=====

1 bfb

CAS #: 460-00-4

3.803	3.900	-0.097	95	996608		100.00- 100.00	100.00
3.803	3.900	-0.097	50	261056		15.00- 40.00	26.19
3.803	3.900	-0.097	75	425344		30.00- 60.00	42.68
3.803	3.900	-0.097	96	63608		5.00- 9.00	6.38
3.803	3.900	-0.097	173	6008		0.00- 2.00	0.85
3.803	3.900	-0.097	174	705472		50.00- 100.00	70.79
3.803	3.900	-0.097	175	51496		5.00- 9.00	7.30
3.803	3.900	-0.097	176	681408		95.00- 101.00	96.59
3.803	3.900	-0.097	177	42960		5.00- 9.00	6.30

Date : 12-NOV-2007 12:01

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00



Date : 12-NOV-2007 12:01

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	26.19
75	30.00 - 60.00% of mass 95	42.68
96	5.00 - 9.00% of mass 95	6.38
173	Less than 2.00% of mass 174	0.60 (0.85)
174	50.00 - 100.00% of mass 95	70.79
175	5.00 - 9.00% of mass 174	5.17 (7.30)
176	95.00 - 101.00% of mass 174	68.37 (96.59)
177	5.00 - 9.00% of mass 176	4.31 (6.30)

Date : 12-NOV-2007 12:01

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

Data File: 5111205.d

Spectrum: HP MS 5111205.d, Scan 102: 3.810 min.

Location of Maximum: 95.10

Number of points: 203

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36,00	9119	92,00	20568	154,00	392	244,30	205
37,10	44888	93,10	40256	155,00	3494	245,40	292
38,10	43232	94,00	99728	157,00	962	246,60	295
39,10	21016	95,10	996608	158,90	1547	249,50	326
40,00	4505	96,10	63608	160,80	583	250,80	156
40,90	227	97,20	1564	162,10	150	253,10	202
42,10	175	100,30	362	162,80	546	254,00	786
42,80	1108	103,00	367	163,90	238	257,10	380
44,00	20088	103,90	2549	166,30	320	260,10	258
45,00	11319	105,00	1117	167,90	155	261,00	341
46,10	661	105,90	2508	168,70	285	262,00	380
47,00	18032	107,00	868	169,80	420	263,40	474
48,10	7435	110,20	391	170,80	868	270,10	182
49,10	51760	110,70	232	172,00	1941	271,10	821
50,10	261056	112,10	497	173,00	6008	274,10	189
51,10	72008	112,90	524	174,00	705472	275,10	367
52,10	2399	113,80	276	175,00	51496	279,30	210
52,90	405	114,90	1352	176,00	681408	280,10	225
55,20	2972	115,90	2761	177,00	42960	280,70	597
56,00	13678	116,90	3675	177,90	1240	281,70	806
57,10	26512	117,90	2302	181,30	275	283,60	396
58,00	2348	118,80	3444	181,90	232	286,50	239
60,10	8860	120,00	168	184,40	161	290,70	254
61,00	45368	122,00	842	185,00	383	293,20	451
62,00	50064	124,50	228	185,70	165	295,30	170
63,10	30528	125,10	301	191,50	399	301,50	170
64,00	2443	126,00	1056	194,00	311	303,10	182
65,10	751	128,00	2999	196,60	182	304,40	153
67,00	1799	129,10	1003	197,00	158	306,30	157
68,10	84984	129,90	3268	207,20	1736	309,10	332
69,10	81088	130,90	918	208,20	738	315,80	175
70,10	6873	134,00	440	208,80	169	316,50	524
71,00	334	134,90	1206	209,50	172	317,70	269
72,10	2580	135,90	222	210,10	339	318,80	417
73,00	29608	136,70	1066	210,70	570	320,90	356

Date : 12-NOV-2007 12:01

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

Data File: 5111205.d

Spectrum: HP MS 5111205.d, Scan 102: 3.810 min.

Location of Maximum: 95.10

Number of points: 203

m/z	Y	m/z	Y	m/z	Y	m/z	Y
74.10	142848	137.70	454	214.00	180	321.40	152
75.10	425344	138.90	1422	217.00	487	322.70	160
76.00	33808	141.00	4191	217.50	284	323.70	157
77.00	3544	142.00	483	218.50	367	325.30	229
78.10	4667	142.90	7506	219.90	868	327.60	271
78.90	13334	144.20	439	224.10	432	331.10	340
79.90	3485	145.10	762	225.00	162	332.00	188
81.00	14052	145.90	1790	228.20	208	333.40	234
82.00	3233	147.10	501	228.70	156	334.10	704
83.10	374	148.00	1524	230.00	819	341.90	268
86.10	409	148.70	465	232.90	340	342.40	175
87.10	31552	149.70	1469	234.00	756	343.80	499
88.00	28288	150.70	406	235.20	153	345.80	155
89.70	283	151.20	548	236.70	256	346.80	220
90.30	1033	151.70	702	238.50	650	348.80	191
91.00	3140	153.10	1101	243.30	371		

Report Date: 13-Nov-2007 11:27

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-13nov.b/5111301.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 13-NOV-2007 11:36
 Operator : ct Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2ul #1476-65 50 ng
 Comment :
 Method : /var/chem/msd5.i/5-13nov.b/bfb30.m
 Meth Date : 13-Nov-2007 09:26 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb							
3.810	3.900	-0.090	95	634304		100.00- 100.00	100.00
3.810	3.900	-0.090	50	169086		15.00- 40.00	26.66
3.810	3.900	-0.090	75	288885		30.00- 60.00	45.54
3.810	3.900	-0.090	96	41776		5.00- 9.00	6.59
3.810	3.900	-0.090	173	1600		0.00- 2.00	0.41
3.810	3.900	-0.090	174	389406		50.00- 100.00	61.39
3.810	3.900	-0.090	175	29272		5.00- 9.00	7.52
3.810	3.900	-0.090	176	379392		95.00- 101.00	97.43
3.810	3.900	-0.090	177	23577		5.00- 9.00	6.21

Date : 13-NOV-2007 11:36

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: ct

Column phase:

Column diameter: 2.00



Date : 13-NOV-2007 11:36

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: ct

Column phase:

Column diameter: 2.00

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	26.66
75	30.00 - 60.00% of mass 95	45.54
96	5.00 - 9.00% of mass 95	6.59
173	Less than 2.00% of mass 174	0.25 (0.41)
174	50.00 - 100.00% of mass 95	61.39
175	5.00 - 9.00% of mass 174	4.61 (7.52)
176	95.00 - 101.00% of mass 174	59.81 (97.43)
177	5.00 - 9.00% of mass 176	3.72 (6.21)

Date : 13-NOV-2007 11:36

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: ct

Column phase:

Column diameter: 2.00

Data File: 5111301.d

Spectrum: Avg. Scans 101-103 (3.81), Background Scan 96

Location of Maximum: 95.00

Number of points: 206

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	7266	103.00	533	162.00	54	253.00	15
37.00	33640	104.00	1547	163.00	282	254.00	286
38.00	29152	105.00	137	164.00	203	255.00	42
39.00	14159	106.00	1845	165.00	95	256.00	92
40.00	652	107.00	944	167.00	253	258.00	172
43.00	10	108.00	313	168.00	522	261.00	93
45.00	8414	110.00	249	169.00	274	262.00	245
46.00	980	111.00	600	170.00	683	265.00	211
47.00	9950	112.00	352	171.00	702	267.00	311
48.00	4612	113.00	69	172.00	1887	272.00	183
49.00	35008	115.00	1006	173.00	1600	273.00	131
50.00	169024	116.00	814	174.00	389376	279.00	343
51.00	56072	117.00	2882	175.00	29272	281.00	762
52.00	2489	118.00	1225	176.00	379392	283.00	99
55.00	1699	119.00	2811	177.00	23576	290.00	259
56.00	9519	120.00	208	178.00	1449	291.00	219
57.00	18488	121.00	90	180.00	56	294.00	84
58.00	835	122.00	139	181.00	268	296.00	108
59.00	259	123.00	265	183.00	74	297.00	140
60.00	6272	124.00	110	185.00	214	300.00	231
61.00	30008	125.00	602	189.00	142	301.00	72
62.00	28472	126.00	592	190.00	109	302.00	112
63.00	20720	128.00	1149	193.00	36	305.00	256
64.00	1581	129.00	466	194.00	221	307.00	170
65.00	817	130.00	2024	195.00	118	308.00	78
67.00	961	131.00	634	197.00	65	309.00	51
68.00	54800	132.00	160	199.00	77	311.00	61
69.00	54816	133.00	310	201.00	118	312.00	161
70.00	3978	134.00	455	203.00	130	315.00	87
72.00	2245	135.00	515	204.00	62	316.00	229
73.00	23784	136.00	91	208.00	21	318.00	260
74.00	89960	137.00	922	210.00	82	321.00	121
75.00	288832	138.00	564	214.00	86	322.00	631
76.00	25160	139.00	326	216.00	247	324.00	126
77.00	2419	140.00	347	219.00	232	325.00	87

Date : 13-NOV-2007 11:36

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: ct

Column phase:

Column diameter: 2.00

Data File: 5111301.d

Spectrum: Avg. Scans 101-103 (3.81), Background Scan 96

Location of Maximum: 95.00

Number of points: 206

m/z	Y	m/z	Y	m/z	Y	m/z	Y
78.00	1213	141.00	3959	223.00	276	326.00	440
79.00	9390	142.00	793	225.00	122	327.00	57
80.00	2355	143.00	5060	226.00	91	331.00	147
81.00	8687	144.00	53	229.00	255	332.00	134
82.00	1771	145.00	147	231.00	154	333.00	116
86.00	440	146.00	814	234.00	62	335.00	89
87.00	17888	147.00	20	236.00	75	336.00	319
88.00	20448	148.00	1388	237.00	68	338.00	110
89.00	348	150.00	313	238.00	111	341.00	219
91.00	1036	153.00	645	241.00	55	343.00	140
92.00	15548	154.00	348	242.00	52	344.00	112
93.00	23368	155.00	688	244.00	263	345.00	119
94.00	66704	156.00	198	247.00	86	346.00	59
95.00	634304	157.00	810	248.00	232	347.00	44
96.00	41776	159.00	987	249.00	153	349.00	160
97.00	1019	160.00	129	251.00	83		
101.00	62	161.00	389	252.00	390		

Report Date: 19-Nov-2007 00:23

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-19nov.b/5111901.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 19-NOV-2007 00:33
 Operator : ab Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2uL #1476-65 50 ng
 Comment :
 Method : /var/chem/msd5.i/5-19nov.b/bfb30.m
 Meth Date : 19-Nov-2007 00:23 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

1 bfb

CAS #: 460-00-4

3.810	3.900	-0.090	95	993301		100.00- 100.00	100.00
3.810	3.900	-0.090	50	261826		15.00- 40.00	26.36
3.810	3.900	-0.090	75	471886		30.00- 60.00	47.51
3.810	3.900	-0.090	96	66493		5.00- 9.00	6.69
3.810	3.900	-0.090	173	4811		0.00- 2.00	0.76
3.810	3.900	-0.090	174	636565		50.00- 100.00	64.09
3.810	3.900	-0.090	175	46616		5.00- 9.00	7.32
3.810	3.900	-0.090	176	619498		95.00- 101.00	97.32
3.810	3.900	-0.090	177	37874		5.00- 9.00	6.11

Date : 19-NOV-2007 00:33

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: ab

Column phase:

Column diameter: 2.00



Date : 19-NOV-2007 00:33

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: ab

Column phase:

Column diameter: 2.00

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100.00% relative abundance	100.00
50	15.00 - 40.00% of mass 95	26.36
75	30.00 - 60.00% of mass 95	47.51
96	5.00 - 9.00% of mass 95	6.69
173	Less than 2.00% of mass 174	0.48 (0.76)
174	50.00 - 100.00% of mass 95	64.09
175	5.00 - 9.00% of mass 174	4.69 (7.32)
176	95.00 - 101.00% of mass 174	62.37 (97.32)
177	5.00 - 9.00% of mass 176	3.81 (6.11)

Date : 19-NOV-2007 00:33

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: ab

Column phase:

Column diameter: 2.00

Data File: 5111901.d

Spectrum: Avg. Scans 101-103 (3.81), Background Scan 96

Location of Maximum: 95.00

Number of points: 228

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	10571	97.00	1471	159.00	728	251.00	74
37.00	61408	98.00	19	161.00	945	252.00	76
38.00	51488	99.00	223	162.00	229	257.00	102
39.00	21096	101.00	111	163.00	394	258.00	95
40.00	290	103.00	85	164.00	311	259.00	187
41.00	518	104.00	2891	165.00	118	260.00	99
44.00	5241	105.00	1085	166.00	234	261.00	114
45.00	10939	106.00	2306	167.00	207	264.00	4
46.00	628	107.00	738	168.00	464	268.00	220
47.00	17000	108.00	350	169.00	467	269.00	457
48.00	6166	109.00	508	170.00	714	271.00	282
49.00	46688	110.00	335	171.00	1222	274.00	194
50.00	261824	111.00	621	172.00	42	275.00	159
51.00	83344	112.00	503	173.00	4811	277.00	82
52.00	4374	113.00	658	174.00	636544	278.00	470
53.00	297	114.00	173	175.00	46616	280.00	60
54.00	244	115.00	433	176.00	619456	282.00	205
55.00	3528	116.00	2464	177.00	37872	283.00	68
56.00	14693	117.00	4294	178.00	1531	284.00	54
57.00	27632	118.00	2384	182.00	96	286.00	218
58.00	1633	119.00	3555	185.00	123	288.00	226
60.00	9728	120.00	422	186.00	124	289.00	278
61.00	49024	121.00	337	188.00	196	293.00	144
62.00	47264	122.00	31	189.00	94	294.00	284
63.00	32584	123.00	390	190.00	53	296.00	53
64.00	2219	124.00	830	193.00	255	297.00	121
65.00	119	125.00	473	194.00	85	298.00	16
66.00	210	126.00	536	196.00	83	301.00	67
67.00	2367	127.00	328	197.00	50	303.00	336
68.00	89808	128.00	2314	199.00	53	305.00	219
69.00	84920	129.00	2002	200.00	287	307.00	136
70.00	5464	130.00	2967	201.00	271	308.00	221
71.00	183	131.00	1151	204.00	141	310.00	110
72.00	3437	134.00	192	205.00	233	314.00	103
73.00	35464	135.00	753	206.00	245	315.00	110

Date : 19-NOV-2007 00:33

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: ab

Column phase:

Column diameter: 2.00

Data File: 5111901.d

Spectrum: Avg. Scans 101-103 (3.81), Background Scan 96

Location of Maximum: 95.00

Number of points: 228

m/z	Y	m/z	Y	m/z	Y	m/z	Y
74.00	146560	136.00	202	209.00	121	318.00	175
75.00	471872	137.00	715	210.00	315	320.00	323
76.00	39192	138.00	324	212.00	102	324.00	90
77.00	3322	139.00	160	215.00	427	325.00	100
78.00	2899	140.00	905	216.00	70	326.00	54
79.00	13604	141.00	6338	217.00	111	327.00	85
80.00	5043	142.00	901	218.00	135	329.00	125
81.00	14167	143.00	6229	221.00	364	330.00	62
82.00	2940	144.00	104	223.00	74	331.00	63
83.00	904	145.00	476	224.00	208	333.00	92
84.00	149	146.00	276	227.00	82	335.00	66
85.00	219	147.00	392	228.00	67	339.00	175
86.00	621	148.00	1772	231.00	239	340.00	55
87.00	30744	149.00	464	235.00	94	341.00	17
88.00	30376	150.00	756	237.00	66	342.00	277
89.00	1107	151.00	215	238.00	69	344.00	95
90.00	45	152.00	412	239.00	319	345.00	129
91.00	2158	153.00	223	240.00	210	346.00	76
92.00	22152	154.00	857	244.00	72	348.00	334
93.00	36112	155.00	1309	247.00	315		
94.00	108128	156.00	374	248.00	154		
95.00	993280	157.00	1381	249.00	155		
96.00	66488	158.00	309	250.00	147		

Report Date: 27-Nov-2007 08:47

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-27nov.b/5112701.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 27-NOV-2007 08:56
 Operator : cb Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2uL #1476-65 50 ng
 Comment :
 Method : /var/chem/msd5.i/5-27nov.b/bfb30.m
 Meth Date : 27-Nov-2007 08:47 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb					CAS #: 460-00-4	
3.796	3.900	-0.104	95	690854		100.00- 100.00	100.00
3.796	3.900	-0.104	50	201322		15.00- 40.00	29.14
3.796	3.900	-0.104	75	336719		30.00- 60.00	48.74
3.796	3.900	-0.104	96	45282		5.00- 9.00	6.55
3.796	3.900	-0.104	173	2714		0.00- 2.00	0.65
3.796	3.900	-0.104	174	419349		50.00- 100.00	60.70
3.796	3.900	-0.104	175	29427		5.00- 9.00	7.02
3.796	3.900	-0.104	176	412821		95.00- 101.00	98.44
3.796	3.900	-0.104	177	24457		5.00- 9.00	5.92

Date : 27-NOV-2007 08:56

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00



Date : 27-NOV-2007 08:56

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

1 bfb

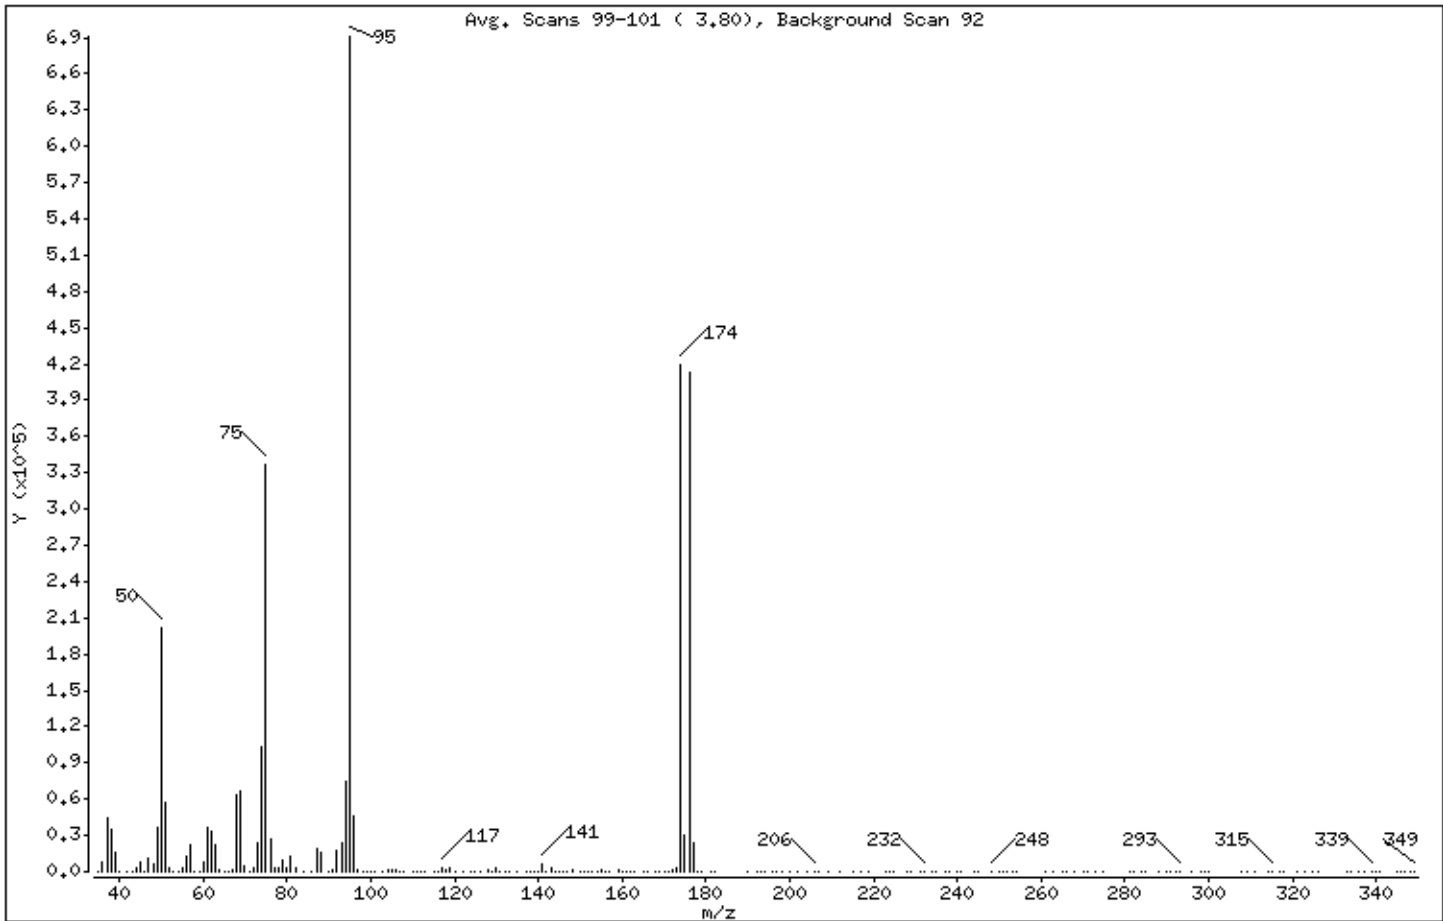

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	29.14
75	30.00 - 60.00% of mass 95	48.74
96	5.00 - 9.00% of mass 95	6.55
173	Less than 2.00% of mass 174	0.39 (0.65)
174	50.00 - 100.00% of mass 95	60.70
175	5.00 - 9.00% of mass 174	4.26 (7.02)
176	95.00 - 101.00% of mass 174	59.76 (98.44)
177	5.00 - 9.00% of mass 176	3.54 (5.92)

Date : 27-NOV-2007 08:56

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

Data File: 5112701.d

Spectrum: Avg. Scans 99-101 (3.80), Background Scan 92

Location of Maximum: 95.00

Number of points: 214

m/z	Y	m/z	Y	m/z	Y	m/z	Y
35.00	357	93.00	23432	156.00	358	245.00	259
36.00	8617	94.00	74888	157.00	604	248.00	367
37.00	43720	95.00	690816	159.00	874	250.00	190
38.00	35504	96.00	45280	160.00	67	251.00	157
39.00	15127	97.00	1469	161.00	613	252.00	134
40.00	688	98.00	283	162.00	56	253.00	11
42.00	5	99.00	52	163.00	463	254.00	213
43.00	300	100.00	294	165.00	298	261.00	58
44.00	3014	101.00	153	166.00	6	263.00	68
45.00	8490	103.00	94	168.00	215	265.00	220
46.00	528	104.00	2273	169.00	416	266.00	98
47.00	11577	105.00	1166	170.00	289	268.00	265
48.00	6464	106.00	2312	171.00	267	270.00	262
49.00	36152	107.00	314	172.00	1472	271.00	306
50.00	201280	108.00	80	173.00	2714	273.00	113
51.00	57200	110.00	535	174.00	419328	275.00	104
52.00	2553	111.00	473	175.00	29424	281.00	140
53.00	94	112.00	151	176.00	412800	282.00	191
54.00	210	113.00	774	177.00	24456	284.00	120
55.00	2389	115.00	598	178.00	754	285.00	132
56.00	12151	116.00	770	179.00	319	288.00	103
57.00	21488	117.00	2927	181.00	98	290.00	59
58.00	491	118.00	2302	182.00	171	291.00	135
59.00	179	119.00	2849	190.00	189	292.00	107
60.00	7160	120.00	23	192.00	341	293.00	393
61.00	36696	122.00	250	193.00	209	296.00	117
62.00	33968	124.00	29	194.00	115	298.00	183
63.00	22080	125.00	422	196.00	109	299.00	112
64.00	2166	126.00	204	197.00	130	300.00	173
65.00	776	128.00	1289	198.00	106	308.00	219
66.00	100	129.00	793	200.00	319	309.00	77
67.00	2051	130.00	2553	202.00	187	311.00	131
68.00	64168	131.00	706	204.00	175	314.00	72
69.00	67272	132.00	258	206.00	428	315.00	469
70.00	4599	133.00	211	207.00	85	317.00	98

Date : 27-NOV-2007 08:56

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

Data File: 5112701.d

Spectrum: Avg. Scans 99-101 (3.80), Background Scan 92

Location of Maximum: 95.00

Number of points: 214

m/z	Y	m/z	Y	m/z	Y	m/z	Y
71.00	427	135.00	671	209.00	378	318.00	148
72.00	2768	137.00	729	212.00	136	321.00	144
73.00	23816	138.00	157	215.00	197	323.00	76
74.00	103328	139.00	120	217.00	138	325.00	59
75.00	336704	140.00	287	219.00	154	326.00	63
76.00	27720	141.00	5907	223.00	151	333.00	140
77.00	2928	142.00	585	224.00	63	334.00	119
78.00	2767	143.00	3621	225.00	109	336.00	318
79.00	10156	144.00	266	228.00	56	337.00	178
80.00	2842	145.00	148	229.00	76	339.00	355
81.00	12633	146.00	629	231.00	11	340.00	263
82.00	2425	147.00	158	232.00	245	341.00	170
84.00	51	148.00	1520	234.00	200	345.00	54
86.00	731	150.00	775	235.00	192	346.00	73
87.00	18864	151.00	108	237.00	130	347.00	275
88.00	16266	152.00	356	238.00	94	348.00	249
90.00	334	153.00	443	240.00	230	349.00	148
91.00	1978	154.00	154	241.00	233		
92.00	16848	155.00	1487	244.00	81		

Report Date: 28-Dec-2007 08:30

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-28dec.b/5122801.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 28-DEC-2007 08:40
 Operator : cb Inst ID: msd5.i
 Smp Info : BFB Tune Check
 Misc Info : 2uL #1476-65 50 ng
 Comment :
 Method : /var/chem/msd5.i/5-28dec.b/bfb30.m
 Meth Date : 28-Dec-2007 08:30 Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
1	bfb					CAS #: 460-00-4	
3.789	3.900	-0.111	95	1679328		100.00- 100.00	100.00
3.789	3.900	-0.111	50	475138		15.00- 40.00	28.29
3.789	3.900	-0.111	75	794112		30.00- 60.00	47.29
3.789	3.900	-0.111	96	107874		5.00- 9.00	6.42
3.789	3.900	-0.111	173	6935		0.00- 2.00	0.68
3.789	3.900	-0.111	174	1019783		50.00- 100.00	60.73
3.789	3.900	-0.111	175	74978		5.00- 9.00	7.35
3.789	3.900	-0.111	176	1001941		95.00- 101.00	98.25
3.789	3.900	-0.111	177	65221		5.00- 9.00	6.51

Date : 28-DEC-2007 08:40

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00



Date : 28-DEC-2007 08:40

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	28.29
75	30.00 - 60.00% of mass 95	47.29
96	5.00 - 9.00% of mass 95	6.42
173	Less than 2.00% of mass 174	0.41 (0.68)
174	50.00 - 100.00% of mass 95	60.73
175	5.00 - 9.00% of mass 174	4.46 (7.35)
176	95.00 - 101.00% of mass 174	59.66 (98.25)
177	5.00 - 9.00% of mass 176	3.88 (6.51)

Date : 28-DEC-2007 08:40

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

Data File: 5122801.d

Spectrum: Avg. Scans 98-100 (3.79), Background Scan 92

Location of Maximum: 95.00

Number of points: 199

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	14821	90.00	95	151.00	27	236.00	53
37.00	99608	91.00	5211	152.00	94	238.00	72
38.00	86320	92.00	44280	153.00	1576	239.00	69
39.00	37232	93.00	64792	154.00	879	240.00	317
42.00	423	94.00	186496	155.00	3387	242.00	84
43.00	500	95.00	1678848	156.00	596	244.00	64
44.00	5963	96.00	107872	157.00	2218	247.00	158
45.00	21640	97.00	2810	158.00	367	248.00	129
46.00	1746	98.00	628	159.00	1253	249.00	444
47.00	34720	103.00	272	161.00	1725	251.00	309
48.00	10928	104.00	4974	162.00	131	252.00	149
49.00	89040	105.00	1436	163.00	150	254.00	409
50.00	475136	106.00	4198	165.00	646	257.00	135
51.00	143296	107.00	484	166.00	134	259.00	66
52.00	6228	109.00	305	167.00	677	263.00	88
53.00	454	110.00	224	168.00	357	265.00	196
54.00	103	111.00	1394	169.00	470	266.00	331
55.00	4989	112.00	838	170.00	605	268.00	100
56.00	27336	113.00	976	171.00	1236	270.00	96
57.00	57560	115.00	1065	172.00	2975	271.00	244
58.00	1802	116.00	3552	173.00	6935	273.00	53
59.00	281	117.00	7015	174.00	1019776	275.00	149
60.00	13739	118.00	3442	175.00	74976	278.00	88
61.00	81632	119.00	4443	176.00	1001920	279.00	122
62.00	76544	120.00	444	177.00	65216	280.00	95
63.00	59408	122.00	424	178.00	2109	281.00	110
64.00	4635	123.00	536	179.00	78	283.00	99
65.00	833	124.00	733	182.00	241	286.00	76
67.00	4505	125.00	629	183.00	146	289.00	90
68.00	158912	126.00	669	185.00	487	297.00	167
69.00	153984	128.00	4423	187.00	118	298.00	88
70.00	9932	129.00	1850	190.00	182	299.00	611
71.00	347	130.00	4753	193.00	58	302.00	59
72.00	6292	131.00	1116	197.00	95	304.00	252
73.00	62600	135.00	1632	201.00	237	305.00	10

Date : 28-DEC-2007 08:40

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: cb

Column phase:

Column diameter: 2.00

Data File: 5122801.d

Spectrum: Avg. Scans 98-100 (3.79), Background Scan 92

Location of Maximum: 95.00

Number of points: 199

m/z	Y	m/z	Y	m/z	Y	m/z	Y
74.00	246464	136.00	366	202.00	272	306.00	200
75.00	794112	137.00	1922	203.00	194	308.00	76
76.00	63952	138.00	170	204.00	381	309.00	102
77.00	6187	139.00	500	207.00	233	310.00	125
78.00	4300	140.00	1102	208.00	41	312.00	238
79.00	24232	141.00	11486	213.00	70	313.00	162
80.00	8283	142.00	1205	214.00	63	314.00	141
81.00	23880	143.00	10230	217.00	96	324.00	146
82.00	4955	144.00	912	220.00	103	329.00	85
83.00	1078	145.00	907	222.00	50	336.00	222
84.00	154	146.00	2155	226.00	199	337.00	95
85.00	158	147.00	1304	229.00	359	341.00	168
86.00	1625	148.00	2957	230.00	177	343.00	304
87.00	50000	149.00	1023	232.00	269	346.00	185
88.00	49920	150.00	1467	235.00	215		

Shipping/ Receiving Documents



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: _____ GEI Consultants, Inc.
ATTENTION: _____ Ms. Sarah Aldridge
FAX #: _____ 860-368-5307
FROM: _____ Sample Receiving
Workorder #: _____ 0712439
of pages (Including Cover): _____ 1

1/9/2008

Thank you for selecting Air Toxics Ltd. We have received your samples and have found discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Bryanna Langley at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

The following discrepancy has been observed:

The canister valve on sample UW AMS5 was received open and a brass plug used to seal the canister was loose. The sample vented to ambient pressure during shipment. Sample UW AMS5 was cancelled at your request.

Your prompt response is appreciated.

AIR TOXICS LTD.

Sample Transportation Notice

Relinquishing signature on this document indicates that sample is being shipped in compliance with all applicable local, State, Federal, national, and international laws, regulations and ordinances of any kind. Air Toxics Limited assumes no liability with respect to the collection, handling, or shipping of these samples. Relinquishing signature also indicates agreement to hold harmless, defend, and indemnify Air Toxics Limited against any claim, demand, or action of any kind, related to the collection, handling, or shipping of samples. D.O.T. Hotline (800) 457-4522

180 BLUE RAVINE ROAD, SUITE B
FOLSOM, CA 95630-4719
(916) 985-1000 FAX: (916) 985-1020

Contact	Company: GEL Consultants, Inc.	Project Info:	Turn Around Time:
Address: 455 Winding Brook Glastonbury CT 06033	Phone: 860-368-5300 Cell:	P.O. #	<input checked="" type="checkbox"/> Normal
Collected By: Signature: <i>Thomas R. Temple</i>	Project #	051140 - 8 - 1703	<input type="checkbox"/> Rush
	Project Name	BayShore QU1 Southern cell	Specify _____
		Air Monitoring	

Lab I.D.	Field Sample I.D.	Canister #	Date & Time	Analyses Requested	Carister Pressure/Vacuum Initial Final Receipt
Q1A	UW AMS 5	34008	12/19/07 0600-1400	TO-15 + Naphthalene	
Q2A	DW AMS 3	34317	12/19/07 0600-1400	TO-15 + Naphthalene	

Relinquished By: (Signature) Date/Time <i>Thomas R. Temple</i> 12/19/07 1415	Received By: (Signature) Date/Time <i>MAJ MINT ST</i> 12/20/07
Relinquished By: (Signature) Date/Time	Received By: (Signature) Date/Time
Relinquished By: (Signature) Date/Time	Received By: (Signature) Date/Time

Notes: use flow controllers included
Initial and final can pressures in inches Hg
Send Data Pack to Lisa McDonough and EDD to
datagroup@geiconsultants.com

Lab	Shipper Name	Air Bill #	Opened By	Temp. (C)	Condition	Checked/Sealed/Inspected?	Work Order #
Use Only	FedEx	863512570588	<i>[Signature]</i>	NA	Good	Yes <input type="checkbox"/> No <input type="checkbox"/> None <input checked="" type="checkbox"/>	0712489



AN ENVIRONMENTAL ANALYTICAL LABORATORY

SAMPLE RECEIPT SUMMARY

WORKORDER 0712439

Client

Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Drive
Suite 201
Glastonbury, CT 06033

Phone

860-368-5300

Fax

860-368-5307

Date Promised: 01/08/08

Date Completed: 1/7/08

Date Received: 12/20/07

PO#: NR

Project#: 061140-8-1703 BayShore OU1 Southern cell
Air Monitorin

Total \$: \$ 399.00

Logged By: MG

Sales Rep: ANS

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A(cancelled)	UW AMS5	Modified TO-15	12/19/2007	0.0 "Hg	\$0.00
02A	DW AMS3	Modified TO-15	12/19/2007	4.5 "Hg	\$225.00
03A	Lab Blank	Modified TO-15	NA	NA	\$0.00
04A	CCV	Modified TO-15	NA	NA	\$0.00
05A	LCS	Modified TO-15	NA	NA	\$0.00
Misc. Charges 6 Liter Summa Canister (2) @ \$50.00 each., Shipment 54019					\$100.00
Blue Body Flow Controller (2) @ \$35.00 each., Shipment 54019					\$70.00
Fuel Surcharge (2) @ \$2.00 each.					\$4.00

Note: Samples received after 3 P.M. PST are considered to be received on the following work day.
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

BILL TO: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Drive
Suite 201
Glastonbury, CT 06033

Analysis Code: TO-14A

TERMS:

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

Sample Discrepancy Report

Identification

Initiated By: T. Gayer

Date: 12/26/07

Discrepancy Type: (circle all that apply)

I. II. III.

Workorder(s) affected: 0712439 ~~01A~~ ^{Rev 12/26/07}

Sample(s) affected: 01A

I. Sample Receipt Discrepancies

Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative

Narration not required:

- COC was not filled out in ink.
- Sample container (cartridge/tube/VOA vial) was received broken, however sample was intact.
- Flow controller used - canister samples received at ambient or under pressure.
- No brass cap on canister.
- VOA vial for RSK-175 analysis received with headspace bubble <5mm.

Narration Required:

- COC improperly relinquished / received.
- Sample tags / can numbers do not match the COC.
- Samples received at wrong temperature (up to 10°C); ice / blue ice (circle one) was present. A temp. blank was / was not present (circle one).
- Custody Seal on the outside of the container was broken / improperly placed (circle one).
- Other (describe below).

Describe the Discrepancy: _____

II. Sample Receipt/Screening Discrepancies requiring CSR notification

Document on Cover Page of Sample Receipt Confirmation and in Receiving Notes of Lab Narrative

If Section II. is filled out CSR must be notified within 24 hrs of Initiation

- COC was not received with samples.
- Analysis method(s) is not specified / incorrectly specified (circle one) on the COC.
- Number of samples on the COC does not match the number of samples that were received.
- Samples were received expired.
- Sampling date / time (sulfur only) is not documented for some / any samples (circle one).
- Sample received with significant (pooling) volume of H₂O in the Tedlar Bag.
- Sample container (cartridge/tube/VOA vial/DNPH Bottle, etc.) was received broken / leaking (circle one); sample can / cannot be analyzed (circle one).
- VOA vial for RSK-175 analysis received with headspace bubble >5mm.
- Samples for RSK-175 CO₂ analysis received preserved with HCl.
- Tedlar Bag received leaking / flat (circle one). Sample can / cannot (circle one) be analyzed.
- Canister was at ambient pressure at time of pressurization and (check all that apply): canister failed leak check on two manifolds, canister valve was open, brass nut was loose. Sample can / cannot be analyzed (circle one).
- Tedlar bag / canister received emitting a strong odor; sample can / cannot (circle one) be analyzed.
- Canister sample received with a vacuum difference >7.0"Hg between the receipt vac. and the final vac. reported on the COC, indicating loss of vacuum.
- Canister sample received at >15"Hg (not identified as a Trip/Field Blank).
- Trip Blank received at low vacuum (< 25"Hg).
- Tedlar Bag for Sulfur analysis has metal fitting.
- Incorrect sampling media / container for analysis requested.
- Sample was received at ≥ 10°C.
- Other (describe below)

Initials: TG
(if not the original initiator)

Date: 12/26/07

CSR Notified
(see section below)

Describe the Discrepancy: Noticed canister valve was open and the brass nut was loose during pressurization

If Section III. Is filled out CSR must be notified within 24 hrs of Initiation

- Tedlar Bag found to be leaking at the time of analysis; sample can / cannot (circle one) be analyzed.
- Tedlar Bag found to be flat at the time of analysis.
- Canister found to be leaking at the time of analysis.
- Tedlar Bag received at low volume; sample cannot be analyzed.
- Sulfur samples received with insufficient time to analyze prior to expiration.
- VOST tube saturated; bag dilution necessary.
- Sample loss due to instrument malfunction / broken glassware.
- Other (describe below).

Initials: _____
(if not the original initiator)

Date: _____

CSR Notified
(see section below)

Team Lead Initials: _____

Date: _____

Describe the Discrepancy: _____

Client Services Use Only

Client Services Notification

CSR notified: _____

Date: _____

Action:

- It is not necessary to notify the client. Narrate the discrepancy by documenting on cover page of Sample Receipt Confirmation and in Receiving Notes/Analytical Notes of Lab Narrative.

CSR Initials: _____ Date: _____

- Client notification required. See attached client contact / email, or comments below:

Client Notification:

Person notified: BRIAN SREELY Date: 1-2-08

Comments: CANCEL SAMPLE. SEE EMAIL.

Lab notified Name: _____ Date: _____

Additional Notifications

CSR notified: _____

Date: _____

Action:

- It is not necessary to notify the client. Narrate the discrepancy by documenting on cover page of Sample Receipt Confirmation and in Receiving Notes/Analytical Notes of Lab Narrative.

CSR Initials: _____ Date: _____

- Client notification required. See attached client contact / email, or comments below:

Client Notification:

Person notified: _____ Date: _____

Comments: _____

Lab notified Name: _____ Date: _____

- Additional notifications attached.

Other Records

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	

DATA REVIEW CHECKLIST

Work Order #:

0712439

- | | | | | | |
|-------------------------------------|-------------------------------------|--------------------------|-------------------------------------|--------------------------|--|
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Analysis/Reporting vs. Project Profile/SOP requirements checked (i.e. 100% Dups, J-Flag to MDL, etc) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | The final report has the correct reporting list, special units, and header info. |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Lab Narrative is correct (proper method & description/Receiving & Analytical notes correct) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Corrective Action issued - # _____ |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Unusual circumstances have been documented in the notes section below |

LUMEN validation report present and initialed

CIRCLE (YES / NO)

- | | | | | | |
|-------------------------------------|--------------------------|-------------------------------------|--------------------------|--------------------------|---|
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Lab Blank, CCV, LCS and DUP met QC criteria |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Hold time is met for all samples |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Appropriate data qualifier flags are applied |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Manual integrations for samples and QC are properly documented |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Samples analyzed within the project or method specific clock |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Retention times have been verified |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Appropriate ICAL(s) included |
| <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | At least one result per sample is verified against the target quant sheets/raw data |

- | | | | | | |
|-------------------------------------|-------------------------------------|--------------------------|-------------------------------------|--------------------------|---|
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Dilution factor correctly calculated (sample load volume, syringe and bag dilutions, can pressurization(s)) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Correct amount of sample analyzed (i.e. sample not over-diluted) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Spectra verified - documentation of spectral defense included (Section 5A of eCVP pkg) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | TICs resemble reference spectra |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | TICs between duplicate samples are consistent |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Checked samples for trends (i.e. Influent>Effluent, Landfill or Ambient etc) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Special units for all samples in the final report are correctly calculated |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Manually entered results checked (i.e. special CCV compounds) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | TPH/NMOC (verify calculations and correct reference compound used) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Chain of Custody scanned correctly |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Verify sample id's vs. chain of custody |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Samples pressurized w/ appropriate gas (N ₂ or He) <input type="checkbox"/> Tedlar Bag only |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Final pressure consistent with canister size (6L vs. 1L) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Verify receipt pressures against logbook and Target |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> | Verify canister ID #'s |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Extra printed copies are provided per client profile |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Final invoice amount correct (adjusted for TAT, Penalties, Re-issue Charges etc.) |
| <input checked="" type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input checked="" type="checkbox"/> | <input type="checkbox"/> | Client LUMEN report reviewed for accuracy and completeness |

Notes: (to include: noting samples with QA/QC problems, Blanks with positive hits, narratives, etc.)

A/R: 0 out CCV, 1 out LCS

M/Q:

A
(Analytical Review/Date)

CB 12/31/07

R/T
(Reporting Review/Date)

R: C Taylor 1-7-08

M
(Management Review/Date)

1/7/08

Q
(QA Review/Date)

T: _____

Not Applicable