



***Air
Toxics LTD.***
Laboratory Services Since 1989

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

COMPREHENSIVE VALIDATION PACKAGE

Modified TO-15

INVENTORY SHEET

Work Order #: 0801560

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	21
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	22	29
b. Surrogate Recover Summary Form (If Applicable)	30	30
c. Internal Standard Summary Form (If Applicable)	31	31
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	32	206
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	207	220
i. Second Source LCS(Summary + Raw Data)	221	234
j. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	235	236
l. GC/MS Tune (Results + Raw Data)	237	265
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	266	267
b. Chain-of-Custody Records	268	268
c. Sample Log-In Sheet	269	269
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	--	--
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	270	272
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	273	274
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	--	--
i. <u>Data Review Check Sheet</u>	275	275

Comments:

Completed by:

Kara McKiernan

Kara McKiernan / Document Control

2/19/08

(Signature)

(Print Name & Title)

(Date)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

WORK ORDER #: 0801560

Work Order Summary

CLIENT: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Drive
Suite 201
Glastonbury, CT 06033

BILL TO: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Drive
Suite 201
Glastonbury, CT 06033

PHONE: 860-368-5300

P.O. # NR

FAX: 860-368-5307


PROJECT # 061140-8-1703 BayShore OU1 Southern

DATE RECEIVED: 01/31/2008

CONTACT: cell Air Monitorin
Bryanna Langley

DATE COMPLETED: 02/12/2008

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>	<u>FINAL PRESSURE</u>
01A	DW AMS 3	Modified TO-15	8.0 "Hg	5 psi
02A	UW AMS 5	Modified TO-15	6.5 "Hg	5 psi
03A	Lab Blank	Modified TO-15	NA	NA
04A	CCV	Modified TO-15	NA	NA
05A	LCS	Modified TO-15	NA	NA

CERTIFIED BY: 

DATE: 02/13/08

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004
NY NELAP - 11291, UT NELAP - 9166389892

Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,
Accreditation number: E87680, Effective date: 07/01/07, Expiration date: 06/30/08

Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards

This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

LABORATORY NARRATIVE
Modified TO-15
GEI Consultants, Inc.
Workorder# 0801560



Two 6 Liter Summa Canister samples were received on January 31, 2008. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

This workorder was independently validated prior to submittal using 'USEPA National Functional Guidelines' as generally applied to the analysis of volatile organic compounds in air. A rules-based, logic driven, independent validation engine was employed to assess completeness, evaluate pass/fail of relevant project quality control requirements and verification of all quantified amounts.

Method modifications taken to run these samples are summarized in the table below. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	+/- 30% Difference	<= 30% Difference with two allowed out up to <=40%.; flag and narrate outliers
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

Receiving Notes

There were no receiving discrepancies.

Analytical Notes

All Quality Control Limit failures and affected sample results are noted by flags. Each flag is defined at the bottom of this Case Narrative and on each Sample Result Summary page. Target compound non-detects in the samples that are associated with high bias in QC analyses have not been flagged.

Definition of Data Qualifying Flags

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

B - Compound present in laboratory blank greater than reporting limit (background subtraction no performed).

J - Estimated value.

E - Exceeds instrument calibration range.

S - Saturated peak.

- Q - Exceeds quality control limits.
- U - Compound analyzed for but not detected above the reporting limit.
- UJ- Non-detected compound associated with low bias in the CCV
- N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

- a-File was requantified
- b-File was quantified by a second column and detector
- r1-File was requantified for the purpose of reissue

Table 1

Client Sample ID	Lab Sample ID	Date Collected	Date Received	Date Extracted	Sample	Sample Extract		
					Holding Time (Days)	Date Analyzed	Holding Time (Days)	Sample Condition
DW AMS 3	0801560-01A	1/30/2008	1/31/2008	NA	5	2/ 4/2008	NA	Good
UW AMS 5	0801560-02A	1/30/2008	1/31/2008	NA	5	2/ 4/2008	NA	Good
Lab Blank	0801560-03A	NA	NA	NA	NA	2/ 3/2008	NA	Good
CCV	0801560-04A	NA	NA	NA	NA	2/ 3/2008	NA	Good
LCS	0801560-05A	NA	NA	NA	NA	2/ 3/2008	NA	Good

Sample Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds
MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: DW AMS 3

Lab ID#: 0801560-01A

No Detections Were Found.



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: DW AMS 3

Lab ID#: 0801560-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020315	Date of Collection:	1/30/08
Dil. Factor:	1.83	Date of Analysis:	2/4/08 01:28 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.92	Not Detected	4.5	Not Detected
Freon 114	0.92	Not Detected	6.4	Not Detected
Vinyl Chloride	0.92	Not Detected	2.3	Not Detected
Bromomethane	0.92	Not Detected	3.6	Not Detected
Chloroethane	0.92	Not Detected	2.4	Not Detected
Freon 11	0.92	Not Detected	5.1	Not Detected
1,1-Dichloroethene	0.92	Not Detected	3.6	Not Detected
Freon 113	0.92	Not Detected	7.0	Not Detected
Methylene Chloride	0.92	Not Detected	3.2	Not Detected
1,1-Dichloroethane	0.92	Not Detected	3.7	Not Detected
cis-1,2-Dichloroethene	0.92	Not Detected	3.6	Not Detected
Chloroform	0.92	Not Detected	4.5	Not Detected
1,1,1-Trichloroethane	0.92	Not Detected	5.0	Not Detected
Carbon Tetrachloride	0.92	Not Detected	5.8	Not Detected
Benzene	0.92	Not Detected	2.9	Not Detected
1,2-Dichloroethane	0.92	Not Detected	3.7	Not Detected
Trichloroethene	0.92	Not Detected	4.9	Not Detected
1,2-Dichloropropane	0.92	Not Detected	4.2	Not Detected
cis-1,3-Dichloropropene	0.92	Not Detected	4.2	Not Detected
Toluene	0.92	Not Detected	3.4	Not Detected
trans-1,3-Dichloropropene	0.92	Not Detected	4.2	Not Detected
1,1,2-Trichloroethane	0.92	Not Detected	5.0	Not Detected
Tetrachloroethene	0.92	Not Detected	6.2	Not Detected
1,2-Dibromoethane (EDB)	0.92	Not Detected	7.0	Not Detected
Chlorobenzene	0.92	Not Detected	4.2	Not Detected
Ethyl Benzene	0.92	Not Detected	4.0	Not Detected
m,p-Xylene	0.92	Not Detected	4.0	Not Detected
o-Xylene	0.92	Not Detected	4.0	Not Detected
Styrene	0.92	Not Detected	3.9	Not Detected
1,1,2,2-Tetrachloroethane	0.92	Not Detected	6.3	Not Detected
1,3,5-Trimethylbenzene	0.92	Not Detected	4.5	Not Detected
1,2,4-Trimethylbenzene	0.92	Not Detected	4.5	Not Detected
1,3-Dichlorobenzene	0.92	Not Detected	5.5	Not Detected
1,4-Dichlorobenzene	0.92	Not Detected	5.5	Not Detected
alpha-Chlorotoluene	0.92	Not Detected	4.7	Not Detected
1,2-Dichlorobenzene	0.92	Not Detected	5.5	Not Detected
1,3-Butadiene	0.92	Not Detected	2.0	Not Detected
Hexane	0.92	Not Detected	3.2	Not Detected
Cyclohexane	0.92	Not Detected	3.1	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: DW AMS 3

Lab ID#: 0801560-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020315	Date of Collection:	1/30/08
Dil. Factor:	1.83	Date of Analysis:	2/4/08 01:28 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.92	Not Detected	3.7	Not Detected
Bromodichloromethane	0.92	Not Detected	6.1	Not Detected
Dibromochloromethane	0.92	Not Detected	7.8	Not Detected
Cumene	0.92	Not Detected	4.5	Not Detected
Propylbenzene	0.92	Not Detected	4.5	Not Detected
Chloromethane	3.7	Not Detected	7.6	Not Detected
1,2,4-Trichlorobenzene	3.7	Not Detected	27	Not Detected
Hexachlorobutadiene	3.7	Not Detected	39	Not Detected
Acetone	3.7	Not Detected	8.7	Not Detected
Carbon Disulfide	0.92	Not Detected	2.8	Not Detected
2-Propanol	3.7	Not Detected	9.0	Not Detected
trans-1,2-Dichloroethene	0.92	Not Detected	3.6	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.92	Not Detected	2.7	Not Detected
Tetrahydrofuran	0.92	Not Detected	2.7	Not Detected
1,4-Dioxane	3.7	Not Detected	13	Not Detected
4-Methyl-2-pentanone	0.92	Not Detected	3.7	Not Detected
2-Hexanone	3.7	Not Detected	15	Not Detected
Bromoform	0.92	Not Detected	9.4	Not Detected
4-Ethyltoluene	0.92	Not Detected	4.5	Not Detected
Ethanol	3.7	Not Detected	6.9	Not Detected
Methyl tert-butyl ether	0.92	Not Detected	3.3	Not Detected
3-Chloropropene	3.7	Not Detected	11	Not Detected
2,2,4-Trimethylpentane	0.92	Not Detected	4.3	Not Detected
Naphthalene	3.7	Not Detected	19	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	108	70-130
1,2-Dichloroethane-d4	92	70-130
4-Bromofluorobenzene	94	70-130

Report Date: 12-Feb-2008 18:23

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/03Feb2008.b/t020315.d
 Lab Smp Id: 0801560-01A
 Inj Date : 04-FEB-2008 01:28
 Operator : ab Inst ID: msdt.i
 Smp Info : 200mL #23988
 Misc Info : 8.0"Hg-5psi
 Comment :
 Method : /chem/msdt.i/03Feb2008.b/t14q1213e.m
 Meth Date : 03-Feb-2008 18:54 dmendoza Quant Type: ISTD
 Cal Date : 25-JAN-2008 13:09 Cal File: t012506.d
 Als bottle: 1
 Dil Factor: 1.83000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	341537	25.0000		80.00- 120.00	100.00	
13.886	13.886	(1.000)	128	261983			29.43- 129.43	76.71	
13.858	13.886	(1.000)	49	377289			119.82- 219.82	110.47	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1249407	25.0000		80.00- 120.00	100.00	
15.628	15.628	(1.000)	88	210913			0.00- 66.60	16.88	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1211327	25.0000		80.00- 120.00	100.00	
20.798	20.798	(1.000)	82	682305			5.74- 105.74	56.33	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.076)	65	501975	23.0842	23.084	80.00- 120.00	100.00	
14.936	14.936	(1.076)	67	249951			3.93- 103.93	49.79	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1281750	27.0437	27.044	80.00- 120.00	100.00	
18.199	18.199	(1.165)	70	143621			0.00- 61.06	11.21	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 113 Toluene-d8 (continued)

18.199	18.199	(1.165)	100	864879			18.52- 118.52	67.48
--------	--------	---------	-----	--------	--	--	---------------	-------

\$ 137 Bromofluorobenzene

CAS #: 460-00-4

22.789	22.789	(1.096)	174	780494	23.4926	23.492	80.00- 120.00	100.00
22.789	22.789	(1.096)	95	981445			75.43- 175.43	125.75
22.789	22.789	(1.096)	176	766752			47.55- 147.55	98.24

Report Date: 12-Feb-2008 18:23

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msdt.i
Lab File ID: t020315.d
Lab Smp Id: 0801560-01ACalibration Date: 03-FEB-2008
Calibration Time: 15:01

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m

Misc Info: 8.0"Hg-5psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	323259	193955	452563	341537	5.65
97 1,4-Difluorobenze	1297188	778313	1816063	1249407	-3.68
126 Chlorobenzene-d5	1219852	731911	1707793	1211327	-0.70

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 03Feb2008
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0801560-01A
Level: LOW Operator: ab
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 2926Spectra.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m
Misc Info: 8.0"Hg-5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 90 1,2-Dichloroethane	25.000	23.084	92.34	70-130
\$ 113 Toluene-d8	25.000	27.044	108.17	70-130
\$ 137 Bromofluorobenzene	25.000	23.492	93.97	70-130

Data File: /chem/msdt,i/03Feb2008,b/t020315.d

Date : 04-FEB-2008 01:28

Client ID:


Sample Info: 200mL #23988

Column phase: RTX-624

Instrument: msdt,i

Operator: ab

Column diameter: 0.53

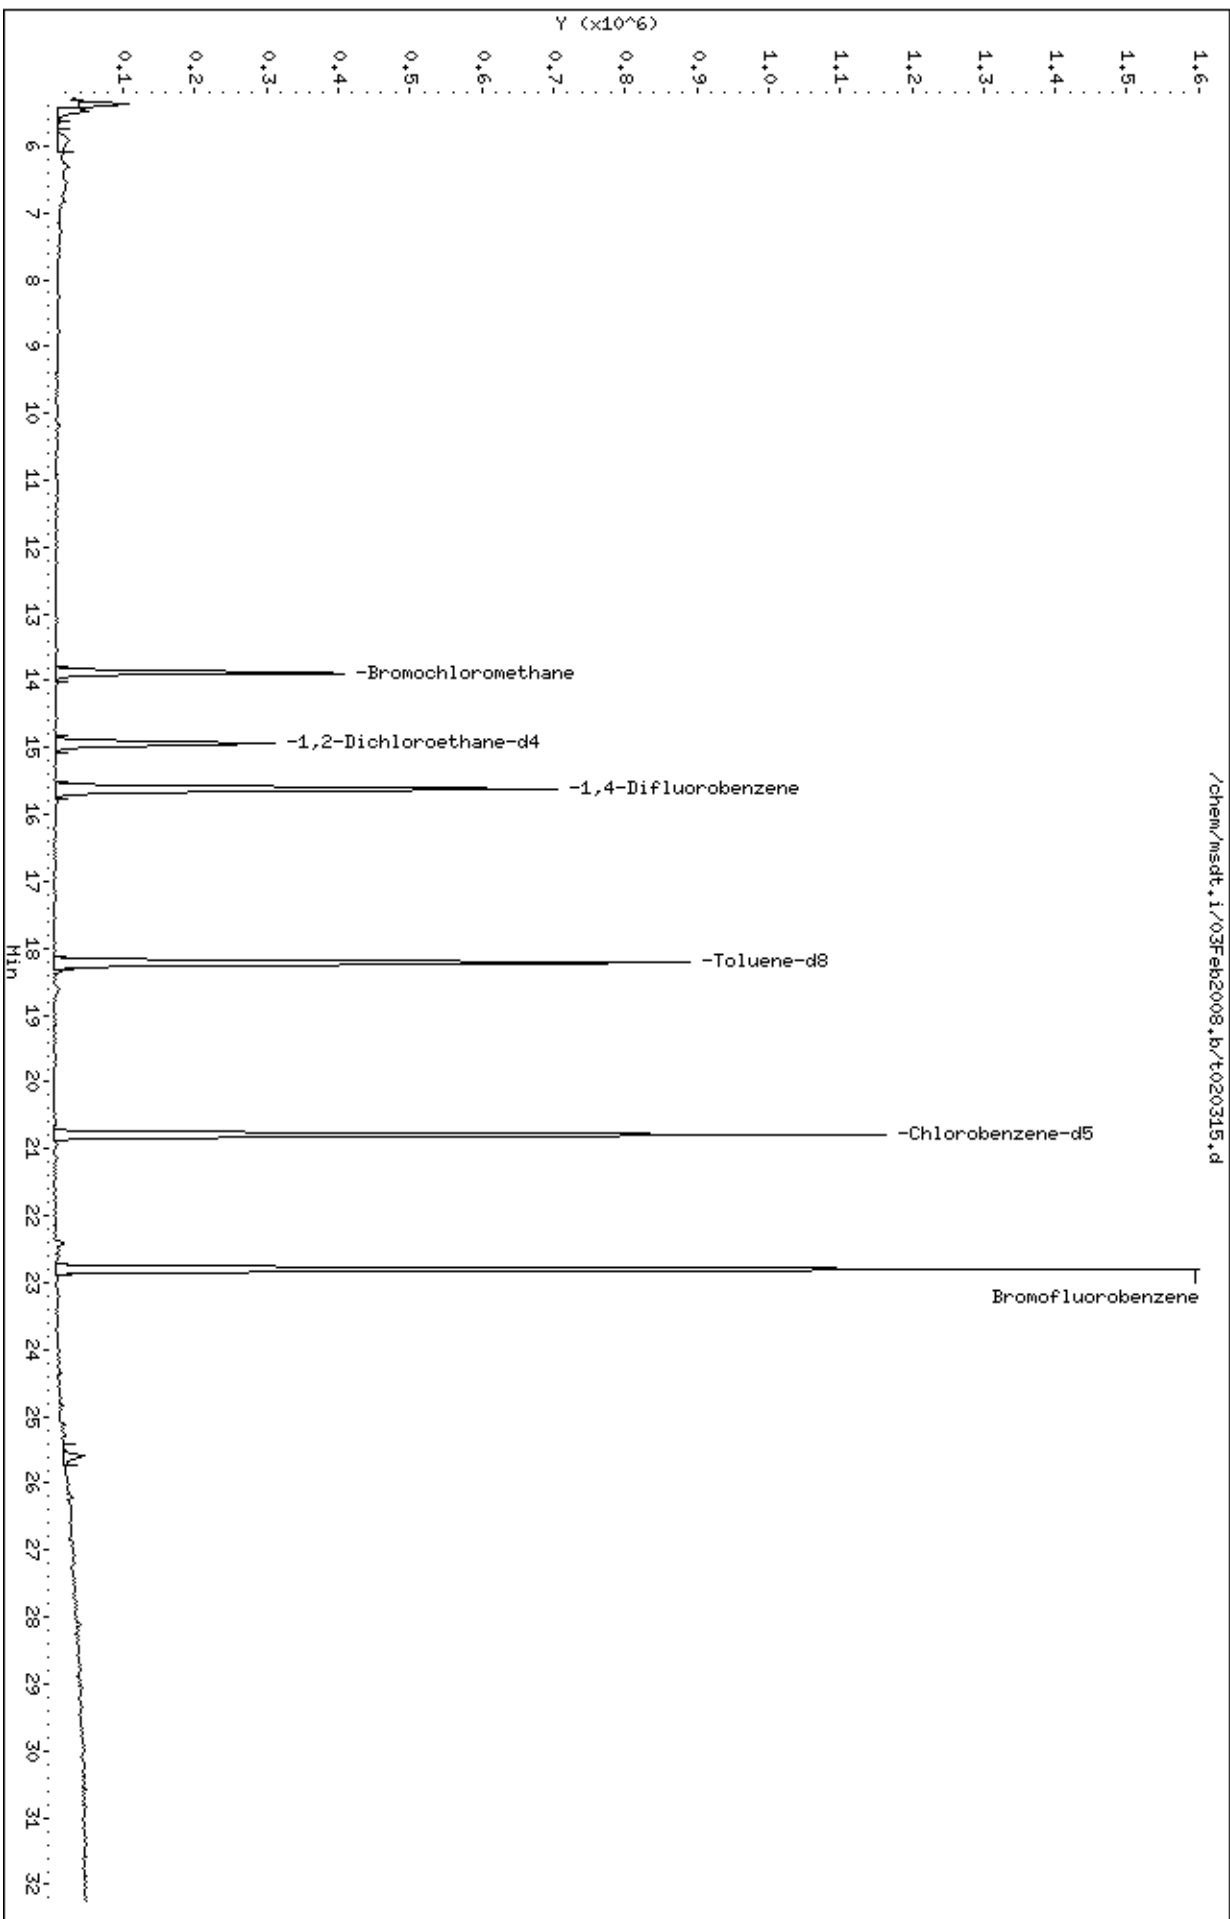



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Summary of Detected Compounds
MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: UW AMS 5

Lab ID#: 0801560-02A

No Detections Were Found.



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: UW AMS 5

Lab ID#: 0801560-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020316	Date of Collection:	1/30/08
Dil. Factor:	1.71	Date of Analysis:	2/4/08 02:18 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.86	Not Detected	4.2	Not Detected
Freon 114	0.86	Not Detected	6.0	Not Detected
Vinyl Chloride	0.86	Not Detected	2.2	Not Detected
Bromomethane	0.86	Not Detected	3.3	Not Detected
Chloroethane	0.86	Not Detected	2.2	Not Detected
Freon 11	0.86	Not Detected	4.8	Not Detected
1,1-Dichloroethene	0.86	Not Detected	3.4	Not Detected
Freon 113	0.86	Not Detected	6.6	Not Detected
Methylene Chloride	0.86	Not Detected	3.0	Not Detected
1,1-Dichloroethane	0.86	Not Detected	3.5	Not Detected
cis-1,2-Dichloroethene	0.86	Not Detected	3.4	Not Detected
Chloroform	0.86	Not Detected	4.2	Not Detected
1,1,1-Trichloroethane	0.86	Not Detected	4.7	Not Detected
Carbon Tetrachloride	0.86	Not Detected	5.4	Not Detected
Benzene	0.86	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.86	Not Detected	3.5	Not Detected
Trichloroethene	0.86	Not Detected	4.6	Not Detected
1,2-Dichloropropane	0.86	Not Detected	4.0	Not Detected
cis-1,3-Dichloropropene	0.86	Not Detected	3.9	Not Detected
Toluene	0.86	Not Detected	3.2	Not Detected
trans-1,3-Dichloropropene	0.86	Not Detected	3.9	Not Detected
1,1,2-Trichloroethane	0.86	Not Detected	4.7	Not Detected
Tetrachloroethene	0.86	Not Detected	5.8	Not Detected
1,2-Dibromoethane (EDB)	0.86	Not Detected	6.6	Not Detected
Chlorobenzene	0.86	Not Detected	3.9	Not Detected
Ethyl Benzene	0.86	Not Detected	3.7	Not Detected
m,p-Xylene	0.86	Not Detected	3.7	Not Detected
o-Xylene	0.86	Not Detected	3.7	Not Detected
Styrene	0.86	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.86	Not Detected	5.9	Not Detected
1,3,5-Trimethylbenzene	0.86	Not Detected	4.2	Not Detected
1,2,4-Trimethylbenzene	0.86	Not Detected	4.2	Not Detected
1,3-Dichlorobenzene	0.86	Not Detected	5.1	Not Detected
1,4-Dichlorobenzene	0.86	Not Detected	5.1	Not Detected
alpha-Chlorotoluene	0.86	Not Detected	4.4	Not Detected
1,2-Dichlorobenzene	0.86	Not Detected	5.1	Not Detected
1,3-Butadiene	0.86	Not Detected	1.9	Not Detected
Hexane	0.86	Not Detected	3.0	Not Detected
Cyclohexane	0.86	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: UW AMS 5

Lab ID#: 0801560-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020316	Date of Collection:	1/30/08
Dil. Factor:	1.71	Date of Analysis:	2/4/08 02:18 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.86	Not Detected	3.5	Not Detected
Bromodichloromethane	0.86	Not Detected	5.7	Not Detected
Dibromochloromethane	0.86	Not Detected	7.3	Not Detected
Cumene	0.86	Not Detected	4.2	Not Detected
Propylbenzene	0.86	Not Detected	4.2	Not Detected
Chloromethane	3.4	Not Detected	7.1	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	Not Detected	8.1	Not Detected
Carbon Disulfide	0.86	Not Detected	2.7	Not Detected
2-Propanol	3.4	Not Detected	8.4	Not Detected
trans-1,2-Dichloroethene	0.86	Not Detected	3.4	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.86	Not Detected	2.5	Not Detected
Tetrahydrofuran	0.86	Not Detected	2.5	Not Detected
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.86	Not Detected	3.5	Not Detected
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.86	Not Detected	8.8	Not Detected
4-Ethyltoluene	0.86	Not Detected	4.2	Not Detected
Ethanol	3.4	Not Detected	6.4	Not Detected
Methyl tert-butyl ether	0.86	Not Detected	3.1	Not Detected
3-Chloropropene	3.4	Not Detected	11	Not Detected
2,2,4-Trimethylpentane	0.86	Not Detected	4.0	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	106	70-130
1,2-Dichloroethane-d4	94	70-130
4-Bromofluorobenzene	96	70-130

Report Date: 12-Feb-2008 18:23

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/03Feb2008.b/t020316.d
 Lab Smp Id: 0801560-02A
 Inj Date : 04-FEB-2008 02:18
 Operator : ab Inst ID: msdt.i
 Smp Info : 200mL #34343
 Misc Info : 6.5"Hg-5psi
 Comment :
 Method : /chem/msdt.i/03Feb2008.b/t14q1213e.m
 Meth Date : 03-Feb-2008 18:54 dmendoza Quant Type: ISTD
 Cal Date : 25-JAN-2008 13:09 Cal File: t012506.d
 Als bottle: 1
 Dil Factor: 1.71000
 Integrator: HP RTE Compound Sublist: AT04.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	330741	25.0000		80.00- 120.00	100.00	
13.886	13.886	(1.000)	128	254951			29.43- 129.43	77.08	
13.858	13.886	(1.000)	49	376544			119.82- 219.82	113.85	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1233922	25.0000		80.00- 120.00	100.00	
15.628	15.628	(1.000)	88	198383			0.00- 66.60	16.08	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1179960	25.0000		80.00- 120.00	100.00	
20.798	20.798	(1.000)	82	669730			5.74- 105.74	56.76	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.076)	65	493764	23.4478	23.448	80.00- 120.00	100.00	
14.936	14.936	(1.076)	67	243778			3.93- 103.93	49.37	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1246510	26.6302	26.630	80.00- 120.00	100.00	
18.199	18.199	(1.165)	70	142338			0.00- 61.06	11.42	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 113 Toluene-d8 (continued)

18.199 18.199 (1.165) 100 833753 18.52- 118.52 66.89

\$ 137 Bromofluorobenzene

CAS #: 460-00-4

22.789 22.789 (1.096) 174 778440 24.0536 24.054 80.00- 120.00 100.00

22.789 22.789 (1.096) 95 963276 75.43- 175.43 123.74

22.789 22.789 (1.096) 176 744774 47.55- 147.55 95.68

Report Date: 12-Feb-2008 18:23

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARYInstrument ID: msdt.i
Lab File ID: t020316.d
Lab Smp Id: 0801560-02ACalibration Date: 03-FEB-2008
Calibration Time: 15:01

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m

Misc Info: 6.5"Hg-5psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	323259	193955	452563	330741	2.31
97 1,4-Difluorobenze	1297188	778313	1816063	1233922	-4.88
126 Chlorobenzene-d5	1219852	731911	1707793	1179960	-3.27

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 03Feb2008
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: 0801560-02A
Level: LOW Operator: ab
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 2926Spectra.spk Quant Type: ISTD
Sublist File: AT04.sub
Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m
Misc Info: 6.5"Hg-5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 90 1,2-Dichloroethane	25.000	23.448	93.79	70-130
\$ 113 Toluene-d8	25.000	26.630	106.52	70-130
\$ 137 Bromofluorobenzene	25.000	24.054	96.21	70-130

Data File: /chem/msdt,i/03Feb2008,b/t020316.d

Date : 04-FEB-2008 02:18

Client ID:

Sample Info: 200mL #34343


Column phase: RTX-624

Instrument: msdt,i

Operator: ab

Column diameter: 0.53

/chem/msdt,i/03Feb2008,b/t020316.d

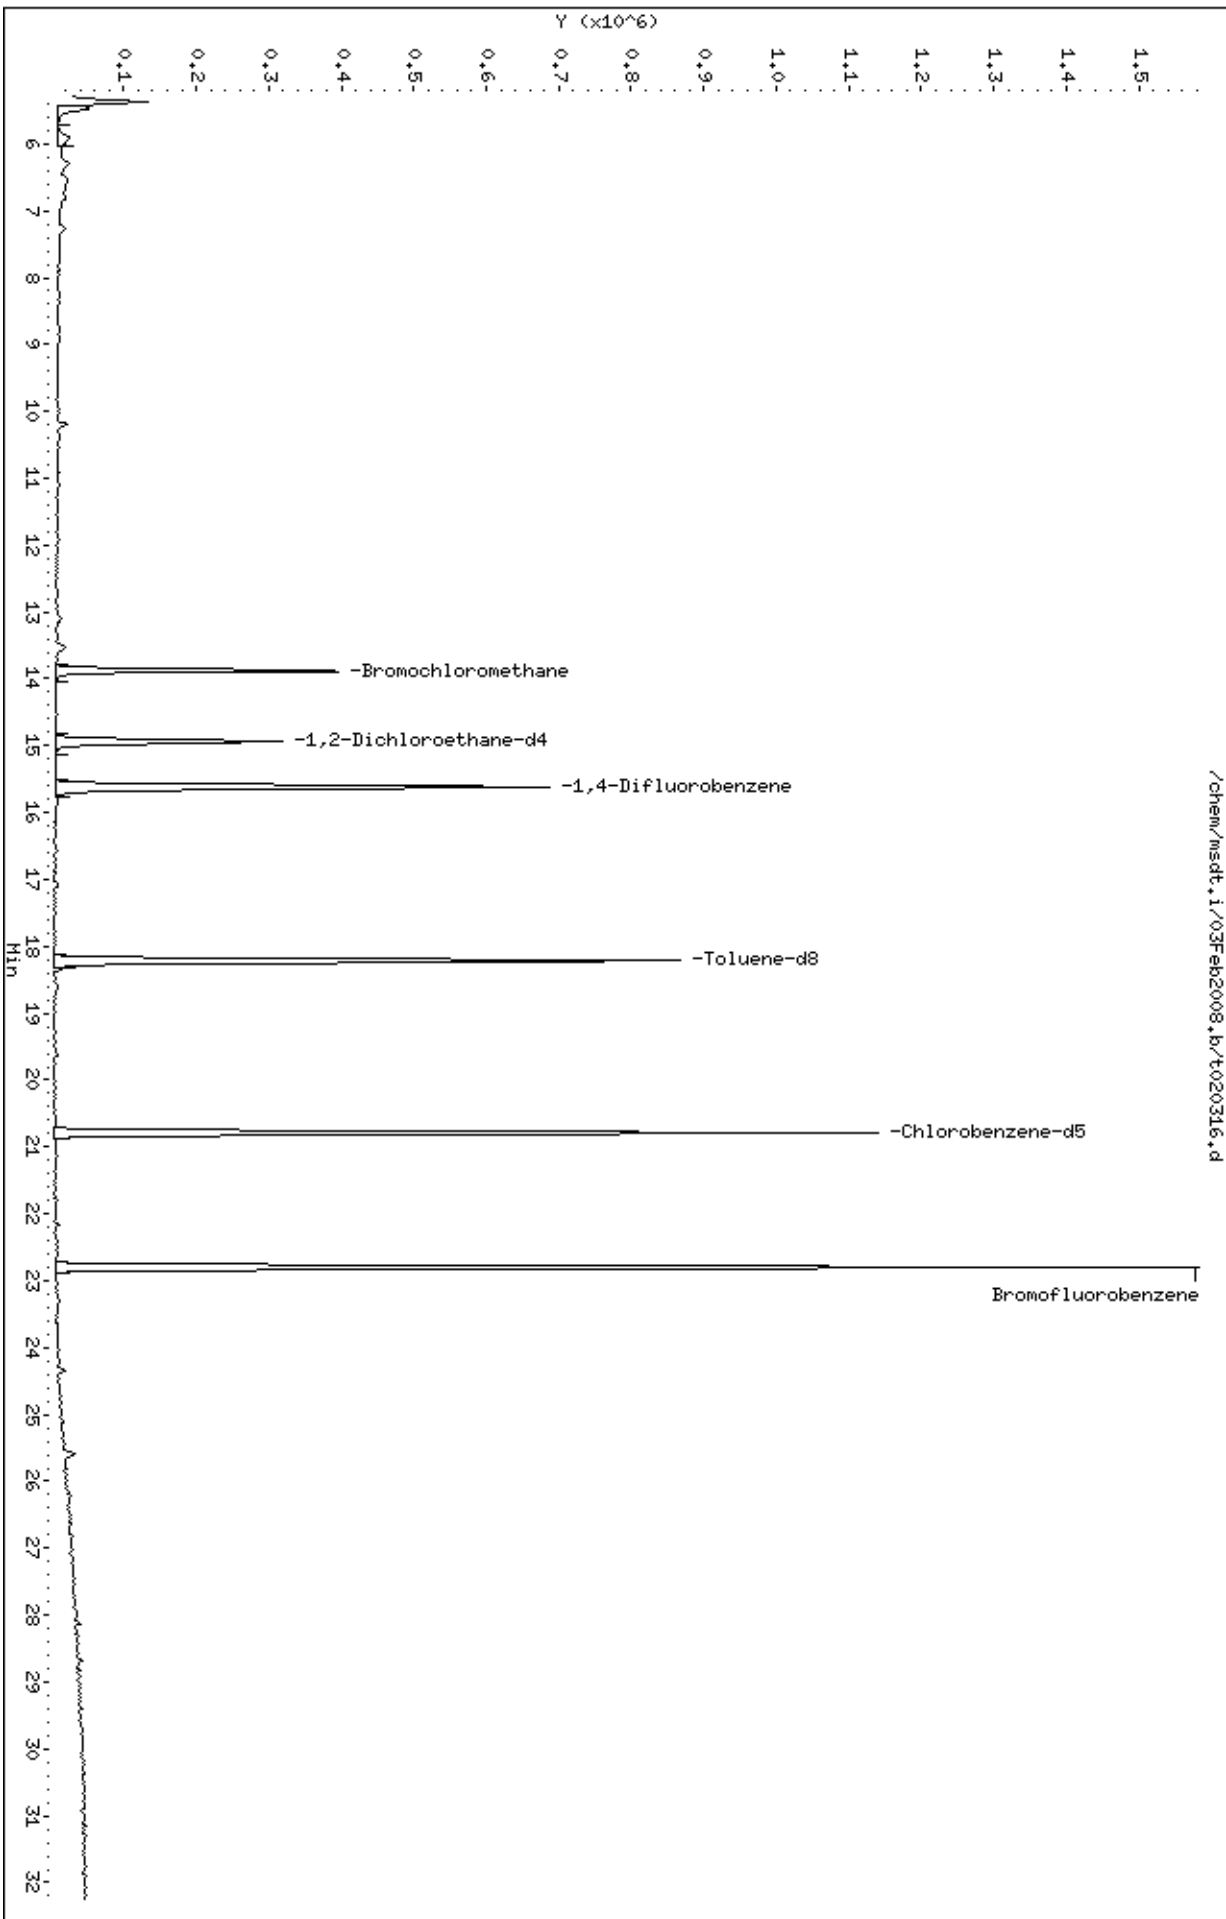

QC Results and Raw Data



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0801560-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020304	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 2/3/08 04:33 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0801560-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020304	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 2/3/08 04:33 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected	2.0	Not Detected
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	108	70-130
1,2-Dichloroethane-d4	97	70-130
4-Bromofluorobenzene	93	70-130

Report Date: 03-Feb-2008 16:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/03Feb2008.b/t020304.d
 Lab Smp Id: lab Blank Client Smp ID: Lab Blank
 Inj Date : 03-FEB-2008 16:33
 Operator : xp Inst ID: msdt.i
 Smp Info : 200mL #12009
 Misc Info : Humid
 Comment :
 Method : /chem/msdt.i/03Feb2008.b/t14q1213e.m
 Meth Date : 03-Feb-2008 15:20 dmendoza Quant Type: ISTD
 Cal Date : 25-JAN-2008 13:09 Cal File: t012506.d
 Als bottle: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	324973	25.0000		80.00- 120.00	100.00	
13.886	13.886	(1.000)	128	253977			29.43- 129.43	78.15	
13.886	13.858	(1.000)	49	375927			119.82- 219.82	115.68	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1245386	25.0000		80.00- 120.00	100.00	
15.628	15.628	(1.000)	88	208529			0.00- 66.60	16.74	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1218207	25.0000		80.00- 120.00	100.00	
20.798	20.798	(1.000)	82	688922			5.74- 105.74	56.55	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.076)	65	500200	24.1751	24.175	80.00- 120.00	100.00	
14.936	14.936	(1.076)	67	246129			3.93- 103.93	49.21	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1279492	27.0832	27.083	80.00- 120.00	100.00	
18.199	18.199	(1.165)	70	148115			0.00- 61.06	11.58	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
== =====

\$ 113 Toluene-d8 (continued)

18.199 18.199 (1.165) 100 874228 18.52- 118.52 68.33

\$ 137 Bromofluorobenzene

CAS #: 460-00-4

22.789 22.789 (1.096) 174 776669 23.2454 23.245 80.00- 120.00 100.00

22.789 22.789 (1.096) 95 962204 75.43- 175.43 123.89

22.789 22.789 (1.096) 176 758186 47.55- 147.55 97.62

Report Date: 03-Feb-2008 16:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 03-FEB-2008

Lab File ID: t020304.d

Calibration Time: 15:01

Lab Smp Id: lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: xp

Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m

Misc Info: Humid

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	323259	193955	452563	324973	0.53
97 1,4-Difluorobenze	1297188	778313	1816063	1245386	-3.99
126 Chlorobenzene-d5	1219852	731911	1707793	1218207	-0.13

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 03Feb2008
Sample Matrix: GAS Fraction: VOA
Lab Smp Id: lab Blank Client Smp ID: Lab Blank
Level: LOW Operator: xp
Data Type: MS DATA SampleType: SAMPLE
SpikeList File: 2926Spectra.spk Quant Type: ISTD
Sublist File: AT04ENSR.sub
Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m
Misc Info: Humid

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 90 1,2-Dichloroethane	25.000	24.175	96.70	70-130
\$ 113 Toluene-d8	25.000	27.083	108.33	70-130
\$ 137 Bromofluorobenzene	25.000	23.245	92.98	70-130

Data File: /chem/msdt,i/03Feb2008,b/t020304.d

Date : 03-FEB-2008 16:33

Client ID: Lab Blank

Sample Info: 200mL #12009


Column phase: RTX-624

Instrument: msdt,i

Operator: xp

Column diameter: 0.53

/chem/msdt,i/03Feb2008,b/t020304.d

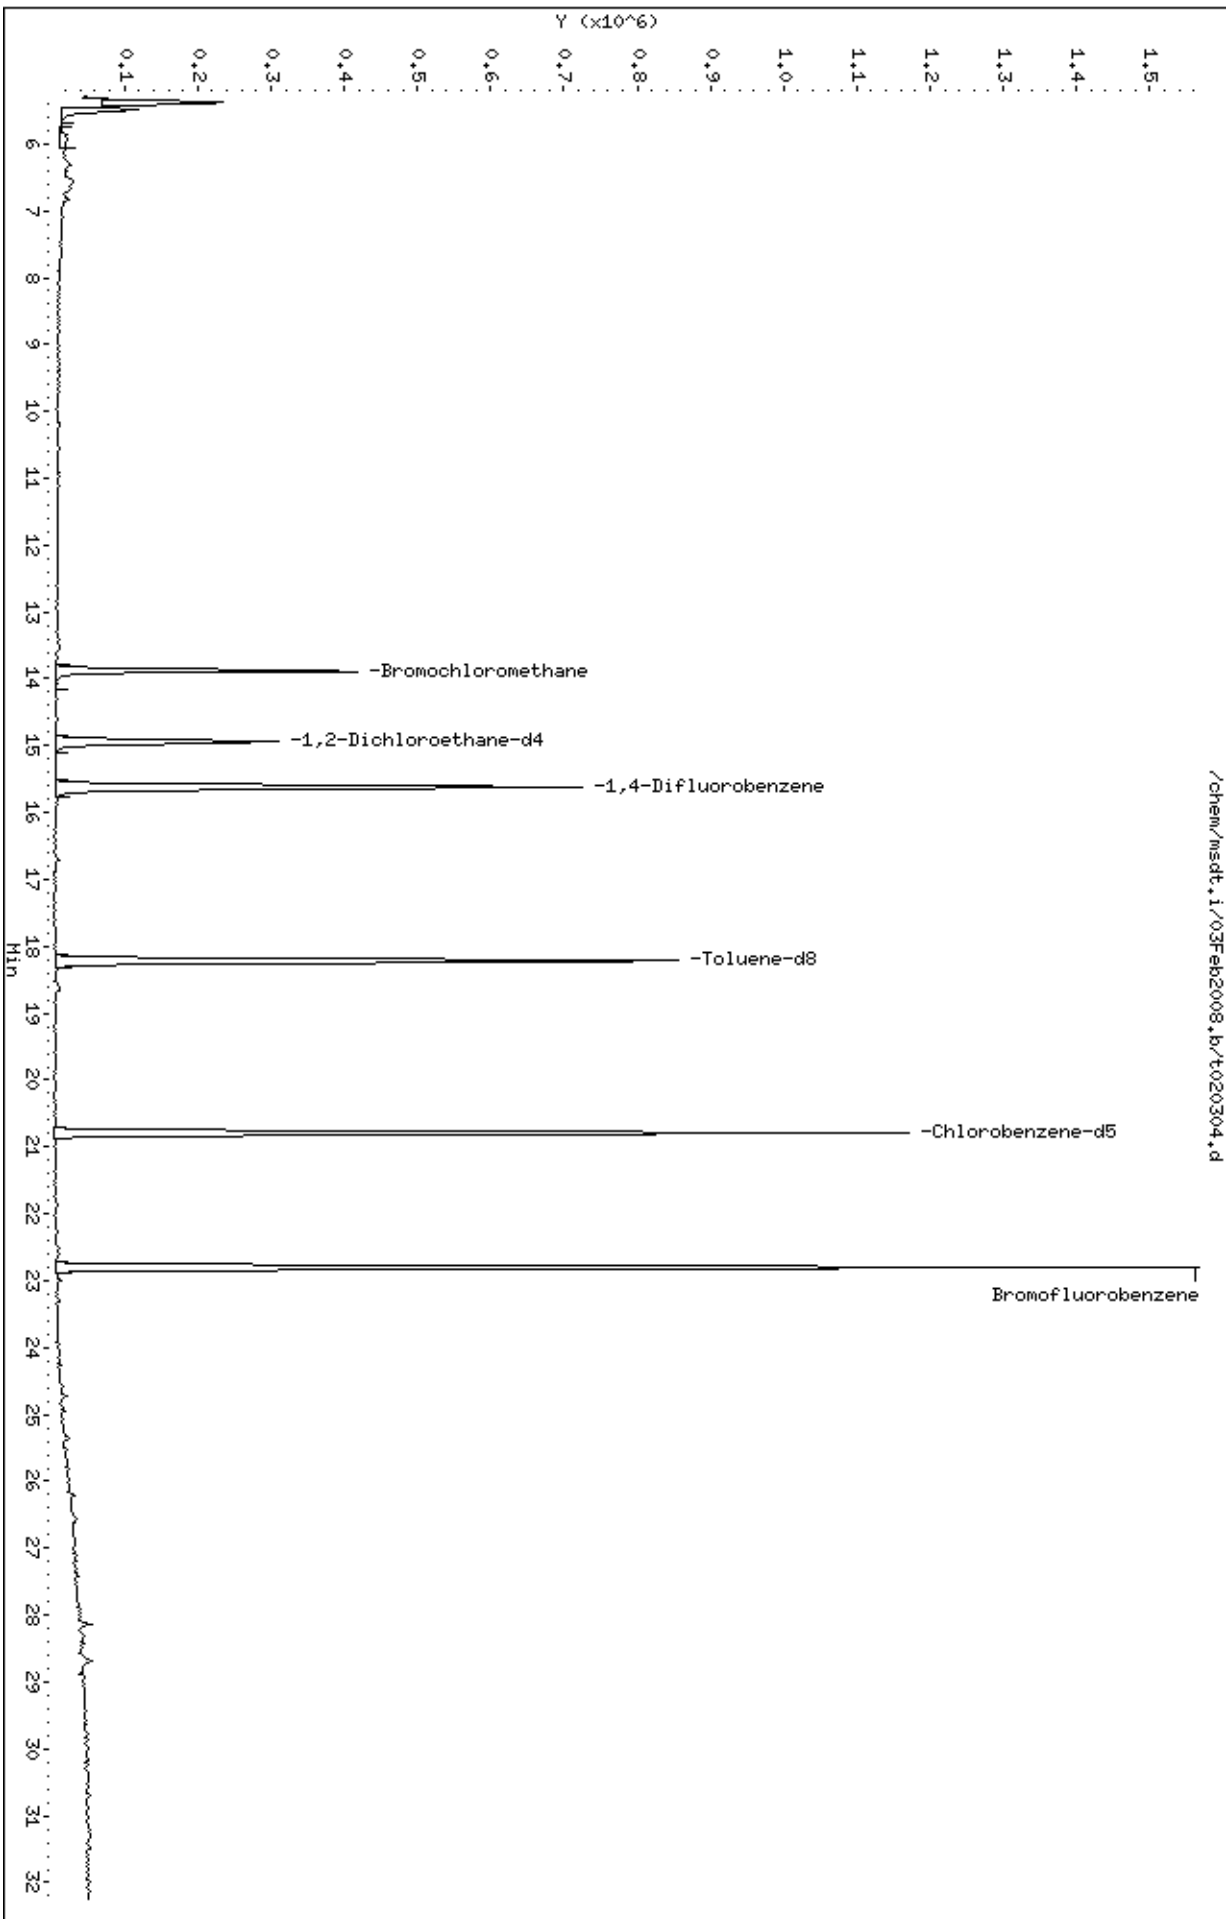

LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0801560

	CLIENT SAMPLE NO.	SURROGATE % RECOVERY						TOTAL OUT
		1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#	
01	DW AMS 3	92		108		94		0
02	UW AMS 5	94		106		96		0
03	Lab Blank	97		108		93		0
04	CCV	103		108		96		0
05	LCS	100		106		95		0
06								0
07								0
08								0
09								0
10								0
11								0
12								0
13								0
14								0
15								0
16								0
17								0
18								0
19								0
20								0
21								0
22								0
23								0
24								0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

* Designates values outside of QC limits

LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD
 Lab File ID: t020302.d
 Instrument ID: msdt.i

SDG No: 0801560
 Date Analyzed: 02/03/2008
 Time Analyzed: 03:01 PM

	Chlorobenzene-d5		RT		1,4-Difluorobenzene		RT		Bromochloromethane		RT	
	Area	#		#	Area	#		#	Area	#		#
	24-HOUR STD	1219852		20.8	1297188		15.63		323259		13.89	
	UPPER LIMIT	1707793		21.13	1816063		15.96		452563		14.22	
	LOWER LIMIT	731911		20.47	778313		15.30		193955		13.56	
	CLIENT SAMPLE NO											
01	DW AMS 3	1211327		20.8	1249407		15.63		341537		13.89	
02	UW AMS 5	1179960		20.8	1233922		15.63		330741		13.89	
03	Lab Blank	1218207		20.8	1245386		15.63		324973		13.89	
04	CCV	1219852		20.8	1297188		15.63		323259		13.89	
05	LCS	1254995		20.8	1343796		15.63		339461		13.89	
06												
07												
08												
09												
10												
11												
12												
13												
14												
15												
16												
17												
18												
19												
20												
21												
22												

'Area Upper Limit=+40% of internal standard area'
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT
 RT Lower Limit=-0.33 minutes of internal standard RT

* Designates values outside of QC limits

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Calibration File Names:

- Level 1: /chem/msdt.i/13Dec2007.b/t121310.d
- Level 2: /chem/msdt.i/16Jan2008.b/t011608.d
- Level 3: /chem/msdt.i/25Jan2008.b/t012504.d
- Level 4: /chem/msdt.i/16Jan2008.b/t011604.d
- Level 5: /chem/msdt.i/25Jan2008.b/t012505.d
- Level 6: /chem/msdt.i/16Jan2008.b/t011605.d
- Level 7: /chem/msdt.i/25Jan2008.b/t012506.d

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	___	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
1 Dimethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
204 Propane	+++++	+++++	0.29962	0.32447	0.30263	0.29227	0.30085	4.929
2 Isobutylene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
3 Acetaldehyde	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
4 2-Methyl-1-Butene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
5 Freon 143a	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
6 Freon142b	+++++	+++++	3.08653	3.00915	3.53508	+++++	3.23048	7.285

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
7 Propanal	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
8 Freon 14	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
9 Freon 13	+++++	+++++	3.04829	3.07678	3.13145	+++++		
	3.42476						3.17032	5.460
199 Vinyl Fluoride	+++++	+++++	0.76573	+++++	0.76590	+++++		
	0.47518						0.66894	25.084
13 Freon 134a	+++++	+++++	1.38440	1.32417	1.51576	+++++		
	1.48957						1.42848	6.284
10 Bromoethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
11 Propylene	+++++	+++++	0.70578	0.71805	0.65380	0.63314		
	0.62764						0.66768	6.255
15 Freon 152a	+++++	+++++	0.92721	0.66273	0.71513	+++++		
	0.73806						0.76079	15.162
12 Dichlorodifluoromethane/Fr12	+++++	3.97468	4.32102	4.84823	4.47789	4.42973		
	4.22044						4.37866	6.655
17 Freon 22	+++++	+++++	0.39765	0.37366	0.40074	+++++		
	0.39163						0.39092	3.098

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000		
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	% RSD
	200.000							
	Level 7							
14 2,3-Dimethylbutane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
16 Freon 114	+++++	2.32278	2.53064	3.23968	3.11448	3.06128		
	2.90616						2.86250	12.582
18 Chloromethane	+++++	+++++	1.01700	0.96604	0.88370	0.94394		
	0.92490						0.94711	5.217
21 Isobutane	+++++	+++++	2.08245	+++++	2.09100	+++++		
	2.01177						2.06174	2.109
20 Vinyl Chloride	+++++	0.88270	1.14648	1.30894	1.25479	1.28727		
	1.22751						1.18461	13.367
19 Butane	+++++	+++++	0.20998	0.26199	0.25935	0.24850		
	0.23330						0.24262	8.845
22 1,3-Butadiene	+++++	0.71853	0.85769	1.03955	1.01395	0.99572		
	0.92299						0.92474	13.084
26 Methanol	+++++	+++++	0.43916	0.27587	0.28466	+++++		
	0.29382						0.32338	23.977
25 Bromomethane	+++++	1.01327	1.17226	1.31389	1.29715	1.34974		
	1.38088						1.25453	11.007
28 2,4-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
27 Chloroethane	200.000 0.65651	0.50003	0.53398	0.71944	0.68949	0.69314		0.63210	14.554
29 Isopentane	1.29308	+++++	1.29517	1.45895	1.40134	1.38252		1.36621	5.239
30 2-Butanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
34 Dichlorofluoromethane/Fr21	2.50716	+++++	2.54089	2.34650	2.62565	+++++		2.50505	4.665
35 1-Pentene	1.35851	+++++	1.38741	+++++	1.43371	+++++		1.39321	2.723
31 Trichlorofluoromethane/Fr11	4.77418	3.87754	4.64132	5.56838	5.34096	5.16563		4.89467	12.393
37 Pentane	2.04655	+++++	1.87503	2.52225	2.39638	2.13339		2.19472	11.966
32 3-Methyl-1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
33 Vinyl Bromide	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
36 Methacrylonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
38 Ethanol	200.000 0.33637	+++++	0.26632	0.34866	0.35944	0.34902		0.33196	11.324
39 Ethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
40 Freon123a	2.02517	+++++	1.79398	1.78001	2.15034	+++++		1.93737	9.348
41 Freon123	2.75397	+++++	2.47248	2.50454	2.91059	+++++		2.66040	7.853
44 Acrolein	0.38090	+++++	0.34653	+++++	0.40647	+++++		0.37797	7.958
42 Freon 113	2.20694	1.96268	2.07987	2.35100	2.31070	2.30613		2.20289	6.946
43 1,1-Dichloroethene	2.03228	1.34194	1.86298	2.15199	2.09288	2.10298		1.93084	15.819
45 Acetone	0.55974	+++++	0.58549	0.62159	0.63428	0.59638		0.59950	4.923
46 2-Propanol	1.91807	+++++	1.64554	2.14997	2.16339	2.05269		1.98593	10.780
48 Ethyl acrylate	0.07357	+++++	0.05860	+++++	0.07082	+++++		0.06766	11.780

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
47 Carbon Disulfide	+++++	2.81195	3.34684	3.94302	3.91636	4.03685		
	4.03308						3.68135	13.536
49 Iodomethane	+++++	+++++	3.14942	+++++	3.85935	+++++		
	3.99178						3.66685	12.353
50 Methyl Methacrylate	+++++	+++++	0.34870	+++++	0.44246	+++++		
	0.44354						0.41157	13.229
23 Methyl acetate	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
51 3-Chloropropene	+++++	+++++	0.51758	0.63344	0.66908	0.67264		
	0.64877						0.62830	10.170
52 Acetonitrile	+++++	+++++	0.80223	+++++	0.44702	+++++		
	0.44229						0.56385	36.616
53 2-Methylpentane	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
55 Cyclopentene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
56 Cyclopentane	+++++	+++++	0.77409	+++++	0.97451	+++++		
	0.93084						0.89315	11.800
54 Methylene Chloride	+++++	1.26471	1.19310	1.28466	1.23919	1.18576		
	1.14830						1.21929	4.275

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
57 tert-Butyl-Alcohol	+++++	+++++	1.80493	1.95511	2.98361	+++++		
	2.79397						2.38441	24.775
58 Freon143a	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
59 2,3,4-Trimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
60 MTBE	+++++	2.86778	3.17953	4.70062	4.68724	4.63328		
	4.45264						4.08685	20.410
61 trans-1,2-Dichloroethene	+++++	1.16841	1.36846	1.59737	1.60693	1.58666		
	1.54862						1.47941	11.920
62 Acrylonitrile	+++++	+++++	0.85828	+++++	0.94889	+++++		
	0.90459						0.90392	5.012
66 1-Hexene	+++++	+++++	0.63120	+++++	0.92100	+++++		
	0.93536						0.82919	20.696
63 2-Pentanone	+++++	+++++	0.56835	+++++	0.80169	+++++		
	0.81748						0.72917	19.131
64 Pentanal	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
65 Hexane	+++++	1.57867	1.69330	2.32975	2.33470	2.28726		
	2.10047						2.05402	16.401

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
67 2,4,4-Trimethyl-1-pentene	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
	+++++						+++++	+++++
68 Isopropyl ether	+++++	+++++	3.05046	3.11756	3.99770	+++++		
	4.22863						3.59859	16.735
69 Vinyl Acetate	+++++	+++++	0.20790	0.39420	0.42239	0.41174		
	0.39644						0.36654	24.398
70 1,1-Dichloroethane	+++++	1.89113	2.33908	2.90168	2.91414	2.81166		
	2.62404						2.58029	15.534
71 1-Propanol	+++++	+++++	0.22966	0.19476	0.26447	+++++		
	0.25614						0.23626	13.288
24 Chloroprene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
72 2,4,4-Trimethyl-2-pentene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
73 t-Butylethyl Ether	+++++	+++++	3.16677	3.48183	4.44427	+++++		
	4.62588						3.92969	18.186
74 Butanal	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
77 Ethyl Acetate	+++++	+++++	0.37523	0.36665	0.44766	+++++		
	0.44002						0.40739	10.395

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
78 2,2-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
75 2-Butanone	+++++	0.45590	0.48939	0.78234	0.81777	0.80248		0.68300	24.136
76 cis-1,2-Dichloroethene	+++++	1.42102	1.76263	2.03003	2.00229	1.88647		1.81216	12.248
79 Methyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
80 Tetrahydrofuran	+++++	0.62943	0.97571	1.29337	1.28127	1.22096		1.08841	23.310
82 Chloroform	1.93020	2.22348	2.95375	3.71813	3.62342	3.45338		3.01922	23.070
84 2,3-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
83 1,1,1-Trichloroethane	+++++	2.71849	3.26457	4.14088	3.99320	3.90473		3.61566	14.808
85 Cyclohexane	+++++	1.15872	1.50949	2.10026	2.12733	2.12851		1.84523	22.340
86 1-Bromo-2-Chloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
88 1,1-Dichloropropene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
87 Carbon Tetrachloride	+++++	2.41406	3.39973	4.11587	3.91507	3.78677		3.52165	17.133
99 Isobutanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
89 2,2,4-Trimethylpentane	+++++	3.37333	4.16527	6.15007	5.92173	5.82002		5.14568	21.740
91 Benzene	0.79154	0.74919	0.97744	1.11276	1.11446	1.11006		0.99818	16.470
92 tert-amyl-Methyl Ether	+++++	+++++	2.74382	3.09909	4.09898	+++++		3.58558	22.035
96 2-Heptanone	+++++	+++++	1.24936	1.55886	2.50284	+++++		2.01400	35.863
93 1,2-Dichloroethane	+++++	0.38488	0.48190	0.55269	0.54393	0.52114		0.49858	12.289
94 Heptane	+++++	0.20489	0.26652	0.35522	0.36144	0.35262		0.31708	20.836
95 Thiophene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	—	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	200.000							
	Level 7							
98 1-Butanol	+++++	+++++	0.11758	0.13858	0.22474	+++++		
	0.26717						0.18702	37.829
100 trans-1,4-dichloro-2-butene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
101 Trichloroethene	+++++	0.30755	0.42243	0.51510	0.50522	0.50991		
	0.50712						0.46122	17.993
102 Methyl Cyclohexane	+++++	1.53754	1.83216	2.72792	2.68033	2.67359		
	2.58776						2.33988	22.131
103 Alphamethylstyrene	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++
104 1,2-Dichloropropane	+++++	0.20715	0.30400	0.37024	0.37518	0.36979		
	0.37498						0.33356	20.315
106 1,4-Dioxane	+++++	+++++	0.22203	0.25610	0.27595	0.27947		
	0.28905						0.26452	10.060
105 Dibromomethane	+++++	+++++	0.51713	+++++	0.53966	+++++		
	0.52443						0.52707	2.181
107 Bromodichloromethane	+++++	0.50534	0.74489	0.89564	0.89167	0.88402		
	0.89199						0.80226	19.543
108 Epichlorohydrin	+++++	+++++	+++++	+++++	+++++	+++++		
	+++++						+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
200 2-Chloroethyl vinyl ether	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
109 Dodecane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
110 cis-1,3-Dichloropropene	+++++	0.30640	0.44286	0.60133	0.61573	0.62097	0.53720	24.865
111 4-Methyl-2-pentanone	+++++	0.13796	0.16184	0.27386	0.28990	0.29574	0.24442	30.435 <-
112 Octane	+++++	+++++	0.33718	0.37862	0.36858	0.35118	0.35661	4.689
114 Toluene	+++++	0.83239	1.12981	1.30873	1.30346	1.31419	1.20407	16.359
115 Undecane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
116 trans-1,3-Dichloropropene	+++++	0.41700	0.58275	0.77519	0.78627	0.74429	0.67657	21.773
117 1,1,2-Trichloroethane	+++++	0.28851	0.44339	0.58010	0.56523	0.53027	0.49075	22.392
120 Tetrachloroethene	+++++	0.45983	0.65186	0.79375	0.76614	0.71998	0.68395	17.565

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
121 2-Hexanone	+++++	+++++	0.20168	0.43260	0.45733	0.45334		
	0.46385						0.40176	27.992
118 1,3-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
119 Butyl Acetate	+++++	+++++	0.27684	0.28132	0.41784	+++++		
	0.43295						0.35224	24.052
122 Dibromochloromethane	+++++	0.51738	0.75336	1.02108	1.00364	0.94813		
	0.93216						0.86263	22.495
123 1,2-Dibromoethane	+++++	0.53395	0.72494	0.94104	0.94272	0.90240		
	0.90865						0.82562	19.905
127 Chlorobenzene	+++++	0.79354	1.15589	1.34681	1.30993	1.27196		
	1.27332						1.19191	17.233
124 Nonane	+++++	+++++	0.62153	0.85249	0.90555	0.82620		
	0.80999						0.80315	13.422
128 Ethyl Benzene	+++++	0.37185	0.51078	0.69793	0.69334	0.67176		
	0.67623						0.60365	22.126
125 1,1,1,2-Tetrachloroethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
129 m,p-Xylene	+++++	0.35609	0.60513	0.87709	0.87632	0.86382		
	0.87668						0.74252	29.317

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
130 o-Xylene	200.000 0.82624	0.36187	0.54084	0.82436	0.82113	0.81038		0.69747	28.523
131 Styrene	1.40128	0.54597	0.81319	1.33208	1.33982	1.34932		1.13028	31.851 <-
132 alpha-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
133 Bromoform	1.03034	0.52557	0.75472	1.02838	1.03414	1.02241		0.89926	23.733
134 Cumene	2.34324	1.13283	1.63286	2.28786	2.29534	2.26956		1.99362	25.051
135 Cyclohexanone	0.54440	+++++	0.28767	0.33246	0.50189	+++++		0.41660	30.143
140 1,1,2,2-Tetrachloroethane	1.27586	0.60007	0.98357	1.22729	1.23921	1.23277		1.09313	24.111
136 Bromobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
138 1,2,3-Trichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
142 Propylbenzene	2.97981	1.54927	2.01199	2.86787	2.86164	2.85800		2.52143	23.555

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
139 Decane	200.000 1.02738	+++++	0.64606	1.04271	1.08433	1.02284		0.96466	18.633
144 beta-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
145 4-Ethyltoluene	2.56845	1.07008	1.67504	2.47369	2.47772	2.47705		2.12367	28.889
141 2-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
147 1,3,5-Trimethylbenzene	2.07944	0.84480	1.39338	2.01760	2.03818	1.99616		1.72826	29.133
143 4-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
146 Diisobutyl Ketone	1.31745	+++++	0.67675	0.81426	1.22647	+++++		1.00873	30.862
148 tert-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
150 1,2,4-Trimethylbenzene	1.98573	0.81716	1.16747	1.86021	1.91982	1.90073		1.60852	30.567 <-
201 Pentachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
152 D-Limonene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
149 sec-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
151 bis(2-chloroethyl)ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
153 p-Cymene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
155 1,3-Dichlorobenzene	+++++	0.77778	1.12187	1.31936	1.35186	1.34638		1.21736	19.308
154 1,2,3-Trimethylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
156 1,4-Dichlorobenzene	+++++	0.85904	1.14176	1.35507	1.40212	1.39375		1.26490	17.794
157 Indan	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
159 alpha-Chlorotoluene	+++++	0.93964	1.28514	1.86740	2.06379	2.10823		1.75030	29.699
158 Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
160 Indene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
161 1,2-Dichlorobenzene	+++++	0.78507	1.01883	1.24430	1.30815	1.30062		1.16735	18.925
203 Hexachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
162 1,2-Dibromo-3-Chloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
163 Aniline	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
164 Isooctyl Alcohol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
165 1,2,4-Trichlorobenzene	+++++	+++++	0.51685	0.61758	0.91884	0.93633		0.80071	27.357
166 Hexachlorobutadiene	+++++	+++++	0.58993	0.60351	0.79170	0.81049		0.73084	17.094
167 Naphthalene	+++++	+++++	0.74401	0.94656	1.57407	1.60183		1.31984	33.576 <-
202 1,2,3-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09
 Quant Method : ISTD
 Origin : Disabled
 Target Version : 3.50
 Integrator : HP RTE
 Method file : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Cal Date : 25-Jan-2008 15:06 sruth
 Curve Type : Average

Compound	0.20000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
168 Quinoline	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
169 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
170 Isooctyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
\$ 90 1,2-Dichloroethane-d4	1.57449	1.47659	1.55272	1.65486	1.69109	1.59880		1.59173	4.367
\$ 113 Toluene-d8	0.93064	0.93484	0.94284	0.93991	0.94100	0.96874		0.94836	1.975
\$ 137 Bromofluorobenzene	0.68044	0.68452	0.69466	0.68353	0.67899	0.67591		0.68567	1.344

Calibration History

Method : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Start Cal Date: 13-DEC-2007 21:35
 End Cal Date : 25-JAN-2008 13:09

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.20000		
13-DEC-2007 21:35	AFCEElow	/chem/msdt.i/13Dec2007.b/t121310.d
Cal Level: 2 , Cal Amount: 0.50000		
16-JAN-2008 13:05	sp5d	/chem/msdt.i/16Jan2008.b/t011608.d
14-DEC-2007 09:58	AT04low+ENSR	/chem/msdt.i/13Dec2007.b/t121319.d
Cal Level: 3 , Cal Amount: 2.00000		
25-JAN-2008 11:27	sp12e	/chem/msdt.i/25Jan2008.b/t012504.d
16-JAN-2008 13:05	sp5d	/chem/msdt.i/16Jan2008.b/t011608.d
02-JAN-2008 10:39	sp22c	/chem/msdt.i/02Jan2008.b/t010202.d
19-DEC-2007 10:31	sp1b	/chem/msdt.i/19Dec2007.b/t121902.d
13-DEC-2007 23:51	AT04mdl+ENSR	/chem/msdt.i/13Dec2007.b/t121312.d
Cal Level: 4 , Cal Amount: 25.00000		
16-JAN-2008 10:18	sp5d	/chem/msdt.i/16Jan2008.b/t011604.d
02-JAN-2008 11:18	sp22c	/chem/msdt.i/02Jan2008.b/t010203.d
14-DEC-2007 00:40	AT04mdl+ENSR	/chem/msdt.i/13Dec2007.b/t121313.d
Cal Level: 5 , Cal Amount: 50.00000		
25-JAN-2008 12:14	sp12e	/chem/msdt.i/25Jan2008.b/t012505.d
16-JAN-2008 13:44	sp5d	/chem/msdt.i/16Jan2008.b/t011609.d
02-JAN-2008 12:02	sp22c	/chem/msdt.i/02Jan2008.b/t010204.d
19-DEC-2007 11:12	sp1b	/chem/msdt.i/19Dec2007.b/t121903.d
14-DEC-2007 01:23	AT04mdl+ENSR	/chem/msdt.i/13Dec2007.b/t121314.d
Cal Level: 6 , Cal Amount: 100.00000		
16-JAN-2008 10:57	sp5d	/chem/msdt.i/16Jan2008.b/t011605.d
14-DEC-2007 02:20	AT04mdl+ENSR	/chem/msdt.i/13Dec2007.b/t121315.d

-----+
| Cal Level: 7 , Cal Amount: 200.00000 |
-----+
-----+
-----+

25-JAN-2008 13:09	sp12e	/chem/msdt.i/25Jan2008.b/t012506.d
16-JAN-2008 11:40	sp5d	/chem/msdt.i/16Jan2008.b/t011606.d
02-JAN-2008 12:48	sp22c	/chem/msdt.i/02Jan2008.b/t010205.d
19-DEC-2007 12:21	sp1b	/chem/msdt.i/19Dec2007.b/t121904.d
14-DEC-2007 03:20	AT04mdl+ENSR	/chem/msdt.i/13Dec2007.b/t121316.d

-----+
-----+
-----+

Continuing Calibration

Ccal Level Mode: GLOBAL LEVEL 5

-----+
| Ccal Level: 5 , Ccal Amount: 50.000 |
-----+
-----+
-----+

25-JAN-2008 09:00	AT04ENSR	/chem/msdt.i/25Jan2008.b/t012502.d
-------------------	----------	------------------------------------

-----+
-----+
-----+

| Ccal Level: 5 , Ccal Amount: 50.000 |
-----+
-----+
-----+

25-JAN-2008 12:14	sp12eCCV	/chem/msdt.i/25Jan2008.b/t012505a.d
-------------------	----------	-------------------------------------

-----+
-----+
-----+

| Ccal Level: 5 , Ccal Amount: 50.000 |
-----+
-----+
-----+

25-JAN-2008 12:14	sp12e	/chem/msdt.i/25Jan2008.b/t012505.d
-------------------	-------	------------------------------------

-----+
-----+
-----+

Initial Calibration Narrative

A 7 point initial calibration was analyzed on MSD-T on December 13, 2007.

The following compounds used 0.2 ppbv as the lowest calibration concentration:

Chloroform and Benzene.

As noted on the accompanying analytical run log, the following points; 0.2ppbv, 0.5ppbv, and 2.0ppbv, were re-analyzed due to:

- a. an incorrect load

As noted on the accompanying analytical run log, the following point, 0.5ppbv, was re-analyzed due to:

- a. anomalous unacceptable linearity for various compounds

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	17.1e1
75	30.0 - 60.0% of mass 95	49.10
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.55
173	Less than 2.0% of mass 174	(0.77) ¹
174	Greater than 50.0% of mass 95	71.6e1e
175	5.0 - 9.0% of mass 174	(7.25) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(92.03) ¹
177	5.0 - 9.0% of mass 176	(6.41e) ²

BFB Injection Date: 12/13/07
 BFB Injection Time: 17:12
 BFB File ID: T121305
 Tekmar Purge Flow: 22.6 mL/min
 Vacuum: 4.24 x 10⁻⁵
 ISS Std #: 1443-356 Exp. Date: 2/5/08
 BCM 280754
 1,4-DFB 102601
 CB-d5 1033655
 Verified CCV IS vs ICAL mid-point (-40% D) *js*

Verify 176/174 m/z Ratio: $\frac{1290640}{1237521} \times 1000 = 97.021$

NOAH Cart #: NA File #: NA

File ID: T1213142
 Compound: Tol-DB
 Initials: *js*

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{sample}}}{\text{Areas}} \times \text{Conc.}_{\text{IS}} \times \text{RRF}$

$= \frac{(1112825)}{(1182601)} \times (25.0) \times (0.94836) = 24.806$

Reported Result: 24.806

#	File #	Sample / Client Name	Can #	Pressure	Am't Loaded	DF	Date Analyzed	Time Analyzed	Review Init	Comments
1	T121305	BFB Trace Check	140764	50 mg	2.0 µL	1.00	12/15/07	1417	SAS	
2	01e	System Blank	12009	Vuumed	800 µL	1.00		1743	SAS	
3	07	ICAL Level 1	1443538	0.2 µg/hr	0.2 µL	1.00		1854	SAS	Bad load
4	08			0.5 µg/hr	0.5 µL			1950	SAS	
5	09			2.0 µg/hr	2.0 µL			2046	SAS	
6	10	ICAL Level 1	1443538	0.2 µg/hr	0.2 µL	1.00		2135	SAS	
7	11			0.5 µg/hr	0.5 µL	1.00		2221	SAS	
8	12			2.0 µg/hr	2.0 µL	1.00		2351	SAS	
9	13			25 µg/hr	25 µL	1.00	12/14/07	0040	SAS	

James Brennan
 Signature

12/14/07
 Date

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	23.13
75	30.0 - 60.0% of mass 95	57.50
95	Base peak, 100.00% relative abundance	100
96	5.0 - 9.0% of mass 95	6.51
173	Less than 2.0% of mass 174	(0.90) ¹
174	Greater than 50.0% of mass 95	67.22
175	5.0 - 9.0% of mass 174	(7.36) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(96.57) ¹
177	5.0 - 9.0% of mass 176	(6.54) ²

BFB Injection Date: 12/19/07
 BFB Injection Time: 09:36
 BFB File ID: 6121901
 Tekmar Purge Flow: _____
 Vacuum: _____
 IS/S Std #: 1443-355 Exp. Date: 2/5/08
 BCM: 226250
 1,4-DFB: 954801
 CB-d5: 877836
 Verified CCV IS vs ICAL mid-point (-40% D) *[Signature]*

Verify 176/174 m/z Ratio: $\frac{682346/706622 \times 100}{96.57} = 66.57$

NOAH Cart #: 219 File #: 219

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{Sample}}}{\text{Area}_{\text{Std}}} \times \text{Conc.}_{\text{Std}} \times \text{RRF}$

$= \frac{(939704)}{(954801)} \times (25.0) \times (0.94836) = 25.944$ ppbv

Reported Result: 25.944 ppbv

File ID: 6121906
 Compound: T61-DB
 Initials: *[Signature]*

Use	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init	Comments
✓	6121901	BFB Time Chart	146264	50ppb	2ul	100	12/19/07	09:36	<i>[Signature]</i>	
✓	02	ICAL Lead 3	143-388	20ppb	20ul			10:31	<i>[Signature]</i>	614812136
✓	03	↓	↓	50ppb	50ul			11:12	<i>[Signature]</i>	SP16
✓	04	↓	↓	20ppb	20ul			12:21	<i>[Signature]</i>	
X	05	CCV-1 (20ppb)	1443-355	50ppb	50ul			13:21	<i>[Signature]</i>	
✓	06	CCV-1	↓	↓	↓			14:31	<i>[Signature]</i>	Short list only
✓	07	US-1	158-168	↓	↓			15:32	<i>[Signature]</i>	No RTEK ↓
✓	08	Lab blank	12009	Humid	20ul			16:32	<i>[Signature]</i>	
✓	09	0312264	34465	4.5% (4.5% →)	200ul	1.58		17:23	<i>[Signature]</i>	

[Signature]
 Signature

12/19/07
 Date

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	20.05
75	30.0 - 60.0% of mass 95	52.29
95	Base peak, 100.00% relative abundance	100
96	5.0 - 9.0% of mass 95	6.53
173	Less than 2.0% of mass 174	(0.84) ¹
174	Greater than 50.0% of mass 95	73.21
175	5.0 - 9.0% of mass 174	(7.30) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(95.95) ¹
177	5.0 - 9.0% of mass 176	(6.42) ²

BFB Injection Date: 1/2/08
 BFB Injection Time: 0834
 BFB File ID: 610201
 Tekmar Purge Flow: 22.7 mL/min
 Vacuum: 4.78e-5
 IS/Std #: 1443-398 Exp. Date: 3/08/08
 BCM: 360824
 1,4-DFB: 1320902
 CB-d5: 1313800

Verified CCV IS vs ICAL mid-point (-40%^{AD}) NR

Verify 176/174 m/z Ratio: $\frac{1192769/1243078 \times 100}{95.95} = 95.95$

NOAH Cart #: NR

File #: NR

File #: NR

Calculation Check:

ppbv of compound = $\frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} \times \text{RRF}$

$= \frac{(1393281)}{(1320902)} \times (25.0) \times (0.94836) = 27.806$

File ID: 612010206
 Compound: 701-DB
 Initials: SPAL

Reported Result 27.806

Use	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	610201	BFB Time Check 1/17-64	50mg	200mL	100	1/2/08	0834	SPAL		
✓	02	TRH Level 3	1443-399	200mL	2.0mL		1039	SPAL		61401213c
✓	03			5.0mL			1118	SPAL		MEDH1213b
✓	04			5.0mL			1202	SPAL		SP22c
✓	05			200mL			1248	SPAL		
✓	06	CCV-1 (200ppb)	1576-197	50ppb	50mL		1410	SPAL		2out
✓	07	CS-1	1576-168				1525	SPAL		2out
✓	08	Lab blank	1209	Hermit	200mL		1623	NR		
✓	09	Lab Blank					1744	NR		

SPAL
 Signature

1/2/08
 Date

@ Air Toxics Ltd.

MSD-T

Logbook #: 1599

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	20.21
75	30.0 - 60.0% of mass 95	53.23
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.44
173	Less than 2.0% of mass 174	(0.84) ¹
174	Greater than 50.0% of mass 95	73.02
175	5.0 - 9.0% of mass 174	(7.38) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(96.81) ¹
177	5.0 - 9.0% of mass 176	(10.52) ²

BFB Injection Date: 11/16/08
 BFB Injection Time: 0829
 BFB File ID: T011601
 Tekmar Purge Flow: N/A
 Vacuum: N/A
 IS/S Std #: 1443-398 Exp. Date: 3/24/02
 BCM 349330
 1,4-DFB 1314503
 CB-d5 1287161
 Verified CCV IS vs ICAL mid-point (-40%^d) for
initials

NOAH Cart #: NA File #: NA

Calculation Check:

pbv of compound = $\frac{\text{Area}_{\text{Sample}}}{\text{Area}_{\text{std}}} \times \frac{\text{Conc}_{\text{std}}}{\text{RRF}} = \frac{(1315462)}{(1314503)} \times \frac{(25.00)}{(0.94830)} = 26.38053$

Reported Result 26.380

Verify 176/174 m/z Ratio: $\frac{96.81}{73.02} = 1.326$

File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
T011601	BESTUNE Blank	14174	50ppm	2ul	1.00	11/16/08	0829	fo/cb	
02	CGU-1 #1576-197	200ppm	50ppm	50ml			0850	fo/cb	
03	LDS-1 #1576-169	200ppm	50ppm	50ml			0934	fo/cb	
04	TVAHWA level 4	200ppm	25ppm	25ml			1018	fo/cb	#1443-403 SP4 TVAH
05		200ppm	100ppm	100ml			1057	fo/cb	
06		200ppm	200ppm	200ml			1140	fo/cb	
07	System Blank	12009	Humid	200ml			1218	fo/cb	
08	SPICAL level 23	200ppm	200ppm	200ml			1305	fo/cb	SP 5d #1443-403
09	SPICAL level 5	200ppm	50ppm	50ml			1344	fo/cb	

Signature Chunmyr

Date 11/16/08

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	19.63
75	30.0 - 60.0% of mass 95	52.14
95	Base peak, 100.00% relative abundance	100
96	5.0 - 9.0% of mass 95	6.40
173	Less than 2.0% of mass 174	(0.82) ¹
174	Greater than 50.0% of mass 95	76.53
175	5.0 - 9.0% of mass 174	(7.20) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(96.22) ¹
177	5.0 - 9.0% of mass 176	(6.67) ²

BFB Injection Date: 12/5/08
 BFB Injection Time: 0813
 BFB File ID: 4012501
 Tekmar Purge Flow: _____
 Vacuum: 4.24e-5
 IS/Std #: 1445-398 Exp. Date: 3/29/08
 BCM: 313448
 1,4-DFB: 1165419
 CB-d5: 1132615
 Verified CCV IS vs ICAL mid-point (-40%^d) initials

Verify 176/174 m/z Ratio: 1081888/1124352 x 100 = 96.22% NOAH Cart #: 218 File #: 218

Calculation Check:
 ppbv of compound = $\frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \frac{\text{Conc}_{\text{std}}}{\text{RRF}}$
 = $\frac{(1163164)}{(1165419)} \times \frac{(25.0)}{(0.99836)} = 26.310$
 Reported Result: 26.310
 File ID: _____
 Compound: TOL-D8
 Initials: gpc

Use	File #	Sample/Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	T012501	PERE TOL Check	1176-65	50psi	3uL	100	12/5/08	0813	gpc	
✓	02	CVV-1 (100ppbv)	1526-1978	50psi	100uL		0900	gpc	gpc	0.01T
✓	03	115-1	1526-1679				0951	gpc	gpc	0.01T
✓	04	ICHL Level 3	1526-236	2.0ppbv	2.0mL		1127	gpc	gpc	t14g1213e
✓	05		5	50ppbv	50mL		1214	gpc	gpc	sp18e
✓	06		7	20ppbv	200mL		1309	gpc	gpc	
✓	07	Lab blank	33668	Humid	200mL		1529	gpc	gpc	short list
✓	08	0801392A-01A	11 bag	Humid	50mL	400	1616	gpc	gpc	100x
✓	09	0801393A-01A	11 bag	Humid	50mL	400	1822	gpc	gpc	

Signature: [Signature] Date: 12/5/08
 Revision 08/2007 Page 267

Air Toxics Ltd.
 Modified EPA Methods TO-14A/TO-15
 Internal Standard and Associated Target Compounds and Surrogates

Bromochloromethane
Target Compounds:
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
3-Chloropropene
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
2,2,4-Trimethylpentane
Surrogates:
1,2-Dichloroethane-d4

1,4-Difluorobenzene
Target Compounds:
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
Surrogates:
Toluene-d8

Chlorobenzene-d5
Target Compounds:
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
Surrogates:
Bromofluorobenzene

Report Date: 14-Dec-2007 11:45

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121320.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 14-DEC-2007 11:17
 Operator : sjr Inst ID: msdt.i
 Smp Info : 50mL #1576-168
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 10:44 ealcan Quant Type: ISTD
 Cal Date : 14-DEC-2007 03:20 Cal File: t121316.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE (PPBV)	(PPBV)					
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858 (1.000)	130	297931	25.0000		50.00-	150.00	100.00	
13.858	13.858 (1.000)	128	235151			26.73-	126.73	78.93	
13.858	13.858 (1.000)	49	457359			83.94-	183.94	153.51	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628 (1.000)	114	1225805	25.0000		50.00-	150.00	100.00	
15.600	15.628 (1.000)	88	200996			0.00-	65.84	16.40	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798 (1.000)	117	1087987	25.0000		50.00-	150.00	100.00	
20.798	20.798 (1.000)	82	618909			5.33-	105.33	56.89	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936 (1.078)	65	479945	25.3015	25.302	50.00-	150.00	100.00	
14.936	14.936 (1.078)	67	266508			3.93-	103.93	55.53	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199 (1.165)	98	1159315	24.9314	24.931	50.00-	150.00	100.00	
18.199	18.199 (1.165)	70	130009			0.00-	61.06	11.21	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE (PPEV) (PPBV) TARGET RANGE RATIO
 == == ===== == ===== ===== =====

\$ 113 Toluene-d8 (continued)

18.199 18.199 (1.165) 100 805306 18.52- 118.52 69.46

\$ 137 Bromofluorobenzene

CAS #: 460-00-4

22.789 22.789 (1.096) 174 761756 25.5279 25.528 50.00- 150.00 100.00

22.789 22.789 (1.096) 95 960617 74.37- 174.37 126.11

22.789 22.789 (1.096) 176 748218 47.63- 147.63 98.22

11 Propylene

CAS #: 115-07-1

5.812 5.812 (0.419) 41 407486 51.2114 51.211 50.00- 150.00 100.00

5.812 5.812 (0.419) 42 278355 17.44- 117.44 68.31

5.812 5.812 (0.419) 39 330847 31.05- 131.05 81.19

12 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

5.923 5.923 (0.427) 85 2690700 51.5642 51.564 50.00- 150.00 100.00

5.923 5.923 (0.427) 87 871018 0.00- 82.50 32.37

16 Freon 114

CAS #: 76-14-2

6.282 6.282 (0.453) 135 1918203 56.2307 56.231 50.00- 150.00 100.00

6.282 6.282 (0.453) 137 605566 0.00- 81.78 31.57

18 Chloromethane

CAS #: 74-87-3

6.531 6.559 (0.471) 50 528383 46.8136 46.814 50.00- 150.00 100.00

6.531 6.559 (0.471) 52 175192 0.00- 83.59 33.16

20 Vinyl Chloride

CAS #: 75-01-4

6.863 6.890 (0.495) 62 764253 54.1358 54.136 50.00- 150.00 100.00

6.890 6.890 (0.497) 64 246222 0.00- 94.54 32.22

22 1,3-Butadiene

CAS #: 106-99-0

6.973 6.946 (0.503) 54 603285 54.7429 54.743 50.00- 150.00 100.00

6.946 6.946 (0.501) 39 556460 61.08- 161.08 92.24

25 Bromomethane

CAS #: 74-83-9

7.913 7.913 (0.571) 94 800969 53.5745 53.574 50.00- 150.00 100.00

7.913 7.913 (0.571) 96 732818 44.93- 144.93 91.49

27 Chloroethane

CAS #: 75-00-3

8.162 8.190 (0.589) 64 433707 57.5752 57.575 50.00- 150.00 100.00

8.162 8.190 (0.589) 49 106353 0.00- 76.61 24.52

8.162 8.190 (0.589) 66 140432 0.00- 85.87 32.38

31 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

8.770 8.771 (0.633) 101 3269104 56.0441 56.044 50.00- 150.00 100.00

8.770 8.771 (0.633) 103 2117698 15.72- 115.72 64.78

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
38 Ethanol						CAS #:	64-17-5			
9.241	9.241	(0.667)	45	239080	60.4335	60.434	50.00-	150.00	100.00	
9.241	9.241	(0.667)	43	60855			0.00-	74.87	25.45	
9.241	9.241	(0.667)	46	90830			0.00-	88.05	37.99	

42 Freon 113						CAS #:	76-13-1			
9.959	9.959	(0.719)	151	1615940	61.5542	61.554	50.00-	150.00	100.00	
9.959	9.959	(0.719)	153	1032178			15.26-	115.26	63.87	
9.932	9.959	(0.717)	101	2112556			81.18-	181.18	130.73	

43 1,1-Dichloroethene						CAS #:	75-35-4			
10.042	10.042	(0.725)	61	1438019	62.4946	62.494	50.00-	150.00	100.00	
10.042	10.042	(0.725)	96	910052			16.16-	116.16	63.29	
10.042	10.042	(0.725)	98	584422			0.00-	91.50	40.64	

45 Acetone						CAS #:	67-64-1			
10.181	10.181	(0.735)	58	378148	52.9297	52.930	50.00-	150.00	100.00	
10.181	10.181	(0.735)	43	1188293			264.94-	364.94	314.24	

46 2-Propanol						CAS #:	67-63-0			
10.374	10.374	(0.749)	45	1354669	57.2391	57.239	50.00-	150.00	100.00	
10.374	10.374	(0.749)	43	331688			0.00-	78.96	24.48	
10.374	10.374	(0.749)	59	58484			0.00-	54.05	4.32	

47 Carbon Disulfide						CAS #:	75-15-0			
10.540	10.540	(0.761)	76	2469156	56.2815	56.282	50.00-	150.00	100.00	

51 3-Chloropropene						CAS #:	107-05-1			
10.817	10.817	(0.781)	76	417374	55.7417	55.742	50.00-	150.00	100.00	
10.817	10.817	(0.781)	41	855586			176.05-	276.05	204.99	

54 Methylene Chloride						CAS #:	75-09-2			
11.093	11.093	(0.800)	49	796452	54.8123	54.812	50.00-	150.00	100.00	
11.093	11.093	(0.800)	84	777691			44.80-	144.80	97.64	
11.093	11.093	(0.800)	51	249342			0.00-	83.78	31.31	

60 MTBE						CAS #:	1634-04-4			
11.452	11.453	(0.826)	73	2948507	60.5394	60.539	50.00-	150.00	100.00	
11.452	11.453	(0.826)	57	536190			0.00-	69.37	18.19	
11.452	11.453	(0.826)	41	498181			0.00-	70.94	16.90	

61 trans-1,2-Dichloroethene						CAS #:	156-60-5			
11.535	11.535	(0.832)	96	998183	56.6170	56.617	50.00-	150.00	100.00	
11.535	11.535	(0.832)	61	1324537			84.61-	184.61	132.69	
11.535	11.535	(0.832)	98	640437			15.85-	115.85	64.16	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
65 Hexane					CAS #: 110-54-3				
11.895	11.895	(0.858)	57	1447152	59.1198	59.120	50.00-	150.00	100.00
11.895	11.895	(0.858)	43	807876			8.15-	108.15	55.83
11.895	11.895	(0.858)	86	273943			0.00-	69.59	18.93

69 Vinyl Acetate					CAS #: 108-05-4				
12.365	12.337	(0.892)	86	266315	60.9681	60.968	50.00-	150.00	100.00
12.337	12.337	(0.890)	43	2203777			903.58-	1003.58	827.51

70 1,1-Dichloroethane					CAS #: 75-34-3				
12.365	12.365	(0.892)	63	1840962	59.8689	59.869	50.00-	150.00	100.00
12.365	12.365	(0.892)	65	595247			0.00-	83.37	32.33

75 2-Butanone					CAS #: 78-93-3				
13.388	13.388	(0.966)	72	512054	62.9098	62.910	50.00-	150.00	100.00
13.388	13.388	(0.966)	43	1555813			271.22-	371.22	303.84
13.388	13.388	(0.966)	57	140713			0.00-	78.78	27.48

76 cis-1,2-Dichloroethene					CAS #: 156-59-2				
13.416	13.416	(0.968)	61	1201965	55.6569	55.657	50.00-	150.00	100.00
13.416	13.416	(0.968)	96	1004620			29.23-	129.23	83.58
13.416	13.416	(0.968)	98	645816			0.16-	100.16	53.73

80 Tetrahydrofuran					CAS #: 109-99-9				
13.858	13.858	(1.000)	42	766179	59.0695	59.069	50.00-	150.00	100.00
13.858	13.858	(1.000)	71	430316			0.61-	100.61	56.16
13.858	13.858	(1.000)	72	458315			8.31-	108.31	59.82

82 Chloroform					CAS #: 67-66-3				
13.941	13.941	(1.006)	83	2244713	62.3864	62.386	50.00-	150.00	100.00
13.941	13.941	(1.006)	85	1463131			18.46-	118.46	65.18

83 1,1,1-Trichloroethane					CAS #: 71-55-6				
14.273	14.273	(1.030)	97	2515274	58.3743	58.374	50.00-	150.00	100.00
14.273	14.273	(1.030)	99	1614810			13.89-	113.89	64.20

85 Cyclohexane					CAS #: 110-82-7				
14.300	14.300	(1.032)	84	1353375	61.5448	61.545	50.00-	150.00	100.00
14.300	14.300	(1.032)	56	1256976			43.75-	143.75	92.88
14.300	14.300	(1.032)	41	628833			1.66-	101.66	46.46

87 Carbon Tetrachloride					CAS #: 56-23-5				
14.522	14.522	(1.048)	119	2395660	57.0825	57.082	50.00-	150.00	100.00
14.522	14.522	(1.048)	117	2520039			54.19-	154.19	105.19

89 2,2,4-Trimethylpentane					CAS #: 540-84-1				
14.881	14.881	(1.074)	57	3545944	57.8247	57.825	50.00-	150.00	100.00

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
89 2,2,4-Trimethylpentane (continued)									
14.881	14.881	(1.074)	56	1141294			0.00- 83.27	32.19	
14.881	14.881	(1.074)	41	879371			0.00- 77.74	24.80	

91 Benzene CAS #: 71-43-2									
14.964	14.964	(0.958)	78	2894004	59.1301	59.130	50.00- 150.00	100.00	
14.964	14.964	(0.958)	77	656988			0.00- 73.32	22.70	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.075	15.075	(0.965)	62	1382649	56.5579	56.558	50.00- 150.00	100.00	
15.075	15.075	(0.965)	64	452098			0.00- 82.87	32.70	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	918490	59.0785	59.078	50.00- 150.00	100.00	
15.185	15.185	(0.972)	43	1149487			77.61- 177.61	125.15	
15.185	15.185	(0.972)	57	722874			32.99- 132.99	78.70	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	1302106	57.5778	57.578	50.00- 150.00	100.00	
16.070	16.070	(1.028)	130	1210308			45.55- 145.55	92.95	
16.070	16.070	(1.028)	97	834926			15.22- 115.22	64.12	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.568	16.568	(1.060)	63	945570	57.8152	57.815	50.00- 150.00	100.00	
16.568	16.568	(1.060)	62	681613			23.00- 123.00	72.08	
16.568	16.568	(1.060)	41	498335			8.64- 108.64	52.70	

106 1,4-Dioxane CAS #: 123-91-1									
16.678	16.678	(1.067)	88	706088	54.4400	54.440	50.00- 150.00	100.00	
16.678	16.678	(1.067)	58	380445			5.85- 105.85	53.88	
16.678	16.678	(1.067)	57	134496			0.00- 69.86	19.05	

107 Bromodichloromethane CAS #: 75-27-4									
16.982	16.982	(1.087)	83	2298371	58.4285	58.428	50.00- 150.00	100.00	
16.982	16.982	(1.087)	85	1481812			16.51- 116.51	64.47	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	1559791	59.2171	59.217	50.00- 150.00	100.00	
17.784	17.784	(1.138)	77	499741			0.00- 83.76	32.04	
17.784	17.784	(1.138)	39	633346			0.00- 94.73	40.60	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.950	17.950	(1.149)	58	748743	62.4757	62.476	50.00- 150.00	100.00	
17.950	17.950	(1.149)	43	1625109			168.02- 268.02	217.04	
17.978	17.950	(1.150)	85	406600			2.69- 102.69	54.30	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	ON-COL		FINAL	TARGET RANGE	RATIO	
				RESPONSE	(PPEV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	3488711	59.0924	59.092	50.00- 150.00	100.00	
18.337	18.337	(1.173)	92	2137294			9.70- 109.70	61.26	

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	1723281	58.5278	58.528	50.00- 150.00	100.00	
18.752	18.752	(0.902)	77	549331			0.00- 82.23	31.88	
18.752	18.752	(0.902)	39	643249			0.00- 88.37	37.33	

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.111	(0.919)	97	1249369	58.4987	58.499	50.00- 150.00	100.00	
19.111	19.111	(0.919)	99	780443			15.96- 115.96	62.47	
19.111	19.111	(0.919)	83	1032830			36.03- 136.03	82.67	

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	1718550	57.7366	57.736	50.00- 150.00	100.00	
19.277	19.277	(0.927)	129	1188790			20.82- 120.82	69.17	
19.277	19.277	(0.927)	131	1136428			18.42- 118.42	66.13	

121 2-Hexanone						CAS #: 591-78-6			
19.416	19.416	(0.934)	58	1015166	58.0616	58.062	50.00- 150.00	100.00	
19.416	19.416	(0.934)	43	1585312			120.66- 220.66	156.16	
19.416	19.416	(0.934)	100	231322			0.00- 74.50	22.79	

122 Dibromochloromethane						CAS #: 124-48-1			
19.803	19.803	(0.952)	129	2201707	58.6480	58.648	50.00- 150.00	100.00	
19.803	19.803	(0.952)	127	1695177			25.33- 125.33	76.99	

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.051	20.052	(0.964)	107	2032005	56.5540	56.554	50.00- 150.00	100.00	
20.051	20.052	(0.964)	109	1861574			41.12- 141.12	91.61	

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.853	(1.003)	112	2917621	56.2474	56.247	50.00- 150.00	100.00	
20.853	20.853	(1.003)	114	903390			0.00- 80.99	30.96	
20.853	20.853	(1.003)	77	1746502			25.73- 125.73	59.86	

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	1522313	57.9476	57.948	50.00- 150.00	100.00	
20.936	20.936	(1.007)	91	4802757			266.56- 366.56	315.49	

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	1930516	59.7422	59.742	50.00- 150.00	100.00	
21.130	21.130	(1.016)	91	3845669			157.11- 257.11	199.20	

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	1848646	60.9039	60.904	50.00- 150.00	100.00	

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	3849311				166.77- 266.77	208.22

131 Styrene CAS #: 100-42-5									
21.876	21.876	(1.052)	104	3016308	61.3208	61.321		50.00- 150.00	100.00
21.876	21.876	(1.052)	78	1506910				12.82- 112.82	49.96

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	2332121	59.5912	59.591		50.00- 150.00	100.00
22.291	22.291	(1.072)	171	1192867				0.34- 100.34	51.15

134 Cumene CAS #: 98-82-8									
22.429	22.429	(1.078)	105	5299298	61.0792	61.079		50.00- 150.00	100.00
22.429	22.429	(1.078)	120	1367193				0.00- 74.52	25.80
22.429	22.429	(1.078)	51	403151				51.79- 151.79	7.61

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	2780728	58.4525	58.452		50.00- 150.00	100.00
23.010	23.010	(1.106)	85	1796107				17.66- 117.66	64.59

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	6617883	60.3099	60.310		50.00- 150.00	100.00
23.121	23.121	(1.112)	120	1462761				0.00- 71.52	22.10
23.121	23.121	(1.112)	105	239586				0.00- 53.54	3.62

145 4-Ethyltoluene CAS #: 622-96-8									
23.286	23.286	(1.120)	105	5652075	61.1557	61.156		50.00- 150.00	100.00
23.286	23.286	(1.120)	120	1678224				0.00- 79.85	29.69

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	4580475	60.9001	60.900		50.00- 150.00	100.00
23.397	23.397	(1.125)	120	2226842				0.29- 100.29	48.62

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	4351654	62.1648	62.165		50.00- 150.00	100.00
24.033	24.033	(1.156)	120	2012408				0.00- 94.69	46.24

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	3071747	57.9806	57.980		50.00- 150.00	100.00
24.586	24.586	(1.182)	148	1961928				14.61- 114.61	63.87
24.586	24.586	(1.182)	111	1275284				0.00- 92.01	41.52

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	3136467	56.9774	56.977		50.00- 150.00	100.00
24.724	24.724	(1.189)	148	1982548				13.83- 113.83	63.21
24.724	24.724	(1.189)	111	1254870				0.00- 89.75	40.01

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	ON-COL		FINAL	TARGET RANGE	RATIO	
				RESPONSE	(PPEV)	(PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

159 alpha-Chlorotoluene					CAS #: 100-44-7				
24.945	24.945	(1.199)	91	4855343	63.7416	63.742	50.00- 150.00	100.00	
24.945	24.945	(1.199)	126	929617			0.00- 69.65	19.15	

161 1,2-Dichlorobenzene					CAS #: 95-50-1				
25.360	25.360	(1.219)	146	2974913	58.5585	58.558	50.00- 150.00	100.00	
25.360	25.360	(1.219)	148	1879900			14.36- 114.36	63.19	
25.360	25.360	(1.219)	111	1279017			0.00- 92.81	42.99	

165 1,2,4-Trichlorobenzene					CAS #: 120-82-1				
28.153	28.153	(1.354)	180	2325679	66.7403	66.740	50.00- 150.00	100.00(R)	
28.153	28.153	(1.354)	182	2211551			45.41- 145.41	95.09	

166 Hexachlorobutadiene					CAS #: 87-68-3				
28.319	28.319	(1.362)	225	2017457	63.4304	63.430	50.00- 150.00	100.00	
28.319	28.319	(1.362)	223	1250920			13.46- 113.46	62.00	

29 Isopentane					CAS #: 78-78-4				
8.273	8.273	(0.597)	43	849178	52.1561	52.156	50.00- 150.00	100.00	
8.273	8.273	(0.597)	57	670085			26.79- 126.79	78.91	

19 Butane					CAS #: 106-97-8				
6.780	6.780	(0.489)	58	156054	53.9715	53.972	50.00- 150.00	100.00	
6.807	6.780	(0.491)	43	1081106			640.46- 740.46	692.78	

102 Methyl Cyclohexane					CAS #: 108-87-2				
16.346	16.346	(1.180)	83	1666583	59.7664	59.766	50.00- 150.00	100.00	
16.346	16.346	(1.180)	98	774998			0.00- 95.49	46.50	
16.346	16.346	(1.180)	55	1083399			16.76- 116.76	65.01	

167 Naphthalene					CAS #: 91-20-3				
28.678	28.678	(1.379)	128	3569617	62.1466	62.146	50.00- 150.00	100.00	
28.678	28.678	(1.379)	127	436768			0.00- 62.56	12.24	

QC Flag Legend

R - Spike/Surrogate failed recovery limits.

Report Date: 14-Dec-2007 11:45

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121320.d

Calibration Time: 01:23

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	297931	6.12
97 1,4-Difluorobenze	1182601	709561	1655641	1225805	3.65
126 Chlorobenzene-d5	1033655	620193	1447117	1087987	5.26

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.


RECOVERY REPORT

Client Name: Client SDG: 13Dec2007
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: sjr
 Data Type: MS DATA SampleType: LCS
 SpikeList File: 2926Spectra.spk Quant Type: ISTD
 Sublist File: AT04ENSR.sub
 Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Misc Info: 200ppbv -> 50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
12 Dichlorodifluorome	50.000	51.564	103.13	70-130
16 Freon 114	50.000	56.231	112.46	70-130
18 Chloromethane	50.000	46.814	93.63	70-130
20 Vinyl Chloride	50.000	54.136	108.27	70-130
22 1,3-Butadiene	50.000	54.743	109.49	60-140
25 Bromomethane	50.000	53.574	107.15	70-130
27 Chloroethane	50.000	57.575	115.15	70-130
31 Trichlorofluoromet	50.000	56.044	112.09	70-130
38 Ethanol	50.000	60.434	120.87	60-140
42 Freon 113	50.000	61.554	123.11	70-130
43 1,1-Dichloroethene	50.000	62.494	124.99	70-130
45 Acetone	50.000	52.930	105.86	60-140
47 Carbon Disulfide	50.000	56.282	112.56	60-140
46 2-Propanol	50.000	57.239	114.48	60-140
54 Methylene Chloride	50.000	54.812	109.62	70-130
60 MTBE	50.000	60.539	121.08	60-140
61 trans-1,2-Dichloro	50.000	56.617	113.23	60-140
65 Hexane	50.000	59.120	118.24	60-140
69 Vinyl Acetate	50.000	60.968	121.94	60-140
70 1,1-Dichloroethane	50.000	59.869	119.74	70-130
76 cis-1,2-Dichloroet	50.000	55.657	111.31	70-130
75 2-Butanone	50.000	62.910	125.82	60-140
80 Tetrahydrofuran	50.000	59.069	118.14	60-140
82 Chloroform	50.000	62.386	124.77	70-130
85 Cyclohexane	50.000	61.545	123.09	60-140
83 1,1,1-Trichloroeth	50.000	58.374	116.75	70-130
87 Carbon Tetrachlori	50.000	57.082	114.16	70-130
91 Benzene	50.000	59.130	118.26	70-130
93 1,2-Dichloroethane	50.000	56.558	113.12	70-130
94 Heptane	50.000	59.078	118.16	60-140
101 Trichloroethene	50.000	57.578	115.16	70-130
104 1,2-Dichloropropan	50.000	57.815	115.63	70-130
106 1,4-Dioxane	50.000	54.440	108.88	60-140

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
107 Bromodichlorometha	50.000	58.428	116.86	60-140
110 cis-1,3-Dichloropr	50.000	59.217	118.43	70-130
111 4-Methyl-2-pentano	50.000	62.476	124.95	60-140
114 Toluene	50.000	59.092	118.18	70-130
116 trans-1,3-Dichloro	50.000	58.528	117.06	70-130
117 1,1,2-Trichloroeth	50.000	58.499	117.00	70-130
120 Tetrachloroethene	50.000	57.736	115.47	70-130
121 2-Hexanone	50.000	58.062	116.12	60-140
122 Dibromochlorometha	50.000	58.648	117.30	60-140
123 1,2-Dibromoethane	50.000	56.554	113.11	70-130
127 Chlorobenzene	50.000	56.247	112.49	70-130
128 Ethyl Benzene	50.000	57.948	115.90	70-130
129 m,p-Xylene	50.000	59.742	119.48	70-130
130 o-Xylene	50.000	60.904	121.81	70-130
131 Styrene	50.000	61.321	122.64	70-130
133 Bromoform	50.000	59.591	119.18	60-140
140 1,1,2,2-Tetrachlor	50.000	58.452	116.91	70-130
145 4-Ethyltoluene	50.000	61.156	122.31	60-140
147 1,3,5-Trimethylben	50.000	60.900	121.80	70-130
150 1,2,4-Trimethylben	50.000	62.165	124.33	70-130
155 1,3-Dichlorobenzen	50.000	57.980	115.96	70-130
156 1,4-Dichlorobenzen	50.000	56.977	113.95	70-130
159 alpha-Chlorotoluen	50.000	63.742	127.48	70-130
161 1,2-Dichlorobenzen	50.000	58.558	117.12	70-130
165 1,2,4-Trichloroben	50.000	66.740	133.48*	70-130
166 Hexachlorobutadien	50.000	63.430	126.86	70-130
142 Propylbenzene	50.000	60.310	120.62	60-140
134 Cumene	50.000	61.079	122.16	60-140
51 3-Chloropropene	50.000	55.742	111.48	60-140
89 2,2,4-Trimethylpen	50.000	57.825	115.65	60-140
19 Butane	50.000	53.972	107.94	70-130
29 Isopentane	50.000	52.156	104.31	70-130
102 Methyl Cyclohexane	50.000	59.766	119.53	70-130
11 Propylene	50.000	51.211	102.42	60-140
167 Naphthalene	50.000	62.146	124.29	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 90 1,2-Dichloroethane	25.000	25.302	101.21	70-130
\$ 113 Toluene-d8	25.000	24.931	99.73	70-130
\$ 137 Bromofluorobenzene	25.000	25.528	102.11	70-130

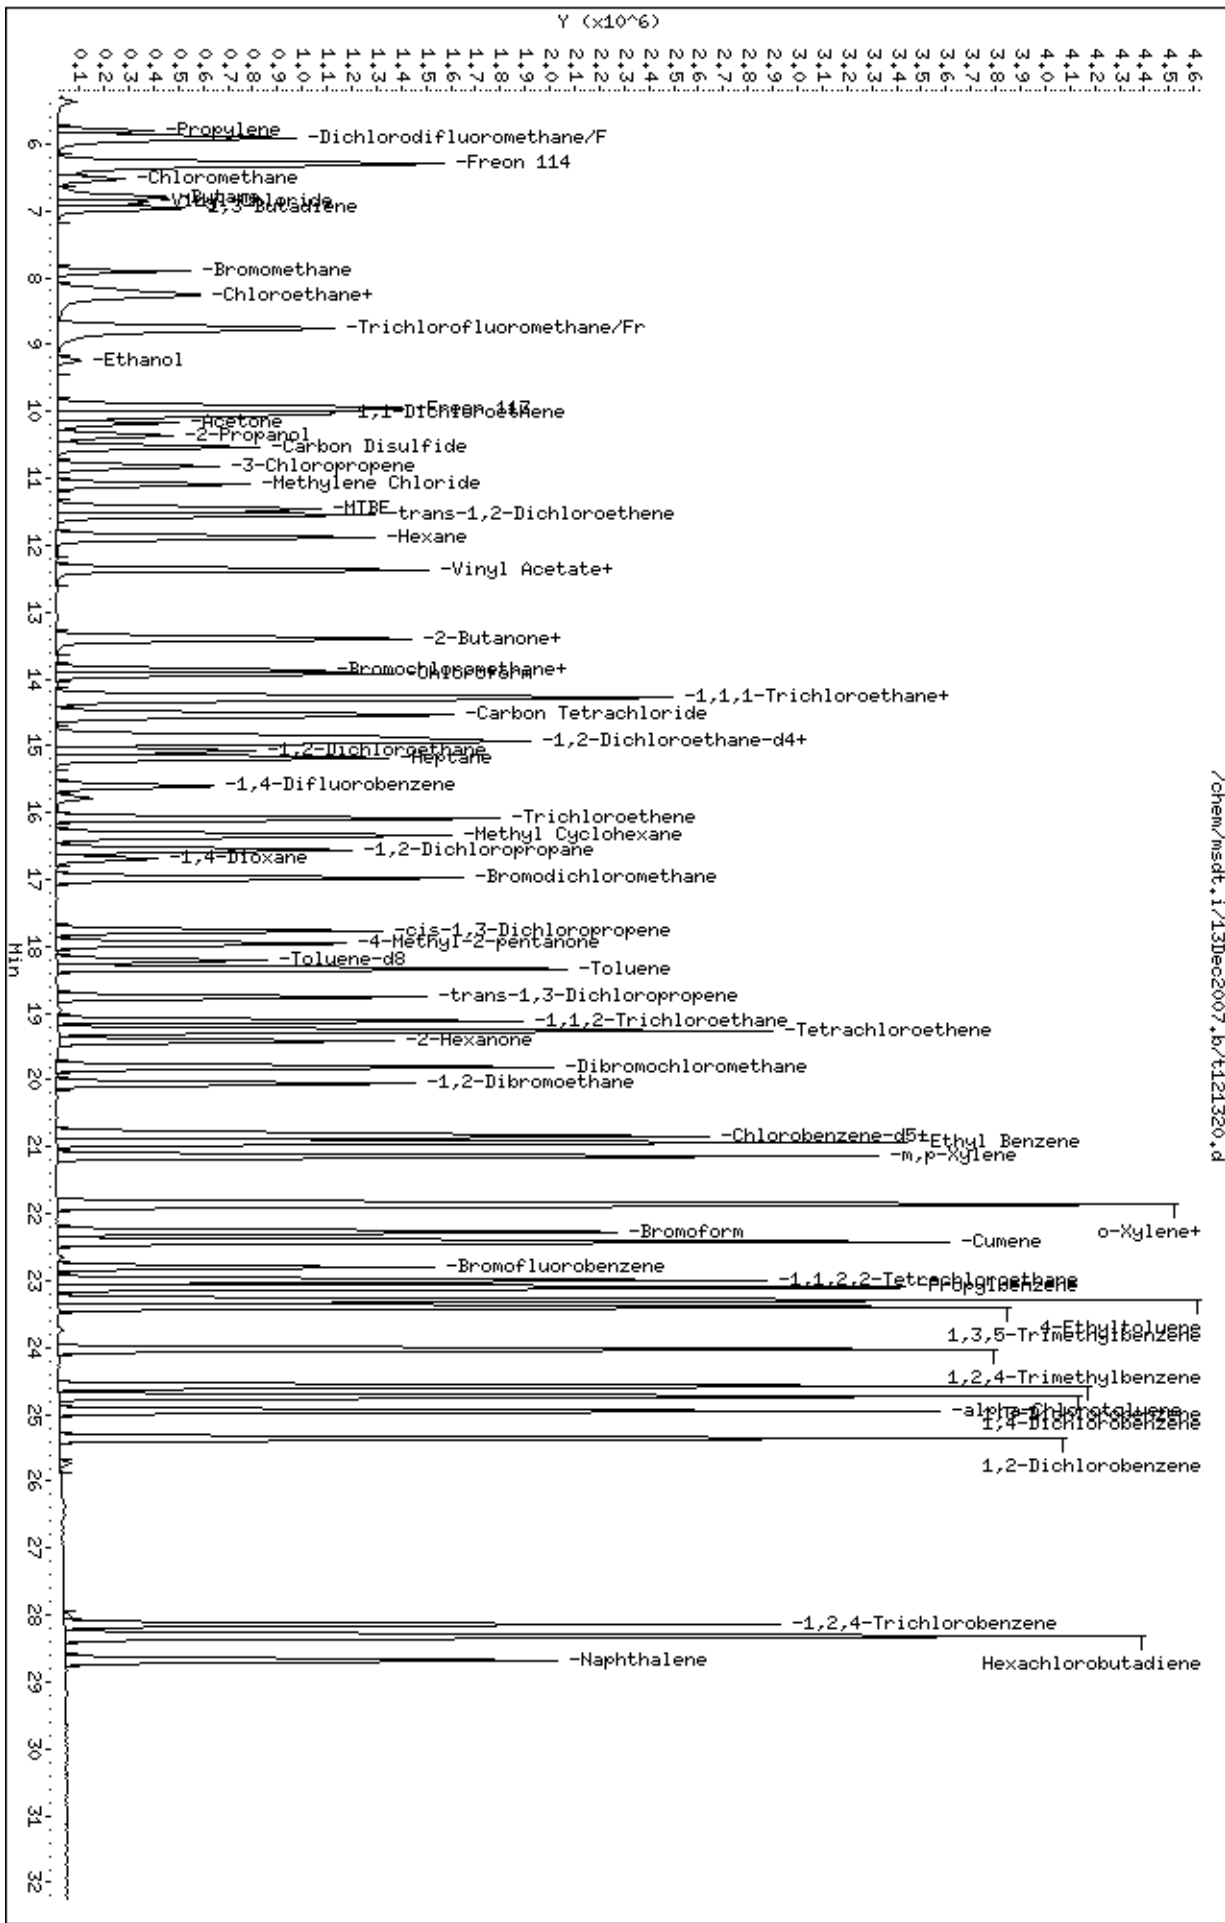

Report Date: 14-Dec-2007 10:40

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121310.d
 Lab Smp Id: ICAL Client Smp ID: Level 1
 Inj Date : 13-DEC-2007 21:35
 Operator : srs Inst ID: msdt.i
 Smp Info : 0.2mL #1443-378
 Misc Info : 200ppbv -> 0.2ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 10:40 ealcan Quant Type: ISTD
 Cal Date : 13-DEC-2007 21:35 Cal File: t121310.d
 Als bottle: 1 Calibration Sample, Level: 1
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AFCEElow.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	254701	25.0000			50.00- 150.00	100.00
13.858	13.858	(1.000)	128	196886				26.73- 126.73	77.30
13.858	13.858	(1.000)	49	266898				83.94- 183.94	104.79

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1022222	25.0000			50.00- 150.00	100.00
15.628	15.628	(1.000)	88	159600				0.00- 65.84	15.61

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	910794	25.0000			50.00- 150.00	100.00
20.798	20.798	(1.000)	82	506164				5.33- 105.33	55.57

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.078)	65	401025	25.0000	24.729		50.00- 150.00	100.00
14.936	14.936	(1.078)	67	202074				3.93- 103.93	50.39

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	951323	25.0000	24.533		50.00- 150.00	100.00
18.199	18.199	(1.165)	70	104571				0.00- 61.06	10.99

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	647039			18.52- 118.52	68.01	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	619737	25.0000	24.809	50.00- 150.00	100.00	
22.789	22.789	(1.096)	95	779613			74.37- 174.37	125.80	
22.789	22.789	(1.096)	176	609005			47.63- 147.63	98.27	

82 Chloroform									
						CAS #: 67-66-3			
13.941	13.941	(1.006)	83	3933	0.20000	0.1279	50.00- 150.00	100.00(a)	
13.941	13.941	(1.006)	85	2994			18.46- 118.46	76.13	

91 Benzene									
						CAS #: 71-43-2			
14.964	14.964	(0.958)	78	6473	0.20000	0.1586	50.00- 150.00	100.00(a)	
14.964	14.964	(0.958)	77	1476			0.00- 73.32	22.80	

131 Styrene									
						CAS #: 100-42-5			
21.876	21.876	(1.052)	104	2393	0.20000	0.05811	50.00- 150.00	100.00(a)	
21.849	21.849	(1.051)	78	2697			12.82- 112.82	112.70	

134 Cumene									
						CAS #: 98-82-8			
22.429	22.429	(1.078)	105	6626	0.20000	0.09123	50.00- 150.00	100.00(a)	
22.429	22.429	(1.078)	120	1421			0.00- 74.52	21.45	
22.789	22.789	(1.096)	51	37750			51.79- 151.79	569.73	

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 14-Dec-2007 10:40

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121310.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: srs

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 0.2ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	254701	-9.28
97 1,4-Difluorobenze	1182601	709561	1655641	1022222	-13.56
126 Chlorobenzene-d5	1033655	620193	1447117	910794	-11.89

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/13Dec2007,b/t121310.d

Date : 13-DEC-2007 21:35

Client ID: Level 1

Sample Info: 0.2mL #1443-378


Column phase: RTX-624

Instrument: msdt,i

Operator: srs

Column diameter: 0.53

/chem/msdt,i/13Dec2007,b/t121310.d

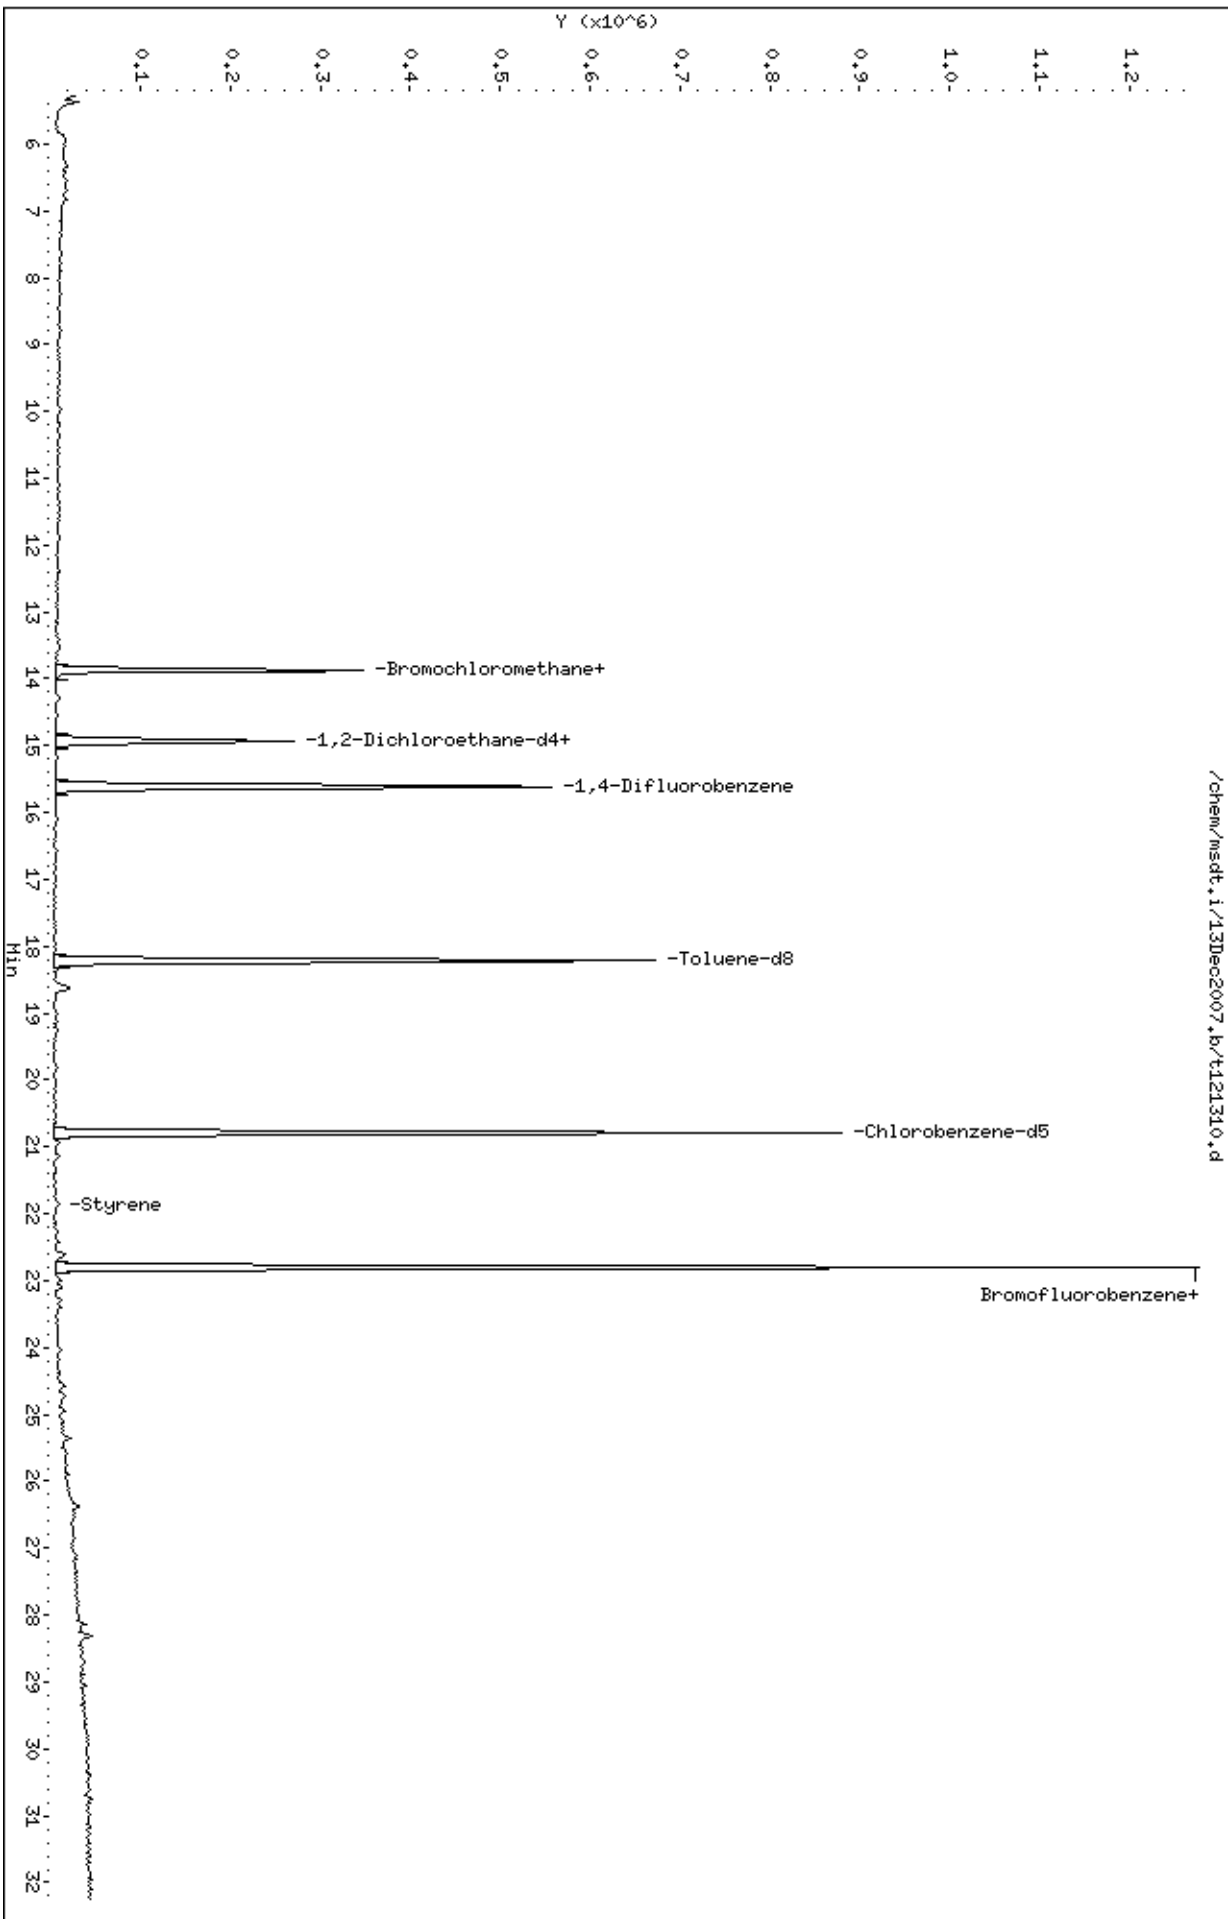

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/16Jan2008.b/t011608.d
 Lab Smp Id: TVH ICAL Client Smp ID: Level 3
 Inj Date : 16-JAN-2008 13:05
 Operator : lo Inst ID: msdt.i
 Smp Info : 2ml #1443-403
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/t14q1213d.m
 Meth Date : 16-Jan-2008 14:59 lover Quant Type: ISTD
 Cal Date : 16-JAN-2008 13:05 Cal File: t011608.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5d.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	325455	25.0000			50.00- 150.00	100.00
13.886	13.886	(1.000)	128	256909				27.05- 127.05	78.94
13.858	13.858	(1.000)	49	371229				61.34- 161.34	114.06

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1069240	25.0000			50.00- 150.00	100.00
15.628	15.628	(1.000)	88	169750				0.00- 65.73	15.88

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1107452	25.0000			50.00- 150.00	100.00
20.798	20.798	(1.000)	82	616797				5.94- 105.94	55.70

204 Propane CAS #: 74-98-6									
5.840	5.840	(0.421)	43	7801	2.00000	1.992		50.00- 150.00	100.00
5.812	5.812	(0.419)	44	25823				107.53- 207.53	331.02

37 Pentane CAS #: 109-66-0									
8.936	8.936	(0.644)	43	48819	2.00000	1.709		50.00- 150.00	100.00(a)
8.964	8.964	(0.646)	57	7450				0.00- 67.03	15.26

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
37 Pentane (continued)									
8.936	8.936	(0.644)	72	4638			0.00- 62.09	9.50	

112 Octane									
						CAS #: 111-65-9			
18.282	18.282	(1.170)	57	28842	2.00000	1.891	50.00- 150.00	100.00(a)	
18.282	18.282	(1.170)	85	33355			82.32- 182.32	115.65	
18.282	18.282	(1.170)	43	62064			166.39- 266.39	215.19	

124 Nonane									
						CAS #: 111-84-2			
20.964	20.964	(1.008)	43	55065	2.00000	1.548	50.00- 150.00	100.00(a)	
20.964	20.964	(1.008)	57	55025			52.38- 152.38	99.93	
20.964	20.964	(1.008)	85	23489			0.00- 95.58	42.66	

139 Decane									
						CAS #: 124-18-5			
23.204	23.204	(1.116)	57	57238	2.00000	1.339	50.00- 150.00	100.00(a)	
23.204	23.204	(1.116)	71	24835			0.00- 93.78	43.39	
23.231	23.231	(1.117)	142	2695			0.00- 54.94	4.71	

QC Flag Legend

a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 16-JAN-2008

Lab File ID: t011608.d

Calibration Time: 13:44

Lab Smp Id: TVH ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lo

Method File: /chem/msdt.i/16Jan2008.b/t14q1213d.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	325810	195486	456134	325455	-0.11
97 1,4-Difluorobenze	1168077	700846	1635308	1069240	-8.46
126 Chlorobenzene-d5	1103278	661967	1544589	1107452	0.38

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/16Jan2008,b/t011608.d

Date : 16-Jan-2008 13:05

Client ID: Level 3

Sample Info: 2ml #1443-403


Column phase: RTX-624

Instrument: msdt,i

Operator: lo

Column diameter: 0.53

/chem/msdt,i/16Jan2008,b/t011608.d

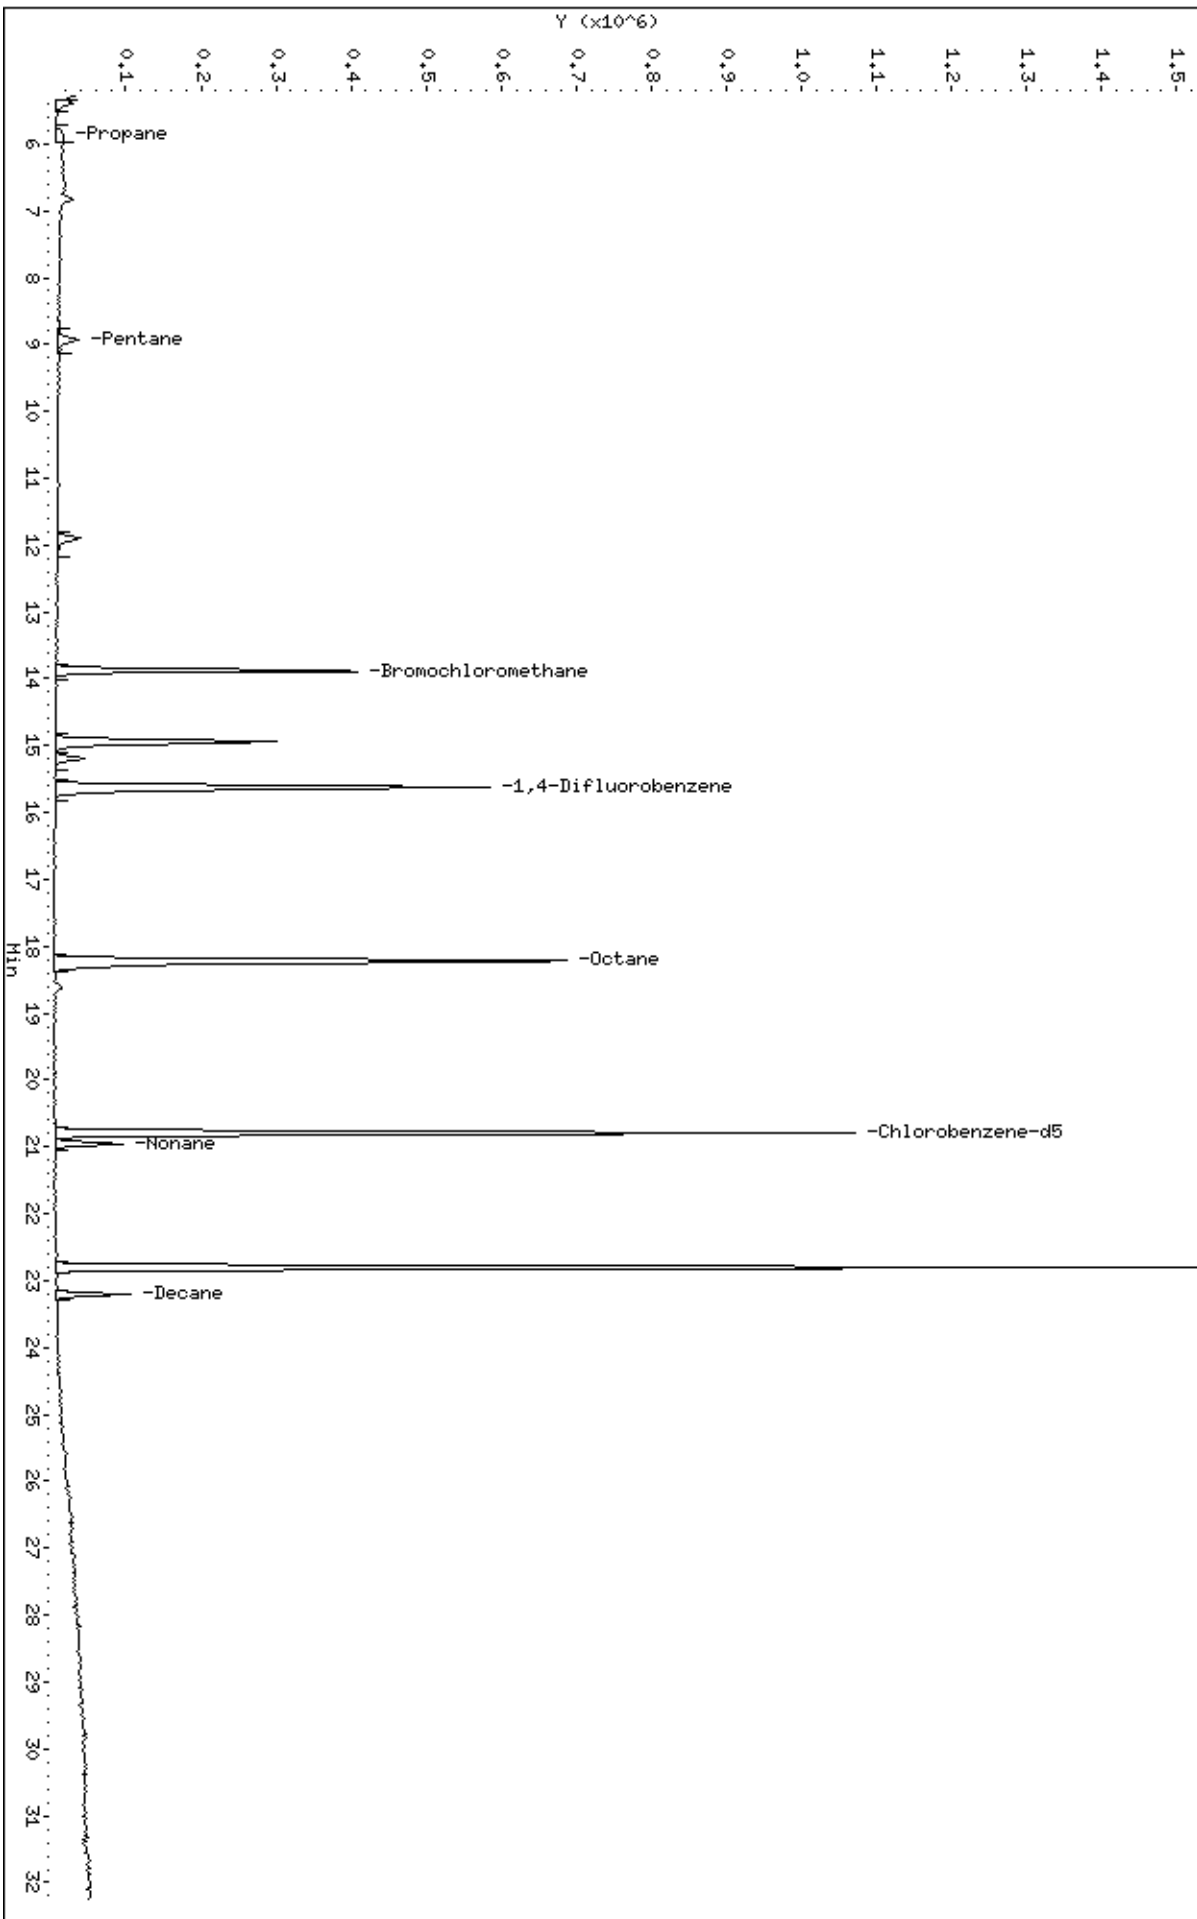

Report Date: 14-Dec-2007 10:40

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121319.d
 Lab Smp Id: ICAL Client Smp ID: Level 2
 Inj Date : 14-DEC-2007 09:58
 Operator : sjr Inst ID: msdt.i
 Smp Info : 0.5ml #1443-378
 Misc Info : 200ppbv -> 0.5ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 10:40 ealcan Quant Type: ISTD
 Cal Date : 14-DEC-2007 09:58 Cal File: t121319.d
 Als bottle: 1 Calibration Sample, Level: 2
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04low+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	299081	25.0000			50.00- 150.00	100.00
13.858	13.858	(1.000)	128	230570				26.73- 126.73	77.09
13.858	13.858	(1.000)	49	302565				83.94- 183.94	101.16

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1174268	25.0000			50.00- 150.00	100.00
15.600	15.600	(1.000)	88	185107				0.00- 65.84	15.76

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1056467	25.0000			50.00- 150.00	100.00
20.798	20.798	(1.000)	82	574906				5.33- 105.33	54.42

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.937	14.937	(1.078)	65	441620	25.0000	23.192		50.00- 150.00	100.00
14.937	14.937	(1.078)	67	225003				3.93- 103.93	50.95

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1097753	25.0000	24.644		50.00- 150.00	100.00
18.199	18.199	(1.165)	70	123408				0.00- 61.06	11.24

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

\$ 113 Toluene-d8 (continued)										
18.199	18.199	(1.165)	100	757368			18.52- 118.52	68.99		

\$ 137 Bromofluorobenzene										
						CAS #:	460-00-4			
22.789	22.789	(1.096)	174	723170	25.0000	24.958	50.00- 150.00	100.00		
22.789	22.789	(1.096)	95	913519			74.37- 174.37	126.32		
22.789	22.789	(1.096)	176	707774			47.63- 147.63	97.87		

12 Dichlorodifluoromethane/Fr12						CAS #:	75-71-8			
5.923	5.923	(0.427)	85	23775	0.50000	0.4539	50.00- 150.00	100.00(a)		
5.923	5.923	(0.427)	87	7400			0.00- 82.50	31.13		

16 Freon 114						CAS #:	76-14-2			
6.310	6.310	(0.455)	135	13894	0.50000	0.4057	50.00- 150.00	100.00(a)		
6.282	6.282	(0.453)	137	4541			0.00- 81.78	32.68		

20 Vinyl Chloride						CAS #:	75-01-4			
6.863	6.863	(0.495)	62	5280	0.50000	0.3726	50.00- 150.00	100.00(a)		
6.891	6.891	(0.497)	64	4819			0.00- 94.54	91.27		

22 1,3-Butadiene						CAS #:	106-99-0			
6.946	6.946	(0.501)	54	4298	0.50000	0.3885	50.00- 150.00	100.00(a)		
6.946	6.946	(0.501)	39	6927			61.08- 161.08	161.17		

25 Bromomethane						CAS #:	74-83-9			
7.914	7.914	(0.571)	94	6061	0.50000	0.4038	50.00- 150.00	100.00(a)		
7.914	7.914	(0.571)	96	6144			44.93- 144.93	101.37		

27 Chloroethane						CAS #:	75-00-3			
8.162	8.162	(0.589)	64	2991	0.50000	0.3955	50.00- 150.00	100.00(a)		
0.000	1.000	(0.000)	49	0			0.00- 76.61	0.00		
8.190	8.190	(0.591)	66	1285			0.00- 85.87	42.96		

31 Trichlorofluoromethane/Fr11						CAS #:	75-69-4			
8.771	8.771	(0.633)	101	23194	0.50000	0.3961	50.00- 150.00	100.00(a)		
8.771	8.771	(0.633)	103	15578			15.72- 115.72	67.16		

42 Freon 113						CAS #:	76-13-1			
9.904	9.904	(0.715)	151	11740	0.50000	0.4455	50.00- 150.00	100.00(a)		
9.960	9.960	(0.719)	153	8316			15.26- 115.26	70.83		
9.932	9.932	(0.717)	101	15617			81.18- 181.18	133.02		

43 1,1-Dichloroethene						CAS #:	75-35-4			
10.015	10.015	(0.723)	61	8027	0.50000	0.3475	50.00- 150.00	100.00(a)		
10.015	10.015	(0.723)	96	7012			16.16- 116.16	87.36		
10.043	10.043	(0.725)	98	4041			0.00- 91.50	50.34		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

47	Carbon Disulfide					CAS #:	75-15-0		
10.513	10.513	(0.759)	76	16820	0.50000	0.3819	50.00- 150.00	100.00(a)	

54	Methylene Chloride					CAS #:	75-09-2		
11.093	11.093	(0.800)	49	7565	0.50000	0.5186	50.00- 150.00	100.00	
11.093	11.093	(0.800)	84	8165			44.80- 144.80	107.93	
11.093	11.093	(0.800)	51	3108			0.00- 83.78	41.08	

60	MTBE					CAS #:	1634-04-4		
11.453	11.453	(0.826)	73	17154	0.50000	0.3508	50.00- 150.00	100.00(a)	
11.453	11.453	(0.826)	57	3460			0.00- 69.37	20.17	
11.453	11.453	(0.826)	41	4376			0.00- 70.94	25.51	

61	trans-1,2-Dichloroethene					CAS #:	156-60-5		
11.536	11.536	(0.832)	96	6989	0.50000	0.3949	50.00- 150.00	100.00(a)	
11.536	11.536	(0.832)	61	8323			84.61- 184.61	119.09	
11.536	11.536	(0.832)	98	4963			15.85- 115.85	71.01	

65	Hexane					CAS #:	110-54-3		
11.895	11.895	(0.858)	57	9443	0.50000	0.3843	50.00- 150.00	100.00(a)	
11.895	11.895	(0.858)	43	5403			8.15- 108.15	57.22	
11.895	11.895	(0.858)	86	2251			0.00- 69.59	23.84	

70	1,1-Dichloroethane					CAS #:	75-34-3		
12.365	12.365	(0.892)	63	11312	0.50000	0.3664	50.00- 150.00	100.00(a)	
12.365	12.365	(0.892)	65	3770			0.00- 83.37	33.33	

75	2-Butanone					CAS #:	78-93-3		
13.388	13.388	(0.966)	72	2727	0.50000	0.3337	50.00- 150.00	100.00(a)	
13.388	13.388	(0.966)	43	7626			271.22- 371.22	279.65	
0.000	1.000	(0.000)	57	0			0.00- 78.78	0.00	

76	cis-1,2-Dichloroethene					CAS #:	156-59-2		
13.416	13.416	(0.968)	61	8500	0.50000	0.3921	50.00- 150.00	100.00(a)	
13.416	13.416	(0.968)	96	6368			29.23- 129.23	74.92	
13.416	13.416	(0.968)	98	3654			0.16- 100.16	42.99	

80	Tetrahydrofuran					CAS #:	109-99-9		
13.858	13.858	(1.000)	42	3765	0.50000	0.2892	50.00- 150.00	100.00(a)	
13.858	13.858	(1.000)	71	1508			0.61- 100.61	40.05	
13.858	13.858	(1.000)	72	2387			8.31- 108.31	63.40	

82	Chloroform					CAS #:	67-66-3		
13.941	13.941	(1.006)	83	13300	0.50000	0.3682	50.00- 150.00	100.00(a)	
13.941	13.941	(1.006)	85	9141			18.46- 118.46	68.73	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

83	1,1,1-Trichloroethane					CAS #:	71-55-6		
14.273	14.273	(1.030)	97	16261	0.50000	0.3759	50.00-	150.00	100.00(a)
14.273	14.273	(1.030)	99	9023			13.89-	113.89	55.49

85	Cyclohexane					CAS #:	110-82-7		
14.301	14.301	(1.032)	84	6931	0.50000	0.3140	50.00-	150.00	100.00(a)
14.273	14.273	(1.030)	56	5912			43.75-	143.75	85.30
14.301	14.301	(1.032)	41	4069			1.66-	101.66	58.71

87	Carbon Tetrachloride					CAS #:	56-23-5		
14.522	14.522	(1.048)	119	14440	0.50000	0.3427	50.00-	150.00	100.00(a)
14.522	14.522	(1.048)	117	14659			54.19-	154.19	101.52

91	Benzene					CAS #:	71-43-2		
14.964	14.964	(0.958)	78	17595	0.50000	0.3753	50.00-	150.00	100.00(a)
14.964	14.964	(0.958)	77	4671			0.00-	73.32	26.55

89	2,2,4-Trimethylpentane					CAS #:	540-84-1		
14.881	14.881	(1.074)	57	20178	0.50000	0.3278	50.00-	150.00	100.00(a)
14.881	14.881	(1.074)	56	6838			0.00-	83.27	33.89
14.881	14.881	(1.074)	41	6564			0.00-	77.74	32.53

93	1,2-Dichloroethane					CAS #:	107-06-2		
15.075	15.075	(0.965)	62	9039	0.50000	0.3860	50.00-	150.00	100.00(a)
15.075	15.075	(0.965)	64	2946			0.00-	82.87	32.59

94	Heptane					CAS #:	142-82-5		
15.158	15.158	(0.970)	71	4812	0.50000	0.3231	50.00-	150.00	100.00(a)
15.158	15.158	(0.970)	43	5690			77.61-	177.61	118.25
15.185	15.185	(0.972)	57	4588			32.99-	132.99	95.34

101	Trichloroethene					CAS #:	79-01-6		
16.070	16.070	(1.028)	95	7223	0.50000	0.3334	50.00-	150.00	100.00(a)
16.070	16.070	(1.028)	130	7085			45.55-	145.55	98.09
16.070	16.070	(1.028)	97	4879			15.22-	115.22	67.55

104	1,2-Dichloropropane					CAS #:	78-87-5		
16.568	16.568	(1.060)	63	4865	0.50000	0.3105	50.00-	150.00	100.00(a)
16.568	16.568	(1.060)	62	3769			23.00-	123.00	77.47
16.540	16.540	(1.058)	41	3444			8.64-	108.64	70.79

107	Bromodichloromethane					CAS #:	75-27-4		
16.983	16.983	(1.087)	83	11868	0.50000	0.3149	50.00-	150.00	100.00(a)
16.983	16.983	(1.087)	85	8406			16.51-	116.51	70.83

110	cis-1,3-Dichloropropene					CAS #:	10061-01-5		
17.784	17.784	(1.138)	75	7196	0.50000	0.2852	50.00-	150.00	100.00(a)

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
110 cis-1,3-Dichloropropene (continued)									
17.784	17.784	(1.138)	77	2850			0.00- 83.76	39.61	
17.784	17.784	(1.138)	39	3450			0.00- 94.73	47.94	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.978	17.978	(1.150)	58	3240	0.50000	0.2822	50.00- 150.00	100.00(a)	
17.950	17.950	(1.149)	43	5756			168.02- 268.02	177.65	
0.000	1.000	(0.000)	85	0			2.69- 102.69	0.00	

114 Toluene CAS #: 108-88-3									
18.337	18.337	(1.173)	91	19549	0.50000	0.3456	50.00- 150.00	100.00(a)	
18.337	18.337	(1.173)	92	11525			9.70- 109.70	58.95	

116 trans-1,3-Dichloropropene CAS #: 10061-02-6									
18.752	18.752	(0.902)	75	8811	0.50000	0.3082	50.00- 150.00	100.00(a)	
18.752	18.752	(0.902)	77	3281			0.00- 82.23	37.24	
18.752	18.752	(0.902)	39	3884			0.00- 88.37	44.08	

117 1,1,2-Trichloroethane CAS #: 79-00-5									
19.112	19.112	(0.919)	97	6096	0.50000	0.2939	50.00- 150.00	100.00(a)	
19.112	19.112	(0.919)	99	4743			15.96- 115.96	77.81	
19.112	19.112	(0.919)	83	6053			36.03- 136.03	99.29	

120 Tetrachloroethene CAS #: 127-18-4									
19.277	19.277	(0.927)	166	9716	0.50000	0.3362	50.00- 150.00	100.00(a)	
19.277	19.277	(0.927)	129	7138			20.82- 120.82	73.47	
19.277	19.277	(0.927)	131	6558			18.42- 118.42	67.50	

122 Dibromochloromethane CAS #: 124-48-1									
19.803	19.803	(0.952)	129	10932	0.50000	0.2999	50.00- 150.00	100.00(a)	
19.803	19.803	(0.952)	127	7608			25.33- 125.33	69.59	

123 1,2-Dibromoethane CAS #: 106-93-4									
20.052	20.052	(0.964)	107	11282	0.50000	0.3234	50.00- 150.00	100.00(a)	
20.052	20.052	(0.964)	109	9675			41.12- 141.12	85.76	

127 Chlorobenzene CAS #: 108-90-7									
20.854	20.854	(1.003)	112	16767	0.50000	0.3329	50.00- 150.00	100.00(a)	
20.854	20.854	(1.003)	114	4786			0.00- 80.99	28.54	
20.798	20.798	(1.000)	77	21537			25.73- 125.73	128.45	

128 Ethyl Benzene CAS #: 100-41-4									
20.936	20.936	(1.007)	106	7857	0.50000	0.3080	50.00- 150.00	100.00(a)	
20.936	20.936	(1.007)	91	25011			266.56- 366.56	318.33	

129 m,p-Xylene CAS #: 108-38-3									
21.130	21.130	(1.016)	106	7524	0.50000	0.2398	50.00- 150.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
129 m,p-Xylene (continued)									
21.130	21.130	(1.016)	91	17422			157.11- 257.11	231.55	

130 o-Xylene CAS #: 95-47-6									
21.849	21.849	(1.051)	106	7646	0.50000	0.2594	50.00- 150.00	100.00(a)	
21.849	21.849	(1.051)	91	18394			166.77- 266.77	240.57	

131 Styrene CAS #: 100-42-5									
21.877	21.877	(1.052)	104	11536	0.50000	0.2415	50.00- 150.00	100.00(a)	
21.877	21.877	(1.052)	78	6541			12.82- 112.82	56.70	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	11105	0.50000	0.2922	50.00- 150.00	100.00(a)	
22.291	22.291	(1.072)	171	5041			0.34- 100.34	45.39	

134 Cumene CAS #: 98-82-8									
22.430	22.430	(1.078)	105	23936	0.50000	0.2841	50.00- 150.00	100.00(a)	
22.430	22.430	(1.078)	120	5184			0.00- 74.52	21.66	
22.402	22.402	(1.077)	51	2418			51.79- 151.79	10.10	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	12679	0.50000	0.2745	50.00- 150.00	100.00(a)	
23.010	23.010	(1.106)	85	10161			17.66- 117.66	80.14	

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	32735	0.50000	0.3072	50.00- 150.00	100.00(a)	
23.121	23.121	(1.112)	120	6387			0.00- 71.52	19.51	
23.121	23.121	(1.112)	105	1068			0.00- 53.54	3.26	

145 4-Ethyltoluene CAS #: 622-96-8									
23.287	23.287	(1.120)	105	22610	0.50000	0.2519	50.00- 150.00	100.00(a)	
23.287	23.287	(1.120)	120	6972			0.00- 79.85	30.84	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	17850	0.50000	0.2444	50.00- 150.00	100.00(a)	
23.397	23.397	(1.125)	120	9909			0.29- 100.29	55.51	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	17266	0.50000	0.2540	50.00- 150.00	100.00(a)	
24.033	24.033	(1.156)	120	7344			0.00- 94.69	42.53	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	16434	0.50000	0.3194	50.00- 150.00	100.00(a)	
24.586	24.586	(1.182)	148	11163			14.61- 114.61	67.93	
24.586	24.586	(1.182)	111	7060			0.00- 92.01	42.96	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

156	1,4-Dichlorobenzene			CAS #: 106-46-7					
24.724	24.724	(1.189)	146	18151	0.50000	0.3396	50.00- 150.00	100.00(a)	
24.724	24.724	(1.189)	148	12225			13.83- 113.83	67.35	
24.724	24.724	(1.189)	111	6800			0.00- 89.75	37.46	

159	alpha-Chlorotoluene			CAS #: 100-44-7					
24.946	24.946	(1.199)	91	19854	0.50000	0.2684	50.00- 150.00	100.00(a)	
24.946	24.946	(1.199)	126	4039			0.00- 69.65	20.34	

161	1,2-Dichlorobenzene			CAS #: 95-50-1					
25.360	25.360	(1.219)	146	16588	0.50000	0.3363	50.00- 150.00	100.00(a)	
25.360	25.360	(1.219)	148	10652			14.36- 114.36	64.22	
25.360	25.360	(1.219)	111	6669			0.00- 92.81	40.20	

102	Methyl Cyclohexane			CAS #: 108-87-2					
16.347	16.347	(1.180)	83	9197	0.50000	0.3286	50.00- 150.00	100.00(a)	
16.347	16.347	(1.180)	98	3570			0.00- 95.49	38.82	
16.347	16.347	(1.180)	55	6146			16.76- 116.76	66.83	

QC Flag Legend

a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).

Report Date: 14-Dec-2007 10:40

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121319.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 0.5ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	299081	6.53
97 1,4-Difluorobenze	1182601	709561	1655641	1174268	-0.70
126 Chlorobenzene-d5	1033655	620193	1447117	1056467	2.21

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/13Dec2007,b/t121319.d

Date : 14-DEC-2007 09:58

Client ID: Level 2

Sample Info: 0.5ml #1443-378


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/13Dec2007,b/t121319.d

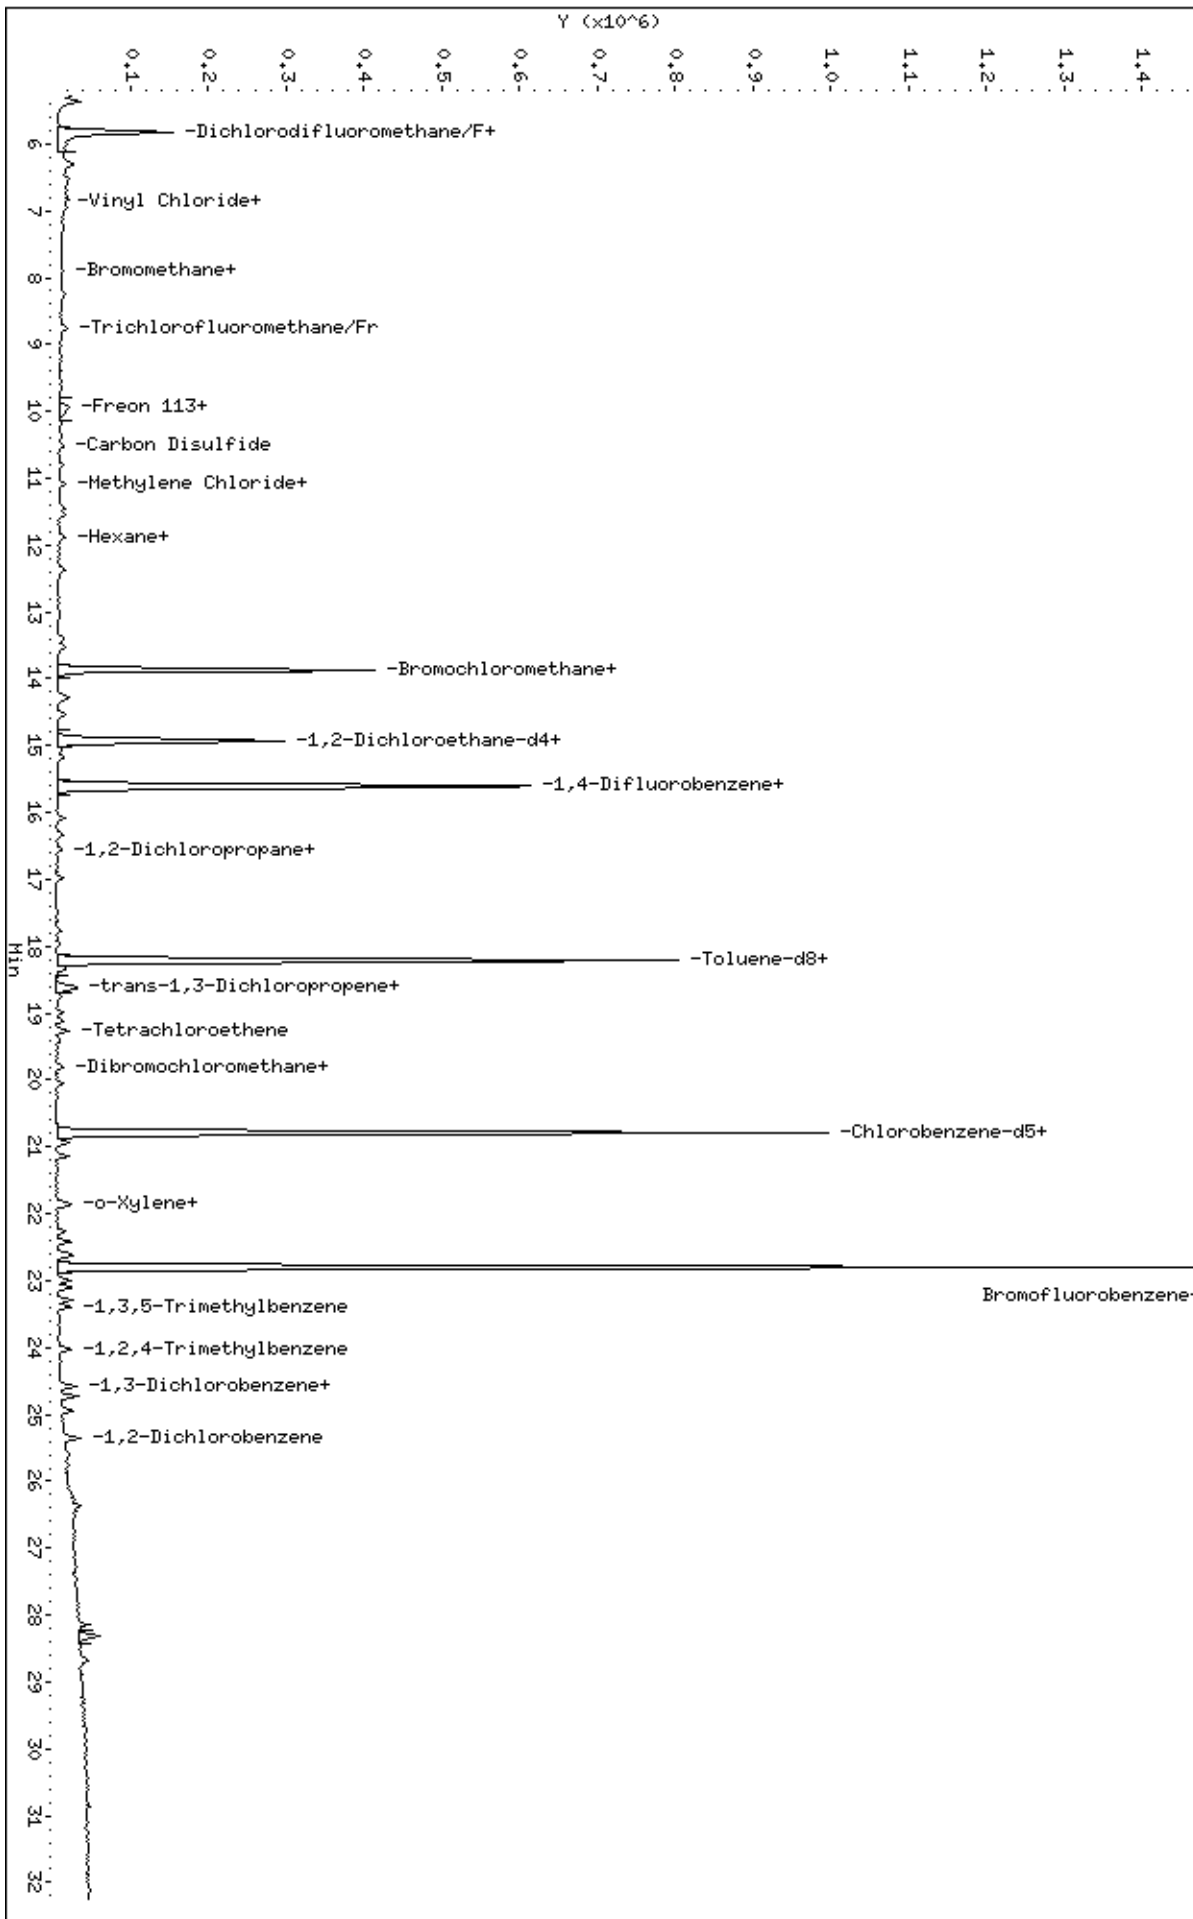

Report Date: 25-Jan-2008 14:48

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/25Jan2008.b/t012504.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 25-JAN-2008 11:27
 Operator : sjr Inst ID: msdt.i
 Smp Info : 2.0mL #1576-236
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Meth Date : 25-Jan-2008 14:48 sruth Quant Type: ISTD
 Cal Date : 25-JAN-2008 11:27 Cal File: t012504.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp12e.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	342500	25.0000		50.00- 150.00	100.00	
13.858	13.858	(1.000)	128	260401			26.56- 126.56	76.03	
13.858	13.858	(1.000)	49	361137			59.90- 159.90	105.44	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1131238	25.0000		50.00- 150.00	100.00	
15.628	15.628	(1.000)	88	176362			0.00- 65.68	15.59	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1094274	25.0000		50.00- 150.00	100.00	
20.798	20.798	(1.000)	82	615187			6.02- 106.02	56.22	

21 Isobutane CAS #: 75-28-5									
6.337	6.337	(0.457)	43	57059	2.00000	2.000	50.00- 150.00	100.00	
6.337	6.337	(0.457)	42	18501			0.00- 82.42	32.42	
6.365	6.365	(0.459)	58	1610			0.00- 52.82	2.82	

35 1-Pentene CAS #: 109-67-1									
8.798	8.798	(0.635)	55	38015	2.00000	2.000	50.00- 150.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
35 1-Pentene (continued)									
8.798	8.798	(0.635)	42	34115			39.74- 139.74	89.74	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

44 Acrolein CAS #: 107-02-8									
9.904	9.904	(0.715)	55	9495	2.00000	2.000	50.00- 150.00	100.00	
9.877	9.877	(0.713)	56	13529			92.49- 192.49	142.49	

48 Ethyl acrylate CAS #: 140-88-5									
16.153	16.153	(1.034)	99	5303	2.00000	2.000	50.00- 150.00	100.00	
16.153	16.153	(1.034)	45	4862			41.68- 141.68	91.68	
16.153	16.153	(1.034)	55	52003			930.63-1030.63	980.63	

49 Iodomethane CAS #: 74-88-4									
10.430	10.430	(0.753)	142	86294	2.00000	2.000	50.00- 150.00	100.00	
10.430	10.430	(0.753)	127	42077			0.00- 98.76	48.76	

50 Methyl Methacrylate CAS #: 80-62-6									
16.568	16.568	(1.060)	41	31557	2.00000	2.000	50.00- 150.00	100.00	
16.568	16.568	(1.060)	69	31735			50.56- 150.56	100.56	
16.568	16.568	(1.060)	100	11767			0.00- 87.29	37.29	

52 Acetonitrile CAS #: 75-05-8									
10.900	10.900	(0.786)	40	21981	2.00000	2.000	50.00- 150.00	100.00	
10.900	10.900	(0.786)	41	21070			45.86- 145.86	95.86	
10.900	10.900	(0.786)	38	3981			0.00- 68.11	18.11	

56 Cyclopentane CAS #: 287-92-3									
11.093	11.093	(0.800)	70	21210	2.00000	2.000	50.00- 150.00	100.00	
11.093	11.093	(0.800)	55	26182			73.44- 173.44	123.44	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

62 Acrylonitrile CAS #: 107-13-1									
11.646	11.646	(0.840)	53	23517	2.00000	2.000	50.00- 150.00	100.00	
11.646	11.646	(0.840)	52	19516			32.99- 132.99	82.99	

63 2-Pentanone CAS #: 107-87-9									
16.374	16.374	(1.048)	43	51435	2.00000	2.000	50.00- 150.00	100.00	
16.374	16.374	(1.048)	58	4827			0.00- 59.38	9.38	
16.374	16.374	(1.048)	86	12444			0.00- 74.19	24.19	

66 1-Hexene CAS #: 592-41-6									
11.784	11.784	(0.850)	55	17295	2.00000	2.000	50.00- 150.00	100.00	
11.784	11.784	(0.850)	41	28923			117.23- 217.23	167.23	
11.784	11.784	(0.850)	84	10957			13.35- 113.35	63.35	

AMOUNTS

RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
105 Dibromomethane						CAS #: 74-95-3		
16.789	16.789	(1.074)	174	46800	2.00000	2.000	50.00- 150.00	100.00
16.789	16.789	(1.074)	93	48172			52.93- 152.93	102.93
16.789	16.789	(1.074)	95	39358			34.10- 134.10	84.10

Report Date: 25-Jan-2008 14:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 25-JAN-2008

Lab File ID: t012504.d

Calibration Time: 09:00

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/25Jan2008.b/t14q1213e.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	313448	188069	438827	342500	9.27
97 1,4-Difluorobenze	1165419	699251	1631587	1131238	-2.93
126 Chlorobenzene-d5	1132615	679569	1585661	1094274	-3.39

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.86	-0.20
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/25Jan2008,b/t012504.d

Date: 25-JAN-2008 11:27

Client ID: Level 3

Sample Info: 2.0mL #1576-236


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/25Jan2008,b/t012504.d

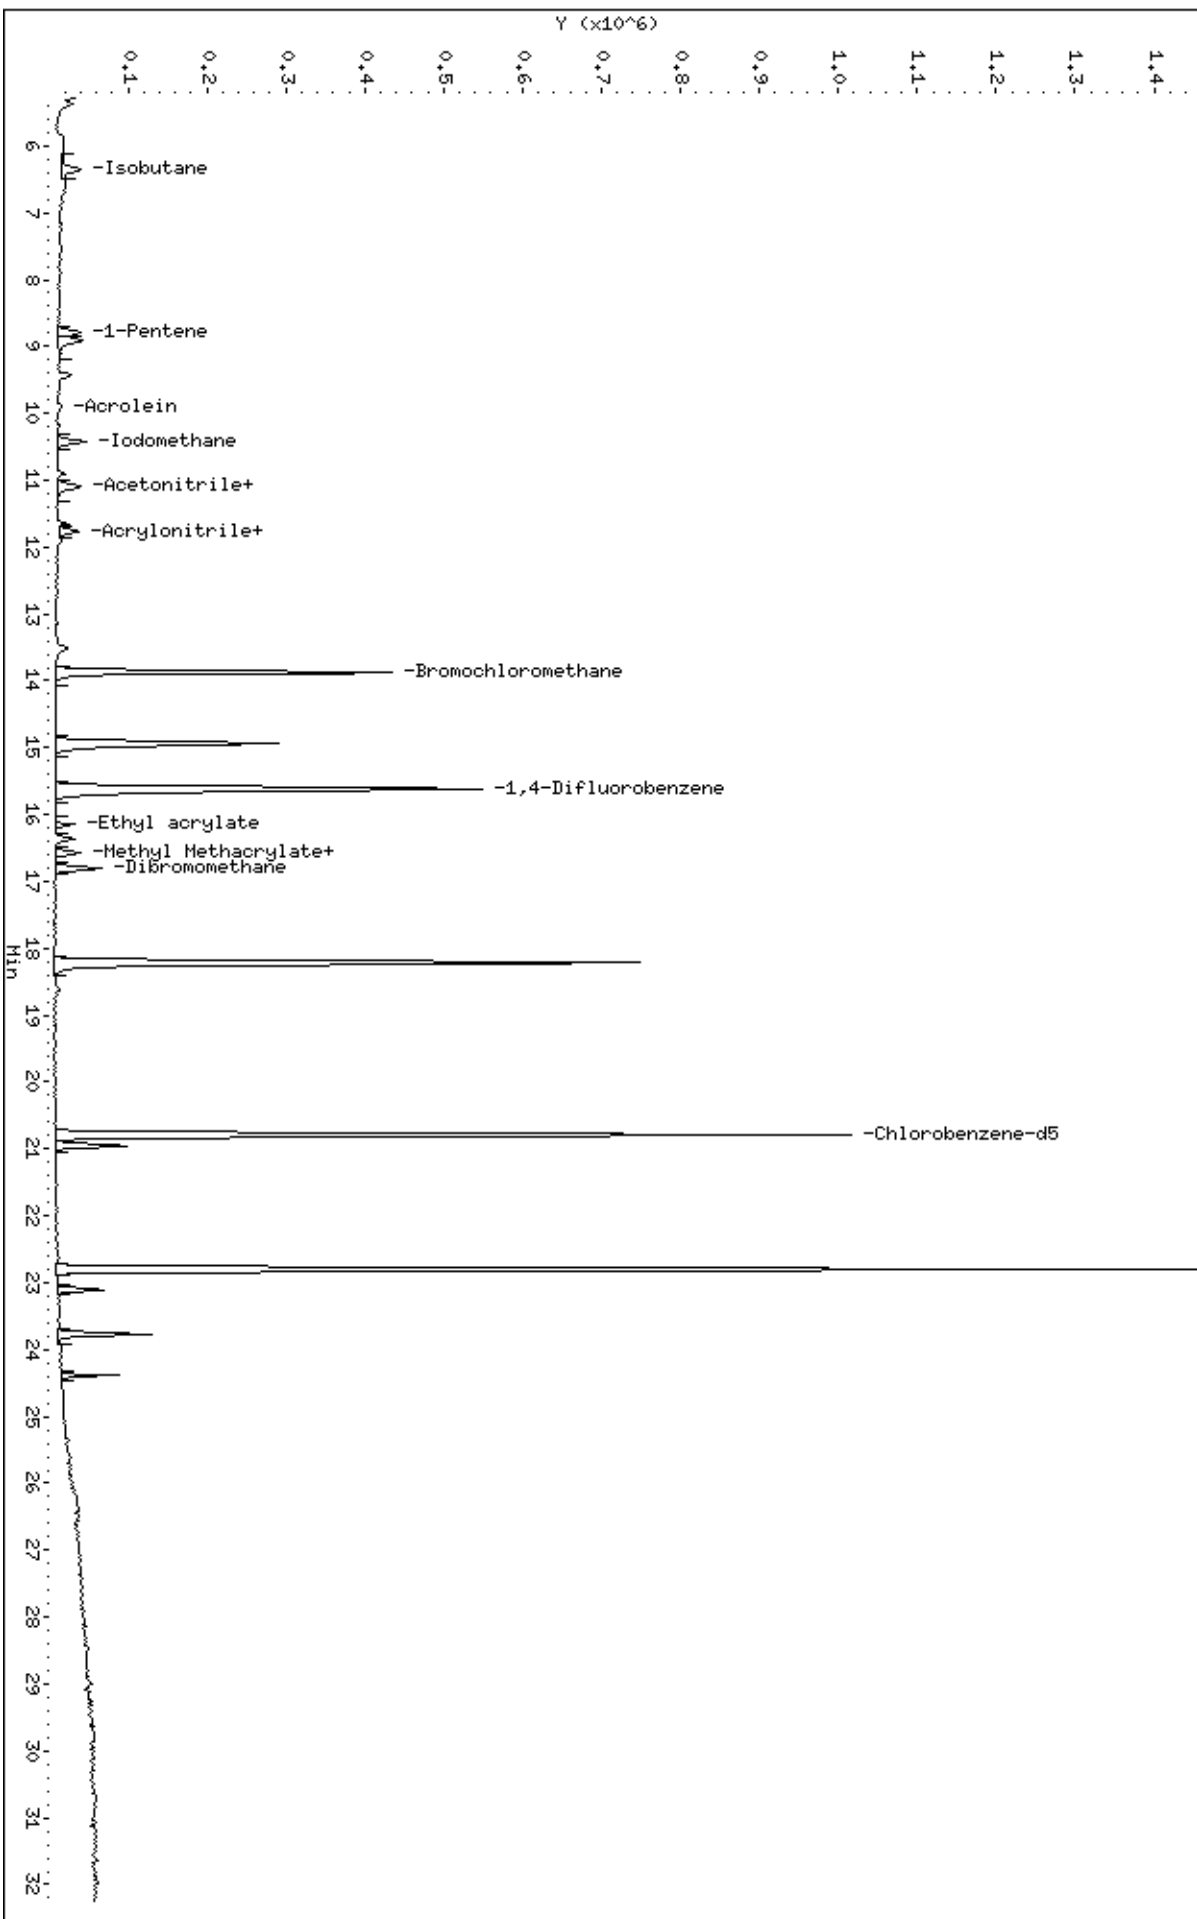

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/16Jan2008.b/t011608.d
 Lab Smp Id: TVH ICAL Client Smp ID: Level 3
 Inj Date : 16-JAN-2008 13:05
 Operator : lo Inst ID: msdt.i
 Smp Info : 2ml #1443-403
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/t14q1213d.m
 Meth Date : 16-Jan-2008 14:59 lover Quant Type: ISTD
 Cal Date : 16-JAN-2008 13:05 Cal File: t011608.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5d.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	325455	25.0000			50.00- 150.00	100.00
13.886	13.886	(1.000)	128	256909				27.05- 127.05	78.94
13.858	13.858	(1.000)	49	371229				61.34- 161.34	114.06

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1069240	25.0000			50.00- 150.00	100.00
15.628	15.628	(1.000)	88	169750				0.00- 65.73	15.88

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1107452	25.0000			50.00- 150.00	100.00
20.798	20.798	(1.000)	82	616797				5.94- 105.94	55.70

204 Propane CAS #: 74-98-6									
5.840	5.840	(0.421)	43	7801	2.00000	1.992		50.00- 150.00	100.00
5.812	5.812	(0.419)	44	25823				107.53- 207.53	331.02

37 Pentane CAS #: 109-66-0									
8.936	8.936	(0.644)	43	48819	2.00000	1.709		50.00- 150.00	100.00(a)
8.964	8.964	(0.646)	57	7450				0.00- 67.03	15.26

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
37 Pentane (continued)									
8.936	8.936	(0.644)	72	4638			0.00- 62.09	9.50	

112 Octane									
						CAS #: 111-65-9			
18.282	18.282	(1.170)	57	28842	2.00000	1.891	50.00- 150.00	100.00(a)	
18.282	18.282	(1.170)	85	33355			82.32- 182.32	115.65	
18.282	18.282	(1.170)	43	62064			166.39- 266.39	215.19	

124 Nonane									
						CAS #: 111-84-2			
20.964	20.964	(1.008)	43	55065	2.00000	1.548	50.00- 150.00	100.00(a)	
20.964	20.964	(1.008)	57	55025			52.38- 152.38	99.93	
20.964	20.964	(1.008)	85	23489			0.00- 95.58	42.66	

139 Decane									
						CAS #: 124-18-5			
23.204	23.204	(1.116)	57	57238	2.00000	1.339	50.00- 150.00	100.00(a)	
23.204	23.204	(1.116)	71	24835			0.00- 93.78	43.39	
23.231	23.231	(1.117)	142	2695			0.00- 54.94	4.71	

QC Flag Legend

a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 16-JAN-2008

Lab File ID: t011608.d

Calibration Time: 13:44

Lab Smp Id: TVH ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lo

Method File: /chem/msdt.i/16Jan2008.b/t14q1213d.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	325810	195486	456134	325455	-0.11
97 1,4-Difluorobenze	1168077	700846	1635308	1069240	-8.46
126 Chlorobenzene-d5	1103278	661967	1544589	1107452	0.38

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/16Jan2008,b/t011608.d

Date : 16-Jan-2008 13:05

Client ID: Level 3

Sample Info: 2ml #1443-403


Column phase: RTX-624

Instrument: msdt,i

Operator: lo

Column diameter: 0.53

/chem/msdt,i/16Jan2008,b/t011608.d

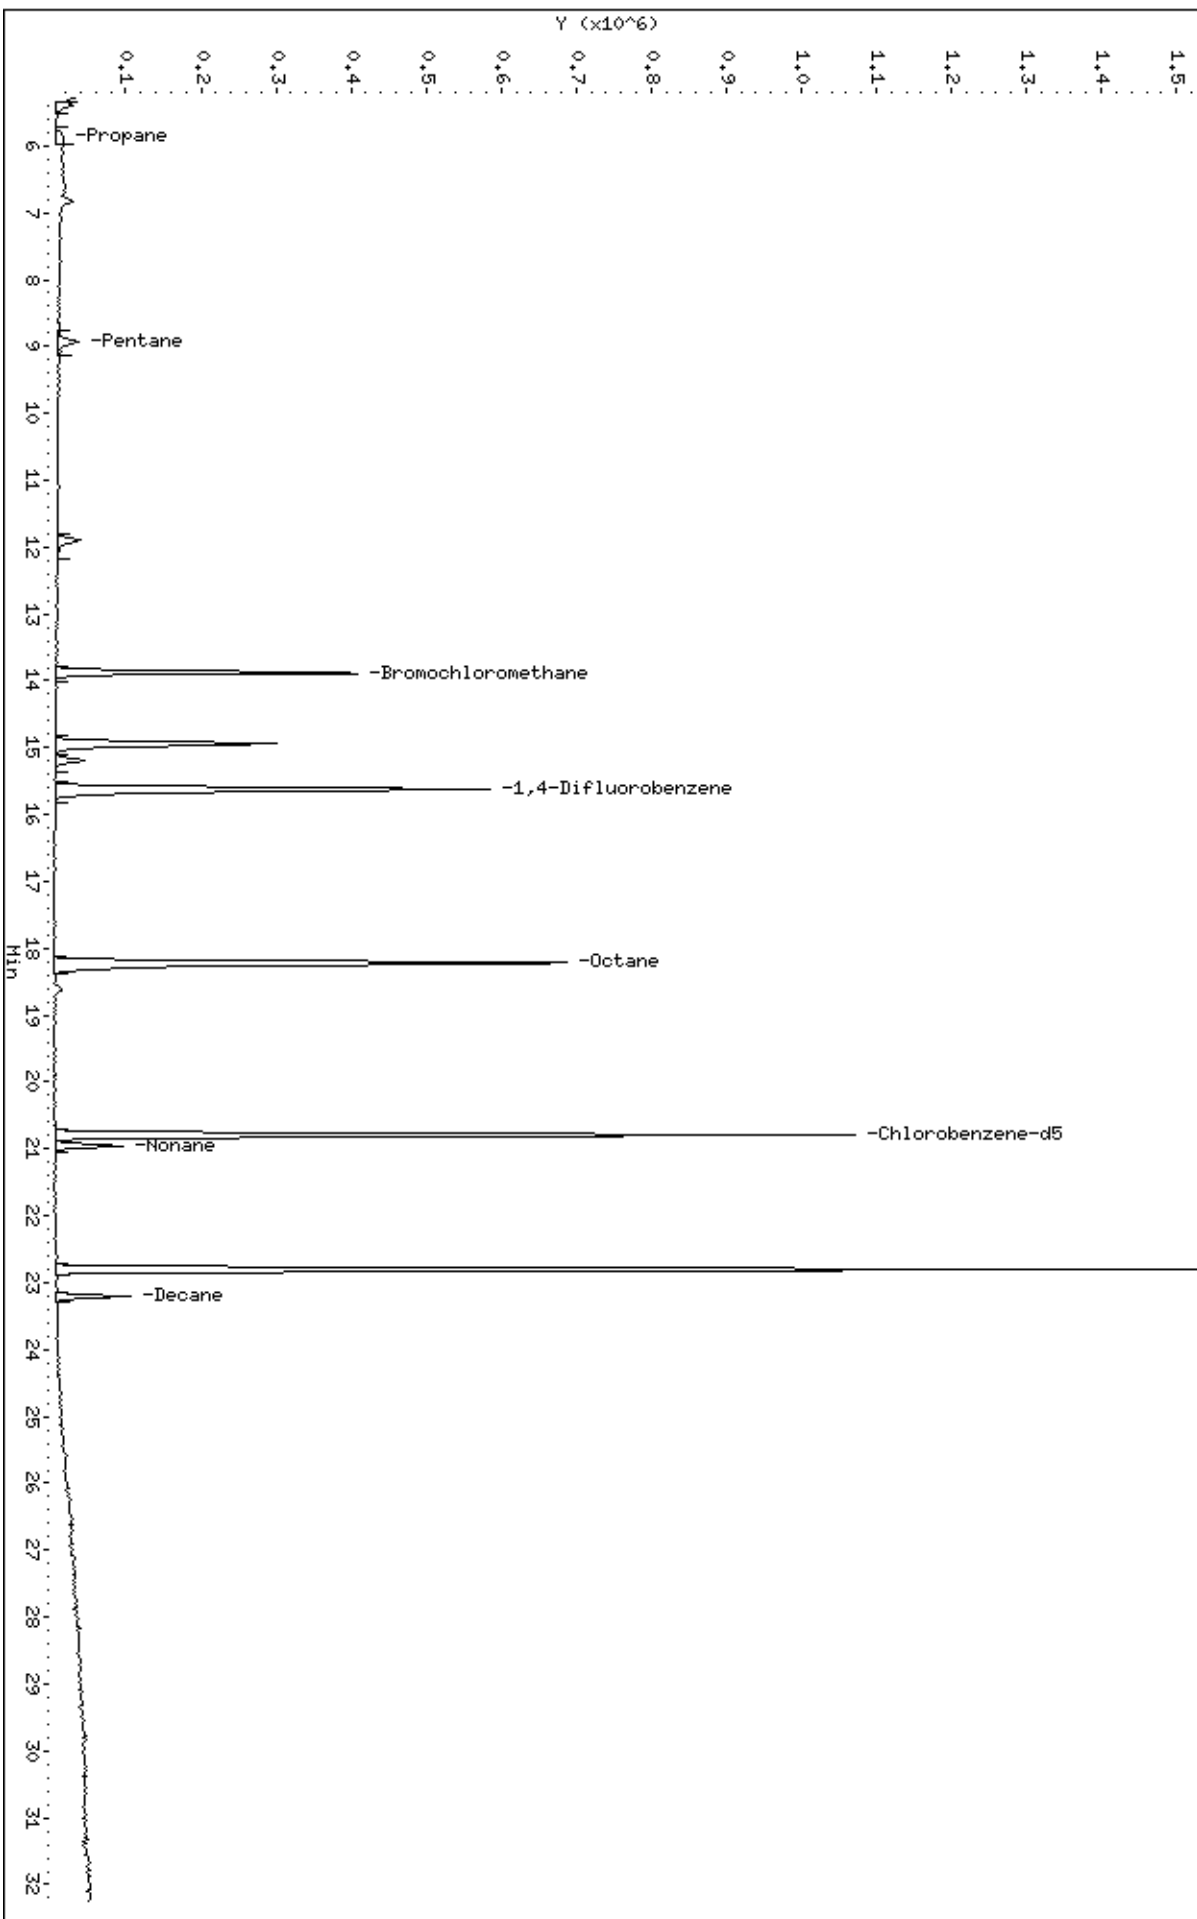

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/02Jan2008.b/t010202.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 02-JAN-2008 10:39
 Operator : sjr Inst ID: msdt.i
 Smp Info : 2.0ml #1443-399
 Misc Info : 200ppbv -> 2.0ppbv (12ppbv MeOH)
 Comment :
 Method : /chem/msdt.i/02Jan2008.b/t14q1213c.m
 Meth Date : 02-Jan-2008 15:46 sruth Quant Type: ISTD
 Cal Date : 02-JAN-2008 10:39 Cal File: t010202.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp22c.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.865	13.865	(1.000)	130	356282	25.0000		50.00- 150.00	100.00	
13.865	13.865	(1.000)	128	267623			26.86- 126.86	75.12	
13.865	13.865	(1.000)	49	396005			74.17- 174.17	111.15	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.607	15.607	(1.000)	114	1262976	25.0000		50.00- 150.00	100.00	
15.607	15.607	(1.000)	88	207338			0.00- 66.07	16.42	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.805	20.805	(1.000)	117	1299796	25.0000		50.00- 150.00	100.00	
20.805	20.805	(1.000)	82	731602			5.77- 105.77	56.29	

6 Freon142b CAS #: 75-68-3									
6.436	6.436	(0.464)	65	87974	2.00000	1.911	50.00- 150.00	100.00(a)	
6.436	6.436	(0.464)	45	19662			0.00- 71.17	22.35	

9 Freon 13 CAS #: 75-72-9									
5.394	5.394	(0.389)	69	86884	2.00000	1.923	50.00- 150.00	100.00(aH)	
5.422	5.422	(0.391)	85	27150			0.00- 83.23	31.25	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
9 Freon 13 (continued)									
5.422	5.422	(0.391)	87	9388			0.00- 60.80	10.81	

13 Freon 134a CAS #: 811-97-2									
5.675	5.675	(0.409)	83	39459	2.00000	1.938	50.00- 150.00	100.00(a)	
5.675	5.675	(0.409)	69	32663			29.59- 129.59	82.78	

15 Freon 152a CAS #: 75-37-6									
5.844	5.844	(0.422)	65	26428	2.00000	2.438	50.00- 150.00	100.00	
5.844	5.844	(0.422)	51	47671			125.61- 225.61	180.38	
5.844	5.844	(0.422)	47	12639			0.00- 95.62	47.82	

17 Freon 22 CAS #: 75-45-6									
5.985	5.985	(0.432)	67	11334	2.00000	2.034	50.00- 150.00	100.00	
5.985	5.985	(0.432)	51	55603			424.04- 524.04	490.59	
6.013	6.013	(0.434)	85	1213			0.00- 60.14	10.70	

26 Methanol CAS #: 67-56-1									
7.562	7.562	(0.545)	31	75103	12.0000	16.296	50.00- 150.00	100.00(a)	
7.562	7.562	(0.545)	32	217717			127.28- 227.28	289.89	

34 Dichlorofluoromethane/Fr21 CAS #: 75-43-4									
8.717	8.717	(0.629)	67	72422	2.00000	2.029	50.00- 150.00	100.00	
8.717	8.717	(0.629)	69	22711			0.00- 82.55	31.36	
8.717	8.717	(0.629)	35	4161			0.00- 55.68	5.75	

40 Freon123a CAS #: 354-23-4									
9.579	9.579	(0.691)	67	51133	2.00000	1.852	50.00- 150.00	100.00(a)	
9.579	9.579	(0.691)	117	39948			33.27- 133.27	78.13	

41 Freon123 CAS #: 306-83-2									
9.718	9.718	(0.701)	83	70472	2.00000	1.859	50.00- 150.00	100.00(a)	
9.718	9.718	(0.701)	133	15074			0.00- 72.56	21.39	
9.718	9.718	(0.701)	85	50873			21.04- 121.04	72.19	

57 tert-Butyl-Alcohol CAS #: 75-65-0									
11.155	11.155	(0.805)	59	51445	2.00000	1.514	50.00- 150.00	100.00(a)	
11.155	11.155	(0.805)	41	15086			0.00- 79.32	29.32	
11.183	11.183	(0.807)	57	5619			0.00- 60.92	10.92	

68 Isopropyl ether CAS #: 108-20-3									
12.289	12.289	(0.886)	45	86946	2.00000	1.695	50.00- 150.00	100.00(a)	
12.289	12.289	(0.886)	87	27675			0.00- 81.01	31.83	
12.289	12.289	(0.886)	59	10751			0.00- 61.81	12.37	

71 1-Propanol CAS #: 71-23-8									
12.427	12.427	(0.896)	42	6546	2.00000	1.944	50.00- 150.00	100.00(a)	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	====	=====	=====	=====	=====	=====		
71 1-Propanol (continued)										
12.427	12.427	(0.896)	59	5021			61.64- 161.64	76.70		
12.400	12.400	(0.894)	41	6066			40.91- 140.91	92.67		

73 t-Butylethyl Ether										
						CAS #: 637-92-3				
12.925	12.925	(0.932)	59	90261	2.00000	1.612	50.00- 150.00	100.00(a)		
12.925	12.925	(0.932)	87	38086			0.00- 93.11	42.20		
12.925	12.925	(0.932)	41	20573			0.00- 70.41	22.79		

77 Ethyl Acetate										
						CAS #: 141-78-6				
13.395	13.395	(0.966)	45	10695	2.00000	1.842	50.00- 150.00	100.00(a)		
13.395	13.395	(0.966)	61	9600			49.68- 149.68	89.76		
13.395	13.395	(0.966)	43	69150			615.05- 715.05	646.56		

92 tert-amyl-Methyl Ether										
						CAS #: 994-05-8				
14.999	14.999	(1.082)	73	78206	2.00000	1.530	50.00- 150.00	100.00(a)		
14.999	14.999	(1.082)	87	20895			0.00- 74.91	26.72		
14.999	14.999	(1.082)	55	22867			0.00- 76.64	29.24		

96 2-Heptanone										
						CAS #: 110-43-0				
21.966	21.966	(1.584)	58	35610	2.00000	1.241	50.00- 150.00	100.00(a)		
21.966	21.966	(1.584)	43	54036			98.27- 198.27	151.74		

98 1-Butanol										
						CAS #: 71-36-3				
15.801	15.801	(1.012)	56	11880	2.00000	1.257	50.00- 150.00	100.00(a)		
15.801	15.801	(1.012)	41	11073			28.59- 128.59	93.21		
15.773	15.773	(1.011)	43	7397			6.69- 106.69	62.26		

119 Butyl Acetate										
						CAS #: 123-86-4				
19.533	19.533	(1.252)	56	27971	2.00000	1.572	50.00- 150.00	100.00(a)		
19.533	19.533	(1.252)	73	15140			0.00- 95.25	54.13		
19.533	19.533	(1.252)	43	58602			169.61- 269.61	209.51		

135 Cyclohexanone										
						CAS #: 108-94-1				
22.741	22.741	(1.093)	55	29913	2.00000	1.381	50.00- 150.00	100.00(a)		
22.741	22.741	(1.093)	98	14914			2.09- 102.09	49.86		
22.741	22.741	(1.093)	42	19724			15.79- 115.79	65.94		

146 Diisobutyl Ketone										
						CAS #: 108-83-8				
23.542	23.542	(1.132)	57	70371	2.00000	1.342	50.00- 150.00	100.00(a)		
23.570	23.570	(1.133)	85	68500			46.68- 146.68	97.34		
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00		

QC Flag Legend

- a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).
- H - Operator selected an alternate compound hit.

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 02-JAN-2008

Lab File ID: t010202.d

Calibration Time: 12:02

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/02Jan2008.b/t14q1213c.m

Misc Info: 200ppbv -> 2.0ppbv (12ppbv MeOH)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	338913	203348	474478	356282	5.12
97 1,4-Difluorobenze	1251078	750647	1751509	1262976	0.95
126 Chlorobenzene-d5	1269166	761500	1776832	1299796	2.41

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.61	-0.18
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/02Jan2008,b/t010202.d

Date : 02-JAN-2008 10:39

Client ID: Level 3

Sample Info: 2.0ml #1443-399


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

Page 1

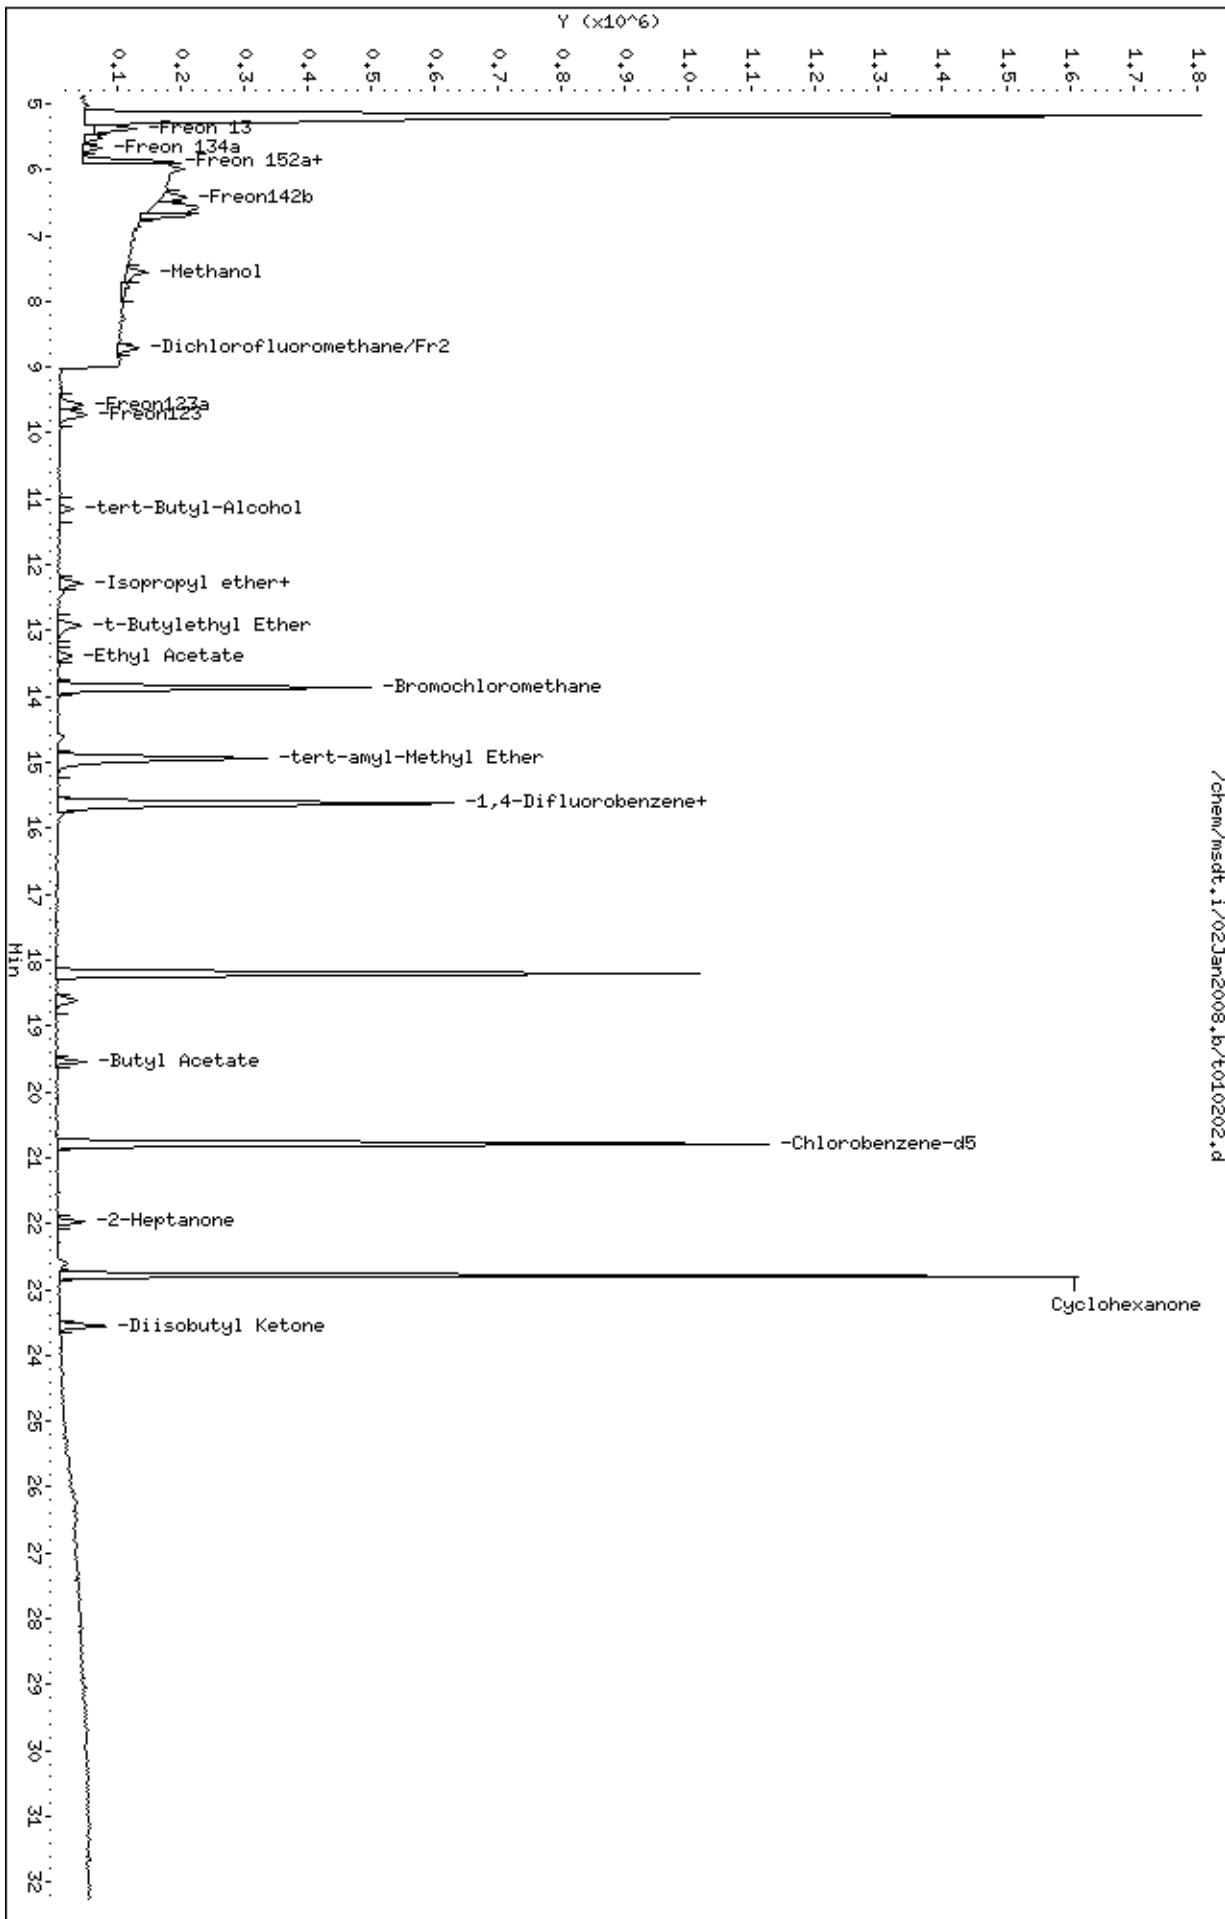

Report Date: 19-Dec-2007 12:55

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/19Dec2007.b/t121902.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 19-DEC-2007 10:31
 Operator : sjr Inst ID: msdt.i
 Smp Info : 2.0ml #1443-388
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msdt.i/19Dec2007.b/t14q1213b.m
 Meth Date : 19-Dec-2007 12:54 sruth Quant Type: ISTD
 Cal Date : 19-DEC-2007 10:31 Cal File: t121902.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: splb.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.865	13.865	(1.000)	130	215661	25.0000		50.00- 150.00	100.00	
13.865	13.865	(1.000)	128	169262			27.34- 127.34	78.49	
13.865	13.865	(1.000)	49	261041			80.38- 180.38	121.04	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.635	15.635	(1.000)	114	903019	25.0000		50.00- 150.00	100.00	
15.607	15.607	(1.000)	88	147178			0.00- 65.86	16.30	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.805	20.805	(1.000)	117	821598	25.0000		50.00- 150.00	100.00	
20.805	20.805	(1.000)	82	468836			6.00- 106.00	57.06	

199 Vinyl Fluoride CAS #: 75-02-5									
5.591	5.591	(0.403)	46	13211	2.00000	2.289	50.00- 150.00	100.00	
5.591	5.591	(0.403)	45	9106			20.20- 120.20	68.93	
0.000	1.000	(0.000)	47	0			0.00- 52.23	0.00	

Report Date: 19-Dec-2007 12:55

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 19-DEC-2007

Lab File ID: t121902.d

Calibration Time: 11:12

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/19Dec2007.b/t14q1213b.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	204685	122811	286559	215661	5.36
97 1,4-Difluorobenze	866754	520052	1213456	903019	4.18
126 Chlorobenzene-d5	784408	470645	1098171	821598	4.74

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/19Dec2007,b/t121902.d

Date : 19-DEC-2007 10:31

Client ID: Level 3

Sample Info: 2.0ml #1443-388


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/19Dec2007,b/t121902.d

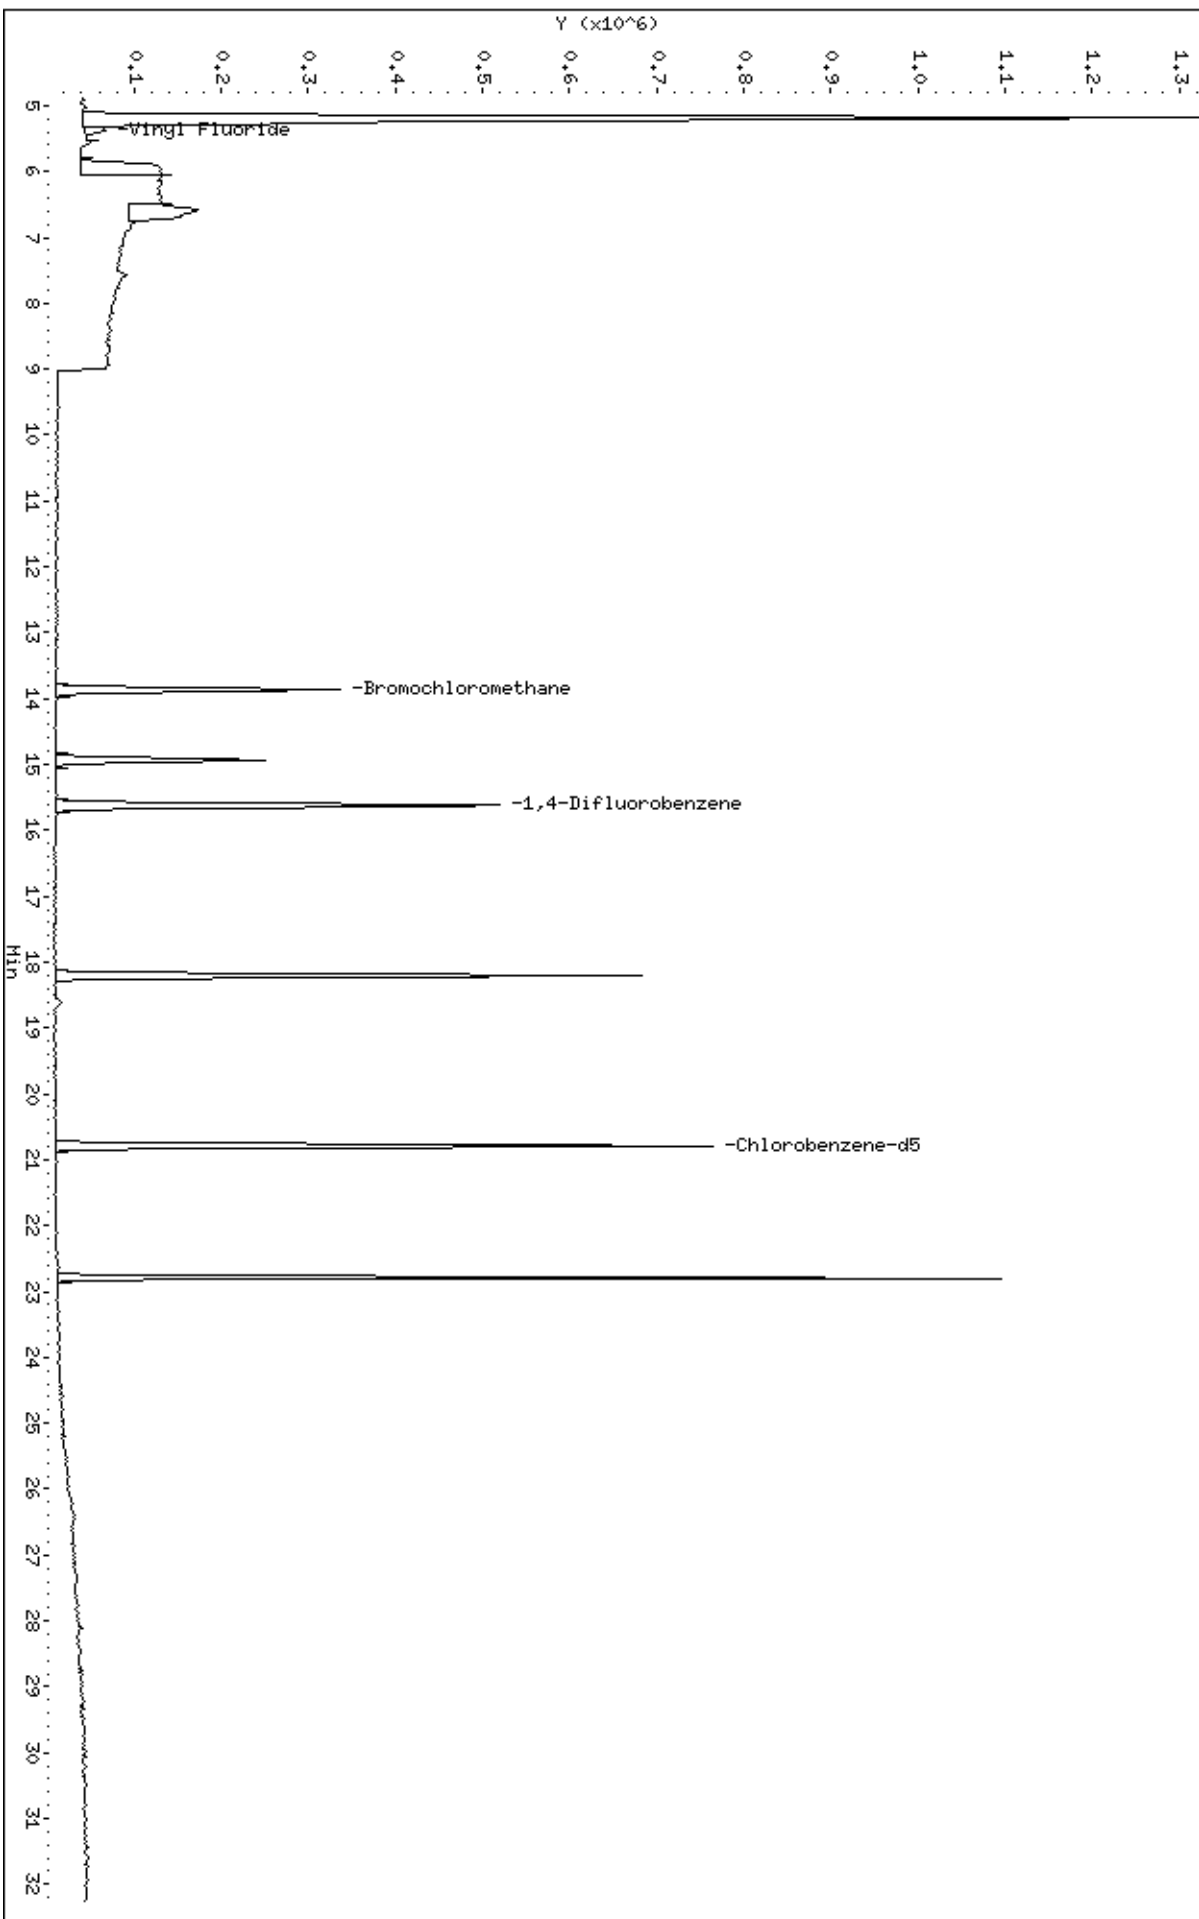

Report Date: 14-Dec-2007 15:21

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121312.d
 Lab Smp Id: ICAL Client Smp ID: Level 3
 Inj Date : 13-DEC-2007 23:51
 Operator : ab Inst ID: msdt.i
 Smp Info : 2.0mL #1443-378
 Misc Info : 200ppbv -> 2.0ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 15:00 ealcan Quant Type: ISTD
 Cal Date : 13-DEC-2007 23:51 Cal File: t121312.d
 Als bottle: 1 Calibration Sample, Level: 3
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	253123	25.0000		50.00- 150.00	100.00	
13.858	13.858	(1.000)	128	189889			26.73- 126.73	75.02	
13.858	13.858	(1.000)	49	271657			83.94- 183.94	107.32	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	995600	25.0000		50.00- 150.00	100.00	
15.628	15.628	(1.000)	88	160893			0.00- 65.84	16.16	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	905969	25.0000		50.00- 150.00	100.00	
20.798	20.798	(1.000)	82	502409			5.33- 105.33	55.46	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.937	14.936	(1.078)	65	393030	25.0000	24.387	50.00- 150.00	100.00	
14.937	14.936	(1.078)	67	191168			3.93- 103.93	48.64	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	938688	25.0000	24.854	50.00- 150.00	100.00	
18.199	18.199	(1.165)	70	104583			0.00- 61.06	11.14	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	645460			18.52- 118.52	68.76	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	629343	25.0000	25.328	50.00- 150.00	100.00	
22.789	22.789	(1.096)	95	759914			74.37- 174.37	120.75	
22.789	22.789	(1.096)	176	609315			47.63- 147.63	96.82	

11 Propylene									
						CAS #: 115-07-1			
5.812	5.812	(0.419)	41	14292	2.00000	2.114	50.00- 150.00	100.00	
5.812	5.812	(0.419)	42	9311			17.44- 117.44	65.15	
5.812	5.812	(0.419)	39	12206			31.05- 131.05	85.41	

12 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
5.923	5.923	(0.427)	85	87500	2.00000	1.974	50.00- 150.00	100.00	
5.923	5.923	(0.427)	87	30510			0.00- 82.50	34.87	

16 Freon 114									
						CAS #: 76-14-2			
6.310	6.282	(0.455)	135	51245	2.00000	1.768	50.00- 150.00	100.00	
6.310	6.282	(0.455)	137	15742			0.00- 81.78	30.72	

18 Chloromethane									
						CAS #: 74-87-3			
6.559	6.559	(0.473)	50	20594	2.00000	2.148	50.00- 150.00	100.00	
6.559	6.559	(0.473)	52	7143			0.00- 83.59	34.69	

20 Vinyl Chloride									
						CAS #: 75-01-4			
6.891	6.890	(0.497)	62	23216	2.00000	1.936	50.00- 150.00	100.00	
6.891	6.890	(0.497)	64	8115			0.00- 94.54	34.96	

22 1,3-Butadiene									
						CAS #: 106-99-0			
6.973	6.946	(0.503)	54	17368	2.00000	1.855	50.00- 150.00	100.00	
6.973	6.946	(0.503)	39	19080			61.08- 161.08	109.86	

25 Bromomethane									
						CAS #: 74-83-9			
7.914	7.913	(0.571)	94	23738	2.00000	1.869	50.00- 150.00	100.00	
7.914	7.913	(0.571)	96	22027			44.93- 144.93	92.80	

27 Chloroethane									
						CAS #: 75-00-3			
8.190	8.190	(0.591)	64	10813	2.00000	1.690	50.00- 150.00	100.00	
8.190	8.190	(0.591)	49	3122			0.00- 76.61	28.87	
8.190	8.190	(0.591)	66	4250			0.00- 85.87	39.31	

31 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
8.771	8.771	(0.633)	101	93986	2.00000	1.896	50.00- 150.00	100.00	
8.771	8.771	(0.633)	103	62888			15.72- 115.72	66.91	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
38 Ethanol						CAS #:	64-17-5			
9.241	9.241	(0.667)	45	5393	2.00000	1.605	50.00-	150.00	100.00(a)	
9.241	9.241	(0.667)	43	1469			0.00-	74.87	27.25	
9.241	9.241	(0.667)	46	2169			0.00-	88.05	40.23	

42 Freon 113						CAS #:	76-13-1			
9.960	9.959	(0.719)	151	42117	2.00000	1.888	50.00-	150.00	100.00	
9.960	9.959	(0.719)	153	27300			15.26-	115.26	64.82	
9.960	9.959	(0.719)	101	55911			81.18-	181.18	132.75	

43 1,1-Dichloroethene						CAS #:	75-35-4			
10.043	10.042	(0.725)	61	37725	2.00000	1.930	50.00-	150.00	100.00	
10.043	10.042	(0.725)	96	22076			16.16-	116.16	58.52	
10.043	10.042	(0.725)	98	13704			0.00-	91.50	36.33	

45 Acetone						CAS #:	67-64-1			
10.181	10.181	(0.735)	58	11856	2.00000	1.953	50.00-	150.00	100.00(a)	
10.181	10.181	(0.735)	43	38480			264.94-	364.94	324.54	

46 2-Propanol						CAS #:	67-63-0			
10.374	10.374	(0.749)	45	33322	2.00000	1.657	50.00-	150.00	100.00(a)	
10.402	10.374	(0.751)	43	13428			0.00-	78.96	40.30	
10.374	10.374	(0.749)	59	1250			0.00-	54.05	3.75	

47 Carbon Disulfide						CAS #:	75-15-0			
10.540	10.540	(0.761)	76	67773	2.00000	1.818	50.00-	150.00	100.00	

51 3-Chloropropene						CAS #:	107-05-1			
10.817	10.817	(0.781)	76	10481	2.00000	1.648	50.00-	150.00	100.00	
10.817	10.817	(0.781)	41	26558			176.05-	276.05	253.39	

54 Methylene Chloride						CAS #:	75-09-2			
11.093	11.093	(0.800)	49	24160	2.00000	1.957	50.00-	150.00	100.00	
11.093	11.093	(0.800)	84	20453			44.80-	144.80	84.66	
11.093	11.093	(0.800)	51	8522			0.00-	83.78	35.27	

60 MTBE						CAS #:	1634-04-4			
11.453	11.453	(0.826)	73	64385	2.00000	1.556	50.00-	150.00	100.00	
11.453	11.453	(0.826)	57	13318			0.00-	69.37	20.69	
11.453	11.453	(0.826)	41	15966			0.00-	70.94	24.80	

61 trans-1,2-Dichloroethene						CAS #:	156-60-5			
11.536	11.535	(0.832)	96	27711	2.00000	1.850	50.00-	150.00	100.00	
11.536	11.535	(0.832)	61	39510			84.61-	184.61	142.58	
11.536	11.535	(0.832)	98	18112			15.85-	115.85	65.36	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
65 Hexane						CAS #: 110-54-3			
11.895	11.895	(0.858)	57	34289	2.00000	1.649	50.00- 150.00	100.00	
11.895	11.895	(0.858)	43	21142			8.15- 108.15	61.66	
11.895	11.895	(0.858)	86	6159			0.00- 69.59	17.96	

69 Vinyl Acetate						CAS #: 108-05-4			
12.365	12.337	(0.892)	86	4210	2.00000	1.134	50.00- 150.00	100.00(a)	
12.365	12.337	(0.892)	43	50455			903.58-1003.58	1198.31	

70 1,1-Dichloroethane						CAS #: 75-34-3			
12.365	12.365	(0.892)	63	47366	2.00000	1.813	50.00- 150.00	100.00	
12.365	12.365	(0.892)	65	16860			0.00- 83.37	35.60	

75 2-Butanone						CAS #: 78-93-3			
13.388	13.388	(0.966)	72	9910	2.00000	1.433	50.00- 150.00	100.00	
13.388	13.388	(0.966)	43	36718			271.22- 371.22	370.49	
13.388	13.388	(0.966)	57	2780			0.00- 78.78	28.05	

76 cis-1,2-Dichloroethene						CAS #: 156-59-2			
13.416	13.416	(0.968)	61	35693	2.00000	1.945	50.00- 150.00	100.00	
13.416	13.416	(0.968)	96	27122			29.23- 129.23	75.99	
13.416	13.416	(0.968)	98	18038			0.16- 100.16	50.54	

80 Tetrahydrofuran						CAS #: 109-99-9			
13.858	13.858	(1.000)	42	19758	2.00000	1.793	50.00- 150.00	100.00	
13.858	13.858	(1.000)	71	9972			0.61- 100.61	50.47	
13.858	13.858	(1.000)	72	10244			8.31- 108.31	51.85	

82 Chloroform						CAS #: 67-66-3			
13.941	13.941	(1.006)	83	59813	2.00000	1.957	50.00- 150.00	100.00	
13.941	13.941	(1.006)	85	41889			18.46- 118.46	70.03	

83 1,1,1-Trichloroethane						CAS #: 71-55-6			
14.273	14.273	(1.030)	97	66107	2.00000	1.806	50.00- 150.00	100.00	
14.273	14.273	(1.030)	99	45667			13.89- 113.89	69.08	

85 Cyclohexane						CAS #: 110-82-7			
14.301	14.300	(1.032)	84	30567	2.00000	1.636	50.00- 150.00	100.00	
14.301	14.300	(1.032)	56	30213			43.75- 143.75	98.84	
14.301	14.300	(1.032)	41	16170			1.66- 101.66	52.90	

87 Carbon Tetrachloride						CAS #: 56-23-5			
14.549	14.522	(1.050)	119	68844	2.00000	1.931	50.00- 150.00	100.00	
14.522	14.522	(1.048)	117	69338			54.19- 154.19	100.72	

91 Benzene						CAS #: 71-43-2			
14.964	14.964	(0.958)	78	77851	2.00000	1.958	50.00- 150.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 Benzene (continued)									
14.964	14.964	(0.958)	77	17638			0.00- 73.32	22.66	

89 2,2,4-Trimethylpentane CAS #: 540-84-1									
14.881	14.881	(1.074)	57	84346	2.00000	1.619	50.00- 150.00	100.00	
14.881	14.881	(1.074)	56	29647			0.00- 83.27	35.15	
14.881	14.881	(1.074)	41	25447			0.00- 77.74	30.17	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.075	15.075	(0.965)	62	38382	2.00000	1.933	50.00- 150.00	100.00	
15.075	15.075	(0.965)	64	13114			0.00- 82.87	34.17	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	21228	2.00000	1.681	50.00- 150.00	100.00	
15.185	15.185	(0.972)	43	28158			77.61- 177.61	132.64	
15.185	15.185	(0.972)	57	17386			32.99- 132.99	81.90	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	33646	2.00000	1.832	50.00- 150.00	100.00	
16.070	16.070	(1.028)	130	32994			45.55- 145.55	98.06	
16.070	16.070	(1.028)	97	22399			15.22- 115.22	66.57	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.568	16.568	(1.060)	63	24213	2.00000	1.823	50.00- 150.00	100.00	
16.568	16.568	(1.060)	62	17688			23.00- 123.00	73.05	
16.568	16.568	(1.060)	41	14945			8.64- 108.64	61.73	

106 1,4-Dioxane CAS #: 123-91-1									
16.678	16.678	(1.067)	88	17684	2.00000	1.679	50.00- 150.00	100.00(a)	
16.706	16.678	(1.069)	58	10078			5.85- 105.85	56.99	
16.678	16.678	(1.067)	57	3752			0.00- 69.86	21.22	

107 Bromodichloromethane CAS #: 75-27-4									
16.983	16.982	(1.087)	83	59329	2.00000	1.857	50.00- 150.00	100.00	
16.983	16.982	(1.087)	85	40077			16.51- 116.51	67.55	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	35273	2.00000	1.649	50.00- 150.00	100.00	
17.784	17.784	(1.138)	77	11450			0.00- 83.76	32.46	
17.784	17.784	(1.138)	39	17935			0.00- 94.73	50.85	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.978	17.950	(1.150)	58	12890	2.00000	1.324	50.00- 150.00	100.00	
17.978	17.950	(1.150)	43	32252			168.02- 268.02	250.21	
17.978	17.950	(1.150)	85	6644			2.69- 102.69	51.54	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		

114 Toluene						CAS #:	108-88-3			
18.337	18.337	(1.173)	91	89987	2.00000	1.877	50.00-	150.00	100.00	
18.337	18.337	(1.173)	92	51337			9.70-	109.70	57.05	

116 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
18.752	18.752	(0.902)	75	42236	2.00000	1.723	50.00-	150.00	100.00	
18.752	18.752	(0.902)	77	12133			0.00-	82.23	28.73	
18.752	18.752	(0.902)	39	13953			0.00-	88.37	33.04	

117 1,1,2-Trichloroethane						CAS #:	79-00-5			
19.112	19.111	(0.919)	97	32136	2.00000	1.807	50.00-	150.00	100.00	
19.112	19.111	(0.919)	99	20573			15.96-	115.96	64.02	
19.112	19.111	(0.919)	83	26593			36.03-	136.03	82.75	

120 Tetrachloroethene						CAS #:	127-18-4			
19.277	19.277	(0.927)	166	47245	2.00000	1.906	50.00-	150.00	100.00	
19.277	19.277	(0.927)	129	32576			20.82-	120.82	68.95	
19.277	19.277	(0.927)	131	34590			18.42-	118.42	73.21	

121 2-Hexanone						CAS #:	591-78-6			
19.416	19.416	(0.934)	58	14617	2.00000	1.004	50.00-	150.00	100.00(a)	
19.416	19.416	(0.934)	43	28752			120.66-	220.66	196.70	
19.416	19.416	(0.934)	100	4246			0.00-	74.50	29.05	

122 Dibromochloromethane						CAS #:	124-48-1			
19.803	19.803	(0.952)	129	54602	2.00000	1.747	50.00-	150.00	100.00	
19.803	19.803	(0.952)	127	41416			25.33-	125.33	75.85	

123 1,2-Dibromoethane						CAS #:	106-93-4			
20.052	20.052	(0.964)	107	52542	2.00000	1.756	50.00-	150.00	100.00	
20.052	20.052	(0.964)	109	47342			41.12-	141.12	90.10	

127 Chlorobenzene						CAS #:	108-90-7			
20.854	20.853	(1.003)	112	83776	2.00000	1.940	50.00-	150.00	100.00	
20.854	20.853	(1.003)	114	26381			0.00-	80.99	31.49	
20.854	20.853	(1.003)	77	60726			25.73-	125.73	72.49	

128 Ethyl Benzene						CAS #:	100-41-4			
20.936	20.936	(1.007)	106	37020	2.00000	1.692	50.00-	150.00	100.00	
20.936	20.936	(1.007)	91	117271			266.56-	366.56	316.77	

129 m,p-Xylene						CAS #:	108-38-3			
21.130	21.130	(1.016)	106	43858	2.00000	1.630	50.00-	150.00	100.00	
21.130	21.130	(1.016)	91	92062			157.11-	257.11	209.91	

130 o-Xylene						CAS #:	95-47-6			
21.849	21.849	(1.051)	106	39199	2.00000	1.551	50.00-	150.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	85614			166.77- 266.77	218.40	

131 Styrene CAS #: 100-42-5									
21.877	21.876	(1.052)	104	58938	2.00000	1.439	50.00- 150.00	100.00	
21.877	21.876	(1.052)	78	33809			12.82- 112.82	57.36	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	54700	2.00000	1.678	50.00- 150.00	100.00	
22.291	22.291	(1.072)	171	28713			0.34- 100.34	52.49	

134 Cumene CAS #: 98-82-8									
22.430	22.429	(1.078)	105	118346	2.00000	1.638	50.00- 150.00	100.00	
22.430	22.429	(1.078)	120	30709			0.00- 74.52	25.95	
22.430	22.429	(1.078)	51	9444			51.79- 151.79	7.98	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	71287	2.00000	1.800	50.00- 150.00	100.00	
23.010	23.010	(1.106)	85	44544			17.66- 117.66	62.49	

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	145824	2.00000	1.596	50.00- 150.00	100.00	
23.121	23.121	(1.112)	120	31501			0.00- 71.52	21.60	
23.093	23.121	(1.110)	105	5527			0.00- 53.54	3.79	

145 4-Ethyltoluene CAS #: 622-96-8									
23.287	23.286	(1.120)	105	121403	2.00000	1.578	50.00- 150.00	100.00	
23.287	23.286	(1.120)	120	35104			0.00- 79.85	28.92	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	100989	2.00000	1.612	50.00- 150.00	100.00	
23.397	23.397	(1.125)	120	49919			0.29- 100.29	49.43	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	84615	2.00000	1.452	50.00- 150.00	100.00	
24.033	24.033	(1.156)	120	36189			0.00- 94.69	42.77	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	81310	2.00000	1.843	50.00- 150.00	100.00	
24.586	24.586	(1.182)	148	51498			14.61- 114.61	63.34	
24.586	24.586	(1.182)	111	33757			0.00- 92.01	41.52	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	82752	2.00000	1.805	50.00- 150.00	100.00	
24.724	24.724	(1.189)	148	49857			13.83- 113.83	60.25	
24.724	24.724	(1.189)	111	33486			0.00- 89.75	40.47	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

159	alpha-Chlorotoluene					CAS #: 100-44-7			
24.946	24.945	(1.199)	91	93144	2.00000	1.468	50.00- 150.00	100.00	
24.946	24.945	(1.199)	126	18635			0.00- 69.65	20.01	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
25.360	25.360	(1.219)	146	73842	2.00000	1.746	50.00- 150.00	100.00	
25.360	25.360	(1.219)	148	48650			14.36- 114.36	65.88	
25.360	25.360	(1.219)	111	32099			0.00- 92.81	43.47	

165	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
28.153	28.153	(1.354)	180	37460	2.00000	1.291	50.00- 150.00	100.00(a)	
28.153	28.153	(1.354)	182	35834			45.41- 145.41	95.66	

166	Hexachlorobutadiene					CAS #: 87-68-3			
28.319	28.319	(1.362)	225	42757	2.00000	1.614	50.00- 150.00	100.00(a)	
28.319	28.319	(1.362)	223	28345			13.46- 113.46	66.29	

19	Butane					CAS #: 106-97-8			
6.808	6.780	(0.491)	58	4252	2.00000	1.731	50.00- 150.00	100.00(a)	
6.808	6.780	(0.491)	43	34824			640.46- 740.46	819.00	

29	Isopentane					CAS #: 78-78-4			
8.273	8.273	(0.597)	43	26227	2.00000	1.896	50.00- 150.00	100.00(a)	
8.273	8.273	(0.597)	57	19023			26.79- 126.79	72.53	

102	Methyl Cyclohexane					CAS #: 108-87-2			
16.347	16.346	(1.180)	83	37101	2.00000	1.566	50.00- 150.00	100.00	
16.347	16.346	(1.180)	98	18806			0.00- 95.49	50.69	
16.347	16.346	(1.180)	55	25754			16.76- 116.76	69.42	

167	Naphthalene					CAS #: 91-20-3			
28.678	28.678	(1.379)	128	53924	2.00000	1.127	50.00- 150.00	100.00(a)	
28.678	28.678	(1.379)	127	7316			0.00- 62.56	13.57	

QC Flag Legend

a - Target compound detected but, quantitated amount
 Below Limit Of Quantitation(BLOQ).

Report Date: 14-Dec-2007 15:21

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121312.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	253123	-9.84
97 1,4-Difluorobenze	1182601	709561	1655641	995600	-15.81
126 Chlorobenzene-d5	1033655	620193	1447117	905969	-12.35

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/13Dec2007,b/t121312.d

Date: 13-DEC-2007 23:51

Client ID: Level 3

Sample Info: 2.0mL #1443-378


Column phase: RTX-624

Instrument: msdt,i

Operator: ab

Column diameter: 0.53

/chem/msdt,i/13Dec2007,b/t121312.d

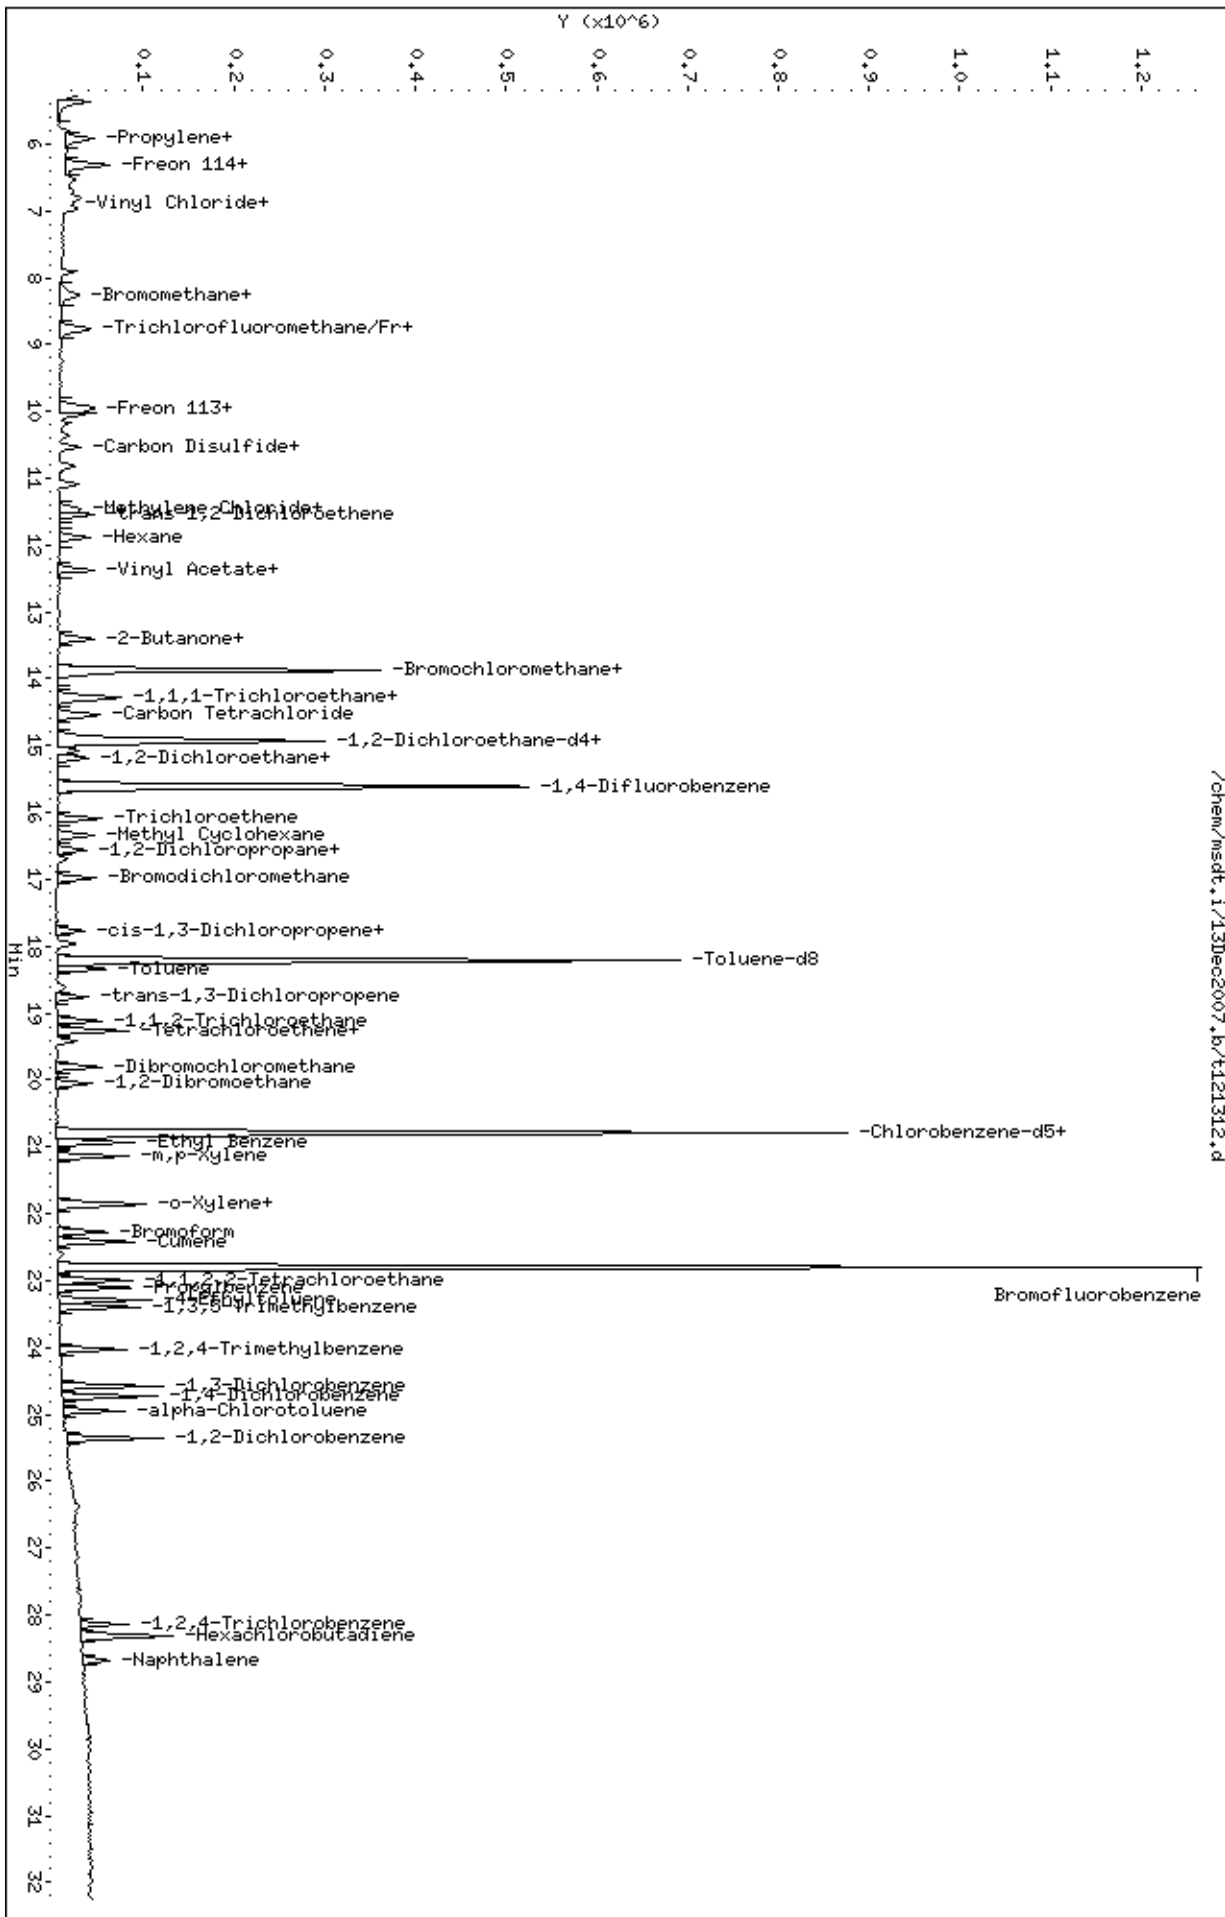

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/16Jan2008.b/t011604.d
 Lab Smp Id: TVH ICAL Client Smp ID: Level 4
 Inj Date : 16-JAN-2008 10:18
 Operator : lo Inst ID: msdt.i
 Smp Info : 25ml #1443-403
 Misc Info : 200ppbv -> 25ppbv
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/t14q1213d.m
 Meth Date : 16-Jan-2008 14:59 lover Quant Type: ISTD
 Cal Date : 16-JAN-2008 10:18 Cal File: t011604.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5d.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	354443	25.0000		50.00- 150.00	100.00	
13.858	13.858	(1.000)	128	278113			27.05- 127.05	78.46	
13.858	13.858	(1.000)	49	388700			61.34- 161.34	109.67	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1290708	25.0000		50.00- 150.00	100.00	
15.628	15.628	(1.000)	88	201235			0.00- 65.73	15.59	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1277501	25.0000		50.00- 150.00	100.00	
20.798	20.798	(1.000)	82	709977			5.94- 105.94	55.58	

204 Propane CAS #: 74-98-6									
5.785	5.785	(0.417)	43	115006	25.0000	26.963	50.00- 150.00	100.00	
5.785	5.785	(0.417)	44	147259			107.53- 207.53	128.04	

37 Pentane CAS #: 109-66-0									
8.909	8.909	(0.643)	43	893995	25.0000	28.731	50.00- 150.00	100.00	
8.909	8.909	(0.643)	57	158200			0.00- 67.03	17.70	

AMOUNTS

RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
37 Pentane (continued)								
8.909	8.909	(0.643)	72	118079			0.00- 62.09	13.21

112 Octane								
						CAS #: 111-65-9		
18.282	18.282	(1.170)	57	488691	25.0000	26.543	50.00- 150.00	100.00
18.282	18.282	(1.170)	85	661526			82.32- 182.32	135.37
18.282	18.282	(1.170)	43	1051925			166.39- 266.39	215.25

124 Nonane								
						CAS #: 111-84-2		
20.964	20.964	(1.008)	43	1089052	25.0000	26.536	50.00- 150.00	100.00
20.964	20.964	(1.008)	57	1134408			52.38- 152.38	104.16
20.964	20.964	(1.008)	85	508808			0.00- 95.58	46.72

139 Decane								
						CAS #: 124-18-5		
23.204	23.204	(1.116)	57	1332064	25.0000	27.023	50.00- 150.00	100.00
23.204	23.204	(1.116)	71	588024			0.00- 93.78	44.14
23.204	23.204	(1.116)	142	65676			0.00- 54.94	4.93

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 16-JAN-2008

Lab File ID: t011604.d

Calibration Time: 13:44

Lab Smp Id: TVH ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lo

Method File: /chem/msdt.i/16Jan2008.b/t14q1213d.m

Misc Info: 200ppbv -> 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	325810	195486	456134	354443	8.79
97 1,4-Difluorobenze	1168077	700846	1635308	1290708	10.50
126 Chlorobenzene-d5	1103278	661967	1544589	1277501	15.79

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.86	-0.20
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/16Jan2008,b/t011604.d

Date : 16-Jan-2008 10:18

Client ID: Level 4


Sample Info: 25ml #1443-403

Column phase: RTX-624

Instrument: msdt,i

Operator: lo

Column diameter: 0.53

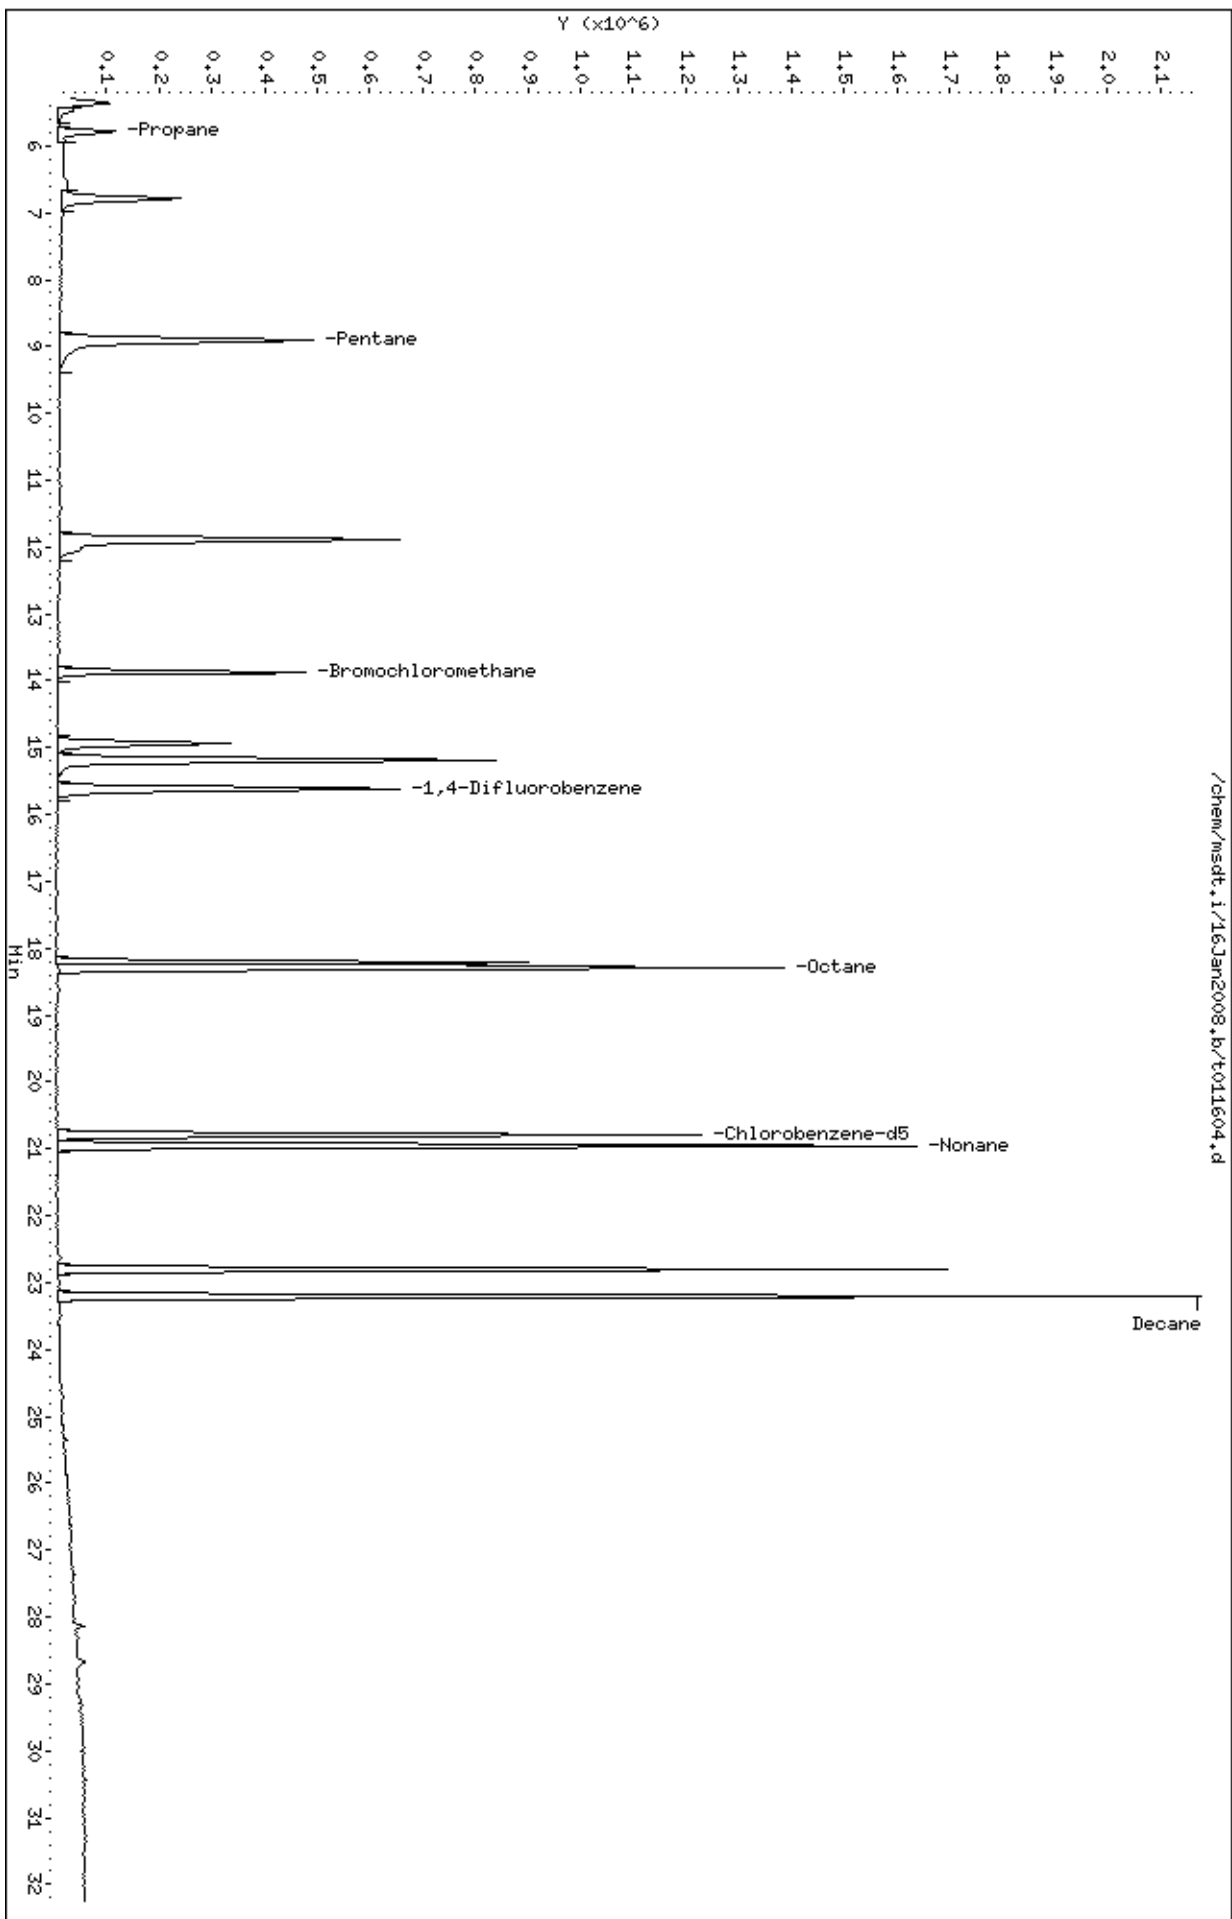

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/02Jan2008.b/t010203.d
 Lab Smp Id: ICAL Client Smp ID: Level 4
 Inj Date : 02-JAN-2008 11:18
 Operator : sjr Inst ID: msdt.i
 Smp Info : 8.0ml #1443-399
 Misc Info : 200ppbv -> 8.0ppbv (48ppbv MeOH)
 Comment :
 Method : /chem/msdt.i/02Jan2008.b/t14q1213c.m
 Meth Date : 02-Jan-2008 15:47 sruth Quant Type: ISTD
 Cal Date : 02-JAN-2008 11:18 Cal File: t010203.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp22c.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.865	13.865	(1.000)	130	341024	25.0000		50.00- 150.00	100.00	
13.865	13.865	(1.000)	128	271284			26.86- 126.86	79.55	
13.865	13.865	(1.000)	49	404499			74.17- 174.17	118.61	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.635	15.635	(1.000)	114	1262666	25.0000		50.00- 150.00	100.00	
15.635	15.635	(1.000)	88	203375			0.00- 66.07	16.11	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.805	20.805	(1.000)	117	1287536	25.0000		50.00- 150.00	100.00	
20.805	20.805	(1.000)	82	739635			5.77- 105.77	57.45	

6 Freon142b CAS #: 75-68-3									
6.408	6.408	(0.462)	65	328382	8.00000	7.452	50.00- 150.00	100.00	
6.408	6.408	(0.462)	45	70365			0.00- 71.17	21.43	

9 Freon 13 CAS #: 75-72-9									
5.394	5.394	(0.389)	69	335762	8.00000	7.764	50.00- 150.00	100.00(H)	
5.394	5.394	(0.389)	85	116750			0.00- 83.23	34.77	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
9 Freon 13 (continued)									
5.394	5.394	(0.389)	87	37057			0.00- 60.80	11.04	

13 Freon 134a CAS #: 811-97-2									
5.675	5.675	(0.409)	83	144504	8.00000	7.416	50.00- 150.00	100.00	
5.675	5.675	(0.409)	69	113113			29.59- 129.59	78.28	

15 Freon 152a CAS #: 75-37-6									
5.844	5.844	(0.422)	65	72322	8.00000	6.969	50.00- 150.00	100.00	
5.844	5.844	(0.422)	51	129634			125.61- 225.61	179.25	
5.844	5.844	(0.422)	47	32766			0.00- 95.62	45.31	

17 Freon 22 CAS #: 75-45-6									
5.985	5.985	(0.432)	67	40777	8.00000	7.647	50.00- 150.00	100.00	
5.985	5.985	(0.432)	51	185475			424.04- 524.04	454.85	
5.985	5.985	(0.432)	85	4437			0.00- 60.14	10.88	

26 Methanol CAS #: 67-56-1									
7.534	7.534	(0.543)	31	180633	48.0000	40.949	50.00- 150.00	100.00(a)	
7.534	7.534	(0.543)	32	289814			127.28- 227.28	160.44	

34 Dichlorofluoromethane/Fr21 CAS #: 75-43-4									
8.717	8.717	(0.629)	67	256068	8.00000	7.494	50.00- 150.00	100.00	
8.717	8.717	(0.629)	69	85184			0.00- 82.55	33.27	
8.717	8.717	(0.629)	35	14499			0.00- 55.68	5.66	

40 Freon123a CAS #: 354-23-4									
9.580	9.580	(0.691)	67	194248	8.00000	7.350	50.00- 150.00	100.00	
9.580	9.580	(0.691)	117	168537			33.27- 133.27	86.76	

41 Freon123 CAS #: 306-83-2									
9.718	9.718	(0.701)	83	273315	8.00000	7.531	50.00- 150.00	100.00	
9.718	9.718	(0.701)	133	66894			0.00- 72.56	24.48	
9.718	9.718	(0.701)	85	192964			21.04- 121.04	70.60	

57 tert-Butyl-Alcohol CAS #: 75-65-0									
11.156	11.156	(0.805)	59	213357	8.00000	6.560	50.00- 150.00	100.00	
11.156	11.156	(0.805)	41	53502			0.00- 79.32	25.08	
11.156	11.156	(0.805)	57	24564			0.00- 60.92	11.51	

68 Isopropyl ether CAS #: 108-20-3									
12.289	12.289	(0.886)	45	340212	8.00000	6.931	50.00- 150.00	100.00	
12.289	12.289	(0.886)	87	103397			0.00- 81.01	30.39	
12.289	12.289	(0.886)	59	42496			0.00- 61.81	12.49	

71 1-Propanol CAS #: 71-23-8									
12.400	12.400	(0.894)	42	21254	8.00000	6.595	50.00- 150.00	100.00	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	====	=====	=====	=====	=====	=====		
71 1-Propanol (continued)										
12.400	12.400	(0.894)	59	25946			61.64- 161.64	122.08		
12.400	12.400	(0.894)	41	19680			40.91- 140.91	92.59		

73 t-Butylethyl Ether										
						CAS #: 637-92-3				
12.925	12.925	(0.932)	59	379964	8.00000	7.088	50.00- 150.00	100.00		
12.925	12.925	(0.932)	87	162993			0.00- 93.11	42.90		
12.925	12.925	(0.932)	41	78140			0.00- 70.41	20.57		

77 Ethyl Acetate										
						CAS #: 141-78-6				
13.395	13.395	(0.966)	45	40012	8.00000	7.200	50.00- 150.00	100.00		
13.395	13.395	(0.966)	61	40641			49.68- 149.68	101.57		
13.395	13.395	(0.966)	43	261880			615.05- 715.05	654.50		

92 tert-amyl-Methyl Ether										
						CAS #: 994-05-8				
14.999	14.999	(1.082)	73	338197	8.00000	6.914	50.00- 150.00	100.00		
14.999	14.999	(1.082)	87	78081			0.00- 74.91	23.09		
14.999	14.999	(1.082)	55	87128			0.00- 76.64	25.76		

96 2-Heptanone										
						CAS #: 110-43-0				
21.967	21.967	(1.584)	58	170115	8.00000	6.192	50.00- 150.00	100.00		
21.967	21.967	(1.584)	43	257136			98.27- 198.27	151.15		

98 1-Butanol										
						CAS #: 71-36-3				
15.801	15.801	(1.011)	56	55993	8.00000	5.928	50.00- 150.00	100.00		
15.801	15.801	(1.011)	41	41768			28.59- 128.59	74.60		
15.801	15.801	(1.011)	43	31471			6.69- 106.69	56.21		

119 Butyl Acetate										
						CAS #: 123-86-4				
19.533	19.533	(1.249)	56	113668	8.00000	6.389	50.00- 150.00	100.00		
19.533	19.533	(1.249)	73	46398			0.00- 95.25	40.82		
19.533	19.533	(1.249)	43	257446			169.61- 269.61	226.49		

135 Cyclohexanone										
						CAS #: 108-94-1				
22.741	22.741	(1.093)	55	136978	8.00000	6.384	50.00- 150.00	100.00		
22.741	22.741	(1.093)	98	70849			2.09- 102.09	51.72		
22.741	22.741	(1.093)	42	91502			15.79- 115.79	66.80		

146 Diisobutyl Ketone										
						CAS #: 108-83-8				
23.570	23.570	(1.133)	57	335486	8.00000	6.458	50.00- 150.00	100.00		
23.570	23.570	(1.133)	85	326099			46.68- 146.68	97.20		
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00		

QC Flag Legend

- a - Target compound detected but, quantitated amount
Below Limit Of Quantitation(BLOQ).
- H - Operator selected an alternate compound hit.

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 02-JAN-2008

Lab File ID: t010203.d

Calibration Time: 12:02

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/02Jan2008.b/t14q1213c.m

Misc Info: 200ppbv -> 8.0ppbv (48ppbv MeOH)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	338913	203348	474478	341024	0.62
97 1,4-Difluorobenze	1251078	750647	1751509	1262666	0.93
126 Chlorobenzene-d5	1269166	761500	1776832	1287536	1.45

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/02Jan2008,b/t010203.d

Date : 02-JAN-2008 11:18

Client ID: Level 4


Sample Info: 8.0ml #1443-399

Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

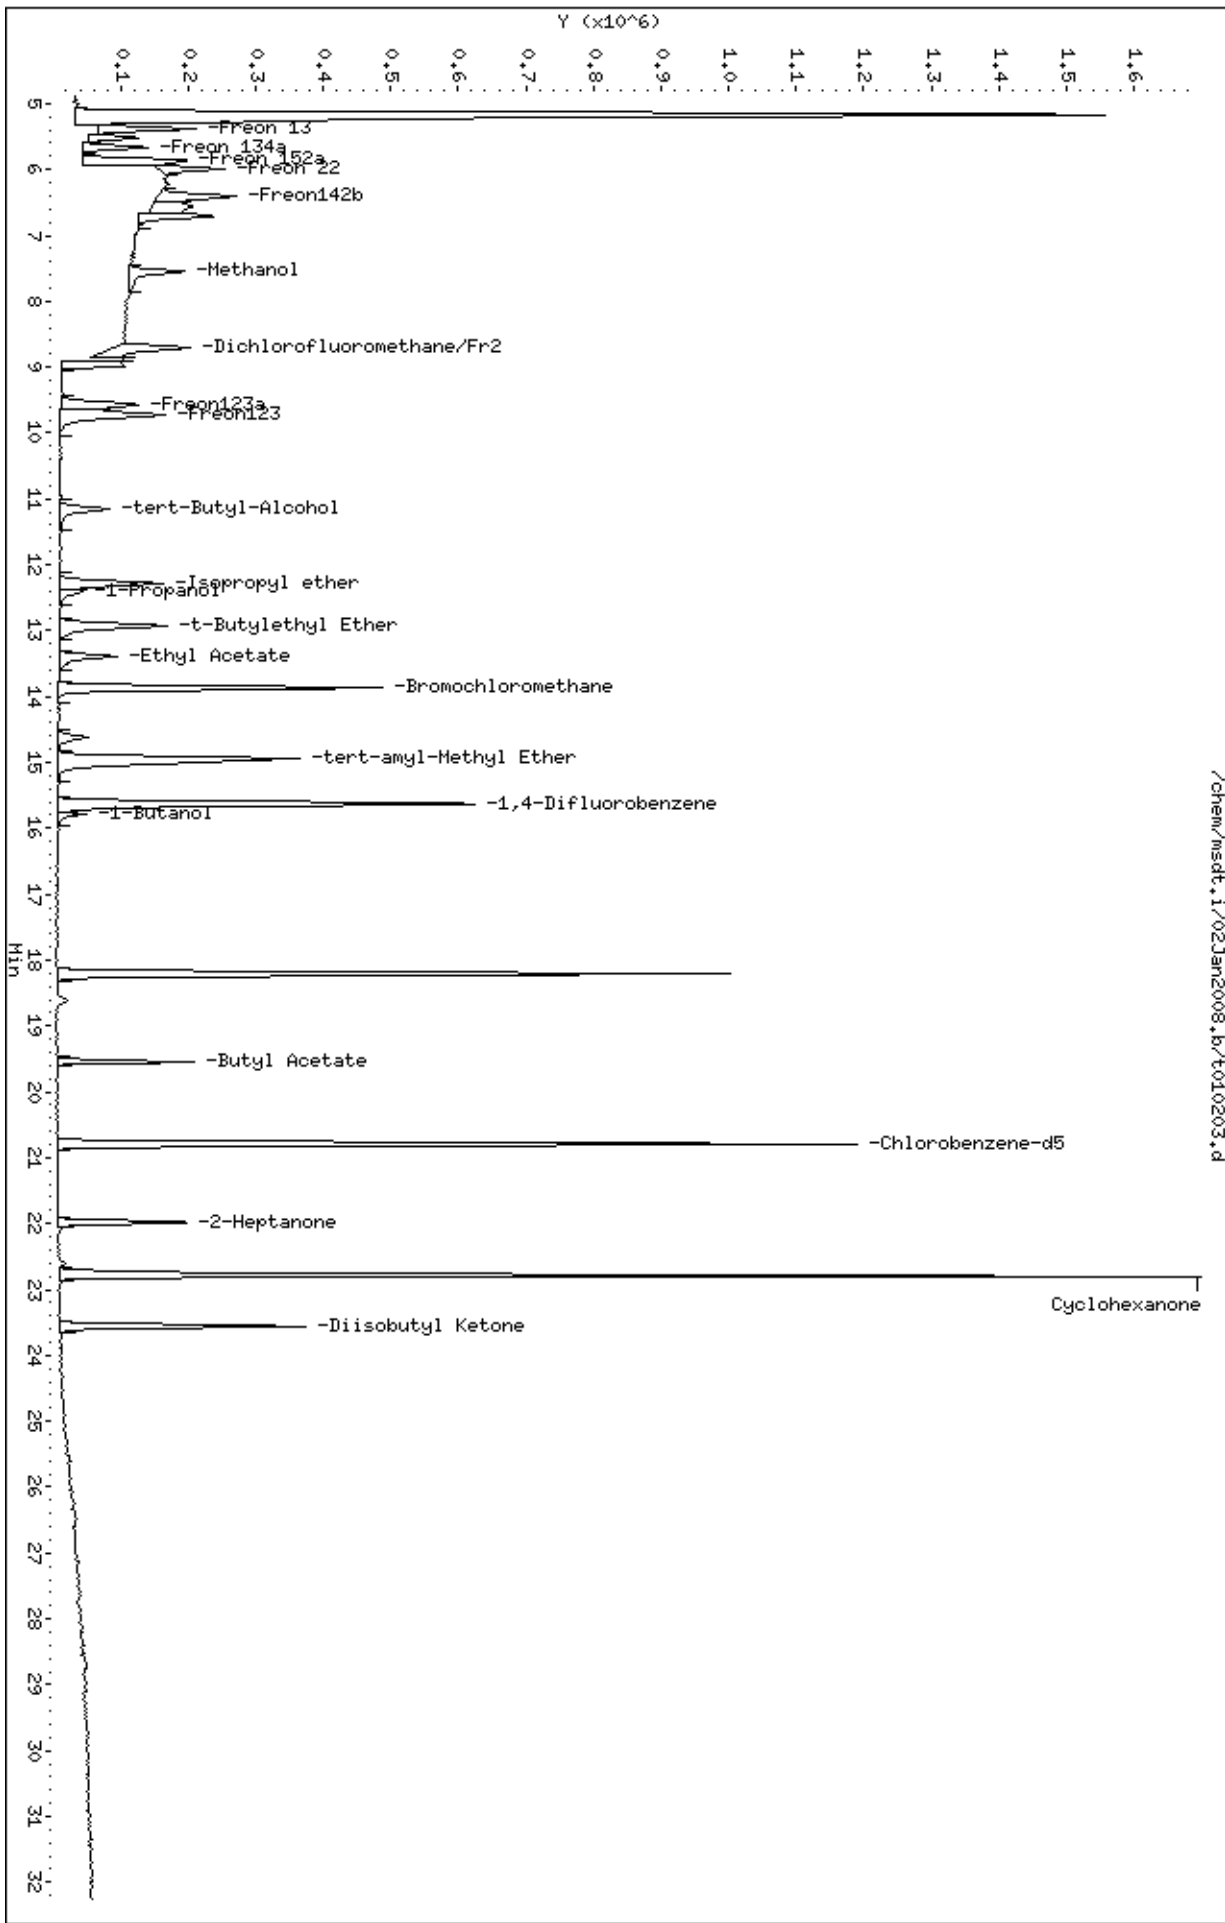

Report Date: 14-Dec-2007 10:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121313.d
 Lab Smp Id: ICAL Client Smp ID: Level 4
 Inj Date : 14-DEC-2007 00:40
 Operator : ab Inst ID: msdt.i
 Smp Info : 25mL #1443-378
 Misc Info : 200ppbv -> 25ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 10:41 ealcan Quant Type: ISTD
 Cal Date : 14-DEC-2007 00:40 Cal File: t121313.d
 Als bottle: 1 Calibration Sample, Level: 4
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	259446	25.0000			50.00- 150.00	100.00
13.858	13.858	(1.000)	128	199212				26.73- 126.73	76.78
13.858	13.858	(1.000)	49	354443				83.94- 183.94	136.62

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1118582	25.0000			50.00- 150.00	100.00
15.628	15.628	(1.000)	88	170822				0.00- 65.84	15.27

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	965763	25.0000			50.00- 150.00	100.00
20.798	20.798	(1.000)	82	541824				5.33- 105.33	56.10

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.078)	65	429347	25.0000	25.992		50.00- 150.00	100.00
14.936	14.936	(1.078)	67	234126				3.93- 103.93	54.53

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1051366	25.0000	24.777		50.00- 150.00	100.00
18.199	18.199	(1.165)	70	118669				0.00- 61.06	11.29

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	723574			18.52- 118.52	68.82	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	660127	25.0000	24.922	50.00- 150.00	100.00	
22.789	22.789	(1.096)	95	818482			74.37- 174.37	123.99	
22.789	22.789	(1.096)	176	647788			47.63- 147.63	98.13	

11 Propylene									
						CAS #: 115-07-1			
5.812	5.812	(0.419)	41	186294	25.0000	26.886	50.00- 150.00	100.00	
5.812	5.812	(0.419)	42	120745			17.44- 117.44	64.81	
5.812	5.812	(0.419)	39	142255			31.05- 131.05	76.36	

12 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
5.923	5.923	(0.427)	85	1257853	25.0000	27.681	50.00- 150.00	100.00	
5.923	5.923	(0.427)	87	403784			0.00- 82.50	32.10	

16 Freon 114									
						CAS #: 76-14-2			
6.310	6.310	(0.455)	135	840521	25.0000	28.294	50.00- 150.00	100.00	
6.310	6.310	(0.455)	137	264736			0.00- 81.78	31.50	

18 Chloromethane									
						CAS #: 74-87-3			
6.559	6.559	(0.473)	50	250634	25.0000	25.499	50.00- 150.00	100.00	
6.559	6.559	(0.473)	52	84268			0.00- 83.59	33.62	

20 Vinyl Chloride									
						CAS #: 75-01-4			
6.890	6.890	(0.497)	62	339598	25.0000	27.624	50.00- 150.00	100.00	
6.890	6.890	(0.497)	64	112478			0.00- 94.54	33.12	

22 1,3-Butadiene									
						CAS #: 106-99-0			
6.973	6.973	(0.503)	54	269708	25.0000	28.104	50.00- 150.00	100.00	
6.973	6.973	(0.503)	39	258065			61.08- 161.08	95.68	

25 Bromomethane									
						CAS #: 74-83-9			
7.913	7.913	(0.571)	94	340883	25.0000	26.183	50.00- 150.00	100.00	
7.913	7.913	(0.571)	96	321255			44.93- 144.93	94.24	

27 Chloroethane									
						CAS #: 75-00-3			
8.190	8.190	(0.591)	64	186657	25.0000	28.454	50.00- 150.00	100.00	
8.190	8.190	(0.591)	49	50575			0.00- 76.61	27.10	
8.190	8.190	(0.591)	66	62344			0.00- 85.87	33.40	

31 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
8.771	8.771	(0.633)	101	1444693	25.0000	28.441	50.00- 150.00	100.00	
8.798	8.798	(0.635)	103	942573			15.72- 115.72	65.24	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Ethanol						CAS #: 64-17-5			
9.241	9.241	(0.667)	45	90458	25.0000	26.257	50.00- 150.00	100.00	
9.241	9.241	(0.667)	43	22819			0.00- 74.87	25.23	
9.241	9.241	(0.667)	46	35587			0.00- 88.05	39.34	

42 Freon 113						CAS #: 76-13-1			
9.959	9.959	(0.719)	151	609957	25.0000	26.681	50.00- 150.00	100.00	
9.959	9.959	(0.719)	153	388227			15.26- 115.26	63.65	
9.959	9.959	(0.719)	101	789206			81.18- 181.18	129.39	

43 1,1-Dichloroethene						CAS #: 75-35-4			
10.042	10.042	(0.725)	61	558324	25.0000	27.863	50.00- 150.00	100.00	
10.042	10.042	(0.725)	96	331435			16.16- 116.16	59.36	
10.042	10.042	(0.725)	98	218916			0.00- 91.50	39.21	

45 Acetone						CAS #: 67-64-1			
10.181	10.181	(0.735)	58	161269	25.0000	25.921	50.00- 150.00	100.00	
10.181	10.181	(0.735)	43	523182			264.94- 364.94	324.42	

46 2-Propanol						CAS #: 67-63-0			
10.374	10.374	(0.749)	45	557802	25.0000	27.065	50.00- 150.00	100.00	
10.374	10.374	(0.749)	43	151241			0.00- 78.96	27.11	
10.374	10.374	(0.749)	59	21376			0.00- 54.05	3.83	

47 Carbon Disulfide						CAS #: 75-15-0			
10.540	10.540	(0.761)	76	1023000	25.0000	26.777	50.00- 150.00	100.00	

51 3-Chloropropene						CAS #: 107-05-1			
10.817	10.817	(0.781)	76	164343	25.0000	25.204	50.00- 150.00	100.00	
10.817	10.817	(0.781)	41	374175			176.05- 276.05	227.68	

54 Methylene Chloride						CAS #: 75-09-2			
11.093	11.093	(0.800)	49	333301	25.0000	26.340	50.00- 150.00	100.00	
11.121	11.121	(0.802)	84	301227			44.80- 144.80	90.38	
11.093	11.093	(0.800)	51	100571			0.00- 83.78	30.17	

60 MTBE						CAS #: 1634-04-4			
11.453	11.453	(0.826)	73	1219558	25.0000	28.754	50.00- 150.00	100.00	
11.453	11.453	(0.826)	57	231992			0.00- 69.37	19.02	
11.453	11.453	(0.826)	41	235047			0.00- 70.94	19.27	

61 trans-1,2-Dichloroethene						CAS #: 156-60-5			
11.563	11.563	(0.834)	96	414431	25.0000	26.993	50.00- 150.00	100.00	
11.535	11.535	(0.832)	61	585305			84.61- 184.61	141.23	
11.563	11.563	(0.834)	98	264190			15.85- 115.85	63.75	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
65 Hexane						CAS #: 110-54-3			
11.895	11.895	(0.858)	57	604445	25.0000	28.356	50.00- 150.00	100.00	
11.895	11.895	(0.858)	43	360648			8.15- 108.15	59.67	
11.895	11.895	(0.858)	86	111423			0.00- 69.59	18.43	

69 Vinyl Acetate						CAS #: 108-05-4			
12.365	12.365	(0.892)	86	102274	25.0000	26.887	50.00- 150.00	100.00	
12.365	12.365	(0.892)	43	915962			903.58-1003.58	895.60	

70 1,1-Dichloroethane						CAS #: 75-34-3			
12.365	12.365	(0.892)	63	752830	25.0000	28.114	50.00- 150.00	100.00	
12.365	12.365	(0.892)	65	250044			0.00- 83.37	33.21	

75 2-Butanone						CAS #: 78-93-3			
13.388	13.388	(0.966)	72	202976	25.0000	28.636	50.00- 150.00	100.00	
13.388	13.388	(0.966)	43	668188			271.22- 371.22	329.20	
13.388	13.388	(0.966)	57	61553			0.00- 78.78	30.33	

76 cis-1,2-Dichloroethene						CAS #: 156-59-2			
13.416	13.416	(0.968)	61	526682	25.0000	28.006	50.00- 150.00	100.00	
13.416	13.416	(0.968)	96	418137			29.23- 129.23	79.39	
13.416	13.416	(0.968)	98	270287			0.16- 100.16	51.32	

80 Tetrahydrofuran						CAS #: 109-99-9			
13.858	13.858	(1.000)	42	335559	25.0000	29.708	50.00- 150.00	100.00	
13.858	13.858	(1.000)	71	172932			0.61- 100.61	51.54	
13.858	13.858	(1.000)	72	189306			8.31- 108.31	56.42	

82 Chloroform						CAS #: 67-66-3			
13.941	13.941	(1.006)	83	964655	25.0000	30.787	50.00- 150.00	100.00	
13.941	13.941	(1.006)	85	628295			18.46- 118.46	65.13	

83 1,1,1-Trichloroethane						CAS #: 71-55-6			
14.273	14.273	(1.030)	97	1074336	25.0000	28.632	50.00- 150.00	100.00	
14.273	14.273	(1.030)	99	705682			13.89- 113.89	65.69	

85 Cyclohexane						CAS #: 110-82-7			
14.300	14.300	(1.032)	84	544905	25.0000	28.455	50.00- 150.00	100.00	
14.300	14.300	(1.032)	56	526173			43.75- 143.75	96.56	
14.300	14.300	(1.032)	41	279845			1.66- 101.66	51.36	

87 Carbon Tetrachloride						CAS #: 56-23-5			
14.549	14.549	(1.050)	119	1067846	25.0000	29.218	50.00- 150.00	100.00	
14.549	14.549	(1.050)	117	1131591			54.19- 154.19	105.97	

91 Benzene						CAS #: 71-43-2			
14.964	14.964	(0.958)	78	1244709	25.0000	27.870	50.00- 150.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 Benzene (continued)									
14.964	14.964	(0.958)	77	283061			0.00- 73.32	22.74	

89 2,2,4-Trimethylpentane CAS #: 540-84-1									
14.881	14.881	(1.074)	57	1595612	25.0000	29.880	50.00- 150.00	100.00	
14.881	14.881	(1.074)	56	531006			0.00- 83.27	33.28	
14.881	14.881	(1.074)	41	418578			0.00- 77.74	26.23	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.075	15.075	(0.965)	62	618232	25.0000	27.713	50.00- 150.00	100.00	
15.075	15.075	(0.965)	64	201769			0.00- 82.87	32.64	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	397338	25.0000	28.007	50.00- 150.00	100.00	
15.185	15.185	(0.972)	43	526730			77.61- 177.61	132.56	
15.185	15.185	(0.972)	57	318773			32.99- 132.99	80.23	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	576180	25.0000	27.920	50.00- 150.00	100.00	
16.098	16.098	(1.030)	130	544641			45.55- 145.55	94.53	
16.070	16.070	(1.028)	97	367300			15.22- 115.22	63.75	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.568	16.568	(1.060)	63	414149	25.0000	27.750	50.00- 150.00	100.00	
16.568	16.568	(1.060)	62	295902			23.00- 123.00	71.45	
16.568	16.568	(1.060)	41	228890			8.64- 108.64	55.27	

106 1,4-Dioxane CAS #: 123-91-1									
16.706	16.706	(1.069)	88	286469	25.0000	24.204	50.00- 150.00	100.00	
16.678	16.678	(1.067)	58	164984			5.85- 105.85	57.59	
16.678	16.678	(1.067)	57	59526			0.00- 69.86	20.78	

107 Bromodichloromethane CAS #: 75-27-4									
16.982	16.982	(1.087)	83	1001845	25.0000	27.910	50.00- 150.00	100.00	
16.982	16.982	(1.087)	85	648554			16.51- 116.51	64.74	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	672636	25.0000	27.984	50.00- 150.00	100.00	
17.784	17.784	(1.138)	77	217801			0.00- 83.76	32.38	
17.784	17.784	(1.138)	39	287212			0.00- 94.73	42.70	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.978	17.978	(1.150)	58	306334	25.0000	28.011	50.00- 150.00	100.00	
17.978	17.978	(1.150)	43	691978			168.02- 268.02	225.89	
17.978	17.978	(1.150)	85	164591			2.69- 102.69	53.73	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	1463921	25.0000	27.173	50.00- 150.00	100.00	
18.337	18.337	(1.173)	92	887473			9.70- 109.70	60.62	

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	748647	25.0000	28.644	50.00- 150.00	100.00	
18.752	18.752	(0.902)	77	239049			0.00- 82.23	31.93	
18.752	18.752	(0.902)	39	292488			0.00- 88.37	39.07	

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.111	(0.919)	97	560236	25.0000	29.552	50.00- 150.00	100.00	
19.111	19.111	(0.919)	99	345266			15.96- 115.96	61.63	
19.111	19.111	(0.919)	83	458453			36.03- 136.03	81.83	

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	766575	25.0000	29.013	50.00- 150.00	100.00	
19.277	19.277	(0.927)	129	552392			20.82- 120.82	72.06	
19.277	19.277	(0.927)	131	524021			18.42- 118.42	68.36	

121 2-Hexanone						CAS #: 591-78-6			
19.416	19.416	(0.934)	58	417787	25.0000	26.919	50.00- 150.00	100.00	
19.416	19.416	(0.934)	43	676979			120.66- 220.66	162.04	
19.416	19.416	(0.934)	100	94866			0.00- 74.50	22.71	

122 Dibromochloromethane						CAS #: 124-48-1			
19.803	19.803	(0.952)	129	986119	25.0000	29.592	50.00- 150.00	100.00	
19.803	19.803	(0.952)	127	762924			25.33- 125.33	77.37	

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.051	20.051	(0.964)	107	908821	25.0000	28.495	50.00- 150.00	100.00	
20.051	20.051	(0.964)	109	856430			41.12- 141.12	94.24	

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.853	(1.003)	112	1300699	25.0000	28.249	50.00- 150.00	100.00	
20.853	20.853	(1.003)	114	417951			0.00- 80.99	32.13	
20.853	20.853	(1.003)	77	766059			25.73- 125.73	58.90	

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	674031	25.0000	28.904	50.00- 150.00	100.00	
20.936	20.936	(1.007)	91	2119576			266.56- 366.56	314.46	

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	847060	25.0000	29.531	50.00- 150.00	100.00	
21.130	21.130	(1.016)	91	1673192			157.11- 257.11	197.53	

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	796134	25.0000	29.548	50.00- 150.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	1653816			166.77- 266.77	207.73	

131 Styrene CAS #: 100-42-5									
21.876	21.876	(1.052)	104	1286469	25.0000	29.464	50.00- 150.00	100.00	
21.876	21.876	(1.052)	78	644076			12.82- 112.82	50.07	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	993176	25.0000	28.590	50.00- 150.00	100.00	
22.291	22.291	(1.072)	171	512772			0.34- 100.34	51.63	

134 Cumene CAS #: 98-82-8									
22.429	22.429	(1.078)	105	2209535	25.0000	28.690	50.00- 150.00	100.00	
22.429	22.429	(1.078)	120	577492			0.00- 74.52	26.14	
22.429	22.429	(1.078)	51	170049			51.79- 151.79	7.70	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	1185275	25.0000	28.068	50.00- 150.00	100.00	
23.010	23.010	(1.106)	85	777360			17.66- 117.66	65.58	

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	2769679	25.0000	28.435	50.00- 150.00	100.00	
23.121	23.121	(1.112)	120	622533			0.00- 71.52	22.48	
23.121	23.121	(1.112)	105	99520			0.00- 53.54	3.59	

145 4-Ethyltoluene CAS #: 622-96-8									
23.286	23.286	(1.120)	105	2388998	25.0000	29.120	50.00- 150.00	100.00	
23.286	23.286	(1.120)	120	711885			0.00- 79.85	29.80	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	1948520	25.0000	29.185	50.00- 150.00	100.00	
23.397	23.397	(1.125)	120	951484			0.29- 100.29	48.83	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	1796520	25.0000	28.912	50.00- 150.00	100.00	
24.033	24.033	(1.156)	120	838259			0.00- 94.69	46.66	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	1274193	25.0000	27.095	50.00- 150.00	100.00	
24.586	24.586	(1.182)	148	815817			14.61- 114.61	64.03	
24.586	24.586	(1.182)	111	534889			0.00- 92.01	41.98	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	1308673	25.0000	26.782	50.00- 150.00	100.00	
24.724	24.724	(1.189)	148	836466			13.83- 113.83	63.92	
24.724	24.724	(1.189)	111	530820			0.00- 89.75	40.56	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

159	alpha-Chlorotoluene					CAS #: 100-44-7			
24.945	24.945	(1.199)	91	1803467	25.0000	26.672	50.00- 150.00	100.00	
24.945	24.945	(1.199)	126	354583			0.00- 69.65	19.66	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
25.360	25.360	(1.219)	146	1201698	25.0000	26.648	50.00- 150.00	100.00	
25.360	25.360	(1.219)	148	775882			14.36- 114.36	64.57	
25.360	25.360	(1.219)	111	524362			0.00- 92.81	43.64	

165	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
28.153	28.153	(1.354)	180	596437	25.0000	19.282	50.00- 150.00	100.00	
28.153	28.153	(1.354)	182	570634			45.41- 145.41	95.67	

166	Hexachlorobutadiene					CAS #: 87-68-3			
28.319	28.319	(1.362)	225	582849	25.0000	20.644	50.00- 150.00	100.00	
28.319	28.319	(1.362)	223	367468			13.46- 113.46	63.05	

19	Butane					CAS #: 106-97-8			
6.807	6.807	(0.491)	58	67972	25.0000	26.995	50.00- 150.00	100.00	
6.807	6.807	(0.491)	43	480139			640.46- 740.46	706.38	

29	Isopentane					CAS #: 78-78-4			
8.273	8.273	(0.597)	43	378518	25.0000	26.697	50.00- 150.00	100.00	
8.273	8.273	(0.597)	57	287062			26.79- 126.79	75.84	

102	Methyl Cyclohexane					CAS #: 108-87-2			
16.346	16.346	(1.180)	83	707748	25.0000	29.146	50.00- 150.00	100.00	
16.346	16.346	(1.180)	98	325087			0.00- 95.49	45.93	
16.346	16.346	(1.180)	55	477451			16.76- 116.76	67.46	

167	Naphthalene					CAS #: 91-20-3			
28.678	28.678	(1.379)	128	914156	25.0000	17.930	50.00- 150.00	100.00	
28.678	28.678	(1.379)	127	112682			0.00- 62.56	12.33	

Report Date: 14-Dec-2007 10:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121313.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	259446	-7.59
97 1,4-Difluorobenze	1182601	709561	1655641	1118582	-5.41
126 Chlorobenzene-d5	1033655	620193	1447117	965763	-6.57

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/13Dec2007,b/t121313.d
Date: 14-DEC-2007 00:40
Client ID: Level 4
Sample Info: 25mL #1443-378

Column phase: RTX-624

Instrument: msdt,i
Operator: ab
Column diameter: 0.53

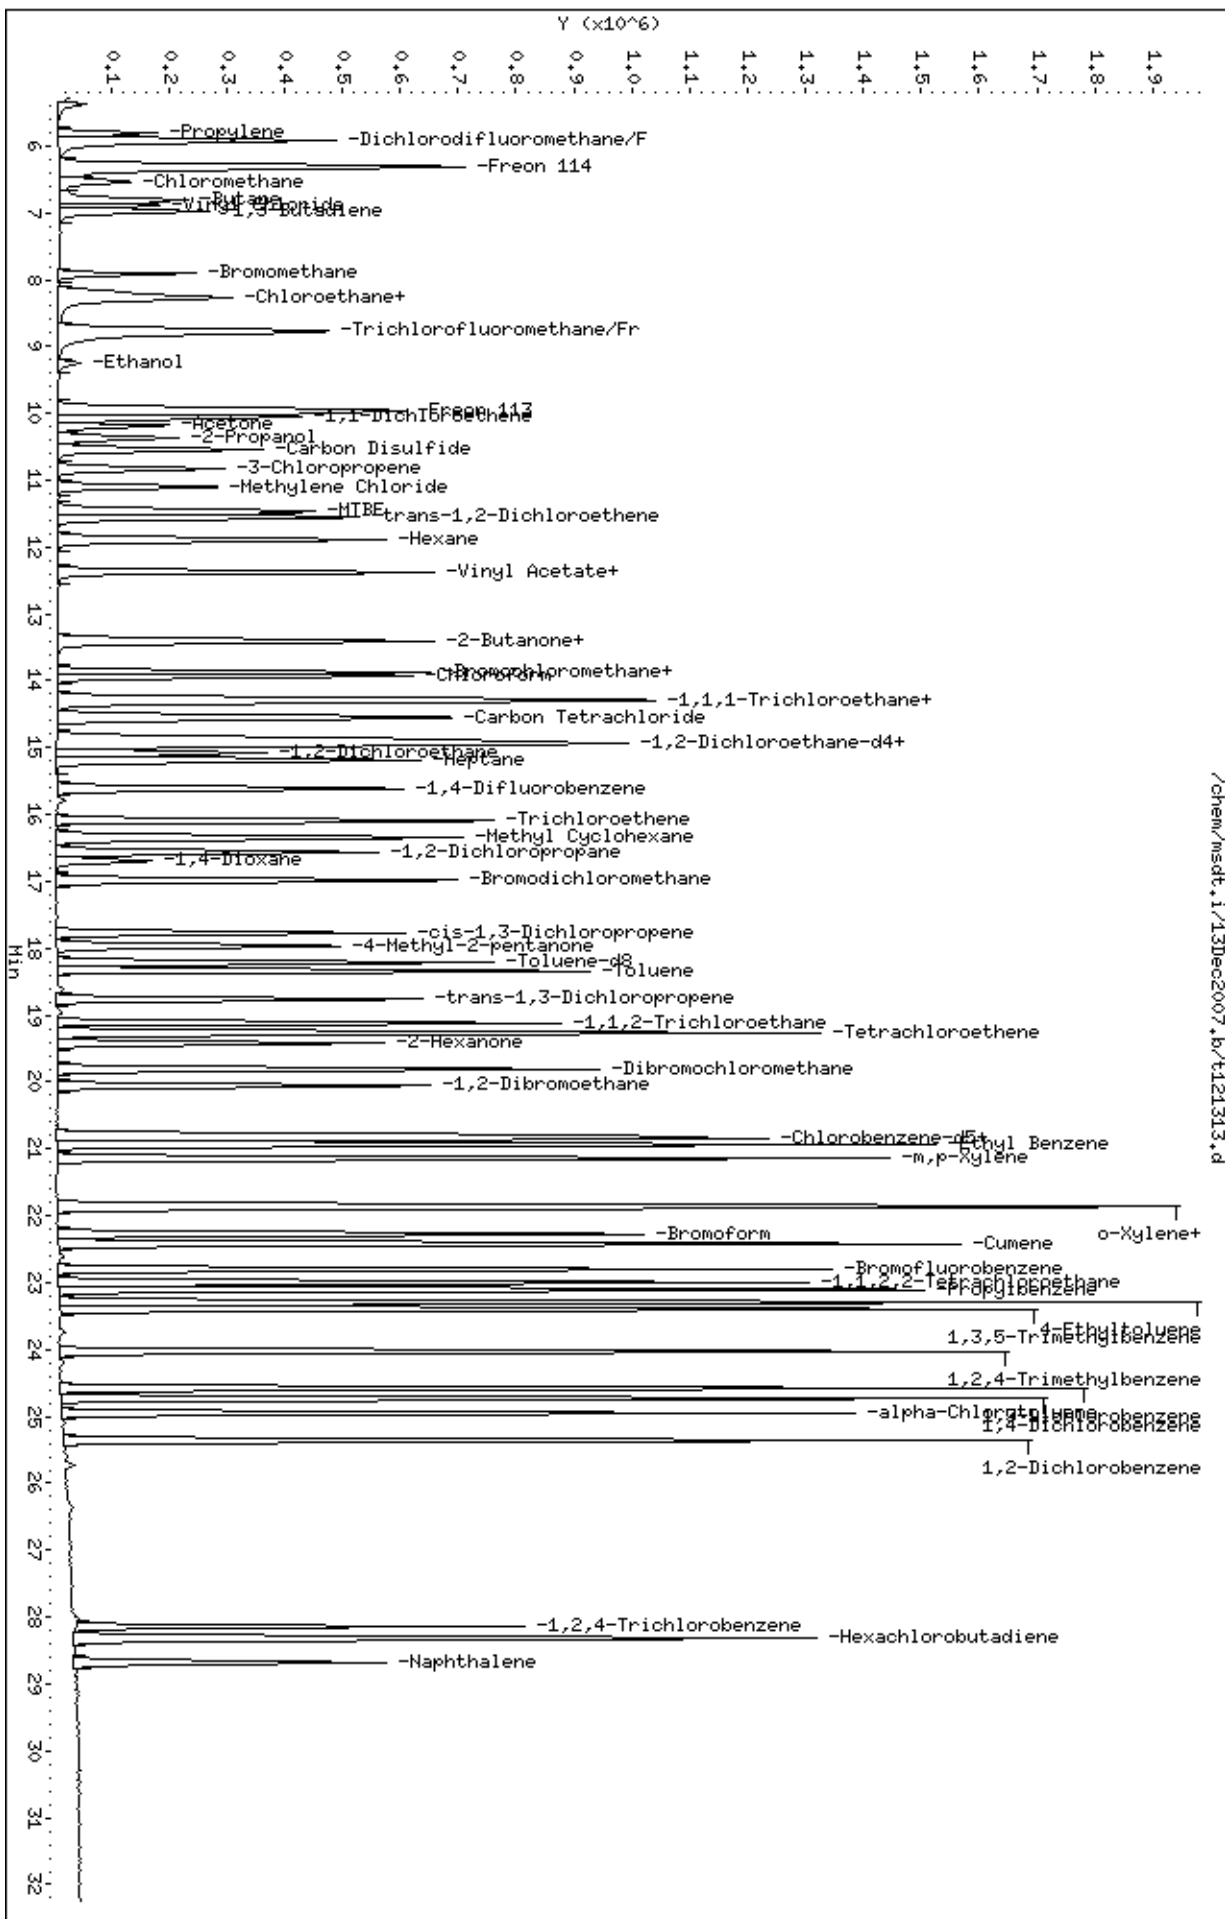

Report Date: 25-Jan-2008 14:48

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/25Jan2008.b/t012505.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 25-JAN-2008 12:14
 Operator : sjr Inst ID: msdt.i
 Smp Info : 50mL #1576-236
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Meth Date : 25-Jan-2008 14:48 sruth Quant Type: ISTD
 Cal Date : 25-JAN-2008 12:14 Cal File: t012505.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp12e.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	334161	25.0000			80.00- 120.00	100.00
13.886	13.886	(1.000)	128	249475				24.66- 124.66	74.66
13.858	13.858	(1.000)	49	347599				54.02- 154.02	104.02

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1198449	25.0000			80.00- 120.00	100.00
15.628	15.628	(1.000)	88	185758				0.00- 65.50	15.50

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1112878	25.0000			80.00- 120.00	100.00
20.798	20.798	(1.000)	82	622378				5.74- 105.74	55.93

21 Isobutane CAS #: 75-28-5									
6.337	6.337	(0.456)	43	1397462	50.0000	50.102		80.00- 120.00	100.00(A)
6.337	6.337	(0.456)	42	465933				0.00- 82.88	33.34
6.337	6.337	(0.456)	58	39014				0.00- 52.81	2.79

35 1-Pentene CAS #: 109-67-1									
8.798	8.798	(0.634)	55	958179	50.0000	50.820		80.00- 120.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
35 1-Pentene (continued)									
8.798	8.798	(0.634)	42	904948			42.09- 142.09	94.44	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

44 Acrolein CAS #: 107-02-8									
9.904	9.904	(0.713)	55	271656	50.0000	53.980	80.00- 120.00	100.00	
9.904	9.904	(0.713)	56	383857			91.89- 191.89	141.30	

48 Ethyl acrylate CAS #: 140-88-5									
16.153	16.153	(1.034)	99	169759	50.0000	54.724	80.00- 120.00	100.00	
16.153	16.153	(1.034)	45	153422			40.38- 140.38	90.38	
16.153	16.153	(1.034)	55	1817719			1020.76-1120.76	1070.76	

49 Iodomethane CAS #: 74-88-4									
10.429	10.429	(0.751)	142	2579289	50.0000	55.065	80.00- 120.00	100.00	
10.429	10.429	(0.751)	127	1196696			0.00- 97.58	46.40	

50 Methyl Methacrylate CAS #: 80-62-6									
16.568	16.568	(1.060)	41	1060538	50.0000	55.926	80.00- 120.00	100.00	
16.568	16.568	(1.060)	69	1029907			48.84- 148.84	97.11	
16.568	16.568	(1.060)	100	416782			0.00- 88.29	39.30	

52 Acetonitrile CAS #: 75-05-8									
10.899	10.899	(0.785)	40	298751	50.0000	35.783	80.00- 120.00	100.00	
10.899	10.899	(0.785)	41	575875			94.31- 194.31	192.76	
10.899	10.899	(0.785)	38	84869			0.00- 73.26	28.41	

56 Cyclopentane CAS #: 287-92-3									
11.121	11.121	(0.801)	70	651288	50.0000	55.731	80.00- 120.00	100.00	
11.121	11.121	(0.801)	55	767193			70.62- 170.62	117.80	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

62 Acrylonitrile CAS #: 107-13-1									
11.646	11.646	(0.839)	53	634164	50.0000	52.507	80.00- 120.00	100.00	
11.646	11.646	(0.839)	52	545625			34.51- 134.51	86.04	

63 2-Pentanone CAS #: 107-87-9									
16.374	16.374	(1.048)	43	1921570	50.0000	58.516	80.00- 120.00	100.00(A)	
16.374	16.374	(1.048)	58	176990			0.00- 59.30	9.21	
16.374	16.374	(1.048)	86	457959			0.00- 74.01	23.83	

66 1-Hexene CAS #: 592-41-6									
11.784	11.784	(0.849)	55	615522	50.0000	59.335	80.00- 120.00	100.00	
11.784	11.784	(0.849)	41	869120			104.22- 204.22	141.20	
11.784	11.784	(0.849)	84	294457			5.60- 105.60	47.84	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
105 Dibromomethane						CAS #: 74-95-3			
16.789	16.789	(1.074)	174	1293509	50.0000	51.066	80.00- 120.00	100.00	
16.789	16.789	(1.074)	93	1289980			51.33- 151.33	99.73	
16.789	16.789	(1.074)	95	1076231			33.65- 133.65	83.20	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 25-Jan-2008 14:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 25-JAN-2008

Lab File ID: t012505.d

Calibration Time: 12:14

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/25Jan2008.b/t14q1213e.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	334161	200497	467825	334161	0.00
97 1,4-Difluorobenze	1198449	719069	1677829	1198449	0.00
126 Chlorobenzene-d5	1112878	667727	1558029	1112878	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt.i/25Jan2008.b/t012505.d

Date: 25-Jan-2008 12:14

Client ID: Level 5

Sample Info: 50mL #1576-236


Column phase: RTX-624

Instrument: msdt.i

Operator: sjr

Column diameter: 0.53

/chem/msdt.i/25Jan2008.b/t012505.d

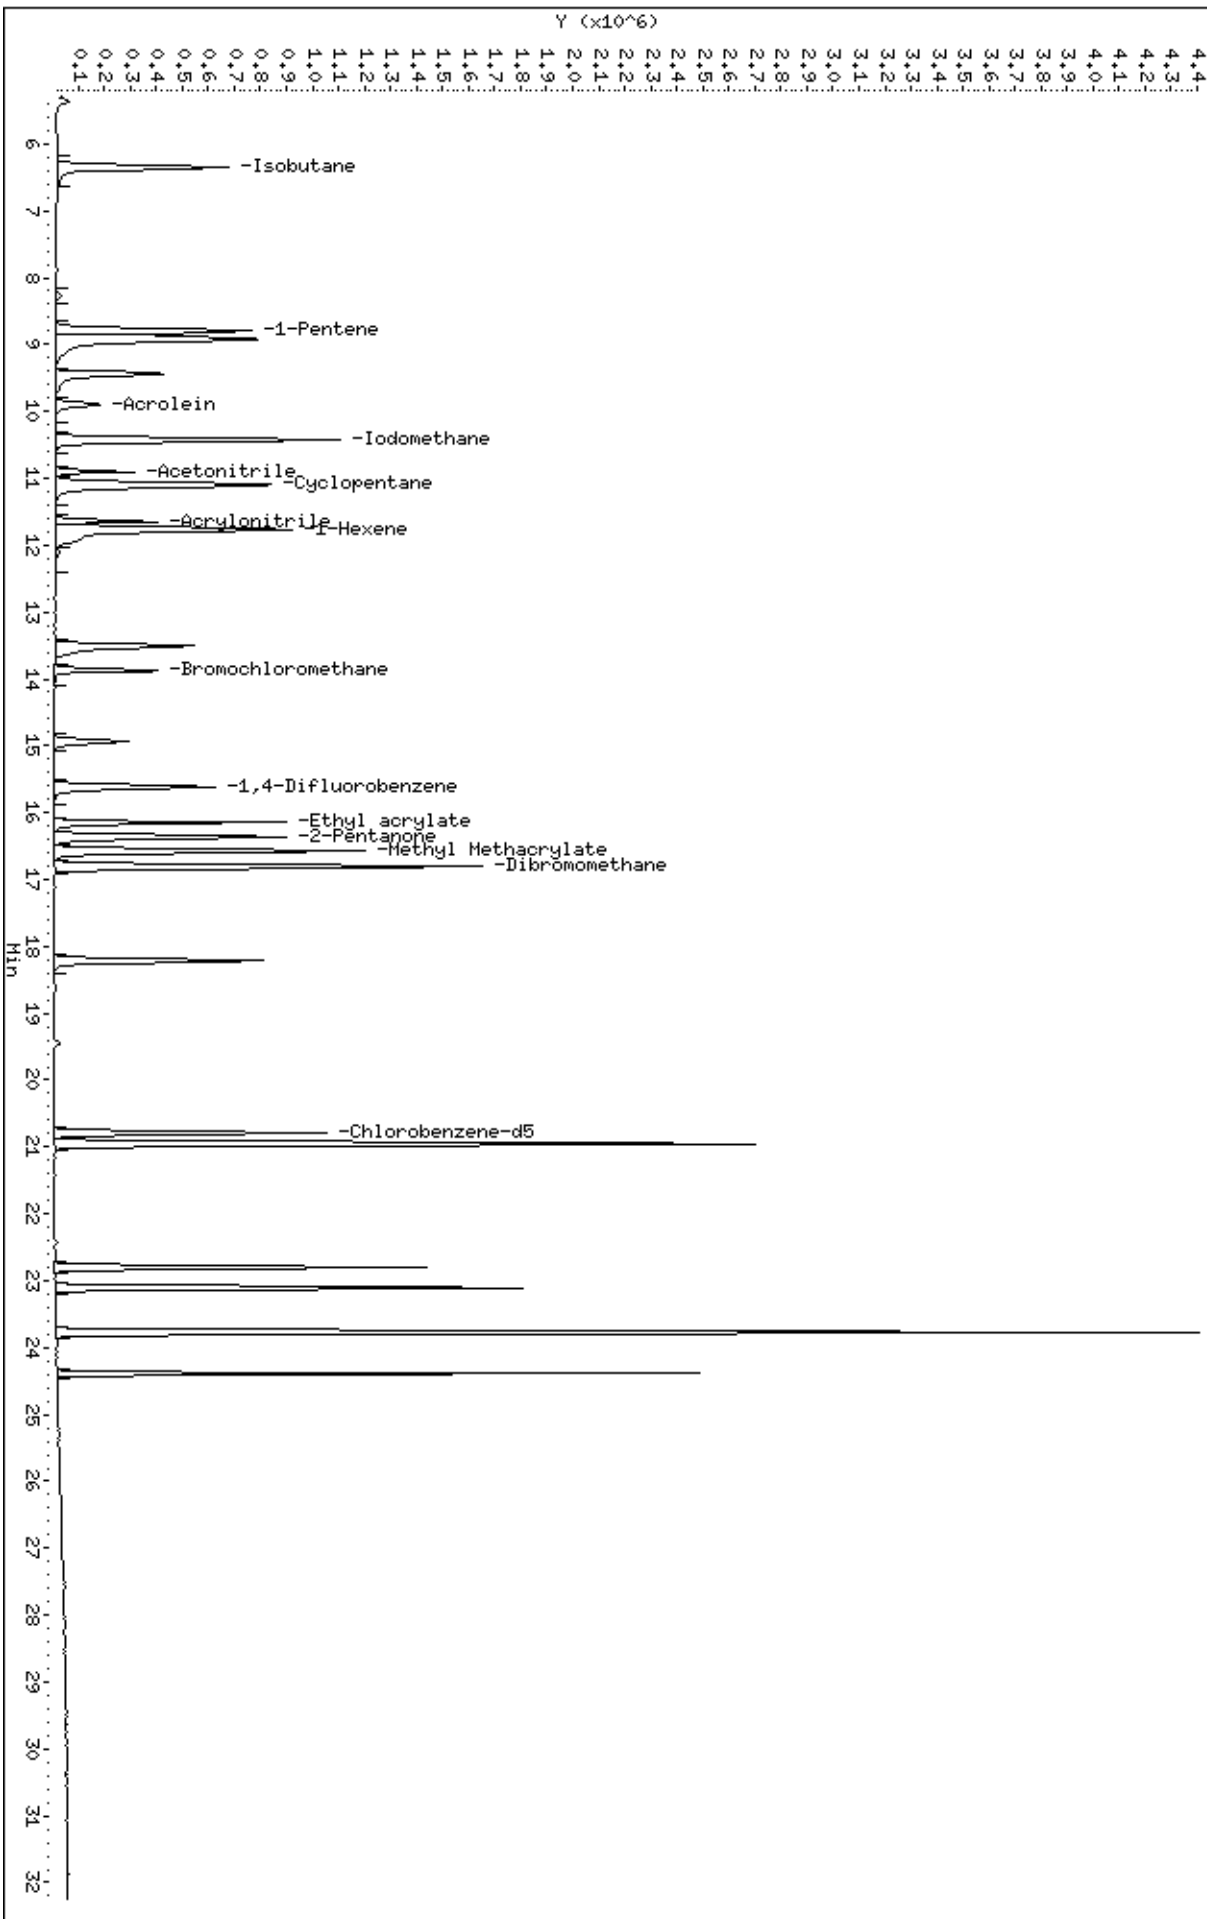

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/16Jan2008.b/t011609.d
 Lab Smp Id: TVH ICAL Client Smp ID: Level 5
 Inj Date : 16-JAN-2008 13:44
 Operator : lo Inst ID: msdt.i
 Smp Info : 50ml #1443-403
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/t14q1213d.m
 Meth Date : 16-Jan-2008 14:59 lover Quant Type: ISTD
 Cal Date : 16-JAN-2008 13:44 Cal File: t011609.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5d.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	325810	25.0000			80.00- 120.00	100.00
13.886	13.886	(1.000)	128	246013				25.51- 125.51	75.51
13.886	13.886	(1.000)	49	374594				64.97- 164.97	114.97

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1168077	25.0000			80.00- 120.00	100.00
15.628	15.628	(1.000)	88	185409				0.00- 65.87	15.87

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1103278	25.0000			80.00- 120.00	100.00
20.798	20.798	(1.000)	82	635614				5.94- 105.94	57.61

204 Propane CAS #: 74-98-6									
5.812	5.812	(0.419)	43	197200	50.0000	50.296		80.00- 120.00	100.00
5.812	5.812	(0.419)	44	230065				107.53- 207.53	116.67

37 Pentane CAS #: 109-66-0									
8.937	8.937	(0.644)	43	1561530	50.0000	54.594		80.00- 120.00	100.00
8.937	8.937	(0.644)	57	270071				0.00- 67.03	17.30

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
37 Pentane (continued)									
8.937	8.937	(0.644)	72	198371			0.00- 62.09	12.70	

112 Octane									
						CAS #: 111-65-9			
18.282	18.282	(1.170)	57	861060	50.0000	51.679	80.00- 120.00	100.00	
18.282	18.282	(1.170)	85	1164239			82.32- 182.32	135.21	
18.282	18.282	(1.170)	43	1900329			166.39- 266.39	220.70	

124 Nonane									
						CAS #: 111-84-2			
20.964	20.964	(1.008)	43	1998154	50.0000	56.375	80.00- 120.00	100.00	
20.964	20.964	(1.008)	57	2028290			52.38- 152.38	101.51	
20.964	20.964	(1.008)	85	907436			0.00- 95.58	45.41	

139 Decane									
						CAS #: 124-18-5			
23.204	23.204	(1.116)	57	2392634	50.0000	56.202	80.00- 120.00	100.00	
23.204	23.204	(1.116)	71	1050200			0.00- 93.78	43.89	
23.204	23.204	(1.116)	142	117203			0.00- 54.94	4.90	

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 16-JAN-2008

Lab File ID: t011609.d

Calibration Time: 13:44

Lab Smp Id: TVH ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lo

Method File: /chem/msdt.i/16Jan2008.b/t14q1213d.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	325810	195486	456134	325810	0.00
97 1,4-Difluorobenze	1168077	700846	1635308	1168077	0.00
126 Chlorobenzene-d5	1103278	661967	1544589	1103278	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/16Jan2008,b/t011609.d

Date : 16-Jan-2008 13:44

Client ID: Level 5


Sample Info: 50ml #1443-403

Column phase: RTX-624

Instrument: msdt,i

Operator: lo

Column diameter: 0.53

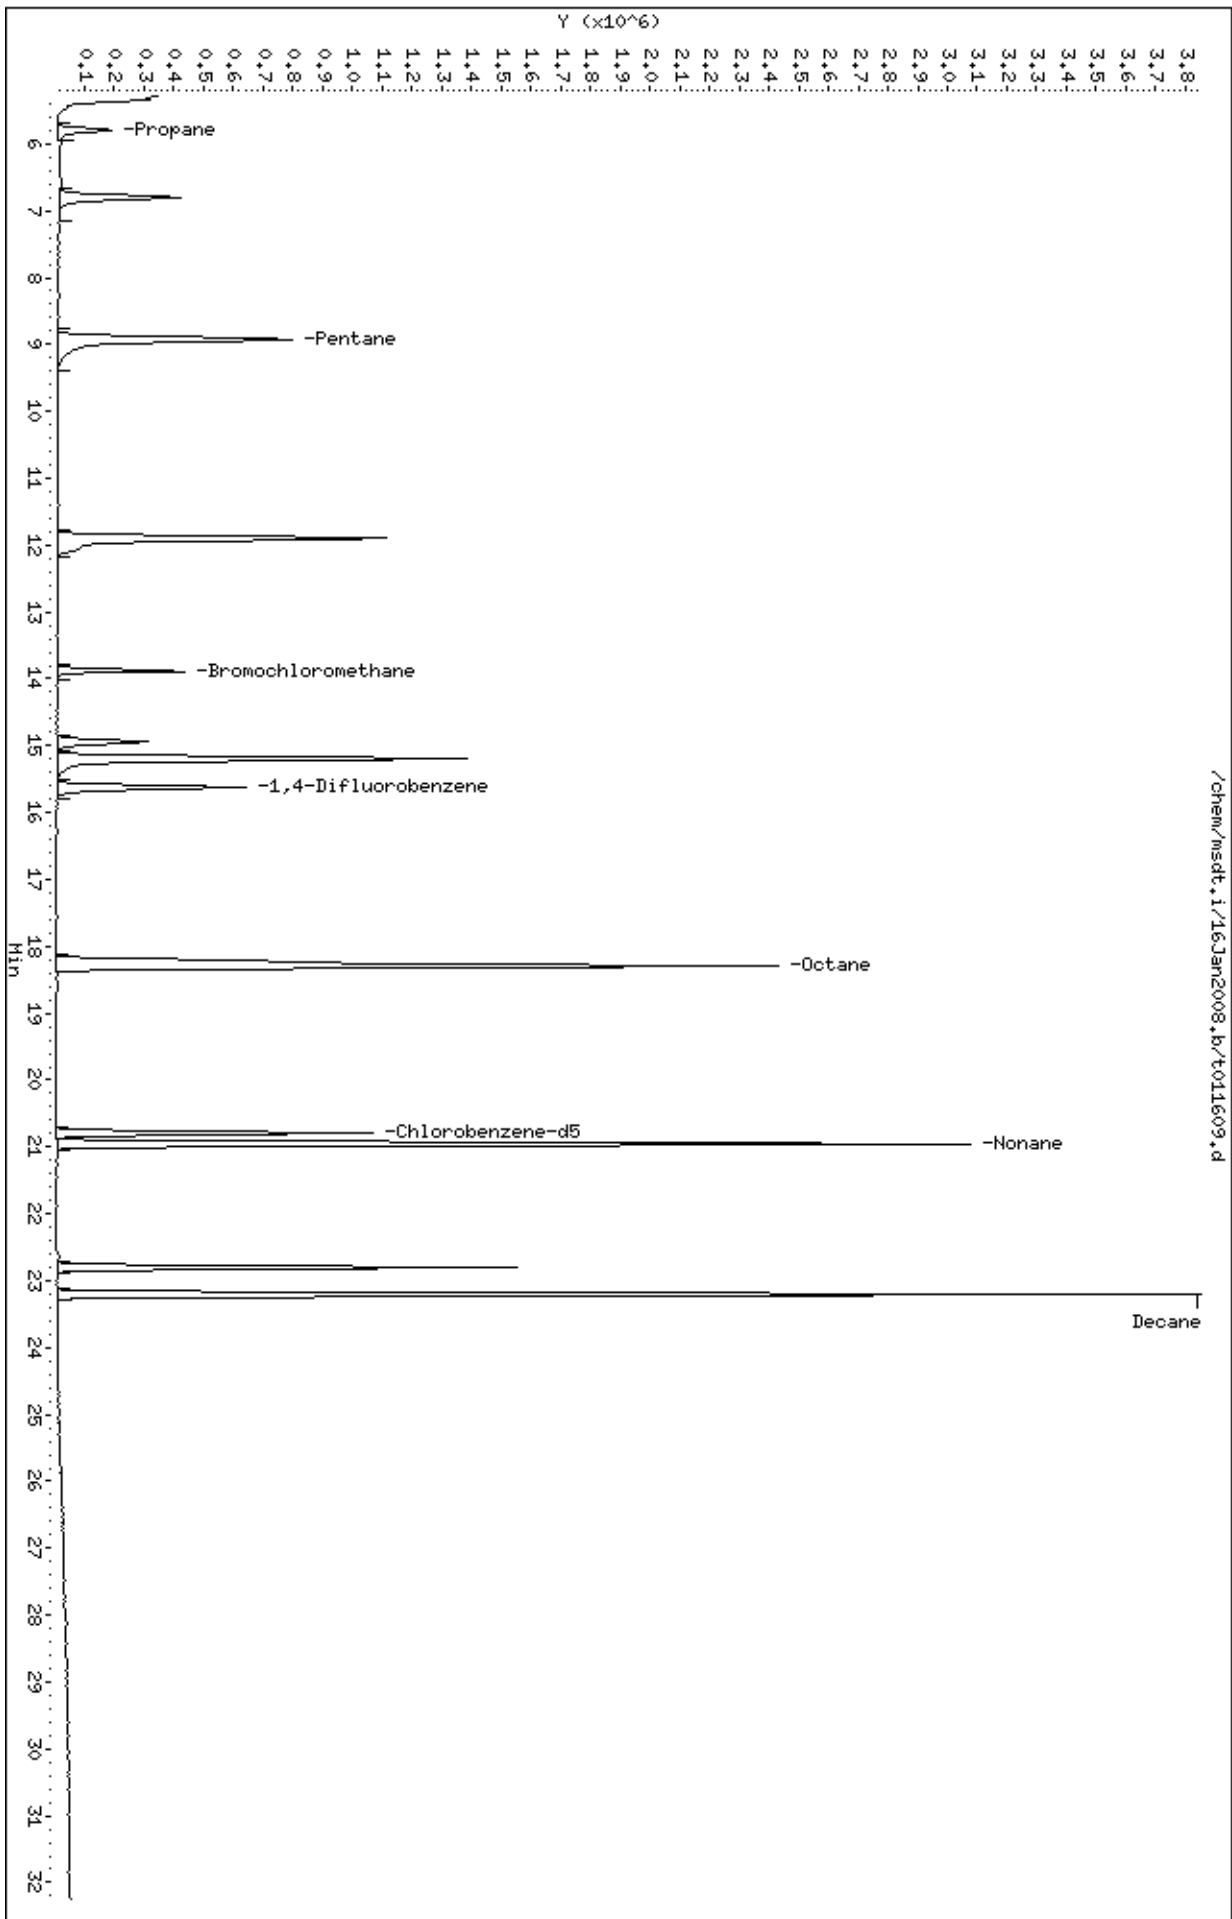

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/02Jan2008.b/t010204.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 02-JAN-2008 12:02
 Operator : sjr Inst ID: msdt.i
 Smp Info : 50ml #1443-399
 Misc Info : 200ppbv -> 50ppbv (300ppbv MeOH)
 Comment :
 Method : /chem/msdt.i/02Jan2008.b/t14q1213c.m
 Meth Date : 02-Jan-2008 15:47 sruth Quant Type: ISTD
 Cal Date : 02-JAN-2008 12:02 Cal File: t010204.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp22c.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.865	13.865	(1.000)	130	338913	25.0000			80.00- 120.00	100.00
13.865	13.865	(1.000)	128	254032				24.95- 124.95	74.95
13.865	13.865	(1.000)	49	382548				62.87- 162.87	112.87

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.635	15.635	(1.000)	114	1251078	25.0000			80.00- 120.00	100.00
15.635	15.635	(1.000)	88	204292				0.00- 66.33	16.33

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.805	20.805	(1.000)	117	1269166	25.0000			80.00- 120.00	100.00
20.805	20.805	(1.000)	82	718652				5.77- 105.77	56.62

6 Freon142b CAS #: 75-68-3									
6.408	6.408	(0.462)	65	2396168	50.0000	54.714		80.00- 120.00	100.00
6.408	6.408	(0.462)	45	473169				0.00- 71.17	19.75

9 Freon 13 CAS #: 75-72-9									
5.394	5.394	(0.389)	69	2122581	50.0000	49.387		80.00- 120.00	100.00(H)
5.394	5.394	(0.389)	85	737984				0.00- 83.23	34.77

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
9 Freon 13 (continued)									
5.394	5.394	(0.389)	87	233951			0.00- 60.80	11.02	

13 Freon 134a CAS #: 811-97-2									
5.675	5.675	(0.409)	83	1027420	50.0000	53.055	80.00- 120.00	100.00	
5.675	5.675	(0.409)	69	796196			29.59- 129.59	77.49	

15 Freon 152a CAS #: 75-37-6									
5.844	5.844	(0.422)	65	484736	50.0000	47.000	80.00- 120.00	100.00	
5.844	5.844	(0.422)	51	840680			125.61- 225.61	173.43	
5.844	5.844	(0.422)	47	216912			0.00- 95.62	44.75	

17 Freon 22 CAS #: 75-45-6									
5.985	5.985	(0.432)	67	271635	50.0000	51.256	80.00- 120.00	100.00	
5.985	5.985	(0.432)	51	1294835			424.04- 524.04	476.68	
5.985	5.985	(0.432)	85	24008			0.00- 60.14	8.84	

26 Methanol CAS #: 67-56-1									
7.534	7.534	(0.543)	31	1157692	300.000	264.08	80.00- 120.00	100.00	
7.534	7.534	(0.543)	32	943528			31.50- 131.50	81.50	

34 Dichlorofluoromethane/Fr21 CAS #: 75-43-4									
8.717	8.717	(0.629)	67	1779732	50.0000	52.407	80.00- 120.00	100.00	
8.717	8.717	(0.629)	69	587706			0.00- 82.55	33.02	
8.717	8.717	(0.629)	35	100429			0.00- 55.68	5.64	

40 Freon123a CAS #: 354-23-4									
9.580	9.580	(0.691)	67	1457554	50.0000	55.496	80.00- 120.00	100.00	
9.580	9.580	(0.691)	117	1237895			33.27- 133.27	84.93	

41 Freon123 CAS #: 306-83-2									
9.718	9.718	(0.701)	83	1972873	50.0000	54.702	80.00- 120.00	100.00	
9.718	9.718	(0.701)	133	430326			0.00- 72.56	21.81	
9.718	9.718	(0.701)	85	1387787			21.04- 121.04	70.34	

57 tert-Butyl-Alcohol CAS #: 75-65-0									
11.156	11.156	(0.805)	59	2022367	50.0000	62.565	80.00- 120.00	100.00	
11.156	11.156	(0.805)	41	442486			0.00- 79.32	21.88	
11.156	11.156	(0.805)	57	215102			0.00- 60.92	10.64	

68 Isopropyl ether CAS #: 108-20-3									
12.289	12.289	(0.886)	45	2709742	50.0000	55.545	80.00- 120.00	100.00	
12.289	12.289	(0.886)	87	834732			0.00- 81.01	30.80	
12.289	12.289	(0.886)	59	286378			0.00- 61.81	10.57	

71 1-Propanol CAS #: 71-23-8									
12.400	12.400	(0.894)	42	179265	50.0000	55.970	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
71 1-Propanol (continued)									
12.400	12.400	(0.894)	59	244040			61.64- 161.64	136.13	
12.400	12.400	(0.894)	41	156800			40.91- 140.91	87.47	

73 t-Butylethyl Ether									
						CAS #: 637-92-3			
12.925	12.925	(0.932)	59	3012445	50.0000	56.547	80.00- 120.00	100.00	
12.925	12.925	(0.932)	87	1332920			0.00- 93.11	44.25	
12.925	12.925	(0.932)	41	537994			0.00- 70.41	17.86	

77 Ethyl Acetate									
						CAS #: 141-78-6			
13.395	13.395	(0.966)	45	303435	50.0000	54.942	80.00- 120.00	100.00	
13.395	13.395	(0.966)	61	326819			49.68- 149.68	107.71	
13.395	13.395	(0.966)	43	2106113			615.05- 715.05	694.09	

92 tert-amyl-Methyl Ether									
						CAS #: 994-05-8			
14.999	14.999	(1.082)	73	2778392	50.0000	57.159	80.00- 120.00	100.00	
14.999	14.999	(1.082)	87	692542			0.00- 74.91	24.93	
14.999	14.999	(1.082)	55	692160			0.00- 76.64	24.91	

96 2-Heptanone									
						CAS #: 110-43-0			
21.967	21.967	(1.584)	58	1696491	50.0000	62.136	80.00- 120.00	100.00	
21.967	21.967	(1.584)	43	2407439			98.27- 198.27	141.91	

98 1-Butanol									
						CAS #: 71-36-3			
15.801	15.801	(1.011)	56	562340	50.0000	60.086	80.00- 120.00	100.00	
15.801	15.801	(1.011)	41	382171			28.59- 128.59	67.96	
15.801	15.801	(1.011)	43	290179			6.69- 106.69	51.60	

119 Butyl Acetate									
						CAS #: 123-86-4			
19.533	19.533	(1.249)	56	1045491	50.0000	59.312	80.00- 120.00	100.00	
19.533	19.533	(1.249)	73	426525			0.00- 90.80	40.80	
19.533	19.533	(1.249)	43	2329735			172.84- 272.84	222.84	

135 Cyclohexanone									
						CAS #: 108-94-1			
22.741	22.741	(1.093)	55	1273954	50.0000	60.235	80.00- 120.00	100.00	
22.741	22.741	(1.093)	98	677426			2.09- 102.09	53.18	
22.741	22.741	(1.093)	42	839599			15.79- 115.79	65.90	

146 Diisobutyl Ketone									
						CAS #: 108-83-8			
23.570	23.570	(1.133)	57	3113179	50.0000	60.792	80.00- 120.00	100.00	
23.570	23.570	(1.133)	85	2973314			45.51- 145.51	95.51	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

QC Flag Legend

H - Operator selected an alternate compound hit.

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 02-JAN-2008

Lab File ID: t010204.d

Calibration Time: 12:02

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/02Jan2008.b/t14q1213c.m

Misc Info: 200ppbv -> 50ppbv (300ppbv MeOH)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	338913	203348	474478	338913	0.00
97 1,4-Difluorobenze	1251078	750647	1751509	1251078	0.00
126 Chlorobenzene-d5	1269166	761500	1776832	1269166	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/02Jan2008,b/t010204.d

Date : 02-Jan-2008 12:02

Client ID: Level 5

Sample Info: 50ml #1443-399


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/02Jan2008,b/t010204.d

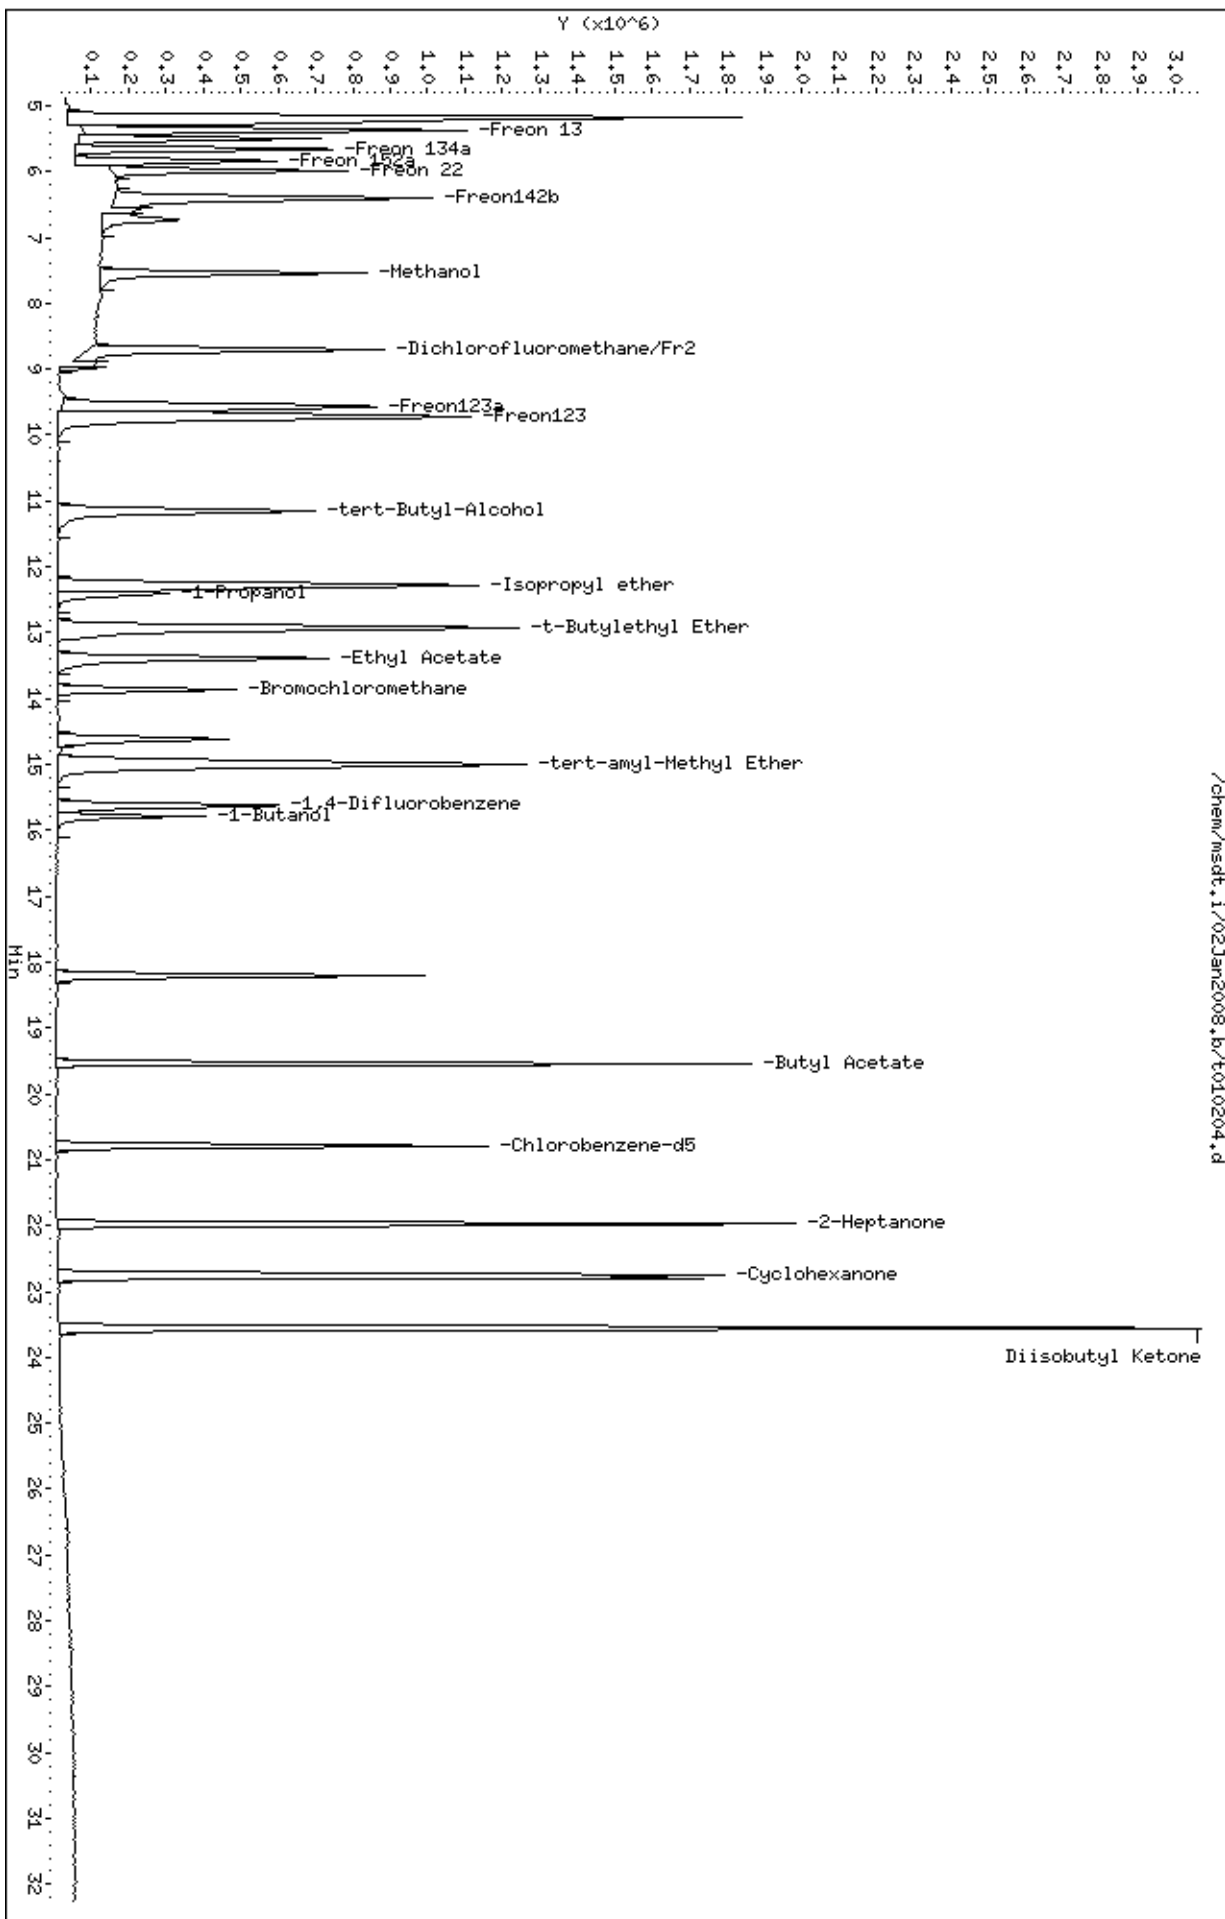

Report Date: 19-Dec-2007 12:55

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/19Dec2007.b/t121903.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 19-DEC-2007 11:12
 Operator : sjr Inst ID: msdt.i
 Smp Info : 50ml #1443-388
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/19Dec2007.b/t14q1213b.m
 Meth Date : 19-Dec-2007 12:55 sruth Quant Type: ISTD
 Cal Date : 19-DEC-2007 11:12 Cal File: t121903.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: splb.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	CAL-AMT	ON-COL	RESPONSE (PPBV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.865	13.865	(1.000)	130	204685	25.0000			80.00- 120.00	100.00
13.865	13.865	(1.000)	128	158127				27.25- 127.25	77.25
13.865	13.865	(1.000)	49	250268				72.27- 172.27	122.27

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.635	15.635	(1.000)	114	866754	25.0000			80.00- 120.00	100.00
15.607	15.607	(1.000)	88	138874				0.00- 66.02	16.02

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.805	20.805	(1.000)	117	784408	25.0000			80.00- 120.00	100.00
20.805	20.805	(1.000)	82	459725				6.00- 106.00	58.61

199 Vinyl Fluoride CAS #: 75-02-5									
5.563	5.563	(0.401)	46	313536	50.0000	57.248		80.00- 120.00	100.00
5.563	5.563	(0.401)	45	220658				20.20- 120.20	70.38
5.563	5.563	(0.401)	47	7196				0.00- 52.23	2.30

Report Date: 19-Dec-2007 12:55

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 19-DEC-2007

Lab File ID: t121903.d

Calibration Time: 11:12

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/19Dec2007.b/t14q1213b.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	204685	122811	286559	204685	0.00
97 1,4-Difluorobenze	866754	520052	1213456	866754	0.00
126 Chlorobenzene-d5	784408	470645	1098171	784408	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/19Dec2007,b/t121903.d

Date : 19-DEC-2007 11:12

Client ID: Level 5

Sample Info: 50ml #1443-388


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/19Dec2007,b/t121903.d

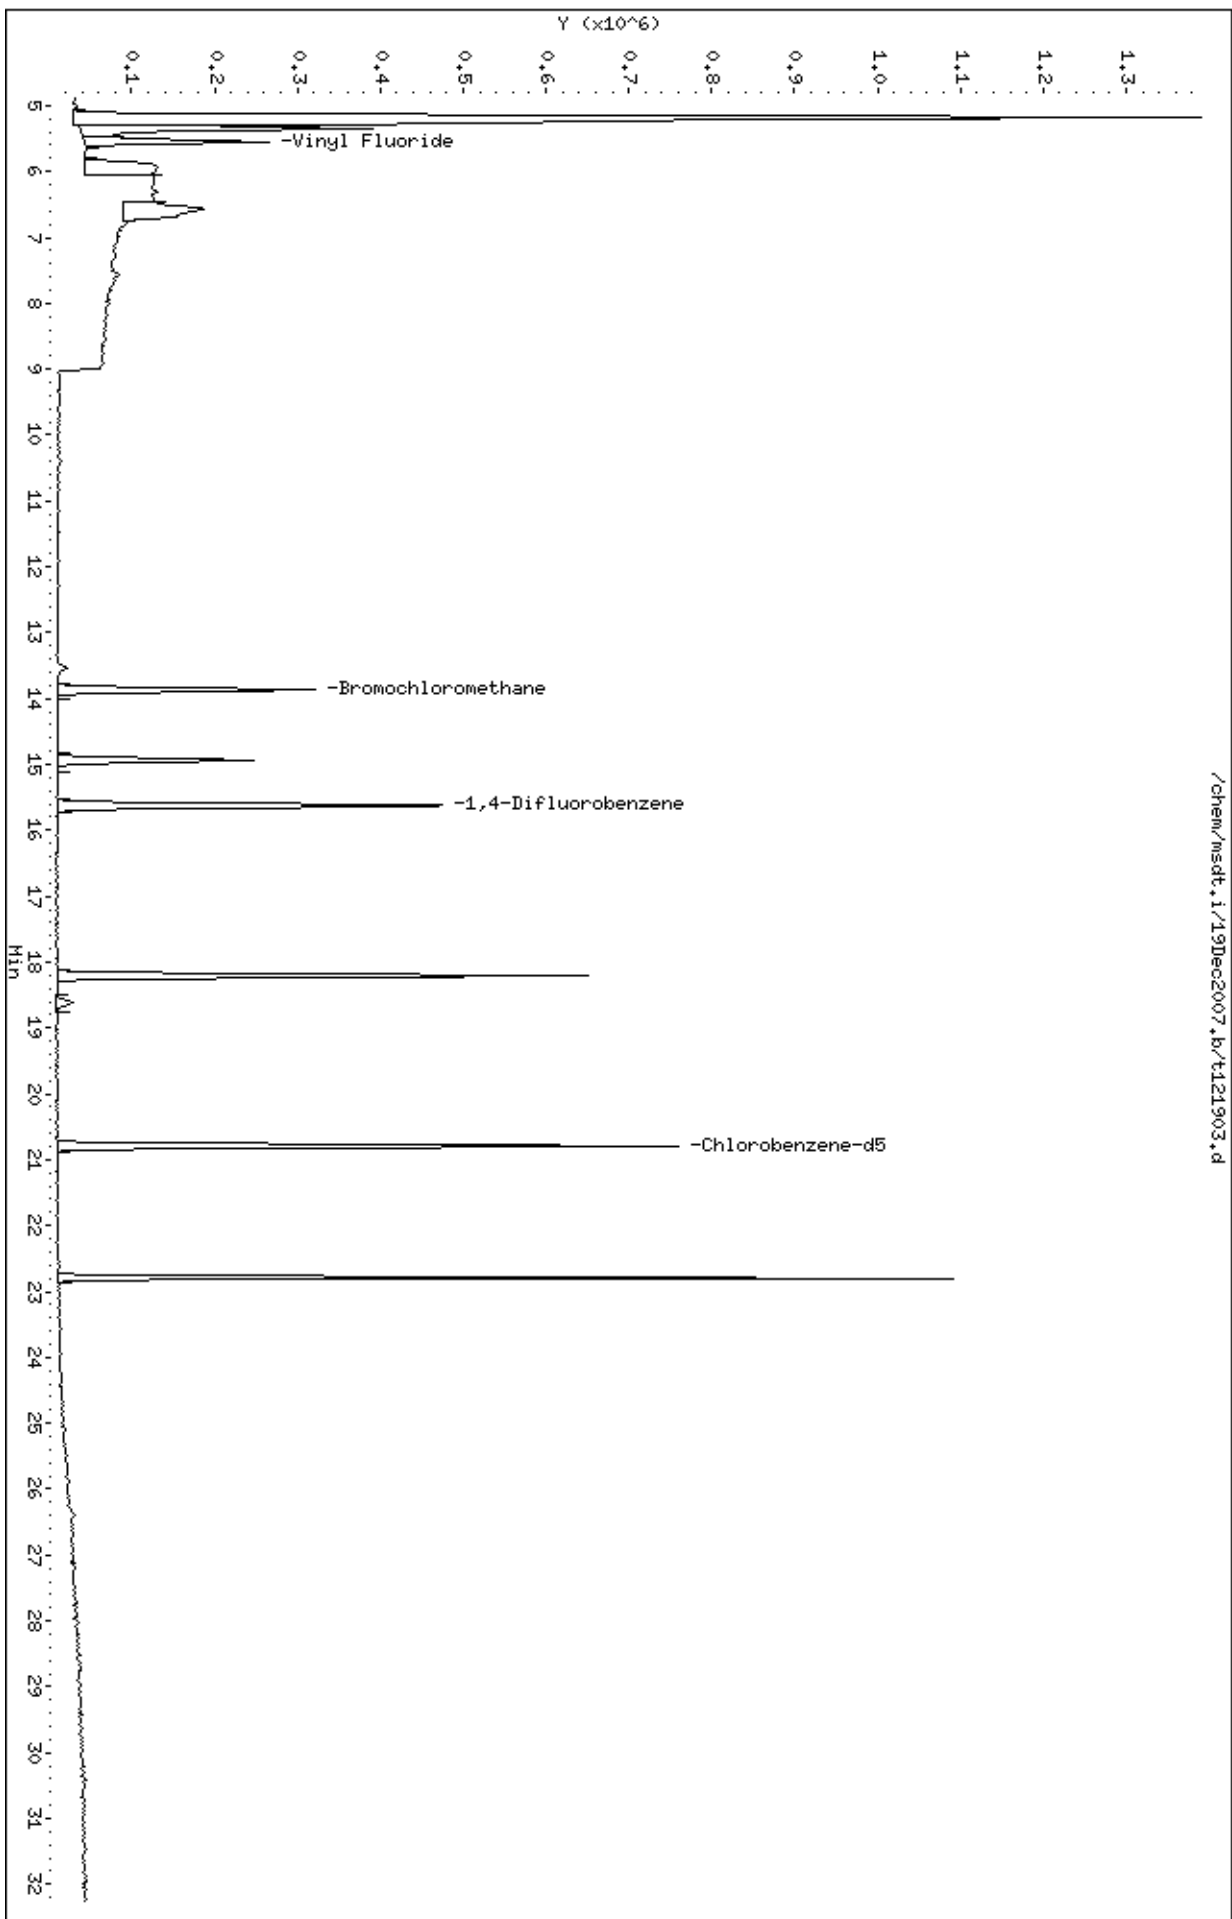

Report Date: 14-Dec-2007 10:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121314.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 14-DEC-2007 01:23
 Operator : ab Inst ID: msdt.i
 Smp Info : 50mL #1443-378
 Misc Info : 200ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 10:41 ealcan Quant Type: ISTD
 Cal Date : 14-DEC-2007 01:23 Cal File: t121314.d
 Als bottle: 1 Calibration Sample, Level: 5
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	280754	25.0000		80.00- 120.00	100.00	
13.858	13.858	(1.000)	128	216293			27.04- 127.04	77.04	
13.858	13.858	(1.000)	49	441722			107.33- 207.33	157.33	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.627	15.627	(1.000)	114	1182601	25.0000		80.00- 120.00	100.00	
15.627	15.627	(1.000)	88	189706			0.00- 66.04	16.04	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1033655	25.0000		80.00- 120.00	100.00	
20.798	20.798	(1.000)	82	580729			5.33- 105.33	56.18	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.078)	65	474779	25.0000	26.560	80.00- 120.00	100.00	
14.936	14.936	(1.078)	67	263656			3.93- 103.93	55.53	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1112825	25.0000	24.806	80.00- 120.00	100.00	
18.199	18.199	(1.165)	70	121364			0.00- 61.06	10.91	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	762411			18.52- 118.52	68.51	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	701844	25.0000	24.756	80.00- 120.00	100.00	
22.789	22.789	(1.096)	95	870075			73.97- 173.97	123.97	
22.789	22.789	(1.096)	176	675526			46.25- 146.25	96.25	

11 Propylene									
						CAS #: 115-07-1			
5.812	5.812	(0.419)	41	367115	50.0000	48.960	80.00- 120.00	100.00	
5.812	5.812	(0.419)	42	251333			17.44- 117.44	68.46	
5.812	5.812	(0.419)	39	292684			31.05- 131.05	79.73	

12 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
5.922	5.922	(0.427)	85	2514370	50.0000	51.133	80.00- 120.00	100.00	
5.922	5.922	(0.427)	87	809335			0.00- 82.50	32.19	

16 Freon 114									
						CAS #: 76-14-2			
6.310	6.310	(0.455)	135	1748803	50.0000	54.401	80.00- 120.00	100.00	
6.310	6.310	(0.455)	137	560038			0.00- 81.78	32.02	

18 Chloromethane									
						CAS #: 74-87-3			
6.558	6.558	(0.473)	50	496205	50.0000	46.652	80.00- 120.00	100.00	
6.558	6.558	(0.473)	52	164249			0.00- 83.59	33.10	

20 Vinyl Chloride									
						CAS #: 75-01-4			
6.890	6.890	(0.497)	62	704576	50.0000	52.962	80.00- 120.00	100.00	
6.890	6.890	(0.497)	64	224540			0.00- 94.54	31.87	

22 1,3-Butadiene									
						CAS #: 106-99-0			
6.973	6.973	(0.503)	54	569340	50.0000	54.824	80.00- 120.00	100.00	
6.973	6.973	(0.503)	39	539956			61.08- 161.08	94.84	

25 Bromomethane									
						CAS #: 74-83-9			
7.913	7.913	(0.571)	94	728362	50.0000	51.699	80.00- 120.00	100.00	
7.913	7.913	(0.571)	96	673434			42.46- 142.46	92.46	

27 Chloroethane									
						CAS #: 75-00-3			
8.190	8.190	(0.591)	64	387152	50.0000	54.539	80.00- 120.00	100.00	
8.190	8.190	(0.591)	49	98158			0.00- 76.61	25.35	
8.190	8.190	(0.591)	66	126925			0.00- 85.87	32.78	

31 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
8.770	8.770	(0.633)	101	2998989	50.0000	54.559	80.00- 120.00	100.00	
8.798	8.798	(0.635)	103	1933148			14.46- 114.46	64.46	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Ethanol						CAS #: 64-17-5			
9.240	9.240	(0.667)	45	201828	50.0000	54.138	80.00- 120.00	100.00	
9.240	9.240	(0.667)	43	47423			0.00- 74.87	23.50	
9.240	9.240	(0.667)	46	71873			0.00- 88.05	35.61	

42 Freon 113						CAS #: 76-13-1			
9.959	9.959	(0.719)	151	1297474	50.0000	52.447	80.00- 120.00	100.00	
9.959	9.959	(0.719)	153	825911			13.66- 113.66	63.66	
9.959	9.959	(0.719)	101	1700298			81.05- 181.05	131.05	

43 1,1-Dichloroethene						CAS #: 75-35-4			
10.042	10.042	(0.725)	61	1175169	50.0000	54.196	80.00- 120.00	100.00	
10.042	10.042	(0.725)	96	727601			11.91- 111.91	61.91	
10.042	10.042	(0.725)	98	478832			0.00- 90.75	40.75	

45 Acetone						CAS #: 67-64-1			
10.180	10.180	(0.735)	58	356154	50.0000	52.901	80.00- 120.00	100.00	
10.180	10.180	(0.735)	43	1090436			264.94- 364.94	306.17	

46 2-Propanol						CAS #: 67-63-0			
10.374	10.374	(0.749)	45	1214761	50.0000	54.468	80.00- 120.00	100.00	
10.374	10.374	(0.749)	43	305977			0.00- 78.96	25.19	
10.374	10.374	(0.749)	59	52752			0.00- 54.05	4.34	

47 Carbon Disulfide						CAS #: 75-15-0			
10.540	10.540	(0.761)	76	2199066	50.0000	53.192	80.00- 120.00	100.00	

51 3-Chloropropene						CAS #: 107-05-1			
10.816	10.816	(0.781)	76	375694	50.0000	53.245	80.00- 120.00	100.00	
10.816	10.816	(0.781)	41	814899			176.05- 276.05	216.90	

54 Methylene Chloride						CAS #: 75-09-2			
11.121	11.121	(0.802)	49	695817	50.0000	50.816	80.00- 120.00	100.00	
11.121	11.121	(0.802)	84	650464			43.48- 143.48	93.48	
11.093	11.093	(0.800)	51	210009			0.00- 83.78	30.18	

60 MTBE						CAS #: 1634-04-4			
11.452	11.452	(0.826)	73	2631922	50.0000	57.345	80.00- 120.00	100.00	
11.452	11.452	(0.826)	57	489079			0.00- 68.58	18.58	
11.452	11.452	(0.826)	41	474112			0.00- 70.94	18.01	

61 trans-1,2-Dichloroethene						CAS #: 156-60-5			
11.563	11.563	(0.834)	96	902306	50.0000	54.310	80.00- 120.00	100.00	
11.535	11.535	(0.832)	61	1235705			86.95- 186.95	136.95	
11.563	11.563	(0.834)	98	585255			15.85- 115.85	64.86	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
65 Hexane						CAS #: 110-54-3			
11.895	11.895	(0.858)	57	1310950	50.0000	56.832	80.00- 120.00	100.00	
11.895	11.895	(0.858)	43	750630			8.15- 108.15	57.26	
11.895	11.895	(0.858)	86	247373			0.00- 69.59	18.87	

69 Vinyl Acetate						CAS #: 108-05-4			
12.365	12.365	(0.892)	86	237177	50.0000	57.619	80.00- 120.00	100.00	
12.365	12.365	(0.892)	43	2061006			903.58-1003.58	868.97	

70 1,1-Dichloroethane						CAS #: 75-34-3			
12.365	12.365	(0.892)	63	1636313	50.0000	56.469	80.00- 120.00	100.00	
12.365	12.365	(0.892)	65	532741			0.00- 82.56	32.56	

75 2-Butanone						CAS #: 78-93-3			
13.388	13.388	(0.966)	72	459184	50.0000	59.866	80.00- 120.00	100.00	
13.388	13.388	(0.966)	43	1459792			267.91- 367.91	317.91	
13.388	13.388	(0.966)	57	130061			0.00- 78.78	28.32	

76 cis-1,2-Dichloroethene						CAS #: 156-59-2			
13.415	13.415	(0.968)	61	1124304	50.0000	55.246	80.00- 120.00	100.00	
13.415	13.415	(0.968)	96	922567			32.06- 132.06	82.06	
13.415	13.415	(0.968)	98	585970			2.12- 102.12	52.12	

80 Tetrahydrofuran						CAS #: 109-99-9			
13.858	13.858	(1.000)	42	719446	50.0000	58.860	80.00- 120.00	100.00	
13.858	13.858	(1.000)	71	399206			5.49- 105.49	55.49	
13.858	13.858	(1.000)	72	426036			8.31- 108.31	59.22	

82 Chloroform						CAS #: 67-66-3			
13.941	13.941	(1.006)	83	2034581	50.0000	60.006	80.00- 120.00	100.00	
13.941	13.941	(1.006)	85	1333960			15.56- 115.56	65.56	

83 1,1,1-Trichloroethane						CAS #: 71-55-6			
14.273	14.273	(1.030)	97	2242211	50.0000	55.221	80.00- 120.00	100.00	
14.273	14.273	(1.030)	99	1441590			14.29- 114.29	64.29	

85 Cyclohexane						CAS #: 110-82-7			
14.300	14.300	(1.032)	84	1194512	50.0000	57.644	80.00- 120.00	100.00	
14.300	14.300	(1.032)	56	1127927			44.43- 144.43	94.43	
14.300	14.300	(1.032)	41	578614			0.00- 98.44	48.44	

87 Carbon Tetrachloride						CAS #: 56-23-5			
14.549	14.549	(1.050)	119	2198342	50.0000	55.586	80.00- 120.00	100.00	
14.549	14.549	(1.050)	117	2336314			56.28- 156.28	106.28	

91 Benzene						CAS #: 71-43-2			
14.964	14.964	(0.958)	78	2635930	50.0000	55.825	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 Benzene (continued)									
14.964	14.964	(0.958)	77	593809			0.00- 73.32	22.53	

89 2,2,4-Trimethylpentane CAS #: 540-84-1									
14.881	14.881	(1.074)	57	3325101	50.0000	57.541	80.00- 120.00	100.00	
14.881	14.881	(1.074)	56	1059732			0.00- 83.27	31.87	
14.881	14.881	(1.074)	41	831921			0.00- 77.74	25.02	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.074	15.074	(0.965)	62	1286496	50.0000	54.547	80.00- 120.00	100.00	
15.074	15.074	(0.965)	64	417784			0.00- 82.87	32.47	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	854877	50.0000	56.996	80.00- 120.00	100.00	
15.185	15.185	(0.972)	43	1093335			77.61- 177.61	127.89	
15.185	15.185	(0.972)	57	666503			32.99- 132.99	77.96	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	1194942	50.0000	54.769	80.00- 120.00	100.00	
16.097	16.097	(1.030)	130	1138948			45.31- 145.31	95.31	
16.070	16.070	(1.028)	97	767823			14.26- 114.26	64.26	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.567	16.567	(1.060)	63	887372	50.0000	56.239	80.00- 120.00	100.00	
16.567	16.567	(1.060)	62	630220			21.02- 121.02	71.02	
16.567	16.567	(1.060)	41	472758			3.28- 103.28	53.28	

106 1,4-Dioxane CAS #: 123-91-1									
16.706	16.706	(1.069)	88	652676	50.0000	52.160	80.00- 120.00	100.00	
16.678	16.678	(1.067)	58	358152			4.87- 104.87	54.87	
16.678	16.678	(1.067)	57	124748			0.00- 69.86	19.11	

107 Bromodichloromethane CAS #: 75-27-4									
16.982	16.982	(1.087)	83	2108983	50.0000	55.573	80.00- 120.00	100.00	
16.982	16.982	(1.087)	85	1368522			14.89- 114.89	64.89	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	1456319	50.0000	57.309	80.00- 120.00	100.00	
17.784	17.784	(1.138)	77	468364			0.00- 82.16	32.16	
17.784	17.784	(1.138)	39	603250			0.00- 91.42	41.42	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.978	17.978	(1.150)	58	685682	50.0000	59.304	80.00- 120.00	100.00	
17.978	17.978	(1.150)	43	1495261			168.02- 268.02	218.07	
17.978	17.978	(1.150)	85	362745			2.69- 102.69	52.90	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	3082954	50.0000	54.127	80.00- 120.00	100.00	
18.337	18.337	(1.173)	92	1881001			11.01- 111.01	61.01	

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	1625459	50.0000	58.107	80.00- 120.00	100.00	
18.752	18.752	(0.902)	77	512060			0.00- 81.50	31.50	
18.752	18.752	(0.902)	39	623130			0.00- 88.34	38.34	

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.111	(0.919)	97	1168508	50.0000	57.588	80.00- 120.00	100.00	
19.111	19.111	(0.919)	99	733041			12.73- 112.73	62.73	
19.111	19.111	(0.919)	83	970540			33.06- 133.06	83.06	

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	1583839	50.0000	56.008	80.00- 120.00	100.00	
19.277	19.277	(0.927)	129	1111891			20.20- 120.20	70.20	
19.277	19.277	(0.927)	131	1056147			16.68- 116.68	66.68	

121 2-Hexanone						CAS #: 591-78-6			
19.415	19.415	(0.934)	58	945435	50.0000	56.916	80.00- 120.00	100.00	
19.415	19.415	(0.934)	43	1556583			114.64- 214.64	164.64	
19.415	19.415	(0.934)	100	216547			0.00- 74.50	22.90	

122 Dibromochloromethane						CAS #: 124-48-1			
19.802	19.802	(0.952)	129	2074833	50.0000	58.173	80.00- 120.00	100.00	
19.802	19.802	(0.952)	127	1594727			25.33- 125.33	76.86	

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.051	20.051	(0.964)	107	1948890	50.0000	57.092	80.00- 120.00	100.00	
20.051	20.051	(0.964)	109	1807854			42.76- 142.76	92.76	

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.853	(1.003)	112	2708027	50.0000	54.951	80.00- 120.00	100.00	
20.853	20.853	(1.003)	114	854936			0.00- 81.57	31.57	
20.853	20.853	(1.003)	77	1608685			9.40- 109.40	59.40	

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	1433357	50.0000	57.429	80.00- 120.00	100.00	
20.936	20.936	(1.007)	91	4507460			266.56- 366.56	314.47	

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	1811619	50.0000	59.010	80.00- 120.00	100.00	
21.130	21.130	(1.016)	91	3573510			157.11- 257.11	197.26	

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	1697530	50.0000	58.865	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	3528058			157.83- 257.83	207.83	

131 Styrene CAS #: 100-42-5									
21.876	21.876	(1.052)	104	2769832	50.0000	59.270	80.00- 120.00	100.00	
21.876	21.876	(1.052)	78	1391335			0.23- 100.23	50.23	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	2137893	50.0000	57.500	80.00- 120.00	100.00	
22.291	22.291	(1.072)	171	1089642			0.97- 100.97	50.97	

134 Cumene CAS #: 98-82-8									
22.429	22.429	(1.078)	105	4745185	50.0000	57.567	80.00- 120.00	100.00	
22.429	22.429	(1.078)	120	1246050			0.00- 74.52	26.26	
22.429	22.429	(1.078)	51	367539			51.79- 151.79	7.75	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	2561833	50.0000	56.682	80.00- 120.00	100.00	
23.010	23.010	(1.106)	85	1662931			14.91- 114.91	64.91	

142 Propylbenzene CAS #: 103-65-1									
23.120	23.120	(1.112)	91	5915902	50.0000	56.746	80.00- 120.00	100.00	
23.120	23.120	(1.112)	120	1310417			0.00- 71.52	22.15	
23.120	23.120	(1.112)	105	204977			0.00- 53.54	3.46	

145 4-Ethyltoluene CAS #: 622-96-8									
23.286	23.286	(1.120)	105	5122208	50.0000	58.336	80.00- 120.00	100.00	
23.286	23.286	(1.120)	120	1542902			0.00- 80.12	30.12	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	4213554	50.0000	58.966	80.00- 120.00	100.00	
23.397	23.397	(1.125)	120	2054847			0.29- 100.29	48.77	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	3968857	50.0000	59.676	80.00- 120.00	100.00	
24.033	24.033	(1.156)	120	1804573			0.00- 94.69	45.47	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	2794714	50.0000	55.524	80.00- 120.00	100.00	
24.586	24.586	(1.182)	148	1792584			14.61- 114.61	64.14	
24.586	24.586	(1.182)	111	1172086			0.00- 92.01	41.94	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	2898614	50.0000	55.424	80.00- 120.00	100.00	
24.724	24.724	(1.189)	148	1859249			13.83- 113.83	64.14	
24.724	24.724	(1.189)	111	1169424			0.00- 89.75	40.34	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

159	alpha-Chlorotoluene					CAS #: 100-44-7			
24.945	24.945	(1.199)	91	4266491	50.0000	58.955	80.00- 120.00	100.00	
24.945	24.945	(1.199)	126	813802			0.00- 69.65	19.07	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
25.360	25.360	(1.219)	146	2704352	50.0000	56.031	80.00- 120.00	100.00	
25.360	25.360	(1.219)	148	1717775			13.52- 113.52	63.52	
25.360	25.360	(1.219)	111	1172197			0.00- 93.34	43.34	

165	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
28.153	28.153	(1.354)	180	1899522	50.0000	57.376	80.00- 120.00	100.00	
28.153	28.153	(1.354)	182	1802315			44.88- 144.88	94.88	

166	Hexachlorobutadiene					CAS #: 87-68-3			
28.318	28.318	(1.362)	225	1636693	50.0000	54.164	80.00- 120.00	100.00	
28.318	28.318	(1.362)	223	1020467			13.46- 113.46	62.35	

19	Butane					CAS #: 106-97-8			
6.807	6.807	(0.491)	58	145628	50.0000	53.447	80.00- 120.00	100.00	
6.807	6.807	(0.491)	43	991608			640.46- 740.46	680.92	

29	Isopentane					CAS #: 78-78-4			
8.273	8.273	(0.597)	43	786861	50.0000	51.285	80.00- 120.00	100.00	
8.273	8.273	(0.597)	57	622373			26.79- 126.79	79.10	

102	Methyl Cyclohexane					CAS #: 108-87-2			
16.346	16.346	(1.180)	83	1505024	50.0000	57.275	80.00- 120.00	100.00	
16.346	16.346	(1.180)	98	693672			0.00- 95.49	46.09	
16.346	16.346	(1.180)	55	981217			16.76- 116.76	65.20	

167	Naphthalene					CAS #: 91-20-3			
28.678	28.678	(1.379)	128	3254088	50.0000	59.631	80.00- 120.00	100.00	
28.678	28.678	(1.379)	127	395691			0.00- 62.56	12.16	

Report Date: 14-Dec-2007 10:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121314.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	280754	0.00
97 1,4-Difluorobenze	1182601	709561	1655641	1182601	0.00
126 Chlorobenzene-d5	1033655	620193	1447117	1033655	0.00


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

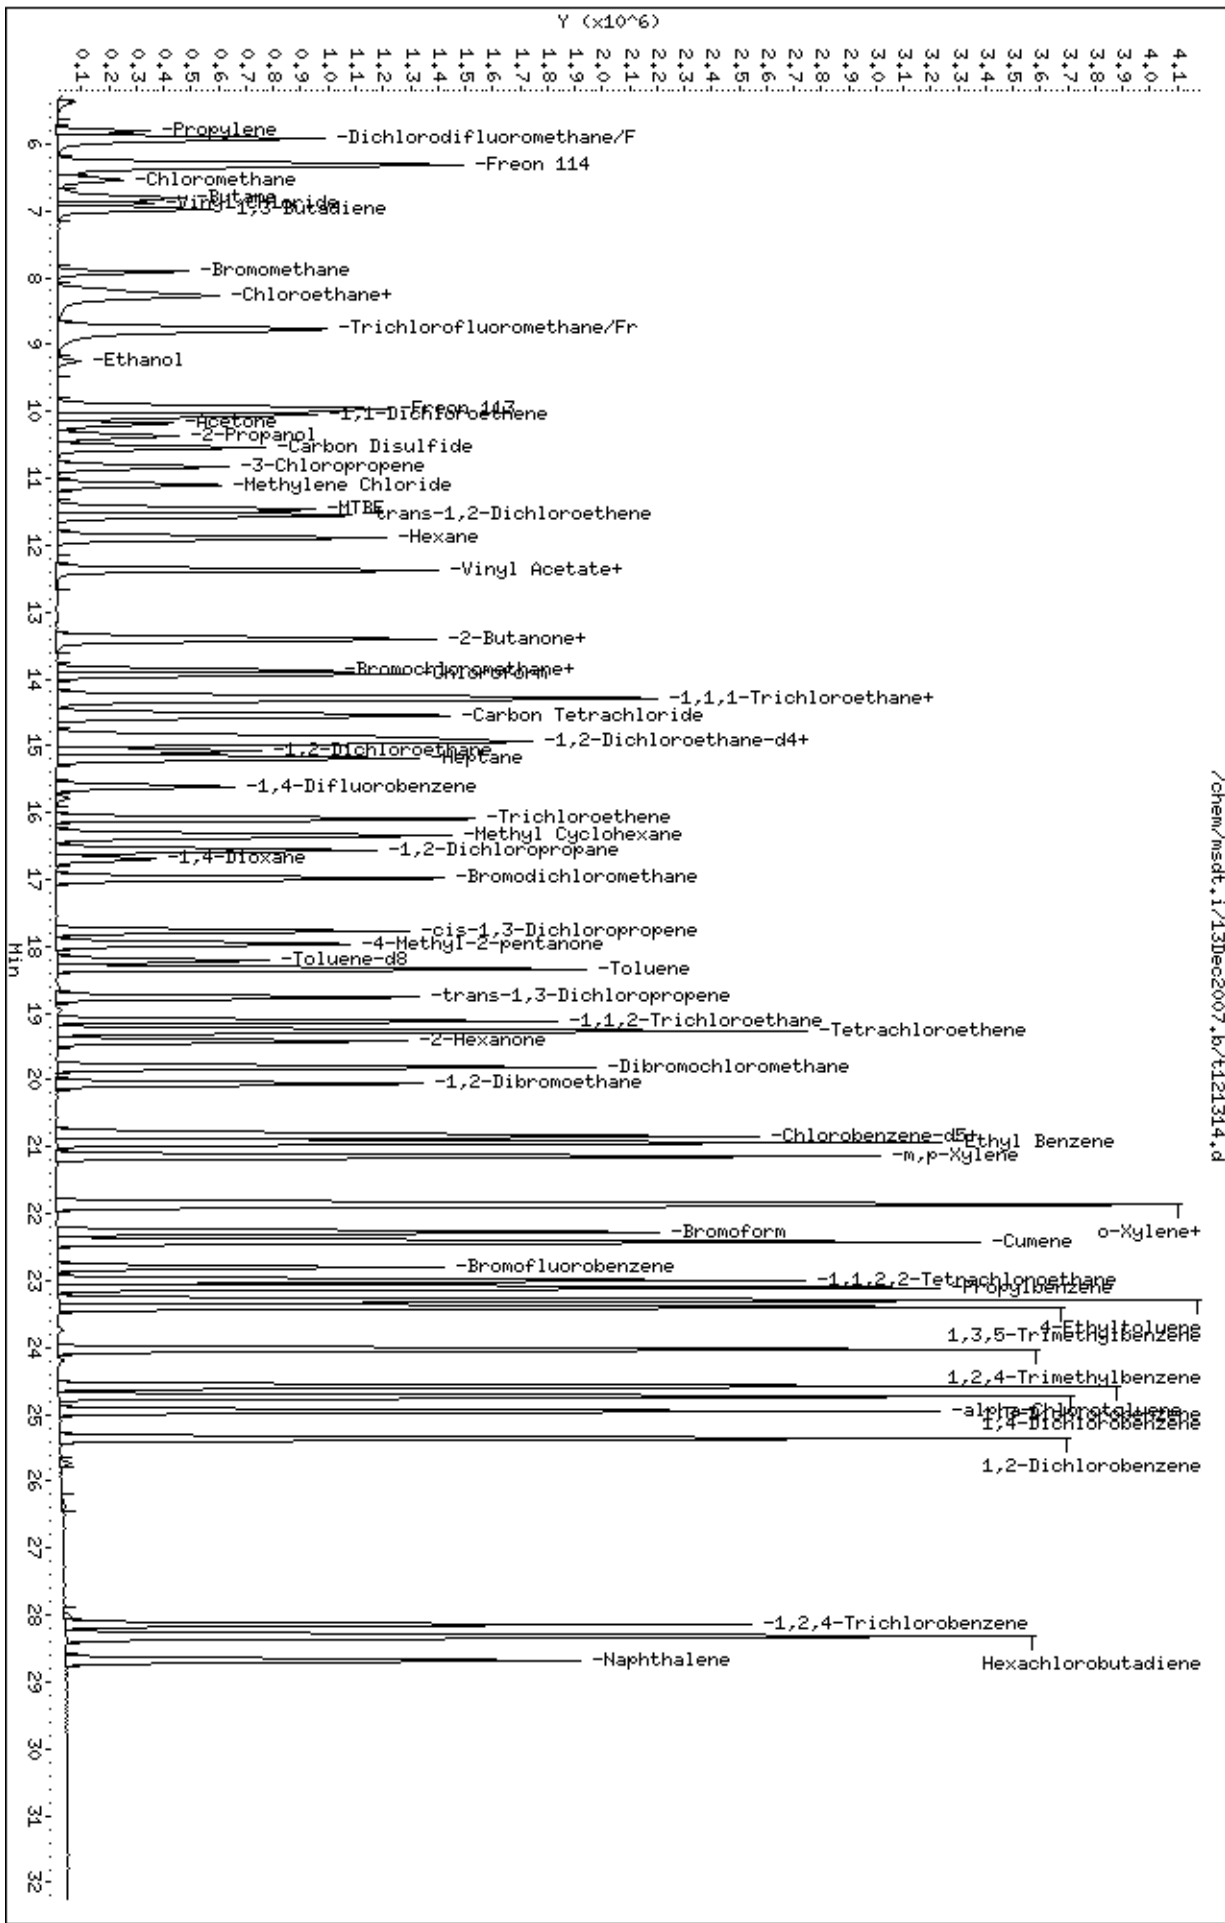

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/16Jan2008.b/t011605.d
 Lab Smp Id: TVH ICAL Client Smp ID: Level 6
 Inj Date : 16-JAN-2008 10:57
 Operator : lo Inst ID: msdt.i
 Smp Info : 100ml #1443-403
 Misc Info : 200ppbv -> 100ppbv
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/t14q1213d.m
 Meth Date : 16-Jan-2008 14:59 lover Quant Type: ISTD
 Cal Date : 16-JAN-2008 10:57 Cal File: t011605.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5d.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	345966	25.0000		50.00- 150.00	100.00	
13.886	13.886	(1.000)	128	253065			27.05- 127.05	73.15	
13.886	13.886	(1.000)	49	382263			61.34- 161.34	110.49	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1279009	25.0000		50.00- 150.00	100.00	
15.628	15.628	(1.000)	88	198610			0.00- 65.73	15.53	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1244720	25.0000		50.00- 150.00	100.00	
20.798	20.798	(1.000)	82	690393			5.94- 105.94	55.47	

204 Propane CAS #: 74-98-6									
5.812	5.812	(0.419)	43	404465	100.000	97.149	50.00- 150.00	100.00	
5.812	5.812	(0.419)	44	436872			107.53- 207.53	108.01	

37 Pentane CAS #: 109-66-0									
8.937	8.937	(0.644)	43	2952324	100.000	97.206	50.00- 150.00	100.00	
8.937	8.937	(0.644)	57	527668			0.00- 67.03	17.87	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
37 Pentane (continued)									
8.937	8.937	(0.644)	72	382651			0.00- 62.09	12.96	

112 Octane									
						CAS #: 111-65-9			
18.282	18.282	(1.170)	57	1796645	100.000	98.478	50.00- 150.00	100.00	
18.282	18.282	(1.170)	85	2465395			82.32- 182.32	137.22	
18.282	18.282	(1.170)	43	3869293			166.39- 266.39	215.36	

124 Nonane									
						CAS #: 111-84-2			
20.964	20.964	(1.008)	43	4113568	100.000	102.87	50.00- 150.00	100.00	
20.964	20.964	(1.008)	57	4242172			52.38- 152.38	103.13	
20.964	20.964	(1.008)	85	1922797			0.00- 95.58	46.74	

139 Decane									
						CAS #: 124-18-5			
23.204	23.204	(1.116)	57	5092622	100.000	106.03	50.00- 150.00	100.00	
23.204	23.204	(1.116)	71	2235651			0.00- 93.78	43.90	
23.204	23.204	(1.116)	142	256663			0.00- 54.94	5.04	

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 16-JAN-2008

Lab File ID: t011605.d

Calibration Time: 13:44

Lab Smp Id: TVH ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lo

Method File: /chem/msdt.i/16Jan2008.b/t14q1213d.m

Misc Info: 200ppbv -> 100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	325810	195486	456134	345966	6.19
97 1,4-Difluorobenze	1168077	700846	1635308	1279009	9.50
126 Chlorobenzene-d5	1103278	661967	1544589	1244720	12.82

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt.i/16Jan2008.b/t011605.d
Date: 16-Jan-2008 10:57
Client ID: Level 6
Sample Info: 100ml #1443-403

Column phase: RTX-624

Instrument: msdt.i
Operator: lo
Column diameter: 0.53

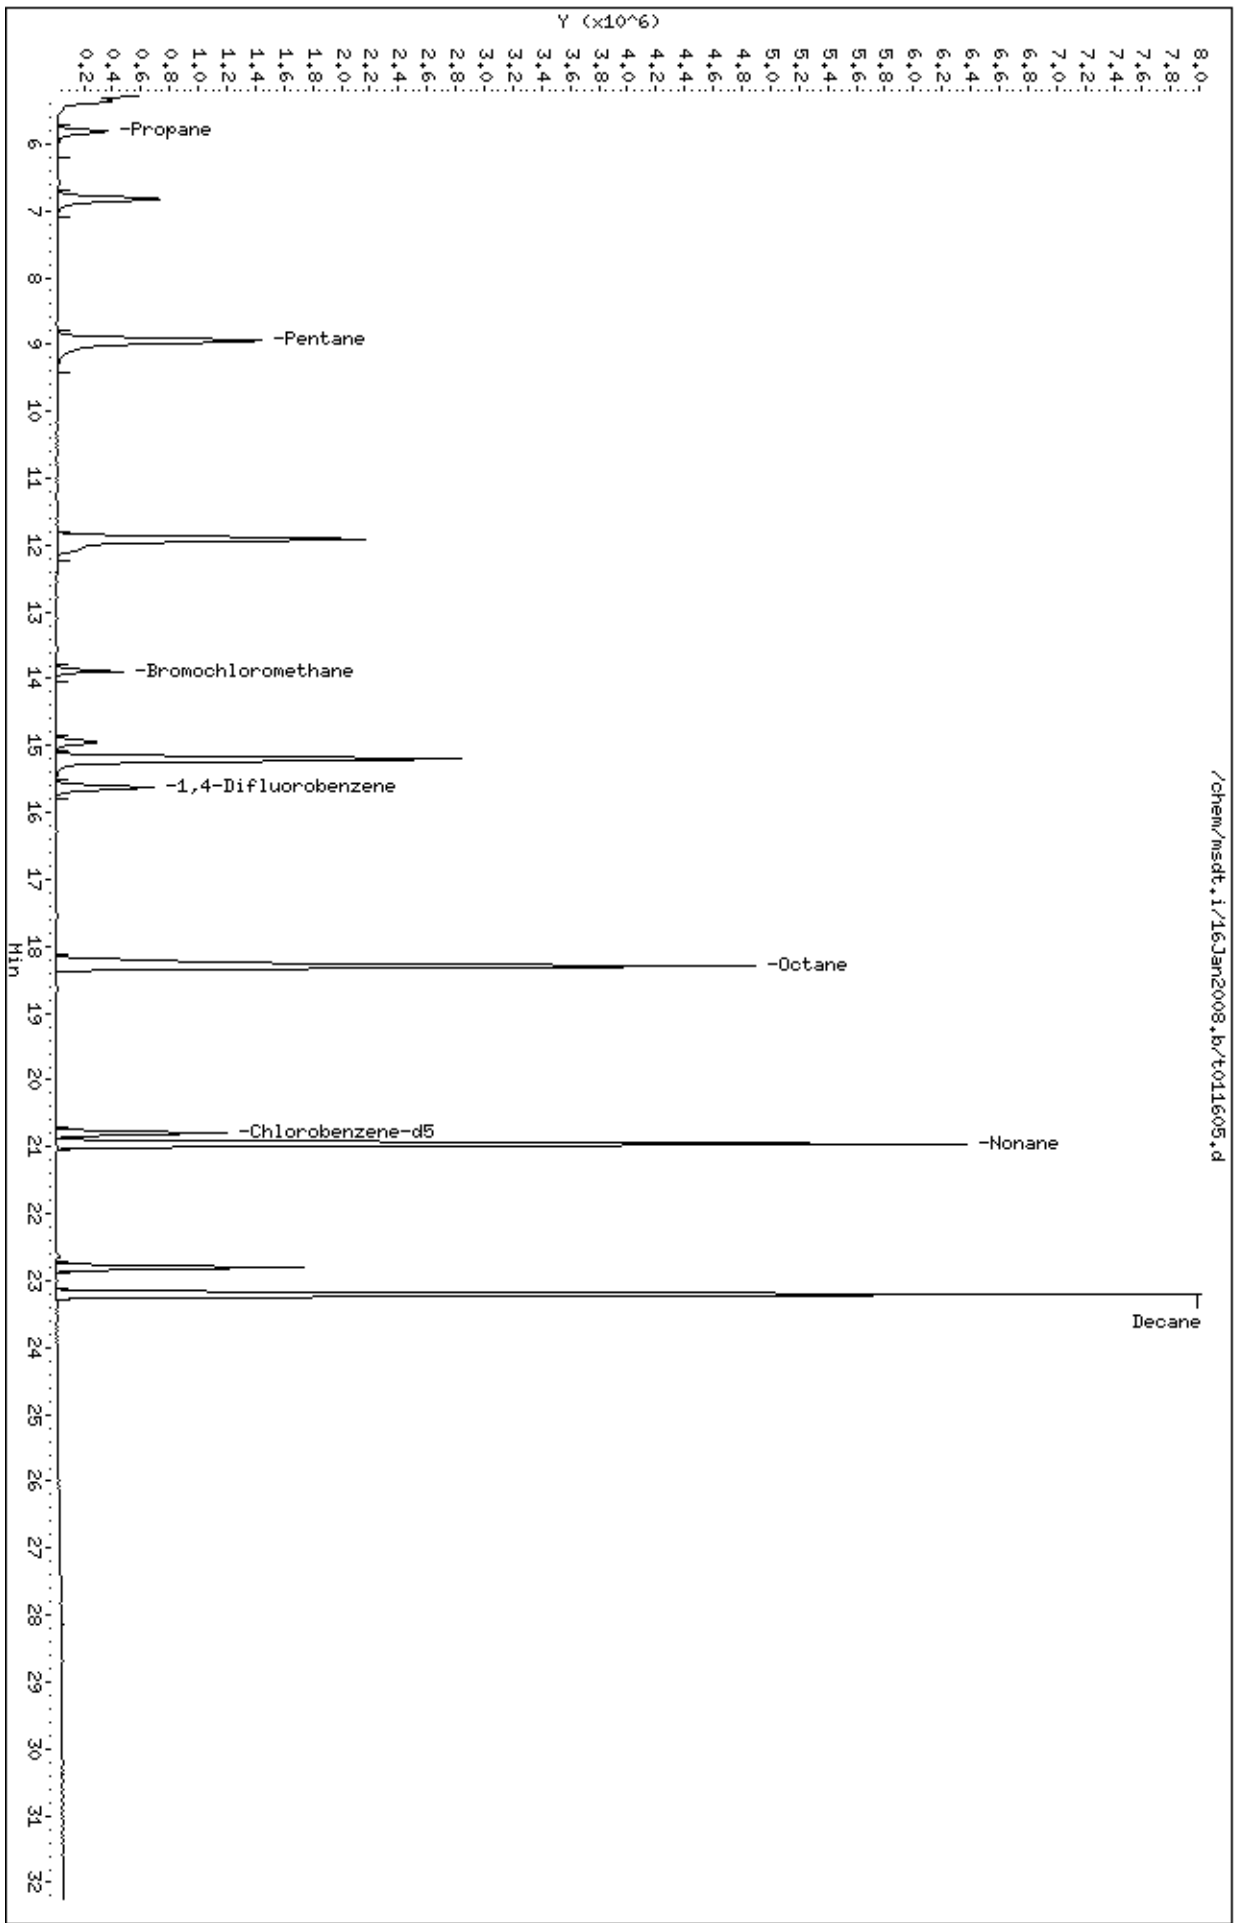

Report Date: 14-Dec-2007 10:41

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121315.d
 Lab Smp Id: ICAL Client Smp ID: Level 5
 Inj Date : 14-DEC-2007 02:20
 Operator : ab Inst ID: msdt.i
 Smp Info : 100mL #1443-378
 Misc Info : 200ppbv -> 100ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 10:41 ealcan Quant Type: ISTD
 Cal Date : 14-DEC-2007 02:20 Cal File: t121315.d
 Als bottle: 1 Calibration Sample, Level: 6
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	285950	25.0000		50.00- 150.00	100.00	
13.886	13.886	(1.000)	128	220525			26.73- 126.73	77.12	
13.858	13.858	(1.000)	49	561636			83.94- 183.94	196.41	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1189157	25.0000		50.00- 150.00	100.00	
15.628	15.628	(1.000)	88	192374			0.00- 65.84	16.18	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1095777	25.0000		50.00- 150.00	100.00	
20.798	20.798	(1.000)	82	594512			5.33- 105.33	54.25	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.076)	65	457177	25.0000	25.111	50.00- 150.00	100.00	
14.936	14.936	(1.076)	67	290358			3.93- 103.93	63.51	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1151984	25.0000	25.537	50.00- 150.00	100.00	
18.199	18.199	(1.165)	70	124410			0.00- 61.06	10.80	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	783583			18.52- 118.52	68.02	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	740649	25.0000	24.644	50.00- 150.00	100.00	
22.789	22.789	(1.096)	95	928797			74.37- 174.37	125.40	
22.789	22.789	(1.096)	176	729017			47.63- 147.63	98.43	

11 Propylene									
						CAS #: 115-07-1			
5.840	5.840	(0.421)	41	724191	100.000	94.827	50.00- 150.00	100.00	
5.840	5.840	(0.421)	42	516660			17.44- 117.44	71.34	
5.840	5.840	(0.421)	39	598885			31.05- 131.05	82.70	

12 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
5.950	5.950	(0.429)	85	5066727	100.000	101.17	50.00- 150.00	100.00	
5.950	5.950	(0.429)	87	1632077			0.00- 82.50	32.21	

16 Freon 114									
						CAS #: 76-14-2			
6.310	6.310	(0.454)	135	3501493	100.000	106.94	50.00- 150.00	100.00	
6.310	6.310	(0.454)	137	1118965			0.00- 81.78	31.96	

18 Chloromethane									
						CAS #: 74-87-3			
6.559	6.559	(0.472)	50	1079673	100.000	99.664	50.00- 150.00	100.00	
6.559	6.559	(0.472)	52	355741			0.00- 83.59	32.95	

20 Vinyl Chloride									
						CAS #: 75-01-4			
6.890	6.890	(0.496)	62	1472383	100.000	108.66	50.00- 150.00	100.00	
6.890	6.890	(0.496)	64	463707			0.00- 94.54	31.49	

22 1,3-Butadiene									
						CAS #: 106-99-0			
6.973	6.973	(0.502)	54	1138899	100.000	107.68	50.00- 150.00	100.00	
6.973	6.973	(0.502)	39	1068848			61.08- 161.08	93.85	

25 Bromomethane									
						CAS #: 74-83-9			
7.941	7.941	(0.572)	94	1543838	100.000	107.59	50.00- 150.00	100.00	
7.941	7.941	(0.572)	96	1447987			44.93- 144.93	93.79	

27 Chloroethane									
						CAS #: 75-00-3			
8.190	8.190	(0.590)	64	792816	100.000	109.66	50.00- 150.00	100.00	
8.190	8.190	(0.590)	49	199260			0.00- 76.61	25.13	
8.190	8.190	(0.590)	66	263973			0.00- 85.87	33.30	

31 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
8.798	8.798	(0.634)	101	5908446	100.000	105.54	50.00- 150.00	100.00	
8.798	8.798	(0.634)	103	3829839			15.72- 115.72	64.82	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Ethanol						CAS #: 64-17-5			
9.241	9.241	(0.665)	45	399210	100.000	105.14	50.00- 150.00	100.00	
9.241	9.241	(0.665)	43	93829			0.00- 74.87	23.50	
9.241	9.241	(0.665)	46	147777			0.00- 88.05	37.02	

42 Freon 113						CAS #: 76-13-1			
9.960	9.960	(0.717)	151	2637753	100.000	104.69	50.00- 150.00	100.00	
9.960	9.960	(0.717)	153	1670440			15.26- 115.26	63.33	
9.960	9.960	(0.717)	101	3421241			81.18- 181.18	129.70	

43 1,1-Dichloroethene						CAS #: 75-35-4			
10.042	10.042	(0.723)	61	2405391	100.000	108.92	50.00- 150.00	100.00	
10.042	10.042	(0.723)	96	1531560			16.16- 116.16	63.67	
10.042	10.042	(0.723)	98	983285			0.00- 91.50	40.88	

45 Acetone						CAS #: 67-64-1			
10.208	10.208	(0.735)	58	682138	100.000	99.480	50.00- 150.00	100.00	
10.208	10.208	(0.735)	43	2077971			264.94- 364.94	304.63	

46 2-Propanol						CAS #: 67-63-0			
10.374	10.374	(0.747)	45	2347871	100.000	103.36	50.00- 150.00	100.00	
10.374	10.374	(0.747)	43	545939			0.00- 78.96	23.25	
10.374	10.374	(0.747)	59	100787			0.00- 54.05	4.29	

47 Carbon Disulfide						CAS #: 75-15-0			
10.540	10.540	(0.759)	76	4617349	100.000	109.66	50.00- 150.00	100.00	

51 3-Chloropropene						CAS #: 107-05-1			
10.817	10.817	(0.779)	76	769367	100.000	107.06	50.00- 150.00	100.00	
10.817	10.817	(0.779)	41	1586728			176.05- 276.05	206.24	

54 Methylene Chloride						CAS #: 75-09-2			
11.121	11.121	(0.801)	49	1356272	100.000	97.250	50.00- 150.00	100.00	
11.121	11.121	(0.801)	84	1323374			44.80- 144.80	97.57	
11.121	11.121	(0.801)	51	436381			0.00- 83.78	32.18	

60 MTBE						CAS #: 1634-04-4			
11.453	11.453	(0.825)	73	5299544	100.000	113.37	50.00- 150.00	100.00	
11.453	11.453	(0.825)	57	975878			0.00- 69.37	18.41	
11.453	11.453	(0.825)	41	906604			0.00- 70.94	17.11	

61 trans-1,2-Dichloroethene						CAS #: 156-60-5			
11.563	11.563	(0.833)	96	1814819	100.000	107.25	50.00- 150.00	100.00	
11.563	11.563	(0.833)	61	2417703			84.61- 184.61	133.22	
11.563	11.563	(0.833)	98	1166471			15.85- 115.85	64.27	

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
65 Hexane						CAS #:	110-54-3	
11.895	11.895	(0.857)	57	2616166	100.000	111.35	50.00- 150.00	100.00
11.895	11.895	(0.857)	43	1438222			8.15- 108.15	54.97
11.895	11.895	(0.857)	86	492697			0.00- 69.59	18.83

69 Vinyl Acetate						CAS #:	108-05-4	
12.365	12.365	(0.890)	86	470953	100.000	112.33	50.00- 150.00	100.00
12.365	12.365	(0.890)	43	4009258			903.58-1003.58	851.31

70 1,1-Dichloroethane						CAS #:	75-34-3	
12.393	12.393	(0.892)	63	3215973	100.000	108.97	50.00- 150.00	100.00
12.393	12.393	(0.892)	65	1034766			0.00- 83.37	32.18

75 2-Butanone						CAS #:	78-93-3	
13.388	13.388	(0.964)	72	917876	100.000	117.49	50.00- 150.00	100.00
13.388	13.388	(0.964)	43	2834828			271.22- 371.22	308.85
13.388	13.388	(0.964)	57	260683			0.00- 78.78	28.40

76 cis-1,2-Dichloroethene						CAS #:	156-59-2	
13.416	13.416	(0.966)	61	2157750	100.000	104.10	50.00- 150.00	100.00
13.416	13.416	(0.966)	96	1808427			29.23- 129.23	83.81
13.416	13.416	(0.966)	98	1161688			0.16- 100.16	53.84

80 Tetrahydrofuran						CAS #:	109-99-9	
13.858	13.858	(0.998)	42	1396529	100.000	112.18	50.00- 150.00	100.00
13.858	13.858	(0.998)	71	774983			0.61- 100.61	55.49
13.858	13.858	(0.998)	72	847199			8.31- 108.31	60.66

82 Chloroform						CAS #:	67-66-3	
13.941	13.941	(1.004)	83	3949977	100.000	114.38	50.00- 150.00	100.00
13.941	13.941	(1.004)	85	2573976			18.46- 118.46	65.16

83 1,1,1-Trichloroethane						CAS #:	71-55-6	
14.273	14.273	(1.028)	97	4466230	100.000	107.99	50.00- 150.00	100.00
14.273	14.273	(1.028)	99	2898803			13.89- 113.89	64.90

85 Cyclohexane						CAS #:	110-82-7	
14.300	14.300	(1.030)	84	2434590	100.000	115.35	50.00- 150.00	100.00
14.300	14.300	(1.030)	56	2279859			43.75- 143.75	93.64
14.300	14.300	(1.030)	41	1142321			1.66- 101.66	46.92

87 Carbon Tetrachloride						CAS #:	56-23-5	
14.549	14.549	(1.048)	119	4331306	100.000	107.53	50.00- 150.00	100.00
14.549	14.549	(1.048)	117	4610539			54.19- 154.19	106.45

91 Benzene						CAS #:	71-43-2	
14.964	14.964	(0.958)	78	5280134	100.000	111.21	50.00- 150.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 Benzene (continued)									
14.964	14.964	(0.958)	77	1196818			0.00- 73.32	22.67	

89 2,2,4-Trimethylpentane CAS #: 540-84-1									
14.881	14.881	(1.072)	57	6656939	100.000	113.10	50.00- 150.00	100.00	
14.881	14.881	(1.072)	56	2142057			0.00- 83.27	32.18	
14.881	14.881	(1.072)	41	1647005			0.00- 77.74	24.74	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.075	15.075	(0.965)	62	2478887	100.000	104.52	50.00- 150.00	100.00	
15.075	15.075	(0.965)	64	804644			0.00- 82.87	32.46	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	1677297	100.000	111.21	50.00- 150.00	100.00	
15.185	15.185	(0.972)	43	2124729			77.61- 177.61	126.68	
15.185	15.185	(0.972)	57	1333886			32.99- 132.99	79.53	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	2425463	100.000	110.56	50.00- 150.00	100.00	
16.098	16.098	(1.030)	130	2226060			45.55- 145.55	91.78	
16.070	16.070	(1.028)	97	1551198			15.22- 115.22	63.95	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.568	16.568	(1.060)	63	1758972	100.000	110.86	50.00- 150.00	100.00	
16.568	16.568	(1.060)	62	1266741			23.00- 123.00	72.02	
16.568	16.568	(1.060)	41	917277			8.64- 108.64	52.15	

106 1,4-Dioxane CAS #: 123-91-1									
16.678	16.678	(1.067)	88	1329351	100.000	105.65	50.00- 150.00	100.00	
16.678	16.678	(1.067)	58	717333			5.85- 105.85	53.96	
16.678	16.678	(1.067)	57	243463			0.00- 69.86	18.31	

107 Bromodichloromethane CAS #: 75-27-4									
16.982	16.982	(1.087)	83	4204975	100.000	110.19	50.00- 150.00	100.00	
16.982	16.982	(1.087)	85	2713802			16.51- 116.51	64.54	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	2953715	100.000	115.59	50.00- 150.00	100.00	
17.784	17.784	(1.138)	77	950984			0.00- 83.76	32.20	
17.784	17.784	(1.138)	39	1202923			0.00- 94.73	40.73	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.978	17.978	(1.150)	58	1406724	100.000	121.00	50.00- 150.00	100.00	
17.950	17.950	(1.149)	43	3070799			168.02- 268.02	218.29	
17.978	17.978	(1.150)	85	739817			2.69- 102.69	52.59	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	6251105	100.000	109.14	50.00- 150.00	100.00	
18.337	18.337	(1.173)	92	3804780			9.70- 109.70	60.87	

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	3262320	100.000	110.01	50.00- 150.00	100.00	
18.752	18.752	(0.902)	77	1035660			0.00- 82.23	31.75	
18.752	18.752	(0.902)	39	1217213			0.00- 88.37	37.31	

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.111	(0.919)	97	2324244	100.000	108.05	50.00- 150.00	100.00	
19.111	19.111	(0.919)	99	1478232			15.96- 115.96	63.60	
19.111	19.111	(0.919)	83	1934175			36.03- 136.03	83.22	

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	3155738	100.000	105.27	50.00- 150.00	100.00	
19.277	19.277	(0.927)	129	2191062			20.82- 120.82	69.43	
19.277	19.277	(0.927)	131	2092982			18.42- 118.42	66.32	

121 2-Hexanone						CAS #: 591-78-6			
19.416	19.416	(0.934)	58	1987055	100.000	112.84	50.00- 150.00	100.00	
19.416	19.416	(0.934)	43	3164314			120.66- 220.66	159.25	
19.416	19.416	(0.934)	100	463660			0.00- 74.50	23.33	

122 Dibromochloromethane						CAS #: 124-48-1			
19.803	19.803	(0.952)	129	4155741	100.000	109.91	50.00- 150.00	100.00	
19.803	19.803	(0.952)	127	3199761			25.33- 125.33	77.00	

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.052	20.052	(0.964)	107	3955303	100.000	109.30	50.00- 150.00	100.00	
20.052	20.052	(0.964)	109	3667501			41.12- 141.12	92.72	

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.853	(1.003)	112	5575117	100.000	106.72	50.00- 150.00	100.00	
20.853	20.853	(1.003)	114	1741170			0.00- 80.99	31.23	
20.853	20.853	(1.003)	77	3312976			25.73- 125.73	59.42	

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	2944411	100.000	111.28	50.00- 150.00	100.00	
20.936	20.936	(1.007)	91	9385002			266.56- 366.56	318.74	

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	3786212	100.000	116.34	50.00- 150.00	100.00	
21.130	21.130	(1.016)	91	7546980			157.11- 257.11	199.33	

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	3551995	100.000	116.19	50.00- 150.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	7434607			166.77- 266.77	209.31	

131 Styrene CAS #: 100-42-5									
21.876	21.876	(1.052)	104	5914203	100.000	119.38	50.00- 150.00	100.00	
21.876	21.876	(1.052)	78	2949426			12.82- 112.82	49.87	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	4481325	100.000	113.69	50.00- 150.00	100.00	
22.291	22.291	(1.072)	171	2295005			0.34- 100.34	51.21	

134 Cumene CAS #: 98-82-8									
22.429	22.429	(1.078)	105	9947717	100.000	113.84	50.00- 150.00	100.00	
22.429	22.429	(1.078)	120	2551560			0.00- 74.52	25.65	
22.429	22.429	(1.078)	51	743683			51.79- 151.79	7.48	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	5403373	100.000	112.77	50.00- 150.00	100.00	
23.010	23.010	(1.106)	85	3522540			17.66- 117.66	65.19	

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	12526916	100.000	113.35	50.00- 150.00	100.00	
23.121	23.121	(1.112)	120	2739588			0.00- 71.52	21.87	
23.121	23.121	(1.112)	105	452641			0.00- 53.54	3.61	

145 4-Ethyltoluene CAS #: 622-96-8									
23.287	23.287	(1.120)	105	10857177	100.000	116.64	50.00- 150.00	100.00	
23.287	23.287	(1.120)	120	3211721			0.00- 79.85	29.58	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	8749363	100.000	115.50	50.00- 150.00	100.00	
23.397	23.397	(1.125)	120	4278572			0.29- 100.29	48.90	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	8331110	100.000	118.17	50.00- 150.00	100.00	
24.033	24.033	(1.156)	120	3834206			0.00- 94.69	46.02	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	5901308	100.000	110.60	50.00- 150.00	100.00	
24.586	24.586	(1.182)	148	3753394			14.61- 114.61	63.60	
24.586	24.586	(1.182)	111	2459190			0.00- 92.01	41.67	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	6108963	100.000	110.19	50.00- 150.00	100.00	
24.724	24.724	(1.189)	148	3878518			13.83- 113.83	63.49	
24.724	24.724	(1.189)	111	2438232			0.00- 89.75	39.91	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

159	alpha-Chlorotoluene					CAS #: 100-44-7			
24.946	24.946	(1.199)	91	9240613	100.000	120.45	50.00- 150.00	100.00	
24.946	24.946	(1.199)	126	1772001			0.00- 69.65	19.18	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
25.360	25.360	(1.219)	146	5700776	100.000	111.42	50.00- 150.00	100.00	
25.360	25.360	(1.219)	148	3626695			14.36- 114.36	63.62	
25.360	25.360	(1.219)	111	2473610			0.00- 92.81	43.39	

165	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
28.153	28.153	(1.354)	180	4104037	100.000	116.94	50.00- 150.00	100.00	
28.153	28.153	(1.354)	182	3915717			45.41- 145.41	95.41	

166	Hexachlorobutadiene					CAS #: 87-68-3			
28.319	28.319	(1.362)	225	3552461	100.000	110.90	50.00- 150.00	100.00	
28.319	28.319	(1.362)	223	2207569			13.46- 113.46	62.14	

19	Butane					CAS #: 106-97-8			
6.808	6.808	(0.490)	58	284238	100.000	102.42	50.00- 150.00	100.00	
6.808	6.808	(0.490)	43	1944395			640.46- 740.46	684.07	

29	Isopentane					CAS #: 78-78-4			
8.273	8.273	(0.596)	43	1581328	100.000	101.19	50.00- 150.00	100.00	
8.273	8.273	(0.596)	57	1260063			26.79- 126.79	79.68	

102	Methyl Cyclohexane					CAS #: 108-87-2			
16.347	16.347	(1.177)	83	3058051	100.000	114.26	50.00- 150.00	100.00	
16.347	16.347	(1.177)	98	1404590			0.00- 95.49	45.93	
16.347	16.347	(1.177)	55	1985443			16.76- 116.76	64.93	

167	Naphthalene					CAS #: 91-20-3			
28.678	28.678	(1.379)	128	7020979	100.000	121.36	50.00- 150.00	100.00	
28.678	28.678	(1.379)	127	856788			0.00- 62.56	12.20	

Report Date: 14-Dec-2007 10:41

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121315.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	285950	1.85
97 1,4-Difluorobenze	1182601	709561	1655641	1189157	0.55
126 Chlorobenzene-d5	1033655	620193	1447117	1095777	6.01


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.89	0.20
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

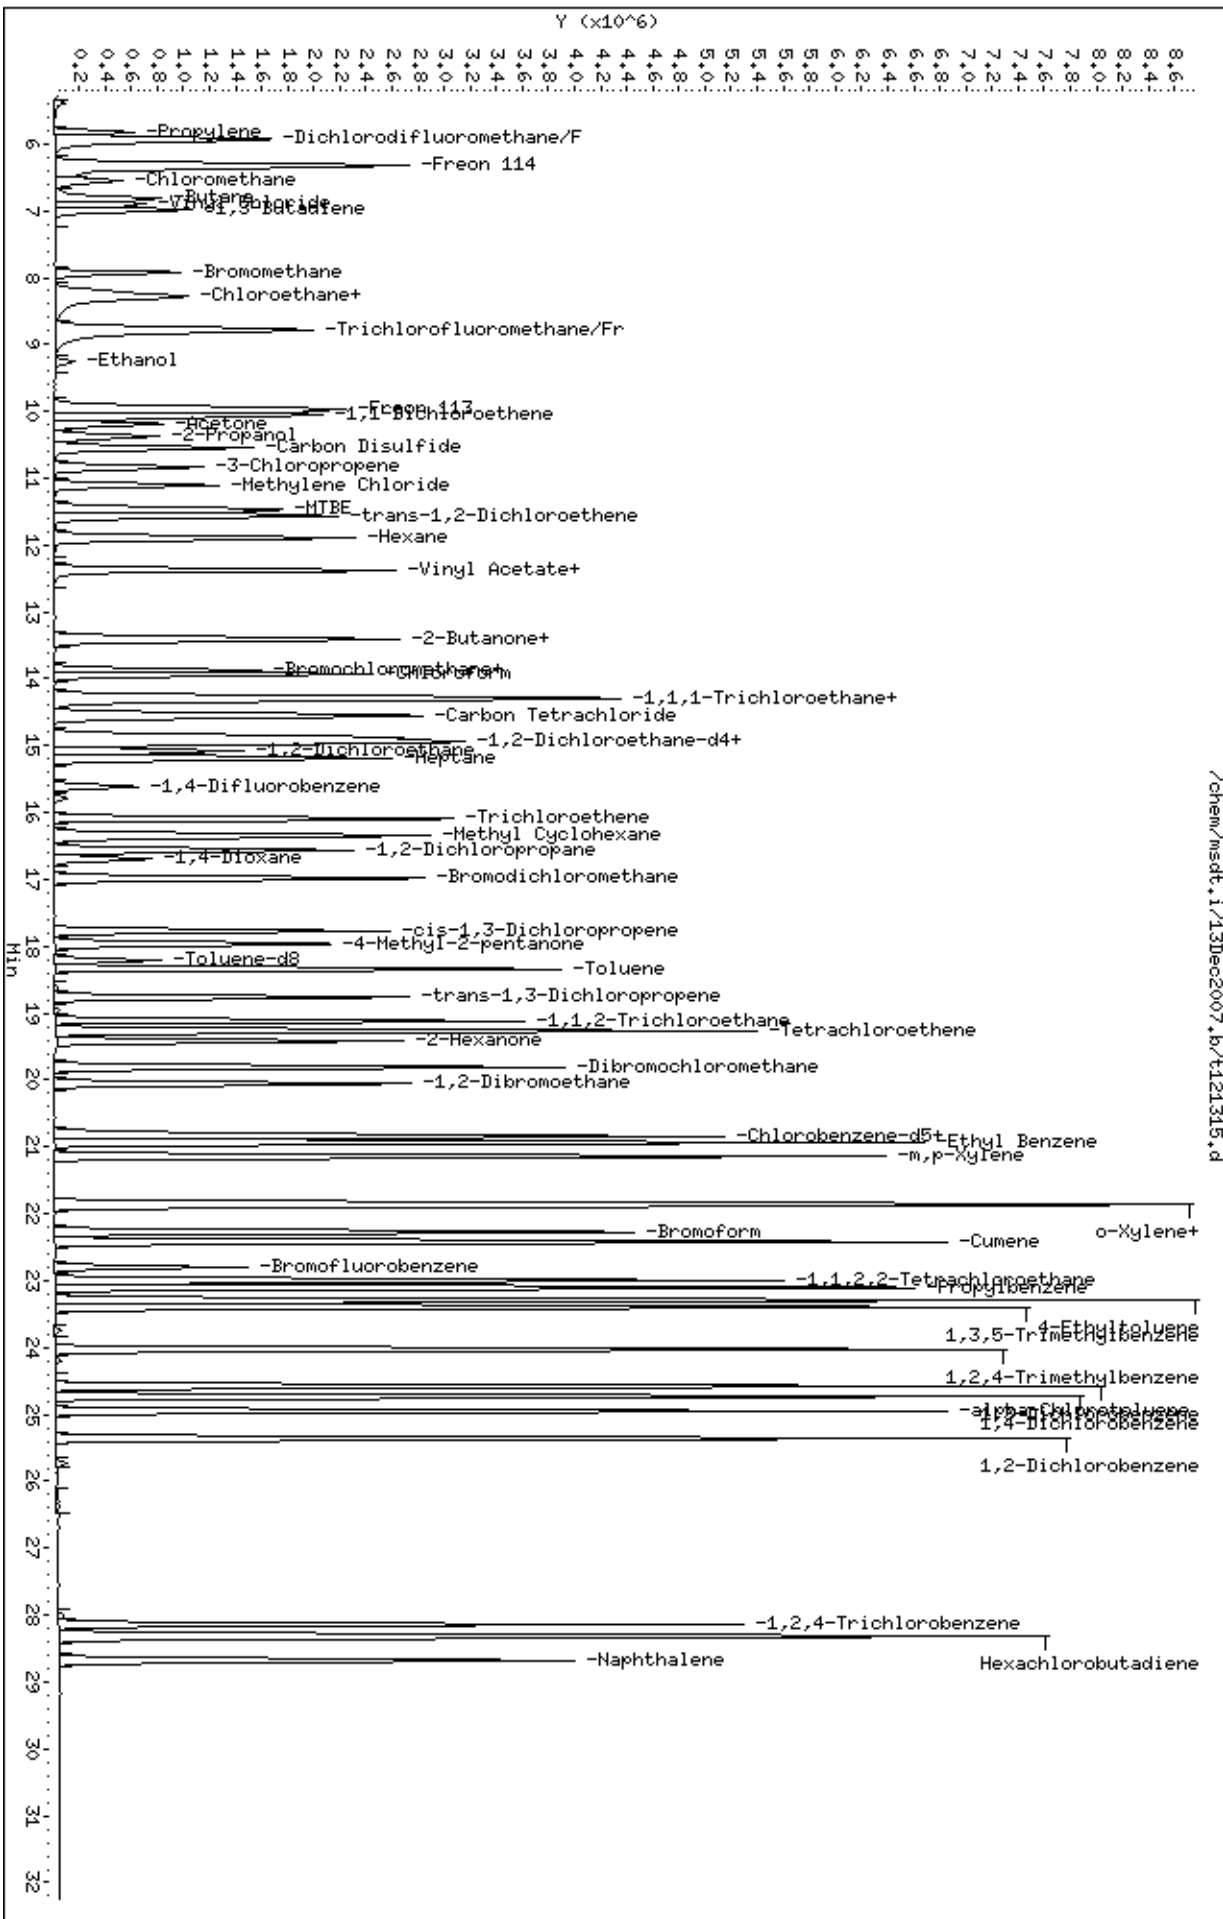

Report Date: 25-Jan-2008 14:48

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/25Jan2008.b/t012506.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 25-JAN-2008 13:09
 Operator : sjr Inst ID: msdt.i
 Smp Info : 200mL #1576-236
 Misc Info : 200ppbv -> 200ppbv
 Comment :
 Method : /chem/msdt.i/25Jan2008.b/t14q1213e.m
 Meth Date : 25-Jan-2008 14:48 sruth Quant Type: ISTD
 Cal Date : 25-JAN-2008 13:09 Cal File: t012506.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp12e.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5								
13.886	13.886	(1.000)	130	325344	25.0000		50.00- 150.00	100.00
13.886	13.886	(1.000)	128	257143			26.42- 126.42	79.04
13.858	13.858	(1.000)	49	353099			58.08- 158.08	108.53

* 97 1,4-Difluorobenzene CAS #: 540-36-3								
15.628	15.628	(1.000)	114	1181826	25.0000		50.00- 150.00	100.00
15.628	15.628	(1.000)	88	186547			0.00- 65.62	15.78

* 126 Chlorobenzene-d5 CAS #: 3114-55-4								
20.798	20.798	(1.000)	117	1178108	25.0000		50.00- 150.00	100.00
20.798	20.798	(1.000)	82	647900			5.74- 105.74	54.99

21 Isobutane CAS #: 75-28-5								
6.365	6.365	(0.458)	43	5236150	200.000	195.15	50.00- 150.00	100.00(A)
6.365	6.365	(0.458)	42	1765051			0.00- 82.88	33.71
6.365	6.365	(0.458)	58	157521			0.00- 52.81	3.01

35 1-Pentene CAS #: 109-67-1								
8.826	8.826	(0.636)	55	3535864	200.000	195.02	50.00- 150.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
35 1-Pentene (continued)									
8.826	8.826	(0.636)	42	3620819			42.09- 142.09	102.40	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

44 Acrolein CAS #: 107-02-8									
9.904	9.904	(0.713)	55	991388	200.000	201.55	50.00- 150.00	100.00	
9.904	9.904	(0.713)	56	1427617			91.89- 191.89	144.00	

48 Ethyl acrylate CAS #: 140-88-5									
16.153	16.153	(1.034)	99	695572	200.000	217.46	50.00- 150.00	100.00(A)	
16.153	16.153	(1.034)	45	619000			41.03- 141.03	88.99	
16.153	16.153	(1.034)	55	7469331			975.70-1075.70	1073.84	

49 Iodomethane CAS #: 74-88-4									
10.429	10.429	(0.751)	142	10389623	200.000	217.72	50.00- 150.00	100.00(A)	
10.429	10.429	(0.751)	127	4694999			0.00- 96.78	45.19	

50 Methyl Methacrylate CAS #: 80-62-6									
16.568	16.568	(1.060)	41	4193478	200.000	215.54	50.00- 150.00	100.00(A)	
16.568	16.568	(1.060)	69	4128331			48.84- 148.84	98.45	
16.568	16.568	(1.060)	100	1679924			0.00- 88.29	40.06	

52 Acetonitrile CAS #: 75-05-8									
10.900	10.900	(0.785)	40	1151183	200.000	156.88	50.00- 150.00	100.00	
10.900	10.900	(0.785)	41	2161847			94.31- 194.31	187.79	
10.900	10.900	(0.785)	38	320062			0.00- 73.26	27.80	

56 Cyclopentane CAS #: 287-92-3									
11.121	11.121	(0.801)	70	2422737	200.000	208.44	50.00- 150.00	100.00(A)	
11.121	11.121	(0.801)	55	2862041			69.79- 169.79	118.13	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

62 Acrylonitrile CAS #: 107-13-1									
11.646	11.646	(0.839)	53	2354411	200.000	200.15	50.00- 150.00	100.00	
11.646	11.646	(0.839)	52	1953819			34.51- 134.51	82.99	

63 2-Pentanone CAS #: 107-87-9									
16.374	16.374	(1.048)	43	7728950	200.000	224.22	50.00- 150.00	100.00(A)	
16.374	16.374	(1.048)	58	705315			0.00- 59.30	9.13	
16.374	16.374	(1.048)	86	1856601			0.00- 74.01	24.02	

66 1-Hexene CAS #: 592-41-6									
11.784	11.784	(0.849)	55	2434512	200.000	225.61	50.00- 150.00	100.00(A)	
11.784	11.784	(0.849)	41	3357938			104.22- 204.22	137.93	
11.784	11.784	(0.849)	84	1158242			5.60- 105.60	47.58	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
105 Dibromomethane						CAS #: 74-95-3			
16.789	16.789	(1.074)	174	4958237	200.000	199.00	50.00- 150.00	100.00	
16.789	16.789	(1.074)	93	5022086			51.33- 151.33	101.29	
16.789	16.789	(1.074)	95	4162966			33.65- 133.65	83.96	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 25-Jan-2008 14:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 25-JAN-2008

Lab File ID: t012506.d

Calibration Time: 12:14

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/25Jan2008.b/t14q1213e.m

Misc Info: 200ppbv -> 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	334161	200497	467825	325344	-2.64
97 1,4-Difluorobenze	1198449	719069	1677829	1181826	-1.39
126 Chlorobenzene-d5	1112878	667727	1558029	1178108	5.86

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/25Jan2008,b/t012506.d

Date : 25-Jan-2008 13:09

Client ID: Level 7

Sample Info: 200mL #1576-236


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/25Jan2008,b/t012506.d

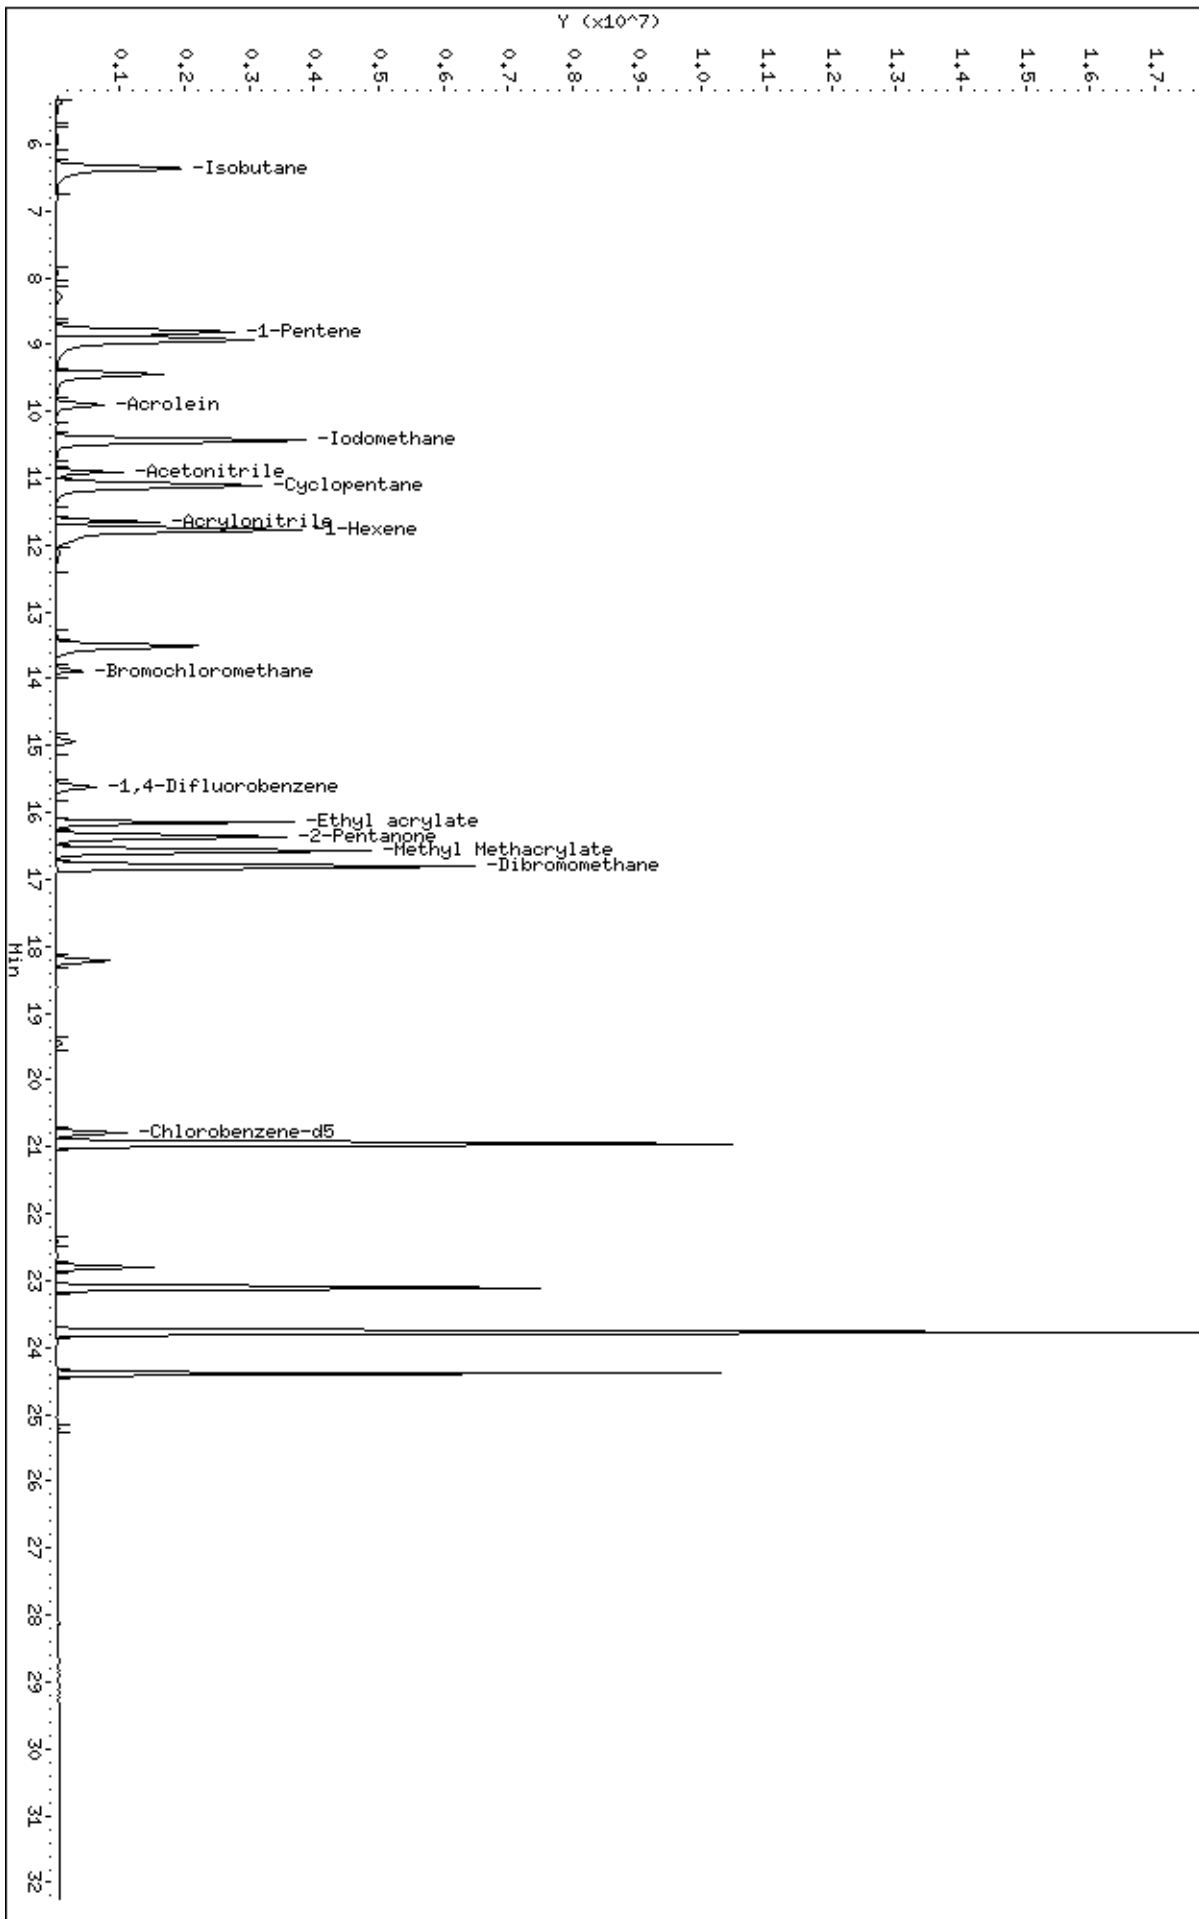

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/16Jan2008.b/t011606.d
 Lab Smp Id: TVH ICAL Client Smp ID: Level 7
 Inj Date : 16-JAN-2008 11:40
 Operator : lo Inst ID: msdt.i
 Smp Info : 200ml #1443-403
 Misc Info : 200ppbv -> 200ppbv
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/t14q1213d.m
 Meth Date : 16-Jan-2008 14:59 lover Quant Type: ISTD
 Cal Date : 16-JAN-2008 11:40 Cal File: t011606.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp5d.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	336026	25.0000		50.00- 150.00	100.00	
13.886	13.886	(1.000)	128	254374			27.05- 127.05	75.70	
13.858	13.858	(1.000)	49	364872			61.34- 161.34	108.58	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1237454	25.0000		50.00- 150.00	100.00	
15.628	15.628	(1.000)	88	195279			0.00- 65.73	15.78	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1248057	25.0000		50.00- 150.00	100.00	
20.798	20.798	(1.000)	82	689894			5.94- 105.94	55.28	

204 Propane CAS #: 74-98-6									
5.812	5.812	(0.419)	43	766807	200.000	189.63	50.00- 150.00	100.00	
5.812	5.812	(0.419)	44	796932			107.53- 207.53	103.93	

37 Pentane CAS #: 109-66-0									
8.909	8.909	(0.642)	43	5501543	200.000	186.50	50.00- 150.00	100.00	
8.937	8.937	(0.644)	57	983125			0.00- 67.03	17.87	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
37 Pentane (continued)									
8.937	8.937	(0.644)	72	711570			0.00- 62.09	12.93	

112 Octane									
						CAS #: 111-65-9			
18.282	18.282	(1.170)	57	3439840	200.000	194.88	50.00- 150.00	100.00	
18.282	18.282	(1.170)	85	4752117			82.32- 182.32	138.15	
18.282	18.282	(1.170)	43	7410802			166.39- 266.39	215.44	

124 Nonane									
						CAS #: 111-84-2			
20.964	20.964	(1.008)	43	8087264	200.000	201.70	50.00- 150.00	100.00	
20.964	20.964	(1.008)	57	8343782			52.38- 152.38	103.17	
20.964	20.964	(1.008)	85	3750913			0.00- 95.58	46.38	

139 Decane									
						CAS #: 124-18-5			
23.204	23.204	(1.116)	57	10257782	200.000	213.00	50.00- 150.00	100.00(A)	
23.204	23.204	(1.116)	71	4469764			0.00- 93.78	43.57	
23.204	23.204	(1.116)	142	525229			0.00- 54.94	5.12	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 16-Jan-2008 14:59

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 16-JAN-2008

Lab File ID: t011606.d

Calibration Time: 13:44

Lab Smp Id: TVH ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lo

Method File: /chem/msdt.i/16Jan2008.b/t14q1213d.m

Misc Info: 200ppbv -> 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	325810	195486	456134	336026	3.14
97 1,4-Difluorobenze	1168077	700846	1635308	1237454	5.94
126 Chlorobenzene-d5	1103278	661967	1544589	1248057	13.12

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/16Jan2008,b/t011606.d

Date : 16-Jan-2008 11:40

Client ID: Level 7


Sample Info: 200ml #1443-403

Column phase: RTX-624

Instrument: msdt,i

Operator: lo

Column diameter: 0.53

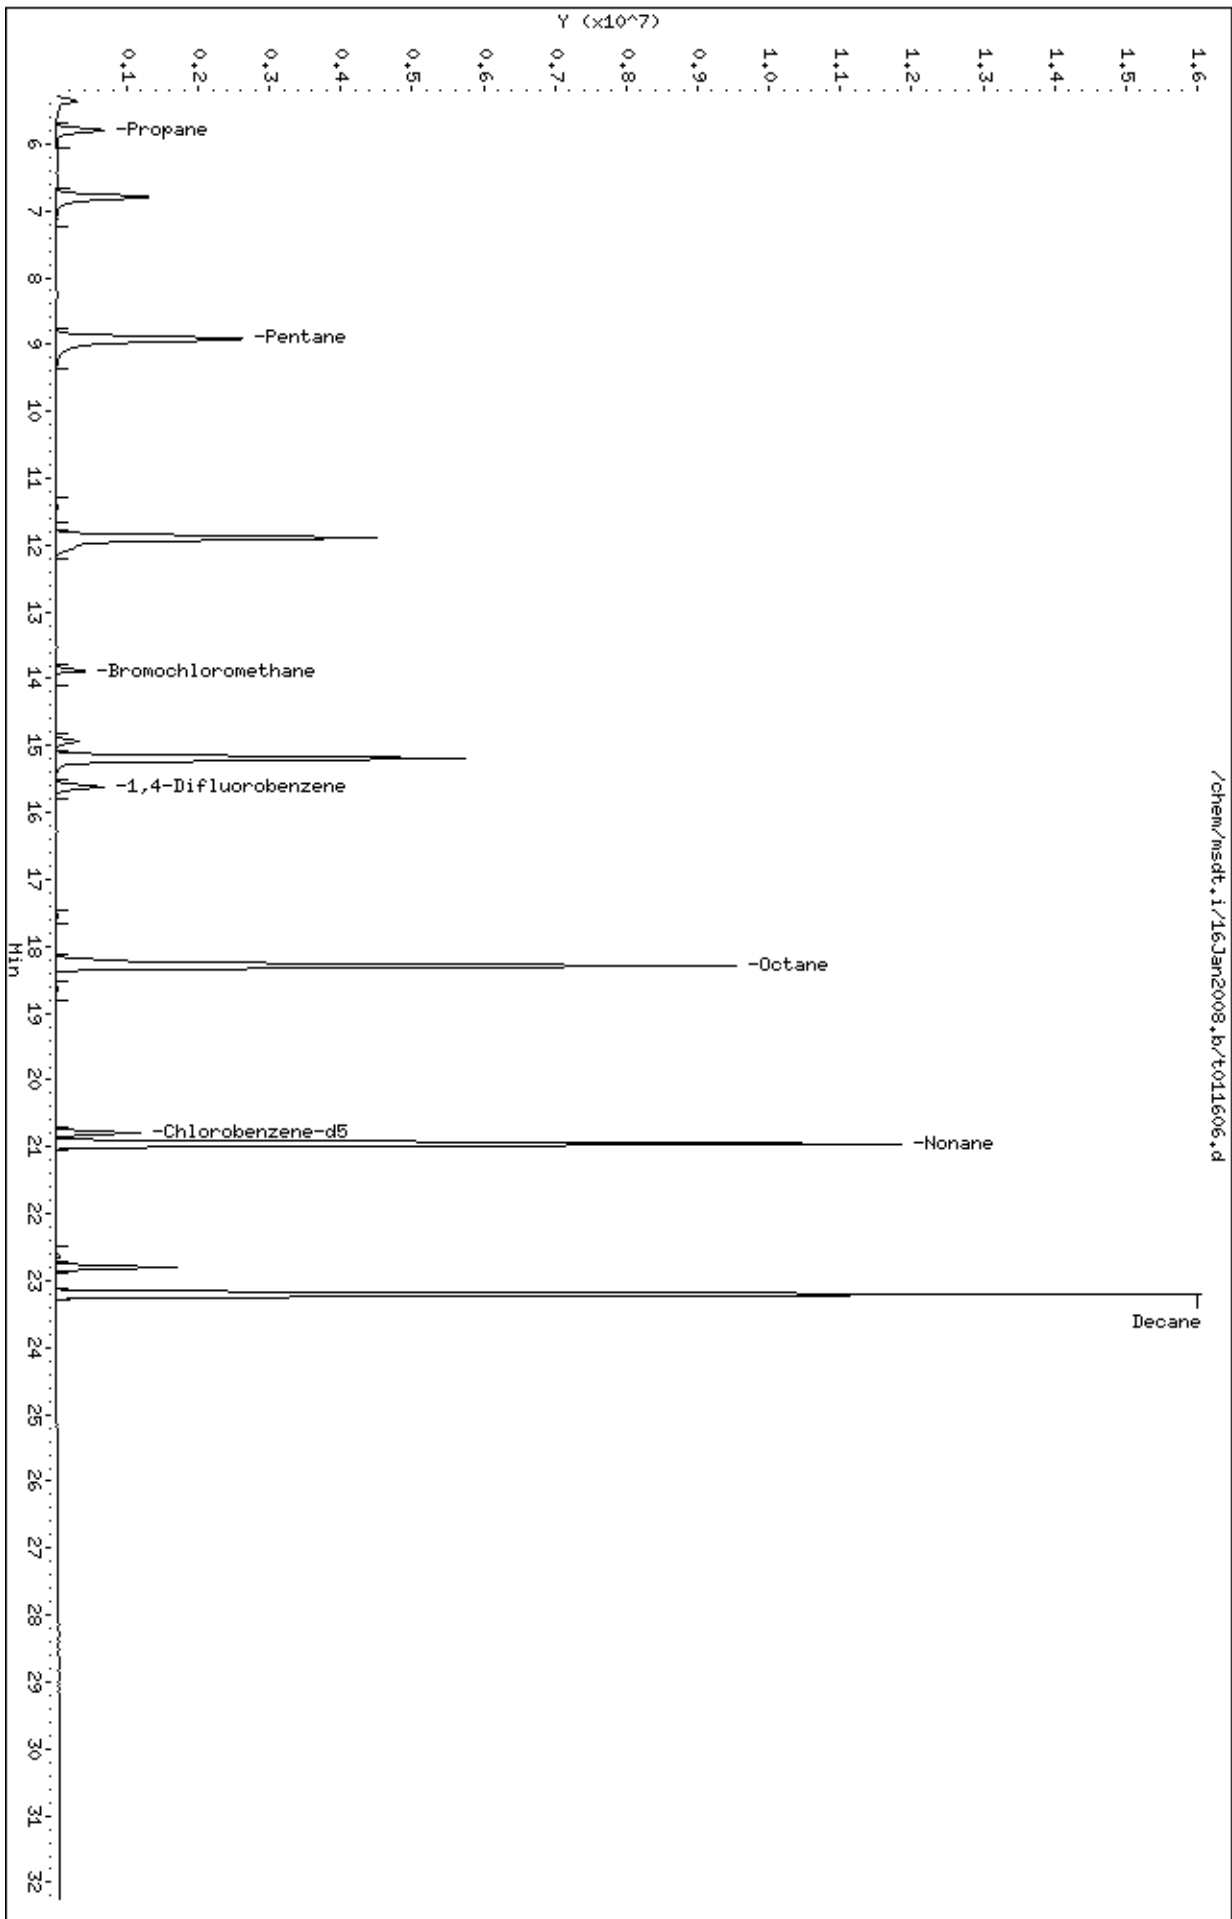

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/02Jan2008.b/t010205.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 02-JAN-2008 12:48
 Operator : sjr Inst ID: msdt.i
 Smp Info : 200ml #1443-399
 Misc Info : 200ppbv -> 200ppbv (1200ppbv MeOH)
 Comment :
 Method : /chem/msdt.i/02Jan2008.b/t14q1213c.m
 Meth Date : 02-Jan-2008 15:47 sruth Quant Type: ISTD
 Cal Date : 02-JAN-2008 12:48 Cal File: t010205.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: sp22c.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.865	13.865	(1.000)	130	342802	25.0000		50.00- 150.00	100.00	
13.865	13.865	(1.000)	128	268144			26.86- 126.86	78.22	
13.865	13.865	(1.000)	49	404262			74.17- 174.17	117.93	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.635	15.635	(1.000)	114	1259545	25.0000		50.00- 150.00	100.00	
15.607	15.607	(1.000)	88	206409			0.00- 66.07	16.39	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.805	20.805	(1.000)	117	1262417	25.0000		50.00- 150.00	100.00	
20.805	20.805	(1.000)	82	725213			5.77- 105.77	57.45	

6 Freon142b CAS #: 75-68-3									
6.407	6.407	(0.462)	65	9025712	200.000	203.76	50.00- 150.00	100.00	
6.407	6.407	(0.462)	45	1781406			0.00- 71.17	19.74	

9 Freon 13 CAS #: 75-72-9									
5.394	5.394	(0.389)	69	9392123	200.000	216.05	50.00- 150.00	100.00(AH)	
5.394	5.394	(0.389)	85	3016168			0.00- 83.23	32.11	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
9 Freon 13 (continued)									
5.394	5.394	(0.389)	87	971094			0.00- 60.80	10.34	

13 Freon 134a CAS #: 811-97-2									
5.675	5.675	(0.409)	83	4085014	200.000	208.55	50.00- 150.00	100.00(A)	
5.675	5.675	(0.409)	69	3260048			29.59- 129.59	79.81	

15 Freon 152a CAS #: 75-37-6									
5.844	5.844	(0.422)	65	2024077	200.000	194.03	50.00- 150.00	100.00	
5.844	5.844	(0.422)	51	3428125			125.61- 225.61	169.37	
5.844	5.844	(0.422)	47	902442			0.00- 95.62	44.59	

17 Freon 22 CAS #: 75-45-6									
5.985	5.985	(0.432)	67	1074014	200.000	200.36	50.00- 150.00	100.00	
5.985	5.985	(0.432)	51	5534587			424.04- 524.04	515.32	
5.985	5.985	(0.432)	85	104632			0.00- 60.14	9.74	

26 Methanol CAS #: 67-56-1									
7.534	7.534	(0.543)	31	4834637	1200.00	1090.3	50.00- 150.00	100.00	
7.534	7.534	(0.543)	32	3571349			127.28- 227.28	73.87	

34 Dichlorofluoromethane/Fr21 CAS #: 75-43-4									
8.717	8.717	(0.629)	67	6875679	200.000	200.17	50.00- 150.00	100.00	
8.717	8.717	(0.629)	69	2226087			0.00- 82.55	32.38	
8.717	8.717	(0.629)	35	378185			0.00- 55.68	5.50	

40 Freon123a CAS #: 354-23-4									
9.552	9.552	(0.689)	67	5553857	200.000	209.06	50.00- 150.00	100.00(A)	
9.552	9.552	(0.689)	117	4722976			33.27- 133.27	85.04	

41 Freon123 CAS #: 306-83-2									
9.718	9.718	(0.701)	83	7552537	200.000	207.03	50.00- 150.00	100.00(A)	
9.718	9.718	(0.701)	133	1633548			0.00- 72.56	21.63	
9.718	9.718	(0.701)	85	5332112			21.04- 121.04	70.60	

57 tert-Butyl-Alcohol CAS #: 75-65-0									
11.155	11.155	(0.805)	59	7662239	200.000	234.35	50.00- 150.00	100.00(A)	
11.155	11.155	(0.805)	41	1567171			0.00- 79.32	20.45	
11.155	11.155	(0.805)	57	796228			0.00- 60.92	10.39	

68 Isopropyl ether CAS #: 108-20-3									
12.261	12.261	(0.884)	45	11596659	200.000	235.02	50.00- 150.00	100.00(A)	
12.289	12.289	(0.886)	87	3510582			0.00- 81.01	30.27	
12.289	12.289	(0.886)	59	1295848			0.00- 61.81	11.17	

71 1-Propanol CAS #: 71-23-8									
12.400	12.400	(0.894)	42	702442	200.000	216.83	50.00- 150.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
71 1-Propanol (continued)									
12.400	12.400	(0.894)	59	1005858			61.64- 161.64	143.19	
12.400	12.400	(0.894)	41	698074			40.91- 140.91	99.38	

73 t-Butylethyl Ether									
						CAS #: 637-92-3			
12.925	12.925	(0.932)	59	12686099	200.000	235.43	50.00- 150.00	100.00(A)	
12.925	12.925	(0.932)	87	5569469			0.00- 93.11	43.90	
12.925	12.925	(0.932)	41	2116982			0.00- 70.41	16.69	

77 Ethyl Acetate									
						CAS #: 141-78-6			
13.367	13.367	(0.964)	45	1206713	200.000	216.02	50.00- 150.00	100.00(A)	
13.367	13.367	(0.964)	61	1309042			49.68- 149.68	108.48	
13.367	13.367	(0.964)	43	8453365			615.05- 715.05	700.53	

92 tert-amyl-Methyl Ether									
						CAS #: 994-05-8			
14.999	14.999	(1.082)	73	12067757	200.000	245.45	50.00- 150.00	100.00(A)	
14.999	14.999	(1.082)	87	2947080			0.00- 74.91	24.42	
14.999	14.999	(1.082)	55	2738156			0.00- 76.64	22.69	

96 2-Heptanone									
						CAS #: 110-43-0			
21.966	21.966	(1.584)	58	7527722	200.000	272.58	50.00- 150.00	100.00(A)	
21.966	21.966	(1.584)	43	10588425			98.27- 198.27	140.66	

98 1-Butanol									
						CAS #: 71-36-3			
15.773	15.773	(1.009)	56	2692052	200.000	285.71	50.00- 150.00	100.00(A)	
15.773	15.773	(1.009)	41	1770416			28.59- 128.59	65.76	
15.773	15.773	(1.009)	43	1349879			6.69- 106.69	50.14	

119 Butyl Acetate									
						CAS #: 123-86-4			
19.533	19.533	(1.249)	56	4362567	200.000	245.83	50.00- 150.00	100.00(A)	
19.533	19.533	(1.249)	73	1802604			0.00- 95.25	41.32	
19.533	19.533	(1.249)	43	9764375			169.61- 269.61	223.82	

135 Cyclohexanone									
						CAS #: 108-94-1			
22.741	22.741	(1.093)	55	5498067	200.000	261.35	50.00- 150.00	100.00(A)	
22.741	22.741	(1.093)	98	2946743			2.09- 102.09	53.60	
22.741	22.741	(1.093)	42	3547789			15.79- 115.79	64.53	

146 Diisobutyl Ketone									
						CAS #: 108-83-8			
23.570	23.570	(1.133)	57	13305333	200.000	261.21	50.00- 150.00	100.00(A)	
23.570	23.570	(1.133)	85	12939186			46.68- 146.68	97.25	
0.000	1.000	(0.000)	0	0			0.00- 50.00	0.00	

QC Flag Legend

- A - Target compound detected but, quantitated amount exceeded maximum amount.
- H - Operator selected an alternate compound hit.

Report Date: 02-Jan-2008 15:47

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 02-JAN-2008

Lab File ID: t010205.d

Calibration Time: 12:02

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/02Jan2008.b/t14q1213c.m

Misc Info: 200ppbv -> 200ppbv (1200ppbv MeOH)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	338913	203348	474478	342802	1.15
97 1,4-Difluorobenze	1251078	750647	1751509	1259545	0.68
126 Chlorobenzene-d5	1269166	761500	1776832	1262417	-0.53

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.


AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/02Jan2008,b/t010205.d
Date : 02-JAN-2008 12:48
Client ID: Level 7
Sample Info: 200ml #1443-399
Column phase: RTX-624

Instrument: msdt,i
Operator: sjr
Column diameter: 0.53

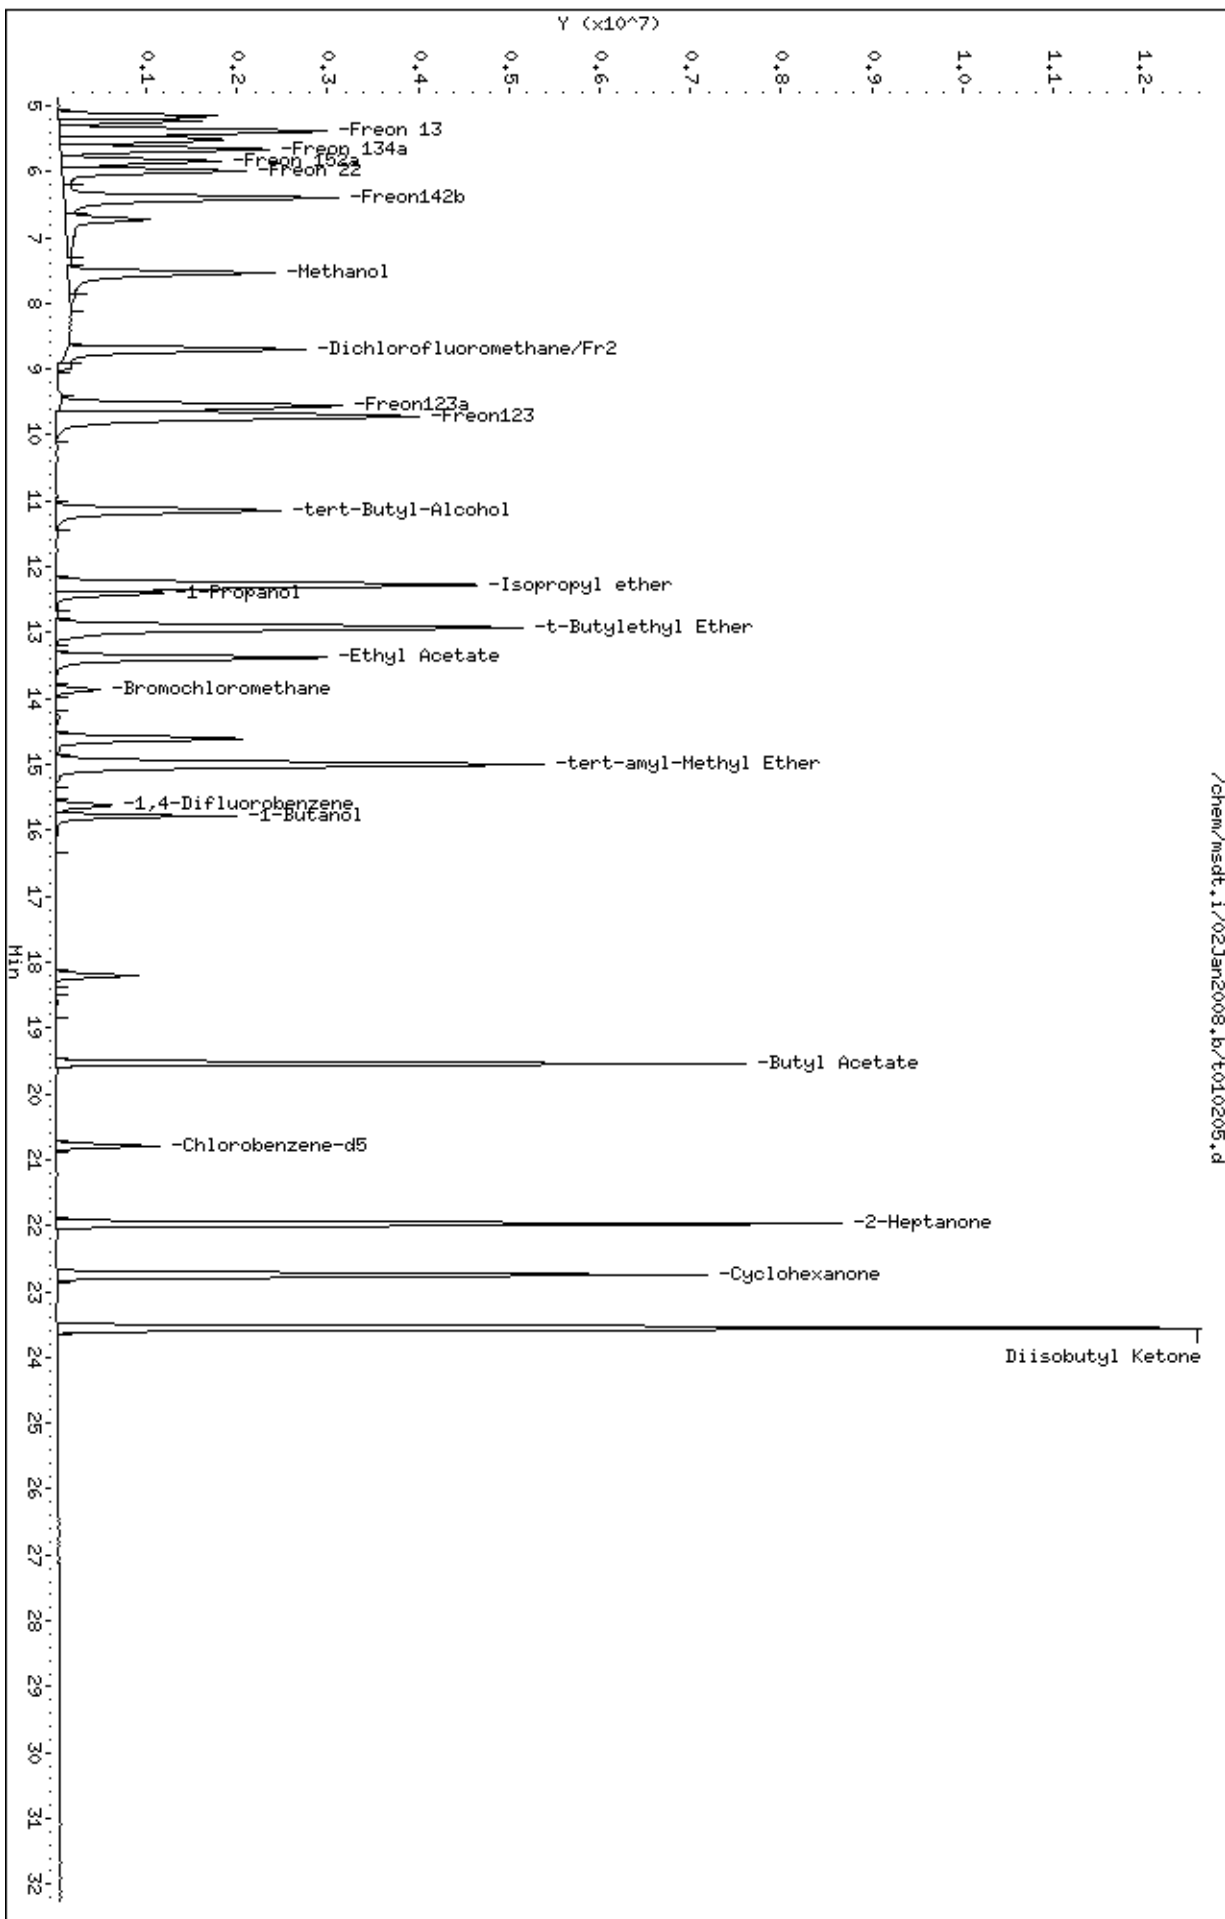

Report Date: 19-Dec-2007 12:55

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/19Dec2007.b/t121904.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 19-DEC-2007 12:21
 Operator : sjr Inst ID: msdt.i
 Smp Info : 200ml #1443-388
 Misc Info : 200ppbv -> 200ppbv
 Comment :
 Method : /chem/msdt.i/19Dec2007.b/t14q1213b.m
 Meth Date : 19-Dec-2007 12:55 sruth Quant Type: ISTD
 Cal Date : 19-DEC-2007 12:21 Cal File: t121904.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: splb.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

* 81	Bromochloromethane					CAS #:	74-97-5	
13.865	13.865	(1.000)	130	208290	25.0000		50.00- 150.00	100.00
13.865	13.865	(1.000)	128	168001			27.34- 127.34	80.66
13.865	13.865	(1.000)	49	262276			80.38- 180.38	125.92

* 97	1,4-Difluorobenzene					CAS #:	540-36-3	
15.635	15.635	(1.000)	114	816150	25.0000		50.00- 150.00	100.00
15.607	15.607	(1.000)	88	133813			0.00- 65.86	16.40

* 126	Chlorobenzene-d5					CAS #:	3114-55-4	
20.805	20.805	(1.000)	117	777569	25.0000		50.00- 150.00	100.00
20.805	20.805	(1.000)	82	460481			6.00- 106.00	59.22

199	Vinyl Fluoride					CAS #:	75-02-5	
5.563	5.563	(0.401)	46	791803	200.000	142.07	50.00- 150.00	100.00
5.563	5.563	(0.401)	45	564402			20.20- 120.20	71.28
5.563	5.563	(0.401)	47	17143			0.00- 52.23	2.17

Report Date: 19-Dec-2007 12:55

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 19-DEC-2007

Lab File ID: t121904.d

Calibration Time: 11:12

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: sjr

Method File: /chem/msdt.i/19Dec2007.b/t14q1213b.m

Misc Info: 200ppbv -> 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	204685	122811	286559	208290	1.76
97 1,4-Difluorobenze	866754	520052	1213456	816150	-5.84
126 Chlorobenzene-d5	784408	470645	1098171	777569	-0.87

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.87	13.54	14.20	13.87	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.81	20.48	21.14	20.81	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/19Dec2007,b/t121904.d

Date : 19-DEC-2007 12:21

Client ID: Level 7

Sample Info: 200ml #1443-388


Column phase: RTX-624

Instrument: msdt,i

Operator: sjr

Column diameter: 0.53

/chem/msdt,i/19Dec2007,b/t121904.d

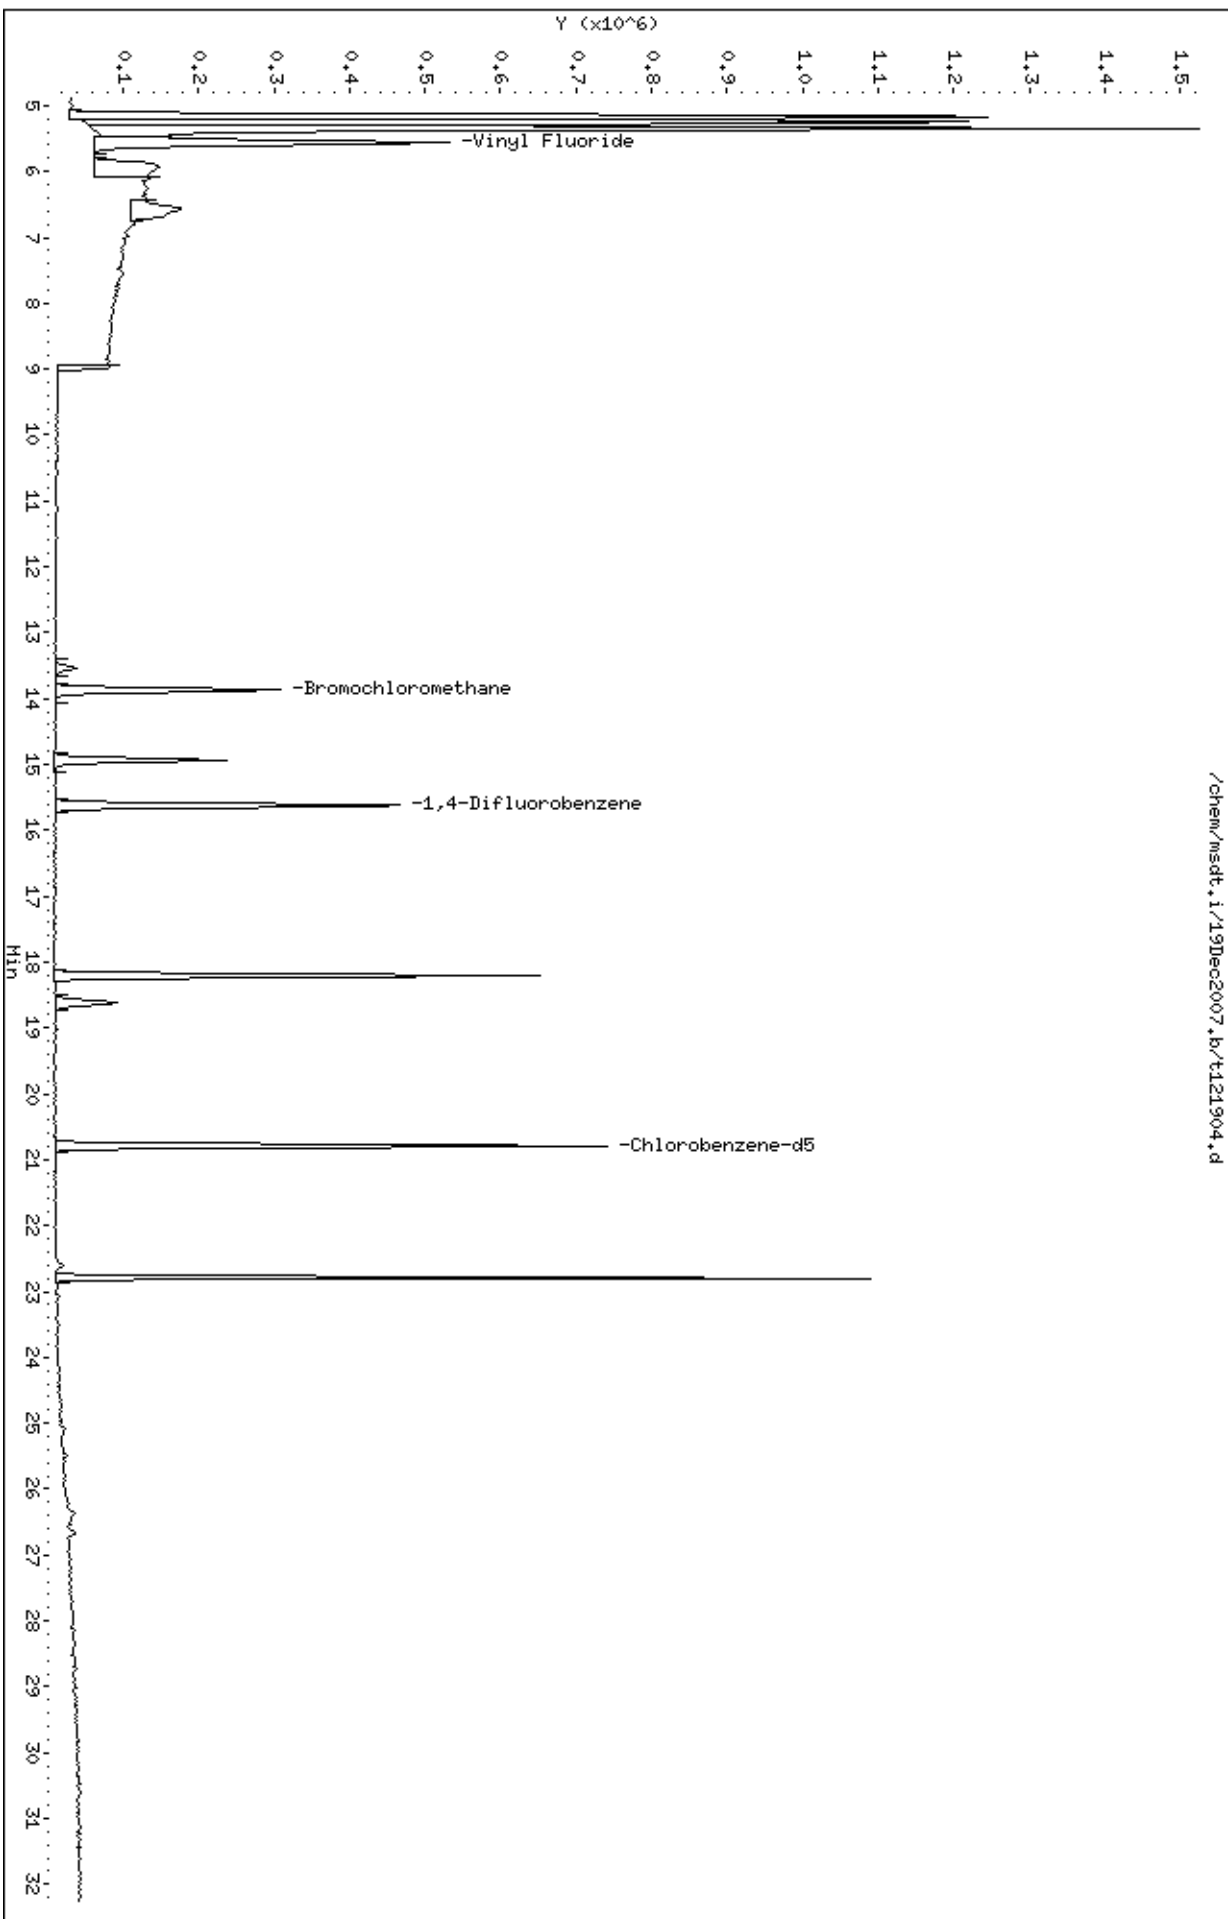

Report Date: 14-Dec-2007 15:24

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/13Dec2007.b/t121316.d
 Lab Smp Id: ICAL Client Smp ID: Level 7
 Inj Date : 14-DEC-2007 03:20
 Operator : ab Inst ID: msdt.i
 Smp Info : 200mL #1443-378
 Misc Info : 200ppbv -> 200ppbv
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/t14q1213a.m
 Meth Date : 14-Dec-2007 15:15 ealcan Quant Type: ISTD
 Cal Date : 14-DEC-2007 03:20 Cal File: t121316.d
 Als bottle: 1 Calibration Sample, Level: 7
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04mdl+ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.858	13.858	(1.000)	130	312072	25.0000			50.00- 150.00	100.00
13.858	13.858	(1.000)	128	237887				26.73- 126.73	76.23
13.941	13.858	(1.000)	49	868225				83.94- 183.94	278.21

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1219072	25.0000			50.00- 150.00	100.00
15.600	15.628	(1.000)	88	196561				0.00- 65.84	16.12

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1122977	25.0000			50.00- 150.00	100.00
20.798	20.798	(1.000)	82	635548				5.33- 105.33	56.59

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.937	(1.078)	65	497300	25.0000	25.028		50.00- 150.00	100.00
14.936	14.937	(1.078)	67	364757				3.93- 103.93	73.35

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1195364	25.0000	25.849		50.00- 150.00	100.00
18.199	18.199	(1.165)	70	132917				0.00- 61.06	11.12

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	813027			18.52- 118.52	68.02	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	787955	25.0000	25.583	50.00- 150.00	100.00	
22.789	22.789	(1.096)	95	973590			74.37- 174.37	123.56	
22.789	22.789	(1.096)	176	763981			47.63- 147.63	96.96	

11 Propylene									
						CAS #: 115-07-1			
5.812	5.812	(0.419)	41	1566944	200.000	188.00	50.00- 150.00	100.00	
5.812	5.812	(0.419)	42	1072505			17.44- 117.44	68.45	
5.812	5.812	(0.419)	39	1271044			31.05- 131.05	81.12	

12 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
5.923	5.923	(0.427)	85	10536645	200.000	192.77	50.00- 150.00	100.00	
5.923	5.923	(0.427)	87	3375730			0.00- 82.50	32.04	

16 Freon 114									
						CAS #: 76-14-2			
6.282	6.310	(0.453)	135	7255444	200.000	203.05	50.00- 150.00	100.00(A)	
6.282	6.310	(0.453)	137	2321055			0.00- 81.78	31.99	

18 Chloromethane									
						CAS #: 74-87-3			
6.559	6.559	(0.473)	50	2309072	200.000	195.31	50.00- 150.00	100.00	
6.559	6.559	(0.473)	52	757911			0.00- 83.59	32.82	

20 Vinyl Chloride									
						CAS #: 75-01-4			
6.890	6.891	(0.497)	62	3064561	200.000	207.24	50.00- 150.00	100.00(A)	
6.890	6.891	(0.497)	64	994470			0.00- 94.54	32.45	

22 1,3-Butadiene									
						CAS #: 106-99-0			
6.946	6.973	(0.501)	54	2304326	200.000	199.62	50.00- 150.00	100.00	
6.946	6.973	(0.501)	39	2084103			61.08- 161.08	90.44	

25 Bromomethane									
						CAS #: 74-83-9			
7.913	7.914	(0.571)	94	3447481	200.000	220.14	50.00- 150.00	100.00(A)	
7.913	7.914	(0.571)	96	3166350			44.93- 144.93	91.85	

27 Chloroethane									
						CAS #: 75-00-3			
8.190	8.190	(0.591)	64	1639035	200.000	207.72	50.00- 150.00	100.00(A)	
8.190	8.190	(0.591)	49	399052			0.00- 76.61	24.35	
8.190	8.190	(0.591)	66	548680			0.00- 85.87	33.48	

31 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
8.771	8.771	(0.633)	101	11919103	200.000	195.08	50.00- 150.00	100.00	
8.771	8.771	(0.633)	103	7714237			15.72- 115.72	64.72	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
38 Ethanol						CAS #: 64-17-5			
9.241	9.241	(0.667)	45	839782	200.000	202.66	50.00- 150.00	100.00(A)	
9.241	9.241	(0.667)	43	185565			0.00- 74.87	22.10	
9.241	9.241	(0.667)	46	312090			0.00- 88.05	37.16	

42 Freon 113						CAS #: 76-13-1			
9.959	9.960	(0.719)	151	5509795	200.000	200.37	50.00- 150.00	100.00(A)	
9.959	9.960	(0.719)	153	3528539			15.26- 115.26	64.04	
9.959	9.960	(0.719)	101	7165404			81.18- 181.18	130.05	

43 1,1-Dichloroethene						CAS #: 75-35-4			
10.042	10.043	(0.725)	61	5073732	200.000	210.51	50.00- 150.00	100.00(A)	
10.042	10.043	(0.725)	96	3289501			16.16- 116.16	64.83	
10.042	10.043	(0.725)	98	2116439			0.00- 91.50	41.71	

45 Acetone						CAS #: 67-64-1			
10.181	10.181	(0.735)	58	1397444	200.000	186.74	50.00- 150.00	100.00	
10.181	10.181	(0.735)	43	4140165			264.94- 364.94	296.27	

46 2-Propanol						CAS #: 67-63-0			
10.374	10.374	(0.749)	45	4788607	200.000	193.16	50.00- 150.00	100.00	
10.374	10.402	(0.749)	43	1071504			0.00- 78.96	22.38	
10.374	10.374	(0.749)	59	216385			0.00- 54.06	4.52	

47 Carbon Disulfide						CAS #: 75-15-0			
10.540	10.540	(0.761)	76	10068884	200.000	219.11	50.00- 150.00	100.00(A)	

51 3-Chloropropene						CAS #: 107-05-1			
10.817	10.817	(0.781)	76	1619707	200.000	206.52	50.00- 150.00	100.00(A)	
10.817	10.817	(0.781)	41	3270693			176.05- 276.05	201.93	

54 Methylene Chloride						CAS #: 75-09-2			
11.093	11.093	(0.800)	49	2866818	200.000	188.36	50.00- 150.00	100.00	
11.093	11.093	(0.800)	84	2820606			44.80- 144.80	98.39	
11.093	11.093	(0.800)	51	891412			0.00- 83.78	31.09	

60 MTBE						CAS #: 1634-04-4			
11.453	11.453	(0.826)	73	11116354	200.000	217.90	50.00- 150.00	100.00(A)	
11.453	11.453	(0.826)	57	2038614			0.00- 69.38	18.34	
11.453	11.453	(0.826)	41	1796774			0.00- 70.94	16.16	

61 trans-1,2-Dichloroethene						CAS #: 156-60-5			
11.535	11.536	(0.832)	96	3866249	200.000	209.36	50.00- 150.00	100.00(A)	
11.535	11.536	(0.832)	61	5033633			84.61- 184.61	130.19	
11.535	11.536	(0.832)	98	2487334			15.85- 115.85	64.33	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
65 Hexane						CAS #: 110-54-3			
11.895	11.895	(0.858)	57	5243992	200.000	204.52	50.00- 150.00	100.00(A)	
11.895	11.895	(0.858)	43	2845385			8.15- 108.15	54.26	
11.895	11.895	(0.858)	86	999308			0.00- 69.59	19.06	

69 Vinyl Acetate						CAS #: 108-05-4			
12.337	12.365	(0.890)	86	989746	200.000	216.32	50.00- 150.00	100.00(A)	
12.337	12.365	(0.890)	43	8004290			903.55-1003.55	808.72	

70 1,1-Dichloroethane						CAS #: 75-34-3			
12.365	12.365	(0.892)	63	6551116	200.000	203.39	50.00- 150.00	100.00(A)	
12.365	12.365	(0.892)	65	2125637			0.00- 83.37	32.45	

75 2-Butanone						CAS #: 78-93-3			
13.388	13.388	(0.966)	72	1872760	200.000	219.66	50.00- 150.00	100.00(A)	
13.388	13.388	(0.966)	43	5660672			271.22- 371.22	302.26	
13.388	13.388	(0.966)	57	526953			0.00- 78.78	28.14	

76 cis-1,2-Dichloroethene						CAS #: 156-59-2			
13.416	13.416	(0.968)	61	4420251	200.000	195.40	50.00- 150.00	100.00	
13.416	13.416	(0.968)	96	3765367			29.23- 129.23	85.18	
13.416	13.416	(0.968)	98	2414828			0.16- 100.16	54.63	

80 Tetrahydrofuran						CAS #: 109-99-9			
13.858	13.858	(1.000)	42	2820394	200.000	207.59	50.00- 150.00	100.00(A)	
13.858	13.858	(1.000)	71	1625183			0.61- 100.61	57.62	
13.858	13.858	(1.000)	72	1747925			8.31- 108.31	61.97	

82 Chloroform						CAS #: 67-66-3			
13.941	13.941	(1.006)	83	8069375	200.000	214.11	50.00- 150.00	100.00(A)	
13.941	13.941	(1.006)	85	5268385			18.46- 118.46	65.29	

83 1,1,1-Trichloroethane						CAS #: 71-55-6			
14.273	14.273	(1.030)	97	9167706	200.000	203.12	50.00- 150.00	100.00(A)	
14.273	14.273	(1.030)	99	5916514			13.89- 113.89	64.54	

85 Cyclohexane						CAS #: 110-82-7			
14.300	14.301	(1.032)	84	5110679	200.000	221.88	50.00- 150.00	100.00(A)	
14.300	14.301	(1.032)	56	4727310			43.75- 143.75	92.50	
14.300	14.301	(1.032)	41	2304581			1.66- 101.66	45.09	

87 Carbon Tetrachloride						CAS #: 56-23-5			
14.522	14.549	(1.048)	119	8734069	200.000	198.68	50.00- 150.00	100.00	
14.522	14.522	(1.048)	117	9328668			54.19- 154.19	106.81	

91 Benzene						CAS #: 71-43-2			
14.964	14.964	(0.958)	78	11038237	200.000	226.78	50.00- 150.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 Benzene (continued)									
14.964	14.964	(0.958)	77	2501344			0.00- 73.32	22.66	

89 2,2,4-Trimethylpentane CAS #: 540-84-1									
14.881	14.881	(1.074)	57	13590492	200.000	211.58	50.00- 150.00	100.00(A)	
14.881	14.881	(1.074)	56	4365676			0.00- 83.27	32.12	
14.881	14.881	(1.074)	41	3296011			0.00- 77.74	24.25	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.075	15.075	(0.965)	62	4944178	200.000	203.36	50.00- 150.00	100.00(A)	
15.075	15.075	(0.965)	64	1613087			0.00- 82.87	32.63	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	3528120	200.000	228.19	50.00- 150.00	100.00(A)	
15.185	15.185	(0.972)	43	4297565			77.60- 177.60	121.81	
15.185	15.185	(0.972)	57	2763251			32.99- 132.99	78.32	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	4945707	200.000	219.90	50.00- 150.00	100.00(A)	
16.070	16.070	(1.028)	130	4517850			45.55- 145.55	91.35	
16.070	16.070	(1.028)	97	3166262			15.22- 115.22	64.02	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.568	16.568	(1.060)	63	3656991	200.000	224.84	50.00- 150.00	100.00(A)	
16.568	16.568	(1.060)	62	2602507			23.00- 123.00	71.17	
16.568	16.568	(1.060)	41	1842432			8.64- 108.64	50.38	

106 1,4-Dioxane CAS #: 123-91-1									
16.678	16.678	(1.067)	88	2819010	200.000	218.55	50.00- 150.00	100.00(A)	
16.678	16.706	(1.067)	58	1489392			5.85- 105.85	52.83	
16.678	16.678	(1.067)	57	524866			0.00- 69.86	18.62	

107 Bromodichloromethane CAS #: 75-27-4									
16.982	16.983	(1.087)	83	8699153	200.000	222.37	50.00- 150.00	100.00(A)	
16.982	16.983	(1.087)	85	5572863			16.51- 116.51	64.06	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	6201914	200.000	236.75	50.00- 150.00	100.00(A)	
17.784	17.784	(1.138)	77	2006516			0.00- 83.76	32.35	
17.784	17.784	(1.138)	39	2471443			0.00- 94.73	39.85	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.950	17.978	(1.149)	58	2996318	200.000	251.40	50.00- 150.00	100.00(A)	
17.950	17.978	(1.149)	43	6468814			168.02- 268.02	215.89	
17.978	17.978	(1.150)	85	1616456			2.69- 102.69	53.95	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	13027911	200.000	221.89	50.00- 150.00	100.00(A)	
18.337	18.337	(1.173)	92	7910961			9.70- 109.70	60.72	

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	6772915	200.000	222.86	50.00- 150.00	100.00(A)	
18.752	18.752	(0.902)	77	2158329			0.00- 82.23	31.87	
18.752	18.752	(0.902)	39	2511684			0.00- 88.37	37.08	

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.112	(0.919)	97	4824323	200.000	218.85	50.00- 150.00	100.00(A)	
19.111	19.112	(0.919)	99	3039888			15.96- 115.96	63.01	
19.111	19.112	(0.919)	83	4062451			36.03- 136.03	84.21	

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	6398042	200.000	208.25	50.00- 150.00	100.00(A)	
19.277	19.277	(0.927)	129	4443301			20.82- 120.82	69.45	
19.277	19.277	(0.927)	131	4203833			18.42- 118.42	65.70	

121 2-Hexanone						CAS #: 591-78-6			
19.416	19.416	(0.934)	58	4167104	200.000	230.91	50.00- 150.00	100.00(A)	
19.416	19.416	(0.934)	43	6517267			120.66- 220.66	156.40	
19.416	19.416	(0.934)	100	966067			0.00- 74.50	23.18	

122 Dibromochloromethane						CAS #: 124-48-1			
19.803	19.803	(0.952)	129	8374369	200.000	216.12	50.00- 150.00	100.00(A)	
19.803	19.803	(0.952)	127	6438017			25.33- 125.33	76.88	

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.052	20.052	(0.964)	107	8163116	200.000	220.11	50.00- 150.00	100.00(A)	
20.052	20.052	(0.964)	109	7505261			41.12- 141.12	91.94	

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.854	(1.003)	112	11439297	200.000	213.66	50.00- 150.00	100.00(A)	
20.853	20.854	(1.003)	114	3541405			0.00- 80.99	30.96	
20.853	20.854	(1.003)	77	6932745			25.73- 125.73	60.60	

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	6075128	200.000	224.05	50.00- 150.00	100.00(A)	
20.936	20.936	(1.007)	91	19688559			266.55- 366.55	324.08	

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	7875956	200.000	236.14	50.00- 150.00	100.00(A)	
21.130	21.130	(1.016)	91	15938104			157.11- 257.11	202.36	

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	7422754	200.000	236.92	50.00- 150.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	15859161			166.77- 266.77	213.66	

131 Styrene CAS #: 100-42-5									
21.876	21.877	(1.052)	104	12588804	200.000	247.95	50.00- 150.00	100.00(A)	
21.876	21.877	(1.052)	78	6176714			12.82- 112.82	49.07	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	9256344	200.000	229.15	50.00- 150.00	100.00(A)	
22.291	22.291	(1.072)	171	4748752			0.34- 100.34	51.30	

134 Cumene CAS #: 98-82-8									
22.429	22.430	(1.078)	105	21051206	200.000	235.07	50.00- 150.00	100.00(A)	
22.429	22.430	(1.078)	120	5362747			0.00- 74.52	25.47	
22.429	22.430	(1.078)	51	1571705			51.79- 151.79	7.47	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	11462069	200.000	233.43	50.00- 150.00	100.00(A)	
23.010	23.010	(1.106)	85	7393737			17.66- 117.66	64.51	

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	26770074	200.000	236.36	50.00- 150.00	100.00(A)	
23.121	23.121	(1.112)	120	5740764			0.00- 71.52	21.44	
23.121	23.093	(1.112)	105	944899			0.00- 53.54	3.53	

145 4-Ethyltoluene CAS #: 622-96-8									
23.286	23.287	(1.120)	105	23074463	200.000	241.89	50.00- 150.00	100.00(A)	
23.286	23.287	(1.120)	120	6686312			0.00- 79.85	28.98	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	18681312	200.000	240.64	50.00- 150.00	100.00(A)	
23.397	23.397	(1.125)	120	8987396			0.29- 100.29	48.11	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	17839460	200.000	246.90	50.00- 150.00	100.00(A)	
24.033	24.033	(1.156)	120	8064377			0.00- 94.69	45.21	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	12459839	200.000	227.86	50.00- 150.00	100.00(A)	
24.586	24.586	(1.182)	148	7893057			14.61- 114.61	63.35	
24.586	24.586	(1.182)	111	5125486			0.00- 92.01	41.14	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	12915436	200.000	227.31	50.00- 150.00	100.00(A)	
24.724	24.724	(1.189)	148	8205818			13.83- 113.83	63.53	
24.724	24.724	(1.189)	111	5136295			0.00- 89.75	39.77	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

159	alpha-Chlorotoluene					CAS #: 100-44-7			
24.945	24.946	(1.199)	91	20102245	200.000	255.68	50.00- 150.00	100.00(A)	
24.945	24.946	(1.199)	126	3786738			0.00- 69.65	18.84	

161	1,2-Dichlorobenzene					CAS #: 95-50-1			
25.360	25.360	(1.219)	146	12102325	200.000	230.80	50.00- 150.00	100.00(A)	
25.360	25.360	(1.219)	148	7672377			14.36- 114.36	63.40	
25.360	25.360	(1.219)	111	5192689			0.00- 92.81	42.91	

165	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
28.153	28.153	(1.354)	180	9109354	200.000	253.27	50.00- 150.00	100.00(A)	
28.153	28.153	(1.354)	182	8614863			45.41- 145.41	94.57	

166	Hexachlorobutadiene					CAS #: 87-68-3			
28.319	28.319	(1.362)	225	7713243	200.000	234.95	50.00- 150.00	100.00(A)	
28.319	28.319	(1.362)	223	4841161			13.46- 113.46	62.76	

19	Butane					CAS #: 106-97-8			
6.780	6.808	(0.489)	58	582454	200.000	192.31	50.00- 150.00	100.00	
6.780	6.808	(0.489)	43	3920775			672.59- 772.59	673.15	

29	Isopentane					CAS #: 78-78-4			
8.273	8.273	(0.597)	43	3228269	200.000	189.29	50.00- 150.00	100.00	
8.273	8.273	(0.597)	57	2596521			26.79- 126.79	80.43	

102	Methyl Cyclohexane					CAS #: 108-87-2			
16.346	16.347	(1.180)	83	6460529	200.000	221.19	50.00- 150.00	100.00(A)	
16.346	16.347	(1.180)	98	2935311			0.00- 95.49	45.43	
16.346	16.347	(1.180)	55	4166015			16.76- 116.76	64.48	

167	Naphthalene					CAS #: 91-20-3			
28.678	28.678	(1.379)	128	15566479	200.000	262.57	50.00- 150.00	100.00(A)	
28.678	28.678	(1.379)	127	1884718			0.00- 62.56	12.11	

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 14-Dec-2007 15:24

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 14-DEC-2007

Lab File ID: t121316.d

Calibration Time: 01:23

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ab

Method File: /chem/msdt.i/13Dec2007.b/t14q1213a.m

Misc Info: 200ppbv -> 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	280754	168452	393056	312072	11.15
97 1,4-Difluorobenze	1182601	709561	1655641	1219072	3.08
126 Chlorobenzene-d5	1033655	620193	1447117	1122977	8.64


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.86	13.53	14.19	13.86	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

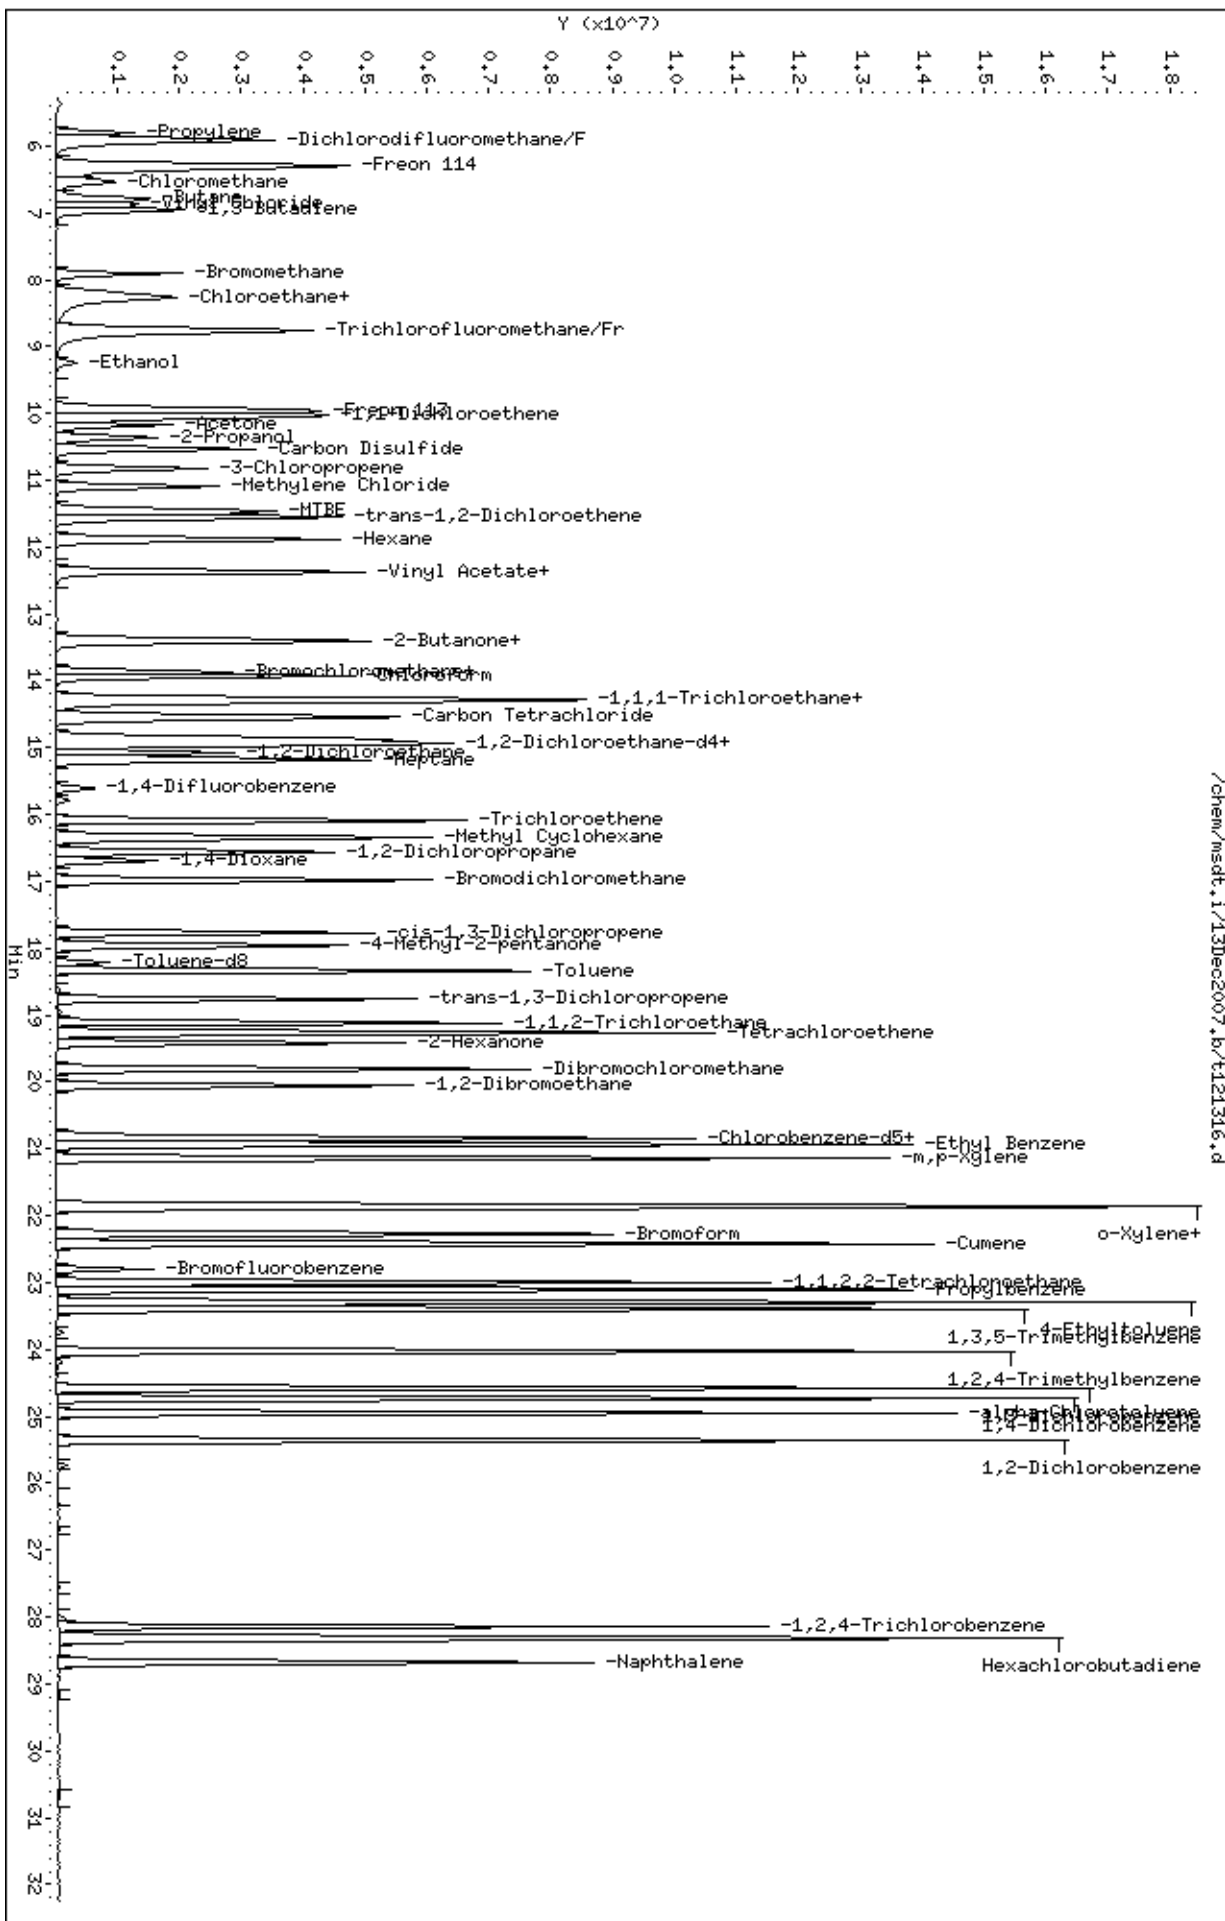



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0801560-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020302	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 2/3/08 03:01 PM

Compound	%Recovery
Freon 12	109
Freon 114	110
Vinyl Chloride	119
Bromomethane	106
Chloroethane	118
Freon 11	107
1,1-Dichloroethene	115
Freon 113	110
Methylene Chloride	108
1,1-Dichloroethane	114
cis-1,2-Dichloroethene	112
Chloroform	119
1,1,1-Trichloroethane	112
Carbon Tetrachloride	110
Benzene	119
1,2-Dichloroethane	116
Trichloroethene	113
1,2-Dichloropropane	121
cis-1,3-Dichloropropene	120
Toluene	113
trans-1,3-Dichloropropene	111
1,1,2-Trichloroethane	111
Tetrachloroethene	109
1,2-Dibromoethane (EDB)	109
Chlorobenzene	107
Ethyl Benzene	112
m,p-Xylene	116
o-Xylene	118
Styrene	115
1,1,2,2-Tetrachloroethane	119
1,3,5-Trimethylbenzene	124
1,2,4-Trimethylbenzene	128
1,3-Dichlorobenzene	116
1,4-Dichlorobenzene	116
alpha-Chlorotoluene	116
1,2-Dichlorobenzene	118
1,3-Butadiene	111
Hexane	113
Cyclohexane	121



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0801560-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020302	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 2/3/08 03:01 PM

Compound	%Recovery
Heptane	116
Bromodichloromethane	115
Dibromochloromethane	111
Cumene	116
Propylbenzene	117
Chloromethane	110
1,2,4-Trichlorobenzene	117
Hexachlorobutadiene	124
Acetone	105
Carbon Disulfide	114
2-Propanol	108
trans-1,2-Dichloroethene	112
2-Butanone (Methyl Ethyl Ketone)	113
Tetrahydrofuran	122
1,4-Dioxane	108
4-Methyl-2-pentanone	131 Q
2-Hexanone	113
Bromoform	117
4-Ethyltoluene	121
Ethanol	114
Methyl tert-butyl ether	113
3-Chloropropene	110
2,2,4-Trimethylpentane	108
Naphthalene	110

Q = Exceeds Quality Control limits.

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	108	70-130
1,2-Dichloroethane-d4	103	70-130
4-Bromofluorobenzene	96	70-130

Report Date: 03-Feb-2008 15:20

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msdt.i Injection Date: 03-FEB-2008 15:01
 Lab File ID: t020302.d Init. Cal. Date(s): 13-DEC-2007 25-JAN-2008
 Analysis Type: AIR Init. Cal. Times: 21:35 13:09
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /chem/msdt.i/03Feb2008.b/t14q1213e.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 90 1,2-Dichloroethane-d4	1.59173	1.64216	0.010	-3.16865	30.00000	Averaged
\$ 113 Toluene-d8	0.94836	1.02692	0.010	-8.28406	30.00000	Averaged
\$ 137 Bromofluorobenzene	0.68567	0.65889	0.010	3.90656	30.00000	Averaged
11 Propylene	0.66768	0.77535	0.010	-16.12551	30.00000	Averaged
12 Dichlorodifluoromethane/Fr1	4.37866	4.79151	0.010	-9.42852	30.00000	Averaged
16 Freon 114	2.86250	3.15938	0.010	-10.37112	30.00000	Averaged
18 Chloromethane	0.94711	1.04740	0.010	-10.58918	30.00000	Averaged
20 Vinyl Chloride	1.18461	1.41371	0.010	-19.33896	30.00000	Averaged
22 1,3-Butadiene	0.92474	1.02904	0.010	-11.27866	30.00000	Averaged
25 Bromomethane	1.25453	1.33222	0.010	-6.19243	30.00000	Averaged
27 Chloroethane	0.63210	0.74566	0.010	-17.96613	30.00000	Averaged
31 Trichlorofluoromethane/Fr11	4.89467	5.25697	0.010	-7.40207	30.00000	Averaged
38 Ethanol	0.33196	0.37718	0.010	-13.62236	30.00000	Averaged
42 Freon 113	2.20289	2.41250	0.010	-9.51531	30.00000	Averaged
43 1,1-Dichloroethene	1.93084	2.22986	0.010	-15.48667	30.00000	Averaged
45 Acetone	0.59950	0.62940	0.010	-4.98811	30.00000	Averaged
46 2-Propanol	1.98593	2.15534	0.010	-8.53007	30.00000	Averaged
47 Carbon Disulfide	3.68135	4.21647	0.010	-14.53601	30.00000	Averaged
51 3-Chloropropene	0.62830	0.69023	0.010	-9.85613	30.00000	Averaged
54 Methylene Chloride	1.21929	1.31710	0.010	-8.02239	30.00000	Averaged
60 MTBE	4.08685	4.62569	0.010	-13.18468	30.00000	Averaged
61 trans-1,2-Dichloroethene	1.47941	1.65384	0.010	-11.79047	30.00000	Averaged
65 Hexane	2.05402	2.32744	0.010	-13.31099	30.00000	Averaged
69 Vinyl Acetate	0.36654	0.40431	0.010	-10.30675	30.00000	Averaged
70 1,1-Dichloroethane	2.58029	2.95627	0.010	-14.57121	30.00000	Averaged
75 2-Butanone	0.68300	0.77285	0.010	-13.15474	30.00000	Averaged
76 cis-1,2-Dichloroethene	1.81216	2.02806	0.010	-11.91375	30.00000	Averaged
80 Tetrahydrofuran	1.08841	1.32348	0.010	-21.59826	30.00000	Averaged
82 Chloroform	3.01922	3.58816	0.010	-18.84378	30.00000	Averaged
83 1,1,1-Trichloroethane	3.61566	4.04348	0.010	-11.83226	30.00000	Averaged
85 Cyclohexane	1.84523	2.22668	0.010	-20.67236	30.00000	Averaged
87 Carbon Tetrachloride	3.52165	3.87020	0.010	-9.89723	30.00000	Averaged
89 2,2,4-Trimethylpentane	5.14568	5.53259	0.010	-7.51915	30.00000	Averaged
91 Benzene	0.99818	1.18906	0.010	-19.12259	30.00000	Averaged
93 1,2-Dichloroethane	0.49858	0.57721	0.010	-15.77024	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msdt.i Injection Date: 03-FEB-2008 15:01
 Lab File ID: t020302.d Init. Cal. Date(s): 13-DEC-2007 25-JAN-2008
 Analysis Type: AIR Init. Cal. Times: 21:35 13:09
 Lab Sample ID: CCV-1 Quant Type: ISTD
 Method: /chem/msdt.i/03Feb2008.b/t14q1213e.m

COMPOUND	RRF / AMOUNT	RF50	MIN	RRF	%D / %DRIFT	MAX	%D / %DRIFT	CURVE TYPE
94 Heptane	0.31708	0.36892	0.010	-16.35144	30.00000	Averaged		
101 Trichloroethene	0.46122	0.52236	0.010	-13.25583	30.00000	Averaged		
104 1,2-Dichloropropane	0.33356	0.40477	0.010	-21.34822	30.00000	Averaged		
106 1,4-Dioxane	0.26452	0.28540	0.010	-7.89219	30.00000	Averaged		
107 Bromodichloromethane	0.80226	0.92180	0.010	-14.90041	30.00000	Averaged		
110 cis-1,3-Dichloropropene	0.53720	0.64538	0.010	-20.13801	30.00000	Averaged		
111 4-Methyl-2-pentanone	0.24442	0.31971	0.010	-30.80144	30.00000	Averaged	<-	
114 Toluene	1.20407	1.36536	0.010	-13.39512	30.00000	Averaged		
116 trans-1,3-Dichloropropene	0.67657	0.74840	0.010	-10.61704	30.00000	Averaged		
117 1,1,2-Trichloroethane	0.49075	0.54568	0.010	-11.19237	30.00000	Averaged		
120 Tetrachloroethene	0.68395	0.74752	0.010	-9.29321	30.00000	Averaged		
121 2-Hexanone	0.40176	0.45469	0.010	-13.17499	30.00000	Averaged		
122 Dibromochloromethane	0.86263	0.95590	0.010	-10.81291	30.00000	Averaged		
123 1,2-Dibromoethane	0.82562	0.90122	0.010	-9.15790	30.00000	Averaged		
127 Chlorobenzene	1.19191	1.27647	0.010	-7.09436	30.00000	Averaged		
128 Ethyl Benzene	0.60365	0.67496	0.010	-11.81354	30.00000	Averaged		
129 m,p-Xylene	0.74252	0.85881	0.010	-15.66169	30.00000	Averaged		
130 o-Xylene	0.69747	0.82197	0.010	-17.84963	30.00000	Averaged		
131 Styrene	1.13028	1.30003	0.010	-15.01925	30.00000	Averaged		
133 Bromoform	0.89926	1.04958	0.010	-16.71629	30.00000	Averaged		
134 Cumene	1.99362	2.30639	0.010	-15.68887	30.00000	Averaged		
140 1,1,2,2-Tetrachloroethane	1.09313	1.29922	0.010	-18.85363	30.00000	Averaged		
142 Propylbenzene	2.52143	2.95029	0.010	-17.00867	30.00000	Averaged		
145 4-Ethyltoluene	2.12367	2.56847	0.010	-20.94493	30.00000	Averaged		
147 1,3,5-Trimethylbenzene	1.72826	2.13922	0.010	-23.77887	30.00000	Averaged		
150 1,2,4-Trimethylbenzene	1.60852	2.05739	0.010	-27.90615	30.00000	Averaged		
155 1,3-Dichlorobenzene	1.21736	1.41638	0.010	-16.34837	30.00000	Averaged		
156 1,4-Dichlorobenzene	1.26490	1.47012	0.010	-16.22430	30.00000	Averaged		
159 alpha-Chlorotoluene	1.75030	2.02929	0.010	-15.93919	30.00000	Averaged		
161 1,2-Dichlorobenzene	1.16735	1.37559	0.010	-17.83913	30.00000	Averaged		
165 1,2,4-Trichlorobenzene	0.80071	0.93660	0.010	-16.97089	30.00000	Averaged		
166 Hexachlorobutadiene	0.73084	0.90900	0.010	-24.37720	30.00000	Averaged		
29 Isopentane	1.36621	1.51107	0.010	-10.60305	30.00000	Averaged		
19 Butane	0.24262	0.27184	0.010	-12.04003	30.00000	Averaged		
102 Methyl Cyclohexane	2.33988	2.68299	0.010	-14.66334	30.00000	Averaged		
167 Naphthalene	1.31984	1.45179	0.010	-9.99759	30.00000	Averaged		

Report Date: 03-Feb-2008 15:20

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/03Feb2008.b/t020302.d
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1
 Inj Date : 03-FEB-2008 15:01
 Operator : xp Inst ID: msdt.i
 Smp Info : 100mL #1576-197A
 Misc Info : 100ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/03Feb2008.b/t14q1213e.m
 Meth Date : 03-Feb-2008 15:20 dmendoza Quant Type: ISTD
 Cal Date : 25-JAN-2008 13:09 Cal File: t012506.d
 Als bottle: 1 Continuing Calibration Sample
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	323259	25.0000			80.00- 120.00	100.00
13.886	13.886	(1.000)	128	256771				29.43- 129.43	79.43
13.858	13.858	(1.000)	49	548973				119.82- 219.82	169.82

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1297188	25.0000			80.00- 120.00	100.00
15.628	15.628	(1.000)	88	215314				0.00- 66.60	16.60

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1219852	25.0000			80.00- 120.00	100.00
20.798	20.798	(1.000)	82	685772				5.74- 105.74	56.22

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.076)	65	530845	25.0000	25.792		80.00- 120.00	100.00
14.936	14.936	(1.076)	67	299386				3.93- 103.93	56.40

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1332112	25.0000	27.071		80.00- 120.00	100.00
18.199	18.199	(1.165)	70	153965				0.00- 61.06	11.56

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

\$ 113 Toluene-d8 (continued)									
18.199	18.199	(1.165)	100	902233			18.52- 118.52	67.73	

\$ 137 Bromofluorobenzene									
						CAS #: 460-00-4			
22.789	22.789	(1.096)	174	803745	25.0000	24.023	80.00- 120.00	100.00	
22.789	22.789	(1.096)	95	1008157			75.43- 175.43	125.43	
22.789	22.789	(1.096)	176	784066			47.55- 147.55	97.55	

11 Propylene									
						CAS #: 115-07-1			
5.812	5.812	(0.419)	41	501278	50.0000	58.063	80.00- 120.00	100.00	
5.812	5.812	(0.419)	42	345256			17.44- 117.44	68.88	
5.812	5.812	(0.419)	39	398777			31.05- 131.05	79.55	

12 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
5.923	5.923	(0.427)	85	3097799	50.0000	54.714	80.00- 120.00	100.00	
5.923	5.923	(0.427)	87	975657			0.00- 82.50	31.50	

16 Freon 114									
						CAS #: 76-14-2			
6.310	6.310	(0.454)	135	2042595	50.0000	55.186	80.00- 120.00	100.00	
6.310	6.310	(0.454)	137	647303			0.00- 81.78	31.69	

18 Chloromethane									
						CAS #: 74-87-3			
6.531	6.531	(0.470)	50	677166	50.0000	55.294	80.00- 120.00	100.00	
6.531	6.531	(0.470)	52	229142			0.00- 83.59	33.84	

20 Vinyl Chloride									
						CAS #: 75-01-4			
6.890	6.890	(0.496)	62	913988	50.0000	59.669	80.00- 120.00	100.00	
6.890	6.890	(0.496)	64	302881			0.00- 94.54	33.14	

22 1,3-Butadiene									
						CAS #: 106-99-0			
6.973	6.973	(0.502)	54	665291	50.0000	55.639	80.00- 120.00	100.00	
6.973	6.973	(0.502)	39	637476			61.08- 161.08	95.82	

25 Bromomethane									
						CAS #: 74-83-9			
7.913	7.913	(0.570)	94	861304	50.0000	53.096	80.00- 120.00	100.00	
7.913	7.913	(0.570)	96	810404			44.09- 144.09	94.09	

27 Chloroethane									
						CAS #: 75-00-3			
8.190	8.190	(0.590)	64	482085	50.0000	58.983	80.00- 120.00	100.00	
8.190	8.190	(0.590)	49	122835			0.00- 76.61	25.48	
8.190	8.190	(0.590)	66	158623			0.00- 85.87	32.90	

31 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
8.771	8.771	(0.632)	101	3398733	50.0000	53.701	80.00- 120.00	100.00	
8.771	8.771	(0.632)	103	2212961			15.11- 115.11	65.11	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
38 Ethanol						CAS #: 64-17-5			
9.241	9.241	(0.665)	45	243856	50.0000	56.811	80.00- 120.00	100.00	
9.241	9.241	(0.665)	43	55358			0.00- 74.87	22.70	
9.241	9.241	(0.665)	46	89092			0.00- 88.05	36.53	

42 Freon 113						CAS #: 76-13-1			
9.960	9.960	(0.717)	151	1559724	50.0000	54.758	80.00- 120.00	100.00	
9.960	9.960	(0.717)	153	995739			13.84- 113.84	63.84	
9.960	9.960	(0.717)	101	2031428			80.24- 180.24	130.24	

43 1,1-Dichloroethene						CAS #: 75-35-4			
10.042	10.042	(0.723)	61	1441649	50.0000	57.743	80.00- 120.00	100.00	
10.042	10.042	(0.723)	96	878286			10.92- 110.92	60.92	
10.042	10.042	(0.723)	98	576309			0.00- 89.98	39.98	

45 Acetone						CAS #: 67-64-1			
10.181	10.181	(0.733)	58	406918	50.0000	52.494	80.00- 120.00	100.00	
10.181	10.181	(0.733)	43	1322994			264.94- 364.94	325.13	

46 2-Propanol						CAS #: 67-63-0			
10.374	10.374	(0.747)	45	1393465	50.0000	54.265	80.00- 120.00	100.00	
10.374	10.374	(0.747)	43	363425			0.00- 78.96	26.08	
10.374	10.374	(0.747)	59	60238			0.00- 54.06	4.32	

47 Carbon Disulfide						CAS #: 75-15-0			
10.540	10.540	(0.759)	76	2726027	50.0000	57.268	80.00- 120.00	100.00	

51 3-Chloropropene						CAS #: 107-05-1			
10.817	10.817	(0.779)	76	446246	50.0000	54.928	80.00- 120.00	100.00	
10.817	10.817	(0.779)	41	988631			176.05- 276.05	221.54	

54 Methylene Chloride						CAS #: 75-09-2			
11.093	11.093	(0.799)	49	851531	50.0000	54.011	80.00- 120.00	100.00	
11.121	11.121	(0.801)	84	754402			38.59- 138.59	88.59	
11.093	11.093	(0.799)	51	262792			0.00- 83.78	30.86	

60 MTBE						CAS #: 1634-04-4			
11.453	11.453	(0.825)	73	2990594	50.0000	56.592	80.00- 120.00	100.00	
11.453	11.453	(0.825)	57	569858			0.00- 69.06	19.06	
11.453	11.453	(0.825)	41	557289			0.00- 70.94	18.63	

61 trans-1,2-Dichloroethene						CAS #: 156-60-5			
11.563	11.563	(0.833)	96	1069237	50.0000	55.895	80.00- 120.00	100.00	
11.536	11.536	(0.831)	61	1486226			89.00- 189.00	139.00	
11.563	11.563	(0.833)	98	682315			15.85- 115.85	63.81	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
65 Hexane						CAS #: 110-54-3			
11.895	11.895	(0.857)	57	1504730	50.0000	56.655	80.00- 120.00	100.00	
11.895	11.895	(0.857)	43	853478			8.15- 108.15	56.72	
11.895	11.895	(0.857)	86	275095			0.00- 69.59	18.28	

69 Vinyl Acetate						CAS #: 108-05-4			
12.365	12.365	(0.890)	86	261397	50.0000	55.153	80.00- 120.00	100.00	
12.365	12.365	(0.890)	43	2343234			903.55-1003.55	896.43	

70 1,1-Dichloroethane						CAS #: 75-34-3			
12.365	12.365	(0.890)	63	1911282	50.0000	57.286	80.00- 120.00	100.00	
12.365	12.365	(0.890)	65	622222			0.00- 82.56	32.56	

75 2-Butanone						CAS #: 78-93-3			
13.388	13.388	(0.964)	72	499660	50.0000	56.577	80.00- 120.00	100.00	
13.388	13.388	(0.964)	43	1695283			289.29- 389.29	339.29	
13.388	13.388	(0.964)	57	148744			0.00- 78.78	29.77	

76 cis-1,2-Dichloroethene						CAS #: 156-59-2			
13.416	13.416	(0.966)	61	1311177	50.0000	55.957	80.00- 120.00	100.00	
13.416	13.416	(0.966)	96	1054763			30.44- 130.44	80.44	
13.416	13.416	(0.966)	98	672111			1.26- 101.26	51.26	

80 Tetrahydrofuran						CAS #: 109-99-9			
13.858	13.858	(0.998)	42	855657	50.0000	60.799	80.00- 120.00	100.00	
13.858	13.858	(0.998)	71	455033			3.18- 103.18	53.18	
13.858	13.858	(0.998)	72	489842			8.31- 108.31	57.25	

82 Chloroform						CAS #: 67-66-3			
13.941	13.941	(1.004)	83	2319811	50.0000	59.422	80.00- 120.00	100.00	
13.941	13.941	(1.004)	85	1507515			14.98- 114.98	64.98	

83 1,1,1-Trichloroethane						CAS #: 71-55-6			
14.273	14.273	(1.028)	97	2614185	50.0000	55.916	80.00- 120.00	100.00	
14.273	14.273	(1.028)	99	1695474			14.86- 114.86	64.86	

85 Cyclohexane						CAS #: 110-82-7			
14.300	14.300	(1.030)	84	1439593	50.0000	60.336	80.00- 120.00	100.00	
14.300	14.300	(1.030)	56	1417317			48.45- 148.45	98.45	
14.300	14.300	(1.030)	41	736407			1.15- 101.15	51.15	

87 Carbon Tetrachloride						CAS #: 56-23-5			
14.549	14.549	(1.048)	119	2502156	50.0000	54.949	80.00- 120.00	100.00	
14.549	14.549	(1.048)	117	2656938			56.19- 156.19	106.19	

89 2,2,4-Trimethylpentane						CAS #: 540-84-1			
14.881	14.881	(1.072)	57	3576925	50.0000	53.760	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
89 2,2,4-Trimethylpentane (continued)									
14.881	14.881	(1.072)	56	1163007			0.00- 83.27	32.51	
14.881	14.881	(1.072)	41	928356			0.00- 77.74	25.95	

91 Benzene CAS #: 71-43-2									
14.964	14.964	(0.958)	78	3084868	50.0000	59.561	80.00- 120.00	100.00	
14.964	14.964	(0.958)	77	697162			0.00- 73.32	22.60	

93 1,2-Dichloroethane CAS #: 107-06-2									
15.075	15.075	(0.965)	62	1497502	50.0000	57.885	80.00- 120.00	100.00	
15.075	15.075	(0.965)	64	486198			0.00- 82.87	32.47	

94 Heptane CAS #: 142-82-5									
15.185	15.185	(0.972)	71	957124	50.0000	58.176	80.00- 120.00	100.00	
15.185	15.185	(0.972)	43	1296335			77.60- 177.60	135.44	
15.185	15.185	(0.972)	57	804037			32.99- 132.99	84.01	

101 Trichloroethene CAS #: 79-01-6									
16.070	16.070	(1.028)	95	1355201	50.0000	56.628	80.00- 120.00	100.00	
16.098	16.098	(1.030)	130	1245488			41.90- 141.90	91.90	
16.070	16.070	(1.028)	97	863743			13.74- 113.74	63.74	

104 1,2-Dichloropropane CAS #: 78-87-5									
16.568	16.568	(1.060)	63	1050115	50.0000	60.674	80.00- 120.00	100.00	
16.568	16.568	(1.060)	62	771504			23.47- 123.47	73.47	
16.568	16.568	(1.060)	41	588871			6.08- 106.08	56.08	

106 1,4-Dioxane CAS #: 123-91-1									
16.706	16.706	(1.069)	88	740427	50.0000	53.946	80.00- 120.00	100.00	
16.678	16.678	(1.067)	58	427316			7.71- 107.71	57.71	
16.678	16.678	(1.067)	57	149276			0.00- 69.86	20.16	

107 Bromodichloromethane CAS #: 75-27-4									
16.982	16.982	(1.087)	83	2391489	50.0000	57.450	80.00- 120.00	100.00	
16.982	16.982	(1.087)	85	1557348			15.12- 115.12	65.12	

110 cis-1,3-Dichloropropene CAS #: 10061-01-5									
17.784	17.784	(1.138)	75	1674370	50.0000	60.069	80.00- 120.00	100.00	
17.784	17.784	(1.138)	77	536497			0.00- 82.04	32.04	
17.784	17.784	(1.138)	39	739901			0.00- 94.19	44.19	

111 4-Methyl-2-pentanone CAS #: 108-10-1									
17.978	17.978	(1.150)	58	829441	50.0000	65.401	80.00- 120.00	100.00	
17.950	17.950	(1.149)	43	1863289			168.02- 268.02	224.64	
17.978	17.978	(1.150)	85	417221			2.69- 102.69	50.30	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	3542251	50.0000	56.698	80.00- 120.00	100.00	
18.337	18.337	(1.173)	92	2158951			10.95- 110.95	60.95	

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	1825870	50.0000	55.308	80.00- 120.00	100.00	
18.752	18.752	(0.902)	77	580447			0.00- 81.79	31.79	
18.752	18.752	(0.902)	39	738656			0.00- 90.46	40.46	

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.111	(0.919)	97	1331291	50.0000	55.596	80.00- 120.00	100.00	
19.111	19.111	(0.919)	99	843694			13.37- 113.37	63.37	
19.111	19.111	(0.919)	83	1126205			34.59- 134.59	84.59	

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	1823719	50.0000	54.647	80.00- 120.00	100.00	
19.277	19.277	(0.927)	129	1249733			18.53- 118.53	68.53	
19.277	19.277	(0.927)	131	1194995			15.53- 115.53	65.53	

121 2-Hexanone						CAS #: 591-78-6			
19.416	19.416	(0.934)	58	1109308	50.0000	56.587	80.00- 120.00	100.00	
19.416	19.416	(0.934)	43	1830646			115.03- 215.03	165.03	
19.416	19.416	(0.934)	100	237792			0.00- 74.50	21.44	

122 Dibromochloromethane						CAS #: 124-48-1			
19.803	19.803	(0.952)	129	2332116	50.0000	55.406	80.00- 120.00	100.00	
19.803	19.803	(0.952)	127	1798012			25.33- 125.33	77.10	

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.052	20.052	(0.964)	107	2198722	50.0000	54.579	80.00- 120.00	100.00	
20.052	20.052	(0.964)	109	2046751			43.09- 143.09	93.09	

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.853	(1.003)	112	3114200	50.0000	53.547	80.00- 120.00	100.00	
20.853	20.853	(1.003)	114	962421			0.00- 80.90	30.90	
20.853	20.853	(1.003)	77	1914779			11.49- 111.49	61.49	

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	1646707	50.0000	55.907	80.00- 120.00	100.00	
20.936	20.936	(1.007)	91	5265106			266.55- 366.55	319.74	

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	2095248	50.0000	57.831	80.00- 120.00	100.00	
21.130	21.130	(1.016)	91	4214727			157.11- 257.11	201.16	

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	2005352	50.0000	58.925	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 o-Xylene (continued)									
21.849	21.849	(1.051)	91	4255060			162.19- 262.19	212.19	

131 Styrene CAS #: 100-42-5									
21.876	21.876	(1.052)	104	3171701	50.0000	57.510	80.00- 120.00	100.00	
21.876	21.876	(1.052)	78	1613279			0.86- 100.86	50.86	

133 Bromoform CAS #: 75-25-2									
22.291	22.291	(1.072)	173	2560673	50.0000	58.358	80.00- 120.00	100.00	
22.291	22.291	(1.072)	171	1297797			0.68- 100.68	50.68	

134 Cumene CAS #: 98-82-8									
22.429	22.429	(1.078)	105	5626918	50.0000	57.844	80.00- 120.00	100.00	
22.429	22.429	(1.078)	120	1445153			0.00- 74.52	25.68	
22.429	22.429	(1.078)	51	483855			51.79- 151.79	8.60	

140 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
23.010	23.010	(1.106)	83	3169722	50.0000	59.427	80.00- 120.00	100.00	
23.010	23.010	(1.106)	85	2060171			15.00- 115.00	65.00	

142 Propylbenzene CAS #: 103-65-1									
23.121	23.121	(1.112)	91	7197840	50.0000	58.504	80.00- 120.00	100.00	
23.121	23.121	(1.112)	120	1552606			0.00- 71.52	21.57	
23.121	23.121	(1.112)	105	259202			0.00- 53.54	3.60	

145 4-Ethyltoluene CAS #: 622-96-8									
23.287	23.287	(1.120)	105	6266315	50.0000	60.472	80.00- 120.00	100.00	
23.287	23.287	(1.120)	120	1865460			0.00- 79.77	29.77	

147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
23.397	23.397	(1.125)	105	5219065	50.0000	61.889	80.00- 120.00	100.00	
23.397	23.397	(1.125)	120	2555631			0.29- 100.29	48.97	

150 1,2,4-Trimethylbenzene CAS #: 95-63-6									
24.033	24.033	(1.156)	105	5019436	50.0000	63.953	80.00- 120.00	100.00	
24.033	24.033	(1.156)	120	2327738			0.00- 94.69	46.37	

155 1,3-Dichlorobenzene CAS #: 541-73-1									
24.586	24.586	(1.182)	146	3455549	50.0000	58.174	80.00- 120.00	100.00	
24.586	24.586	(1.182)	148	2195648			14.61- 114.61	63.54	
24.586	24.586	(1.182)	111	1419178			0.00- 92.01	41.07	

156 1,4-Dichlorobenzene CAS #: 106-46-7									
24.724	24.724	(1.189)	146	3586650	50.0000	58.112	80.00- 120.00	100.00	
24.724	24.724	(1.189)	148	2274520			13.83- 113.83	63.42	
24.724	24.724	(1.189)	111	1431252			0.00- 89.75	39.90	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

159 alpha-Chlorotoluene						CAS #: 100-44-7			
24.946	24.946	(1.199)	91	4950861	50.0000	57.970	80.00- 120.00	100.00	
24.946	24.946	(1.199)	126	942456			0.00- 69.65	19.04	

161 1,2-Dichlorobenzene						CAS #: 95-50-1			
25.360	25.360	(1.219)	146	3356044	50.0000	58.920	80.00- 120.00	100.00	
25.360	25.360	(1.219)	148	2132374			13.54- 113.54	63.54	
25.360	25.360	(1.219)	111	1428825			0.00- 92.57	42.57	

165 1,2,4-Trichlorobenzene						CAS #: 120-82-1			
28.153	28.153	(1.354)	180	2285035	50.0000	58.485	80.00- 120.00	100.00	
28.153	28.153	(1.354)	182	2174215			45.15- 145.15	95.15	

166 Hexachlorobutadiene						CAS #: 87-68-3			
28.319	28.319	(1.362)	225	2217692	50.0000	62.188	80.00- 120.00	100.00	
28.319	28.319	(1.362)	223	1383115			13.46- 113.46	62.37	

29 Isopentane						CAS #: 78-78-4			
8.273	8.273	(0.596)	43	976935	50.0000	55.302	80.00- 120.00	100.00	
8.273	8.273	(0.596)	57	739303			26.79- 126.79	75.68	

19 Butane						CAS #: 106-97-8			
6.807	6.807	(0.490)	58	175747	50.0000	56.020	80.00- 120.00	100.00	
6.807	6.807	(0.490)	43	1193572			672.59- 772.59	679.14	

102 Methyl Cyclohexane						CAS #: 108-87-2			
16.347	16.347	(1.177)	83	1734602	50.0000	57.332	80.00- 120.00	100.00	
16.347	16.347	(1.177)	98	772120			0.00- 95.49	44.51	
16.347	16.347	(1.177)	55	1191934			16.76- 116.76	68.72	

167 Naphthalene						CAS #: 91-20-3			
28.678	28.678	(1.379)	128	3541941	50.0000	54.999	80.00- 120.00	100.00	
28.678	28.678	(1.379)	127	427778			0.00- 62.56	12.08	

Report Date: 03-Feb-2008 15:20

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 03-FEB-2008

Lab File ID: t020302.d

Calibration Time: 15:01

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: xp

Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m

Misc Info: 100ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	323259	193955	452563	323259	0.00
97 1,4-Difluorobenze	1297188	778313	1816063	1297188	0.00
126 Chlorobenzene-d5	1219852	731911	1707793	1219852	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/03Feb2008,b/t020302.d
 Date: 03-FEB-2008 15:01
 Client ID: CCV-1
 Sample Info: 100mL #1576-197A

Column phase: RTX-624

Instrument: msdt,i
 Operator: xp
 Column diameter: 0.53

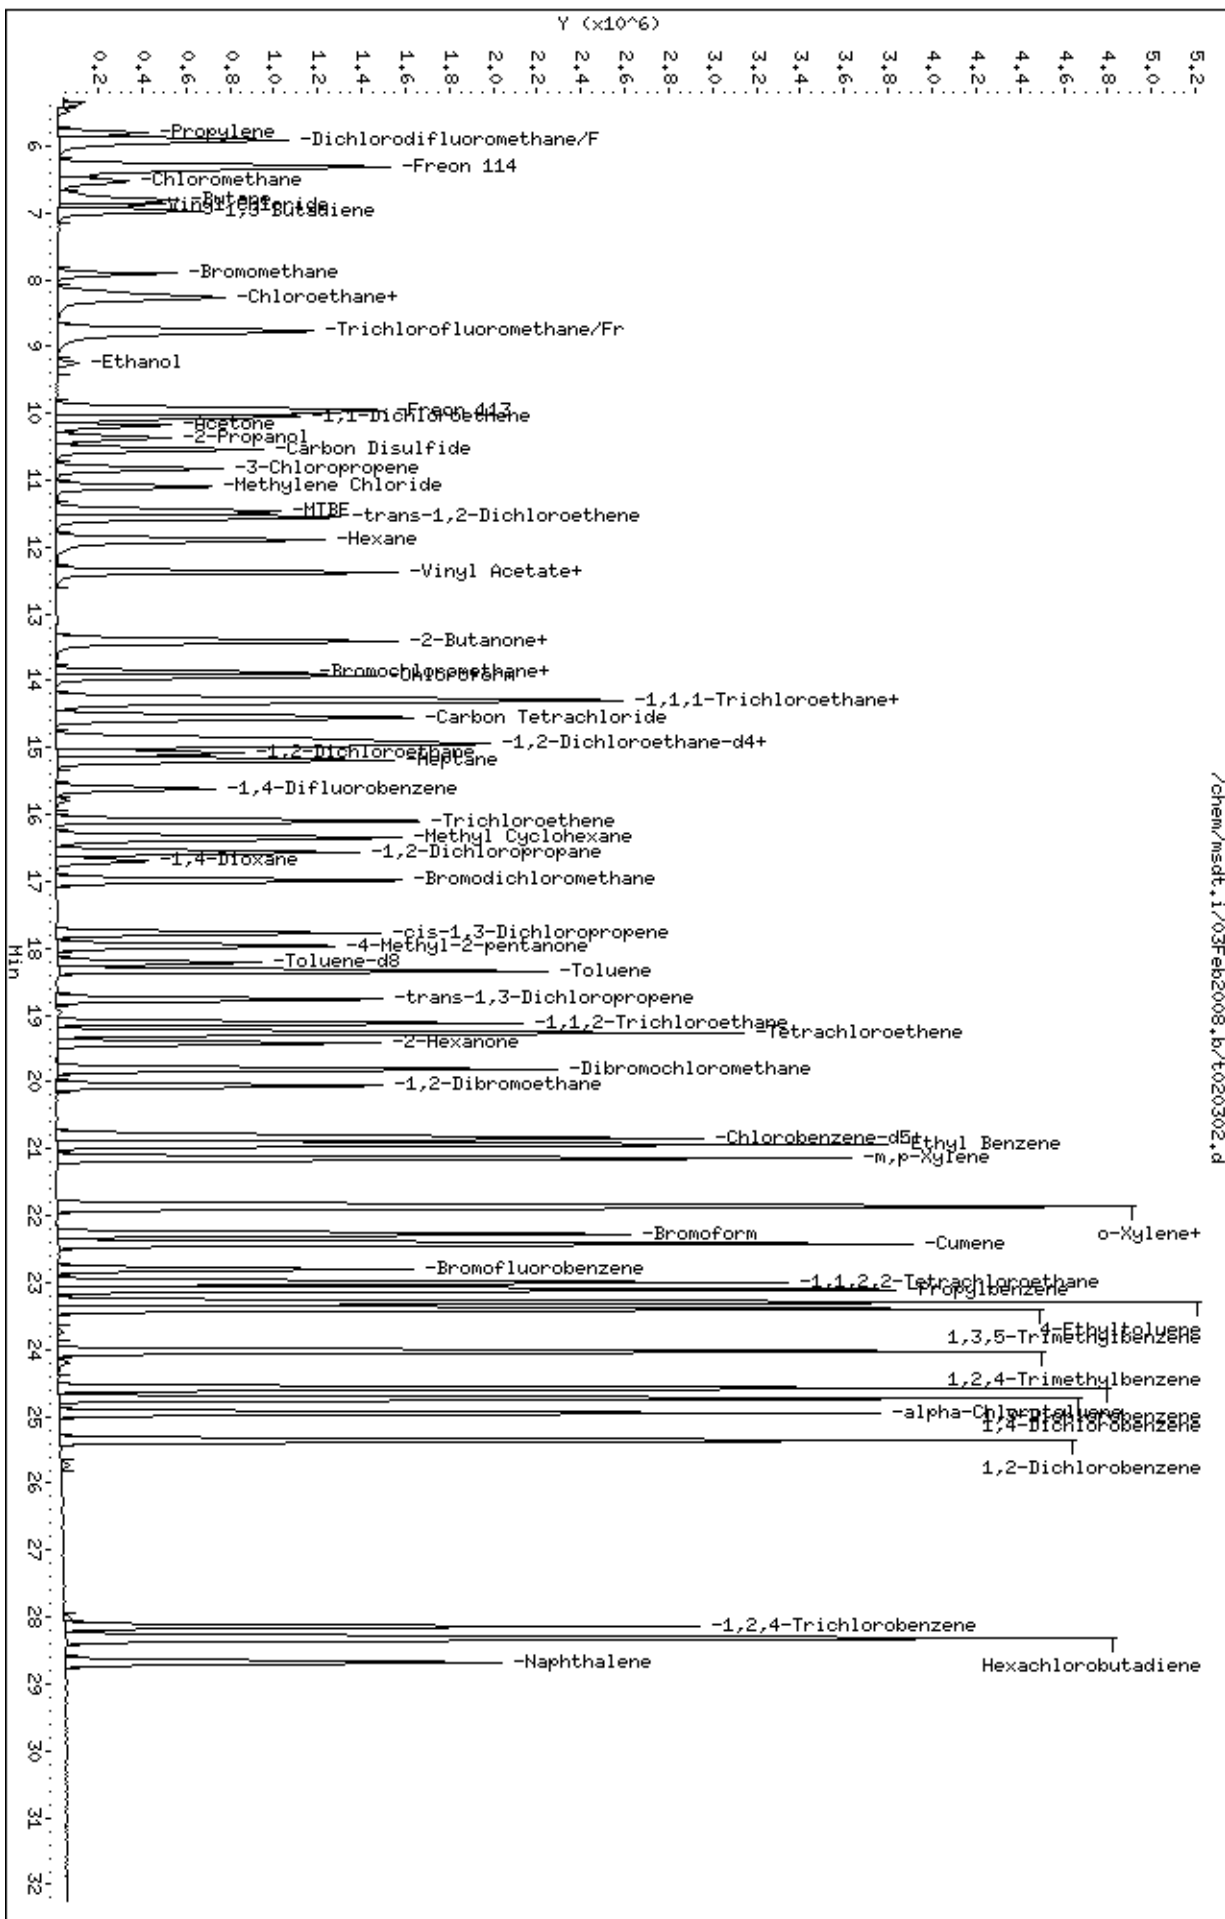



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0801560-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020303	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 2/3/08 03:47 PM

Compound	%Recovery
Freon 12	103
Freon 114	105
Vinyl Chloride	113
Bromomethane	107
Chloroethane	111
Freon 11	101
1,1-Dichloroethene	124
Freon 113	117
Methylene Chloride	112
1,1-Dichloroethane	116
cis-1,2-Dichloroethene	110
Chloroform	116
1,1,1-Trichloroethane	107
Carbon Tetrachloride	105
Benzene	119
1,2-Dichloroethane	116
Trichloroethene	112
1,2-Dichloropropane	119
cis-1,3-Dichloropropene	118
Toluene	117
trans-1,3-Dichloropropene	110
1,1,2-Trichloroethane	110
Tetrachloroethene	109
1,2-Dibromoethane (EDB)	104
Chlorobenzene	104
Ethyl Benzene	108
m,p-Xylene	111
o-Xylene	114
Styrene	109
1,1,2,2-Tetrachloroethane	114
1,3,5-Trimethylbenzene	116
1,2,4-Trimethylbenzene	120
1,3-Dichlorobenzene	112
1,4-Dichlorobenzene	109
alpha-Chlorotoluene	119
1,2-Dichlorobenzene	111
1,3-Butadiene	105
Hexane	109
Cyclohexane	116



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0801560-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	t020303	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 2/3/08 03:47 PM

Compound	%Recovery
Heptane	114
Bromodichloromethane	114
Dibromochloromethane	109
Cumene	114
Propylbenzene	115
Chloromethane	105
1,2,4-Trichlorobenzene	112
Hexachlorobutadiene	114
Acetone	114
Carbon Disulfide	112
2-Propanol	109
trans-1,2-Dichloroethene	110
2-Butanone (Methyl Ethyl Ketone)	114
Tetrahydrofuran	119
1,4-Dioxane	110
4-Methyl-2-pentanone	131
2-Hexanone	111
Bromoform	113
4-Ethyltoluene	117
Ethanol	112
Methyl tert-butyl ether	110
3-Chloropropene	110
2,2,4-Trimethylpentane	105
Naphthalene	89

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	106	70-130
1,2-Dichloroethane-d4	100	70-130
4-Bromofluorobenzene	95	70-130

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 03Feb2008
 Sample Matrix: GAS Fraction: VOA
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Level: LOW Operator: xp
 Data Type: MS DATA SampleType: LCS
 SpikeList File: 2926Spectra.spk Quant Type: ISTD
 Sublist File: AT04ENSR.sub
 Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m
 Misc Info: 100ppbv -> 50ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
12 Dichlorodifluorome	50.000	51.561	103.12	70-130
16 Freon 114	50.000	52.364	104.73	70-130
18 Chloromethane	50.000	52.353	104.71	70-130
20 Vinyl Chloride	50.000	56.696	113.39	70-130
22 1,3-Butadiene	50.000	52.603	105.21	60-140
25 Bromomethane	50.000	53.307	106.61	70-130
27 Chloroethane	50.000	55.417	110.83	70-130
31 Trichlorofluoromet	50.000	50.656	101.31	70-130
38 Ethanol	50.000	56.151	112.30	60-140
42 Freon 113	50.000	58.742	117.48	70-130
43 1,1-Dichloroethene	50.000	62.153	124.31	70-130
45 Acetone	50.000	56.938	113.88	60-140
47 Carbon Disulfide	50.000	55.884	111.77	60-140
46 2-Propanol	50.000	54.659	109.32	60-140
54 Methylene Chloride	50.000	56.237	112.47	70-130
60 MTBE	50.000	54.812	109.62	60-140
61 trans-1,2-Dichloro	50.000	55.094	110.19	60-140
65 Hexane	50.000	54.452	108.90	60-140
69 Vinyl Acetate	50.000	53.844	107.69	60-140
70 1,1-Dichloroethane	50.000	57.933	115.87	70-130
76 cis-1,2-Dichloroet	50.000	55.241	110.48	70-130
75 2-Butanone	50.000	56.970	113.94	60-140
80 Tetrahydrofuran	50.000	59.670	119.34	60-140
82 Chloroform	50.000	58.268	116.54	70-130
85 Cyclohexane	50.000	58.100	116.20	60-140
83 1,1,1-Trichloroeth	50.000	53.738	107.48	70-130
87 Carbon Tetrachlori	50.000	52.336	104.67	70-130
91 Benzene	50.000	59.305	118.61	70-130
93 1,2-Dichloroethane	50.000	58.047	116.09	70-130
94 Heptane	50.000	57.135	114.27	60-140
101 Trichloroethene	50.000	56.177	112.35	70-130
104 1,2-Dichloropropan	50.000	59.613	119.23	70-130
106 1,4-Dioxane	50.000	54.925	109.85	60-140

Report Date: 04-Feb-2008 08:17

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
107 Bromodichlorometha	50.000	57.239	114.48	60-140
110 cis-1,3-Dichloropr	50.000	58.823	117.65	70-130
111 4-Methyl-2-pentano	50.000	65.300	130.60	60-140
114 Toluene	50.000	58.392	116.78	70-130
116 trans-1,3-Dichloro	50.000	54.790	109.58	70-130
117 1,1,2-Trichloroeth	50.000	54.800	109.60	70-130
120 Tetrachloroethene	50.000	54.374	108.75	70-130
121 2-Hexanone	50.000	55.489	110.98	60-140
122 Dibromochlorometha	50.000	54.549	109.10	60-140
123 1,2-Dibromoethane	50.000	52.054	104.11	70-130
127 Chlorobenzene	50.000	52.055	104.11	70-130
128 Ethyl Benzene	50.000	54.142	108.28	70-130
129 m,p-Xylene	50.000	55.435	110.87	70-130
130 o-Xylene	50.000	57.114	114.23	70-130
131 Styrene	50.000	54.627	109.25	70-130
133 Bromoform	50.000	56.736	113.47	60-140
140 1,1,2,2-Tetrachlor	50.000	57.150	114.30	70-130
145 4-Ethyltoluene	50.000	58.318	116.64	60-140
147 1,3,5-Trimethylben	50.000	58.028	116.06	70-130
150 1,2,4-Trimethylben	50.000	59.763	119.53	70-130
155 1,3-Dichlorobenzen	50.000	55.751	111.50	70-130
156 1,4-Dichlorobenzen	50.000	54.456	108.91	70-130
159 alpha-Chlorotoluen	50.000	59.476	118.95	70-130
161 1,2-Dichlorobenzen	50.000	55.571	111.14	70-130
165 1,2,4-Trichloroben	50.000	56.025	112.05	70-130
166 Hexachlorobutadien	50.000	57.199	114.40	70-130
142 Propylbenzene	50.000	57.385	114.77	60-140
134 Cumene	50.000	57.053	114.11	60-140
51 3-Chloropropene	50.000	55.131	110.26	60-140
89 2,2,4-Trimethylpen	50.000	52.419	104.84	60-140
19 Butane	50.000	53.603	107.21	70-130
29 Isopentane	50.000	51.271	102.54	70-130
102 Methyl Cyclohexane	50.000	55.811	111.62	70-130
11 Propylene	50.000	56.746	113.49	60-140
167 Naphthalene	50.000	44.743	89.49	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 90 1,2-Dichloroethane	25.000	24.908	99.63	70-130
\$ 113 Toluene-d8	25.000	26.642	106.57	70-130
\$ 137 Bromofluorobenzene	25.000	23.698	94.79	70-130

Report Date: 04-Feb-2008 08:17

Air Toxics Ltd.

AMBIENT AIR METHOD TO14

Data file : /chem/msdt.i/03Feb2008.b/t020303.d
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1
 Inj Date : 03-FEB-2008 15:47
 Operator : xp Inst ID: msdt.i
 Smp Info : 100mL #1576-169A
 Misc Info : 100ppbv -> 50ppbv
 Comment :
 Method : /chem/msdt.i/03Feb2008.b/t14q1213e.m
 Meth Date : 03-Feb-2008 18:54 dmendoza Quant Type: ISTD
 Cal Date : 25-JAN-2008 13:09 Cal File: t012506.d
 Als bottle: 1 QC Sample: LCS
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: AT04ENSR.sub
 Target Version: 3.50 Sample Matrix: AIR
 Processing Host: eeyore

Concentration Formula: Amt * DF * CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	(PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 81 Bromochloromethane CAS #: 74-97-5									
13.886	13.886	(1.000)	130	339461	25.0000		80.00- 120.00	100.00	
13.886	13.886	(1.000)	128	256566			29.43- 129.43	75.58	
13.858	13.886	(1.000)	49	565025			119.82- 219.82	166.45	

* 97 1,4-Difluorobenzene CAS #: 540-36-3									
15.628	15.628	(1.000)	114	1343796	25.0000		80.00- 120.00	100.00	
15.628	15.628	(1.000)	88	212063			0.00- 66.60	15.78	

* 126 Chlorobenzene-d5 CAS #: 3114-55-4									
20.798	20.798	(1.000)	117	1254995	25.0000		80.00- 120.00	100.00	
20.798	20.798	(1.000)	82	716844			5.74- 105.74	57.12	

\$ 90 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
14.936	14.936	(1.076)	65	538333	24.9076	24.908	80.00- 120.00	100.00	
14.936	14.936	(1.076)	67	301415			3.93- 103.93	55.99	

\$ 113 Toluene-d8 CAS #: 2037-26-5									
18.199	18.199	(1.165)	98	1358128	26.6425	26.642	80.00- 120.00	100.00	
18.199	18.199	(1.165)	70	154623			0.00- 61.06	11.39	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	(PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 113 Toluene-d8 (continued)

18.199	18.199	(1.165)	100	941323			18.52- 118.52	69.31
--------	--------	---------	-----	--------	--	--	---------------	-------

\$ 137 Bromofluorobenzene

CAS #: 460-00-4

22.789	22.789	(1.096)	174	815693	23.6978	23.698	80.00- 120.00	100.00
22.789	22.789	(1.096)	95	1036166			75.43- 175.43	127.03
22.789	22.789	(1.096)	176	797693			47.55- 147.55	97.79

11 Propylene

CAS #: 115-07-1

5.812	5.812	(0.419)	41	514467	56.7463	56.746	80.00- 120.00	100.00
5.812	5.812	(0.419)	42	355216			17.44- 117.44	69.05
5.812	5.812	(0.419)	39	406594			31.05- 131.05	79.03

12 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

5.923	5.923	(0.427)	85	3065588	51.5611	51.561	80.00- 120.00	100.00
5.923	5.923	(0.427)	87	973997			0.00- 82.50	31.77

16 Freon 114

CAS #: 76-14-2

6.310	6.310	(0.454)	135	2035306	52.3642	52.364	80.00- 120.00	100.00
6.310	6.310	(0.454)	137	658550			0.00- 81.78	32.36

18 Chloromethane

CAS #: 74-87-3

6.531	6.531	(0.470)	50	673277	52.3531	52.353	80.00- 120.00	100.00
6.531	6.531	(0.470)	52	222840			0.00- 83.59	33.10

20 Vinyl Chloride

CAS #: 75-01-4

6.890	6.890	(0.496)	62	911967	56.6960	56.696	80.00- 120.00	100.00
6.890	6.890	(0.496)	64	300845			0.00- 94.54	32.99

22 1,3-Butadiene

CAS #: 106-99-0

6.973	6.973	(0.502)	54	660512	52.6032	52.603	80.00- 120.00	100.00
6.973	6.973	(0.502)	39	615888			61.08- 161.08	93.24

25 Bromomethane

CAS #: 74-83-9

7.913	7.913	(0.570)	94	908059	53.3067	53.307	80.00- 120.00	100.00
7.913	7.913	(0.570)	96	849010			44.09- 144.09	93.50

27 Chloroethane

CAS #: 75-00-3

8.190	8.190	(0.590)	64	475643	55.4173	55.417	80.00- 120.00	100.00
8.190	8.190	(0.590)	49	124337			0.00- 76.61	26.14
8.190	8.190	(0.590)	66	156543			0.00- 85.87	32.91

31 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

8.770	8.771	(0.632)	101	3366698	50.6560	50.656	80.00- 120.00	100.00
8.770	8.771	(0.632)	103	2175871			15.11- 115.11	64.63

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPEV)	FINAL	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
38 Ethanol						CAS #: 64-17-5				
9.241	9.241	(0.665)	45	253102	56.1508	56.151	80.00- 120.00	100.00		
9.241	9.241	(0.665)	43	59976			0.00- 74.87	23.70		
9.241	9.241	(0.665)	46	99201			0.00- 88.05	39.19		

42 Freon 113						CAS #: 76-13-1				
9.959	9.960	(0.717)	151	1757070	58.7418	58.742	80.00- 120.00	100.00		
9.959	9.960	(0.717)	153	1122199			13.84- 113.84	63.87		
9.959	9.960	(0.717)	101	2270733			80.24- 180.24	129.23		

43 1,1-Dichloroethene						CAS #: 75-35-4				
10.042	10.042	(0.723)	61	1629522	62.1533	62.153	80.00- 120.00	100.00		
10.042	10.042	(0.723)	96	1019764			10.92- 110.92	62.58		
10.042	10.042	(0.723)	98	645579			0.00- 89.98	39.62		

45 Acetone						CAS #: 67-64-1				
10.181	10.181	(0.733)	58	463489	56.9381	56.938	80.00- 120.00	100.00		
10.181	10.181	(0.733)	43	1388652			264.94- 364.94	299.61		

46 2-Propanol						CAS #: 67-63-0				
10.374	10.374	(0.747)	45	1473931	54.6591	54.659	80.00- 120.00	100.00		
10.374	10.374	(0.747)	43	374052			0.00- 78.96	25.38		
10.374	10.374	(0.747)	59	62924			0.00- 54.06	4.27		

47 Carbon Disulfide						CAS #: 75-15-0				
10.540	10.540	(0.759)	76	2793453	55.8836	55.884	80.00- 120.00	100.00		

51 3-Chloropropene						CAS #: 107-05-1				
10.817	10.817	(0.779)	76	470346	55.1313	55.131	80.00- 120.00	100.00		
10.817	10.817	(0.779)	41	1007536			176.05- 276.05	214.21		

54 Methylene Chloride						CAS #: 75-09-2				
11.093	11.093	(0.799)	49	931060	56.2370	56.237	80.00- 120.00	100.00		
11.121	11.093	(0.801)	84	842150			38.59- 138.59	90.45		
11.093	11.093	(0.799)	51	283194			0.00- 83.78	30.42		

60 MTBE						CAS #: 1634-04-4				
11.452	11.453	(0.825)	73	3041681	54.8119	54.812	80.00- 120.00	100.00		
11.452	11.453	(0.825)	57	577469			0.00- 69.06	18.99		
11.452	11.453	(0.825)	41	552981			0.00- 70.94	18.18		

61 trans-1,2-Dichloroethene						CAS #: 156-60-5				
11.563	11.563	(0.833)	96	1106722	55.0935	55.094	80.00- 120.00	100.00		
11.535	11.563	(0.831)	61	1489753			89.00- 189.00	134.61		
11.563	11.563	(0.833)	98	713514			15.85- 115.85	64.47		

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
65 Hexane						CAS #: 110-54-3			
11.895	11.895	(0.857)	57	1518699	54.4523	54.452		80.00- 120.00	100.00
11.895	11.895	(0.857)	43	867320				8.15- 108.15	57.11
11.895	11.895	(0.857)	86	277489				0.00- 69.59	18.27

69 Vinyl Acetate						CAS #: 108-05-4			
12.365	12.365	(0.890)	86	267981	53.8439	53.844		80.00- 120.00	100.00
12.365	12.365	(0.890)	43	2414108				903.55-1003.55	900.85

70 1,1-Dichloroethane						CAS #: 75-34-3			
12.365	12.365	(0.890)	63	2029753	57.9329	57.933		80.00- 120.00	100.00
12.365	12.365	(0.890)	65	654589				0.00- 82.56	32.25

75 2-Butanone						CAS #: 78-93-3			
13.388	13.388	(0.964)	72	528345	56.9700	56.970		80.00- 120.00	100.00
13.388	13.388	(0.964)	43	1725815				289.29- 389.29	326.65
13.388	13.388	(0.964)	57	151924				0.00- 78.78	28.75

76 cis-1,2-Dichloroethene						CAS #: 156-59-2			
13.416	13.416	(0.966)	61	1359276	55.2409	55.241		80.00- 120.00	100.00
13.416	13.416	(0.966)	96	1086648				30.44- 130.44	79.94
13.416	13.416	(0.966)	98	695326				1.26- 101.26	51.15

80 Tetrahydrofuran						CAS #: 109-99-9			
13.858	13.858	(0.998)	42	881864	59.6706	59.670		80.00- 120.00	100.00
13.858	13.858	(0.998)	71	469304				3.18- 103.18	53.22
13.858	13.858	(0.998)	72	495975				8.31- 108.31	56.24

82 Chloroform						CAS #: 67-66-3			
13.941	13.941	(1.004)	83	2388757	58.2676	58.268		80.00- 120.00	100.00
13.941	13.941	(1.004)	85	1563693				14.98- 114.98	65.46

83 1,1,1-Trichloroethane						CAS #: 71-55-6			
14.273	14.273	(1.028)	97	2638247	53.7375	53.738		80.00- 120.00	100.00
14.273	14.273	(1.028)	99	1703942				14.86- 114.86	64.59

85 Cyclohexane						CAS #: 110-82-7			
14.300	14.300	(1.030)	84	1455709	58.0997	58.100		80.00- 120.00	100.00
14.300	14.300	(1.030)	56	1415745				48.45- 148.45	97.25
14.300	14.300	(1.030)	41	743099				1.15- 101.15	51.05

87 Carbon Tetrachloride						CAS #: 56-23-5			
14.549	14.549	(1.048)	119	2502643	52.3362	52.336		80.00- 120.00	100.00
14.549	14.549	(1.048)	117	2615564				56.19- 156.19	104.51

89 2,2,4-Trimethylpentane						CAS #: 540-84-1			
14.881	14.881	(1.072)	57	3662551	52.4193	52.419		80.00- 120.00	100.00

CONCENTRATIONS

RT	EXP RT (REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====
89 2,2,4-Trimethylpentane (continued)							
14.881	14.881 (1.072)	56	1185027			0.00- 83.27	32.36
14.881	14.881 (1.072)	41	937454			0.00- 77.74	25.60

91 Benzene CAS #: 71-43-2							
14.964	14.964 (0.958)	78	3181963	59.3051	59.305	80.00- 120.00	100.00
14.964	14.964 (0.958)	77	725696			0.00- 73.32	22.81

93 1,2-Dichloroethane CAS #: 107-06-2							
15.075	15.075 (0.965)	62	1555640	58.0468	58.047	80.00- 120.00	100.00
15.075	15.075 (0.965)	64	498424			0.00- 82.87	32.04

94 Heptane CAS #: 142-82-5							
15.185	15.185 (0.972)	71	973773	57.1348	57.135	80.00- 120.00	100.00
15.185	15.185 (0.972)	43	1340086			77.60- 177.60	137.62
15.185	15.185 (0.972)	57	830878			32.99- 132.99	85.33

101 Trichloroethene CAS #: 79-01-6							
16.098	16.070 (1.030)	95	1392706	56.1767	56.177	80.00- 120.00	100.00
16.098	16.070 (1.030)	130	1267684			41.90- 141.90	91.02
16.098	16.070 (1.030)	97	887260			13.74- 113.74	63.71

104 1,2-Dichloropropane CAS #: 78-87-5							
16.568	16.568 (1.060)	63	1068828	59.6134	59.613	80.00- 120.00	100.00
16.568	16.568 (1.060)	62	761625			23.47- 123.47	71.26
16.568	16.568 (1.060)	41	587075			6.08- 106.08	54.93

106 1,4-Dioxane CAS #: 123-91-1							
16.706	16.706 (1.069)	88	780952	54.9252	54.925	80.00- 120.00	100.00
16.678	16.706 (1.067)	58	440318			7.71- 107.71	56.38
16.678	16.706 (1.067)	57	149173			0.00- 69.86	19.10

107 Bromodichloromethane CAS #: 75-27-4							
17.010	16.982 (1.088)	83	2468326	57.2394	57.239	80.00- 120.00	100.00
17.010	16.982 (1.088)	85	1597835			15.12- 115.12	64.73

110 cis-1,3-Dichloropropene CAS #: 10061-01-5							
17.784	17.784 (1.138)	75	1698548	58.8229	58.823	80.00- 120.00	100.00
17.784	17.784 (1.138)	77	557779			0.00- 82.04	32.84
17.784	17.784 (1.138)	39	747928			0.00- 94.19	44.03

111 4-Methyl-2-pentanone CAS #: 108-10-1							
17.978	17.978 (1.150)	58	857917	65.2998	65.300	80.00- 120.00	100.00
17.978	17.978 (1.150)	43	1930810			168.02- 268.02	225.06
17.978	17.978 (1.150)	85	422923			2.69- 102.69	49.30

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				(PPEV)	(PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====

114 Toluene						CAS #: 108-88-3			
18.337	18.337	(1.173)	91	3779209	58.3923	58.392	80.00-	120.00	100.00
18.337	18.337	(1.173)	92	2289713			10.95-	110.95	60.59

116 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
18.752	18.752	(0.902)	75	1860847	54.7896	54.790	80.00-	120.00	100.00
18.780	18.752	(0.903)	77	586118			0.00-	81.79	31.50
18.752	18.752	(0.902)	39	743806			0.00-	90.46	39.97

117 1,1,2-Trichloroethane						CAS #: 79-00-5			
19.111	19.111	(0.919)	97	1350042	54.8005	54.800	80.00-	120.00	100.00
19.111	19.111	(0.919)	99	858527			13.37-	113.37	63.59
19.111	19.111	(0.919)	83	1139248			34.59-	134.59	84.39

120 Tetrachloroethene						CAS #: 127-18-4			
19.277	19.277	(0.927)	166	1866889	54.3737	54.374	80.00-	120.00	100.00
19.277	19.277	(0.927)	129	1275790			18.53-	118.53	68.34
19.277	19.277	(0.927)	131	1217158			15.53-	115.53	65.20

121 2-Hexanone						CAS #: 591-78-6			
19.416	19.416	(0.934)	58	1119109	55.4889	55.489	80.00-	120.00	100.00
19.416	19.416	(0.934)	43	1838322			115.03-	215.03	164.27
19.416	19.416	(0.934)	100	239594			0.00-	74.50	21.41

122 Dibromochloromethane						CAS #: 124-48-1			
19.803	19.803	(0.952)	129	2362157	54.5487	54.549	80.00-	120.00	100.00
19.803	19.803	(0.952)	127	1809093			25.33-	125.33	76.59

123 1,2-Dibromoethane						CAS #: 106-93-4			
20.051	20.052	(0.964)	107	2157439	52.0546	52.054	80.00-	120.00	100.00
20.051	20.052	(0.964)	109	2009037			43.09-	143.09	93.12

127 Chlorobenzene						CAS #: 108-90-7			
20.853	20.853	(1.003)	112	3114613	52.0546	52.055	80.00-	120.00	100.00
20.853	20.853	(1.003)	114	980772			0.00-	80.90	31.49
20.853	20.853	(1.003)	77	1941288			11.49-	111.49	62.33

128 Ethyl Benzene						CAS #: 100-41-4			
20.936	20.936	(1.007)	106	1640673	54.1421	54.142	80.00-	120.00	100.00
20.936	20.936	(1.007)	91	5241109			266.55-	366.55	319.45

129 m,p-Xylene						CAS #: 108-38-3			
21.130	21.130	(1.016)	106	2066292	55.4346	55.435	80.00-	120.00	100.00
21.130	21.130	(1.016)	91	4161146			157.11-	257.11	201.38

130 o-Xylene						CAS #: 95-47-6			
21.849	21.849	(1.051)	106	1999723	57.1140	57.114	80.00-	120.00	100.00

CONCENTRATIONS

RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
130 o-Xylene (continued)								
21.849	21.849	(1.051)	91	4226038			162.19- 262.19	211.33

131 Styrene						CAS #: 100-42-5		
21.876	21.876	(1.052)	104	3099535	54.6274	54.627	80.00- 120.00	100.00
21.876	21.876	(1.052)	78	1594785			0.86- 100.86	51.45

133 Bromoform						CAS #: 75-25-2		
22.291	22.291	(1.072)	173	2561238	56.7365	56.736	80.00- 120.00	100.00
22.291	22.291	(1.072)	171	1306981			0.68- 100.68	51.03

134 Cumene						CAS #: 98-82-8		
22.429	22.429	(1.078)	105	5709828	57.0531	57.053	80.00- 120.00	100.00
22.429	22.429	(1.078)	120	1472204			0.00- 74.52	25.78
22.429	22.429	(1.078)	51	482506			51.79- 151.79	8.45

140 1,1,2,2-Tetrachloroethane						CAS #: 79-34-5		
23.010	23.010	(1.106)	83	3136123	57.1505	57.150	80.00- 120.00	100.00
23.010	23.010	(1.106)	85	2016674			15.00- 115.00	64.30

142 Propylbenzene						CAS #: 103-65-1		
23.121	23.121	(1.112)	91	7263472	57.3846	57.385	80.00- 120.00	100.00
23.121	23.121	(1.112)	120	1572539			0.00- 71.52	21.65
23.121	23.121	(1.112)	105	265152			0.00- 53.54	3.65

145 4-Ethyltoluene						CAS #: 622-96-8		
23.286	23.287	(1.120)	105	6217130	58.3178	58.318	80.00- 120.00	100.00
23.286	23.287	(1.120)	120	1819277			0.00- 79.77	29.26

147 1,3,5-Trimethylbenzene						CAS #: 108-67-8		
23.397	23.397	(1.125)	105	5034384	58.0277	58.028	80.00- 120.00	100.00
23.397	23.397	(1.125)	120	2432356			0.29- 100.29	48.31

150 1,2,4-Trimethylbenzene						CAS #: 95-63-6		
24.033	24.033	(1.156)	105	4825730	59.7633	59.763	80.00- 120.00	100.00
24.033	24.033	(1.156)	120	2219746			0.00- 94.69	46.00

155 1,3-Dichlorobenzene						CAS #: 541-73-1		
24.586	24.586	(1.182)	146	3407013	55.7510	55.751	80.00- 120.00	100.00
24.586	24.586	(1.182)	148	2166186			14.61- 114.61	63.58
24.586	24.586	(1.182)	111	1400740			0.00- 92.01	41.11

156 1,4-Dichlorobenzene						CAS #: 106-46-7		
24.724	24.724	(1.189)	146	3457815	54.4559	54.456	80.00- 120.00	100.00
24.724	24.724	(1.189)	148	2201745			13.83- 113.83	63.67
24.724	24.724	(1.189)	111	1364174			0.00- 89.75	39.45

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	

159 alpha-Chlorotoluene						CAS #:	100-44-7		
24.945	24.946	(1.199)	91	5225866	59.4762	59.476	80.00-	120.00	100.00
24.945	24.946	(1.199)	126	989528			0.00-	69.65	18.94

161 1,2-Dichlorobenzene						CAS #:	95-50-1		
25.360	25.360	(1.219)	146	3256519	55.5713	55.571	80.00-	120.00	100.00
25.360	25.360	(1.219)	148	2099965			13.54-	113.54	64.48
25.360	25.360	(1.219)	111	1397702			0.00-	92.57	42.92

165 1,2,4-Trichlorobenzene						CAS #:	120-82-1		
28.153	28.153	(1.354)	180	2251956	56.0248	56.025	80.00-	120.00	100.00
28.153	28.153	(1.354)	182	2136911			45.15-	145.15	94.89

166 Hexachlorobutadiene						CAS #:	87-68-3		
28.319	28.319	(1.362)	225	2098533	57.1993	57.199	80.00-	120.00	100.00
28.319	28.319	(1.362)	223	1313992			13.46-	113.46	62.61

29 Isopentane						CAS #:	78-78-4		
8.273	8.273	(0.596)	43	951127	51.2709	51.271	80.00-	120.00	100.00
8.273	8.273	(0.596)	57	733717			26.79-	126.79	77.14

19 Butane						CAS #:	106-97-8		
6.807	6.807	(0.490)	58	176593	53.6030	53.603	80.00-	120.00	100.00
6.807	6.807	(0.490)	43	1201424			672.59-	772.59	680.34

102 Methyl Cyclohexane						CAS #:	108-87-2		
16.346	16.347	(1.177)	83	1773223	55.8109	55.811	80.00-	120.00	100.00
16.346	16.347	(1.177)	98	808775			0.00-	95.49	45.61
16.346	16.347	(1.177)	55	1224192			16.76-	116.76	69.04

167 Naphthalene						CAS #:	91-20-3		
28.678	28.678	(1.379)	128	2964501	44.7434	44.743	80.00-	120.00	100.00
28.678	28.678	(1.379)	127	364094			0.00-	62.56	12.28

Report Date: 04-Feb-2008 08:17

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS
AREA AND RT SUMMARY

Instrument ID: msdt.i

Calibration Date: 03-FEB-2008

Lab File ID: t020303.d

Calibration Time: 15:01

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: xp

Method File: /chem/msdt.i/03Feb2008.b/t14q1213e.m

Misc Info: 100ppbv -> 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	323259	193955	452563	339461	5.01
97 1,4-Difluorobenze	1297188	778313	1816063	1343796	3.59
126 Chlorobenzene-d5	1219852	731911	1707793	1254995	2.88

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
81 Bromochloromethan	13.89	13.56	14.22	13.89	0.00
97 1,4-Difluorobenze	15.63	15.30	15.96	15.63	0.00
126 Chlorobenzene-d5	20.80	20.47	21.13	20.80	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msdt,i/03Feb2008,b/t020303.d
 Date: 03-FEB-2008 15:47
 Client ID: LCS-1
 Sample Info: 100mL #1576-169A

Column phase: RTX-624

Instrument: msdt,i
 Operator: xp
 Column diameter: 0.53

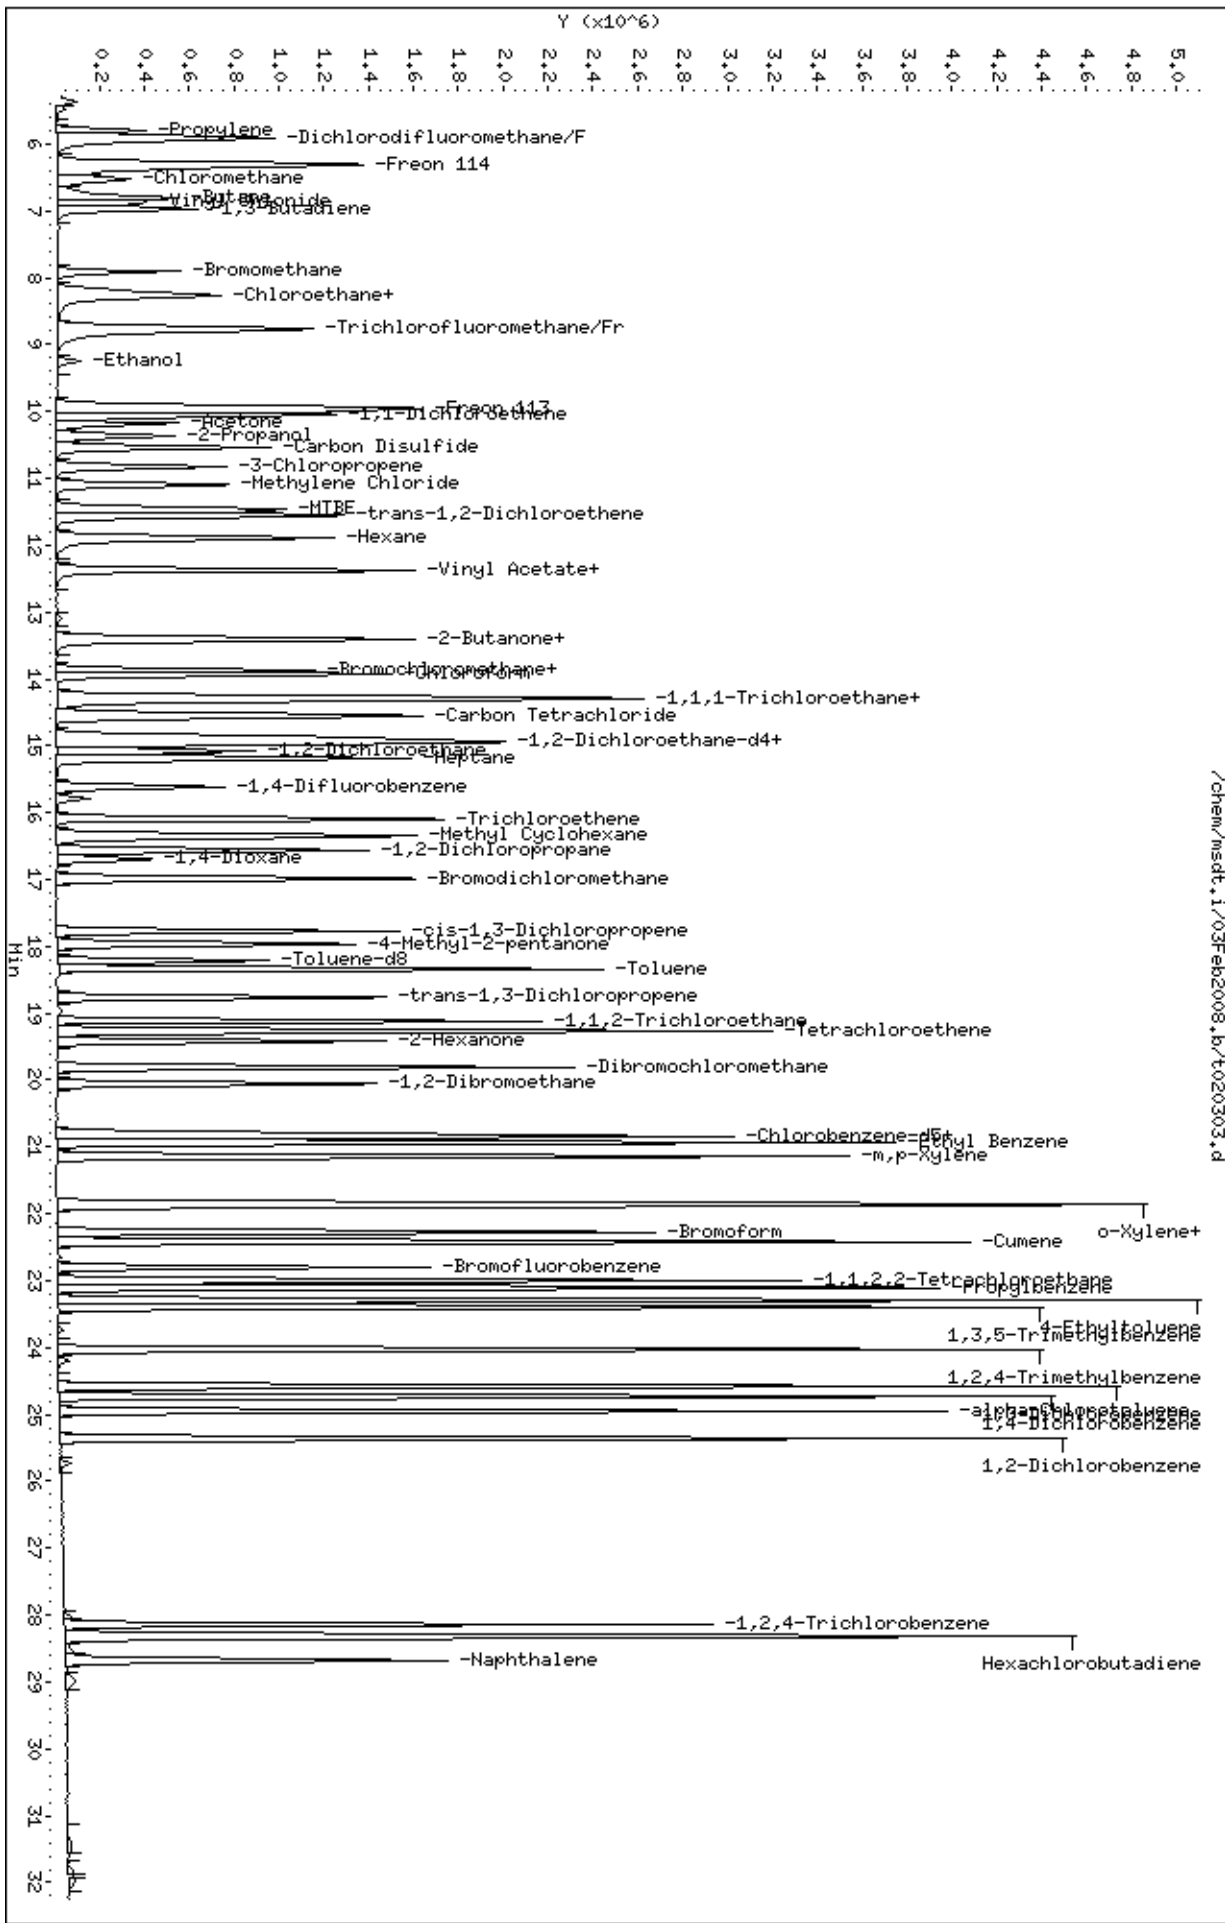

ION ABUNDANCE CRITERIA **% REL. ABUNDANCE** BFB Injection Date: 2/03/08 BFB Injection Time: 14:17:19 XP 2/3/2008

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	22.94
75	30.0 - 60.0% of mass 95	48.91
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.68
173	Less than 2.0% of mass 174	(0.00) ¹
174	Greater than 50.0% of mass 95	88.49
175	5.0 - 9.0% of mass 174	(1.37) ¹
176	Greater than 95.0% but less than 101.0% of mass 174	(96.84) ¹
177	5.0 - 9.0% of mass 176	(6.68) ²

BFB File ID: 7020301
 Tekmar Purge Flow: Z
 Vacuum: 6.42
 IS/S Std #: 1443-348 Exp. Date: 3/28/08
 BCM 323 259
 1,4-DFB 1297,188
 CB-d5 1,219,872
 Verified CCVIS vs ICAL mid-point (-40%^{AD}) XP

Verify 176/174 m/z Ratio: 1.537 ¹ - value in parenthesis is % mass 174 ² - value in parenthesis is % mass 176
 $1.537 \times 100\% = 153.7\%$

Calculation Check:

$$\frac{\text{ppbv of compound}}{\text{Area}_{\text{Sample}}} \times \text{Conc. in Areas} = \frac{\text{Conc. in Areas}}{\text{RRF}} \times \left(\frac{\text{Area}_{\text{Sample}}}{\text{RRF}} \right)$$

$$= \frac{1.332,112}{1.297,188} \times \left(\frac{25.0}{0.94836} \right) = 27.071$$
 Reported Result 27.571

NOAH Cart #: WA File #: WA
 File ID: T020302
 Compound: T01-d8
 Initials: XP

Use	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	T020301	BFB TIME blank	#1476-107	500	2ul	1.00	2-2-2008	1417	XP/BO	
✓	02	CCV-1	#1720774	500psi	100ul	1.00		1509	XP/	
✓	03	LC5-1	#1976-1604	500psi	100ul	1.00		0547	XP/	
✓	04	Leb Blank	2008	Hand	200ul	1.00		1633	XP/	
✓	05	0801545 001A	3246	600psi	200ul	1.68		1730	XP/	
✓	06	034	33079	3511psi	200ul	1.52		1808	XP/	
✓	07	0802034-01A	2831	551psi	200ul	1.60		1847	XP/	
✓	08	024	33329	551psi	200ul	1.71		1925	XP/	
✓	09	024	24222	7.11psi	200ul	1.79		2004	XP/	

James Downings
 Signature

2/4/08
 Date

10	X	T 020310	0802034-04A	20948	6.5-11.7 sps	1.0 ml	336	2-3-2008	2092	209	557 matrix
11	✓	11	System Blank	12009	Humid	200ml	100	↓	430	209	RR @ 2.5ml
12	X	12	0802034-04A	20948	6.5-11.7 sps	100x + 1.50ml	340	↓	211	209	
13	✓	13	↓ -04A	↓	↓	85ml	1370	↓	2317	209	
14	✓	14	0801538-01A	24085	7.0-14.5 sps	200ml	105	2/4/08	0712	209	
15	✓	15	0801560-01A	23988	7.0-14.5 sps	200ml	163	↓	0128	209	
16	✓	16	↓ -02A	34343	6.5-11.5 sps	↓	171	↓	0215	209	
17	✓	17	0802034-01A	33164	10-14.5 sps	↓	139	↓	0308	209	
18	✓	18	↓ -02A	25336	30-44.5 sps	↓	144	↓	0409	209	
19	✓	19	↓ -03A	33164	1.0-1.5 sps	↓	139	↓	0456	209	1/6" BT04 Med
20											
21											
22											
23											
24											
25											
26											
27											
28											
29											
30											
31											
32											

Comments:

See 2/4/08

Jana Orensky
Signature

2/4/08
Date

Report Date: 13-Dec-2007 17:14

Air Toxics Ltd.

Data file : /chem/msdt.i/13Dec2007.b/t121305.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 13-DEC-2007 17:17
 Operator : srs Inst ID: msdt.i
 Smp Info : 2uL #1467-64;BFB Tune check;BFB Tune check
 Misc Info : 50ng
 Comment :
 Method : /chem/msdt.i/13Dec2007.b/bfb.m
 Meth Date : 23-Mar-2007 09:33 tsanfel Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
1 bfb						CAS #: 460-00-4	
8.110	8.228	-0.118	95	1614284		100.00- 100.00	100.00
8.110	8.228	-0.118	50	284354		15.00- 40.00	17.61
8.110	8.228	-0.118	75	792583		30.00- 60.00	49.10
8.110	8.228	-0.118	96	105678		5.00- 9.00	6.55
8.110	8.228	-0.118	173	9541		0.00- 2.00	0.77
8.110	8.228	-0.118	174	1237538		50.00- 100.00	76.66
8.110	8.228	-0.118	175	89501		5.00- 9.00	7.23
8.110	8.228	-0.118	176	1200814		95.00- 101.00	97.03
8.110	8.228	-0.118	177	77529		5.00- 9.00	6.46

Date : 13-DEC-2007 17:17

Client ID: BFB

Instrument: msdt.i


Sample Info: 2uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

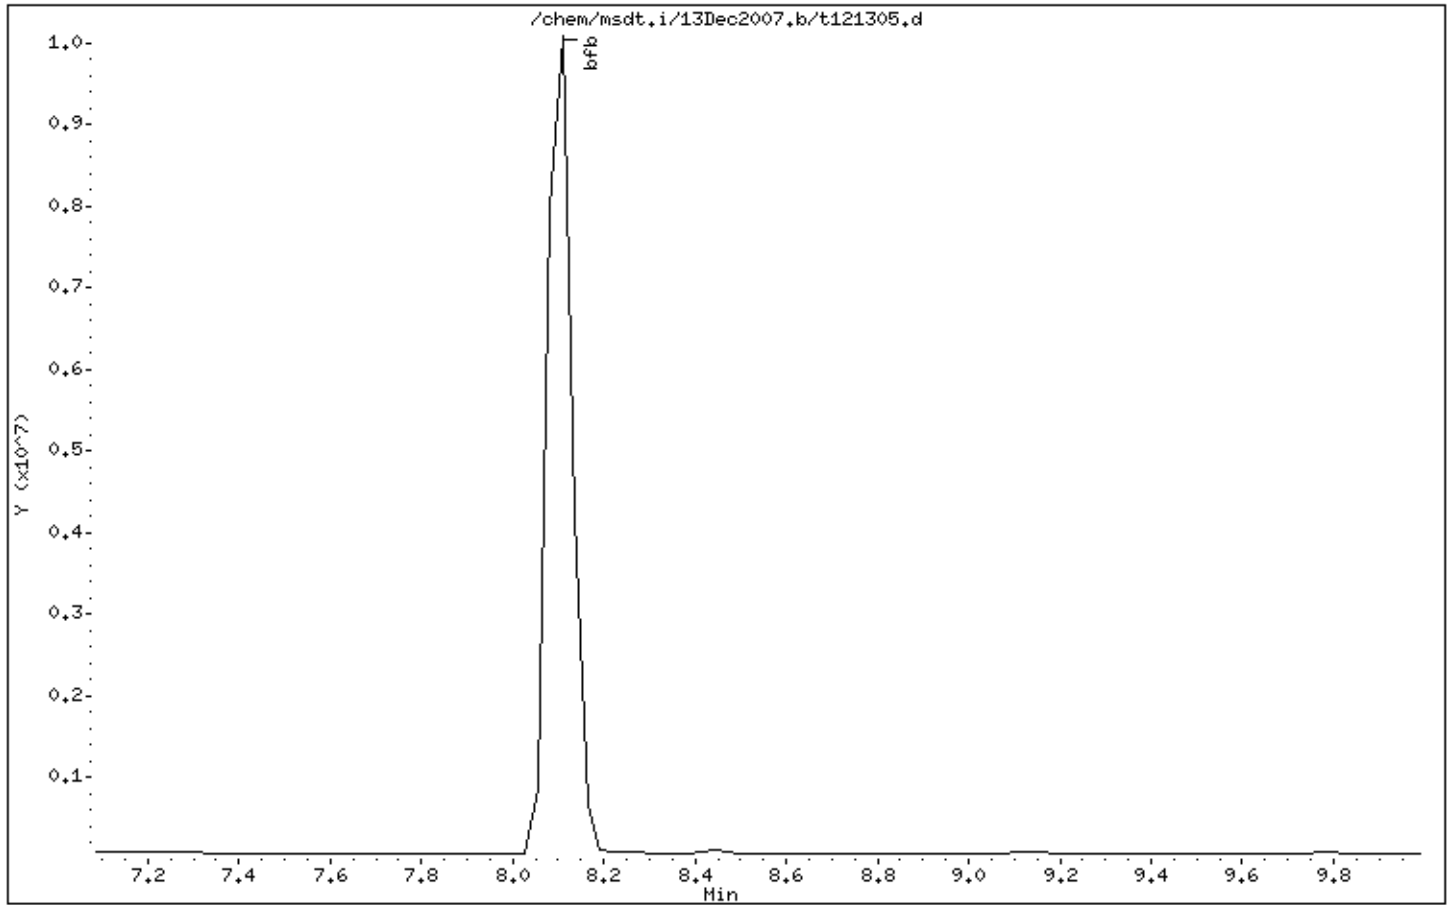

Date : 13-DEC-2007 17:17

Client ID: BFB

Instrument: msdt.i

Sample Info: 2uL #1467-64;BFB Tune check;BFB Tune check


Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

1 bfb

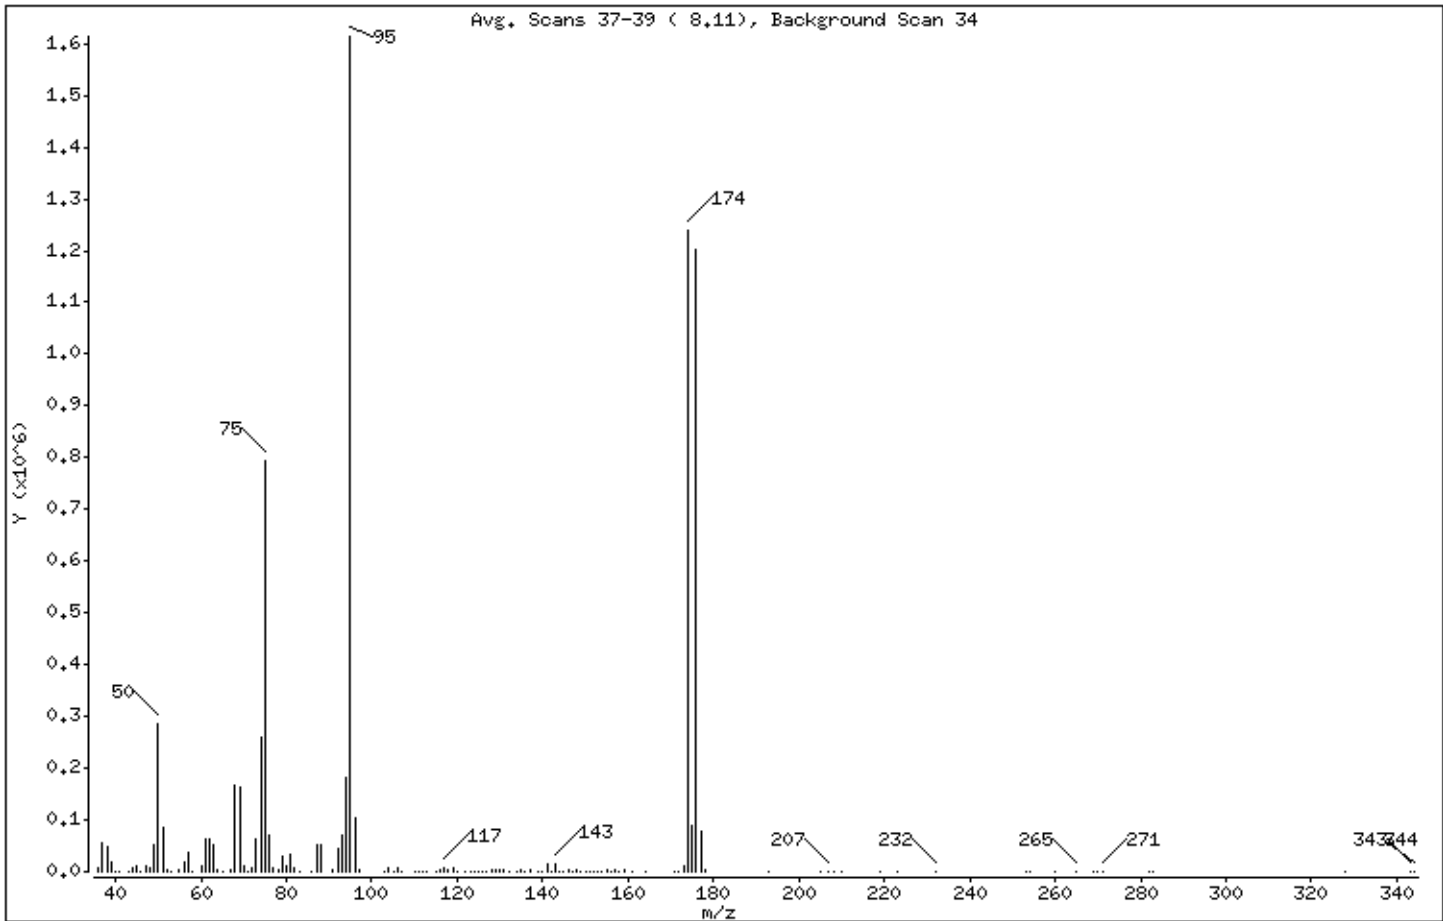

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	17.61
75	30.00 - 60.00% of mass 95	49.10
96	5.00 - 9.00% of mass 95	6.55
173	Less than 2.00% of mass 174	0.59 (0.77)
174	50.00 - 100.00% of mass 95	76.66
175	5.00 - 9.00% of mass 174	5.54 (7.23)
176	95.00 - 101.00% of mass 174	74.39 (97.03)
177	5.00 - 9.00% of mass 176	4.80 (6.46)

Date : 13-DEC-2007 17:17

Client ID: BFB

Instrument: msdt.i

Sample Info: 2uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

Data File: t121305.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 135

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	8956	74.00	259200	120.00	22	157.00	2717
37.00	54184	75.00	792576	122.00	280	158.00	274
38.00	48664	76.00	69168	123.00	479	159.00	1956
39.00	20136	77.00	7890	124.00	777	161.00	1767
40.00	816	78.00	4526	125.00	619	164.00	105
41.00	289	79.00	31240	126.00	562	171.00	334
43.00	245	80.00	10074	127.00	761	172.00	1391
44.00	5759	81.00	33360	128.00	5079	173.00	9541
45.00	11344	82.00	7267	129.00	2310	174.00	1237504
46.00	1064	83.00	673	130.00	5146	175.00	89496
47.00	12800	86.00	1234	131.00	2216	176.00	1200640
48.00	6441	87.00	53392	132.00	350	177.00	77528
49.00	53304	88.00	52592	134.00	567	178.00	2433
50.00	284352	91.00	4313	135.00	1989	193.00	272
51.00	84176	92.00	44096	136.00	490	205.00	129
52.00	3625	93.00	68696	137.00	2126	207.00	1490
53.00	229	94.00	182336	139.00	303	208.00	38
55.00	2625	95.00	1613824	140.00	886	210.00	116
56.00	19192	96.00	105672	141.00	13199	219.00	135
57.00	37840	97.00	3229	142.00	1564	223.00	133
58.00	1503	103.00	585	143.00	14142	232.00	152
60.00	11735	104.00	5709	144.00	777	253.00	301
61.00	62392	105.00	1813	145.00	1163	254.00	309
62.00	63872	106.00	5759	146.00	1917	260.00	132
63.00	51064	107.00	1486	147.00	1207	265.00	340
64.00	4579	110.00	584	148.00	3396	269.00	147
65.00	724	111.00	1003	149.00	1107	270.00	237
67.00	3638	112.00	707	150.00	1654	271.00	279
68.00	165440	113.00	930	151.00	222	282.00	156
69.00	163328	115.00	1224	152.00	645	283.00	225
70.00	11389	116.00	4543	153.00	1097	328.00	102
71.00	534	117.00	8344	154.00	799	343.00	216
72.00	7410	118.00	4789	155.00	3775	344.00	321
73.00	62552	119.00	6693	156.00	748		

Report Date: 19-Dec-2007 09:57

Air Toxics Ltd.

Data file : /chem/msdt.i/19Dec2007.b/t121901.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 19-DEC-2007 09:36
 Operator : sjr Inst ID: msdt.i
 Smp Info : 2.0uL #1467-64;BFB Tune check;BFB Tune check
 Misc Info : 50ng
 Comment :
 Method : /chem/msdt.i/19Dec2007.b/bfb.m
 Meth Date : 23-Mar-2007 09:33 tsanfel Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE (ug/L) (ug/L) TARGET RANGE RATIO

1 bfb CAS #: 460-00-4

8.110	8.228	-0.118	95	1051246	100.00-	100.00	100.00
8.110	8.228	-0.118	50	243178	15.00-	40.00	23.13
8.110	8.228	-0.118	75	604420	30.00-	60.00	57.50
8.110	8.228	-0.118	96	68386	5.00-	9.00	6.51
8.110	8.228	-0.118	173	6331	0.00-	2.00	0.90
8.110	8.228	-0.118	174	706602	50.00-	100.00	67.22
8.110	8.228	-0.118	175	52002	5.00-	9.00	7.36
8.110	8.228	-0.118	176	682346	95.00-	101.00	96.57
8.110	8.228	-0.118	177	44606	5.00-	9.00	6.54

Date : 19-DEC-2007 09:36

Client ID: BFB

Instrument: msdt.i


Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

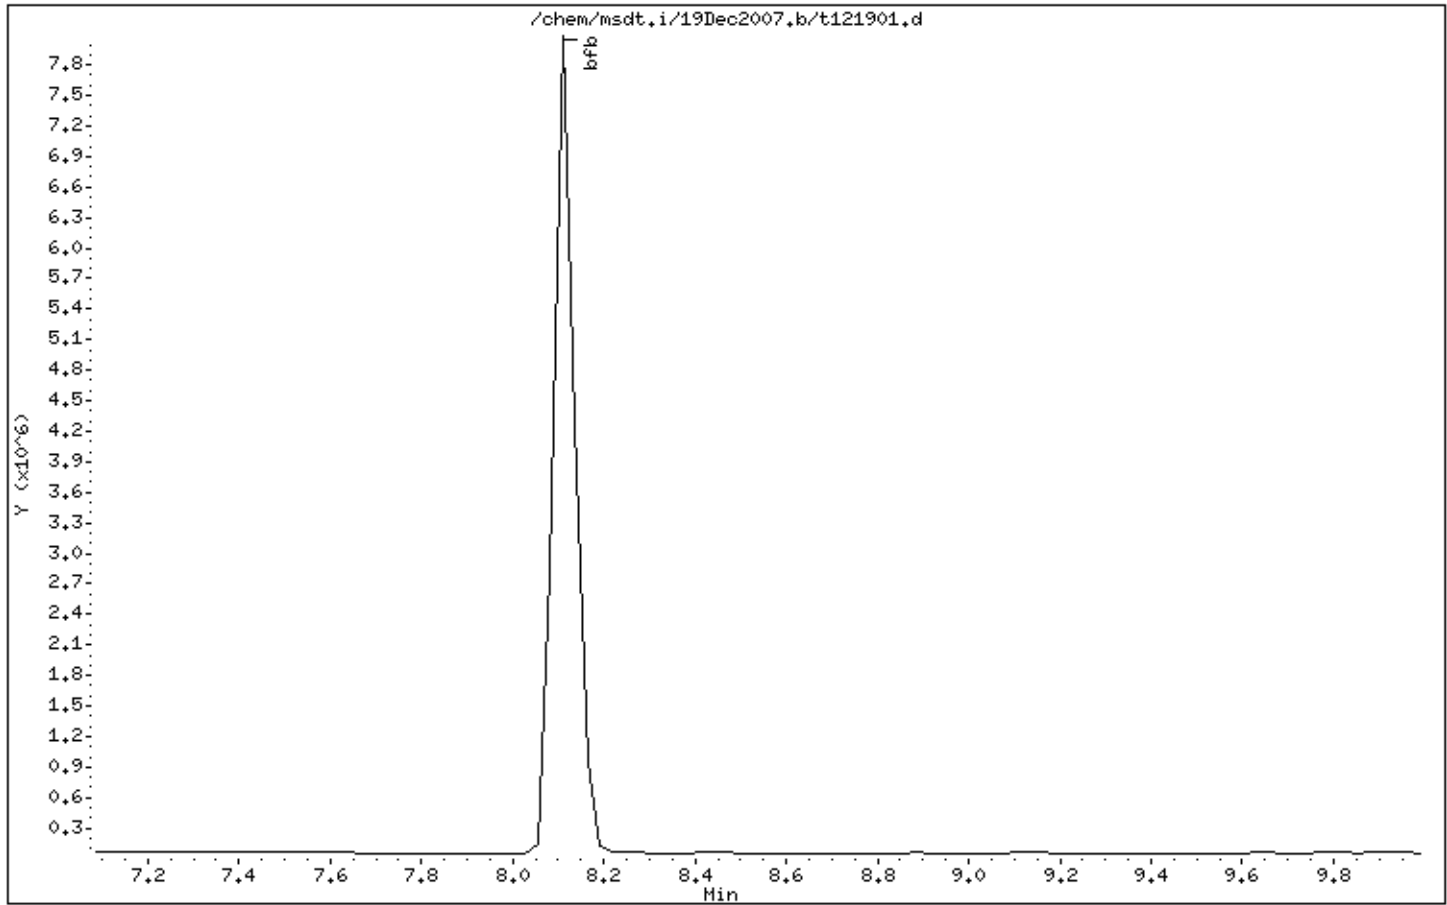

Date : 19-DEC-2007 09:36

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check


Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

1 bfb

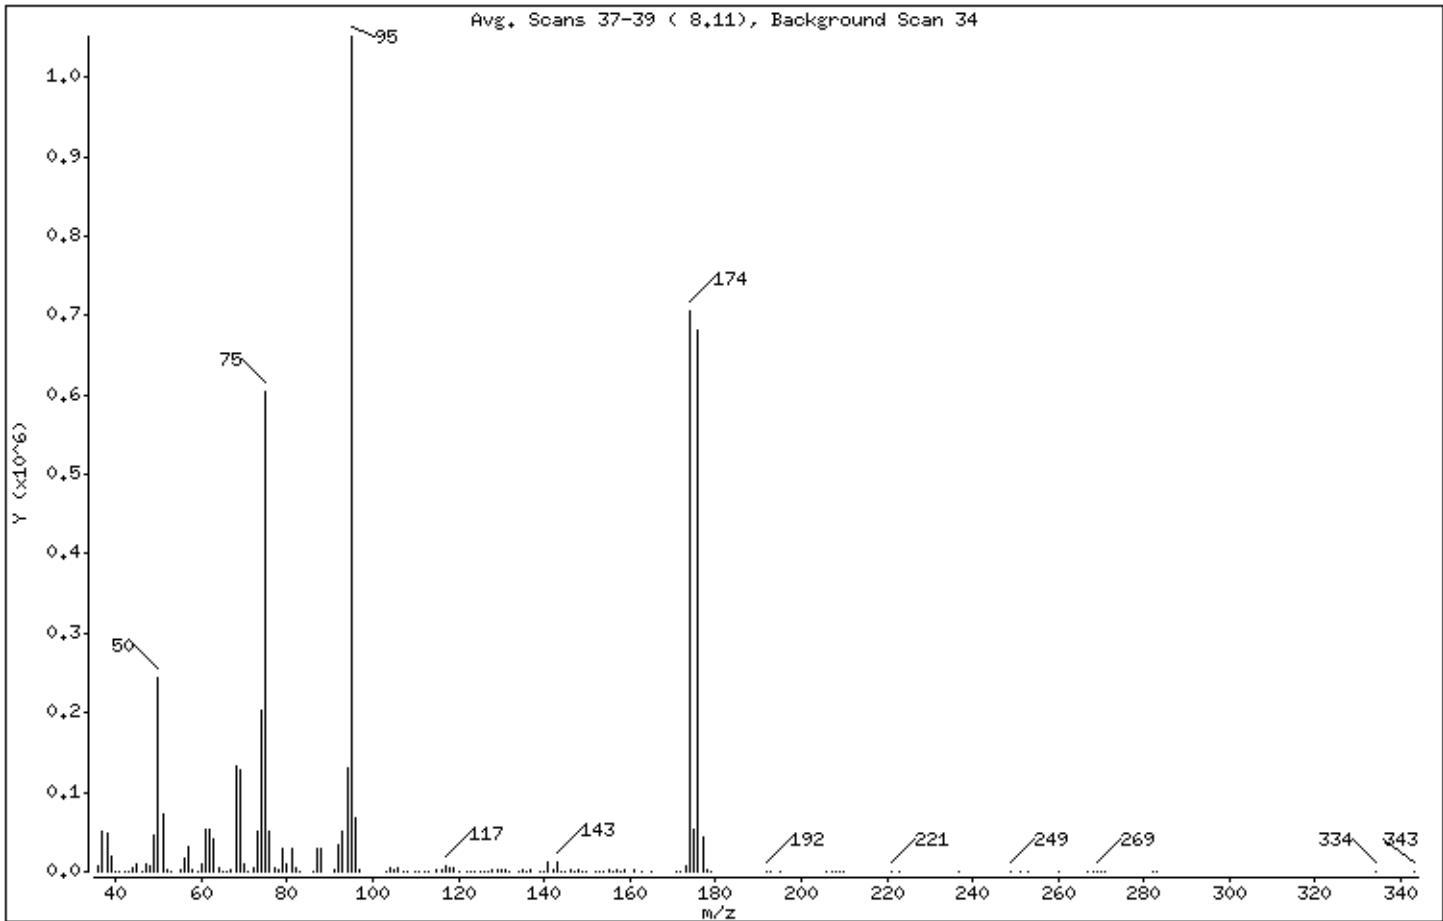

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	23.13
75	30.00 - 60.00% of mass 95	57.50
96	5.00 - 9.00% of mass 95	6.51
173	Less than 2.00% of mass 174	0.60 (0.90)
174	50.00 - 100.00% of mass 95	67.22
175	5.00 - 9.00% of mass 174	4.95 (7.36)
176	95.00 - 101.00% of mass 174	64.91 (96.57)
177	5.00 - 9.00% of mass 176	4.24 (6.54)

Date : 19-DEC-2007 09:36

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64:BFB Tune check:BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

Data File: t121901.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 144

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	8404	74.00	202944	123.00	251	171.00	148
37.00	51416	75.00	604416	124.00	560	172.00	1122
38.00	48400	76.00	51776	125.00	287	173.00	6331
39.00	18552	77.00	5349	126.00	453	174.00	706560
40.00	581	78.00	2761	127.00	587	175.00	52000
41.00	155	79.00	28920	128.00	3622	176.00	682304
42.00	225	80.00	8739	129.00	1867	177.00	44600
43.00	223	81.00	29160	130.00	3552	178.00	1519
44.00	5233	82.00	5925	131.00	1626	179.00	247
45.00	10265	83.00	511	132.00	268	192.00	411
46.00	851	86.00	711	134.00	558	193.00	239
47.00	9916	87.00	29568	135.00	1700	195.00	407
48.00	6396	88.00	28888	136.00	286	206.00	102
49.00	44920	91.00	3447	137.00	1807	207.00	141
50.00	243136	92.00	32808	139.00	400	208.00	312
51.00	71584	93.00	50512	140.00	747	209.00	264
52.00	2963	94.00	130432	141.00	12045	210.00	114
53.00	182	95.00	1051136	142.00	1435	221.00	244
55.00	2744	96.00	68384	143.00	12451	223.00	100
56.00	16310	97.00	1806	144.00	642	237.00	113
57.00	31816	103.00	550	145.00	1175	249.00	427
58.00	1351	104.00	4540	146.00	1415	251.00	219
59.00	122	105.00	1775	147.00	791	253.00	199
60.00	9406	106.00	4379	148.00	2533	260.00	19
61.00	52072	107.00	1168	149.00	907	267.00	70
62.00	53240	108.00	100	150.00	1151	268.00	103
63.00	41832	110.00	619	152.00	399	269.00	170
64.00	3785	111.00	855	153.00	697	270.00	151
65.00	1027	112.00	653	154.00	602	271.00	106
66.00	114	113.00	936	155.00	2555	282.00	109
67.00	2705	115.00	1237	156.00	569	283.00	84
68.00	132928	116.00	3577	157.00	1758	334.00	101
69.00	128280	117.00	6470	158.00	513	343.00	105
70.00	9093	118.00	3806	159.00	1348		
71.00	273	119.00	4926	161.00	1590		

Date : 19-DEC-2007 09:36

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

Data File: t121901.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 144

m/z	Y	m/z	Y	m/z	Y	m/z	Y
72.00	5797	120.00	115	163.00	607		
73.00	50888	122.00	265	165.00	386		

Report Date: 02-Jan-2008 08:39

Air Toxics Ltd.

Data file : /chem/msdt.i/02Jan2008.b/t010201.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 02-JAN-2008 08:34
 Operator : sjr Inst ID: msdt.i
 Smp Info : 2.0uL #1467-64;BFB Tune check;BFB Tune check
 Misc Info : 50ng
 Comment :
 Method : /chem/msdt.i/02Jan2008.b/bfb.m
 Meth Date : 23-Mar-2007 09:33 tsanfel Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb							
8.110	8.228	-0.118	95	1698012		100.00- 100.00	100.00
8.110	8.228	-0.118	50	340490		15.00- 40.00	20.05
8.110	8.228	-0.118	75	887898		30.00- 60.00	52.29
8.110	8.228	-0.118	96	110941		5.00- 9.00	6.53
8.110	8.228	-0.118	173	10451		0.00- 2.00	0.84
8.110	8.228	-0.118	174	1243078		50.00- 100.00	73.21
8.110	8.228	-0.118	175	90701		5.00- 9.00	7.30
8.110	8.228	-0.118	176	1192769		95.00- 101.00	95.95
8.110	8.228	-0.118	177	76632		5.00- 9.00	6.42

Date : 02-JAN-2008 08:34

Client ID: BFB

Instrument: msdt.i


Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

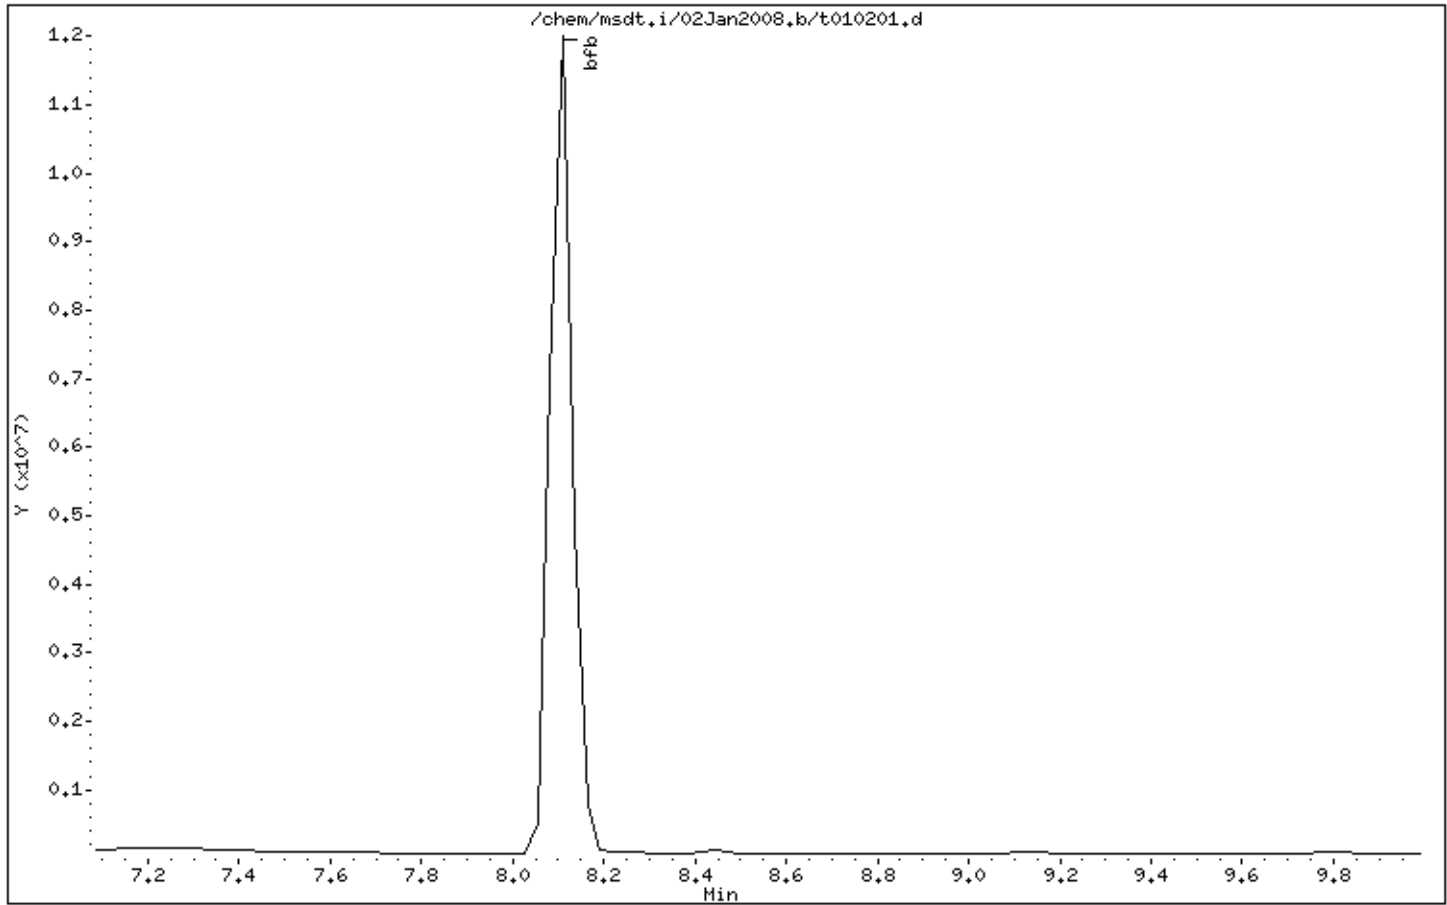

Date : 02-JAN-2008 08:34

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check


Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

1 bfb

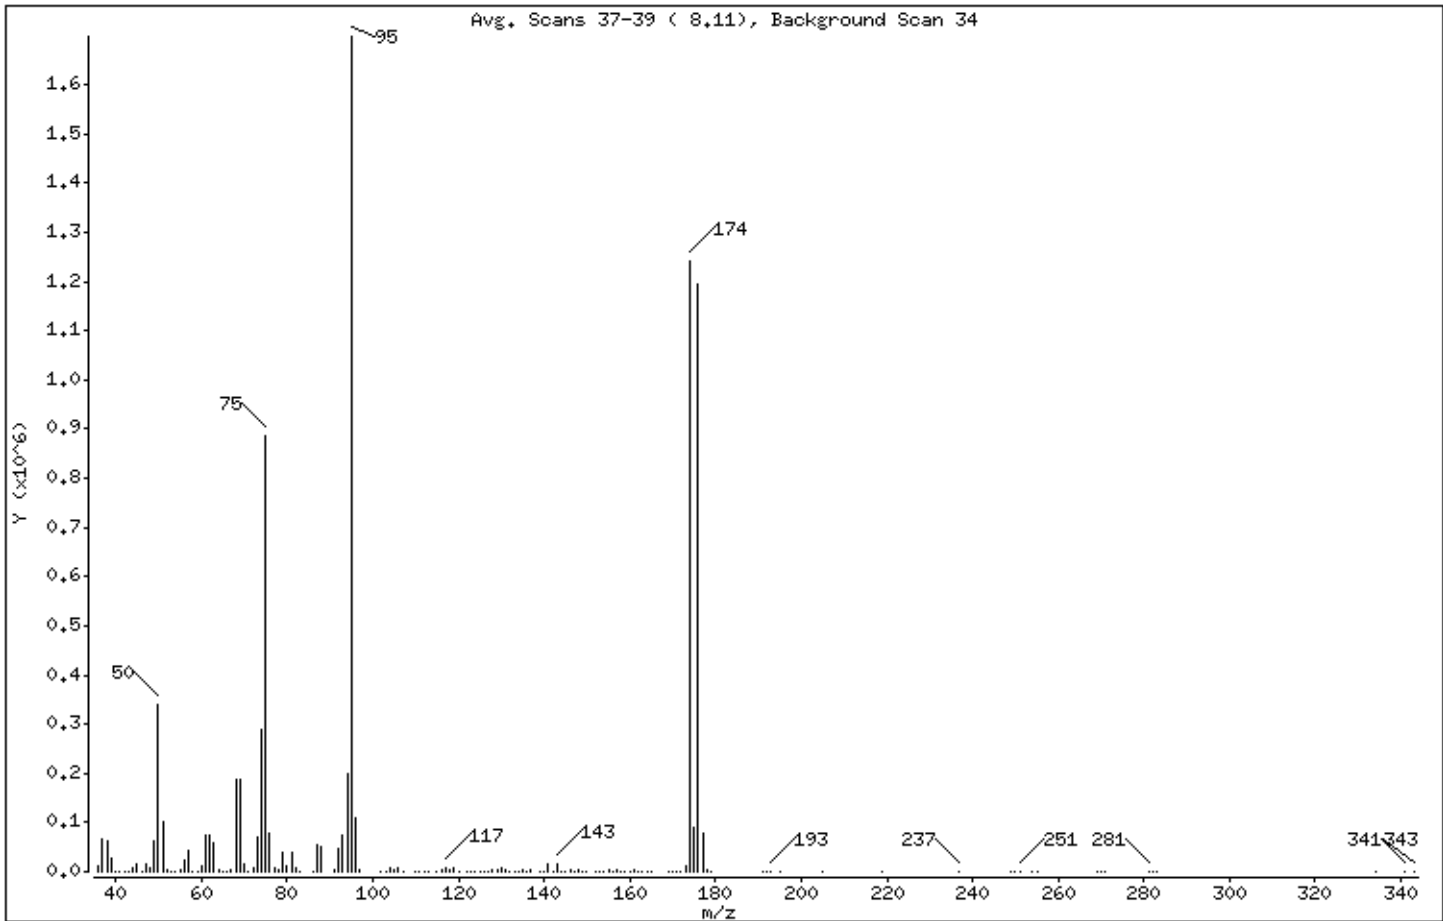

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	20.05
75	30.00 - 60.00% of mass 95	52.29
96	5.00 - 9.00% of mass 95	6.53
173	Less than 2.00% of mass 174	0.62 (0.84)
174	50.00 - 100.00% of mass 95	73.21
175	5.00 - 9.00% of mass 174	5.34 (7.30)
176	95.00 - 101.00% of mass 174	70.25 (95.95)
177	5.00 - 9.00% of mass 176	4.51 (6.42)

Date : 02-JAN-2008 08:34

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

Data File: t010201.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 148

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	11487	74.00	289280	124.00	994	164.00	108
37.00	68160	75.00	887872	125.00	663	165.00	363
38.00	62856	76.00	77688	126.00	343	169.00	110
39.00	26120	77.00	7887	127.00	221	170.00	237
40.00	520	78.00	4819	128.00	5520	171.00	508
41.00	385	79.00	38392	129.00	2512	172.00	1718
42.00	188	80.00	11848	130.00	5968	173.00	10451
43.00	878	81.00	38648	131.00	2606	174.00	1242624
44.00	7177	82.00	8401	132.00	180	175.00	90696
45.00	14287	83.00	934	133.00	802	176.00	1192448
46.00	358	86.00	1189	134.00	722	177.00	76632
47.00	15841	87.00	54736	135.00	2357	178.00	2372
48.00	7914	88.00	51512	136.00	597	179.00	169
49.00	62992	91.00	5742	137.00	2524	191.00	463
50.00	340480	92.00	48568	139.00	597	192.00	79
51.00	99712	93.00	75752	140.00	923	193.00	733
52.00	4178	94.00	198848	141.00	15623	195.00	232
53.00	541	95.00	1697792	142.00	1907	205.00	212
54.00	76	96.00	110936	143.00	16464	219.00	108
55.00	3773	97.00	3268	144.00	968	237.00	130
56.00	22080	102.00	113	145.00	1566	249.00	19
57.00	44304	103.00	561	146.00	2061	250.00	106
58.00	1584	104.00	6295	147.00	1147	251.00	253
59.00	16	105.00	2648	148.00	3938	254.00	238
60.00	13129	106.00	6097	149.00	898	255.00	122
61.00	73808	107.00	1598	150.00	1624	269.00	1
62.00	73992	110.00	805	152.00	871	270.00	126
63.00	59512	111.00	1096	153.00	1228	271.00	109
64.00	5466	112.00	801	154.00	936	281.00	693
65.00	990	113.00	1148	155.00	3995	282.00	107
66.00	104	115.00	1411	156.00	645	283.00	37
67.00	4092	116.00	5598	157.00	2735	334.00	26
68.00	186624	117.00	9636	158.00	476	341.00	103
69.00	186240	118.00	5127	159.00	1880	343.00	55
70.00	14011	119.00	7633	160.00	100		

Date : 02-JAN-2008 08:34

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

Data File: t010201.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 148

m/z	Y	m/z	Y	m/z	Y	m/z	Y
71.00	724	120.00	485	161.00	2272		
72.00	8196	122.00	402	162.00	134		
73.00	69520	123.00	347	163.00	68		

Report Date: 16-Jan-2008 08:25

Air Toxics Ltd.

Data file : /chem/msdt.i/16Jan2008.b/t011601.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 16-JAN-2008 08:29
 Operator : lo Inst ID: msdt.i
 Smp Info : 2.0uL #1467-64;BFB Tune check;BFB Tune check
 Misc Info : 50ng
 Comment :
 Method : /chem/msdt.i/16Jan2008.b/bfb.m
 Meth Date : 23-Mar-2007 09:33 tsanfel Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb							
8.137	8.228	-0.091	95	1303901		100.00- 100.00	100.00
8.137	8.228	-0.091	50	263567		15.00- 40.00	20.21
8.137	8.228	-0.091	75	694063		30.00- 60.00	53.23
8.137	8.228	-0.091	96	84241		5.00- 9.00	6.46
8.137	8.228	-0.091	173	7992		0.00- 2.00	0.84
8.137	8.228	-0.091	174	952106		50.00- 100.00	73.02
8.137	8.228	-0.091	175	70253		5.00- 9.00	7.38
8.137	8.228	-0.091	176	922222		95.00- 101.00	96.86
8.137	8.228	-0.091	177	60104		5.00- 9.00	6.52

Date : 16-JAN-2008 08:29

Client ID: BFB

Instrument: msdt,i


Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: lo

Column phase:

Column diameter: 2.00

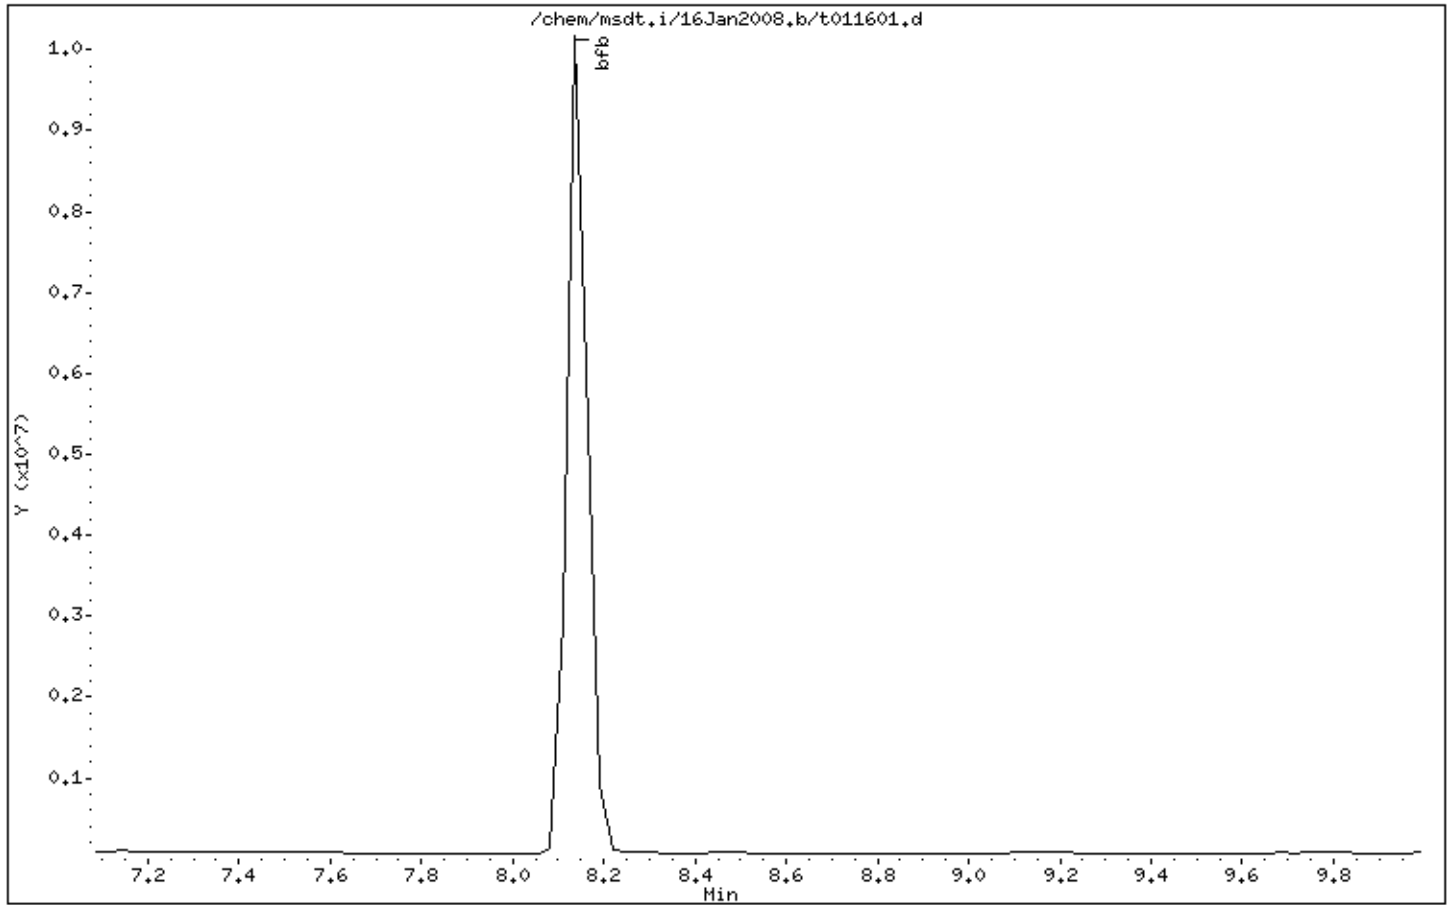

Date : 16-JAN-2008 08:29

Client ID: BFB

Instrument: msdt,i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check


Volume Injected (uL): 1.0

Operator: lo

Column phase:

Column diameter: 2.00

1 bfb

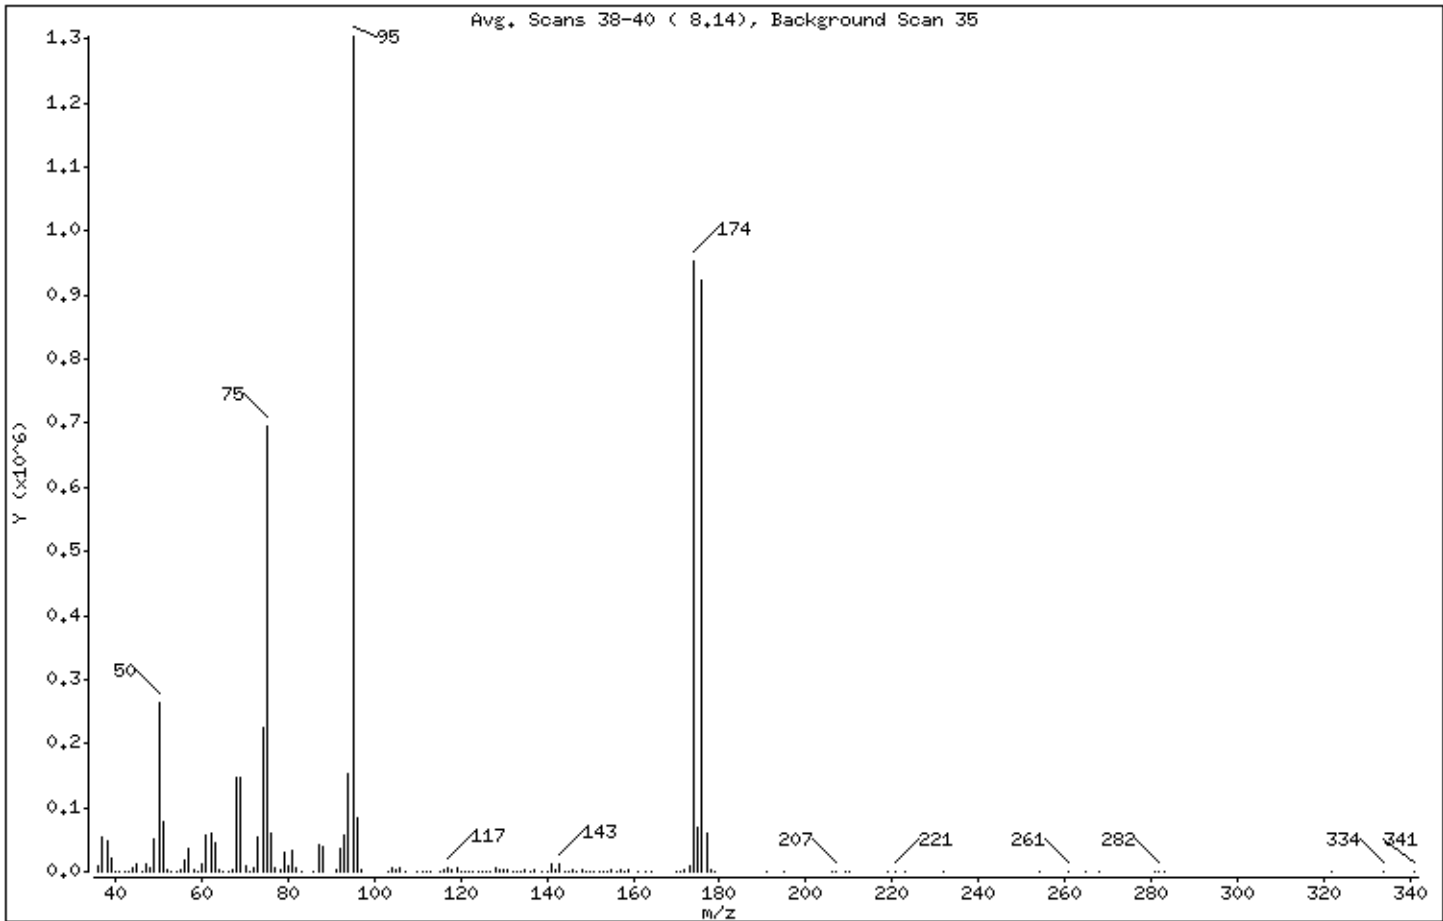

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	20.21
75	30.00 - 60.00% of mass 95	53.23
96	5.00 - 9.00% of mass 95	6.46
173	Less than 2.00% of mass 174	0.61 (0.84)
174	50.00 - 100.00% of mass 95	73.02
175	5.00 - 9.00% of mass 174	5.39 (7.38)
176	95.00 - 101.00% of mass 174	70.73 (96.86)
177	5.00 - 9.00% of mass 176	4.61 (6.52)

Date : 16-JAN-2008 08:29

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: lo

Column phase:

Column diameter: 2.00

Data File: t011601.d

Spectrum: Avg. Scans 38-40 (8.14), Background Scan 35

Location of Maximum: 95.00

Number of points: 144

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	9383	73.00	55232	122.00	273	161.00	1444
37.00	54488	74.00	224320	123.00	386	163.00	134
38.00	49408	75.00	694016	124.00	490	164.00	122
39.00	19984	76.00	59296	125.00	107	170.00	147
40.00	466	77.00	6537	126.00	376	171.00	313
41.00	210	78.00	3532	127.00	579	172.00	1510
42.00	14	79.00	29192	128.00	4530	173.00	7992
43.00	467	80.00	9193	129.00	2408	174.00	952064
44.00	5705	81.00	31568	130.00	4277	175.00	70248
45.00	10785	82.00	6777	131.00	1704	176.00	922176
46.00	454	83.00	900	132.00	158	177.00	60104
47.00	12079	86.00	1114	133.00	63	178.00	1546
48.00	6071	87.00	41832	134.00	24	179.00	13
49.00	50256	88.00	39928	135.00	1570	191.00	620
50.00	263552	91.00	4347	136.00	558	195.00	489
51.00	78816	92.00	36936	137.00	1996	206.00	145
52.00	3487	93.00	57640	139.00	308	207.00	699
53.00	428	94.00	151552	140.00	764	209.00	338
54.00	101	95.00	1303552	141.00	11643	210.00	101
55.00	3050	96.00	84240	142.00	1665	219.00	117
56.00	18296	97.00	2771	143.00	12844	221.00	290
57.00	34992	103.00	626	144.00	615	223.00	149
58.00	1511	104.00	4987	145.00	1212	232.00	258
59.00	70	105.00	1799	146.00	1754	254.00	44
60.00	10883	106.00	5117	147.00	822	261.00	135
61.00	56616	107.00	1404	148.00	3165	265.00	280
62.00	58864	110.00	379	149.00	629	268.00	114
63.00	44976	111.00	957	150.00	1327	281.00	240
64.00	4091	112.00	754	151.00	137	282.00	302
65.00	1174	113.00	907	152.00	466	283.00	125
66.00	116	115.00	1123	153.00	771	322.00	112
67.00	3039	116.00	4221	154.00	954	334.00	417
68.00	146880	117.00	6589	155.00	2834	341.00	213
69.00	146944	118.00	4243	156.00	497		
70.00	9993	119.00	6031	157.00	2080		

Date : 16-JAN-2008 08:29

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1467-64;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: lo

Column phase:

Column diameter: 2.00

Data File: t011601.d

Spectrum: Avg. Scans 38-40 (8.14), Background Scan 35

Location of Maximum: 95.00

Number of points: 144

m/z	Y	m/z	Y	m/z	Y	m/z	Y
71.00	514	120.00	376	158.00	298		
72.00	5864	121.00	146	159.00	1654		

Report Date: 25-Jan-2008 08:25

Air Toxics Ltd.

Data file : /chem/msdt.i/25Jan2008.b/t012501.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 25-JAN-2008 08:13
 Operator : sjr Inst ID: msdt.i
 Smp Info : 2.0uL #1476-65;BFB Tune check;BFB Tune check
 Misc Info : 50ng
 Comment :
 Method : /chem/msdt.i/25Jan2008.b/bfb.m
 Meth Date : 23-Mar-2007 09:33 tsanfel Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb							
8.137	8.228	-0.091	95	1469184		100.00- 100.00	100.00
8.137	8.228	-0.091	50	288352		15.00- 40.00	19.63
8.137	8.228	-0.091	75	766093		30.00- 60.00	52.14
8.137	8.228	-0.091	96	94079		5.00- 9.00	6.40
8.137	8.228	-0.091	173	9258		0.00- 2.00	0.82
8.137	8.228	-0.091	174	1124352		50.00- 100.00	76.53
8.137	8.228	-0.091	175	81005		5.00- 9.00	7.20
8.137	8.228	-0.091	176	1081888		95.00- 101.00	96.22
8.137	8.228	-0.091	177	72160		5.00- 9.00	6.67

Date : 25-JAN-2008 08:13

Client ID: BFB

Instrument: msdt.i


Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

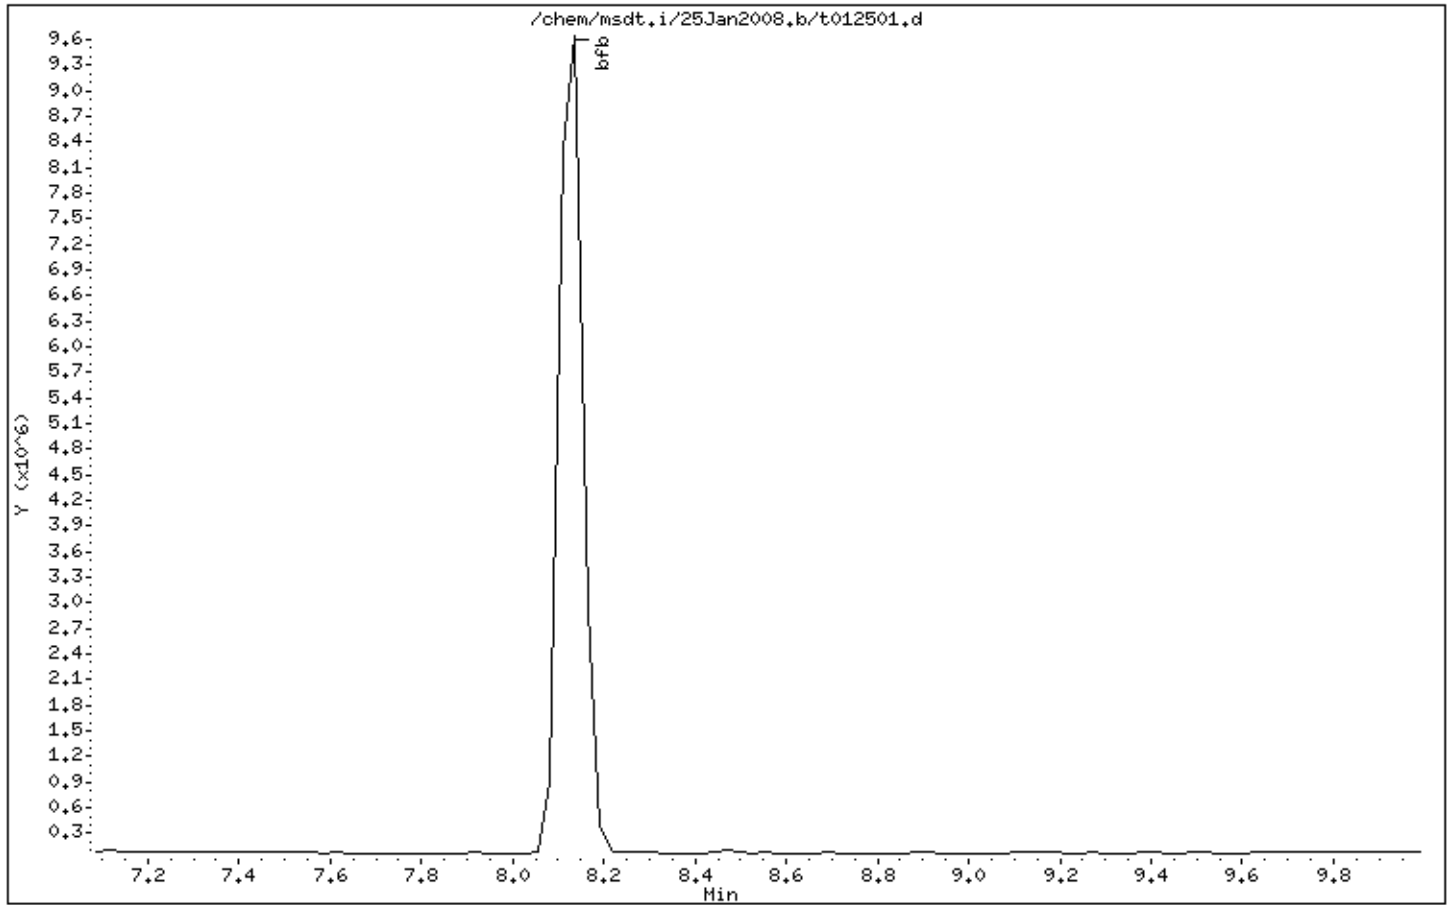

Date : 25-JAN-2008 08:13

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check


Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

1 bfb

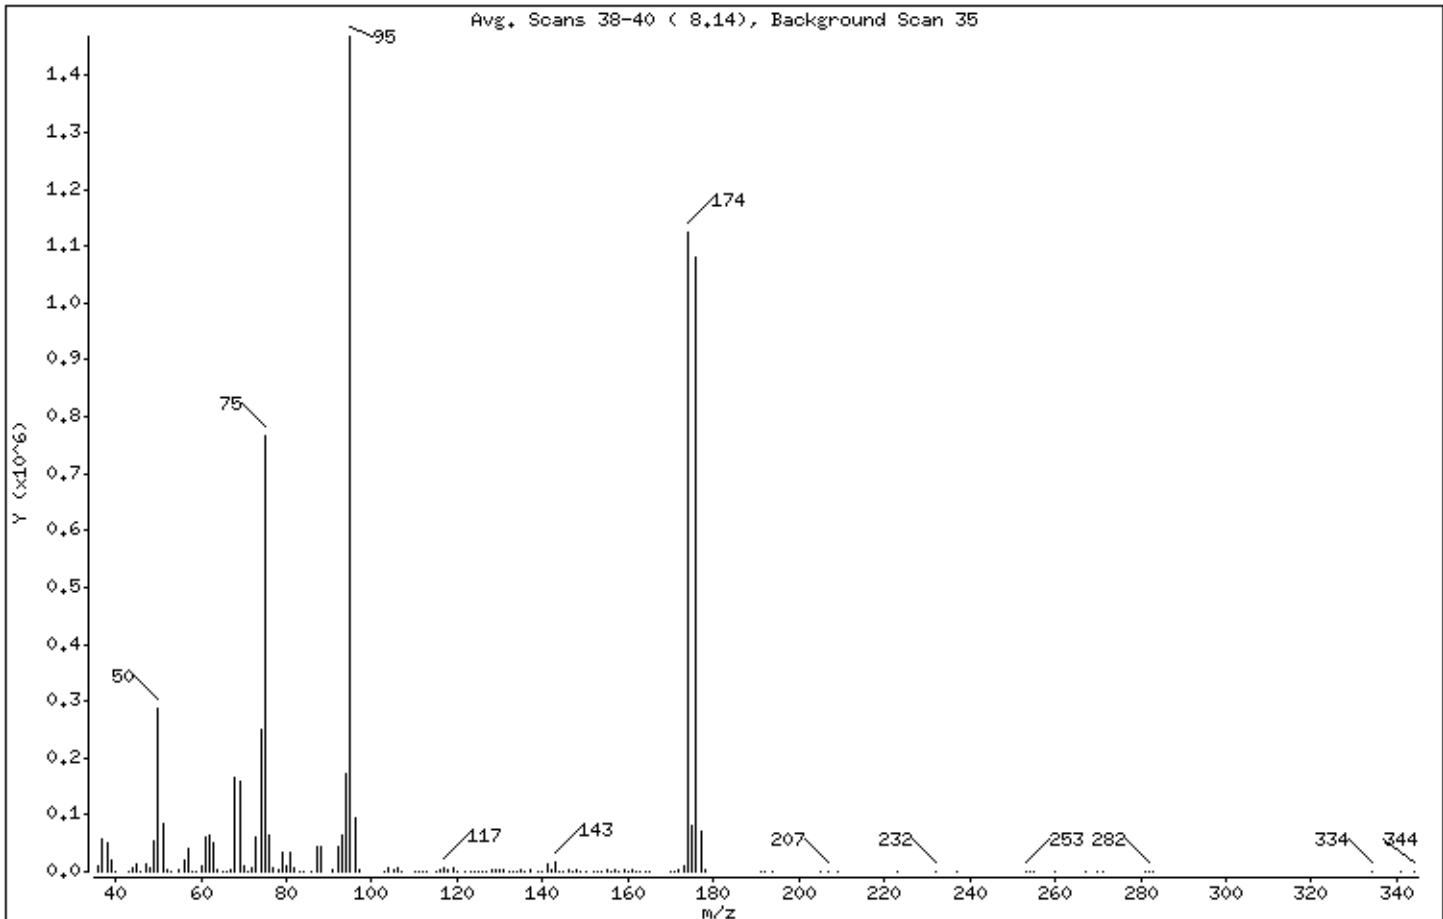

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	19.63
75	30.00 - 60.00% of mass 95	52.14
96	5.00 - 9.00% of mass 95	6.40
173	Less than 2.00% of mass 174	0.63 (0.82)
174	50.00 - 100.00% of mass 95	76.53
175	5.00 - 9.00% of mass 174	5.51 (7.20)
176	95.00 - 101.00% of mass 174	73.64 (96.22)
177	5.00 - 9.00% of mass 176	4.91 (6.67)

Date : 25-JAN-2008 08:13

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1476-65:BFB Tune check:BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

Data File: t012501.d

Spectrum: Avg. Scans 38-40 (8,14), Background Scan 35

Location of Maximum: 95.00

Number of points: 144

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	10049	76.00	64584	125.00	531	164.00	125
37.00	58088	77.00	6626	126.00	709	165.00	4
38.00	52328	78.00	4364	127.00	833	170.00	272
39.00	21704	79.00	33592	128.00	4368	171.00	142
40.00	243	80.00	10541	129.00	2649	172.00	1982
43.00	391	81.00	35240	130.00	5007	173.00	9258
44.00	6051	82.00	7723	131.00	1950	174.00	1124352
45.00	12270	83.00	683	132.00	404	175.00	81000
46.00	698	84.00	100	133.00	476	176.00	1081856
47.00	12175	86.00	904	134.00	515	177.00	72160
48.00	7091	87.00	44136	135.00	2048	178.00	2206
49.00	53768	88.00	44056	136.00	127	191.00	660
50.00	288320	91.00	4400	137.00	2503	192.00	449
51.00	83656	92.00	42480	139.00	318	194.00	106
52.00	3648	93.00	65000	140.00	1000	205.00	170
53.00	251	94.00	173888	141.00	14570	207.00	1408
55.00	3087	95.00	1468928	142.00	1711	209.00	73
56.00	19632	96.00	94072	143.00	15466	223.00	104
57.00	38848	97.00	2693	144.00	860	232.00	194
58.00	1444	103.00	569	145.00	1169	237.00	102
59.00	296	104.00	5697	146.00	2025	253.00	297
60.00	11614	105.00	2205	147.00	1087	254.00	255
61.00	62264	106.00	5245	148.00	3765	255.00	103
62.00	65376	107.00	1430	149.00	907	260.00	61
63.00	51680	110.00	706	150.00	1663	267.00	39
64.00	4686	111.00	911	152.00	744	270.00	97
65.00	971	112.00	866	153.00	979	271.00	242
66.00	105	113.00	988	154.00	825	281.00	423
67.00	3014	115.00	1287	155.00	3366	282.00	655
68.00	163904	116.00	4730	156.00	780	283.00	406
69.00	159168	117.00	7854	157.00	2525	334.00	476
70.00	11529	118.00	4775	158.00	443	341.00	125
71.00	432	119.00	6744	159.00	1914	344.00	129
72.00	7166	120.00	295	160.00	136		
73.00	61008	122.00	291	161.00	2128		

Date : 25-JAN-2008 08:13

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: sjr

Column phase:

Column diameter: 2.00

Data File: t012501.d

Spectrum: Avg. Scans 38-40 (8.14), Background Scan 35

Location of Maximum: 95.00

Number of points: 144

m/z	Y	m/z	Y	m/z	Y	m/z	Y
74.00	251264	123.00	453	162.00	103		
75.00	766080	124.00	802	163.00	214		

Report Date: 03-Feb-2008 14:39

Air Toxics Ltd.

Data file : /chem/msdt.i/03Feb2008.b/t020301.d
 Lab Smp Id: Client Smp ID: BFB
 Inj Date : 03-FEB-2008 14:33
 Operator : xp Inst ID: msdt.i
 Smp Info : 2.0uL #1476-65;BFB Tune check;BFB Tune check
 Misc Info : 50ng
 Comment :
 Method : /chem/msdt.i/03Feb2008.b/bfb.m
 Meth Date : 23-Mar-2007 09:33 tsanfel Quant Type: ESTD
 Cal Date : Cal File:
 Als bottle: 1 QC Sample: BFB
 Dil Factor: 1.00000
 Integrator: HP RTE Compound Sublist: all.sub
 Target Version: 3.50 Sample Matrix: WATER
 Processing Host: eeyore

Concentration Formula: Amt * DF * Uf * Vf * Vi * CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	DLT RT	MASS	RESPONSE (ug/L)	(ug/L)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

CAS #: 460-00-4

1 bfb							
8.110	8.228	-0.118	95	2073393		100.00- 100.00	100.00
8.110	8.228	-0.118	50	388061		15.00- 40.00	18.72
8.110	8.228	-0.118	75	1053148		30.00- 60.00	50.79
8.110	8.228	-0.118	96	132705		5.00- 9.00	6.40
8.110	8.228	-0.118	173	12438		0.00- 2.00	0.78
8.110	8.228	-0.118	174	1586896		50.00- 100.00	76.54
8.110	8.228	-0.118	175	117168		5.00- 9.00	7.38
8.110	8.228	-0.118	176	1537330		95.00- 101.00	96.88
8.110	8.228	-0.118	177	101198		5.00- 9.00	6.58

Date : 03-FEB-2008 14:33

Client ID: BFB

Instrument: msdt.i


Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: xp

Column phase:

Column diameter: 2.00

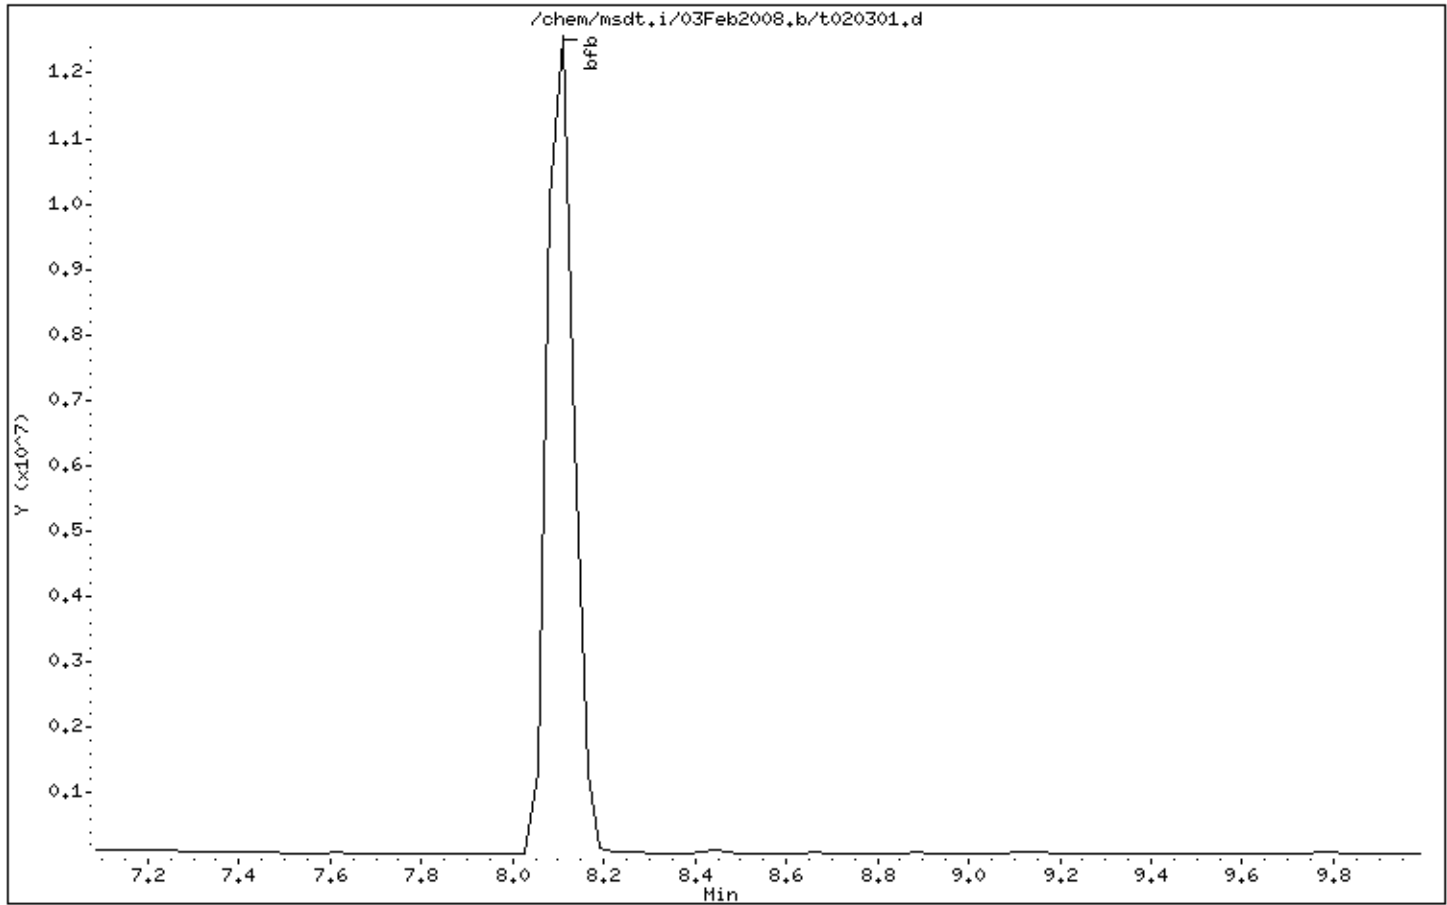

Date : 03-FEB-2008 14:33

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check


Volume Injected (uL): 1.0

Operator: xp

Column phase:

Column diameter: 2.00

1 bfb

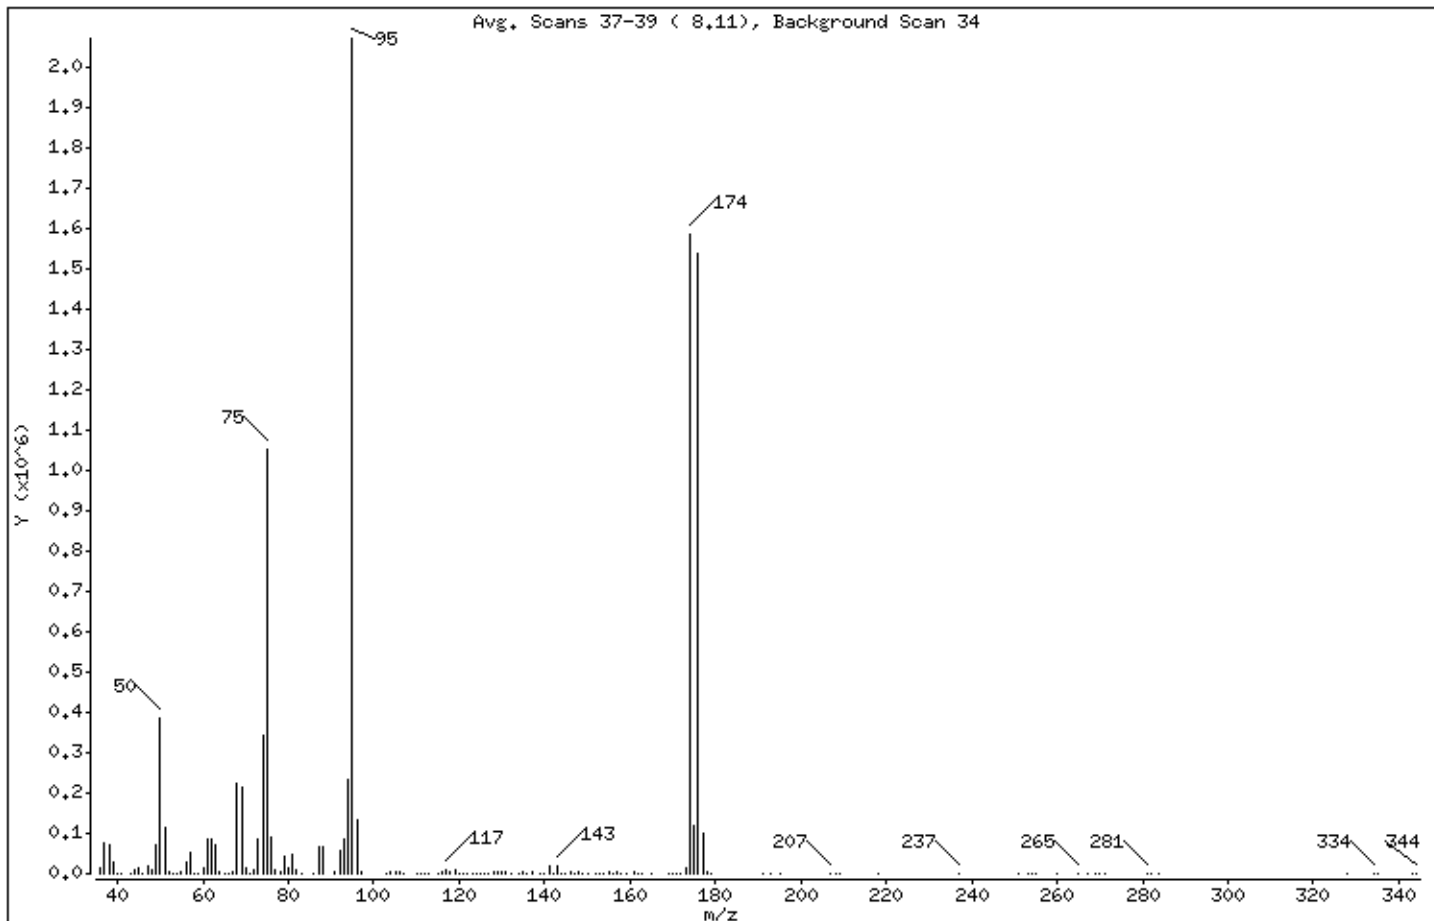

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	18.72
75	30.00 - 60.00% of mass 95	50.79
96	5.00 - 9.00% of mass 95	6.40
173	Less than 2.00% of mass 174	0.60 (0.78)
174	50.00 - 100.00% of mass 95	76.54
175	5.00 - 9.00% of mass 174	5.65 (7.38)
176	95.00 - 101.00% of mass 174	74.15 (96.88)
177	5.00 - 9.00% of mass 176	4.88 (6.58)

Date : 03-FEB-2008 14:33

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: xp

Column phase:

Column diameter: 2.00

Data File: t020301.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 149

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	12949	75.00	1052672	125.00	649	171.00	484
37.00	76472	76.00	89592	126.00	675	172.00	2221
38.00	70392	77.00	9467	127.00	888	173.00	12438
39.00	29680	78.00	6010	128.00	6168	174.00	1586688
40.00	852	79.00	43552	129.00	3218	175.00	117168
41.00	211	80.00	13927	130.00	6467	176.00	1537024
43.00	593	81.00	45808	131.00	2592	177.00	101192
44.00	8532	82.00	10514	132.00	372	178.00	2977
45.00	15701	83.00	1131	134.00	672	179.00	181
46.00	1172	86.00	1564	135.00	2931	191.00	307
47.00	17112	87.00	68904	136.00	676	193.00	101
48.00	9706	88.00	67232	137.00	2779	195.00	114
49.00	73448	91.00	5660	139.00	595	207.00	1525
50.00	388032	92.00	56648	140.00	1015	208.00	30
51.00	115280	93.00	87456	141.00	17016	209.00	4
52.00	4820	94.00	235776	142.00	2058	218.00	101
53.00	490	95.00	2073088	143.00	17080	237.00	102
54.00	112	96.00	132672	144.00	1054	251.00	243
55.00	4021	97.00	3689	145.00	1636	253.00	206
56.00	26864	103.00	663	146.00	2759	254.00	119
57.00	52240	104.00	6733	147.00	1164	255.00	103
58.00	2024	105.00	2640	148.00	4637	260.00	90
59.00	254	106.00	7113	149.00	958	265.00	277
60.00	16026	107.00	1905	150.00	1890	267.00	57
61.00	87128	110.00	790	152.00	1005	269.00	467
62.00	87432	111.00	1195	153.00	1395	270.00	17
63.00	69440	112.00	939	154.00	1142	271.00	100
64.00	5783	113.00	1154	155.00	4007	281.00	687
65.00	825	115.00	2128	156.00	1004	282.00	102
66.00	137	116.00	6234	157.00	3115	284.00	329
67.00	4539	117.00	10733	158.00	550	328.00	101
68.00	222848	118.00	5770	159.00	2118	334.00	414
69.00	215936	119.00	9167	161.00	2454	335.00	102
70.00	16008	120.00	300	162.00	275	343.00	184
71.00	548	121.00	119	163.00	155	344.00	152

Date : 03-FEB-2008 14:33

Client ID: BFB

Instrument: msdt.i

Sample Info: 2.0uL #1476-65;BFB Tune check;BFB Tune check

Volume Injected (uL): 1.0

Operator: xp

Column phase:

Column diameter: 2.00

Data File: t020301.d

Spectrum: Avg. Scans 37-39 (8.11), Background Scan 34

Location of Maximum: 95.00

Number of points: 149

m/z	Y	m/z	Y	m/z	Y	m/z	Y
72.00	9345	122.00	453	165.00	457		
73.00	84800	123.00	560	169.00	110		
74.00	343936	124.00	951	170.00	459		

Shipping/ Receiving Documents



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: _____ GEI Consultants, Inc. _____
ATTENTION: _____ Ms. Sarah Aldridge _____
FAX #: _____ 860-368-5307 _____
FROM: _____ Sample Receiving _____
Workorder #: _____ 0801560 _____
of pages (Including Cover): _____ 1 _____

2/19/2008

Thank you for selecting Air Toxics Ltd. We have received your samples and have found no discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Bryanna Langley at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

AIR TOXICS LTD.

AN ENVIRONMENTAL ANALYTICAL LABORATORY

CHAIN-OF-CUSTODY RECORD

Sample Transportation Notice

Relinquishing signature on this document indicates that sample is being shipped in compliance with all applicable local, State, Federal, national, and international laws, regulations and ordinances of any kind. Air Toxics Limited assumes no liability with respect to the collection, handling, or shipping of these samples. Relinquishing signature also indicates agreement to hold harmless, defend, and indemnify Air Toxics Limited against any claim, demand, or action of any kind, related to the collection, handling, or shipping of samples. D.O.T. Hotline (800) 457-4822

190 BLUE RAVINE ROAD, SUITE B
 FOLSOM, CA 95630-4719
 (916) 985-1000 FAX: (916) 985-1020

Contact Company: GEL Consultants, Inc. Address: 455 Winding Brook Glastonbury, CT 06033 Phone: 860-388-5300 Cell:		Project Info: P.O. #: _____ Project #: 06140-8-1708 Project Name: Bayshore 0J1 Southern cell Air Monitoring		Turn Around Time: <input checked="" type="checkbox"/> Normal <input type="checkbox"/> Rush _____ Specify: _____	
Collected By: Signature: <i>[Signature]</i>					

Lab ID	Field Sample ID	CR#	Date & Time	Analyses Requested	Canister Pressure/Vacuum Initial	Final	Receipt
O1A	WILLIAMS 3	23988	01/20/08 0600/1400	TO-15 + Naphthalene	29.5	-8.0	
O2A	WILLIAMS 5	34343	0600/1400	TO-15 + Naphthalene	29.5	-6.7	

Relinquished By: (Signature) <i>[Signature]</i> Date/Time: 01/20/08 1430 Received By: (Signature) <i>[Signature]</i> Date/Time: 01/20/08 1330	Relinquished By: (Signature) <i>[Signature]</i> Date/Time: _____ Received By: (Signature) <i>[Signature]</i> Date/Time: _____
Relinquished By: (Signature) <i>[Signature]</i> Date/Time: _____ Received By: (Signature) <i>[Signature]</i> Date/Time: _____	Relinquished By: (Signature) <i>[Signature]</i> Date/Time: _____ Received By: (Signature) <i>[Signature]</i> Date/Time: _____

Notes: use flow controllers included
 Initial and final can pressures in inches Hg!
 Send Data Pack to Lisa McDonough and EDD to datagroup@gelconsultants.com

Lab Use Only Shipper Name: FedEx Air Bill #: 5629 1704 5334 Opened By: MG Temp (C): MF Condition: Good Custody Seal Intact: <input checked="" type="checkbox"/> None Work Order #: 080150
--



AN ENVIRONMENTAL ANALYTICAL LABORATORY

SAMPLE RECEIPT SUMMARY

WORKORDER 0801560

Client	Phone	Date Promised: 02/14/08
Ms. Sarah Aldridge	860-368-5300	Date Completed: 2/13/08
GEI Consultants, Inc.		Date Received: 1/31/08
455 Winding Brook Drive	Fax	PO#: NR
Suite 201	860-368-5307	Project#: 061140-8-1703 BayShore OU1 Southern cell
Glastonbury, CT 06033		Air Monitorin
Sales Rep: ANS		Total \$: \$ 624.00
		Logged By: MG

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A	DW AMS 3	Modified TO-15	1/30/2008	8.0 "Hg	\$225.00
02A	UW AMS 5	Modified TO-15	1/30/2008	6.5 "Hg	\$225.00
03A	Lab Blank	Modified TO-15	NA	NA	\$0.00
04A	CCV	Modified TO-15	NA	NA	\$0.00
05A	LCS	Modified TO-15	NA	NA	\$0.00
Misc. Charges 6 Liter Summa Canister (2) @ \$50.00 each., Shipment 54020					\$100.00
Blue Body Flow Controller (2) @ \$35.00 each., Shipment 54020					\$70.00
Fuel Surcharge (2) @ \$2.00 each.					\$4.00

Note: Samples received after 3 P.M. PST are considered to be received on the following work day.
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

BILL TO: Ms. Sarah Aldridge
GEI Consultants, Inc.
455 Winding Brook Drive
Suite 201
Glastonbury, CT 06033

Analysis Code: TO-14A

TERMS:

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

Other Records

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	

Compound Listing

Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	

DATA REVIEW CHECKLIST

Work Order #:

0801560

A	R	T	M	Q
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
NA	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
NA	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>

- Analysis/Reporting vs. Project Profile/SOP requirements checked (i.e. 100% Dups, J-Flag to MDL, etc)
- The final report has the correct reporting list, special units, and header info.
- Lab Narrative is correct (proper method & description/Receiving & Analytical notes correct)
- Corrective Action issued - # _____
- Unusual circumstances have been documented in the notes section below

LUMEN validation report present and initialed

CIRCLE (YES / NO)

<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Lab Blank, CCV, LCS and DUP met QC criteria
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Hold time is met for all samples
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Appropriate data qualifier flags are applied
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Manual integrations for samples and QC are properly documented
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Samples analyzed within the project or method specific clock
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Retention times have been verified
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	Appropriate ICAL(s) included
<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	At least one result per sample is verified against the target quant sheets/raw data

- Dilution factor correctly calculated (sample load volume, syringe and bag dilutions, can pressurization(s))
- Correct amount of sample analyzed (i.e. sample not over-diluted)
- Spectra verified - documentation of spectral defense included (Section 5A of eCVP pkg)
- TICs resemble reference spectra
- TICs between duplicate samples are consistent
- NA Checked samples for trends (i.e. Influent>Effluent, Landfill or Ambient etc)
- Special units for all samples in the final report are correctly calculated
- Manually entered results checked (i.e. special CCV compounds)
- TPH/NMOC (verify calculations and correct reference compound used)
- Chain of Custody scanned correctly
- Verify sample id's vs. chain of custody
- Samples pressurized w/ appropriate gas (N₂ or He) Tedlar Bag only
- Final pressure consistent with canister size (6L vs. 1L)
- Verify receipt pressures against logbook and Target
- Verify canister ID #'s
- Extra printed copies are provided per client profile
- Final invoice amount correct (adjusted for TAT, Penalties, Re-issue Charges etc.)
- Client LUMEN report reviewed for accuracy and completeness

Notes: (to include: noting samples with QA/QC problems, Blanks with positive hits, narratives, etc.)

A/R: 1 out CCV, 0 out LCS

M/O:

A
(Analytical Review/Date)

CB 2/4/08

R/T

(Reporting Review/Date)

R: [Signature] 2/12/08

M

(Management Review/Date)

[Signature] 2/13/08

Q

(QA Review/Date)

T: _____

Not Applicable