



**Air  
Toxics LTD.**  
*Laboratory Services Since 1989*

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**COMPREHENSIVE VALIDATION PACKAGE**

Modified TO-15

**INVENTORY SHEET**

Work Order #: 0804565

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	23
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	24	31
b. Surrogate Recover Summary Form (If Applicable)	32	32
c. Internal Standard Summary Form (If Applicable)	33	33
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	34	132
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	133	147
i. Second Source LCS(Summary + Raw Data)	148	162
j. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	163	164
l. GC/MS Tune (Results + Raw Data)	165	174
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	175	176
b. Chain-of-Custody Records	177	177
c. Sample Log-In Sheet	178	178
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	--	--
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	179	181
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	182	183
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	--	--
i. <u>Data Review Check Sheet</u>	184	184

Comments:

Completed by:

**Kara McKiernan**

(Signature)

Kara McKiernan / Document Control

( Print Name & Title)

5/12/08

(Date)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**WORK ORDER #: 0804565**

Work Order Summary

**CLIENT:** Ms. Theresa Landgraff  
GEI Consultants, Inc.  
110 Walt Whitman Road  
Suite 204  
Huntington Station, NY 11746

**BILL TO:** Ms. Theresa Landgraff  
GEI Consultants, Inc.  
110 Walt Whitman Road  
Suite 204  
Huntington Station, NY 11746

**PHONE:** 631-760-9300 x 12

**P.O. #** NR

**FAX:**

**PROJECT #** 061140-8-1703 BayShore OU1 Southern

**DATE RECEIVED:** 04/24/2008

**CONTACT:** cell Air Monitorin  
Bryanna Langley

**DATE COMPLETED:** 05/06/2008

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>	<u>FINAL PRESSURE</u>
01A	AMS UW	Modified TO-15	3.0 "Hg	5 psi
02A	AMS DW	Modified TO-15	6.5 "Hg	5 psi
03A	Lab Blank	Modified TO-15	NA	NA
04A	CCV	Modified TO-15	NA	NA
05A	LCS	Modified TO-15	NA	NA

CERTIFIED BY: 

DATE: 05/07/08

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004  
NY NELAP - 11291, UT NELAP - 9166389892, AZ Licensure AZ0719

Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,  
Accreditation number: E87680, Effective date: 07/01/07, Expiration date: 06/30/08

Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards

This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630  
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

**LABORATORY NARRATIVE**  
**Modified TO-15**  
**GEI Consultants, Inc.**  
**Workorder# 0804565**

Two 6 Liter Summa Canister samples were received on April 24, 2008. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

This workorder was independently validated prior to submittal using 'USEPA National Functional Guidelines' as generally applied to the analysis of volatile organic compounds in air. A rules-based, logic driven, independent validation engine was employed to assess completeness, evaluate pass/fail of relevant project quality control requirements and verification of all quantified amounts.

Method modifications taken to run these samples are summarized in the table below. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	+/- 30% Difference	<=/= 30% Difference with two allowed out up to <=/=40%.; flag and narrate outliers
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

**Receiving Notes**

There were no receiving discrepancies.

**Analytical Notes**

There were no analytical discrepancies.

**Definition of Data Qualifying Flags**

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

B - Compound present in laboratory blank greater than reporting limit (background subtraction no performed).

J - Estimated value.

E - Exceeds instrument calibration range.

S - Saturated peak.

Q - Exceeds quality control limits.



---

AN ENVIRONMENTAL ANALYTICAL LABORATORY

- U - Compound analyzed for but not detected above the reporting limit.
- UJ- Non-detected compound associated with low bias in the CCV
- N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

- a-File was requantified
- b-File was quantified by a second column and detector
- r1-File was requantified for the purpose of reissue

**Table 1**

<b>Client Sample ID</b>	<b>Lab Sample ID</b>	<b>Date Collected</b>	<b>Date Received</b>	<b>Date Extracted</b>	<b>Sample Holding Time (Days)</b>	<b>Date Analyzed</b>	<b>Sample Extract Holding Time (Days)</b>	<b>Sample Condition</b>
AMS UW	0804565-01A	4/23/2008	4/24/2008	NA	9	5/ 2/2008	NA	Good
AMS DW	0804565-02A	4/23/2008	4/24/2008	NA	9	5/ 2/2008	NA	Good
Lab Blank	0804565-03A	NA	NA	NA	NA	5/ 2/2008	NA	Good
CCV	0804565-04A	NA	NA	NA	NA	5/ 2/2008	NA	Good
LCS	0804565-05A	NA	NA	NA	NA	5/ 2/2008	NA	Good

## **Sample Results and Raw Data**



AN ENVIRONMENTAL ANALYTICAL LABORATORY

---

**Summary of Detected Compounds**  
**MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN**

**Client Sample ID: AMS UW**

**Lab ID#: 0804565-01A**

<b>Compound</b>	<b>Rpt. Limit (ppbv)</b>	<b>Amount (ppbv)</b>	<b>Rpt. Limit (uG/m3)</b>	<b>Amount (uG/m3)</b>
Toluene	0.74	1.3	2.8	4.9





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS UW

Lab ID#: 0804565-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050212	Date of Collection:	4/23/08
Dil. Factor:	1.49	Date of Analysis:	5/2/08 02:16 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.74	Not Detected	3.7	Not Detected
Freon 114	0.74	Not Detected	5.2	Not Detected
Vinyl Chloride	0.74	Not Detected	1.9	Not Detected
Bromomethane	0.74	Not Detected	2.9	Not Detected
Chloroethane	0.74	Not Detected	2.0	Not Detected
Freon 11	0.74	Not Detected	4.2	Not Detected
1,1-Dichloroethene	0.74	Not Detected	3.0	Not Detected
Freon 113	0.74	Not Detected	5.7	Not Detected
Methylene Chloride	0.74	Not Detected	2.6	Not Detected
1,1-Dichloroethane	0.74	Not Detected	3.0	Not Detected
cis-1,2-Dichloroethene	0.74	Not Detected	3.0	Not Detected
Chloroform	0.74	Not Detected	3.6	Not Detected
1,1,1-Trichloroethane	0.74	Not Detected	4.1	Not Detected
Carbon Tetrachloride	0.74	Not Detected	4.7	Not Detected
Benzene	0.74	Not Detected	2.4	Not Detected
1,2-Dichloroethane	0.74	Not Detected	3.0	Not Detected
Trichloroethene	0.74	Not Detected	4.0	Not Detected
1,2-Dichloropropane	0.74	Not Detected	3.4	Not Detected
cis-1,3-Dichloropropene	0.74	Not Detected	3.4	Not Detected
Toluene	0.74	1.3	2.8	4.9
trans-1,3-Dichloropropene	0.74	Not Detected	3.4	Not Detected
1,1,2-Trichloroethane	0.74	Not Detected	4.1	Not Detected
Tetrachloroethene	0.74	Not Detected	5.0	Not Detected
1,2-Dibromoethane (EDB)	0.74	Not Detected	5.7	Not Detected
Chlorobenzene	0.74	Not Detected	3.4	Not Detected
Ethyl Benzene	0.74	Not Detected	3.2	Not Detected
m,p-Xylene	0.74	Not Detected	3.2	Not Detected
o-Xylene	0.74	Not Detected	3.2	Not Detected
Styrene	0.74	Not Detected	3.2	Not Detected
1,1,1,2-Tetrachloroethane	0.74	Not Detected	5.1	Not Detected
1,3,5-Trimethylbenzene	0.74	Not Detected	3.7	Not Detected
1,2,4-Trimethylbenzene	0.74	Not Detected	3.7	Not Detected
1,3-Dichlorobenzene	0.74	Not Detected	4.5	Not Detected
1,4-Dichlorobenzene	0.74	Not Detected	4.5	Not Detected
alpha-Chlorotoluene	0.74	Not Detected	3.8	Not Detected
1,2-Dichlorobenzene	0.74	Not Detected	4.5	Not Detected
1,3-Butadiene	0.74	Not Detected	1.6	Not Detected
Hexane	0.74	Not Detected	2.6	Not Detected
Cyclohexane	0.74	Not Detected	2.6	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS UW

Lab ID#: 0804565-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050212	Date of Collection:	4/23/08
Dil. Factor:	1.49	Date of Analysis:	5/2/08 02:16 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.74	Not Detected	3.0	Not Detected
Bromodichloromethane	0.74	Not Detected	5.0	Not Detected
Dibromochloromethane	0.74	Not Detected	6.3	Not Detected
Cumene	0.74	Not Detected	3.7	Not Detected
Propylbenzene	0.74	Not Detected	3.7	Not Detected
Chloromethane	3.0	Not Detected	6.2	Not Detected
1,2,4-Trichlorobenzene	3.0	Not Detected	22	Not Detected
Hexachlorobutadiene	3.0	Not Detected	32	Not Detected
Acetone	3.0	Not Detected	7.1	Not Detected
Carbon Disulfide	0.74	Not Detected	2.3	Not Detected
2-Propanol	3.0	Not Detected	7.3	Not Detected
trans-1,2-Dichloroethene	0.74	Not Detected	3.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.74	Not Detected	2.2	Not Detected
Tetrahydrofuran	0.74	Not Detected	2.2	Not Detected
1,4-Dioxane	3.0	Not Detected	11	Not Detected
4-Methyl-2-pentanone	0.74	Not Detected	3.0	Not Detected
2-Hexanone	3.0	Not Detected	12	Not Detected
Bromoform	0.74	Not Detected	7.7	Not Detected
4-Ethyltoluene	0.74	Not Detected	3.7	Not Detected
Ethanol	3.0	Not Detected	5.6	Not Detected
Methyl tert-butyl ether	0.74	Not Detected	2.7	Not Detected
3-Chloropropene	3.0	Not Detected	9.3	Not Detected
2,2,4-Trimethylpentane	0.74	Not Detected	3.5	Not Detected
Naphthalene	3.0	Not Detected	16	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	88	70-130
1,2-Dichloroethane-d4	78	70-130
4-Bromofluorobenzene	113	70-130

Report Date: 07-May-2008 14:16

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-02may.b/5050212.d  
 Lab Smp Id: 0804565-01A  
 Inj Date : 02-MAY-2008 14:16  
 Operator : srs Inst ID: msd5.i  
 Smp Info : 200mL #11298  
 Misc Info : 3.0"Hg -> 5psi  
 Comment :  
 Method : /chem/msd5.i/5-02may.b/t14q424a.m  
 Meth Date : 02-May-2008 16:50 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1  
 Dil Factor: 1.49000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				( PPBV)	( PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 71	Bromochloromethane					CAS #: 74-97-5		
8.087	8.059	(1.000)	130	255678	25.0000	80.00- 120.00	100.00	
8.087	8.059	(1.000)	128	195625		50.87- 110.87	76.51	
8.059	8.059	(1.000)	49	395436		129.59- 189.59	154.66	
-----								
* 92	1,4-Difluorobenzene					CAS #: 540-36-3		
9.939	9.939	(1.000)	114	915719	25.0000	80.00- 120.00	100.00	
9.911	9.939	(1.000)	88	130749		0.00- 43.72	14.28	
-----								
* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.999	14.999	(1.000)	117	821742	25.0000	80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	378568		0.00- 30.00	46.07	
-----								
\$ 84	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.137	9.137	(1.130)	65	251706	19.3953	80.00- 120.00	100.00	
9.137	9.137	(1.130)	67	136052		0.00- 30.00	54.05	
-----								
\$ 107	Toluene-d8					CAS #: 2037-26-5		
12.704	12.704	(1.278)	98	767440	22.0539	80.00- 120.00	100.00	
12.704	12.704	(1.278)	70	69322		0.00- 30.00	9.03	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
== =====

\$ 107 Toluene-d8 (continued)

12.704 12.704 (1.278) 100 512640 0.00- 30.00 66.80

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575 16.575 (1.105) 174 562692 28.2009 28.201 80.00- 120.00 100.00

16.575 16.575 (1.105) 95 657325 79.99- 139.99 116.82

16.575 16.575 (1.105) 176 532135 64.67- 124.67 94.57

108 Toluene

CAS #: 108-88-3

12.815 12.815 (1.289) 91 39358 0.88097 1.313 80.00- 120.00 100.00

12.815 12.815 (1.289) 92 22250 29.74- 89.74 56.53

Report Date: 07-May-2008 14:16

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARYInstrument ID: msd5.i  
Lab File ID: 5050212.d  
Lab Smp Id: 0804565-01ACalibration Date: 02-MAY-2008  
Calibration Time: 07:55

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: srs

Method File: /chem/msd5.i/5-02may.b/t14q424a.m

Misc Info: 3.0"Hg -&gt; 5psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	339808	203885	475731	255678	-24.76
92 1,4-Difluorobenze	1321223	792734	1849712	915719	-30.69
125 Chlorobenzene-d5	1146934	688160	1605708	821742	-28.35

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.09	0.34
92 1,4-Difluorobenze	9.94	9.61	10.27	9.94	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-02may  
Sample Matrix: GAS Fraction: VOA  
Lab Smp Id: 0804565-01A  
Level: LOW Operator: srs  
Data Type: MS DATA SampleType: SAMPLE  
SpikeList File: 2926Spectra.spk Quant Type: ISTD  
Sublist File: AT08.sub  
Method File: /chem/msd5.i/5-02may.b/t14q424a.m  
Misc Info: 3.0"Hg -> 5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	19.395	77.58	70-130
\$ 107 Toluene-d8	25.000	22.054	88.22	70-130
\$ 138 Bromofluorobenzene	25.000	28.201	112.80	70-130

Data File: /chem/msd5.1/5-02may.b/5050212.d

Date : 02-MAY-2008 14:16

Client ID:

Sample Info: 200mL #11298


Column phase: RTX-624

Instrument: msd5.1

Operator: srs

Column diameter: 0.53

/chem/msd5.1/5-02may.b/5050212.d



Date : 02-MAY-2008 14:16

Client ID:

Instrument: msd5.i

Sample Info: 200mL #11298







Operator: srs

Column phase: RTX-624

Column diameter: 0.53

108 Toluene

Concentration: 1,313 PPBV







AN ENVIRONMENTAL ANALYTICAL LABORATORY

---

**Summary of Detected Compounds**  
**MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN**

**Client Sample ID: AMS DW**

**Lab ID#: 0804565-02A**

<b>Compound</b>	<b>Rpt. Limit (ppbv)</b>	<b>Amount (ppbv)</b>	<b>Rpt. Limit (uG/m3)</b>	<b>Amount (uG/m3)</b>
Toluene	0.86	1.7	3.2	6.3



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS DW

Lab ID#: 0804565-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050213	Date of Collection:	4/23/08
Dil. Factor:	1.71	Date of Analysis:	5/2/08 02:49 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.86	Not Detected	4.2	Not Detected
Freon 114	0.86	Not Detected	6.0	Not Detected
Vinyl Chloride	0.86	Not Detected	2.2	Not Detected
Bromomethane	0.86	Not Detected	3.3	Not Detected
Chloroethane	0.86	Not Detected	2.2	Not Detected
Freon 11	0.86	Not Detected	4.8	Not Detected
1,1-Dichloroethene	0.86	Not Detected	3.4	Not Detected
Freon 113	0.86	Not Detected	6.6	Not Detected
Methylene Chloride	0.86	Not Detected	3.0	Not Detected
1,1-Dichloroethane	0.86	Not Detected	3.5	Not Detected
cis-1,2-Dichloroethene	0.86	Not Detected	3.4	Not Detected
Chloroform	0.86	Not Detected	4.2	Not Detected
1,1,1-Trichloroethane	0.86	Not Detected	4.7	Not Detected
Carbon Tetrachloride	0.86	Not Detected	5.4	Not Detected
Benzene	0.86	Not Detected	2.7	Not Detected
1,2-Dichloroethane	0.86	Not Detected	3.5	Not Detected
Trichloroethene	0.86	Not Detected	4.6	Not Detected
1,2-Dichloropropane	0.86	Not Detected	4.0	Not Detected
cis-1,3-Dichloropropene	0.86	Not Detected	3.9	Not Detected
Toluene	0.86	1.7	3.2	6.3
trans-1,3-Dichloropropene	0.86	Not Detected	3.9	Not Detected
1,1,2-Trichloroethane	0.86	Not Detected	4.7	Not Detected
Tetrachloroethene	0.86	Not Detected	5.8	Not Detected
1,2-Dibromoethane (EDB)	0.86	Not Detected	6.6	Not Detected
Chlorobenzene	0.86	Not Detected	3.9	Not Detected
Ethyl Benzene	0.86	Not Detected	3.7	Not Detected
m,p-Xylene	0.86	Not Detected	3.7	Not Detected
o-Xylene	0.86	Not Detected	3.7	Not Detected
Styrene	0.86	Not Detected	3.6	Not Detected
1,1,2,2-Tetrachloroethane	0.86	Not Detected	5.9	Not Detected
1,3,5-Trimethylbenzene	0.86	Not Detected	4.2	Not Detected
1,2,4-Trimethylbenzene	0.86	Not Detected	4.2	Not Detected
1,3-Dichlorobenzene	0.86	Not Detected	5.1	Not Detected
1,4-Dichlorobenzene	0.86	Not Detected	5.1	Not Detected
alpha-Chlorotoluene	0.86	Not Detected	4.4	Not Detected
1,2-Dichlorobenzene	0.86	Not Detected	5.1	Not Detected
1,3-Butadiene	0.86	Not Detected	1.9	Not Detected
Hexane	0.86	Not Detected	3.0	Not Detected
Cyclohexane	0.86	Not Detected	2.9	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS DW

Lab ID#: 0804565-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050213	Date of Collection:	4/23/08
Dil. Factor:	1.71	Date of Analysis:	5/2/08 02:49 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.86	Not Detected	3.5	Not Detected
Bromodichloromethane	0.86	Not Detected	5.7	Not Detected
Dibromochloromethane	0.86	Not Detected	7.3	Not Detected
Cumene	0.86	Not Detected	4.2	Not Detected
Propylbenzene	0.86	Not Detected	4.2	Not Detected
Chloromethane	3.4	Not Detected	7.1	Not Detected
1,2,4-Trichlorobenzene	3.4	Not Detected	25	Not Detected
Hexachlorobutadiene	3.4	Not Detected	36	Not Detected
Acetone	3.4	Not Detected	8.1	Not Detected
Carbon Disulfide	0.86	Not Detected	2.7	Not Detected
2-Propanol	3.4	Not Detected	8.4	Not Detected
trans-1,2-Dichloroethene	0.86	Not Detected	3.4	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.86	Not Detected	2.5	Not Detected
Tetrahydrofuran	0.86	Not Detected	2.5	Not Detected
1,4-Dioxane	3.4	Not Detected	12	Not Detected
4-Methyl-2-pentanone	0.86	Not Detected	3.5	Not Detected
2-Hexanone	3.4	Not Detected	14	Not Detected
Bromoform	0.86	Not Detected	8.8	Not Detected
4-Ethyltoluene	0.86	Not Detected	4.2	Not Detected
Ethanol	3.4	Not Detected	6.4	Not Detected
Methyl tert-butyl ether	0.86	Not Detected	3.1	Not Detected
3-Chloropropene	3.4	Not Detected	11	Not Detected
2,2,4-Trimethylpentane	0.86	Not Detected	4.0	Not Detected
Naphthalene	3.4	Not Detected	18	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	89	70-130
1,2-Dichloroethane-d4	82	70-130
4-Bromofluorobenzene	107	70-130

Report Date: 07-May-2008 14:16

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-02may.b/5050213.d  
 Lab Smp Id: 0804565-02A  
 Inj Date : 02-MAY-2008 14:49  
 Operator : srs Inst ID: msd5.i  
 Smp Info : 200mL #34364  
 Misc Info : 6.5"Hg -> 5psi  
 Comment :  
 Method : /chem/msd5.i/5-02may.b/t14q424a.m  
 Meth Date : 02-May-2008 16:50 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1  
 Dil Factor: 1.71000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				( PPBV)	( PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 71	Bromochloromethane					CAS #: 74-97-5		
8.087	8.059	(1.000)	130	250028	25.0000	80.00- 120.00	100.00	
8.087	8.059	(1.000)	128	196788		50.87- 110.87	78.71	
8.059	8.059	(1.000)	49	388965		129.59- 189.59	155.57	
-----								
* 92	1,4-Difluorobenzene					CAS #: 540-36-3		
9.939	9.939	(1.000)	114	901323	25.0000	80.00- 120.00	100.00	
9.911	9.939	(1.000)	88	132459		0.00- 43.72	14.70	
-----								
* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.999	14.999	(1.000)	117	832449	25.0000	80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	381611		0.00- 30.00	45.84	
-----								
\$ 84	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.137	9.137	(1.130)	65	261533	20.6080	20.608 80.00- 120.00	100.00	
9.137	9.137	(1.130)	67	135669		0.00- 30.00	51.87	
-----								
\$ 107	Toluene-d8					CAS #: 2037-26-5		
12.704	12.704	(1.278)	98	766035	22.3651	22.365 80.00- 120.00	100.00	
12.704	12.704	(1.278)	70	65603		0.00- 30.00	8.56	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
== =====

\$ 107 Toluene-d8 (continued)

12.704 12.704 (1.278) 100 519412 0.00- 30.00 67.81

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575 16.575 (1.105) 174 538793 26.6558 26.656 80.00- 120.00 100.00

16.575 16.575 (1.105) 95 618729 79.99- 139.99 114.84

16.575 16.575 (1.105) 176 532514 64.67- 124.67 98.83

108 Toluene

CAS #: 108-88-3

12.815 12.815 (1.289) 91 42881 0.97516 1.668 80.00- 120.00 100.00

12.815 12.815 (1.289) 92 26253 29.74- 89.74 61.22

Report Date: 07-May-2008 14:16

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i  
 Lab File ID: 5050213.d  
 Lab Smp Id: 0804565-02A  
 Analysis Type: VOA  
 Quant Type: ISTD  
 Operator: srs  
 Method File: /chem/msd5.i/5-02may.b/t14q424a.m  
 Misc Info: 6.5"Hg -> 5psi

Calibration Date: 02-MAY-2008  
 Calibration Time: 07:55  
 Level: LOW  
 Sample Type: AIR

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	339808	203885	475731	250028	-26.42
92 1,4-Difluorobenze	1321223	792734	1849712	901323	-31.78
125 Chlorobenzene-d5	1146934	688160	1605708	832449	-27.42

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.09	0.34
92 1,4-Difluorobenze	9.94	9.61	10.27	9.94	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-02may  
Sample Matrix: GAS Fraction: VOA  
Lab Smp Id: 0804565-02A  
Level: LOW Operator: srs  
Data Type: MS DATA SampleType: SAMPLE  
SpikeList File: 2926Spectra.spk Quant Type: ISTD  
Sublist File: AT08.sub  
Method File: /chem/msd5.i/5-02may.b/t14q424a.m  
Misc Info: 6.5"Hg -> 5psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	20.608	82.43	70-130
\$ 107 Toluene-d8	25.000	22.365	89.46	70-130
\$ 138 Bromofluorobenzene	25.000	26.656	106.62	70-130

Data File: /chem/msd5.1/5-02may.b/5050213.d

Date: 02-MAY-2008 14:49

Client ID:

Sample Info: 200mL #34364


Column phase: RTX-624

Instrument: msd5.1

Operator: sps

Column diameter: 0.53

/chem/msd5.1/5-02may.b/5050213.d





Date : 02-MAY-2008 14:49

Client ID:

Instrument: msd5.i

Sample Info: 200mL #34364







Operator: srs

Column phase: RTX-624

Column diameter: 0.53

108 Toluene

Concentration: 1,668 PPBV



## **QC Results and Raw Data**



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0804565-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050204	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 5/2/08 09:23 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0804565-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050204	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 5/2/08 09:23 AM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected	2.0	Not Detected
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	90	70-130
1,2-Dichloroethane-d4	80	70-130
4-Bromofluorobenzene	104	70-130

Report Date: 07-May-2008 14:44

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-02may.b/5050204.d  
 Lab Smp Id: Lab Blank Client Smp ID: Lab Blank  
 Inj Date : 02-MAY-2008 09:23  
 Operator : srs Inst ID: msd5.i  
 Smp Info : 200mL #12941  
 Misc Info : Cart #15/ Leg #8  
 Comment :  
 Method : /var/chem/msd5.i/5-02may.b/t14q424a.m  
 Meth Date : 02-May-2008 16:50 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				( PPBV )	( PPBV )			
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 71	Bromochloromethane					CAS #: 74-97-5		
8.087	8.059	(1.000)	130	273720	25.0000	80.00- 120.00	100.00	
8.087	8.059	(1.000)	128	210261		50.87- 110.87	76.82	
8.059	8.059	(1.000)	49	429587		129.59- 189.59	156.94	
-----								
* 92	1,4-Difluorobenzene					CAS #: 540-36-3		
9.939	9.939	(1.000)	114	978352	25.0000	80.00- 120.00	100.00	
9.912	9.939	(1.000)	88	133144		0.00- 43.72	13.61	
-----								
* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.999	14.999	(1.000)	117	904787	25.0000	80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	413522		0.00- 30.00	45.70	
-----								
\$ 84	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.137	9.137	(1.130)	65	278846	20.0704	20.070 80.00- 120.00	100.00	
9.137	9.137	(1.130)	67	149711		0.00- 30.00	53.69	
-----								
\$ 107	Toluene-d8					CAS #: 2037-26-5		
12.704	12.704	(1.278)	98	832952	22.4041	22.404 80.00- 120.00	100.00	
12.704	12.704	(1.278)	70	78838		0.00- 30.00	9.47	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
== =====

\$ 107 Toluene-d8 (continued)

12.704 12.704 (1.278) 100 552267 0.00- 30.00 66.30

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575 16.575 (1.105) 174 573181 26.0900 26.090 80.00- 120.00 100.00

16.575 16.575 (1.105) 95 670695 79.99- 139.99 117.01

16.575 16.575 (1.105) 176 547961 64.67- 124.67 95.60

Report Date: 07-May-2008 14:44

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 02-MAY-2008

Lab File ID: 5050204.d

Calibration Time: 07:55

Lab Smp Id: Lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: srs

Method File: /var/chem/msd5.i/5-02may.b/t14q424a.m

Misc Info: Cart #15/ Leg #8

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	339808	203885	475731	273720	-19.45
92 1,4-Difluorobenze	1321223	792734	1849712	978352	-25.95
125 Chlorobenzene-d5	1146934	688160	1605708	904787	-21.11

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.09	0.34
92 1,4-Difluorobenze	9.94	9.61	10.27	9.94	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-02may  
Sample Matrix: GAS Fraction: VOA  
Lab Smp Id: Lab Blank Client Smp ID: Lab Blank  
Level: LOW Operator: srs  
Data Type: MS DATA SampleType: SAMPLE  
SpikeList File: 2926Spectra.spk Quant Type: ISTD  
Sublist File: AT08.sub  
Method File: /var/chem/msd5.i/5-02may.b/t14q424a.m  
Misc Info: Cart #15/ Leg #8

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	20.070	80.28	70-130
\$ 107 Toluene-d8	25.000	22.404	89.62	70-130
\$ 138 Bromofluorobenzene	25.000	26.090	104.36	70-130




Data File: /chem/msd5.1/5-02may.b/5050204.d  
Date : 02-MAY-2008 09:23  
Client ID: Lab Blank  
Sample Info: 200mL #12941

Column phase: RTX-624

Instrument: msd5.1  
Operator: srs  
Column diameter: 0.53

/chem/msd5.1/5-02may.b/5050204.d



# LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0804565

	CLIENT SAMPLE NO.	SURROGATE % RECOVERY						TOTAL OUT
		1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#	
01	AMS UW	78		88		113		0
02	AMS DW	82		89		107		0
03	Lab Blank	80		90		104		0
04	CCV	87		90		110		0
05	LCS	82		92		107		0
06								0
07								0
08								0
09								0
10								0
11								0
12								0
13								0
14								0
15								0
16								0
17								0
18								0
19								0
20								0
21								0
22								0
23								0
24								0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

\* Designates values outside of QC limits

# LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan

INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD  
 Lab File ID: 5050202.d  
 Instrument ID: msd5.i

SDG No: 0804565  
 Date Analyzed: 05/02/2008  
 Time Analyzed: 07:55 AM

	Chlorobenzene-d5			1,4-Difluorobenzene			Bromochloromethane			
	Area	#	RT	Area	#	RT	Area	#	RT	
24-HOUR STD	1146934		15	1321223		9.94	339808		8.06	
UPPER LIMIT	1605708		15.33	1849712		10.27	475731		08.39	
LOWER LIMIT	688160		14.67	792734		09.61	203885		07.73	
CLIENT SAMPLE NO										
01	AMS UW	821742		15	915719		9.94	255678		8.09
02	AMS DW	832449		15	901323		9.94	250028		8.09
03	Lab Blank	904787		15	978352		9.94	273720		8.09
04	CCV	1146934		15	1321223		9.94	339808		8.06
05	LCS	954742		15	1035215		9.91	279575		8.06
06										
07										
08										
09										
10										
11										
12										
13										
14										
15										
16										
17										
18										
19										
20										
21										
22										

'Area Upper Limit=+40% of internal standard area'  
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT  
 RT Lower Limit=-0.33 minutes of internal standard RT

\* Designates values outside of QC limits



Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	Level 7	RRF	% RSD
8 Dichlorodifluoromethane/Fr12	200.000 +++++	2.65175 3.20397	2.66596	3.61957	3.38330	3.11572		3.10671	12.469
9 Freon 114	+++++	2.03286 2.51929	2.07870	3.06026	2.81589	2.67780		2.53080	16.154
10 Chloromethane	+++++	+++++	1.99632	2.66910	2.48169	2.26860		2.33479	10.881
11 Butane	+++++	+++++	0.46720	0.56323	0.52069	0.50107		0.50491	7.764
12 1,3-Butadiene	2.68364 1.82755	1.24930	1.42563	2.03263	1.99948	1.90640		1.87495	24.739
13 Vinyl Chloride	+++++	1.53130 1.95144	1.45895	2.29544	2.11603	2.02012		1.89555	17.504
14 Methanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
15 Bromomethane	+++++	0.87840 1.16069	0.75647	1.17367	1.20731	1.18131		1.05964	18.132
16 Dichlorofluoromethane/Fr21	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
17 Isopentane	+++++	+++++	2.42579 3.09571	3.51099	3.39504	3.21805		3.12912	13.561

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
18 Pentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
19 Chloroethane	+++++	0.80965	0.70216	1.13837	1.02942	0.99913		0.94135	16.813
20 Trichlorofluoromethane/Fr11	+++++	2.35230	2.64117	3.74397	3.60173	3.41655		3.16868	17.471
21 Dimethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
22 Freon123a	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
23 Freon 13	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
24 Freon123	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
25 Acrolein	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
26 Ethanol	+++++	+++++	0.53043	0.86770	0.86700	0.75735		0.74860	18.494
27 Isobutylene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
28 Acetaldehyde	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
29 Freon143a	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
30 Freon 113	+++++	1.59753	1.65562	2.28010	2.11527	2.07237		1.95225	13.819
31 1,1-Dichloroethene	+++++	1.89339	1.95441	2.96826	2.85293	2.75857		2.50732	18.618
32 Acetone	+++++	+++++	0.79187	1.02568	1.00082	1.01356		0.96038	10.043
33 Methyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
34 Acetonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
35 Carbon Disulfide	+++++	3.50442	3.39393	5.05180	4.82791	4.70780		4.32685	16.311
36 2-Propanol	+++++	+++++	2.45298	3.87834	3.95950	3.99153		3.62782	18.168
37 tert-Butyl-Alcohol	+++++	+++++	1.89445	2.34598	2.02399	1.73016		1.85830	20.809

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
38 3-Chloropropene	+++++	+++++	0.40776	0.86612	0.83706	0.81927			
	0.79121							0.74428	25.539
39 Acrylonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
40 2-Methyl-1-Butene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
41 Vinyl Bromide	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
42 1-Pentene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
43 Methylene Chloride	+++++	2.17125	1.77048	2.63289	2.46455	2.36073			
	2.25166							2.27526	12.997
44 Ethyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
45 Ethanol-high	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
46 MTBE	+++++	1.50269	1.14477	2.77839	2.62016	2.61014			
	2.39535							2.17525	31.271 <-
47 trans-1,2-Dichloroethene	+++++	1.23473	1.34224	1.94190	1.84917	1.74383			
	1.68711							1.63316	17.330



Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
48 Propanal	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
49 Isopropyl ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
50 Bromoethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
51 Hexane	+++++ 3.43484	2.13256	2.44252	3.90550	3.75261	3.60689		3.21249	23.027
52 Chloroprene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
53 Iodomethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
54 2,3-Dimethylbutane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
55 1,1-Dichloroethane	+++++ 3.10393	2.54792	2.30414	3.49157	3.38363	3.24591		3.01285	15.902
56 Vinyl Acetate	+++++ 0.45966	+++++	0.21633	0.47604	0.46702	0.46313		0.41643	26.902
57 Ethyl-tert-butyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
58 1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
59 1,3-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
60 2,2-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
61 Ethyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
62 Methyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
63 2,4-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
64 1-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
65 Butanal	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
66 cis-1,2-Dichloroethene	+++++	1.57054	1.76262	2.59796	2.49411	2.36025	2.26367	2.17486	19.051
67 2-Butanone	+++++	0.39124	0.56473	0.90127	0.85795	0.86355	0.83105	0.73496	28.258

## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
68 2-Butanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
69 3-Methyl-1-Hexene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
70 Tetrahydrofuran	+++++	3.12236	2.04898	3.08667	2.98625	2.82001	2.73517	2.79990	14.191
72 Chloroform	3.79671	2.43454	1.99490	3.21927	3.04948	2.89534	2.79007	2.88290	19.898
73 1,1-Dichloropropene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
74 Cyclohexane	+++++	1.60203	1.48208	2.56583	2.48008	2.34492	2.27598	2.12515	21.853
75 1,1,1-Trichloroethane	+++++	2.59165	1.90373	3.05491	2.98910	2.82189	2.70083	2.67702	15.555
76 Isobutanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
77 Carbon Tetrachloride	+++++	2.07641	1.63147	2.83501	2.68823	2.61239	2.53549	2.39650	18.949
78 tert-amyl-Methyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
79 2,3-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
80 2,2,4-Trimethylpentane	+++++	7.24855	6.55974	11.20063	10.70025	10.31372		9.26895	20.695
81 Benzene	1.77995	0.93441	0.89335	1.40203	1.30564	1.25939		1.25391	23.838
82 1-Methoxy-2-Propanol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
83 2,3,4-Trimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
85 1,2-Dichloroethane	+++++	0.37029	0.35822	0.53913	0.50406	0.48155		0.45123	16.179
86 2-Pentanone	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
87 Pentanal	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
88 Ethyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
89 Octane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
90 Heptane	+++++	0.10275	0.11105	0.16131	0.15633	0.14724	0.14362	0.13705	17.753
91 1-Butanol	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
93 Trichloroethene	+++++	0.42200	0.36136	0.54488	0.50789	0.48570	0.46779	0.46494	14.021
94 Methyl Cyclohexane	+++++	0.57515	0.51058	0.81870	0.77118	0.73095	0.70658	0.68552	17.305
95 Dibromomethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
96 Methyl Methacrylate	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
97 1-Nitropropane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
98 1,2-Dichloropropane	+++++	0.33302	0.30841	0.49807	0.47028	0.44700	0.43003	0.41447	18.465
99 1,4-Dioxane	+++++	+++++	0.19738	0.30839	0.30453	0.28778	0.27612	0.27484	16.451
100 Bromodichloromethane	+++++	0.44096	0.43854	0.74973	0.69860	0.66766	0.64534	0.60680	22.093

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
101 1-Methoxy-2-propyl acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
102 Epichlorohydrin	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
103 cis-1,3-Dichloropropene	+++++	0.35708	0.33551	0.55599	0.54965	0.53126		0.47482	21.193
104 Decane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
105 alpha-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
106 4-Methyl-2-pentanone	+++++	0.22063	0.22108	0.41191	0.38852	0.38260		0.33266	26.338
108 Toluene	+++++	0.95590	0.98045	1.46944	1.37141	1.29243		1.21969	17.133
109 trans-1,4-dichloro-2-butene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
110 beta-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
111 Dicyclopentadiene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
112 Alphamethylstyrene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
113 trans-1,3-Dichloropropene	+++++	0.35839	0.33336	0.54838	0.56417	0.53521		0.48163	21.977
114 1,1,2-Trichloroethane	+++++	0.34807	0.30137	0.51241	0.49192	0.45132		0.42511	19.522
115 D-Limonene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
116 Tetrachloroethene	+++++	0.39536	0.46767	0.64596	0.62702	0.58770		0.55196	17.876
117 Bis(2-chloroethyl) ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
118 Butyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
119 2-Hexanone	+++++	+++++	0.34169	0.53643	0.55892	0.54822		0.50928	18.496
120 Dibromochloromethane	+++++	0.44513	0.46481	0.74068	0.72564	0.68286		0.62784	21.570
121 Undecane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000	0.50000	2.000	25.000	50.000	100.000	RRF	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6		
	200.000							
	Level 7							
122 1,2-Dibromoethane	0.94638	0.47758	0.51462	0.79651	0.77738	0.72873		
	0.73410						0.71076	23.048
123 1,1,1,2-Tetrachloroethane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
124 1-chloro-2-Bromopropane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
126 Chlorobenzene	+++++	0.78396	0.81168	1.19936	1.13646	1.06827		
	1.07096						1.01178	17.083
127 Nonane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
128 Ethyl Benzene	+++++	0.39688	0.43686	0.66089	0.65065	0.61255		
	0.59948						0.55955	20.296
129 Dodecane	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
130 m,p-Xylene	+++++	0.47090	0.54238	0.83373	0.80773	0.75893		
	0.76066						0.69572	21.690
131 2-Heptanone	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
132 o-Xylene	+++++	0.48149	0.48141	0.77972	0.75810	0.70358		
	0.69827						0.65043	20.688



Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
133 Styrene	1.26494 1.12924	0.67856	0.70280	1.21935	1.20021	1.13989		1.04786	23.708
134 Bromoform	+++++ 0.68286	0.47281	0.38311	0.69206	0.70268	0.67871		0.60204	22.929
135 Cyclohexanone	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
136 Cumene	2.51615 1.63719	1.41128	1.50925	2.28295	2.20880	2.09577		1.95163	21.959
137 Bromobenzene	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
139 1,2,3-Trichloropropane	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
140 2-Chlorotoluene	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
141 1,1,2,2-Tetrachloroethane	+++++ 0.97450	0.79632	0.79917	1.10121	1.06443	1.01446		0.95835	13.738
142 Propylbenzene	+++++ 1.97137	1.72459	1.76470	2.57632	2.57292	2.41591		2.17097	18.310
143 4-Chlorotoluene	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
144 4-Ethyltoluene	+++++	1.39175	1.54045	2.37218	2.42153	2.27393			
	1.80049							1.96672	22.802
145 Aniline	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
146 Diisobutyl Ketone	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
147 1,3,5-Trimethylbenzene	2.11823	1.26866	1.34535	2.08359	2.03283	1.94078			
	1.46101							1.75006	21.408
148 Isooctyl Alcohol	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
149 tert-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
150 Pentachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
151 sec-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
152 1,2,4-Trimethylbenzene	1.60994	0.98072	1.09745	1.69185	1.67993	1.61865			
	1.60198							1.46865	20.248
153 p-Cymene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
154 1,2,3-Trimethylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
155 1,3-Dichlorobenzene	+++++	0.84053	0.87148	1.13219	1.11736	1.07281		1.01978	12.654
156 1,4-Dichlorobenzene	+++++	1.00233	1.08949	1.43149	1.45097	1.39977		1.28420	14.874
157 alpha-Chlorotoluene	+++++	0.81198	1.05023	1.69854	1.84875	1.92279		1.44493	31.316 <-
158 Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
159 1,2-Dichlorobenzene	+++++	0.84670	1.02235	1.12726	1.12945	1.09132		1.04603	10.124
160 Hexachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
161 1,2-Dibromo-3-Chloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
162 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
163 1,2,4-Trichlorobenzene	+++++	+++++	0.85576	0.70648	0.75774	0.74671		0.76931	7.172

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 24-APR-2008 13:56  
 End Cal Date : 24-APR-2008 18:31  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Cal Date : 25-Apr-2008 09:57 sscott  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	25.000 Level 4	50.000 Level 5	100.000 Level 6	200.000 Level 7	RRF	% RSD
164 Hexachlorobutadiene	+++++	+++++	0.51444	0.52054	0.52223	0.50424		0.51903	2.085
165 Naphthalene	+++++	+++++	2.74543	2.50445	2.88705	2.81975		2.46443	25.609
166 1,2,3-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
167 Isooctyl Acrylate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
192 Cyclopentene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
193 Cyclopentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
\$ 84 1,2-Dichloroethane-d4	+++++	1.29246	1.13364	1.27531	1.28494	1.25825		1.26895	6.032
\$ 107 Toluene-d8	+++++	0.96474	0.91332	0.96077	0.97210	0.93754		0.95003	2.270
\$ 138 Bromofluorobenzene	+++++	0.59686	0.59255	0.61523	0.61442	0.60310		0.60703	1.834

Calibration History

Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
Start Cal Date: 24-APR-2008 13:56  
End Cal Date : 24-APR-2008 18:31

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.30000		
24-APR-2008 13:56	AFCEElow	/var/chem/msd5.i/5-24apr.b/5042413.d
Cal Level: 2 , Cal Amount: 0.50000		
24-APR-2008 14:23	AT08Low	/var/chem/msd5.i/5-24apr.b/5042414.d
Cal Level: 3 , Cal Amount: 2.00000		
24-APR-2008 18:31	AT08mdl	/var/chem/msd5.i/5-24apr.b/5042421.d
Cal Level: 4 , Cal Amount: 25.00000		
24-APR-2008 15:19	AT08mdl	/var/chem/msd5.i/5-24apr.b/5042416.d
Cal Level: 5 , Cal Amount: 50.00000		
24-APR-2008 15:47	AT08mdl	/var/chem/msd5.i/5-24apr.b/5042417.d
Cal Level: 6 , Cal Amount: 100.00000		
24-APR-2008 16:15	AT08mdl	/var/chem/msd5.i/5-24apr.b/5042418.d
Cal Level: 7 , Cal Amount: 200.00000		
24-APR-2008 16:48	AT08mdl	/var/chem/msd5.i/5-24apr.b/5042419.d

Continuing Calibration  
Ccal Level Mode: GLOBAL LEVEL 5

```
| Ccal Level: 5 , Ccal Amount: 50.000 |
+=====+
| 24-APR-2008 15:47 |AT08mdl          |/var/chem/msd5.i/5-24apr.b/5042417a.d |
+-----+-----+-----+
| Ccal Level: 5 , Ccal Amount: 50.000 |
+=====+
| 24-APR-2008 15:47 |AT08mdl          |/var/chem/msd5.i/5-24apr.b/5042417.d |
+-----+-----+-----+
```

@ Air Toxics Ltd.

# MSD-5

Logbook #: 1637

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	23.52
75	30.0 - 60.0% of mass 95	41.44
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.34
173	Less than 2.0% of mass 174	(0.65) <sup>1</sup>
174	Greater than 50.0% of mass 95	96.24
175	5.0 - 9.0% of mass 174	(7.33) <sup>1</sup>
176	Greater than 95.0% but less than 101.0% of mass 174	(96.92) <sup>1</sup>
177	5.0 - 9.0% of mass 176	(6.23) <sup>2</sup>

<sup>1</sup> - value in parenthesis is % mass 174      <sup>2</sup> - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio:  $\frac{952284}{991872} \times 150 = 96.92$

### Calculation Check:

ppbv of compound =  $\frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} \times \text{RRF}$

$= \frac{(1200024)}{(1234462)} \times (25.0) \times (0.95003) = 25.581$

Reported Result: 25.581

File ID: 5042417  
 Compound: Toluene-d8  
 Initials: KR

BFB Injection Date: 5042412  
 BFB Injection Time: 1323  
 BFB File ID: 5042412  
 Tekmar Purge Flow: 13.3 L/min  
 Vacuum: 6.5 in Hg  
 IS/Std #: 1541-103      Exp. Date: 7-4-08  
 BCM: 296697  
 1,4-DFB: 1234462  
 CB-d5: 1186736  
 Verified CCV IS vs ICAL mid-point (-40%D) KR

NOAH Cart #: 118      File #: 5042408 / 5042424

%	File #	Sample / Client Name	Can #	Pressure	Ami Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	5042412	BFB Toluene Check	142025	50psi	20µl	150	4/24/08	1323	KR	
✓	13	ICAL Level 1	1412-1	0.3 psi	0.5 µl			1356	SA	
✓	14			0.5 psi	0.5 µl			1423	SA	
X	15			2.0 psi	20 µl			MS1	KR	
✓	16			2.5 psi	0.5 µl			1519	KR	
✓	17			5.0 psi	50 µl			1547	KR	
✓	18			10.0 psi	100 µl			1615	KR	
✓	19			20.0 psi	200 µl			1648	KR	
✓	20	System Blank	12944	Blank	200 µl			1720	KR	

Signature: *[Handwritten Signature]*

Date: 4/24-08

10	✓	5042421	ICAL level 3	1612-1	2.0ppbv	2.0ml	1.00	4/24/08	1831	RR	
11	✓	22	ICS (200ppb)	1576338	50ppbv	50ml	1.00		1922	RR	ICAL ICS
12	X	23	System Blank	12941	Humid	200ml	1.00		2034	RR	
13	✓	24	Lab Blank	↓	↓	↓	↓		2136	RR	Get Cert #8, leg 1
14	✓	25	0304306A - 01AA	1359	45% <sub>15</sub> ssi	75ml	6.35		2230	RR	RR 45ml
15	X	26	-02A	3224	25% <sub>15</sub> ssi	16ml	2.20		2258	RR	RR 10ml
16	✓	27	-01A	1359	45% <sub>15</sub> ssi	45ml	10.6		2397	RR	
17	✓	28	-02A	3224	25% <sub>15</sub> ssi	10ml	44.0	4/25/08	0028	RR	
18	✓	29	-03A	1368	55% <sub>15</sub> ssi	200ml	2.47		0101	RR	
19	✓	30	-04A	3212	85% <sub>15</sub> ssi	↓	2.52		0133	RR	
20	✓	31	-05A	2208	50% <sub>15</sub> ssi	↓	2.42		0206	RR	
21	✓	32	-06A	9469	40% <sub>15</sub> ssi	15ml	31.1		0233	RR	
22	✓	33	-07A	1457	50% <sub>15</sub> ssi	200ml	2.42		0306	RR	
23	✓	34	-09A	1387	285% <sub>15</sub> ssi	↓	1.00		0339	RR	trip blank
24	✓	35	0304306A	1612	45% <sub>15</sub> ssi	200ml	2.33	4/25/08	0305	RR	
25											
26											
27											
28											
29											
30											
31											
32											

Comments: Fluo Controller S/N# AD92038

Actual: 25.0ml/min

NIST Fluo Beaker S/N# 2057744

Desired: 22.6ml/min

4/25/08

*[Signature]*

Signature

4/24/08

Date



### **Initial Calibration Narrative**

A seven point initial calibration was analyzed on MSD-5 on 4/24/2008. As noted on the accompanying analytical run log, the following point, ICAL Level 3, was re-analyzed due to:

- a. anomalous unacceptable linearity for Methyl tert-Butyl Ether, 2-Butanone, Chloroform, Benzene, Styrene, Cumene, 1,3,5-Trimethylbenzene and alpha-Chlorotoluene.

The following compounds used either 0.3ppbv as the lowest calibration concentration: 1,3-Butadiene, Chloroform, Benzene, Cumene, Styrene, 1,2-Dibromoethane, 1,2,4-Trimethylbenzene and 1,3,5-Trimethylbenzene.

Air Toxics Ltd.  
 Modified EPA Methods TO-14A/TO-15  
 Internal Standard and Associated Target Compounds and Surrogates

Bromochloromethane
<b>Target Compounds:</b>
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
3-Chloropropene
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
2,2,4-Trimethylpentane
<b>Surrogates:</b>
1,2-Dichloroethane-d4

1,4-Difluorobenzene
<b>Target Compounds:</b>
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
<b>Surrogates:</b>
Toluene-d8

Chlorobenzene-d5
<b>Target Compounds:</b>
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
<b>Surrogates:</b>
Bromofluorobenzene

Report Date: 25-Apr-2008 09:11

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042422.d  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Inj Date : 24-APR-2008 19:22  
 Operator : kr Inst ID: msd5.i  
 Smp Info : 50mL #1576-338  
 Misc Info : 50ppbv (200ppbv)  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:10 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1 QC Sample: LCS  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				( PPBV)	( PPBV)			
==	=====	=====	====	=====	=====	=====	=====	=====
-----								
* 71	Bromochloromethane					CAS #: 74-97-5		
8.059	8.059	(1.000)	130	331589	25.0000	70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	256337		47.51- 107.51	77.31	
8.059	8.059	(1.000)	49	602288		158.47- 218.47	181.64	
-----								
* 92	1,4-Difluorobenzene					CAS #: 540-36-3		
9.911	9.912	(1.000)	114	1351053	25.0000	70.00- 130.00	100.00	
9.911	9.912	(1.000)	88	192850		0.00- 44.75	14.27	
-----								
* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.999	14.999	(1.000)	117	1255534	25.0000	70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	613156		0.00- 30.00	48.84	
-----								
\$ 84	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.137	9.137	(1.134)	65	396044	23.5310	70.00- 130.00	100.00	
9.110	9.137	(1.130)	67	237937		0.00- 30.00	60.08	
-----								
\$ 107	Toluene-d8					CAS #: 2037-26-5		
12.704	12.704	(1.282)	98	1238972	24.1319	70.00- 130.00	100.00	
12.676	12.704	(1.279)	70	118132		0.00- 30.00	9.53	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== =====

\$ 107 Toluene-d8 (continued)

12.704 12.704 (1.282) 100 863921 0.00- 30.00 69.73

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575 16.575 (1.105) 174 777354 25.4987 25.499 70.00- 130.00 100.00

16.575 16.575 (1.105) 95 999529 98.07- 158.07 128.58

16.575 16.575 (1.105) 176 748102 65.46- 125.46 96.24

6 Propylene

CAS #: 115-07-1

2.253 2.280 (0.280) 41 1501366 58.3569 58.357 70.00- 130.00 100.00

2.253 2.280 (0.280) 42 981130 0.00- 30.00 65.35

2.253 2.280 (0.280) 39 1049981 0.00- 30.00 69.94

8 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.336 2.336 (0.290) 85 2188824 53.1190 53.119 70.00- 130.00 100.00

2.336 2.336 (0.290) 87 715403 0.00- 30.00 32.68

9 Freon 114

CAS #: 76-14-2

2.446 2.474 (0.304) 135 1940441 57.8073 57.807 70.00- 130.00 100.00

2.446 2.474 (0.304) 137 610608 2.03- 62.03 31.47

10 Chloromethane

CAS #: 74-87-3

2.584 2.640 (0.321) 50 1682776 54.3398 54.340 70.00- 130.00 100.00

2.584 2.640 (0.321) 52 479349 0.00- 30.00 28.49

13 Vinyl Chloride

CAS #: 75-01-4

2.750 2.778 (0.341) 62 1479192 58.8342 58.834 70.00- 130.00 100.00

2.750 2.778 (0.341) 64 440380 0.00- 30.00 29.77

12 1,3-Butadiene

CAS #: 106-99-0

2.750 2.778 (0.341) 54 1328688 53.4286 53.428 70.00- 130.00 100.00

2.750 2.778 (0.341) 39 1646858 0.00- 30.00 123.95

15 Bromomethane

CAS #: 74-83-9

3.276 3.276 (0.406) 94 816130 58.0684 58.068 70.00- 130.00 100.00

3.276 3.276 (0.406) 96 771726 62.86- 122.86 94.56

19 Chloroethane

CAS #: 75-00-3

3.386 3.442 (0.420) 64 734549 58.8314 58.831 70.00- 130.00 100.00

3.386 3.442 (0.420) 49 229784 0.00- 30.00 31.28

3.386 3.442 (0.420) 66 231068 0.00- 30.00 31.46

20 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.718 3.746 (0.461) 101 2408013 57.2955 57.295 70.00- 130.00 100.00

3.718 3.746 (0.461) 103 1574807 33.46- 93.46 65.40

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== =====

26 Ethanol CAS #: 64-17-5  
 4.077 4.133 (0.506) 45 612260 61.6631 61.663 70.00- 130.00 100.00  
 4.077 4.133 (0.506) 43 117827 0.00- 30.00 19.24  
 4.077 4.133 (0.506) 46 244574 0.00- 30.00 39.95

30 Freon 113 CAS #: 76-13-1  
 4.520 4.548 (0.561) 151 1640606 63.3591 63.359 70.00- 130.00 100.00  
 4.520 4.548 (0.561) 153 1061988 33.20- 93.20 64.73  
 4.520 4.548 (0.561) 101 2190742 106.78- 166.78 133.53

31 1,1-Dichloroethene CAS #: 75-35-4  
 4.575 4.575 (0.568) 61 2110296 63.4562 63.456 70.00- 130.00 100.00  
 4.575 4.575 (0.568) 96 1195787 23.41- 83.41 56.66  
 4.575 4.575 (0.568) 98 751299 4.01- 64.01 35.60

32 Acetone CAS #: 67-64-1  
 4.713 4.741 (0.585) 58 693397 54.4350 54.435 70.00- 130.00 100.00  
 4.713 4.741 (0.585) 43 2347609 0.00- 30.00 338.57

36 2-Propanol CAS #: 67-63-0  
 4.907 4.935 (0.609) 45 2771921 57.6069 57.607 70.00- 130.00 100.00  
 4.907 4.935 (0.609) 43 639999 0.00- 30.00 23.09  
 4.935 4.935 (0.612) 59 90037 0.00- 30.00 3.25

35 Carbon Disulfide CAS #: 75-15-0  
 4.907 4.935 (0.609) 76 3263951 56.8737 56.874 70.00- 130.00 100.00

38 3-Chloropropene CAS #: 107-05-1  
 5.183 5.211 (0.643) 76 576722 58.4210 58.421 70.00- 130.00 100.00  
 5.183 5.211 (0.643) 41 2265985 0.00- 30.00 392.91

43 Methylene Chloride CAS #: 75-09-2  
 5.432 5.460 (0.674) 49 1772014 58.7187 58.719 70.00- 130.00 100.00  
 5.432 5.460 (0.674) 84 1028336 26.74- 86.74 58.03  
 5.432 5.460 (0.674) 51 549037 0.00- 30.00 30.98

46 MTBE CAS #: 1634-04-4  
 5.764 5.764 (0.715) 73 1797365 62.2970 62.297 70.00- 130.00 100.00  
 5.764 5.764 (0.715) 57 537907 0.00- 59.41 29.93  
 5.764 5.764 (0.715) 41 606240 0.00- 30.00 33.73

47 trans-1,2-Dichloroethene CAS #: 156-60-5  
 5.819 5.819 (0.722) 96 1232976 56.9201 56.920 70.00- 130.00 100.00  
 5.819 5.819 (0.722) 61 1925292 130.65- 190.65 156.15  
 5.819 5.819 (0.722) 98 766450 0.00- 30.00 62.16

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== =====

51 Hexane CAS #: 110-54-3  
 6.151 6.151 (0.763) 57 2479052 58.1814 58.181 70.00- 130.00 100.00  
 6.151 6.151 (0.763) 43 1863890 0.00- 30.00 75.19  
 6.151 6.151 (0.763) 86 367075 0.00- 30.00 14.81

56 Vinyl Acetate CAS #: 108-05-4  
 6.649 6.649 (0.825) 86 312699 56.6136 56.614 70.00- 130.00 100.00  
 6.649 6.649 (0.825) 43 4150559 0.00- 30.00 1327.33  
 6.649 6.649 (0.825) 42 313026 0.00- 30.00 100.10

55 1,1-Dichloroethane CAS #: 75-34-3  
 6.594 6.594 (0.818) 63 2287723 57.2487 57.249 70.00- 130.00 100.00  
 6.594 6.594 (0.818) 65 700142 0.00- 59.62 30.60

67 2-Butanone CAS #: 78-93-3  
 7.644 7.644 (0.949) 72 581995 59.7027 59.703 70.00- 130.00 100.00  
 7.644 7.644 (0.949) 43 3136421 533.62- 593.62 538.91  
 7.644 7.644 (0.949) 57 212445 0.00- 30.00 36.50

66 cis-1,2-Dichloroethene CAS #: 156-59-2  
 7.617 7.617 (0.945) 61 1615757 56.0125 56.012 70.00- 130.00 100.00  
 7.617 7.617 (0.945) 96 1180723 42.00- 102.00 73.08  
 7.617 7.617 (0.945) 98 770418 15.56- 75.56 47.68

70 Tetrahydrofuran CAS #: 109-99-9  
 8.031 8.031 (0.997) 42 1853020 49.8973 49.897 70.00- 130.00 100.00  
 8.031 8.031 (0.997) 71 496644 0.00- 56.55 26.80  
 8.031 8.031 (0.997) 72 578454 0.00- 30.00 31.22

72 Chloroform CAS #: 67-66-3  
 8.197 8.197 (1.017) 83 1962704 51.3292 51.329 70.00- 130.00 100.00  
 8.197 8.197 (1.017) 85 1266070 35.57- 95.57 64.51

75 1,1,1-Trichloroethane CAS #: 71-55-6  
 8.446 8.446 (1.048) 97 1875433 52.8190 52.819 70.00- 130.00 100.00  
 8.446 8.446 (1.048) 99 1201320 34.21- 94.21 64.06

74 Cyclohexane CAS #: 110-82-7  
 8.418 8.419 (1.045) 84 1571870 55.7656 55.766 70.00- 130.00 100.00  
 8.418 8.419 (1.045) 56 2309787 117.94- 177.94 146.95  
 8.418 8.419 (1.045) 41 1349350 54.92- 114.92 85.84

77 Carbon Tetrachloride CAS #: 56-23-5  
 8.667 8.667 (1.075) 119 1729266 54.4032 54.403 70.00- 130.00 100.00  
 8.667 8.667 (1.075) 117 1767130 74.41- 134.41 102.19

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	FINAL	( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	
-----										
80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.082	9.110	(1.127)	57	6763489	55.0149	55.015	70.00-	130.00	100.00	
9.082	9.110	(1.127)	56	2215708			0.00-	30.00	32.76	
9.082	9.110	(1.127)	41	1785312			0.00-	30.00	26.40	
-----										
81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	3452029	50.9419	50.942	70.00-	130.00	100.00	
9.082	9.082	(0.916)	77	807997			0.00-	30.00	23.41	
-----										
85	1,2-Dichloroethane					CAS #: 107-06-2				
9.276	9.276	(0.936)	62	1332609	54.6477	54.648	70.00-	130.00	100.00	
9.276	9.276	(0.936)	64	403024			0.00-	30.00	30.24	
-----										
90	Heptane					CAS #: 142-82-5				
9.469	9.469	(0.955)	100	429408	57.9773	57.977	70.00-	130.00	100.00	
9.469	9.469	(0.955)	43	2845947			0.00-	30.00	662.76	
9.469	9.469	(0.955)	71	1240380			0.00-	30.00	288.86	
-----										
93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	1330615	52.9574	52.957	70.00-	130.00	100.00	
10.326	10.326	(1.042)	130	1368069			70.08-	130.08	102.81	
10.326	10.326	(1.042)	97	872410			35.30-	95.30	65.56	
-----										
98	1,2-Dichloropropane					CAS #: 78-87-5				
10.824	10.852	(1.092)	63	1206440	53.8619	53.862	70.00-	130.00	100.00	
10.824	10.852	(1.092)	62	838099			41.10-	101.10	69.47	
10.824	10.852	(1.092)	41	796076			36.18-	96.18	65.99	
-----										
99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.117)	88	760792	51.2217	51.222	70.00-	130.00	100.00	
11.073	11.073	(1.117)	58	594446			47.45-	107.45	78.14	
11.073	11.073	(1.117)	57	189225			0.00-	30.00	24.87	
-----										
100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.151)	83	1818101	55.4417	55.442	70.00-	130.00	100.00	
11.405	11.405	(1.151)	85	1169331			34.05-	94.05	64.32	
-----										
103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	1410863	54.9828	54.983	70.00-	130.00	100.00	
12.317	12.317	(1.243)	77	453184			1.82-	61.82	32.12	
12.289	12.317	(1.240)	39	932797			36.40-	96.40	66.12	
-----										
106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.593	12.594	(1.271)	58	1020712	56.7766	56.776	70.00-	130.00	100.00	
12.593	12.594	(1.271)	43	2973888			0.00-	30.00	291.35	
12.593	12.594	(1.271)	85	387521			0.00-	30.00	37.97	
-----										

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL ( PPEV)	FINAL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
108 Toluene						CAS #:	108-88-3			
12.815	12.815	(1.293)	91	3651425	55.3965	55.396	70.00-	130.00	100.00	
12.815	12.815	(1.293)	92	2140020			27.75-	87.75	58.61	
-----										
113 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.368	13.368	(0.891)	75	1369740	56.6289	56.629	70.00-	130.00	100.00	
13.368	13.368	(0.891)	77	445466			2.38-	62.38	32.52	
13.340	13.368	(0.889)	39	929200			35.96-	95.96	67.84	
-----										
114 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.644	13.644	(0.910)	97	1160208	54.3428	54.343	70.00-	130.00	100.00	
13.644	13.644	(0.910)	99	754821			33.83-	93.83	65.06	
13.644	13.644	(0.910)	83	970858			52.70-	112.70	83.68	
-----										
116 Tetrachloroethene						CAS #:	127-18-4			
13.699	13.700	(0.913)	166	1558346	56.2167	56.217	70.00-	130.00	100.00	
13.672	13.700	(0.912)	129	1147833			44.73-	104.73	73.66	
13.699	13.700	(0.913)	131	1110599			40.60-	100.60	71.27	
-----										
119 2-Hexanone						CAS #:	591-78-6			
14.004	14.004	(0.934)	58	1418073	55.4439	55.444	70.00-	130.00	100.00	
14.004	14.004	(0.934)	43	2882593			181.71-	241.71	203.28	
14.004	14.004	(0.934)	100	265430			0.00-	30.00	18.72	
-----										
120 Dibromochloromethane						CAS #:	124-48-1			
14.197	14.197	(0.947)	129	1793150	56.8695	56.870	70.00-	130.00	100.00	
14.197	14.197	(0.947)	127	1397788			0.00-	30.00	77.95	
-----										
122 1,2-Dibromoethane						CAS #:	106-93-4			
14.363	14.363	(0.958)	107	1827951	51.2100	51.210	70.00-	130.00	100.00	
14.363	14.363	(0.958)	109	1742982			65.00-	125.00	95.35	
-----										
126 Chlorobenzene						CAS #:	108-90-7			
15.027	15.027	(1.002)	112	2766941	54.4534	54.453	70.00-	130.00	100.00	
15.027	15.027	(1.002)	114	894424			2.42-	62.42	32.33	
15.027	15.027	(1.002)	77	1534400			27.34-	87.34	55.45	
-----										
128 Ethyl Benzene						CAS #:	100-41-4			
15.165	15.165	(1.011)	106	1565115	55.6953	55.695	70.00-	130.00	100.00	
15.165	15.165	(1.011)	91	4622099			0.00-	30.00	295.32	
-----										
130 m,p-Xylene						CAS #:	108-38-3			
15.331	15.331	(1.022)	106	1960833	56.1199	56.120	70.00-	130.00	100.00	
15.331	15.331	(1.022)	91	3721181			0.00-	30.00	189.78	
-----										
132 o-Xylene						CAS #:	95-47-6			
15.856	15.856	(1.057)	106	1819294	55.6949	55.695	70.00-	130.00	100.00	



CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL ( PPEV)	FINAL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	3660830			170.15- 230.15	201.22	
-----									
133 Styrene CAS #: 100-42-5									
15.911	15.912	(1.061)	104	2931227	55.7004	55.700	70.00- 130.00	100.00	
15.911	15.912	(1.061)	78	1274197			13.62- 73.62	43.47	
-----									
134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1718733	56.8452	56.845	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	891098			22.36- 82.36	51.85	
-----									
141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	2575821	53.5184	53.518	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	1661047			36.19- 96.19	64.49	
-----									
144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	5650417	57.2070	57.207	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	1733895			0.17- 60.17	30.69	
-----									
147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	4853979	55.2275	55.228	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	2492259			0.00- 30.00	51.34	
-----									
152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	3966816	53.7820	53.782	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	1931371			17.48- 77.48	48.69	
-----									
155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	2749774	53.6909	53.691	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	1768031			0.00- 30.00	64.30	
17.764	17.764	(1.184)	111	1078980			0.00- 30.00	39.24	
-----									
156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	3509232	54.4114	54.411	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	2205151			0.00- 30.00	62.84	
17.847	17.847	(1.190)	111	1290286			0.00- 30.00	36.77	
-----									
157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	4578753	63.0975	63.098	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	1021388			0.00- 30.00	22.31	
-----									
159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	2713296	51.6494	51.649	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	1744720			32.26- 92.26	64.30	
18.206	18.206	(1.214)	111	1007933			7.92- 67.92	37.15	
-----									

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	FINAL	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
163	1,2,4-Trichlorobenzene					CAS #:	120-82-1			
19.506	19.478	(1.300)	180	1856820	48.0595	48.060	70.00-	130.00	100.00	
19.506	19.478	(1.300)	182	1733882			63.09-	123.09	93.38	
-----										
164	Hexachlorobutadiene					CAS #:	87-68-3			
19.589	19.589	(1.306)	225	1235747	47.4073	47.407	70.00-	130.00	100.00	
19.589	19.589	(1.306)	223	767698			32.88-	92.88	62.12	
-----										
142	Propylbenzene					CAS #:	103-65-1			
16.824	16.824	(1.122)	91	6158985	56.4894	56.489	70.00-	130.00	100.00	
16.824	16.824	(1.122)	120	1467611			0.00-	30.00	23.83	
16.824	16.824	(1.122)	105	225979			0.00-	30.00	3.67	
-----										
136	Cumene					CAS #:	98-82-8			
16.326	16.326	(1.088)	105	5437672	55.4789	55.479	70.00-	130.00	100.00	
16.326	16.326	(1.088)	120	1545766			0.00-	30.00	28.43	
16.326	16.326	(1.088)	51	603564			0.00-	30.00	11.10	
-----										
165	Naphthalene					CAS #:	91-20-3			
19.672	19.672	(1.312)	128	6993033	56.5017	56.502	70.00-	130.00	100.00	
19.672	19.672	(1.312)	127	870934			0.00-	30.00	12.45	
-----										
37	tert-Butyl-Alcohol					CAS #:	75-65-0			
5.570	5.571	(0.691)	59	1352031	54.8543	54.854	70.00-	130.00	100.00	
5.570	5.571	(0.691)	41	403229			0.00-	30.00	29.82	
5.570	5.571	(0.691)	57	130878			0.00-	30.00	9.68	
-----										
11	Butane					CAS #:	106-97-8			
2.667	2.695	(0.331)	58	365901	54.6376	54.638	70.00-	130.00	100.00	
2.667	2.695	(0.331)	43	3031457			0.00-	30.00	828.49	
-----										
17	Isopentane					CAS #:	78-78-4			
3.414	3.414	(0.424)	43	2287263	55.1105	55.110	70.00-	130.00	100.00	
3.414	3.414	(0.424)	57	1324654			0.00-	30.00	57.91	
3.414	3.414	(0.424)	72	121895			0.00-	30.00	5.33	
-----										
94	Methyl Cyclohexane					CAS #:	108-87-2			
10.547	10.548	(1.064)	83	2017061	54.4459	54.446	70.00-	130.00	100.00	
10.547	10.548	(1.064)	98	995005			0.00-	30.00	49.33	
10.547	10.548	(1.064)	55	1888579			0.00-	30.00	93.63	
-----										

Report Date: 25-Apr-2008 09:11

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042422.d

Calibration Time: 15:47

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 50ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	331589	11.76
92 1,4-Difluorobenze	1234462	740677	1728247	1351053	9.44
125 Chlorobenzene-d5	1186736	712042	1661430	1255534	5.80

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-24apr  
 Sample Matrix: GAS Fraction: VOA  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Level: LOW Operator: kr  
 Data Type: MS DATA SampleType: LCS  
 SpikeList File: 2926Spectra.spk Quant Type: ISTD  
 Sublist File: AT08.sub  
 Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Misc Info: 50ppbv (200ppbv)

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
8 Dichlorodifluorome	50.000	53.119	106.24	70-130
9 Freon 114	50.000	57.807	115.61	70-130
10 Chloromethane	50.000	54.340	108.68	70-130
13 Vinyl Chloride	50.000	58.834	117.67	70-130
12 1,3-Butadiene	50.000	53.428	106.86	60-140
15 Bromomethane	50.000	58.068	116.14	70-130
19 Chloroethane	50.000	58.831	117.66	70-130
20 Trichlorofluoromet	50.000	57.295	114.59	70-130
26 Ethanol	50.000	61.663	123.33	60-140
30 Freon 113	50.000	63.359	126.72	70-130
31 1,1-Dichloroethene	50.000	63.456	126.91	70-130
35 Carbon Disulfide	50.000	56.874	113.75	60-140
32 Acetone	50.000	54.435	108.87	60-140
36 2-Propanol	50.000	57.607	115.21	60-140
38 3-Chloropropene	50.000	58.421	116.84	60-140
43 Methylene Chloride	50.000	58.719	117.44	70-130
46 MTBE	50.000	62.297	124.59	60-140
47 trans-1,2-Dichloro	50.000	56.920	113.84	60-140
51 Hexane	50.000	58.181	116.36	60-140
55 1,1-Dichloroethane	50.000	57.249	114.50	70-130
66 cis-1,2-Dichloroet	50.000	56.012	112.03	70-130
67 2-Butanone	50.000	59.703	119.41	60-140
70 Tetrahydrofuran	50.000	49.897	99.79	60-140
72 Chloroform	50.000	51.329	102.66	70-130
74 Cyclohexane	50.000	55.766	111.53	60-140
75 1,1,1-Trichloroeth	50.000	52.819	105.64	70-130
56 Vinyl Acetate	50.000	56.614	113.23	60-140
77 Carbon Tetrachlori	50.000	54.403	108.81	70-130
80 2,2,4-Trimethylpen	50.000	55.015	110.03	60-140
81 Benzene	50.000	50.942	101.88	70-130
85 1,2-Dichloroethane	50.000	54.648	109.30	70-130
90 Heptane	50.000	57.977	115.95	60-140
93 Trichloroethene	50.000	52.957	105.91	70-130

Report Date: 25-Apr-2008 09:11

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
98 1,2-Dichloropropan	50.000	53.862	107.72	70-130
99 1,4-Dioxane	50.000	51.222	102.44	60-140
100 Bromodichlorometha	50.000	55.442	110.88	60-140
103 cis-1,3-Dichloropr	50.000	54.983	109.97	70-130
106 4-Methyl-2-pentano	50.000	56.776	113.55	60-140
108 Toluene	50.000	55.396	110.79	70-130
113 trans-1,3-Dichloro	50.000	56.629	113.26	70-130
114 1,1,2-Trichloroeth	50.000	54.343	108.69	70-130
116 Tetrachloroethene	50.000	56.217	112.43	70-130
119 2-Hexanone	50.000	55.444	110.89	60-140
120 Dibromochlorometha	50.000	56.870	113.74	60-140
122 1,2-Dibromoethane	50.000	51.210	102.42	70-130
126 Chlorobenzene	50.000	54.453	108.91	70-130
128 Ethyl Benzene	50.000	55.695	111.39	70-130
130 m,p-Xylene	50.000	56.120	112.24	70-130
132 o-Xylene	50.000	55.695	111.39	70-130
133 Styrene	50.000	55.700	111.40	70-130
134 Bromoform	50.000	56.845	113.69	60-140
136 Cumene	50.000	55.479	110.96	60-140
141 1,1,2,2-Tetrachlor	50.000	53.518	107.04	70-130
142 Propylbenzene	50.000	56.489	112.98	60-140
144 4-Ethyltoluene	50.000	57.207	114.41	60-140
147 1,3,5-Trimethylben	50.000	55.228	110.46	70-130
152 1,2,4-Trimethylben	50.000	53.782	107.56	70-130
155 1,3-Dichlorobenzen	50.000	53.691	107.38	70-130
156 1,4-Dichlorobenzen	50.000	54.411	108.82	70-130
157 alpha-Chlorotoluen	50.000	63.098	126.20	70-130
159 1,2-Dichlorobenzen	50.000	51.649	103.30	70-130
163 1,2,4-Trichloroben	50.000	48.060	96.12	70-130
164 Hexachlorobutadien	50.000	47.407	94.81	70-130
6 Propylene	50.000	58.357	116.71	70-130
165 Naphthalene	50.000	56.502	113.00	60-140
11 Butane	50.000	54.638	109.28	70-130
17 Isopentane	50.000	55.110	110.22	70-130
94 Methyl Cyclohexane	50.000	54.446	108.89	70-130
37 tert-Butyl-Alcohol	50.000	54.854	109.71	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	23.531	94.12	70-130
\$ 107 Toluene-d8	25.000	24.132	96.53	70-130
\$ 138 Bromofluorobenzene	25.000	25.499	101.99	70-130




Data File: /var/chem/msd5.1/5-24apr.lb/5042422.d  
 Date: 24-APR-2008 19:22  
 Client ID: LCS-1  
 Sample Info: 50ml #1576-338

Column phase: RTX-624

Instrument: msd5.1  
 Operator: kr  
 Column diameter: 0.53

/var/chem/msd5.1/5-24apr.lb/5042422.d



Report Date: 25-Apr-2008 09:56

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042413.d  
 Lab Smp Id: ICAL Client Smp ID: Level 1  
 Inj Date : 24-APR-2008 13:56  
 Operator : ct Inst ID: msd5.i  
 Smp Info : 0.3mL #1612-1  
 Misc Info : 200ppbv -> 0.3ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:56 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 13:56 Cal File: 5042413.d  
 Als bottle: 1 Calibration Sample, Level: 1  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AFCEElow.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5								
8.087	8.087	(1.000)	130	347911	25.0000		70.00- 130.00	100.00
8.087	8.087	(1.000)	128	272556			47.51- 107.51	78.34
8.059	8.059	(1.000)	49	681188			158.47- 218.47	195.79
-----								
* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.939	9.939	(1.000)	114	1408281	25.0000		70.00- 130.00	100.00
9.939	9.939	(1.000)	88	206198			0.00- 44.75	14.64
-----								
* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	1340111	25.0000		70.00- 130.00	100.00
14.999	14.999	(1.000)	82	682751			0.00- 30.00	50.95
-----								
\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.137	9.137	(1.130)	65	428192	25.0000	24.248	70.00- 130.00	100.00
9.137	9.137	(1.130)	67	231082			0.00- 30.00	53.97
-----								
\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.704	12.704	(1.278)	98	1331352	25.0000	24.877	70.00- 130.00	100.00
12.704	12.704	(1.278)	70	124186			0.00- 30.00	9.33



AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.278)	100	895544			0.00- 30.00	67.27		
-----										
\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	778281	25.0000	23.918	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	1052808			98.07- 158.07	135.27		
16.575	16.575	(1.105)	176	738882			65.46- 125.46	94.94		
-----										
12 1,3-Butadiene										
						CAS #: 106-99-0				
2.806	2.806	(0.347)	54	11204	0.30000	0.4294	70.00- 130.00	100.00		
2.806	2.806	(0.347)	39	14982			0.00- 30.00	133.72		
-----										
72 Chloroform										
						CAS #: 67-66-3				
8.197	8.197	(1.014)	83	15851	0.30000	0.3951	70.00- 130.00	100.00		
8.225	8.225	(1.017)	85	12242			35.57- 95.57	77.23		
-----										
81 Benzene										
						CAS #: 71-43-2				
9.110	9.110	(0.917)	78	30080	0.30000	0.4258	70.00- 130.00	100.00		
9.110	9.110	(0.917)	77	6703			0.00- 30.00	22.28		
-----										
133 Styrene										
						CAS #: 100-42-5				
15.911	15.911	(1.061)	104	20342	0.30000	0.3622	70.00- 130.00	100.00		
15.911	15.911	(1.061)	78	7793			13.62- 73.62	38.31		
-----										
136 Cumene										
						CAS #: 98-82-8				
16.326	16.326	(1.088)	105	40463	0.30000	0.3868	70.00- 130.00	100.00		
16.326	16.326	(1.088)	120	9413			0.00- 30.00	23.26		
16.326	16.326	(1.088)	51	4243			0.00- 30.00	10.49		
-----										
122 1,2-Dibromoethane										
						CAS #: 106-93-4				
14.363	14.363	(0.958)	107	15219	0.30000	0.3994	70.00- 130.00	100.00		
14.363	14.363	(0.958)	109	12601			65.00- 125.00	82.80		
-----										
147 1,3,5-Trimethylbenzene										
						CAS #: 108-67-8				
17.045	17.045	(1.136)	105	34064	0.30000	0.3631	70.00- 130.00	100.00		
17.045	17.045	(1.136)	120	16125			0.00- 30.00	47.34		
-----										
152 1,2,4-Trimethylbenzene										
						CAS #: 95-63-6				
17.460	17.460	(1.164)	105	25890	0.30000	0.3289	70.00- 130.00	100.00		
17.460	17.460	(1.164)	120	14157			17.48- 77.48	54.68		
-----										

Report Date: 25-Apr-2008 09:56

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042413.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 0.3ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	347911	17.26
92 1,4-Difluorobenze	1234462	740677	1728247	1408281	14.08
125 Chlorobenzene-d5	1186736	712042	1661430	1340111	12.92

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.09	0.34
92 1,4-Difluorobenze	9.91	9.58	10.24	9.94	0.28
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /var/chem/msd5.i/5-24apr.b/5042413.d

Date: 24-APR-2008 13:56

Client ID: Level 1

Sample Info: 0.3mL #1612-1


Column phase: RTX-624

Instrument: msd5.i

Operator: ct

Column diameter: 0.53

/var/chem/msd5.i/5-24apr.b/5042413.d



Report Date: 25-Apr-2008 09:56

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042414.d  
 Lab Smp Id: ICAL Client Smp ID: Level 2  
 Inj Date : 24-APR-2008 14:23  
 Operator : ct Inst ID: msd5.i  
 Smp Info : 0.5mL #1612-1  
 Misc Info : 200ppbv -> 0.5ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:56 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 14:23 Cal File: 5042414.d  
 Als bottle: 1 Calibration Sample, Level: 2  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08Low.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable

Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	RESPONSE ( PPBV)	( PPBV)	=====	=====	=====
-----								
* 71	Bromochloromethane			CAS #: 74-97-5				
8.059	8.059	(1.000)	130	277835	25.0000	70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	217706		47.51- 107.51	78.36	
8.059	8.059	(1.000)	49	561450		158.47- 218.47	202.08	
-----								
* 92	1,4-Difluorobenzene			CAS #: 540-36-3				
9.912	9.912	(1.000)	114	1146928	25.0000	70.00- 130.00	100.00	
9.912	9.912	(1.000)	88	181619		0.00- 44.75	15.84	
-----								
* 125	Chlorobenzene-d5			CAS #: 3114-55-4				
14.999	14.999	(1.000)	117	1152362	25.0000	70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	582440		0.00- 30.00	50.54	
-----								
\$ 84	1,2-Dichloroethane-d4			CAS #: 17060-07-0				
9.137	9.137	(1.134)	65	359092	25.0000	25.463 70.00- 130.00	100.00	
9.137	9.137	(1.134)	67	192215		0.00- 30.00	53.53	
-----								
\$ 107	Toluene-d8			CAS #: 2037-26-5				
12.704	12.704	(1.282)	98	1106484	25.0000	25.387 70.00- 130.00	100.00	
12.704	12.704	(1.282)	70	101230		0.00- 30.00	9.15	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	717757			0.00- 30.00	64.87		
-----										
\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	687794	25.0000	24.581	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	909715			98.07- 158.07	132.27		
16.575	16.575	(1.105)	176	646289			65.46- 125.46	93.97		
-----										
8 Dichlorodifluoromethane/Fr12						CAS #: 75-71-8				
2.336	2.336	(0.290)	85	14735	0.50000	0.4268	70.00- 130.00	100.00(a)		
2.308	2.308	(0.286)	87	5312			0.00- 30.00	36.05		
-----										
9 Freon 114						CAS #: 76-14-2				
2.474	2.474	(0.307)	135	11296	0.50000	0.4016	70.00- 130.00	100.00(a)		
2.474	2.474	(0.307)	137	4390			2.03- 62.03	38.86		
-----										
13 Vinyl Chloride						CAS #: 75-01-4				
2.750	2.750	(0.341)	62	8509	0.50000	0.4039	70.00- 130.00	100.00(a)		
2.806	2.806	(0.348)	64	2266			0.00- 30.00	26.63		
-----										
12 1,3-Butadiene						CAS #: 106-99-0				
2.750	2.750	(0.341)	54	6942	0.50000	0.3332	70.00- 130.00	100.00(a)		
2.750	2.750	(0.341)	39	12011			0.00- 30.00	173.02		
-----										
15 Bromomethane						CAS #: 74-83-9				
3.276	3.276	(0.406)	94	4881	0.50000	0.4145	70.00- 130.00	100.00(a)		
3.276	3.276	(0.406)	96	4193			62.86- 122.86	85.90		
-----										
19 Chloroethane						CAS #: 75-00-3				
3.442	3.442	(0.427)	64	4499	0.50000	0.4300	70.00- 130.00	100.00(a)		
3.386	3.386	(0.420)	49	1073			0.00- 30.00	23.85		
3.442	3.442	(0.427)	66	1478			0.00- 30.00	32.85		
-----										
20 Trichlorofluoromethane/Fr11						CAS #: 75-69-4				
3.746	3.746	(0.465)	101	13071	0.50000	0.3712	70.00- 130.00	100.00(a)		
3.746	3.746	(0.465)	103	9023			33.46- 93.46	69.03		
-----										
30 Freon 113						CAS #: 76-13-1				
4.548	4.548	(0.564)	151	8877	0.50000	0.4092	70.00- 130.00	100.00(a)		
4.520	4.520	(0.561)	153	6357			33.20- 93.20	71.61		
4.520	4.520	(0.561)	101	13515			106.78- 166.78	152.25		
-----										
31 1,1-Dichloroethene						CAS #: 75-35-4				
4.575	4.575	(0.568)	61	10521	0.50000	0.3776	70.00- 130.00	100.00(a)		
4.575	4.575	(0.568)	96	7168			23.41- 83.41	68.13		
4.575	4.575	(0.568)	98	4260			4.01- 64.01	40.49		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
35	Carbon Disulfide					CAS #: 75-15-0			
4.935	4.935	(0.612)	76	19473	0.50000	0.4050	70.00- 130.00	100.00(a)	
-----									
43	Methylene Chloride					CAS #: 75-09-2			
5.460	5.460	(0.678)	49	12065	0.50000	0.4771	70.00- 130.00	100.00(a)	
5.460	5.460	(0.678)	84	6592			26.74- 86.74	54.64	
5.460	5.460	(0.678)	51	3946			0.00- 30.00	32.71	
-----									
46	MTBE					CAS #: 1634-04-4			
5.792	5.792	(0.719)	73	8350	0.50000	0.3454	70.00- 130.00	100.00(a)	
5.764	5.764	(0.715)	57	2440			0.00- 59.41	29.22	
5.764	5.764	(0.715)	41	6408			0.00- 30.00	76.74	
-----									
47	trans-1,2-Dichloroethene					CAS #: 156-60-5			
5.847	5.847	(0.726)	96	6861	0.50000	0.3780	70.00- 130.00	100.00(a)	
5.819	5.819	(0.722)	61	11342			130.65- 190.65	165.31	
5.819	5.819	(0.722)	98	4845			0.00- 30.00	70.62	
-----									
51	Hexane					CAS #: 110-54-3			
6.151	6.151	(0.763)	57	11850	0.50000	0.3319	70.00- 130.00	100.00(a)	
6.179	6.179	(0.767)	43	12060			0.00- 30.00	101.77	
6.151	6.151	(0.763)	86	1332			0.00- 30.00	11.24	
-----									
55	1,1-Dichloroethane					CAS #: 75-34-3			
6.621	6.621	(0.822)	63	14158	0.50000	0.4228	70.00- 130.00	100.00(a)	
6.621	6.621	(0.822)	65	5303			0.00- 59.62	37.46	
-----									
67	2-Butanone					CAS #: 78-93-3			
7.727	7.727	(0.959)	72	2174	0.50000	0.2662	70.00- 130.00	100.00(Ta)	
7.727	7.727	(0.959)	43	13273			533.62- 593.62	610.53	
0.000	1.000	(0.000)	57	0			0.00- 30.00	0.00	
-----									
66	cis-1,2-Dichloroethene					CAS #: 156-59-2			
7.617	7.617	(0.945)	61	8727	0.50000	0.3611	70.00- 130.00	100.00(a)	
7.644	7.644	(0.949)	96	8736			42.00- 102.00	100.10	
7.617	7.617	(0.945)	98	4499			15.56- 75.56	51.55	
-----									
70	Tetrahydrofuran					CAS #: 109-99-9			
8.059	8.059	(1.000)	42	17350	0.50000	0.5576	70.00- 130.00	100.00	
8.059	8.059	(1.000)	71	3685			0.00- 56.55	21.24	
8.059	8.059	(1.000)	72	5090			0.00- 30.00	29.34	
-----									
72	Chloroform					CAS #: 67-66-3			
8.197	8.197	(1.017)	83	13528	0.50000	0.4222	70.00- 130.00	100.00(a)	
8.197	8.197	(1.017)	85	8999			35.57- 95.57	66.52	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
75	1,1,1-Trichloroethane					CAS #:	71-55-6			
8.446	8.446	(1.048)	97	14401	0.50000	0.4840	70.00-	130.00	100.00(a)	
8.446	8.446	(1.048)	99	8817			34.21-	94.21	61.22	
-----										
74	Cyclohexane					CAS #:	110-82-7			
8.419	8.419	(1.045)	84	8902	0.50000	0.3769	70.00-	130.00	100.00(a)	
8.419	8.419	(1.045)	56	13184			117.94-	177.94	148.10	
8.391	8.391	(1.041)	41	12303			54.92-	114.92	138.20	
-----										
77	Carbon Tetrachloride					CAS #:	56-23-5			
8.667	8.667	(1.075)	119	11538	0.50000	0.4332	70.00-	130.00	100.00(a)	
8.667	8.667	(1.075)	117	10755			74.41-	134.41	93.21	
-----										
80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.082	9.082	(1.127)	57	40278	0.50000	0.3910	70.00-	130.00	100.00(a)	
9.082	9.082	(1.127)	56	14695			0.00-	30.00	36.48	
9.082	9.082	(1.127)	41	10179			0.00-	30.00	25.27	
-----										
81	Benzene					CAS #:	71-43-2			
9.110	9.110	(0.919)	78	21434	0.50000	0.3726	70.00-	130.00	100.00(a)	
9.082	9.082	(0.916)	77	4787			0.00-	30.00	22.33	
-----										
85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	8494	0.50000	0.4103	70.00-	130.00	100.00(a)	
9.276	9.276	(0.936)	64	3903			0.00-	30.00	45.95	
-----										
90	Heptane					CAS #:	142-82-5			
9.497	9.497	(0.958)	100	2357	0.50000	0.3749	70.00-	130.00	100.00(a)	
9.497	9.497	(0.958)	43	18119			0.00-	30.00	768.73	
9.497	9.497	(0.958)	71	6780			0.00-	30.00	287.65	
-----										
93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	9680	0.50000	0.4538	70.00-	130.00	100.00(a)	
10.354	10.354	(1.045)	130	11025			70.08-	130.08	113.89	
10.326	10.326	(1.042)	97	6050			35.30-	95.30	62.50	
-----										
98	1,2-Dichloropropane					CAS #:	78-87-5			
10.852	10.852	(1.095)	63	7639	0.50000	0.4017	70.00-	130.00	100.00(a)	
10.852	10.852	(1.095)	62	5930			41.10-	101.10	77.63	
10.852	10.852	(1.095)	41	8538			36.18-	96.18	111.77	
-----										
100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	10115	0.50000	0.3633	70.00-	130.00	100.00(a)	
11.405	11.405	(1.151)	85	6880			34.05-	94.05	68.02	
-----										
103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	8191	0.50000	0.3760	70.00-	130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
103 cis-1,3-Dichloropropene (continued)									
12.289	12.289	(1.240)	77	3322			1.82- 61.82	40.56	
12.289	12.289	(1.240)	39	8231			36.40- 96.40	100.49	
-----									
106 4-Methyl-2-pentanone CAS #: 108-10-1									
12.621	12.621	(1.273)	58	5061	0.50000	0.3316	70.00- 130.00	100.00(a)	
12.621	12.621	(1.273)	43	14619			0.00- 30.00	288.86	
12.621	12.621	(1.273)	85	1358			0.00- 30.00	26.83	
-----									
108 Toluene CAS #: 108-88-3									
12.815	12.815	(1.293)	91	21927	0.50000	0.3919	70.00- 130.00	100.00(a)	
12.815	12.815	(1.293)	92	12865			27.75- 87.75	58.67	
-----									
113 trans-1,3-Dichloropropene CAS #: 10061-02-6									
13.368	13.368	(0.891)	75	8260	0.50000	0.3721	70.00- 130.00	100.00(a)	
13.368	13.368	(0.891)	77	2948			2.38- 62.38	35.69	
13.368	13.368	(0.891)	39	6149			35.96- 95.96	74.44	
-----									
114 1,1,2-Trichloroethane CAS #: 79-00-5									
13.644	13.644	(0.910)	97	8022	0.50000	0.4094	70.00- 130.00	100.00(a)	
13.644	13.644	(0.910)	99	5555			33.83- 93.83	69.25	
13.644	13.644	(0.910)	83	6649			52.70- 112.70	82.88	
-----									
116 Tetrachloroethene CAS #: 127-18-4									
13.700	13.700	(0.913)	166	9112	0.50000	0.3581	70.00- 130.00	100.00(a)	
13.700	13.700	(0.913)	129	8860			44.73- 104.73	97.23	
13.700	13.700	(0.913)	131	7599			40.60- 100.60	83.40	
-----									
120 Dibromochloromethane CAS #: 124-48-1									
14.197	14.197	(0.947)	129	10259	0.50000	0.3545	70.00- 130.00	100.00(a)	
14.197	14.197	(0.947)	127	8062			0.00- 30.00	78.58	
-----									
122 1,2-Dibromoethane CAS #: 106-93-4									
14.363	14.363	(0.958)	107	11007	0.50000	0.3360	70.00- 130.00	100.00(a)	
14.363	14.363	(0.958)	109	12260			65.00- 125.00	111.38	
-----									
126 Chlorobenzene CAS #: 108-90-7									
15.027	15.027	(1.002)	112	18068	0.50000	0.3874	70.00- 130.00	100.00(a)	
15.027	15.027	(1.002)	114	6582			2.42- 62.42	36.43	
14.999	14.999	(1.000)	77	19212			27.34- 87.34	106.33	
-----									
128 Ethyl Benzene CAS #: 100-41-4									
15.165	15.165	(1.011)	106	9147	0.50000	0.3546	70.00- 130.00	100.00(a)	
15.165	15.165	(1.011)	91	27710			0.00- 30.00	302.94	
-----									
130 m,p-Xylene CAS #: 108-38-3									
15.331	15.331	(1.022)	106	10853	0.50000	0.3384	70.00- 130.00	100.00(a)	



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
130 m,p-Xylene (continued)									
15.331	15.331	(1.022)	91	23146			0.00- 30.00	213.27	
-----									
132 o-Xylene CAS #: 95-47-6									
15.856	15.856	(1.057)	106	11097	0.50000	0.3701	70.00- 130.00	100.00(a)	
15.856	15.856	(1.057)	91	23614			170.15- 230.15	212.80	
-----									
133 Styrene CAS #: 100-42-5									
15.912	15.912	(1.061)	104	15639	0.50000	0.3238	70.00- 130.00	100.00(a)	
15.912	15.912	(1.061)	78	7243			13.62- 73.62	46.31	
-----									
134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	10897	0.50000	0.3927	70.00- 130.00	100.00(a)	
16.160	16.160	(1.077)	171	4351			22.36- 82.36	39.93	
-----									
141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	18353	0.50000	0.4155	70.00- 130.00	100.00(a)	
16.796	16.796	(1.120)	85	10987			36.19- 96.19	59.86	
-----									
144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	32076	0.50000	0.3538	70.00- 130.00	100.00(a)	
16.962	16.962	(1.131)	120	10605			0.17- 60.17	33.06	
-----									
147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	29239	0.50000	0.3624	70.00- 130.00	100.00(a)	
17.045	17.045	(1.136)	120	13512			0.00- 30.00	46.21	
-----									
152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	22603	0.50000	0.3339	70.00- 130.00	100.00(a)	
17.460	17.460	(1.164)	120	11788			17.48- 77.48	52.15	
-----									
155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	19372	0.50000	0.4121	70.00- 130.00	100.00(a)	
17.764	17.764	(1.184)	148	11946			0.00- 30.00	61.67	
17.764	17.764	(1.184)	111	7757			0.00- 30.00	40.04	
-----									
156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	23101	0.50000	0.3902	70.00- 130.00	100.00(a)	
17.847	17.847	(1.190)	148	16561			0.00- 30.00	71.69	
17.847	17.847	(1.190)	111	8938			0.00- 30.00	38.69	
-----									
157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	18714	0.50000	0.2810	70.00- 130.00	100.00(a)	
17.985	17.985	(1.199)	126	4078			0.00- 30.00	21.79	
-----									
159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	19514	0.50000	0.4047	70.00- 130.00	100.00(a)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
159 1,2-Dichlorobenzene (continued)									
18.206	18.206	(1.214)	148	13947			32.26- 92.26	71.47	
18.206	18.206	(1.214)	111	8507			7.92- 67.92	43.59	
-----									
142 Propylbenzene CAS #: 103-65-1									
16.824	16.824	(1.122)	91	39747	0.50000	0.3972	70.00- 130.00	100.00(a)	
16.824	16.824	(1.122)	120	8834			0.00- 30.00	22.23	
16.824	16.824	(1.122)	105	1916			0.00- 30.00	4.82	
-----									
136 Cumene CAS #: 98-82-8									
16.326	16.326	(1.088)	105	32526	0.50000	0.3616	70.00- 130.00	100.00(a)	
16.326	16.326	(1.088)	120	8088			0.00- 30.00	24.87	
16.326	16.326	(1.088)	51	4145			0.00- 30.00	12.74	
-----									
94 Methyl Cyclohexane CAS #: 108-87-2									
10.548	10.548	(1.064)	83	13193	0.50000	0.4195	70.00- 130.00	100.00(a)	
10.575	10.575	(1.067)	98	7591			0.00- 30.00	57.54	
10.548	10.548	(1.064)	55	15298			0.00- 30.00	115.96	
-----									

QC Flag Legend

- T - Target compound detected outside RT window.
- a - Target compound detected but, quantitated amount Below Limit Of Quantitation(BLOQ).

Report Date: 25-Apr-2008 09:56

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042414.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 0.5ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	277835	-6.36
92 1,4-Difluorobenze	1234462	740677	1728247	1146928	-7.09
125 Chlorobenzene-d5	1186736	712042	1661430	1152362	-2.90

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /var/chem/msd5.1/5-24apr.lb/5042414.d

Date: 24-APR-2008 14:23

Client ID: Level 2

Sample Info: 0.5mL #1612-1


Column phase: RTX-624

Instrument: msd5.1

Operator: ct

Column diameter: 0.53

/var/chem/msd5.1/5-24apr.lb/5042414.d



Report Date: 25-Apr-2008 09:58

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042421.d  
 Lab Smp Id: ICAL Client Smp ID: Level 3  
 Inj Date : 24-APR-2008 18:31  
 Operator : kr Inst ID: msd5.i  
 Smp Info : 2.0mL #1612-1  
 Misc Info : 200ppbv -> 2.0ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:57 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 18:31 Cal File: 5042421.d  
 Als bottle: 1 Calibration Sample, Level: 3  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	
* 71 Bromochloromethane CAS #: 74-97-5								
8.059	8.059	(1.000)	130	316701	25.0000	70.00- 130.00	100.00	
8.059	8.059	(1.000)	128	241810		47.51- 107.51	76.35	
8.059	8.059	(1.000)	49	585510		158.47- 218.47	184.88	
-----								
* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.912	9.912	(1.000)	114	1264461	25.0000	70.00- 130.00	100.00	
9.912	9.912	(1.000)	88	187922		0.00- 44.75	14.86	
-----								
* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	1173690	25.0000	70.00- 130.00	100.00	
14.999	14.999	(1.000)	82	576977		0.00- 30.00	49.16	
-----								
\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.137	9.137	(1.134)	65	359025	25.0000	22.334 70.00- 130.00	100.00	
9.137	9.137	(1.134)	67	206220		0.00- 30.00	57.44	
-----								
\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.704	12.704	(1.282)	98	1154854	25.0000	24.034 70.00- 130.00	100.00	
12.704	12.704	(1.282)	70	100616		0.00- 30.00	8.71	

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	760885			0.00- 30.00	65.89		
-----										
\$ 138 Bromofluorobenzene										
						CAS #: 460-00-4				
16.575	16.575	(1.105)	174	695467	25.0000	24.403	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	911131			98.07- 158.07	131.01		
16.575	16.575	(1.105)	176	672459			65.46- 125.46	96.69		
-----										
6 Propylene						CAS #: 115-07-1				
2.280	2.280	(0.283)	41	39296	2.00000	1.599	70.00- 130.00	100.00(a)		
2.253	2.253	(0.280)	42	32979			0.00- 30.00	83.92		
2.280	2.280	(0.283)	39	29125			0.00- 30.00	74.12		
-----										
8 Dichlorodifluoromethane/Fr12						CAS #: 75-71-8				
2.336	2.336	(0.290)	85	67545	2.00000	1.716	70.00- 130.00	100.00		
2.336	2.336	(0.290)	87	21517			0.00- 30.00	31.86		
-----										
9 Freon 114						CAS #: 76-14-2				
2.474	2.474	(0.307)	135	52666	2.00000	1.643	70.00- 130.00	100.00		
2.474	2.474	(0.307)	137	16221			2.03- 62.03	30.80		
-----										
10 Chloromethane						CAS #: 74-87-3				
2.612	2.612	(0.324)	50	50579	2.00000	1.710	70.00- 130.00	100.00(a)		
2.584	2.584	(0.321)	52	16560			0.00- 30.00	32.74		
-----										
13 Vinyl Chloride						CAS #: 75-01-4				
2.778	2.778	(0.345)	62	36964	2.00000	1.539	70.00- 130.00	100.00		
2.750	2.750	(0.341)	64	13783			0.00- 30.00	37.29		
-----										
12 1,3-Butadiene						CAS #: 106-99-0				
2.778	2.778	(0.345)	54	36120	2.00000	1.521	70.00- 130.00	100.00		
2.778	2.778	(0.345)	39	44008			0.00- 30.00	121.84		
-----										
15 Bromomethane						CAS #: 74-83-9				
3.276	3.276	(0.406)	94	19166	2.00000	1.428	70.00- 130.00	100.00		
3.276	3.276	(0.406)	96	21026			62.86- 122.86	109.70		
-----										
19 Chloroethane						CAS #: 75-00-3				
3.442	3.442	(0.427)	64	17790	2.00000	1.492	70.00- 130.00	100.00		
3.469	3.469	(0.430)	49	6005			0.00- 30.00	33.75		
3.442	3.442	(0.427)	66	4509			0.00- 30.00	25.35		
-----										
20 Trichlorofluoromethane/Fr11						CAS #: 75-69-4				
3.746	3.746	(0.465)	101	66917	2.00000	1.667	70.00- 130.00	100.00		
3.746	3.746	(0.465)	103	43085			33.46- 93.46	64.39		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPBV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.105	4.105	(0.509)	45	13439	2.00000	1.417	70.00- 130.00	100.00(a)	
4.160	4.160	(0.516)	43	6438			0.00- 30.00	47.91	
4.133	4.133	(0.513)	46	7798			0.00- 30.00	58.03	
-----									
30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	41947	2.00000	1.696	70.00- 130.00	100.00	
4.520	4.520	(0.561)	153	27443			33.20- 93.20	65.42	
4.520	4.520	(0.561)	101	52727			106.78- 166.78	125.70	
-----									
31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	49517	2.00000	1.559	70.00- 130.00	100.00	
4.575	4.575	(0.568)	96	28440			23.41- 83.41	57.43	
4.603	4.603	(0.571)	98	18088			4.01- 64.01	36.53	
-----									
32 Acetone						CAS #: 67-64-1			
4.741	4.741	(0.588)	58	20063	2.00000	1.649	70.00- 130.00	100.00(a)	
4.741	4.741	(0.588)	43	52742			0.00- 30.00	262.88	
-----									
36 2-Propanol						CAS #: 67-63-0			
4.935	4.935	(0.612)	45	62149	2.00000	1.352	70.00- 130.00	100.00(a)	
4.962	4.962	(0.616)	43	21178			0.00- 30.00	34.08	
4.962	4.962	(0.616)	59	2534			0.00- 30.00	4.08	
-----									
35 Carbon Disulfide						CAS #: 75-15-0			
4.935	4.935	(0.612)	76	85989	2.00000	1.569	70.00- 130.00	100.00	
-----									
38 3-Chloropropene						CAS #: 107-05-1			
5.211	5.211	(0.647)	76	10331	2.00000	1.096	70.00- 130.00	100.00(a)	
5.183	5.183	(0.643)	41	49775			0.00- 30.00	481.80	
-----									
43 Methylene Chloride						CAS #: 75-09-2			
5.460	5.460	(0.677)	49	44857	2.00000	1.556	70.00- 130.00	100.00	
5.460	5.460	(0.677)	84	23987			26.74- 86.74	53.47	
5.460	5.460	(0.677)	51	16130			0.00- 30.00	35.96	
-----									
46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	29004	2.00000	1.052	70.00- 130.00	100.00	
5.792	5.792	(0.719)	57	10028			0.00- 59.41	34.57	
5.764	5.764	(0.715)	41	8664			0.00- 30.00	29.87	
-----									
47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	34007	2.00000	1.644	70.00- 130.00	100.00	
5.819	5.819	(0.722)	61	49974			130.65- 190.65	146.95	
5.819	5.819	(0.722)	98	21792			0.00- 30.00	64.08	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #:	110-54-3		
6.179	6.179	(0.767)	57	61884	2.00000	1.521	70.00- 130.00	100.00	
6.179	6.179	(0.767)	43	51813			0.00- 30.00	83.73	
6.179	6.179	(0.767)	86	10440			0.00- 30.00	16.87	
-----									
55 1,1-Dichloroethane						CAS #:	75-34-3		
6.594	6.594	(0.818)	63	58378	2.00000	1.530	70.00- 130.00	100.00	
6.594	6.594	(0.818)	65	18441			0.00- 59.62	31.59	
-----									
67 2-Butanone						CAS #:	78-93-3		
7.700	7.700	(0.955)	72	14308	2.00000	1.537	70.00- 130.00	100.00	
7.700	7.700	(0.955)	43	69454			533.62- 593.62	485.42	
7.700	7.700	(0.955)	57	4538			0.00- 30.00	31.72	
-----									
66 cis-1,2-Dichloroethene						CAS #:	156-59-2		
7.644	7.644	(0.949)	61	44658	2.00000	1.621	70.00- 130.00	100.00	
7.644	7.644	(0.949)	96	29532			42.00- 102.00	66.13	
7.644	7.644	(0.949)	98	21238			15.56- 75.56	47.56	
-----									
70 Tetrahydrofuran						CAS #:	109-99-9		
8.059	8.059	(1.000)	42	51913	2.00000	1.464	70.00- 130.00	100.00	
8.059	8.059	(1.000)	71	15340			0.00- 56.55	29.55	
8.059	8.059	(1.000)	72	19201			0.00- 30.00	36.99	
-----									
72 Chloroform						CAS #:	67-66-3		
8.197	8.197	(1.017)	83	50543	2.00000	1.384	70.00- 130.00	100.00	
8.197	8.197	(1.017)	85	33956			35.57- 95.57	67.18	
-----									
75 1,1,1-Trichloroethane						CAS #:	71-55-6		
8.446	8.446	(1.048)	97	48233	2.00000	1.422	70.00- 130.00	100.00	
8.446	8.446	(1.048)	99	30235			34.21- 94.21	62.69	
-----									
74 Cyclohexane						CAS #:	110-82-7		
8.418	8.418	(1.045)	84	37550	2.00000	1.395	70.00- 130.00	100.00	
8.418	8.418	(1.045)	56	60462			117.94- 177.94	161.02	
8.418	8.418	(1.045)	41	38853			54.92- 114.92	103.47	
-----									
56 Vinyl Acetate						CAS #:	108-05-4		
6.704	6.704	(0.832)	86	5481	2.00000	1.039	70.00- 130.00	100.00(a)	
6.677	6.677	(0.828)	43	81210			0.00- 30.00	1481.66	
6.704	6.704	(0.832)	42	6947			0.00- 30.00	126.75	
-----									
77 Carbon Tetrachloride						CAS #:	56-23-5		
8.667	8.667	(1.075)	119	41335	2.00000	1.362	70.00- 130.00	100.00	
8.695	8.695	(1.079)	117	44195			74.41- 134.41	106.92	
-----									



AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.082	9.082	(1.127)	57	166198	2.00000	1.415	70.00-	130.00	100.00	
9.082	9.082	(1.127)	56	54553			0.00-	30.00	32.82	
9.082	9.082	(1.127)	41	44648			0.00-	30.00	26.86	
-----										
81	Benzene					CAS #:	71-43-2			
9.082	9.082	(0.916)	78	90369	2.00000	1.425	70.00-	130.00	100.00	
9.082	9.082	(0.916)	77	24694			0.00-	30.00	27.33	
-----										
85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	36236	2.00000	1.588	70.00-	130.00	100.00	
9.276	9.276	(0.936)	64	12544			0.00-	30.00	34.62	
-----										
90	Heptane					CAS #:	142-82-5			
9.497	9.497	(0.958)	100	11233	2.00000	1.620	70.00-	130.00	100.00	
9.497	9.497	(0.958)	43	75190			0.00-	30.00	669.37	
9.497	9.497	(0.958)	71	33986			0.00-	30.00	302.55	
-----										
93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	36554	2.00000	1.554	70.00-	130.00	100.00	
10.326	10.326	(1.042)	130	35474			70.08-	130.08	97.05	
10.326	10.326	(1.042)	97	22227			35.30-	95.30	60.81	
-----										
98	1,2-Dichloropropane					CAS #:	78-87-5			
10.852	10.852	(1.095)	63	31198	2.00000	1.488	70.00-	130.00	100.00	
10.852	10.852	(1.095)	62	23924			41.10-	101.10	76.68	
10.852	10.852	(1.095)	41	28196			35.89-	95.89	90.38	
-----										
99	1,4-Dioxane					CAS #:	123-91-1			
11.073	11.073	(1.117)	88	19966	2.00000	1.436	70.00-	130.00	100.00(a)	
11.073	11.073	(1.117)	58	16158			47.45-	107.45	80.93	
11.073	11.073	(1.117)	57	5847			0.00-	30.00	29.28	
-----										
100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	44361	2.00000	1.445	70.00-	130.00	100.00	
11.405	11.405	(1.151)	85	28053			34.05-	94.05	63.24	
-----										
103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	33939	2.00000	1.413	70.00-	130.00	100.00	
12.317	12.317	(1.243)	77	12853			1.82-	61.82	37.87	
12.317	12.317	(1.243)	39	25221			36.40-	96.40	74.31	
-----										
106	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.621	12.621	(1.273)	58	22364	2.00000	1.329	70.00-	130.00	100.00	
12.621	12.621	(1.273)	43	80802			0.00-	30.00	361.30	
12.621	12.621	(1.273)	85	9589			0.00-	30.00	42.88	
-----										

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
108 Toluene						CAS #:	108-88-3			
12.815	12.815	(1.293)	91	99179	2.00000	1.608	70.00-	130.00	100.00	
12.815	12.815	(1.293)	92	55204			27.75-	87.75	55.66	
-----										
113 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.368	13.368	(0.891)	75	31301	2.00000	1.384	70.00-	130.00	100.00	
13.368	13.368	(0.891)	77	10410			2.38-	62.38	33.26	
13.368	13.368	(0.891)	39	23737			35.96-	95.96	75.83	
-----										
114 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.644	13.644	(0.910)	97	28297	2.00000	1.418	70.00-	130.00	100.00	
13.644	13.644	(0.910)	99	21084			33.83-	93.83	74.51	
13.644	13.644	(0.910)	83	29005			52.70-	112.70	102.50	
-----										
116 Tetrachloroethene						CAS #:	127-18-4			
13.699	13.699	(0.913)	166	43912	2.00000	1.694	70.00-	130.00	100.00	
13.699	13.699	(0.913)	129	32984			44.73-	104.73	75.11	
13.699	13.699	(0.913)	131	31741			40.60-	100.60	72.28	
-----										
119 2-Hexanone						CAS #:	591-78-6			
14.031	14.031	(0.935)	58	32083	2.00000	1.342	70.00-	130.00	100.00(a)	
14.031	14.031	(0.935)	43	68432			181.71-	241.71	213.30	
14.031	14.031	(0.935)	100	5813			0.00-	30.00	18.12	
-----										
120 Dibromochloromethane						CAS #:	124-48-1			
14.197	14.197	(0.947)	129	43643	2.00000	1.481	70.00-	130.00	100.00	
14.197	14.197	(0.947)	127	34730			0.00-	30.00	79.58	
-----										
122 1,2-Dibromoethane						CAS #:	106-93-4			
14.363	14.363	(0.958)	107	48320	2.00000	1.448	70.00-	130.00	100.00	
14.363	14.363	(0.958)	109	45975			65.00-	125.00	95.15	
-----										
126 Chlorobenzene						CAS #:	108-90-7			
15.054	15.054	(1.004)	112	76213	2.00000	1.604	70.00-	130.00	100.00	
15.054	15.054	(1.004)	114	27179			2.42-	62.42	35.66	
15.027	15.027	(1.002)	77	52925			27.34-	87.34	69.44	
-----										
128 Ethyl Benzene						CAS #:	100-41-4			
15.165	15.165	(1.011)	106	41019	2.00000	1.561	70.00-	130.00	100.00	
15.165	15.165	(1.011)	91	123814			0.00-	30.00	301.85	
-----										
130 m,p-Xylene						CAS #:	108-38-3			
15.331	15.331	(1.022)	106	50927	2.00000	1.559	70.00-	130.00	100.00	
15.331	15.331	(1.022)	91	93398			0.00-	30.00	183.40	
-----										
132 o-Xylene						CAS #:	95-47-6			
15.856	15.856	(1.057)	106	45202	2.00000	1.480	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	88326			170.15- 230.15	195.40	
-----									
133 Styrene									
15.911	15.911	(1.061)	104	65990	2.00000	1.341	70.00- 130.00	100.00	
15.911	15.911	(1.061)	78	28916			13.62- 73.62	43.82	
-----									
134 Bromoform									
16.160	16.160	(1.077)	173	35972	2.00000	1.273	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	19320			22.36- 82.36	53.71	
-----									
141 1,1,2,2-Tetrachloroethane									
16.796	16.796	(1.120)	83	75038	2.00000	1.668	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	46417			36.19- 96.19	61.86	
-----									
144 4-Ethyltoluene									
16.962	16.962	(1.131)	105	144641	2.00000	1.566	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	46697			0.17- 60.17	32.28	
-----									
147 1,3,5-Trimethylbenzene									
17.045	17.045	(1.136)	105	126322	2.00000	1.537	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	62212			0.00- 30.00	49.25	
-----									
152 1,2,4-Trimethylbenzene									
17.460	17.460	(1.164)	105	103045	2.00000	1.494	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	53182			17.48- 77.48	51.61	
-----									
155 1,3-Dichlorobenzene									
17.764	17.764	(1.184)	146	81828	2.00000	1.709	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	58561			0.00- 30.00	71.57	
17.764	17.764	(1.184)	111	35547			0.00- 30.00	43.44	
-----									
156 1,4-Dichlorobenzene									
17.847	17.847	(1.190)	146	102298	2.00000	1.697	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	63549			0.00- 30.00	62.12	
17.847	17.847	(1.190)	111	41468			0.00- 30.00	40.54	
-----									
157 alpha-Chlorotoluene									
17.985	17.985	(1.199)	91	98612	2.00000	1.454	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	19904			0.00- 30.00	20.18	
-----									
159 1,2-Dichlorobenzene									
18.206	18.206	(1.214)	146	95994	2.00000	1.955	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	60744			32.26- 92.26	63.28	
18.206	18.206	(1.214)	111	33700			7.92- 67.92	35.11	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
163	1,2,4-Trichlorobenzene					CAS #:	120-82-1		
19.506	19.506	(1.300)	180	80352	2.00000	2.225	70.00-	130.00	100.00
19.506	19.506	(1.300)	182	76117			63.09-	123.09	94.73
-----									
164	Hexachlorobutadiene					CAS #:	87-68-3		
19.589	19.589	(1.306)	225	48303	2.00000	1.982	70.00-	130.00	100.00(a)
19.589	19.589	(1.306)	223	29341			32.88-	92.88	60.74
-----									
142	Propylbenzene					CAS #:	103-65-1		
16.824	16.824	(1.122)	91	165697	2.00000	1.626	70.00-	130.00	100.00
16.852	16.852	(1.123)	120	39713			0.00-	30.00	23.97
16.824	16.824	(1.122)	105	6884			0.00-	30.00	4.15
-----									
136	Cumene					CAS #:	98-82-8		
16.326	16.326	(1.088)	105	141711	2.00000	1.547	70.00-	130.00	100.00
16.326	16.326	(1.088)	120	37390			0.00-	30.00	26.38
16.326	16.326	(1.088)	51	16354			0.00-	30.00	11.54
-----									
165	Naphthalene					CAS #:	91-20-3		
19.672	19.672	(1.312)	128	257783	2.00000	2.228	70.00-	130.00	100.00
19.672	19.672	(1.312)	127	32076			0.00-	30.00	12.44
-----									
37	tert-Butyl-Alcohol					CAS #:	75-65-0		
5.598	5.598	(0.695)	59	47998	2.00000	2.039	70.00-	130.00	100.00
5.598	5.598	(0.695)	41	15347			0.00-	30.00	31.97
5.598	5.598	(0.695)	57	4957			0.00-	30.00	10.33
-----									
11	Butane					CAS #:	106-97-8		
2.695	2.695	(0.334)	58	11837	2.00000	1.851	70.00-	130.00	100.00(a)
2.695	2.695	(0.334)	43	84412			0.00-	30.00	713.12
-----									
17	Isopentane					CAS #:	78-78-4		
3.414	3.414	(0.424)	43	61460	2.00000	1.550	70.00-	130.00	100.00(a)
3.414	3.414	(0.424)	57	35263			0.00-	30.00	57.38
3.414	3.414	(0.424)	72	4953			0.00-	30.00	8.06
-----									
94	Methyl Cyclohexane					CAS #:	108-87-2		
10.547	10.547	(1.064)	83	51649	2.00000	1.490	70.00-	130.00	100.00
10.547	10.547	(1.064)	98	23708			0.00-	30.00	45.90
10.547	10.547	(1.064)	55	46015			0.00-	30.00	89.09
-----									

QC Flag Legend

a - Target compound detected but, quantitated amount  
 Below Limit Of Quantitation(BLOQ).

Report Date: 25-Apr-2008 09:58

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042421.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	316701	6.74
92 1,4-Difluorobenze	1234462	740677	1728247	1264461	2.43
125 Chlorobenzene-d5	1186736	712042	1661430	1173690	-1.10

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.


RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /var/chem/msd5.1/5-24apr.lb/5042421.d  
 Date: 24-APR-2008 18:31  
 Client ID: Level 3  
 Sample Info: 2.0mL #1612-1  
 Column phase: RTX-624

Instrument: msd5.1  
 Operator: kr  
 Column diameter: 0.53

/var/chem/msd5.1/5-24apr.lb/5042421.d



Report Date: 25-Apr-2008 09:57

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042416.d  
 Lab Smp Id: ICAL Client Smp ID: Level 4  
 Inj Date : 24-APR-2008 15:19  
 Operator : ct Inst ID: msd5.i  
 Smp Info : 25mL #1612-1  
 Misc Info : 200ppbv -> 25ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:57 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 15:19 Cal File: 5042416.d  
 Als bottle: 1 Calibration Sample, Level: 4  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	CAL-AMT	ON-COL	RESPONSE ( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5								
8.059	8.059	(1.000)	130	285626	25.0000		70.00- 130.00	100.00
8.059	8.059	(1.000)	128	224398			47.51- 107.51	78.56
8.059	8.059	(1.000)	49	550973			158.47- 218.47	192.90
-----								
* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.911	9.911	(1.000)	114	1185571	25.0000		70.00- 130.00	100.00
9.911	9.911	(1.000)	88	183959			0.00- 44.75	15.52
-----								
* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	1185917	25.0000		70.00- 130.00	100.00
14.999	14.999	(1.000)	82	582491			0.00- 30.00	49.12
-----								
\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.110	9.110	(1.130)	65	364263	25.0000	25.125	70.00- 130.00	100.00
9.110	9.110	(1.130)	67	206074			0.00- 30.00	56.57
-----								
\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.704	12.704	(1.282)	98	1139064	25.0000	25.283	70.00- 130.00	100.00
12.676	12.676	(1.279)	70	104653			0.00- 30.00	9.19

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	787127			0.00- 30.00	69.10		
-----										
\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.575	16.575	(1.105)	174	729616	25.0000	25.338	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	910513			98.07- 158.07	124.79		
16.575	16.575	(1.105)	176	687841			65.46- 125.46	94.27		
-----										
6 Propylene										
						CAS #:	115-07-1			
2.253	2.253	(0.280)	41	647416	25.0000	29.214	70.00- 130.00	100.00		
2.253	2.253	(0.280)	42	412965			0.00- 30.00	63.79		
2.253	2.253	(0.280)	39	444951			0.00- 30.00	68.73		
-----										
8 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.336	2.336	(0.290)	85	1033842	25.0000	29.127	70.00- 130.00	100.00		
2.336	2.336	(0.290)	87	332090			0.00- 30.00	32.12		
-----										
9 Freon 114										
						CAS #:	76-14-2			
2.446	2.446	(0.304)	135	874089	25.0000	30.230	70.00- 130.00	100.00		
2.446	2.446	(0.304)	137	281841			2.03- 62.03	32.24		
-----										
10 Chloromethane										
						CAS #:	74-87-3			
2.584	2.584	(0.321)	50	762365	25.0000	28.580	70.00- 130.00	100.00		
2.584	2.584	(0.321)	52	230237			0.00- 30.00	30.20		
-----										
13 Vinyl Chloride										
						CAS #:	75-01-4			
2.750	2.750	(0.341)	62	655638	25.0000	30.274	70.00- 130.00	100.00		
2.778	2.778	(0.345)	64	185335			0.00- 30.00	28.27		
-----										
12 1,3-Butadiene										
						CAS #:	106-99-0			
2.750	2.750	(0.341)	54	580573	25.0000	27.102	70.00- 130.00	100.00		
2.750	2.750	(0.341)	39	747482			0.00- 30.00	128.75		
-----										
15 Bromomethane										
						CAS #:	74-83-9			
3.276	3.276	(0.406)	94	335231	25.0000	27.690	70.00- 130.00	100.00		
3.276	3.276	(0.406)	96	319842			62.86- 122.86	95.41		
-----										
19 Chloroethane										
						CAS #:	75-00-3			
3.386	3.386	(0.420)	64	325147	25.0000	30.232	70.00- 130.00	100.00		
3.386	3.386	(0.420)	49	105404			0.00- 30.00	32.42		
3.386	3.386	(0.420)	66	100339			0.00- 30.00	30.86		
-----										
20 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.718	3.718	(0.461)	101	1069374	25.0000	29.539	70.00- 130.00	100.00		
3.718	3.718	(0.461)	103	693269			33.46- 93.46	64.83		
-----										



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.077	4.077	(0.506)	45	247838	25.0000	28.977	70.00- 130.00	100.00	
4.077	4.077	(0.506)	43	51483			0.00- 30.00	20.77	
4.077	4.077	(0.506)	46	101468			0.00- 30.00	40.94	
-----									
30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	651257	25.0000	29.198	70.00- 130.00	100.00	
4.520	4.520	(0.561)	153	413396			33.20- 93.20	63.48	
4.520	4.520	(0.561)	101	875164			106.78- 166.78	134.38	
-----									
31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	847811	25.0000	29.596	70.00- 130.00	100.00	
4.575	4.575	(0.568)	96	453547			23.41- 83.41	53.50	
4.575	4.575	(0.568)	98	290271			4.01- 64.01	34.24	
-----									
32 Acetone						CAS #: 67-64-1			
4.713	4.713	(0.585)	58	292961	25.0000	26.700	70.00- 130.00	100.00	
4.713	4.713	(0.585)	43	993979			0.00- 30.00	339.29	
-----									
36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	1107755	25.0000	26.726	70.00- 130.00	100.00	
4.907	4.907	(0.609)	43	277149			0.00- 30.00	25.02	
4.935	4.935	(0.612)	59	35085			0.00- 30.00	3.17	
-----									
35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	1442925	25.0000	29.189	70.00- 130.00	100.00	
-----									
38 3-Chloropropene						CAS #: 107-05-1			
5.183	5.183	(0.643)	76	247385	25.0000	29.092	70.00- 130.00	100.00	
5.183	5.183	(0.643)	41	977529			0.00- 30.00	395.14	
-----									
43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	752023	25.0000	28.930	70.00- 130.00	100.00	
5.432	5.432	(0.674)	84	408684			26.74- 86.74	54.34	
5.432	5.432	(0.674)	51	219939			0.00- 30.00	29.25	
-----									
46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	793580	25.0000	31.932	70.00- 130.00	100.00	
5.764	5.764	(0.715)	57	227132			0.00- 59.41	28.62	
5.764	5.764	(0.715)	41	276010			0.00- 30.00	34.78	
-----									
47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	554656	25.0000	29.726	70.00- 130.00	100.00	
5.819	5.819	(0.722)	61	881505			130.65- 190.65	158.93	
5.819	5.819	(0.722)	98	333865			0.00- 30.00	60.19	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	1115512	25.0000	30.393	70.00- 130.00	100.00	
6.151	6.151	(0.763)	43	821438			0.00- 30.00	73.64	
6.151	6.151	(0.763)	86	162908			0.00- 30.00	14.60	
-----									
55 1,1-Dichloroethane						CAS #: 75-34-3			
6.593	6.593	(0.818)	63	997284	25.0000	28.972	70.00- 130.00	100.00	
6.593	6.593	(0.818)	65	302386			0.00- 59.62	30.32	
-----									
67 2-Butanone						CAS #: 78-93-3			
7.672	7.672	(0.952)	72	257425	25.0000	30.657	70.00- 130.00	100.00	
7.672	7.672	(0.952)	43	1413867			533.62- 593.62	549.23	
7.672	7.672	(0.952)	57	95815			0.00- 30.00	37.22	
-----									
66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	742044	25.0000	29.864	70.00- 130.00	100.00	
7.617	7.617	(0.945)	96	534183			42.00- 102.00	71.99	
7.617	7.617	(0.945)	98	342055			15.56- 75.56	46.10	
-----									
70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	881634	25.0000	27.560	70.00- 130.00	100.00	
8.031	8.031	(0.997)	71	233108			0.00- 56.55	26.44	
8.031	8.031	(0.997)	72	256200			0.00- 30.00	29.06	
-----									
72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	919508	25.0000	27.917	70.00- 130.00	100.00	
8.197	8.197	(1.017)	85	608465			35.57- 95.57	66.17	
-----									
75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.446	8.446	(1.048)	97	872562	25.0000	28.529	70.00- 130.00	100.00	
8.446	8.446	(1.048)	99	569362			34.21- 94.21	65.25	
-----									
74 Cyclohexane						CAS #: 110-82-7			
8.418	8.418	(1.045)	84	732869	25.0000	30.184	70.00- 130.00	100.00	
8.418	8.418	(1.045)	56	1109565			117.94- 177.94	151.40	
8.418	8.418	(1.045)	41	648732			54.92- 114.92	88.52	
-----									
56 Vinyl Acetate						CAS #: 108-05-4			
6.649	6.649	(0.825)	86	135969	25.0000	28.578	70.00- 130.00	100.00	
6.649	6.649	(0.825)	43	1800501			0.00- 30.00	1324.20	
6.649	6.649	(0.825)	42	135618			0.00- 30.00	99.74	
-----									
77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	809752	25.0000	29.574	70.00- 130.00	100.00	
8.667	8.667	(1.075)	117	829941			74.41- 134.41	102.49	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.082	9.082	(1.127)	57	3199191	25.0000	30.210	70.00- 130.00	100.00		
9.082	9.082	(1.127)	56	1048397			0.00- 30.00	32.77		
9.082	9.082	(1.127)	41	879607			0.00- 30.00	27.49		
-----										
81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	1662202	25.0000	27.953	70.00- 130.00	100.00		
9.082	9.082	(0.916)	77	401144			0.00- 30.00	24.13		
-----										
85	1,2-Dichloroethane					CAS #: 107-06-2				
9.275	9.275	(0.936)	62	639172	25.0000	29.870	70.00- 130.00	100.00		
9.275	9.275	(0.936)	64	191516			0.00- 30.00	29.96		
-----										
90	Heptane					CAS #: 142-82-5				
9.497	9.497	(0.958)	100	191246	25.0000	29.426	70.00- 130.00	100.00		
9.469	9.469	(0.955)	43	1358301			0.00- 30.00	710.24		
9.469	9.469	(0.955)	71	583422			0.00- 30.00	305.06		
-----										
93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	645994	25.0000	29.299	70.00- 130.00	100.00		
10.326	10.326	(1.042)	130	649464			70.08- 130.08	100.54		
10.326	10.326	(1.042)	97	423720			35.30- 95.30	65.59		
-----										
98	1,2-Dichloropropane					CAS #: 78-87-5				
10.824	10.824	(1.092)	63	590497	25.0000	30.043	70.00- 130.00	100.00		
10.824	10.824	(1.092)	62	421585			41.10- 101.10	71.39		
10.824	10.824	(1.092)	41	393185			36.18- 96.18	66.59		
-----										
99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.117)	88	365623	25.0000	28.052	70.00- 130.00	100.00		
11.073	11.073	(1.117)	58	287443			47.45- 107.45	78.62		
11.073	11.073	(1.117)	57	91573			0.00- 30.00	25.05		
-----										
100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.151)	83	888862	25.0000	30.888	70.00- 130.00	100.00		
11.405	11.405	(1.151)	85	564475			34.05- 94.05	63.51		
-----										
103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	659162	25.0000	29.274	70.00- 130.00	100.00		
12.317	12.317	(1.243)	77	212260			1.82- 61.82	32.20		
12.289	12.289	(1.240)	39	448572			36.40- 96.40	68.05		
-----										
106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.593	12.593	(1.271)	58	488354	25.0000	30.956	70.00- 130.00	100.00		
12.593	12.593	(1.271)	43	1389181			0.00- 30.00	284.46		
12.593	12.593	(1.271)	85	172642			0.00- 30.00	35.35		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	1742127	25.0000	30.119	70.00- 130.00	100.00	
12.815	12.815	(1.293)	92	999300			27.75- 87.75	57.36	
-----									
113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	650332	25.0000	28.465	70.00- 130.00	100.00	
13.368	13.368	(0.891)	77	205311			2.38- 62.38	31.57	
13.340	13.340	(0.889)	39	436230			35.96- 95.96	67.08	
-----									
114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	607671	25.0000	30.133	70.00- 130.00	100.00	
13.644	13.644	(0.910)	99	378908			33.83- 93.83	62.35	
13.644	13.644	(0.910)	83	500596			52.70- 112.70	82.38	
-----									
116 Tetrachloroethene						CAS #: 127-18-4			
13.699	13.699	(0.913)	166	766059	25.0000	29.258	70.00- 130.00	100.00	
13.672	13.672	(0.912)	129	558167			44.73- 104.73	72.86	
13.699	13.699	(0.913)	131	540031			40.60- 100.60	70.49	
-----									
119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	636158	25.0000	26.333	70.00- 130.00	100.00	
14.004	14.004	(0.934)	43	1417316			181.71- 241.71	222.79	
14.031	14.031	(0.935)	100	119132			0.00- 30.00	18.73	
-----									
120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	878389	25.0000	29.493	70.00- 130.00	100.00	
14.197	14.197	(0.947)	127	679236			0.00- 30.00	77.33	
-----									
122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	944591	25.0000	28.016	70.00- 130.00	100.00	
14.363	14.363	(0.958)	109	879006			65.00- 125.00	93.06	
-----									
126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	1422341	25.0000	29.635	70.00- 130.00	100.00	
15.027	15.027	(1.002)	114	445186			2.42- 62.42	31.30	
15.027	15.027	(1.002)	77	789587			27.34- 87.34	55.51	
-----									
128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	783761	25.0000	29.528	70.00- 130.00	100.00	
15.165	15.165	(1.011)	91	2367524			0.00- 30.00	302.07	
-----									
130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	988735	25.0000	29.959	70.00- 130.00	100.00	
15.331	15.331	(1.022)	91	1878162			0.00- 30.00	189.96	
-----									
132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	924678	25.0000	29.969	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	1831701			170.15- 230.15	198.09	
-----									
133 Styrene									
15.911	15.911	(1.061)	104	1446050	25.0000	29.092	70.00- 130.00	100.00	
15.911	15.911	(1.061)	78	632988			13.62- 73.62	43.77	
-----									
134 Bromoform									
16.160	16.160	(1.077)	173	820728	25.0000	28.738	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	418753			22.36- 82.36	51.02	
-----									
141 1,1,2,2-Tetrachloroethane									
16.796	16.796	(1.120)	83	1305949	25.0000	28.727	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	864420			36.19- 96.19	66.19	
-----									
144 4-Ethyltoluene									
16.962	16.962	(1.131)	105	2813209	25.0000	30.154	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	861180			0.17- 60.17	30.61	
-----									
147 1,3,5-Trimethylbenzene									
17.045	17.045	(1.136)	105	2470967	25.0000	29.764	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	1227367			0.00- 30.00	49.67	
-----									
152 1,2,4-Trimethylbenzene									
17.460	17.460	(1.164)	105	2006394	25.0000	28.800	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	980532			17.48- 77.48	48.87	
-----									
155 1,3-Dichlorobenzene									
17.764	17.764	(1.184)	146	1342680	25.0000	27.756	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	859949			0.00- 30.00	64.05	
17.764	17.764	(1.184)	111	516783			0.00- 30.00	38.49	
-----									
156 1,4-Dichlorobenzene									
17.847	17.847	(1.190)	146	1697632	25.0000	27.867	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	1078748			0.00- 30.00	63.54	
17.847	17.847	(1.190)	111	651277			0.00- 30.00	38.36	
-----									
157 alpha-Chlorotoluene									
17.985	17.985	(1.199)	91	2014324	25.0000	29.388	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	436309			0.00- 30.00	21.66	
-----									
159 1,2-Dichlorobenzene									
18.206	18.206	(1.214)	146	1336842	25.0000	26.942	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	846017			32.26- 92.26	63.28	
18.206	18.206	(1.214)	111	523291			7.92- 67.92	39.14	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
-----									
163	1,2,4-Trichlorobenzene				CAS #: 120-82-1				
19.478	19.478	(1.299)	180	837828	25.0000	22.958	70.00- 130.00	100.00	
19.478	19.478	(1.299)	182	785143			63.09- 123.09	93.71	
-----									
164	Hexachlorobutadiene				CAS #: 87-68-3				
19.589	19.589	(1.306)	225	617318	25.0000	25.072	70.00- 130.00	100.00	
19.561	19.561	(1.304)	223	369052			32.88- 92.88	59.78	
-----									
142	Propylbenzene				CAS #: 103-65-1				
16.824	16.824	(1.122)	91	3055307	25.0000	29.668	70.00- 130.00	100.00	
16.824	16.824	(1.122)	120	724624			0.00- 30.00	23.72	
16.824	16.824	(1.122)	105	115597			0.00- 30.00	3.78	
-----									
136	Cumene				CAS #: 98-82-8				
16.326	16.326	(1.088)	105	2707385	25.0000	29.244	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	746735			0.00- 30.00	27.58	
16.326	16.326	(1.088)	51	297960			0.00- 30.00	11.01	
-----									
165	Naphthalene				CAS #: 91-20-3				
19.672	19.672	(1.312)	128	2970069	25.0000	25.406	70.00- 130.00	100.00	
19.672	19.672	(1.312)	127	377742			0.00- 30.00	12.72	
-----									
37	tert-Butyl-Alcohol				CAS #: 75-65-0				
5.570	5.570	(0.691)	59	670072	25.0000	31.561	70.00- 130.00	100.00	
5.570	5.570	(0.691)	41	202733			0.00- 30.00	30.26	
5.570	5.570	(0.691)	57	66598			0.00- 30.00	9.94	
-----									
11	Butane				CAS #: 106-97-8				
2.667	2.667	(0.331)	58	160873	25.0000	27.888	70.00- 130.00	100.00	
2.667	2.667	(0.331)	43	1344888			0.00- 30.00	835.99	
-----									
17	Isopentane				CAS #: 78-78-4				
3.414	3.414	(0.424)	43	1002829	25.0000	28.051	70.00- 130.00	100.00	
3.414	3.414	(0.424)	57	578489			0.00- 30.00	57.69	
3.414	3.414	(0.424)	72	50818			0.00- 30.00	5.07	
-----									
94	Methyl Cyclohexane				CAS #: 108-87-2				
10.547	10.547	(1.064)	83	970622	25.0000	29.857	70.00- 130.00	100.00	
10.547	10.547	(1.064)	98	473924			0.00- 30.00	48.83	
10.547	10.547	(1.064)	55	923547			0.00- 30.00	95.15	
-----									

Report Date: 25-Apr-2008 09:57

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042416.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	285626	-3.73
92 1,4-Difluorobenze	1234462	740677	1728247	1185571	-3.96
125 Chlorobenzene-d5	1186736	712042	1661430	1185917	-0.07


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.





Report Date: 25-Apr-2008 09:57

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042417.d  
 Lab Smp Id: ICAL Client Smp ID: Level 5  
 Inj Date : 24-APR-2008 15:47  
 Operator : ct Inst ID: msd5.i  
 Smp Info : 50mL #1612-1  
 Misc Info : 200ppbv -> 50ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:57 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 15:47 Cal File: 5042417.d  
 Als bottle: 1 Calibration Sample, Level: 5  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable

Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 71	Bromochloromethane						CAS #: 74-97-5	
8.059	8.059	(1.000)	130	296697	25.0000		80.00- 120.00	100.00
8.059	8.059	(1.000)	128	229958			47.51- 107.51	77.51
8.059	8.059	(1.000)	49	559185			158.47- 218.47	188.47
-----								
* 92	1,4-Difluorobenzene						CAS #: 540-36-3	
9.912	9.912	(1.000)	114	1234462	25.0000		80.00- 120.00	100.00
9.912	9.912	(1.000)	88	182091			0.00- 44.75	14.75
-----								
* 125	Chlorobenzene-d5						CAS #: 3114-55-4	
14.999	14.999	(1.000)	117	1186736	25.0000		80.00- 120.00	100.00
14.999	14.999	(1.000)	82	600713			20.62- 80.62	50.62
-----								
\$ 84	1,2-Dichloroethane-d4						CAS #: 17060-07-0	
9.137	9.137	(1.134)	65	381239	25.0000	25.315	80.00- 120.00	100.00
9.110	9.110	(1.130)	67	231370			30.69- 90.69	60.69
-----								
\$ 107	Toluene-d8						CAS #: 2037-26-5	
12.704	12.704	(1.282)	98	1200024	25.0000	25.581	80.00- 120.00	100.00
12.677	12.677	(1.279)	70	112385			0.00- 39.37	9.37

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	805326			37.11- 97.11	67.11		
-----										
\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.575	16.575	(1.105)	174	729157	25.0000	25.304	80.00- 120.00	100.00		
16.575	16.575	(1.105)	95	933806			98.07- 158.07	128.07		
16.575	16.575	(1.105)	176	696072			65.46- 125.46	95.46		
-----										
6 Propylene						CAS #:	115-07-1			
2.253	2.253	(0.280)	41	1265724	50.0000	54.983	80.00- 120.00	100.00		
2.253	2.253	(0.280)	42	802373			33.39- 93.39	63.39		
2.253	2.253	(0.280)	39	878627			39.42- 99.42	69.42		
-----										
8 Dichlorodifluoromethane/Fr12						CAS #:	75-71-8			
2.336	2.336	(0.290)	85	2007632	50.0000	54.451	80.00- 120.00	100.00		
2.336	2.336	(0.290)	87	648300			2.29- 62.29	32.29		
-----										
9 Freon 114						CAS #:	76-14-2			
2.446	2.446	(0.304)	135	1670931	50.0000	55.632	80.00- 120.00	100.00		
2.446	2.446	(0.304)	137	535164			2.03- 62.03	32.03		
-----										
10 Chloromethane						CAS #:	74-87-3			
2.585	2.585	(0.321)	50	1472622	50.0000	53.146	80.00- 120.00	100.00		
2.585	2.585	(0.321)	52	440257			0.00- 59.90	29.90		
-----										
13 Vinyl Chloride						CAS #:	75-01-4			
2.750	2.750	(0.341)	62	1255638	50.0000	55.816	80.00- 120.00	100.00		
2.778	2.778	(0.345)	64	377005			0.02- 60.02	30.02		
-----										
12 1,3-Butadiene						CAS #:	106-99-0			
2.750	2.750	(0.341)	54	1186480	50.0000	53.321	80.00- 120.00	100.00		
2.750	2.750	(0.341)	39	1474124			94.24- 154.24	124.24		
-----										
15 Bromomethane						CAS #:	74-83-9			
3.276	3.276	(0.406)	94	716413	50.0000	56.968	80.00- 120.00	100.00		
3.276	3.276	(0.406)	96	665263			62.86- 122.86	92.86		
-----										
19 Chloroethane						CAS #:	75-00-3			
3.386	3.386	(0.420)	64	610852	50.0000	54.678	80.00- 120.00	100.00		
3.414	3.414	(0.424)	49	192538			1.52- 61.52	31.52		
3.386	3.386	(0.420)	66	186794			0.58- 60.58	30.58		
-----										
20 Trichlorofluoromethane/Fr11						CAS #:	75-69-4			
3.718	3.718	(0.461)	101	2137246	50.0000	56.833	80.00- 120.00	100.00		
3.718	3.718	(0.461)	103	1356302			33.46- 93.46	63.46		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.078	4.078	(0.506)	45	514471	50.0000	57.908	80.00- 120.00	100.00	
4.078	4.078	(0.506)	43	91694			0.00- 47.82	17.82	
4.078	4.078	(0.506)	46	202258			9.31- 69.31	39.31	
-----									
30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	1255191	50.0000	54.175	80.00- 120.00	100.00	
4.520	4.520	(0.561)	153	793240			33.20- 93.20	63.20	
4.520	4.520	(0.561)	101	1716913			106.78- 166.78	136.78	
-----									
31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	1692914	50.0000	56.892	80.00- 120.00	100.00	
4.575	4.575	(0.568)	96	904151			23.41- 83.41	53.41	
4.575	4.575	(0.568)	98	575810			4.01- 64.01	34.01	
-----									
32 Acetone						CAS #: 67-64-1			
4.714	4.714	(0.585)	58	593883	50.0000	52.106	80.00- 120.00	100.00	
4.714	4.714	(0.585)	43	2077338			319.79- 379.79	349.79	
-----									
36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	2349546	50.0000	54.571	80.00- 120.00	100.00	
4.907	4.907	(0.609)	43	557862			0.00- 53.74	23.74	
4.907	4.907	(0.609)	59	78709			0.00- 33.35	3.35	
-----									
35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	2864850	50.0000	55.790	80.00- 120.00	100.00	
-----									
38 3-Chloropropene						CAS #: 107-05-1			
5.184	5.184	(0.643)	76	496706	50.0000	56.233	80.00- 120.00	100.00	
5.184	5.184	(0.643)	41	1959446			364.49- 424.49	394.49	
-----									
43 Methylene Chloride						CAS #: 75-09-2			
5.432	5.432	(0.674)	49	1462447	50.0000	54.160	80.00- 120.00	100.00	
5.432	5.432	(0.674)	84	829798			26.74- 86.74	56.74	
5.432	5.432	(0.674)	51	425057			0.00- 59.06	29.06	
-----									
46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	1554787	50.0000	60.227	80.00- 120.00	100.00	
5.764	5.764	(0.715)	57	457233			0.00- 59.41	29.41	
5.764	5.764	(0.715)	41	536295			4.49- 64.49	34.49	
-----									
47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	1097288	50.0000	56.613	80.00- 120.00	100.00	
5.819	5.819	(0.722)	61	1762833			130.65- 190.65	160.65	
5.819	5.819	(0.722)	98	679562			31.93- 91.93	61.93	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	2226777	50.0000	58.407	80.00- 120.00	100.00	
6.151	6.151	(0.763)	43	1617720			42.65- 102.65	72.65	
6.151	6.151	(0.763)	86	312865			0.00- 44.05	14.05	
-----									
55 1,1-Dichloroethane						CAS #: 75-34-3			
6.594	6.594	(0.818)	63	2007827	50.0000	56.153	80.00- 120.00	100.00	
6.594	6.594	(0.818)	65	594800			0.00- 59.62	29.62	
-----									
67 2-Butanone						CAS #: 78-93-3			
7.644	7.644	(0.949)	72	509100	50.0000	58.367	80.00- 120.00	100.00	
7.644	7.644	(0.949)	43	2869395			533.62- 593.62	563.62	
7.644	7.644	(0.949)	57	199433			9.17- 69.17	39.17	
-----									
66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	1479989	50.0000	57.340	80.00- 120.00	100.00	
7.617	7.617	(0.945)	96	1065640			42.00- 102.00	72.00	
7.617	7.617	(0.945)	98	674303			15.56- 75.56	45.56	
-----									
70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	1772021	50.0000	53.328	80.00- 120.00	100.00	
8.031	8.031	(0.997)	71	470494			0.00- 56.55	26.55	
8.031	8.031	(0.997)	72	516579			0.00- 59.15	29.15	
-----									
72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	1809544	50.0000	52.889	80.00- 120.00	100.00	
8.197	8.197	(1.017)	85	1186543			35.57- 95.57	65.57	
-----									
75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.446	8.446	(1.048)	97	1773716	50.0000	55.829	80.00- 120.00	100.00	
8.446	8.446	(1.048)	99	1138949			34.21- 94.21	64.21	
-----									
74 Cyclohexane						CAS #: 110-82-7			
8.419	8.419	(1.045)	84	1471665	50.0000	58.351	80.00- 120.00	100.00	
8.419	8.419	(1.045)	56	2177201			117.94- 177.94	147.94	
8.419	8.419	(1.045)	41	1249724			54.92- 114.92	84.92	
-----									
56 Vinyl Acetate						CAS #: 108-05-4			
6.649	6.649	(0.825)	86	277124	50.0000	56.073	80.00- 120.00	100.00	
6.649	6.649	(0.825)	43	3681296			1298.39-1358.39	1328.39	
6.649	6.649	(0.825)	42	282192			71.83- 131.83	101.83	
-----									
77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	1595179	50.0000	56.086	80.00- 120.00	100.00	
8.667	8.667	(1.075)	117	1665494			74.41- 134.41	104.41	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.082	9.082	(1.127)	57	6349467	50.0000	57.721	80.00- 120.00	100.00		
9.082	9.082	(1.127)	56	2085450			2.84- 62.84	32.84		
9.082	9.082	(1.127)	41	1682302			0.00- 56.50	26.50		
-----										
81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	3223515	50.0000	52.062	80.00- 120.00	100.00		
9.082	9.082	(0.916)	77	774352			0.00- 54.02	24.02		
-----										
85	1,2-Dichloroethane					CAS #: 107-06-2				
9.276	9.276	(0.936)	62	1244483	50.0000	55.854	80.00- 120.00	100.00		
9.276	9.276	(0.936)	64	376709			0.27- 60.27	30.27		
-----										
90	Heptane					CAS #: 142-82-5				
9.469	9.469	(0.955)	100	385958	50.0000	57.032	80.00- 120.00	100.00		
9.469	9.469	(0.955)	43	2671822			662.26- 722.26	692.26		
9.469	9.469	(0.955)	71	1156296			269.59- 329.59	299.59		
-----										
93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	1253951	50.0000	54.620	80.00- 120.00	100.00		
10.326	10.326	(1.042)	130	1254939			70.08- 130.08	100.08		
10.326	10.326	(1.042)	97	818864			35.30- 95.30	65.30		
-----										
98	1,2-Dichloropropane					CAS #: 78-87-5				
10.824	10.824	(1.092)	63	1161085	50.0000	56.733	80.00- 120.00	100.00		
10.824	10.824	(1.092)	62	825513			41.10- 101.10	71.10		
10.824	10.824	(1.092)	41	765048			35.89- 95.89	65.89		
-----										
99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.117)	88	751865	50.0000	55.402	80.00- 120.00	100.00		
11.073	11.073	(1.117)	58	582323			47.45- 107.45	77.45		
11.073	11.073	(1.117)	57	188946			0.00- 55.13	25.13		
-----										
100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.151)	83	1724779	50.0000	57.563	80.00- 120.00	100.00		
11.405	11.405	(1.151)	85	1104648			34.05- 94.05	64.05		
-----										
103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	1357048	50.0000	57.880	80.00- 120.00	100.00		
12.317	12.317	(1.243)	77	431759			1.82- 61.82	31.82		
12.289	12.289	(1.240)	39	901145			36.40- 96.40	66.40		
-----										
106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.594	12.594	(1.271)	58	959235	50.0000	58.396	80.00- 120.00	100.00		
12.594	12.594	(1.271)	43	2789086			260.76- 320.76	290.76		
12.594	12.594	(1.271)	85	363200			7.86- 67.86	37.86		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	3385901	50.0000	56.220	80.00- 120.00	100.00	
12.815	12.815	(1.293)	92	1955292			27.75- 87.75	57.75	
-----									
113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	1339031	50.0000	58.568	80.00- 120.00	100.00	
13.368	13.368	(0.891)	77	433574			2.38- 62.38	32.38	
13.340	13.340	(0.889)	39	883201			35.96- 95.96	65.96	
-----									
114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	1167567	50.0000	57.858	80.00- 120.00	100.00	
13.644	13.644	(0.910)	99	745284			33.83- 93.83	63.83	
13.644	13.644	(0.910)	83	965561			52.70- 112.70	82.70	
-----									
116 Tetrachloroethene						CAS #: 127-18-4			
13.700	13.700	(0.913)	166	1488209	50.0000	56.799	80.00- 120.00	100.00	
13.672	13.672	(0.912)	129	1112208			44.73- 104.73	74.73	
13.672	13.672	(0.912)	131	1050639			40.60- 100.60	70.60	
-----									
119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	1326582	50.0000	54.874	80.00- 120.00	100.00	
14.004	14.004	(0.934)	43	2808501			181.71- 241.71	211.71	
14.004	14.004	(0.934)	100	250860			0.00- 48.91	18.91	
-----									
120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	1722283	50.0000	57.788	80.00- 120.00	100.00	
14.197	14.197	(0.947)	127	1346503			48.18- 108.18	78.18	
-----									
122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	1845098	50.0000	54.687	80.00- 120.00	100.00	
14.363	14.363	(0.958)	109	1752779			65.00- 125.00	95.00	
-----									
126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	2697354	50.0000	56.161	80.00- 120.00	100.00	
15.027	15.027	(1.002)	114	874398			2.42- 62.42	32.42	
15.027	15.027	(1.002)	77	1546623			27.34- 87.34	57.34	
-----									
128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	1544298	50.0000	58.140	80.00- 120.00	100.00	
15.165	15.165	(1.011)	91	4661881			271.88- 331.88	301.88	
-----									
130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	1917128	50.0000	58.050	80.00- 120.00	100.00	
15.331	15.331	(1.022)	91	3640544			159.90- 219.90	189.90	
-----									
132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	1799335	50.0000	58.277	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	3601342			170.15- 230.15	200.15	
-----									
133 Styrene CAS #: 100-42-5									
15.912	15.912	(1.061)	104	2848660	50.0000	57.270	80.00- 120.00	100.00	
15.884	15.884	(1.059)	78	1242597			13.62- 73.62	43.62	
-----									
134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1667802	50.0000	58.358	80.00- 120.00	100.00	
16.160	16.160	(1.077)	171	873332			22.36- 82.36	52.36	
-----									
141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	2526396	50.0000	55.534	80.00- 120.00	100.00	
16.796	16.796	(1.120)	85	1672300			36.19- 96.19	66.19	
-----									
144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	5747427	50.0000	61.562	80.00- 120.00	100.00	
16.962	16.962	(1.131)	120	1734194			0.17- 60.17	30.17	
-----									
147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	4824861	50.0000	58.079	80.00- 120.00	100.00	
17.045	17.045	(1.136)	120	2459390			20.97- 80.97	50.97	
-----									
152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	3987255	50.0000	57.193	80.00- 120.00	100.00	
17.460	17.460	(1.164)	120	1893138			17.48- 77.48	47.48	
-----									
155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	2652020	50.0000	54.784	80.00- 120.00	100.00	
17.764	17.764	(1.184)	148	1693624			33.86- 93.86	63.86	
17.764	17.764	(1.184)	111	1027732			8.75- 68.75	38.75	
-----									
156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	3443847	50.0000	56.493	80.00- 120.00	100.00	
17.847	17.847	(1.190)	148	2158560			32.68- 92.68	62.68	
17.847	17.847	(1.190)	111	1305873			7.92- 67.92	37.92	
-----									
157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	4387960	50.0000	63.974	80.00- 120.00	100.00	
17.985	17.985	(1.199)	126	978171			0.00- 52.29	22.29	
-----									
159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	2680729	50.0000	53.988	80.00- 120.00	100.00	
18.206	18.206	(1.214)	148	1669080			32.26- 92.26	62.26	
18.206	18.206	(1.214)	111	1016658			7.92- 67.92	37.92	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.478	19.478	(1.299)	180	1798465	50.0000	49.248	80.00- 120.00	100.00	
19.478	19.478	(1.299)	182	1674208			63.09- 123.09	93.09	
-----									
164	Hexachlorobutadiene					CAS #: 87-68-3			
19.561	19.561	(1.304)	225	1239505	50.0000	50.308	80.00- 120.00	100.00	
19.561	19.561	(1.304)	223	779439			32.88- 92.88	62.88	
-----									
142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	6106747	50.0000	59.257	80.00- 120.00	100.00	
16.824	16.824	(1.122)	120	1455407			0.00- 53.83	23.83	
16.824	16.824	(1.122)	105	224499			0.00- 33.68	3.68	
-----									
136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	5242531	50.0000	56.589	80.00- 120.00	100.00	
16.326	16.326	(1.088)	120	1439389			0.00- 57.46	27.46	
16.326	16.326	(1.088)	51	573438			0.00- 40.94	10.94	
-----									
165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	6852340	50.0000	58.574	80.00- 120.00	100.00	
19.672	19.672	(1.312)	127	865966			0.00- 42.64	12.64	
-----									
37	tert-Butyl-Alcohol					CAS #: 75-65-0			
5.571	5.571	(0.691)	59	1201021	50.0000	54.458	80.00- 120.00	100.00	
5.571	5.571	(0.691)	41	358675			0.00- 59.86	29.86	
5.571	5.571	(0.691)	57	117291			0.00- 39.77	9.77	
-----									
11	Butane					CAS #: 106-97-8			
2.667	2.667	(0.331)	58	308974	50.0000	51.563	80.00- 120.00	100.00	
2.667	2.667	(0.331)	43	2593192			809.29- 869.29	839.29	
-----									
17	Isopentane					CAS #: 78-78-4			
3.414	3.414	(0.424)	43	2014595	50.0000	54.249	80.00- 120.00	100.00	
3.414	3.414	(0.424)	57	1152362			27.20- 87.20	57.20	
3.414	3.414	(0.424)	72	109124			0.00- 35.42	5.42	
-----									
94	Methyl Cyclohexane					CAS #: 108-87-2			
10.548	10.548	(1.064)	83	1903994	50.0000	56.248	80.00- 120.00	100.00	
10.548	10.548	(1.064)	98	914284			18.02- 78.02	48.02	
10.548	10.548	(1.064)	55	1780789			63.53- 123.53	93.53	
-----									



Report Date: 25-Apr-2008 09:57

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042417.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	296697	0.00
92 1,4-Difluorobenze	1234462	740677	1728247	1234462	0.00
125 Chlorobenzene-d5	1186736	712042	1661430	1186736	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /var/chem/msd5.1/5-24apr.lb/5042417.d  
Date: 24-APR-2008 15:47  
Client ID: Level 5  
Sample Info: 50ml #1612-1

Column phase: RTX-624

Instrument: msd5.1  
Operator: ct  
Column diameter: 0.53

/var/chem/msd5.1/5-24apr.lb/5042417.d



Report Date: 25-Apr-2008 09:57

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042418.d  
 Lab Smp Id: ICAL Client Smp ID: Level 6  
 Inj Date : 24-APR-2008 16:15  
 Operator : ct Inst ID: msd5.i  
 Smp Info : 100mL #1612-1  
 Misc Info : 200ppbv -> 100ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:57 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:15 Cal File: 5042418.d  
 Als bottle: 1 Calibration Sample, Level: 6  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5								
8.059	8.059	(1.000)	130	314768	25.0000		70.00- 130.00	100.00
8.059	8.059	(1.000)	128	248758			47.51- 107.51	79.03
8.059	8.059	(1.000)	49	580314			158.47- 218.47	184.36
-----								
* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.912	9.912	(1.000)	114	1315322	25.0000		70.00- 130.00	100.00
9.912	9.912	(1.000)	88	196055			0.00- 44.75	14.91
-----								
* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	1284080	25.0000		70.00- 130.00	100.00
14.999	14.999	(1.000)	82	619374			0.00- 30.00	48.23
-----								
\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.137	9.137	(1.134)	65	396058	25.0000	24.789	70.00- 130.00	100.00
9.110	9.110	(1.130)	67	268730			0.00- 30.00	67.85
-----								
\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.704	12.704	(1.282)	98	1233164	25.0000	24.671	70.00- 130.00	100.00
12.677	12.677	(1.279)	70	116387			0.00- 30.00	9.44

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	908053			0.00- 30.00	73.64		
-----										
\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.575	16.575	(1.105)	174	774429	25.0000	24.838	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	998473			98.07- 158.07	128.93		
16.575	16.575	(1.105)	176	747257			65.46- 125.46	96.49		
-----										
6 Propylene										
						CAS #:	115-07-1			
2.280	2.280	(0.283)	41	2440914	100.000	99.946	70.00- 130.00	100.00		
2.253	2.253	(0.280)	42	1599974			0.00- 30.00	65.55		
2.253	2.253	(0.280)	39	1753358			0.00- 30.00	71.83		
-----										
8 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.336	2.336	(0.290)	85	3922921	100.000	100.29	70.00- 130.00	100.00		
2.336	2.336	(0.290)	87	1252030			0.00- 30.00	31.92		
-----										
9 Freon 114										
						CAS #:	76-14-2			
2.474	2.474	(0.307)	135	3371549	100.000	105.81	70.00- 130.00	100.00		
2.474	2.474	(0.307)	137	1073787			2.03- 62.03	31.85		
-----										
10 Chloromethane										
						CAS #:	74-87-3			
2.585	2.585	(0.321)	50	2856326	100.000	97.165	70.00- 130.00	100.00		
2.585	2.585	(0.321)	52	824954			0.00- 30.00	28.88		
-----										
13 Vinyl Chloride										
						CAS #:	75-01-4			
2.778	2.778	(0.345)	62	2543479	100.000	106.57	70.00- 130.00	100.00		
2.750	2.750	(0.341)	64	773361			0.00- 30.00	30.41		
-----										
12 1,3-Butadiene										
						CAS #:	106-99-0			
2.750	2.750	(0.341)	54	2400295	100.000	101.68	70.00- 130.00	100.00		
2.750	2.750	(0.341)	39	3132487			0.00- 30.00	130.50		
-----										
15 Bromomethane										
						CAS #:	74-83-9			
3.276	3.276	(0.406)	94	1487359	100.000	111.48	70.00- 130.00	100.00		
3.276	3.276	(0.406)	96	1400297			62.86- 122.86	94.15		
-----										
19 Chloroethane										
						CAS #:	75-00-3			
3.414	3.414	(0.424)	64	1257981	100.000	106.14	70.00- 130.00	100.00		
3.414	3.414	(0.424)	49	400265			0.00- 30.00	31.82		
3.414	3.414	(0.424)	66	376428			0.00- 30.00	29.92		
-----										
20 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.718	3.718	(0.461)	101	4301685	100.000	107.82	70.00- 130.00	100.00		
3.718	3.718	(0.461)	103	2775017			33.46- 93.46	64.51		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.105	4.105	(0.509)	45	953552	100.000	101.17	70.00- 130.00	100.00	
4.078	4.078	(0.506)	43	182300			0.00- 30.00	19.12	
4.105	4.105	(0.509)	46	377945			0.00- 30.00	39.64	
-----									
30 Freon 113						CAS #: 76-13-1			
4.520	4.520	(0.561)	151	2609263	100.000	106.15	70.00- 130.00	100.00	
4.520	4.520	(0.561)	153	1639413			33.20- 93.20	62.83	
4.520	4.520	(0.561)	101	3537010			106.78- 166.78	135.56	
-----									
31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	3473232	100.000	110.02	70.00- 130.00	100.00	
4.575	4.575	(0.568)	96	1894768			23.41- 83.41	54.55	
4.575	4.575	(0.568)	98	1194936			4.01- 64.01	34.40	
-----									
32 Acetone						CAS #: 67-64-1			
4.714	4.714	(0.585)	58	1276148	100.000	105.54	70.00- 130.00	100.00	
4.714	4.714	(0.585)	43	4245872			0.00- 30.00	332.71	
-----									
36 2-Propanol						CAS #: 67-63-0			
4.907	4.907	(0.609)	45	5025627	100.000	110.02	70.00- 130.00	100.00	
4.907	4.907	(0.609)	43	1114984			0.00- 30.00	22.19	
4.935	4.935	(0.612)	59	173881			0.00- 30.00	3.46	
-----									
35 Carbon Disulfide						CAS #: 75-15-0			
4.907	4.907	(0.609)	76	5927459	100.000	108.80	70.00- 130.00	100.00	
-----									
38 3-Chloropropene						CAS #: 107-05-1			
5.184	5.184	(0.643)	76	1031514	100.000	110.07	70.00- 130.00	100.00	
5.184	5.184	(0.643)	41	4029364			0.00- 30.00	390.63	
-----									
43 Methylene Chloride						CAS #: 75-09-2			
5.460	5.460	(0.678)	49	2972326	100.000	103.76	70.00- 130.00	100.00	
5.460	5.460	(0.678)	84	1666810			26.74- 86.74	56.08	
5.460	5.460	(0.678)	51	906839			0.00- 30.00	30.51	
-----									
46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	3286350	100.000	119.99	70.00- 130.00	100.00	
5.764	5.764	(0.715)	57	944732			0.00- 59.41	28.75	
5.764	5.764	(0.715)	41	1089741			0.00- 30.00	33.16	
-----									
47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.820	5.820	(0.722)	96	2195607	100.000	106.78	70.00- 130.00	100.00	
5.820	5.820	(0.722)	61	3566115			130.65- 190.65	162.42	
5.820	5.820	(0.722)	98	1440978			0.00- 30.00	65.63	
-----									

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
51 Hexane						CAS #: 110-54-3		
6.151	6.151	(0.763)	57	4541336	100.000	112.28	70.00- 130.00	100.00
6.151	6.151	(0.763)	43	3333952			0.00- 30.00	73.41
6.151	6.151	(0.763)	86	649745			0.00- 30.00	14.31
-----								
55 1,1-Dichloroethane						CAS #: 75-34-3		
6.594	6.594	(0.818)	63	4086831	100.000	107.74	70.00- 130.00	100.00
6.594	6.594	(0.818)	65	1240469			0.00- 59.62	30.35
-----								
67 2-Butanone						CAS #: 78-93-3		
7.644	7.644	(0.949)	72	1087267	100.000	117.50	70.00- 130.00	100.00
7.644	7.644	(0.949)	43	5975832			533.62- 593.62	549.62
7.644	7.644	(0.949)	57	402232			0.00- 30.00	36.99
-----								
66 cis-1,2-Dichloroethene						CAS #: 156-59-2		
7.617	7.617	(0.945)	61	2971725	100.000	108.52	70.00- 130.00	100.00
7.617	7.617	(0.945)	96	2158501			42.00- 102.00	72.63
7.617	7.617	(0.945)	98	1368417			15.56- 75.56	46.05
-----								
70 Tetrahydrofuran						CAS #: 109-99-9		
8.031	8.031	(0.997)	42	3550590	100.000	100.72	70.00- 130.00	100.00
8.031	8.031	(0.997)	71	975161			0.00- 56.55	27.46
8.031	8.031	(0.997)	72	1041547			0.00- 30.00	29.33
-----								
72 Chloroform						CAS #: 67-66-3		
8.197	8.197	(1.017)	83	3645445	100.000	100.43	70.00- 130.00	100.00
8.197	8.197	(1.017)	85	2413134			35.57- 95.57	66.20
-----								
75 1,1,1-Trichloroethane						CAS #: 71-55-6		
8.446	8.446	(1.048)	97	3552968	100.000	105.41	70.00- 130.00	100.00
8.446	8.446	(1.048)	99	2315201			34.21- 94.21	65.16
-----								
74 Cyclohexane						CAS #: 110-82-7		
8.419	8.419	(1.045)	84	2952425	100.000	110.34	70.00- 130.00	100.00
8.419	8.419	(1.045)	56	4407200			117.94- 177.94	149.27
8.419	8.419	(1.045)	41	2531714			54.92- 114.92	85.75
-----								
56 Vinyl Acetate						CAS #: 108-05-4		
6.649	6.649	(0.825)	86	583109	100.000	111.21	70.00- 130.00	100.00
6.649	6.649	(0.825)	43	7883295			0.00- 30.00	1351.94
6.649	6.649	(0.825)	42	592840			0.00- 30.00	101.67
-----								
77 Carbon Tetrachloride						CAS #: 56-23-5		
8.667	8.667	(1.075)	119	3289193	100.000	109.01	70.00- 130.00	100.00
8.667	8.667	(1.075)	117	3404621			74.41- 134.41	103.51
-----								

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.082	9.082	(1.127)	57	12985712	100.000	111.27	70.00- 130.00	100.00		
9.082	9.082	(1.127)	56	4231091			0.00- 30.00	32.58		
9.082	9.082	(1.127)	41	3417069			0.00- 30.00	26.31		
-----										
81	Benzene					CAS #: 71-43-2				
9.082	9.082	(0.916)	78	6626036	100.000	100.44	70.00- 130.00	100.00		
9.082	9.082	(0.916)	77	1590099			0.00- 30.00	24.00		
-----										
85	1,2-Dichloroethane					CAS #: 107-06-2				
9.276	9.276	(0.936)	62	2533583	100.000	106.72	70.00- 130.00	100.00		
9.276	9.276	(0.936)	64	774150			0.00- 30.00	30.56		
-----										
90	Heptane					CAS #: 142-82-5				
9.469	9.469	(0.955)	100	774680	100.000	107.44	70.00- 130.00	100.00		
9.469	9.469	(0.955)	43	5511038			0.00- 30.00	711.40		
9.469	9.469	(0.955)	71	2339309			0.00- 30.00	301.97		
-----										
93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.042)	95	2555389	100.000	104.46	70.00- 130.00	100.00		
10.326	10.326	(1.042)	130	2572320			70.08- 130.08	100.66		
10.326	10.326	(1.042)	97	1657921			35.30- 95.30	64.88		
-----										
98	1,2-Dichloropropane					CAS #: 78-87-5				
10.824	10.824	(1.092)	63	2351812	100.000	107.85	70.00- 130.00	100.00		
10.824	10.824	(1.092)	62	1670240			41.10- 101.10	71.02		
10.824	10.824	(1.092)	41	1539312			35.89- 95.89	65.45		
-----										
99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.117)	88	1514081	100.000	104.71	70.00- 130.00	100.00		
11.045	11.045	(1.114)	58	1198335			47.45- 107.45	79.15		
11.045	11.045	(1.114)	57	367908			0.00- 30.00	24.30		
-----										
100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.151)	83	3512764	100.000	110.03	70.00- 130.00	100.00		
11.405	11.405	(1.151)	85	2247411			34.05- 94.05	63.98		
-----										
103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.243)	75	2795099	100.000	111.89	70.00- 130.00	100.00		
12.317	12.317	(1.243)	77	873735			1.82- 61.82	31.26		
12.290	12.290	(1.240)	39	1864963			36.40- 96.40	66.72		
-----										
106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.594	12.594	(1.271)	58	2012977	100.000	115.01	70.00- 130.00	100.00		
12.594	12.594	(1.271)	43	5799162			0.00- 30.00	288.09		
12.594	12.594	(1.271)	85	756868			0.00- 30.00	37.60		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	6799867	100.000	105.96	70.00- 130.00	100.00	
12.815	12.815	(1.293)	92	3949523			27.75- 87.75	58.08	
-----									
113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	2749028	100.000	111.12	70.00- 130.00	100.00	
13.368	13.368	(0.891)	77	878914			2.38- 62.38	31.97	
13.340	13.340	(0.889)	39	1852744			35.96- 95.96	67.40	
-----									
114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	2318128	100.000	106.16	70.00- 130.00	100.00	
13.644	13.644	(0.910)	99	1481339			33.83- 93.83	63.90	
13.644	13.644	(0.910)	83	1927248			52.70- 112.70	83.14	
-----									
116 Tetrachloroethene						CAS #: 127-18-4			
13.700	13.700	(0.913)	166	3018605	100.000	106.47	70.00- 130.00	100.00	
13.672	13.672	(0.912)	129	2217386			44.73- 104.73	73.46	
13.672	13.672	(0.912)	131	2127282			40.60- 100.60	70.47	
-----									
119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	2815847	100.000	107.65	70.00- 130.00	100.00	
14.004	14.004	(0.934)	43	5773980			181.71- 241.71	205.05	
14.004	14.004	(0.934)	100	516128			0.00- 30.00	18.33	
-----									
120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	3507409	100.000	108.76	70.00- 130.00	100.00	
14.197	14.197	(0.947)	127	2722629			0.00- 30.00	77.63	
-----									
122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	3742992	100.000	102.53	70.00- 130.00	100.00	
14.363	14.363	(0.958)	109	3553213			65.00- 125.00	94.93	
-----									
126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	5486966	100.000	105.58	70.00- 130.00	100.00	
15.027	15.027	(1.002)	114	1748902			2.42- 62.42	31.87	
15.027	15.027	(1.002)	77	3069131			27.34- 87.34	55.93	
-----									
128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	3146243	100.000	109.47	70.00- 130.00	100.00	
15.165	15.165	(1.011)	91	9281194			0.00- 30.00	294.99	
-----									
130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	3898092	100.000	109.08	70.00- 130.00	100.00	
15.331	15.331	(1.022)	91	7520504			0.00- 30.00	192.93	
-----									
132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	3613806	100.000	108.17	70.00- 130.00	100.00	



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	7237921			170.15- 230.15	200.29	
-----									
133 Styrene									
15.912	15.912	(1.061)	104	5854848	100.000	108.78	70.00- 130.00	100.00	
15.884	15.884	(1.059)	78	2563307			13.62- 73.62	43.78	
-----									
134 Bromoform									
16.160	16.160	(1.077)	173	3486091	100.000	112.74	70.00- 130.00	100.00	
16.160	16.160	(1.077)	171	1801542			22.36- 82.36	51.68	
-----									
141 1,1,2,2-Tetrachloroethane									
16.796	16.796	(1.120)	83	5210590	100.000	105.85	70.00- 130.00	100.00	
16.796	16.796	(1.120)	85	3388691			36.19- 96.19	65.03	
-----									
144 4-Ethyltoluene									
16.962	16.962	(1.131)	105	11679639	100.000	115.62	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	3544828			0.17- 60.17	30.35	
-----									
147 1,3,5-Trimethylbenzene									
17.045	17.045	(1.136)	105	9968466	100.000	110.90	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	5012079			0.00- 30.00	50.28	
-----									
152 1,2,4-Trimethylbenzene									
17.460	17.460	(1.164)	105	8313910	100.000	110.21	70.00- 130.00	100.00	
17.460	17.460	(1.164)	120	4000534			17.48- 77.48	48.12	
-----									
155 1,3-Dichlorobenzene									
17.764	17.764	(1.184)	146	5510278	100.000	105.20	70.00- 130.00	100.00	
17.764	17.764	(1.184)	148	3513745			0.00- 30.00	63.77	
17.764	17.764	(1.184)	111	2125940			0.00- 30.00	38.58	
-----									
156 1,4-Dichlorobenzene									
17.847	17.847	(1.190)	146	7189666	100.000	109.00	70.00- 130.00	100.00	
17.847	17.847	(1.190)	148	4568353			0.00- 30.00	63.54	
17.847	17.847	(1.190)	111	2698565			0.00- 30.00	37.53	
-----									
157 alpha-Chlorotoluene									
17.985	17.985	(1.199)	91	9876085	100.000	133.07	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	2108481			0.00- 30.00	21.35	
-----									
159 1,2-Dichlorobenzene									
18.206	18.206	(1.214)	146	5605355	100.000	104.33	70.00- 130.00	100.00	
18.206	18.206	(1.214)	148	3547077			32.26- 92.26	63.28	
18.206	18.206	(1.214)	111	2122789			7.92- 67.92	37.87	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
163	1,2,4-Trichlorobenzene					CAS #:	120-82-1		
19.478	19.478	(1.299)	180	3835334	100.000	97.062	70.00- 130.00	100.00	
19.478	19.478	(1.299)	182	3604409			63.09- 123.09	93.98	
-----									
164	Hexachlorobutadiene					CAS #:	87-68-3		
19.589	19.589	(1.306)	225	2589942	100.000	97.150	70.00- 130.00	100.00	
19.561	19.561	(1.304)	223	1626954			32.88- 92.88	62.82	
-----									
142	Propylbenzene					CAS #:	103-65-1		
16.824	16.824	(1.122)	91	12408875	100.000	111.28	70.00- 130.00	100.00	
16.824	16.824	(1.122)	120	2948155			0.00- 30.00	23.76	
16.824	16.824	(1.122)	105	455606			0.00- 30.00	3.67	
-----									
136	Cumene					CAS #:	98-82-8		
16.326	16.326	(1.088)	105	10764532	100.000	107.38	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	2988638			0.00- 30.00	27.76	
16.326	16.326	(1.088)	51	1195170			0.00- 30.00	11.10	
-----									
165	Naphthalene					CAS #:	91-20-3		
19.672	19.672	(1.312)	128	14483126	100.000	114.42	70.00- 130.00	100.00	
19.672	19.672	(1.312)	127	1844073			0.00- 30.00	12.73	
-----									
37	tert-Butyl-Alcohol					CAS #:	75-65-0		
5.571	5.571	(0.691)	59	2178401	100.000	93.105	70.00- 130.00	100.00	
5.571	5.571	(0.691)	41	632443			0.00- 30.00	29.03	
5.571	5.571	(0.691)	57	223430			0.00- 30.00	10.26	
-----									
11	Butane					CAS #:	106-97-8		
2.695	2.695	(0.334)	58	630877	100.000	99.239	70.00- 130.00	100.00	
2.695	2.695	(0.334)	43	5188662			0.00- 30.00	822.45	
-----									
17	Isopentane					CAS #:	78-78-4		
3.414	3.414	(0.424)	43	4051759	100.000	102.84	70.00- 130.00	100.00	
3.414	3.414	(0.424)	57	2352330			0.00- 30.00	58.06	
3.414	3.414	(0.424)	72	217959			0.00- 30.00	5.38	
-----									
94	Methyl Cyclohexane					CAS #:	108-87-2		
10.548	10.548	(1.064)	83	3845733	100.000	106.63	70.00- 130.00	100.00	
10.548	10.548	(1.064)	98	1899896			0.00- 30.00	49.40	
10.548	10.548	(1.064)	55	3637361			0.00- 30.00	94.58	
-----									

Report Date: 25-Apr-2008 09:57

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042418.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	314768	6.09
92 1,4-Difluorobenze	1234462	740677	1728247	1315322	6.55
125 Chlorobenzene-d5	1186736	712042	1661430	1284080	8.20

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /var/chem/msd5.1/5-24apr.b/5042418.d  
 Date: 24-APR-2008 16:15  
 Client ID: Level 6  
 Sample Info: 100mL #1612-1

Column phase: RTX-624

Instrument: msd5.1  
 Operator: ct  
 Column diameter: 0.53

/var/chem/msd5.1/5-24apr.b/5042418.d

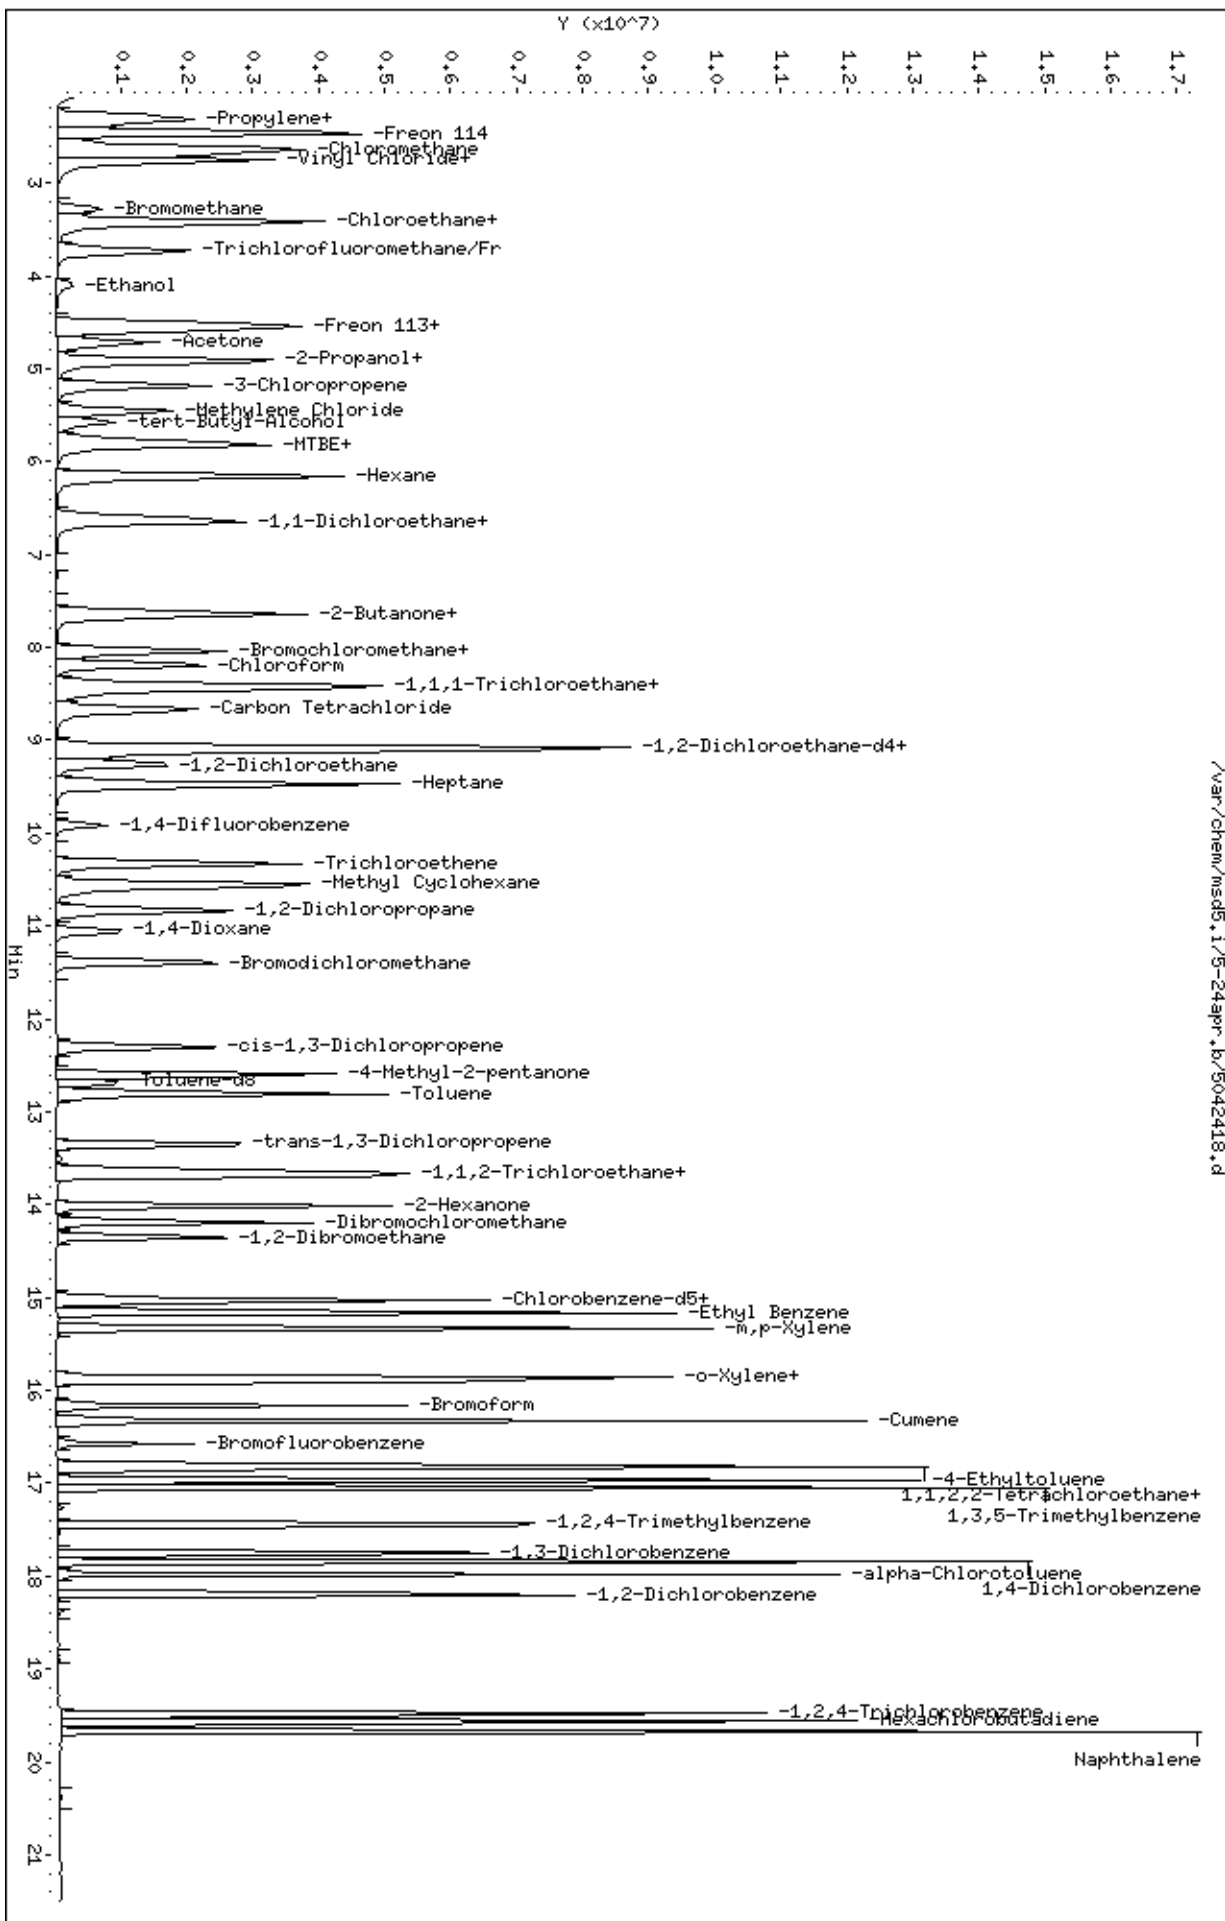

Report Date: 25-Apr-2008 09:57

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /var/chem/msd5.i/5-24apr.b/5042419.d  
 Lab Smp Id: ICAL Client Smp ID: Level 7  
 Inj Date : 24-APR-2008 16:48  
 Operator : ct Inst ID: msd5.i  
 Smp Info : 200mL #1612-1  
 Misc Info : 200ppbv -> 200ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/t14q424a.m  
 Meth Date : 25-Apr-2008 09:57 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1 Calibration Sample, Level: 7  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5								
8.059	8.059	(1.000)	130	352862	25.0000		70.00- 130.00	100.00
8.059	8.059	(1.000)	128	268957			47.51- 107.51	76.22
8.059	8.059	(1.000)	49	640070			158.47- 218.47	181.39
-----								
* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.912	9.912	(1.000)	114	1473295	25.0000		70.00- 130.00	100.00
9.912	9.912	(1.000)	88	224238			0.00- 44.75	15.22
-----								
* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	1390786	25.0000		70.00- 130.00	100.00
14.999	14.999	(1.000)	82	680691			0.00- 30.00	48.94
-----								
\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.137	9.137	(1.134)	65	483087	25.0000	26.972	70.00- 130.00	100.00
9.137	9.137	(1.134)	67	358743			0.00- 30.00	74.26
-----								
\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.704	12.704	(1.282)	98	1402148	25.0000	25.044	70.00- 130.00	100.00
12.704	12.704	(1.282)	70	130299			0.00- 30.00	9.29

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
\$ 107 Toluene-d8 (continued)										
12.704	12.704	(1.282)	100	1039657			0.00- 30.00	74.15		
-----										
\$ 138 Bromofluorobenzene										
						CAS #:	460-00-4			
16.575	16.575	(1.105)	174	862338	25.0000	25.536	70.00- 130.00	100.00		
16.575	16.575	(1.105)	95	1132134			98.07- 158.07	131.29		
16.575	16.575	(1.105)	176	830968			65.46- 125.46	96.36		
-----										
6 Propylene										
						CAS #:	115-07-1			
2.280	2.280	(0.283)	41	5107080	200.000	186.54	70.00- 130.00	100.00		
2.280	2.280	(0.283)	42	3363444			0.00- 30.00	65.86		
2.280	2.280	(0.283)	39	3561660			0.00- 30.00	69.74		
-----										
8 Dichlorodifluoromethane/Fr12										
						CAS #:	75-71-8			
2.336	2.336	(0.290)	85	9044480	200.000	206.26	70.00- 130.00	100.00(A)		
2.336	2.336	(0.290)	87	2921180			0.00- 30.00	32.30		
-----										
9 Freon 114										
						CAS #:	76-14-2			
2.474	2.474	(0.307)	135	7111706	200.000	199.09	70.00- 130.00	100.00		
2.474	2.474	(0.307)	137	2247924			2.03- 62.03	31.61		
-----										
10 Chloromethane										
						CAS #:	74-87-3			
2.640	2.640	(0.328)	50	6374787	200.000	193.44	70.00- 130.00	100.00		
2.612	2.612	(0.324)	52	1815130			0.00- 30.00	28.47		
-----										
13 Vinyl Chloride										
						CAS #:	75-01-4			
2.778	2.778	(0.345)	62	5508708	200.000	205.90	70.00- 130.00	100.00(A)		
2.778	2.778	(0.345)	64	1648992			0.00- 30.00	29.93		
-----										
12 1,3-Butadiene										
						CAS #:	106-99-0			
2.778	2.778	(0.345)	54	5158992	200.000	194.94	70.00- 130.00	100.00		
2.778	2.778	(0.345)	39	7042916			0.00- 30.00	136.52		
-----										
15 Bromomethane										
						CAS #:	74-83-9			
3.276	3.276	(0.406)	94	3276503	200.000	219.07	70.00- 130.00	100.00(A)		
3.276	3.276	(0.406)	96	3090905			62.86- 122.86	94.34		
-----										
19 Chloroethane										
						CAS #:	75-00-3			
3.442	3.442	(0.427)	64	2736428	200.000	205.95	70.00- 130.00	100.00(A)		
3.442	3.442	(0.427)	49	826850			0.00- 30.00	30.22		
3.442	3.442	(0.427)	66	801237			0.00- 30.00	29.28		
-----										
20 Trichlorofluoromethane/Fr11										
						CAS #:	75-69-4			
3.746	3.746	(0.465)	101	9192370	200.000	205.53	70.00- 130.00	100.00(A)		
3.746	3.746	(0.465)	103	5982295			33.46- 93.46	65.08		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.133	4.133	(0.513)	45	2033987	200.000	192.50	70.00- 130.00	100.00	
4.133	4.133	(0.513)	43	361341			0.00- 30.00	17.77	
4.105	4.105	(0.509)	46	823219			0.00- 30.00	40.47	
-----									
30 Freon 113						CAS #: 76-13-1			
4.548	4.548	(0.564)	151	5624864	200.000	204.13	70.00- 130.00	100.00(A)	
4.548	4.548	(0.564)	153	3574666			33.20- 93.20	63.55	
4.520	4.520	(0.561)	101	7597698			106.78- 166.78	135.07	
-----									
31 1,1-Dichloroethene						CAS #: 75-35-4			
4.575	4.575	(0.568)	61	7385705	200.000	208.70	70.00- 130.00	100.00(A)	
4.575	4.575	(0.568)	96	4072724			23.41- 83.41	55.14	
4.575	4.575	(0.568)	98	2614739			4.01- 64.01	35.40	
-----									
32 Acetone						CAS #: 67-64-1			
4.741	4.741	(0.588)	58	2738118	200.000	202.00	70.00- 130.00	100.00(A)	
4.741	4.741	(0.588)	43	8955763			0.00- 30.00	327.08	
-----									
36 2-Propanol						CAS #: 67-63-0			
4.935	4.935	(0.612)	45	10887206	200.000	212.62	70.00- 130.00	100.00(A)	
4.935	4.935	(0.612)	43	2375852			0.00- 30.00	21.82	
4.935	4.935	(0.612)	59	373309			0.00- 30.00	3.43	
-----									
35 Carbon Disulfide						CAS #: 75-15-0			
4.935	4.935	(0.612)	76	12633168	200.000	206.86	70.00- 130.00	100.00(A)	
-----									
38 3-Chloropropene						CAS #: 107-05-1			
5.211	5.211	(0.647)	76	2233511	200.000	212.61	70.00- 130.00	100.00(A)	
5.184	5.184	(0.643)	41	8775245			0.00- 30.00	392.89	
-----									
43 Methylene Chloride						CAS #: 75-09-2			
5.460	5.460	(0.678)	49	6356189	200.000	197.92	70.00- 130.00	100.00	
5.460	5.460	(0.678)	84	3614985			26.74- 86.74	56.87	
5.460	5.460	(0.678)	51	1909630			0.00- 30.00	30.04	
-----									
46 MTBE						CAS #: 1634-04-4			
5.764	5.764	(0.715)	73	6761828	200.000	220.24	70.00- 130.00	100.00(A)	
5.764	5.764	(0.715)	57	1993273			0.00- 59.41	29.48	
5.764	5.764	(0.715)	41	2156763			0.00- 30.00	31.90	
-----									
47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.819	5.819	(0.722)	96	4762530	200.000	206.61	70.00- 130.00	100.00(A)	
5.819	5.819	(0.722)	61	7581725			130.65- 190.65	159.20	
5.819	5.819	(0.722)	98	3033575			0.00- 30.00	63.70	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.151	6.151	(0.763)	57	9696208	200.000	213.84	70.00- 130.00	100.00(A)	
6.151	6.151	(0.763)	43	7062800			0.00- 30.00	72.84	
6.151	6.151	(0.763)	86	1386116			0.00- 30.00	14.30	
-----									
55 1,1-Dichloroethane						CAS #: 75-34-3			
6.594	6.594	(0.818)	63	8762075	200.000	206.05	70.00- 130.00	100.00(A)	
6.594	6.594	(0.818)	65	2628137			0.00- 59.62	29.99	
-----									
67 2-Butanone						CAS #: 78-93-3			
7.644	7.644	(0.949)	72	2345963	200.000	226.15	70.00- 130.00	100.00(A)	
7.644	7.644	(0.949)	43	12916794			533.62- 593.62	550.60	
7.644	7.644	(0.949)	57	880571			0.00- 30.00	37.54	
-----									
66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.617	7.617	(0.945)	61	6390097	200.000	208.17	70.00- 130.00	100.00(A)	
7.644	7.644	(0.949)	96	4639467			42.00- 102.00	72.60	
7.644	7.644	(0.949)	98	2977322			15.56- 75.56	46.59	
-----									
70 Tetrahydrofuran						CAS #: 109-99-9			
8.031	8.031	(0.997)	42	7721108	200.000	195.38	70.00- 130.00	100.00	
8.031	8.031	(0.997)	71	2098899			0.00- 56.55	27.18	
8.031	8.031	(0.997)	72	2287344			0.00- 30.00	29.62	
-----									
72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	7876085	200.000	193.56	70.00- 130.00	100.00	
8.197	8.197	(1.017)	85	5137314			35.57- 95.57	65.23	
-----									
75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.446	8.446	(1.048)	97	7624161	200.000	201.78	70.00- 130.00	100.00(A)	
8.446	8.446	(1.048)	99	4913489			34.21- 94.21	64.45	
-----									
74 Cyclohexane						CAS #: 110-82-7			
8.419	8.419	(1.045)	84	6424844	200.000	214.19	70.00- 130.00	100.00(A)	
8.419	8.419	(1.045)	56	9468340			117.94- 177.94	147.37	
8.419	8.419	(1.045)	41	5523951			54.92- 114.92	85.98	
-----									
56 Vinyl Acetate						CAS #: 108-05-4			
6.649	6.649	(0.825)	86	1297564	200.000	220.76	70.00- 130.00	100.00(A)	
6.649	6.649	(0.825)	43	17238605			0.00- 30.00	1328.54	
6.649	6.649	(0.825)	42	1264566			0.00- 30.00	97.46	
-----									
77 Carbon Tetrachloride						CAS #: 56-23-5			
8.667	8.667	(1.075)	119	7157412	200.000	211.60	70.00- 130.00	100.00(A)	
8.667	8.667	(1.075)	117	7386429			74.41- 134.41	103.20	
-----									



AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.110	9.110	(1.130)	57	27073929	200.000	206.94	70.00-	130.00	100.00(A)	
9.110	9.110	(1.130)	56	8885401			0.00-	30.00	32.82	
9.082	9.082	(1.127)	41	7111432			0.00-	30.00	26.27	
-----										
81	Benzene					CAS #:	71-43-2			
9.082	9.082	(0.916)	78	14174332	200.000	191.82	70.00-	130.00	100.00	
9.082	9.082	(0.916)	77	3314071			0.00-	30.00	23.38	
-----										
85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	5352598	200.000	201.29	70.00-	130.00	100.00(A)	
9.276	9.276	(0.936)	64	1685351			0.00-	30.00	31.49	
-----										
90	Heptane					CAS #:	142-82-5			
9.469	9.469	(0.955)	100	1692801	200.000	209.59	70.00-	130.00	100.00(A)	
9.469	9.469	(0.955)	43	11661836			0.00-	30.00	688.91	
9.469	9.469	(0.955)	71	5029086			0.00-	30.00	297.09	
-----										
93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	5513535	200.000	201.23	70.00-	130.00	100.00(A)	
10.326	10.326	(1.042)	130	5615613			70.08-	130.08	101.85	
10.326	10.326	(1.042)	97	3601372			35.30-	95.30	65.32	
-----										
98	1,2-Dichloropropane					CAS #:	78-87-5			
10.852	10.852	(1.095)	63	5068481	200.000	207.51	70.00-	130.00	100.00(A)	
10.852	10.852	(1.095)	62	3591431			41.10-	101.10	70.86	
10.824	10.824	(1.092)	41	3369953			35.89-	95.89	66.49	
-----										
99	1,4-Dioxane					CAS #:	123-91-1			
11.073	11.073	(1.117)	88	3254437	200.000	200.93	70.00-	130.00	100.00(A)	
11.045	11.045	(1.114)	58	2568539			47.45-	107.45	78.92	
11.045	11.045	(1.114)	57	804051			0.00-	30.00	24.71	
-----										
100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	7606196	200.000	212.70	70.00-	130.00	100.00(A)	
11.405	11.405	(1.151)	85	4928723			34.05-	94.05	64.80	
-----										
103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	6121950	200.000	218.78	70.00-	130.00	100.00(A)	
12.317	12.317	(1.243)	77	1962590			1.82-	61.82	32.06	
12.289	12.289	(1.240)	39	4121778			36.40-	96.40	67.33	
-----										
106	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.594	12.594	(1.271)	58	4375216	200.000	223.18	70.00-	130.00	100.00(A)	
12.594	12.594	(1.271)	43	12883456			0.00-	30.00	294.46	
12.594	12.594	(1.271)	85	1665949			0.00-	30.00	38.08	
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.293)	91	14715034	200.000	204.72	70.00- 130.00	100.00(A)	
12.815	12.815	(1.293)	92	8671052			27.75- 87.75	58.93	
-----									
113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	6122303	200.000	228.50	70.00- 130.00	100.00(A)	
13.368	13.368	(0.891)	77	1968332			2.38- 62.38	32.15	
13.340	13.340	(0.889)	39	4120372			35.96- 95.96	67.30	
-----									
114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	4957823	200.000	209.64	70.00- 130.00	100.00(A)	
13.644	13.644	(0.910)	99	3128935			33.83- 93.83	63.11	
13.644	13.644	(0.910)	83	4145012			52.70- 112.70	83.61	
-----									
116 Tetrachloroethene						CAS #: 127-18-4			
13.700	13.700	(0.913)	166	6542999	200.000	213.08	70.00- 130.00	100.00(A)	
13.700	13.700	(0.913)	129	4826911			44.73- 104.73	73.77	
13.700	13.700	(0.913)	131	4613990			40.60- 100.60	70.52	
-----									
119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	6243382	200.000	220.36	70.00- 130.00	100.00(A)	
14.004	14.004	(0.934)	43	13047855			181.71- 241.71	208.99	
14.004	14.004	(0.934)	100	1164686			0.00- 30.00	18.65	
-----									
120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	7876482	200.000	225.51	70.00- 130.00	100.00(A)	
14.197	14.197	(0.947)	127	6027229			0.00- 30.00	76.52	
-----									
122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	8167826	200.000	206.57	70.00- 130.00	100.00(A)	
14.363	14.363	(0.958)	109	7783744			65.00- 125.00	95.30	
-----									
126 Chlorobenzene						CAS #: 108-90-7			
15.027	15.027	(1.002)	112	11915794	200.000	211.70	70.00- 130.00	100.00(A)	
15.027	15.027	(1.002)	114	3825212			2.42- 62.42	32.10	
15.027	15.027	(1.002)	77	6622460			27.34- 87.34	55.58	
-----									
128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	6669942	200.000	214.27	70.00- 130.00	100.00(A)	
15.165	15.165	(1.011)	91	19182168			0.00- 30.00	287.59	
-----									
130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	8463274	200.000	218.67	70.00- 130.00	100.00(A)	
15.331	15.331	(1.022)	91	15951348			0.00- 30.00	188.48	
-----									
132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	7769123	200.000	214.71	70.00- 130.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	15509343			170.15- 230.15	199.63	
-----									
133 Styrene CAS #: 100-42-5									
15.912	15.912	(1.061)	104	12564258	200.000	215.53	70.00- 130.00	100.00(A)	
15.884	15.884	(1.059)	78	5530760			13.62- 73.62	44.02	
-----									
134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	7597747	200.000	226.85	70.00- 130.00	100.00(A)	
16.160	16.160	(1.077)	171	3935735			22.36- 82.36	51.80	
-----									
141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	10842623	200.000	203.37	70.00- 130.00	100.00(A)	
16.796	16.796	(1.120)	85	7047201			36.19- 96.19	65.00	
-----									
144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	20032744	200.000	183.10	70.00- 130.00	100.00	
16.962	16.962	(1.131)	120	7434755			0.17- 60.17	37.11	
-----									
147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	16255633	200.000	166.97	70.00- 130.00	100.00	
17.045	17.045	(1.136)	120	10370188			0.00- 30.00	63.79	
-----									
152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	17824050	200.000	218.16	70.00- 130.00	100.00(A)	
17.460	17.460	(1.164)	120	8503418			17.48- 77.48	47.71	
-----									
155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	12064563	200.000	212.66	70.00- 130.00	100.00(A)	
17.764	17.764	(1.184)	148	7653912			0.00- 30.00	63.44	
17.764	17.764	(1.184)	111	4515582			0.00- 30.00	37.43	
-----									
156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	14810772	200.000	207.31	70.00- 130.00	100.00(A)	
17.847	17.847	(1.190)	148	9446744			0.00- 30.00	63.78	
17.847	17.847	(1.190)	111	5597817			0.00- 30.00	37.80	
-----									
157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	14878836	200.000	185.10	70.00- 130.00	100.00	
17.985	17.985	(1.199)	126	4649264			0.00- 30.00	31.25	
-----									
159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	11783737	200.000	202.50	70.00- 130.00	100.00(A)	
18.206	18.206	(1.214)	148	7589145			32.26- 92.26	64.40	
18.206	18.206	(1.214)	111	4450169			7.92- 67.92	37.77	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
163	1,2,4-Trichlorobenzene						CAS #: 120-82-1		
19.478	19.478	(1.299)	180	8677009	200.000	202.74	70.00- 130.00	100.00(A)	
19.478	19.478	(1.299)	182	8215187			63.09- 123.09	94.68	
-----									
164	Hexachlorobutadiene						CAS #: 87-68-3		
19.589	19.589	(1.306)	225	5938360	200.000	205.66	70.00- 130.00	100.00(A)	
19.589	19.589	(1.306)	223	3675205			32.88- 92.88	61.89	
-----									
142	Propylbenzene						CAS #: 103-65-1		
16.824	16.824	(1.122)	91	21934020	200.000	181.61	70.00- 130.00	100.00	
16.824	16.824	(1.122)	120	6278971			0.00- 30.00	28.63	
16.824	16.824	(1.122)	105	966431			0.00- 30.00	4.41	
-----									
136	Cumene						CAS #: 98-82-8		
16.326	16.326	(1.088)	105	18215849	200.000	167.78	70.00- 130.00	100.00	
16.326	16.326	(1.088)	120	6300885			0.00- 30.00	34.59	
16.326	16.326	(1.088)	51	2546769			0.00- 30.00	13.98	
-----									
165	Naphthalene						CAS #: 91-20-3		
19.672	19.672	(1.312)	128	15192378	200.000	110.81	70.00- 130.00	100.00	
19.672	19.672	(1.312)	127	3972851			0.00- 30.00	26.15	
-----									
37	tert-Butyl-Alcohol						CAS #: 75-65-0		
5.571	5.571	(0.691)	59	3661067	200.000	139.58	70.00- 130.00	100.00	
5.571	5.571	(0.691)	41	1129400			0.00- 30.00	30.85	
5.571	5.571	(0.691)	57	369514			0.00- 30.00	10.09	
-----									
11	Butane						CAS #: 106-97-8		
2.695	2.695	(0.334)	58	1333404	200.000	187.10	70.00- 130.00	100.00	
2.695	2.695	(0.334)	43	11208143			0.00- 30.00	840.57	
-----									
17	Isopentane						CAS #: 78-78-4		
3.414	3.414	(0.424)	43	8738867	200.000	197.86	70.00- 130.00	100.00	
3.414	3.414	(0.424)	57	5087014			0.00- 30.00	58.21	
3.414	3.414	(0.424)	72	465640			0.00- 30.00	5.33	
-----									
94	Methyl Cyclohexane						CAS #: 108-87-2		
10.548	10.548	(1.064)	83	8327997	200.000	206.14	70.00- 130.00	100.00(A)	
10.575	10.575	(1.067)	98	4021726			0.00- 30.00	48.29	
10.548	10.548	(1.064)	55	7780951			0.00- 30.00	93.43	
-----									

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 25-Apr-2008 09:57

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 24-APR-2008

Lab File ID: 5042419.d

Calibration Time: 15:47

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: ct

Method File: /var/chem/msd5.i/5-24apr.b/t14q424a.m

Misc Info: 200ppbv -&gt; 200ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	296697	178018	415376	352862	18.93
92 1,4-Difluorobenze	1234462	740677	1728247	1473295	19.35
125 Chlorobenzene-d5	1186736	712042	1661430	1390786	17.19

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.91	9.58	10.24	9.91	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /var/chem/msd5.1/5-24apr.lb/5042419.d  
 Date: 24-APR-2008 16:48  
 Client ID: Level 7  
 Sample Info: 2000ML #1612-1

Column phase: RTX-624

Instrument: msd5.1  
 Operator: ct  
 Column diameter: 0.53

/var/chem/msd5.1/5-24apr.lb/5042419.d





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0804565-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050202	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 5/2/08 07:55 AM

Compound	%Recovery
Freon 12	86
Freon 114	120
Vinyl Chloride	112
Bromomethane	122
Chloroethane	112
Freon 11	104
1,1-Dichloroethene	96
Freon 113	120
Methylene Chloride	90
1,1-Dichloroethane	91
cis-1,2-Dichloroethene	88
Chloroform	83
1,1,1-Trichloroethane	84
Carbon Tetrachloride	90
Benzene	87
1,2-Dichloroethane	93
Trichloroethene	91
1,2-Dichloropropane	83
cis-1,3-Dichloropropene	88
Toluene	87
trans-1,3-Dichloropropene	100
1,1,2-Trichloroethane	99
Tetrachloroethene	113
1,2-Dibromoethane (EDB)	98
Chlorobenzene	101
Ethyl Benzene	103
m,p-Xylene	101
o-Xylene	100
Styrene	101
1,1,2,2-Tetrachloroethane	92
1,3,5-Trimethylbenzene	102
1,2,4-Trimethylbenzene	101
1,3-Dichlorobenzene	109
1,4-Dichlorobenzene	106
alpha-Chlorotoluene	117
1,2-Dichlorobenzene	107
1,3-Butadiene	101
Hexane	96
Cyclohexane	91



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0804565-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050202	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 5/2/08 07:55 AM

Compound	%Recovery
Heptane	98
Bromodichloromethane	91
Dibromochloromethane	107
Cumene	99
Propylbenzene	98
Chloromethane	94
1,2,4-Trichlorobenzene	109
Hexachlorobutadiene	111
Acetone	96
Carbon Disulfide	108
2-Propanol	93
trans-1,2-Dichloroethene	108
2-Butanone (Methyl Ethyl Ketone)	94
Tetrahydrofuran	81
1,4-Dioxane	86
4-Methyl-2-pentanone	88
2-Hexanone	92
Bromoform	113
4-Ethyltoluene	102
Ethanol	105
Methyl tert-butyl ether	95
3-Chloropropene	105
2,2,4-Trimethylpentane	84
Naphthalene	114

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	90	70-130
1,2-Dichloroethane-d4	87	70-130
4-Bromofluorobenzene	110	70-130



Report Date: 02-May-2008 08:09

## Air Toxics Ltd.

## CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i                      Injection Date: 02-MAY-2008 07:55  
 Lab File ID: 5050202.d                    Init. Cal. Date(s): 24-APR-2008 24-APR-2008  
 Analysis Type: AIR                         Init. Cal. Times: 13:56 18:31  
 Lab Sample ID: CCV-1                      Quant Type: ISTD  
 Method: /var/chem/msd5.i/5-02may.b/t14q424a.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 84 1,2-Dichloroethane-d4	1.26895	1.10276	0.010	13.09663	30.00000	Averaged
\$ 107 Toluene-d8	0.95003	0.85060	0.010	10.46592	30.00000	Averaged
\$ 138 Bromofluorobenzene	0.60703	0.66864	0.010	-10.14959	30.00000	Averaged
6 Propylene	1.93970	1.81121	0.010	6.62435	30.00000	Averaged
8 Dichlorodifluoromethane/Fr1	3.10671	2.67927	0.010	13.75856	30.00000	Averaged
9 Freon 114	2.53080	3.03194	0.010	-19.80162	30.00000	Averaged
10 Chloromethane	2.33479	2.19110	0.010	6.15441	30.00000	Averaged
13 Vinyl Chloride	1.89555	2.13248	0.010	-12.49956	30.00000	Averaged
12 1,3-Butadiene	1.87495	1.89032	0.010	-0.81979	30.00000	Averaged
15 Bromomethane	1.05964	1.29863	0.010	-22.55365	30.00000	Averaged
19 Chloroethane	0.94135	1.05947	0.010	-12.54800	30.00000	Averaged
20 Trichlorofluoromethane/Fr11	3.16868	3.28673	0.010	-3.72546	30.00000	Averaged
26 Ethanol	0.74860	0.78446	0.010	-4.78954	30.00000	Averaged
30 Freon 113	1.95225	2.33372	0.010	-19.54025	30.00000	Averaged
31 1,1-Dichloroethene	2.50732	2.40986	0.010	3.88704	30.00000	Averaged
32 Acetone	0.96038	0.92695	0.010	3.48085	30.00000	Averaged
36 2-Propanol	3.62782	3.38632	0.010	6.65697	30.00000	Averaged
35 Carbon Disulfide	4.32685	4.66662	0.010	-7.85262	30.00000	Averaged
38 3-Chloropropene	0.74428	0.78447	0.010	-5.39963	30.00000	Averaged
43 Methylene Chloride	2.27526	2.04754	0.010	10.00840	30.00000	Averaged
46 MTBE	2.17525	2.06827	0.010	4.91820	30.00000	Averaged
47 trans-1,2-Dichloroethene	1.63316	1.75990	0.010	-7.76032	30.00000	Averaged
51 Hexane	3.21249	3.08095	0.010	4.09469	30.00000	Averaged
56 Vinyl Acetate	0.41643	0.42263	0.010	-1.48808	30.00000	Averaged
55 1,1-Dichloroethane	3.01285	2.74006	0.010	9.05429	30.00000	Averaged
67 2-Butanone	0.73496	0.69448	0.010	5.50806	30.00000	Averaged
66 cis-1,2-Dichloroethene	2.17486	1.91990	0.010	11.72281	30.00000	Averaged
70 Tetrahydrofuran	2.79990	2.27042	0.010	18.91100	30.00000	Averaged
72 Chloroform	2.88290	2.38241	0.010	17.36068	30.00000	Averaged
75 1,1,1-Trichloroethane	2.67702	2.24976	0.010	15.96038	30.00000	Averaged
74 Cyclohexane	2.12515	1.94428	0.010	8.51120	30.00000	Averaged
77 Carbon Tetrachloride	2.39650	2.15364	0.010	10.13372	30.00000	Averaged
80 2,2,4-Trimethylpentane	9.26895	7.74528	0.010	16.43848	30.00000	Averaged
81 Benzene	1.25391	1.08837	0.010	13.20228	30.00000	Averaged
85 1,2-Dichloroethane	0.45123	0.42105	0.010	6.68738	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i                      Injection Date: 02-MAY-2008 07:55  
 Lab File ID: 5050202.d                    Init. Cal. Date(s): 24-APR-2008 24-APR-2008  
 Analysis Type: AIR                         Init. Cal. Times: 13:56 18:31  
 Lab Sample ID: CCV-1                      Quant Type: ISTD  
 Method: /var/chem/msd5.i/5-02may.b/t14q424a.m

COMPOUND	RRF / AMOUNT	RF50	MIN RRF	%D / %DRIFT	MAX %D / %DRIFT	CURVE TYPE
90 Heptane	0.13705	0.13458	0.010	1.80120	30.00000	Averaged
93 Trichloroethene	0.46494	0.42226	0.010	9.17860	30.00000	Averaged
98 1,2-Dichloropropane	0.41447	0.34523	0.010	16.70621	30.00000	Averaged
99 1,4-Dioxane	0.27484	0.23704	0.010	13.75434	30.00000	Averaged
100 Bromodichloromethane	0.60680	0.55222	0.010	8.99565	30.00000	Averaged
103 cis-1,3-Dichloropropene	0.47482	0.41732	0.010	12.10891	30.00000	Averaged
106 4-Methyl-2-pentanone	0.33266	0.29317	0.010	11.87192	30.00000	Averaged
108 Toluene	1.21969	1.06356	0.010	12.80037	30.00000	Averaged
113 trans-1,3-Dichloropropene	0.48163	0.48109	0.010	0.11256	30.00000	Averaged
114 1,1,2-Trichloroethane	0.42511	0.41947	0.010	1.32697	30.00000	Averaged
116 Tetrachloroethene	0.55196	0.62588	0.010	-13.39192	30.00000	Averaged
119 2-Hexanone	0.50928	0.46842	0.010	8.02329	30.00000	Averaged
120 Dibromochloromethane	0.62784	0.67089	0.010	-6.85663	30.00000	Averaged
122 1,2-Dibromoethane	0.71076	0.69330	0.010	2.45627	30.00000	Averaged
126 Chlorobenzene	1.01178	1.02665	0.010	-1.47012	30.00000	Averaged
128 Ethyl Benzene	0.55955	0.57821	0.010	-3.33412	30.00000	Averaged
130 m,p-Xylene	0.69572	0.70019	0.010	-0.64292	30.00000	Averaged
132 o-Xylene	0.65043	0.65138	0.010	-0.14601	30.00000	Averaged
133 Styrene	1.04786	1.05820	0.010	-0.98670	30.00000	Averaged
134 Bromoform	0.60204	0.67950	0.010	-12.86620	30.00000	Averaged
141 1,1,2,2-Tetrachloroethane	0.95835	0.87716	0.010	8.47147	30.00000	Averaged
144 4-Ethyltoluene	1.96672	2.00260	0.010	-1.82447	30.00000	Averaged
147 1,3,5-Trimethylbenzene	1.75006	1.78352	0.010	-1.91183	30.00000	Averaged
152 1,2,4-Trimethylbenzene	1.46865	1.47923	0.010	-0.72094	30.00000	Averaged
155 1,3-Dichlorobenzene	1.01978	1.10942	0.010	-8.79014	30.00000	Averaged
156 1,4-Dichlorobenzene	1.28420	1.35994	0.010	-5.89732	30.00000	Averaged
157 alpha-Chlorotoluene	1.44493	1.69363	0.010	-17.21205	30.00000	Averaged
159 1,2-Dichlorobenzene	1.04603	1.12159	0.010	-7.22389	30.00000	Averaged
163 1,2,4-Trichlorobenzene	0.76931	0.84220	0.010	-9.47511	30.00000	Averaged
164 Hexachlorobutadiene	0.51903	0.57675	0.010	-11.11923	30.00000	Averaged
142 Propylbenzene	2.17097	2.11750	0.010	2.46290	30.00000	Averaged
136 Cumene	1.95163	1.93660	0.010	0.76976	30.00000	Averaged
165 Naphthalene	2.46443	2.82351	0.010	-14.57078	30.00000	Averaged
37 tert-Butyl-Alcohol	1.85830	1.49987	0.010	19.28812	40.00000	Averaged
11 Butane	0.50491	0.49744	0.010	1.47874	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msd5.i                    Injection Date: 02-MAY-2008 07:55  
Lab File ID: 5050202.d                Init. Cal. Date(s): 24-APR-2008 24-APR-2008  
Analysis Type: AIR                    Init. Cal. Times: 13:56                    18:31  
Lab Sample ID: CCV-1                  Quant Type: ISTD  
Method: /var/chem/msd5.i/5-02may.b/t14q424a.m

COMPOUND	RRF / AMOUNT	RF50	MIN	MAX	CURVE TYPE	
17 Isopentane	3.12912	3.07046	0.010	1.87464	30.00000	Averaged
94 Methyl Cyclohexane	0.68552	0.60128	0.010	12.28905	30.00000	Averaged

Report Date: 02-May-2008 08:09

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-02may.b/5050202.d  
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1  
 Inj Date : 02-MAY-2008 07:55  
 Operator : kr Inst ID: msd5.i  
 Smp Info : 50mL #1612-1  
 Misc Info : 200ppbv -> 50ppbv  
 Comment :  
 Method : /var/chem/msd5.i/5-02may.b/t14q424a.m  
 Meth Date : 02-May-2008 08:09 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1 Continuing Calibration Sample  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
* 71 Bromochloromethane CAS #: 74-97-5								
8.059	8.059	(1.000)	130	339808	25.0000		80.00- 120.00	100.00
8.059	8.059	(1.000)	128	274801			50.87- 110.87	80.87
8.059	8.059	(1.000)	49	542292			129.59- 189.59	159.59
-----								
* 92 1,4-Difluorobenzene CAS #: 540-36-3								
9.939	9.939	(1.000)	114	1321223	25.0000		80.00- 120.00	100.00
9.912	9.912	(1.000)	88	181226			0.00- 43.72	13.72
-----								
* 125 Chlorobenzene-d5 CAS #: 3114-55-4								
14.999	14.999	(1.000)	117	1146934	25.0000		80.00- 120.00	100.00
14.999	14.999	(1.000)	82	537132			0.00- 30.00	46.83
-----								
\$ 84 1,2-Dichloroethane-d4 CAS #: 17060-07-0								
9.137	9.137	(1.134)	65	374725	25.0000	21.726	80.00- 120.00	100.00
9.137	9.137	(1.134)	67	218013			0.00- 30.00	58.18
-----								
\$ 107 Toluene-d8 CAS #: 2037-26-5								
12.704	12.704	(1.278)	98	1123833	25.0000	22.384	80.00- 120.00	100.00
12.704	12.704	(1.278)	70	100809			0.00- 30.00	8.97

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 107 Toluene-d8 (continued)									
12.704	12.704	(1.278)	100	795724			0.00- 30.00	70.80	
-----									
\$ 138 Bromofluorobenzene									
						CAS #: 460-00-4			
16.575	16.575	(1.105)	174	766890	25.0000	27.537	80.00- 120.00	100.00	
16.575	16.575	(1.105)	95	843524			79.99- 139.99	109.99	
16.575	16.575	(1.105)	176	726014			64.67- 124.67	94.67	
-----									
6 Propylene									
						CAS #: 115-07-1			
2.308	2.308	(0.286)	41	1230926	50.0000	46.688	80.00- 120.00	100.00	
2.308	2.308	(0.286)	42	819417			0.00- 30.00	66.57	
2.308	2.308	(0.286)	39	836154			0.00- 30.00	67.93	
-----									
8 Dichlorodifluoromethane/Fr12									
						CAS #: 75-71-8			
2.363	2.363	(0.293)	85	1820880	50.0000	43.121	80.00- 120.00	100.00	
2.363	2.363	(0.293)	87	592037			0.00- 30.00	32.51	
-----									
9 Freon 114									
						CAS #: 76-14-2			
2.474	2.474	(0.307)	135	2060557	50.0000	59.901	80.00- 120.00	100.00	
2.474	2.474	(0.307)	137	647849			1.44- 61.44	31.44	
-----									
10 Chloromethane									
						CAS #: 74-87-3			
2.612	2.612	(0.324)	50	1489107	50.0000	46.923	80.00- 120.00	100.00	
2.612	2.612	(0.324)	52	432615			0.00- 30.00	29.05	
-----									
13 Vinyl Chloride									
						CAS #: 75-01-4			
2.806	2.806	(0.348)	62	1449270	50.0000	56.250	80.00- 120.00	100.00	
2.806	2.806	(0.348)	64	440997			0.00- 30.00	30.43	
-----									
12 1,3-Butadiene									
						CAS #: 106-99-0			
2.778	2.778	(0.345)	54	1284693	50.0000	50.410	80.00- 120.00	100.00	
2.778	2.778	(0.345)	39	1499492			0.00- 30.00	116.72	
-----									
15 Bromomethane									
						CAS #: 74-83-9			
3.303	3.303	(0.410)	94	882571	50.0000	61.277	80.00- 120.00	100.00	
3.303	3.303	(0.410)	96	845424			65.79- 125.79	95.79	
-----									
19 Chloroethane									
						CAS #: 75-00-3			
3.442	3.442	(0.427)	64	720034	50.0000	56.274	80.00- 120.00	100.00	
3.442	3.442	(0.427)	49	205085			0.00- 30.00	28.48	
3.442	3.442	(0.427)	66	225163			0.00- 30.00	31.27	
-----									
20 Trichlorofluoromethane/Fr11									
						CAS #: 75-69-4			
3.746	3.746	(0.465)	101	2233715	50.0000	51.863	80.00- 120.00	100.00	
3.746	3.746	(0.465)	103	1481384			36.32- 96.32	66.32	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
26 Ethanol						CAS #: 64-17-5			
4.105	4.105	(0.509)	45	533129	50.0000	52.395	80.00- 120.00	100.00	
4.105	4.105	(0.509)	43	99607			0.00- 30.00	18.68	
4.105	4.105	(0.509)	46	216737			0.00- 30.00	40.65	
-----									
30 Freon 113						CAS #: 76-13-1			
4.548	4.548	(0.564)	151	1586037	50.0000	59.770	80.00- 120.00	100.00	
4.548	4.548	(0.564)	153	1005557			33.40- 93.40	63.40	
4.548	4.548	(0.564)	101	1977134			94.66- 154.66	124.66	
-----									
31 1,1-Dichloroethene						CAS #: 75-35-4			
4.603	4.603	(0.571)	61	1637780	50.0000	48.056	80.00- 120.00	100.00	
4.603	4.603	(0.571)	96	1046165			33.88- 93.88	63.88	
4.603	4.603	(0.571)	98	675071			11.22- 71.22	41.22	
-----									
32 Acetone						CAS #: 67-64-1			
4.741	4.741	(0.588)	58	629972	50.0000	48.260	80.00- 120.00	100.00	
4.741	4.741	(0.588)	43	1943357			0.00- 30.00	308.48	
-----									
36 2-Propanol						CAS #: 67-63-0			
4.935	4.935	(0.612)	45	2301399	50.0000	46.672	80.00- 120.00	100.00	
4.935	4.935	(0.612)	43	494009			0.00- 30.00	21.47	
4.935	4.935	(0.612)	59	81223			0.00- 30.00	3.53	
-----									
35 Carbon Disulfide						CAS #: 75-15-0			
4.935	4.935	(0.612)	76	3171515	50.0000	53.926	80.00- 120.00	100.00	
-----									
38 3-Chloropropene						CAS #: 107-05-1			
5.211	5.211	(0.647)	76	533139	50.0000	52.700	80.00- 120.00	100.00	
5.211	5.211	(0.647)	41	1897580			0.00- 30.00	355.93	
-----									
43 Methylene Chloride						CAS #: 75-09-2			
5.460	5.460	(0.677)	49	1391544	50.0000	44.996	80.00- 120.00	100.00	
5.460	5.460	(0.677)	84	893082			34.18- 94.18	64.18	
5.460	5.460	(0.677)	51	424173			0.00- 30.00	30.48	
-----									
46 MTBE						CAS #: 1634-04-4			
5.792	5.792	(0.719)	73	1405628	50.0000	47.541	80.00- 120.00	100.00	
5.792	5.792	(0.719)	57	400205			0.00- 58.47	28.47	
5.792	5.792	(0.719)	41	452209			0.00- 30.00	32.17	
-----									
47 trans-1,2-Dichloroethene						CAS #: 156-60-5			
5.847	5.847	(0.726)	96	1196057	50.0000	53.880	80.00- 120.00	100.00	
5.847	5.847	(0.726)	61	1624479			105.82- 165.82	135.82	
5.847	5.847	(0.726)	98	766053			0.00- 30.00	64.05	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
51 Hexane						CAS #: 110-54-3			
6.179	6.179	(0.767)	57	2093863	50.0000	47.953	80.00- 120.00	100.00	
6.179	6.179	(0.767)	43	1494992			0.00- 30.00	71.40	
6.179	6.179	(0.767)	86	332491			0.00- 30.00	15.88	
-----									
56 Vinyl Acetate						CAS #: 108-05-4			
6.677	6.677	(0.828)	86	287226	50.0000	50.744	80.00- 120.00	100.00	
6.677	6.677	(0.828)	43	3402219			0.00- 30.00	1184.51	
6.677	6.677	(0.828)	42	261561			0.00- 30.00	91.06	
-----									
55 1,1-Dichloroethane						CAS #: 75-34-3			
6.621	6.621	(0.822)	63	1862190	50.0000	45.473	80.00- 120.00	100.00	
6.621	6.621	(0.822)	65	548098			0.00- 59.43	29.43	
-----									
67 2-Butanone						CAS #: 78-93-3			
7.672	7.672	(0.952)	72	471980	50.0000	47.246	80.00- 120.00	100.00	
7.672	7.672	(0.952)	43	2504874			500.72- 560.72	530.72	
7.672	7.672	(0.952)	57	166620			0.00- 30.00	35.30	
-----									
66 cis-1,2-Dichloroethene						CAS #: 156-59-2			
7.644	7.644	(0.949)	61	1304798	50.0000	44.138	80.00- 120.00	100.00	
7.644	7.644	(0.949)	96	1055097			50.86- 110.86	80.86	
7.644	7.644	(0.949)	98	682162			22.28- 82.28	52.28	
-----									
70 Tetrahydrofuran						CAS #: 109-99-9			
8.059	8.059	(1.000)	42	1543012	50.0000	40.544	80.00- 120.00	100.00	
8.059	8.059	(1.000)	71	443682			0.00- 58.75	28.75	
8.059	8.059	(1.000)	72	483338			0.00- 30.00	31.32	
-----									
72 Chloroform						CAS #: 67-66-3			
8.197	8.197	(1.017)	83	1619126	50.0000	41.320	80.00- 120.00	100.00	
8.197	8.197	(1.017)	85	1052501			35.00- 95.00	65.00	
-----									
75 1,1,1-Trichloroethane						CAS #: 71-55-6			
8.446	8.446	(1.048)	97	1528972	50.0000	42.020	80.00- 120.00	100.00	
8.446	8.446	(1.048)	99	1017181			36.53- 96.53	66.53	
-----									
74 Cyclohexane						CAS #: 110-82-7			
8.418	8.418	(1.045)	84	1321363	50.0000	45.744	80.00- 120.00	100.00	
8.418	8.418	(1.045)	56	1801287			106.32- 166.32	136.32	
8.418	8.418	(1.045)	41	1067481			50.79- 110.79	80.79	
-----									
77 Carbon Tetrachloride						CAS #: 56-23-5			
8.695	8.695	(1.079)	119	1463653	50.0000	44.933	80.00- 120.00	100.00	
8.695	8.695	(1.079)	117	1516431			73.61- 133.61	103.61	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.110	9.110	(1.130)	57	5263822	50.0000	41.781	80.00- 120.00	100.00		
9.110	9.110	(1.130)	56	1723311			0.00- 30.00	32.74		
9.110	9.110	(1.130)	41	1463042			0.00- 30.00	27.79		
-----										
81	Benzene					CAS #: 71-43-2				
9.110	9.110	(0.917)	78	2875949	50.0000	43.399	80.00- 120.00	100.00		
9.110	9.110	(0.917)	77	684905			0.00- 30.00	23.81		
-----										
85	1,2-Dichloroethane					CAS #: 107-06-2				
9.276	9.276	(0.933)	62	1112614	50.0000	46.656	80.00- 120.00	100.00		
9.276	9.276	(0.933)	64	331330			0.00- 30.00	29.78		
-----										
90	Heptane					CAS #: 142-82-5				
9.497	9.497	(0.955)	100	355624	50.0000	49.099	80.00- 120.00	100.00		
9.497	9.497	(0.955)	43	2212339			0.00- 30.00	622.10		
9.497	9.497	(0.955)	71	953263			0.00- 30.00	268.05		
-----										
93	Trichloroethene					CAS #: 79-01-6				
10.326	10.326	(1.039)	95	1115803	50.0000	45.411	80.00- 120.00	100.00		
10.354	10.354	(1.042)	130	1251078			82.12- 142.12	112.12		
10.326	10.326	(1.039)	97	724508			34.93- 94.93	64.93		
-----										
98	1,2-Dichloropropane					CAS #: 78-87-5				
10.852	10.852	(1.092)	63	912244	50.0000	41.647	80.00- 120.00	100.00		
10.852	10.852	(1.092)	62	655904			41.90- 101.90	71.90		
10.852	10.852	(1.092)	41	685283			45.12- 105.12	75.12		
-----										
99	1,4-Dioxane					CAS #: 123-91-1				
11.073	11.073	(1.114)	88	626358	50.0000	43.123	80.00- 120.00	100.00		
11.073	11.073	(1.114)	58	480608			46.73- 106.73	76.73		
11.073	11.073	(1.114)	57	152120			0.00- 30.00	24.29		
-----										
100	Bromodichloromethane					CAS #: 75-27-4				
11.405	11.405	(1.147)	83	1459208	50.0000	45.502	80.00- 120.00	100.00		
11.405	11.405	(1.147)	85	954332			35.40- 95.40	65.40		
-----										
103	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.317	12.317	(1.239)	75	1102749	50.0000	43.946	80.00- 120.00	100.00		
12.317	12.317	(1.239)	77	360015			2.65- 62.65	32.65		
12.317	12.317	(1.239)	39	823224			44.65- 104.65	74.65		
-----										
106	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.594	12.594	(1.267)	58	774680	50.0000	44.064	80.00- 120.00	100.00		
12.594	12.594	(1.267)	43	2336334			0.00- 30.00	301.59		
12.594	12.594	(1.267)	85	309381			0.00- 30.00	39.94		
-----										



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
108 Toluene						CAS #: 108-88-3			
12.815	12.815	(1.289)	91	2810404	50.0000	43.600	80.00- 120.00	100.00	
12.815	12.815	(1.289)	92	1678966			29.74- 89.74	59.74	
-----									
113 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.368	13.368	(0.891)	75	1103548	50.0000	49.944	80.00- 120.00	100.00	
13.368	13.368	(0.891)	77	369144			3.45- 63.45	33.45	
13.368	13.368	(0.891)	39	786645			41.28- 101.28	71.28	
-----									
114 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.644	13.644	(0.910)	97	962215	50.0000	49.336	80.00- 120.00	100.00	
13.644	13.644	(0.910)	99	610707			33.47- 93.47	63.47	
13.644	13.644	(0.910)	83	773435			50.38- 110.38	80.38	
-----									
116 Tetrachloroethene						CAS #: 127-18-4			
13.700	13.700	(0.913)	166	1435690	50.0000	56.696	80.00- 120.00	100.00	
13.700	13.700	(0.913)	129	1000451			39.68- 99.68	69.68	
13.700	13.700	(0.913)	131	971717			37.68- 97.68	67.68	
-----									
119 2-Hexanone						CAS #: 591-78-6			
14.004	14.004	(0.934)	58	1074491	50.0000	45.988	80.00- 120.00	100.00	
14.004	14.004	(0.934)	43	2300666			184.12- 244.12	214.12	
14.031	14.031	(0.935)	100	213094			0.00- 30.00	19.83	
-----									
120 Dibromochloromethane						CAS #: 124-48-1			
14.197	14.197	(0.947)	129	1538929	50.0000	53.428	80.00- 120.00	100.00	
14.197	14.197	(0.947)	127	1197305			0.00- 30.00	77.80	
-----									
122 1,2-Dibromoethane						CAS #: 106-93-4			
14.363	14.363	(0.958)	107	1590337	50.0000	48.772	80.00- 120.00	100.00	
14.363	14.363	(0.958)	109	1531149			66.28- 126.28	96.28	
-----									
126 Chlorobenzene						CAS #: 108-90-7			
15.054	15.054	(1.004)	112	2355011	50.0000	50.735	80.00- 120.00	100.00	
15.054	15.054	(1.004)	114	760666			2.30- 62.30	32.30	
15.027	15.027	(1.002)	77	1237929			22.57- 82.57	52.57	
-----									
128 Ethyl Benzene						CAS #: 100-41-4			
15.165	15.165	(1.011)	106	1326330	50.0000	51.667	80.00- 120.00	100.00	
15.165	15.165	(1.011)	91	3809297			0.00- 30.00	287.21	
-----									
130 m,p-Xylene						CAS #: 108-38-3			
15.331	15.331	(1.022)	106	1606154	50.0000	50.321	80.00- 120.00	100.00	
15.331	15.331	(1.022)	91	2991377			0.00- 30.00	186.24	
-----									
132 o-Xylene						CAS #: 95-47-6			
15.856	15.856	(1.057)	106	1494173	50.0000	50.073	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT (PPEV)	ON-COL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	2921261			165.51- 225.51	195.51	
-----									
133 Styrene CAS #: 100-42-5									
15.911	15.911	(1.061)	104	2427365	50.0000	50.493	80.00- 120.00	100.00	
15.911	15.911	(1.061)	78	1047145			13.14- 73.14	43.14	
-----									
134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1558685	50.0000	56.433	80.00- 120.00	100.00	
16.160	16.160	(1.077)	171	807538			21.81- 81.81	51.81	
-----									
141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	2012098	50.0000	45.764	80.00- 120.00	100.00	
16.796	16.796	(1.120)	85	1306112			34.91- 94.91	64.91	
-----									
144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	4593711	50.0000	50.912	80.00- 120.00	100.00	
16.962	16.962	(1.131)	120	1449634			1.56- 61.56	31.56	
-----									
147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	4091167	50.0000	50.956	80.00- 120.00	100.00	
17.045	17.045	(1.136)	120	2119446			0.00- 30.00	51.81	
-----									
152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	3393167	50.0000	50.360	80.00- 120.00	100.00	
17.460	17.460	(1.164)	120	1701193			20.14- 80.14	50.14	
-----									
155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	2544872	50.0000	54.395	80.00- 120.00	100.00	
17.764	17.764	(1.184)	148	1652259			0.00- 30.00	64.93	
17.764	17.764	(1.184)	111	907035			0.00- 30.00	35.64	
-----									
156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	3119514	50.0000	52.949	80.00- 120.00	100.00	
17.847	17.847	(1.190)	148	2004270			0.00- 30.00	64.25	
17.847	17.847	(1.190)	111	1135476			0.00- 30.00	36.40	
-----									
157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	3884966	50.0000	58.606	80.00- 120.00	100.00	
17.985	17.985	(1.199)	126	899725			0.00- 30.00	23.16	
-----									
159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	2572787	50.0000	53.612	80.00- 120.00	100.00	
18.206	18.206	(1.214)	148	1663019			34.64- 94.64	64.64	
18.206	18.206	(1.214)	111	925952			5.99- 65.99	35.99	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
163	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
19.506	19.506	(1.300)	180	1931905	50.0000	54.738	80.00- 120.00	100.00	
19.506	19.506	(1.300)	182	1800010			63.17- 123.17	93.17	
-----									
164	Hexachlorobutadiene					CAS #: 87-68-3			
19.589	19.589	(1.306)	225	1322982	50.0000	55.560	80.00- 120.00	100.00	
19.589	19.589	(1.306)	223	841257			33.59- 93.59	63.59	
-----									
142	Propylbenzene					CAS #: 103-65-1			
16.824	16.824	(1.122)	91	4857266	50.0000	48.768	80.00- 120.00	100.00	
16.824	16.824	(1.122)	120	1244170			0.00- 30.00	25.61	
16.824	16.824	(1.122)	105	182705			0.00- 30.00	3.76	
-----									
136	Cumene					CAS #: 98-82-8			
16.326	16.326	(1.088)	105	4442312	50.0000	49.615	80.00- 120.00	100.00	
16.326	16.326	(1.088)	120	1261943			0.00- 30.00	28.41	
16.326	16.326	(1.088)	51	472841			0.00- 30.00	10.64	
-----									
165	Naphthalene					CAS #: 91-20-3			
19.672	19.672	(1.312)	128	6476769	50.0000	57.285	80.00- 120.00	100.00	
19.672	19.672	(1.312)	127	798966			0.00- 30.00	12.34	
-----									
37	tert-Butyl-Alcohol					CAS #: 75-65-0			
5.598	5.598	(0.695)	59	1019336	50.0000	40.356	80.00- 120.00	100.00	
5.598	5.598	(0.695)	41	290826			0.00- 30.00	28.53	
5.598	5.598	(0.695)	57	99473			0.00- 30.00	9.76	
-----									
11	Butane					CAS #: 106-97-8			
2.695	2.695	(0.334)	58	338069	50.0000	49.261	80.00- 120.00	100.00	
2.695	2.695	(0.334)	43	2752077			0.00- 30.00	814.06	
-----									
17	Isopentane					CAS #: 78-78-4			
3.442	3.442	(0.427)	43	2086733	50.0000	49.063	80.00- 120.00	100.00	
3.442	3.442	(0.427)	57	1308875			0.00- 30.00	62.72	
3.442	3.442	(0.427)	72	131795			0.00- 30.00	6.32	
-----									
94	Methyl Cyclohexane					CAS #: 108-87-2			
10.575	10.575	(1.064)	83	1588846	50.0000	43.855	80.00- 120.00	100.00	
10.575	10.575	(1.064)	98	807434			0.00- 30.00	50.82	
10.575	10.575	(1.064)	55	1460460			0.00- 30.00	91.92	
-----									

Report Date: 02-May-2008 08:09

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 02-MAY-2008

Lab File ID: 5050202.d

Calibration Time: 07:55

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd5.i/5-02may.b/t14q424a.m

Misc Info: 200ppbv -&gt; 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	339808	203885	475731	339808	0.00
92 1,4-Difluorobenze	1321223	792734	1849712	1321223	0.00
125 Chlorobenzene-d5	1146934	688160	1605708	1146934	0.00


COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.94	9.61	10.27	9.94	0.00
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0804565-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	5050203	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 5/2/08 08:22 AM

Compound	%Recovery
Freon 12	97
Freon 114	122
Vinyl Chloride	115
Bromomethane	128
Chloroethane	115
Freon 11	103
1,1-Dichloroethene	106
Freon 113	132 Q
Methylene Chloride	97
1,1-Dichloroethane	94
cis-1,2-Dichloroethene	89
Chloroform	84
1,1,1-Trichloroethane	88
Carbon Tetrachloride	92
Benzene	93
1,2-Dichloroethane	103
Trichloroethene	99
1,2-Dichloropropane	91
cis-1,3-Dichloropropene	96
Toluene	100
trans-1,3-Dichloropropene	103
1,1,2-Trichloroethane	99
Tetrachloroethene	116
1,2-Dibromoethane (EDB)	97
Chlorobenzene	104
Ethyl Benzene	104
m,p-Xylene	104
o-Xylene	104
Styrene	101
1,1,2,2-Tetrachloroethane	97
1,3,5-Trimethylbenzene	104
1,2,4-Trimethylbenzene	102
1,3-Dichlorobenzene	109
1,4-Dichlorobenzene	107
alpha-Chlorotoluene	116
1,2-Dichlorobenzene	107
1,3-Butadiene	100
Hexane	96
Cyclohexane	94



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0804565-05A

**MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN**

<b>File Name:</b>	<b>5050203</b>	<b>Date of Collection: NA</b>
<b>Dil. Factor:</b>	<b>1.00</b>	<b>Date of Analysis: 5/2/08 08:22 AM</b>

<b>Compound</b>	<b>%Recovery</b>
Heptane	103
Bromodichloromethane	101
Dibromochloromethane	109
Cumene	104
Propylbenzene	103
Chloromethane	94
1,2,4-Trichlorobenzene	112
Hexachlorobutadiene	107
Acetone	100
Carbon Disulfide	109
2-Propanol	95
trans-1,2-Dichloroethene	107
2-Butanone (Methyl Ethyl Ketone)	102
Tetrahydrofuran	78
1,4-Dioxane	94
4-Methyl-2-pentanone	98
2-Hexanone	93
Bromoform	114
4-Ethyltoluene	108
Ethanol	100
Methyl tert-butyl ether	106
3-Chloropropene	112
2,2,4-Trimethylpentane	86
Naphthalene	127

Q = Exceeds Quality Control limits.

**Container Type: NA - Not Applicable**

<b>Surrogates</b>	<b>%Recovery</b>	<b>Method Limits</b>
Toluene-d8	92	70-130
1,2-Dichloroethane-d4	82	70-130
4-Bromofluorobenzene	107	70-130

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 5-02may  
 Sample Matrix: GAS Fraction: VOA  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Level: LOW Operator: kr  
 Data Type: MS DATA SampleType: LCS  
 SpikeList File: 2926Spectra.spk Quant Type: ISTD  
 Sublist File: AT08.sub  
 Method File: /var/chem/msd5.i/5-02may.b/t14q424a.m  
 Misc Info: 50ppbv (200ppbv)

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
8 Dichlorodifluorome	50.000	48.696	97.39	70-130
9 Freon 114	50.000	61.104	122.21	70-130
10 Chloromethane	50.000	46.819	93.64	70-130
13 Vinyl Chloride	50.000	57.416	114.83	70-130
12 1,3-Butadiene	50.000	49.947	99.89	60-140
15 Bromomethane	50.000	63.787	127.57	70-130
19 Chloroethane	50.000	57.324	114.65	70-130
20 Trichlorofluoromet	50.000	51.346	102.69	70-130
26 Ethanol	50.000	50.198	100.40	60-140
30 Freon 113	50.000	65.906	131.81*	70-130
31 1,1-Dichloroethene	50.000	52.880	105.76	70-130
35 Carbon Disulfide	50.000	54.632	109.26	60-140
32 Acetone	50.000	50.215	100.43	60-140
36 2-Propanol	50.000	47.745	95.49	60-140
38 3-Chloropropene	50.000	55.757	111.51	60-140
43 Methylene Chloride	50.000	48.737	97.47	70-130
46 MTBE	50.000	53.262	106.52	60-140
47 trans-1,2-Dichloro	50.000	53.662	107.32	60-140
51 Hexane	50.000	47.820	95.64	60-140
55 1,1-Dichloroethane	50.000	47.212	94.43	70-130
66 cis-1,2-Dichloroet	50.000	44.463	88.93	70-130
67 2-Butanone	50.000	50.771	101.54	60-140
70 Tetrahydrofuran	50.000	39.125	78.25	60-140
72 Chloroform	50.000	42.194	84.39	70-130
74 Cyclohexane	50.000	47.132	94.26	60-140
75 1,1,1-Trichloroeth	50.000	43.929	87.86	70-130
56 Vinyl Acetate	50.000	49.121	98.24	60-140
77 Carbon Tetrachlori	50.000	45.923	91.85	70-130
80 2,2,4-Trimethylpen	50.000	42.804	85.61	60-140
81 Benzene	50.000	46.432	92.86	70-130
85 1,2-Dichloroethane	50.000	51.417	102.83	70-130
90 Heptane	50.000	51.390	102.78	60-140
93 Trichloroethene	50.000	49.576	99.15	70-130



Report Date: 02-May-2008 08:43

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
98 1,2-Dichloropropan	50.000	45.745	91.49	70-130
99 1,4-Dioxane	50.000	46.812	93.62	60-140
100 Bromodichlorometha	50.000	50.352	100.70	60-140
103 cis-1,3-Dichloropr	50.000	47.771	95.54	70-130
106 4-Methyl-2-pentano	50.000	48.976	97.95	60-140
108 Toluene	50.000	49.796	99.59	70-130
113 trans-1,3-Dichloro	50.000	51.672	103.34	70-130
114 1,1,2-Trichloroeth	50.000	49.635	99.27	70-130
116 Tetrachloroethene	50.000	57.829	115.66	70-130
119 2-Hexanone	50.000	46.461	92.92	60-140
120 Dibromochlorometha	50.000	54.645	109.29	60-140
122 1,2-Dibromoethane	50.000	48.628	97.26	70-130
126 Chlorobenzene	50.000	51.842	103.68	70-130
128 Ethyl Benzene	50.000	51.864	103.73	70-130
130 m,p-Xylene	50.000	51.776	103.55	70-130
132 o-Xylene	50.000	51.808	103.62	70-130
133 Styrene	50.000	50.673	101.35	70-130
134 Bromoform	50.000	57.113	114.23	60-140
136 Cumene	50.000	52.162	104.32	60-140
141 1,1,2,2-Tetrachlor	50.000	48.337	96.67	70-130
142 Propylbenzene	50.000	51.741	103.48	60-140
144 4-Ethyltoluene	50.000	54.270	108.54	60-140
147 1,3,5-Trimethylben	50.000	51.816	103.63	70-130
152 1,2,4-Trimethylben	50.000	50.924	101.85	70-130
155 1,3-Dichlorobenzen	50.000	54.470	108.94	70-130
156 1,4-Dichlorobenzen	50.000	53.720	107.44	70-130
157 alpha-Chlorotoluen	50.000	58.216	116.43	70-130
159 1,2-Dichlorobenzen	50.000	53.379	106.76	70-130
163 1,2,4-Trichloroben	50.000	56.217	112.43	70-130
164 Hexachlorobutadien	50.000	53.723	107.45	70-130
6 Propylene	50.000	50.951	101.90	70-130
165 Naphthalene	50.000	63.370	126.74	60-140
11 Butane	50.000	52.073	104.15	70-130
17 Isopentane	50.000	48.247	96.49	70-130
94 Methyl Cyclohexane	50.000	47.810	95.62	70-130
37 tert-Butyl-Alcohol	50.000	43.380	86.76	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 84 1,2-Dichloroethane	25.000	20.547	82.19	70-130
\$ 107 Toluene-d8	25.000	23.036	92.14	70-130
\$ 138 Bromofluorobenzene	25.000	26.677	106.71	70-130



Report Date: 02-May-2008 08:43

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14A/TO15

Data file : /chem/msd5.i/5-02may.b/5050203.d  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Inj Date : 02-MAY-2008 08:22  
 Operator : kr Inst ID: msd5.i  
 Smp Info : 50mL #1576-338  
 Misc Info : 50ppbv (200ppbv)  
 Comment :  
 Method : /var/chem/msd5.i/5-02may.b/t14q424a.m  
 Meth Date : 02-May-2008 08:09 sscott Quant Type: ISTD  
 Cal Date : 24-APR-2008 16:48 Cal File: 5042419.d  
 Als bottle: 1 QC Sample: LCS  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS								
RT	EXP RT	(REL RT)	MASS	RESPONSE		TARGET RANGE	RATIO	
				( PPBV)	( PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 71	Bromochloromethane					CAS #: 74-97-5		
8.059	8.059	(1.000)	130	279575	25.0000	80.00- 120.00	100.00	
8.059	8.059	(1.000)	128	211484		50.87- 110.87	75.64	
8.059	8.059	(1.000)	49	439129		129.59- 189.59	157.07	
-----								
* 92	1,4-Difluorobenzene					CAS #: 540-36-3		
9.911	9.939	(1.000)	114	1035215	25.0000	80.00- 120.00	100.00	
9.911	9.912	(1.000)	88	148692		0.00- 43.72	14.36	
-----								
* 125	Chlorobenzene-d5					CAS #: 3114-55-4		
14.999	14.999	(1.000)	117	954742	25.0000	80.00- 120.00	100.00	
14.999	14.999	(1.000)	82	434923		0.00- 30.00	45.55	
-----								
\$ 84	1,2-Dichloroethane-d4					CAS #: 17060-07-0		
9.110	9.137	(1.130)	65	291570	20.5467	20.547 80.00- 120.00	100.00	
9.110	9.137	(1.130)	67	172054		0.00- 30.00	59.01	
-----								
\$ 107	Toluene-d8					CAS #: 2037-26-5		
12.704	12.704	(1.282)	98	906210	23.0357	23.036 80.00- 120.00	100.00	
12.676	12.704	(1.279)	70	82624		0.00- 30.00	9.12	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT (REL RT)	MASS	RESPONSE	( PPEV)	( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

\$ 107 Toluene-d8 (continued)

12.704	12.704 (1.282)	100	640372			0.00- 30.00	70.66
--------	----------------	-----	--------	--	--	-------------	-------

\$ 138 Bromofluorobenzene

CAS #: 460-00-4

16.575	16.575 (1.105)	174	618442	26.6772	26.677	80.00- 120.00	100.00
16.575	16.575 (1.105)	95	705553			79.99- 139.99	114.09
16.575	16.575 (1.105)	176	602002			64.67- 124.67	97.34

6 Propylene

CAS #: 115-07-1

2.253	2.308 (0.280)	41	1105208	50.9507	50.951	80.00- 120.00	100.00
2.253	2.308 (0.280)	42	729392			0.00- 30.00	66.00
2.253	2.308 (0.280)	39	755223			0.00- 30.00	68.33

8 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.308	2.363 (0.286)	85	1691823	48.6961	48.696	80.00- 120.00	100.00
2.336	2.363 (0.290)	87	538856			0.00- 30.00	31.85

9 Freon 114

CAS #: 76-14-2

2.446	2.474 (0.304)	135	1729379	61.1044	61.104	80.00- 120.00	100.00
2.446	2.474 (0.304)	137	546597			1.44- 61.44	31.61

10 Chloromethane

CAS #: 74-87-3

2.584	2.612 (0.321)	50	1222459	46.8195	46.819	80.00- 120.00	100.00
2.584	2.612 (0.321)	52	366030			0.00- 30.00	29.94

13 Vinyl Chloride

CAS #: 75-01-4

2.778	2.806 (0.345)	62	1217097	57.4157	57.416	80.00- 120.00	100.00
2.750	2.806 (0.341)	64	370471			0.00- 30.00	30.44

12 1,3-Butadiene

CAS #: 106-99-0

2.750	2.778 (0.341)	54	1047278	49.9474	49.947	80.00- 120.00	100.00
2.750	2.778 (0.341)	39	1190600			0.00- 30.00	113.69

15 Bromomethane

CAS #: 74-83-9

3.276	3.303 (0.406)	94	755878	63.7870	63.787	80.00- 120.00	100.00
3.276	3.303 (0.406)	96	723639			65.79- 125.79	95.73

19 Chloroethane

CAS #: 75-00-3

3.386	3.442 (0.420)	64	603454	57.3236	57.324	80.00- 120.00	100.00
3.386	3.442 (0.420)	49	165785			0.00- 30.00	27.47
3.386	3.442 (0.420)	66	187012			0.00- 30.00	30.99

20 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

3.718	3.746 (0.461)	101	1819471	51.3461	51.346	80.00- 120.00	100.00
3.718	3.746 (0.461)	103	1200218			36.32- 96.32	65.97

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== ===== =====

26 Ethanol CAS #: 64-17-5  
 4.077 4.105 (0.506) 45 420237 50.1978 50.198 80.00- 120.00 100.00  
 4.077 4.105 (0.506) 43 83692 0.00- 30.00 19.92  
 4.077 4.105 (0.506) 46 175438 0.00- 30.00 41.75

30 Freon 113 CAS #: 76-13-1  
 4.520 4.548 (0.561) 151 1438873 65.9065 65.906 80.00- 120.00 100.00(R)  
 4.520 4.548 (0.561) 153 908095 33.40- 93.40 63.11  
 4.520 4.548 (0.561) 101 1806482 94.66- 154.66 125.55

31 1,1-Dichloroethene CAS #: 75-35-4  
 4.575 4.603 (0.568) 61 1482737 52.8804 52.880 80.00- 120.00 100.00  
 4.575 4.603 (0.568) 96 1002317 33.88- 93.88 67.60  
 4.575 4.603 (0.568) 98 620494 11.22- 71.22 41.85

32 Acetone CAS #: 67-64-1  
 4.713 4.741 (0.585) 58 539306 50.2148 50.215 80.00- 120.00 100.00  
 4.713 4.741 (0.585) 43 1619303 0.00- 30.00 300.26

36 2-Propanol CAS #: 67-63-0  
 4.907 4.935 (0.609) 45 1937013 47.7449 47.745 80.00- 120.00 100.00  
 4.907 4.935 (0.609) 43 434760 0.00- 30.00 22.44  
 4.907 4.935 (0.609) 59 66859 0.00- 30.00 3.45

35 Carbon Disulfide CAS #: 75-15-0  
 4.907 4.935 (0.609) 76 2643479 54.6316 54.632 80.00- 120.00 100.00

38 3-Chloropropene CAS #: 107-05-1  
 5.183 5.211 (0.643) 76 464083 55.7569 55.757 80.00- 120.00 100.00  
 5.183 5.211 (0.643) 41 1564724 0.00- 30.00 337.16

43 Methylene Chloride CAS #: 75-09-2  
 5.432 5.460 (0.674) 49 1240083 48.7372 48.737 80.00- 120.00 100.00  
 5.432 5.460 (0.674) 84 798745 34.18- 94.18 64.41  
 5.432 5.460 (0.674) 51 379015 0.00- 30.00 30.56

46 MTBE CAS #: 1634-04-4  
 5.764 5.792 (0.715) 73 1295653 53.2623 53.262 80.00- 120.00 100.00  
 5.764 5.792 (0.715) 57 366609 0.00- 58.47 28.30  
 5.764 5.792 (0.715) 41 404610 0.00- 30.00 31.23

47 trans-1,2-Dichloroethene CAS #: 156-60-5  
 5.819 5.847 (0.722) 96 980064 53.6619 53.662 80.00- 120.00 100.00  
 5.819 5.847 (0.722) 61 1351021 105.82- 165.82 137.85  
 5.819 5.847 (0.722) 98 627894 0.00- 30.00 64.07

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == =====

51 Hexane CAS #: 110-54-3  
 6.151 6.179 (0.763) 57 1717942 47.8198 47.820 80.00- 120.00 100.00  
 6.151 6.179 (0.763) 43 1245046 0.00- 30.00 72.47  
 6.151 6.179 (0.763) 86 271891 0.00- 30.00 15.83

56 Vinyl Acetate CAS #: 108-05-4  
 6.649 6.677 (0.825) 86 228757 49.1212 49.121 80.00- 120.00 100.00  
 6.649 6.677 (0.825) 43 2813901 0.00- 30.00 1230.08  
 6.649 6.677 (0.825) 42 214831 0.00- 30.00 93.91

55 1,1-Dichloroethane CAS #: 75-34-3  
 6.594 6.621 (0.818) 63 1590723 47.2125 47.212 80.00- 120.00 100.00  
 6.594 6.621 (0.818) 65 470711 0.00- 59.43 29.59

67 2-Butanone CAS #: 78-93-3  
 7.644 7.672 (0.949) 72 417289 50.7707 50.771 80.00- 120.00 100.00  
 7.644 7.672 (0.949) 43 2093361 500.72- 560.72 501.66  
 7.644 7.672 (0.949) 57 143226 0.00- 30.00 34.32

66 cis-1,2-Dichloroethene CAS #: 156-59-2  
 7.617 7.644 (0.945) 61 1081419 44.4635 44.463 80.00- 120.00 100.00  
 7.617 7.644 (0.945) 96 897497 50.86- 110.86 82.99  
 7.617 7.644 (0.945) 98 574344 22.28- 82.28 53.11

70 Tetrahydrofuran CAS #: 109-99-9  
 8.031 8.059 (0.997) 42 1225069 39.1253 39.125 80.00- 120.00 100.00  
 8.031 8.059 (0.997) 71 351926 0.00- 58.75 28.73  
 8.031 8.059 (0.997) 72 377228 0.00- 30.00 30.79

72 Chloroform CAS #: 67-66-3  
 8.197 8.197 (1.017) 83 1360320 42.1941 42.194 80.00- 120.00 100.00  
 8.197 8.197 (1.017) 85 903286 35.00- 95.00 66.40

75 1,1,1-Trichloroethane CAS #: 71-55-6  
 8.446 8.446 (1.048) 97 1315125 43.9295 43.929 80.00- 120.00 100.00  
 8.446 8.446 (1.048) 99 852357 36.53- 96.53 64.81

74 Cyclohexane CAS #: 110-82-7  
 8.418 8.418 (1.045) 84 1120118 47.1318 47.132 80.00- 120.00 100.00  
 8.418 8.418 (1.045) 56 1543343 106.32- 166.32 137.78  
 8.418 8.418 (1.045) 41 871389 50.79- 110.79 77.79

77 Carbon Tetrachloride CAS #: 56-23-5  
 8.667 8.695 (1.075) 119 1230747 45.9232 45.923 80.00- 120.00 100.00  
 8.667 8.695 (1.075) 117 1268340 73.61- 133.61 103.05

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
80	2,2,4-Trimethylpentane					CAS #:	540-84-1			
9.082	9.110	(1.127)	57	4436812	42.8036	42.804	80.00-	120.00	100.00	
9.082	9.110	(1.127)	56	1437953			0.00-	30.00	32.41	
9.082	9.110	(1.127)	41	1215420			0.00-	30.00	27.39	
-----										
81	Benzene					CAS #:	71-43-2			
9.082	9.110	(0.916)	78	2410864	46.4318	46.432	80.00-	120.00	100.00	
9.082	9.110	(0.916)	77	567482			0.00-	30.00	23.54	
-----										
85	1,2-Dichloroethane					CAS #:	107-06-2			
9.276	9.276	(0.936)	62	960720	51.4172	51.417	80.00-	120.00	100.00	
9.276	9.276	(0.936)	64	291292			0.00-	30.00	30.32	
-----										
90	Heptane					CAS #:	142-82-5			
9.469	9.497	(0.955)	100	291639	51.3898	51.390	80.00-	120.00	100.00	
9.469	9.497	(0.955)	43	1863923			0.00-	30.00	639.12	
9.469	9.497	(0.955)	71	813356			0.00-	30.00	278.89	
-----										
93	Trichloroethene					CAS #:	79-01-6			
10.326	10.326	(1.042)	95	954445	49.5755	49.576	80.00-	120.00	100.00	
10.326	10.354	(1.042)	130	1033751			82.12-	142.12	108.31	
10.326	10.326	(1.042)	97	603715			34.93-	94.93	63.25	
-----										
98	1,2-Dichloropropane					CAS #:	78-87-5			
10.824	10.852	(1.092)	63	785103	45.7451	45.745	80.00-	120.00	100.00	
10.824	10.852	(1.092)	62	556681			41.90-	101.90	70.91	
10.824	10.852	(1.092)	41	544366			45.12-	105.12	69.34	
-----										
99	1,4-Dioxane					CAS #:	123-91-1			
11.073	11.073	(1.117)	88	532753	46.8118	46.812	80.00-	120.00	100.00	
11.073	11.073	(1.117)	58	396038			46.73-	106.73	74.34	
11.073	11.073	(1.117)	57	128084			0.00-	30.00	24.04	
-----										
100	Bromodichloromethane					CAS #:	75-27-4			
11.405	11.405	(1.151)	83	1265189	50.3519	50.352	80.00-	120.00	100.00	
11.405	11.405	(1.151)	85	798487			35.40-	95.40	63.11	
-----										
103	cis-1,3-Dichloropropene					CAS #:	10061-01-5			
12.317	12.317	(1.243)	75	939246	47.7709	47.771	80.00-	120.00	100.00	
12.317	12.317	(1.243)	77	298186			2.65-	62.65	31.75	
12.289	12.317	(1.240)	39	674686			44.65-	104.65	71.83	
-----										
106	4-Methyl-2-pentanone					CAS #:	108-10-1			
12.593	12.594	(1.271)	58	674643	48.9759	48.976	80.00-	120.00	100.00	
12.593	12.594	(1.271)	43	2015124			0.00-	30.00	298.69	
12.593	12.594	(1.271)	85	266556			0.00-	30.00	39.51	
-----										

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL ( PPEV)	FINAL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
108 Toluene						CAS #:	108-88-3			
12.815	12.815	(1.293)	91	2514989	49.7964	49.796	80.00-	120.00	100.00	
12.815	12.815	(1.293)	92	1450131			29.74-	89.74	57.66	
-----										
113 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.368	13.368	(0.891)	75	950424	51.6725	51.672	80.00-	120.00	100.00	
13.368	13.368	(0.891)	77	304351			3.45-	63.45	32.02	
13.340	13.368	(0.889)	39	663706			41.28-	101.28	69.83	
-----										
114 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.644	13.644	(0.910)	97	805821	49.6349	49.635	80.00-	120.00	100.00	
13.644	13.644	(0.910)	99	514847			33.47-	93.47	63.89	
13.644	13.644	(0.910)	83	665154			50.38-	110.38	82.54	
-----										
116 Tetrachloroethene						CAS #:	127-18-4			
13.699	13.700	(0.913)	166	1219000	57.8292	57.829	80.00-	120.00	100.00	
13.672	13.700	(0.912)	129	848404			39.68-	99.68	69.60	
13.672	13.700	(0.912)	131	805248			37.68-	97.68	66.06	
-----										
119 2-Hexanone						CAS #:	591-78-6			
14.004	14.004	(0.934)	58	903634	46.4612	46.461	80.00-	120.00	100.00	
14.004	14.004	(0.934)	43	1968361			184.12-	244.12	217.83	
14.004	14.031	(0.934)	100	183992			0.00-	30.00	20.36	
-----										
120 Dibromochloromethane						CAS #:	124-48-1			
14.197	14.197	(0.947)	129	1310216	54.6447	54.645	80.00-	120.00	100.00	
14.197	14.197	(0.947)	127	999784			0.00-	30.00	76.31	
-----										
122 1,2-Dibromoethane						CAS #:	106-93-4			
14.363	14.363	(0.958)	107	1319951	48.6285	48.628	80.00-	120.00	100.00	
14.363	14.363	(0.958)	109	1230707			66.28-	126.28	93.24	
-----										
126 Chlorobenzene						CAS #:	108-90-7			
15.027	15.054	(1.002)	112	2003137	51.8416	51.842	80.00-	120.00	100.00	
15.027	15.054	(1.002)	114	638978			2.30-	62.30	31.90	
15.027	15.027	(1.002)	77	1079609			22.57-	82.57	53.90	
-----										
128 Ethyl Benzene						CAS #:	100-41-4			
15.165	15.165	(1.011)	106	1108276	51.8636	51.864	80.00-	120.00	100.00	
15.165	15.165	(1.011)	91	3231795			0.00-	30.00	291.61	
-----										
130 m,p-Xylene						CAS #:	108-38-3			
15.331	15.331	(1.022)	106	1375652	51.7758	51.776	80.00-	120.00	100.00	
15.331	15.331	(1.022)	91	2542621			0.00-	30.00	184.83	
-----										
132 o-Xylene						CAS #:	95-47-6			
15.856	15.856	(1.057)	106	1286892	51.8081	51.808	80.00-	120.00	100.00	



CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
132 o-Xylene (continued)									
15.856	15.856	(1.057)	91	2523720			165.51- 225.51	196.11	
-----									
133 Styrene CAS #: 100-42-5									
15.911	15.911	(1.061)	104	2027792	50.6728	50.673	80.00- 120.00	100.00	
15.911	15.911	(1.061)	78	884167			13.14- 73.14	43.60	
-----									
134 Bromoform CAS #: 75-25-2									
16.160	16.160	(1.077)	173	1313126	57.1129	57.113	80.00- 120.00	100.00	
16.160	16.160	(1.077)	171	684835			21.81- 81.81	52.15	
-----									
141 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
16.796	16.796	(1.120)	83	1769079	48.3367	48.337	80.00- 120.00	100.00	
16.796	16.796	(1.120)	85	1153288			34.91- 94.91	65.19	
-----									
144 4-Ethyltoluene CAS #: 622-96-8									
16.962	16.962	(1.131)	105	4076167	54.2704	54.270	80.00- 120.00	100.00	
16.962	16.962	(1.131)	120	1290826			1.56- 61.56	31.67	
-----									
147 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.045	17.045	(1.136)	105	3463086	51.8159	51.816	80.00- 120.00	100.00	
17.045	17.045	(1.136)	120	1821089			0.00- 30.00	52.59	
-----									
152 1,2,4-Trimethylbenzene CAS #: 95-63-6									
17.460	17.460	(1.164)	105	2856207	50.9245	50.924	80.00- 120.00	100.00	
17.460	17.460	(1.164)	120	1456293			20.14- 80.14	50.99	
-----									
155 1,3-Dichlorobenzene CAS #: 541-73-1									
17.764	17.764	(1.184)	146	2121355	54.4702	54.470	80.00- 120.00	100.00	
17.764	17.764	(1.184)	148	1362903			0.00- 30.00	64.25	
17.764	17.764	(1.184)	111	757127			0.00- 30.00	35.69	
-----									
156 1,4-Dichlorobenzene CAS #: 106-46-7									
17.847	17.847	(1.190)	146	2634623	53.7203	53.720	80.00- 120.00	100.00	
17.847	17.847	(1.190)	148	1696027			0.00- 30.00	64.37	
17.847	17.847	(1.190)	111	939262			0.00- 30.00	35.65	
-----									
157 alpha-Chlorotoluene CAS #: 100-44-7									
17.985	17.985	(1.199)	91	3212469	58.2165	58.216	80.00- 120.00	100.00	
17.985	17.985	(1.199)	126	786258			0.00- 30.00	24.48	
-----									
159 1,2-Dichlorobenzene CAS #: 95-50-1									
18.206	18.206	(1.214)	146	2132354	53.3788	53.379	80.00- 120.00	100.00	
18.206	18.206	(1.214)	148	1376386			34.64- 94.64	64.55	
18.206	18.206	(1.214)	111	728103			5.99- 65.99	34.15	
-----									

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	FINAL	( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	
-----										
163	1,2,4-Trichlorobenzene					CAS #: 120-82-1				
19.478	19.506	(1.299)	180	1651635	56.2168	56.217	80.00-	120.00	100.00	
19.478	19.506	(1.299)	182	1545426			63.17-	123.17	93.57	
-----										
164	Hexachlorobutadiene					CAS #: 87-68-3				
19.589	19.589	(1.306)	225	1064888	53.7232	53.723	80.00-	120.00	100.00	
19.561	19.589	(1.304)	223	665793			33.59-	93.59	62.52	
-----										
142	Propylbenzene					CAS #: 103-65-1				
16.824	16.824	(1.122)	91	4289802	51.7413	51.741	80.00-	120.00	100.00	
16.824	16.824	(1.122)	120	1059115			0.00-	30.00	24.69	
16.824	16.824	(1.122)	105	156294			0.00-	30.00	3.64	
-----										
136	Cumene					CAS #: 98-82-8				
16.326	16.326	(1.088)	105	3887745	52.1621	52.162	80.00-	120.00	100.00	
16.326	16.326	(1.088)	120	1104278			0.00-	30.00	28.40	
16.326	16.326	(1.088)	51	422953			0.00-	30.00	10.88	
-----										
165	Naphthalene					CAS #: 91-20-3				
19.672	19.672	(1.312)	128	5964133	63.3702	63.370	80.00-	120.00	100.00	
19.672	19.672	(1.312)	127	728707			0.00-	30.00	12.22	
-----										
37	tert-Butyl-Alcohol					CAS #: 75-65-0				
5.571	5.598	(0.691)	59	901507	43.3804	43.380	80.00-	120.00	100.00	
5.571	5.598	(0.691)	41	253447			0.00-	30.00	28.11	
5.571	5.598	(0.691)	57	88126			0.00-	30.00	9.78	
-----										
11	Butane					CAS #: 106-97-8				
2.667	2.695	(0.331)	58	294022	52.0727	52.073	80.00-	120.00	100.00	
2.667	2.695	(0.331)	43	2302803			0.00-	30.00	783.21	
-----										
17	Isopentane					CAS #: 78-78-4				
3.414	3.442	(0.424)	43	1688321	48.2474	48.247	80.00-	120.00	100.00	
3.414	3.442	(0.424)	57	1033406			0.00-	30.00	61.21	
3.414	3.442	(0.424)	72	102833			0.00-	30.00	6.09	
-----										
94	Methyl Cyclohexane					CAS #: 108-87-2				
10.547	10.575	(1.064)	83	1357159	47.8100	47.810	80.00-	120.00	100.00	
10.547	10.575	(1.064)	98	682491			0.00-	30.00	50.29	
10.547	10.575	(1.064)	55	1254312			0.00-	30.00	92.42	
-----										

QC Flag Legend

R - Spike/Surrogate failed recovery limits.

Report Date: 02-May-2008 08:43

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msd5.i

Calibration Date: 02-MAY-2008

Lab File ID: 5050203.d

Calibration Time: 07:55

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: kr

Method File: /var/chem/msd5.i/5-02may.b/t14q424a.m

Misc Info: 50ppbv (200ppbv)

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	339808	203885	475731	279575	-17.73
92 1,4-Difluorobenze	1321223	792734	1849712	1035215	-21.65
125 Chlorobenzene-d5	1146934	688160	1605708	954742	-16.76

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
71 Bromochloromethan	8.06	7.73	8.39	8.06	0.00
92 1,4-Difluorobenze	9.94	9.61	10.27	9.91	-0.28
125 Chlorobenzene-d5	15.00	14.67	15.33	15.00	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.


RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Data File: /chem/msd5.1/5-02may.b/5050203.d  
Date: 02-MAY-2008 08:22  
Client ID: LCS-1  
Sample Info: 50mL #1576-338

Column phase: RTX-624

Instrument: msd5.1  
Operator: kp  
Column diameter: 0.53

/chem/msd5.1/5-02may.b/5050203.d

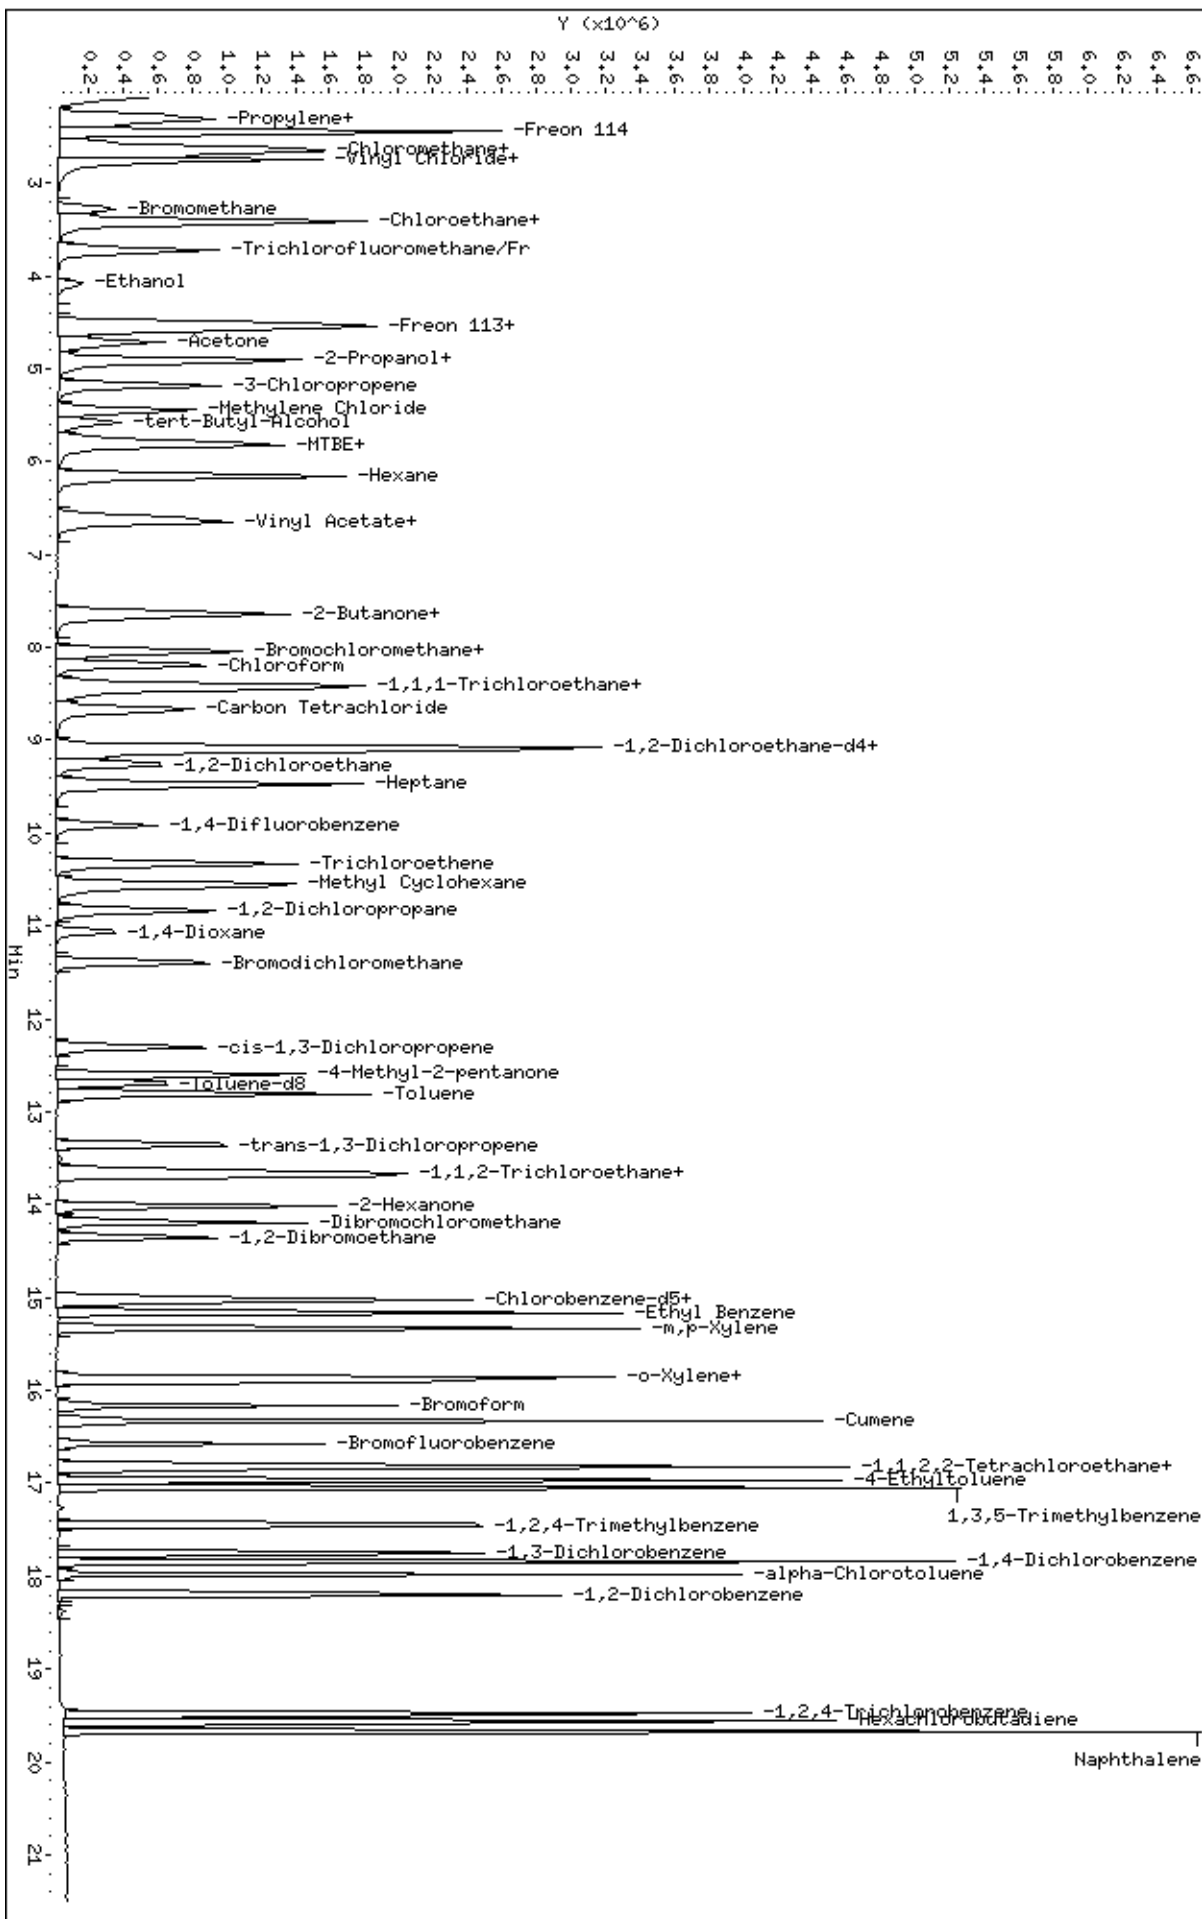

ION ABUNDANCE CRITERIA

% REL. ABUNDANCE

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	26.49
75	30.0 - 60.0% of mass 95	42.76
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	6.52
173	Less than 2.0% of mass 174	( 0.73 ) <sup>1</sup>
174	Greater than 50.0% of mass 95	50.01
175	5.0 - 9.0% of mass 174	( 6.52 ) <sup>1</sup>
176	Greater than 95.0% but less than 101.0% of mass 174	( 95.92 ) <sup>1</sup>
177	5.0 - 9.0% of mass 176	( 6.68 ) <sup>2</sup>

<sup>1</sup> - value in parenthesis is % mass 174      <sup>2</sup> - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio:

$$\frac{(95.92)(174)}{(95.92)(176)} = 95.923$$

NOAH Cart #: 9

File #: S05015

BFB Injection Date: 5/21/07  
 BFB Injection Time: 0724  
 BFB File ID: S050201  
 Tekmar Purge Flow: 13.5 mL/min  
 Vacuum: 10.14 x 10<sup>-4</sup> Torr  
 IS/S Std #: 1591-153      Exp. Date: 7/4/08  
 BCM: 33809  
 1,4-DFB: 1321223  
 CB-d5: 1412931  
 Verified CCV IS vs ICAL mid-point (-40% D) 945

Calculation Check:

$$\text{ppbv of compound} = \frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} \times \text{RRF} = \left( \frac{1125533}{1321223} \right) \times \left( \frac{255000}{0.9550025} \right) = 223835$$

Reported Result: 22384

File ID: S050202  
 Compound: Toluene-D8  
 Initials: 94

g	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
1	S050201	BFB Run Check	111825	520g	2.1g	100	5/21/07	0721	94	
2	02	1612-1 200gpbu	CV-1	50gpbu	50g			0755	94	
3	03	1576-338 800gpbu	LS-1	50gpbu	50g			0702	94	
4	04	Lab Blank	12511	Handled	Handled			0525	94	Cont #15 Log #8
5	05	Cont #5 Log #6						1016	94	
6	06	030413A-01A	34343	150gpbu	250g	139		1005	94	
7	07		34417	70gpbu		136		1038	94	
8	08		13512	100gpbu		201		1210	94	
9	09		10924	30gpbu		146		1243	94	

Signature: *[Handwritten Signature]*

Date: 5/21/07

@ Air Toxics Ltd.

MSD-5

Logbook #: 1637

	✓	SO50210	08041034-119	3004p	70% -5%	2000	175	9/20/08	1311e	94	1500x PRC 2000
10	✓										
11	X	11	08041550-014	22005	80% -15%	2000	200		1315	94	
12	✓	12	08041505-014	10208	80% -5%	2000	179		141e	95	
13	✓	13	↓ 024	74304	65% ↓	↓	121		1419	96	
14		14	08041550-014	22005	80% -15%	2000	200	↓			1500x
15											
16											
17											
18											
19											
20											
21											
22											
23											
24											
25											
26											
27											
28											
29											
30											
31											
32											

Comments:

Signature

5/2/08

Date

Report Date: 24-Apr-2008 13:12

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-24apr.b/5042412.d  
 Lab Smp Id: Client Smp ID: BFB  
 Inj Date : 24-APR-2008 13:23  
 Operator : srs Inst ID: msd5.i  
 Smp Info : BFB Tune Check  
 Misc Info : 2uL #1476-279 50 ng  
 Comment :  
 Method : /var/chem/msd5.i/5-24apr.b/bfb30.m  
 Meth Date : 24-Apr-2008 13:12 Quant Type: ESTD  
 Cal Date : Cal File:  
 Als bottle: 1 QC Sample: BFB  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: all.sub  
 Target Version: 3.50 Sample Matrix: WATER  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* Uf \* Vf \* Vi \* CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE ( ug/L) ( ug/L) TARGET RANGE RATIO  
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE	( ug/L)	( ug/L)	TARGET RANGE	RATIO
1	bfb					CAS #: 460-00-4		
3.803	3.900	-0.097	95	1236184			100.00- 100.00	100.00
3.803	3.900	-0.097	50	290786			15.00- 40.00	23.52
3.803	3.900	-0.097	75	512259			30.00- 60.00	41.44
3.803	3.900	-0.097	96	78390			5.00- 9.00	6.34
3.803	3.900	-0.097	173	6418			0.00- 2.00	0.65
3.803	3.900	-0.097	174	991924			50.00- 100.00	80.24
3.803	3.900	-0.097	175	69740			5.00- 9.00	7.03
3.803	3.900	-0.097	176	952447			95.00- 101.00	96.02
3.803	3.900	-0.097	177	59357			5.00- 9.00	6.23

Date : 24-APR-2008 13:23

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00





Date : 24-APR-2008 13:23

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	23.52
75	30.00 - 60.00% of mass 95	41.44
96	5.00 - 9.00% of mass 95	6.34
173	Less than 2.00% of mass 174	0.52 ( 0.65)
174	50.00 - 100.00% of mass 95	80.24
175	5.00 - 9.00% of mass 174	5.64 ( 7.03)
176	95.00 - 101.00% of mass 174	77.05 ( 96.02)
177	5.00 - 9.00% of mass 176	4.80 ( 6.23)

Date : 24-APR-2008 13:23

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

Data File: 5042412.d

Spectrum: Avg. Scans 100-102 ( 3.80), Background Scan 92

Location of Maximum: 95.00

Number of points: 223

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	11260	97.00	1891	160.00	105	246.00	316
37.00	66904	99.00	127	161.00	540	247.00	111
38.00	60528	101.00	187	162.00	37	248.00	97
39.00	26368	103.00	128	163.00	155	249.00	186
40.00	615	104.00	2500	164.00	289	250.00	147
42.00	377	105.00	1058	165.00	419	252.00	178
43.00	142	106.00	2727	166.00	399	253.00	85
44.00	6663	107.00	455	167.00	533	254.00	121
45.00	12954	108.00	12	168.00	76	258.00	166
46.00	1002	109.00	272	169.00	691	259.00	125
47.00	16984	110.00	552	170.00	468	263.00	212
48.00	7635	111.00	586	171.00	246	264.00	107
49.00	57752	112.00	321	172.00	1340	265.00	52
50.00	290752	113.00	491	173.00	6418	266.00	68
51.00	87024	115.00	1287	174.00	991872	267.00	253
52.00	2833	116.00	2516	175.00	69736	268.00	79
53.00	12	117.00	4810	176.00	952384	270.00	394
55.00	2647	118.00	3530	177.00	59352	271.00	160
56.00	15731	119.00	3426	178.00	2119	272.00	154
57.00	31752	120.00	373	181.00	71	275.00	61
58.00	925	121.00	403	183.00	458	280.00	112
59.00	455	122.00	3	184.00	98	281.00	61
60.00	8750	123.00	34	187.00	138	285.00	68
61.00	50472	124.00	1046	189.00	323	290.00	59
62.00	50696	125.00	73	190.00	57	292.00	31
63.00	35912	126.00	148	191.00	155	295.00	58
64.00	2593	128.00	3251	193.00	199	298.00	149
65.00	544	129.00	1866	195.00	60	300.00	57
66.00	371	130.00	3165	196.00	221	303.00	32
67.00	2620	131.00	1667	199.00	148	304.00	4
68.00	96080	132.00	74	201.00	84	307.00	288
69.00	95880	134.00	32	202.00	320	309.00	67
70.00	6660	135.00	1560	203.00	288	310.00	179
71.00	521	136.00	387	205.00	228	311.00	282
72.00	5181	137.00	1134	206.00	53	312.00	160

Date : 24-APR-2008 13:23

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

Data File: 5042412.d

Spectrum: Avg. Scans 100-102 ( 3.80), Background Scan 92

Location of Maximum: 95.00

Number of points: 223

m/z	Y	m/z	Y	m/z	Y	m/z	Y
73.00	39176	138.00	76	207.00	300	315.00	111
74.00	150592	139.00	542	208.00	89	316.00	10
75.00	512256	141.00	6323	209.00	124	317.00	50
76.00	44928	142.00	845	210.00	240	320.00	4
77.00	6391	143.00	5708	211.00	88	325.00	81
78.00	2856	144.00	541	214.00	274	326.00	161
79.00	14514	145.00	399	216.00	58	327.00	190
80.00	4693	146.00	1829	217.00	254	329.00	392
81.00	12705	147.00	1033	218.00	99	330.00	228
82.00	3160	148.00	2525	224.00	74	332.00	90
83.00	487	149.00	885	227.00	66	333.00	107
86.00	1916	150.00	881	229.00	92	334.00	67
87.00	47136	151.00	325	231.00	70	335.00	140
88.00	44416	152.00	305	232.00	149	336.00	81
90.00	52	153.00	735	234.00	172	337.00	19
91.00	2621	154.00	273	235.00	228	338.00	83
92.00	25008	155.00	2711	238.00	123	342.00	105
93.00	40080	156.00	577	239.00	140	345.00	111
94.00	126424	157.00	1619	241.00	170	348.00	327
95.00	1235968	158.00	65	243.00	184	350.00	115
96.00	78384	159.00	1362	245.00	165		

Report Date: 02-May-2008 07:10

Air Toxics Ltd.

Data file : /var/chem/msd5.i/5-02may.b/5050201.d  
 Lab Smp Id: Client Smp ID: BFB  
 Inj Date : 02-MAY-2008 07:21  
 Operator : srs Inst ID: msd5.i  
 Smp Info : BFB Tune Check  
 Misc Info : 2uL #1476-279 50 ng  
 Comment :  
 Method : /var/chem/msd5.i/5-02may.b/bfb30.m  
 Meth Date : 02-May-2008 07:10 Quant Type: ESTD  
 Cal Date : Cal File:  
 Als bottle: 1 QC Sample: BFB  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: all.sub  
 Target Version: 3.50 Sample Matrix: WATER  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* Uf \* Vf \* Vi \* CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE ( ug/L) ( ug/L) TARGET RANGE RATIO  
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE	( ug/L)	( ug/L)	TARGET RANGE	RATIO
1	bfb						CAS #: 460-00-4	
3.803	3.900	-0.097	95	1105696			100.00- 100.00	100.00
3.803	3.900	-0.097	50	292897			15.00- 40.00	26.49
3.803	3.900	-0.097	75	472810			30.00- 60.00	42.76
3.803	3.900	-0.097	96	72062			5.00- 9.00	6.52
3.803	3.900	-0.097	173	7311			0.00- 2.00	0.73
3.803	3.900	-0.097	174	995215			50.00- 100.00	90.01
3.803	3.900	-0.097	175	65362			5.00- 9.00	6.57
3.803	3.900	-0.097	176	954624			95.00- 101.00	95.92
3.803	3.900	-0.097	177	63829			5.00- 9.00	6.69

Data File: /var/chem/msd5.i/5-02may.b/5050201.d

Page 1

Date : 02-MAY-2008 07:21

Client ID: BFB

Instrument: msd5.i


Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00



Date : 02-MAY-2008 07:21

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check


Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

1 bfb



m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	26.49
75	30.00 - 60.00% of mass 95	42.76
96	5.00 - 9.00% of mass 95	6.52
173	Less than 2.00% of mass 174	0.66 ( 0.73)
174	50.00 - 100.00% of mass 95	90.01
175	5.00 - 9.00% of mass 174	5.91 ( 6.57)
176	95.00 - 101.00% of mass 174	86.34 ( 95.92)
177	5.00 - 9.00% of mass 176	5.77 ( 6.69)

Date : 02-MAY-2008 07:21

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

Data File: 5050201.d

Spectrum: Avg. Scans 100-102 ( 3.80), Background Scan 92

Location of Maximum: 95.00

Number of points: 214

m/z	Y	m/z	Y	m/z	Y	m/z	Y
35,00	221	92,00	25528	153,00	499	256,00	67
36,00	11477	93,00	38560	154,00	333	257,00	151
37,00	65736	94,00	112192	155,00	3275	258,00	81
38,00	60368	95,00	1105408	156,00	546	265,00	212
39,00	24992	96,00	72056	157,00	2022	266,00	151
40,00	1335	97,00	1648	158,00	341	270,00	236
41,00	283	98,00	202	159,00	1249	271,00	174
43,00	552	99,00	120	160,00	288	275,00	105
44,00	4123	101,00	138	161,00	1418	277,00	63
45,00	13280	104,00	2268	163,00	157	282,00	250
46,00	759	105,00	688	164,00	158	284,00	115
47,00	15584	106,00	2699	166,00	285	285,00	147
48,00	8288	107,00	394	167,00	514	287,00	158
49,00	54592	110,00	334	168,00	340	290,00	169
50,00	292864	111,00	629	169,00	166	291,00	260
51,00	81312	112,00	186	170,00	1117	292,00	187
52,00	3468	113,00	232	171,00	543	294,00	247
54,00	58	115,00	1041	172,00	1845	296,00	213
55,00	2925	116,00	2109	173,00	7311	298,00	76
56,00	15481	117,00	4052	174,00	995200	299,00	503
57,00	28736	118,00	2001	175,00	65360	301,00	70
58,00	1948	119,00	3378	176,00	954624	302,00	272
59,00	288	120,00	320	177,00	63824	303,00	55
60,00	9403	121,00	136	178,00	1623	304,00	268
61,00	46840	123,00	547	179,00	211	306,00	77
62,00	44824	124,00	242	181,00	278	309,00	69
63,00	36016	125,00	125	189,00	125	310,00	89
64,00	2957	126,00	331	196,00	209	312,00	280
65,00	709	127,00	293	201,00	331	314,00	78
66,00	58	128,00	2517	202,00	209	315,00	15
67,00	2868	129,00	1505	204,00	303	317,00	140
68,00	91512	130,00	3988	207,00	1014	318,00	90
69,00	89200	131,00	1059	208,00	333	320,00	152
70,00	6166	132,00	349	211,00	127	323,00	137
71,00	646	133,00	509	215,00	85	325,00	97

Date : 02-MAY-2008 07:21

Client ID: BFB

Instrument: msd5.i

Sample Info: BFB Tune Check

Volume Injected (uL): 1.0

Operator: srs

Column phase:

Column diameter: 2.00

Data File: 5050201.d

Spectrum: Avg. Scans 100-102 ( 3.80), Background Scan 92

Location of Maximum: 95.00

Number of points: 214

m/z	Y	m/z	Y	m/z	Y	m/z	Y
72,00	4534	134,00	120	216,00	15	327,00	166
73,00	36304	135,00	1073	219,00	79	328,00	230
74,00	143936	136,00	512	221,00	325	330,00	159
75,00	472768	137,00	775	224,00	86	331,00	143
76,00	42512	138,00	549	226,00	81	332,00	102
77,00	6250	139,00	76	227,00	273	333,00	206
78,00	1982	140,00	877	228,00	182	335,00	82
79,00	13697	141,00	6390	231,00	99	336,00	219
80,00	4196	142,00	645	233,00	94	337,00	85
81,00	13842	143,00	6454	234,00	127	338,00	88
82,00	2426	144,00	661	235,00	482	339,00	71
83,00	421	145,00	649	236,00	139	340,00	41
84,00	24	146,00	1542	237,00	213	341,00	115
85,00	158	147,00	518	245,00	246	343,00	200
86,00	1179	148,00	2197	247,00	73	346,00	84
87,00	45008	149,00	602	248,00	147	347,00	96
88,00	37816	150,00	751	250,00	86	349,00	58
89,00	696	151,00	65	251,00	69		
91,00	2697	152,00	494	253,00	600		



## **Shipping/ Receiving Documents**



---

AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B  
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020  
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: \_\_\_\_\_ GEI Consultants, Inc. \_\_\_\_\_  
ATTENTION: \_\_\_\_\_ Ms. Theresa Landgraff \_\_\_\_\_  
FAX #: \_\_\_\_\_  
FROM: \_\_\_\_\_ Sample Receiving \_\_\_\_\_  
Workorder #: \_\_\_\_\_ 0804565 \_\_\_\_\_  
# of pages (Including Cover): \_\_\_\_\_ 1 \_\_\_\_\_

5/12/2008

Thank you for selecting Air Toxics Ltd. We have received your samples and have found no discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Bryanna Langley at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

# AIR TOXICS LTD.

## Sample Transportation Notice

Relinquishing signature on this document indicates that sample is being shipped in compliance with all applicable local, State, Federal, national, and international laws, regulations and ordinances of any kind. Air Toxics Limited assumes no liability with respect to the collection, handling, or shipping of these samples. Relinquishing signature also indicates agreement to hold harmless, defend, and indemnify Air Toxics Limited against any claim, demand, or action of any kind, related to the collection, handling, or shipping of samples. D.O.T. Hotline (800) 487-4922

180 BLUE RAVINE ROAD, SUITE B  
FOLSOM, CA 95630-4719

(916) 985-1000 FAX: (916) 985-1020

<b>Contact:</b>	GEI Consultants, Inc.	<b>Project Info:</b>	<b>Turn Around Time:</b>
<b>Company:</b>	465 Winding Brook Glastonbury CT 06033	P.O. #	<input checked="" type="checkbox"/> Normal
<b>Address:</b>	860-368-5300 Cell	Project #	<input type="checkbox"/> Rush
<b>Phone:</b>		Project Name	Specify _____
<b>Collected By Signature:</b>	<i>[Signature]</i>	BayShore OVI Southern call Air Monitoring	

Lab ID	Field Sample ID	Date & Time	Analyses Requested	Canister Pressure/Inlet Initial	Final	Receipt
ORA	AMS WU	6/16-16/16 / 4-23-08	TO-15 + Naphthalene	-30	-3	
ORA	AMS DW	6/15-14/15 / 4-23-08	TO-15 + Naphthalene	-30	-7	

<b>Relinquished By (Signature) Date/Time:</b>	<i>[Signature]</i> 4-23-2008	<b>Received By (Signature) Date/Time:</b>	<i>[Signature]</i> 04-24-08
<b>Relinquished By (Signature) Date/Time:</b>	<i>[Signature]</i> 4-23-2008	<b>Received By (Signature) Date/Time:</b>	<i>[Signature]</i> 04-24-08
<b>Relinquished By (Signature) Date/Time:</b>		<b>Received By (Signature) Date/Time:</b>	

<b>Lab Use Only</b>	<b>Shipper Name:</b> Air Bill #	<b>Opened By:</b>	<b>Temp (C):</b>	<b>Condition:</b>	<b>Client/Seals Intact:</b>	<b>Work Order #:</b>
	FedEx 8631 8554 8750	ADN	na	good	Yes No None	0804565

Notes: used flow controllers included  
Initial and final can pressures in inches Hg  
Send Data Pack to Lisa McDonough and EDD to detagroup@geiconsultants.com



AN ENVIRONMENTAL ANALYTICAL LABORATORY

### SAMPLE RECEIPT SUMMARY

#### WORKORDER 0804565

<b>Client</b>	<b>Phone</b>	<b>Date Promised:</b> 05/08/08
Ms. Theresa Landgraff	631-760-9300 x 12	<b>Date Completed:</b> 5/7/08
GEI Consultants, Inc.		<b>Date Received:</b> 4/24/08
110 Walt Whitman Road	<b>Fax</b>	<b>PO#:</b> NR
Suite 204		<b>Project#:</b> 061140-8-1703 BayShore OU1 Southern cell
Huntington Station, NY 11746		Air Monitorin
<b>Sales Rep:</b> TB		<b>Total \$:</b> \$ 624.00
		<b>Logged By:</b> MG

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A	AMS UW	Modified TO-15	4/23/2008	3.0 "Hg	\$225.00
02A	AMS DW	Modified TO-15	4/23/2008	6.5 "Hg	\$225.00
03A	Lab Blank	Modified TO-15	NA	NA	\$0.00
04A	CCV	Modified TO-15	NA	NA	\$0.00
05A	LCS	Modified TO-15	NA	NA	\$0.00
Misc. Charges 6 Liter Summa Canister (2) @ \$50.00 each., Shipment 58428					\$100.00
Blue Body Flow Controller (2) @ \$35.00 each., Shipment 58428					\$70.00
Fuel Surcharge (2) @ \$2.00 each.					\$4.00

**Note:** Samples received after 3 P.M. PST are considered to be received on the following work day.  
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

**BILL TO:** Ms. Theresa Landgraff  
GEI Consultants, Inc.  
110 Walt Whitman Road  
Suite 204  
Huntington Station, NY 11746

Analysis Code: TO-14A

**TERMS:**

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630  
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

## **Other Records**

## DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

## DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

# Compound Listing

## Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	



# Compound Listing

## Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	

DATA REVIEW CHECKLIST

Work Order #:

0804565

A R T M Q

- Analysis/Reporting vs. Project Profile/SOP requirements checked (i.e. 100% Dups, J-Flag to MDL, etc)
The final report has the correct reporting list, special units, and header info.
Lab Narrative is correct (proper method & description/Receiving & Analytical notes correct)
Corrective Action issued - #
Unusual circumstances have been documented in the notes section below

LUMEN validation report present and initialed

CIRCLE (YES / NO)

- Lab Blank, CCV, LCS and DUP met QC criteria
Hold time is met for all samples
Appropriate data qualifier flags are applied
Manual integrations for samples and QC are properly documented
Samples analyzed within the project or method specific clock
Retention times have been verified
Appropriate ICAL(s) included
At least one result per sample is verified against the target quant sheets/raw data

- Dilution factor correctly calculated (sample load volume, syringe and bag dilutions, can pressurization(s))
Correct amount of sample analyzed (i.e. sample not over-diluted)
Spectra verified - documentation of spectral defense included (Section 5A of eCVP pkg)
TICs resemble reference spectra
TICs between duplicate samples are consistent
Checked samples for trends (i.e. Influent>Effluent, Landfill or Ambient etc)
Special units for all samples in the final report are correctly calculated
Manually entered results checked (i.e. special CCV compounds)
TPH/NMOC (verify calculations and correct reference compound used)
Chain of Custody scanned correctly
Verify sample id's vs. chain of custody
Samples pressurized w/ appropriate gas (N2 or He)
Final pressure consistent with canister size (6L vs. 1L)
Verify receipt pressures against logbook and Target
Verify canister ID #'s
Extra printed copies are provided per client profile
Final invoice amount correct (adjusted for TAT, Penalties, Re-issue Charges etc.)
Client LUMEN report reviewed for accuracy and completeness

Notes: (to include: noting samples with QA/QC problems, Blanks with positive hits, narratives, etc.)

A/R: Doubt in CCV

M/Q:

(Analytical Review/Date) (Reporting Review/Date) (Management Review/Date) (QA Review/Date)
5/20/08 R: Mr 5/7/08 5/7/08

T:

**Not Applicable**