



***Air  
Toxics LTD.***  
*Laboratory Services Since 1989*

Electronic Comprehensive Validation Package (eCVP)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

### COMPREHENSIVE VALIDATION PACKAGE

Modified TO-15

### INVENTORY SHEET

Work Order #: 0807494

	Page Nos.	
	From	To
1. Work Order Cover Page & Laboratory Narrative	1	4
a. <u>Lumen Validation Report</u>	--	--
2. Sample Results and Raw Data (Organized by Sample)	5	27
a. ATL Sample Results Form		
b. Target Compound Raw Data		
-Internal Standard Area and Retention Time Summary		
-Surrogate Recovery Summary (If Applicable)		
-Chromatogram(s) and Ion Profiles (If Applicable)		
3. QC Results and Raw Data		
a. Method Blank (Results+ Raw Data)	28	35
b. Surrogate Recover Summary Form (If Applicable)	36	36
c. Internal Standard Summary Form (If Applicable)	37	37
d. Duplicate Results Summary Sheet	--	--
e. Matrix Spike/Matrix Spike Duplicate (Results + Raw Data)	--	--
f. Initial Calibration Data (Summary Sheet + Raw Data)	38	133
g. MDL Study (If Applicable)	--	--
h. Continuing Calibration Verification Data (Summary Sheet	134	148
i. Second Source LCS(Summary + Raw Data)	149	162
j. Extraction Logs	--	--
k. Instrument Run Logs/Software Verification	163	163
l. GC/MS Tune (Results + Raw Data)	164	171
4. Shipping/Receiving Documents		
a. Login Receipt Summary Sheet	172	173
b. Chain-of-Custody Records	174	174
c. Sample Log-In Sheet	175	175
d. Misc Shipping/Receiving Records (list of individual records)		
<u>Sample Receipt Discrepancy Report</u>	--	--
5. Other Records (describe or list)		
a. <u>Manual Spectral Defense</u>	--	--
b. <u>Manual Integrations</u>	--	--
c. <u>Manual Calculations</u>	--	--
d. <u>Canister Dilution Factors</u>	176	178
e. <u>Laboratory Corrective Action Request</u>	--	--
f. <u>CAS Number Reference</u>	179	180
g. <u>Variance Table</u>	--	--
h. <u>Canister Certification</u>	--	--
i. <u>Data Review Check Sheet</u>	181	181

Comments:

Completed by:

**Kara McKiernan**

Kara McKiernan / Document Control

8/12/08

(Signature)

( Print Name & Title)

(Date)



AN ENVIRONMENTAL ANALYTICAL LABORATORY

**WORK ORDER #: 0807494**

Work Order Summary

**CLIENT:** Ms. Theresa Landgraff  
GEI Consultants, Inc.  
110 Walt Whitman Road  
Suite 204  
Huntington Station, NY 11746

**BILL TO:** Ms. Theresa Landgraff  
GEI Consultants, Inc.  
110 Walt Whitman Road  
Suite 204  
Huntington Station, NY 11746

**PHONE:** 631-760-9300 x 12

**P.O. #** NR

**FAX:**

**PROJECT #** 061140-8-1703 BayShore OU1 Southern

**DATE RECEIVED:** 07/25/2008

**CONTACT:** cell Air Monitorin  
Bryanna Langley

**DATE COMPLETED:** 08/05/2008

<u>FRACTION #</u>	<u>NAME</u>	<u>TEST</u>	<u>RECEIPT VAC./PRES.</u>	<u>FINAL PRESSURE</u>
01A	AMS 4 DW	Modified TO-15	7.5 "Hg	5 psi
02A	AMS 3 DW	Modified TO-15	8.0 "Hg	5 psi
03A	Lab Blank	Modified TO-15	NA	NA
04A	CCV	Modified TO-15	NA	NA
05A	LCS	Modified TO-15	NA	NA

CERTIFIED BY: 

DATE: 08/06/08

Laboratory Director

Certification numbers: CA NELAP - 02110CA, LA NELAP/LELAP- AI 30763, NJ NELAP - CA004  
NY NELAP - 11291, UT NELAP - 9166389892, AZ Licensure AZ0719

Name of Accrediting Agency: NELAP/Florida Department of Health, Scope of Application: Clean Air Act,  
Accreditation number: E87680, Effective date: 07/01/07, Expiration date: 06/30/08

Air Toxics Ltd. certifies that the test results contained in this report meet all requirements of the NELAC standards

This report shall not be reproduced, except in full, without the written approval of Air Toxics Ltd.

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630  
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

**LABORATORY NARRATIVE**

**Modified TO-15  
GEI Consultants, Inc.  
Workorder# 0807494**

Two 6 Liter Summa Canister samples were received on July 25, 2008. The laboratory performed analysis via modified EPA Method TO-15 using GC/MS in the full scan mode. The method involves concentrating up to 0.2 liters of air. The concentrated aliquot is then flash vaporized and swept through a water management system to remove water vapor. Following dehumidification, the sample passes directly into the GC/MS for analysis.

This workorder was independently validated prior to submittal using 'USEPA National Functional Guidelines' as generally applied to the analysis of volatile organic compounds in air. A rules-based, logic driven, independent validation engine was employed to assess completeness, evaluate pass/fail of relevant project quality control requirements and verification of all quantified amounts.

Method modifications taken to run these samples are summarized in the table below. Specific project requirements may over-ride the ATL modifications.

<i>Requirement</i>	<i>TO-15</i>	<i>ATL Modifications</i>
Daily CCV	<= 30% Difference	<= 30% Difference; Compounds exceeding this criterion and associated data are flagged and narrated.
Sample collection media	Summa canister	ATL recommends use of summa canisters to insure data defensibility, but will report results from Tedlar bags at client request
Method Detection Limit	Follow 40CFR Pt.136 App. B	The MDL met all relevant requirements in Method TO-15 (statistical MDL less than the LOQ). The concentration of the spiked replicate may have exceeded 10X the calculated MDL in some cases

**Receiving Notes**

There were no receiving discrepancies.

**Analytical Notes**

There were no analytical discrepancies.

**Definition of Data Qualifying Flags**

Eight qualifiers may have been used on the data analysis sheets and indicates as follows:

B - Compound present in laboratory blank greater than reporting limit (background subtraction no performed).

J - Estimated value.

E - Exceeds instrument calibration range.

S - Saturated peak.

Q - Exceeds quality control limits.



---

AN ENVIRONMENTAL ANALYTICAL LABORATORY

- U - Compound analyzed for but not detected above the reporting limit.
- UJ- Non-detected compound associated with low bias in the CCV
- N - The identification is based on presumptive evidence.

File extensions may have been used on the data analysis sheets and indicates as follows:

- a-File was requantified
- b-File was quantified by a second column and detector
- r1-File was requantified for the purpose of reissue

**Table 1**

<b>Client Sample ID</b>	<b>Lab Sample ID</b>	<b>Date Collected</b>	<b>Date Received</b>	<b>Date Extracted</b>	<b>Sample Holding Time (Days)</b>	<b>Date Analyzed</b>	<b>Sample Extract Holding Time (Days)</b>	<b>Sample Condition</b>
AMS 4 DW	0807494-01A	7/23/2008	7/25/2008	NA	12	8/ 4/2008	NA	Good
AMS 3 DW	0807494-02A	7/23/2008	7/25/2008	NA	12	8/ 4/2008	NA	Good
Lab Blank	0807494-03A	NA	NA	NA	NA	8/ 4/2008	NA	Good
CCV	0807494-04A	NA	NA	NA	NA	8/ 4/2008	NA	Good
LCS	0807494-05A	NA	NA	NA	NA	8/ 4/2008	NA	Good

## **Sample Results and Raw Data**



AN ENVIRONMENTAL ANALYTICAL LABORATORY

## Summary of Detected Compounds MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: AMS 4 DW

Lab ID#: 0807494-01A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Acetone	3.6	8.0	8.5	19
Carbon Disulfide	0.90	8.2	2.8	26
2-Butanone (Methyl Ethyl Ketone)	0.90	2.4	2.6	7.0
Ethanol	3.6	4.1	6.7	7.8





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS 4 DW

Lab ID#: 0807494-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080406	Date of Collection: 7/23/08
Dil. Factor:	1.79	Date of Analysis: 8/4/08 01:39 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.90	Not Detected	4.4	Not Detected
Freon 114	0.90	Not Detected	6.2	Not Detected
Vinyl Chloride	0.90	Not Detected	2.3	Not Detected
Bromomethane	0.90	Not Detected	3.5	Not Detected
Chloroethane	0.90	Not Detected	2.4	Not Detected
Freon 11	0.90	Not Detected	5.0	Not Detected
1,1-Dichloroethene	0.90	Not Detected	3.5	Not Detected
Freon 113	0.90	Not Detected	6.8	Not Detected
Methylene Chloride	0.90	Not Detected	3.1	Not Detected
1,1-Dichloroethane	0.90	Not Detected	3.6	Not Detected
cis-1,2-Dichloroethene	0.90	Not Detected	3.5	Not Detected
Chloroform	0.90	Not Detected	4.4	Not Detected
1,1,1-Trichloroethane	0.90	Not Detected	4.9	Not Detected
Carbon Tetrachloride	0.90	Not Detected	5.6	Not Detected
Benzene	0.90	Not Detected	2.8	Not Detected
1,2-Dichloroethane	0.90	Not Detected	3.6	Not Detected
Trichloroethene	0.90	Not Detected	4.8	Not Detected
1,2-Dichloropropane	0.90	Not Detected	4.1	Not Detected
cis-1,3-Dichloropropene	0.90	Not Detected	4.1	Not Detected
Toluene	0.90	Not Detected	3.4	Not Detected
trans-1,3-Dichloropropene	0.90	Not Detected	4.1	Not Detected
1,1,2-Trichloroethane	0.90	Not Detected	4.9	Not Detected
Tetrachloroethene	0.90	Not Detected	6.1	Not Detected
1,2-Dibromoethane (EDB)	0.90	Not Detected	6.9	Not Detected
Chlorobenzene	0.90	Not Detected	4.1	Not Detected
Ethyl Benzene	0.90	Not Detected	3.9	Not Detected
m,p-Xylene	0.90	Not Detected	3.9	Not Detected
o-Xylene	0.90	Not Detected	3.9	Not Detected
Styrene	0.90	Not Detected	3.8	Not Detected
1,1,2,2-Tetrachloroethane	0.90	Not Detected	6.1	Not Detected
1,3,5-Trimethylbenzene	0.90	Not Detected	4.4	Not Detected
1,2,4-Trimethylbenzene	0.90	Not Detected	4.4	Not Detected
1,3-Dichlorobenzene	0.90	Not Detected	5.4	Not Detected
1,4-Dichlorobenzene	0.90	Not Detected	5.4	Not Detected
alpha-Chlorotoluene	0.90	Not Detected	4.6	Not Detected
1,2-Dichlorobenzene	0.90	Not Detected	5.4	Not Detected
1,3-Butadiene	0.90	Not Detected	2.0	Not Detected
Hexane	0.90	Not Detected	3.2	Not Detected
Cyclohexane	0.90	Not Detected	3.1	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS 4 DW

Lab ID#: 0807494-01A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080406	Date of Collection: 7/23/08
Dil. Factor:	1.79	Date of Analysis: 8/4/08 01:39 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.90	Not Detected	3.7	Not Detected
Bromodichloromethane	0.90	Not Detected	6.0	Not Detected
Dibromochloromethane	0.90	Not Detected	7.6	Not Detected
Cumene	0.90	Not Detected	4.4	Not Detected
Propylbenzene	0.90	Not Detected	4.4	Not Detected
Chloromethane	3.6	Not Detected	7.4	Not Detected
1,2,4-Trichlorobenzene	3.6	Not Detected	26	Not Detected
Hexachlorobutadiene	3.6	Not Detected	38	Not Detected
Acetone	3.6	8.0	8.5	19
Carbon Disulfide	0.90	8.2	2.8	26
2-Propanol	3.6	Not Detected	8.8	Not Detected
trans-1,2-Dichloroethene	0.90	Not Detected	3.5	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.90	2.4	2.6	7.0
Tetrahydrofuran	0.90	Not Detected	2.6	Not Detected
1,4-Dioxane	3.6	Not Detected	13	Not Detected
4-Methyl-2-pentanone	0.90	Not Detected	3.7	Not Detected
2-Hexanone	3.6	Not Detected	15	Not Detected
Bromoform	0.90	Not Detected	9.2	Not Detected
4-Ethyltoluene	0.90	Not Detected	4.4	Not Detected
Ethanol	3.6	4.1	6.7	7.8
Methyl tert-butyl ether	0.90	Not Detected	3.2	Not Detected
3-Chloropropene	3.6	Not Detected	11	Not Detected
2,2,4-Trimethylpentane	0.90	Not Detected	4.2	Not Detected
Naphthalene	3.6	Not Detected	19	Not Detected

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	100	70-130
1,2-Dichloroethane-d4	102	70-130
4-Bromofluorobenzene	99	70-130

Report Date: 05-Aug-2008 15:38

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/04Aug2008.b/g080406.d  
 Lab Smp Id: 0807494-01A  
 Inj Date : 04-AUG-2008 13:39  
 Operator : mlk Inst ID: msdg.i  
 Smp Info : 500mL #34022  
 Misc Info : 7.5"Hg ->5.0psi  
 Comment :  
 Method : /chem/msdg.i/04Aug2008.b/t14q702a.m  
 Meth Date : 05-Aug-2008 07:59 lrandolp Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1  
 Dil Factor: 1.79000  
 Integrator: HP RTE Compound Sublist: TO15qN.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPBV)	( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	301690	10.0000		80.00- 120.00	100.00	
9.002	9.002	(1.000)	128	245046			0.00- 30.00	81.22	
9.002	9.002	(1.000)	49	766961			0.00- 30.00	254.22	
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1209647	10.0000		80.00- 120.00	100.00	
10.186	10.186	(1.000)	88	200749			0.00- 47.07	16.60	
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1240009	10.0000		80.00- 120.00	100.00	
15.319	15.319	(1.000)	82	780675			0.00- 30.00	62.96	
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.667	9.668	(1.074)	65	588007	10.1546	10.154	80.00- 120.00	100.00	
9.667	9.668	(1.074)	67	273901			0.00- 30.00	46.58	
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1244407	9.95128	9.951	80.00- 120.00	100.00	
12.499	12.499	(1.227)	70	159348			0.00- 42.14	12.81	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== =====

\$ 59 Toluene-d8 (continued)

12.499 12.499 (1.227) 100 783015 33.87- 93.87 62.92

\$ 81 Bromofluorobenzene

CAS #: 460-00-4

17.226 17.226 (1.125) 174 711646 9.87945 9.879 80.00- 120.00 100.00

17.200 17.226 (1.123) 95 1066879 118.60- 178.60 149.92

17.226 17.226 (1.125) 176 674527 67.33- 127.33 94.78

17 Ethanol

CAS #: 64-17-5

6.225 6.225 (0.692) 45 48840 2.31513 4.144 80.00- 120.00 100.00

6.225 6.225 (0.692) 43 9811 0.00- 30.00 20.09

6.225 6.225 (0.692) 46 17439 0.00- 30.00 35.71

20 Carbon Disulfide

CAS #: 75-15-0

6.499 6.500 (0.722) 76 436154 4.58451 8.206 80.00- 120.00 100.00

21 Acetone

CAS #: 67-64-1

6.637 6.637 (0.737) 43 506435 4.48916 8.036 80.00- 120.00 100.00

6.637 6.637 (0.737) 58 106349 0.00- 30.00 21.00

37 2-Butanone

CAS #: 78-93-3

8.792 8.792 (0.977) 72 28603 1.31958 2.362 80.00- 120.00 100.00

8.792 8.792 (0.977) 43 244004 728.42- 788.42 853.05

8.792 8.792 (0.977) 57 13979 0.00- 30.00 48.87

Report Date: 05-Aug-2008 15:38

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 04-AUG-2008

Lab File ID: g080406.d

Calibration Time: 09:59

Lab Smp Id: 0807494-01A

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: mlk

Method File: /chem/msdg.i/04Aug2008.b/t14q702a.m

Misc Info: 7.5"Hg -&gt;5.0psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	318312	190987	445637	301690	-5.22
51 1,4-Difluorobenze	1208514	725108	1691920	1209647	0.09
72 Chlorobenzene-d5	1189759	713855	1665663	1240009	4.22

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 04Aug2008  
Sample Matrix: GAS Fraction: VOA  
Lab Smp Id: 0807494-01A  
Level: LOW Operator: mlk  
Data Type: MS DATA SampleType: SAMPLE  
SpikeList File: Spectra.spk Quant Type: ISTD  
Sublist File: T015qN.sub  
Method File: /chem/msdg.i/04Aug2008.b/t14q702a.m  
Misc Info: 7.5"Hg ->5.0psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 47 1,2-Dichloroethane	10.000	10.154	101.55	70-130
\$ 59 Toluene-d8	10.000	9.951	99.51	70-130
\$ 81 Bromofluorobenzene	10.000	9.879	98.79	70-130

Date : 04-AUG-2008 13:39

Client ID:


Instrument: msdg.i

Sample Info: 500mL #34022

Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

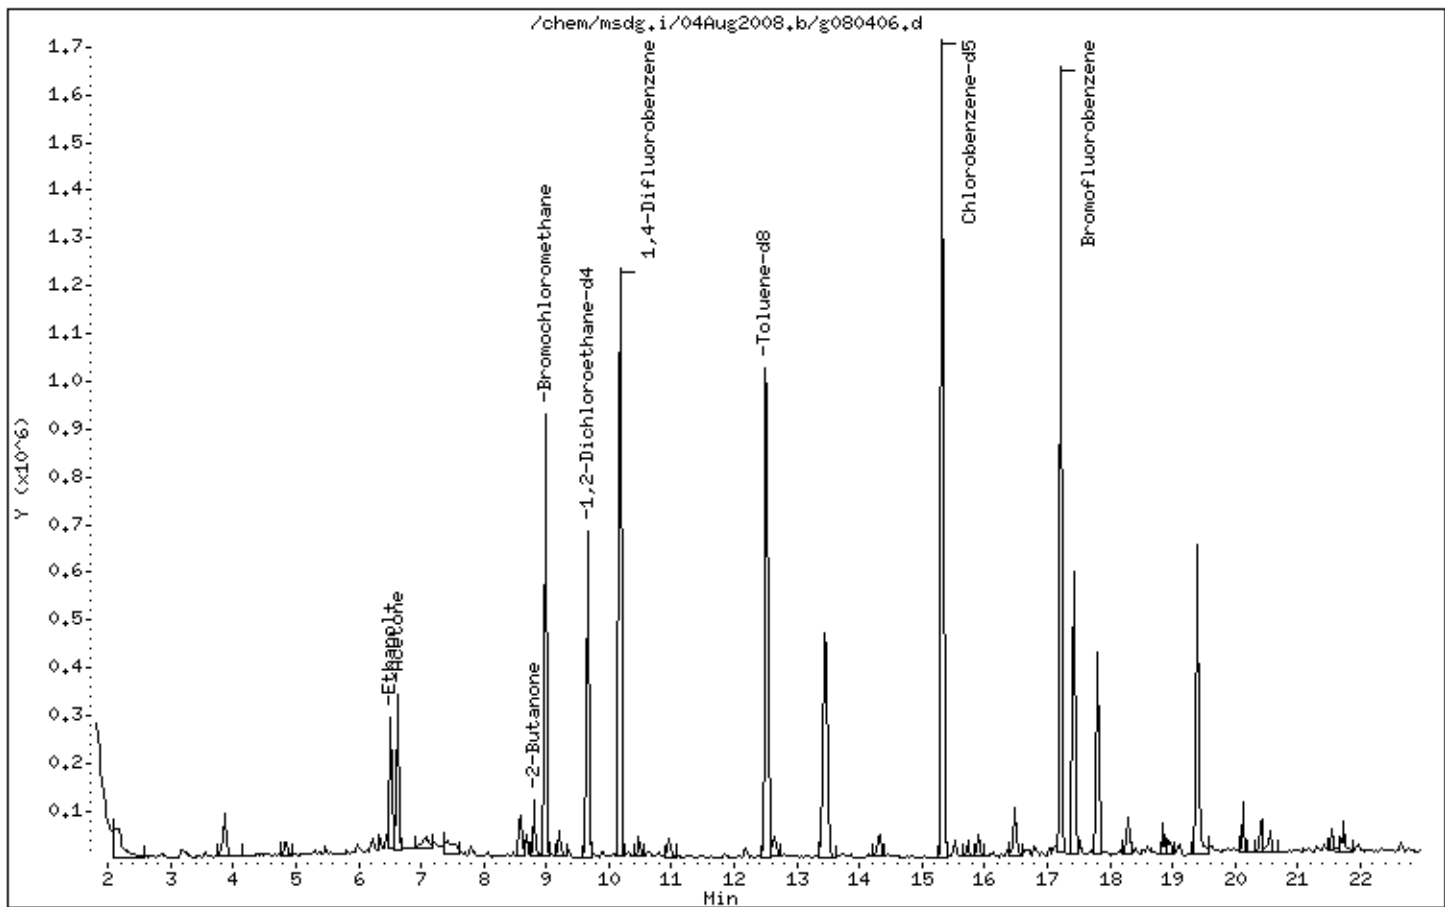

Date : 04-AUG-2008 13:39

Client ID:

Instrument: msdg.i

Sample Info: 500mL #34022








Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

17 Ethanol

Concentration: 4,144 PPBV

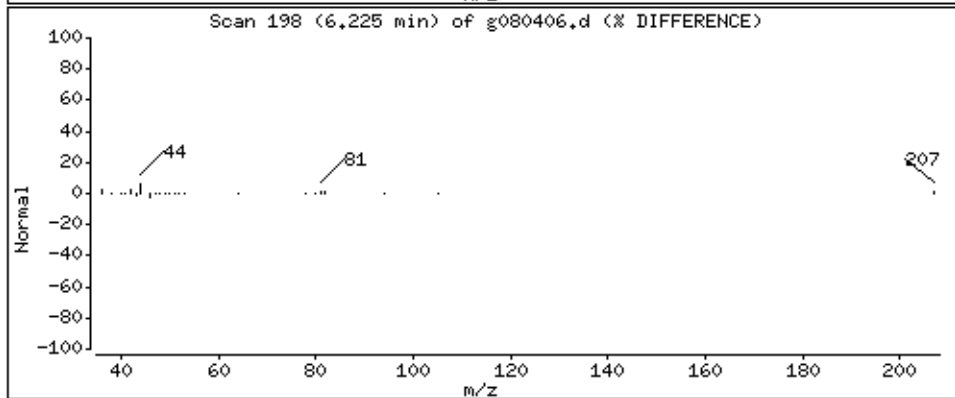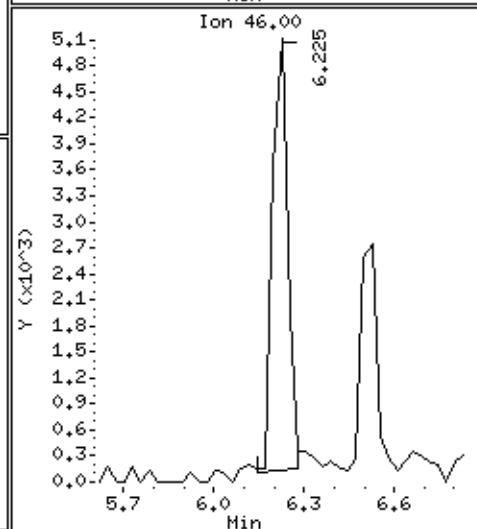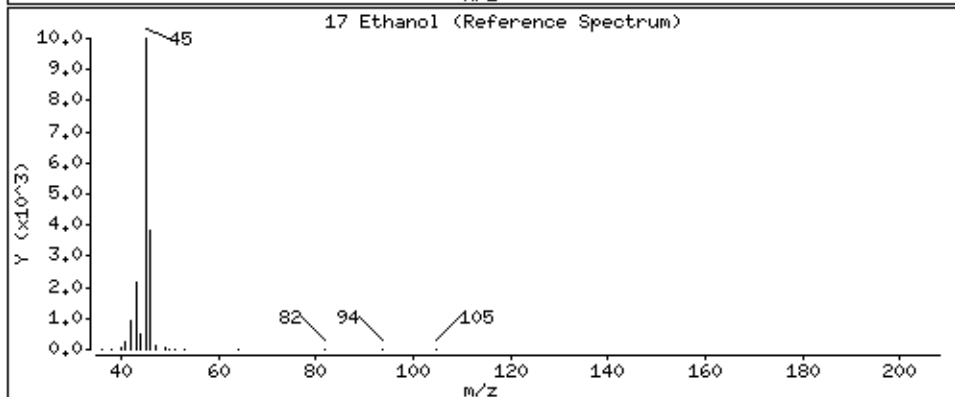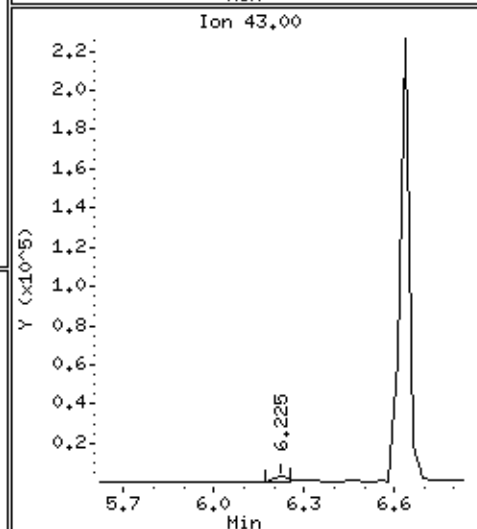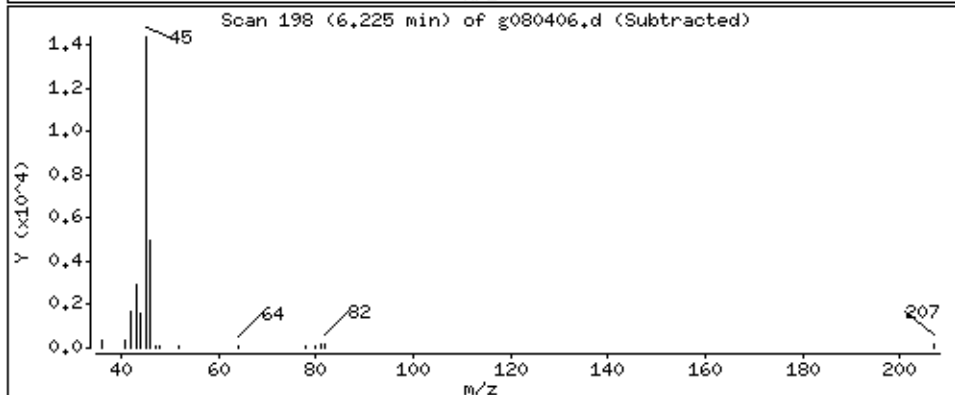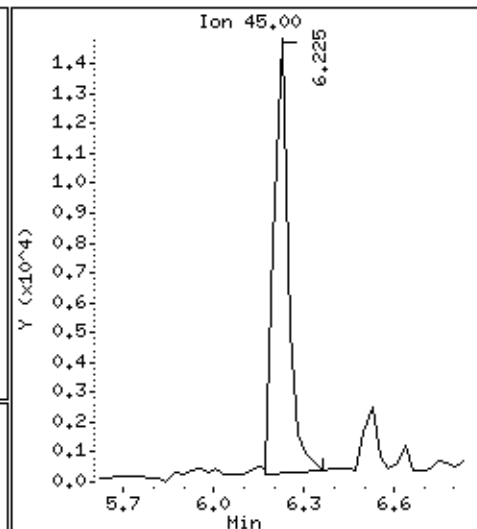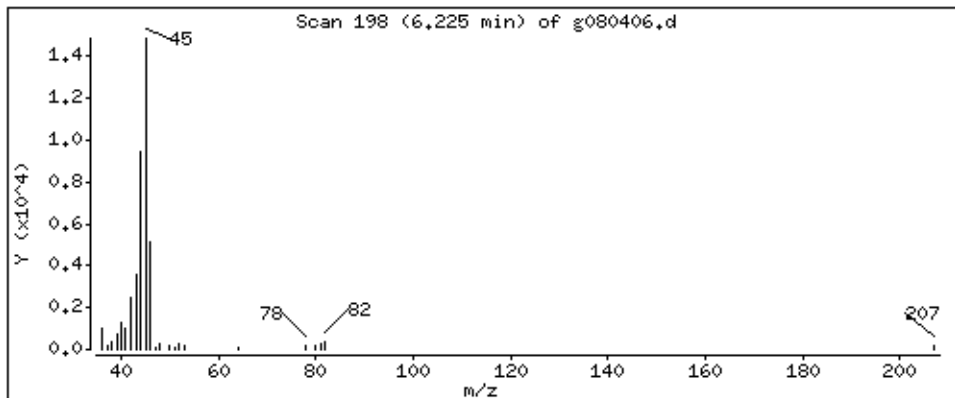



Date : 04-AUG-2008 13:39

Client ID:

Instrument: msdg.i

Sample Info: 500mL #34022






Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

20 Carbon Disulfide

Concentration: 8.206 PPBV

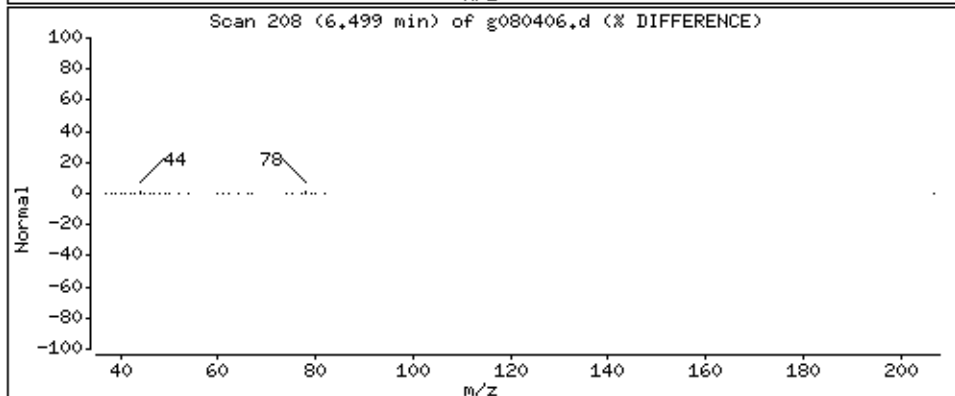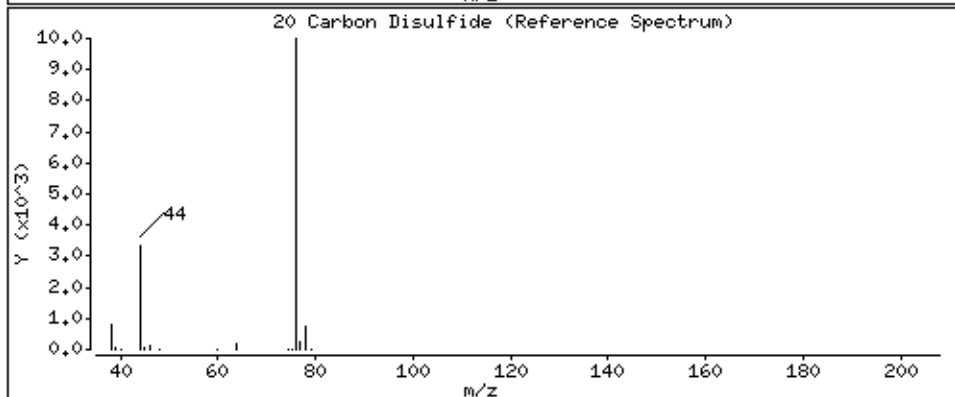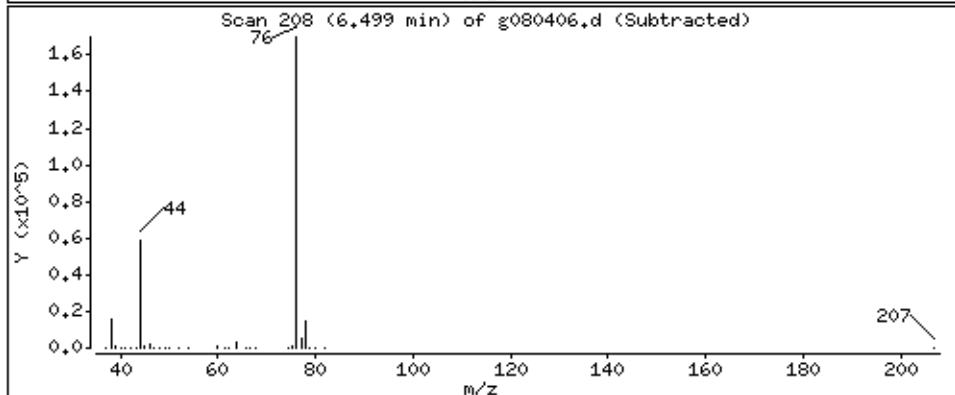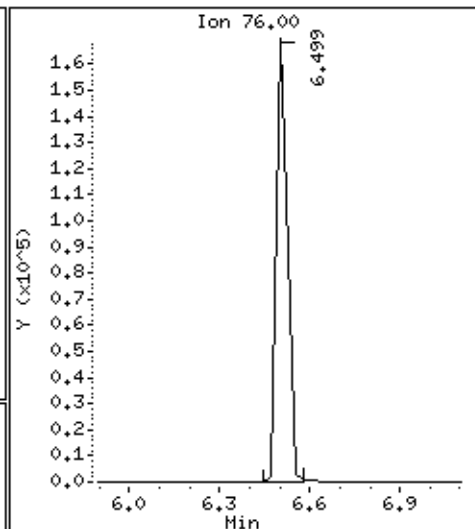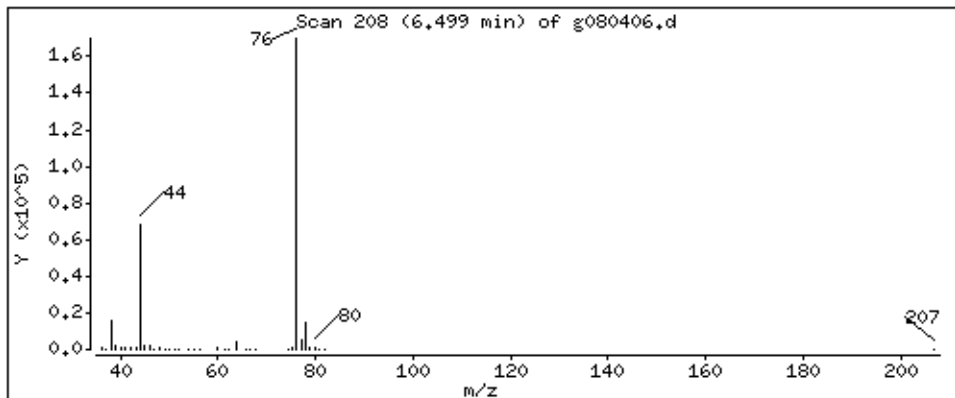

Date : 04-AUG-2008 13:39

Client ID:

Instrument: msdg.i

Sample Info: 500mL #34022







Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

21 Acetone

Concentration: 8.036 PPBV

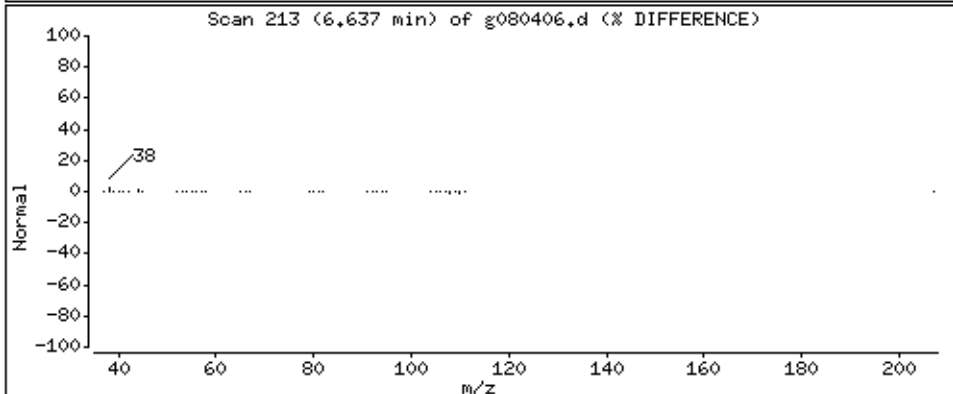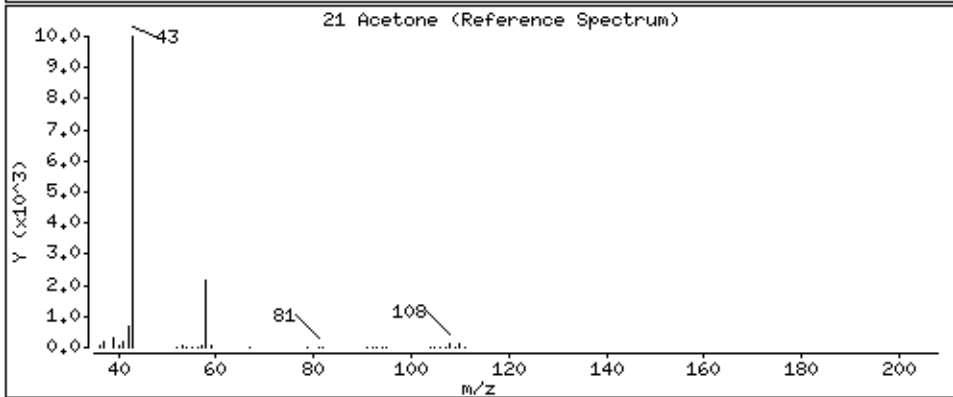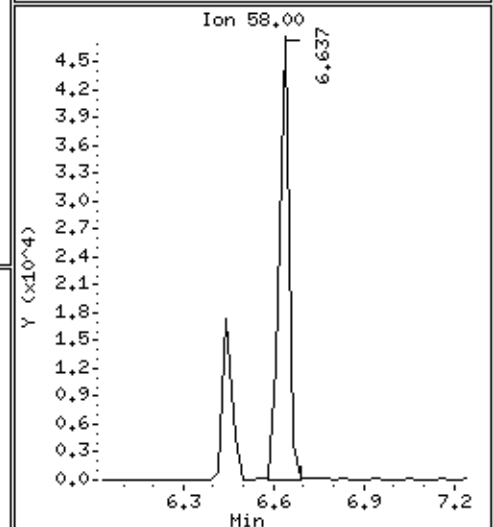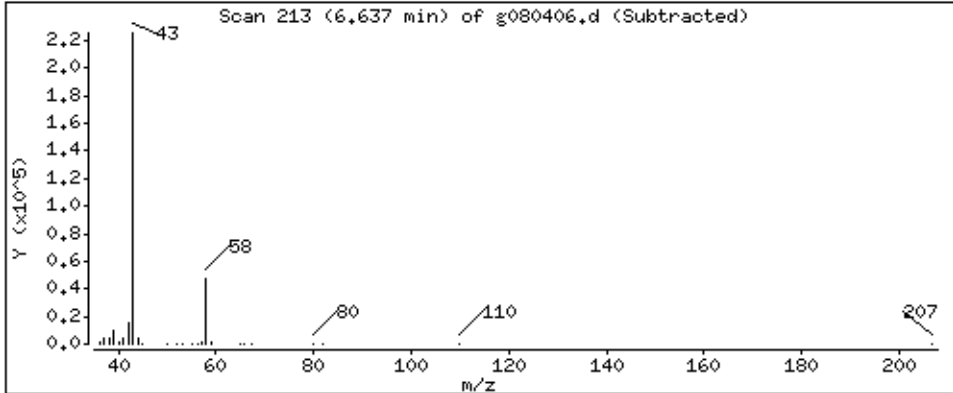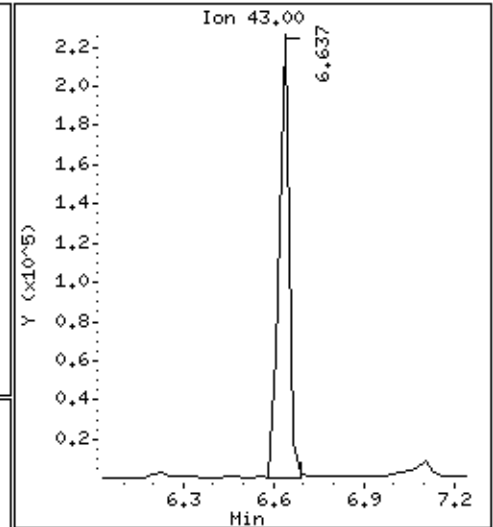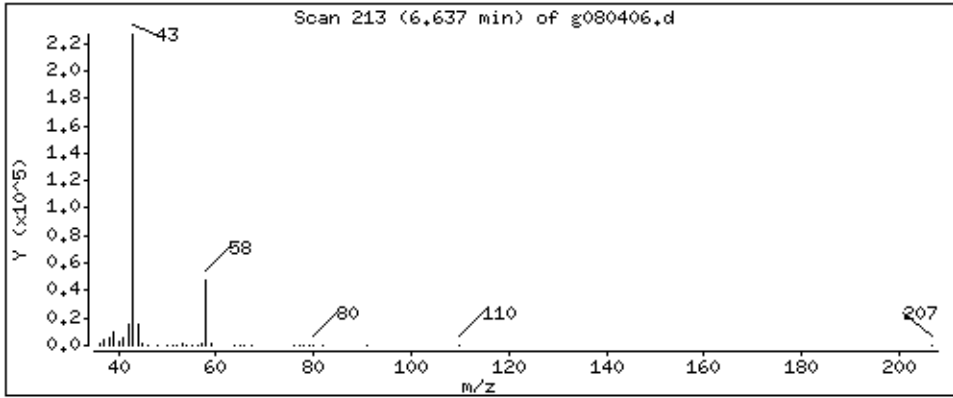

Date : 04-AUG-2008 13:39

Client ID:

Instrument: msdg.i

Sample Info: 500mL #34022








Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

37 2-Butanone

Concentration: 2,362 PPBV

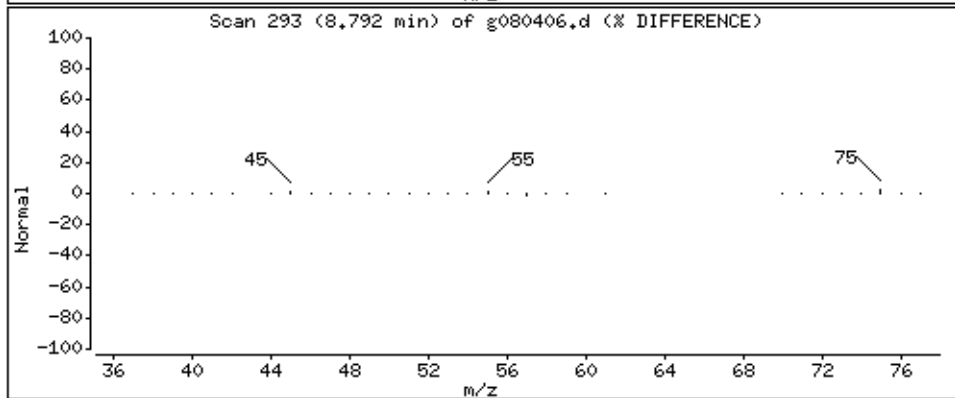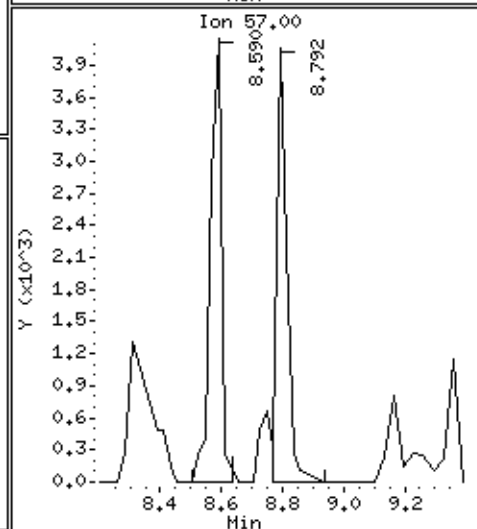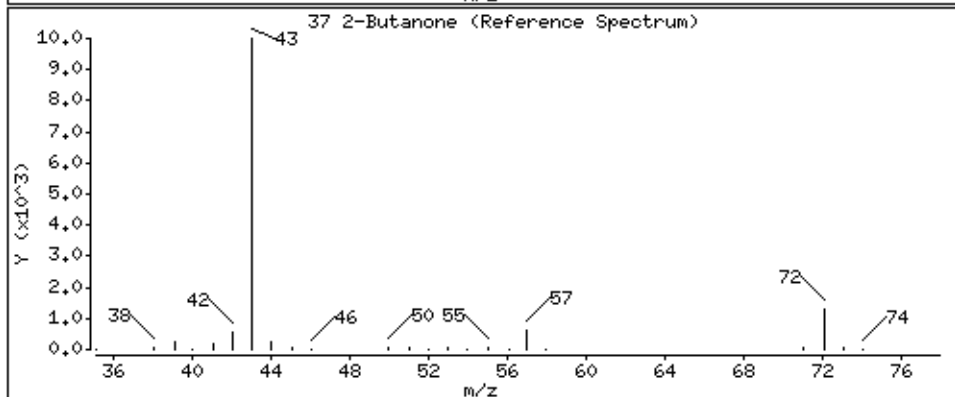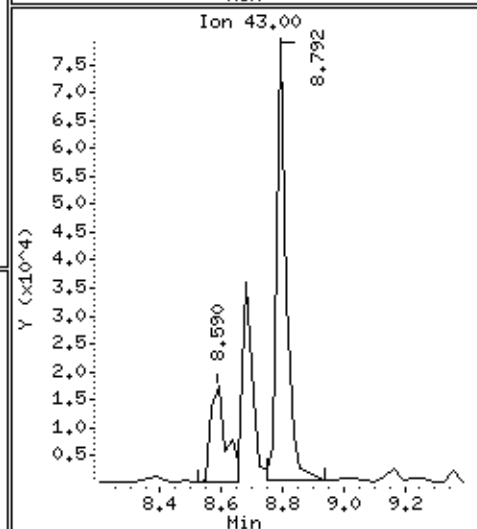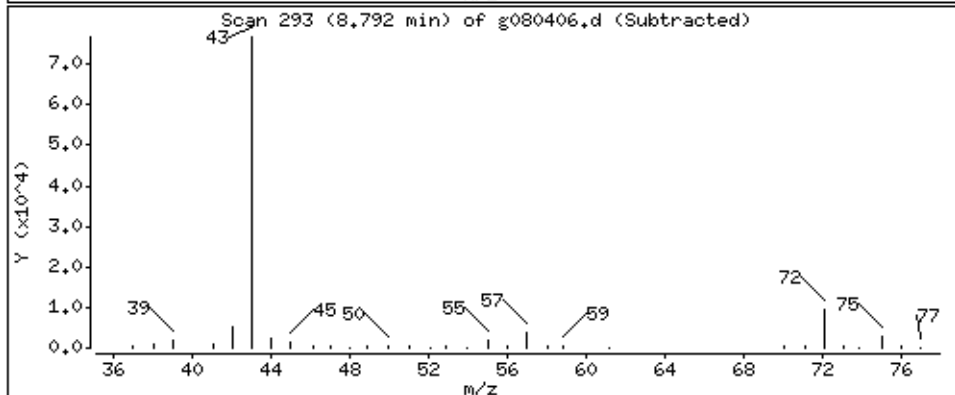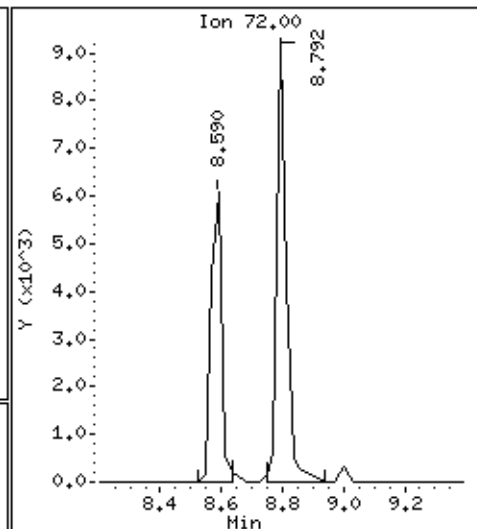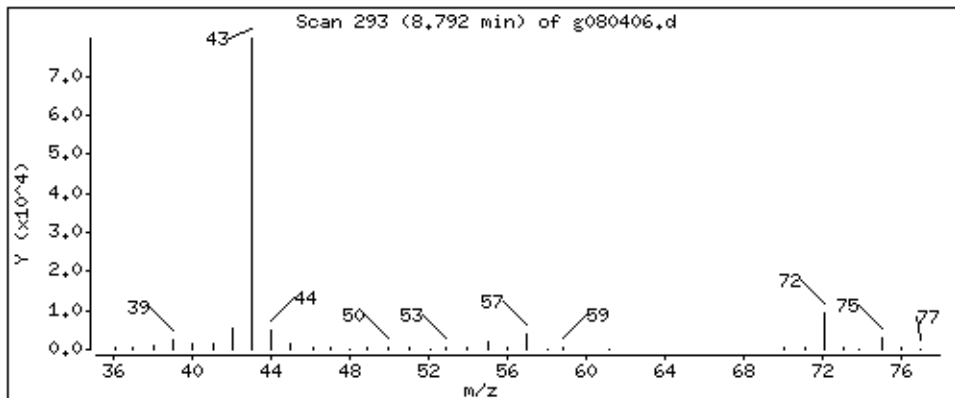



AN ENVIRONMENTAL ANALYTICAL LABORATORY

---

## Summary of Detected Compounds

### MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

Client Sample ID: AMS 3 DW

Lab ID#: 0807494-02A

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Acetone	3.7	4.8	8.7	11
Ethanol	3.7	3.4 J	6.9	6.4 J



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS 3 DW

Lab ID#: 0807494-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080407	Date of Collection: 7/23/08
Dil. Factor:	1.83	Date of Analysis: 8/4/08 02:26 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.92	Not Detected	4.5	Not Detected
Freon 114	0.92	Not Detected	6.4	Not Detected
Vinyl Chloride	0.92	Not Detected	2.3	Not Detected
Bromomethane	0.92	Not Detected	3.6	Not Detected
Chloroethane	0.92	Not Detected	2.4	Not Detected
Freon 11	0.92	Not Detected	5.1	Not Detected
1,1-Dichloroethene	0.92	Not Detected	3.6	Not Detected
Freon 113	0.92	Not Detected	7.0	Not Detected
Methylene Chloride	0.92	Not Detected	3.2	Not Detected
1,1-Dichloroethane	0.92	Not Detected	3.7	Not Detected
cis-1,2-Dichloroethene	0.92	Not Detected	3.6	Not Detected
Chloroform	0.92	Not Detected	4.5	Not Detected
1,1,1-Trichloroethane	0.92	Not Detected	5.0	Not Detected
Carbon Tetrachloride	0.92	Not Detected	5.8	Not Detected
Benzene	0.92	Not Detected	2.9	Not Detected
1,2-Dichloroethane	0.92	Not Detected	3.7	Not Detected
Trichloroethene	0.92	Not Detected	4.9	Not Detected
1,2-Dichloropropane	0.92	Not Detected	4.2	Not Detected
cis-1,3-Dichloropropene	0.92	Not Detected	4.2	Not Detected
Toluene	0.92	Not Detected	3.4	Not Detected
trans-1,3-Dichloropropene	0.92	Not Detected	4.2	Not Detected
1,1,2-Trichloroethane	0.92	Not Detected	5.0	Not Detected
Tetrachloroethene	0.92	Not Detected	6.2	Not Detected
1,2-Dibromoethane (EDB)	0.92	Not Detected	7.0	Not Detected
Chlorobenzene	0.92	Not Detected	4.2	Not Detected
Ethyl Benzene	0.92	Not Detected	4.0	Not Detected
m,p-Xylene	0.92	Not Detected	4.0	Not Detected
o-Xylene	0.92	Not Detected	4.0	Not Detected
Styrene	0.92	Not Detected	3.9	Not Detected
1,1,2,2-Tetrachloroethane	0.92	Not Detected	6.3	Not Detected
1,3,5-Trimethylbenzene	0.92	Not Detected	4.5	Not Detected
1,2,4-Trimethylbenzene	0.92	Not Detected	4.5	Not Detected
1,3-Dichlorobenzene	0.92	Not Detected	5.5	Not Detected
1,4-Dichlorobenzene	0.92	Not Detected	5.5	Not Detected
alpha-Chlorotoluene	0.92	Not Detected	4.7	Not Detected
1,2-Dichlorobenzene	0.92	Not Detected	5.5	Not Detected
1,3-Butadiene	0.92	Not Detected	2.0	Not Detected
Hexane	0.92	Not Detected	3.2	Not Detected
Cyclohexane	0.92	Not Detected	3.1	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: AMS 3 DW

Lab ID#: 0807494-02A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080407	Date of Collection:	7/23/08
Dil. Factor:	1.83	Date of Analysis:	8/4/08 02:26 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.92	Not Detected	3.7	Not Detected
Bromodichloromethane	0.92	Not Detected	6.1	Not Detected
Dibromochloromethane	0.92	Not Detected	7.8	Not Detected
Cumene	0.92	Not Detected	4.5	Not Detected
Propylbenzene	0.92	Not Detected	4.5	Not Detected
Chloromethane	3.7	Not Detected	7.6	Not Detected
1,2,4-Trichlorobenzene	3.7	Not Detected	27	Not Detected
Hexachlorobutadiene	3.7	Not Detected	39	Not Detected
Acetone	3.7	4.8	8.7	11
Carbon Disulfide	0.92	Not Detected	2.8	Not Detected
2-Propanol	3.7	Not Detected	9.0	Not Detected
trans-1,2-Dichloroethene	0.92	Not Detected	3.6	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.92	Not Detected	2.7	Not Detected
Tetrahydrofuran	0.92	Not Detected	2.7	Not Detected
1,4-Dioxane	3.7	Not Detected	13	Not Detected
4-Methyl-2-pentanone	0.92	Not Detected	3.7	Not Detected
2-Hexanone	3.7	Not Detected	15	Not Detected
Bromoform	0.92	Not Detected	9.4	Not Detected
4-Ethyltoluene	0.92	Not Detected	4.5	Not Detected
Ethanol	3.7	3.4 J	6.9	6.4 J
Methyl tert-butyl ether	0.92	Not Detected	3.3	Not Detected
3-Chloropropene	3.7	Not Detected	11	Not Detected
2,2,4-Trimethylpentane	0.92	Not Detected	4.3	Not Detected
Naphthalene	3.7	Not Detected	19	Not Detected

J = Estimated value.

Container Type: 6 Liter Summa Canister

Surrogates	%Recovery	Method Limits
Toluene-d8	102	70-130
1,2-Dichloroethane-d4	97	70-130
4-Bromofluorobenzene	96	70-130

Report Date: 05-Aug-2008 15:39

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/04Aug2008.b/g080407.d  
 Lab Smp Id: 0807494-02A  
 Inj Date : 04-AUG-2008 14:26  
 Operator : mlk Inst ID: msdg.i  
 Smp Info : 500mL #24233  
 Misc Info : 8.0"Hg ->5.0psi  
 Comment :  
 Method : /chem/msdg.i/04Aug2008.b/t14q702a.m  
 Meth Date : 05-Aug-2008 07:59 lrandolp Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1  
 Dil Factor: 1.83000  
 Integrator: HP RTE Compound Sublist: TO15qN.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPBV)	( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	321816	10.0000		80.00- 120.00	100.00	
9.002	9.002	(1.000)	128	248013			0.00- 30.00	77.07	
9.002	9.002	(1.000)	49	781168			0.00- 30.00	242.74	
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1218887	10.0000		80.00- 120.00	100.00	
10.186	10.186	(1.000)	88	197082			0.00- 47.07	16.17	
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1225378	10.0000		80.00- 120.00	100.00	
15.319	15.319	(1.000)	82	773214			0.00- 30.00	63.10	
-----									
§ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668	(1.074)	65	598620	9.69134	9.691	80.00- 120.00	100.00	
9.668	9.668	(1.074)	67	284305			0.00- 30.00	47.49	
-----									
§ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1286416	10.2092	10.209	80.00- 120.00	100.00	
12.499	12.499	(1.227)	70	159634			0.00- 42.14	12.41	

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 59 Toluene-d8 (continued)

12.499	12.499	(1.227)	100	814743			33.87- 93.87	63.33
--------	--------	---------	-----	--------	--	--	--------------	-------

\$ 81 Bromofluorobenzene

CAS #: 460-00-4

17.226	17.226	(1.125)	174	680181	9.55538	9.555	80.00- 120.00	100.00
17.201	17.226	(1.123)	95	1021216			118.60- 178.60	150.14
17.226	17.226	(1.125)	176	670205			67.33- 127.33	98.53

17 Ethanol

CAS #: 64-17-5

6.225	6.225	(0.692)	45	41989	1.86590	3.415	80.00- 120.00	100.00(a)
6.225	6.225	(0.692)	43	10293			0.00- 30.00	24.51
6.225	6.225	(0.692)	46	17912			0.00- 30.00	42.66

21 Acetone

CAS #: 67-64-1

6.637	6.637	(0.737)	43	315102	2.61846	4.792	80.00- 120.00	100.00
6.637	6.637	(0.737)	58	65551			0.00- 30.00	20.80

QC Flag Legend

a - Target compound detected but, quantitated amount  
Below Limit Of Quantitation(BLOQ).



Report Date: 05-Aug-2008 15:39

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 04-AUG-2008

Lab File ID: g080407.d

Calibration Time: 09:59

Lab Smp Id: 0807494-02A

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: mlk

Method File: /chem/msdg.i/04Aug2008.b/t14q702a.m

Misc Info: 8.0"Hg -&gt;5.0psi

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	318312	190987	445637	321816	1.10
51 1,4-Difluorobenze	1208514	725108	1691920	1218887	0.86
72 Chlorobenzene-d5	1189759	713855	1665663	1225378	2.99

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 04Aug2008  
Sample Matrix: GAS Fraction: VOA  
Lab Smp Id: 0807494-02A  
Level: LOW Operator: mlk  
Data Type: MS DATA SampleType: SAMPLE  
SpikeList File: Spectra.spk Quant Type: ISTD  
Sublist File: T015qN.sub  
Method File: /chem/msdg.i/04Aug2008.b/t14q702a.m  
Misc Info: 8.0"Hg ->5.0psi

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 47 1,2-Dichloroethane	10.000	9.691	96.91	70-130
\$ 59 Toluene-d8	10.000	10.209	102.09	70-130
\$ 81 Bromofluorobenzene	10.000	9.555	95.55	70-130

Date : 04-AUG-2008 14:26

Client ID:


Instrument: msdg,i

Sample Info: 500mL #24233

Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

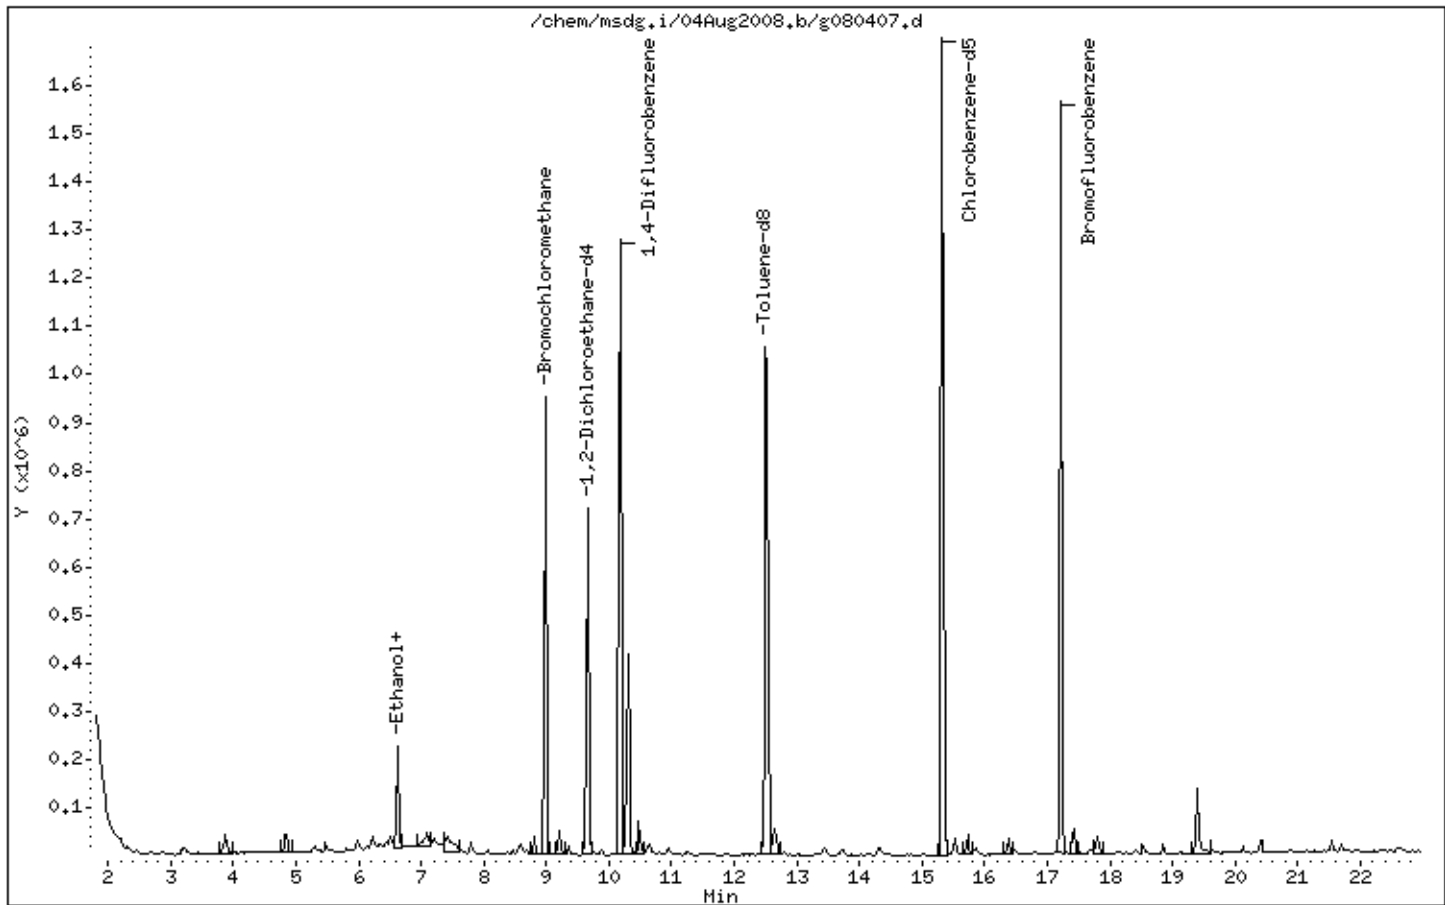

Date : 04-AUG-2008 14:26

Client ID:

Instrument: msdg.i

Sample Info: 500mL #24233








Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

17 Ethanol

Concentration: 3.415 PPBV

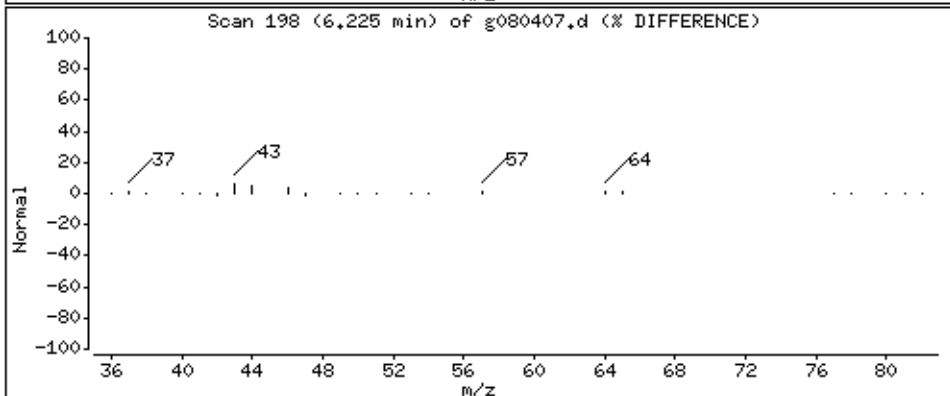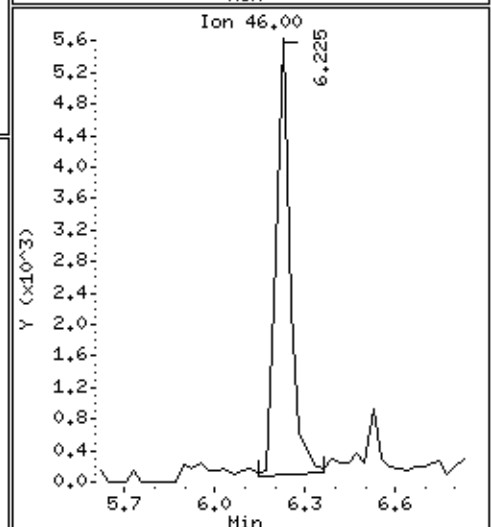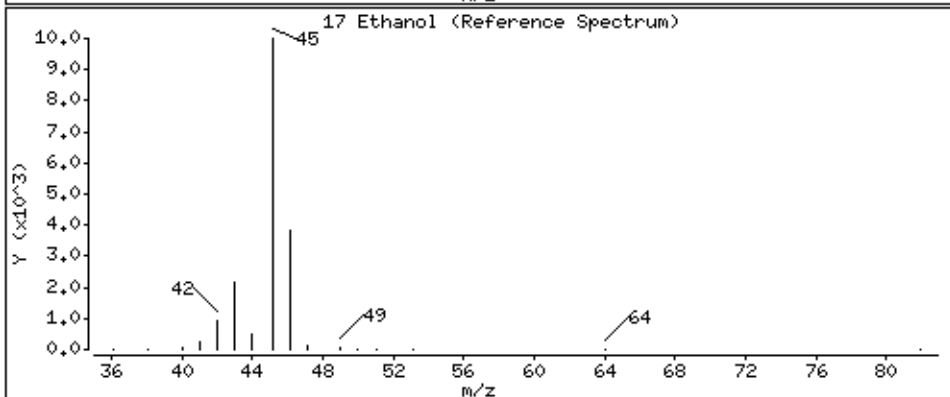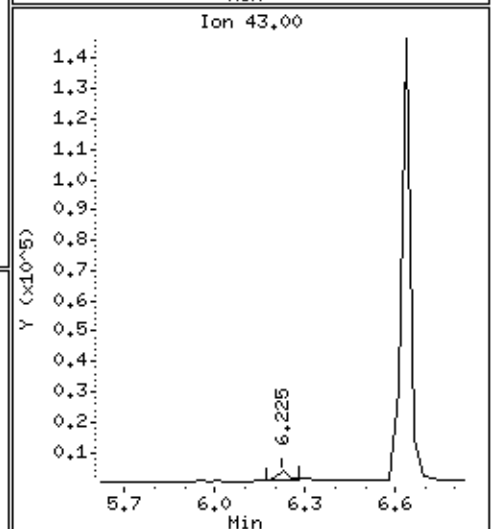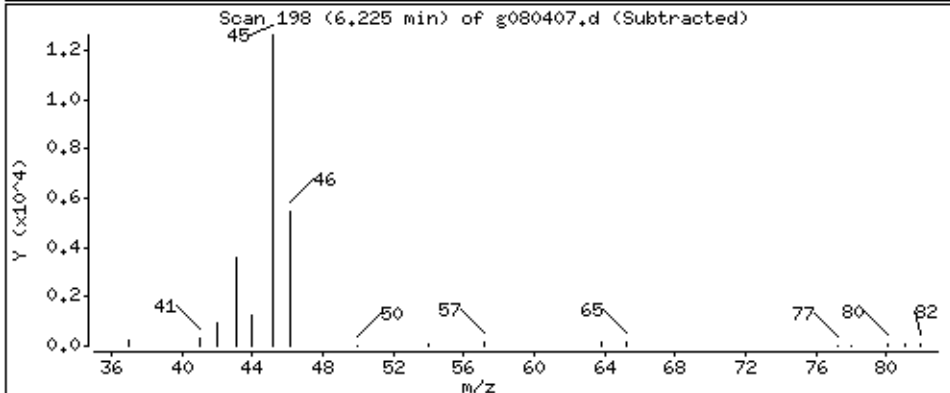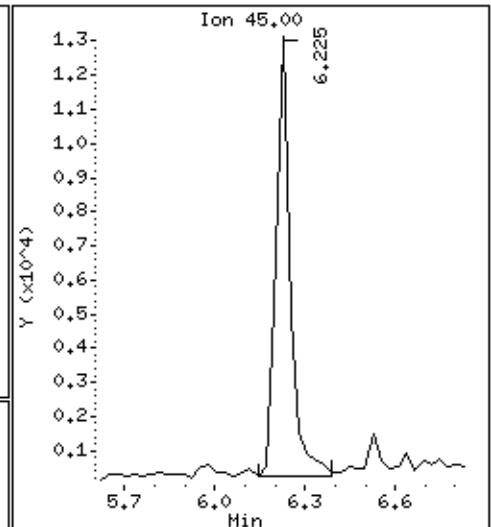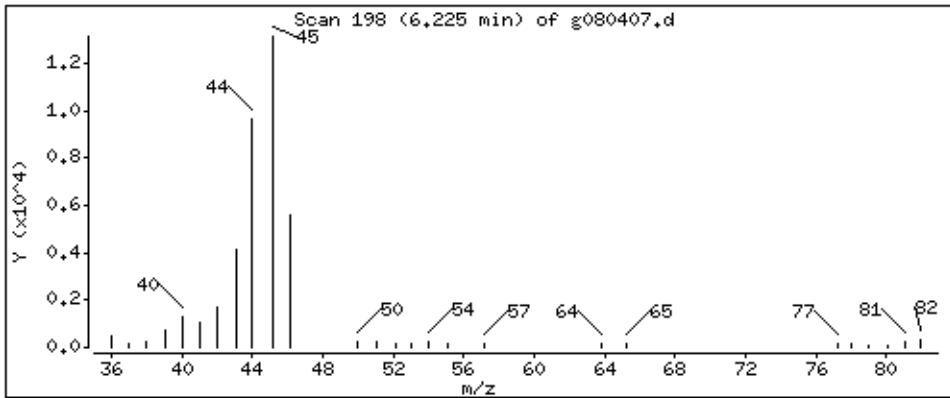

Date : 04-AUG-2008 14:26

Client ID:

Instrument: msdg.i

Sample Info: 500mL #24233







Operator: mlk

Column phase: RTX-624

Column diameter: 0.32

21 Acetone

Concentration: 4.792 PPBV

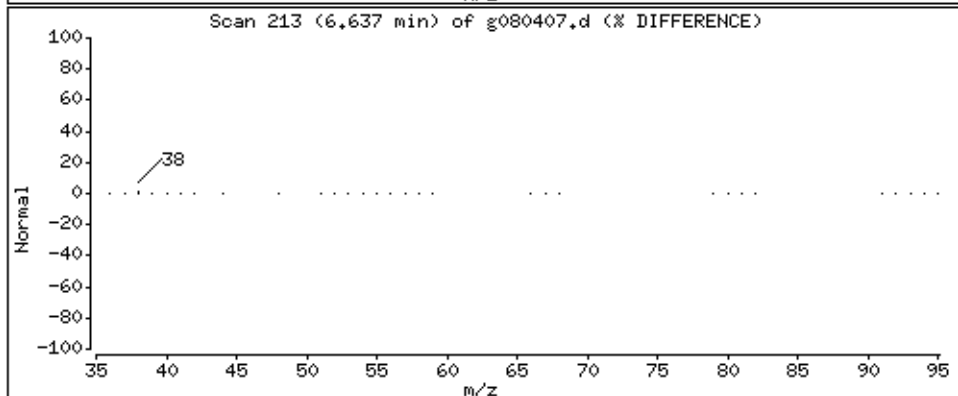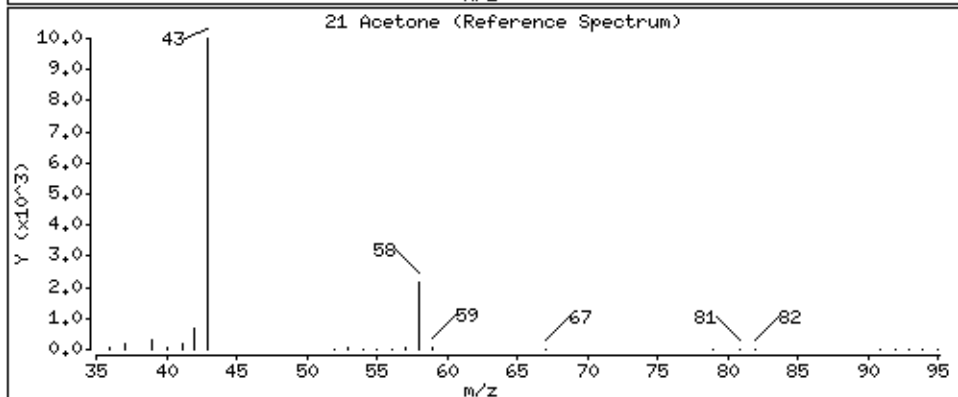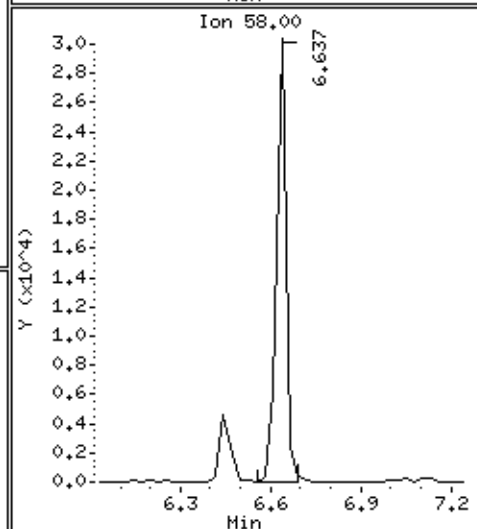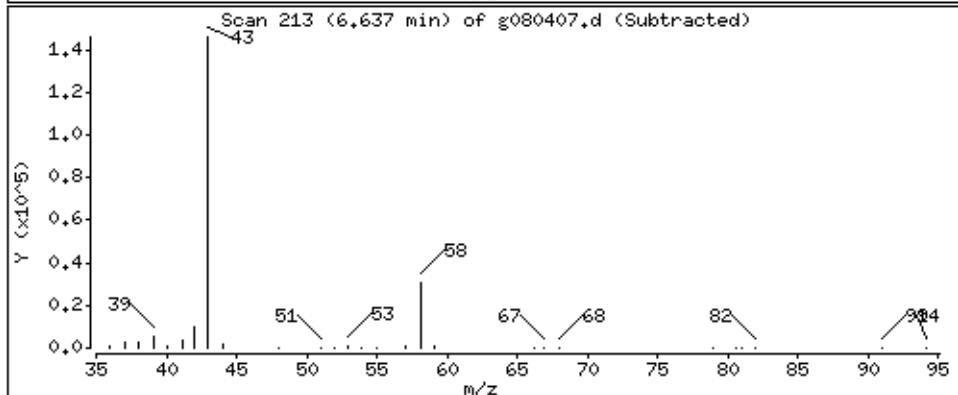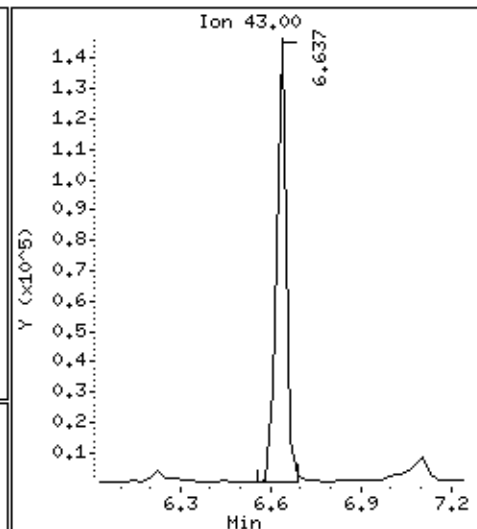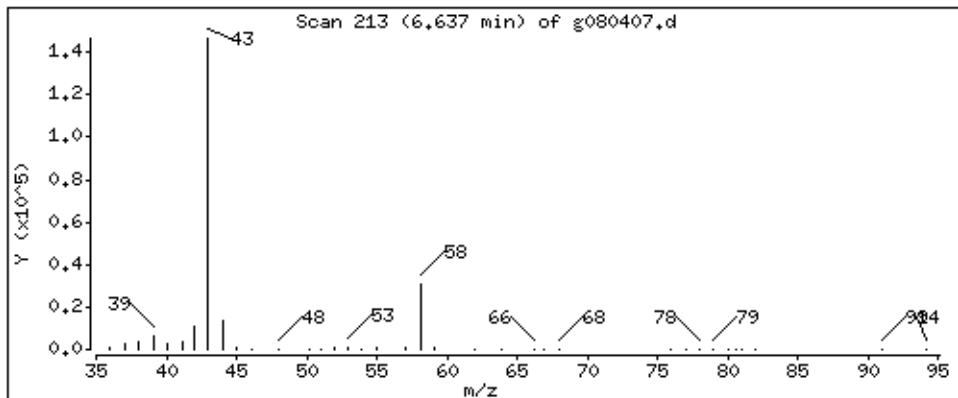

## **QC Results and Raw Data**



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0807494-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080405	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 8/4/08 12:46 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Freon 12	0.50	Not Detected	2.5	Not Detected
Freon 114	0.50	Not Detected	3.5	Not Detected
Vinyl Chloride	0.50	Not Detected	1.3	Not Detected
Bromomethane	0.50	Not Detected	1.9	Not Detected
Chloroethane	0.50	Not Detected	1.3	Not Detected
Freon 11	0.50	Not Detected	2.8	Not Detected
1,1-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Freon 113	0.50	Not Detected	3.8	Not Detected
Methylene Chloride	0.50	Not Detected	1.7	Not Detected
1,1-Dichloroethane	0.50	Not Detected	2.0	Not Detected
cis-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
Chloroform	0.50	Not Detected	2.4	Not Detected
1,1,1-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Carbon Tetrachloride	0.50	Not Detected	3.1	Not Detected
Benzene	0.50	Not Detected	1.6	Not Detected
1,2-Dichloroethane	0.50	Not Detected	2.0	Not Detected
Trichloroethene	0.50	Not Detected	2.7	Not Detected
1,2-Dichloropropane	0.50	Not Detected	2.3	Not Detected
cis-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
Toluene	0.50	Not Detected	1.9	Not Detected
trans-1,3-Dichloropropene	0.50	Not Detected	2.3	Not Detected
1,1,2-Trichloroethane	0.50	Not Detected	2.7	Not Detected
Tetrachloroethene	0.50	Not Detected	3.4	Not Detected
1,2-Dibromoethane (EDB)	0.50	Not Detected	3.8	Not Detected
Chlorobenzene	0.50	Not Detected	2.3	Not Detected
Ethyl Benzene	0.50	Not Detected	2.2	Not Detected
m,p-Xylene	0.50	Not Detected	2.2	Not Detected
o-Xylene	0.50	Not Detected	2.2	Not Detected
Styrene	0.50	Not Detected	2.1	Not Detected
1,1,2,2-Tetrachloroethane	0.50	Not Detected	3.4	Not Detected
1,3,5-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,2,4-Trimethylbenzene	0.50	Not Detected	2.4	Not Detected
1,3-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,4-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
alpha-Chlorotoluene	0.50	Not Detected	2.6	Not Detected
1,2-Dichlorobenzene	0.50	Not Detected	3.0	Not Detected
1,3-Butadiene	0.50	Not Detected	1.1	Not Detected
Hexane	0.50	Not Detected	1.8	Not Detected
Cyclohexane	0.50	Not Detected	1.7	Not Detected



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: Lab Blank

Lab ID#: 0807494-03A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080405	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 8/4/08 12:46 PM

Compound	Rpt. Limit (ppbv)	Amount (ppbv)	Rpt. Limit (uG/m3)	Amount (uG/m3)
Heptane	0.50	Not Detected	2.0	Not Detected
Bromodichloromethane	0.50	Not Detected	3.4	Not Detected
Dibromochloromethane	0.50	Not Detected	4.2	Not Detected
Cumene	0.50	Not Detected	2.4	Not Detected
Propylbenzene	0.50	Not Detected	2.4	Not Detected
Chloromethane	2.0	Not Detected	4.1	Not Detected
1,2,4-Trichlorobenzene	2.0	Not Detected	15	Not Detected
Hexachlorobutadiene	2.0	Not Detected	21	Not Detected
Acetone	2.0	Not Detected	4.8	Not Detected
Carbon Disulfide	0.50	Not Detected	1.6	Not Detected
2-Propanol	2.0	Not Detected	4.9	Not Detected
trans-1,2-Dichloroethene	0.50	Not Detected	2.0	Not Detected
2-Butanone (Methyl Ethyl Ketone)	0.50	Not Detected	1.5	Not Detected
Tetrahydrofuran	0.50	Not Detected	1.5	Not Detected
1,4-Dioxane	2.0	Not Detected	7.2	Not Detected
4-Methyl-2-pentanone	0.50	Not Detected	2.0	Not Detected
2-Hexanone	2.0	Not Detected	8.2	Not Detected
Bromoform	0.50	Not Detected	5.2	Not Detected
4-Ethyltoluene	0.50	Not Detected	2.4	Not Detected
Ethanol	2.0	Not Detected	3.8	Not Detected
Methyl tert-butyl ether	0.50	Not Detected	1.8	Not Detected
3-Chloropropene	2.0	Not Detected	6.3	Not Detected
2,2,4-Trimethylpentane	0.50	Not Detected	2.3	Not Detected
Naphthalene	2.0	Not Detected	10	Not Detected

Container Type: NA - Not Applicable

Surrogates	%Recovery	Method Limits
Toluene-d8	101	70-130
1,2-Dichloroethane-d4	100	70-130
4-Bromofluorobenzene	96	70-130



Report Date: 04-Aug-2008 12:55

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/04Aug2008.b/g080405.d  
 Lab Smp Id: Lab Blank Client Smp ID: Lab Blank  
 Inj Date : 04-AUG-2008 12:46  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 500mL #25246  
 Misc Info : humid  
 Comment :  
 Method : /chem/msdg.i/04Aug2008.b/t14q702a.m  
 Meth Date : 04-Aug-2008 11:28 lrandolp Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08Q.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE	( PPBV)	( PPBV)				
==	=====	=====	=====	=====	=====	=====		=====	
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002 (1.000)	130	299394	10.0000		80.00-	120.00	100.00	
9.002	9.002 (1.000)	128	229136			0.00-	30.00	76.53	
9.002	9.002 (1.000)	49	753586			0.00-	30.00	251.70	
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186 (1.000)	114	1147567	10.0000		80.00-	120.00	100.00	
10.186	10.186 (1.000)	88	187936			0.00-	47.07	16.38	
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319 (1.000)	117	1129158	10.0000		80.00-	120.00	100.00	
15.319	15.319 (1.000)	82	718188			0.00-	30.00	63.60	
-----									
§ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668 (1.074)	65	573940	9.98766	9.988	80.00-	120.00	100.00	
9.668	9.668 (1.074)	67	276215			0.00-	30.00	48.13	
-----									
§ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499 (1.227)	98	1197375	10.0932	10.093	80.00-	120.00	100.00	
12.499	12.499 (1.227)	70	144826			0.00-	42.14	12.10	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
== =====

\$ 59 Toluene-d8 (continued)

12.499 12.499 (1.227) 100 758988 33.87- 93.87 63.39

\$ 81 Bromofluorobenzene

CAS #: 460-00-4

17.226 17.226 (1.125) 174 633341 9.65554 9.656 80.00- 120.00 100.00

17.201 17.226 (1.123) 95 942281 118.60- 178.60 148.78

17.226 17.226 (1.125) 176 629001 67.33- 127.33 99.31

Report Date: 04-Aug-2008 12:55

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 04-AUG-2008

Lab File ID: g080405.d

Calibration Time: 09:59

Lab Smp Id: Lab Blank

Client Smp ID: Lab Blank

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/04Aug2008.b/t14q702a.m

Misc Info: humid

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	318312	190987	445637	299394	-5.94
51 1,4-Difluorobenze	1208514	725108	1691920	1147567	-5.04
72 Chlorobenzene-d5	1189759	713855	1665663	1129158	-5.09

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 04Aug2008  
Sample Matrix: GAS Fraction: VOA  
Lab Smp Id: Lab Blank Client Smp ID: Lab Blank  
Level: LOW Operator: lmr  
Data Type: MS DATA SampleType: SAMPLE  
SpikeList File: Spectra.spk Quant Type: ISTD  
Sublist File: AT08Q.sub  
Method File: /chem/msdg.i/04Aug2008.b/t14q702a.m  
Misc Info: humid

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 47 1,2-Dichloroethane	10.000	9.988	99.88	70-130
\$ 59 Toluene-d8	10.000	10.093	100.93	70-130
\$ 81 Bromofluorobenzene	10.000	9.656	96.56	70-130

Date : 04-AUG-2008 12:46

Client ID: Lab Blank


Instrument: msdg,i

Sample Info: 500mL #25246

Operator: lmr

Column phase: RTX-624

Column diameter: 0.32

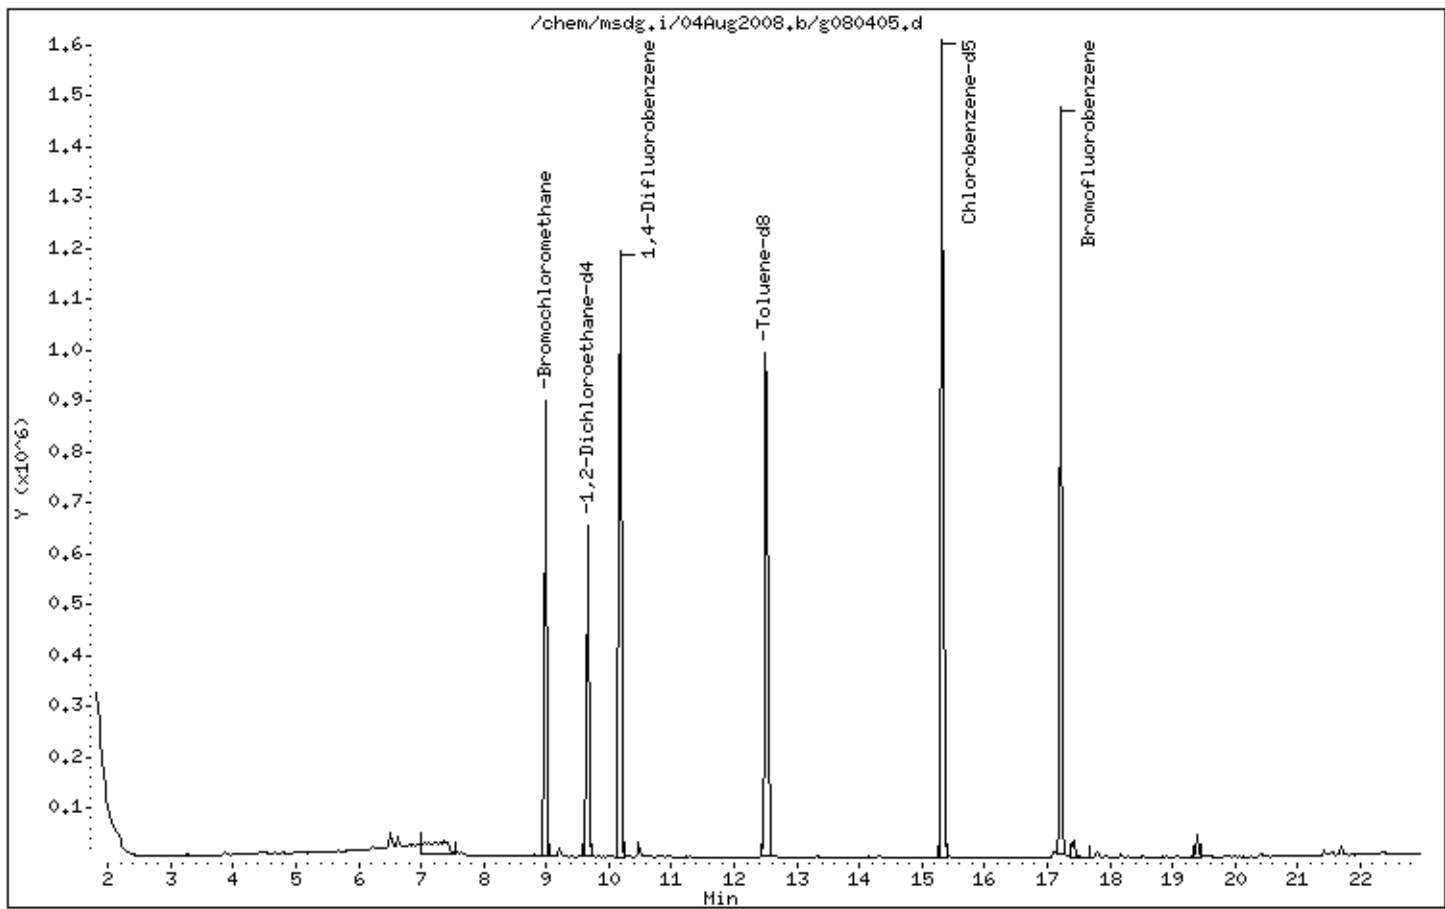

# LEVEL-IV VALIDATABLE

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

SURROGATE RECOVERY FORM

Lab Name: AIR TOXICS LIMITED.

SDG No.: 0807494

CLIENT SAMPLE NO.	SURROGATE % RECOVERY							
	1,2-Dichloroethane-d 4	#	Toluene-d8	#	4-Bromofluorobenze ne	#	#	TOTAL OUT
01	AMS 4 DW	102		100		99		0
02	AMS 3 DW	97		102		96		0
03	Lab Blank	100		101		96		0
04	CCV	104		106		104		0
05	LCS	102		103		100		0
06								0
07								0
08								0
09								0
10								0
11								0
12								0
13								0
14								0
15								0
16								0
17								0
18								0
19								0
20								0
21								0
22								0
23								0
24								0

Surrogate Recovery Limits

1,2-Dichloroethane-d4 70 - 130

Toluene-d8 70 - 130

4-Bromofluorobenzene 70 - 130

\* Designates values outside of QC limits

# LEVEL-IV VALIDATABLE

Modified EPA Method TO-15 GC/MS Full Scan

INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: AIR TOXICS, LTD  
 Lab File ID: q080402.d  
 Instrument ID: msdq.i

SDG No: 0807494  
 Date Analyzed: 08/04/2008  
 Time Analyzed: 09:59 AM

	Chlorobenzene-d5			1,4-Difluorobenzene			Bromochloromethane		
	Area	#	RT	Area	#	RT	Area	#	RT
24-HOUR STD	1189759		15.32	1208514		10.19	318312		9
UPPER LIMIT	1665663		15.65	1691920		10.52	445637		09.33
LOWER LIMIT	713855		14.99	725108		09.86	190987		08.67
CLIENT SAMPLE NO									
01 AMS 4 DW	1240009		15.32	1209647		10.19	301690		9
02 AMS 3 DW	1225378		15.32	1218887		10.19	321816		9
03 Lab Blank	1129158		15.32	1147567		10.19	299394		9
04 CCV	1189759		15.32	1208514		10.19	318312		9
05 LCS	1085504		15.32	1174713		10.19	310013		9
06									
07									
08									
09									
10									
11									
12									
13									
14									
15									
16									
17									
18									
19									
20									
21									
22									

'Area Upper Limit=+40% of internal standard area'  
 'Area Lower Limit=-40% of internal standard area'

RT Upper Limit=+0.33 minutes of internal standard RT  
 RT Lower Limit=-0.33 minutes of internal standard RT

\* Designates values outside of QC limits

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Calibration File Names:

- Level 1: /chem/msdg.i/02Jul2008.b/g070204.d
- Level 2: /chem/msdg.i/02Jul2008.b/g070205.d
- Level 3: /chem/msdg.i/02Jul2008.b/g070206.d
- Level 4: /chem/msdg.i/02Jul2008.b/g070202.d
- Level 5: /chem/msdg.i/02Jul2008.b/g070207.d
- Level 6: /chem/msdg.i/02Jul2008.b/g070208.d
- Level 7: /chem/msdg.i/02Jul2008.b/g070209.d

Compound	0.30000	0.50000	2.000	10.000	25.000	50.000	___	% RSD
	Level 1	Level 2	Level 3	Level 4	Level 5	Level 6	RRF	
	100.000							
	Level 7							
3 Freon 134a	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
4 Propylene	+++++	1.69705	1.28271	1.35271	1.30467	1.31950	1.38441	11.230
5 Freon 152A	+++++	+++++	+++++	+++++	+++++	+++++	+++++	+++++
6 Dichlorodifluoromethane/Fr12	+++++	3.73040	3.01076	3.22743	2.93436	2.92748	3.12081	10.318
7 Freon 114	+++++	1.76812	1.65259	1.75550	1.59555	1.31808	1.57325	12.491
8 Chloromethane	+++++	2.10315	2.20815	2.19223	1.99147	2.25611	2.12923	5.013
183 Butane	+++++	0.22914	0.25167	0.25634	0.25137	0.24377	0.24835	4.272



Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
9 Vinyl Chloride	100.000 1.13383	1.36424	1.08708	1.14157	1.09789	1.11391		1.15642	8.983
10 1,3-Butadiene	1.32784 1.31861	1.29460	1.13344	1.19142	1.30418	1.21032		1.25434	6.015
11 Bromomethane	+++++ 0.65287	0.58250	0.51841	0.55884	0.56555	0.53364		0.56863	8.301
12 Freon 22	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
13 Chloroethane	+++++ 0.46150	0.38151	0.38348	0.46719	0.44805	0.44929		0.43183	9.009
14 Isopentane	+++++ 1.26610	1.17586	1.27112	1.28829	1.25724	1.26742		1.25434	3.171
15 Vinyl Bromide	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
16 Trichlorofluoromethane/Fr11	+++++ 3.46935	3.62928	3.98984	4.15787	3.84121	3.48925		3.76280	7.446
23 Pentane	+++++ +++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
17 Ethanol	+++++ 0.69642	0.69862	0.78421	0.66565	0.65546	0.69520		0.69926	6.487

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
22 Acrolein	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
18 1,1-Dichloroethene	+++++	0.68997	0.60915	0.68889	0.55609	0.53318		0.60047	12.466
19 Freon 113	+++++	1.93016	1.33606	1.70294	1.26063	1.12384		1.40429	24.254
20 Carbon Disulfide	+++++	3.87801	2.98541	3.68970	2.88164	2.73750		3.15345	15.866
21 Acetone	+++++	3.67885	4.45936	3.50480	3.81915	3.46138		3.73936	10.093
24 2-Propanol	+++++	3.04487	4.27610	3.61695	4.14951	3.53278		3.74741	12.002
25 3-Chloroprene	+++++	0.44076	0.43049	0.52425	0.44137	0.54149		0.46456	11.724
26 2-Methylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
176 Methyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
27 Acetonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
28 Methylene Chloride	100.000 0.63330	1.07632	0.78663	1.03282	0.71275	0.91261		0.85907	20.685
29 MTBE	3.11124	3.00204	4.00148	3.10993	4.11183	2.75287		3.34823	16.880
30 trans-1,2-Dichloroethene	0.52127	0.91071	0.89462	0.87494	0.88029	0.76188		0.80728	18.548
179 tert-Butyl Alcohol	3.57093	2.62521	3.23409	2.88892	3.45824	2.77301		3.09173	12.482
31 Acrylonitrile	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
32 Hexane	2.79339	2.61839	2.73707	3.02970	3.06152	2.93872		2.86313	6.119
33 1,1-Dichloroethane	2.74303	3.19066	2.98796	3.01807	2.92569	2.75789		2.93722	5.765
182 Isopropyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
34 Chlorprene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
35 Vinyl Acetate	5.50143	6.04160	5.26536	6.48473	6.53517	6.51628		6.05743	9.216

## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
174 2,4-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
180 Ethyl tert-Butyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
184 2,2-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
36 cis-1,2-Dichloroethene	+++++ 0.78583	0.84821	0.84215	0.94079	0.88952	0.81981		0.85438	6.364
37 2-Butanone	+++++ 0.67457	0.65460	0.71384	0.78438	0.78191	0.70159		0.71848	7.542
169 Ethyl Acetate	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
38 Tetrahydrofuran	+++++ 3.29551	2.82866	3.20102	2.89749	3.25010	2.87602		3.05813	6.940
40 Chloroform	3.42006 2.72873	3.13680	3.09237	3.06071	3.06307	2.75411		3.03655	7.794
41 Cyclohexane	+++++ 1.91122	1.96974	2.08341	2.23917	2.17983	1.96985		2.05887	6.348
42 1,1,1-Trichloroethane	+++++ 2.93745	3.28393	3.06651	3.27894	3.19136	2.94794		3.11769	5.030

## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
43 2,3-Dimethylpentane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
44 Carbon Tetrachloride	+++++	3.10000	3.04511	2.60060	2.55497	2.91377		2.84631	7.918
46 Benzene	1.17872	1.19578	1.21156	1.26242	1.23701	1.03384		1.15301	9.994
45 2,2,4-Trimethylpentane	+++++	3.24134	3.04769	3.34390	3.26647	3.19760		3.21714	3.055
48 1,2-Dichloroethane	+++++	0.69251	0.72073	0.73628	0.75456	0.65933		0.70601	5.286
181 tert-Amyl Methyl Ether	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
49 Heptane	+++++	1.00577	1.12136	1.33490	1.42170	1.27954		1.23504	12.141
50 Thiophene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
52 Trichloroethene	+++++	0.52125	0.48002	0.51097	0.50382	0.42687		0.47256	10.949
2 Methylcyclohexane	+++++	2.79122	2.80110	3.09914	3.01289	2.76069		2.85676	5.700

## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
53 1,2-Dichloropropane	100.000 0.48529	0.50890	0.51110	0.52675	0.55118	0.48618		0.51157	4.900
54 1,4-Dioxane	0.26285	0.23379	0.24521	0.27513	0.29372	0.25681		0.26125	8.175
66 Dibromomethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
55 Bromodichloromethane	0.79501	0.78473	0.80580	0.87484	0.91606	0.79922		0.82928	6.431
56 cis-1,3-Dichloropropene	0.62162	0.51111	0.54276	0.65325	0.71019	0.62781		0.61112	11.948
58 4-Methyl-2-pentanone	1.75877	1.22552	1.45324	1.66082	1.88225	1.67153		1.60869	14.579
60 Toluene	1.24810	1.28955	1.34422	1.45931	1.50287	1.28246		1.35442	7.661
57 Octane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
61 trans-1,3-Dichloropropene	0.74606	0.59649	0.63532	0.76333	0.82183	0.76299		0.72100	11.962
63 1,1,2-Trichloroethane	0.46743	0.52157	0.54162	0.56247	0.56535	0.50573		0.52736	7.081

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
64 Tetrachloroethene	100.000	0.69199	0.69792	0.74733	0.73467	0.63693		0.67972	9.770
62 1,3-Dichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
67 2-Hexanone	0.77617	0.51921	0.61044	0.74152	0.81981	0.74071		0.70131	16.162
68 Dibromochloromethane	0.79154	0.78184	0.79625	0.91860	0.93583	0.84666		0.84512	8.007
69 1,2-Dibromoethane	0.15649	0.26657	0.27727	0.23885	0.26088	0.23815	0.21836	0.23665	17.165
71 Hexachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
73 Chlorobenzene	1.14570	1.39948	1.37319	1.41986	1.42213	1.24519		1.33426	8.500
74 Ethyl Benzene	0.62089	0.64659	0.68095	0.75952	0.76646	0.67737		0.69196	8.564
168 1,1,1,2-Tetrachloroethane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
173 Nonane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++

## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
75 m,p-Xylene	100.000	0.71433	0.84308	0.94656	0.96843	0.84846		0.84950	11.444
76 1,3,5-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
77 o-Xylene	0.74085	0.65968	0.76703	0.89619	0.92785	0.79571		0.79789	12.516
78 Styrene	1.20371	0.83922	1.04055	1.26953	1.47991	1.49212	1.31045	1.23364	18.964
79 Bromoform	0.73994	0.73592	0.76139	0.86929	0.90086	0.81073		0.80302	8.671
170 alpha-Pinene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
80 Cumene	2.12579	1.80217	1.91338	2.26614	2.66646	2.71236	2.35877	2.26358	15.381
82 1,1,2,2-Tetrachloroethane	1.21341	1.40240	1.41228	1.47969	1.49371	1.31318		1.38578	7.666
83 Propylbenzene	1.97430	2.81941	3.14403	3.50301	3.50843	3.02105		2.99504	18.989
65 1,2,3-Trichloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++



## Air Toxics Ltd.

## INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
172 2-Chlorotoluene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
84 4-Ethyltoluene	+++++	+++++	+++++	+++++	2.99311	2.57119		2.45625	24.534
175 Decane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
85 1,3,5-Trimethylbenzene	1.67800	1.90166	2.20002	2.38115	2.45273	2.10426		2.07118	14.312
86 tert-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
87 1,2,4-Trimethylbenzene	1.43836	1.63165	1.93092	2.29064	2.37462	2.08797		1.94441	17.407
88 sec-Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
89 1,3-Dichlorobenzene	+++++	1.27382	1.29445	1.48098	1.46236	1.27508		1.32478	9.295
70 p-Cymene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
90 1,4-Dichlorobenzene	+++++	1.34402	1.39562	1.52516	1.50514	1.31120		1.37250	9.981

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
171 1,2,3-Trimethylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
91 alpha-chlorotoluene	+++++	1.13013	1.39949	1.88998	2.10712	2.01552		1.72308	22.062
92 Indan	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
93 Butylbenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
94 1,2-Dichlorobenzene	+++++	1.26148	1.29339	1.41512	1.38217	1.21075		1.27376	9.546
95 Indene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
177 1,2-Dibromo-3-Chloropropane	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
96 1,2,4-Trichlorobenzene	+++++	1.02647	0.91850	1.13629	1.05392	1.03482		1.00766	9.422
97 Hexachlorobutadiene	+++++	0.91669	0.84566	1.00438	0.89558	0.83484		0.86530	11.936
98 Naphthalene	+++++	1.70392	1.75700	2.34233	2.24743	2.24453		2.03792	13.543

Air Toxics Ltd.

INITIAL CALIBRATION DATA

Start Cal Date : 02-JUL-2008 08:28  
 End Cal Date : 02-JUL-2008 13:24  
 Quant Method : ISTD  
 Origin : Disabled  
 Target Version : 3.50  
 Integrator : HP RTE  
 Method file : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Cal Date : 03-Jul-2008 13:25 cleonard  
 Curve Type : Average

Compound	0.30000 Level 1	0.50000 Level 2	2.000 Level 3	10.000 Level 4	25.000 Level 5	50.000 Level 6	Level 7	RRF	% RSD
178 1,2,3-Trichlorobenzene	+++++	+++++	+++++	+++++	+++++	+++++		+++++	+++++
\$ 47 1,2-Dichloroethane-d4	1.90933 2.09479	1.98207	1.80107	1.82545	1.87311	1.94981		1.91937	5.240
\$ 59 Toluene-d8	1.00416 1.05982	0.99583	1.04667	1.05361	1.05013	1.02619		1.03377	2.460
\$ 81 Bromofluorobenzene	0.56930 0.57033	0.57384	0.57197	0.58262	0.60193	0.59635		0.58091	2.288

Calibration History

Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
Start Cal Date: 02-JUL-2008 08:28  
End Cal Date : 02-JUL-2008 13:24

Initial Calibration

Injection Date	Sublist	Calibration File
Cal Level: 1 , Cal Amount: 0.30000		
02-JUL-2008 09:43	AFCEElow	/chem/msdg.i/02Jul2008.b/g070204.d
Cal Level: 2 , Cal Amount: 0.50000		
02-JUL-2008 10:12	Hilocurve+Ensr	/chem/msdg.i/02Jul2008.b/g070205.d
Cal Level: 3 , Cal Amount: 2.00000		
02-JUL-2008 11:01	AT08mdl	/chem/msdg.i/02Jul2008.b/g070206.d
Cal Level: 4 , Cal Amount: 10.00000		
02-JUL-2008 08:28	AT08mdl	/chem/msdg.i/02Jul2008.b/g070202.d
Cal Level: 5 , Cal Amount: 25.00000		
02-JUL-2008 11:32	AT08mdl	/chem/msdg.i/02Jul2008.b/g070207.d
Cal Level: 6 , Cal Amount: 50.00000		
02-JUL-2008 12:20	AT08mdl	/chem/msdg.i/02Jul2008.b/g070208.d
Cal Level: 7 , Cal Amount: 100.00000		
02-JUL-2008 13:24	AT08	/chem/msdg.i/02Jul2008.b/g070209.d

Continuing Calibration  
Ccal Level Mode: GLOBAL LEVEL 5

```
| Ccal Level: 5 , Ccal Amount: 25.000 |
+=====+
|02-JUL-2008 11:32 |AT08mdl          |/chem/msdg.i/02Jul2008.b/g070207a.d |
+-----+-----+-----+-----+
| Ccal Level: 5 , Ccal Amount: 25.000 |
+=====+
|02-JUL-2008 11:32 |AT08mdl          |/chem/msdg.i/02Jul2008.b/g070207.d |
+-----+-----+-----+-----+
```

**Initial Calibration Narrative**

A 7-point initial calibration curve with a linear range of 0.30ppbv to 100ppbv was analyzed on 7/02/08 on MSD-G.

@ Air Toxics Ltd.

MSD-G

BCM : 35 0533  
 1,4-DFB: 1324034  
 CB-d5: 1242028

ION ABUNDANCE CRITERIA % REL. ABUNDANCE

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	31.52
75	30.0 - 60.0% of mass 95	52.60
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	0.66
173	Less than 2.0% of mass 174	( 0.81 ) <sup>1</sup>
174	Greater than 50.0% of mass 95	69.40
175	5.0 - 9.0% of mass 174	( 7.06 ) <sup>1</sup>
176	Greater than 95.0% but less than 101.0% of mass 174	( 97.26 ) <sup>1</sup>
177	5.0 - 9.0% of mass 176	( 0.48 ) <sup>2</sup>

BFB Injection Date: 7/21/08 Logbook #: 1640

BFB Injection Time: 0802

BFB File ID: G670201

Tekmar Purge Flow: -A 7218

Vacuum: 6.10x10<sup>-6</sup>

IS/S Std.#:	1541-145	Exp. Date:	8/4/08
BCM	<del>50554</del>	IC	<del>20330</del> S14
14-DFB	1260887	IC	1272384
CB-d5	<del>11348</del>	IC	11767824 #1100

Verified CCV IS vs ICAL mid-point (-40% D) UC

NOAH Cart #: NA File #: NA

Verify 176/174 m/z Ratio:  $\frac{153824}{416024} \times 100 = 99.26$

Calculation Check:

ppbv of compound =  $\frac{\text{Area}_{\text{sample}}}{\text{Area}_{\text{std}}} \times \text{Conc.}_{\text{std}} \times \text{RRF}$

$= \frac{(1265268)}{(1200887)} \times (12.0) = 10.079$

Reported Result: 10.079

File ID:	G076202
Compound:	Taralig
Initials:	UC

Use	File #	Sample / Client Name	Can #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
✓	G070201	REF TUNE CHECK	1470-431	50mg	2ul	100	7/2/08	0602	UC	
✓	02	ICAL 10/15/07	1541	10ppb	200ul			0608	UC	
✓	03	SYSTEM BLANK	-	dm	500ul			0913	UC	
✓	04	ICAL Lvl 1	1012	0.3ppb	75ml			0943	UC	
✓	05			0.5ppb	125ml			1012	UC	
✓	06			2.0ppb	500ml			1101	UC	
✓	07			25ppb	500ml			1132	UC	CV
✓	08			50ppb	125ml			1220	UC	
✓	09			100ppb	250ml			1324	UC	F1467029

Signature 

Date 7/12/08

@ Air Toxics Ltd.

MSD-G

Logbook #: 1640

10	X	G070210	TUAL LV18	10/12/05	200ppbv	500ML	1.00	7/12/05	1357	U	
11	X	11	SYSTEM BLANK	—	DIY	500ML			1501	U	
12	V	12	LCS-1 (500ppbv)	10/11/05	250ppbv	250ML			1550	U	TUAL LCS
13		13	LCS0 (500ppbv)	10/11/05	1	1					
14											
15											
16											
17											
18											
19											
20											
21											
22											
23											
24											
25											
26											
27											
28											
29											
30											
31											
32											







Comments:

UQ 7/12/05



Sample: ICAL Type: CALIB\_7 Inj.Date: 02-JUL-2008 13:24

- \*\* 39 Bromochlorometl
- \*\* 51 1,4-Difluorobei
- \*\* 72 Chlorobenzene-
- \*\* 47 1,2-Dichloroetl
- \*\* 59 Toluene-d8
- \*\* 61 Bromofluoroben:
- + 4 Propylene
- + 6 Dichlorodifluo
- + 7 Freon 114
- + 8 Chloromethane
- + 9 Vinyl Chloride
- + 10 1,3-Butadiene
- + 11 Bromomethane
- + 13 Chloroethane
- + 16 Trichlorofluor
- + 17 Ethanol
- + 19 Freon 113
- + 18 1,1-Dichloroetl
- + 21 Acetone
- + 24 2-Propanol
- + 20 Carbon Disulfid
- + 28 Methylene Chlo
- + 29 MTBE
- + 30 trans-1,2-Dich
- + 32 Hexane

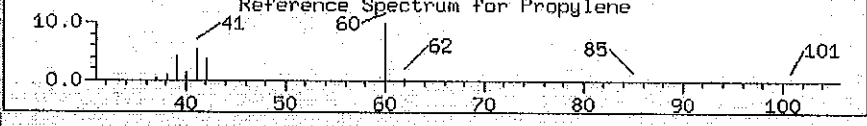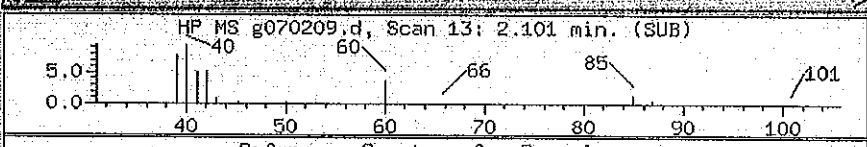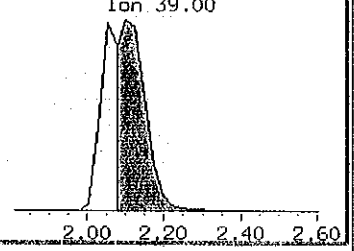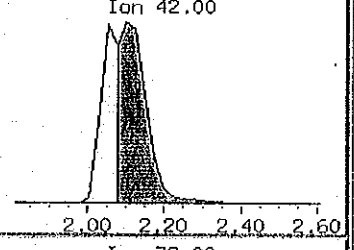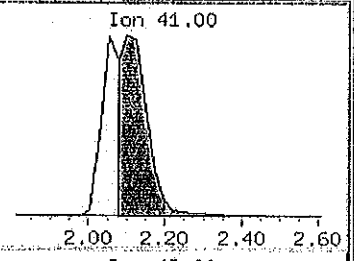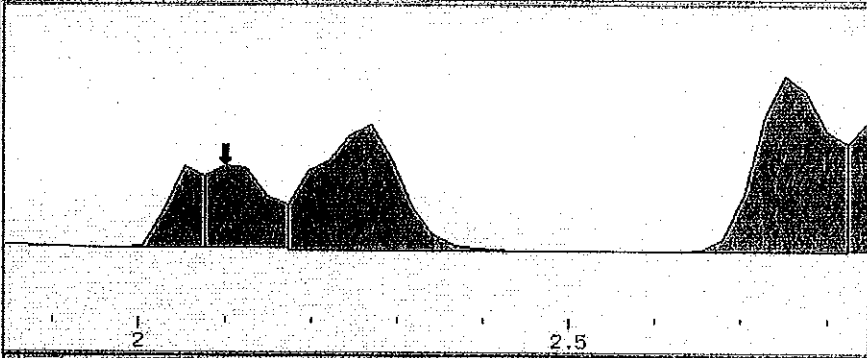

g070209.d

Hit#	RT(min)	Response	Amount	Conc	Ratio	Flags	Report:
1	2.053	2029129	44.520	44.520	100	A	
	2.053	1356851			67		
	2.053	1536485			76		
2	2.101	3381825	74.199	74.199	100	A	
	2.101	2260993			67		
	2.101	2519438			74		





Team VOC

Date / Initial	7/3/08 LP
Poor Integration	
Split Peak	✓
Peak Tailing	
Background Subtraction	
Zoom In	
Missed Peak	
Merged Peaks	

Manual Int


Process Spectra Help

Time: [ 2.101 ]  
 Area: [ 4649991 ]  
 Height: [ 606949 ]  
 Snap to Data  
 Snap to Int Marks  
 Overlap Peaks  
 Assign Baseline  
 Split Peak

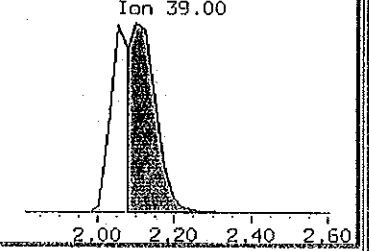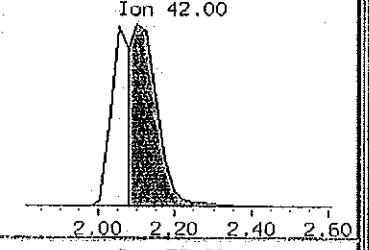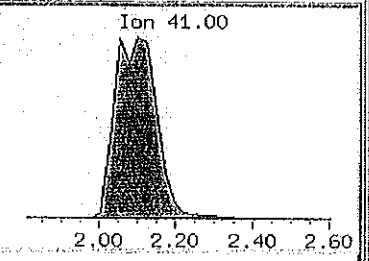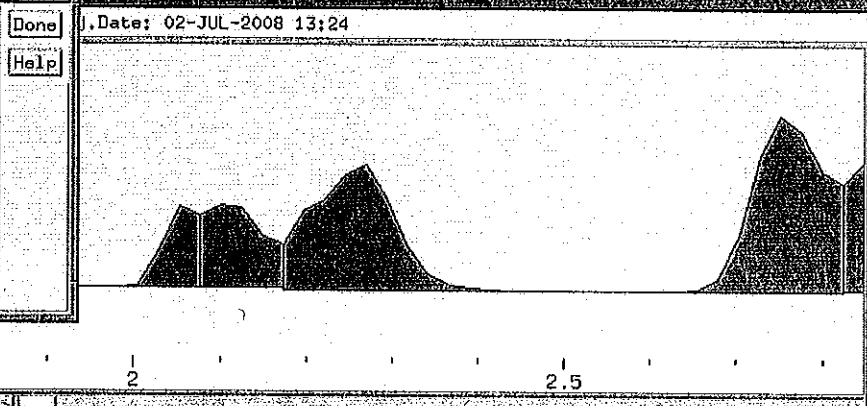

- + 13 Chloroethane
- + 16 Trichlorofluor
- + 17 Ethanol
- + 19 Freon 113
- + 18 1,1-Dichloroetl
- + 21 Acetone
- + 24 2-Propanol
- + 20 Carbon Disulf
- + 28 Methylene Chlo
- + 29 MTBE
- + 30 trans-1,2-Dich
- + 32 Hexane

g070209.d

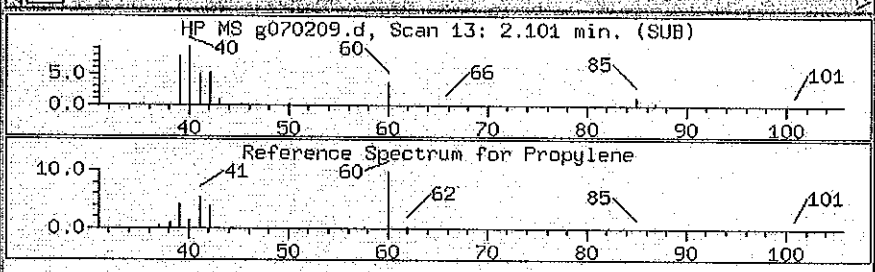

Hit#	RT(min)	Response	Amount	Conc	Ratio	Flags	Report:
1	2.101	4649991	97.501	97.501	100	AM	
	2.101	2260993			49		
	2.101	2515438			54		

- Mark Propylene Undetected.

Team VOC

Date / Initial	7/13/08 @ JWC
Poor Integration	
Split Peak	✓
Peak Tailing	
Background Subtraction	
Zoom In	
Missed Peak	
Merged Peaks	

Air Toxics Ltd.  
 Modified EPA Methods TO-14A/TO-15 Low Level  
 Internal Standard and Associated Target Compounds and Surrogates

<b>Bromochloromethane</b>
<b>Target Compounds:</b>
Freon 12
Freon 114
Chloromethane
Vinyl Chloride
1,3-Butadiene
Bromomethane
Chloroethane
Freon 11
Ethanol
Freon 113
1,1-Dichloroethene
Acetone
2-Propanol
Carbon Disulfide
Methylene Chloride
Methyl tert-butyl ether
trans-1,2-Dichloroethene
Hexane
1,1-Dichloroethane
2-Butanone (Methyl Ethyl Ketone)
cis-1,2-Dichloroethene
Tetrahydrofuran
Chloroform
1,1,1-Trichloroethane
Cyclohexane
Carbon Tetrachloride
<b>Surrogates:</b>
1,2-Dichloroethane-d4

<b>1,4-Difluorobenzene</b>
<b>Target Compounds:</b>
Benzene
1,2-Dichloroethane
Heptane
Trichloroethene
1,2-Dichloropropane
1,4-Dioxane
Bromodichloromethane
cis-1,3-Dichloropropene
4-Methyl-2-pentanone
Toluene
<b>Surrogates:</b>
Toluene-d8

<b>Chlorobenzene-d5</b>
<b>Target Compounds:</b>
trans-1,3-Dichloropropene
1,1,2-Trichloroethane
Tetrachloroethene
2-Hexanone
Dibromochloromethane
1,2-Dibromoethane (EDB)
Chlorobenzene
Ethyl Benzene
m,p-Xylene
o-Xylene
Styrene
Bromoform
Cumene
1,1,2,2-Tetrachloroethane
Propylbenzene
4-Ethyltoluene
1,3,5-Trimethylbenzene
1,2,4-Trimethylbenzene
1,3-Dichlorobenzene
1,4-Dichlorobenzene
alpha-Chlorotoluene
1,2-Dichlorobenzene
1,2,4-Trichlorobenzene
Hexachlorobutadiene
<b>Surrogates:</b>
Bromofluorobenzene

Report Date: 03-Jul-2008 14:14

Air Toxics Ltd.

AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070212.d  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Inj Date : 02-JUL-2008 15:50  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 250ml #1541-153;LCS-1;LCS-1  
 Misc Info : 50ppbv -> 25ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 14:14 lrandolp Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1 QC Sample: LCS  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
		ON-COL		FINAL		TARGET RANGE		RATIO	
RT	EXP RT (REL RT)	MASS	RESPONSE	( PPBV)	( PPBV)				
==	=====	=====	=====	=====	=====	=====		=====	
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002 (1.000)	130	331456	10.0000		80.00-	120.00	100.00	
9.002	9.002 (1.000)	128	258406			0.00-	30.00	77.96	
9.002	9.002 (1.000)	49	891173			0.00-	30.00	268.87	
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186 (1.000)	114	1362037	10.0000		80.00-	120.00	100.00	
10.186	10.186 (1.000)	88	229117			0.00-	46.78	16.82	
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319 (1.000)	117	1287365	10.0000		80.00-	120.00	100.00	
15.319	15.319 (1.000)	82	822577			0.00-	30.00	63.90	
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668 (1.074)	65	652194	10.2516	10.252	80.00-	120.00	100.00	
9.668	9.668 (1.074)	67	363202			0.00-	30.00	55.69	
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499 (1.227)	98	1470013	10.4402	10.440	80.00-	120.00	100.00	
12.499	12.499 (1.227)	70	177484			0.00-	42.14	12.07	

Report Date: 03-Jul-2008 14:14

## CONCENTRATIONS

ON-COL FINAL

RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====

\$ 59 Toluene-d8 (continued)

12.499	12.499	(1.227)	100	927337			34.50- 94.50	63.08
--------	--------	---------	-----	--------	--	--	--------------	-------

\$ 81 Bromofluorobenzene

CAS #: 460-00-4

17.226	17.226	(1.125)	174	737476	9.86143	9.861	80.00- 120.00	100.00
--------	--------	---------	-----	--------	---------	-------	---------------	--------

17.201	17.201	(1.123)	95	1118145			113.13- 173.13	151.62
--------	--------	---------	----	---------	--	--	----------------	--------

17.226	17.226	(1.125)	176	713940			66.52- 126.52	96.81
--------	--------	---------	-----	--------	--	--	---------------	-------

4 Propylene

CAS #: 115-07-1

2.149	2.101	(0.239)	41	1091086	23.7776	23.778	80.00- 120.00	100.00
-------	-------	---------	----	---------	---------	--------	---------------	--------

2.149	2.125	(0.239)	42	717137			0.00- 30.00	65.73
-------	-------	---------	----	--------	--	--	-------------	-------

2.149	2.125	(0.239)	39	791447			0.00- 30.00	72.54
-------	-------	---------	----	--------	--	--	-------------	-------

6 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.294	2.270	(0.255)	85	2140682	20.6947	20.695	80.00- 120.00	100.00
-------	-------	---------	----	---------	---------	--------	---------------	--------

2.294	2.270	(0.255)	87	690149			1.53- 61.53	32.24
-------	-------	---------	----	--------	--	--	-------------	-------

7 Freon 114

CAS #: 76-14-2

2.752	2.752	(0.306)	135	1077377	20.6607	20.661	80.00- 120.00	100.00
-------	-------	---------	-----	---------	---------	--------	---------------	--------

2.752	2.752	(0.306)	137	359684			0.00- 30.00	33.39
-------	-------	---------	-----	--------	--	--	-------------	-------

2.752	2.752	(0.306)	85	1788275			0.00- 30.00	165.98
-------	-------	---------	----	---------	--	--	-------------	--------

8 Chloromethane

CAS #: 74-87-3

2.872	2.872	(0.319)	50	1675984	23.7477	23.748	80.00- 120.00	100.00
-------	-------	---------	----	---------	---------	--------	---------------	--------

2.872	2.872	(0.319)	52	483332			0.00- 30.00	28.84
-------	-------	---------	----	--------	--	--	-------------	-------

9 Vinyl Chloride

CAS #: 75-01-4

3.308	3.291	(0.367)	62	871696	22.7417	22.742	80.00- 120.00	100.00
-------	-------	---------	----	--------	---------	--------	---------------	--------

3.325	3.308	(0.369)	64	273889			0.00- 59.65	31.42
-------	-------	---------	----	--------	--	--	-------------	-------

10 1,3-Butadiene

CAS #: 106-99-0

3.412	3.430	(0.379)	54	996899	23.9778	23.978	80.00- 120.00	100.00
-------	-------	---------	----	--------	---------	--------	---------------	--------

3.412	3.430	(0.379)	39	1242541			0.00- 30.00	124.64
-------	-------	---------	----	---------	--	--	-------------	--------

11 Bromomethane

CAS #: 74-83-9

4.350	4.351	(0.483)	94	345044	18.3069	18.307	80.00- 120.00	100.00
-------	-------	---------	----	--------	---------	--------	---------------	--------

4.350	4.351	(0.483)	96	325718			64.87- 124.87	94.40
-------	-------	---------	----	--------	--	--	---------------	-------

13 Chloroethane

CAS #: 75-00-3

4.724	4.724	(0.525)	64	338867	23.6748	23.675	80.00- 120.00	100.00
-------	-------	---------	----	--------	---------	--------	---------------	--------

4.724	4.724	(0.525)	49	144132			0.00- 30.00	42.53
-------	-------	---------	----	--------	--	--	-------------	-------

4.724	4.724	(0.525)	66	100571			0.00- 30.00	29.68
-------	-------	---------	----	--------	--	--	-------------	-------

16 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

5.304	5.304	(0.589)	101	2555514	20.4900	20.490	80.00- 120.00	100.00
-------	-------	---------	-----	---------	---------	--------	---------------	--------

5.304	5.304	(0.589)	103	1652816			33.99- 93.99	64.68
-------	-------	---------	-----	---------	--	--	--------------	-------

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT (REL RT)	MASS	RESPONSE	( PPEV)	( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

17 Ethanol						CAS #: 64-17-5		
6.225	6.225 (0.692)	45	538303	23.2253	23.225	80.00- 120.00	100.00	
6.225	6.225 (0.692)	43	109035			0.00- 30.00	20.26	
6.225	6.225 (0.692)	46	202573			0.00- 30.00	37.63	

19 Freon 113						CAS #: 76-13-1		
6.390	6.390 (0.710)	151	988653	21.2404	21.240	80.00- 120.00	100.00	
6.390	6.390 (0.710)	153	631479			31.73- 91.73	63.87	
6.390	6.390 (0.710)	101	1377377			0.00- 30.00	139.32	

18 1,1-Dichloroethene						CAS #: 75-35-4		
6.335	6.335 (0.704)	98	486800	24.4586	24.459	80.00- 120.00	100.00	
6.335	6.335 (0.704)	61	2176639			0.00- 30.00	447.13	
6.335	6.335 (0.704)	96	775426			0.00- 30.00	159.29	

21 Acetone						CAS #: 67-64-1		
6.637	6.637 (0.737)	43	2905369	23.4411	23.441	80.00- 120.00	100.00	
6.637	6.637 (0.737)	58	636084			0.00- 30.00	21.89	

24 2-Propanol						CAS #: 67-63-0		
7.049	7.049 (0.783)	45	3250505	26.1694	26.169	80.00- 120.00	100.00	
7.049	7.049 (0.783)	43	660224			0.00- 30.00	20.31	
7.049	7.049 (0.783)	59	98458			0.00- 30.00	3.03	

20 Carbon Disulfide						CAS #: 75-15-0		
6.500	6.500 (0.722)	76	2345966	22.4445	22.444	80.00- 120.00	100.00	

28 Methylene Chloride						CAS #: 75-09-2		
7.213	7.213 (0.801)	84	605929	21.2797	21.280	80.00- 120.00	100.00	
7.213	7.213 (0.801)	49	1915606			297.52- 357.52	316.14	
7.213	7.213 (0.801)	51	547394			0.00- 30.00	90.34	

29 MTBE						CAS #: 1634-04-4		
7.515	7.515 (0.835)	73	2566151	23.1228	23.123	80.00- 120.00	100.00	
7.515	7.515 (0.835)	57	1282061			0.00- 30.00	49.96	
7.543	7.543 (0.838)	41	2047510			0.00- 30.00	79.79	

30 trans-1,2-Dichloroethene						CAS #: 156-60-5		
7.515	7.515 (0.835)	98	447386	16.7198	16.720	80.00- 120.00	100.00	
7.515	7.515 (0.835)	61	1899426			0.00- 30.00	424.56	
7.515	7.515 (0.835)	96	717047			0.00- 30.00	160.27	

32 Hexane						CAS #: 110-54-3		
7.790	7.790 (0.865)	57	2570795	27.0895	27.089	80.00- 120.00	100.00	
7.790	7.790 (0.865)	43	2208838			0.00- 30.00	85.92	
7.790	7.790 (0.865)	86	259527			0.00- 30.00	10.10	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL ( PPEV)	FINAL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
33	1,1-Dichloroethane					CAS #: 75-34-3				
8.092	8.092	(0.899)	63	2469218	25.3628	25.363	80.00- 120.00	100.00		
8.092	8.092	(0.899)	65	731350			0.00- 59.84	29.62		
-----										
37	2-Butanone					CAS #: 78-93-3				
8.792	8.792	(0.977)	72	586006	24.6071	24.607	80.00- 120.00	100.00		
8.792	8.792	(0.977)	43	4557673			672.66- 732.66	777.75		
8.792	8.792	(0.977)	57	275071			0.00- 30.00	46.94		
-----										
36	cis-1,2-Dichloroethene					CAS #: 156-59-2				
8.747	8.748	(0.972)	98	709295	25.0465	25.046	80.00- 120.00	100.00		
8.747	8.748	(0.972)	61	2035759			241.26- 301.26	287.01		
8.747	8.748	(0.972)	96	1084945			128.30- 188.30	152.96		
-----										
38	Tetrahydrofuran					CAS #: 109-99-9				
9.002	9.002	(1.000)	42	2712310	26.7582	26.758	80.00- 120.00	100.00		
9.002	9.002	(1.000)	71	536989			0.00- 30.00	19.80		
9.002	9.002	(1.000)	72	584774			0.00- 30.00	21.56		
-----										
40	Chloroform					CAS #: 67-66-3				
9.099	9.099	(1.011)	83	2357343	23.4216	23.422	80.00- 120.00	100.00		
9.099	9.099	(1.011)	85	1460768			33.23- 93.23	61.97		
-----										
42	1,1,1-Trichloroethane					CAS #: 71-55-6				
9.229	9.229	(1.025)	97	2462550	23.8301	23.830	80.00- 120.00	100.00		
9.229	9.229	(1.025)	99	1589541			33.51- 93.51	64.55		
-----										
41	Cyclohexane					CAS #: 110-82-7				
9.197	9.197	(1.022)	84	1700001	24.9112	24.911	80.00- 120.00	100.00		
9.197	9.197	(1.022)	56	3180536			0.00- 30.00	187.09		
9.197	9.197	(1.022)	41	2179796			0.00- 30.00	128.22		
-----										
44	Carbon Tetrachloride					CAS #: 56-23-5				
9.359	9.359	(1.040)	119	2334035	24.7400	24.740	80.00- 120.00	100.00		
9.359	9.359	(1.040)	117	2440589			73.88- 133.88	104.57		
-----										
46	Benzene					CAS #: 71-43-2				
9.638	9.639	(0.946)	78	3492009	22.2359	22.236	80.00- 120.00	100.00		
9.638	9.639	(0.946)	77	816789			0.00- 30.00	23.39		
-----										
48	1,2-Dichloroethane					CAS #: 107-06-2				
9.755	9.755	(0.958)	62	2209922	22.9813	22.981	80.00- 120.00	100.00		
9.755	9.755	(0.958)	64	671165			0.00- 30.00	30.37		
-----										
49	Heptane					CAS #: 142-82-5				
9.871	9.872	(0.969)	43	4247341	25.2492	25.249	80.00- 120.00	100.00		

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				( PPEV)	( PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
49 Heptane (continued)									
9.871	9.872	(0.969)	57	1704202				0.00- 30.00	40.12
9.871	9.872	(0.969)	100	345780				0.00- 30.00	8.14
-----									
52 Trichloroethene					CAS #: 79-01-6				
10.475	10.475	(1.028)	130	1356745	21.0791	21.079		80.00- 120.00	100.00
10.475	10.475	(1.028)	95	1493649				0.00- 30.00	110.09
10.475	10.475	(1.028)	97	952798				0.00- 30.00	70.23
-----									
53 1,2-Dichloropropane					CAS #: 78-87-5				
10.861	10.861	(1.066)	63	1643093	23.5815	23.581		80.00- 120.00	100.00
10.861	10.861	(1.066)	62	1169608				40.07- 100.07	71.18
10.861	10.861	(1.066)	41	1408905				61.40- 121.40	85.75
-----									
54 1,4-Dioxane					CAS #: 123-91-1				
11.029	11.029	(1.083)	88	832776	23.4036	23.404		80.00- 120.00	100.00
11.029	11.029	(1.083)	58	861582				64.32- 124.32	103.46
11.029	11.029	(1.083)	57	282393				0.00- 30.00	33.91
-----									
55 Bromodichloromethane					CAS #: 75-27-4				
11.270	11.270	(1.106)	83	2573896	22.7878	22.788		80.00- 120.00	100.00
11.270	11.270	(1.106)	85	1602833				31.92- 91.92	62.27
-----									
56 cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.089	12.090	(1.187)	75	1987033	23.8719	23.872		80.00- 120.00	100.00
12.089	12.090	(1.187)	77	622874				1.56- 61.56	31.35
12.089	12.090	(1.187)	39	1811811				60.10- 120.10	91.18
-----									
58 4-Methyl-2-pentanone					CAS #: 108-10-1				
12.379	12.379	(1.215)	43	5688249	25.9608	25.961		80.00- 120.00	100.00
12.379	12.379	(1.215)	58	1621163				0.00- 30.00	28.50
12.379	12.379	(1.215)	85	492167				0.00- 30.00	8.65
-----									
60 Toluene					CAS #: 108-88-3				
12.644	12.644	(1.241)	91	4361241	23.6411	23.641		80.00- 120.00	100.00
12.644	12.644	(1.241)	92	2551162				28.58- 88.58	58.50
-----									
61 trans-1,3-Dichloropropene					CAS #: 10061-02-6				
13.308	13.308	(0.869)	75	2181049	23.4978	23.498		80.00- 120.00	100.00
13.308	13.308	(0.869)	77	675355				1.05- 61.05	30.96
13.308	13.308	(0.869)	39	1822349				54.43- 114.43	83.55
-----									
63 1,1,2-Trichloroethane					CAS #: 79-00-5				
13.665	13.665	(0.892)	97	1446829	21.3111	21.311		80.00- 120.00	100.00
13.665	13.665	(0.892)	99	899546				32.27- 92.27	62.17
13.665	13.665	(0.892)	83	1314174				59.54- 119.54	90.83
-----									



Report Date: 03-Jul-2008 14:14

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	FINAL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
64 Tetrachloroethene						CAS #:	127-18-4		
13.747	13.747	(0.897)	166	1861137	21.2689	21.269	80.00-	120.00	100.00
13.747	13.747	(0.897)	129	1419389			46.83-	106.83	76.26
13.747	13.747	(0.897)	131	1378858			42.93-	102.93	74.09
-----									
67 2-Hexanone						CAS #:	591-78-6		
14.132	14.132	(0.922)	58	2330675	25.8148	25.815	80.00-	120.00	100.00
14.132	14.132	(0.922)	43	5830118			227.44-	287.44	250.15
14.132	14.132	(0.922)	100	306304			0.00-	30.00	13.14
-----									
68 Dibromochloromethane						CAS #:	124-48-1		
14.352	14.352	(0.937)	129	2388905	21.9573	21.957	80.00-	120.00	100.00
14.352	14.352	(0.937)	208	129405			0.00-	30.00	5.42
-----									
69 1,2-Dibromoethane						CAS #:	106-93-4		
14.516	14.517	(0.948)	107	629175	20.6518	20.652	80.00-	120.00	100.00
14.516	14.517	(0.948)	109	581956			64.21-	124.21	92.50
-----									
73 Chlorobenzene						CAS #:	108-90-7		
15.370	15.370	(1.003)	112	3608115	21.0058	21.006	80.00-	120.00	100.00
15.370	15.370	(1.003)	114	1151551			1.79-	61.79	31.92
15.370	15.370	(1.003)	77	2353756			33.30-	93.30	65.24
-----									
74 Ethyl Benzene						CAS #:	100-41-4		
15.525	15.525	(1.013)	106	1933522	21.7052	21.705	80.00-	120.00	100.00
15.525	15.525	(1.013)	91	6309378			0.00-	30.00	326.32
-----									
75 m,p-Xylene						CAS #:	108-38-3		
15.731	15.731	(1.027)	106	2411723	22.0527	22.053	80.00-	120.00	100.00
15.731	15.731	(1.027)	91	5025580			0.00-	30.00	208.38
-----									
77 o-Xylene						CAS #:	95-47-6		
16.376	16.376	(1.069)	106	2314871	22.5364	22.536	80.00-	120.00	100.00
16.376	16.376	(1.069)	91	5118699			186.60-	246.60	221.12
-----									
78 Styrene						CAS #:	100-42-5		
16.401	16.401	(1.071)	104	3819676	24.0511	24.051	80.00-	120.00	100.00
16.401	16.401	(1.071)	78	2143323			24.82-	84.82	56.11
-----									
79 Bromoform						CAS #:	75-25-2		
16.711	16.711	(1.091)	173	2316928	22.4121	22.412	80.00-	120.00	100.00
16.711	16.711	(1.091)	171	1183478			0.00-	30.00	51.08
-----									
80 Cumene						CAS #:	98-82-8		
16.917	16.917	(1.104)	105	6896905	23.6677	23.668	80.00-	120.00	100.00
16.917	16.917	(1.104)	120	1783960			0.00-	56.16	25.87
-----									

Report Date: 03-Jul-2008 14:14

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE		ON-COL	FINAL	TARGET RANGE	RATIO
				( PPEV)	( PPBV)				
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
82	1,1,2,2-Tetrachloroethane					CAS #: 79-34-5			
17.484	17.484	(1.141)	83	3784884	21.2157	21.216	80.00-	120.00	100.00
17.484	17.484	(1.141)	85	2362580			33.53-	93.53	62.42
-----									
83	Propylbenzene					CAS #: 103-65-1			
17.536	17.536	(1.145)	91	8944699	23.1986	23.199	80.00-	120.00	100.00
17.536	17.536	(1.145)	120	1924388			0.00-	30.00	21.51
-----									
84	4-Ethyltoluene					CAS #: 622-96-8			
17.716	17.716	(1.157)	105	7470156	23.6241	23.624	80.00-	120.00	100.00
17.716	17.716	(1.157)	120	2155379			0.00-	59.12	28.85
-----									
85	1,3,5-Trimethylbenzene					CAS #: 108-67-8			
17.820	17.820	(1.163)	105	5987011	22.4538	22.454	80.00-	120.00	100.00
17.820	17.820	(1.163)	120	2772993			16.79-	76.79	46.32
-----									
87	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
18.413	18.413	(1.202)	105	5898581	23.5645	23.564	80.00-	120.00	100.00
18.413	18.413	(1.202)	120	2568297			13.82-	73.82	43.54
-----									
89	1,3-Dichlorobenzene					CAS #: 541-73-1			
18.929	18.929	(1.236)	146	3670323	21.5208	21.521	80.00-	120.00	100.00
18.929	18.929	(1.236)	148	2326492			0.00-	30.00	63.39
18.929	18.929	(1.236)	111	1620101			0.00-	30.00	44.14
-----									
90	1,4-Dichlorobenzene					CAS #: 106-46-7			
19.083	19.083	(1.246)	146	3702907	20.9571	20.957	80.00-	120.00	100.00
19.083	19.083	(1.246)	148	2326050			0.00-	30.00	62.82
19.083	19.083	(1.246)	111	1564619			0.00-	30.00	42.25
-----									
91	alpha-chlorotoluene					CAS #: 100-44-7			
19.316	19.316	(1.261)	91	5495235	24.7731	24.773	80.00-	120.00	100.00
19.316	19.316	(1.261)	126	1030882			0.00-	30.00	18.76
-----									
94	1,2-Dichlorobenzene					CAS #: 95-50-1			
19.625	19.625	(1.281)	146	3415594	20.8294	20.829	80.00-	120.00	100.00
19.625	19.625	(1.281)	148	2131141			32.78-	92.78	62.39
19.625	19.625	(1.281)	111	1543895			14.53-	74.53	45.20
-----									
96	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
21.430	21.431	(1.399)	180	2947168	22.7189	22.719	80.00-	120.00	100.00
21.430	21.431	(1.399)	182	2819111			65.13-	125.13	95.65
-----									
97	Hexachlorobutadiene					CAS #: 87-68-3			
21.559	21.559	(1.407)	225	2416391	21.6920	21.692	80.00-	120.00	100.00
21.559	21.559	(1.407)	223	1530742			0.00-	30.00	63.35
-----									

Report Date: 03-Jul-2008 14:14

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPEV)	FINAL	( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
-----									
98 Naphthalene						CAS #: 91-20-3			
21.688	21.688	(1.416)	128	6630340	25.2724	25.272		80.00- 120.00	100.00
21.688	21.688	(1.416)	127	817559				0.00- 30.00	12.33
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	358156	23.2596	23.260		80.00- 120.00	100.00
6.994	6.994	(0.777)	41	2598470				0.00- 30.00	725.51
-----									
45 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.638	9.639	(1.071)	56	2627303	24.6385	24.638		80.00- 120.00	100.00
9.638	9.639	(1.071)	99	282282				0.00- 30.00	10.74
9.638	9.639	(1.071)	41	2666345				0.00- 30.00	101.49
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	5387536	26.8334	26.833		80.00- 120.00	100.00
8.174	8.174	(0.908)	42	433421				0.00- 30.00	8.04
8.174	8.174	(0.908)	86	244635				0.00- 30.00	4.54
-----									
183 Butane						CAS #: 106-97-8			
3.221	3.221	(0.358)	58	209234	25.4184	25.418		80.00- 120.00	100.00
3.221	3.221	(0.358)	43	2205138				0.00- 30.00	1053.91
-----									
14 Isopentane						CAS #: 78-78-4			
4.827	4.848	(0.536)	57	961247	23.1204	23.120		80.00- 120.00	100.00
4.827	4.848	(0.536)	43	1803659				0.00- 30.00	187.64
4.827	4.848	(0.536)	42	1546236				0.00- 30.00	160.86
-----									
2 Methylcyclohexane						CAS #: 108-87-2			
10.644	10.644	(1.182)	83	2316601	24.4654	24.465		80.00- 120.00	100.00
10.644	10.644	(1.182)	98	1015473				0.00- 30.00	43.83
10.644	10.644	(1.182)	55	2904806				0.00- 30.00	125.39
-----									
179 tert-Butyl Alcohol						CAS #: 75-65-0			
7.570	7.570	(0.841)	59	2816988	27.4889	27.489		80.00- 120.00	100.00
7.543	7.543	(0.838)	41	2047510				0.00- 30.00	72.68
7.515	7.515	(0.835)	57	1282061				0.00- 30.00	45.51
-----									

Report Date: 03-Jul-2008 14:14

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070212.d

Calibration Time: 11:32

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 50ppbv -&gt; 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	331456	-7.03
51 1,4-Difluorobenze	1324634	794780	1854488	1362037	2.82
72 Chlorobenzene-d5	1242028	745217	1738839	1287365	3.65

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 02Jul2008  
 Sample Matrix: GAS Fraction: VOA  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Level: LOW Operator: lmr  
 Data Type: MS DATA SampleType: LCS  
 SpikeList File: Spectra.spk Quant Type: ISTD  
 Sublist File: AT08.sub  
 Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Misc Info: 50ppbv -> 25ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
6 Dichlorodifluorome	25.000	20.695	82.78	70-130
7 Freon 114	25.000	20.661	82.64	70-130
8 Chloromethane	25.000	23.748	94.99	70-130
9 Vinyl Chloride	25.000	22.742	90.97	70-130
10 1,3-Butadiene	25.000	23.978	95.91	60-140
11 Bromomethane	25.000	18.307	73.23	70-130
13 Chloroethane	25.000	23.675	94.70	70-130
16 Trichlorofluoromet	25.000	20.490	81.96	70-130
17 Ethanol	25.000	23.225	92.90	60-140
19 Freon 113	25.000	21.240	84.96	70-130
18 1,1-Dichloroethene	25.000	24.459	97.83	70-130
21 Acetone	25.000	23.441	93.76	60-140
20 Carbon Disulfide	25.000	22.444	89.78	60-140
24 2-Propanol	25.000	26.169	104.68	60-140
28 Methylene Chloride	25.000	21.280	85.12	70-130
29 MTBE	25.000	23.123	92.49	60-140
30 trans-1,2-Dichloro	25.000	16.720	66.88	60-140
32 Hexane	25.000	27.089	108.36	60-140
33 1,1-Dichloroethane	25.000	25.363	101.45	70-130
36 cis-1,2-Dichloroet	25.000	25.046	100.19	70-130
37 2-Butanone	25.000	24.607	98.43	60-140
38 Tetrahydrofuran	25.000	26.758	107.03	60-140
40 Chloroform	25.000	23.422	93.69	70-130
41 Cyclohexane	25.000	24.911	99.64	60-140
42 1,1,1-Trichloroeth	25.000	23.830	95.32	70-130
44 Carbon Tetrachlori	25.000	24.740	98.96	70-130
46 Benzene	25.000	22.236	88.94	70-130
49 Heptane	25.000	25.249	101.00	60-140
48 1,2-Dichloroethane	25.000	22.981	91.93	70-130
52 Trichloroethene	25.000	21.079	84.32	70-130
53 1,2-Dichloropropan	25.000	23.581	94.33	70-130
54 1,4-Dioxane	25.000	23.404	93.61	60-140
55 Bromodichlorometha	25.000	22.788	91.15	60-140

Report Date: 03-Jul-2008 14:14

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
56 cis-1,3-Dichloropr	25.000	23.872	95.49	70-130
58 4-Methyl-2-pentano	25.000	25.961	103.84	60-140
60 Toluene	25.000	23.641	94.56	70-130
61 trans-1,3-Dichloro	25.000	23.498	93.99	70-130
63 1,1,2-Trichloroeth	25.000	21.311	85.24	70-130
67 2-Hexanone	25.000	25.815	103.26	60-140
64 Tetrachloroethene	25.000	21.269	85.08	70-130
68 Dibromochlorometha	25.000	21.957	87.83	60-140
69 1,2-Dibromoethane	25.000	20.652	82.61	70-130
73 Chlorobenzene	25.000	21.006	84.02	70-130
74 Ethyl Benzene	25.000	21.705	86.82	70-130
75 m,p-Xylene	25.000	22.053	88.21	70-130
77 o-Xylene	25.000	22.536	90.15	70-130
78 Styrene	25.000	24.051	96.20	70-130
79 Bromoform	25.000	22.412	89.65	60-140
80 Cumene	25.000	23.668	94.67	60-140
82 1,1,2,2-Tetrachlor	25.000	21.216	84.86	70-130
83 Propylbenzene	25.000	23.199	92.79	60-140
84 4-Ethyltoluene	25.000	23.624	94.50	60-140
85 1,3,5-Trimethylben	25.000	22.454	89.82	70-130
87 1,2,4-Trimethylben	25.000	23.564	94.26	70-130
89 1,3-Dichlorobenzen	25.000	21.521	86.08	70-130
90 1,4-Dichlorobenzen	25.000	20.957	83.83	70-130
91 alpha-chlorotoluen	25.000	24.773	99.09	70-130
94 1,2-Dichlorobenzen	25.000	20.829	83.32	70-130
96 1,2,4-Trichloroben	25.000	22.719	90.88	70-130
97 Hexachlorobutadien	25.000	21.692	86.77	60-130
98 Naphthalene	25.000	25.272	101.09	60-140
25 3-Chloroprene	25.000	23.260	93.04	60-140
45 2,2,4-Trimethylpen	25.000	24.638	98.55	60-140
179 tert-Butyl Alcohol	25.000	27.489	109.96	60-140
183 Butane	25.000	25.418	101.67	60-140
14 Isopentane	25.000	23.120	92.48	60-140
2 Methylcyclohexane	25.000	24.465	97.86	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 47 1,2-Dichloroethane	10.000	10.252	102.52	70-130
\$ 59 Toluene-d8	10.000	10.440	104.40	70-130
\$ 81 Bromofluorobenzene	10.000	9.861	98.61	70-130

Date : 02-JUL-2008 15:50

Client ID: LCS-1


Instrument: msdg.i

Sample Info: 250ml #1541-153;LCS-1;LCS-1

Operator: lmr

Column phase: RTX-624

Column diameter: 0.32

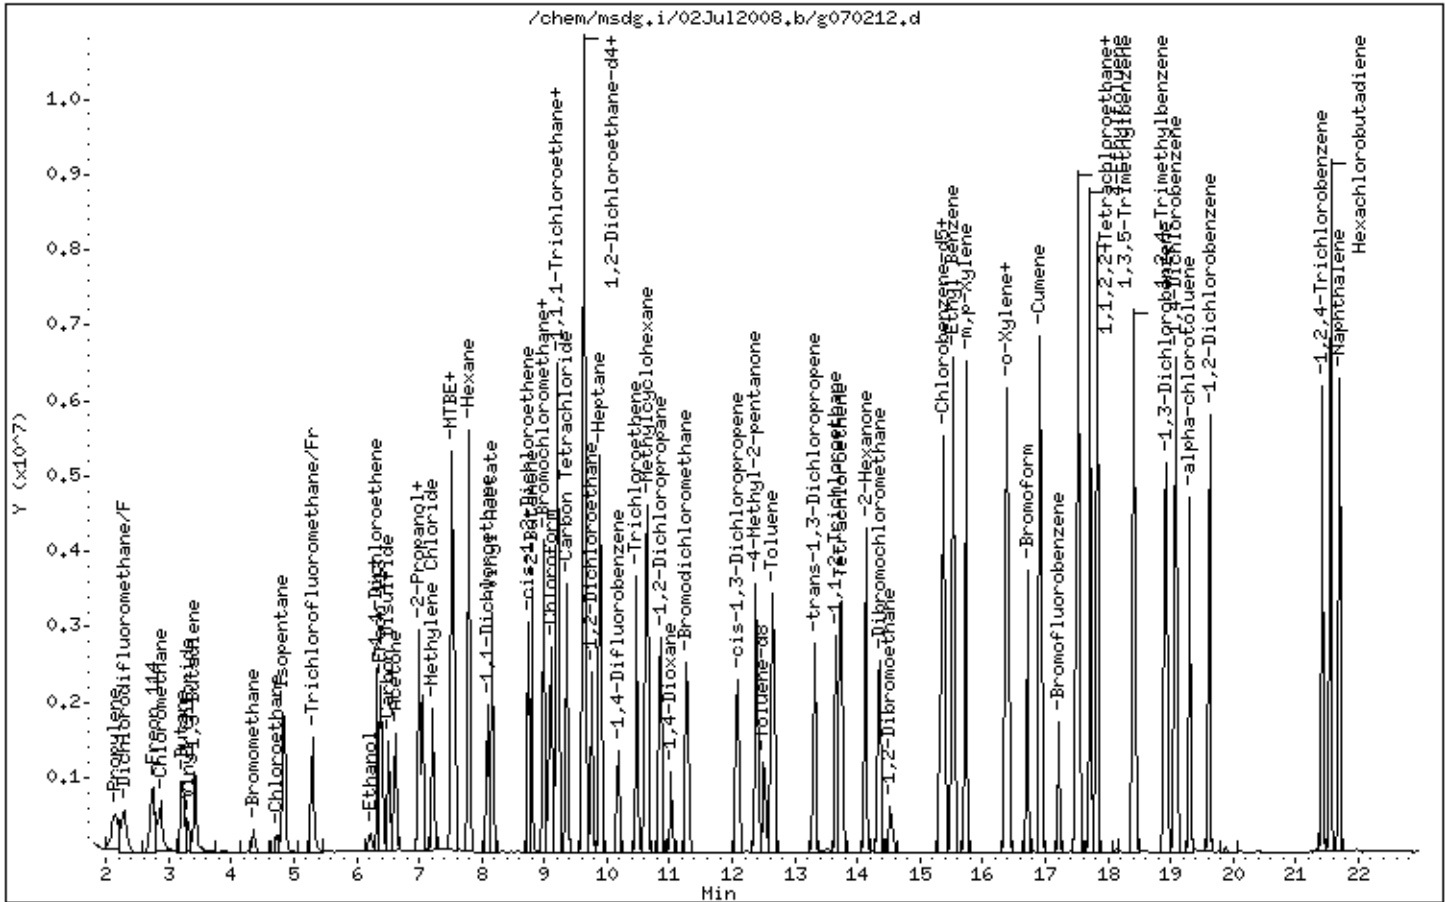

Report Date: 03-Jul-2008 13:48

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070204.d  
 Lab Smp Id: ICAL Client Smp ID: Level 1  
 Inj Date : 02-JUL-2008 09:43  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 75mL #1612-56  
 Misc Info : 2.0ppbv -> 0.3ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:47 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 09:43 Cal File: g070204.d  
 Als bottle: 1 Calibration Sample, Level: 1  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AFCEElow.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 39	Bromochloromethane					CAS #:	74-97-5	
9.002	9.002	(1.000)	130	268631	10.0000		70.00- 130.00	100.00
9.002	9.002	(1.000)	128	199822			0.00- 30.00	74.39
9.002	9.002	(1.000)	49	622008			0.00- 30.00	231.55
-----								
* 51	1,4-Difluorobenzene					CAS #:	540-36-3	
10.186	10.186	(1.000)	114	1147547	10.0000		70.00- 130.00	100.00
10.186	10.186	(1.000)	88	191199			0.00- 46.78	16.66
-----								
* 72	Chlorobenzene-d5					CAS #:	3114-55-4	
15.319	15.319	(1.000)	117	1042115	10.0000		70.00- 130.00	100.00
15.319	15.319	(1.000)	82	630399			0.00- 30.00	60.49
-----								
\$ 47	1,2-Dichloroethane-d4					CAS #:	17060-07-0	
9.668	9.668	(1.074)	65	512906	10.0000	9.948	70.00- 130.00	100.00
9.668	9.668	(1.074)	67	247256			0.00- 30.00	48.21
-----								
\$ 59	Toluene-d8					CAS #:	2037-26-5	
12.499	12.499	(1.227)	98	1152318	10.0000	9.714	70.00- 130.00	100.00
12.499	12.499	(1.227)	70	142314			0.00- 42.14	12.35



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	737490			34.50- 94.50	64.00	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	593275	10.0000	9.800	70.00- 130.00	100.00	
17.201	17.201	(1.123)	95	837644			113.13- 173.13	141.19	
17.226	17.226	(1.125)	176	571216			66.52- 126.52	96.28	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.412	3.412	(0.379)	54	10701	0.30000	0.3176	70.00- 130.00	100.00	
3.412	3.412	(0.379)	39	16557			0.00- 30.00	154.72	
-----									
40 Chloroform CAS #: 67-66-3									
9.099	9.099	(1.011)	83	27562	0.30000	0.3379	70.00- 130.00	100.00	
9.099	9.099	(1.011)	85	17153			33.23- 93.23	62.23	
-----									
46 Benzene CAS #: 71-43-2									
9.638	9.638	(0.946)	78	40579	0.30000	0.3067	70.00- 130.00	100.00	
9.638	9.638	(0.946)	77	9998			0.00- 30.00	24.64	
-----									
78 Styrene CAS #: 100-42-5									
16.427	16.427	(1.072)	104	26237	0.30000	0.2041	70.00- 130.00	100.00	
16.401	16.401	(1.071)	78	16079			24.82- 84.82	61.28	
-----									
80 Cumene CAS #: 98-82-8									
16.917	16.917	(1.104)	105	56342	0.30000	0.2388	70.00- 130.00	100.00	
16.917	16.917	(1.104)	120	15231			0.00- 56.16	27.03	
-----									
69 1,2-Dibromoethane CAS #: 106-93-4									
14.516	14.516	(0.948)	107	8334	0.30000	0.3379	70.00- 130.00	100.00	
14.516	14.516	(0.948)	109	6523			64.21- 124.21	78.27	
-----									
85 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.820	17.820	(1.163)	105	52460	0.30000	0.2430	70.00- 130.00	100.00	
17.820	17.820	(1.163)	120	25934			16.79- 76.79	49.44	
-----									
87 1,2,4-Trimethylbenzene CAS #: 95-63-6									
18.413	18.413	(1.202)	105	44968	0.30000	0.2219	70.00- 130.00	100.00	
18.413	18.413	(1.202)	120	20097			13.82- 73.82	44.69	
-----									

Report Date: 03-Jul-2008 13:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070204.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 2.0ppbv -&gt; 0.3ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	268631	-24.65
51 1,4-Difluorobenze	1324634	794780	1854488	1147547	-13.37
72 Chlorobenzene-d5	1242028	745217	1738839	1042115	-16.10

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 02-JUL-2008 09:43

Client ID: Level 1


Instrument: msdg,i

Sample Info: 75mL #1612-56

Operator: lmr

Column phase: RTX-624

Column diameter: 0.32

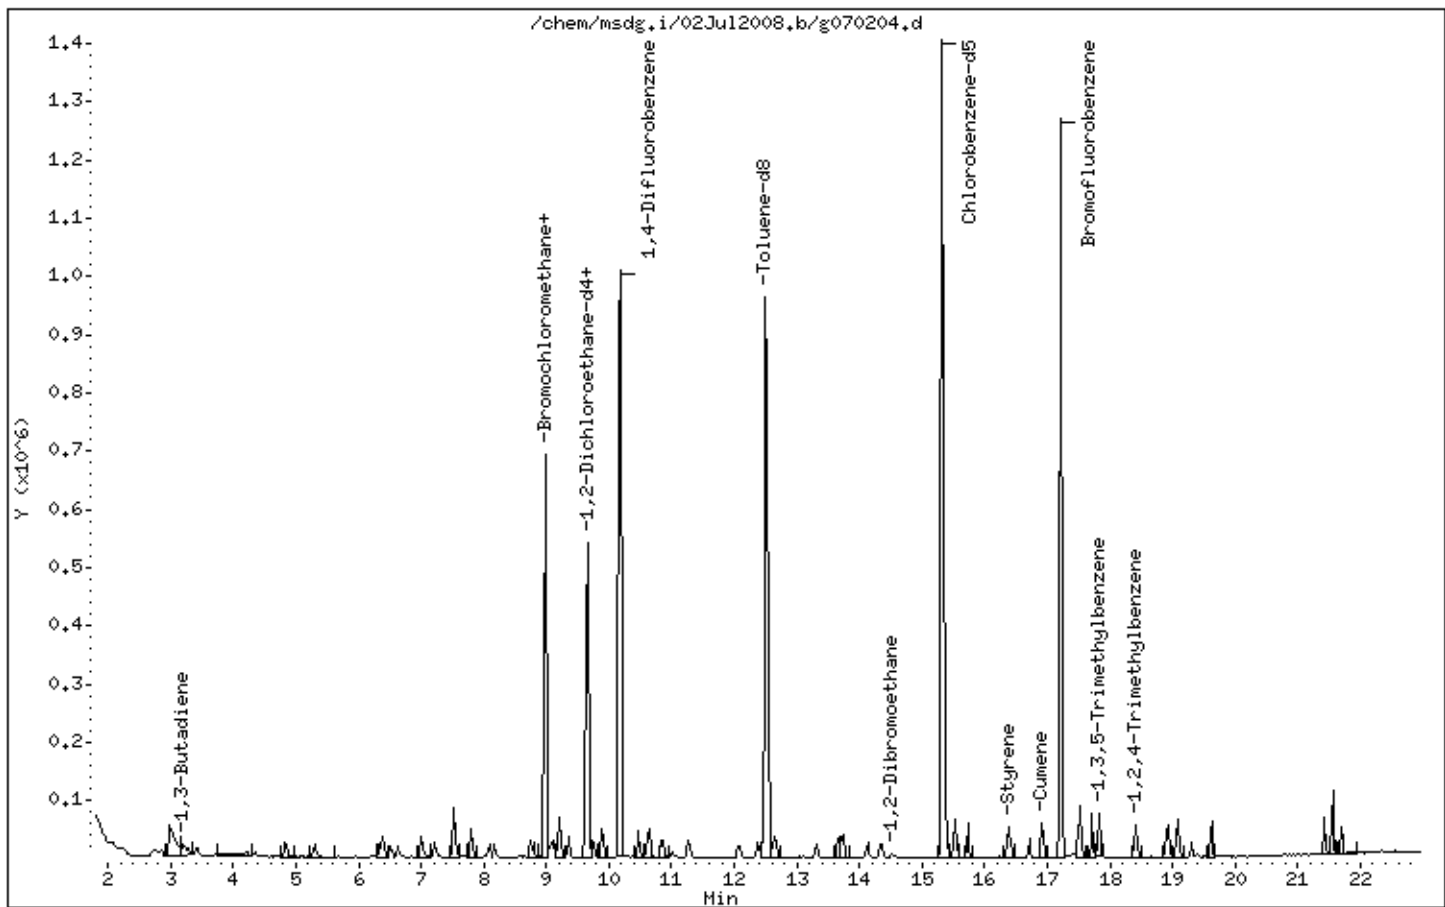

Report Date: 03-Jul-2008 13:48

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070205.d  
 Lab Smp Id: ICAL Client Smp ID: Level 2  
 Inj Date : 02-JUL-2008 10:12  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 125mL #1612-56  
 Misc Info : 2.0ppbv -> 0.5ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:48 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 10:12 Cal File: g070205.d  
 Als bottle: 1 Calibration Sample, Level: 2  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: Hilocurve+Ensr.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 39	Bromochloromethane					CAS #:	74-97-5	
9.002	9.002	(1.000)	130	252155	10.0000		70.00- 130.00	100.00
9.002	9.002	(1.000)	128	197769			0.00- 30.00	78.43
9.002	9.002	(1.000)	49	586693			0.00- 30.00	232.67
-----								
* 51	1,4-Difluorobenzene					CAS #:	540-36-3	
10.186	10.186	(1.000)	114	1088424	10.0000		70.00- 130.00	100.00
10.186	10.186	(1.000)	88	183217			0.00- 46.78	16.83
-----								
* 72	Chlorobenzene-d5					CAS #:	3114-55-4	
15.319	15.319	(1.000)	117	964315	10.0000		70.00- 130.00	100.00
15.319	15.319	(1.000)	82	602426			0.00- 30.00	62.47
-----								
\$ 47	1,2-Dichloroethane-d4					CAS #:	17060-07-0	
9.668	9.668	(1.074)	65	499788	10.0000	10.327	70.00- 130.00	100.00
9.668	9.668	(1.074)	67	237343			0.00- 30.00	47.49
-----								
\$ 59	Toluene-d8					CAS #:	2037-26-5	
12.499	12.499	(1.227)	98	1083880	10.0000	9.633	70.00- 130.00	100.00
12.499	12.499	(1.227)	70	127598			0.00- 42.14	11.77

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	679968			34.50- 94.50	62.73	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	553361	10.0000	9.878	70.00- 130.00	100.00	
17.201	17.201	(1.123)	95	787510			113.13- 173.13	142.31	
17.226	17.226	(1.125)	176	515429			66.52- 126.52	93.15	
-----									
4 Propylene CAS #: 115-07-1									
2.077	2.077	(0.231)	41	21396	0.50000	0.6129	70.00- 130.00	100.00	
2.101	2.101	(0.233)	42	12622			0.00- 30.00	58.99	
2.077	2.077	(0.231)	39	16270			0.00- 30.00	76.04	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.246	2.246	(0.249)	85	47032	0.50000	0.5977	70.00- 130.00	100.00	
2.246	2.246	(0.249)	87	16158			1.53- 61.53	34.36	
-----									
7 Freon 114 CAS #: 76-14-2									
2.728	2.728	(0.303)	135	22292	0.50000	0.5619	70.00- 130.00	100.00	
2.728	2.728	(0.303)	137	7082			0.00- 30.00	31.77	
2.728	2.728	(0.303)	85	37979			0.00- 30.00	170.37	
-----									
8 Chloromethane CAS #: 74-87-3									
2.848	2.848	(0.316)	50	26516	0.50000	0.4939	70.00- 130.00	100.00	
2.848	2.848	(0.316)	52	8315			0.00- 30.00	31.36	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.308	3.308	(0.367)	62	17200	0.50000	0.5898	70.00- 130.00	100.00	
3.291	3.291	(0.366)	64	18530			0.00- 59.65	107.73	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.412	3.412	(0.379)	54	16322	0.50000	0.5160	70.00- 130.00	100.00	
3.412	3.412	(0.379)	39	19101			0.00- 30.00	117.03	
-----									
11 Bromomethane CAS #: 74-83-9									
4.350	4.350	(0.483)	94	7344	0.50000	0.5122	70.00- 130.00	100.00	
4.350	4.350	(0.483)	96	6709			64.87- 124.87	91.35	
-----									
13 Chloroethane CAS #: 75-00-3									
4.724	4.724	(0.525)	64	4810	0.50000	0.4417	70.00- 130.00	100.00	
4.724	4.724	(0.525)	49	2640			0.00- 30.00	54.89	
4.724	4.724	(0.525)	66	1873			0.00- 30.00	38.94	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	45757	0.50000	0.4822	70.00- 130.00	100.00	
5.304	5.304	(0.589)	103	28686			33.99- 93.99	62.69	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPBV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
17 Ethanol						CAS #: 64-17-5			
6.198	6.198	(0.688)	45	8808	0.50000	0.4995	70.00- 130.00	100.00	
6.225	6.225	(0.692)	43	1816			0.00- 30.00	20.62	
6.225	6.225	(0.692)	46	2558			0.00- 30.00	29.04	
-----									
18 1,1-Dichloroethene						CAS #: 75-35-4			
6.335	6.335	(0.704)	98	8699	0.50000	0.5745	70.00- 130.00	100.00	
6.335	6.335	(0.704)	61	30389			0.00- 30.00	349.34	
6.335	6.335	(0.704)	96	13918			0.00- 30.00	160.00	
-----									
19 Freon 113						CAS #: 76-13-1			
6.390	6.390	(0.710)	151	24335	0.50000	0.6872	70.00- 130.00	100.00	
6.390	6.390	(0.710)	153	15348			31.73- 91.73	63.07	
6.390	6.390	(0.710)	101	32286			0.00- 30.00	132.67	
-----									
20 Carbon Disulfide						CAS #: 75-15-0			
6.500	6.500	(0.722)	76	48893	0.50000	0.6149	70.00- 130.00	100.00	
-----									
21 Acetone						CAS #: 67-64-1			
6.637	6.637	(0.737)	43	46382	0.50000	0.4919	70.00- 130.00	100.00	
6.637	6.637	(0.737)	58	11476			0.00- 30.00	24.74	
-----									
24 2-Propanol						CAS #: 67-63-0			
7.021	7.021	(0.780)	45	38389	0.50000	0.4063	70.00- 130.00	100.00	
7.021	7.021	(0.780)	43	11893			0.00- 30.00	30.98	
7.021	7.021	(0.780)	59	1050			0.00- 30.00	2.74	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	5557	0.50000	0.4744	70.00- 130.00	100.00	
6.994	6.994	(0.777)	41	40499			0.00- 30.00	728.79	
-----									
28 Methylene Chloride						CAS #: 75-09-2			
7.213	7.213	(0.801)	84	13570	0.50000	0.6264	70.00- 130.00	100.00	
7.213	7.213	(0.801)	49	34607			297.52- 357.52	255.03	
7.213	7.213	(0.801)	51	11238			0.00- 30.00	82.82	
-----									
29 MTBE						CAS #: 1634-04-4			
7.515	7.515	(0.835)	73	37849	0.50000	0.4483	70.00- 130.00	100.00	
7.515	7.515	(0.835)	57	16985			0.00- 30.00	44.88	
7.515	7.515	(0.835)	41	38715			0.00- 30.00	102.29	
-----									
30 trans-1,2-Dichloroethene						CAS #: 156-60-5			
7.515	7.515	(0.835)	98	11482	0.50000	0.5640	70.00- 130.00	100.00	
7.515	7.515	(0.835)	61	35728			0.00- 30.00	311.17	
7.515	7.515	(0.835)	96	17581			0.00- 30.00	153.12	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
32 Hexane						CAS #: 110-54-3			
7.790	7.790	(0.865)	57	33012	0.50000	0.4572	70.00- 130.00	100.00	
7.790	7.790	(0.865)	43	31726			0.00- 30.00	96.10	
7.790	7.790	(0.865)	86	3670			0.00- 30.00	11.12	
-----									
33 1,1-Dichloroethane						CAS #: 75-34-3			
8.092	8.092	(0.899)	63	40227	0.50000	0.5431	70.00- 130.00	100.00	
8.092	8.092	(0.899)	65	12298			0.00- 59.84	30.57	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	76171	0.50000	0.4987	70.00- 130.00	100.00	
8.174	8.174	(0.908)	42	7124			0.00- 30.00	9.35	
8.174	8.174	(0.908)	86	3018			0.00- 30.00	3.96	
-----									
36 cis-1,2-Dichloroethene						CAS #: 156-59-2			
8.747	8.747	(0.972)	98	10694	0.50000	0.4964	70.00- 130.00	100.00	
8.747	8.747	(0.972)	61	31712			241.26- 301.26	296.54	
8.747	8.747	(0.972)	96	17367			128.30- 188.30	162.40	
-----									
37 2-Butanone						CAS #: 78-93-3			
8.792	8.792	(0.977)	72	8253	0.50000	0.4555	70.00- 130.00	100.00	
8.792	8.792	(0.977)	43	62634			672.66- 732.66	758.92	
8.792	8.792	(0.977)	57	3888			0.00- 30.00	47.11	
-----									
38 Tetrahydrofuran						CAS #: 109-99-9			
9.002	9.002	(1.000)	42	35663	0.50000	0.4625	70.00- 130.00	100.00	
9.002	9.002	(1.000)	71	7173			0.00- 30.00	20.11	
9.002	9.002	(1.000)	72	8848			0.00- 30.00	24.81	
-----									
40 Chloroform						CAS #: 67-66-3			
9.099	9.099	(1.011)	83	39548	0.50000	0.5165	70.00- 130.00	100.00	
9.099	9.099	(1.011)	85	24821			33.23- 93.23	62.76	
-----									
41 Cyclohexane						CAS #: 110-82-7			
9.197	9.197	(1.022)	84	24834	0.50000	0.4784	70.00- 130.00	100.00	
9.197	9.197	(1.022)	56	39484			0.00- 30.00	158.99	
9.197	9.197	(1.022)	41	30302			0.00- 30.00	122.02	
-----									
42 1,1,1-Trichloroethane						CAS #: 71-55-6			
9.229	9.229	(1.025)	97	41403	0.50000	0.5267	70.00- 130.00	100.00	
9.229	9.229	(1.025)	99	25299			33.51- 93.51	61.10	
-----									
44 Carbon Tetrachloride						CAS #: 56-23-5			
9.359	9.359	(1.040)	119	39084	0.50000	0.5446	70.00- 130.00	100.00	
9.359	9.359	(1.040)	117	43473			73.88- 133.88	111.23	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
46 Benzene						CAS #:	71-43-2			
9.638	9.638	(0.946)	78	65076	0.50000	0.5186	70.00- 130.00	100.00		
9.638	9.638	(0.946)	77	15733			0.00- 30.00	24.18		
-----										
45 2,2,4-Trimethylpentane						CAS #:	540-84-1			
9.638	9.638	(1.071)	56	40866	0.50000	0.5038	70.00- 130.00	100.00		
9.638	9.638	(1.071)	99	5296			0.00- 30.00	12.96		
9.638	9.638	(1.071)	41	45568			0.00- 30.00	111.51		
-----										
48 1,2-Dichloroethane						CAS #:	107-06-2			
9.755	9.755	(0.958)	62	37687	0.50000	0.4904	70.00- 130.00	100.00		
9.755	9.755	(0.958)	64	14688			0.00- 30.00	38.97		
-----										
49 Heptane						CAS #:	142-82-5			
9.872	9.872	(0.969)	43	54735	0.50000	0.4072	70.00- 130.00	100.00		
9.872	9.872	(0.969)	57	23356			0.00- 30.00	42.67		
9.872	9.872	(0.969)	100	4286			0.00- 30.00	7.83		
-----										
52 Trichloroethene						CAS #:	79-01-6			
10.475	10.475	(1.028)	130	28367	0.50000	0.5515	70.00- 130.00	100.00		
10.475	10.475	(1.028)	95	28263			0.00- 30.00	99.63		
10.475	10.475	(1.028)	97	18463			0.00- 30.00	65.09		
-----										
53 1,2-Dichloropropane						CAS #:	78-87-5			
10.836	10.836	(1.064)	63	27695	0.50000	0.4974	70.00- 130.00	100.00		
10.836	10.836	(1.064)	62	18905			40.07- 100.07	68.26		
10.861	10.861	(1.066)	41	30026			61.40- 121.40	108.42		
-----										
54 1,4-Dioxane						CAS #:	123-91-1			
11.005	11.005	(1.080)	88	12723	0.50000	0.4474	70.00- 130.00	100.00		
11.029	11.029	(1.083)	58	12675			64.32- 124.32	99.62		
11.029	11.029	(1.083)	57	4978			0.00- 30.00	39.13		
-----										
55 Bromodichloromethane						CAS #:	75-27-4			
11.270	11.270	(1.106)	83	42706	0.50000	0.4731	70.00- 130.00	100.00		
11.270	11.270	(1.106)	85	26651			31.92- 91.92	62.41		
-----										
56 cis-1,3-Dichloropropene						CAS #:	10061-01-5			
12.089	12.089	(1.187)	75	27815	0.50000	0.4182	70.00- 130.00	100.00		
12.089	12.089	(1.187)	77	7774			1.56- 61.56	27.95		
12.065	12.065	(1.185)	39	24232			60.10- 120.10	87.12		
-----										
58 4-Methyl-2-pentanone						CAS #:	108-10-1			
12.379	12.379	(1.215)	43	66694	0.50000	0.3809	70.00- 130.00	100.00		
12.379	12.379	(1.215)	58	18949			0.00- 30.00	28.41		
12.379	12.379	(1.215)	85	6853			0.00- 30.00	10.28		
-----										



AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
60 Toluene						CAS #:	108-88-3			
12.644	12.644	(1.241)	91	70179	0.50000	0.4760	70.00-	130.00	100.00	
12.644	12.644	(1.241)	92	41941			28.58-	88.58	59.76	
-----										
61 trans-1,3-Dichloropropene						CAS #:	10061-02-6			
13.308	13.308	(0.869)	75	28760	0.50000	0.4136	70.00-	130.00	100.00	
13.308	13.308	(0.869)	77	8561			1.05-	61.05	29.77	
13.308	13.308	(0.869)	39	33021			54.43-	114.43	114.82	
-----										
63 1,1,2-Trichloroethane						CAS #:	79-00-5			
13.665	13.665	(0.892)	97	25148	0.50000	0.4945	70.00-	130.00	100.00	
13.665	13.665	(0.892)	99	17065			32.27-	92.27	67.86	
13.665	13.665	(0.892)	83	24278			59.54-	119.54	96.54	
-----										
64 Tetrachloroethene						CAS #:	127-18-4			
13.720	13.720	(0.896)	166	33365	0.50000	0.5090	70.00-	130.00	100.00	
13.747	13.747	(0.897)	129	27468			46.83-	106.83	82.33	
13.747	13.747	(0.897)	131	22898			42.93-	102.93	68.63	
-----										
67 2-Hexanone						CAS #:	591-78-6			
14.132	14.132	(0.922)	58	25034	0.50000	0.3702	70.00-	130.00	100.00	
14.132	14.132	(0.922)	43	66335			227.44-	287.44	264.98	
14.132	14.132	(0.922)	100	3342			0.00-	30.00	13.35	
-----										
68 Dibromochloromethane						CAS #:	124-48-1			
14.352	14.352	(0.937)	129	37697	0.50000	0.4626	70.00-	130.00	100.00	
14.352	14.352	(0.937)	208	1819			0.00-	30.00	4.83	
-----										
69 1,2-Dibromoethane						CAS #:	106-93-4			
14.516	14.516	(0.948)	107	13369	0.50000	0.5858	70.00-	130.00	100.00	
14.516	14.516	(0.948)	109	11875			64.21-	124.21	88.82	
-----										
73 Chlorobenzene						CAS #:	108-90-7			
15.370	15.370	(1.003)	112	67477	0.50000	0.5244	70.00-	130.00	100.00	
15.370	15.370	(1.003)	114	23397			1.79-	61.79	34.67	
15.370	15.370	(1.003)	77	52317			33.30-	93.30	77.53	
-----										
74 Ethyl Benzene						CAS #:	100-41-4			
15.525	15.525	(1.013)	106	31176	0.50000	0.4672	70.00-	130.00	100.00	
15.525	15.525	(1.013)	91	99334			0.00-	30.00	318.62	
-----										
75 m,p-Xylene						CAS #:	108-38-3			
15.731	15.731	(1.027)	106	34442	0.50000	0.4204	70.00-	130.00	100.00	
15.731	15.731	(1.027)	91	72654			0.00-	30.00	210.95	
-----										
77 o-Xylene						CAS #:	95-47-6			
16.376	16.376	(1.069)	106	31807	0.50000	0.4134	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
77 o-Xylene (continued)									
16.376	16.376	(1.069)	91	69614			186.60- 246.60	218.86	
-----									
78 Styrene CAS #: 100-42-5									
16.427	16.427	(1.072)	104	50171	0.50000	0.4217	70.00- 130.00	100.00	
16.401	16.401	(1.071)	78	29267			24.82- 84.82	58.33	
-----									
79 Bromoform CAS #: 75-25-2									
16.711	16.711	(1.091)	173	35483	0.50000	0.4582	70.00- 130.00	100.00	
16.711	16.711	(1.091)	171	17731			0.00- 30.00	49.97	
-----									
80 Cumene CAS #: 98-82-8									
16.917	16.917	(1.104)	105	92255	0.50000	0.4226	70.00- 130.00	100.00	
16.917	16.917	(1.104)	120	26378			0.00- 56.16	28.59	
-----									
82 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
17.484	17.484	(1.141)	83	67618	0.50000	0.5060	70.00- 130.00	100.00	
17.484	17.484	(1.141)	85	42675			33.53- 93.53	63.11	
-----									
83 Propylbenzene CAS #: 103-65-1									
17.536	17.536	(1.145)	91	135940	0.50000	0.4707	70.00- 130.00	100.00	
17.536	17.536	(1.145)	120	28535			0.00- 30.00	20.99	
-----									
84 4-Ethyltoluene CAS #: 622-96-8									
17.716	17.716	(1.157)	105	110142	0.50000	0.4650	70.00- 130.00	100.00	
17.716	17.716	(1.157)	120	32221			0.00- 59.12	29.25	
-----									
85 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.820	17.820	(1.163)	105	91690	0.50000	0.4591	70.00- 130.00	100.00	
17.820	17.820	(1.163)	120	43444			16.79- 76.79	47.38	
-----									
87 1,2,4-Trimethylbenzene CAS #: 95-63-6									
18.413	18.413	(1.202)	105	78671	0.50000	0.4196	70.00- 130.00	100.00	
18.413	18.413	(1.202)	120	33873			13.82- 73.82	43.06	
-----									
89 1,3-Dichlorobenzene CAS #: 541-73-1									
18.929	18.929	(1.236)	146	61418	0.50000	0.4808	70.00- 130.00	100.00	
18.929	18.929	(1.236)	148	37983			0.00- 30.00	61.84	
18.929	18.929	(1.236)	111	27006			0.00- 30.00	43.97	
-----									
90 1,4-Dichlorobenzene CAS #: 106-46-7									
19.083	19.083	(1.246)	146	64803	0.50000	0.4896	70.00- 130.00	100.00	
19.083	19.083	(1.246)	148	41245			0.00- 30.00	63.65	
19.083	19.083	(1.246)	111	28060			0.00- 30.00	43.30	
-----									
91 alpha-chlorotoluene CAS #: 100-44-7									
19.316	19.316	(1.261)	91	54490	0.50000	0.3279	70.00- 130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 alpha-chlorotoluene (continued)									
19.316	19.316	(1.261)	126	10198			0.00- 30.00	18.72	
-----									
94 1,2-Dichlorobenzene CAS #: 95-50-1									
19.625	19.625	(1.281)	146	60823	0.50000	0.4952	70.00- 130.00	100.00	
19.625	19.625	(1.281)	148	38567			32.78- 92.78	63.41	
19.625	19.625	(1.281)	111	26253			14.53- 74.53	43.16	
-----									
96 1,2,4-Trichlorobenzene CAS #: 120-82-1									
21.430	21.430	(1.399)	180	49492	0.50000	0.5093	70.00- 130.00	100.00	
21.430	21.430	(1.399)	182	45990			65.13- 125.13	92.92	
-----									
97 Hexachlorobutadiene CAS #: 87-68-3									
21.559	21.559	(1.407)	225	44199	0.50000	0.5297	70.00- 130.00	100.00	
21.559	21.559	(1.407)	223	29257			0.00- 30.00	66.19	
-----									
98 Naphthalene CAS #: 91-20-3									
21.688	21.688	(1.416)	128	82156	0.50000	0.4180	70.00- 130.00	100.00	
21.688	21.688	(1.416)	127	11596			0.00- 30.00	14.11	
-----									
2 Methylcyclohexane CAS #: 108-87-2									
10.644	10.644	(1.182)	83	35191	0.50000	0.4885	70.00- 130.00	100.00	
10.644	10.644	(1.182)	98	14549			0.00- 30.00	41.34	
10.644	10.644	(1.182)	55	41227			0.00- 30.00	117.15	
-----									
14 Isopentane CAS #: 78-78-4									
4.827	4.827	(0.536)	57	14825	0.50000	0.4687	70.00- 130.00	100.00	
4.827	4.827	(0.536)	43	31490			0.00- 30.00	212.41	
4.827	4.827	(0.536)	42	29689			0.00- 30.00	200.26	
-----									
183 Butane CAS #: 106-97-8									
3.204	3.204	(0.356)	58	2889	0.50000	0.4613	70.00- 130.00	100.00	
3.221	3.221	(0.358)	43	38516			0.00- 30.00	1333.19	
-----									
179 tert-Butyl Alcohol CAS #: 75-65-0									
7.515	7.515	(0.835)	59	33098	0.50000	0.4246	70.00- 130.00	100.00	
7.515	7.515	(0.835)	41	38715			0.00- 30.00	116.97	
7.515	7.515	(0.835)	57	16985			0.00- 30.00	51.32	
-----									

Report Date: 03-Jul-2008 13:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070205.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 2

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 2.0ppbv -&gt; 0.5ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	252155	-29.28
51 1,4-Difluorobenze	1324634	794780	1854488	1088424	-17.83
72 Chlorobenzene-d5	1242028	745217	1738839	964315	-22.36

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 02-JUL-2008 10:12

Client ID: Level 2


Instrument: msdg,i

Sample Info: 125mL #1612-56

Operator: lmr

Column phase: RTx-624

Column diameter: 0.32

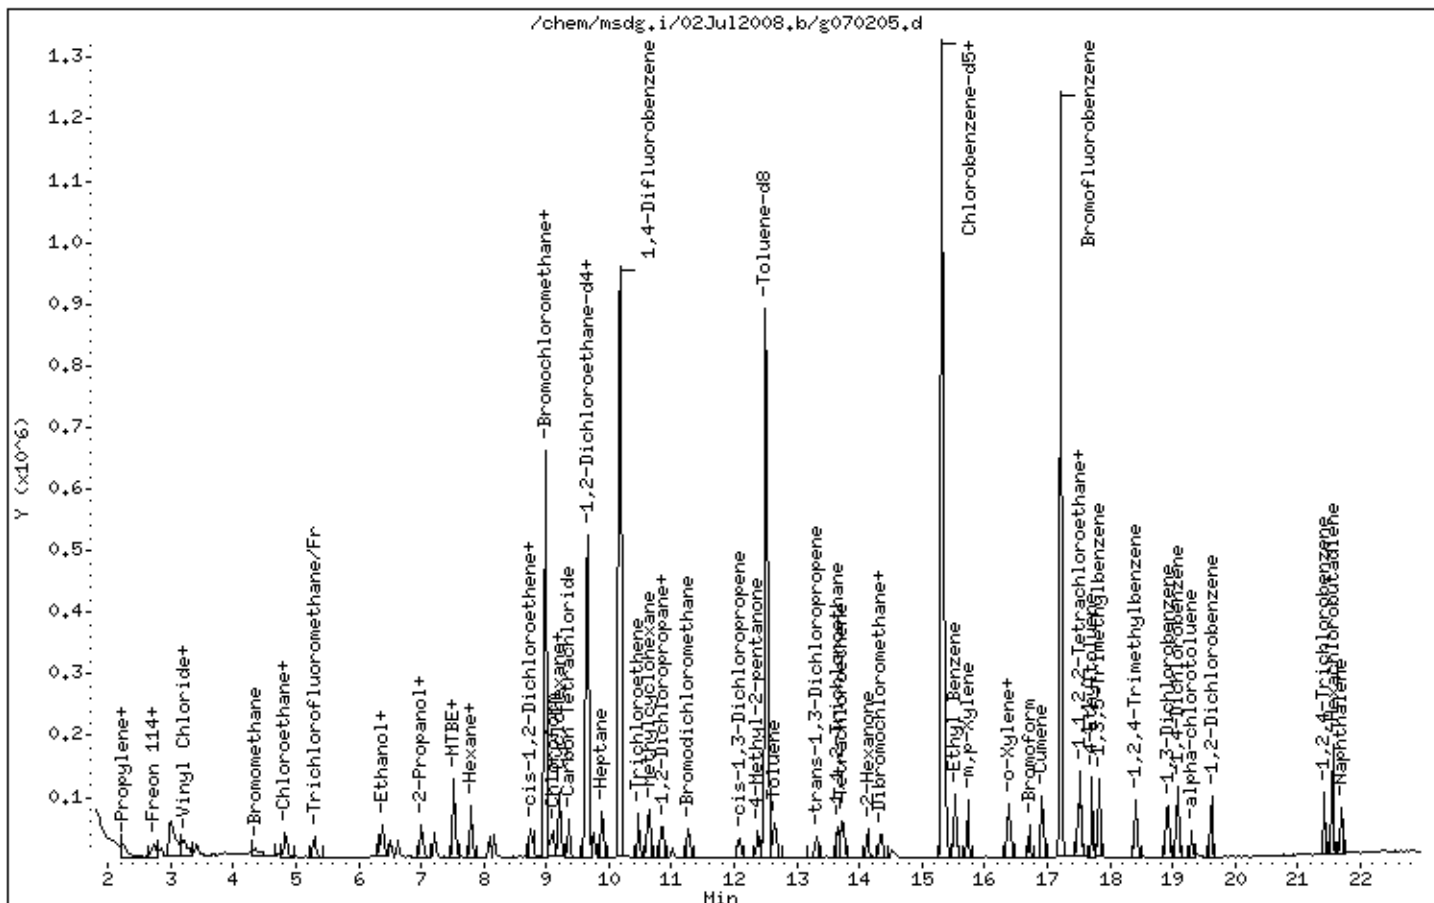

Report Date: 03-Jul-2008 13:48

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070206.d  
 Lab Smp Id: ICAL Client Smp ID: Level 3  
 Inj Date : 02-JUL-2008 11:01  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 500mL #1612-56  
 Misc Info : 2.0ppbv -> 2.0ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:48 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 11:01 Cal File: g070206.d  
 Als bottle: 1 Calibration Sample, Level: 3  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS								
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
-----								
* 39	Bromochloromethane						CAS #: 74-97-5	
9.002	9.002	(1.000)	130	350227	10.0000		70.00- 130.00	100.00
9.002	9.002	(1.000)	128	273114			0.00- 30.00	77.98
9.002	9.002	(1.000)	49	787004			0.00- 30.00	224.71
-----								
* 51	1,4-Difluorobenzene						CAS #: 540-36-3	
10.186	10.186	(1.000)	114	1385748	10.0000		70.00- 130.00	100.00
10.186	10.186	(1.000)	88	236198			0.00- 46.78	17.04
-----								
* 72	Chlorobenzene-d5						CAS #: 3114-55-4	
15.319	15.319	(1.000)	117	1272763	10.0000		70.00- 130.00	100.00
15.319	15.319	(1.000)	82	782023			0.00- 30.00	61.44
-----								
\$ 47	1,2-Dichloroethane-d4						CAS #: 17060-07-0	
9.668	9.668	(1.074)	65	630783	10.0000	9.384	70.00- 130.00	100.00
9.668	9.668	(1.074)	67	314140			0.00- 30.00	49.80
-----								
\$ 59	Toluene-d8						CAS #: 2037-26-5	
12.499	12.499	(1.227)	98	1450415	10.0000	10.125	70.00- 130.00	100.00
12.499	12.499	(1.227)	70	173845			0.00- 42.14	11.99

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	914819			34.50- 94.50	63.07	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	727983	10.0000	9.846	70.00- 130.00	100.00	
17.201	17.201	(1.123)	95	1042823			113.13- 173.13	143.25	
17.226	17.226	(1.125)	176	709021			66.52- 126.52	97.40	
-----									
4 Propylene CAS #: 115-07-1									
2.149	2.149	(0.239)	41	89848	2.00000	1.853	70.00- 130.00	100.00	
2.149	2.149	(0.239)	42	61247			0.00- 30.00	68.17	
2.149	2.149	(0.239)	39	69014			0.00- 30.00	76.81	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.294	2.294	(0.255)	85	210890	2.00000	1.929	70.00- 130.00	100.00	
2.294	2.294	(0.255)	87	69434			1.53- 61.53	32.92	
-----									
7 Freon 114 CAS #: 76-14-2									
2.752	2.752	(0.306)	135	115756	2.00000	2.101	70.00- 130.00	100.00	
2.752	2.752	(0.306)	137	36211			0.00- 30.00	31.28	
2.752	2.752	(0.306)	85	194688			0.00- 30.00	168.19	
-----									
8 Chloromethane CAS #: 74-87-3									
2.872	2.872	(0.319)	50	154671	2.00000	2.074	70.00- 130.00	100.00	
2.896	2.896	(0.322)	52	33803			0.00- 30.00	21.85	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.308	3.308	(0.367)	62	76145	2.00000	1.880	70.00- 130.00	100.00	
3.308	3.308	(0.367)	64	39716			0.00- 59.65	52.16	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.447	3.447	(0.383)	54	79392	2.00000	1.807	70.00- 130.00	100.00	
3.430	3.430	(0.381)	39	116444			0.00- 30.00	146.67	
-----									
11 Bromomethane CAS #: 74-83-9									
4.371	4.371	(0.486)	94	36312	2.00000	1.823	70.00- 130.00	100.00	
4.371	4.371	(0.486)	96	35555			64.87- 124.87	97.92	
-----									
13 Chloroethane CAS #: 75-00-3									
4.724	4.724	(0.525)	64	26861	2.00000	1.776	70.00- 130.00	100.00	
4.724	4.724	(0.525)	49	13579			0.00- 30.00	50.55	
4.724	4.724	(0.525)	66	9607			0.00- 30.00	35.77	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	279470	2.00000	2.121	70.00- 130.00	100.00	
5.304	5.304	(0.589)	103	148968			33.99- 93.99	53.30	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
17 Ethanol						CAS #:	64-17-5			
6.225	6.225	(0.692)	45	54930	2.00000	2.243	70.00- 130.00	100.00		
6.225	6.225	(0.692)	43	13518			0.00- 30.00	24.61		
6.225	6.225	(0.692)	46	21403			0.00- 30.00	38.96		
-----										
19 Freon 113						CAS #:	76-13-1			
6.390	6.390	(0.710)	151	93585	2.00000	1.903	70.00- 130.00	100.00		
6.390	6.390	(0.710)	153	58770			31.73- 91.73	62.80		
6.390	6.390	(0.710)	101	133301			0.00- 30.00	142.44		
-----										
18 1,1-Dichloroethene						CAS #:	75-35-4			
6.335	6.335	(0.704)	98	42668	2.00000	2.029	70.00- 130.00	100.00		
6.335	6.335	(0.704)	61	178424			0.00- 30.00	418.17		
6.335	6.335	(0.704)	96	61313			0.00- 30.00	143.70		
-----										
21 Acetone						CAS #:	67-64-1			
6.637	6.637	(0.737)	43	312358	2.00000	2.385	70.00- 130.00	100.00		
6.637	6.637	(0.737)	58	60599			0.00- 30.00	19.40		
-----										
24 2-Propanol						CAS #:	67-63-0			
7.049	7.049	(0.783)	45	299521	2.00000	2.282	70.00- 130.00	100.00		
7.049	7.049	(0.783)	43	73635			0.00- 30.00	24.58		
7.049	7.049	(0.783)	59	8916			0.00- 30.00	2.98		
-----										
20 Carbon Disulfide						CAS #:	75-15-0			
6.500	6.500	(0.722)	76	209114	2.00000	1.893	70.00- 130.00	100.00		
-----										
28 Methylene Chloride						CAS #:	75-09-2			
7.213	7.213	(0.801)	84	55100	2.00000	1.831	70.00- 130.00	100.00		
7.213	7.213	(0.801)	49	173843			297.52- 357.52	315.50		
7.213	7.213	(0.801)	51	50971			0.00- 30.00	92.51		
-----										
29 MTBE						CAS #:	1634-04-4			
7.543	7.543	(0.838)	73	280285	2.00000	2.390	70.00- 130.00	100.00		
7.543	7.543	(0.838)	57	103268			0.00- 30.00	36.84		
7.543	7.543	(0.838)	41	240230			0.00- 30.00	85.71		
-----										
30 trans-1,2-Dichloroethene						CAS #:	156-60-5			
7.515	7.515	(0.835)	98	62664	2.00000	2.216	70.00- 130.00	100.00		
7.515	7.515	(0.835)	61	206306			0.00- 30.00	329.23		
7.515	7.515	(0.835)	96	107797			0.00- 30.00	172.02		
-----										
32 Hexane						CAS #:	110-54-3			
7.790	7.790	(0.865)	57	191719	2.00000	1.912	70.00- 130.00	100.00		
7.790	7.790	(0.865)	43	172552			0.00- 30.00	90.00		
7.790	7.790	(0.865)	86	22389			0.00- 30.00	11.68		
-----										



AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
33	1,1-Dichloroethane					CAS #: 75-34-3				
8.092	8.092	(0.899)	63	209293	2.00000	2.034	70.00-	130.00	100.00	
8.092	8.092	(0.899)	65	62109			0.00-	59.84	29.68	
-----										
37	2-Butanone					CAS #: 78-93-3				
8.792	8.792	(0.977)	72	50001	2.00000	1.987	70.00-	130.00	100.00	
8.792	8.792	(0.977)	43	353296			672.66-	732.66	706.58	
8.792	8.792	(0.977)	57	22144			0.00-	30.00	44.29	
-----										
36	cis-1,2-Dichloroethene					CAS #: 156-59-2				
8.747	8.747	(0.972)	98	58989	2.00000	1.971	70.00-	130.00	100.00	
8.747	8.747	(0.972)	61	160978			241.26-	301.26	272.89	
8.747	8.747	(0.972)	96	93365			128.30-	188.30	158.28	
-----										
38	Tetrahydrofuran					CAS #: 109-99-9				
9.002	9.002	(1.000)	42	224217	2.00000	2.093	70.00-	130.00	100.00	
9.002	9.002	(1.000)	71	47857			0.00-	30.00	21.34	
9.002	9.002	(1.000)	72	53495			0.00-	30.00	23.86	
-----										
40	Chloroform					CAS #: 67-66-3				
9.099	9.099	(1.011)	83	216606	2.00000	2.037	70.00-	130.00	100.00	
9.099	9.099	(1.011)	85	136911			33.23-	93.23	63.21	
-----										
42	1,1,1-Trichloroethane					CAS #: 71-55-6				
9.229	9.229	(1.025)	97	214795	2.00000	1.967	70.00-	130.00	100.00	
9.229	9.229	(1.025)	99	135334			33.51-	93.51	63.01	
-----										
41	Cyclohexane					CAS #: 110-82-7				
9.197	9.197	(1.022)	84	145933	2.00000	2.024	70.00-	130.00	100.00	
9.197	9.197	(1.022)	56	222474			0.00-	30.00	152.45	
9.197	9.197	(1.022)	41	175978			0.00-	30.00	120.59	
-----										
44	Carbon Tetrachloride					CAS #: 56-23-5				
9.359	9.359	(1.040)	119	213296	2.00000	2.140	70.00-	130.00	100.00	
9.359	9.359	(1.040)	117	214507			73.88-	133.88	100.57	
-----										
46	Benzene					CAS #: 71-43-2				
9.638	9.638	(0.946)	78	335782	2.00000	2.102	70.00-	130.00	100.00	
9.638	9.638	(0.946)	77	78465			0.00-	30.00	23.37	
-----										
48	1,2-Dichloroethane					CAS #: 107-06-2				
9.755	9.755	(0.958)	62	199751	2.00000	2.042	70.00-	130.00	100.00	
9.755	9.755	(0.958)	64	64156			0.00-	30.00	32.12	
-----										
49	Heptane					CAS #: 142-82-5				
9.871	9.871	(0.969)	43	310785	2.00000	1.816	70.00-	130.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
49 Heptane (continued)									
9.871	9.871	(0.969)	57	128058			0.00- 30.00	41.20	
9.871	9.871	(0.969)	100	28174			0.00- 30.00	9.07	
-----									
52 Trichloroethene						CAS #: 79-01-6			
10.475	10.475	(1.028)	130	133036	2.00000	2.032	70.00- 130.00	100.00	
10.475	10.475	(1.028)	95	137329			0.00- 30.00	103.23	
10.475	10.475	(1.028)	97	87403			0.00- 30.00	65.70	
-----									
53 1,2-Dichloropropane						CAS #: 78-87-5			
10.861	10.861	(1.066)	63	141652	2.00000	1.998	70.00- 130.00	100.00	
10.861	10.861	(1.066)	62	99817			40.07- 100.07	70.47	
10.861	10.861	(1.066)	41	131137			61.40- 121.40	92.58	
-----									
54 1,4-Dioxane						CAS #: 123-91-1			
11.029	11.029	(1.083)	88	67959	2.00000	1.877	70.00- 130.00	100.00	
11.029	11.029	(1.083)	58	66544			64.32- 124.32	97.92	
11.029	11.029	(1.083)	57	23172			0.00- 30.00	34.10	
-----									
55 Bromodichloromethane						CAS #: 75-27-4			
11.270	11.270	(1.106)	83	223327	2.00000	1.943	70.00- 130.00	100.00	
11.270	11.270	(1.106)	85	139695			31.92- 91.92	62.55	
-----									
56 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.089	12.089	(1.187)	75	150425	2.00000	1.776	70.00- 130.00	100.00	
12.089	12.089	(1.187)	77	48992			1.56- 61.56	32.57	
12.089	12.089	(1.187)	39	136265			60.10- 120.10	90.59	
-----									
58 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.379	12.379	(1.215)	43	402764	2.00000	1.807	70.00- 130.00	100.00	
12.379	12.379	(1.215)	58	107203			0.00- 30.00	26.62	
12.379	12.379	(1.215)	85	36164			0.00- 30.00	8.98	
-----									
60 Toluene						CAS #: 108-88-3			
12.644	12.644	(1.241)	91	372550	2.00000	1.985	70.00- 130.00	100.00	
12.644	12.644	(1.241)	92	217225			28.58- 88.58	58.31	
-----									
61 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.308	13.308	(0.869)	75	161722	2.00000	1.762	70.00- 130.00	100.00	
13.308	13.308	(0.869)	77	49764			1.05- 61.05	30.77	
13.308	13.308	(0.869)	39	138803			54.43- 114.43	85.83	
-----									
63 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.665	13.665	(0.892)	97	137871	2.00000	2.054	70.00- 130.00	100.00	
13.665	13.665	(0.892)	99	83188			32.27- 92.27	60.34	
13.665	13.665	(0.892)	83	118762			59.54- 119.54	86.14	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
64 Tetrachloroethene						CAS #:	127-18-4			
13.747	13.747	(0.897)	166	177658	2.00000	2.054	70.00-	130.00	100.00	
13.747	13.747	(0.897)	129	135200			46.83-	106.83	76.10	
13.747	13.747	(0.897)	131	131454			42.93-	102.93	73.99	
-----										
67 2-Hexanone						CAS #:	591-78-6			
14.132	14.132	(0.922)	58	155388	2.00000	1.741	70.00-	130.00	100.00	
14.132	14.132	(0.922)	43	404266			227.44-	287.44	260.17	
14.132	14.132	(0.922)	100	22697			0.00-	30.00	14.61	
-----										
68 Dibromochloromethane						CAS #:	124-48-1			
14.352	14.352	(0.937)	129	202688	2.00000	1.884	70.00-	130.00	100.00	
14.352	14.352	(0.937)	208	10568			0.00-	30.00	5.21	
-----										
69 1,2-Dibromoethane						CAS #:	106-93-4			
14.516	14.516	(0.948)	107	60801	2.00000	2.019	70.00-	130.00	100.00	
14.516	14.516	(0.948)	109	56910			64.21-	124.21	93.60	
-----										
73 Chlorobenzene						CAS #:	108-90-7			
15.370	15.370	(1.003)	112	349549	2.00000	2.058	70.00-	130.00	100.00	
15.370	15.370	(1.003)	114	112415			1.79-	61.79	32.16	
15.370	15.370	(1.003)	77	226234			33.30-	93.30	64.72	
-----										
74 Ethyl Benzene						CAS #:	100-41-4			
15.525	15.525	(1.013)	106	173337	2.00000	1.968	70.00-	130.00	100.00	
15.525	15.525	(1.013)	91	558410			0.00-	30.00	322.15	
-----										
75 m,p-Xylene						CAS #:	108-38-3			
15.731	15.731	(1.027)	106	214607	2.00000	1.985	70.00-	130.00	100.00	
15.731	15.731	(1.027)	91	444408			0.00-	30.00	207.08	
-----										
77 o-Xylene						CAS #:	95-47-6			
16.376	16.376	(1.069)	106	195250	2.00000	1.923	70.00-	130.00	100.00	
16.376	16.376	(1.069)	91	423862			186.60-	246.60	217.09	
-----										
78 Styrene						CAS #:	100-42-5			
16.401	16.401	(1.071)	104	323163	2.00000	2.058	70.00-	130.00	100.00	
16.401	16.401	(1.071)	78	180004			24.82-	84.82	55.70	
-----										
79 Bromoform						CAS #:	75-25-2			
16.711	16.711	(1.091)	173	193813	2.00000	1.896	70.00-	130.00	100.00	
16.711	16.711	(1.091)	171	100452			0.00-	30.00	51.83	
-----										
80 Cumene						CAS #:	98-82-8			
16.917	16.917	(1.104)	105	576853	2.00000	2.002	70.00-	130.00	100.00	
16.917	16.917	(1.104)	120	155331			0.00-	56.16	26.93	
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
82	1,1,2,2-Tetrachloroethane					CAS #: 79-34-5			
17.484	17.484	(1.141)	83	359499	2.00000	2.038	70.00- 130.00	100.00	
17.484	17.484	(1.141)	85	232096			33.53- 93.53	64.56	
-----									
83	Propylbenzene					CAS #: 103-65-1			
17.536	17.536	(1.145)	91	800320	2.00000	2.099	70.00- 130.00	100.00	
17.536	17.536	(1.145)	120	178591			0.00- 30.00	22.31	
-----									
84	4-Ethyltoluene					CAS #: 622-96-8			
17.716	17.716	(1.157)	105	673407	2.00000	2.154	70.00- 130.00	100.00	
17.716	17.716	(1.157)	120	190760			0.00- 59.12	28.33	
-----									
85	1,3,5-Trimethylbenzene					CAS #: 108-67-8			
17.820	17.820	(1.163)	105	560022	2.00000	2.124	70.00- 130.00	100.00	
17.820	17.820	(1.163)	120	259865			16.79- 76.79	46.40	
-----									
87	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
18.413	18.413	(1.202)	105	491521	2.00000	1.986	70.00- 130.00	100.00	
18.413	18.413	(1.202)	120	223749			13.82- 73.82	45.52	
-----									
89	1,3-Dichlorobenzene					CAS #: 541-73-1			
18.929	18.929	(1.236)	146	329505	2.00000	1.954	70.00- 130.00	100.00	
18.929	18.929	(1.236)	148	214174			0.00- 30.00	65.00	
18.929	18.929	(1.236)	111	143713			0.00- 30.00	43.61	
-----									
90	1,4-Dichlorobenzene					CAS #: 106-46-7			
19.083	19.083	(1.246)	146	355258	2.00000	2.034	70.00- 130.00	100.00	
19.083	19.083	(1.246)	148	227350			0.00- 30.00	64.00	
19.083	19.083	(1.246)	111	142707			0.00- 30.00	40.17	
-----									
91	alpha-chlorotoluene					CAS #: 100-44-7			
19.315	19.315	(1.261)	91	356243	2.00000	1.624	70.00- 130.00	100.00	
19.315	19.315	(1.261)	126	69329			0.00- 30.00	19.46	
-----									
94	1,2-Dichlorobenzene					CAS #: 95-50-1			
19.625	19.625	(1.281)	146	329235	2.00000	2.031	70.00- 130.00	100.00	
19.625	19.625	(1.281)	148	197431			32.78- 92.78	59.97	
19.625	19.625	(1.281)	111	144589			14.53- 74.53	43.92	
-----									
96	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
21.430	21.430	(1.399)	180	233807	2.00000	1.823	70.00- 130.00	100.00	
21.430	21.430	(1.399)	182	217358			65.13- 125.13	92.96	
-----									
97	Hexachlorobutadiene					CAS #: 87-68-3			
21.559	21.559	(1.407)	225	215264	2.00000	1.955	70.00- 130.00	100.00	
21.559	21.559	(1.407)	223	134237			0.00- 30.00	62.36	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
98 Naphthalene						CAS #: 91-20-3			
21.688	21.688	(1.416)	128	447248	2.00000	1.724	70.00- 130.00	100.00	
21.688	21.688	(1.416)	127	58285			0.00- 30.00	13.03	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	30154	2.00000	1.853	70.00- 130.00	100.00	
6.994	6.994	(0.777)	41	235914			0.00- 30.00	782.36	
-----									
45 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.638	9.638	(1.071)	56	213477	2.00000	1.895	70.00- 130.00	100.00	
9.638	9.638	(1.071)	99	24585			0.00- 30.00	11.52	
9.638	9.638	(1.071)	41	242316			0.00- 30.00	113.51	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	368814	2.00000	1.738	70.00- 130.00	100.00	
8.174	8.174	(0.908)	42	34744			0.00- 30.00	9.42	
8.174	8.174	(0.908)	86	18259			0.00- 30.00	4.95	
-----									
183 Butane						CAS #: 106-97-8			
3.239	3.239	(0.360)	58	17628	2.00000	2.027	70.00- 130.00	100.00	
3.239	3.239	(0.360)	43	187342			0.00- 30.00	1062.75	
-----									
14 Isopentane						CAS #: 78-78-4			
4.848	4.848	(0.539)	57	89036	2.00000	2.027	70.00- 130.00	100.00	
4.848	4.848	(0.539)	43	179816			0.00- 30.00	201.96	
4.848	4.848	(0.539)	42	155371			0.00- 30.00	174.50	
-----									
2 Methylcyclohexane						CAS #: 108-87-2			
10.644	10.644	(1.182)	83	196204	2.00000	1.961	70.00- 130.00	100.00	
10.644	10.644	(1.182)	98	86858			0.00- 30.00	44.27	
10.644	10.644	(1.182)	55	222132			0.00- 30.00	113.21	
-----									
179 tert-Butyl Alcohol						CAS #: 75-65-0			
7.570	7.570	(0.841)	59	226533	2.00000	2.092	70.00- 130.00	100.00	
7.543	7.543	(0.838)	41	240230			0.00- 30.00	106.05	
7.543	7.543	(0.838)	57	103268			0.00- 30.00	45.59	
-----									

Report Date: 03-Jul-2008 13:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070206.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 3

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 2.0ppbv -&gt; 2.0ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	350227	-1.77
51 1,4-Difluorobenze	1324634	794780	1854488	1385748	4.61
72 Chlorobenzene-d5	1242028	745217	1738839	1272763	2.47

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 02-JUL-2008 11:01

Client ID: Level 3


Instrument: msdg.i

Sample Info: 500mL #1612-56

Operator: lmr

Column phase: RTx-624

Column diameter: 0.32

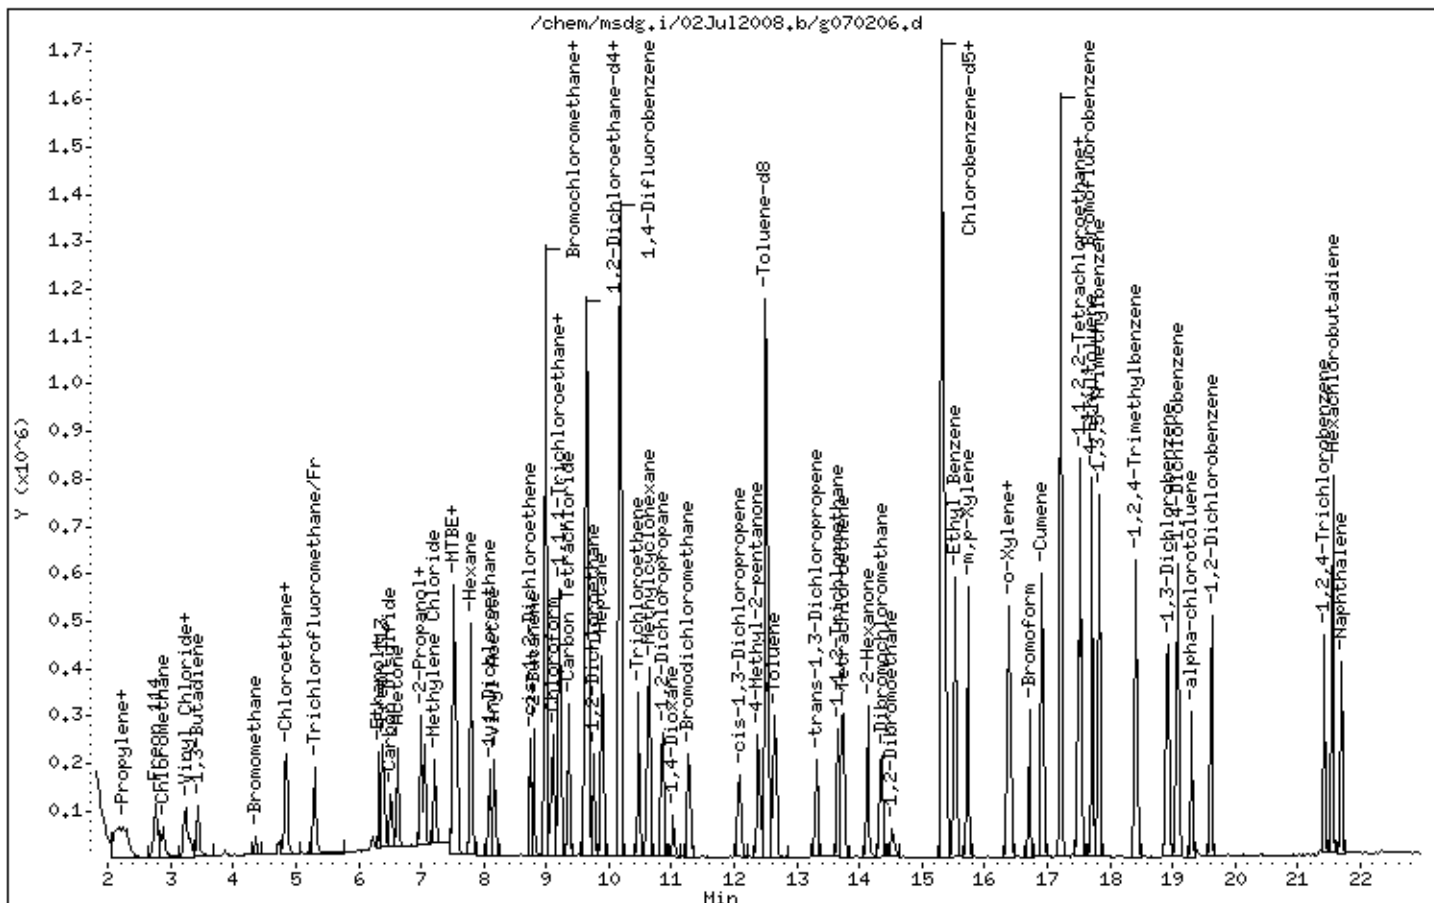

Report Date: 03-Jul-2008 13:47

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070202.d  
 Lab Smp Id: ICAL Client Smp ID: Level 4  
 Inj Date : 02-JUL-2008 08:28  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 200ml #1541-159A  
 Misc Info : 25ppbv -> 10ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:47 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 08:28 Cal File: g070202.d  
 Als bottle: 1 Calibration Sample, Level: 4  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	305594	10.0000			70.00- 130.00	100.00
9.002	9.002	(1.000)	128	227065				0.00- 30.00	74.30
9.002	9.002	(1.000)	49	669589				0.00- 30.00	219.11
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1200887	10.0000			70.00- 130.00	100.00
10.186	10.186	(1.000)	88	194037				0.00- 46.78	16.16
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1113684	10.0000			70.00- 130.00	100.00
15.319	15.319	(1.000)	82	700703				0.00- 30.00	62.92
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668	(1.074)	65	557846	10.0000	9.511		70.00- 130.00	100.00
9.668	9.668	(1.074)	67	282845				0.00- 30.00	50.70
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1265268	10.0000	10.192		70.00- 130.00	100.00
12.499	12.499	(1.227)	70	149796				0.00- 42.14	11.84



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	828841			34.50- 94.50	65.51	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	648860	10.0000	10.030	70.00- 130.00	100.00	
17.201	17.201	(1.123)	95	936915			113.13- 173.13	144.39	
17.226	17.226	(1.125)	176	632021			66.52- 126.52	97.40	
-----									
4 Propylene CAS #: 115-07-1									
2.101	2.101	(0.233)	41	413380	10.0000	9.771	70.00- 130.00	100.00	
2.101	2.101	(0.233)	42	275574			0.00- 30.00	66.66	
2.101	2.101	(0.233)	39	315775			0.00- 30.00	76.39	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.246	2.246	(0.249)	85	986283	10.0000	10.342	70.00- 130.00	100.00	
2.246	2.246	(0.249)	87	315074			1.53- 61.53	31.95	
-----									
7 Freon 114 CAS #: 76-14-2									
2.752	2.752	(0.306)	135	536471	10.0000	11.158	70.00- 130.00	100.00	
2.752	2.752	(0.306)	137	178765			0.00- 30.00	33.32	
2.728	2.728	(0.303)	85	792276			0.00- 30.00	147.68	
-----									
8 Chloromethane CAS #: 74-87-3									
2.848	2.848	(0.316)	50	669931	10.0000	10.296	70.00- 130.00	100.00	
2.848	2.848	(0.316)	52	184976			0.00- 30.00	27.61	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.291	3.291	(0.366)	62	348858	10.0000	9.872	70.00- 130.00	100.00	
3.291	3.291	(0.366)	64	140897			0.00- 59.65	40.39	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.412	3.412	(0.379)	54	364090	10.0000	9.498	70.00- 130.00	100.00	
3.412	3.412	(0.379)	39	475007			0.00- 30.00	130.46	
-----									
11 Bromomethane CAS #: 74-83-9									
4.350	4.350	(0.483)	94	170779	10.0000	9.828	70.00- 130.00	100.00	
4.350	4.350	(0.483)	96	159989			64.87- 124.87	93.68	
-----									
13 Chloroethane CAS #: 75-00-3									
4.723	4.723	(0.525)	64	142769	10.0000	10.819	70.00- 130.00	100.00	
4.723	4.723	(0.525)	49	65115			0.00- 30.00	45.61	
4.723	4.723	(0.525)	66	39815			0.00- 30.00	27.89	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	1270619	10.0000	11.050	70.00- 130.00	100.00	
5.304	5.304	(0.589)	103	786240			33.99- 93.99	61.88	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
17 Ethanol						CAS #: 64-17-5			
6.198	6.198	(0.688)	45	203420	10.0000	9.519	70.00- 130.00	100.00	
6.198	6.198	(0.688)	43	47487			0.00- 30.00	23.34	
6.198	6.198	(0.688)	46	78116			0.00- 30.00	38.40	
-----									
19 Freon 113						CAS #: 76-13-1			
6.390	6.390	(0.710)	151	520409	10.0000	12.127	70.00- 130.00	100.00	
6.390	6.390	(0.710)	153	328024			31.73- 91.73	63.03	
6.390	6.390	(0.710)	101	702175			0.00- 30.00	134.93	
-----									
18 1,1-Dichloroethene						CAS #: 75-35-4			
6.335	6.335	(0.704)	98	210522	10.0000	11.472	70.00- 130.00	100.00	
6.335	6.335	(0.704)	61	798371			0.00- 30.00	379.23	
6.335	6.335	(0.704)	96	333196			0.00- 30.00	158.27	
-----									
21 Acetone						CAS #: 67-64-1			
6.637	6.637	(0.737)	43	1071047	10.0000	9.373	70.00- 130.00	100.00	
6.637	6.637	(0.737)	58	228637			0.00- 30.00	21.35	
-----									
24 2-Propanol						CAS #: 67-63-0			
7.021	7.021	(0.780)	45	1105319	10.0000	9.652	70.00- 130.00	100.00	
7.021	7.021	(0.780)	43	246192			0.00- 30.00	22.27	
7.021	7.021	(0.780)	59	30991			0.00- 30.00	2.80	
-----									
20 Carbon Disulfide						CAS #: 75-15-0			
6.500	6.500	(0.722)	76	1127551	10.0000	11.700	70.00- 130.00	100.00	
-----									
28 Methylene Chloride						CAS #: 75-09-2			
7.213	7.213	(0.801)	84	315623	10.0000	12.022	70.00- 130.00	100.00	
7.213	7.213	(0.801)	49	754782			297.52- 357.52	239.14	
7.213	7.213	(0.801)	51	219323			0.00- 30.00	69.49	
-----									
29 MTBE						CAS #: 1634-04-4			
7.515	7.515	(0.835)	73	950376	10.0000	9.288	70.00- 130.00	100.00	
7.515	7.515	(0.835)	57	380653			0.00- 30.00	40.05	
7.543	7.543	(0.838)	41	859807			0.00- 30.00	90.47	
-----									
30 trans-1,2-Dichloroethene						CAS #: 156-60-5			
7.515	7.515	(0.835)	98	267376	10.0000	10.838	70.00- 130.00	100.00	
7.515	7.515	(0.835)	61	843518			0.00- 30.00	315.48	
7.515	7.515	(0.835)	96	421178			0.00- 30.00	157.52	
-----									
32 Hexane						CAS #: 110-54-3			
7.790	7.790	(0.865)	57	925858	10.0000	10.582	70.00- 130.00	100.00	
7.790	7.790	(0.865)	43	814077			0.00- 30.00	87.93	
7.790	7.790	(0.865)	86	104213			0.00- 30.00	11.26	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	====	=====	=====	=====	=====	=====		
-----										
33	1,1-Dichloroethane					CAS #: 75-34-3				
8.092	8.092	(0.899)	63	922303	10.0000	10.275	70.00- 130.00	100.00		
8.092	8.092	(0.899)	65	271591			0.00- 59.84	29.45		
-----										
37	2-Butanone					CAS #: 78-93-3				
8.792	8.792	(0.977)	72	239701	10.0000	10.917	70.00- 130.00	100.00		
8.792	8.792	(0.977)	43	1642453			672.66- 732.66	685.21		
8.792	8.792	(0.977)	57	94889			0.00- 30.00	39.59		
-----										
36	cis-1,2-Dichloroethene					CAS #: 156-59-2				
8.747	8.747	(0.972)	98	287499	10.0000	11.011	70.00- 130.00	100.00		
8.747	8.747	(0.972)	61	760024			241.26- 301.26	264.36		
8.747	8.747	(0.972)	96	432576			128.30- 188.30	150.46		
-----										
38	Tetrahydrofuran					CAS #: 109-99-9				
9.002	9.002	(1.000)	42	885456	10.0000	9.475	70.00- 130.00	100.00		
9.002	9.002	(1.000)	71	194182			0.00- 30.00	21.93		
9.002	9.002	(1.000)	72	205840			0.00- 30.00	23.25		
-----										
40	Chloroform					CAS #: 67-66-3				
9.099	9.099	(1.011)	83	935335	10.0000	10.080	70.00- 130.00	100.00		
9.099	9.099	(1.011)	85	592874			33.23- 93.23	63.39		
-----										
42	1,1,1-Trichloroethane					CAS #: 71-55-6				
9.229	9.229	(1.025)	97	1002024	10.0000	10.517	70.00- 130.00	100.00		
9.229	9.229	(1.025)	99	634774			33.51- 93.51	63.35		
-----										
41	Cyclohexane					CAS #: 110-82-7				
9.197	9.197	(1.022)	84	684278	10.0000	10.876	70.00- 130.00	100.00		
9.197	9.197	(1.022)	56	1143698			0.00- 30.00	167.14		
9.197	9.197	(1.022)	41	838371			0.00- 30.00	122.52		
-----										
44	Carbon Tetrachloride					CAS #: 56-23-5				
9.359	9.359	(1.040)	119	794728	10.0000	9.137	70.00- 130.00	100.00		
9.359	9.359	(1.040)	117	820930			73.88- 133.88	103.30		
-----										
46	Benzene					CAS #: 71-43-2				
9.638	9.638	(0.946)	78	1516024	10.0000	10.949	70.00- 130.00	100.00		
9.638	9.638	(0.946)	77	349311			0.00- 30.00	23.04		
-----										
48	1,2-Dichloroethane					CAS #: 107-06-2				
9.755	9.755	(0.958)	62	884194	10.0000	10.429	70.00- 130.00	100.00		
9.755	9.755	(0.958)	64	270875			0.00- 30.00	30.64		
-----										
49	Heptane					CAS #: 142-82-5				
9.871	9.871	(0.969)	43	1603068	10.0000	10.808	70.00- 130.00	100.00		

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
49 Heptane (continued)									
9.871	9.871	(0.969)	57	647513			0.00- 30.00	40.39	
9.871	9.871	(0.969)	100	144017			0.00- 30.00	8.98	
-----									
52 Trichloroethene						CAS #: 79-01-6			
10.475	10.475	(1.028)	130	613620	10.0000	10.813	70.00- 130.00	100.00	
10.475	10.475	(1.028)	95	636515			0.00- 30.00	103.73	
10.475	10.475	(1.028)	97	412951			0.00- 30.00	67.30	
-----									
53 1,2-Dichloropropane						CAS #: 78-87-5			
10.860	10.860	(1.066)	63	632568	10.0000	10.297	70.00- 130.00	100.00	
10.860	10.860	(1.066)	62	453247			40.07- 100.07	71.65	
10.860	10.860	(1.066)	41	594341			61.40- 121.40	93.96	
-----									
54 1,4-Dioxane						CAS #: 123-91-1			
11.029	11.029	(1.083)	88	330405	10.0000	10.531	70.00- 130.00	100.00	
11.005	11.005	(1.080)	58	316738			64.32- 124.32	95.86	
11.005	11.005	(1.080)	57	108378			0.00- 30.00	32.80	
-----									
55 Bromodichloromethane						CAS #: 75-27-4			
11.270	11.270	(1.106)	83	1050587	10.0000	10.549	70.00- 130.00	100.00	
11.270	11.270	(1.106)	85	656424			31.92- 91.92	62.48	
-----									
56 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.089	12.089	(1.187)	75	784480	10.0000	10.689	70.00- 130.00	100.00	
12.089	12.089	(1.187)	77	250737			1.56- 61.56	31.96	
12.089	12.089	(1.187)	39	696964			60.10- 120.10	88.84	
-----									
58 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.379	12.379	(1.215)	43	1994454	10.0000	10.324	70.00- 130.00	100.00	
12.379	12.379	(1.215)	58	568218			0.00- 30.00	28.49	
12.379	12.379	(1.215)	85	188069			0.00- 30.00	9.43	
-----									
60 Toluene						CAS #: 108-88-3			
12.644	12.644	(1.241)	91	1752461	10.0000	10.774	70.00- 130.00	100.00	
12.644	12.644	(1.241)	92	1016429			28.58- 88.58	58.00	
-----									
61 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.308	13.308	(0.869)	75	850113	10.0000	10.587	70.00- 130.00	100.00	
13.308	13.308	(0.869)	77	263512			1.05- 61.05	31.00	
13.308	13.308	(0.869)	39	709221			54.43- 114.43	83.43	
-----									
63 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.665	13.665	(0.892)	97	626419	10.0000	10.666	70.00- 130.00	100.00	
13.665	13.665	(0.892)	99	379601			32.27- 92.27	60.60	
13.665	13.665	(0.892)	83	564160			59.54- 119.54	90.06	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
64 Tetrachloroethene						CAS #: 127-18-4			
13.747	13.747	(0.897)	166	832287	10.0000	10.994	70.00- 130.00	100.00	
13.747	13.747	(0.897)	129	639529			46.83- 106.83	76.84	
13.747	13.747	(0.897)	131	614672			42.93- 102.93	73.85	
-----									
67 2-Hexanone						CAS #: 591-78-6			
14.132	14.132	(0.922)	58	825824	10.0000	10.573	70.00- 130.00	100.00	
14.132	14.132	(0.922)	43	2088592			227.44- 287.44	252.91	
14.132	14.132	(0.922)	100	119052			0.00- 30.00	14.42	
-----									
68 Dibromochloromethane						CAS #: 124-48-1			
14.352	14.352	(0.937)	129	1023030	10.0000	10.869	70.00- 130.00	100.00	
14.352	14.352	(0.937)	208	54779			0.00- 30.00	5.35	
-----									
69 1,2-Dibromoethane						CAS #: 106-93-4			
14.516	14.516	(0.948)	107	290533	10.0000	11.024	70.00- 130.00	100.00	
14.516	14.516	(0.948)	109	270643			64.21- 124.21	93.15	
-----									
73 Chlorobenzene						CAS #: 108-90-7			
15.370	15.370	(1.003)	112	1581271	10.0000	10.642	70.00- 130.00	100.00	
15.370	15.370	(1.003)	114	512114			1.79- 61.79	32.39	
15.370	15.370	(1.003)	77	1003344			33.30- 93.30	63.45	
-----									
74 Ethyl Benzene						CAS #: 100-41-4			
15.525	15.525	(1.013)	106	845867	10.0000	10.976	70.00- 130.00	100.00	
15.525	15.525	(1.013)	91	2706168			0.00- 30.00	319.93	
-----									
75 m,p-Xylene						CAS #: 108-38-3			
15.731	15.731	(1.027)	106	1054165	10.0000	11.142	70.00- 130.00	100.00	
15.731	15.731	(1.027)	91	2167357			0.00- 30.00	205.60	
-----									
77 o-Xylene						CAS #: 95-47-6			
16.375	16.375	(1.069)	106	998077	10.0000	11.232	70.00- 130.00	100.00	
16.375	16.375	(1.069)	91	2182762			186.60- 246.60	218.70	
-----									
78 Styrene						CAS #: 100-42-5			
16.401	16.401	(1.071)	104	1648157	10.0000	11.996	70.00- 130.00	100.00	
16.401	16.401	(1.071)	78	885483			24.82- 84.82	53.73	
-----									
79 Bromoform						CAS #: 75-25-2			
16.711	16.711	(1.091)	173	968116	10.0000	10.825	70.00- 130.00	100.00	
16.711	16.711	(1.091)	171	493628			0.00- 30.00	50.99	
-----									
80 Cumene						CAS #: 98-82-8			
16.917	16.917	(1.104)	105	2969590	10.0000	11.780	70.00- 130.00	100.00	
16.917	16.917	(1.104)	120	782854			0.00- 56.16	26.36	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
82	1,1,2,2-Tetrachloroethane					CAS #:	79-34-5			
17.484	17.484	(1.141)	83	1647910	10.0000	10.678	70.00-	130.00	100.00	
17.484	17.484	(1.141)	85	1049768			33.53-	93.53	63.70	
-----										
83	Propylbenzene					CAS #:	103-65-1			
17.536	17.536	(1.145)	91	3901244	10.0000	11.696	70.00-	130.00	100.00	
17.536	17.536	(1.145)	120	862814			0.00-	30.00	22.12	
-----										
84	4-Ethyltoluene					CAS #:	622-96-8			
17.716	17.716	(1.157)	105	3258369	10.0000	11.911	70.00-	130.00	100.00	
17.716	17.716	(1.157)	120	950424			0.00-	59.12	29.17	
-----										
85	1,3,5-Trimethylbenzene					CAS #:	108-67-8			
17.820	17.820	(1.163)	105	2651845	10.0000	11.496	70.00-	130.00	100.00	
17.820	17.820	(1.163)	120	1277500			16.79-	76.79	48.17	
-----										
87	1,2,4-Trimethylbenzene					CAS #:	95-63-6			
18.413	18.413	(1.202)	105	2551044	10.0000	11.781	70.00-	130.00	100.00	
18.413	18.413	(1.202)	120	1135895			13.82-	73.82	44.53	
-----										
89	1,3-Dichlorobenzene					CAS #:	541-73-1			
18.929	18.929	(1.236)	146	1649339	10.0000	11.179	70.00-	130.00	100.00	
18.929	18.929	(1.236)	148	1059071			0.00-	30.00	64.21	
18.929	18.929	(1.236)	111	700584			0.00-	30.00	42.48	
-----										
90	1,4-Dichlorobenzene					CAS #:	106-46-7			
19.083	19.083	(1.246)	146	1698551	10.0000	11.112	70.00-	130.00	100.00	
19.083	19.083	(1.246)	148	1077645			0.00-	30.00	63.44	
19.083	19.083	(1.246)	111	694072			0.00-	30.00	40.86	
-----										
91	alpha-chlorotoluene					CAS #:	100-44-7			
19.315	19.315	(1.261)	91	2104844	10.0000	10.969	70.00-	130.00	100.00(A)	
19.315	19.315	(1.261)	126	415195			0.00-	30.00	19.73	
-----										
94	1,2-Dichlorobenzene					CAS #:	95-50-1			
19.625	19.625	(1.281)	146	1575995	10.0000	11.110	70.00-	130.00	100.00	
19.625	19.625	(1.281)	148	984528			32.78-	92.78	62.47	
19.625	19.625	(1.281)	111	689956			14.53-	74.53	43.78	
-----										
96	1,2,4-Trichlorobenzene					CAS #:	120-82-1			
21.430	21.430	(1.399)	180	1265465	10.0000	11.276	70.00-	130.00	100.00	
21.430	21.430	(1.399)	182	1233963			65.13-	125.13	97.51	
-----										
97	Hexachlorobutadiene					CAS #:	87-68-3			
21.559	21.559	(1.407)	225	1118557	10.0000	11.607	70.00-	130.00	100.00	
21.559	21.559	(1.407)	223	714607			0.00-	30.00	63.89	
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
98 Naphthalene						CAS #: 91-20-3			
21.688	21.688	(1.416)	128	2608619	10.0000	11.494	70.00- 130.00	100.00	
21.688	21.688	(1.416)	127	325955			0.00- 30.00	12.50	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	160209	10.0000	11.285	70.00- 130.00	100.00	
6.994	6.994	(0.777)	41	1008810			0.00- 30.00	629.68	
-----									
45 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.638	9.638	(1.071)	56	1021877	10.0000	10.394	70.00- 130.00	100.00	
9.638	9.638	(1.071)	99	125256			0.00- 30.00	12.26	
9.638	9.638	(1.071)	41	1092561			0.00- 30.00	106.92	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	1981695	10.0000	10.705	70.00- 130.00	100.00	
8.174	8.174	(0.908)	42	173674			0.00- 30.00	8.76	
8.174	8.174	(0.908)	86	101798			0.00- 30.00	5.14	
-----									
183 Butane						CAS #: 106-97-8			
3.221	3.221	(0.358)	58	78335	10.0000	10.322	70.00- 130.00	100.00	
3.221	3.221	(0.358)	43	879789			0.00- 30.00	1123.11	
-----									
14 Isopentane						CAS #: 78-78-4			
4.827	4.827	(0.536)	57	393694	10.0000	10.271	70.00- 130.00	100.00	
4.827	4.827	(0.536)	43	792186			0.00- 30.00	201.22	
4.827	4.827	(0.536)	42	689029			0.00- 30.00	175.02	
-----									
2 Methylcyclohexane						CAS #: 108-87-2			
10.644	10.644	(1.182)	83	947078	10.0000	10.848	70.00- 130.00	100.00	
10.644	10.644	(1.182)	98	425038			0.00- 30.00	44.88	
10.644	10.644	(1.182)	55	1069902			0.00- 30.00	112.97	
-----									
179 tert-Butyl Alcohol						CAS #: 75-65-0			
7.543	7.543	(0.838)	59	882838	10.0000	9.344	70.00- 130.00	100.00	
7.543	7.543	(0.838)	41	859807			0.00- 30.00	97.39	
7.515	7.515	(0.835)	57	380653			0.00- 30.00	43.12	
-----									

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 03-Jul-2008 13:47

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070202.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 4

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 25ppbv -&gt; 10ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	305594	-14.29
51 1,4-Difluorobenze	1324634	794780	1854488	1200887	-9.34
72 Chlorobenzene-d5	1242028	745217	1738839	1113684	-10.33

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Date : 02-JUL-2008 08:28

Client ID: Level 4


Instrument: msdg.i

Sample Info: 200ml #1541-159A

Operator: lmr

Column phase: RTx-624

Column diameter: 0.32

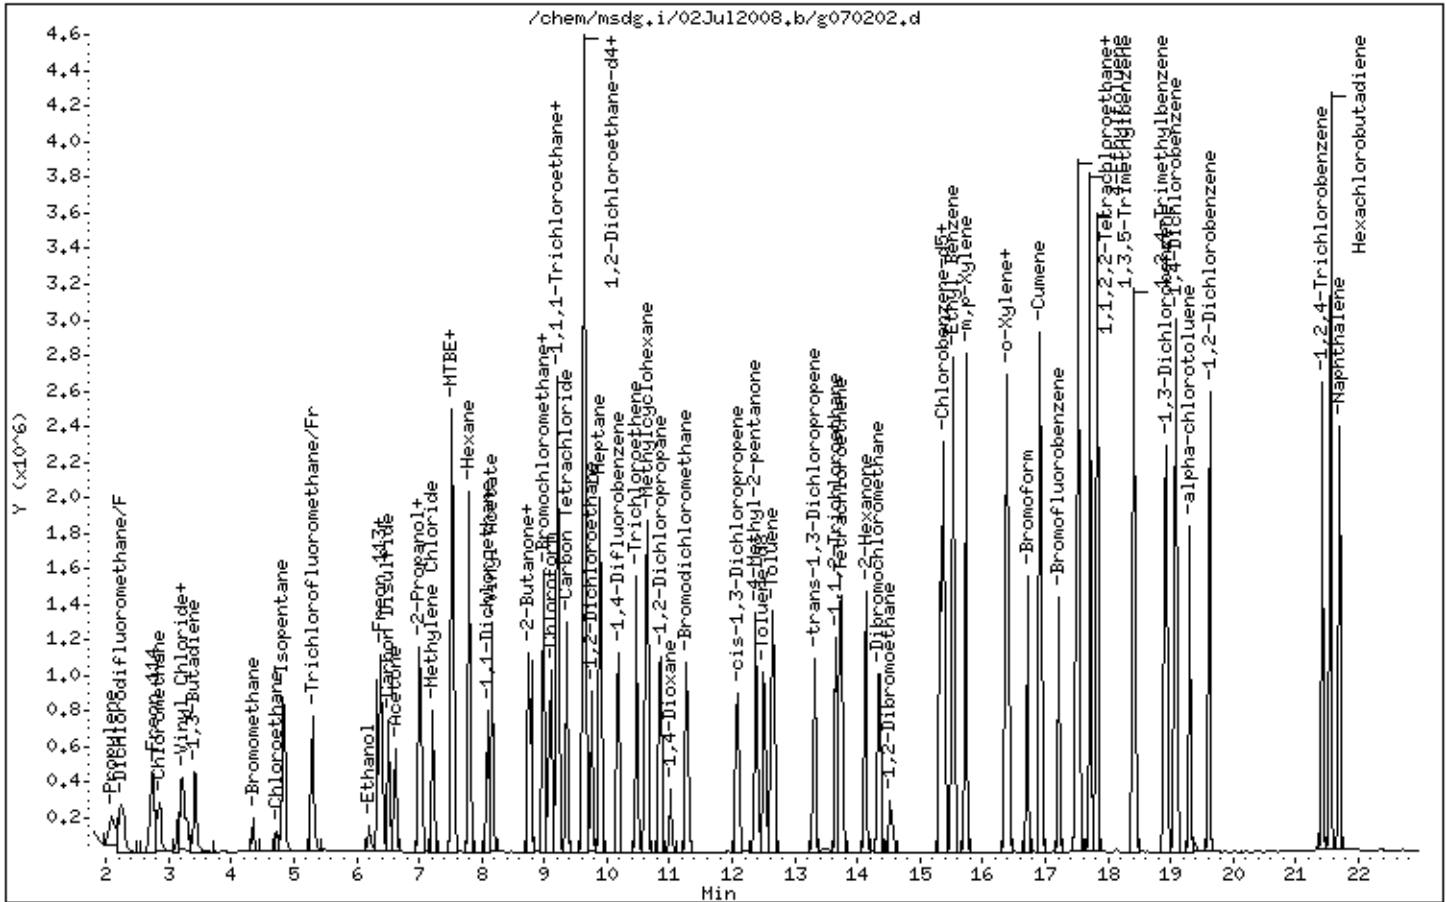

Report Date: 03-Jul-2008 13:48

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070207.d  
 Lab Smp Id: ICAL Client Smp ID: Level 5  
 Inj Date : 02-JUL-2008 11:32  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 500mL #1541-159A  
 Misc Info : 25ppbv -> 25ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:48 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 11:32 Cal File: g070207.d  
 Als bottle: 1 Calibration Sample, Level: 5  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT	ON-COL	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	356533	10.0000		80.00- 120.00	100.00	
9.002	9.002	(1.000)	128	273179			46.62- 106.62	76.62	
9.002	9.002	(1.000)	49	810944			197.45- 257.45	227.45	
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1324634	10.0000		80.00- 120.00	100.00	
10.186	10.186	(1.000)	88	222248			0.00- 46.78	16.78	
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1242028	10.0000		80.00- 120.00	100.00	
15.319	15.319	(1.000)	82	773746			32.30- 92.30	62.30	
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668	(1.074)	65	667825	10.0000	9.759	80.00- 120.00	100.00	
9.668	9.668	(1.074)	67	371698			25.66- 85.66	55.66	
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1391044	10.0000	10.158	80.00- 120.00	100.00	
12.499	12.499	(1.227)	70	168872			0.00- 42.14	12.14	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	897216			34.50- 94.50	64.50	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	747620	10.0000	10.362	80.00- 120.00	100.00	
17.201	17.201	(1.123)	95	1070053			113.13- 173.13	143.13	
17.226	17.226	(1.125)	176	721593			66.52- 126.52	96.52	
-----									
4 Propylene CAS #: 115-07-1									
2.101	2.101	(0.233)	41	1162891	25.0000	23.560	80.00- 120.00	100.00	
2.125	2.125	(0.236)	42	776309			36.76- 96.76	66.76	
2.125	2.125	(0.236)	39	886291			46.21- 106.21	76.21	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.270	2.270	(0.252)	85	2615486	25.0000	23.506	80.00- 120.00	100.00	
2.270	2.270	(0.252)	87	824741			1.53- 61.53	31.53	
-----									
7 Freon 114 CAS #: 76-14-2									
2.752	2.752	(0.306)	135	1422162	25.0000	25.354	80.00- 120.00	100.00	
2.752	2.752	(0.306)	137	466886			2.83- 62.83	32.83	
2.752	2.752	(0.306)	85	2047600			113.98- 173.98	143.98	
-----									
8 Chloromethane CAS #: 74-87-3									
2.872	2.872	(0.319)	50	1775065	25.0000	23.382	80.00- 120.00	100.00	
2.872	2.872	(0.319)	52	510025			0.00- 58.73	28.73	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.291	3.291	(0.366)	62	978589	25.0000	23.735	80.00- 120.00	100.00	
3.308	3.308	(0.367)	64	290180			0.00- 59.65	29.65	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.430	3.430	(0.381)	54	1162461	25.0000	25.993	80.00- 120.00	100.00	
3.430	3.430	(0.381)	39	1512951			100.15- 160.15	130.15	
-----									
11 Bromomethane CAS #: 74-83-9									
4.351	4.351	(0.483)	94	504095	25.0000	24.864	80.00- 120.00	100.00	
4.351	4.351	(0.483)	96	478222			64.87- 124.87	94.87	
-----									
13 Chloroethane CAS #: 75-00-3									
4.724	4.724	(0.525)	64	399358	25.0000	25.938	80.00- 120.00	100.00	
4.724	4.724	(0.525)	49	178678			14.74- 74.74	44.74	
4.724	4.724	(0.525)	66	118390			0.00- 59.65	29.65	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	3423795	25.0000	25.521	80.00- 120.00	100.00	
5.304	5.304	(0.589)	103	2190719			33.99- 93.99	63.99	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
17 Ethanol						CAS #: 64-17-5			
6.225	6.225	(0.692)	45	584235	25.0000	23.434	80.00- 120.00	100.00	
6.225	6.225	(0.692)	43	133682			0.00- 52.88	22.88	
6.225	6.225	(0.692)	46	221520			7.92- 67.92	37.92	
-----									
19 Freon 113						CAS #: 76-13-1			
6.390	6.390	(0.710)	151	1123644	25.0000	22.442	80.00- 120.00	100.00	
6.390	6.390	(0.710)	153	693584			31.73- 91.73	61.73	
6.390	6.390	(0.710)	101	1540169			107.07- 167.07	137.07	
-----									
18 1,1-Dichloroethene						CAS #: 75-35-4			
6.335	6.335	(0.704)	98	495662	25.0000	23.152	80.00- 120.00	100.00	
6.335	6.335	(0.704)	61	2224284			418.75- 478.75	448.75	
6.335	6.335	(0.704)	96	778606			127.08- 187.08	157.08	
-----									
21 Acetone						CAS #: 67-64-1			
6.637	6.637	(0.737)	43	3404134	25.0000	25.533	80.00- 120.00	100.00	
6.637	6.637	(0.737)	58	658265			0.00- 49.34	19.34	
-----									
24 2-Propanol						CAS #: 67-63-0			
7.049	7.049	(0.783)	45	3698595	25.0000	27.682	80.00- 120.00	100.00	
7.049	7.049	(0.783)	43	808587			0.00- 51.86	21.86	
7.049	7.049	(0.783)	59	95237			0.00- 32.57	2.57	
-----									
20 Carbon Disulfide						CAS #: 75-15-0			
6.500	6.500	(0.722)	76	2568503	25.0000	22.845	80.00- 120.00	100.00	
-----									
28 Methylene Chloride						CAS #: 75-09-2			
7.213	7.213	(0.801)	84	635295	25.0000	20.742	80.00- 120.00	100.00	
7.213	7.213	(0.801)	49	2080715			297.52- 357.52	327.52	
7.213	7.213	(0.801)	51	602750			64.88- 124.88	94.88	
-----									
29 MTBE						CAS #: 1634-04-4			
7.515	7.515	(0.835)	73	3665011	25.0000	30.702	80.00- 120.00	100.00	
7.515	7.515	(0.835)	57	1456367			9.74- 69.74	39.74	
7.543	7.543	(0.838)	41	2903852			49.23- 109.23	79.23	
-----									
30 trans-1,2-Dichloroethene						CAS #: 156-60-5			
7.515	7.515	(0.835)	98	784634	25.0000	27.261	80.00- 120.00	100.00	
7.515	7.515	(0.835)	61	2530469			292.50- 352.50	322.50	
7.515	7.515	(0.835)	96	1247007			128.93- 188.93	158.93	
-----									
32 Hexane						CAS #: 110-54-3			
7.790	7.790	(0.865)	57	2728829	25.0000	26.732	80.00- 120.00	100.00	
7.790	7.790	(0.865)	43	2406264			58.18- 118.18	88.18	
7.790	7.790	(0.865)	86	299642			0.00- 40.98	10.98	
-----									

AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
33	1,1-Dichloroethane					CAS #: 75-34-3				
8.092	8.092	(0.899)	63	2607766	25.0000	24.902	80.00-	120.00	100.00	
8.092	8.092	(0.899)	65	778037			0.00-	59.84	29.84	
-----										
37	2-Butanone					CAS #: 78-93-3				
8.792	8.792	(0.977)	72	696945	25.0000	27.207	80.00-	120.00	100.00	
8.792	8.792	(0.977)	43	4897150			672.66-	732.66	702.66	
8.792	8.792	(0.977)	57	288375			11.38-	71.38	41.38	
-----										
36	cis-1,2-Dichloroethene					CAS #: 156-59-2				
8.748	8.748	(0.972)	98	792854	25.0000	26.028	80.00-	120.00	100.00	
8.748	8.748	(0.972)	61	2150666			241.26-	301.26	271.26	
8.748	8.748	(0.972)	96	1255085			128.30-	188.30	158.30	
-----										
38	Tetrahydrofuran					CAS #: 109-99-9				
9.002	9.002	(1.000)	42	2896924	25.0000	26.569	80.00-	120.00	100.00	
9.002	9.002	(1.000)	71	630802			0.00-	51.77	21.77	
9.002	9.002	(1.000)	72	672290			0.00-	53.21	23.21	
-----										
40	Chloroform					CAS #: 67-66-3				
9.099	9.099	(1.011)	83	2730211	25.0000	25.218	80.00-	120.00	100.00	
9.099	9.099	(1.011)	85	1726308			33.23-	93.23	63.23	
-----										
42	1,1,1-Trichloroethane					CAS #: 71-55-6				
9.229	9.229	(1.025)	97	2844559	25.0000	25.591	80.00-	120.00	100.00	
9.229	9.229	(1.025)	99	1806458			33.51-	93.51	63.51	
-----										
41	Cyclohexane					CAS #: 110-82-7				
9.197	9.197	(1.022)	84	1942953	25.0000	26.469	80.00-	120.00	100.00	
9.197	9.197	(1.022)	56	3247665			137.15-	197.15	167.15	
9.197	9.197	(1.022)	41	2422217			94.67-	154.67	124.67	
-----										
44	Carbon Tetrachloride					CAS #: 56-23-5				
9.359	9.359	(1.040)	119	2277328	25.0000	22.441	80.00-	120.00	100.00	
9.359	9.359	(1.040)	117	2365600			73.88-	133.88	103.88	
-----										
46	Benzene					CAS #: 71-43-2				
9.639	9.639	(0.946)	78	4096464	25.0000	26.821	80.00-	120.00	100.00	
9.639	9.639	(0.946)	77	955129			0.00-	53.32	23.32	
-----										
48	1,2-Dichloroethane					CAS #: 107-06-2				
9.755	9.755	(0.958)	62	2498787	25.0000	26.719	80.00-	120.00	100.00	
9.755	9.755	(0.958)	64	761767			0.49-	60.49	30.49	
-----										
49	Heptane					CAS #: 142-82-5				
9.872	9.872	(0.969)	43	4708070	25.0000	28.778	80.00-	120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
49 Heptane (continued)									
9.872	9.872	(0.969)	57	1842409			9.13- 69.13	39.13	
9.872	9.872	(0.969)	100	416044			0.00- 38.84	8.84	
-----									
52 Trichloroethene						CAS #: 79-01-6			
10.475	10.475	(1.028)	130	1668455	25.0000	26.654	80.00- 120.00	100.00	
10.475	10.475	(1.028)	95	1766475			75.87- 135.87	105.87	
10.475	10.475	(1.028)	97	1161362			39.61- 99.61	69.61	
-----									
53 1,2-Dichloropropane						CAS #: 78-87-5			
10.861	10.861	(1.066)	63	1825265	25.0000	26.936	80.00- 120.00	100.00	
10.861	10.861	(1.066)	62	1278921			40.07- 100.07	70.07	
10.861	10.861	(1.066)	41	1668205			61.40- 121.40	91.40	
-----									
54 1,4-Dioxane						CAS #: 123-91-1			
11.029	11.029	(1.083)	88	972671	25.0000	28.107	80.00- 120.00	100.00	
11.029	11.029	(1.083)	58	917454			64.32- 124.32	94.32	
11.029	11.029	(1.083)	57	305117			1.37- 61.37	31.37	
-----									
55 Bromodichloromethane						CAS #: 75-27-4			
11.270	11.270	(1.106)	83	3033603	25.0000	27.616	80.00- 120.00	100.00	
11.270	11.270	(1.106)	85	1878524			31.92- 91.92	61.92	
-----									
56 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.090	12.090	(1.187)	75	2351865	25.0000	29.053	80.00- 120.00	100.00	
12.090	12.090	(1.187)	77	742243			1.56- 61.56	31.56	
12.090	12.090	(1.187)	39	2118944			60.10- 120.10	90.10	
-----									
58 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.379	12.379	(1.215)	43	6233234	25.0000	29.251	80.00- 120.00	100.00	
12.379	12.379	(1.215)	58	1730605			0.00- 57.76	27.76	
12.379	12.379	(1.215)	85	567857			0.00- 39.11	9.11	
-----									
60 Toluene						CAS #: 108-88-3			
12.644	12.644	(1.241)	91	4976893	25.0000	27.740	80.00- 120.00	100.00	
12.644	12.644	(1.241)	92	2915635			28.58- 88.58	58.58	
-----									
61 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.308	13.308	(0.869)	75	2551830	25.0000	28.496	80.00- 120.00	100.00	
13.308	13.308	(0.869)	77	792362			1.05- 61.05	31.05	
13.308	13.308	(0.869)	39	2154585			54.43- 114.43	84.43	
-----									
63 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.665	13.665	(0.892)	97	1755465	25.0000	26.801	80.00- 120.00	100.00	
13.665	13.665	(0.892)	99	1093196			32.27- 92.27	62.27	
13.665	13.665	(0.892)	83	1571881			59.54- 119.54	89.54	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
64 Tetrachloroethene						CAS #: 127-18-4			
13.747	13.747	(0.897)	166	2281209	25.0000	27.021	80.00- 120.00	100.00	
13.747	13.747	(0.897)	129	1752734			46.83- 106.83	76.83	
13.747	13.747	(0.897)	131	1663762			42.93- 102.93	72.93	
-----									
67 2-Hexanone						CAS #: 591-78-6			
14.132	14.132	(0.922)	58	2545575	25.0000	29.224	80.00- 120.00	100.00	
14.132	14.132	(0.922)	43	6553217			227.44- 287.44	257.44	
14.132	14.132	(0.922)	100	368338			0.00- 44.47	14.47	
-----									
68 Dibromochloromethane						CAS #: 124-48-1			
14.352	14.352	(0.937)	129	2905811	25.0000	27.683	80.00- 120.00	100.00	
14.352	14.352	(0.937)	208	154460			0.00- 35.32	5.32	
-----									
69 1,2-Dibromoethane						CAS #: 106-93-4			
14.517	14.517	(0.948)	107	739470	25.0000	25.158	80.00- 120.00	100.00	
14.517	14.517	(0.948)	109	696660			64.21- 124.21	94.21	
-----									
73 Chlorobenzene						CAS #: 108-90-7			
15.370	15.370	(1.003)	112	4415811	25.0000	26.646	80.00- 120.00	100.00	
15.370	15.370	(1.003)	114	1403971			1.79- 61.79	31.79	
15.370	15.370	(1.003)	77	2795050			33.30- 93.30	63.30	
-----									
74 Ethyl Benzene						CAS #: 100-41-4			
15.525	15.525	(1.013)	106	2379904	25.0000	27.691	80.00- 120.00	100.00	
15.525	15.525	(1.013)	91	7738414			295.16- 355.16	325.16	
-----									
75 m,p-Xylene						CAS #: 108-38-3			
15.731	15.731	(1.027)	106	3007033	25.0000	28.500	80.00- 120.00	100.00	
15.731	15.731	(1.027)	91	6238192			177.45- 237.45	207.45	
-----									
77 o-Xylene						CAS #: 95-47-6			
16.376	16.376	(1.069)	106	2881032	25.0000	29.072	80.00- 120.00	100.00	
16.376	16.376	(1.069)	91	6240333			186.60- 246.60	216.60	
-----									
78 Styrene						CAS #: 100-42-5			
16.401	16.401	(1.071)	104	4633127	25.0000	30.238	80.00- 120.00	100.00	
16.401	16.401	(1.071)	78	2539928			24.82- 84.82	54.82	
-----									
79 Bromoform						CAS #: 75-25-2			
16.711	16.711	(1.091)	173	2797247	25.0000	28.046	80.00- 120.00	100.00	
16.711	16.711	(1.091)	171	1444777			21.65- 81.65	51.65	
-----									
80 Cumene						CAS #: 98-82-8			
16.917	16.917	(1.104)	105	8422060	25.0000	29.956	80.00- 120.00	100.00	
16.917	16.917	(1.104)	120	2203228			0.00- 56.16	26.16	
-----									

Report Date: 03-Jul-2008 13:48

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
82	1,1,2,2-Tetrachloroethane					CAS #: 79-34-5			
17.484	17.484	(1.141)	83	4638077	25.0000	26.947	80.00- 120.00	100.00	
17.484	17.484	(1.141)	85	2946371			33.53- 93.53	63.53	
-----									
83	Propylbenzene					CAS #: 103-65-1			
17.536	17.536	(1.145)	91	10893917	25.0000	29.285	80.00- 120.00	100.00	
17.536	17.536	(1.145)	120	2353530			0.00- 51.60	21.60	
-----									
84	4-Ethyltoluene					CAS #: 622-96-8			
17.716	17.716	(1.157)	105	9293812	25.0000	30.464	80.00- 120.00	100.00	
17.716	17.716	(1.157)	120	2706617			0.00- 59.12	29.12	
-----									
85	1,3,5-Trimethylbenzene					CAS #: 108-67-8			
17.820	17.820	(1.163)	105	7615905	25.0000	29.605	80.00- 120.00	100.00	
17.820	17.820	(1.163)	120	3563378			16.79- 76.79	46.79	
-----									
87	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
18.413	18.413	(1.202)	105	7373357	25.0000	30.531	80.00- 120.00	100.00	
18.413	18.413	(1.202)	120	3230759			13.82- 73.82	43.82	
-----									
89	1,3-Dichlorobenzene					CAS #: 541-73-1			
18.929	18.929	(1.236)	146	4540729	25.0000	27.596	80.00- 120.00	100.00	
18.929	18.929	(1.236)	148	2897970			33.82- 93.82	63.82	
18.929	18.929	(1.236)	111	1985948			13.74- 73.74	43.74	
-----									
90	1,4-Dichlorobenzene					CAS #: 106-46-7			
19.083	19.083	(1.246)	146	4673580	25.0000	27.416	80.00- 120.00	100.00	
19.083	19.083	(1.246)	148	2937403			32.85- 92.85	62.85	
19.083	19.083	(1.246)	111	1949392			11.71- 71.71	41.71	
-----									
91	alpha-chlorotoluene					CAS #: 100-44-7			
19.316	19.316	(1.261)	91	6542757	25.0000	30.572	80.00- 120.00	100.00(A)	
19.316	19.316	(1.261)	126	1238175			0.00- 48.92	18.92	
-----									
94	1,2-Dichlorobenzene					CAS #: 95-50-1			
19.625	19.625	(1.281)	146	4291731	25.0000	27.128	80.00- 120.00	100.00	
19.625	19.625	(1.281)	148	2694144			32.78- 92.78	62.78	
19.625	19.625	(1.281)	111	1911185			14.53- 74.53	44.53	
-----									
96	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
21.431	21.431	(1.399)	180	3272503	25.0000	26.148	80.00- 120.00	100.00	
21.431	21.431	(1.399)	182	3113059			65.13- 125.13	95.13	
-----									
97	Hexachlorobutadiene					CAS #: 87-68-3			
21.559	21.559	(1.407)	225	2780854	25.0000	25.875	80.00- 120.00	100.00	
21.559	21.559	(1.407)	223	1761301			33.34- 93.34	63.34	
-----									



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
-----									
98 Naphthalene						CAS #: 91-20-3			
21.688	21.688	(1.416)	128	6978415	25.0000	27.570	80.00- 120.00	100.00	
21.688	21.688	(1.416)	127	862499			0.00- 42.36	12.36	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	393409	25.0000	23.752	80.00- 120.00	100.00	
6.994	6.994	(0.777)	41	3012882			735.84- 795.84	765.84	
-----									
45 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.639	9.639	(1.071)	56	2911515	25.0000	25.383	80.00- 120.00	100.00	
9.639	9.639	(1.071)	99	359142			0.00- 42.34	12.34	
9.639	9.639	(1.071)	41	3279618			82.64- 142.64	112.64	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	5825010	25.0000	26.972	80.00- 120.00	100.00	
8.174	8.174	(0.908)	42	507562			0.00- 38.71	8.71	
8.174	8.174	(0.908)	86	284253			0.00- 34.88	4.88	
-----									
183 Butane						CAS #: 106-97-8			
3.221	3.221	(0.358)	58	224052	25.0000	25.304	80.00- 120.00	100.00	
3.221	3.221	(0.358)	43	2506718			1088.81-1148.81	1118.81	
-----									
14 Isopentane						CAS #: 78-78-4			
4.848	4.848	(0.539)	57	1120615	25.0000	25.058	80.00- 120.00	100.00	
4.848	4.848	(0.539)	43	2262139			171.87- 231.87	201.87	
4.848	4.848	(0.539)	42	1980908			146.77- 206.77	176.77	
-----									
2 Methylcyclohexane						CAS #: 108-87-2			
10.644	10.644	(1.182)	83	2685490	25.0000	26.366	80.00- 120.00	100.00	
10.644	10.644	(1.182)	98	1183998			14.09- 74.09	44.09	
10.644	10.644	(1.182)	55	3086527			84.93- 144.93	114.93	
-----									
179 tert-Butyl Alcohol						CAS #: 75-65-0			
7.570	7.570	(0.841)	59	3082443	25.0000	27.964	80.00- 120.00	100.00	
7.543	7.543	(0.838)	41	2903852			64.21- 124.21	94.21	
7.515	7.515	(0.835)	57	1456367			17.25- 77.25	47.25	
-----									

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 03-Jul-2008 13:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070207.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 5

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 25ppbv -&gt; 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	356533	0.00
51 1,4-Difluorobenze	1324634	794780	1854488	1324634	0.00
72 Chlorobenzene-d5	1242028	745217	1738839	1242028	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.



Report Date: 03-Jul-2008 13:48

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070208.d  
 Lab Smp Id: ICAL Client Smp ID: Level 6  
 Inj Date : 02-JUL-2008 12:20  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 125mL #1612-36  
 Misc Info : 200ppbv -> 50ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:48 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 12:20 Cal File: g070208.d  
 Als bottle: 1 Calibration Sample, Level: 6  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08mdl.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	317124	10.0000			70.00- 130.00	100.00
9.002	9.002	(1.000)	128	239656				0.00- 30.00	75.57
9.002	9.002	(1.000)	49	1027855				0.00- 30.00	324.12
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1253502	10.0000			70.00- 130.00	100.00
10.186	10.186	(1.000)	88	208268				0.00- 46.78	16.61
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1113933	10.0000			70.00- 130.00	100.00
15.319	15.319	(1.000)	82	702621				0.00- 30.00	63.08
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668	(1.074)	65	618330	10.0000	10.158		70.00- 130.00	100.00
9.668	9.668	(1.074)	67	392462				0.00- 30.00	63.47
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1286330	10.0000	9.927		70.00- 130.00	100.00
12.499	12.499	(1.227)	70	148921				0.00- 42.14	11.58

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	829691			34.50- 94.50	64.50	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	664291	10.0000	10.266	70.00- 130.00	100.00	
17.201	17.201	(1.123)	95	972106			113.13- 173.13	146.34	
17.226	17.226	(1.125)	176	643234			66.52- 126.52	96.83	
-----									
4 Propylene CAS #: 115-07-1									
2.101	2.101	(0.233)	41	2092222	50.0000	47.656	70.00- 130.00	100.00(A)	
2.101	2.101	(0.233)	42	1403294			0.00- 30.00	67.07	
2.101	2.101	(0.233)	39	1590911			0.00- 30.00	76.04	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.246	2.246	(0.249)	85	4641866	50.0000	46.902	70.00- 130.00	100.00(A)	
2.246	2.246	(0.249)	87	1484692			1.53- 61.53	31.98	
-----									
7 Freon 114 CAS #: 76-14-2									
2.752	2.752	(0.306)	135	2089978	50.0000	41.890	70.00- 130.00	100.00(A)	
2.752	2.752	(0.306)	137	700460			0.00- 30.00	33.52	
2.752	2.752	(0.306)	85	3502730			0.00- 30.00	167.60	
-----									
8 Chloromethane CAS #: 74-87-3									
2.848	2.848	(0.316)	50	3577339	50.0000	52.980	70.00- 130.00	100.00(A)	
2.848	2.848	(0.316)	52	948589			0.00- 30.00	26.52	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.291	3.291	(0.366)	62	1766244	50.0000	48.162	70.00- 130.00	100.00(A)	
3.291	3.291	(0.366)	64	565012			0.00- 59.65	31.99	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.412	3.412	(0.379)	54	1919109	50.0000	48.245	70.00- 130.00	100.00(A)	
3.412	3.412	(0.379)	39	2407962			0.00- 30.00	125.47	
-----									
11 Bromomethane CAS #: 74-83-9									
4.351	4.351	(0.483)	94	846143	50.0000	46.922	70.00- 130.00	100.00(A)	
4.351	4.351	(0.483)	96	796211			64.87- 124.87	94.10	
-----									
13 Chloroethane CAS #: 75-00-3									
4.724	4.724	(0.525)	64	712398	50.0000	52.021	70.00- 130.00	100.00(A)	
4.724	4.724	(0.525)	49	318202			0.00- 30.00	44.67	
4.724	4.724	(0.525)	66	213330			0.00- 30.00	29.95	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	5532629	50.0000	46.365	70.00- 130.00	100.00(A)	
5.304	5.304	(0.589)	103	3627614			33.99- 93.99	65.57	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
17 Ethanol						CAS #: 64-17-5			
6.198	6.198	(0.688)	45	1102320	50.0000	49.710	70.00- 130.00	100.00(A)	
6.198	6.198	(0.688)	43	245834			0.00- 30.00	22.30	
6.198	6.198	(0.688)	46	416813			0.00- 30.00	37.81	
-----									
19 Freon 113						CAS #: 76-13-1			
6.390	6.390	(0.710)	151	1781989	50.0000	40.015	70.00- 130.00	100.00(A)	
6.390	6.390	(0.710)	153	1144161			31.73- 91.73	64.21	
6.390	6.390	(0.710)	101	2554076			0.00- 30.00	143.33	
-----									
18 1,1-Dichloroethene						CAS #: 75-35-4			
6.335	6.335	(0.704)	98	845421	50.0000	44.397	70.00- 130.00	100.00(A)	
6.335	6.335	(0.704)	61	3840555			0.00- 30.00	454.28	
6.335	6.335	(0.704)	96	1339985			0.00- 30.00	158.50	
-----									
21 Acetone						CAS #: 67-64-1			
6.637	6.637	(0.737)	43	5488433	50.0000	46.283	70.00- 130.00	100.00(A)	
6.637	6.637	(0.737)	58	1082951			0.00- 30.00	19.73	
-----									
24 2-Propanol						CAS #: 67-63-0			
7.021	7.021	(0.780)	45	5601641	50.0000	47.136	70.00- 130.00	100.00(A)	
7.021	7.021	(0.780)	43	1123154			0.00- 30.00	20.05	
7.021	7.021	(0.780)	59	155076			0.00- 30.00	2.77	
-----									
20 Carbon Disulfide						CAS #: 75-15-0			
6.500	6.500	(0.722)	76	4340642	50.0000	43.405	70.00- 130.00	100.00(A)	
-----									
28 Methylene Chloride						CAS #: 75-09-2			
7.213	7.213	(0.801)	84	1447058	50.0000	53.116	70.00- 130.00	100.00(A)	
7.213	7.213	(0.801)	49	3546125			297.52- 357.52	245.06	
7.213	7.213	(0.801)	51	1026325			0.00- 30.00	70.92	
-----									
29 MTBE						CAS #: 1634-04-4			
7.515	7.515	(0.835)	73	4365003	50.0000	41.109	70.00- 130.00	100.00(A)	
7.543	7.543	(0.838)	57	1863755			0.00- 30.00	42.70	
7.543	7.543	(0.838)	41	3753401			0.00- 30.00	85.99	
-----									
30 trans-1,2-Dichloroethene						CAS #: 156-60-5			
7.515	7.515	(0.835)	98	1208047	50.0000	47.188	70.00- 130.00	100.00(A)	
7.515	7.515	(0.835)	61	4050897			0.00- 30.00	335.33	
7.515	7.515	(0.835)	96	1888766			0.00- 30.00	156.35	
-----									
32 Hexane						CAS #: 110-54-3			
7.790	7.790	(0.865)	57	4659696	50.0000	51.320	70.00- 130.00	100.00(A)	
7.790	7.790	(0.865)	43	4112791			0.00- 30.00	88.26	
7.790	7.790	(0.865)	86	494807			0.00- 30.00	10.62	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
33	1,1-Dichloroethane				CAS #: 75-34-3				
8.092	8.092	(0.899)	63	4372960	50.0000	46.947	70.00- 130.00	100.00(A)	
8.092	8.092	(0.899)	65	1318240			0.00- 59.84	30.15	
-----									
37	2-Butanone				CAS #: 78-93-3				
8.792	8.792	(0.977)	72	1112453	50.0000	48.824	70.00- 130.00	100.00(A)	
8.792	8.792	(0.977)	43	8132277			672.66- 732.66	731.02	
8.792	8.792	(0.977)	57	485715			0.00- 30.00	43.66	
-----									
36	cis-1,2-Dichloroethene				CAS #: 156-59-2				
8.748	8.748	(0.972)	98	1299914	50.0000	47.977	70.00- 130.00	100.00(A)	
8.748	8.748	(0.972)	61	3668328			241.26- 301.26	282.20	
8.748	8.748	(0.972)	96	2025914			128.30- 188.30	155.85	
-----									
38	Tetrahydrofuran				CAS #: 109-99-9				
9.002	9.002	(1.000)	42	4560269	50.0000	47.022	70.00- 130.00	100.00(A)	
9.002	9.002	(1.000)	71	951874			0.00- 30.00	20.87	
9.002	9.002	(1.000)	72	1033105			0.00- 30.00	22.65	
-----									
40	Chloroform				CAS #: 67-66-3				
9.099	9.099	(1.011)	83	4366970	50.0000	45.349	70.00- 130.00	100.00(A)	
9.099	9.099	(1.011)	85	2782837			33.23- 93.23	63.72	
-----									
42	1,1,1-Trichloroethane				CAS #: 71-55-6				
9.229	9.229	(1.025)	97	4674314	50.0000	47.278	70.00- 130.00	100.00(A)	
9.229	9.229	(1.025)	99	2984878			33.51- 93.51	63.86	
-----									
41	Cyclohexane				CAS #: 110-82-7				
9.197	9.197	(1.022)	84	3123426	50.0000	47.838	70.00- 130.00	100.00(A)	
9.197	9.197	(1.022)	56	5573864			0.00- 30.00	178.45	
9.197	9.197	(1.022)	41	4032544			0.00- 30.00	129.11	
-----									
44	Carbon Tetrachloride				CAS #: 56-23-5				
9.359	9.359	(1.040)	119	4620134	50.0000	51.185	70.00- 130.00	100.00(A)	
9.359	9.359	(1.040)	117	4810954			73.88- 133.88	104.13	
-----									
46	Benzene				CAS #: 71-43-2				
9.639	9.639	(0.946)	78	6479594	50.0000	44.832	70.00- 130.00	100.00(A)	
9.639	9.639	(0.946)	77	1485240			0.00- 30.00	22.92	
-----									
48	1,2-Dichloroethane				CAS #: 107-06-2				
9.755	9.755	(0.958)	62	4132384	50.0000	46.694	70.00- 130.00	100.00(A)	
9.755	9.755	(0.958)	64	1278053			0.00- 30.00	30.93	
-----									
49	Heptane				CAS #: 142-82-5				
9.872	9.872	(0.969)	43	8019546	50.0000	51.802	70.00- 130.00	100.00(A)	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
49 Heptane (continued)									
9.872	9.872	(0.969)	57	3126708			0.00- 30.00	38.99	
9.872	9.872	(0.969)	100	681431			0.00- 30.00	8.50	
-----									
52 Trichloroethene						CAS #: 79-01-6			
10.475	10.475	(1.028)	130	2675381	50.0000	45.165	70.00- 130.00	100.00(A)	
10.475	10.475	(1.028)	95	2881949			0.00- 30.00	107.72	
10.475	10.475	(1.028)	97	1850499			0.00- 30.00	69.17	
-----									
53 1,2-Dichloropropane						CAS #: 78-87-5			
10.861	10.861	(1.066)	63	3047164	50.0000	47.519	70.00- 130.00	100.00(A)	
10.861	10.861	(1.066)	62	2158424			40.07- 100.07	70.83	
10.861	10.861	(1.066)	41	2762136			61.40- 121.40	90.65	
-----									
54 1,4-Dioxane						CAS #: 123-91-1			
11.029	11.029	(1.083)	88	1609539	50.0000	49.149	70.00- 130.00	100.00(A)	
11.005	11.005	(1.080)	58	1562239			64.32- 124.32	97.06	
11.005	11.005	(1.080)	57	525524			0.00- 30.00	32.65	
-----									
55 Bromodichloromethane						CAS #: 75-27-4			
11.270	11.270	(1.106)	83	5009098	50.0000	48.188	70.00- 130.00	100.00(A)	
11.270	11.270	(1.106)	85	3126948			31.92- 91.92	62.43	
-----									
56 cis-1,3-Dichloropropene						CAS #: 10061-01-5			
12.090	12.090	(1.187)	75	3934825	50.0000	51.365	70.00- 130.00	100.00(A)	
12.090	12.090	(1.187)	77	1240117			1.56- 61.56	31.52	
12.090	12.090	(1.187)	39	3609749			60.10- 120.10	91.74	
-----									
58 4-Methyl-2-pentanone						CAS #: 108-10-1			
12.379	12.379	(1.215)	43	10476320	50.0000	51.953	70.00- 130.00	100.00(A)	
12.379	12.379	(1.215)	58	2920433			0.00- 30.00	27.88	
12.379	12.379	(1.215)	85	932096			0.00- 30.00	8.90	
-----									
60 Toluene						CAS #: 108-88-3			
12.644	12.644	(1.241)	91	8037838	50.0000	47.344	70.00- 130.00	100.00(A)	
12.644	12.644	(1.241)	92	4705127			28.58- 88.58	58.54	
-----									
61 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.308	13.308	(0.869)	75	4249575	50.0000	52.912	70.00- 130.00	100.00(A)	
13.308	13.308	(0.869)	77	1341531			1.05- 61.05	31.57	
13.308	13.308	(0.869)	39	3680624			54.43- 114.43	86.61	
-----									
63 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.665	13.665	(0.892)	97	2816756	50.0000	47.949	70.00- 130.00	100.00(A)	
13.665	13.665	(0.892)	99	1714039			32.27- 92.27	60.85	
13.665	13.665	(0.892)	83	2514038			59.54- 119.54	89.25	
-----									



AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
64 Tetrachloroethene						CAS #: 127-18-4			
13.747	13.747	(0.897)	166	3547472	50.0000	46.852	70.00- 130.00	100.00(A)	
13.747	13.747	(0.897)	129	2785912			46.83- 106.83	78.53	
13.747	13.747	(0.897)	131	2670107			42.93- 102.93	75.27	
-----									
67 2-Hexanone						CAS #: 591-78-6			
14.132	14.132	(0.922)	58	4125516	50.0000	52.809	70.00- 130.00	100.00(A)	
14.132	14.132	(0.922)	43	10609274			227.44- 287.44	257.16	
14.132	14.132	(0.922)	100	574849			0.00- 30.00	13.93	
-----									
68 Dibromochloromethane						CAS #: 124-48-1			
14.352	14.352	(0.937)	129	4715612	50.0000	50.091	70.00- 130.00	100.00(A)	
14.352	14.352	(0.937)	208	250024			0.00- 30.00	5.30	
-----									
69 1,2-Dibromoethane						CAS #: 106-93-4			
14.517	14.517	(0.948)	107	1216166	50.0000	46.134	70.00- 130.00	100.00(A)	
14.517	14.517	(0.948)	109	1116959			64.21- 124.21	91.84	
-----									
73 Chlorobenzene						CAS #: 108-90-7			
15.370	15.370	(1.003)	112	6935283	50.0000	46.662	70.00- 130.00	100.00(A)	
15.370	15.370	(1.003)	114	2222761			1.79- 61.79	32.05	
15.370	15.370	(1.003)	77	4524633			33.30- 93.30	65.24	
-----									
74 Ethyl Benzene						CAS #: 100-41-4			
15.525	15.525	(1.013)	106	3772717	50.0000	48.945	70.00- 130.00	100.00(A)	
15.525	15.525	(1.013)	91	12178830			0.00- 30.00	322.81	
-----									
75 m,p-Xylene						CAS #: 108-38-3			
15.731	15.731	(1.027)	106	4725643	50.0000	49.939	70.00- 130.00	100.00	
15.731	15.731	(1.027)	91	9856342			0.00- 30.00	208.57	
-----									
77 o-Xylene						CAS #: 95-47-6			
16.376	16.376	(1.069)	106	4431850	50.0000	49.864	70.00- 130.00	100.00(A)	
16.376	16.376	(1.069)	91	9834210			186.60- 246.60	221.90	
-----									
78 Styrene						CAS #: 100-42-5			
16.427	16.427	(1.072)	104	7298745	50.0000	53.113	70.00- 130.00	100.00(A)	
16.401	16.401	(1.071)	78	4043454			24.82- 84.82	55.40	
-----									
79 Bromoform						CAS #: 75-25-2			
16.711	16.711	(1.091)	173	4515498	50.0000	50.480	70.00- 130.00	100.00(A)	
16.711	16.711	(1.091)	171	2315275			0.00- 30.00	51.27	
-----									
80 Cumene						CAS #: 98-82-8			
16.917	16.917	(1.104)	105	13137564	50.0000	52.103	70.00- 130.00	100.00(A)	
16.917	16.917	(1.104)	120	3339205			0.00- 56.16	25.42	
-----									

Report Date: 03-Jul-2008 13:48

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
82	1,1,2,2-Tetrachloroethane					CAS #: 79-34-5			
17.484	17.484	(1.141)	83	7313951	50.0000	47.380	70.00- 130.00	100.00(A)	
17.484	17.484	(1.141)	85	4589198			33.53- 93.53	62.75	
-----									
83	Propylbenzene					CAS #: 103-65-1			
17.536	17.536	(1.145)	91	16826230	50.0000	50.434	70.00- 130.00	100.00(A)	
17.536	17.536	(1.145)	120	3611120			0.00- 30.00	21.46	
-----									
84	4-Ethyltoluene					CAS #: 622-96-8			
17.716	17.716	(1.157)	105	14320659	50.0000	52.340	70.00- 130.00	100.00(A)	
17.716	17.716	(1.157)	120	4125836			0.00- 59.12	28.81	
-----									
85	1,3,5-Trimethylbenzene					CAS #: 108-67-8			
17.820	17.820	(1.163)	105	11720026	50.0000	50.798	70.00- 130.00	100.00(A)	
17.820	17.820	(1.163)	120	5445545			16.79- 76.79	46.46	
-----									
87	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
18.413	18.413	(1.202)	105	11629290	50.0000	53.692	70.00- 130.00	100.00(A)	
18.413	18.413	(1.202)	120	5086485			13.82- 73.82	43.74	
-----									
89	1,3-Dichlorobenzene					CAS #: 541-73-1			
18.929	18.929	(1.236)	146	7101777	50.0000	48.124	70.00- 130.00	100.00(A)	
18.929	18.929	(1.236)	148	4554341			0.00- 30.00	64.13	
18.929	18.929	(1.236)	111	3141198			0.00- 30.00	44.23	
-----									
90	1,4-Dichlorobenzene					CAS #: 106-46-7			
19.083	19.083	(1.246)	146	7302948	50.0000	47.767	70.00- 130.00	100.00(A)	
19.083	19.083	(1.246)	148	4613336			0.00- 30.00	63.17	
19.083	19.083	(1.246)	111	3093379			0.00- 30.00	42.36	
-----									
91	alpha-chlorotoluene					CAS #: 100-44-7			
19.316	19.316	(1.261)	91	11225779	50.0000	58.486	70.00- 130.00	100.00(A)	
19.316	19.316	(1.261)	126	2094151			0.00- 30.00	18.65	
-----									
94	1,2-Dichlorobenzene					CAS #: 95-50-1			
19.625	19.625	(1.281)	146	6743453	50.0000	47.526	70.00- 130.00	100.00(A)	
19.625	19.625	(1.281)	148	4277543			32.78- 92.78	63.43	
19.625	19.625	(1.281)	111	3085309			14.53- 74.53	45.75	
-----									
96	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
21.430	21.430	(1.399)	180	5763593	50.0000	51.347	70.00- 130.00	100.00(A)	
21.430	21.430	(1.399)	182	5512402			65.13- 125.13	95.64	
-----									
97	Hexachlorobutadiene					CAS #: 87-68-3			
21.559	21.559	(1.407)	225	4649778	50.0000	48.240	70.00- 130.00	100.00(A)	
21.559	21.559	(1.407)	223	2923058			0.00- 30.00	62.86	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
98 Naphthalene						CAS #: 91-20-3			
21.688	21.688	(1.416)	128	12501282	50.0000	55.069	70.00- 130.00	100.00(A)	
21.688	21.688	(1.416)	127	1536432			0.00- 30.00	12.29	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	858598	50.0000	58.280	70.00- 130.00	100.00(A)	
6.994	6.994	(0.777)	41	5378031			0.00- 30.00	626.37	
-----									
45 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.639	9.639	(1.071)	56	5070184	50.0000	49.696	70.00- 130.00	100.00(A)	
9.639	9.639	(1.071)	99	568577			0.00- 30.00	11.21	
9.639	9.639	(1.071)	41	5472238			0.00- 30.00	107.93	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	10332337	50.0000	53.787	70.00- 130.00	100.00(A)	
8.174	8.174	(0.908)	42	861671			0.00- 30.00	8.34	
8.174	8.174	(0.908)	86	484070			0.00- 30.00	4.69	
-----									
183 Butane						CAS #: 106-97-8			
3.221	3.221	(0.358)	58	386532	50.0000	49.079	70.00- 130.00	100.00(A)	
3.221	3.221	(0.358)	43	4271146			0.00- 30.00	1104.99	
-----									
14 Isopentane						CAS #: 78-78-4			
4.827	4.827	(0.536)	57	2009650	50.0000	50.522	70.00- 130.00	100.00(A)	
4.827	4.827	(0.536)	43	4008252			0.00- 30.00	199.45	
4.827	4.827	(0.536)	42	3460992			0.00- 30.00	172.22	
-----									
2 Methylcyclohexane						CAS #: 108-87-2			
10.644	10.644	(1.182)	83	4377404	50.0000	48.318	70.00- 130.00	100.00(A)	
10.644	10.644	(1.182)	98	1934147			0.00- 30.00	44.18	
10.644	10.644	(1.182)	55	5238454			0.00- 30.00	119.67	
-----									
179 tert-Butyl Alcohol						CAS #: 75-65-0			
7.543	7.543	(0.838)	59	4396946	50.0000	44.846	70.00- 130.00	100.00(A)	
7.543	7.543	(0.838)	41	3753401			0.00- 30.00	85.36	
7.543	7.543	(0.838)	57	1863755			0.00- 30.00	42.39	
-----									

QC Flag Legend

A - Target compound detected but, quantitated amount exceeded maximum amount.

Report Date: 03-Jul-2008 13:48

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070208.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 6

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 200ppbv -&gt; 50ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	317124	-11.05
51 1,4-Difluorobenze	1324634	794780	1854488	1253502	-5.37
72 Chlorobenzene-d5	1242028	745217	1738839	1113933	-10.31

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 02-JUL-2008 12:20

Client ID: Level 6


Instrument: msdg.i

Sample Info: 125mL #1612-36

Operator: lmr

Column phase: RTx-624

Column diameter: 0.32

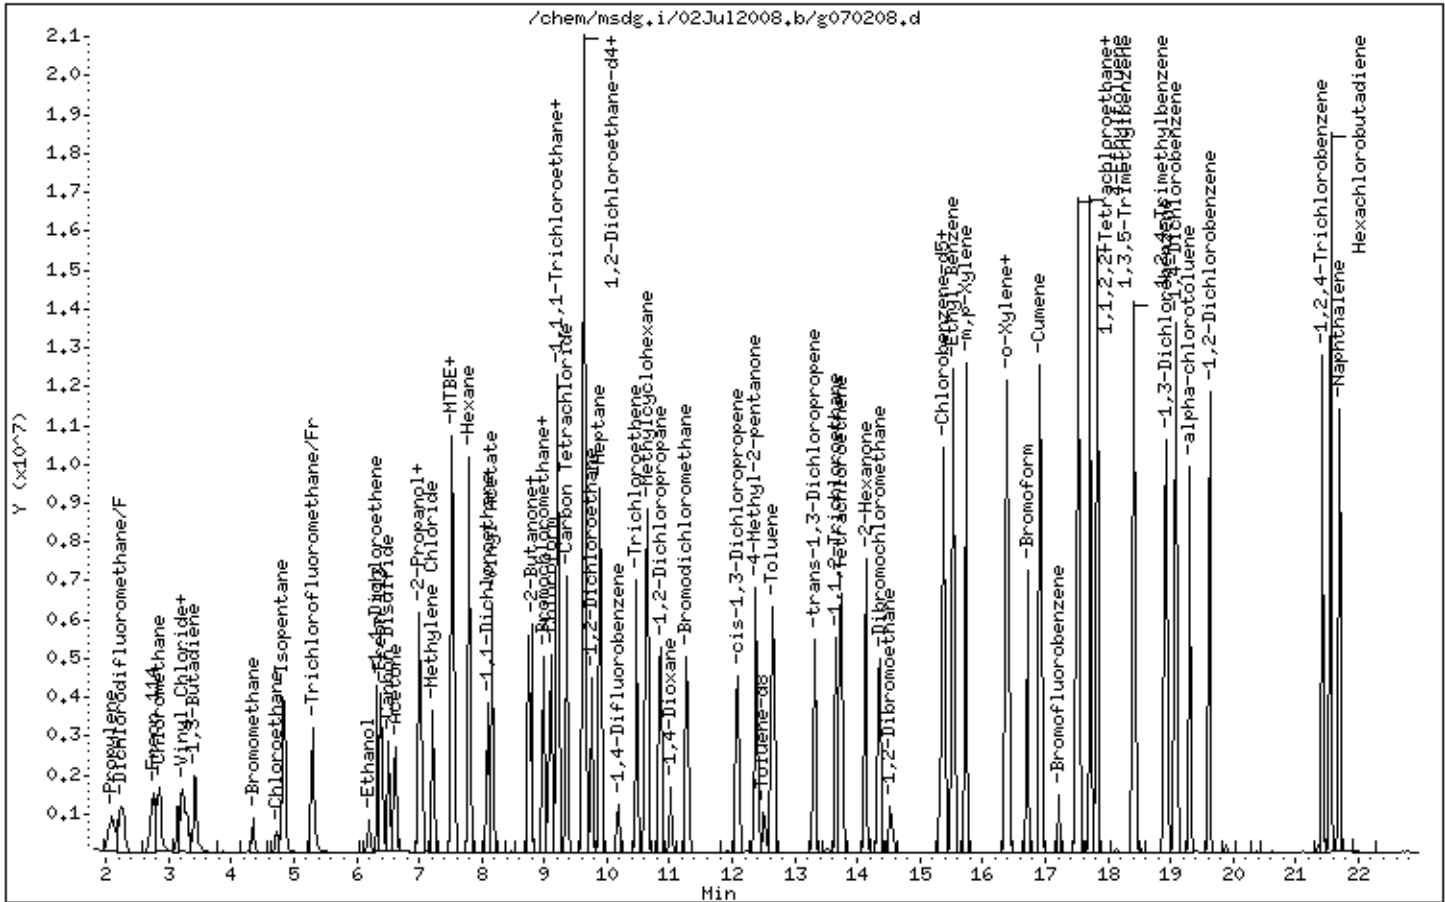

Report Date: 03-Jul-2008 13:49

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/02Jul2008.b/g070209.d  
 Lab Smp Id: ICAL Client Smp ID: Level 7  
 Inj Date : 02-JUL-2008 13:24  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 250mL #1612-36;ICAL;Level 7  
 Misc Info : 200ppbv -> 100ppbv  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/t14q702a.m  
 Meth Date : 03-Jul-2008 13:48 cleonard Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1 Calibration Sample, Level: 7  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	(PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	344490	10.0000			70.00- 130.00	100.00
9.002	9.002	(1.000)	128	273362				0.00- 30.00	79.35
9.002	9.002	(1.000)	49	958707				0.00- 30.00	278.30
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1343190	10.0000			70.00- 130.00	100.00
10.186	10.186	(1.000)	88	223120				0.00- 46.78	16.61
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1247974	10.0000			70.00- 130.00	100.00
15.319	15.319	(1.000)	82	790764				0.00- 30.00	63.36
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.667	9.667	(1.074)	65	721633	10.0000	10.914		70.00- 130.00	100.00
9.667	9.667	(1.074)	67	533355				0.00- 30.00	73.91
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.523	12.523	(1.229)	98	1423542	10.0000	10.252		70.00- 130.00	100.00
12.523	12.523	(1.229)	70	171484				0.00- 42.14	12.05

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.523	12.523	(1.229)	100	929285			34.50- 94.50	65.28	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	711759	10.0000	9.818	70.00- 130.00	100.00	
17.226	17.226	(1.125)	95	1058868			113.13- 173.13	148.77	
17.226	17.226	(1.125)	176	689615			66.52- 126.52	96.89	
-----									
4 Propylene CAS #: 115-07-1									
2.101	2.101	(0.233)	41	4649990	100.000	97.501	70.00- 130.00	100.00(AM)	
2.101	2.101	(0.233)	42	2260993			0.00- 30.00	48.62	
2.101	2.101	(0.233)	39	2515438			0.00- 30.00	54.10	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.270	2.270	(0.252)	85	9971089	100.000	92.747	70.00- 130.00	100.00(A)	
2.270	2.270	(0.252)	87	3180993			1.53- 61.53	31.90	
-----									
7 Freon 114 CAS #: 76-14-2									
2.752	2.752	(0.306)	135	4649411	100.000	85.788	70.00- 130.00	100.00(A)	
2.752	2.752	(0.306)	137	1505180			0.00- 30.00	32.37	
2.752	2.752	(0.306)	85	7660752			0.00- 30.00	164.77	
-----									
8 Chloromethane CAS #: 74-87-3									
2.872	2.872	(0.319)	50	6973408	100.000	95.070	70.00- 130.00	100.00(A)	
2.872	2.872	(0.319)	52	1882892			0.00- 30.00	27.00	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.308	3.308	(0.367)	62	3905923	100.000	98.046	70.00- 130.00	100.00(A)	
3.308	3.308	(0.367)	64	1140600			0.00- 59.65	29.20	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.430	3.430	(0.381)	54	4542467	100.000	105.12	70.00- 130.00	100.00(A)	
3.430	3.430	(0.381)	39	5417773			0.00- 30.00	119.27	
-----									
11 Bromomethane CAS #: 74-83-9									
4.350	4.350	(0.483)	94	2249063	100.000	114.81	70.00- 130.00	100.00(A)	
4.350	4.350	(0.483)	96	2111798			64.87- 124.87	93.90	
-----									
13 Chloroethane CAS #: 75-00-3									
4.723	4.723	(0.525)	64	1589823	100.000	106.87	70.00- 130.00	100.00(A)	
4.723	4.723	(0.525)	49	730940			0.00- 30.00	45.98	
4.723	4.723	(0.525)	66	465151			0.00- 30.00	29.26	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	11951577	100.000	92.201	70.00- 130.00	100.00(A)	
5.304	5.304	(0.589)	103	7699609			33.99- 93.99	64.42	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
17 Ethanol						CAS #: 64-17-5			
6.225	6.225	(0.692)	45	2399107	100.000	99.594	70.00- 130.00	100.00(A)	
6.225	6.225	(0.692)	43	501122			0.00- 30.00	20.89	
6.225	6.225	(0.692)	46	910579			0.00- 30.00	37.95	
-----									
19 Freon 113						CAS #: 76-13-1			
6.390	6.390	(0.710)	151	3693209	100.000	76.343	70.00- 130.00	100.00(A)	
6.390	6.390	(0.710)	153	2310514			31.73- 91.73	62.56	
6.390	6.390	(0.710)	101	5239328			0.00- 30.00	141.86	
-----									
18 1,1-Dichloroethene						CAS #: 75-35-4			
6.335	6.335	(0.704)	98	1810461	100.000	87.522	70.00- 130.00	100.00(A)	
6.335	6.335	(0.704)	61	8218494			0.00- 30.00	453.94	
6.335	6.335	(0.704)	96	2820279			0.00- 30.00	155.78	
-----									
21 Acetone						CAS #: 67-64-1			
6.637	6.637	(0.737)	43	12100592	100.000	93.936	70.00- 130.00	100.00(A)	
6.637	6.637	(0.737)	58	2478666			0.00- 30.00	20.48	
-----									
24 2-Propanol						CAS #: 67-63-0			
7.049	7.049	(0.783)	45	13311865	100.000	103.12	70.00- 130.00	100.00(A)	
7.049	7.049	(0.783)	43	2718147			0.00- 30.00	20.42	
7.049	7.049	(0.783)	59	367159			0.00- 30.00	2.76	
-----									
20 Carbon Disulfide						CAS #: 75-15-0			
6.499	6.499	(0.722)	76	9468135	100.000	87.157	70.00- 130.00	100.00(A)	
-----									
28 Methylene Chloride						CAS #: 75-09-2			
7.213	7.213	(0.801)	84	2181655	100.000	73.719	70.00- 130.00	100.00(A)	
7.213	7.213	(0.801)	49	7072965			297.52- 357.52	324.20	
7.213	7.213	(0.801)	51	2057635			0.00- 30.00	94.32	
-----									
29 MTBE						CAS #: 1634-04-4			
7.543	7.543	(0.838)	73	10717897	100.000	92.922	70.00- 130.00	100.00(A)	
7.543	7.543	(0.838)	57	5405228			0.00- 30.00	50.43	
7.543	7.543	(0.838)	41	8722012			0.00- 30.00	81.38	
-----									
30 trans-1,2-Dichloroethene						CAS #: 156-60-5			
7.515	7.515	(0.835)	98	1795708	100.000	64.570	70.00- 130.00	100.00(A)	
7.515	7.515	(0.835)	61	7856845			0.00- 30.00	437.53	
7.515	7.515	(0.835)	96	2841089			0.00- 30.00	158.22	
-----									
32 Hexane						CAS #: 110-54-3			
7.790	7.790	(0.865)	57	9622932	100.000	97.564	70.00- 130.00	100.00(A)	
7.790	7.790	(0.865)	43	8612017			0.00- 30.00	89.49	
7.790	7.790	(0.865)	86	988072			0.00- 30.00	10.27	
-----									



Report Date: 03-Jul-2008 13:49

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
33	1,1-Dichloroethane				CAS #:		75-34-3		
8.092	8.092	(0.899)	63	9449464	100.000	93.389	70.00-	130.00	100.00(A)
8.092	8.092	(0.899)	65	2818001			0.00-	59.84	29.82
-----									
37	2-Butanone				CAS #:		78-93-3		
8.792	8.792	(0.977)	72	2323826	100.000	93.888	70.00-	130.00	100.00(A)
8.792	8.792	(0.977)	43	16072576			672.66-	732.66	691.64
8.792	8.792	(0.977)	57	1071037			0.00-	30.00	46.09
-----									
36	cis-1,2-Dichloroethene				CAS #:		156-59-2		
8.747	8.747	(0.972)	98	2707099	100.000	91.976	70.00-	130.00	100.00(A)
8.747	8.747	(0.972)	61	8095512			241.26-	301.26	299.05
8.747	8.747	(0.972)	96	4224961			128.30-	188.30	156.07
-----									
38	Tetrahydrofuran				CAS #:		109-99-9		
9.002	9.002	(1.000)	42	11352699	100.000	107.76	70.00-	130.00	100.00(A)
9.002	9.002	(1.000)	71	2261840			0.00-	30.00	19.92
9.002	9.002	(1.000)	72	2402595			0.00-	30.00	21.16
-----									
40	Chloroform				CAS #:		67-66-3		
9.099	9.099	(1.011)	83	9400215	100.000	89.863	70.00-	130.00	100.00(A)
9.099	9.099	(1.011)	85	5880684			33.23-	93.23	62.56
-----									
42	1,1,1-Trichloroethane				CAS #:		71-55-6		
9.229	9.229	(1.025)	97	10119211	100.000	94.219	70.00-	130.00	100.00(A)
9.229	9.229	(1.025)	99	6402451			33.51-	93.51	63.27
-----									
41	Cyclohexane				CAS #:		110-82-7		
9.197	9.197	(1.022)	84	6583954	100.000	92.828	70.00-	130.00	100.00(A)
9.197	9.197	(1.022)	56	12799576			0.00-	30.00	194.41
9.197	9.197	(1.022)	41	9191619			0.00-	30.00	139.61
-----									
44	Carbon Tetrachloride				CAS #:		56-23-5		
9.359	9.359	(1.040)	119	9864181	100.000	100.60	70.00-	130.00	100.00(A)
9.359	9.359	(1.040)	117	10303454			73.88-	133.88	104.45
-----									
46	Benzene				CAS #:		71-43-2		
9.638	9.638	(0.946)	78	12783471	100.000	82.543	70.00-	130.00	100.00(A)
9.638	9.638	(0.946)	77	2961816			0.00-	30.00	23.17
-----									
48	1,2-Dichloroethane				CAS #:		107-06-2		
9.755	9.755	(0.958)	62	9035260	100.000	95.277	70.00-	130.00	100.00(A)
9.755	9.755	(0.958)	64	2725992			0.00-	30.00	30.17
-----									
49	Heptane				CAS #:		142-82-5		
9.871	9.871	(0.969)	43	16749227	100.000	100.97	70.00-	130.00	100.00(A)

Report Date: 03-Jul-2008 13:49

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
49 Heptane (continued)									
9.871	9.871	(0.969)	57	6558697			0.00- 30.00	39.16	
9.901	9.901	(0.972)	100	1316196			0.00- 30.00	7.86	
-----									
52 Trichloroethene					CAS #: 79-01-6				
10.475	10.475	(1.028)	130	5271227	100.000	83.046	70.00- 130.00	100.00(A)	
10.475	10.475	(1.028)	95	5846270			0.00- 30.00	110.91	
10.475	10.475	(1.028)	97	3800269			0.00- 30.00	72.09	
-----									
53 1,2-Dichloropropane					CAS #: 78-87-5				
10.860	10.860	(1.066)	63	6518319	100.000	94.863	70.00- 130.00	100.00(A)	
10.860	10.860	(1.066)	62	4651555			40.07- 100.07	71.36	
10.860	10.860	(1.066)	41	5879424			61.40- 121.40	90.20	
-----									
54 1,4-Dioxane					CAS #: 123-91-1				
11.029	11.029	(1.083)	88	3530588	100.000	100.61	70.00- 130.00	100.00(A)	
11.029	11.029	(1.083)	58	3556856			64.32- 124.32	100.74	
11.029	11.029	(1.083)	57	1187393			0.00- 30.00	33.63	
-----									
55 Bromodichloromethane					CAS #: 75-27-4				
11.270	11.270	(1.106)	83	10678503	100.000	95.868	70.00- 130.00	100.00(A)	
11.270	11.270	(1.106)	85	6647266			31.92- 91.92	62.25	
-----									
56 cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.089	12.089	(1.187)	75	8349589	100.000	101.72	70.00- 130.00	100.00(A)	
12.089	12.089	(1.187)	77	2616724			1.56- 61.56	31.34	
12.089	12.089	(1.187)	39	7851912			60.10- 120.10	94.04	
-----									
58 4-Methyl-2-pentanone					CAS #: 108-10-1				
12.378	12.378	(1.215)	43	23623640	100.000	109.33	70.00- 130.00	100.00(A)	
12.378	12.378	(1.215)	58	6594901			0.00- 30.00	27.92	
12.378	12.378	(1.215)	85	2022756			0.00- 30.00	8.56	
-----									
60 Toluene					CAS #: 108-88-3				
12.644	12.644	(1.241)	91	16764421	100.000	92.150	70.00- 130.00	100.00(A)	
12.644	12.644	(1.241)	92	9795424			28.58- 88.58	58.43	
-----									
61 trans-1,3-Dichloropropene					CAS #: 10061-02-6				
13.308	13.308	(0.869)	75	9310610	100.000	103.48	70.00- 130.00	100.00(A)	
13.308	13.308	(0.869)	77	2898432			1.05- 61.05	31.13	
13.308	13.308	(0.869)	39	8021952			54.43- 114.43	86.16	
-----									
63 1,1,2-Trichloroethane					CAS #: 79-00-5				
13.665	13.665	(0.892)	97	5833395	100.000	88.635	70.00- 130.00	100.00(A)	
13.665	13.665	(0.892)	99	3628195			32.27- 92.27	62.20	
13.665	13.665	(0.892)	83	5308081			59.54- 119.54	90.99	
-----									

Report Date: 03-Jul-2008 13:49

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
64 Tetrachloroethene						CAS #: 127-18-4			
13.747	13.747	(0.897)	166	7107211	100.000	83.784	70.00- 130.00	100.00(A)	
13.747	13.747	(0.897)	129	5583132			46.83- 106.83	78.56	
13.747	13.747	(0.897)	131	5344545			42.93- 102.93	75.20	
-----									
67 2-Hexanone						CAS #: 591-78-6			
14.132	14.132	(0.922)	58	9686458	100.000	110.67	70.00- 130.00	100.00(A)	
14.132	14.132	(0.922)	43	23637592			227.44- 287.44	244.03	
14.132	14.132	(0.922)	100	1260460			0.00- 30.00	13.01	
-----									
68 Dibromochloromethane						CAS #: 124-48-1			
14.352	14.352	(0.937)	129	9878164	100.000	93.660	70.00- 130.00	100.00(A)	
14.352	14.352	(0.937)	208	505889			0.00- 30.00	5.12	
-----									
69 1,2-Dibromoethane						CAS #: 106-93-4			
14.516	14.516	(0.948)	107	1952910	100.000	66.125	70.00- 130.00	100.00(A)	
14.516	14.516	(0.948)	109	1824202			64.21- 124.21	93.41	
-----									
73 Chlorobenzene						CAS #: 108-90-7			
15.370	15.370	(1.003)	112	14298037	100.000	85.868	70.00- 130.00	100.00(A)	
15.370	15.370	(1.003)	114	4564313			1.79- 61.79	31.92	
15.370	15.370	(1.003)	77	9612213			33.30- 93.30	67.23	
-----									
74 Ethyl Benzene						CAS #: 100-41-4			
15.525	15.525	(1.013)	106	7748544	100.000	89.729	70.00- 130.00	100.00(A)	
15.525	15.525	(1.013)	91	23228887			0.00- 30.00	299.78	
-----									
75 m,p-Xylene						CAS #: 108-38-3			
15.731	15.731	(1.027)	106	9686235	100.000	91.366	70.00- 130.00	100.00(A)	
15.731	15.731	(1.027)	91	20768499			0.00- 30.00	214.41	
-----									
77 o-Xylene						CAS #: 95-47-6			
16.375	16.375	(1.069)	106	9245563	100.000	92.851	70.00- 130.00	100.00(A)	
16.375	16.375	(1.069)	91	20752262			186.60- 246.60	224.46	
-----									
78 Styrene						CAS #: 100-42-5			
16.427	16.427	(1.072)	104	15022038	100.000	97.574	70.00- 130.00	100.00(A)	
16.427	16.427	(1.072)	78	8744383			24.82- 84.82	58.21	
-----									
79 Bromoform						CAS #: 75-25-2			
16.711	16.711	(1.091)	173	9234290	100.000	92.145	70.00- 130.00	100.00(A)	
16.711	16.711	(1.091)	171	4755227			0.00- 30.00	51.50	
-----									
80 Cumene						CAS #: 98-82-8			
16.917	16.917	(1.104)	105	26529314	100.000	93.913	70.00- 130.00	100.00(A)	
16.917	16.917	(1.104)	120	6842403			0.00- 56.16	25.79	
-----									

Report Date: 03-Jul-2008 13:49

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
82	1,1,2,2-Tetrachloroethane					CAS #: 79-34-5			
17.484	17.484	(1.141)	83	15142998	100.000	87.561	70.00- 130.00	100.00(A)	
17.510	17.510	(1.143)	85	9442446			33.53- 93.53	62.36	
-----									
83	Propylbenzene					CAS #: 103-65-1			
17.536	17.536	(1.145)	91	24638710	100.000	65.919	70.00- 130.00	100.00(A)	
17.536	17.536	(1.145)	120	7184197			0.00- 30.00	29.16	
-----									
84	4-Ethyltoluene					CAS #: 622-96-8			
17.716	17.716	(1.157)	105	22519053	100.000	73.464	70.00- 130.00	100.00(A)	
17.716	17.716	(1.157)	120	8118582			0.00- 59.12	36.05	
-----									
85	1,3,5-Trimethylbenzene					CAS #: 108-67-8			
17.819	17.819	(1.163)	105	22219639	100.000	85.963	70.00- 130.00	100.00(A)	
17.819	17.819	(1.163)	120	10840999			16.79- 76.79	48.79	
-----									
87	1,2,4-Trimethylbenzene					CAS #: 95-63-6			
18.413	18.413	(1.202)	105	23171149	100.000	95.489	70.00- 130.00	100.00(A)	
18.413	18.413	(1.202)	120	10295106			13.82- 73.82	44.43	
-----									
89	1,3-Dichlorobenzene					CAS #: 541-73-1			
18.929	18.929	(1.236)	146	14501551	100.000	87.713	70.00- 130.00	100.00(A)	
18.929	18.929	(1.236)	148	9163460			0.00- 30.00	63.19	
18.929	18.929	(1.236)	111	6533244			0.00- 30.00	45.05	
-----									
90	1,4-Dichlorobenzene					CAS #: 106-46-7			
19.083	19.083	(1.246)	146	14399422	100.000	84.068	70.00- 130.00	100.00(A)	
19.083	19.083	(1.246)	148	9168470			0.00- 30.00	63.67	
19.083	19.083	(1.246)	111	6377023			0.00- 30.00	44.29	
-----									
91	alpha-chlorotoluene					CAS #: 100-44-7			
19.315	19.315	(1.261)	91	22416470	100.000	104.24	70.00- 130.00	100.00(A)	
19.315	19.315	(1.261)	126	4372977			0.00- 30.00	19.51	
-----									
94	1,2-Dichlorobenzene					CAS #: 95-50-1			
19.625	19.625	(1.281)	146	13473840	100.000	84.761	70.00- 130.00	100.00(A)	
19.625	19.625	(1.281)	148	8509423			32.78- 92.78	63.16	
19.625	19.625	(1.281)	111	6288910			14.53- 74.53	46.67	
-----									
96	1,2,4-Trichlorobenzene					CAS #: 120-82-1			
21.430	21.430	(1.399)	180	10931921	100.000	86.931	70.00- 130.00	100.00(A)	
21.430	21.430	(1.399)	182	10393515			65.13- 125.13	95.07	
-----									
97	Hexachlorobutadiene					CAS #: 87-68-3			
21.559	21.559	(1.407)	225	8668903	100.000	80.277	70.00- 130.00	100.00(A)	
21.559	21.559	(1.407)	223	5478516			0.00- 30.00	63.20	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
98 Naphthalene						CAS #: 91-20-3			
21.688	21.688	(1.416)	128	24114936	100.000	94.818	70.00- 130.00	100.00(A)	
21.688	21.688	(1.416)	127	3055705			0.00- 30.00	12.67	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	1408976	100.000	88.041	70.00- 130.00	100.00(A)	
6.994	6.994	(0.777)	41	10739749			0.00- 30.00	762.24	
-----									
45 2,2,4-Trimethylpentane						CAS #: 540-84-1			
9.638	9.638	(1.071)	56	11043811	100.000	99.649	70.00- 130.00	100.00(A)	
9.638	9.638	(1.071)	99	1127131			0.00- 30.00	10.21	
9.638	9.638	(1.071)	41	11831624			0.00- 30.00	107.13	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	18951871	100.000	90.821	70.00- 130.00	100.00(A)	
8.174	8.174	(0.908)	42	1710179			0.00- 30.00	9.02	
8.174	8.174	(0.908)	86	960938			0.00- 30.00	5.07	
-----									
183 Butane						CAS #: 106-97-8			
3.221	3.221	(0.358)	58	888058	100.000	103.80	70.00- 130.00	100.00(A)	
3.221	3.221	(0.358)	43	9454557			0.00- 30.00	1064.63	
-----									
14 Isopentane						CAS #: 78-78-4			
4.848	4.848	(0.539)	57	4361572	100.000	100.94	70.00- 130.00	100.00(A)	
4.848	4.848	(0.539)	43	8490613			0.00- 30.00	194.67	
4.848	4.848	(0.539)	42	7310404			0.00- 30.00	167.61	
-----									
2 Methylcyclohexane						CAS #: 108-87-2			
10.644	10.644	(1.182)	83	9216867	100.000	93.655	70.00- 130.00	100.00(A)	
10.644	10.644	(1.182)	98	4012850			0.00- 30.00	43.54	
10.644	10.644	(1.182)	55	11814976			0.00- 30.00	128.19	
-----									
179 tert-Butyl Alcohol						CAS #: 75-65-0			
7.570	7.570	(0.841)	59	12301489	100.000	115.50	70.00- 130.00	100.00(A)	
7.543	7.543	(0.838)	41	8722012			0.00- 30.00	70.90	
7.543	7.543	(0.838)	57	5405228			0.00- 30.00	43.94	
-----									

QC Flag Legend

- A - Target compound detected but, quantitated amount exceeded maximum amount.
- M - Compound response manually integrated.

Report Date: 03-Jul-2008 13:49

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 02-JUL-2008

Lab File ID: g070209.d

Calibration Time: 11:32

Lab Smp Id: ICAL

Client Smp ID: Level 7

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /chem/msdg.i/02Jul2008.b/t14q702a.m

Misc Info: 200ppbv -&gt; 100ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	356533	213920	499146	344490	-3.38
51 1,4-Difluorobenze	1324634	794780	1854488	1343190	1.40
72 Chlorobenzene-d5	1242028	745217	1738839	1247974	0.48

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 02-JUL-2008 13:24

Client ID: Level 7


Instrument: msdg.i

Sample Info: 250mL #1612-36;ICAL;Level 7

Operator: lmr

Column phase: RTX-624

Column diameter: 0.32

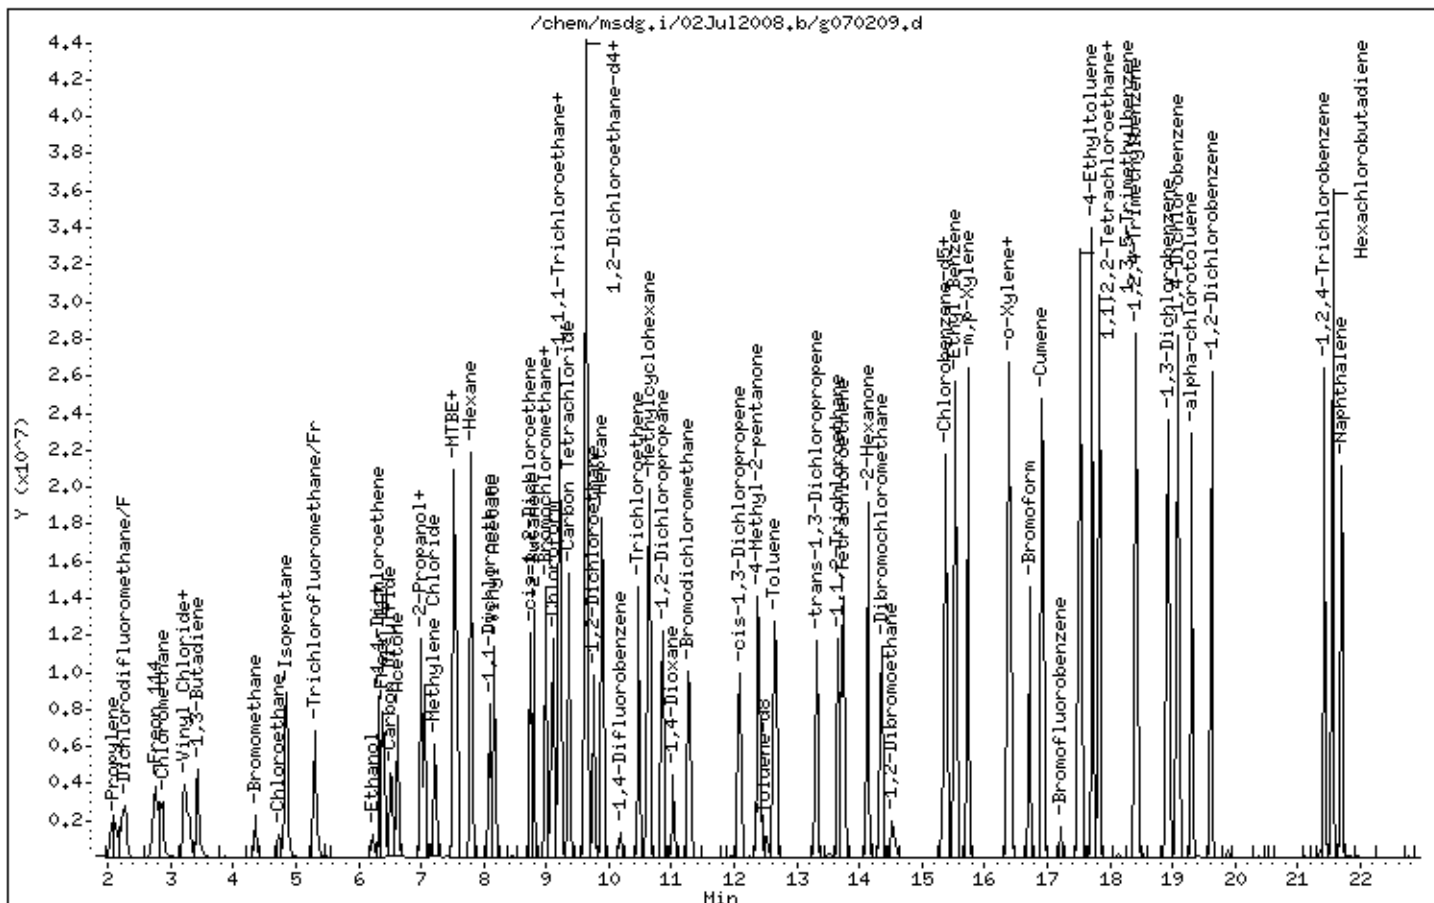



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0807494-04A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080402	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 8/4/08 09:59 AM

Compound	%Recovery
Freon 12	95
Freon 114	101
Vinyl Chloride	102
Bromomethane	101
Chloroethane	116
Freon 11	113
1,1-Dichloroethene	101
Freon 113	96
Methylene Chloride	94
1,1-Dichloroethane	105
cis-1,2-Dichloroethene	108
Chloroform	105
1,1,1-Trichloroethane	113
Carbon Tetrachloride	120
Benzene	111
1,2-Dichloroethane	112
Trichloroethene	108
1,2-Dichloropropane	114
cis-1,3-Dichloropropene	119
Toluene	115
trans-1,3-Dichloropropene	113
1,1,2-Trichloroethane	108
Tetrachloroethene	107
1,2-Dibromoethane (EDB)	108
Chlorobenzene	109
Ethyl Benzene	114
m,p-Xylene	117
o-Xylene	119
Styrene	117
1,1,2,2-Tetrachloroethane	113
1,3,5-Trimethylbenzene	114
1,2,4-Trimethylbenzene	119
1,3-Dichlorobenzene	114
1,4-Dichlorobenzene	112
alpha-Chlorotoluene	129
1,2-Dichlorobenzene	112
1,3-Butadiene	114
Hexane	114
Cyclohexane	114





AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: CCV

Lab ID#: 0807494-04A

**MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN**

<b>File Name:</b>	<b>g080402</b>	<b>Date of Collection: NA</b>
<b>Dil. Factor:</b>	<b>1.00</b>	<b>Date of Analysis: 8/4/08 09:59 AM</b>

<b>Compound</b>	<b>%Recovery</b>
Heptane	124
Bromodichloromethane	116
Dibromochloromethane	113
Cumene	120
Propylbenzene	119
Chloromethane	106
1,2,4-Trichlorobenzene	110
Hexachlorobutadiene	111
Acetone	130
Carbon Disulfide	107
2-Propanol	100
trans-1,2-Dichloroethene	81
2-Butanone (Methyl Ethyl Ketone)	111
Tetrahydrofuran	112
1,4-Dioxane	106
4-Methyl-2-pentanone	114
2-Hexanone	95
Bromoform	115
4-Ethyltoluene	122
Ethanol	90
Methyl tert-butyl ether	111
3-Chloropropene	100
2,2,4-Trimethylpentane	112
Naphthalene	100

**Container Type: NA - Not Applicable**

<b>Surrogates</b>	<b>%Recovery</b>	<b>Method Limits</b>
Toluene-d8	106	70-130
1,2-Dichloroethane-d4	104	70-130
4-Bromofluorobenzene	104	70-130

Report Date: 04-Aug-2008 10:15

## Air Toxics Ltd.

## CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msdg.i                      Injection Date: 04-AUG-2008 09:59  
 Lab File ID: g080402.d                    Init. Cal. Date(s): 02-JUL-2008 02-JUL-2008  
 Analysis Type: AIR                         Init. Cal. Times: 08:28 13:24  
 Lab Sample ID: CCV-1                      Quant Type: ISTD  
 Method: /var/chem/msdg.i/04Aug2008.b/t14q702a.m

COMPOUND	RRF / AMOUNT	RF25	MIN	MAX	CURVE TYPE	
			RRF	%D / %DRIFT	%D / %DRIFT	
\$ 47 1,2-Dichloroethane-d4	1.91937	1.99952	0.010	-4.17561	30.00000	Averaged
\$ 59 Toluene-d8	1.03377	1.09598	0.010	-6.01754	30.00000	Averaged
\$ 81 Bromofluorobenzene	0.58091	0.60201	0.010	-3.63227	30.00000	Averaged
4 Propylene	1.38441	1.35734	0.010	1.95501	30.00000	Averaged
6 Dichlorodifluoromethane/Fr1	3.12081	2.97106	0.010	4.79844	30.00000	Averaged
7 Freon 114	1.57325	1.59090	0.010	-1.12184	30.00000	Averaged
8 Chloromethane	2.12923	2.26877	0.010	-6.55355	30.00000	Averaged
9 Vinyl Chloride	1.15642	1.18564	0.010	-2.52687	30.00000	Averaged
10 1,3-Butadiene	1.25434	1.43146	0.010	-14.12048	30.00000	Averaged
11 Bromomethane	0.56863	0.57370	0.010	-0.89071	30.00000	Averaged
13 Chloroethane	0.43183	0.49994	0.010	-15.77188	30.00000	Averaged
16 Trichlorofluoromethane/Fr11	3.76280	4.24615	0.010	-12.84545	30.00000	Averaged
17 Ethanol	0.69926	0.62616	0.010	10.45387	30.00000	Averaged
19 Freon 113	1.40429	1.34335	0.010	4.33930	30.00000	Averaged
18 1,1-Dichloroethene	0.60047	0.60887	0.010	-1.39818	30.00000	Averaged
21 Acetone	3.73936	4.86959	0.010	-30.22529	30.00000	Averaged <-
24 2-Propanol	3.74741	3.76080	0.010	-0.35754	30.00000	Averaged
25 3-Chloroprene	0.46456	0.46330	0.010	0.27273	30.00000	Averaged
20 Carbon Disulfide	3.15345	3.36781	0.010	-6.79737	30.00000	Averaged
28 Methylene Chloride	0.85907	0.80368	0.010	6.44828	30.00000	Averaged
29 MTBE	3.34823	3.72264	0.010	-11.18216	30.00000	Averaged
30 trans-1,2-Dichloroethene	0.80728	0.65500	0.010	18.86373	30.00000	Averaged
32 Hexane	2.86313	3.27517	0.010	-14.39134	30.00000	Averaged
35 Vinyl Acetate	6.05743	6.25347	0.010	-3.23637	30.00000	Averaged
33 1,1-Dichloroethane	2.93722	3.08211	0.010	-4.93298	30.00000	Averaged
37 2-Butanone	0.71848	0.79986	0.010	-11.32719	30.00000	Averaged
36 cis-1,2-Dichloroethene	0.85438	0.92511	0.010	-8.27778	30.00000	Averaged
38 Tetrahydrofuran	3.05813	3.43297	0.010	-12.25699	30.00000	Averaged
40 Chloroform	3.03655	3.19844	0.010	-5.33151	30.00000	Averaged
42 1,1,1-Trichloroethane	3.11769	3.52744	0.010	-13.14270	30.00000	Averaged
41 Cyclohexane	2.05887	2.34343	0.010	-13.82132	30.00000	Averaged
44 Carbon Tetrachloride	2.84631	3.42404	0.010	-20.29757	30.00000	Averaged
45 2,2,4-Trimethylpentane	3.21714	3.58738	0.010	-11.50835	30.00000	Averaged
46 Benzene	1.15301	1.27693	0.010	-10.74753	30.00000	Averaged
48 1,2-Dichloroethane	0.70601	0.79469	0.010	-12.56030	30.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msdg.i                    Injection Date: 04-AUG-2008 09:59  
 Lab File ID: g080402.d                Init. Cal. Date(s): 02-JUL-2008 02-JUL-2008  
 Analysis Type: AIR                    Init. Cal. Times: 08:28 13:24  
 Lab Sample ID: CCV-1                 Quant Type: ISTD  
 Method: /var/chem/msdg.i/04Aug2008.b/t14q702a.m

COMPOUND	RRF / AMOUNT	RF25	MIN	MAX	CURVE TYPE
			RRF   %D / %DRIFT	%D / %DRIFT	
49 Heptane	1.23504	1.52665	0.010   -23.61137	30.00000	Averaged
52 Trichloroethene	0.47256	0.50866	0.010   -7.63909	30.00000	Averaged
53 1,2-Dichloropropane	0.51157	0.58485	0.010   -14.32618	30.00000	Averaged
54 1,4-Dioxane	0.26125	0.27563	0.010   -5.50394	30.00000	Averaged
55 Bromodichloromethane	0.82928	0.96057	0.010   -15.83249	30.00000	Averaged
56 cis-1,3-Dichloropropene	0.61112	0.72697	0.010   -18.95630	30.00000	Averaged
58 4-Methyl-2-pentanone	1.60869	1.83818	0.010   -14.26593	30.00000	Averaged
60 Toluene	1.35442	1.56187	0.010   -15.31664	30.00000	Averaged
61 trans-1,3-Dichloropropene	0.72100	0.81707	0.010   -13.32427	30.00000	Averaged
63 1,1,2-Trichloroethane	0.52736	0.56743	0.010   -7.59786	30.00000	Averaged
64 Tetrachloroethene	0.67972	0.72607	0.010   -6.81798	30.00000	Averaged
67 2-Hexanone	0.70131	0.66800	0.010   4.74948	30.00000	Averaged
68 Dibromochloromethane	0.84512	0.95434	0.010   -12.92412	30.00000	Averaged
69 1,2-Dibromoethane	0.23665	0.25494	0.010   -7.72637	30.00000	Averaged
73 Chlorobenzene	1.33426	1.45221	0.010   -8.84035	30.00000	Averaged
74 Ethyl Benzene	0.69196	0.78742	0.010   -13.79497	30.00000	Averaged
75 m,p-Xylene	0.84950	0.99079	0.010   -16.63176	30.00000	Averaged
77 o-Xylene	0.79789	0.95199	0.010   -19.31393	30.00000	Averaged
78 Styrene	1.23364	1.44162	0.010   -16.85893	30.00000	Averaged
79 Bromoform	0.80302	0.92729	0.010   -15.47483	30.00000	Averaged
80 Cumene	2.26358	2.72479	0.010   -20.37503	30.00000	Averaged
82 1,1,2,2-Tetrachloroethane	1.38578	1.56588	0.010   -12.99640	30.00000	Averaged
83 Propylbenzene	2.99504	3.55812	0.010   -18.80053	30.00000	Averaged
84 4-Ethyltoluene	2.45625	2.98668	0.010   -21.59520	30.00000	Averaged
85 1,3,5-Trimethylbenzene	2.07118	2.35401	0.010   -13.65545	30.00000	Averaged
87 1,2,4-Trimethylbenzene	1.94441	2.31700	0.010   -19.16249	30.00000	Averaged
89 1,3-Dichlorobenzene	1.32478	1.51082	0.010   -14.04322	30.00000	Averaged
90 1,4-Dichlorobenzene	1.37250	1.53773	0.010   -12.03911	30.00000	Averaged
91 alpha-chlorotoluene	1.72308	2.22604	0.010   -29.18965	30.00000	Averaged
94 1,2-Dichlorobenzene	1.27376	1.42204	0.010   -11.64113	30.00000	Averaged
96 1,2,4-Trichlorobenzene	1.00766	1.10847	0.010   -10.00395	30.00000	Averaged
97 Hexachlorobutadiene	0.86530	0.96336	0.010   -11.33298	30.00000	Averaged
98 Naphthalene	2.03792	2.04540	0.010   -0.36702	30.00000	Averaged
183 Butane	0.24835	0.27405	0.010   -10.34822	30.00000	Averaged
14 Isopentane	1.25434	1.39634	0.010   -11.32105	40.00000	Averaged

Air Toxics Ltd.

CONTINUING CALIBRATION COMPOUNDS

Instrument ID: msdg.i                    Injection Date: 04-AUG-2008 09:59  
Lab File ID: g080402.d                Init. Cal. Date(s): 02-JUL-2008 02-JUL-2008  
Analysis Type: AIR                    Init. Cal. Times: 08:28                    13:24  
Lab Sample ID: CCV-1                 Quant Type: ISTD  
Method: /var/chem/msdg.i/04Aug2008.b/t14q702a.m

COMPOUND	RRF / AMOUNT	RF25	MIN	MAX	CURVE TYPE	
2 Methylcyclohexane	2.85676	3.21671	0.010	-12.59986	40.00000	Averaged
179 tert-Butyl Alcohol	3.09173	3.88460	0.010	-25.64473	40.00000	Averaged

Report Date: 04-Aug-2008 10:15

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/04Aug2008.b/g080402.d  
 Lab Smp Id: CCV-1 Client Smp ID: CCV-1  
 Inj Date : 04-AUG-2008 09:59  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 500ml #1541-162A;CCV-1;CCV-1  
 Misc Info : 25ppbv -> 25ppbv  
 Comment :  
 Method : /var/chem/msdg.i/04Aug2008.b/t14q702a.m  
 Meth Date : 04-Aug-2008 10:15 lrandolp Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1 Continuing Calibration Sample  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08Q.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPBV)	CAL-AMT	ON-COL	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	318312	10.0000			80.00- 120.00	100.00
9.002	9.002	(1.000)	128	246550				0.00- 30.00	77.46
9.002	9.002	(1.000)	49	1083640				0.00- 30.00	340.43
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1208514	10.0000			80.00- 120.00	100.00
10.186	10.186	(1.000)	88	206279				0.00- 47.07	17.07
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1189759	10.0000			80.00- 120.00	100.00
15.319	15.319	(1.000)	82	747360				0.00- 30.00	62.82
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668	(1.074)	65	636471	10.0000	10.418		80.00- 120.00	100.00
9.668	9.668	(1.074)	67	349290				0.00- 30.00	54.88
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1324507	10.0000	10.602		80.00- 120.00	100.00
12.499	12.499	(1.227)	70	160740				0.00- 42.14	12.14

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
\$ 59 Toluene-d8 (continued)									
12.499	12.499	(1.227)	100	846006			33.87- 93.87	63.87	
-----									
\$ 81 Bromofluorobenzene CAS #: 460-00-4									
17.226	17.226	(1.125)	174	716243	10.0000	10.363	80.00- 120.00	100.00	
17.201	17.201	(1.123)	95	1064311			118.60- 178.60	148.60	
17.226	17.226	(1.125)	176	697137			67.33- 127.33	97.33	
-----									
4 Propylene CAS #: 115-07-1									
2.125	2.125	(0.236)	41	1080147	25.0000	24.511	80.00- 120.00	100.00	
2.125	2.125	(0.236)	42	724470			0.00- 30.00	67.07	
2.125	2.125	(0.236)	39	822163			0.00- 30.00	76.12	
-----									
6 Dichlorodifluoromethane/Fr12 CAS #: 75-71-8									
2.294	2.294	(0.255)	85	2364312	25.0000	23.800	80.00- 120.00	100.00	
2.270	2.270	(0.252)	87	759661			2.13- 62.13	32.13	
-----									
7 Freon 114 CAS #: 76-14-2									
2.752	2.752	(0.306)	135	1266004	25.0000	25.280	80.00- 120.00	100.00	
2.752	2.752	(0.306)	137	406218			0.00- 30.00	32.09	
2.752	2.752	(0.306)	85	2120272			0.00- 30.00	167.48	
-----									
8 Chloromethane CAS #: 74-87-3									
2.872	2.872	(0.319)	50	1805443	25.0000	26.638	80.00- 120.00	100.00	
2.872	2.872	(0.319)	52	477661			0.00- 30.00	26.46	
-----									
9 Vinyl Chloride CAS #: 75-01-4									
3.308	3.308	(0.367)	62	943511	25.0000	25.632	80.00- 120.00	100.00	
3.308	3.308	(0.367)	64	276426			0.00- 59.30	29.30	
-----									
10 1,3-Butadiene CAS #: 106-99-0									
3.430	3.430	(0.381)	54	1139130	25.0000	28.530	80.00- 120.00	100.00	
3.430	3.430	(0.381)	39	1469273			0.00- 30.00	128.98	
-----									
11 Bromomethane CAS #: 74-83-9									
4.351	4.351	(0.483)	94	456538	25.0000	25.223	80.00- 120.00	100.00	
4.351	4.351	(0.483)	96	414131			60.71- 120.71	90.71	
-----									
13 Chloroethane CAS #: 75-00-3									
4.724	4.724	(0.525)	64	397845	25.0000	28.943	80.00- 120.00	100.00	
4.724	4.724	(0.525)	49	183822			0.00- 30.00	46.20	
4.724	4.724	(0.525)	66	120714			0.00- 30.00	30.34	
-----									
16 Trichlorofluoromethane/Fr11 CAS #: 75-69-4									
5.304	5.304	(0.589)	101	3379000	25.0000	28.211	80.00- 120.00	100.00	
5.304	5.304	(0.589)	103	2169076			34.19- 94.19	64.19	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
-----									
17 Ethanol						CAS #: 64-17-5			
6.225	6.225	(0.692)	45	498286	25.0000	22.386	80.00- 120.00	100.00	
6.225	6.225	(0.692)	43	116314			0.00- 30.00	23.34	
6.225	6.225	(0.692)	46	190200			0.00- 30.00	38.17	
-----									
19 Freon 113						CAS #: 76-13-1			
6.390	6.390	(0.710)	151	1069012	25.0000	23.915	80.00- 120.00	100.00	
6.390	6.390	(0.710)	153	690523			34.59- 94.59	64.59	
6.390	6.390	(0.710)	101	1501894			0.00- 30.00	140.49	
-----									
18 1,1-Dichloroethene						CAS #: 75-35-4			
6.335	6.335	(0.704)	98	484525	25.0000	25.350	80.00- 120.00	100.00	
6.335	6.335	(0.704)	61	2204595			0.00- 30.00	455.00	
6.335	6.335	(0.704)	96	767558			0.00- 30.00	158.41	
-----									
21 Acetone						CAS #: 67-64-1			
6.637	6.637	(0.737)	43	3875124	25.0000	32.556	80.00- 120.00	100.00	
6.637	6.637	(0.737)	58	773764			0.00- 30.00	19.97	
-----									
24 2-Propanol						CAS #: 67-63-0			
7.049	7.049	(0.783)	45	2992773	25.0000	25.089	80.00- 120.00	100.00	
7.049	7.049	(0.783)	43	665299			0.00- 30.00	22.23	
7.049	7.049	(0.783)	59	85735			0.00- 30.00	2.86	
-----									
25 3-Chloroprene						CAS #: 107-05-1			
6.994	6.994	(0.777)	76	368681	25.0000	24.932	80.00- 120.00	100.00	
6.994	6.994	(0.777)	41	2661857			0.00- 30.00	721.99	
-----									
20 Carbon Disulfide						CAS #: 75-15-0			
6.500	6.500	(0.722)	76	2680032	25.0000	26.699	80.00- 120.00	100.00	
-----									
28 Methylene Chloride						CAS #: 75-09-2			
7.213	7.213	(0.801)	84	639550	25.0000	23.388	80.00- 120.00	100.00	
7.213	7.213	(0.801)	49	2017144			285.40- 345.40	315.40	
7.213	7.213	(0.801)	51	591927			0.00- 30.00	92.55	
-----									
29 MTBE						CAS #: 1634-04-4			
7.515	7.515	(0.835)	73	2962399	25.0000	27.796	80.00- 120.00	100.00	
7.515	7.515	(0.835)	57	1394885			0.00- 30.00	47.09	
7.543	7.543	(0.838)	41	2473579			0.00- 30.00	83.50	
-----									
30 trans-1,2-Dichloroethene						CAS #: 156-60-5			
7.515	7.515	(0.835)	98	521236	25.0000	20.284	80.00- 120.00	100.00	
7.515	7.515	(0.835)	61	2111856			0.00- 30.00	405.16	
7.515	7.515	(0.835)	96	816475			0.00- 30.00	156.64	
-----									

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
32 Hexane						CAS #: 110-54-3			
7.790	7.790	(0.865)	57	2606317	25.0000	28.598	80.00- 120.00	100.00	
7.790	7.790	(0.865)	43	2305776			0.00- 30.00	88.47	
7.790	7.790	(0.865)	86	269223			0.00- 30.00	10.33	
-----									
35 Vinyl Acetate						CAS #: 108-05-4			
8.174	8.174	(0.908)	43	4976385	25.0000	25.809	80.00- 120.00	100.00	
8.174	8.174	(0.908)	42	410482			0.00- 30.00	8.25	
8.174	8.174	(0.908)	86	232615			0.00- 30.00	4.67	
-----									
33 1,1-Dichloroethane						CAS #: 75-34-3			
8.092	8.092	(0.899)	63	2452680	25.0000	26.233	80.00- 120.00	100.00	
8.092	8.092	(0.899)	65	727360			0.00- 59.66	29.66	
-----									
37 2-Butanone						CAS #: 78-93-3			
8.792	8.792	(0.977)	72	636516	25.0000	27.832	80.00- 120.00	100.00	
8.792	8.792	(0.977)	43	4827463			728.42- 788.42	758.42	
8.792	8.792	(0.977)	57	285599			0.00- 30.00	44.87	
-----									
36 cis-1,2-Dichloroethene						CAS #: 156-59-2			
8.748	8.748	(0.972)	98	736183	25.0000	27.069	80.00- 120.00	100.00	
8.748	8.748	(0.972)	61	2110117			256.63- 316.63	286.63	
8.748	8.748	(0.972)	96	1153215			126.65- 186.65	156.65	
-----									
38 Tetrahydrofuran						CAS #: 109-99-9			
9.002	9.002	(1.000)	42	2731888	25.0000	28.064	80.00- 120.00	100.00	
9.002	9.002	(1.000)	71	549256			0.00- 30.00	20.11	
9.002	9.002	(1.000)	72	601445			0.00- 30.00	22.02	
-----									
40 Chloroform						CAS #: 67-66-3			
9.099	9.099	(1.011)	83	2545257	25.0000	26.333	80.00- 120.00	100.00	
9.099	9.099	(1.011)	85	1615867			33.49- 93.49	63.49	
-----									
42 1,1,1-Trichloroethane						CAS #: 71-55-6			
9.229	9.229	(1.025)	97	2807063	25.0000	28.286	80.00- 120.00	100.00	
9.229	9.229	(1.025)	99	1778681			33.36- 93.36	63.36	
-----									
41 Cyclohexane						CAS #: 110-82-7			
9.197	9.197	(1.022)	84	1864856	25.0000	28.455	80.00- 120.00	100.00	
9.197	9.197	(1.022)	56	3319451			0.00- 30.00	178.00	
9.197	9.197	(1.022)	41	2419066			0.00- 30.00	129.72	
-----									
44 Carbon Tetrachloride						CAS #: 56-23-5			
9.359	9.359	(1.040)	119	2724785	25.0000	30.074	80.00- 120.00	100.00	
9.359	9.359	(1.040)	117	2814202			73.28- 133.28	103.28	
-----									



AMOUNTS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====	=====	
-----										
45	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.639	9.639	(1.071)	56	2854768	25.0000	27.877	80.00- 120.00	100.00		
9.639	9.639	(1.071)	99	313245			0.00- 30.00	10.97		
9.639	9.639	(1.071)	41	3028579			0.00- 30.00	106.09		
-----										
46	Benzene					CAS #: 71-43-2				
9.639	9.639	(0.946)	78	3857960	25.0000	27.687	80.00- 120.00	100.00		
9.639	9.639	(0.946)	77	893792			0.00- 30.00	23.17		
-----										
48	1,2-Dichloroethane					CAS #: 107-06-2				
9.755	9.755	(0.958)	62	2400992	25.0000	28.140	80.00- 120.00	100.00		
9.755	9.755	(0.958)	64	739709			0.00- 30.00	30.81		
-----										
49	Heptane					CAS #: 142-82-5				
9.872	9.872	(0.969)	43	4612447	25.0000	30.903	80.00- 120.00	100.00		
9.872	9.872	(0.969)	57	1811870			0.00- 30.00	39.28		
9.872	9.872	(0.969)	100	372605			0.00- 30.00	8.08		
-----										
52	Trichloroethene					CAS #: 79-01-6				
10.475	10.475	(1.028)	130	1536808	25.0000	26.910	80.00- 120.00	100.00		
10.475	10.475	(1.028)	95	1663986			0.00- 30.00	108.28		
10.475	10.475	(1.028)	97	1075786			0.00- 30.00	70.00		
-----										
53	1,2-Dichloropropane					CAS #: 78-87-5				
10.861	10.861	(1.066)	63	1767013	25.0000	28.582	80.00- 120.00	100.00		
10.861	10.861	(1.066)	62	1264088			41.54- 101.54	71.54		
10.861	10.861	(1.066)	41	1604538			60.81- 120.81	90.81		
-----										
54	1,4-Dioxane					CAS #: 123-91-1				
11.029	11.029	(1.083)	88	832756	25.0000	26.376	80.00- 120.00	100.00		
11.029	11.029	(1.083)	58	838297			70.67- 130.67	100.67		
11.029	11.029	(1.083)	57	286247			0.00- 30.00	34.37		
-----										
55	Bromodichloromethane					CAS #: 75-27-4				
11.270	11.270	(1.106)	83	2902160	25.0000	28.958	80.00- 120.00	100.00		
11.270	11.270	(1.106)	85	1786440			31.56- 91.56	61.56		
-----										
56	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.090	12.090	(1.187)	75	2196385	25.0000	29.739	80.00- 120.00	100.00		
12.090	12.090	(1.187)	77	695538			1.67- 61.67	31.67		
12.090	12.090	(1.187)	39	2016662			61.82- 121.82	91.82		
-----										
58	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.379	12.379	(1.215)	43	5553668	25.0000	28.566	80.00- 120.00	100.00		
12.379	12.379	(1.215)	58	1535039			0.00- 30.00	27.64		
12.379	12.379	(1.215)	85	479349			0.00- 30.00	8.63		
-----										

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
60 Toluene									
						CAS #:	108-88-3		
12.644	12.644	(1.241)	91	4718858	25.0000	28.829	80.00-	120.00	100.00
12.644	12.644	(1.241)	92	2747152			28.22-	88.22	58.22
-----									
61 trans-1,3-Dichloropropene									
						CAS #:	10061-02-6		
13.308	13.308	(0.869)	75	2430290	25.0000	28.331	80.00-	120.00	100.00
13.308	13.308	(0.869)	77	768467			1.62-	61.62	31.62
13.308	13.308	(0.869)	39	2065384			54.99-	114.99	84.99
-----									
63 1,1,2-Trichloroethane									
						CAS #:	79-00-5		
13.665	13.665	(0.892)	97	1687769	25.0000	26.899	80.00-	120.00	100.00
13.665	13.665	(0.892)	99	1039434			31.59-	91.59	61.59
13.665	13.665	(0.892)	83	1506598			59.27-	119.27	89.27
-----									
64 Tetrachloroethene									
						CAS #:	127-18-4		
13.747	13.747	(0.897)	166	2159613	25.0000	26.704	80.00-	120.00	100.00
13.747	13.747	(0.897)	129	1668506			47.26-	107.26	77.26
13.747	13.747	(0.897)	131	1619641			45.00-	105.00	75.00
-----									
67 2-Hexanone									
						CAS #:	591-78-6		
14.132	14.132	(0.922)	58	1986905	25.0000	23.813	80.00-	120.00	100.00
14.132	14.132	(0.922)	43	5127313			228.06-	288.06	258.06
14.132	14.132	(0.922)	100	268030			0.00-	30.00	13.49
-----									
68 Dibromochloromethane									
						CAS #:	124-48-1		
14.352	14.352	(0.937)	129	2838597	25.0000	28.231	80.00-	120.00	100.00
14.352	14.352	(0.937)	208	141956			0.00-	30.00	5.00
-----									
69 1,2-Dibromoethane									
						CAS #:	106-93-4		
14.517	14.517	(0.948)	107	758285	25.0000	26.932	80.00-	120.00	100.00
14.517	14.517	(0.948)	109	701058			62.45-	122.45	92.45
-----									
73 Chlorobenzene									
						CAS #:	108-90-7		
15.370	15.370	(1.003)	112	4319451	25.0000	27.210	80.00-	120.00	100.00
15.370	15.370	(1.003)	114	1374425			1.82-	61.82	31.82
15.370	15.370	(1.003)	77	2724168			33.07-	93.07	63.07
-----									
74 Ethyl Benzene									
						CAS #:	100-41-4		
15.525	15.525	(1.013)	106	2342098	25.0000	28.449	80.00-	120.00	100.00
15.525	15.525	(1.013)	91	7561873			0.00-	30.00	322.87
-----									
75 m,p-Xylene									
						CAS #:	108-38-3		
15.731	15.731	(1.027)	106	2946998	25.0000	29.158	80.00-	120.00	100.00
15.731	15.731	(1.027)	91	6110185			0.00-	30.00	207.34
-----									
77 o-Xylene									
						CAS #:	95-47-6		
16.376	16.376	(1.069)	106	2831592	25.0000	29.828	80.00-	120.00	100.00

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
77 o-Xylene (continued)									
16.376	16.376	(1.069)	91	6120674			186.16- 246.16	216.16	
-----									
78 Styrene CAS #: 100-42-5									
16.401	16.401	(1.071)	104	4287956	25.0000	29.215	80.00- 120.00	100.00	
16.401	16.401	(1.071)	78	2396808			25.90- 85.90	55.90	
-----									
79 Bromoform CAS #: 75-25-2									
16.711	16.711	(1.091)	173	2758127	25.0000	28.869	80.00- 120.00	100.00	
16.711	16.711	(1.091)	171	1430837			0.00- 30.00	51.88	
-----									
80 Cumene CAS #: 98-82-8									
16.917	16.917	(1.104)	105	8104598	25.0000	30.094	80.00- 120.00	100.00	
16.917	16.917	(1.104)	120	2137395			0.00- 56.37	26.37	
-----									
82 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
17.484	17.484	(1.141)	83	4657548	25.0000	28.249	80.00- 120.00	100.00	
17.484	17.484	(1.141)	85	2940203			33.13- 93.13	63.13	
-----									
83 Propylbenzene CAS #: 103-65-1									
17.536	17.536	(1.145)	91	10583261	25.0000	29.700	80.00- 120.00	100.00	
17.536	17.536	(1.145)	120	2289532			0.00- 30.00	21.63	
-----									
84 4-Ethyltoluene CAS #: 622-96-8									
17.716	17.716	(1.157)	105	8883575	25.0000	30.399	80.00- 120.00	100.00	
17.716	17.716	(1.157)	120	2604273			0.00- 59.32	29.32	
-----									
85 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.820	17.820	(1.163)	105	7001768	25.0000	28.414	80.00- 120.00	100.00	
17.820	17.820	(1.163)	120	3267523			16.67- 76.67	46.67	
-----									
87 1,2,4-Trimethylbenzene CAS #: 95-63-6									
18.413	18.413	(1.202)	105	6891690	25.0000	29.791	80.00- 120.00	100.00	
18.413	18.413	(1.202)	120	3048663			14.24- 74.24	44.24	
-----									
89 1,3-Dichlorobenzene CAS #: 541-73-1									
18.929	18.929	(1.236)	146	4493789	25.0000	28.511	80.00- 120.00	100.00	
18.929	18.929	(1.236)	148	2836668			0.00- 30.00	63.12	
18.929	18.929	(1.236)	111	1972789			0.00- 30.00	43.90	
-----									
90 1,4-Dichlorobenzene CAS #: 106-46-7									
19.083	19.083	(1.246)	146	4573825	25.0000	28.010	80.00- 120.00	100.00	
19.083	19.083	(1.246)	148	2902912			0.00- 30.00	63.47	
19.083	19.083	(1.246)	111	1956082			0.00- 30.00	42.77	
-----									
91 alpha-Chlorotoluene CAS #: 100-44-7									
19.316	19.316	(1.261)	91	6621124	25.0000	32.297	80.00- 120.00	100.00	

AMOUNTS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	CAL-AMT ( PPEV)	ON-COL ( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
91 alpha-Chlorotoluene (continued)									
19.316	19.316	(1.261)	126	1266108			0.00- 30.00	19.12	
-----									
94 1,2-Dichlorobenzene CAS #: 95-50-1									
19.625	19.625	(1.281)	146	4229709	25.0000	27.910	80.00- 120.00	100.00	
19.625	19.625	(1.281)	148	2681555			33.40- 93.40	63.40	
19.625	19.625	(1.281)	111	1902696			14.98- 74.98	44.98	
-----									
96 1,2,4-Trichlorobenzene CAS #: 120-82-1									
21.430	21.430	(1.399)	180	3297025	25.0000	27.501	80.00- 120.00	100.00	
21.430	21.430	(1.399)	182	3173250			66.25- 126.25	96.25	
-----									
97 Hexachlorobutadiene CAS #: 87-68-3									
21.559	21.559	(1.407)	225	2865421	25.0000	27.833	80.00- 120.00	100.00	
21.559	21.559	(1.407)	223	1793067			0.00- 30.00	62.58	
-----									
98 Naphthalene CAS #: 91-20-3									
21.688	21.688	(1.416)	128	6083840	25.0000	25.092	80.00- 120.00	100.00	
21.688	21.688	(1.416)	127	756699			0.00- 30.00	12.44	
-----									
183 Butane CAS #: 106-97-8									
3.221	3.221	(0.358)	58	218080	25.0000	27.587	80.00- 120.00	100.00	
3.221	3.221	(0.358)	43	2438274			0.00- 30.00	1118.06	
-----									
14 Isopentane CAS #: 78-78-4									
4.827	4.827	(0.536)	57	1111181	25.0000	27.830	80.00- 120.00	100.00	
4.827	4.827	(0.536)	43	2185465			0.00- 30.00	196.68	
4.827	4.827	(0.536)	42	1932376			0.00- 30.00	173.90	
-----									
2 Methylcyclohexane CAS #: 108-87-2									
10.644	10.644	(1.182)	83	2559790	25.0000	28.150	80.00- 120.00	100.00	
10.644	10.644	(1.182)	98	1127894			0.00- 30.00	44.06	
10.644	10.644	(1.182)	55	3134047			0.00- 30.00	122.43	
-----									
179 tert-Butyl Alcohol CAS #: 75-65-0									
7.570	7.570	(0.841)	59	3091288	25.0000	31.411	80.00- 120.00	100.00	
7.543	7.543	(0.838)	41	2473579			0.00- 30.00	80.02	
7.515	7.515	(0.835)	57	1394885			0.00- 30.00	45.12	
-----									

Report Date: 04-Aug-2008 10:15

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 04-AUG-2008

Lab File ID: g080402.d

Calibration Time: 09:59

Lab Smp Id: CCV-1

Client Smp ID: CCV-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /var/chem/msdg.i/04Aug2008.b/t14q702a.m

Misc Info: 25ppbv -&gt; 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	318312	190987	445637	318312	0.00
51 1,4-Difluorobenze	1208514	725108	1691920	1208514	0.00
72 Chlorobenzene-d5	1189759	713855	1665663	1189759	0.00

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 04-AUG-2008 09:59

Client ID: CCV-1


Instrument: msdg.i

Sample Info: 500ml #1541-162A;CCV-1;CCV-1

Operator: lmr

Column phase: RTX-624

Column diameter: 0.32

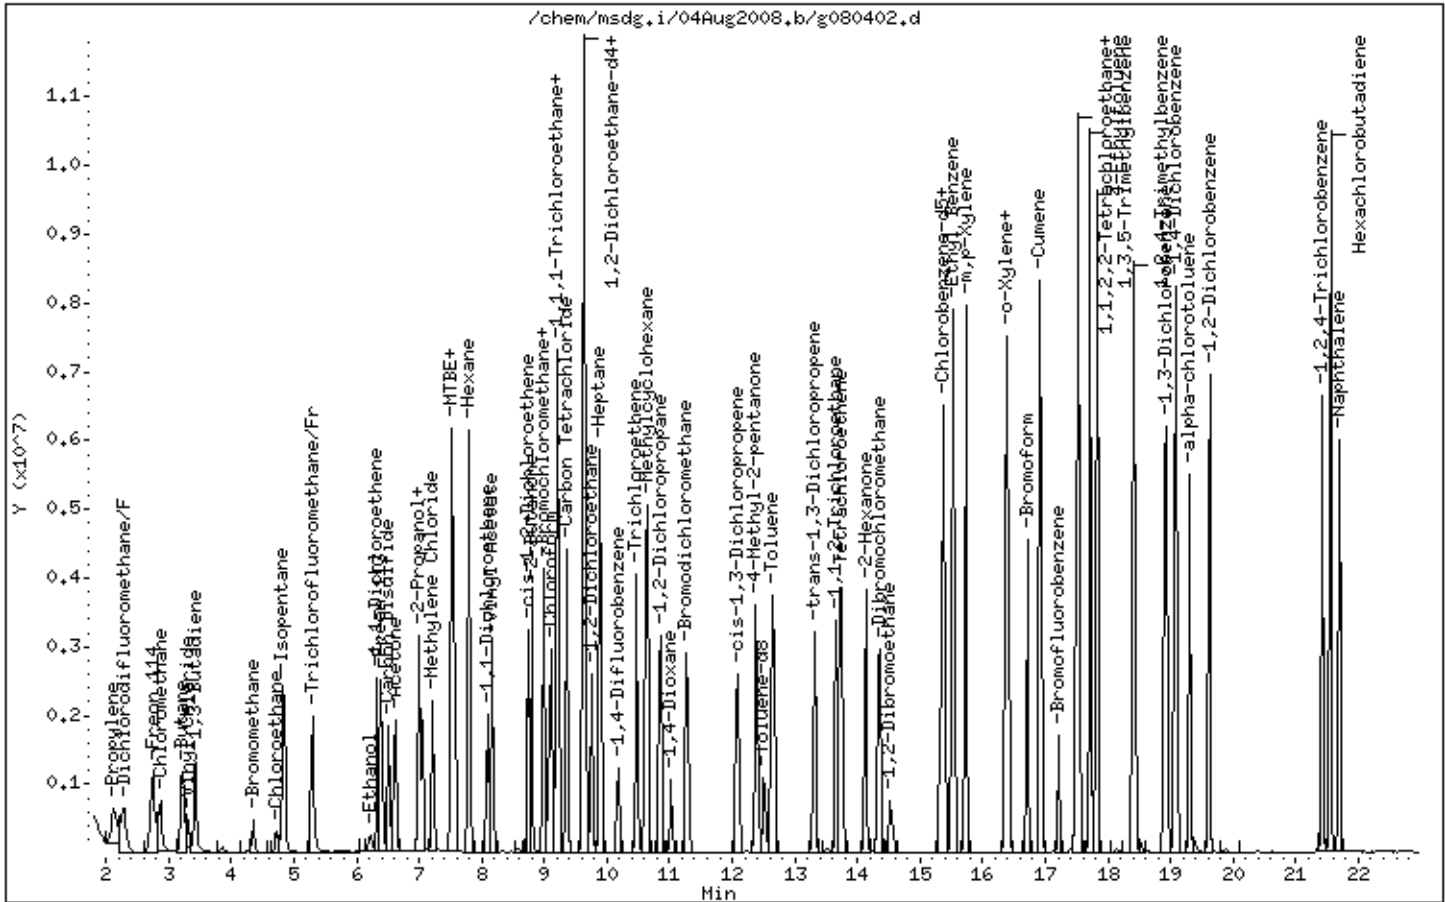



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0807494-05A

MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN

File Name:	g080403	Date of Collection: NA
Dil. Factor:	1.00	Date of Analysis: 8/4/08 10:52 AM

Compound	%Recovery
Freon 12	101
Freon 114	100
Vinyl Chloride	105
Bromomethane	100
Chloroethane	104
Freon 11	103
1,1-Dichloroethene	104
Freon 113	96
Methylene Chloride	90
1,1-Dichloroethane	104
cis-1,2-Dichloroethene	101
Chloroform	100
1,1,1-Trichloroethane	100
Carbon Tetrachloride	108
Benzene	103
1,2-Dichloroethane	107
Trichloroethene	99
1,2-Dichloropropane	106
cis-1,3-Dichloropropene	106
Toluene	109
trans-1,3-Dichloropropene	107
1,1,2-Trichloroethane	102
Tetrachloroethene	103
1,2-Dibromoethane (EDB)	98
Chlorobenzene	101
Ethyl Benzene	104
m,p-Xylene	106
o-Xylene	108
Styrene	113
1,1,2,2-Tetrachloroethane	104
1,3,5-Trimethylbenzene	109
1,2,4-Trimethylbenzene	114
1,3-Dichlorobenzene	105
1,4-Dichlorobenzene	103
alpha-Chlorotoluene	115
1,2-Dichlorobenzene	102
1,3-Butadiene	106
Hexane	112
Cyclohexane	101



AN ENVIRONMENTAL ANALYTICAL LABORATORY

Client Sample ID: LCS

Lab ID#: 0807494-05A

**MODIFIED EPA METHOD TO-15 GC/MS FULL SCAN**

<b>File Name:</b>	<b>g080403</b>	<b>Date of Collection: NA</b>
<b>Dil. Factor:</b>	<b>1.00</b>	<b>Date of Analysis: 8/4/08 10:52 AM</b>

<b>Compound</b>	<b>%Recovery</b>
Heptane	117
Bromodichloromethane	107
Dibromochloromethane	107
Cumene	115
Propylbenzene	113
Chloromethane	107
1,2,4-Trichlorobenzene	118
Hexachlorobutadiene	107
Acetone	100
Carbon Disulfide	96
2-Propanol	104
trans-1,2-Dichloroethene	74
2-Butanone (Methyl Ethyl Ketone)	104
Tetrahydrofuran	110
1,4-Dioxane	101
4-Methyl-2-pentanone	114
2-Hexanone	115
Bromoform	109
4-Ethyltoluene	113
Ethanol	88
Methyl tert-butyl ether	96
3-Chloropropene	97
2,2,4-Trimethylpentane	104
Naphthalene	127

**Container Type: NA - Not Applicable**

<b>Surrogates</b>	<b>%Recovery</b>	<b>Method Limits</b>
Toluene-d8	103	70-130
1,2-Dichloroethane-d4	102	70-130
4-Bromofluorobenzene	100	70-130



Air Toxics Ltd.

RECOVERY REPORT

Client Name: Client SDG: 04Aug2008  
 Sample Matrix: GAS Fraction: VOA  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Level: LOW Operator: lmr  
 Data Type: MS DATA SampleType: LCS  
 SpikeList File: Spectra.spk Quant Type: ISTD  
 Sublist File: AT08Q.sub  
 Method File: /var/chem/msdg.i/04Aug2008.b/t14q702a.m  
 Misc Info: 50ppbv -> 25ppbv

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
6 Dichlorodifluorome	25.000	25.200	100.80	70-130
7 Freon 114	25.000	24.995	99.98	70-130
8 Chloromethane	25.000	26.695	106.78	70-130
9 Vinyl Chloride	25.000	26.280	105.12	70-130
10 1,3-Butadiene	25.000	26.408	105.63	60-140
11 Bromomethane	25.000	25.144	100.58	70-130
13 Chloroethane	25.000	26.142	104.57	70-130
16 Trichlorofluoromet	25.000	25.750	103.00	70-130
17 Ethanol	25.000	21.969	87.88	60-140
19 Freon 113	25.000	24.043	96.17	70-130
18 1,1-Dichloroethene	25.000	25.983	103.93	70-130
21 Acetone	25.000	24.926	99.70	60-140
20 Carbon Disulfide	25.000	23.952	95.81	60-140
24 2-Propanol	25.000	25.950	103.80	60-140
28 Methylene Chloride	25.000	22.426	89.70	70-130
29 MTBE	25.000	23.952	95.81	60-140
30 trans-1,2-Dichloro	25.000	18.486	73.94	60-140
32 Hexane	25.000	27.982	111.93	60-140
33 1,1-Dichloroethane	25.000	26.140	104.56	70-130
36 cis-1,2-Dichloroet	25.000	25.319	101.28	70-130
37 2-Butanone	25.000	25.908	103.63	60-140
38 Tetrahydrofuran	25.000	27.564	110.26	60-140
40 Chloroform	25.000	24.963	99.85	70-130
41 Cyclohexane	25.000	25.176	100.71	60-140
42 1,1,1-Trichloroeth	25.000	25.003	100.01	70-130
44 Carbon Tetrachlori	25.000	27.016	108.06	70-130
46 Benzene	25.000	25.701	102.81	70-130
49 Heptane	25.000	29.326	117.30	60-140
48 1,2-Dichloroethane	25.000	26.738	106.95	70-130
52 Trichloroethene	25.000	24.863	99.45	70-130
53 1,2-Dichloropropan	25.000	26.492	105.97	70-130
54 1,4-Dioxane	25.000	25.368	101.47	60-140
55 Bromodichlorometha	25.000	26.736	106.94	60-140

Report Date: 04-Aug-2008 11:04

SPIKE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
56 cis-1,3-Dichloropr	25.000	26.529	106.12	70-130
58 4-Methyl-2-pentano	25.000	28.617	114.47	60-140
60 Toluene	25.000	27.265	109.06	70-130
61 trans-1,3-Dichloro	25.000	26.808	107.23	70-130
63 1,1,2-Trichloroeth	25.000	25.443	101.77	70-130
67 2-Hexanone	25.000	28.778	115.11	60-140
64 Tetrachloroethene	25.000	25.820	103.28	70-130
68 Dibromochlorometha	25.000	26.717	106.87	60-140
69 1,2-Dibromoethane	25.000	24.550	98.20	70-130
73 Chlorobenzene	25.000	25.223	100.89	70-130
74 Ethyl Benzene	25.000	25.948	103.79	70-130
75 m,p-Xylene	25.000	26.553	106.21	70-130
77 o-Xylene	25.000	26.974	107.90	70-130
78 Styrene	25.000	28.201	112.80	70-130
79 Bromoform	25.000	27.248	108.99	60-140
80 Cumene	25.000	28.855	115.42	60-140
82 1,1,2,2-Tetrachlor	25.000	26.123	104.49	70-130
83 Propylbenzene	25.000	28.201	112.80	60-140
84 4-Ethyltoluene	25.000	28.317	113.27	60-140
85 1,3,5-Trimethylben	25.000	27.322	109.29	70-130
87 1,2,4-Trimethylben	25.000	28.411	113.64	70-130
89 1,3-Dichlorobenzen	25.000	26.320	105.28	70-130
90 1,4-Dichlorobenzen	25.000	25.666	102.66	70-130
91 alpha-Chlorotoluen	25.000	28.728	114.91	70-130
94 1,2-Dichlorobenzen	25.000	25.584	102.34	70-130
96 1,2,4-Trichloroben	25.000	29.600	118.40	70-130
97 Hexachlorobutadien	25.000	26.833	107.33	60-130
98 Naphthalene	25.000	31.679	126.72	60-140
25 3-Chloroprene	25.000	24.348	97.39	60-140
45 2,2,4-Trimethylpen	25.000	26.077	104.31	60-140
179 tert-Butyl Alcohol	25.000	27.208	108.83	60-140
183 Butane	25.000	27.789	111.16	60-140
14 Isopentane	25.000	27.499	109.99	60-140
2 Methylcyclohexane	25.000	25.245	100.98	60-140

SURROGATE COMPOUND	CONC ADDED PPBV	CONC RECOVERED PPBV	% RECOVERED	LIMITS
\$ 47 1,2-Dichloroethane	10.000	10.190	101.91	70-130
\$ 59 Toluene-d8	10.000	10.277	102.77	70-130
\$ 81 Bromofluorobenzene	10.000	9.965	99.65	70-130

Report Date: 04-Aug-2008 11:04

## Air Toxics Ltd.

## AMBIENT AIR METHOD TO14/TO15

Data file : /chem/msdg.i/04Aug2008.b/g080403.d  
 Lab Smp Id: LCS-1 Client Smp ID: LCS-1  
 Inj Date : 04-AUG-2008 10:52  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 250ml #1541-227;LCS-1;LCS-1  
 Misc Info : 50ppbv -> 25ppbv  
 Comment :  
 Method : /var/chem/msdg.i/04Aug2008.b/t14q702a.m  
 Meth Date : 04-Aug-2008 10:15 lrandolp Quant Type: ISTD  
 Cal Date : 02-JUL-2008 13:24 Cal File: g070209.d  
 Als bottle: 1 QC Sample: LCS  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: AT08Q.sub  
 Target Version: 3.50 Sample Matrix: AIR  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* CpndVariable

Cpnd Variable Local Compound Variable

CONCENTRATIONS									
ON-COL FINAL									
RT	EXP RT	(REL RT)	MASS	RESPONSE	( PPBV)	( PPBV)	TARGET RANGE	RATIO	
==	=====	=====	====	=====	=====	=====	=====	=====	
* 39 Bromochloromethane CAS #: 74-97-5									
9.002	9.002	(1.000)	130	310013	10.0000		80.00- 120.00	100.00	
9.002	9.002	(1.000)	128	237686			0.00- 30.00	76.67	
9.002	9.002	(1.000)	49	774787			0.00- 30.00	249.92	
-----									
* 51 1,4-Difluorobenzene CAS #: 540-36-3									
10.186	10.186	(1.000)	114	1174713	10.0000		80.00- 120.00	100.00	
10.186	10.186	(1.000)	88	202910			0.00- 47.07	17.27	
-----									
* 72 Chlorobenzene-d5 CAS #: 3114-55-4									
15.319	15.319	(1.000)	117	1085504	10.0000		80.00- 120.00	100.00	
15.319	15.319	(1.000)	82	675634			0.00- 30.00	62.24	
-----									
\$ 47 1,2-Dichloroethane-d4 CAS #: 17060-07-0									
9.668	9.668	(1.074)	65	606372	10.1906	10.190	80.00- 120.00	100.00	
9.668	9.668	(1.074)	67	336248			0.00- 30.00	55.45	
-----									
\$ 59 Toluene-d8 CAS #: 2037-26-5									
12.499	12.499	(1.227)	98	1248079	10.2775	10.277	80.00- 120.00	100.00	
12.499	12.499	(1.227)	70	149307			0.00- 42.14	11.96	

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPEV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== =====

\$ 59 Toluene-d8 (continued)

12.499 12.499 (1.227) 100 791385 33.87- 93.87 63.41

\$ 81 Bromofluorobenzene

CAS #: 460-00-4

17.226 17.226 (1.125) 174 628392 9.96536 9.965 80.00- 120.00 100.00

17.201 17.201 (1.123) 95 928997 118.60- 178.60 147.84

17.226 17.226 (1.125) 176 608231 67.33- 127.33 96.79

4 Propylene

CAS #: 115-07-1

2.101 2.125 (0.233) 41 1162407 27.0841 27.084 80.00- 120.00 100.00

2.101 2.125 (0.233) 42 762100 0.00- 30.00 65.56

2.101 2.125 (0.233) 39 860705 0.00- 30.00 74.05

6 Dichlorodifluoromethane/Fr12

CAS #: 75-71-8

2.270 2.294 (0.252) 85 2438101 25.2002 25.200 80.00- 120.00 100.00

2.246 2.270 (0.249) 87 759939 2.13- 62.13 31.17

7 Freon 114

CAS #: 76-14-2

2.752 2.752 (0.306) 135 1219089 24.9953 24.995 80.00- 120.00 100.00

2.752 2.752 (0.306) 137 396701 0.00- 30.00 32.54

2.752 2.752 (0.306) 85 1969043 0.00- 30.00 161.52

8 Chloromethane

CAS #: 74-87-3

2.872 2.872 (0.319) 50 1762120 26.6952 26.695 80.00- 120.00 100.00

2.872 2.872 (0.319) 52 472344 0.00- 30.00 26.81

9 Vinyl Chloride

CAS #: 75-01-4

3.308 3.308 (0.367) 62 942169 26.2804 26.280 80.00- 120.00 100.00

3.308 3.308 (0.367) 64 275832 0.00- 59.30 29.28

10 1,3-Butadiene

CAS #: 106-99-0

3.412 3.430 (0.379) 54 1026898 26.4077 26.408 80.00- 120.00 100.00

3.412 3.430 (0.379) 39 1213555 0.00- 30.00 118.18

11 Bromomethane

CAS #: 74-83-9

4.350 4.351 (0.483) 94 443255 25.1444 25.144 80.00- 120.00 100.00

4.350 4.351 (0.483) 96 414346 60.71- 120.71 93.48

13 Chloroethane

CAS #: 75-00-3

4.723 4.724 (0.525) 64 349971 26.1417 26.142 80.00- 120.00 100.00

4.723 4.724 (0.525) 49 153532 0.00- 30.00 43.87

4.723 4.724 (0.525) 66 107188 0.00- 30.00 30.63

16 Trichlorofluoromethane/Fr11

CAS #: 75-69-4

5.304 5.304 (0.589) 101 3003732 25.7496 25.750 80.00- 120.00 100.00

5.304 5.304 (0.589) 103 1891741 34.19- 94.19 62.98

CONCENTRATIONS

ON-COL FINAL

RT EXP RT (REL RT) MASS RESPONSE ( PPBV) ( PPBV) TARGET RANGE RATIO  
 == == ===== == ===== ===== =====

17 Ethanol CAS #: 64-17-5  
 6.225 6.225 (0.692) 45 476247 21.9692 21.969 80.00- 120.00 100.00  
 6.225 6.225 (0.692) 43 104284 0.00- 30.00 21.90  
 6.225 6.225 (0.692) 46 179838 0.00- 30.00 37.76

19 Freon 113 CAS #: 76-13-1  
 6.390 6.390 (0.710) 151 1046721 24.0434 24.043 80.00- 120.00 100.00  
 6.390 6.390 (0.710) 153 653983 34.59- 94.59 62.48  
 6.390 6.390 (0.710) 101 1480628 0.00- 30.00 141.45

18 1,1-Dichloroethene CAS #: 75-35-4  
 6.335 6.335 (0.704) 98 483690 25.9833 25.983 80.00- 120.00 100.00  
 6.335 6.335 (0.704) 61 2202167 0.00- 30.00 455.28  
 6.335 6.335 (0.704) 96 768499 0.00- 30.00 158.88

21 Acetone CAS #: 67-64-1  
 6.637 6.637 (0.737) 43 2889529 24.9258 24.926 80.00- 120.00 100.00  
 6.637 6.637 (0.737) 58 602466 0.00- 30.00 20.85

24 2-Propanol CAS #: 67-63-0  
 7.049 7.049 (0.783) 45 3014690 25.9497 25.950 80.00- 120.00 100.00  
 7.049 7.049 (0.783) 43 652790 0.00- 30.00 21.65  
 7.049 7.049 (0.783) 59 84407 0.00- 30.00 2.80

25 3-Chloroprene CAS #: 107-05-1  
 6.994 6.994 (0.777) 76 350654 24.3475 24.348 80.00- 120.00 100.00  
 6.994 6.994 (0.777) 41 2584007 0.00- 30.00 736.91

20 Carbon Disulfide CAS #: 75-15-0  
 6.500 6.500 (0.722) 76 2341567 23.9519 23.952 80.00- 120.00 100.00

28 Methylene Chloride CAS #: 75-09-2  
 7.213 7.213 (0.801) 84 597250 22.4257 22.426 80.00- 120.00 100.00  
 7.213 7.213 (0.801) 49 1886984 285.40- 345.40 315.95  
 7.213 7.213 (0.801) 51 543174 0.00- 30.00 90.95

29 MTBE CAS #: 1634-04-4  
 7.515 7.515 (0.835) 73 2486183 23.9518 23.952 80.00- 120.00 100.00  
 7.543 7.515 (0.838) 57 1199065 0.00- 30.00 48.23  
 7.543 7.543 (0.838) 41 2015802 0.00- 30.00 81.08

30 trans-1,2-Dichloroethene CAS #: 156-60-5  
 7.515 7.515 (0.835) 98 462640 18.4857 18.486 80.00- 120.00 100.00  
 7.515 7.515 (0.835) 61 1955518 0.00- 30.00 422.69  
 7.515 7.515 (0.835) 96 729919 0.00- 30.00 157.77

CONCENTRATIONS

ON-COL FINAL

RT	EXP RT (REL RT)	MASS	RESPONSE	( PPEV)	( PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====

32 Hexane						CAS #: 110-54-3		
7.790	7.790 (0.865)	57	2483667	27.9816	27.982	80.00- 120.00	100.00	
7.790	7.790 (0.865)	43	2204750			0.00- 30.00	88.77	
7.790	7.790 (0.865)	86	257010			0.00- 30.00	10.35	

35 Vinyl Acetate						CAS #: 108-05-4		
8.174	8.174 (0.908)	43	5171799	27.5406	27.541	80.00- 120.00	100.00	
8.174	8.174 (0.908)	42	442491			0.00- 30.00	8.56	
8.174	8.174 (0.908)	86	240321			0.00- 30.00	4.65	

33 1,1-Dichloroethane						CAS #: 75-34-3		
8.092	8.092 (0.899)	63	2380268	26.1403	26.140	80.00- 120.00	100.00	
8.092	8.092 (0.899)	65	711877			0.00- 59.66	29.91	

37 2-Butanone						CAS #: 78-93-3		
8.792	8.792 (0.977)	72	577083	25.9086	25.908	80.00- 120.00	100.00	
8.792	8.792 (0.977)	43	4405264			728.42- 788.42	763.37	
8.792	8.792 (0.977)	57	262217			0.00- 30.00	45.44	

36 cis-1,2-Dichloroethene						CAS #: 156-59-2		
8.747	8.748 (0.972)	98	670620	25.3188	25.319	80.00- 120.00	100.00	
8.747	8.748 (0.972)	61	1929466			256.63- 316.63	287.71	
8.747	8.748 (0.972)	96	1054743			126.65- 186.65	157.28	

38 Tetrahydrofuran						CAS #: 109-99-9		
9.002	9.002 (1.000)	42	2613252	27.5642	27.564	80.00- 120.00	100.00	
9.002	9.002 (1.000)	71	529660			0.00- 30.00	20.27	
9.002	9.002 (1.000)	72	556540			0.00- 30.00	21.30	

40 Chloroform						CAS #: 67-66-3		
9.099	9.099 (1.011)	83	2349912	24.9627	24.963	80.00- 120.00	100.00	
9.099	9.099 (1.011)	85	1499349			33.49- 93.49	63.80	

42 1,1,1-Trichloroethane						CAS #: 71-55-6		
9.229	9.229 (1.025)	97	2416596	25.0030	25.003	80.00- 120.00	100.00	
9.229	9.229 (1.025)	99	1562170			33.36- 93.36	64.64	

41 Cyclohexane						CAS #: 110-82-7		
9.197	9.197 (1.022)	84	1606951	25.1764	25.176	80.00- 120.00	100.00	
9.197	9.197 (1.022)	56	2877185			0.00- 30.00	179.05	
9.197	9.197 (1.022)	41	2080281			0.00- 30.00	129.46	

44 Carbon Tetrachloride						CAS #: 56-23-5		
9.359	9.359 (1.040)	119	2383885	27.0161	27.016	80.00- 120.00	100.00	
9.359	9.359 (1.040)	117	2464842			73.28- 133.28	103.40	

CONCENTRATIONS										
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO		
==	=====	=====	=====	=====	=====	=====	=====	=====		
-----										
45	2,2,4-Trimethylpentane					CAS #: 540-84-1				
9.638	9.639	(1.071)	56	2600831	26.0773	26.077	80.00-	120.00	100.00	
9.638	9.639	(1.071)	99	291627			0.00-	30.00	11.21	
9.638	9.639	(1.071)	41	2774659			0.00-	30.00	106.68	
-----										
46	Benzene					CAS #: 71-43-2				
9.638	9.639	(0.946)	78	3481131	25.7014	25.701	80.00-	120.00	100.00	
9.638	9.639	(0.946)	77	819638			0.00-	30.00	23.55	
-----										
48	1,2-Dichloroethane					CAS #: 107-06-2				
9.755	9.755	(0.958)	62	2217546	26.7379	26.738	80.00-	120.00	100.00	
9.755	9.755	(0.958)	64	675203			0.00-	30.00	30.45	
-----										
49	Heptane					CAS #: 142-82-5				
9.871	9.872	(0.969)	43	4254635	29.3258	29.326	80.00-	120.00	100.00	
9.871	9.872	(0.969)	57	1686216			0.00-	30.00	39.63	
9.871	9.872	(0.969)	100	361239			0.00-	30.00	8.49	
-----										
52	Trichloroethene					CAS #: 79-01-6				
10.475	10.475	(1.028)	130	1380191	24.8628	24.863	80.00-	120.00	100.00	
10.475	10.475	(1.028)	95	1496093			0.00-	30.00	108.40	
10.475	10.475	(1.028)	97	966118			0.00-	30.00	70.00	
-----										
53	1,2-Dichloropropane					CAS #: 78-87-5				
10.861	10.861	(1.066)	63	1592027	26.4921	26.492	80.00-	120.00	100.00	
10.861	10.861	(1.066)	62	1123559			41.54-	101.54	70.57	
10.861	10.861	(1.066)	41	1431096			60.81-	120.81	89.89	
-----										
54	1,4-Dioxane					CAS #: 123-91-1				
11.029	11.029	(1.083)	88	778537	25.3682	25.368	80.00-	120.00	100.00	
11.029	11.029	(1.083)	58	802295			70.67-	130.67	103.05	
11.029	11.029	(1.083)	57	268255			0.00-	30.00	34.46	
-----										
55	Bromodichloromethane					CAS #: 75-27-4				
11.270	11.270	(1.106)	83	2604473	26.7355	26.736	80.00-	120.00	100.00	
11.270	11.270	(1.106)	85	1608397			31.56-	91.56	61.76	
-----										
56	cis-1,3-Dichloropropene					CAS #: 10061-01-5				
12.089	12.090	(1.187)	75	1904531	26.5294	26.529	80.00-	120.00	100.00	
12.089	12.090	(1.187)	77	601364			1.67-	61.67	31.58	
12.089	12.090	(1.187)	39	1762034			61.82-	121.82	92.52	
-----										
58	4-Methyl-2-pentanone					CAS #: 108-10-1				
12.379	12.379	(1.215)	43	5407883	28.6170	28.617	80.00-	120.00	100.00	
12.379	12.379	(1.215)	58	1507284			0.00-	30.00	27.87	
12.379	12.379	(1.215)	85	455641			0.00-	30.00	8.43	
-----										

CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	ON-COL		FINAL	TARGET RANGE	RATIO	
				RESPONSE	( PPEV)	( PPBV)			
==	=====	=====	=====	=====	=====	=====	=====	=====	=====
-----									
60 Toluene						CAS #: 108-88-3			
12.644	12.644	(1.241)	91	4338089	27.2655	27.265	80.00-	120.00	100.00
12.644	12.644	(1.241)	92	2534392			28.22-	88.22	58.42
-----									
61 trans-1,3-Dichloropropene						CAS #: 10061-02-6			
13.308	13.308	(0.869)	75	2098133	26.8081	26.808	80.00-	120.00	100.00
13.308	13.308	(0.869)	77	672055			1.62-	61.62	32.03
13.308	13.308	(0.869)	39	1762149			54.99-	114.99	83.99
-----									
63 1,1,2-Trichloroethane						CAS #: 79-00-5			
13.665	13.665	(0.892)	97	1456520	25.4434	25.443	80.00-	120.00	100.00
13.665	13.665	(0.892)	99	911073			31.59-	91.59	62.55
13.665	13.665	(0.892)	83	1330364			59.27-	119.27	91.34
-----									
64 Tetrachloroethene						CAS #: 127-18-4			
13.747	13.747	(0.897)	166	1905075	25.8195	25.820	80.00-	120.00	100.00
13.747	13.747	(0.897)	129	1447509			47.26-	107.26	75.98
13.747	13.747	(0.897)	131	1396055			45.00-	105.00	73.28
-----									
67 2-Hexanone						CAS #: 591-78-6			
14.132	14.132	(0.922)	58	2190827	28.7784	28.778	80.00-	120.00	100.00
14.132	14.132	(0.922)	43	5585215			228.06-	288.06	254.94
14.132	14.132	(0.922)	100	290729			0.00-	30.00	13.27
-----									
68 Dibromochloromethane						CAS #: 124-48-1			
14.352	14.352	(0.937)	129	2451003	26.7174	26.717	80.00-	120.00	100.00
14.352	14.352	(0.937)	208	124401			0.00-	30.00	5.08
-----									
69 1,2-Dibromoethane						CAS #: 106-93-4			
14.516	14.517	(0.948)	107	630655	24.5499	24.550	80.00-	120.00	100.00
14.516	14.517	(0.948)	109	570311			62.45-	122.45	90.43
-----									
73 Chlorobenzene						CAS #: 108-90-7			
15.370	15.370	(1.003)	112	3653099	25.2226	25.223	80.00-	120.00	100.00
15.370	15.370	(1.003)	114	1165078			1.82-	61.82	31.89
15.370	15.370	(1.003)	77	2346420			33.07-	93.07	64.23
-----									
74 Ethyl Benzene						CAS #: 100-41-4			
15.525	15.525	(1.013)	106	1949067	25.9485	25.948	80.00-	120.00	100.00
15.525	15.525	(1.013)	91	6287665			0.00-	30.00	322.60
-----									
75 m,p-Xylene						CAS #: 108-38-3			
15.731	15.731	(1.027)	106	2448555	26.5531	26.553	80.00-	120.00	100.00
15.731	15.731	(1.027)	91	5070846			0.00-	30.00	207.10
-----									
77 o-Xylene						CAS #: 95-47-6			
16.376	16.376	(1.069)	106	2336236	26.9740	26.974	80.00-	120.00	100.00



CONCENTRATIONS									
RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO	
==	=====	=====	=====	=====	=====	=====	=====	=====	
77 o-Xylene (continued)									
16.376	16.376	(1.069)	91	5062557			186.16- 246.16	216.70	
-----									
78 Styrene CAS #: 100-42-5									
16.401	16.401	(1.071)	104	3776438	28.2008	28.201	80.00- 120.00	100.00	
16.401	16.401	(1.071)	78	2085935			25.90- 85.90	55.24	
-----									
79 Bromoform CAS #: 75-25-2									
16.711	16.711	(1.091)	173	2375131	27.2476	27.248	80.00- 120.00	100.00	
16.711	16.711	(1.091)	171	1209559			0.00- 30.00	50.93	
-----									
80 Cumene CAS #: 98-82-8									
16.917	16.917	(1.104)	105	7090036	28.8550	28.855	80.00- 120.00	100.00	
16.917	16.917	(1.104)	120	1829987			0.00- 56.37	25.81	
-----									
82 1,1,2,2-Tetrachloroethane CAS #: 79-34-5									
17.484	17.484	(1.141)	83	3929563	26.1228	26.123	80.00- 120.00	100.00	
17.484	17.484	(1.141)	85	2455680			33.13- 93.13	62.49	
-----									
83 Propylbenzene CAS #: 103-65-1									
17.536	17.536	(1.145)	91	9168518	28.2011	28.201	80.00- 120.00	100.00	
17.536	17.536	(1.145)	120	1991547			0.00- 30.00	21.72	
-----									
84 4-Ethyltoluene CAS #: 622-96-8									
17.716	17.716	(1.157)	105	7550067	28.3170	28.317	80.00- 120.00	100.00	
17.716	17.716	(1.157)	120	2222799			0.00- 59.32	29.44	
-----									
85 1,3,5-Trimethylbenzene CAS #: 108-67-8									
17.820	17.820	(1.163)	105	6142831	27.3224	27.322	80.00- 120.00	100.00	
17.820	17.820	(1.163)	120	2888890			16.67- 76.67	47.03	
-----									
87 1,2,4-Trimethylbenzene CAS #: 95-63-6									
18.413	18.413	(1.202)	105	5996625	28.4111	28.411	80.00- 120.00	100.00	
18.413	18.413	(1.202)	120	2602133			14.24- 74.24	43.39	
-----									
89 1,3-Dichlorobenzene CAS #: 541-73-1									
18.929	18.929	(1.236)	146	3784913	26.3197	26.320	80.00- 120.00	100.00	
18.929	18.929	(1.236)	148	2394124			0.00- 30.00	63.25	
18.929	18.929	(1.236)	111	1648587			0.00- 30.00	43.56	
-----									
90 1,4-Dichlorobenzene CAS #: 106-46-7									
19.083	19.083	(1.246)	146	3823816	25.6658	25.666	80.00- 120.00	100.00	
19.083	19.083	(1.246)	148	2411018			0.00- 30.00	63.05	
19.083	19.083	(1.246)	111	1634330			0.00- 30.00	42.74	
-----									
91 alpha-Chlorotoluene CAS #: 100-44-7									
19.315	19.316	(1.261)	91	5373408	28.7285	28.728	80.00- 120.00	100.00	

CONCENTRATIONS

RT	EXP RT	(REL RT)	MASS	RESPONSE	ON-COL (PPEV)	FINAL (PPBV)	TARGET RANGE	RATIO
==	=====	=====	=====	=====	=====	=====	=====	=====
91 alpha-Chlorotoluene (continued)								
19.315	19.316	(1.261)	126	1024073			0.00- 30.00	19.06
-----								
94 1,2-Dichlorobenzene CAS #: 95-50-1								
19.625	19.625	(1.281)	146	3537479	25.5844	25.584	80.00- 120.00	100.00
19.625	19.625	(1.281)	148	2245778			33.40- 93.40	63.49
19.625	19.625	(1.281)	111	1618981			14.98- 74.98	45.77
-----								
96 1,2,4-Trichlorobenzene CAS #: 120-82-1								
21.430	21.430	(1.399)	180	3237710	29.6000	29.600	80.00- 120.00	100.00
21.430	21.430	(1.399)	182	3100974			66.25- 126.25	95.78
-----								
97 Hexachlorobutadiene CAS #: 87-68-3								
21.559	21.559	(1.407)	225	2520403	26.8332	26.833	80.00- 120.00	100.00
21.559	21.559	(1.407)	223	1592585			0.00- 30.00	63.19
-----								
98 Naphthalene CAS #: 91-20-3								
21.688	21.688	(1.416)	128	7007927	31.6789	31.679	80.00- 120.00	100.00
21.688	21.688	(1.416)	127	883164			0.00- 30.00	12.60
-----								
183 Butane CAS #: 106-97-8								
3.221	3.221	(0.358)	58	213948	27.7889	27.789	80.00- 120.00	100.00
3.221	3.221	(0.358)	43	2277013			0.00- 30.00	1064.28
-----								
14 Isopentane CAS #: 78-78-4								
4.848	4.827	(0.539)	57	1069315	27.4986	27.499	80.00- 120.00	100.00
4.848	4.827	(0.539)	43	2068119			0.00- 30.00	193.41
4.827	4.827	(0.536)	42	1787070			0.00- 30.00	167.12
-----								
2 Methylcyclohexane CAS #: 108-87-2								
10.644	10.644	(1.182)	83	2235801	25.2453	25.245	80.00- 120.00	100.00
10.644	10.644	(1.182)	98	991840			0.00- 30.00	44.36
10.644	10.644	(1.182)	55	2771672			0.00- 30.00	123.97
-----								
179 tert-Butyl Alcohol CAS #: 75-65-0								
7.570	7.570	(0.841)	59	2607868	27.2084	27.208	80.00- 120.00	100.00
7.543	7.543	(0.838)	41	2015802			0.00- 30.00	77.30
7.543	7.515	(0.838)	57	1199065			0.00- 30.00	45.98
-----								

Report Date: 04-Aug-2008 11:04

Air Toxics Ltd.

INTERNAL STANDARD COMPOUNDS  
AREA AND RT SUMMARY

Instrument ID: msdg.i

Calibration Date: 04-AUG-2008

Lab File ID: g080403.d

Calibration Time: 09:59

Lab Smp Id: LCS-1

Client Smp ID: LCS-1

Analysis Type: VOA

Level: LOW

Quant Type: ISTD

Sample Type: AIR

Operator: lmr

Method File: /var/chem/msdg.i/04Aug2008.b/t14q702a.m

Misc Info: 50ppbv -&gt; 25ppbv

COMPOUND	STANDARD	AREA LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	318312	190987	445637	310013	-2.61
51 1,4-Difluorobenze	1208514	725108	1691920	1174713	-2.80
72 Chlorobenzene-d5	1189759	713855	1665663	1085504	-8.76

COMPOUND	STANDARD	RT LIMIT		SAMPLE	%DIFF
		LOWER	UPPER		
39 Bromochloromethan	9.00	8.67	9.33	9.00	0.00
51 1,4-Difluorobenze	10.19	9.86	10.52	10.19	0.00
72 Chlorobenzene-d5	15.32	14.99	15.65	15.32	0.00

AREA UPPER LIMIT = + 40% of internal standard area.

AREA LOWER LIMIT = - 40% of internal standard area.

RT UPPER LIMIT = + 0.33 minutes of internal standard RT.

RT LOWER LIMIT = - 0.33 minutes of internal standard RT.

Date : 04-AUG-2008 10:52

Client ID: LCS-1


Instrument: msdg.i

Sample Info: 250ml #1541-227;LCS-1;LCS-1

Operator: lmr

Column phase: RTX-624

Column diameter: 0.32

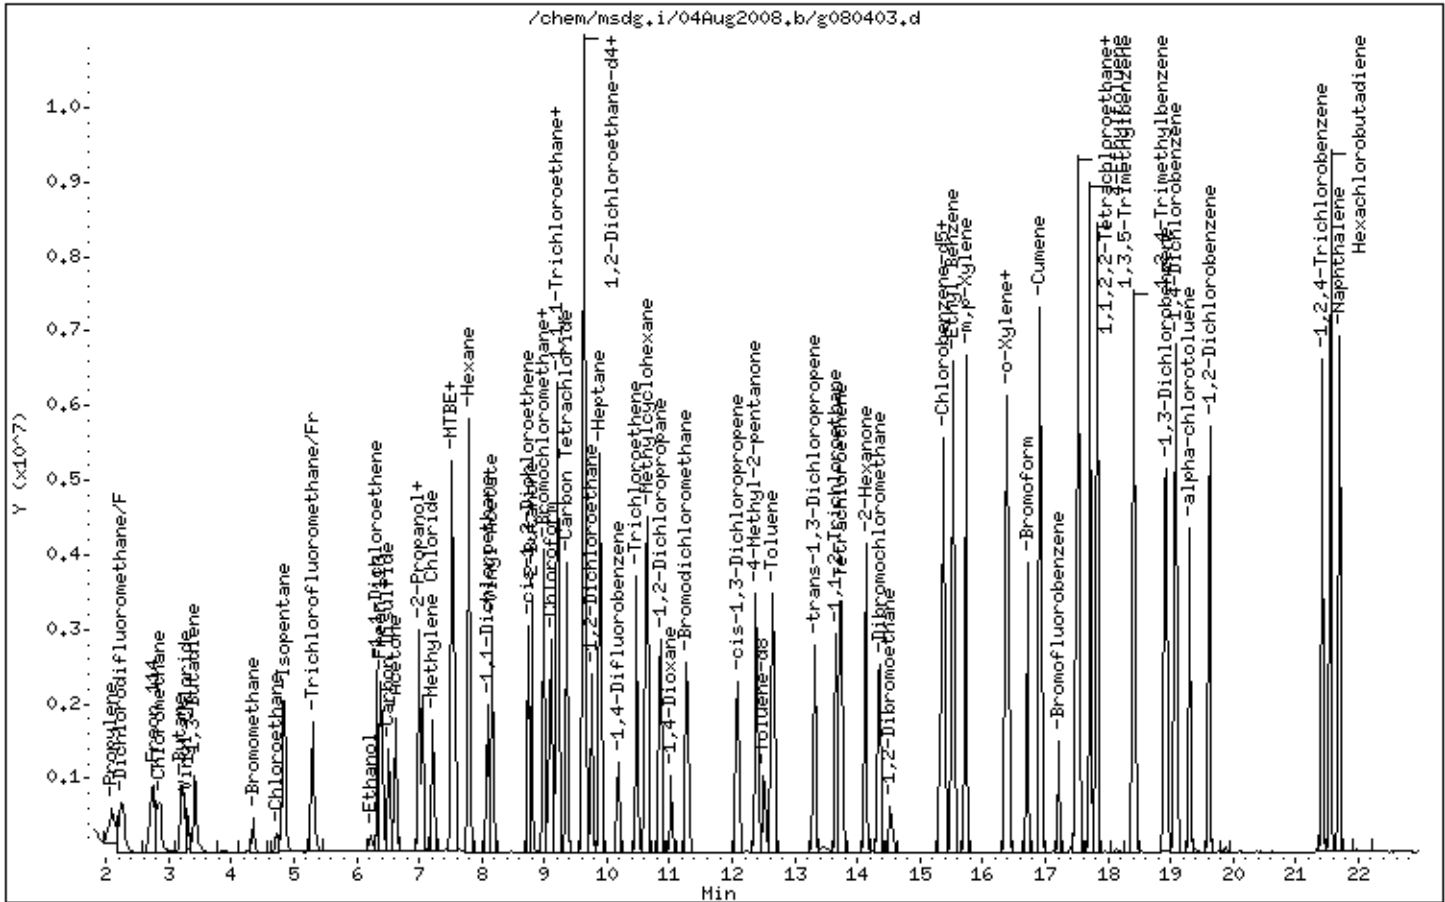

m/z	ION ABUNDANCE CRITERIA	% REL. ABUNDANCE
50	15.0 - 40.0% of mass 95	32.28
75	30.0 - 60.0% of mass 95	52.37
95	Base peak, 100.00% relative abundance	100.00
96	5.0 - 9.0% of mass 95	10.50
173	Less than 2.0% of mass 174	(0.25) <sup>1</sup>
174	Greater than 50.0% of mass 95	65.60
175	5.0 - 9.0% of mass 174	(7.10) <sup>1</sup>
176	Greater than 95.0% but less than 101.0% of mass 174	(95.49) <sup>1</sup>
177	5.0 - 9.0% of mass 176	(6.60) <sup>2</sup>

BFB Injection Date: 8/14/08

BFB Injection Time: 9:12 a

BFB File ID: 0807417-01A

Tekmar Purge Flow: \_\_\_\_\_

Vacuum: 6.10 x 10<sup>-6</sup>

ISIS Std #: <u>1612-77</u>	Exp. Date: <u>10/12/08</u>
BCM: <u>314512</u>	
1,4-DFB: <u>1208314</u>	
CB-d5: <u>1189759</u>	

Verified CVV IS vs ICAL mid-point (-40% $\Delta$ ) 12

1 - value in parenthesis is % mass 174

2 - value in parenthesis is % mass 176

Verify 176/174 m/z Ratio: 420224/440021 x 100 = 95.49

NOAH Cart #: NA File #: MT

Calculation Check:

ppbv of compound =  $\frac{\text{Area}_{\text{Sample}}}{\text{Area}_{\text{Std}}} \times \frac{\text{Conc.}_{\text{Std}}}{\text{RRF}} = \frac{(1324507)}{(1208514)} \times \frac{(10.0)}{(13377)} = 10.602$

Reported Result 10.602

File ID: 2080403

Compound: Tol-d8

Initials: 12

Use	File #	Sample / Client Name	Cart #	Pressure	Amt Loaded	DF	Date Analyzed	Time Analyzed	Review Init.	Comments
1	<u>2080401</u>	<u>BFB Time Check</u>	<u>1324507</u>	<u>50m</u>	<u>2ml</u>	<u>100</u>	<u>8/14/08</u>	<u>0929</u>	<u>12</u>	
2	<u>02</u>	<u>CU-1 (25ppb)</u>	<u>1541-1041</u>	<u>25ppb</u>	<u>500ml</u>			<u>0951</u>	<u>12</u>	
3	<u>03</u>	<u>LCS-1 (50ppb)</u>	<u>1541-327</u>	<u>↓</u>	<u>250ml</u>			<u>1052</u>	<u>12</u>	
4	<u>X</u>	<u>SYSTEM BLANK</u>	<u>-</u>	<u>dry</u>	<u>500ml</u>			<u>1145</u>	<u>12</u>	
5	<u>v</u>	<u>lab BLANK</u>	<u>25346</u>	<u>Manual</u>	<u>↓</u>	<u>↓</u>		<u>1246</u>	<u>12</u>	
6	<u>v</u>	<u>0807494 - 01A</u>	<u>34022</u>	<u>75% 500ml</u>	<u>500ml</u>	<u>179</u>		<u>1339</u>	<u>12</u>	
7	<u>v</u>	<u>07</u>	<u>24234</u>	<u>20% 500ml</u>	<u>↓</u>	<u>183</u>		<u>1426</u>	<u>12</u>	
8	<u>v</u>	<u>0807483 - 01A</u>	<u>14917</u>	<u>20% 500ml</u>	<u>500ml</u>	<u>216</u>		<u>1504</u>	<u>12</u>	
9	<u>v</u>	<u>0807417 - 01A</u>	<u>1077</u>	<u>60% 500ml</u>	<u>500ml</u>	<u>183</u>		<u>1504</u>	<u>12</u>	

Signature

Date

Report Date: 02-Jul-2008 07:51

Air Toxics Ltd.

Data file : /chem/msdg.i/02Jul2008.b/g070201.d  
 Lab Smp Id: BFB Client Smp ID: BFB  
 Inj Date : 02-JUL-2008 08:02  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 2uL #1476-431;BFB Tune Check;BFB Tune Check  
 Misc Info : 50ng  
 Comment :  
 Method : /chem/msdg.i/02Jul2008.b/bfb30.m  
 Meth Date : 26-Feb-2008 11:31 tsanfel Quant Type: ESTD  
 Cal Date : Cal File:  
 Als bottle: 1 QC Sample: BFB  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: all.sub  
 Target Version: 3.50 Sample Matrix: WATER  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* Uf \* Vf \* Vi \* CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE ( ug/L) ( ug/L) TARGET RANGE RATIO

RT	EXP RT	DLT RT	MASS	RESPONSE ( ug/L)	( ug/L)	TARGET RANGE	RATIO
1 bfb						CAS #: 460-00-4	
3.758	3.806	-0.048	95	672384		100.00- 100.00	100.00
3.758	3.806	-0.048	50	212008		15.00- 40.00	31.53
3.758	3.806	-0.048	75	353664		30.00- 60.00	52.60
3.758	3.806	-0.048	96	44803		5.00- 9.00	6.66
3.758	3.806	-0.048	173	3801		0.00- 2.00	0.81
3.758	3.806	-0.048	174	466624		50.00- 100.00	69.40
3.758	3.806	-0.048	175	32957		5.00- 9.00	7.06
3.758	3.806	-0.048	176	453845		95.00- 101.00	97.26
3.758	3.806	-0.048	177	29416		5.00- 9.00	6.48

Date : 02-JUL-2008 08:02

Client ID: BFB

Instrument: msdg.i


Sample Info: 2uL #1476-431;BFB Tune Check;BFB Tune Check

Volume Injected (uL): 1.0

Operator: lmr

Column phase:

Column diameter: 2.00

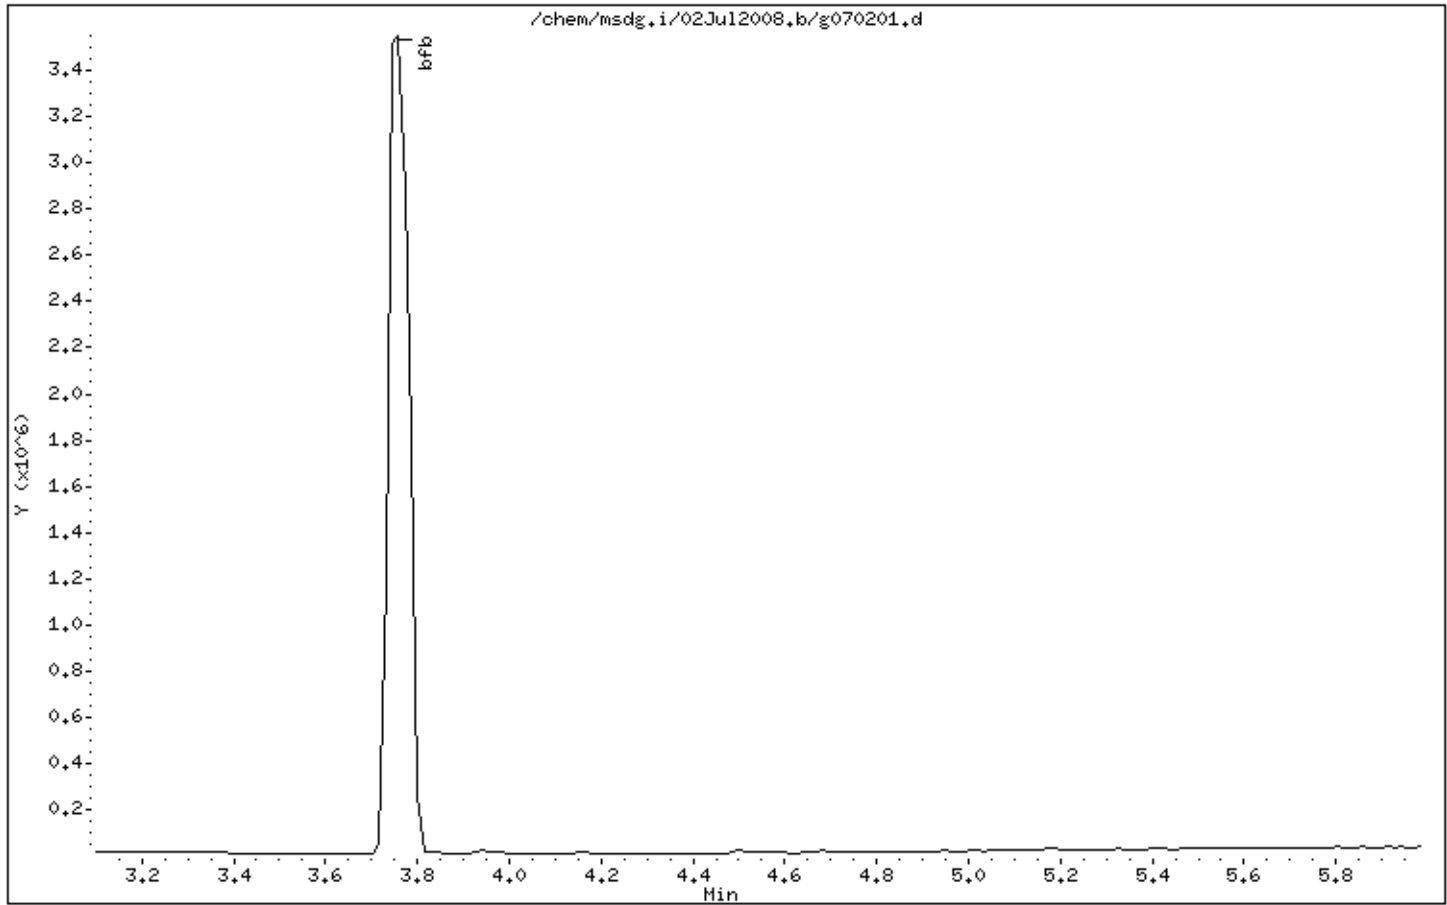

Date : 02-JUL-2008 08:02

Client ID: BFB

Instrument: msdg.i

Sample Info: 2uL #1476-431;BFB Tune Check;BFB Tune Check


Volume Injected (uL): 1.0

Operator: lmr

Column phase:

Column diameter: 2.00

1 bfb

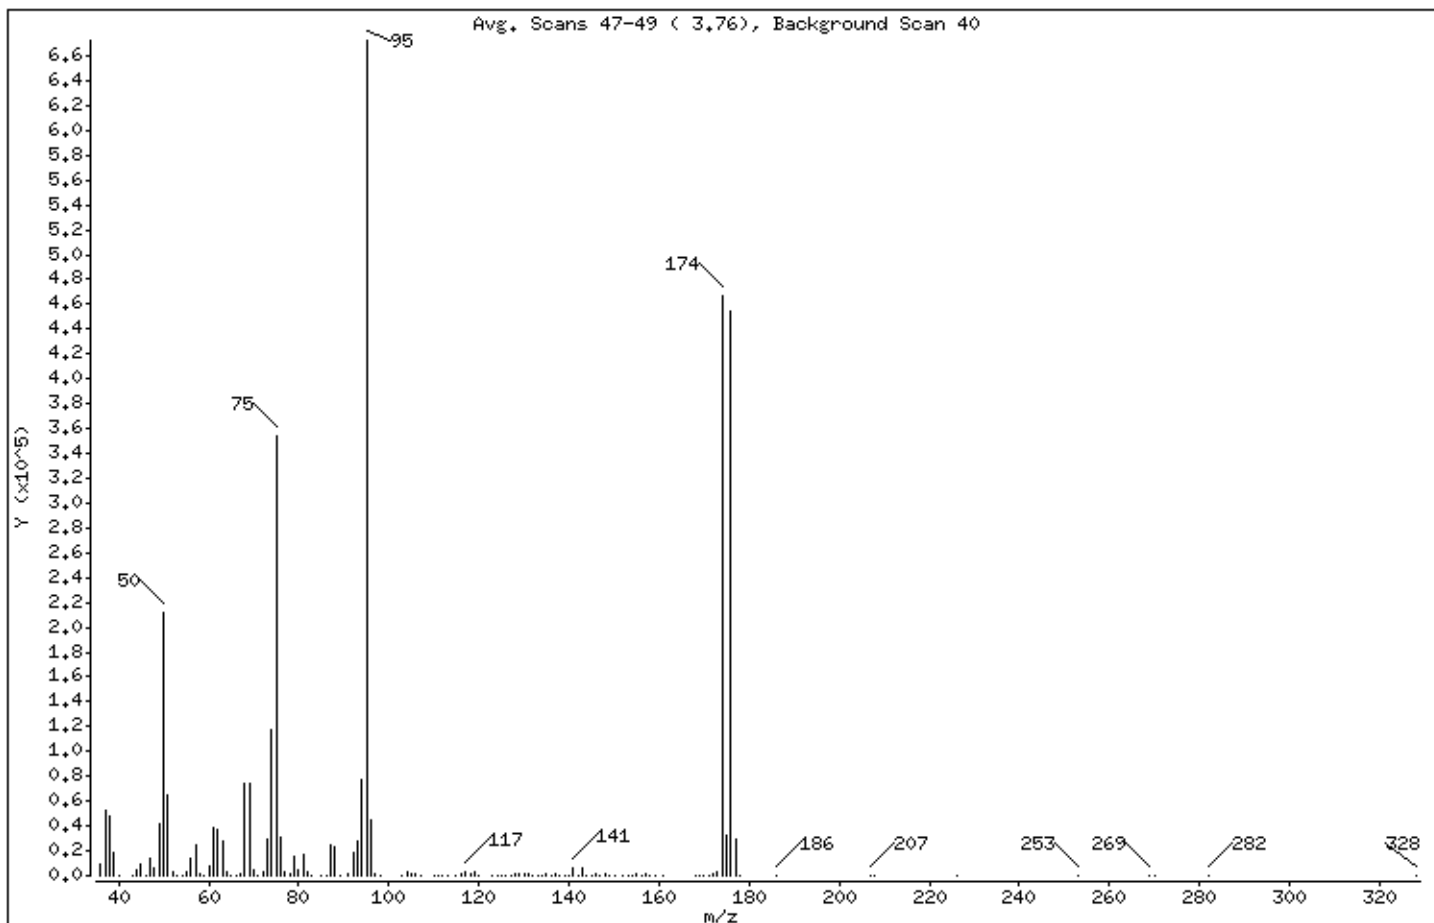

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	31.53
75	30.00 - 60.00% of mass 95	52.60
96	5.00 - 9.00% of mass 95	6.66
173	Less than 2.00% of mass 174	0.57 ( 0.81)
174	50.00 - 100.00% of mass 95	69.40
175	5.00 - 9.00% of mass 174	4.90 ( 7.06)
176	95.00 - 101.00% of mass 174	67.50 ( 97.26)
177	5.00 - 9.00% of mass 176	4.37 ( 6.48)



Date : 02-JUL-2008 08:02

Client ID: BFB

Instrument: msdg.i

Sample Info: 2uL #1476-431;BFB Tune Check;BFB Tune Check

Volume Injected (uL): 1.0

Operator: lmr

Column phase:

Column diameter: 2.00

Data File: g070201.d

Spectrum: Avg. Scans 47-49 ( 3.76), Background Scan 40

Location of Maximum: 95.00

Number of points: 131

m/z	Y	m/z	Y	m/z	Y	m/z	Y
36.00	8842	71.00	187	112.00	405	148.00	1369
37.00	51960	72.00	3260	113.00	495	149.00	326
38.00	47424	73.00	29280	115.00	639	150.00	633
39.00	18984	74.00	117600	116.00	1882	152.00	296
40.00	373	75.00	353664	117.00	3783	153.00	496
43.00	206	76.00	30240	118.00	2283	154.00	304
44.00	4835	77.00	3785	119.00	2902	155.00	1335
45.00	9537	78.00	2035	120.00	34	156.00	411
46.00	618	79.00	15696	123.00	219	157.00	952
47.00	14246	80.00	4917	124.00	369	158.00	348
48.00	5938	81.00	16248	125.00	194	159.00	577
49.00	42488	82.00	3169	126.00	333	161.00	655
50.00	211968	83.00	439	127.00	239	168.00	43
51.00	64504	85.00	46	128.00	2079	169.00	81
52.00	2641	86.00	623	129.00	1049	170.00	145
53.00	116	87.00	24712	130.00	2095	171.00	110
54.00	60	88.00	23896	131.00	792	172.00	1106
55.00	2322	89.00	38	132.00	87	173.00	3801
56.00	13547	91.00	2258	133.00	36	174.00	466624
57.00	24064	92.00	18256	134.00	207	175.00	32952
58.00	1024	93.00	27136	135.00	943	176.00	453824
59.00	80	94.00	77168	136.00	214	177.00	29416
60.00	8136	95.00	672384	137.00	1017	178.00	755
61.00	38824	96.00	44800	138.00	145	186.00	34
62.00	37368	97.00	1598	139.00	192	207.00	90
63.00	27400	98.00	45	140.00	368	208.00	74
64.00	2853	103.00	290	141.00	5691	226.00	71
65.00	601	104.00	2528	142.00	679	253.00	35
66.00	36	105.00	854	143.00	5553	269.00	98
67.00	1474	106.00	2179	144.00	463	270.00	42
68.00	73624	107.00	552	145.00	492	282.00	37
69.00	73568	110.00	436	146.00	828	328.00	40
70.00	5406	111.00	606	147.00	402		

Report Date: 04-Aug-2008 09:18

Air Toxics Ltd.

Data file : /chem/msdg.i/04Aug2008.b/g080401.d  
 Lab Smp Id: BFB Client Smp ID: BFB  
 Inj Date : 04-AUG-2008 09:29  
 Operator : lmr Inst ID: msdg.i  
 Smp Info : 2uL #1476-431;BFB Tune Check;BFB Tune Check  
 Misc Info : 50ng  
 Comment :  
 Method : /chem/msdg.i/04Aug2008.b/bfb30.m  
 Meth Date : 18-Jul-2008 09:34 lrandolp Quant Type: ESTD  
 Cal Date : Cal File:  
 Als bottle: 1 QC Sample: BFB  
 Dil Factor: 1.00000  
 Integrator: HP RTE Compound Sublist: all.sub  
 Target Version: 3.50 Sample Matrix: WATER  
 Processing Host: eeyore

Concentration Formula: Amt \* DF \* Uf \* Vf \* Vi \* CpndVariable

Name	Value	Description
DF	1.00000	Dilution Factor
Uf	1.00000	ng unit correction factor
Vf	1.00000	Volumetric correction factor
Vi	1.00000	Injection Volume

Cpnd Variable Local Compound Variable

CONCENTRATIONS

ON-COL FINAL

RT EXP RT DLT RT MASS RESPONSE ( ug/L) ( ug/L) TARGET RANGE RATIO  
 == =====

RT	EXP RT	DLT RT	MASS	RESPONSE ( ug/L)	( ug/L)	TARGET RANGE	RATIO
1 bfb						CAS #: 460-00-4	
3.758	3.806	-0.048	95	670828		100.00- 100.00	100.00
3.758	3.806	-0.048	50	216538		15.00- 40.00	32.28
3.758	3.806	-0.048	75	351332		30.00- 60.00	52.37
3.758	3.806	-0.048	96	43596		5.00- 9.00	6.50
3.758	3.806	-0.048	173	3738		0.00- 2.00	0.85
3.758	3.806	-0.048	174	440085		50.00- 100.00	65.60
3.758	3.806	-0.048	175	31261		5.00- 9.00	7.10
3.758	3.806	-0.048	176	420257		95.00- 101.00	95.49
3.758	3.806	-0.048	177	27802		5.00- 9.00	6.62

Date : 04-AUG-2008 09:29

Client ID: BFB

Instrument: msdg.i


Sample Info: 2uL #1476-431;BFB Tune Check;BFB Tune Check

Volume Injected (uL): 1.0

Operator: lmr

Column phase:

Column diameter: 2.00

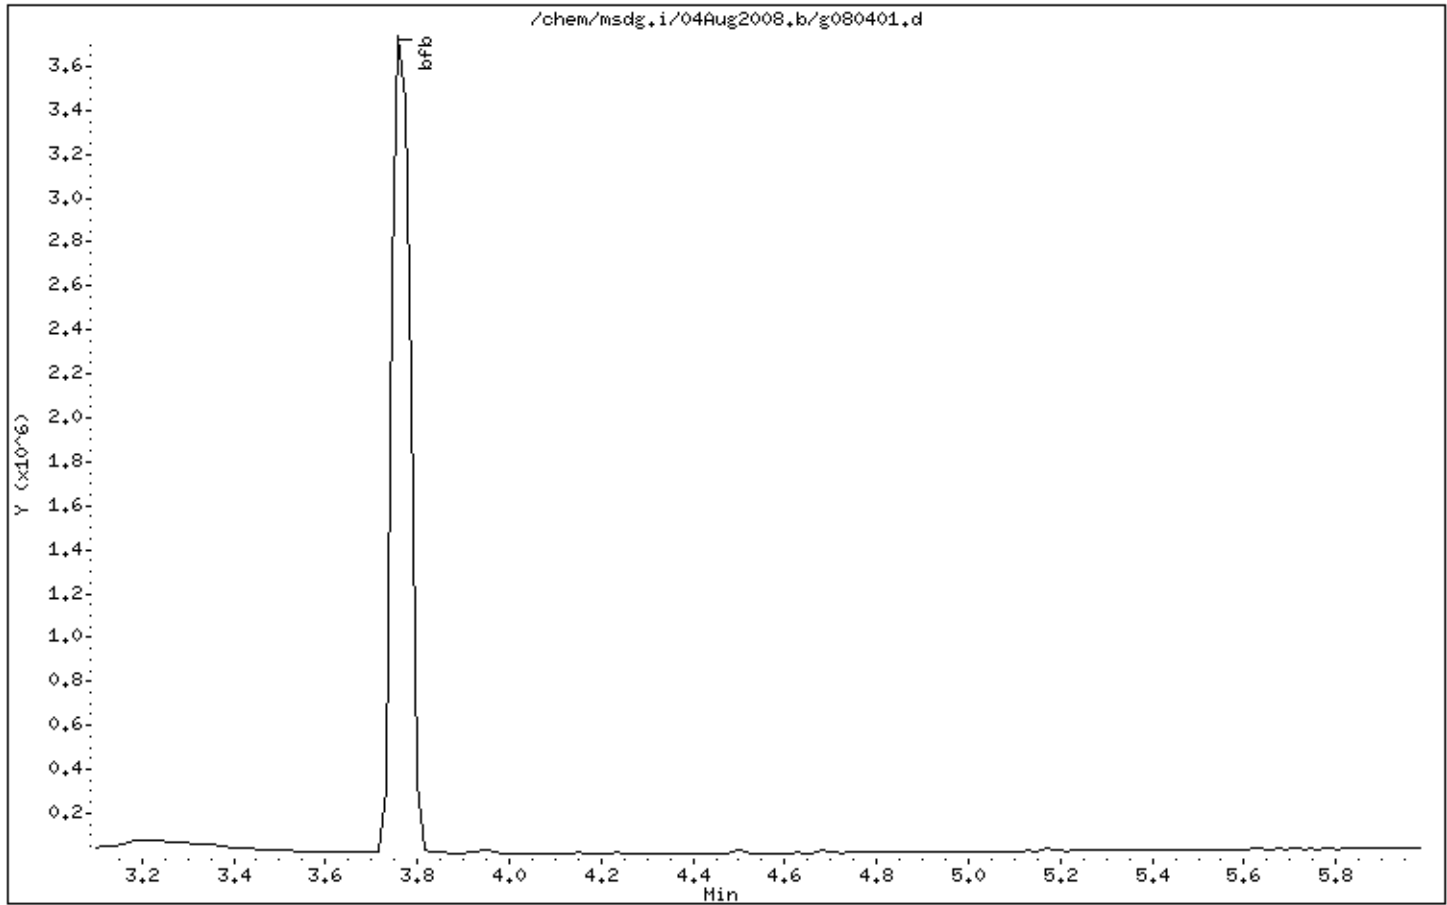

Date : 04-AUG-2008 09:29

Client ID: BFB

Instrument: msdg.i

Sample Info: 2uL #1476-431;BFB Tune Check;BFB Tune Check


Volume Injected (uL): 1.0

Operator: lmr

Column phase:

Column diameter: 2.00

1 bfb

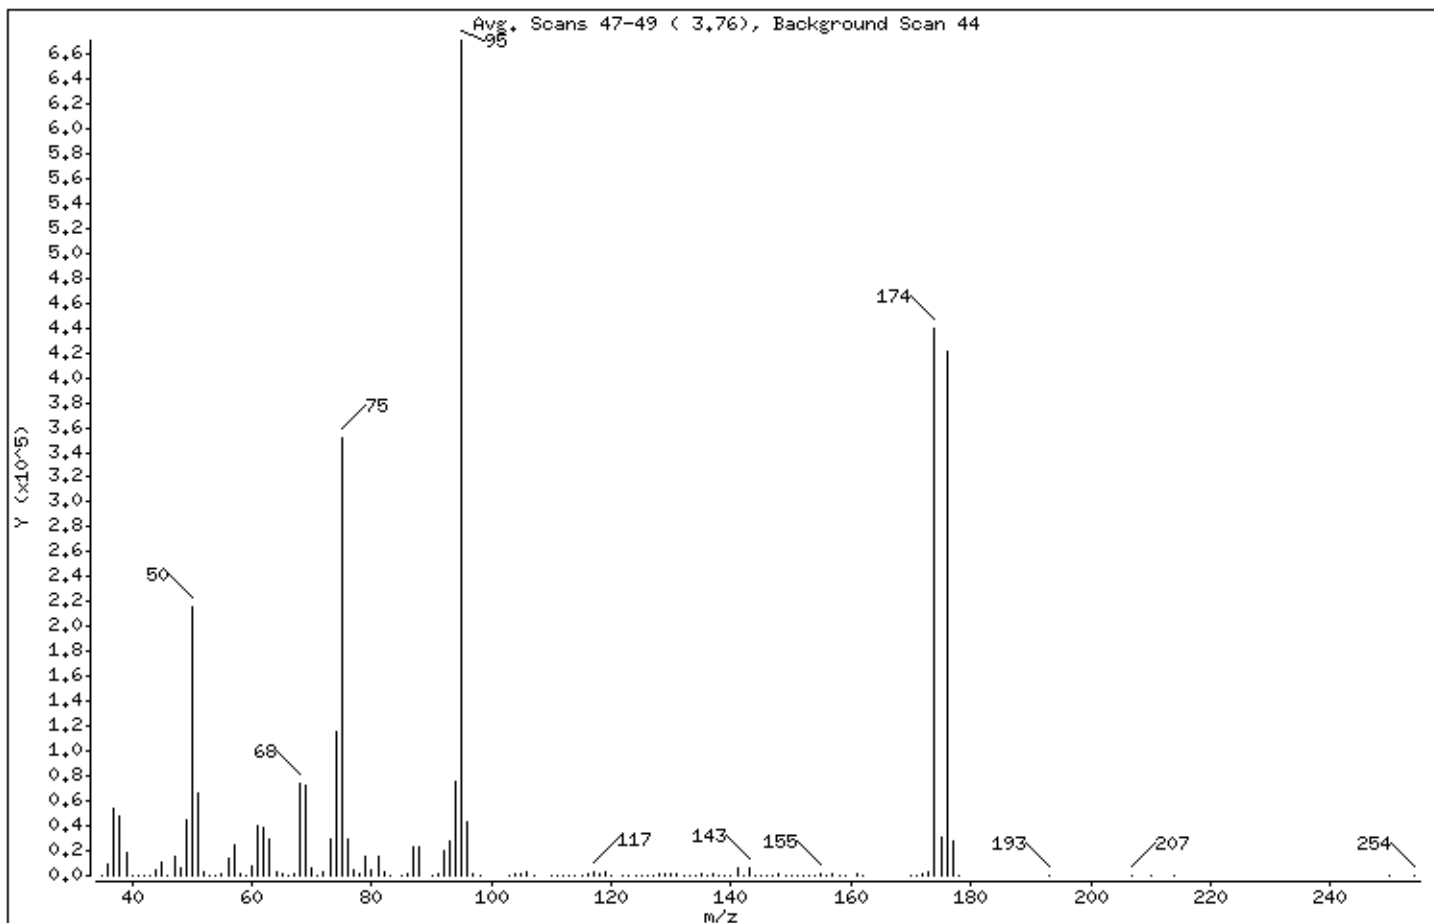

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
95	Base Peak, 100% relative abundance	100.00
50	15.00 - 40.00% of mass 95	32.28
75	30.00 - 60.00% of mass 95	52.37
96	5.00 - 9.00% of mass 95	6.50
173	Less than 2.00% of mass 174	0.56 ( 0.85)
174	50.00 - 100.00% of mass 95	65.60
175	5.00 - 9.00% of mass 174	4.66 ( 7.10)
176	95.00 - 101.00% of mass 174	62.65 ( 95.49)
177	5.00 - 9.00% of mass 176	4.14 ( 6.62)

Date : 04-AUG-2008 09:29

Client ID: BFB

Instrument: msdg.i

Sample Info: 2uL #1476-431;BFB Tune Check;BFB Tune Check

Volume Injected (uL): 1.0

Operator: lmr

Column phase:

Column diameter: 2.00

Data File: g080401.d

Spectrum: Avg. Scans 47-49 ( 3.76), Background Scan 44

Location of Maximum: 95.00

Number of points: 133

m/z	Y	m/z	Y	m/z	Y	m/z	Y
35.00	46	69.00	71896	111.00	485	146.00	703
36.00	9027	70.00	5431	112.00	277	147.00	411
37.00	53856	71.00	192	113.00	431	148.00	1289
38.00	48160	72.00	3588	114.00	41	149.00	435
39.00	18888	73.00	29552	115.00	539	150.00	517
40.00	384	74.00	116008	116.00	2094	151.00	265
41.00	144	75.00	351296	117.00	3562	152.00	374
42.00	233	76.00	29856	118.00	2146	153.00	438
43.00	204	77.00	4003	119.00	3041	154.00	342
44.00	4510	78.00	2261	120.00	351	155.00	1301
45.00	10206	79.00	15701	122.00	190	156.00	428
46.00	482	80.00	4649	123.00	99	157.00	867
47.00	15468	81.00	15582	124.00	333	158.00	265
48.00	5798	82.00	3385	125.00	236	159.00	510
49.00	44664	83.00	412	126.00	289	161.00	846
50.00	216512	85.00	37	127.00	173	162.00	86
51.00	66424	86.00	776	128.00	2117	170.00	53
52.00	2878	87.00	23888	129.00	958	171.00	384
53.00	134	88.00	22608	130.00	1982	172.00	1442
54.00	191	90.00	47	131.00	911	173.00	3738
55.00	2043	91.00	1902	132.00	40	174.00	440064
56.00	13322	92.00	19568	133.00	235	175.00	31256
57.00	24928	93.00	27280	134.00	189	176.00	420224
58.00	960	94.00	75704	135.00	1079	177.00	27800
59.00	249	95.00	670784	136.00	216	178.00	761
60.00	7326	96.00	43592	137.00	1032	193.00	74
61.00	40304	97.00	1303	138.00	33	207.00	192
62.00	38224	98.00	59	139.00	216	210.00	56
63.00	28712	103.00	304	140.00	449	214.00	46
64.00	2429	104.00	2311	141.00	5420	250.00	33
65.00	1147	105.00	1050	142.00	724	254.00	79
66.00	289	106.00	2388	143.00	5870		
67.00	1625	107.00	642	144.00	374		
68.00	74024	110.00	348	145.00	535		

## **Shipping/ Receiving Documents**



---

AN ENVIRONMENTAL ANALYTICAL LABORATORY

**180 Blue Ravine Road, Suite B  
Folsom, CA 95630**

**Phone (916) 985-1000 FAX (916) 985-1020  
Hours 8:00 A.M. to 6:00 P.M. Pacific**

COMPANY: \_\_\_\_\_ GEI Consultants, Inc.  
ATTENTION: \_\_\_\_\_ Ms. Theresa Landgraff  
FAX #: \_\_\_\_\_  
FROM: \_\_\_\_\_ Sample Receiving  
Workorder #: \_\_\_\_\_ 0807494  
# of pages (Including Cover): \_\_\_\_\_ 1

8/12/2008

Thank you for selecting Air Toxics Ltd. We have received your samples and have found no discrepancies. In order to expedite analysis and reporting, please review the attached information for accuracy. Corrections can be faxed to **Bryanna Langley at 916-985-1020**. ATL will proceed with the analysis as specified on the Chain of Custody and Sample Login page.

# AIR TOXICS LTD.

## Sample Transportation Notice

Relinquishing signature on this document indicates that sample is being shipped in compliance with all applicable local, State, Federal, national, and international laws, regulations and ordinances of any kind. Air Toxics Limited assumes no liability with respect to the collection, handling, or shipping of these samples. Relinquishing signature also indicates agreement to hold harmless, defend, and indemnify Air Toxics Limited against any claim, demand or action of any kind, related to the collection, handling, or shipping of samples. D.O.T. Hazmat (900) 457-4222

180 BLUE RAVINE ROAD, SUITE B  
FOLSOM, CA 95630-4719

(916) 985-1000 FAX: (916) 985-1020

Contact

Company **G&I Consultants, Inc.**

Address **455 Winding Brook Glassonbury CT 06033**

Phone **860-368-5300 Cell:**

**Project Info:**

P.O. #

Project # **061140-8-1703**

Project Name

**BayShore OUI Southern cell Air Monitoring**

**Turn Around Time:**

Normal

Rush

Specify \_\_\_\_\_

Collected By: Signature: Mize

Lab I.D.	Field Sample I.D.	Can#	Date & Time	Analyses Requested	Carrier Initial	Pressure Final	Vacuum Receipt
01A	AMS 4	DW	3/4/02	TO-15 + Naphthalene	-30	-10	
02A	AMS 3	UW	2/23/03	TO-15 + Naphthalene	-30	-8.5	

Relinquished By: (Signature) Mize Date/Time 7/23/03 1404

Received By: (Signature) Monica Gregson Date/Time 7/23/03

Relinquished By: (Signature) \_\_\_\_\_ Date/Time \_\_\_\_\_

Received By: (Signature) \_\_\_\_\_ Date/Time \_\_\_\_\_

Relinquished By: (Signature) \_\_\_\_\_ Date/Time \_\_\_\_\_

Received By: (Signature) \_\_\_\_\_ Date/Time \_\_\_\_\_

Shipper Name **AT-Bill #**

Ordered By **MC**

Temp. (C) **MC**

Condition **Good**

Carrier Seals Intact? **None**

Work Order # **0807494**

Use FediEx **8631 8423 4407**

Yes No **None**

Notes: Used flow controllers included  
Initial and final can pressures in inches Hg!  
Send Data Pack to Lisa McDonough and EDD to [datagroup@gaisconsultants.com](mailto:datagroup@gaisconsultants.com)





AN ENVIRONMENTAL ANALYTICAL LABORATORY

# SAMPLE RECEIPT SUMMARY

## WORKORDER 0807494

<b>Client</b>	<b>Phone</b>	<b>Date Promised:</b> 08/08/08
Ms. Theresa Landgraff	631-760-9300 x 12	<b>Date Completed:</b> 8/6/08
GEI Consultants, Inc.		<b>Date Received:</b> 7/25/08
110 Walt Whitman Road	<b>Fax</b>	<b>PO#:</b> NR
Suite 204		<b>Project#:</b> 061140-8-1703 BayShore OU1 Southern cell
Huntington Station, NY 11746		Air Monitorin
<b>Sales Rep:</b> TB		<b>Total \$:</b> \$ 624.00
		<b>Logged By:</b> MW

<u>Fraction</u>	<u>Sample #</u>	<u>Analysis</u>	<u>Collected</u>	<u>Receipt Vac./Pres.</u>	<u>Amount\$</u>
01A	AMS 4 DW	Modified TO-15	7/23/2008	7.5 "Hg	\$225.00
02A	AMS 3 DW	Modified TO-15	7/23/2008	8.0 "Hg	\$225.00
03A	Lab Blank	Modified TO-15	NA	NA	\$0.00
04A	CCV	Modified TO-15	NA	NA	\$0.00
05A	LCS	Modified TO-15	NA	NA	\$0.00
Misc. Charges 6 Liter Summa Canister (2) @ \$50.00 each., Shipment 58431					\$100.00
Blue Body Flow Controller (1) @ \$35.00 each., Shipment 58428					\$35.00
Blue Body Flow Controller (1) @ \$35.00 each., Shipment 58431					\$35.00
Fuel Surcharge (2) @ \$2.00 each.					\$4.00

**Note:** Samples received after 3 P.M. PST are considered to be received on the following work day.  
Atlas Project Name/Profile#: Bay Shore OU1 South Perimeter Air/9699

**BILL TO:** Ms. Theresa Landgraff  
GEI Consultants, Inc.  
110 Walt Whitman Road  
Suite 204  
Huntington Station, NY 11746

Analysis Code: TO-14A

**TERMS:**

Reporting Method: Modified TO-15 + Naph

180 BLUE RAVINE ROAD, SUITE B FOLSOM, CA - 95630  
(916) 985-1000 . (800) 985-5955 . FAX (916) 985-1020

## **Other Records**

## DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Vacuum}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} - [(\text{Initial Pressure ("Hg)}) (14.7 \text{ psi} / 30 \text{ "Hg})]}$$

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.5	1.36	1.71	2.05
1.0	1.39	1.74	2.09
1.5	1.41	1.77	2.13
2.0	1.44	1.80	2.16
2.5	1.46	1.83	2.20
3.0	1.49	1.87	2.24
3.5	1.52	1.90	2.29
4.0	1.55	1.94	2.33
4.5	1.58	1.98	2.38
5.0	1.61	2.02	2.42
5.5	1.64	2.06	2.47
6.0	1.68	2.10	2.53
6.5	1.71	2.15	2.58
7.0	1.75	2.19	2.64
7.5	1.79	2.24	2.69
8.0	1.83	2.29	2.76
8.5	1.87	2.34	2.82
9.0	1.91	2.40	2.89
9.5	1.96	2.46	2.96
10.0	2.01	2.52	3.03
10.5	2.06	2.59	3.11
11.0	2.12	2.65	3.19
11.5	2.17	2.72	3.28
12.0	2.23	2.80	3.37
12.5	2.30	2.88	3.46
13.0	2.36	2.97	3.57
13.5	2.44	3.06	3.67
14.0	2.51	3.15	3.79
14.5	2.59	3.25	3.91
15.0	2.68	3.36	4.04
15.5	2.77	3.48	4.18
16.0	2.87	3.60	4.33
16.5	2.98	3.73	4.49
17.0	3.09	3.88	4.66
17.5	3.22	4.03	4.85
18.0	3.35	4.20	5.05
18.5	3.50	4.38	5.27
19.0	3.65	4.58	5.51
19.5	3.83	4.80	5.77
20.0	4.02	5.04	6.06
20.5	4.23	5.31	6.38

Initial Vacuum ("Hg)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
21.0	4.47	5.60	6.73
21.5	4.73	5.93	7.13
22.0	5.03	6.30	7.58
22.5	5.36	6.72	8.08
23.0	5.74	7.20	8.66
23.5	6.19	7.76	9.32
24.0	6.70	8.40	10.10
24.5	7.31	9.17	11.02
25.0	8.04	10.08	12.12
25.5	8.93	11.20	13.47
26.0	10.05	12.60	15.15
26.5	11.49	14.40	17.32
27.0	13.40	16.80	20.20
27.5	16.08	20.16	24.24
28.0	20.10	25.20	30.31
28.5	26.80	33.61	40.41
29.0	40.20	50.41	60.61

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59

## DILUTION FACTORS

$$\text{Dilution Factor} = \frac{\text{Final Pressure}}{\text{Initial Pressure}} = \frac{14.7 \text{ psi} + \text{Final Pressure (psi)}}{14.7 \text{ psi} + \text{Initial Pressure (psi)}}$$

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
0.0	1.34	1.68	2.02
0.2	1.32	1.66	1.99
0.4	1.30	1.64	1.97
0.6	1.29	1.61	1.94
0.8	1.27	1.59	1.92
1.0	1.25	1.57	1.89
1.2	1.24	1.55	1.87
1.4	1.22	1.53	1.84
1.6	1.21	1.52	1.82
1.8	1.19	1.50	1.80
2.0	1.18	1.48	1.78
2.2	1.17	1.46	1.76
2.4	1.15	1.44	1.74
2.6	1.14	1.43	1.72
2.8	1.13	1.41	1.70
3.0	1.11	1.40	1.68
3.2	1.10	1.38	1.66
3.4	1.09	1.36	1.64
3.6	1.08	1.35	1.62
3.8	1.06	1.34	1.61
4.0	1.05	1.32	1.59
4.2	1.04	1.31	1.57
4.4	1.03	1.29	1.55
4.6	1.02	1.28	1.54
4.8	1.01	1.27	1.52
5.0	1.00	1.25	1.51
5.2	NA	1.24	1.49
5.4	NA	1.23	1.48
5.6	NA	1.22	1.46
5.8	NA	1.20	1.45
6.0	NA	1.19	1.43
6.2	NA	1.18	1.42
6.4	NA	1.17	1.41
6.6	NA	1.16	1.39
6.8	NA	1.15	1.38
7.0	NA	1.14	1.37
7.2	NA	1.13	1.36
7.4	NA	1.12	1.34

Initial Pressure (psi)	5 psi Final Press. Dil. Factor	10 psi Final Press. Dil. Factor	15 psi Final Press. Dil. Factor
7.6	NA	1.11	1.33
7.8	NA	1.10	1.32
8.0	NA	1.09	1.31
8.2	NA	1.08	1.30
8.4	NA	1.07	1.29
8.6	NA	1.06	1.27
8.8	NA	1.05	1.26
9.0	NA	1.04	1.25
9.2	NA	1.03	1.24
9.4	NA	1.02	1.23
9.6	NA	1.02	1.22
9.8	NA	1.01	1.21
10.0	NA	1.00	1.20
10.2	NA	NA	1.19
10.4	NA	NA	1.18
10.6	NA	NA	1.17
10.8	NA	NA	1.16
11.0	NA	NA	1.16
11.2	NA	NA	1.15
11.4	NA	NA	1.14
11.6	NA	NA	1.13
11.8	NA	NA	1.12
12.0	NA	NA	1.11
12.2	NA	NA	1.10
12.4	NA	NA	1.10
12.6	NA	NA	1.09
12.8	NA	NA	1.08
13.0	NA	NA	1.07
13.2	NA	NA	1.06
13.4	NA	NA	1.06
13.6	NA	NA	1.05
13.8	NA	NA	1.04
14.0	NA	NA	1.03
14.2	NA	NA	1.03
14.4	NA	NA	1.02
14.6	NA	NA	1.01
14.8	NA	NA	1.01

# Compound Listing

## Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
75-71-8	Freon 12	0.50	
76-14-2	Freon 114	0.50	
156-59-2	cis-1,2-Dichloroethene	0.50	
67-66-3	Chloroform	0.50	
71-55-6	1,1,1-Trichloroethane	0.50	
56-23-5	Carbon Tetrachloride	0.50	
71-43-2	Benzene	0.50	
107-06-2	1,2-Dichloroethane	0.50	
79-01-6	Trichloroethene	0.50	
78-87-5	1,2-Dichloropropane	0.50	
10061-01-5	cis-1,3-Dichloropropene	0.50	
108-88-3	Toluene	0.50	
10061-02-6	trans-1,3-Dichloropropene	0.50	
79-00-5	1,1,2-Trichloroethane	0.50	
127-18-4	Tetrachloroethene	0.50	
106-93-4	1,2-Dibromoethane (EDB)	0.50	
108-90-7	Chlorobenzene	0.50	
100-41-4	Ethyl Benzene	0.50	
108-38-3	m,p-Xylene	0.50	
95-47-6	o-Xylene	0.50	
100-42-5	Styrene	0.50	
79-34-5	1,1,2,2-Tetrachloroethane	0.50	
108-67-8	1,3,5-Trimethylbenzene	0.50	
95-63-6	1,2,4-Trimethylbenzene	0.50	
541-73-1	1,3-Dichlorobenzene	0.50	
106-46-7	1,4-Dichlorobenzene	0.50	
100-44-7	alpha-Chlorotoluene	0.50	
95-50-1	1,2-Dichlorobenzene	0.50	
106-99-0	1,3-Butadiene	0.50	
110-54-3	Hexane	0.50	
110-82-7	Cyclohexane	0.50	
142-82-5	Heptane	0.50	
75-27-4	Bromodichloromethane	0.50	
124-48-1	Dibromochloromethane	0.50	
98-82-8	Cumene	0.50	
103-65-1	Propylbenzene	0.50	
74-87-3	Chloromethane	2.0	
120-82-1	1,2,4-Trichlorobenzene	2.0	
87-68-3	Hexachlorobutadiene	2.0	
67-64-1	Acetone	2.0	
75-15-0	Carbon Disulfide	0.50	
67-63-0	2-Propanol	2.0	
156-60-5	trans-1,2-Dichloroethene	0.50	
78-93-3	2-Butanone (Methyl Ethyl Ketone)	0.50	
109-99-9	Tetrahydrofuran	0.50	
123-91-1	1,4-Dioxane	2.0	

# Compound Listing

## Modified TO-15 + Naph

CAS Number	Compound	Detection Limit	Type
		ppbv	
108-10-1	4-Methyl-2-pentanone	0.50	
591-78-6	2-Hexanone	2.0	
75-25-2	Bromoform	0.50	
622-96-8	4-Ethyltoluene	0.50	
64-17-5	Ethanol	2.0	
1634-04-4	Methyl tert-butyl ether	0.50	
91-20-3	Naphthalene	2.0	
107-05-1	3-Chloropropene	2.0	
540-84-1	2,2,4-Trimethylpentane	0.50	
2037-26-5	Toluene-d8		
17060-07-0	1,2-Dichloroethane-d4		
460-00-4	4-Bromofluorobenzene		
75-01-4	Vinyl Chloride	0.50	
74-83-9	Bromomethane	0.50	
75-00-3	Chloroethane	0.50	
75-69-4	Freon 11	0.50	
75-35-4	1,1-Dichloroethene	0.50	
76-13-1	Freon 113	0.50	
75-09-2	Methylene Chloride	0.50	
75-34-3	1,1-Dichloroethane	0.50	



**Not Applicable**